



APPENDIX B EUT TEST POSITION PHOTOS

Liquid depth $\geq 15\text{cm}$


- Phantom: SAM-Twin V8.0 P1aP2a; Type: QD 000 P41 AA ; Serial: 1962

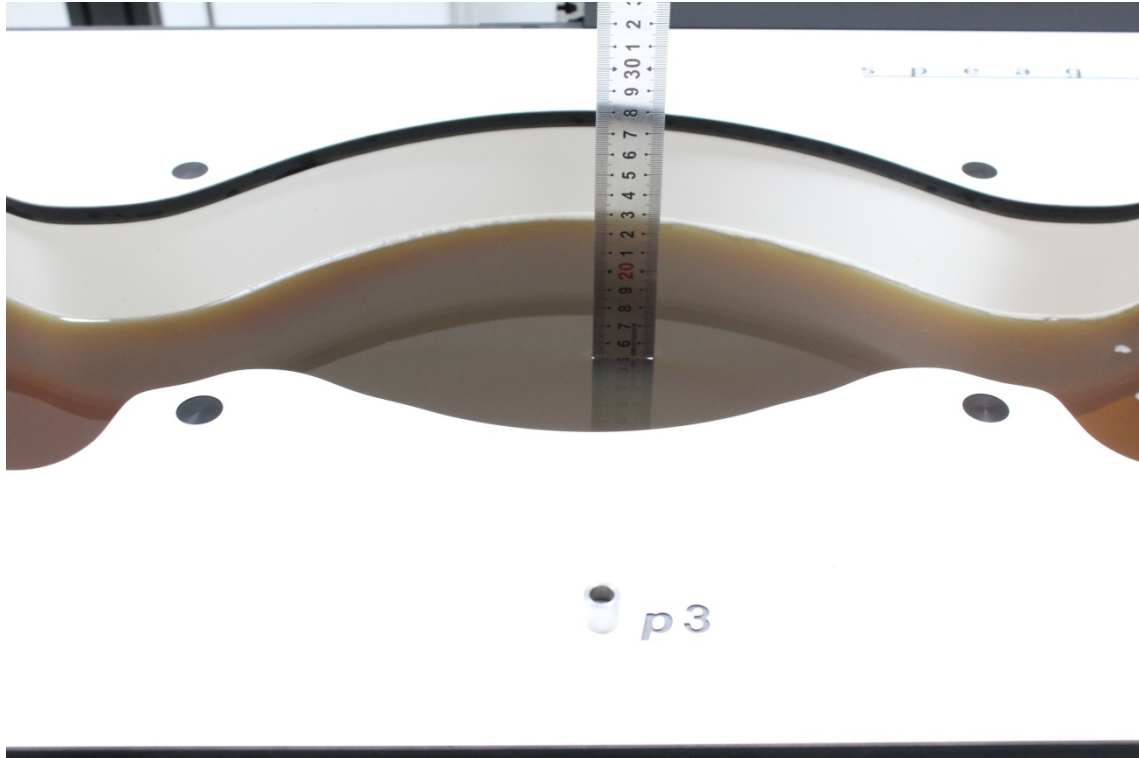


Head Left Cheek Setup Photo

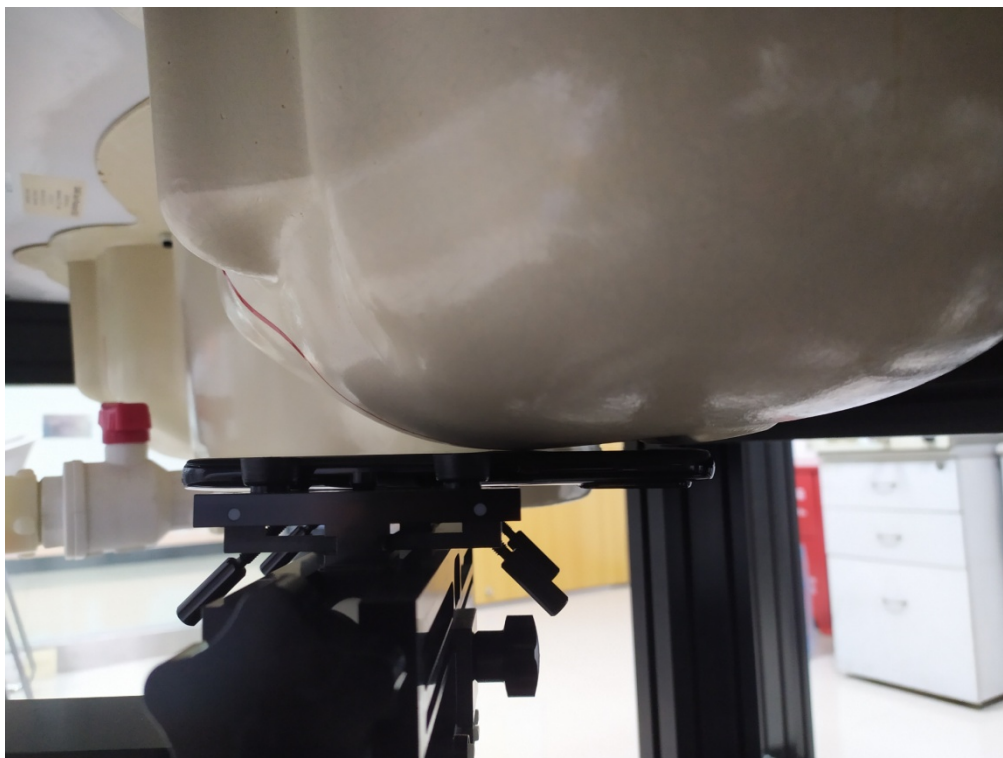

Head Left Tilt Setup Photo

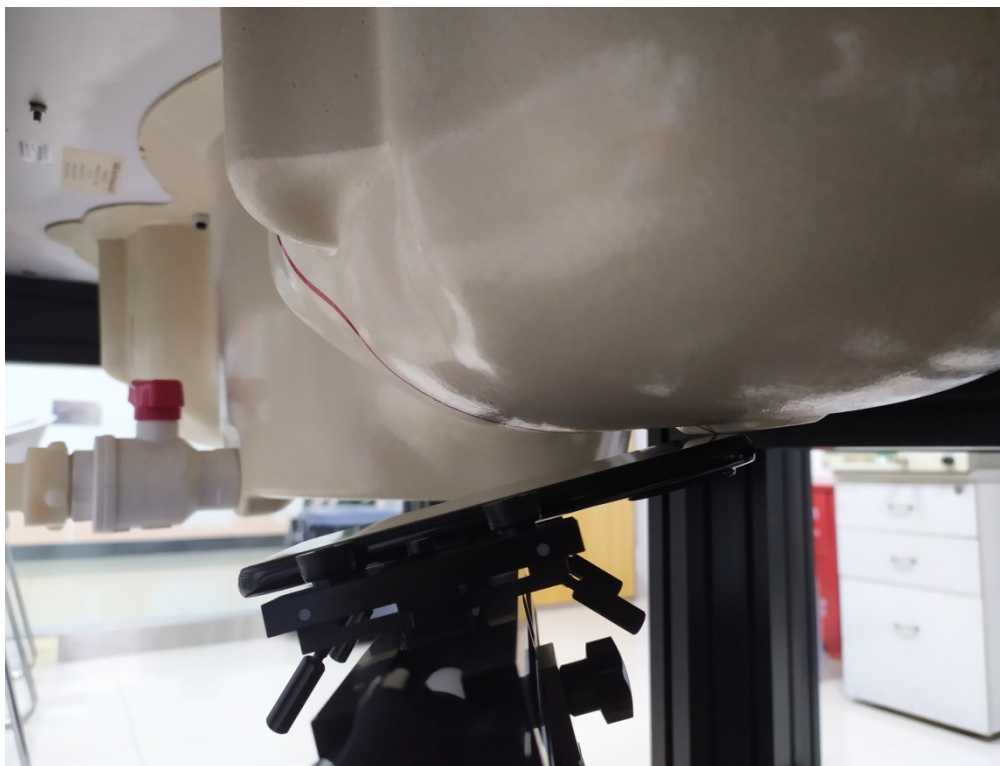


Head Right Cheek Setup Photo

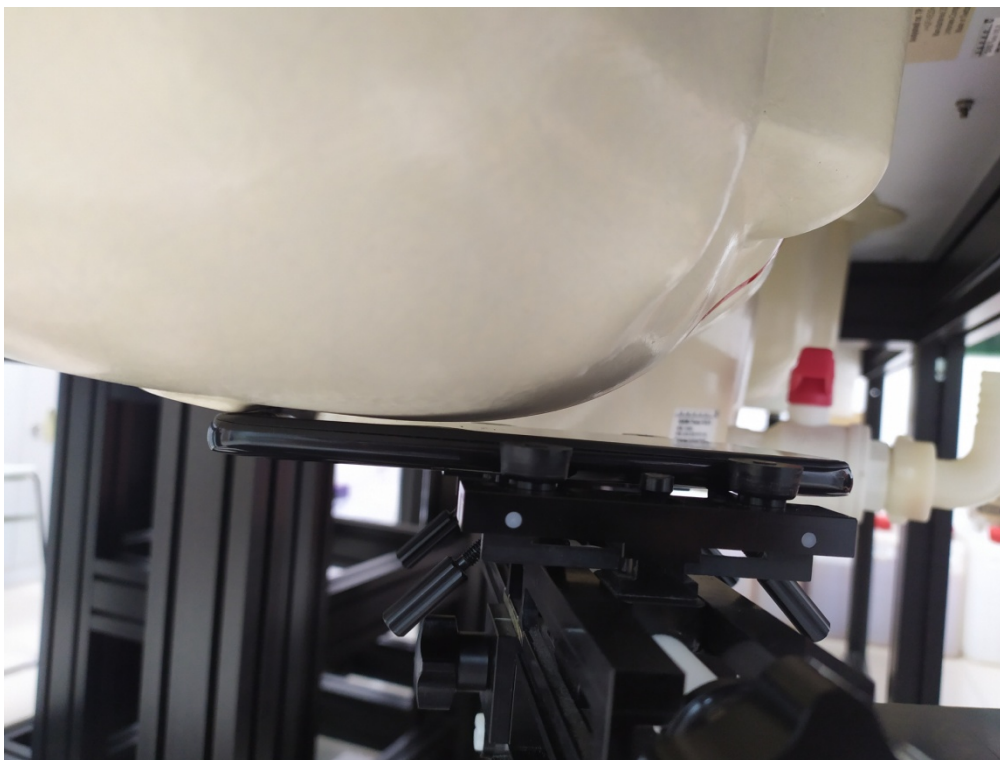


A close-up photograph of the sample holder in the SEM. A red double-headed arrow is superimposed on the image, indicating a distance of 10 mm between the sample and the detector.


Body Left Setup Photo (10mm)

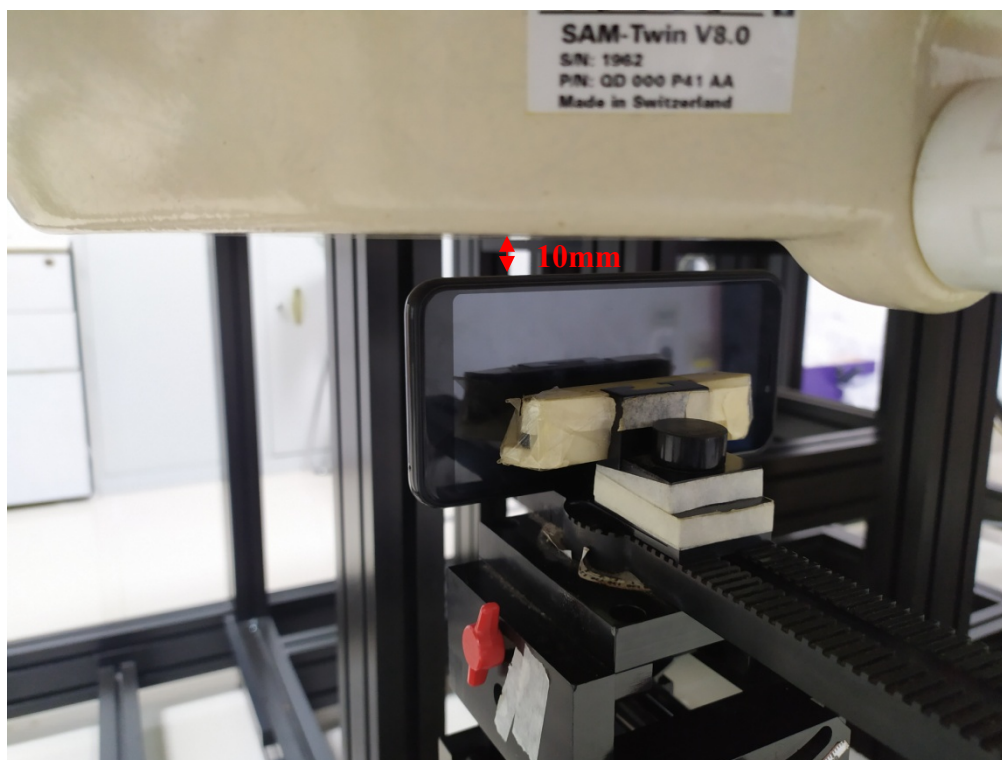

Body Right Setup Photo (10mm)

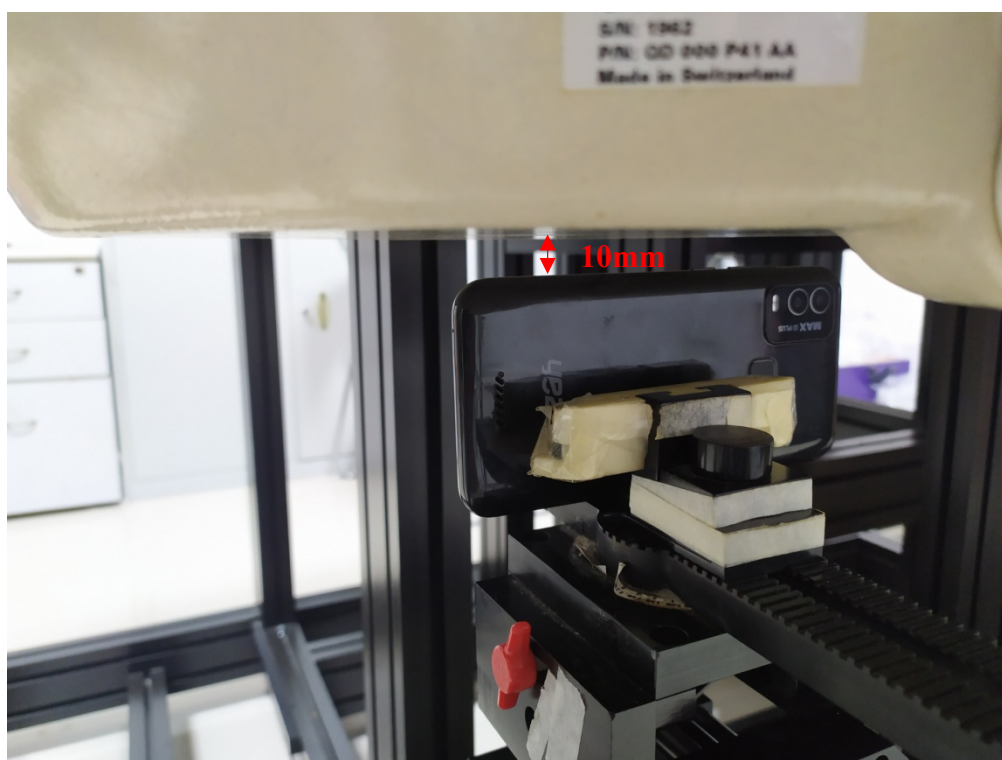

Body Top Setup Photo (10mm)

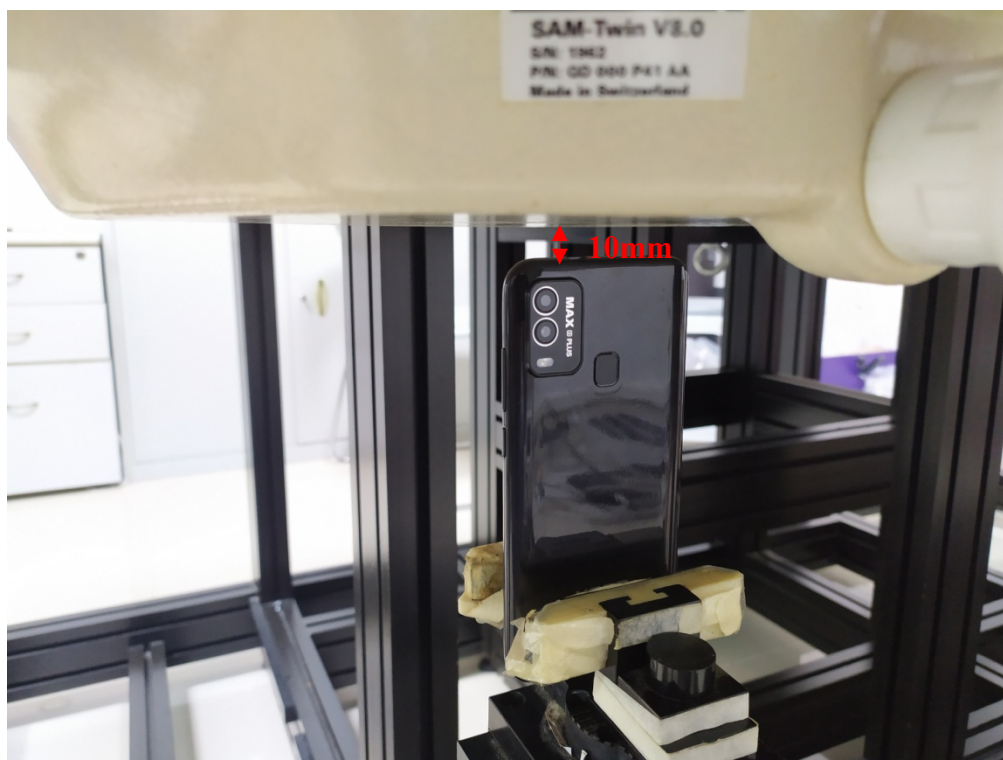

Body Bottom Setup Photo (10mm)

