

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 1 / 44     |

SPIROHOME®  
ULTRASONIC SPIROMETER

The document will be signed after revision.

|             | FUNCTION                                  | DATED | SIGNED |
|-------------|-------------------------------------------|-------|--------|
| Prepared by | Regulatory Affairs<br><b>Deniz SARP</b>   |       |        |
| Reviewed by | Quality Assurance<br><b>Ahmet Gökdere</b> |       |        |
| Approved by | CEO<br><b>Merthan Öztürk</b>              |       |        |

## REVISION RECORD

| REVISION<br>NUMBER | DATE       | COMMENTS      | SIGNED |
|--------------------|------------|---------------|--------|
| 00                 | 24.02.2019 | Initial Issue |        |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 2 / 44     |

# Spirohome® Personal

## User Manual

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 3 / 44     |

# 1. Preface

## 1.1 Spirohome® Personal user manual version history

| Version Number | Publication Date | Description                       |
|----------------|------------------|-----------------------------------|
| Rev.00         | 24.02.2019       | Initial version for market launch |

This revision of the Spirohome® Personal user manual applies to Spirohome® Personal devices with a serial number between S011900001-S011900150.

Version histories of all Spirohome® user manuals can be found on the Spirohome® website [www.spirohome.io](http://www.spirohome.io).

For any queries relating to the revision history of the user manual or product, please contact your Spirohome® dealer or manufacturer.

## 1.2 Intended use of the Spirohome® Personal

The Spirohome® Personal is a prescription device for diagnostic spirometry testing of adult and pediatric patients over the age of 5 who have been diagnosed with a chronic pulmonary disease including, but not limited to, asthma, chronic obstructive pulmonary disease and cystic fibrosis. **It is to be operated in the home setting by competent adult patients or caregivers of patients.**

## 1.3 About this user manual

This user manual should be read by users of the device prior to operating the Spirohome® Personal. Store this user manual in a clean and easily accessible place for future reference.

## 1.4 Legal Information

Contents of the user manual may be subject to change. Please refer to the Spirohome® website for the latest version of user manuals. No part of this manual may be reproduced without the written permission from Inofab.

© İnofab Sağlık Teknolojileri A.Ş., Ankara, Turkey. All rights reserved.

Spirohome® is a registered trademarks of İnofab Sağlık Teknolojileri A.Ş.

Spiroway® s a registered trademarks of İnofab Sağlık Teknolojileri A.Ş.

Bluetooth® is a registered trademark of Bluetooth SIG, Inc.

## 1.5 Electromagnetic Compatibility

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 4 / 44     |

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications made to this equipment not expressly approved by Inofab Sağlık Teknolojileri A.Ş. may void the FCC authorization to operate this equipment.

## 1.6 Product Disposal

This product should not be discarded as regular household waste but as electronic waste according to in accordance with local regulations and returned to a collection point of recycling electric and electronic devices.

Used batteries should be disposed of in designated battery recycling containers in accordance with local laws and regulations

## 1.7 Manufacturer Information



İnofab Sağlık Teknolojileri A.Ş.  
ODTÜ Teknokent Silikon Blok  
K:1 NO:15-A Ankara/Turkey  
Tel: +90 312 988 0308  
[www.spirohome.io](http://www.spirohome.io)

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 5 / 44     |

## Table of Contents

### 1. Preface

- 1.1 Spirohome® Personal user manual version history
- 1.2 Intended use of the Spirohome® Personal
- 1.3 About this user manual
- 1.4 Legal Information
- 1.5 Electromagnetic interference
- 1.6 Product disposal
- 1.7 Manufacturer Information

### 2. Safety Information

- 2.1 Safety warnings and precautions
- 2.2 Restrictions on use and contraindications
- 2.2 Signs and symbols

### 3. About the Spirohome® Personal

- 3.1 Product description
- 3.2 The Spirohome® Personal System
- 3.3 Orderable accessories

### 4. Cybersecurity

- 4.1 About cybersecurity and your Spirohome® Personal
- 4.2 Passwords on the Spirohome® Personal platform
- 4.3 Software Updates
- 4.4 Data back-ups
- 4.5 Security breaches
- 4.6 Lost or stolen devices

### 5. Spirohome® Personal and smart device connectivity

- 5.1 Connectivity of the Spirohome® Personal platform

### 6. Operating the device

- 6.1 How to use the Spirohome® Personal: An overview
- 6.1 Operating environment
- 6.2 Setting up your Spirohome® Personal
- 6.3 Device indicators
- 6.4 Technical features of the Spirohome® Personal
- 6.5 Troubleshooting and error messages

### 7. Spirometry with your Spirohome® Personal

- 7.1 How to perform a spirometry test
- 7.2 Spirometry parameters
- 7.3 Types of breathing maneuvers
- 7.4 Understanding test quality

### 8. Maintenance and Cleaning of your Spirohome® Personal

- 8.1 Cleaning and disinfection of the device

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 6 / 44     |

8.2 Cleaning of the Spiroway® mouthpiece

8.3 Replacing batteries

## 9. Terms of warranty

9.1 Terms of warranty for the Spirohome® Personal

## 10. Appendix

8.1 Electromagnetic compatibility

## 2. Safety Information

### 2.1 Safety warnings and precautions

***Important! Please adhere to the recommendations, warnings and guidelines set out in this user manual as failure to comply may result in measurement errors, display of incorrect results or harm to the user.***

#### **General:**

The manufacturer is not responsible for any damage/harm to either the device or user which has resulted from nonadherence to the warnings, precautions and instructions given in the official device user manual, labeling and other informational material.

In the occurrence of any adverse events, report immediately to your doctor and/or authorities as required by local legislation. The user must also report such incidents to the manufacturer.

#### **Product and components:**

Do not use the device if there is any damage is present on the device or its components upon removal from packaging, and return the product to the supplier.

The Spirohome® Personal must only be used with the original accessories specified and provided by the manufacturer. Use of unspecified mouthpieces may cause inaccurate test readings, or damage/harm to the user and/or device. Do not cause damage to or use the mouthpieces with physically compromised filters.

Do not expose the device to liquids, prevent any liquids from entering the device. In the event of a liquid spill on or around your Spirohome® Personal, immediately remove the batteries and let the device dry thoroughly before use.

#### **Data:**

Only a qualified healthcare professional can make a diagnosis with, in addition to other medical testing and your clinical history, the data presented by the Spirohome® Personal.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 7 / 44     |

Please ensure that your personal data such as height, weight, age, sex and ethnicity are entered according to your current state and that the values are entered correctly.

Regardless of the data presented on the Spirohome® Personal, if you feel unwell or have respiratory illness symptoms please contact your healthcare provider immediately.

Please follow all data security warnings and recommendations for your personal smart device as per its manufacturer's instructions as your personal data, which will include that recorded and stored on the Spirohome® App, may otherwise be at risk. The user is encouraged to not share their Spirohome® app account information with unauthorized parties.

If your Spirohome® Personal is damaged or malfunctioning or you encounter data that you cannot make sense of, contact the manufacturer directly and cease use.

#### **Users:**

Do not use your Spirohome® Personal for any other purpose than its intended use. Spirohome® Personal is not recommended for children under the age of 5.

Do not share your Spirohome® Personal with any other users, including family members, as the Spirohome® Personal and Spiroway® reusable mouthpiece is to be used by a *single user* only. If a new user is to use the device, ensure that the device is cleaned and disinfected (see Maintenance section of this manual), a new mouthpiece is used and a new account is created for the user on the app.

For patients who require assistance by competent caregivers, special warnings regarding the Spirohome® Personal should be provided by the caregiver to the patient prior to using the device.

#### **Testing:**

One 'use' of the spirometer is defined as one complete spirometric testing session (can include up to 8 individual successive spirometry tests). The mouthpiece should be fully inserted before and during a test. Start test again if mouthpiece dislodges during testing.

You **MUST** use a mouthpiece during testing. Blowing into the device directly will cause incorrect measurements and potential harm to both the user and device.

Make sure the base of the device lumen is clear of fingers or any other materials that may be blocking this exit as measurement by the device may be affected.

Do not walk or run while taking a lung function measurement using Spirohome® spirometer. Do not perform a spirometry test with food or objects in oral cavity to avoid risk of choking.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 8 / 44     |

Pulmonary function tests require maximum effort on the part of the patient and may lead to sensations of dizziness or giddiness. Do not perform more than 8 spirometry tests in one spirometry session. If you sense dizziness while performing a test, stop the test immediately and rest.

### ***Environment and storage:***

Store and use the device as specified in this user manual as alternative methods or conditions of storage may affect device function and/or accuracy. Use only in specified environments/conditions (see Operating Environment section of this user manual) to avoid malfunction and/or display of incorrect results.

Store the Spirohome® Personal in dust/dirt and moisture free conditions. You may utilize the pouch provided with the device to keep the device protected. Before each use, always check that the device is free from contaminants and does not have any visible damage.

To prevent damage to the Spirohome® Personal due to battery leakage or oxidation, remove all batteries if the Spirometry module is not to be used or is to be stored for a long period of time.

The Spirohome® Personal should never be used with a charging smart device. Make sure the smart device is unplugged from its charger before conducting a spirometry test.

### ***Maintenance:***

The user should periodically check to ensure that foreign bodies or impurities are not present on visible and accessible areas of the device as this could lead to inaccuracies in test measurements. Coughing or spitting into the device may cause incorrect readings.

All repairs, modifications or reconfigurations must be performed only by the manufacturer, an opened device casing will terminate product warranty.

## **2.2 Restrictions on use and contraindications**

Spirohome® Personal must only be used by a *single user*. If the device will be passed on to a new user, ensure that the personal data of the previous user is erased from device memory and the personal data of the new user is entered into the system prior to conducting any tests.

Do NOT share the Spiroway® reusable mouthpiece, including with family members. Any new user of the device must use a new Spiroway® reusable mouthpiece.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 9 / 44     |

The spirometry tests should only be performed by users who do not experience any shortness of breath and are in good health for performing a lung function test. Test results of patients who do not meet these conditions may not be reliable.

Failure to perform the specific breathing maneuver of a particular spirometry test correctly may lead to inaccurate and/or unacceptable results. Refer to the Breathing Maneuvers section of this user manual for more information.

Some medical conditions may pose a danger to you or affect the validity of spirometry performance and results. These conditions include, but are not limited to, the following: acute disorders (e.g. active lung infection), illness or condition that may cause serious consequences if aggravated by forced expiration (e.g. dissecting / unstable aortic aneurysm, recent/current pneumothorax, recent surgery including ophthalmic, thoracic, abdominal or cerebral aneurysms, unstable angina), recent myocardial infarction (within one month), recent pulmonary embolism, undiagnosed chest conditions (e.g. haemoptysis of unknown origin), nausea, vomiting, severe respiratory distress, physical limitations or cognitive impairment or dementia. ***If you have or suspect having any of the conditions above, consult your healthcare professional before using the Spirohome® Personal.***

## 2.2 Signs and symbols

Please note the following signs and symbols provided for the safe use and storage of your Spirohome® Personal.

| Markings                                                                            | Descriptions                                                                              |
|-------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------|
|  | "Manufacturer"<br>The name and the address of the manufacturer is adjacent to the symbol. |
| 'FCC ID'                                                                            | Unique identifier given by the Federal Communications Commission                          |
| 'Rx Only'                                                                           | Prescription-only device                                                                  |
|  | Disposal in compliance with Waste Electrical and Electronic Equipment Directive           |
|  | Temperature limit                                                                         |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 10 / 44    |

|                                                                                     |                                         |
|-------------------------------------------------------------------------------------|-----------------------------------------|
|    | Humidity limit                          |
|    | Atmospheric pressure limit              |
|    | Do not use if package is damaged        |
|    | Keep away from sunlight                 |
|  | Keep dry                                |
|  | Single use only                         |
|  | Type BF of Medical Electrical Equipment |
| <b>SN</b>                                                                           | Serial Number                           |
| <b>LOT</b>                                                                          | Lot Number                              |
| <b>REF</b>                                                                          | Ref Number                              |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 11 / 44    |

| IP                                                                                | IP Number                                    |
|-----------------------------------------------------------------------------------|----------------------------------------------|
|  | Device includes RF transmitters              |
|  | The instruction manual/booklet must be read. |

### 3. About the Spirohome® Personal

#### 3.1 Product description


The Spirohome® Personal is a portable spirometer that pairs (via Bluetooth®) to smart devices running with iOS or Android. The Spirohome® Personal measures and displays certain parameters of lung function of the user. The user performs a spirometry test as described in the *How to perform a lung function test* section of this user manual. Briefly, as the user exhales into the device through its mouthpiece, internal ultrasonic sensors detect the volume and speed of the expired air, the device converts this information into spirometric data and displays it via the Spirohome® application on a connected smart device. The Spirohome® app prompts and guides the user throughout the test for accurate data collection and display. The Spirohome® app can be downloaded on GooglePlay or on Apple's App Store. The device is powered by 2 x AAA Alkaline batteries. Spirohome® Personal works with the Spiroway® reusable mouthpiece.

#### 3.2 The Spirohome® Personal System

Your Spirohome® Personal System consists of:

- Spirohome® Personal (b)
- Spiroway® reusable mouthpiece(a)
- Spirohome® Personal cap(c)
- 2 x AAA Batteries
- User manual
- Quick start guide
- Carrying pouch(d)

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 12 / 44    |

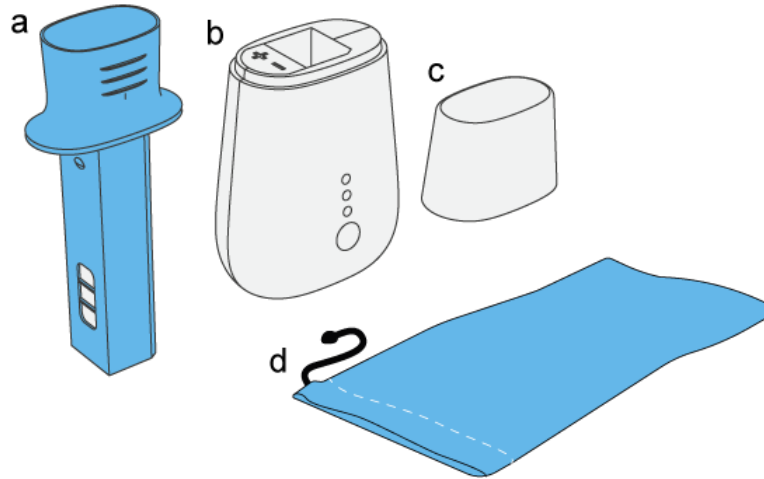

**Caution!:** Please check to ensure that there is no visible damage on any of the components of the Spirohome® Personal. If damage is present, do not use or attempt to repair the device, please contact the manufacturer directly.

**Connected smart device requirements:**

Spirohome® Personal with iOS device: Requires iOS 11.0 or later. Compatible with Iphone 5s or later, iPad Air Wifi or later, and Ipod touch.

Spirohome® Personal with Android device: Requires Android API level 21 (Lollipop 5.0) or later.

**3.3 Orderable accessories**

You can order new or replacement Spirohome® Personal accessories from [www.spirohome.io](http://www.spirohome.io). When placing your order, please be sure to note the accessory reference number.

| Accessory Name                  | Reference Number |
|---------------------------------|------------------|
| Spiroway® Reusable Mouthpiece   | 03000            |
| Spiroway® Disposable Mouthpiece | 04000            |
| Spirohome® Personal Cap         | 01104            |
| Spirohome® Pouch                | 01509            |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 13 / 44    |

## 4. Cybersecurity

To protect your device and data, please read and apply the following guidance.

### 4.1 About cybersecurity and your Spirohome® Personal

The Spirohome® Personal platform involves the connection of your Spirohome® Personal device to the Spirohome® Personal app. The data you enter and record with your Spirohome® Personal device via the Spirohome® Personal app is stored on a SQL-server database.

Spirohome® Personal automatically connects to the network. It will still work off-line, and transfer data to the network as soon as a connection is established. Both the local database (connected smart device) and server-based database (Spirohome® database on the network) is encrypted.

### 4.2 Passwords on the Spirohome® Personal platform

Access to your Spirohome® Personal device is granted through the entry of a username and password which you will create at first set-up of the device and app. It is the responsibility of the user to change or update password information at regular intervals (every 3 months) for ensuring security. Please choose a password that is strong and difficult to be copied by unauthorized users. The minimum requirements for a Spirohome® password is using at least 8 characters, at least one uppercase and one lower case alphabetic characters and at least one number.

### 4.3 Software Updates

In order to improve the Spirohome® app features or incorporate new security features, Spirohome® software updates may be sent to your smart device. Your device will be sent notifications about installing the latest update to the app. If warning notifications for software updates are ignored, access to testing on the app may be barred until the update has been installed. This is to ensure that important improvements to app features and security have been updated for your safety.

### 4.4 Data back-ups

Any data that is stored on Spirohome® servers are periodically backed-up. Spirohome® devices must be connected to a network to allow for data on the device to be transferred, stored and regularly backed-up on Spirohome® servers. For any data that is stored on personal servers or smart devices, it is the responsibility of the user to back this data up.

### 4.5 Security breaches

1. Change password, password is checked every time you log in. Changing password on one connected device will log you out of all connected devices.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 14 / 44    |

- If your password has been breached, try resetting your password through your registered email address by clicking 'Forgot Password'.
- Contact manufacturer

#### 4.6 Lost or stolen devices

If your Spirohome® Personal device is lost or stolen, please report the issue immediately and directly to your Spirohome® Personal provider. Your provider will ensure that your device is locked for use by any unauthorized users.

Your device is paired to your user account. A device cannot be designated to two different user accounts.


## 5. Spirohome® Personal and smart device connectivity

### 5.1 Connectivity of the Spirohome® Personal platform

The Spirohome® platform allows a range of devices to connect to a central network. Several smart devices with the Spirohome® Personal app can connect to and share information on a central database. Access to a patient's information from different devices requires that the same user account information is entered on all devices.

## 6. Operating the device

### 6.1 How to use the Spirohome® Personal: An overview

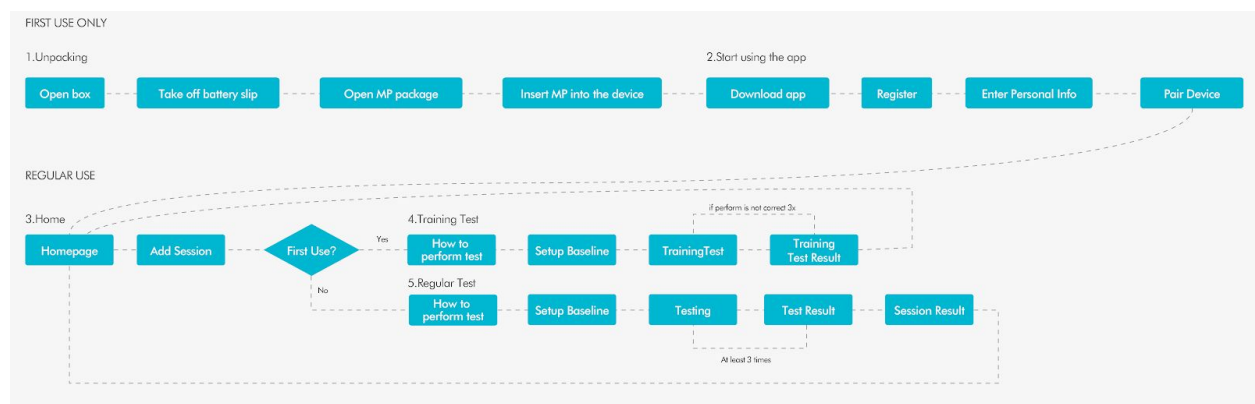

### 6.2 Operating environment

The Spirohome® Personal is designed for use in a home setting. It should not be used in a clinical setting such as a hospital or private clinic.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 15 / 44    |

The *operating conditions* for the Spirohome® Personal is specified as:

Temperature: 15°C to +40°C

Relative Humidity: 5% to 95%

The *storage conditions* for the Spirohome® Personal is specified as:

Temperature: -20°C to +50°C

Relative Humidity: 5% to 95%

Pressure: 500 hPa to 1060 hPa



The Spirohome® Personal should not be used in the presence of inflammable liquids or detergents, nor in the presence of inflammable anaesthetic gases (oxygen or nitrogen).

The device should not be used in direct air currents (e.g. wind), sources of heat or cold, direct sun rays or other sources of light or energy, dust, sand or any other chemical substances.


The instrument may give inaccurate readings if operated in the presence of strong electromagnetic sources, such as electrosurgical equipment, or in the presence of computed tomography (CT) equipment.

The Spirohome® Personal conforms to EN 60601-1, EN 60601-1-11, EN 60601-1-2 and EN 300 328. As this device operates with RF technology, it must be only as specified by the manufacturer, it may to avoid interference to radio communications.

### 6.3 Setting up your Spirohome® Personal

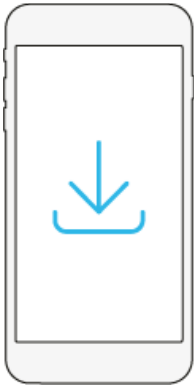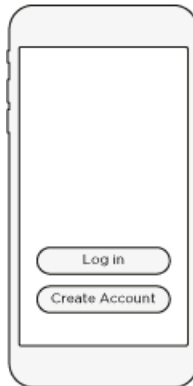
|                                                                                                                                                                                                          |                                                                                                                                                                                                                  |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p><b>1.</b>Download the Spirohome® Personal app from the App Store or Google Play Store onto your smart device.</p>  | <p><b>2.</b> Follow the steps given on the app screen to create a new user account or log in to your existing account.</p>  |
| <p><b>3.</b> Pull out the battery protector (1) and press the power button (2) for one second to switch</p>                                                                                              | <p><b>4.</b> Enable Bluetooth® on your smart device, and select your Spirohome® Personal from</p>                                                                                                                |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 16 / 44    |

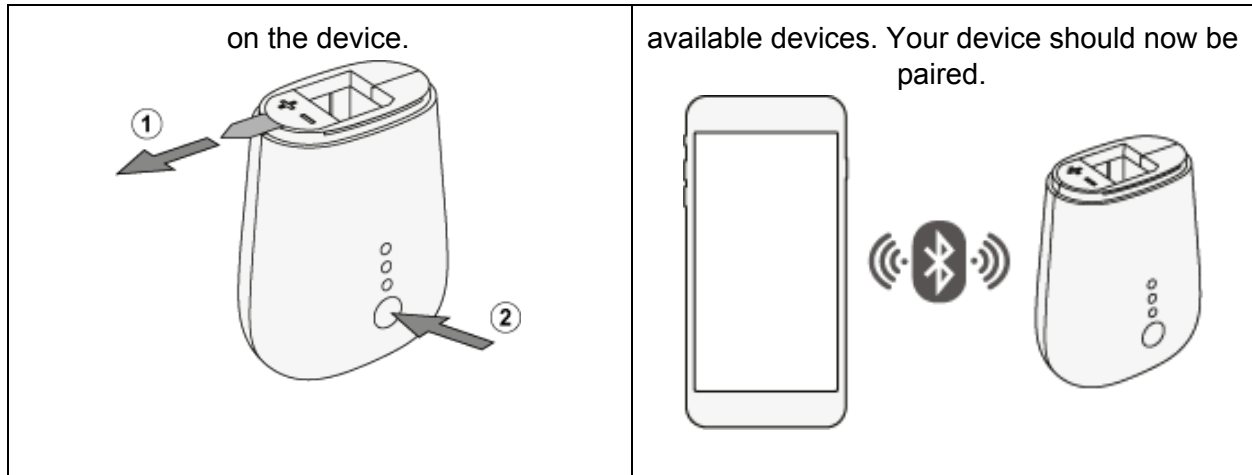

#### 6.4 Device indicators

There are 3 LED lights located on the front of the device. The following picture shows the assigned numbers to each LED.

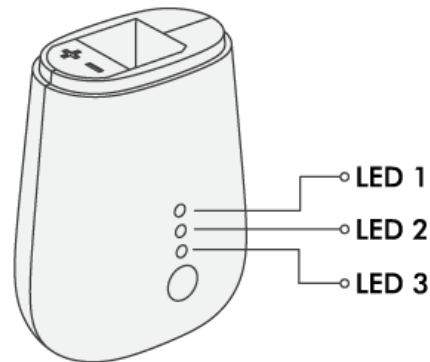

The LED lights may be turned on or flashing various colors and/or in various patterns. The LED lights indicate the current status of the device. Please see the following information for guidance on LED light indications.

| LED Display                                     | Indication/s               |
|-------------------------------------------------|----------------------------|
| None of the LEDs are on                         | The device is switched off |
| LED indicators are consecutively flashing green | The device is switching on |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 17 / 44    |

|                                                              |                                                                                        |
|--------------------------------------------------------------|----------------------------------------------------------------------------------------|
| LED number 3 is constantly flashing green                    | The device is switched on                                                              |
| LED number 2 is fading blue                                  | The device is connected to the app. Bluetooth® connection has been established.        |
| LED number 2 and LEDs 1 and 3 together are flashing in turn. | The baseline is setting up.                                                            |
| LED number 1 is constantly blue.                             | The device is ready for a test.                                                        |
| During a test, LED number 1 is constantly yellow.            | The test has timed-out (there has been no inhalation/exhalation over a period of time) |
| During baseline setup LED number 1 is constantly yellow.     | The baseline setup has been unsuccessful.                                              |
| All LEDs are flashing red.                                   | There is a foreign object between the sensors. (TOF out of range error)                |
| LEDs are consecutively flashing yellow.                      | Over-the-air connection is being established.                                          |
| LED number 3 flashes red three times.                        | Battery low warning.                                                                   |
| LEDs flash in reverse order and remain switched off.         | The device is switching off.                                                           |

## 6.5 Technical features of the Spirohome® Personal

|                                  |                                   |
|----------------------------------|-----------------------------------|
| Flow / Volume measurement method | Ultrasonic Transducer Measurement |
| Power Supply                     | 2 x 1.5V AAA batteries            |
| Dimensions                       | 110 x 63 x 41 mm                  |
| Weight (With batteries)          | 90 g                              |
| Weight (Without batteries)       | 67 g                              |
| Flow range                       | 0 - 14 L/s                        |
| Maximum volume measured          | 10 L                              |
| FVC accuracy (Average)           | ± 2 %                             |
| FEV1 accuracy (Average)          | ± 2 %                             |
| PEF accuracy (Average)           | ± 1.9 %                           |
| Dynamic resistance at 14 L/s     | 68.2 Pa*s/L                       |
| Volume resolution                | 1 mL                              |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 18 / 44    |

|                      |           |
|----------------------|-----------|
| Flow resolution      | 1 mL/s    |
| Medical device class | Class IIA |
| Wireless connection  | BLE 4.2   |

## 6.6 Troubleshooting and error messages

| Problem                                                    | Cause                                      | Solution                                                                                                                         |
|------------------------------------------------------------|--------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------|
| Device Not turning on                                      | Multiple possible causes                   | Check battery orientation and correct polarities!                                                                                |
|                                                            |                                            | Remove the AAA batteries and wait 30 seconds and reinstall AAA batteries                                                         |
|                                                            |                                            | Replace AAA batteries                                                                                                            |
|                                                            |                                            | Check that the battery cap is in the lock position, or if cap is broken, contact manufacturer                                    |
| Spirohome® cannot connect to a smart device via Bluetooth® | Smart device is out of range               | Bring your smart device closer to the Spirohome® device                                                                          |
|                                                            | Smart device Bluetooth® is disabled        | Enable Bluetooth® of your smart device                                                                                           |
|                                                            | Bluetooth® connection not working properly | Your smart device will need Bluetooth® version 4.0 or higher. Find and select Spirohome® Personal from list of detected devices. |
| Test results are inconsistent                              | Spiroway® mouthpiece is dirty              | Clean Spiroway® mouthpiece to ensure that the lumen is not obstructed or replace with a new mouthpiece                           |
|                                                            | Spiroway® mouthpiece is damaged            | Replace Spiroway® mouthpiece                                                                                                     |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 19 / 44    |

|                                                      |                                               |                                                                                                                                                                                                                      |
|------------------------------------------------------|-----------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                      | Spirometry test was performed incorrectly     | Refer to How to Perform a Lung Function Test in user manual or refer video tutorial on app                                                                                                                           |
|                                                      | Spiroway® mouthpiece is installed incorrectly | Refer to the user manual for proper installation of Spiroway® mouthpiece                                                                                                                                             |
| Test does not start - Cannot set up baseline         | Direct air current in environment             | Close the cap of the Spirohome® to avoid effects of environmental flow                                                                                                                                               |
|                                                      |                                               | Place device on a flat surface                                                                                                                                                                                       |
|                                                      |                                               | Remove causes of direct air current e.g. air conditioner, opened window, fan, etc.                                                                                                                                   |
| Test does not start - animated balloon is not moving | Multiple possible causes                      | Quit test and start new test                                                                                                                                                                                         |
|                                                      |                                               | Quit application and start a new test                                                                                                                                                                                |
|                                                      |                                               | Switch device on and off again to reset                                                                                                                                                                              |
| Test Starts before you start blowing                 | Vigorous handling of the device               | Keep device as stable as possible after starting a test                                                                                                                                                              |
| Test does not end and keeps going                    | Inhalation at the end of test not performed   | After a forced exhalation, take a short breath through the spirometer before breaking the seal of your lips around the mouthpiece. The device ends the measurement when it detects a small amount of negative volume |

| Error Messages |                |          |
|----------------|----------------|----------|
| Message        | Possible Cause | Solution |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 20 / 44    |

|          |                                                          |                                                                                                                                  |
|----------|----------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------|
| Error 01 | Bluetooth® is disabled                                   | Enable Bluetooth® on your smart device from its settings menu                                                                    |
| Error 02 | Batteries of the Spirohome® Personal need to be replaced | Replace batteries as described in the Maintenance section of this user manual                                                    |
| Error 03 | Components not attached correctly.                       | Ensure that the mouthpiece is attached to your Spirohome® Personal device correctly                                              |
|          | Sensors are obstructed.                                  | Ensure that the components are clean and clear of foreign body materials.                                                        |
|          | Test was not performed correctly.                        | Repeat the test following the rules and conditions specified in the Performing a Lung Function Test section of this user manual. |
| Error 04 | Flow measurement limit is exceeded                       | Consult the manufacturer or healthcare provider                                                                                  |
| Error 05 | Sensor Error                                             | Consult Manufacturer                                                                                                             |
| Error 06 | Device disconnected during test                          | Relaunch app and start test again                                                                                                |
| Error 07 | Self sensors test failed                                 | Check lumen of device to ensure that sensors are not obstructed                                                                  |
|          |                                                          | Contact Manufacturer                                                                                                             |
| Error 08 | Poor or no internet connection                           | Check to ensure that smart device is connected to the internet                                                                   |

For any other technical queries please call our customer service on +90 312 988 03 08

## 7. Spirometry with your Spirohome® Personal

### 7.1 How to perform a spirometry test

There are several types of tests and different parameter relating to lung function that can be involved in a spirometry test. Each type of spirometry test requires a specific breathing maneuver in order to detect the parameters related to that particular test type. However, the general method of performing a spirometry test remains the same for all test types. Please keep reading for more information about test types, test parameters, breathing maneuvers and understanding the quality of test results.


Note: One spirometry session refers to a full set of spirometry tests performed in one sitting. The recommended number of tests per spirometry session is 3, however, you may perform up to 8 tests. The best values obtained from the spirometry tests performed in one session is displayed

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 21 / 44    |


on the app interface. You also have the option to view the results of each spirometry test performed in a spirometry session separately.

**General method for performing a spirometry test with the Spirohome® Personal:**

1. Remove the Spiroway® reusable mouthpiece from its plastic packaging and insert it all the way into the Spirohome® Personal as shown. A 'click' will be heard when the mouthpiece is inserted correctly all the way into the device.

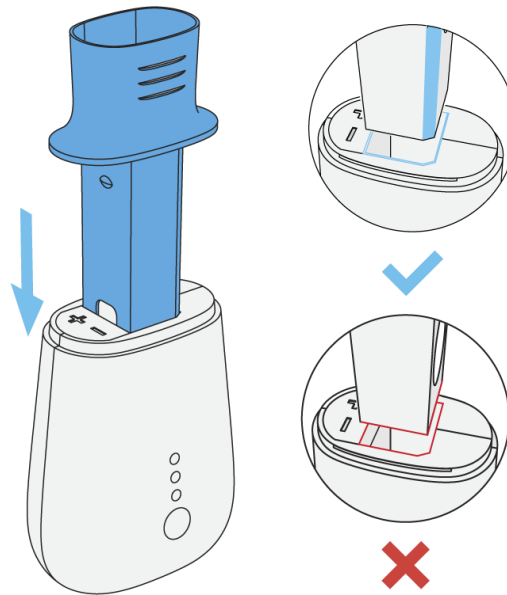

2. Load the Spirohome® Personal App on your smart device and sign in. Tap the 'plus' button (shown) to start a new test.

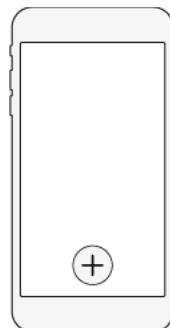


|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 22 / 44    |

3. The first step will be to record a baseline for the device. To perform the baseline setup, place the device cap on and stabilize the device during the baseline setup. Alternatively, place the device on a flat surface and allow the baseline setup to be completed.



4. You will then be prompted to perform a spirometry test. Place the mouthpiece in your mouth, past your teeth, and form a tight seal around the mouthpiece with your lips.

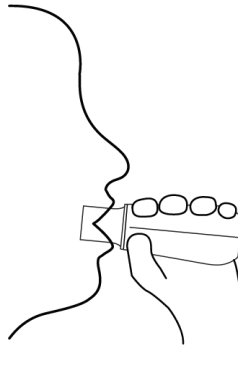

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 23 / 44    |

5. Perform the breathing maneuver related to the specific test you wish to perform. Please see the Breathing Maneuvers section of this user manual for more information.

## 7.2 Spirometry Parameters

**NOTE: Your Spirohome® Personal can measure all of the parameters listed below, however, the set of parameters actually displayed on the app will depend on the level of access to your test results that your Spirohome® user account has been granted.**

The Spirohome® Personal records and displays the following spirometry test data:

| Test | Primary Parameters*                            | Unit |
|------|------------------------------------------------|------|
| FVC  | BEV*                                           | L    |
|      | FEF <sub>25</sub> (MEF <sub>75</sub> )**       | L/s  |
|      | FEF <sub>50</sub> (MEF <sub>75</sub> )**       | L/s  |
|      | FEF <sub>75</sub> (MEF <sub>25</sub> )**       | L/s  |
|      | FEF <sub>25-75</sub> (MMEF <sub>25-75</sub> )* | L/s  |
|      | FEF <sub>50</sub> /FVC**                       | 1/s  |
|      | FET*                                           | s    |
|      | FEV <sub>.75</sub> **                          | L    |
|      | FEV <sub>1</sub> *                             | L    |
|      | FEV <sub>3</sub> **                            | L    |
|      | FEV <sub>6</sub> **                            | L    |
|      | FEV <sub>.75</sub> /FVC**                      | -    |
|      | FEV <sub>1</sub> /FVC*                         | -    |
|      | FEV <sub>3</sub> /FVC**                        | -    |
|      | FEV <sub>6</sub> /FVC**                        | -    |
|      | FEV <sub>.75</sub> /FEV <sub>6</sub> **        | -    |
|      | FEV <sub>1</sub> /FEV <sub>6</sub> **          | -    |

|     |                                                |     |
|-----|------------------------------------------------|-----|
|     | FVC*                                           | L   |
|     | PEF*                                           | L/s |
|     | MET <sub>25-75</sub> **                        | s   |
|     | MMEF/FVC**                                     | 1/s |
| FVL | BEV*                                           | L   |
|     | FEF <sub>25</sub> (MEF <sub>75</sub> )**       | L/s |
|     | FEF <sub>50</sub> (MEF <sub>50</sub> )**       | L/s |
|     | FEF <sub>75</sub> (MEF <sub>25</sub> )**       | L/s |
|     | FEF <sub>25-75</sub> (MMEF <sub>25-75</sub> )* | L/s |
|     | FEF <sub>50</sub> /FVC**                       | -   |
|     | FET*                                           | s   |
|     | FEV <sub>.75</sub> **                          | L   |
|     | FEV <sub>1</sub> *                             | L   |
|     | FEV <sub>3</sub> **                            | L   |
|     | FEV <sub>6</sub> **                            | L   |
|     | FEV <sub>.75</sub> /FVC**                      | -   |
|     | FEV <sub>1</sub> /FVC*                         | -   |
|     | FEV <sub>3</sub> /FVC**                        | -   |
|     | FEV <sub>6</sub> /FVC**                        | -   |
|     | FEV <sub>0.75</sub> /FEV <sub>6</sub> **       | -   |
|     | FEV <sub>1</sub> /FEV <sub>6</sub> **          | -   |
|     | FIF <sub>25-75</sub> **                        | L/s |
|     | FIVC*                                          | L   |
|     | FIV <sub>1</sub> **                            | L   |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 25 / 44    |

|            |                                                           |       |
|------------|-----------------------------------------------------------|-------|
|            | FIV <sub>1</sub> /FIVC (FIR)**                            | -     |
|            | FVC*                                                      | L     |
|            | MET <sub>25-75</sub> **                                   | s     |
|            | MMEF/FVC**                                                | -     |
|            | PEF*                                                      | L/s   |
|            | PIF*                                                      | L/s   |
|            | R <sub>50</sub> (FEF <sub>50</sub> /FIF <sub>50</sub> )** | -     |
| <b>SVC</b> | VC*                                                       | L     |
|            | VCin*                                                     | L     |
|            | VCex*                                                     | L     |
|            | ERV*                                                      | L     |
|            | IC**                                                      | L     |
|            | IRV*                                                      | L     |
|            | VT*                                                       | L     |
| <b>MVV</b> | MVV*                                                      | L/min |
|            | MVV6*                                                     | L/min |
|            | VT*                                                       | L     |
|            | RF*                                                       | 1/min |
|            | MVVtime*                                                  | s     |

\*Primary parameters are displayed as default on the results screen of the app after each spirometry session.

\*\* Secondary parameters are available in the 'See more parameters' section of the app after each spirometry session.

The definition of the parameters detected and displayed by the Spirohome® Personal is given below:

| Abbreviations                        | Definition                                                                                             |
|--------------------------------------|--------------------------------------------------------------------------------------------------------|
| BEV                                  | Back extrapolated volume                                                                               |
| ERV                                  | Expiratory reserve volume - maximal volume of air that can be exhaled from the end-expiratory position |
| FEF <sub>25</sub>                    | Forced expiratory flow at 25% of vital capacity                                                        |
| FEF <sub>25-75</sub>                 | Forced expiratory flow from 25% to 75% of vital capacity                                               |
| FEF <sub>50</sub>                    | Forced expiratory flow at 50% of vital capacity                                                        |
| FEF <sub>75</sub>                    | Forced expiratory flow at 75% of vital capacity                                                        |
| FEF <sub>50</sub> /FVC               | Ratio of FEF <sub>50</sub> to FVC                                                                      |
| FEF <sub>50</sub> /FIF <sub>50</sub> | Ratio of FEF <sub>50</sub> to FIF <sub>50</sub>                                                        |
| FEV <sub>.75</sub>                   | Forced expiratory volume after 0.75 seconds                                                            |
| FEV <sub>1</sub>                     | Forced expiratory volume after 1 second                                                                |
| FEV <sub>3</sub>                     | Forced expiratory volume after 3 seconds                                                               |
| FEV <sub>6</sub>                     | Forced expiratory volume after 6 seconds                                                               |
| FEV <sub>.75</sub> /FVC              | Ratio of FEV <sub>.75</sub> to FVC                                                                     |
| FEV <sub>1</sub> /FVC                | Ratio of FEV <sub>1</sub> to FVC                                                                       |
| FEV <sub>3</sub> /FVC                | Ratio of FEV <sub>3</sub> to FVC                                                                       |
| FEV <sub>6</sub> /FVC                | Ratio of FEV <sub>6</sub> to FVC                                                                       |
| FEV <sub>.75</sub> /FEV <sub>6</sub> | Ratio of FEV <sub>.75</sub> to FEV <sub>6</sub>                                                        |
| FEV <sub>1</sub> /FEV <sub>6</sub>   | Ratio of FEV <sub>1</sub> to FEV <sub>6</sub>                                                          |
| FET                                  | Forced expiratory time                                                                                 |
| FIF <sub>25</sub>                    | Forced inspiratory flow at 25% of vital capacity                                                       |
| FIF <sub>25-75</sub>                 | Forced inspiratory flow from 25% to 75% of vital capacity                                              |
| FIF <sub>75</sub>                    | Forced inspiratory flow at 75% of vital capacity                                                       |
| FIV <sub>1</sub>                     | Forced inspiratory volume after 1 second                                                               |

|                        |                                                                                                         |
|------------------------|---------------------------------------------------------------------------------------------------------|
| FIV <sub>1</sub> /FIVC | Ratio of FIV <sub>1</sub> to FIVC                                                                       |
| FIVC                   | Forced inspiratory vital capacity                                                                       |
| FVC                    | Forced vital capacity                                                                                   |
| IC                     | Inspiratory capacity - the sum of IRV and TV                                                            |
| IRV                    | Inspiratory reserve volume - maximal volume of air that can be inhaled from the end-expiratory position |
| MEF <sub>25</sub>      | Maximal instantaneous forced expiratory flow where 25 % of the FVC remains to be expired                |
| MEF <sub>50</sub>      | Maximal instantaneous forced expiratory flow where 50 % of the FVC remains to be expired                |
| MEF <sub>75</sub>      | Maximal instantaneous forced expiratory flow where 75 % of the FVC remains to be expired                |
| MET <sub>25-75</sub>   | Time between 25% and 75% of the forced expired volume                                                   |
| MIF <sub>25</sub>      | Maximal instantaneous forced inspiratory flow where 25 % of the FVC remains to be expired               |
| MIF <sub>75</sub>      | Maximal instantaneous forced expiratory flow where 75 % of the FVC remains to be expired                |
| MMEF <sub>25-75</sub>  | Mean mid-expiratory flow from 25% to 75% of vital capacity                                              |
| MMEF/FVC               | Ratio of mean mid-expiratory flow to forced vital capacity                                              |
| MVV                    | Maximum voluntary ventilation                                                                           |
| MVV6                   | Maximum voluntary ventilation after 6 seconds                                                           |
| MVVtime                | Time for MVV to be reached                                                                              |
| PEF                    | Peak expiratory flow                                                                                    |
| PIF                    | Peak inspiratory flow                                                                                   |
| R <sub>50</sub>        | Ratio of FEF <sub>50</sub> to FIF <sub>50</sub>                                                         |
| RF                     | Respiratory frequency                                                                                   |
| VC                     | Vital capacity                                                                                          |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 28 / 44    |

|      |                            |
|------|----------------------------|
| VCex | Expiratory vital capacity  |
| VCin | Inspiratory vital capacity |
| VT   | Tidal volume               |

The device also provides a reference value (obtained from large epidemiological studies) based on the patient's height, weight, age, sex and ethnicity. Your spirometry test results compared to the reference value and displayed as a percent predictive value indicator of your respiratory health. Your personal best value for a spirometry session can be discussed and with your healthcare provider for medical interpretation or diagnosis.

**Caution!:** Interpretation of spirometry results or diagnosis of medical conditions, if any, is to be made by a physician or allied health care professional with sufficient training in the performance and interpretation of spirometry.

If you wish for assistance in performing spirometry tests or understanding your test results, please contact your healthcare professional.

### 7.3 Types of breathing maneuvers


The breathing maneuvers involved in spirometry tests are physically-demanding for most patients. Please read the information below for the breathing maneuver you want to perform, and continue with testing only if you feel well enough to do so. Please cease testing if you feel dizzy or unwell.

#### ***The Forced Vital Capacity Test Breathing Maneuver:***

1. Ensure that your device is connected, the test screen is ready.
2. To ready yourself, place the mouthpiece in your mouth (past your teeth and with your lips sealed tightly around it), inhale and exhale normally a couple of times, and then take a slow and deep breath, **filling your lungs completely**. NOTE: You may choose to place the mouthpiece in your mouth after drawing in air and filling your lungs completely, making sure to place the mouthpiece past your teeth and sealing your lips around it before proceeding to the next step.
3. With your **lips sealed tightly around the mouthpiece**, empty your lungs by blow **as hard and fast as you can** into the mouthpiece **for at least 6 seconds** (follow animated

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 29 / 44    |

guide on app screen) without breaking the seal of your lips, and then **inhale a small amount of air to signal the end of your exhalation**. You may use a nose clip to help you exhale through only your mouth during this maneuver.



4. You may remove the mouthpiece from your mouth and resume normal breathing once the breathing maneuver has been completed.
5. Feedback about the test will be displayed on the app screen. You may need to repeat this breathing maneuver until you have acceptable test results. However, **ensure that you have rested between tests** and feel well enough to continue. For more information about test quality grading refer to the *Understanding test quality* section of this user manual.
6. Once all tests have been satisfactorily completed, you will be able to view your session results on the results page of the app.
7. To end the spirometry session, remove mouthpiece, turn off device, and store (you may use product pouch) according to storage requirements until next use. If the mouthpiece requires cleaning, please refer to section 8.2 Cleaning the Spiroway® reusable mouthpiece.

### ***The Flow Volume Loop Test Breathing Maneuver:***

1. Ensure that your device is connected, the test screen is ready.
2. You must enter the environmental temperature as prompted by the app. **The temperature entered must be within 1°C or 1.8°F accuracy.**
3. After confirming the temperature you have entered, you are ready to perform the breathing maneuver.
4. To ready yourself, place the mouthpiece in your mouth (past your teeth and with

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 30 / 44    |

your lips sealed tightly around it), inhale and exhale normally a couple of times, and then take a slow and deep breath, **filling your lungs completely**. NOTE: You may choose to place the mouthpiece in your mouth after drawing in air and filling your lungs completely, making sure to place the mouthpiece past your teeth and sealing your lips around it before proceeding to the next step.

5. With your **lips sealed tightly around the mouthpiece**, empty your lungs by blow **as hard and fast as you can** into the mouthpiece **for at least 6 seconds** (follow animated guide on app screen) without breaking the seal of your lips, and then **inhale a small amount of air to signal the end of your exhalation**. You may use a nose clip to help you exhale through only your mouth during this maneuver.
6. **Without breaking the seal of your lips, now inhale completely filling your lungs.**
7. You may remove the mouthpiece from your mouth and resume normal breathing once the breathing maneuver has been completed.
8. Feedback about the test will be displayed on the app screen. You may need to repeat this breathing maneuver until you have acceptable test results. However, **ensure that you have rested between tests** and feel well enough to continue. For more information about test quality grading refer to the *Understanding test quality* section of this user manual.
9. Once all tests have been satisfactorily completed, you will be able to view your session results on the results page of the app.
10. To end the spirometry session, remove mouthpiece, turn off device, and store (you may use product pouch) according to storage requirements until next use. If the mouthpiece requires cleaning, please refer to section 8.2 Cleaning the Spiroway® reusable mouthpiece.

### ***The Maximum Voluntary Ventilation Test Breathing Maneuver:***

1. Ensure that your device is connected, the test screen is ready.
2. You must enter the environmental temperature as prompted by the app. **The**

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 31 / 44    |

**temperature entered must be within 1°C or 1.8°F accuracy.**

3. After confirming the temperature you have entered, you are ready to perform the breathing maneuver.
4. Place the mouthpiece in your mouth past your teeth and ensure your **lips are tightly sealed around the mouthpiece**.
5. **Inhale and exhale completely filling and emptying your lungs, repeatedly, uninterrupted, without breaking the seal of your lips for at least 12 seconds** (follow animated guide on app screen).
6. You may remove the mouthpiece from your mouth and resume normal breathing once the breathing maneuver has been completed.
7. Feedback about the test will be displayed on the app screen.
8. Once the test has been satisfactorily completed, you will be able to view your session results on the results page of the app.
9. To end the spirometry session, remove mouthpiece, turn off device, and store (you may use product pouch) according to storage requirements until next use. If the mouthpiece requires cleaning, please refer to section 8.2 Cleaning the Spiroway® reusable mouthpiece.

### ***The Slow Vital Capacity Test Breathing Maneuver:***

1. Ensure that your device is connected, the test screen is ready.
2. You must enter the environmental temperature as prompted by the app. **The temperature entered must be within 1°C or 1.8°F accuracy.**
3. After confirming the temperature you have entered, you are ready to perform the breathing maneuver.
4. Place the mouthpiece in your mouth past your teeth, and your **lips are tightly sealed around the mouthpiece** and **inhale and exhale normally**, for 3-5 breaths.
5. When prompted by the app, **fully inhale and then fully exhale**.
10. You may remove the mouthpiece from your mouth and resume normal breathing once the breathing maneuver has been completed.
11. Feedback about the test will be displayed on the app screen. You may need to repeat

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 32 / 44    |

this breathing maneuver until you have acceptable test results. However, **ensure that you have rested between tests** and feel well enough to continue. For more information about test quality grading refer to the *Understanding test quality* section of this user manual.

12. Once all tests have been satisfactorily completed, you will be able to view your session results on the results page of the app.
13. To end the spirometry session, remove mouthpiece, turn off device, and store (you may use product pouch) according to storage requirements until next use. If the mouthpiece requires cleaning, please refer to section 8.2 Cleaning the Spiroway® reusable mouthpiece.

#### 7.4 Understanding test quality

After each test session, a quality grading will be displayed on the app to inform you about how well the breathing maneuver was performed, and if the results are acceptable or not.

Grading of the FVC and FVL tests in children and adults, according to the American Thoracic Society guidelines.

| Grade | Criteria                                                                                                                          |
|-------|-----------------------------------------------------------------------------------------------------------------------------------|
| A     | ≥ 3 acceptable tests with repeatability within 0.150 L<br>For age 2-6, 0.100 L, or 10% of the highest value, whichever is greater |
| B     | ≥ 2 acceptable tests with repeatability within 0.150 L<br>For age 2-6, 0.100 L, or 10% of the highest value, whichever is greater |
| C     | ≥ 2 acceptable tests with repeatability within 0.200 L<br>For age 2-6, 0.150 L, or 10% of the highest value, whichever is greater |
| D     | ≥ 2 acceptable tests with repeatability within 0.250 L<br>For age 2-6, 0.200 L, or 10% of the highest value, whichever is greater |
| E     | One acceptable test                                                                                                               |
| F     | No acceptable tests                                                                                                               |

Grading of the SVC test.

| Grade | Criteria |
|-------|----------|
|-------|----------|

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 33 / 44    |

|   |                                                                                                             |
|---|-------------------------------------------------------------------------------------------------------------|
| A | At least 3 acceptable trials AND the difference between the best VC values is equal to or less than 150 mL. |
| B | At least 2 acceptable trials AND the difference between the best VC values is equal to or less than 150 mL. |
| C | At least 2 acceptable trials but the results are not reproducible according to 'B'.                         |
| D | One acceptable test.                                                                                        |
| F | No acceptable test.                                                                                         |

## 8. Maintenance of your Spirohome® Personal

### 8.1 Calibration-check

Due to the ultrasound-based technology for air flow analysis, routine calibration of your Spirohome® Personal is not necessary. However, it is advised by the American Thoracic Society (ATS) that periodic calibration-checks of spirometers are performed. To check the calibration of your Spirohome® Personal, you may compare the results from your device with spirometry test results you obtain from a clinic or spirometry laboratory.

If you believe that there is a problem with the calibration of the device, contact the manufacturer immediately and do not perform tests with the device.

### 8.2 Cleaning and disinfection of the device

Proper cleaning and disinfection of your Spirohome® Personal is important for safety and hygiene purposes. With regular cleaning, you can prevent the physical buildup of contaminants on your device. A cleaning process must always precede a disinfection process. Disinfection destroys any pathogens such as bacteria, viruses or other microorganisms that might still be present on device surfaces after an initial cleaning process. Regular, thorough cleaning and disinfection of your device protects both you and others from the potential transmission of

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 34 / 44    |

infections resulting from contact with the device. Be sure to wash your hands with soap before and after each use of the device.

The cleaning procedure and disinfection process is described below:


**1. Before beginning the procedure wash hands thoroughly with soap and water.**



**2. Cleaning the Spirohome® Personal**

Remove the Spiroway® reusable mouthpiece from the Spirohome® Personal body if it is inserted. Use a high-level disinfectant (chlorine-based) and wipe for 30 seconds all accessible surfaces of both the device and device cap to remove all visible contaminants as shown below.

**Please be extra careful and gentle when cleaning the sensors to avoid any damage to them.** Perform cleaning at least once a week or whenever the device is visibly contaminated.

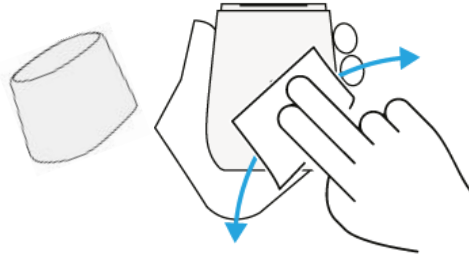

Wipe all accessible surfaces of the device and cap, using moderate pressure, as shown.


**Caution!:** Care must be taken to prevent any excess liquids contained within the wipes from entering the components of the Spirohome® Personal. Never immerse the product in water or any other liquid solution.

**3. Disinfecting the Spirohome® Personal**

After cleaning accessible surfaces of the device with a high-level disinfectant (chlorine-based) wipe, use a second fresh wipe to wipe over all surfaces again with moderate pressure and contact time as recommended by the wipe manufacturer. You should disinfect the Spirohome®

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 35 / 44    |

Personal once a week, always performing the cleaning procedure before the disinfection procedure.

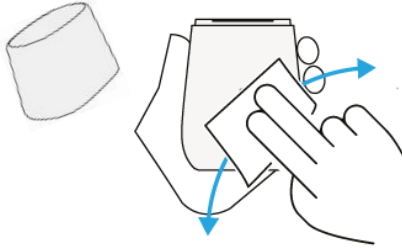

*CaviWipes1™ Disinfectant wipes (Metrex Research LLC) is a high-level disinfectant wipes for this purpose and available at*

<https://www.metrex.com/en-us/products/surface-disinfectants/caviwipes>.

**4. Wash hands thoroughly after performing a cleaning procedure, and before handling the cleaned components again for packing and storage.**



|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 36 / 44    |

## 8.2 Cleaning the Spiroway® reusable mouthpiece

The Spiroway® reusable mouthpiece should be cleaned weekly or whenever it is visibly contaminated. Clean the Spiroway® reusable mouthpiece by gently agitating it in water containing dishwashing liquid, rinsing under clean water, and leaving upright on a lint-free cloth to air-dry completely.

Do not insert the Spiroway® reusable mouthpiece to Spirohome® Personal device until it is completely dry.

Replace the Spiroway® reusable mouthpiece:

- every 3 months
- if the user used the mouthpiece whilst having a bacterial or viral infection
- if the filters are damaged
- whenever a risk of cross-contamination is suspected (such as possible use of the mouthpiece by other users)

### Caution!: Risk of Cross-Contamination

Spirohome® Personal is designed to be used with the Spiroway® reusable mouthpiece. The mouthpiece is indicated for *single-patient-use* only. The mouthpiece must not be used by more than one user to prevent the risk of cross-contamination. Thorough cleaning and disinfection of the device must be performed prior to use by a new user. *A new mouthpiece should be used for each user.*

New mouthpieces can be purchased at [www.spirohome.io](http://www.spirohome.io). See the Orderable Accessories section of this user manual for more information.


## 8.4 Replacing batteries

The Spirohome® Personal should be powered by a standard 1.5V AAA battery. The battery life such batteries will be approximately 6-9 months, assuming daily use of the device. The battery charge level is continuously monitored by the device. When battery charge level is low, the device will not turn on and a 'beeping' sound will notify the user. The batteries of the device should be removed if the device is not going to be used for more than a month.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 37 / 44    |

### ***Instructions for battery replacement***

1. Remove the Spiroway® reusable mouthpiece from the device.

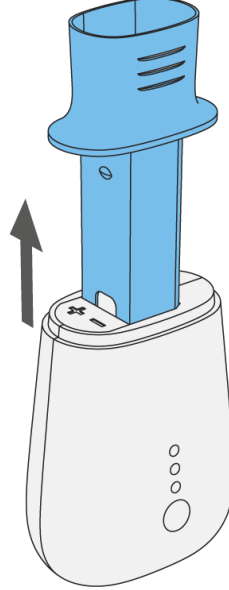

2. Remove the battery cover by sliding it as shown.



3. Remove the dead batteries.



|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 38 / 44    |

4. Place the new batteries in the correct orientation.




5. Slide the battery cover back to the closed position.



6. Insert the Spiroway® reusable mouthpiece in the right orientation. Your device is now ready to use.

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 39 / 44    |

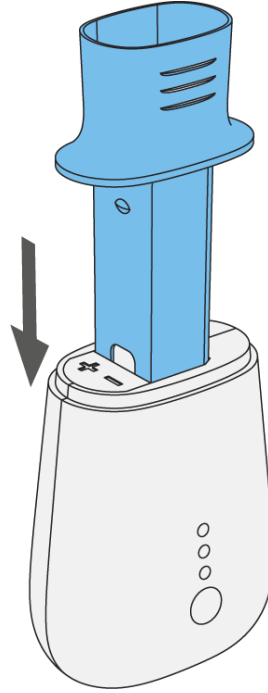

## 9. Terms of warranty

### 9.1 Terms of warranty for the Spirohome® Personal

Spirohome® Personal, together with any accessories provided, is guaranteed for a period of 24 months, effective from the date of purchase, upon the provision of an invoice or sales receipt. The service life of the product is 5 years, effective from the date of purchase.

The user is responsible for checking the product for damage or missing components at the time of purchase or delivery, and claims must be made in writing to the manufacturer.

The customer must return goods for replacement or repair at the customer's expense to the authorized supplier or manufacturer.

Please provide with the returned product a clear written explanation of the fault or problem.

This warranty does not apply, at the discretion of the manufacturer, in the following cases:

- Improper installation or operation of the device
- Use of the product for purposes other than those specified in this user manual
- Damage due to failure to follow instructions
- Damage due to unauthorized repair, modification or reconfiguration performed on the device
- Damage caused by lack of proper care or maintenance
- Damage caused by abnormal physical or electrical stress or defects of the mains electricity supply or of equipment to which the product was connected to

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 40 / 44    |

- If the serial number is altered, deleted, removed or rendered illegible

## 9. Appendix

### 9.1 Electromagnetic Compatibility

Meeting the requirements for EMC (electromagnetic compatibility) and preventing the unsafe use of the device, medical devices including Spirohome® manufactured by Inofab Health Technologies conform to the EN60601-1-2 standard which defines the levels of immunity to electromagnetic interference as well as maximum levels of electromagnetic emissions for medical devices. For details, please see the following tables:

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 41 / 44    |

**Table 1: Emission table for IEC 60601-1-2**

| Guidance and manufacturer's declaration – electromagnetic emissions                                                                                                                                |                |                                                                                                                                                                                                                                      |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Spirohome® battery-operated spirometer devices are intended for use in the electromagnetic environment specified below. Users of these devices should assure that it is used in such environments. |                |                                                                                                                                                                                                                                      |
| Emission Test                                                                                                                                                                                      | Compliance     | Electromagnetic environment - guidance                                                                                                                                                                                               |
| RF emissions CISPR 11                                                                                                                                                                              | Group 1        | The Spirohome® battery-operated devices use RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.                          |
| RF emissions CISPR 11                                                                                                                                                                              | Class B        | The Spirohome® devices are suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. |
| Harmonic emissions IEC 61000-3-2                                                                                                                                                                   | Not applicable |                                                                                                                                                                                                                                      |
| Voltage fluctuations / flicker emissions IEC 61000-3-3                                                                                                                                             | Not applicable |                                                                                                                                                                                                                                      |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 42 / 44    |

**Table 2: Immunity (Stimulation mode) table according to IEC 60601-1-2**

| Guidance and manufacturer's declaration – electromagnetic immunity                                                                                                                                |                                            |                                                                    |                                                                                                                                                     |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------|--------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------|
| Spirohome® battery-operated spirometer devices are intended for use in the electromagnetic environment specified below. Users of these devices should assure that it is used in such environment. |                                            |                                                                    |                                                                                                                                                     |
| Immunity Test Standard                                                                                                                                                                            | IEC 60601 test level                       | Compliance level                                                   | Recommended separation distance                                                                                                                     |
| Electrostatic discharge (ESD) IEC 61000-4-2                                                                                                                                                       | ±2 kV<br>±4 kV<br>±6 kV<br>±8 kV<br>±15 kV | ±8 kV contact<br>±2 kV air<br>±4 kV air<br>±8 kV air<br>±15 kV air | Floor should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.      |
| Electrostatic fast transient / burst IEC 61000-4-4                                                                                                                                                | N/A                                        | NA                                                                 |                                                                                                                                                     |
| Surge IEC 61000-4-5                                                                                                                                                                               | NA                                         | NA                                                                 |                                                                                                                                                     |
| Voltage dips, short interruptions and voltage variations on power supply lines IEC 61000-4-11                                                                                                     | NA                                         | NA                                                                 |                                                                                                                                                     |
| Power frequency (50/60 Hz) magnetic field IEC 61000-4-8                                                                                                                                           | 30 A/m                                     | 30 A/m                                                             | Power frequency magnetic fields should be at levels characteristic of a typical location in a typical domestic, commercial or hospital environment. |

### Guidance and manufacturer's declaration – electromagnetic immunity

Spirohome® battery-operated spirometer devices are intended for use in the electromagnetic environment specified below. Users of these devices should assure that it is used in such environment.

| Immunity test standard                                                     | IEC 60601 test level                     | Compliance level | Recommended separation distance                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
|----------------------------------------------------------------------------|------------------------------------------|------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>Conducted RF<br/>IEC 61000-4-6</p> <p>Radiated RF<br/>IEC 61000-4-3</p> | <p>NA</p> <p>3 V/m 80 MHz to 2.7 GHz</p> | <p>3 V/m</p>     | <p>Portable and mobile RF communications equipment should be used no closer to any part of the Spirohome® devices including cables, than the recommended separation distance calculated from the equation appropriate to the frequency of the transmitter.</p> <p>Recommend separation distance<br/> <math>d = 1.2 \sqrt{P}</math><br/> <math>d = 1.2 \sqrt{P}</math> 80 MHz to 800 MHz<br/> <math>d = 2.3 \sqrt{P}</math> 800 MHz to 2.5 GHz</p> <p>where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters as determined by an electromagnetic site survey,<sup>a</sup> should be less than the compliance level in each frequency range.<sup>b</sup></p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p>  |

|                                                                                  |                                      |                  |            |
|----------------------------------------------------------------------------------|--------------------------------------|------------------|------------|
|  | SPIROHOME® FDA DOSSIER               | Document No      | SUS-FDAD   |
|                                                                                  |                                      | Publication Date | 24.02.2019 |
|                                                                                  | USER MANUAL - PERSONAL<br>SPIROHOME® | Revision Number  | 00         |
|                                                                                  |                                      | Revision Date    | --         |
|                                                                                  |                                      | Page             | 44 / 44    |

Note1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

<sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/ cordless) telephones and land mobile radio, AM and FM radio broadcast, and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Spirohome® devices are used exceeds the applicable RF compliance level above, the Spirohome® device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the Spirohome® device.

<sup>b</sup> Over the frequency range 150 kHz to 80MHz, field strengths should be less than 3 V/m.

#### Recommended separation distances between portable and mobile RF communications equipment.

Spirohome® devices are intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customers or the users of these Spirohome® devices can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Spirohome® device as recommended below, according to the maximum output power of the communications equipment.

| Rated maximum<br>output power of<br>transmitter<br><br>W | Separation distance according to frequency of transmitter<br>m |                     |                    |
|----------------------------------------------------------|----------------------------------------------------------------|---------------------|--------------------|
|                                                          | 150 kHz - 80 MHz                                               | 80 MHz - 800 MHz    | 800 MHz - 2500 MHz |
|                                                          | $d = 0.35 \sqrt{P}$                                            | $d = 0.35 \sqrt{P}$ | $d = 0.7 \sqrt{P}$ |
| 0.01                                                     | 0.12                                                           | 0.12                | 0.23               |
| 0.1                                                      | 0.38                                                           | 0.38                | 0.73               |
| 1                                                        | 1.2                                                            | 1.2                 | 2.3                |
| 10                                                       | 3.8                                                            | 3.8                 | 7.3                |
| 100                                                      | 12                                                             | 12                  | 23                 |

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note: At 80MHz and 800MHz, the separation distance for the higher frequency range applies

Note: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.