

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260102 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.884$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.75, 9.37, 9.43); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227_Edge; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.41 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.04 dB

SAR (1g) = 2.11 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

TSL Correction: Positive only

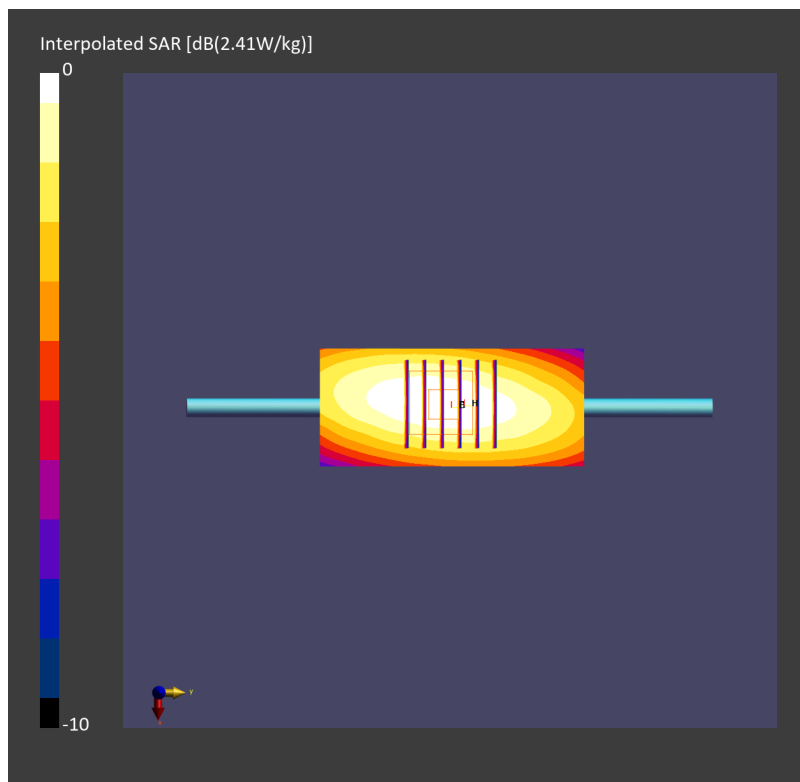

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260107 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.881$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.22 W/kg; SAR (10g) = 1.47 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.46 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.7 %

TSL Correction: Positive only

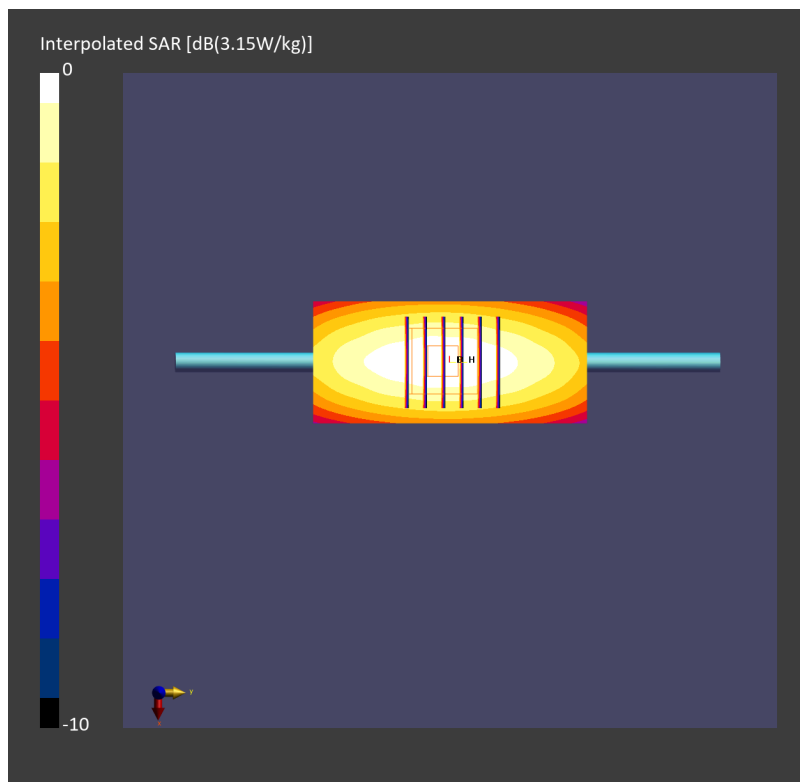

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260122 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.867$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.53 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.30 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

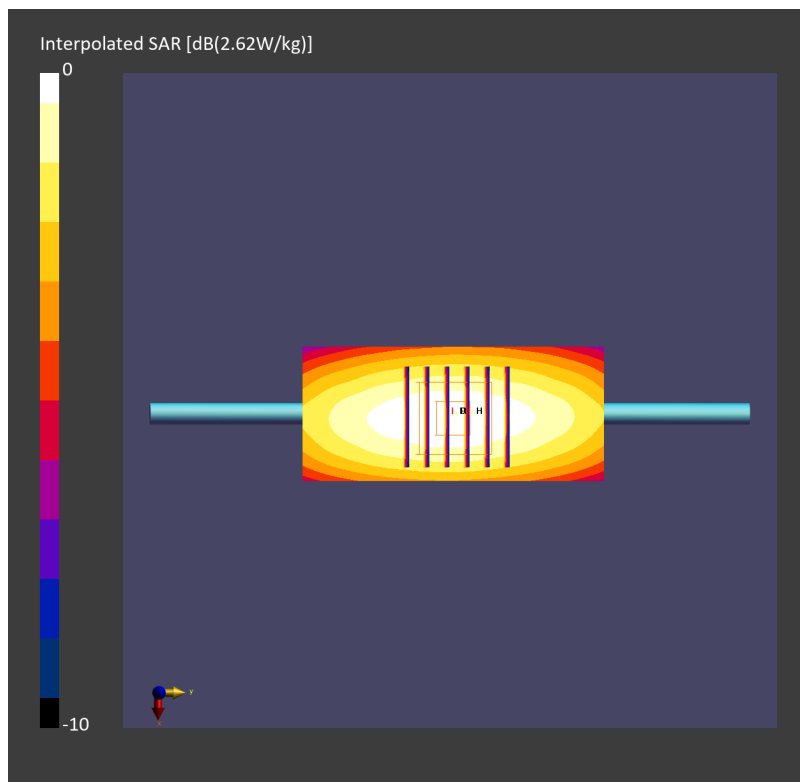

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260103 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(10.0, 9.61, 9.66); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227_Edge; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.20 W/kg; SAR (10g) = 1.44 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.20 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.45 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

TSL Correction: Positive only

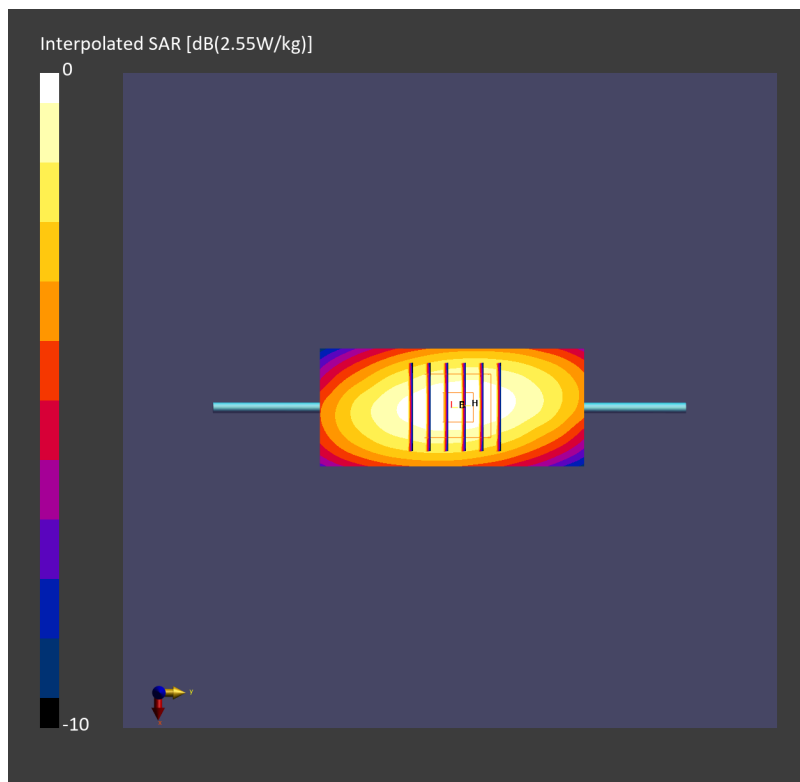

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260107 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.910$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.38 W/kg; SAR (10g) = 1.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.33 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 16.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

TSL Correction: Positive only

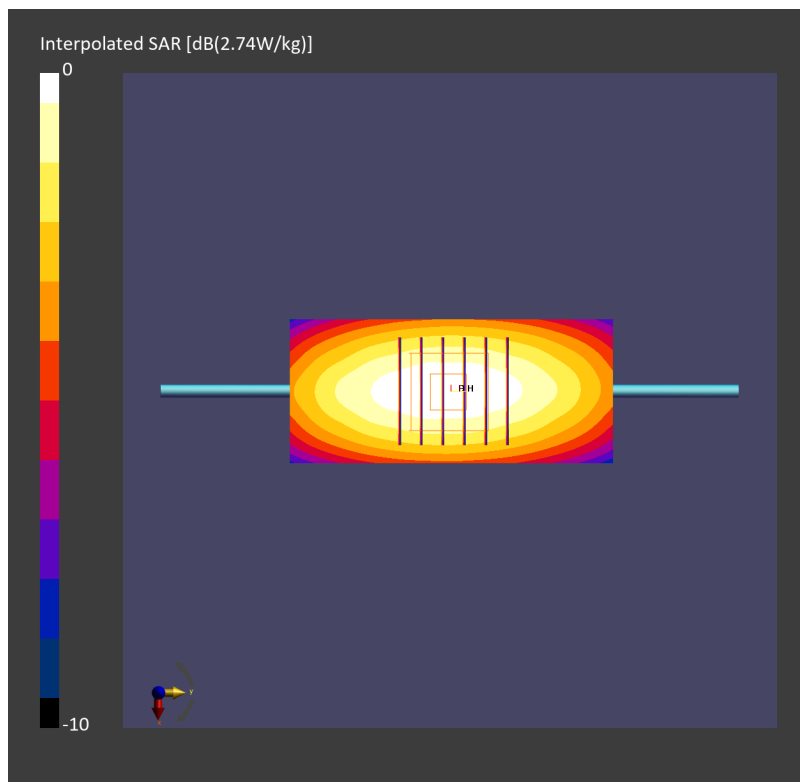

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260122 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.895$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.67 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.75 W/kg; SAR (10g) = 1.66 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

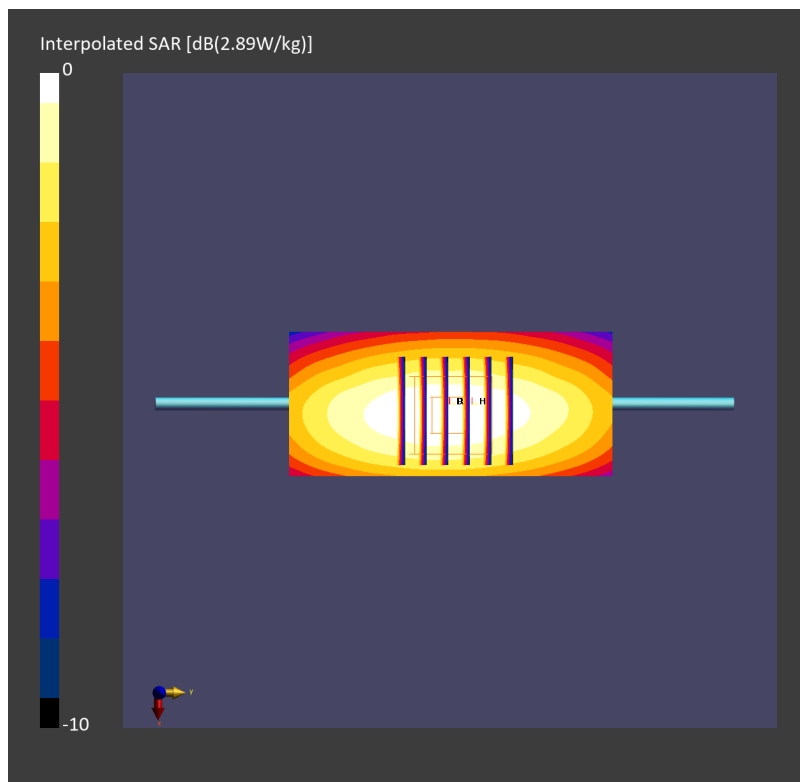

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260108 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.75 W/kg; SAR (10g) = 4.66 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 8.54 W/kg; SAR (8g) = 4.88 W/kg; SAR (10g) = 4.49 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

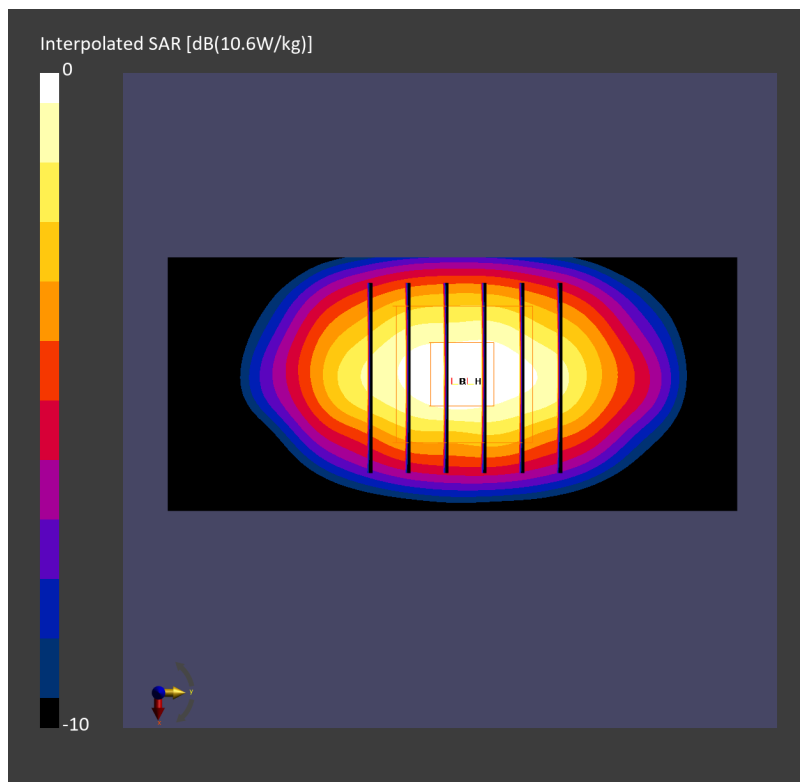

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260115 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.08, 7.96, 7.11); Calibrated: 2025-02-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.83 W/kg; SAR (10g) = 0.965 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.946 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

TSL Correction: Positive only

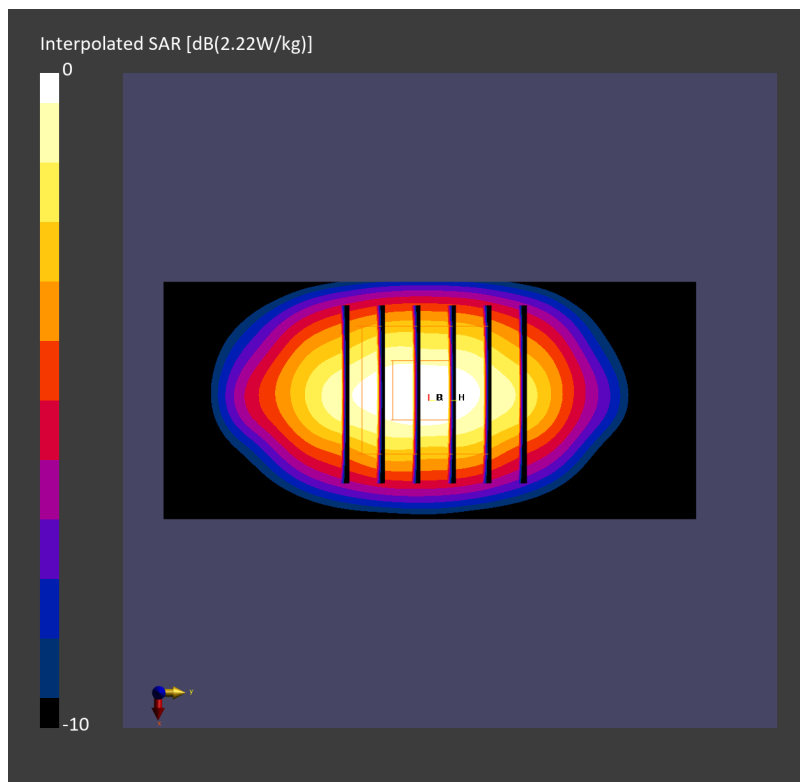

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260123 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.29$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.947 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.952 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

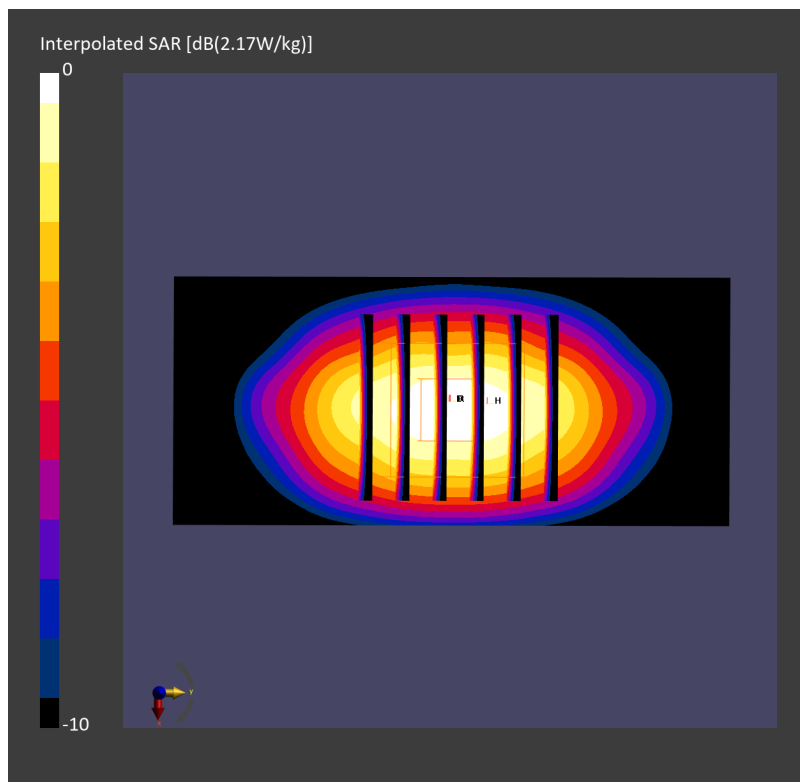

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260108 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.81 W/kg; SAR (10g) = 5.07 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 9.46 W/kg; SAR (8g) = 5.34 W/kg; SAR (10g) = 4.91 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

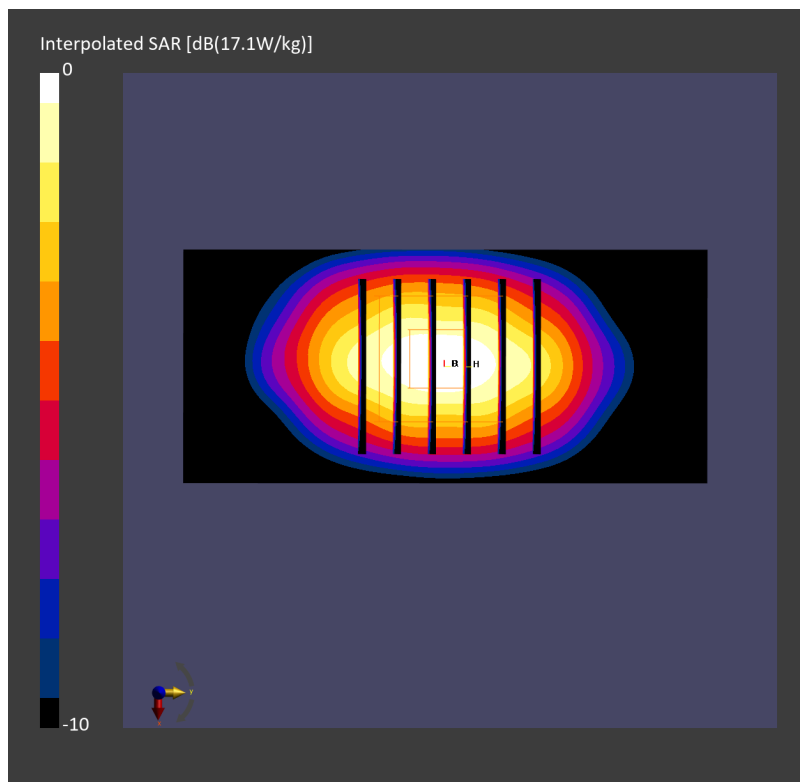

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260115 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.87, 7.73, 6.91); Calibrated: 2025-02-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.997 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.971 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

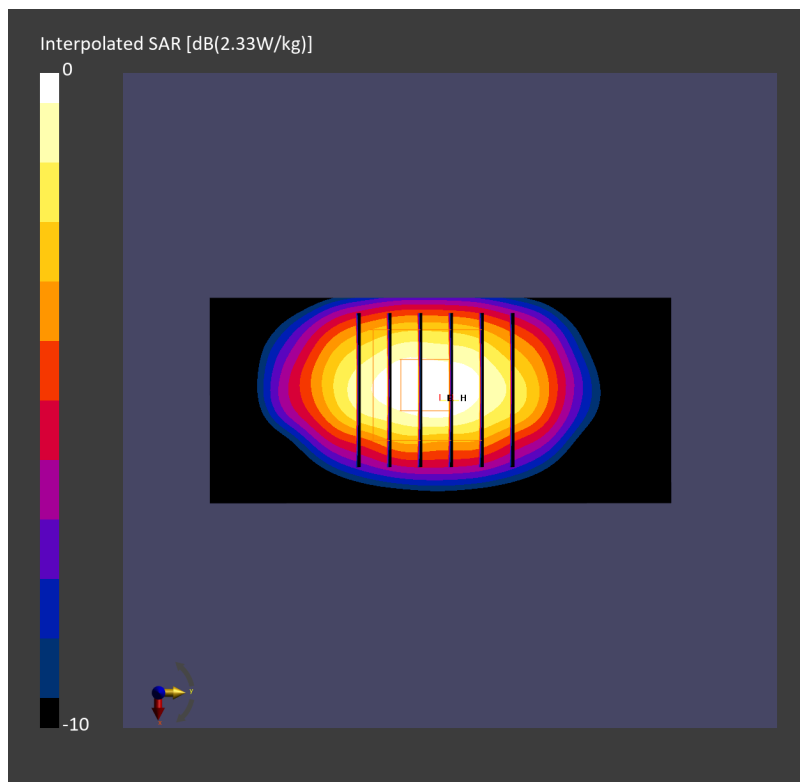

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260123 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 0.943 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.947 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

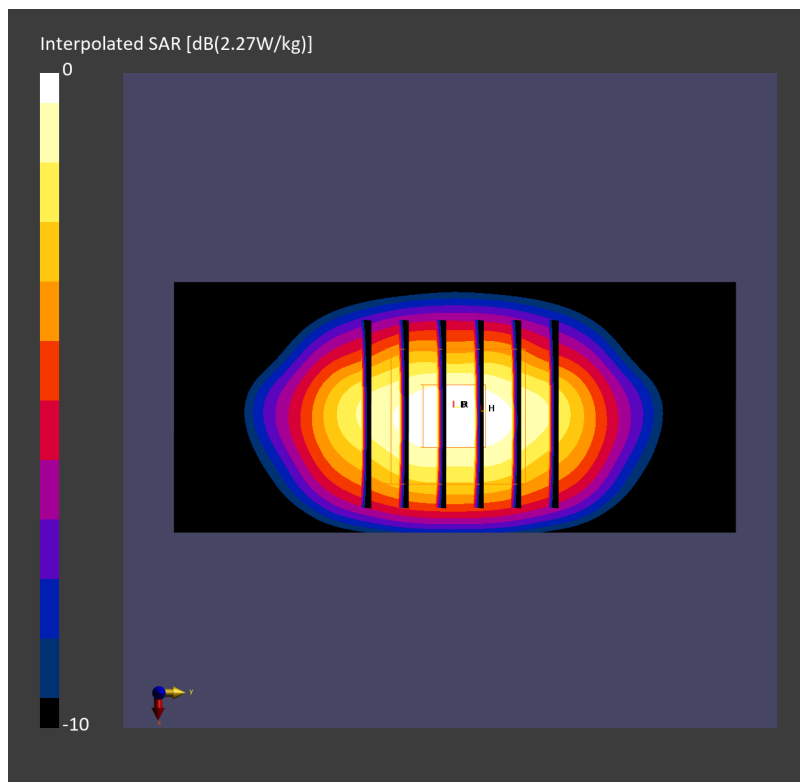

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260104 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.66, 7.36, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.1 W/kg; SAR (10g) = 5.77 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 11.9 W/kg; SAR (8g) = 6.20 W/kg; SAR (10g) = 5.63 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

TSL Correction: Positive only

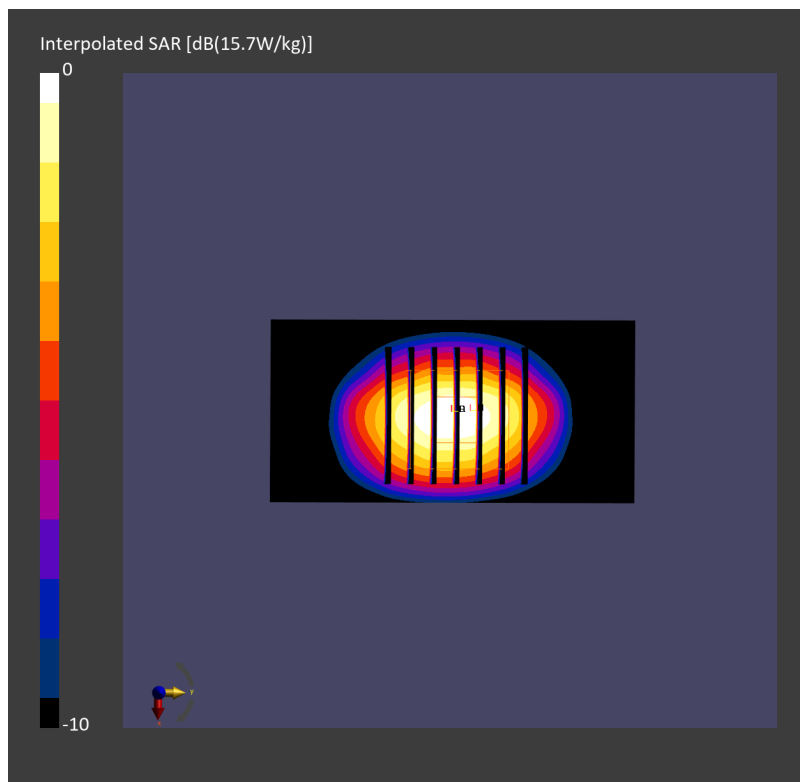

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260109 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.70$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 11.9 W/kg; SAR (10g) = 5.63 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 11.6 W/kg; SAR (8g) = 6.03 W/kg; SAR (10g) = 5.47 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.5 %

TSL Correction: Positive only

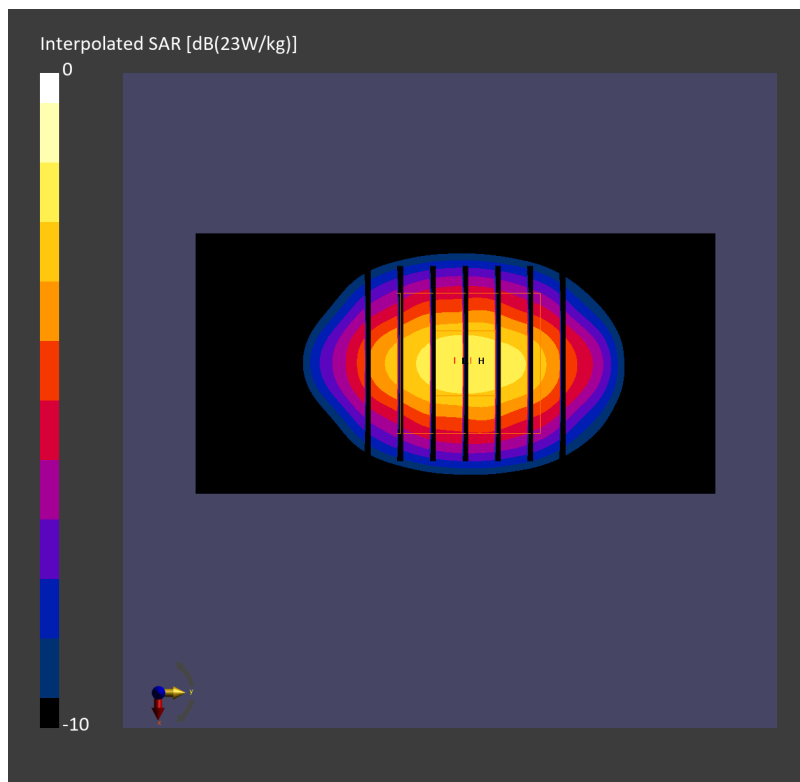

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260124 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.62$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.69 W/kg; SAR (10g) = 2.20 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 4.63 W/kg; SAR (8g) = 2.44 W/kg; SAR (10g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

TSL Correction: Positive only

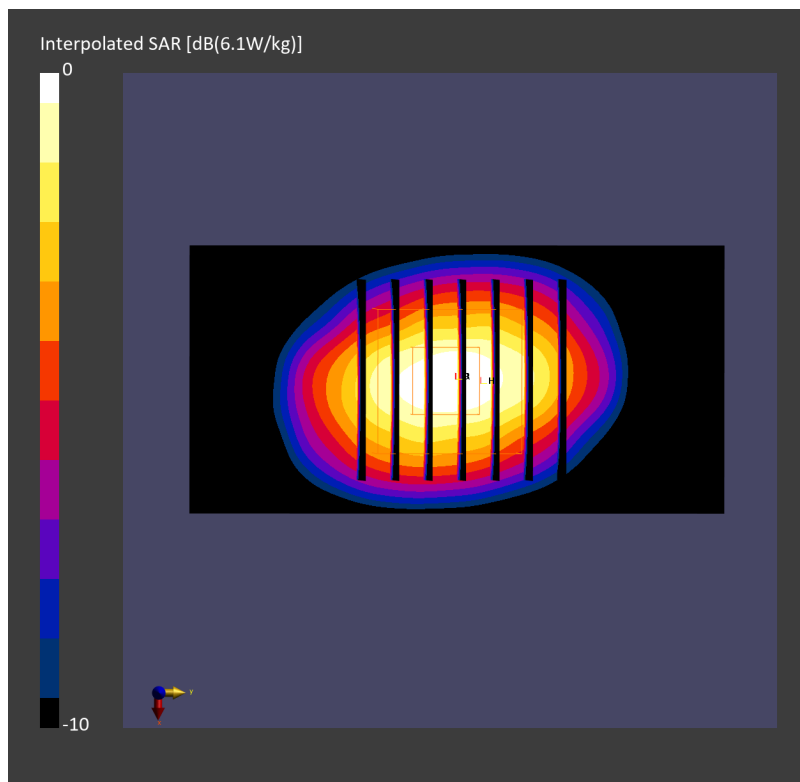

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260105 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.65, 7.35, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.5 W/kg; SAR (10g) = 5.95 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 13.0 W/kg; SAR (8g) = 6.44 W/kg; SAR (10g) = 5.81 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

TSL Correction: Positive only

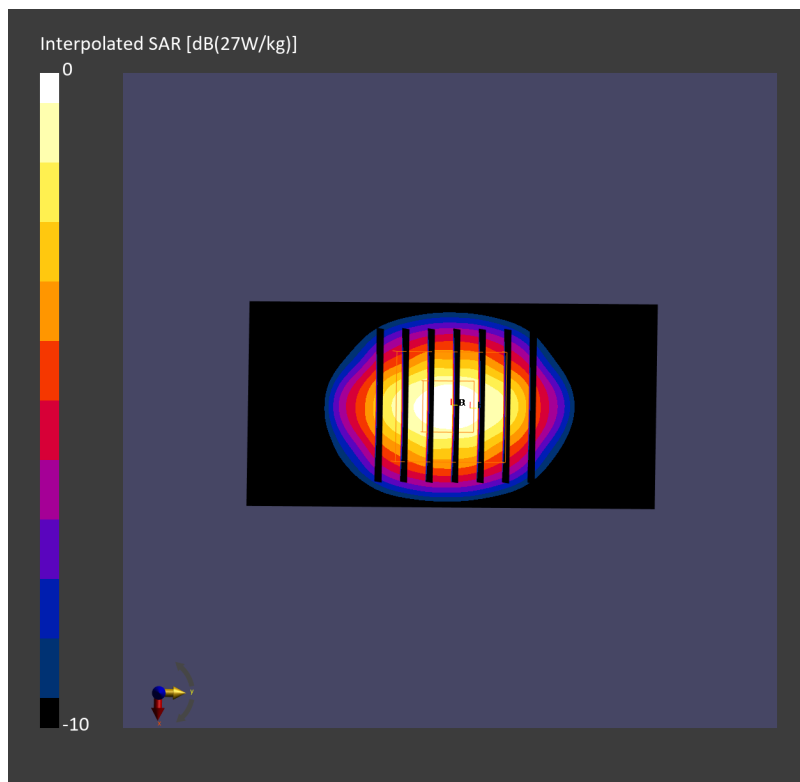

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260109 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.6 W/kg; SAR (10g) = 6.04 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 13.2 W/kg; SAR (8g) = 6.52 W/kg; SAR (10g) = 5.87 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.1 %

TSL Correction: Positive only

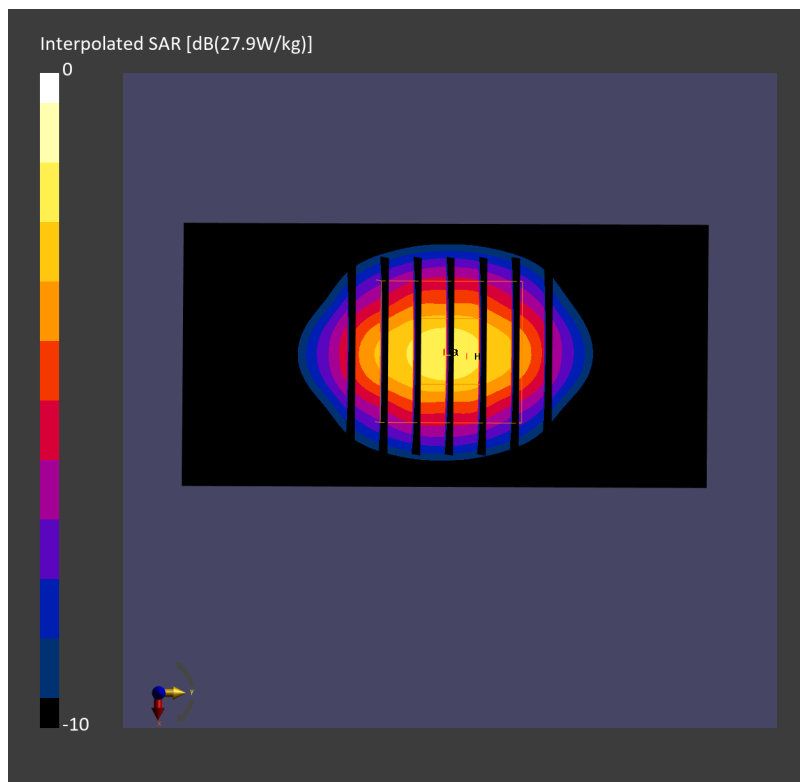

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260124 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.43 W/kg; SAR (10g) = 2.42 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 5.46 W/kg; SAR (8g) = 2.69 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.9 %

TSL Correction: Positive only

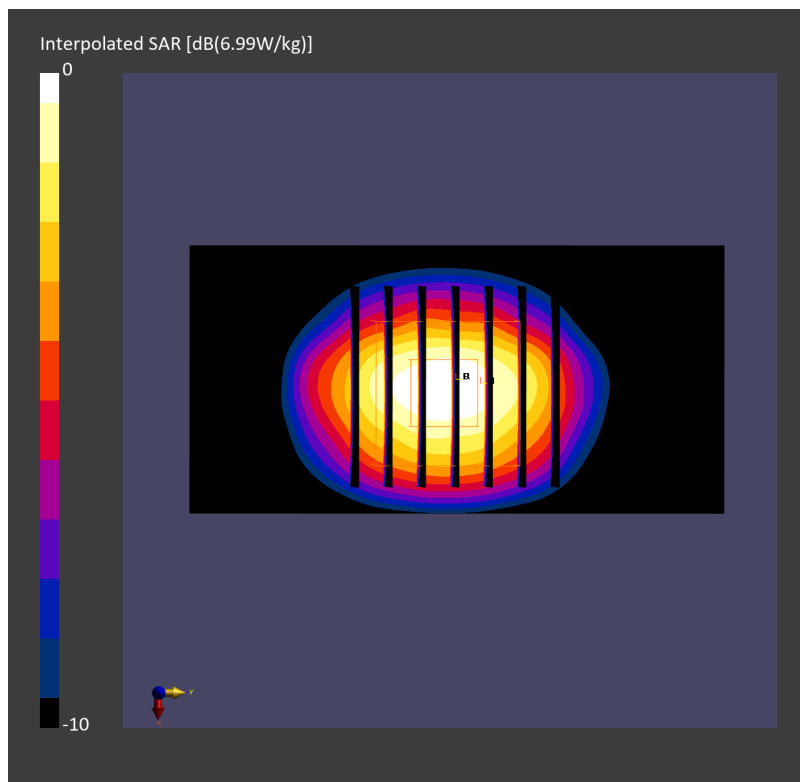

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260110 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.52 W/kg; SAR (10g) = 2.45 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.06 dB

SAR (1g) = 6.42 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.41 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

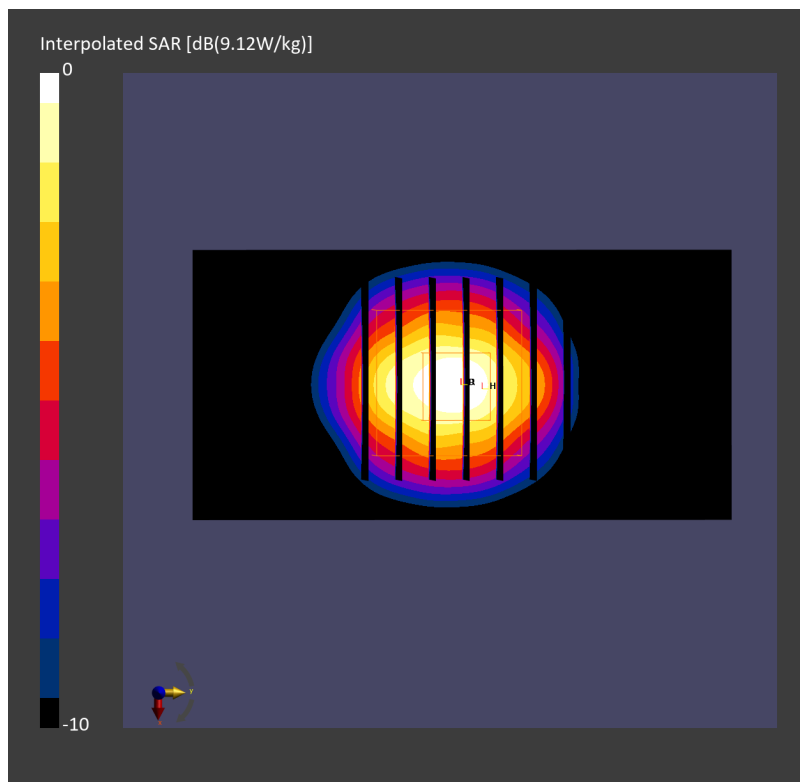

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260118 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.70$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.62 W/kg; SAR (10g) = 2.49 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.45 W/kg; SAR (8g) = 2.74 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

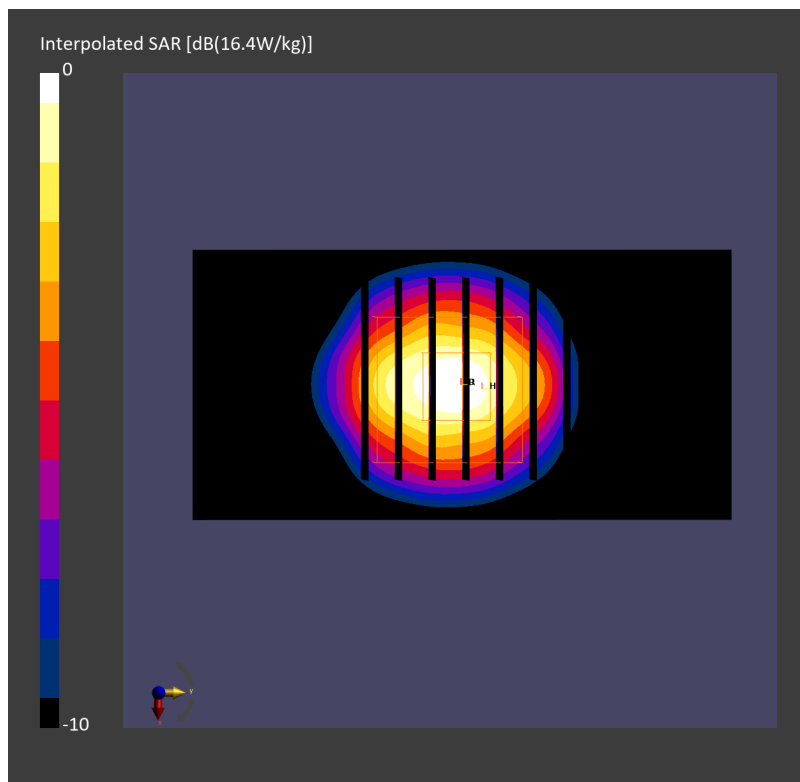

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260125 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.67$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.46 W/kg; SAR (10g) = 2.43 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.49 W/kg; SAR (8g) = 2.78 W/kg; SAR (10g) = 2.46 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.7 %

TSL Correction: Positive only

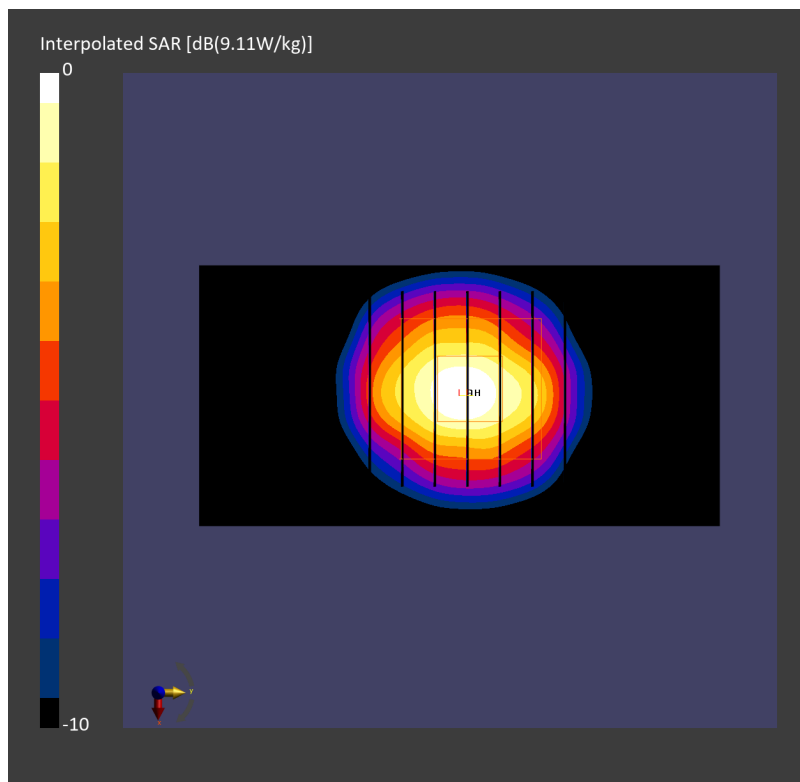

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260110 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.47 W/kg; SAR (10g) = 2.35 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 6.46 W/kg; SAR (8g) = 2.65 W/kg; SAR (10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

TSL Correction: Positive only

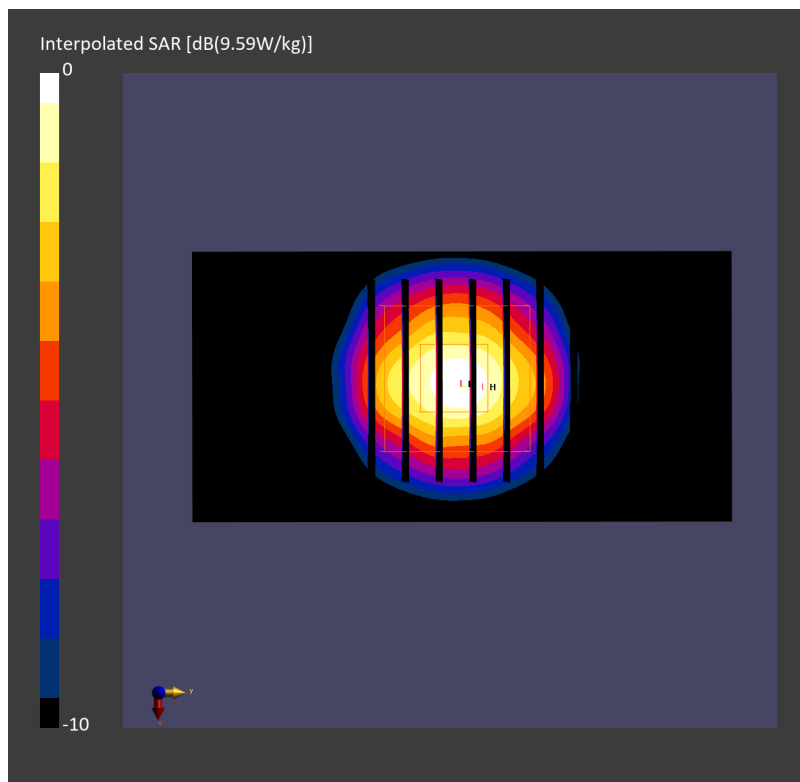

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260119 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.51 W/kg; SAR (10g) = 2.37 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 6.47 W/kg; SAR (8g) = 2.66 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

TSL Correction: Positive only

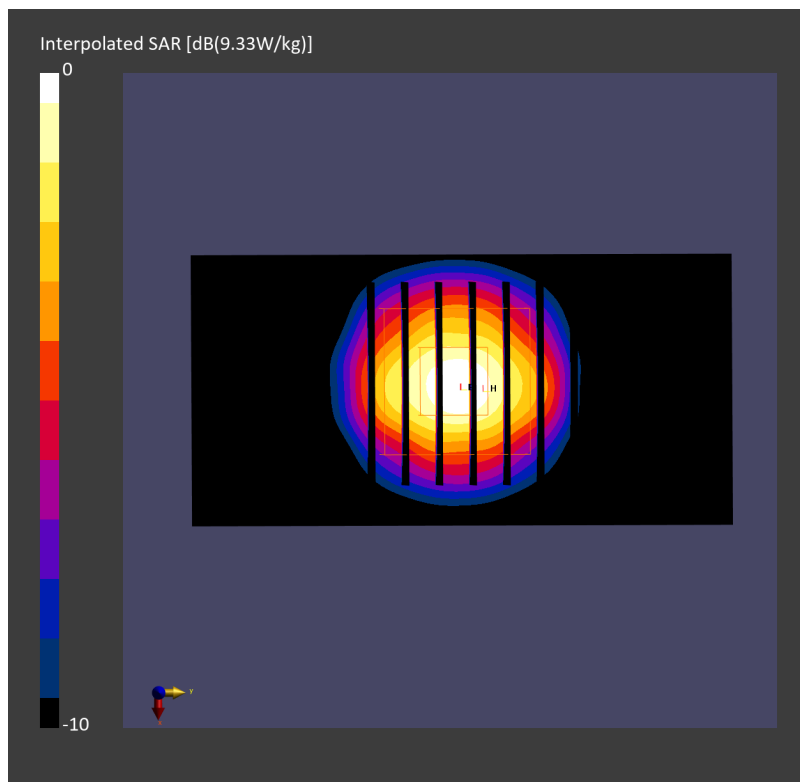

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260125 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.85$ S/m; $\epsilon_r = 36.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.41 W/kg; SAR (10g) = 2.39 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.61 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.41 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

TSL Correction: Positive only

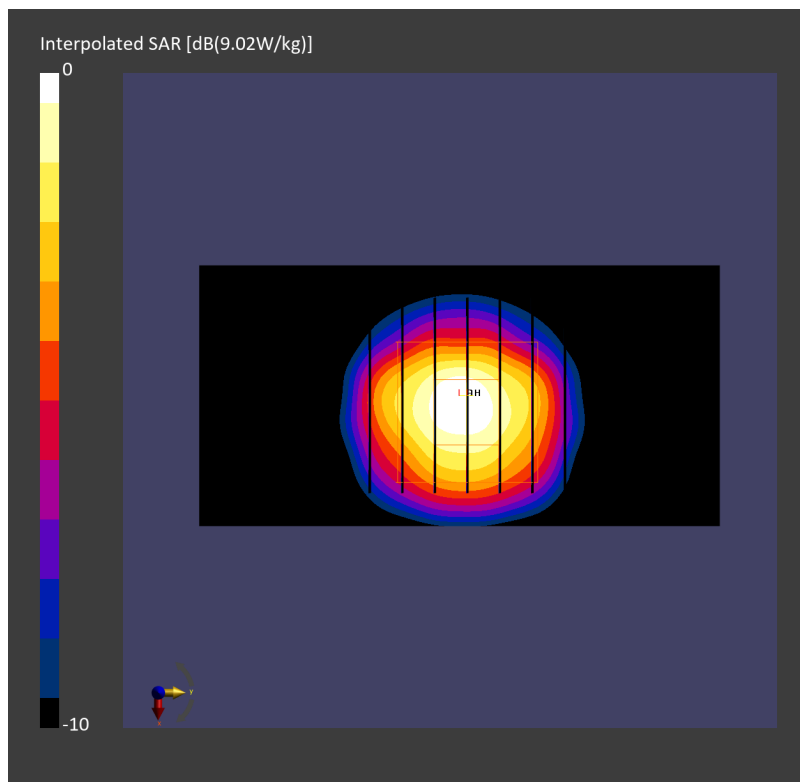

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260110 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.03$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.25 W/kg; SAR (10g) = 2.16 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 6.18 W/kg; SAR (8g) = 2.45 W/kg; SAR (10g) = 2.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 73.0 %

TSL Correction: Positive only

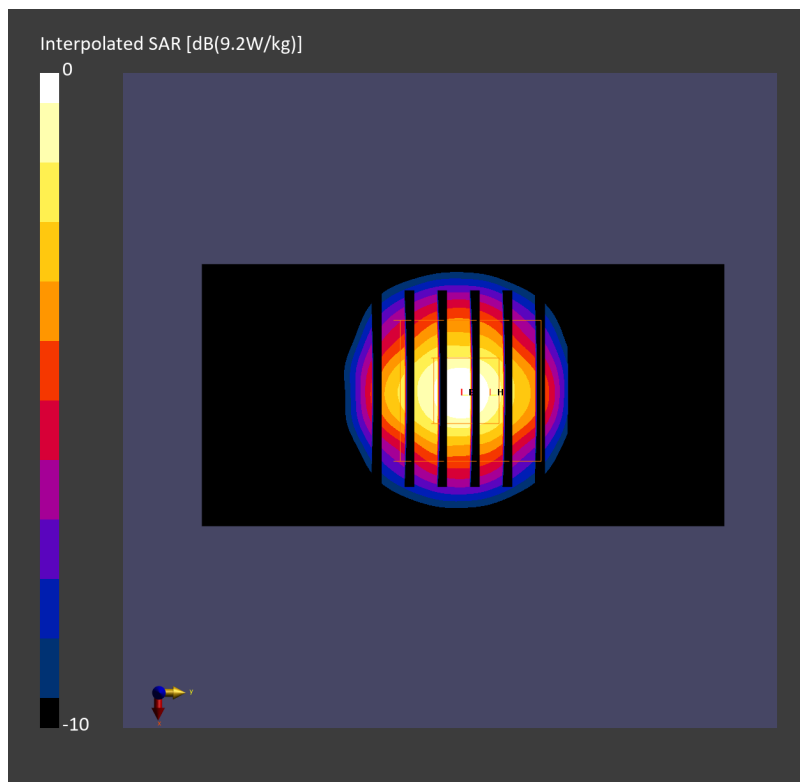

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260120 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.05$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2025-02-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.22 W/kg; SAR (10g) = 2.16 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 6.18 W/kg; SAR (8g) = 2.45 W/kg; SAR (10g) = 2.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 73.1 %

TSL Correction: Positive only

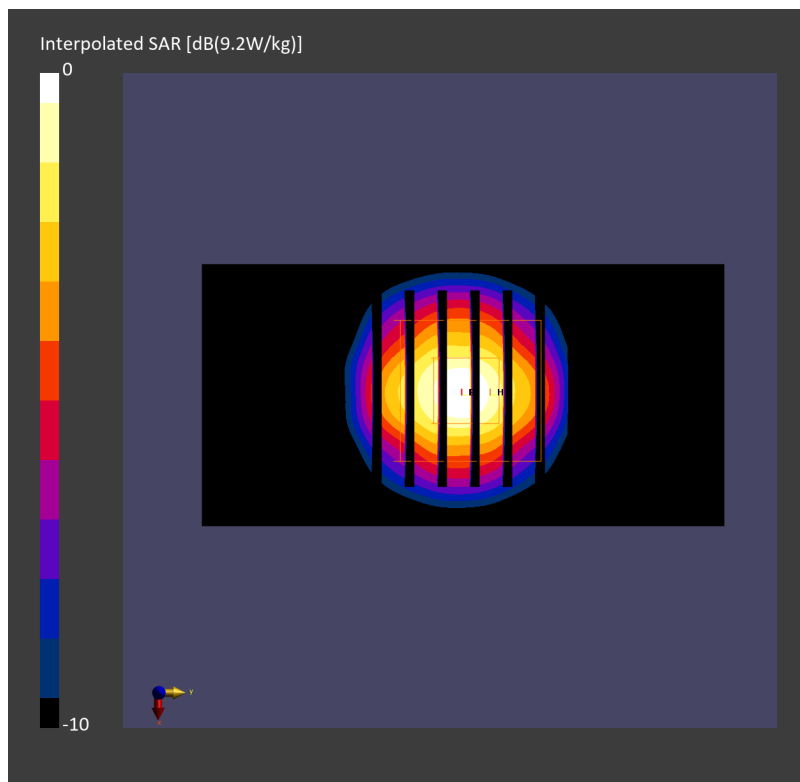

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260125 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.04$ S/m; $\epsilon_r = 36.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.30 W/kg; SAR (10g) = 2.32 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 6.53 W/kg; SAR (8g) = 2.71 W/kg; SAR (10g) = 2.39 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

TSL Correction: Positive only

