

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260224 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.903$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.46 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 2.20 W/kg; SAR (8g) = 1.55 W/kg; SAR (10g) = 1.47 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

TSL Correction: Positive only

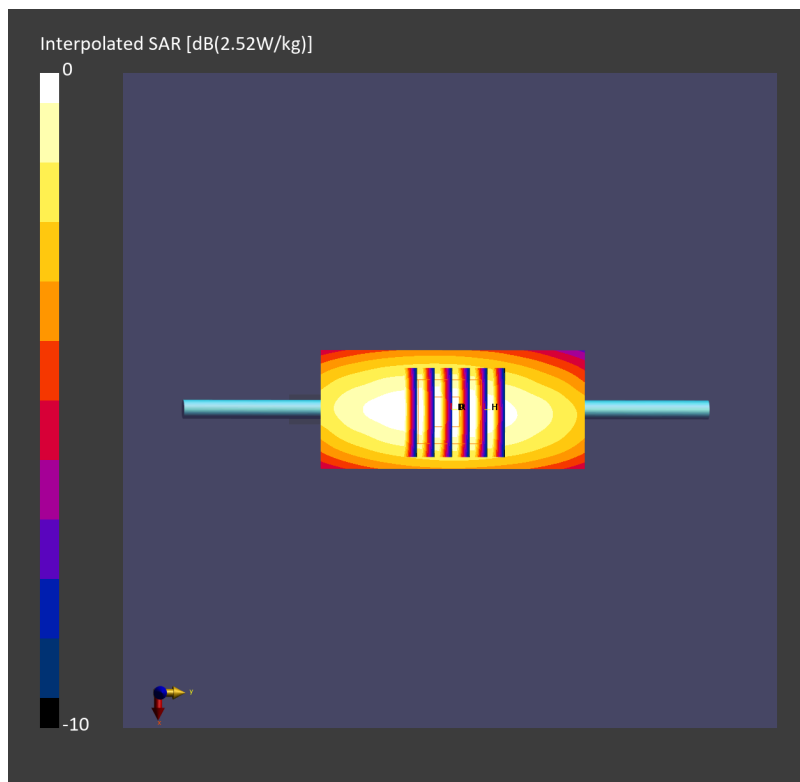

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260226 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.904$ S/m; $\epsilon_r = 44.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(9.46, 9.41, 10.07); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.32 W/kg; SAR (10g) = 1.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.34 W/kg; SAR (8g) = 1.66 W/kg; SAR (10g) = 1.48 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

TSL Correction: Positive only

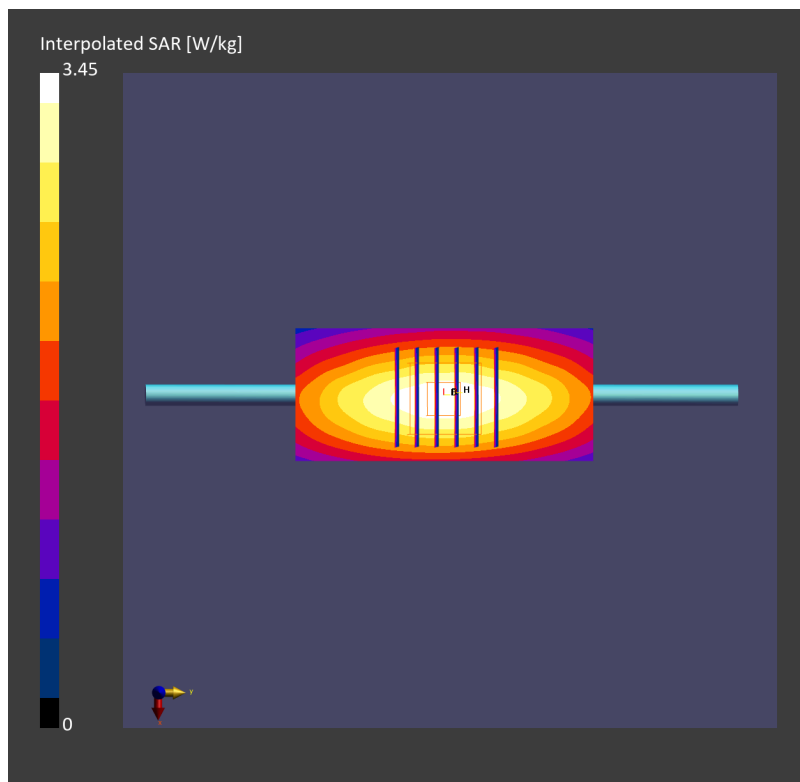

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260310 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.911$ S/m; $\epsilon_r = 44.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(9.23, 9.5, 9.45); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.48 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.5 %

TSL Correction: Positive only

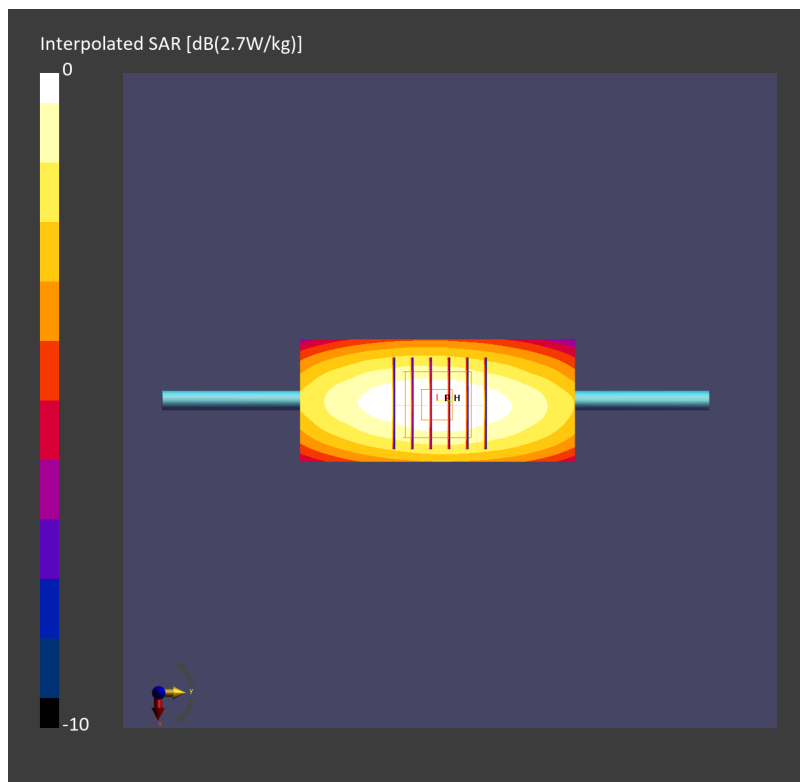

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260224 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.935$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.56 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.05 dB

SAR (1g) = 2.38 W/kg; SAR (8g) = 1.66 W/kg; SAR (10g) = 1.58 W/kg

Smallest distance from peaks to all points 3 dB below = 15.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

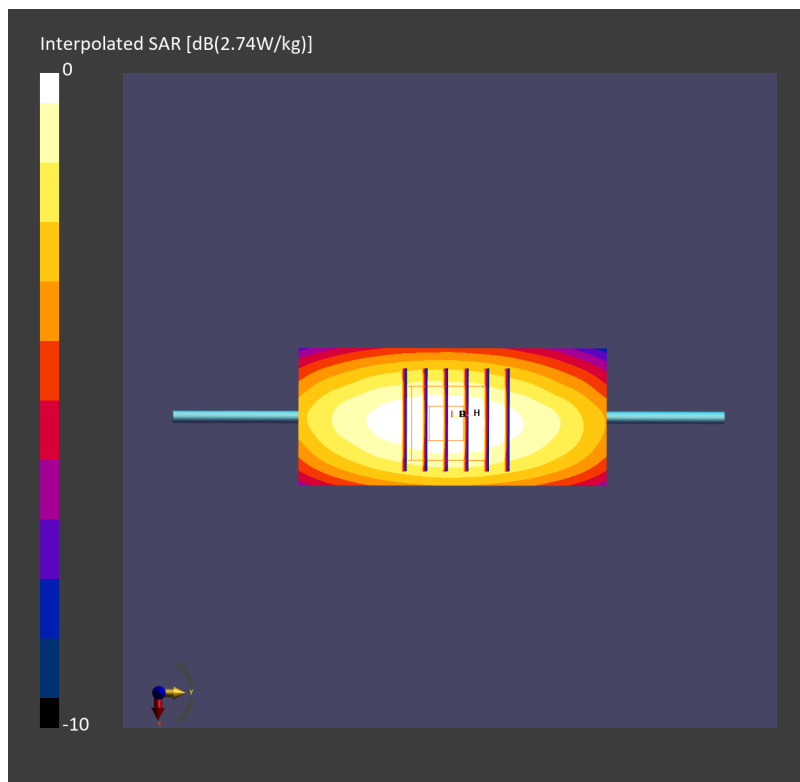

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260226 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.935$ S/m; $\epsilon_r = 44.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(9.11, 9.07, 9.7); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.70 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.58 W/kg; SAR (8g) = 1.83 W/kg; SAR (10g) = 1.67 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

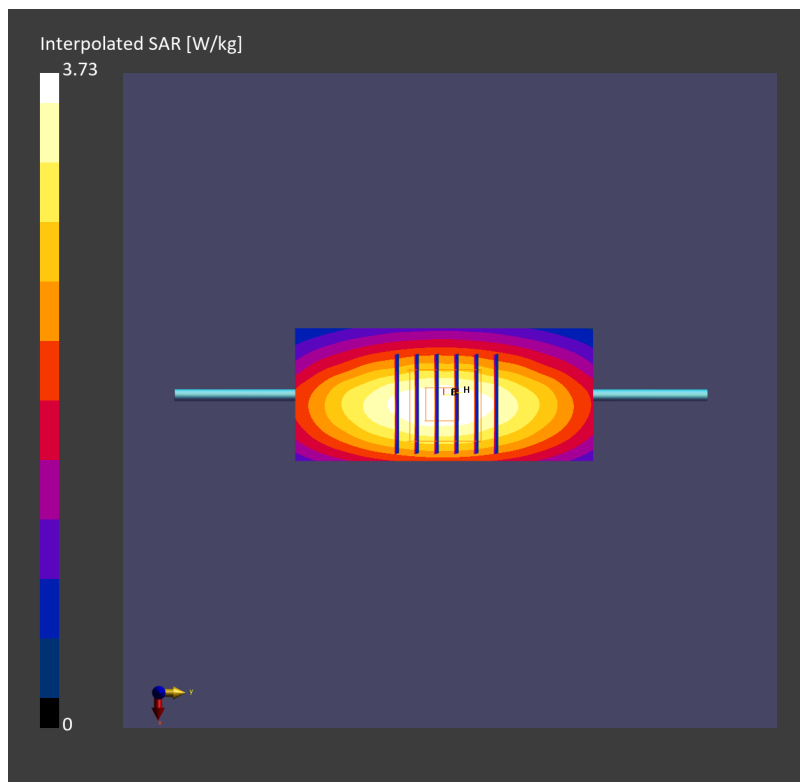

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260311 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.942$ S/m; $\epsilon_r = 44.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(9.13, 9.4, 9.35); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.59 W/kg; SAR (10g) = 1.72 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

TSL Correction: Positive only

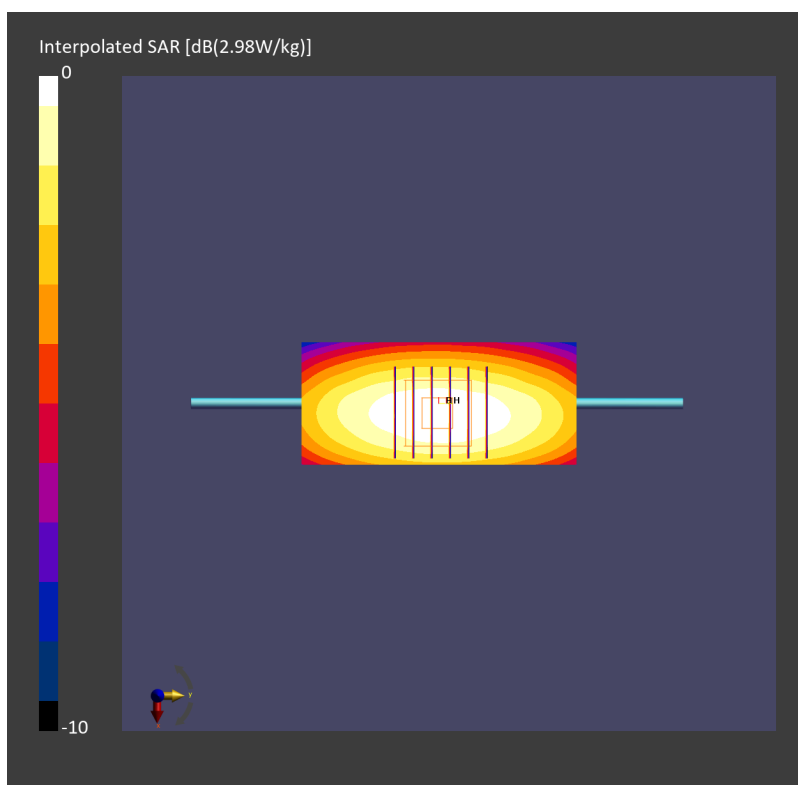

System Check_Head_1750MHz

DUT: D1750V2 - SN1120

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260225 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.08 W/kg; SAR (10g) = 4.84 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 9.00 W/kg; SAR (8g) = 5.30 W/kg; SAR (10g) = 4.90 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

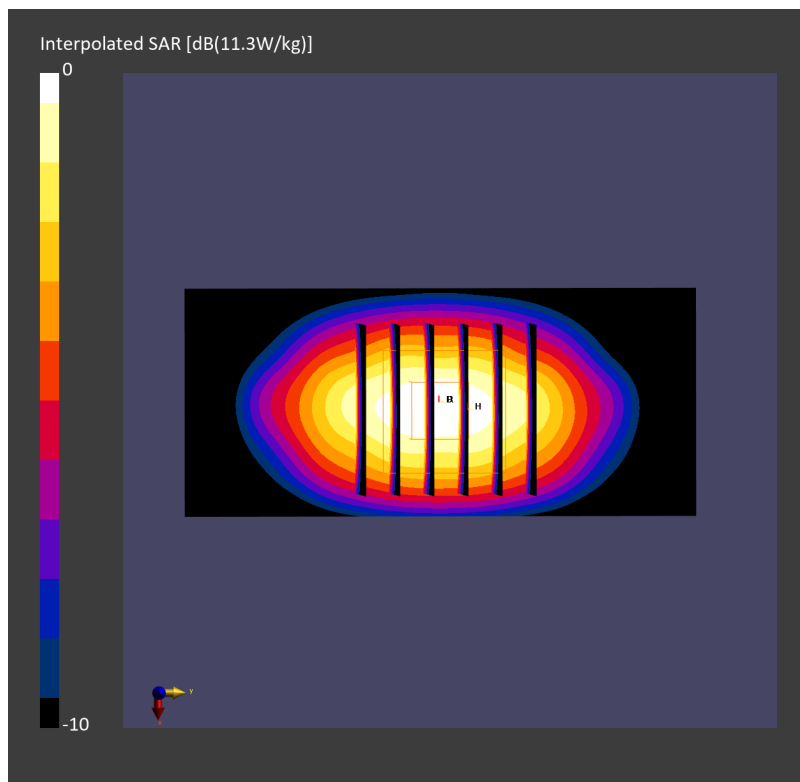

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.7, 7.66, 8.2); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.94 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.3 %

TSL Correction: Positive only

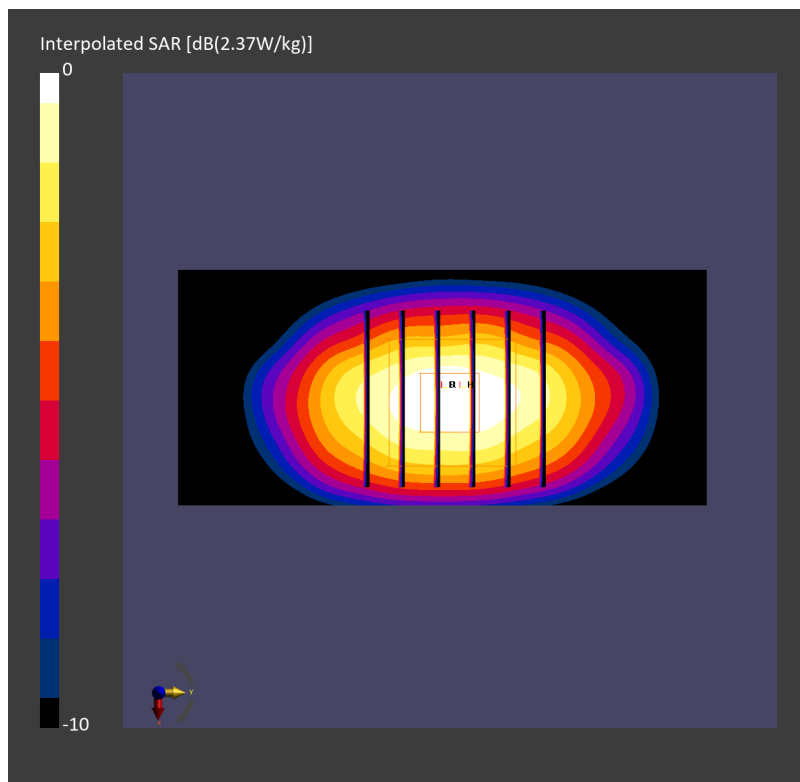

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260307 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.92 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

TSL Correction: Positive only

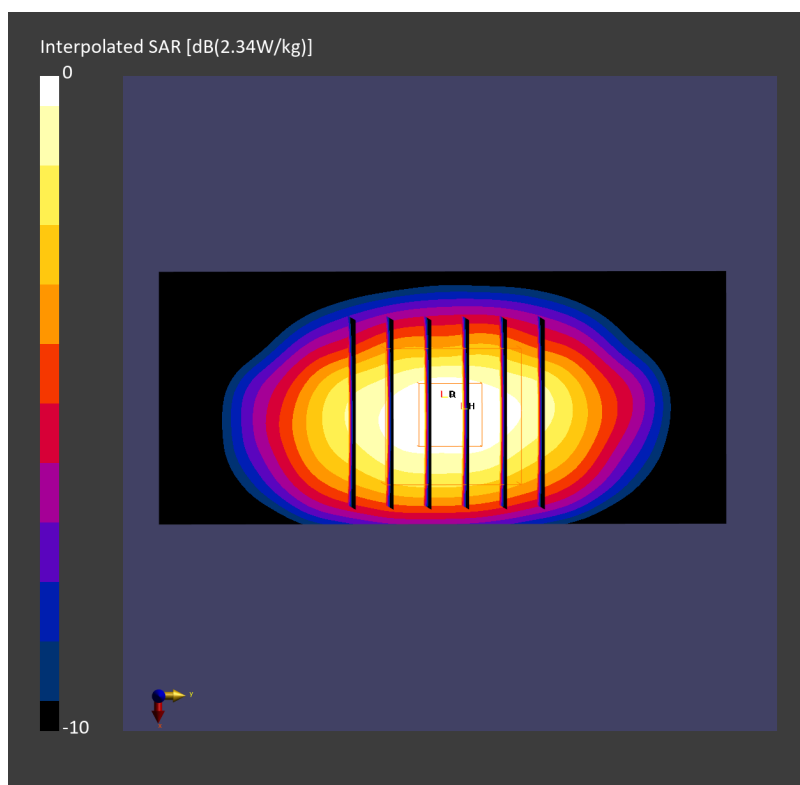

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260225 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.82 W/kg; SAR (10g) = 5.08 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 9.72 W/kg; SAR (8g) = 5.61 W/kg; SAR (10g) = 5.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

TSL Correction: Positive only

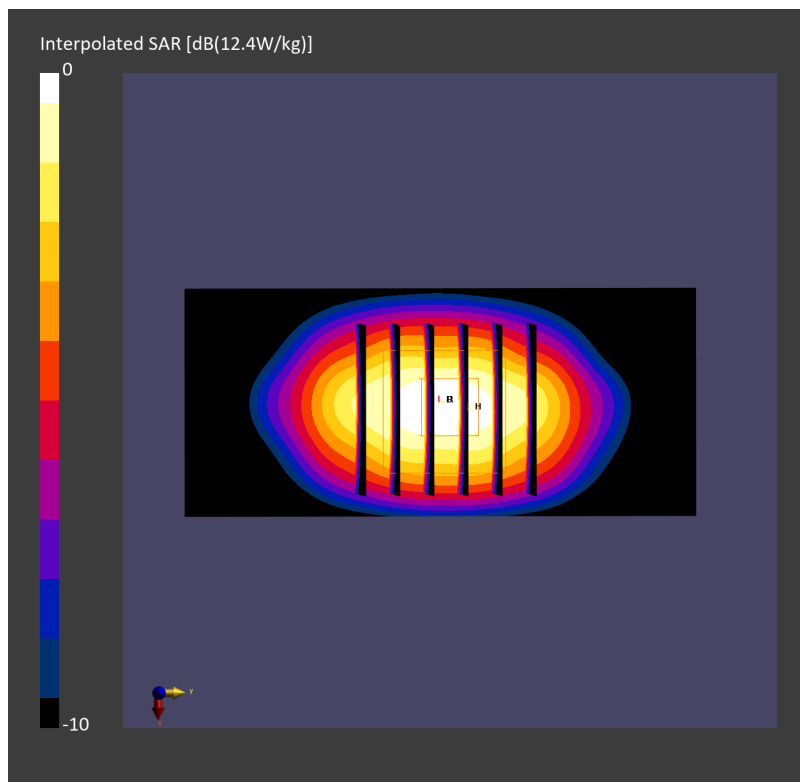

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260228 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.51$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.47, 7.43, 7.95); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.07 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

TSL Correction: Positive only

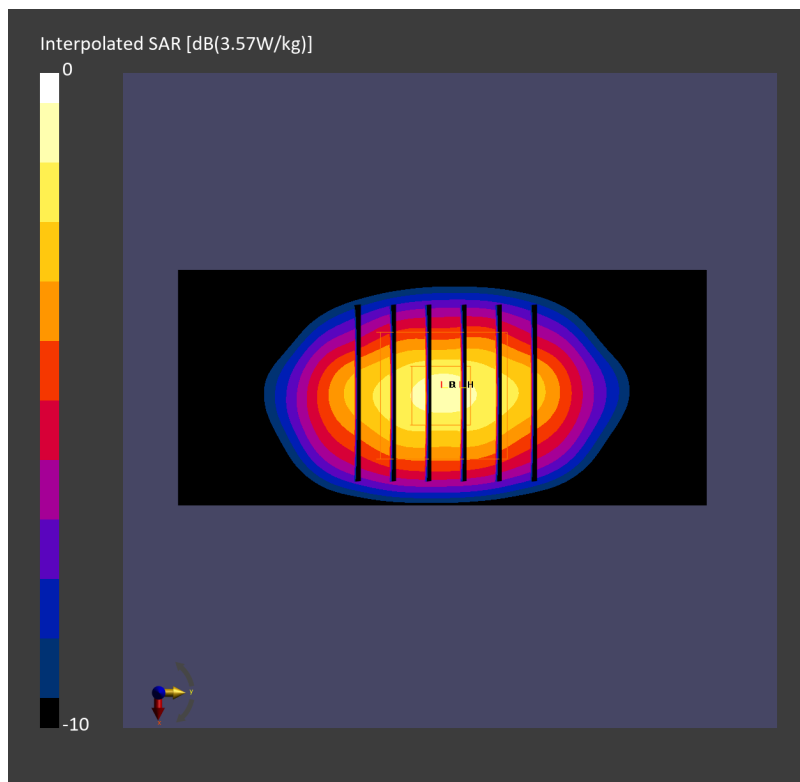

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260302 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.01 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

TSL Correction: Positive only

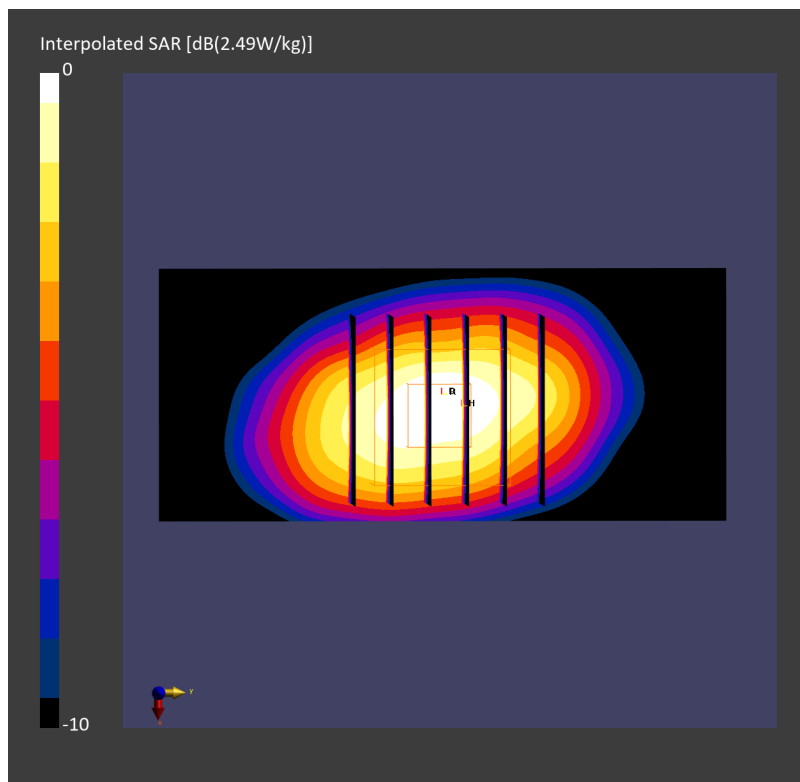

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260226 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.72$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.2 W/kg; SAR (10g) = 5.79 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 12.1 W/kg; SAR (8g) = 6.48 W/kg; SAR (10g) = 5.90 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.2 %

TSL Correction: Positive only

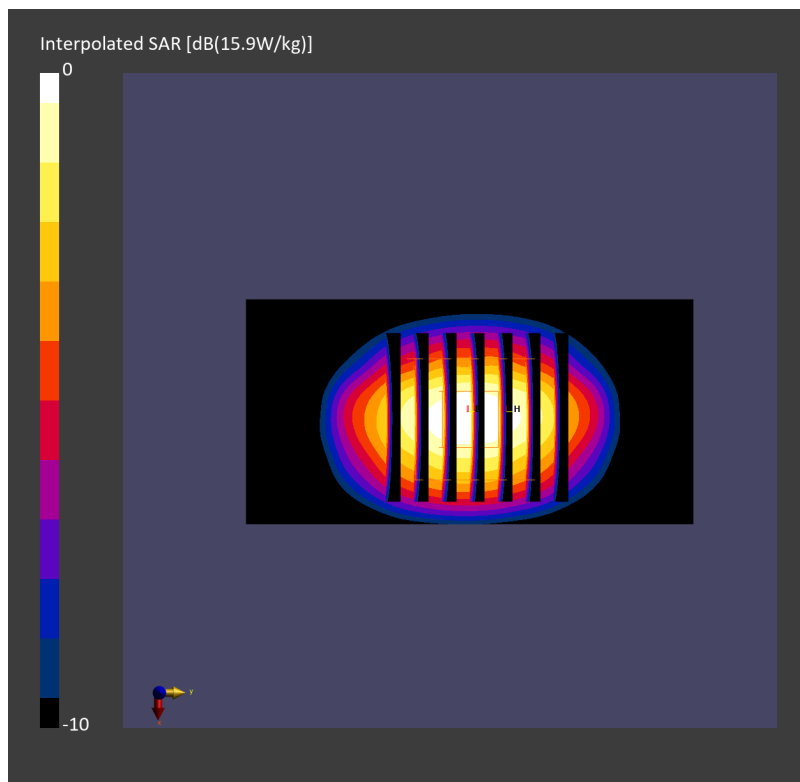

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260301 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.35, 7.31, 7.82); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.43 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

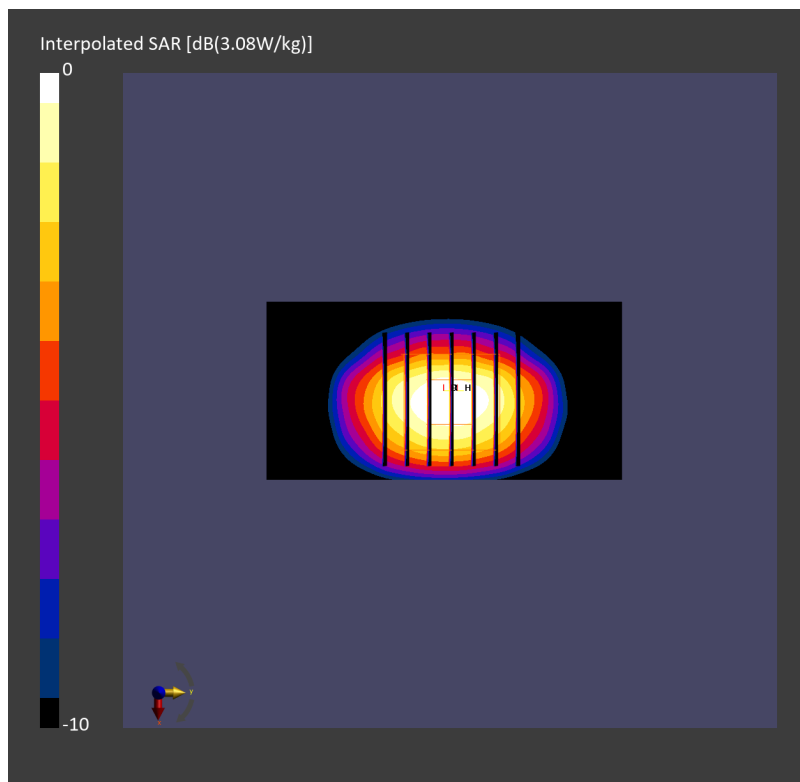

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260304 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.73$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.3 %

TSL Correction: Positive only

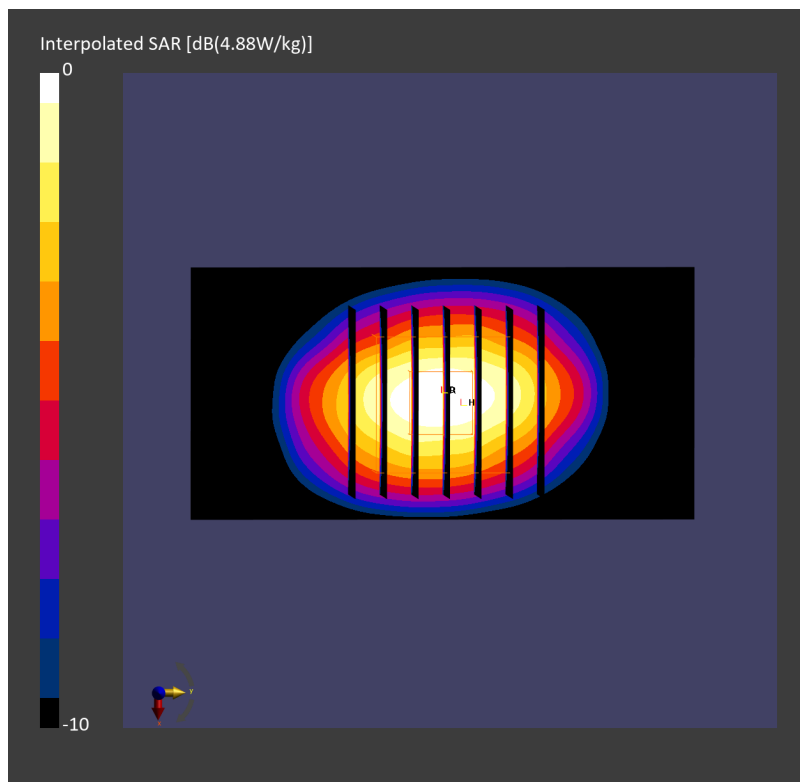

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260216 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(7.02, 7.23, 7.2); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.2 W/kg; SAR (10g) = 6.45 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 14.3 W/kg; SAR (8g) = 7.03 W/kg; SAR (10g) = 6.33 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

TSL Correction: Positive only

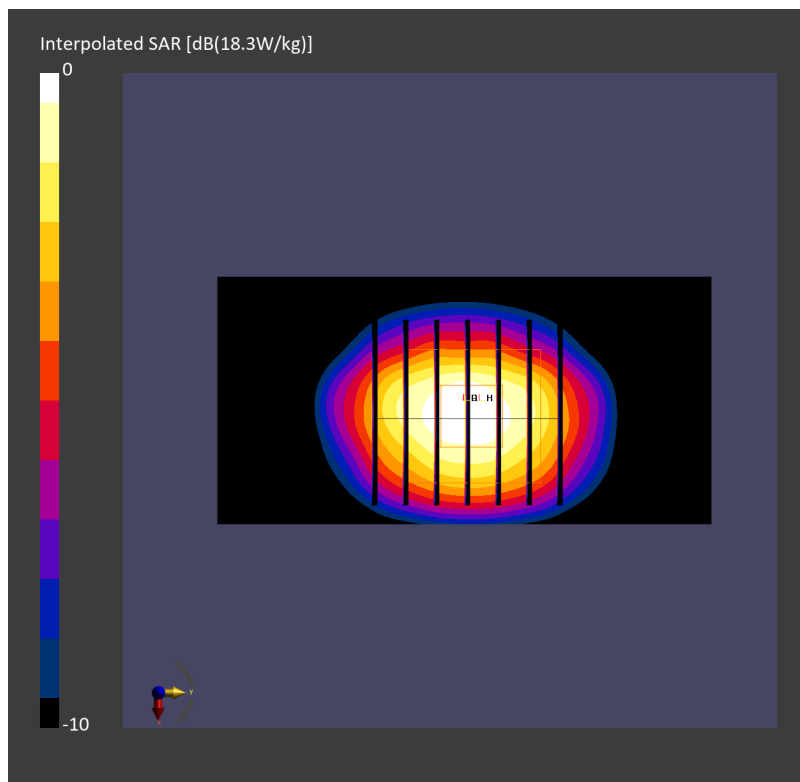

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260222 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.52, 6.42, 6.64); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.7 W/kg; SAR (10g) = 6.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 14.4 W/kg; SAR (8g) = 7.16 W/kg; SAR (10g) = 6.45 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

TSL Correction: Positive only

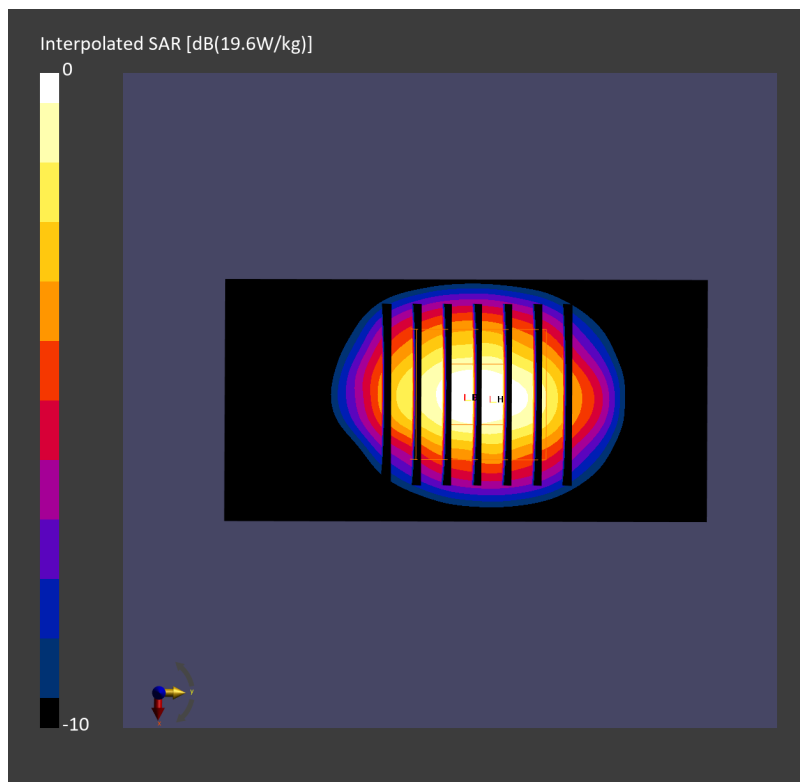

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260226 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.14 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 13.8 W/kg; SAR (8g) = 6.98 W/kg; SAR (10g) = 6.30 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

TSL Correction: Positive only

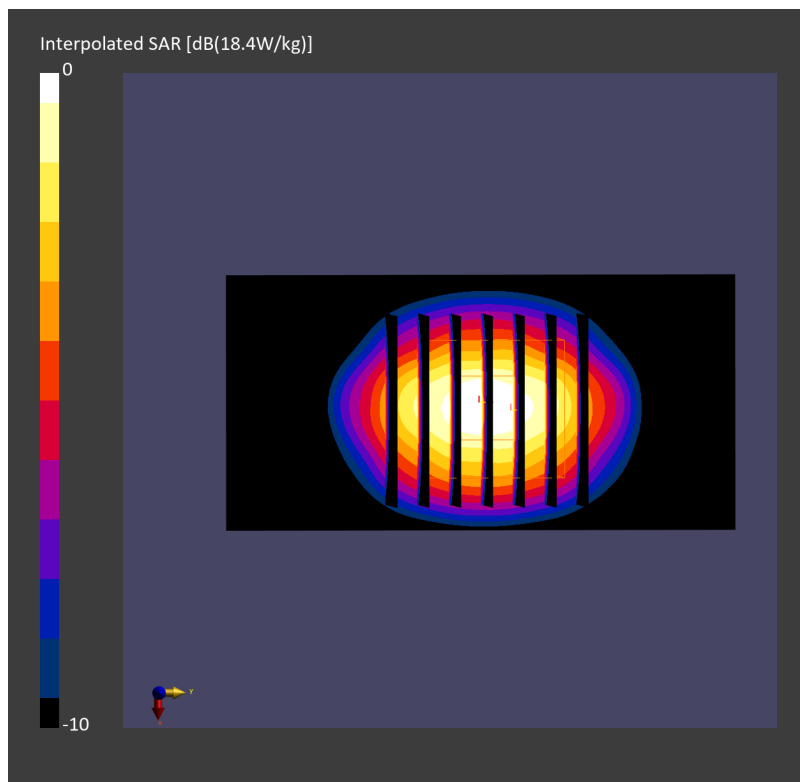

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260302 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.09, 7.06, 7.55); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.77 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

TSL Correction: Positive only

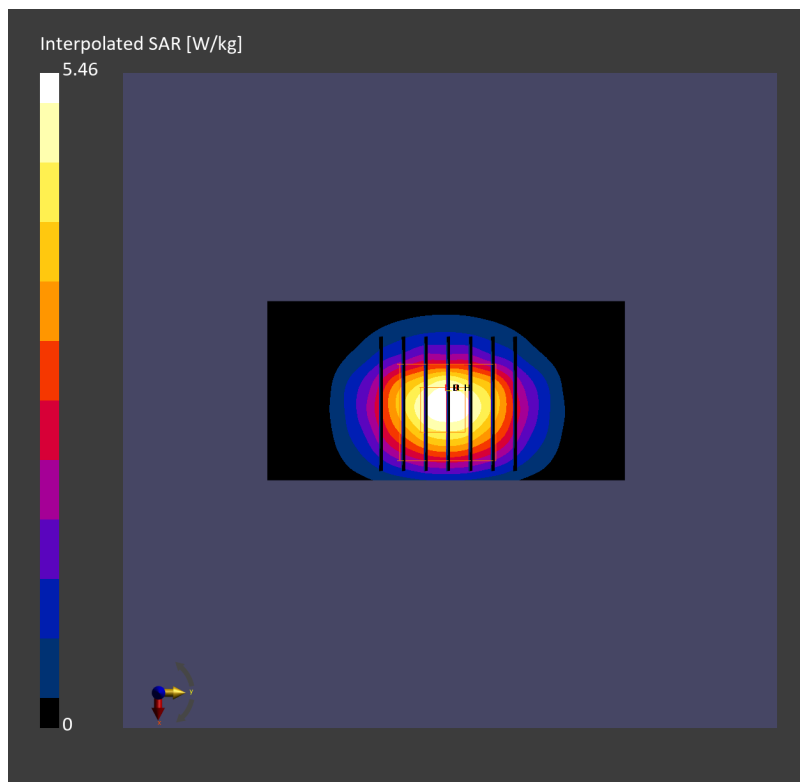

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260306 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.79 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.84 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

TSL Correction: Positive only

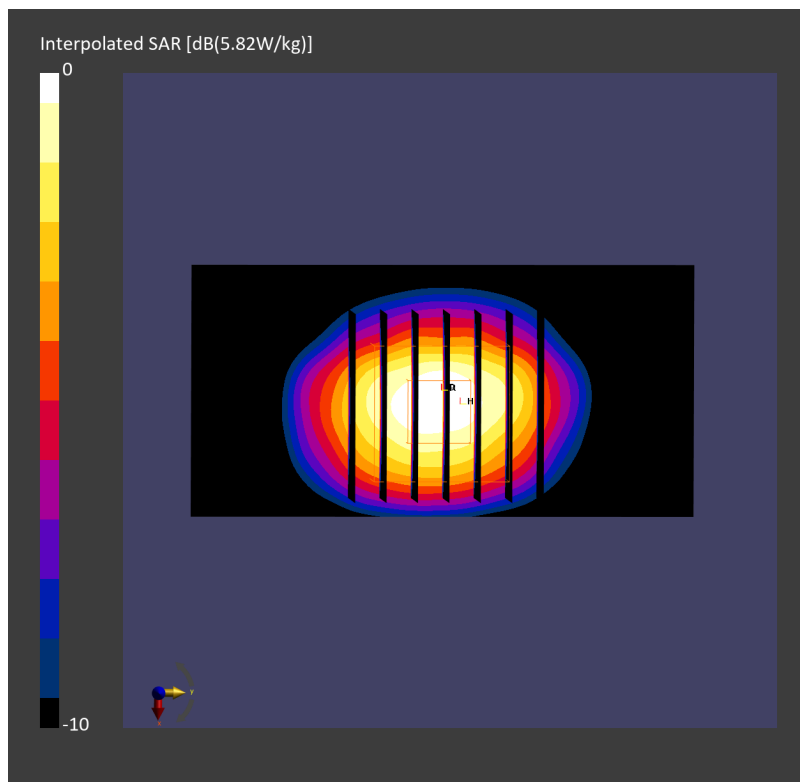

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260214 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.22, 6.13, 6.33); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.32 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

TSL Correction: Positive only

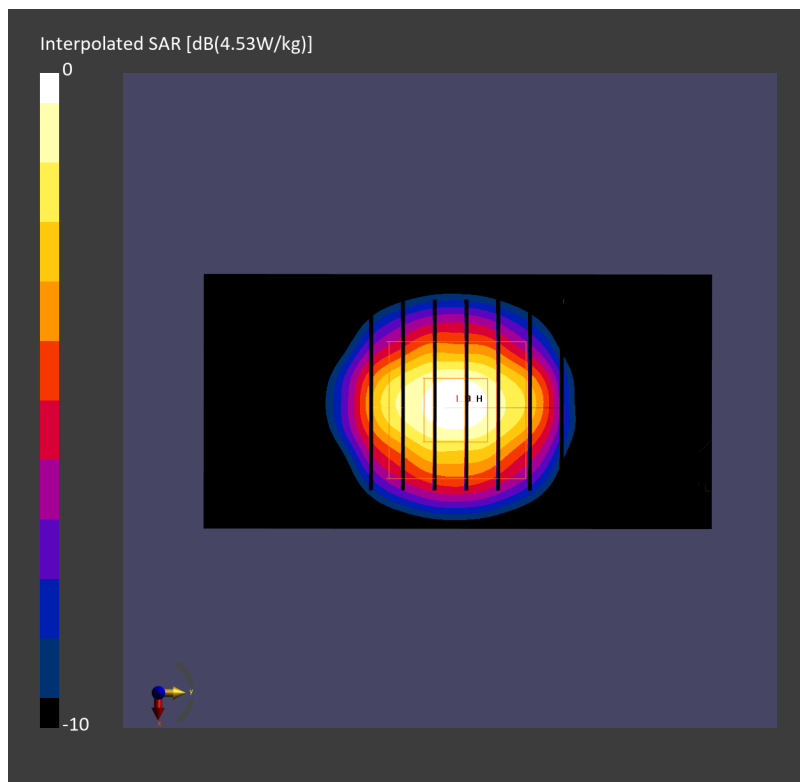

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(6.42, 6.61, 6.58); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.36 W/kg; SAR (10g) = 2.40 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.31 W/kg; SAR (8g) = 2.68 W/kg; SAR (10g) = 2.38 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.3 %

TSL Correction: Positive only

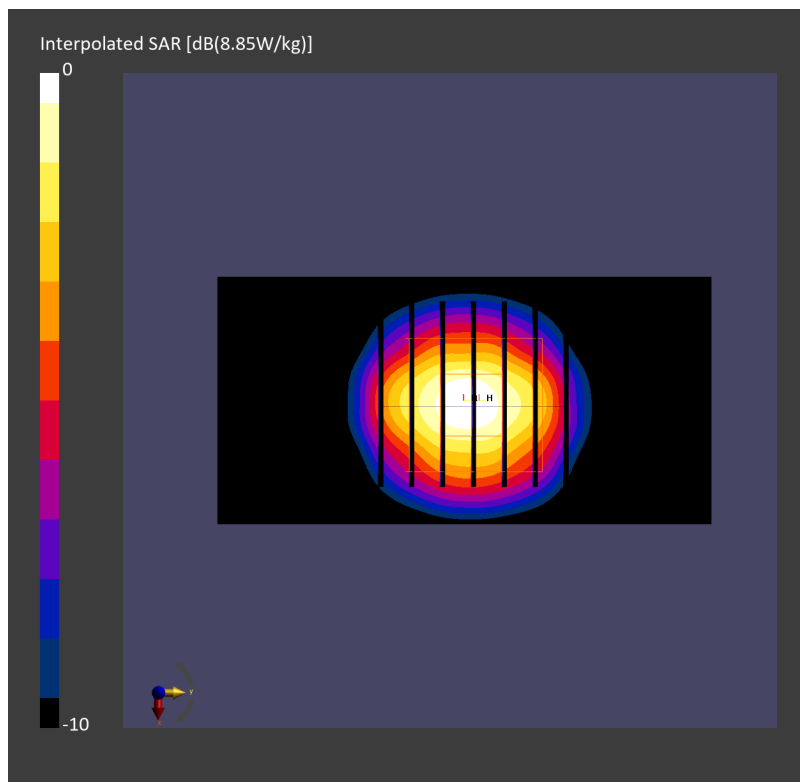

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.09 W/kg; SAR (10g) = 2.68 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 7.08 W/kg; SAR (8g) = 3.06 W/kg; SAR (10g) = 2.71 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

TSL Correction: Positive only

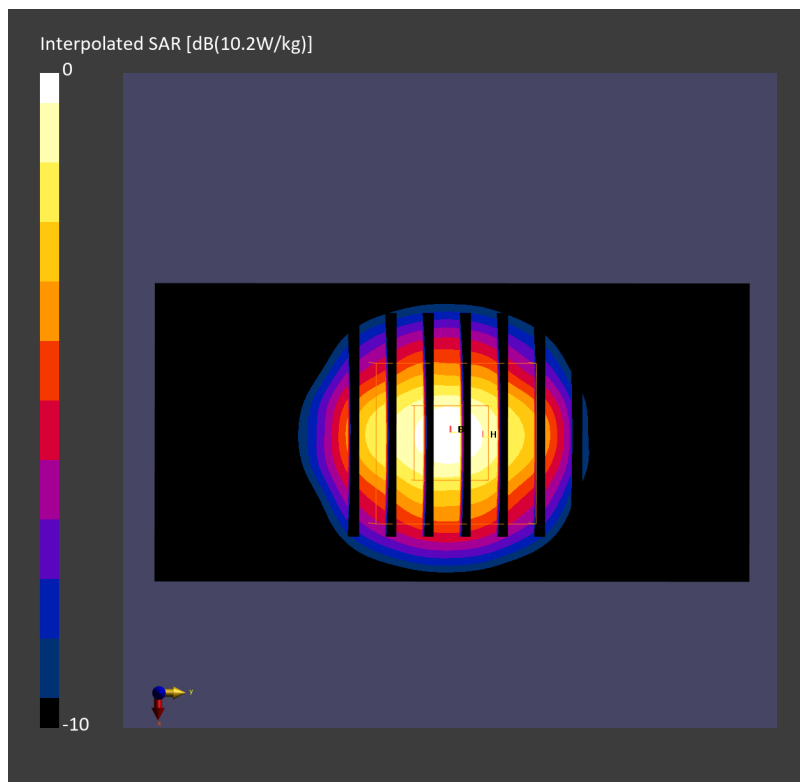

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 36.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.36 W/kg; SAR (10g) = 2.39 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.11 dB

SAR (1g) = 6.39 W/kg; SAR (8g) = 2.79 W/kg; SAR (10g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 78.0 %

TSL Correction: Positive only

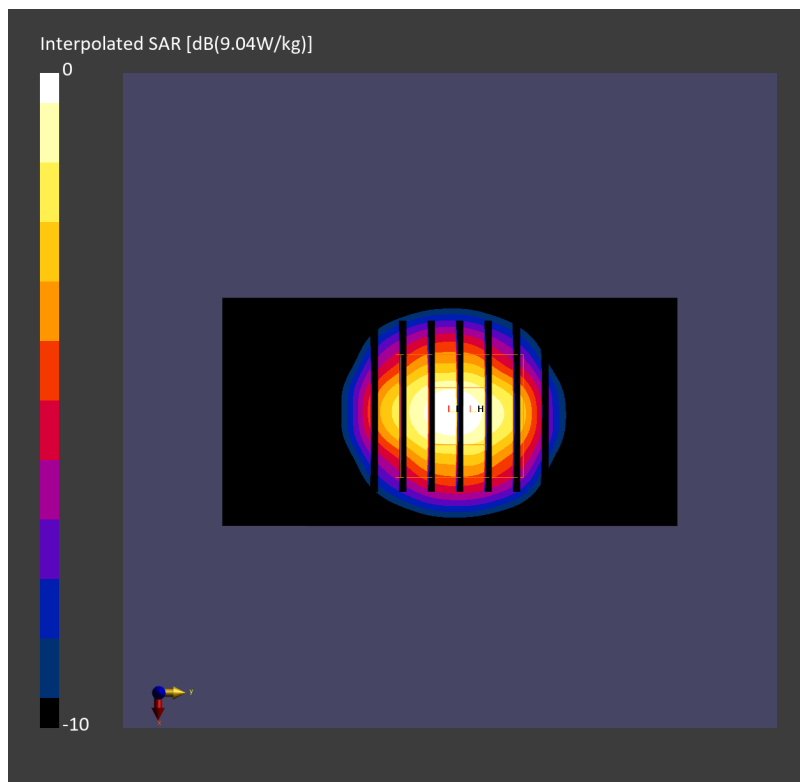

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260303 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.78$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.42, 6.39, 6.83); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.29 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 78.2 %

TSL Correction: Positive only

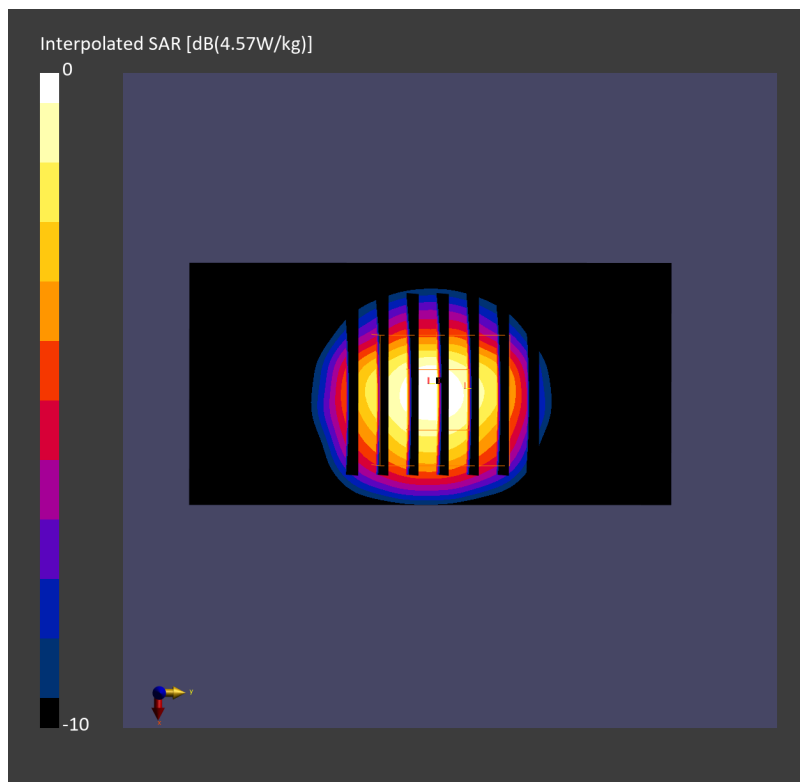

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260214 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.14, 6.04, 6.25); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.58 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

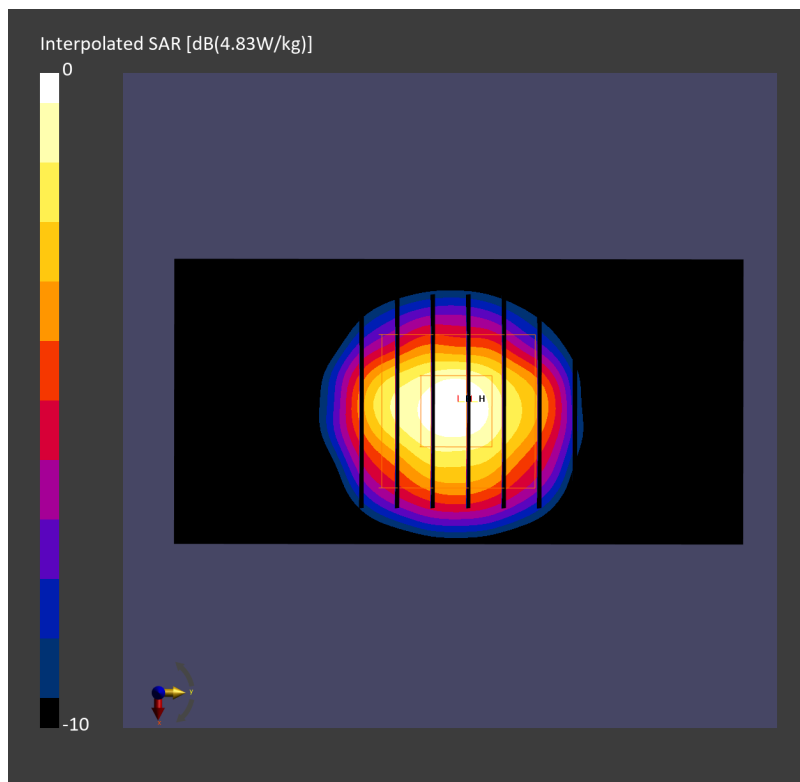

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(6.32, 6.5, 6.47); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.90 W/kg; SAR (10g) = 2.51 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.92 W/kg; SAR (8g) = 2.85 W/kg; SAR (10g) = 2.51 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

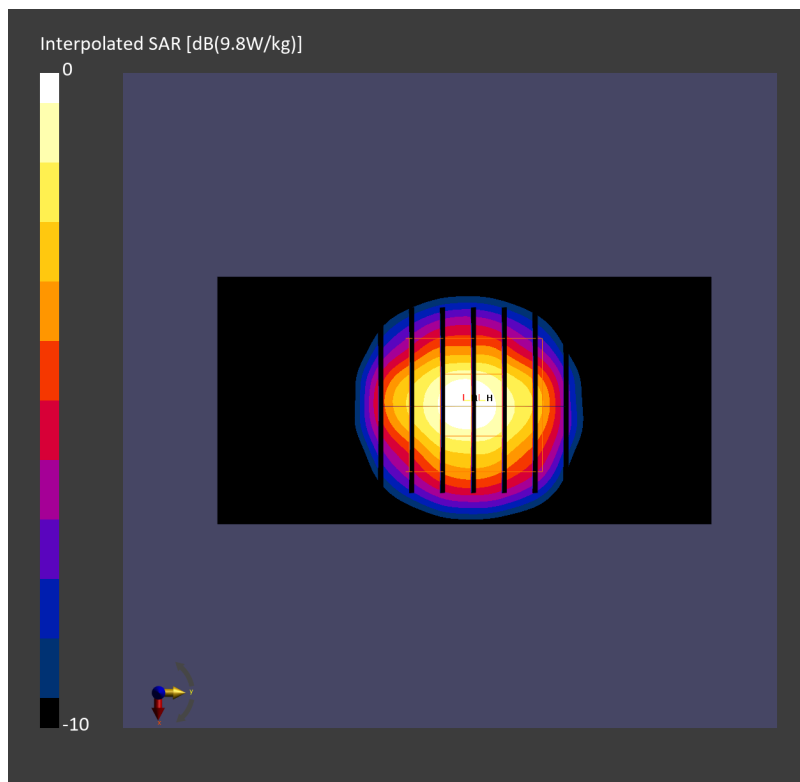

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.08 W/kg; SAR (10g) = 2.56 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 7.14 W/kg; SAR (8g) = 2.97 W/kg; SAR (10g) = 2.62 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.2 %

TSL Correction: Positive only

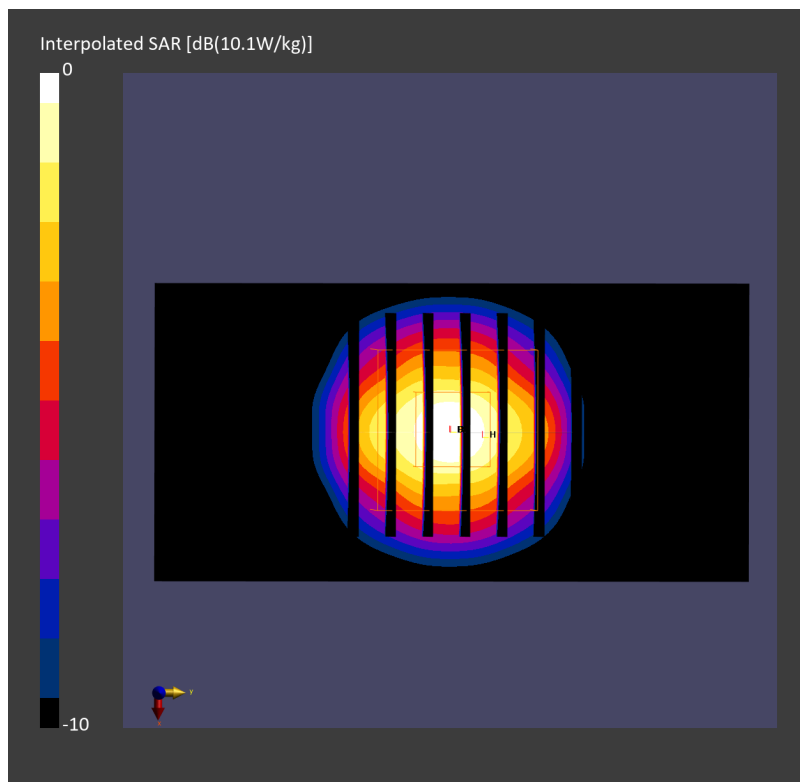

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.43 W/kg; SAR (10g) = 2.36 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 6.85 W/kg; SAR (8g) = 2.89 W/kg; SAR (10g) = 2.55 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

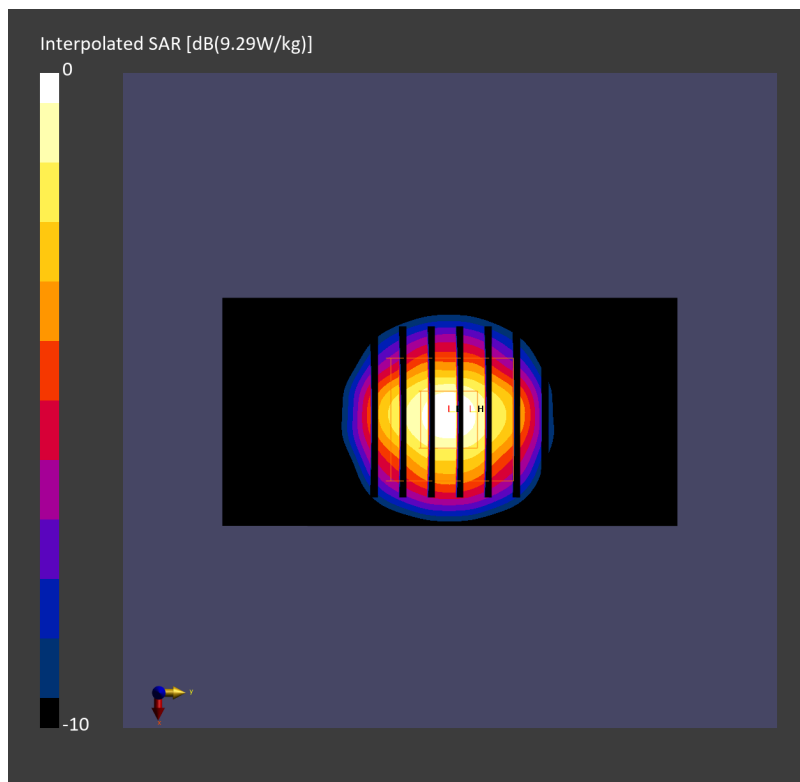

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260303 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.36, 6.33, 6.77); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.38 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.8 %

TSL Correction: Positive only

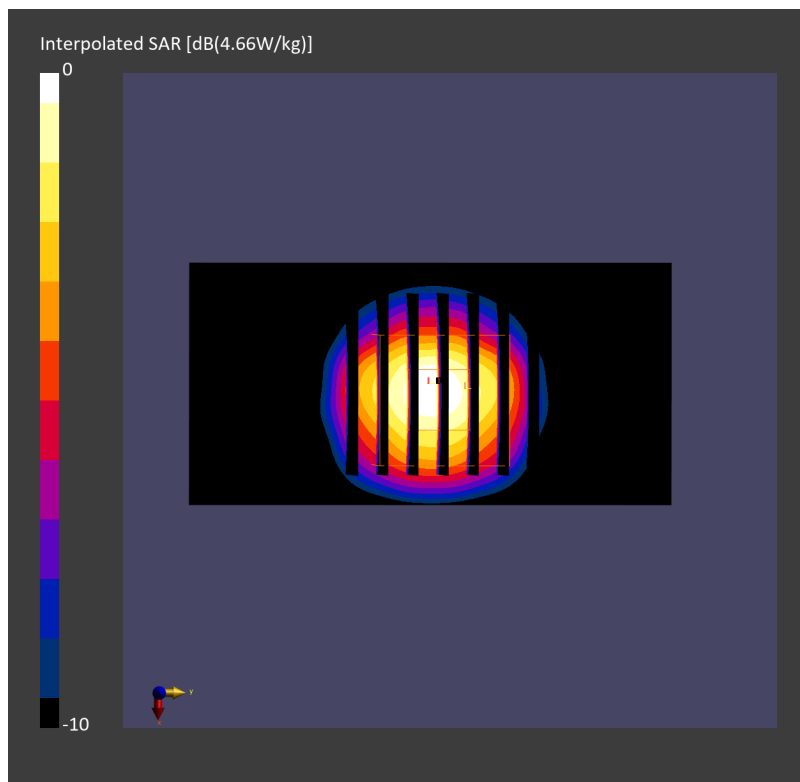

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.11$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7970; ConvF(6.38, 6.57, 6.54); Calibrated: 2026-01-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2025-05-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.51 W/kg; SAR (10g) = 2.28 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.57 W/kg; SAR (8g) = 2.61 W/kg; SAR (10g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

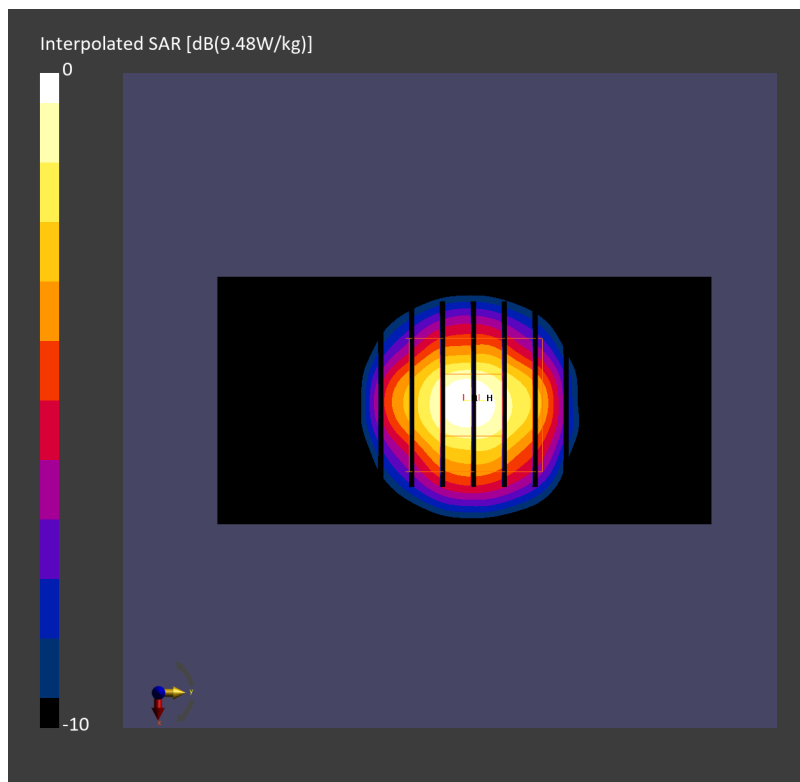

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.79 W/kg; SAR (10g) = 2.37 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.90 W/kg; SAR (8g) = 2.78 W/kg; SAR (10g) = 2.44 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

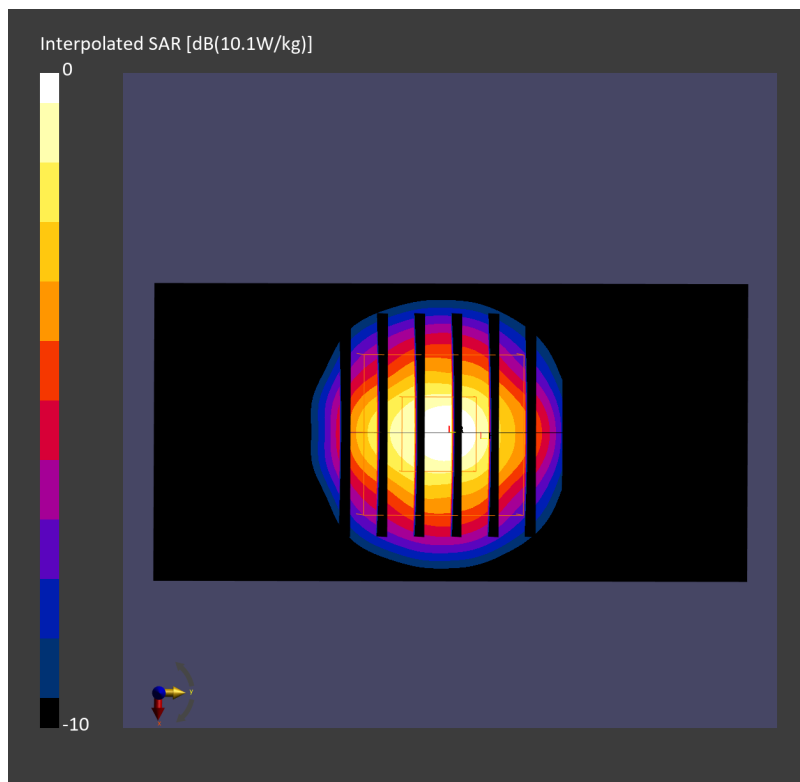

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2157; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.49 W/kg; SAR (10g) = 2.33 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.09 dB

SAR (1g) = 6.79 W/kg; SAR (8g) = 2.76 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

TSL Correction: Positive only

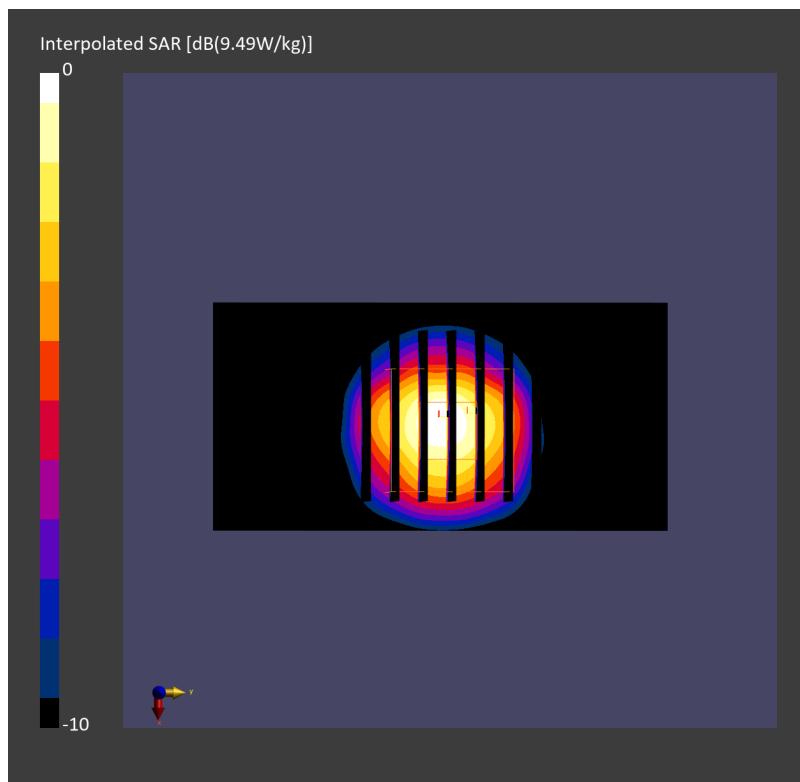

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260303 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.37, 6.34, 6.78); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2025-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.95 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.08 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

