9	Select "Trichloramine measurement" with the up and down arrows then press the "OK" button From there, follow the steps indicated by the trikloram device	
10	Insert the measuring cuvette into the trikloram and press the "OK" button	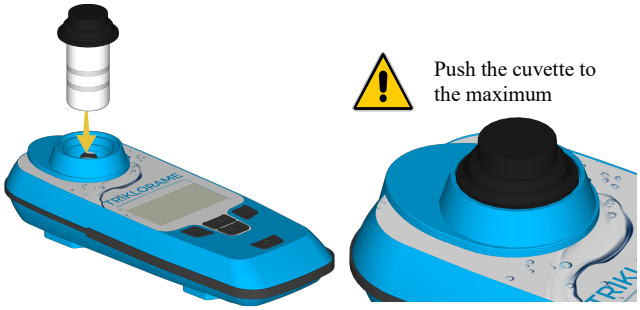
11	Use the up and down arrows to enter the exposure time then press the "OK" button once each digit is selected	
12	Read the value of trichloramine in the air	

13	Press the "OK" button to make a new measurement of trichloramine OR Press the "RETURN" button to return to the main menu OR Press the "OFF" button of the triklorame to turn off the device	

3) Interpretation of the result

The measurement scale will depend on the exposure time.

After a minimum exposure time of 1h30, trichloramine can be measured.

Scale of measurement according to the exposure time :

- Exposure time <2h: 0.3 ~ 5mg/m^3 **(WARNING: on a short exposure time the measurement will be very sensitive to pollution during handling).**
  - Case 1 : trichloramine <0.3mg/m^3: the trikloram will indicate that the value is <0.3mg/m^3 and will not be able to display the exact value.
  - Case 2 : 0.3 <trichloramine <5mg/m^3: trikloramate will indicate the value at ±0.1mg/m3
- Exposure time > or = to 2h: 0 ~ 2mg/m^3
  - Case 1 : 0 <trichloramine <2mg/m^3: trikloram will indicate the value at ±0.1mg/m^3
  - Case 2 : trichloramine> 2mg/m^3: trikloram will indicate that the value is> 2mg/m^3 and will not be able to display the exact value

The determination of the trichloramine concentration may vary due to external pollution during handling (examples: postilion, finger on sampling sample, tweezers tweezer, vat analysis, syringe not or poorly washed before analysis ...)
The influence of external pollution reduces with the increase of the duration of exposure.

4) Error messages

"Error: trichloramine concentration below the measurement scale" :

This message may appear if:

- the measurement made at a trichloramine level which is too low and is not within the minimum measuring range that can be measured
- the analysis cuvette is poorly positioned in the trikloram and contacts with the electrodes are not well done
    - Reposition the cuvette, the cork must fit perfectly into the intended housing

"Error: Trichloramine concentration above the measurement scale":

This message may appear if:

- the measurement carried out has a trichloramine level that is too high and is not within the maximum measuring range that can be measured
- the analysis tank has been polluted
    - Clean the analysis tank by rinsing 3 times with deionized water

For any other value, contact the SYCLOPE Electronique technical department