

LABELING

Original Freigabeformular in TR archiviert.
Original form stored in the technical writing department.

Label sticks inside of the device

FA. Nr. ##### - ## SN YYMMCE#### Removing this label causes loss of warranty. 10000017696 06	 	
MAX. OUTPUT PRESSURE MAX. AUSGANGSDRUCK PRESSION DE SORTIE MAX. MAKS. ÇIKIŞ BASINCI MAX. GASFLOW RATE MAX. GASFLUSS DEBIT DE GAS MAX. MAKS. GAZ AKIMI MAINS VOLTAGE RANGE NETZSPANNUNGSBEREICH PLAGE DE TENSION DU SECTEUR ŞEBEKE GERİLİM ARALIĞI SUPPLY FREQUENCY VERSORGUNGSFREQUENZ FREQUENCE D'ALIMENTATION BESLEME FREKANSI POWER CONSUMPTION LEISTUNGS-AUFNAHME CONSOMM. DE PUISSANCE GÜÇ TÜKETİMİ	75 mmHg 50 l/min AC 100-240 V~ 50/60 Hz AC 100 V ~ 1.05 A AC 240 V ~ 0.50 A	stryker® Distributed by Stryker Endoscopy 5900 Optical Court, San Jose, CA 95138 (USA) (408) 754-2000 (800) 624-4422 www.stryker.com
 YYYY-MM-DD	 	

PNEUMOCLEAR™

W.O.M. WORLD OF MEDICINE GmbH
 Salzufer 8, 10587 Berlin, Germany
 Phone: +49 30 39981-550

CE 0197


TYPE SN / REF	FM300 YYMMCE#### / ####-###-###
--	---

Contains FCC ID: 2AS5K-TSHW42 (01)GTIN
 Contains IC: 25004-TSHW42A (11)YYMMDD
 HVIN: 1430 (21)YYMMCE####


Ge1 EAN
Datamatrix
01 / 11 / 21

Issuing Agency:
GS1

Rear of device

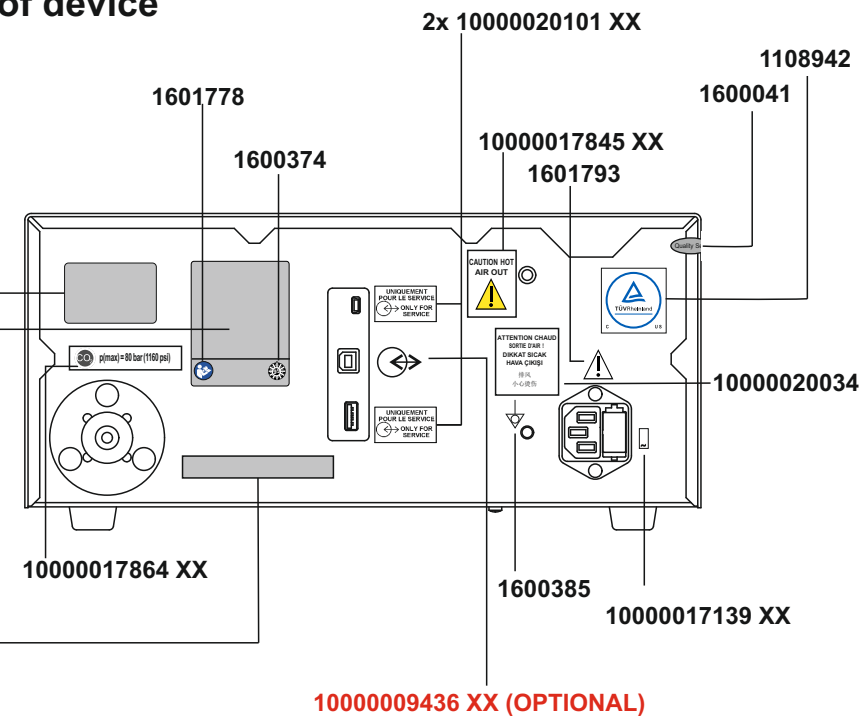

Box

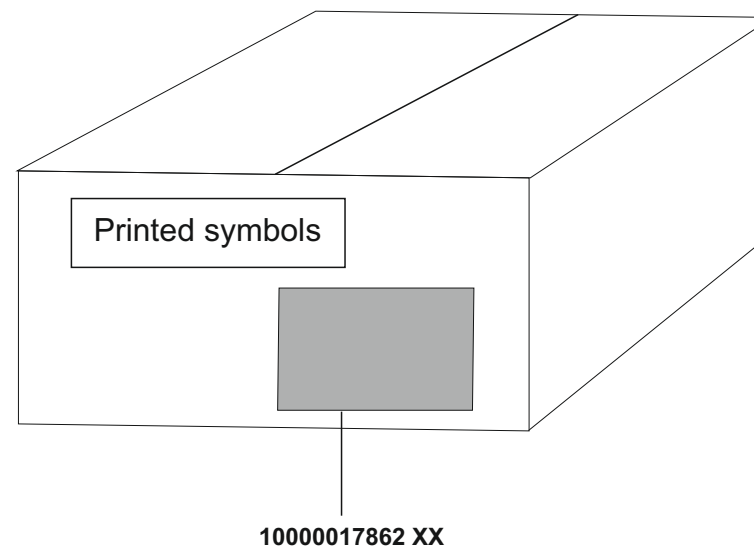

Revision history

Rev. WOM	ÄV Nr.	Change
01	2016001	DataMatrix UDI; Technical Data correction. Position of Quality Seal; Label Transport conditions removed
02	2016378	SIDNE Optional
03	2016502	4 Languages, exchanged label „SIDNE“ with „data transfer“,inserted new label 10000020034
04	2016587	Label 10000017846 XX replaced by 10000020101 XX;
05	2017293	Added: Symbol for australian standard;
06	2020225	Added: FCC-ID/IC-Number

Product Management / Customer

Project Management (R&D)

Regulatory Affairs

WORLD OF MEDICINE / *Approval*

	W.O.M. Item number
--	--------------------

FMT File	10000017696 06.fmt
----------	--------------------

CDR File
10000017696 06.cdr

Name	TR
------	----

Date 03.11.2020

Overview device labels FM300 STRYKER

10000017696 06