RADIO REPORT

FCC 47 CFR Part 15C
ISED Canada RSS-247

Digital transmission systems operating within the 2400 – 2483.5 MHz band

Report Reference No	G0M-2003-8888-TFC247BL-V01
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	DAkkS - Registration number : D-PL-12092-01-03 (ISED) ISED Testing Laboratory site: 3470A-2 DAkkS - Registration number : D-PL-12092-01-04 (FCC) FCC Filed Test Laboratory, Reg.-No.: 96970
Applicant	GWA Hygiene GmbH
Address	Heinrich-Mann-Str. 11 18435 Stralsund GERMANY
Test Specification	47 CFR Part 15C RSS-247, Issue 2, 2017-02 RSS-Gen, Issue 5, Amendment 1, 2019-03
Non-Standard Test Method	None
Equipment under Test (EUT):	
Product Description	Hygiene-Monitoring-System
Model(s)	NosoEx Point of Care / Drucksensor
Additional Model(s)	None
Brand Name(s)	None
Hardware Version(s)	1.7.1
Software Version(s)	2.17
FCC-ID	2AU27NOSOEX002
IC	n/a
Test Result	**PASSED**

Possible test case verdicts:		
Required by standard but not tested	N/T	
Not required by standard	N/R	
Not applicable to EUT	N/A	
Test object does meet the requirement	P(PASS)	
Test object does not meet the requirement	F(FAIL)	
Testing:		
Test Lab Temperature	20 - 23 °C	
Test Lab Humidity	20 – 38 %	
Date of receipt of test item	2020-03-27	
Report:		
Compiled by	Florian Voigt	
Tested by (+ signature) (Responsible for Test)	Florian Voigt supervised by Wilfried Treffke	F. Voigt W. Treffke .....
Approved by (+ signature) (Head of Lab)	Christian Weber	C. Weber .....
Date of Issue	2020-04-29	
Total number of pages	100	
General Remarks:		
The test results presented in this report relate only to the object tested. **The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.** This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.		
Additional Comments:		

VERSION HISTORY

Version History			
Version	Issue Date	Remarks	Revised By
01	2020-04-29	Initial Release	

ABBREVIATIONS AND ACRONYMS

Acronyms	
Acronym	Description
EUT	Equipment Under Test
FCC	Federal Communications Commission
ISED	Innovation, Science and Economic Development Canada
RBW	Resolution bandwidth
RMS	Root mean square
VBW	Video bandwidth
V_{NOM}	Nominal supply voltage

REPORT INDEX

1 Equipment (Test Item) Under Test 6
1.1 Photos – Equipment External 7
1.2 Photos – Equipment Internal 9
1.3 Photos – Test Setup 11
1.4 Support Equipment 14
1.5 Test Modes 15
1.6 Test Frequencies 16
1.7 Sample emission level calculation 17
2 Result Summary 18
3 Test Conditions and Results 19
3.1 Test Conditions and Results - Occupied bandwidth 19
3.2 Test Conditions and Results - 6 dB bandwidth 24
3.3 Test Conditions and Results - Maximum peak conducted output power 29
3.4 Test Conditions and Results - Power spectral density 31
3.5 Test Conditions and Results - Band-edge compliance 36
3.6 Test Conditions and Results - Conducted spurious emissions 40
3.7 Test Conditions and Results - Transmitter radiated emissions 45
3.8 Test Conditions and Results - Receiver radiated emissions 48

ANNEX A Transmitter spurious emissions 51
ANNEX B Receiver spurious emissions 91

1 Equipment (Test Item) Under Test

Description	Hygiene-Monitoring-System	
Model	NosoEx Point of Care / Drucksensor	
Additional Model(s)	None	
Brand Name(s)	None	
Serial Number(s)	201903000000002 (conducted sample) 201903000000005 (radiated sample)	
Hardware Version(s)	1.7.1	
Software Version(s)	2.17	
PMN	n/a	
HVIN	n/a	
FVIN	n/a	
HMN	n/a	
FCC-ID	2AU27NOSOEX002	
IC	n/a	
Equipment type	End Product	
Radio type	Transceiver	
Assigned frequency bands	2400 - 2483.5 MHz	
Radio technology	Bluetooth LE	
Modulation	GFSK	
Number of antenna ports	1	
Antenna	Type	Integrated antenna
	Model	PCB Antenna DN007
	Manufacturer	GWA Hygiene GmbH
	Gain	3.3dBi
Supply Voltage	V_{NOM}	3.0 VDC
Operating Temperature	T_{NOM}	20 °C
AC/DC-Adaptor	N/A	
Manufacturer	GWA Hygiene GmbH Heinrich-Mann-Str. 11 18435 Stralsund GERMANY	

1.1 Photos – Equipment External

EUT top view

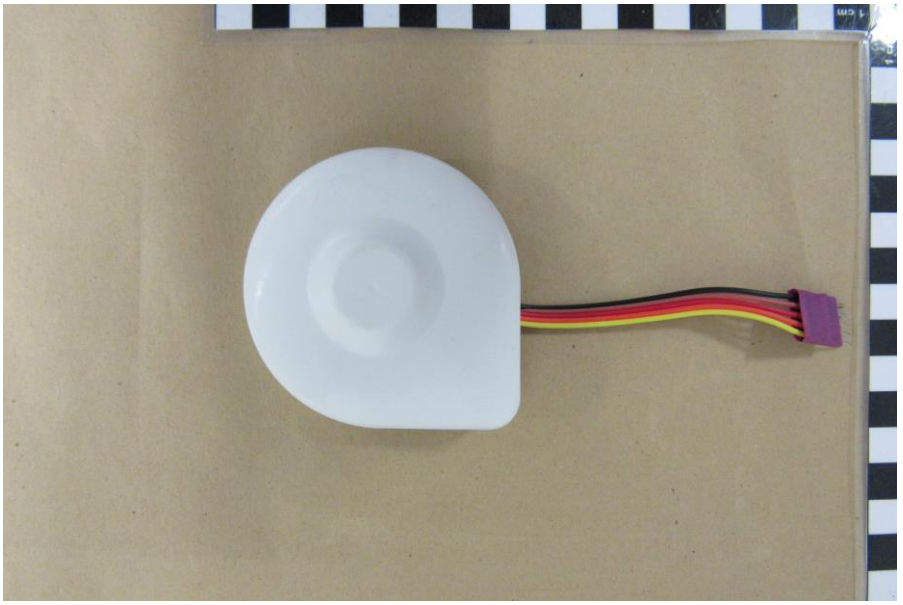

EUT bottom view

Auxiliary Equipment - Programming board
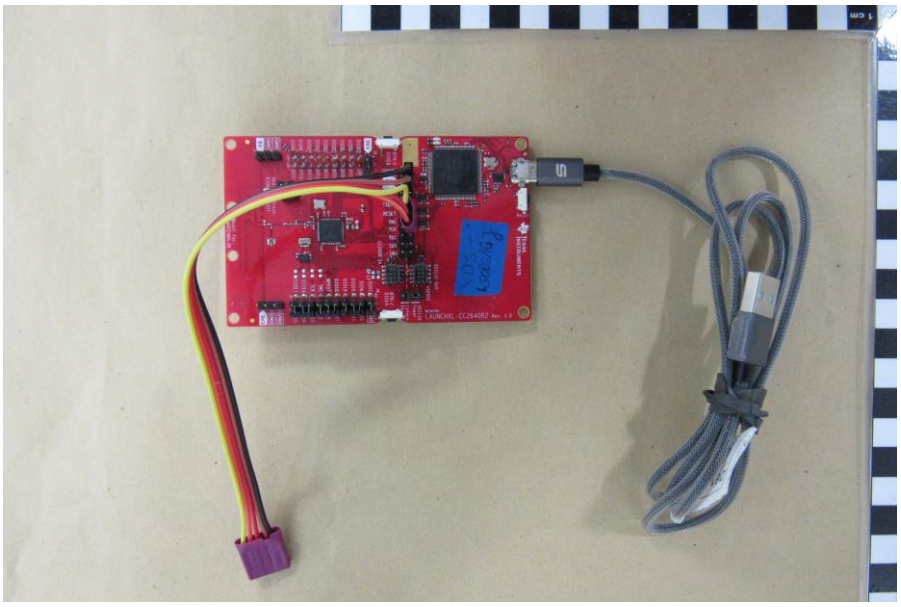

1.2 Photos – Equipment Internal

EUT top cover - back view
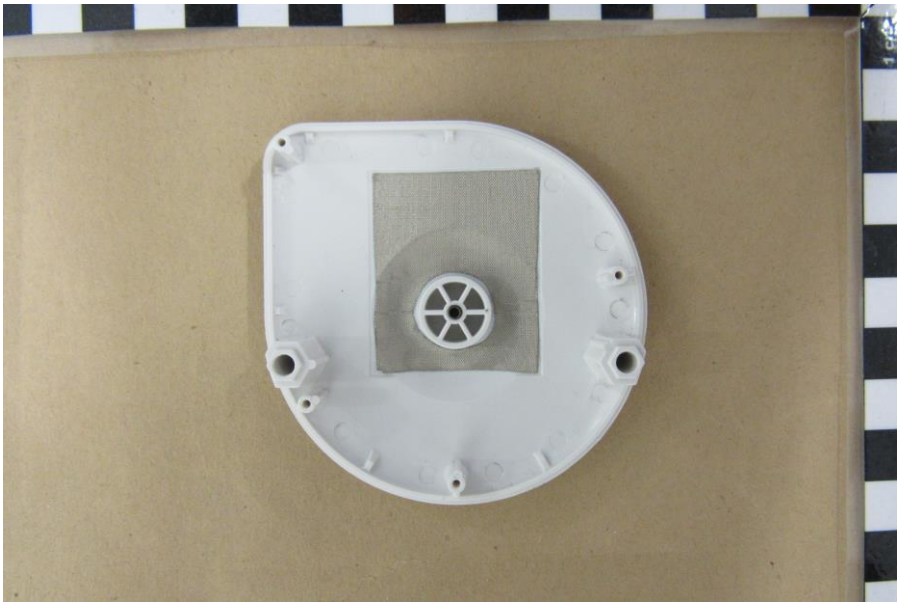

EUT PCB top view
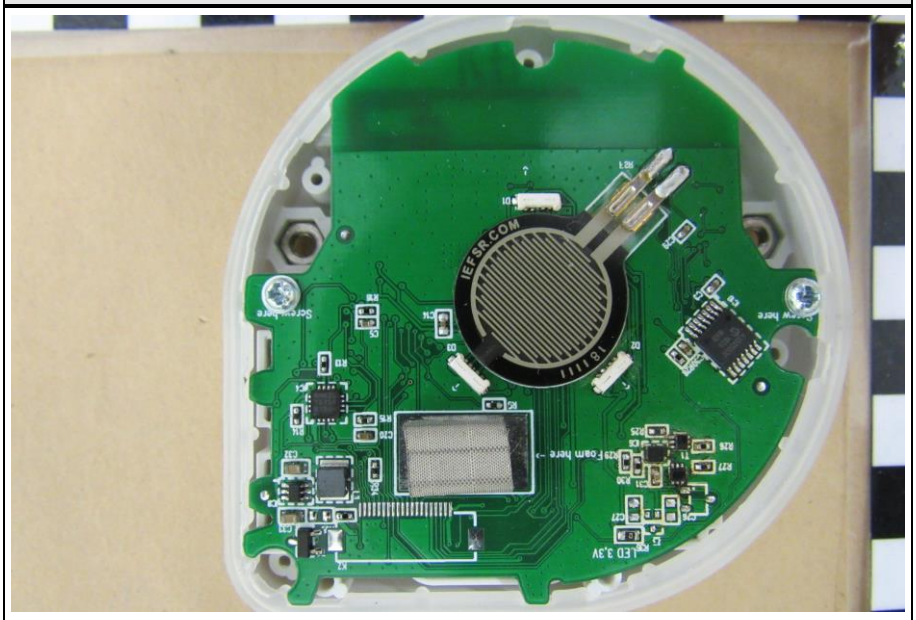

EUT PCB bottom view

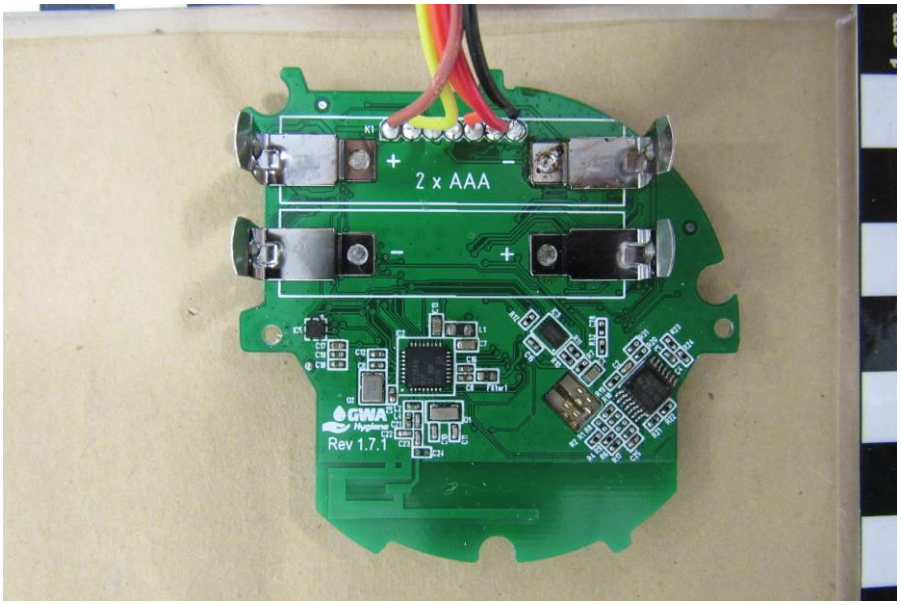

1.3 Photos – Test Setup

Test Setup close view below 1 GHz
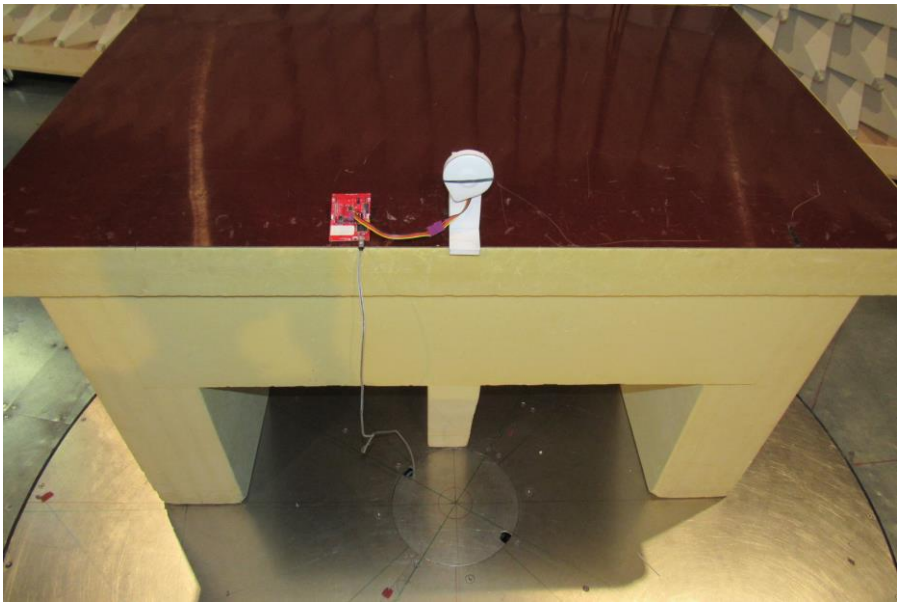

Test Setup 30 - 200 MHz
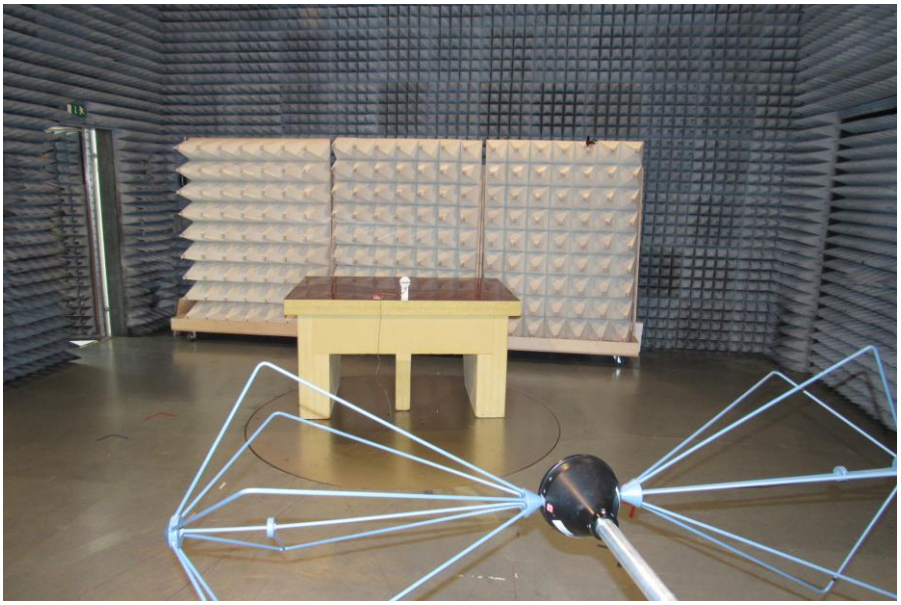

Test Setup 200 - 1000 MHz

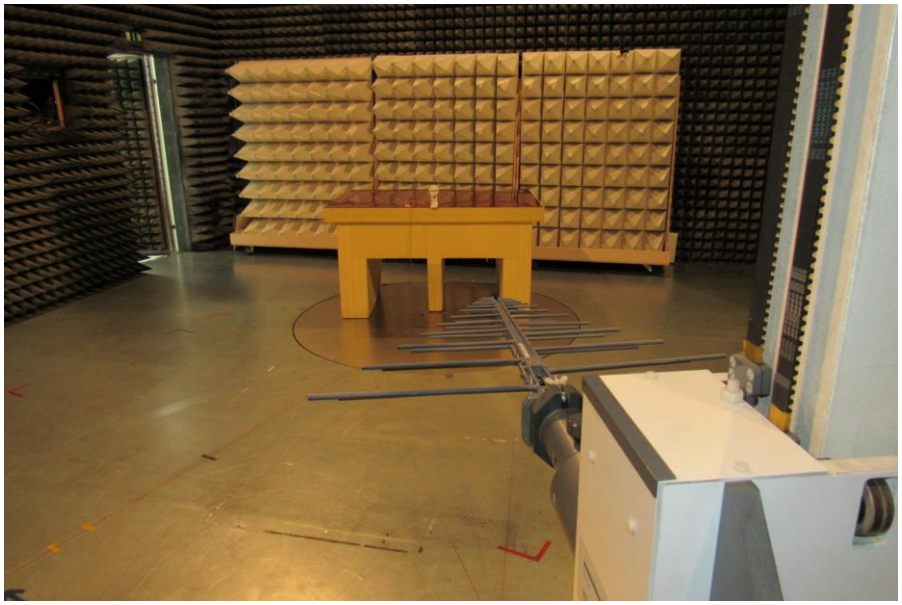

Test Setup close view above 1 GHz

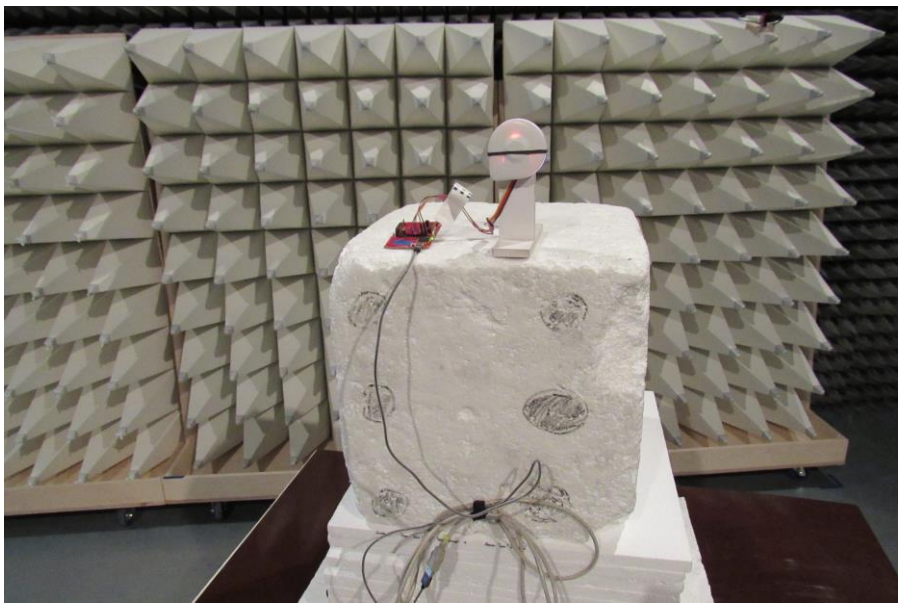

Test Setup 1 - 17 GHz

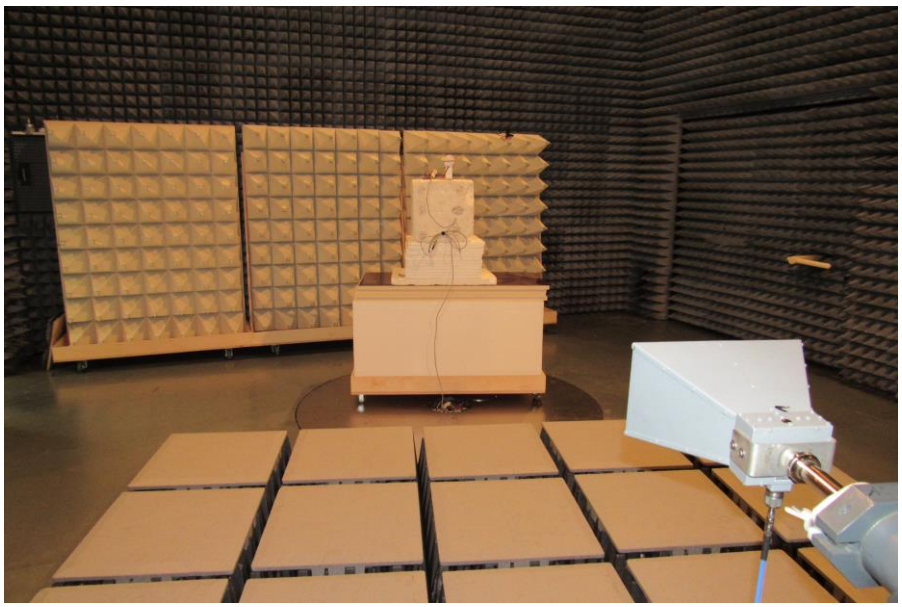

Test Setup 17 - 26 GHz

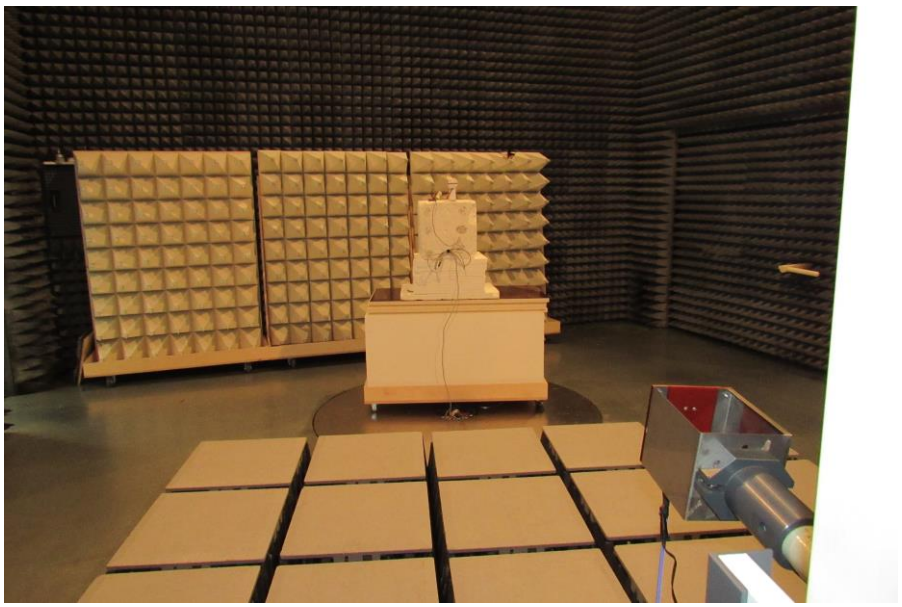

1.4 Support Equipment

Product Type	Device	Manufacturer	Model	Comment
AE	Notebook	Lenovo	ThinkPad T510	
AE	Power Supply AC Adapter	Liteon	ADLX90NLC3A	
CBL	Active USB cable	---	~10m	Setting test modes on EUT and supplying it with power
AE	RF Evaluation Module for Test modes	Texas Instruments	Launchpad CC2640(R2F)	Setting test modes on EUT and supplying it with power
Description:				
AE	Auxiliary Equipment			
SIM	Simulator			
CBL	Connecting Cable			
SFT	Software			
Comment:				

1.5 Test Modes

Mode	Description
GFSK	Mode = Transmit Modulation = GFSK Spreading = None Duty cycle = 100% Data rate = 1Mbit/s (according to customer request) Power setting = 2dBm (software setting)
Receive	Mode = Receive
Comment:	

1.6 Test Frequencies

Designator	Mode	Channel	Frequency [MHz]
F1	Tx / Rx	0	2402
F2	Tx / Rx	19	2440
F3	Tx / Rx	39	2480

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dBµV. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

Reading on Analyzer (dBµV) + A.F. (dB/m) = Net field strength (dBµV/m)

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dBµV/m). The FCC limits are given in units of µV/m. The following formula is used to convert the units of µV/m to dBµV/m:

Limit (dBµV/m) = 20*log (µV/m)

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

Reading + AF	= Net Reading	:	Net reading - FCC limit	= Margin
+21.5 dBµV + 26 dB/m	= 47.5 dBµV/m	:	47.5 dBµV/m - 57.0 dBµV/m	= -9.5 dB

2 Result Summary

FCC 47 CFR Part 15C, ISED RSS-247				
Product Standard Reference	**Requirement**	**Reference Method**	**Result**	**Remarks**
ISED RSS-Gen, Issue 5 (section 6.6)	Occupied Bandwidth	ANSI C63.10-2013	N/R	Informational only
FCC § 15.247(a)(2) ISED RSS-247, Issue 2 (section 5.2)	6 dB Bandwidth	ANSI C63.10-2013	PASS	
FCC § 15.247(b)(1) ISED RSS-247, Issue 2 (section 5.4)	Maximum peak conducted power	ANSI C63.10-2013	PASS	
FCC § 15.247(e) ISED RSS-247, Issue 2 (section 5.2)	Power spectral density	ANSI C63.10-2013	PASS	
FCC § 15.207 ISED RSS-247, Issue 2 (section 3.1)	AC power line conducted emissions	ANSI C63.10-2013	N/R	Can operate from battery only
FCC § 15.247(d) ISED RSS-247, Issue 2 (section 5.5)	Band edge compliance	ANSI C63.10-2013	PASS	
FCC § 15.247(d) ISED RSS-247, Issue 2 (section 5.5)	Conducted spurious emissions	ANSI C63.10-2013	PASS	
FCC § 15.247(d) FCC § 15.209 ISED RSS-Gen, Issue 5 (section 6.13)	Transmitter radiated spurious emissions	ANSI C63.10-2013	PASS	
ISED RSS-247, Issue 2 (section 3.1)	Receiver radiated spurious emissions	ANSI C63.10-2013	PASS	
Comment:				

Possible Test Case Verdicts	
PASS	Test object does meet the requirements
FAIL	Test object does not meet the requirements
N/T	Required by standard but not tested
N/R	Not required by standard for the test object

3 Test Conditions and Results

3.1 Test Conditions and Results - Occupied bandwidth

3.1.1 Information

Test Information	
Reference	ISED RSS-Gen, Issue 5 (section 6.6)
Measurement Method	ANSI C63.10 6.9.3
Operator	Florian Voigt
Date	2020-04-06

3.1.2 Limits

Limits
None (Informational only)

3.1.3 Setup

Test Setup


3.1.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.1.5 Procedure

Test Procedure
1. EUT transmitter is activated in test mode under normal conditions 2. The spectrum analyzer is set to peak detection and maximum hold with a span twice the emission spectrum 3. The resolution bandwidth is set to the range of 1 % to 5 % of the occupied bandwidth 4. The occupied bandwidth is measured with the build-in analyzer function

3.1.6 Results

Test Results		
Mode	Frequency [MHz]	Bandwidth [MHz]
GFSK	2402	1.050
GFSK	2440	1.060
GFSK	2480	1.050

Occupied Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 6.9.3
Operational Mode:	GFSK, Channel: 0, 2402 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Occupied Bandwidth [MHz]:	1.050

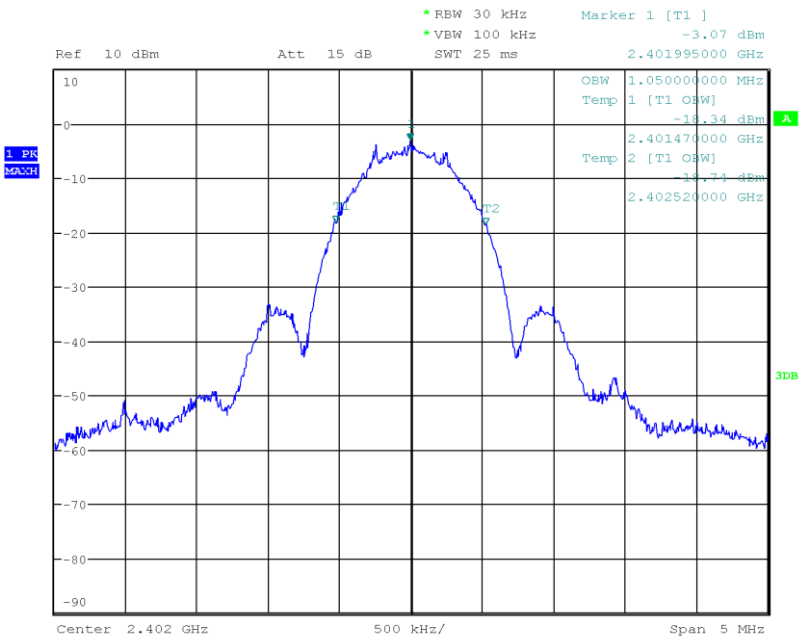

Occupied Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 6.9.3
Operational Mode:	GFSK, Channel: 19, 2440 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Occupied Bandwidth [MHz]:	1.060

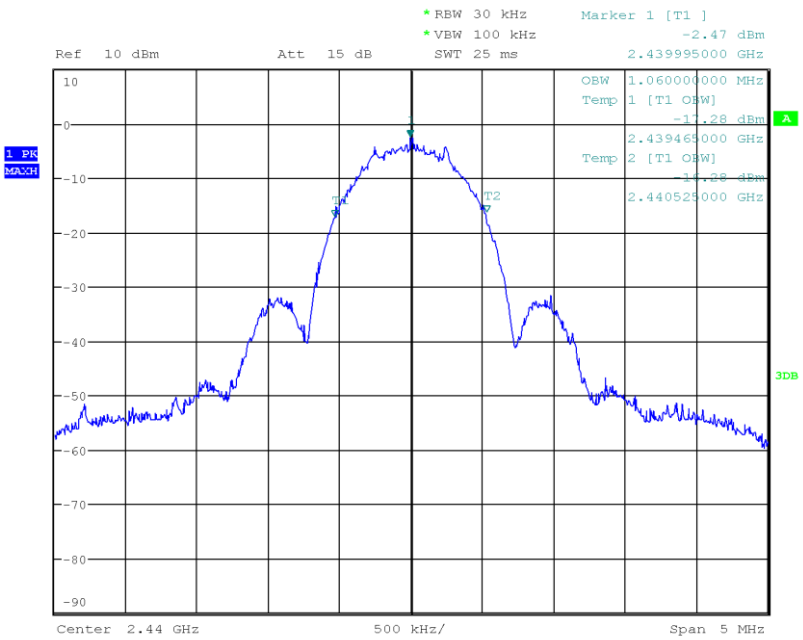

Occupied Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 6.9.3
Operational Mode:	GFSK, Channel: 39, 2480 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Occupied Bandwidth [MHz]:	1.050

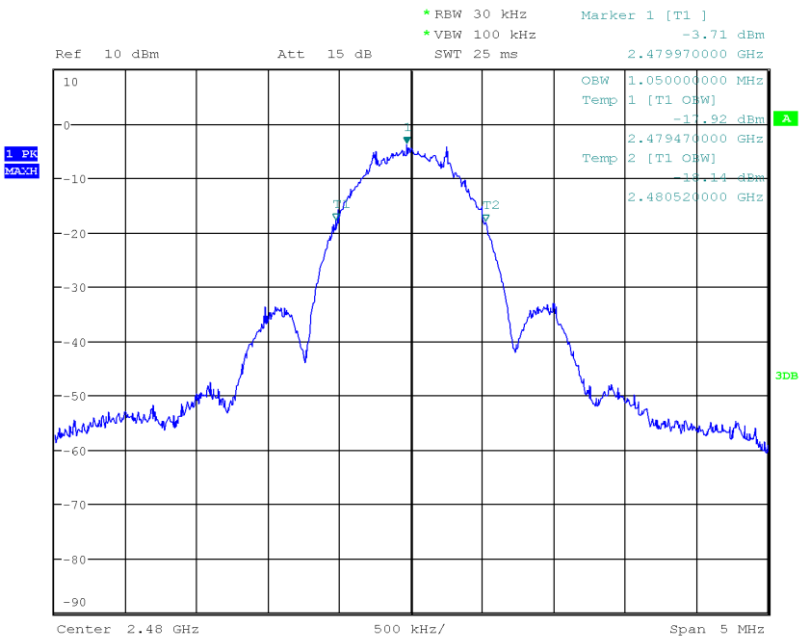

Date: 6.APR.2020 13:35:38

3.2 Test Conditions and Results - 6 dB bandwidth

3.2.1 Information

Test Information	
Reference	FCC § 15.247(a)(2); ISED RSS-247, Issue 2 (section 5.2)
Measurement Method	ANSI C63.10 11.8
Operator	Florian Voigt
Date	2020-04-06

3.2.2 Limits

Limits
≥ 500kHz

3.2.3 Setup

Test Setup


3.2.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.2.5 Procedure

Test Procedure
1. EUT set to test mode 2. Span set to at least twice the emission spectrum 3. Detector set to peak and max hold and RBW is set to 100 kHz 4. Envelope peak value of emission spectrum is selected 5. Marker on envelope of spectrum is set to level of -6 dB to the left of the peak 6. Marker on envelope of spectrum is set to level of -6 dB to the right of the peak 7. 6 dB Bandwidth is determined by marker frequency separation

3.2.6 Results

Test Results				
Mode	Frequency [MHz]	Bandwidth [kHz]	Limit [kHz]	Verdict
GFSK	2402	695	500	PASS
GFSK	2440	715	500	PASS
GFSK	2480	715	500	PASS

DTS (6 dB) Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.8.1 Option 1
Operational Mode:	GFSK, Channel: 0, 2402 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Lower Frequency [MHz]:	2401.650
Upper Frequency [MHz]:	2402.345
6 dB Bandwidth [kHz]:	695

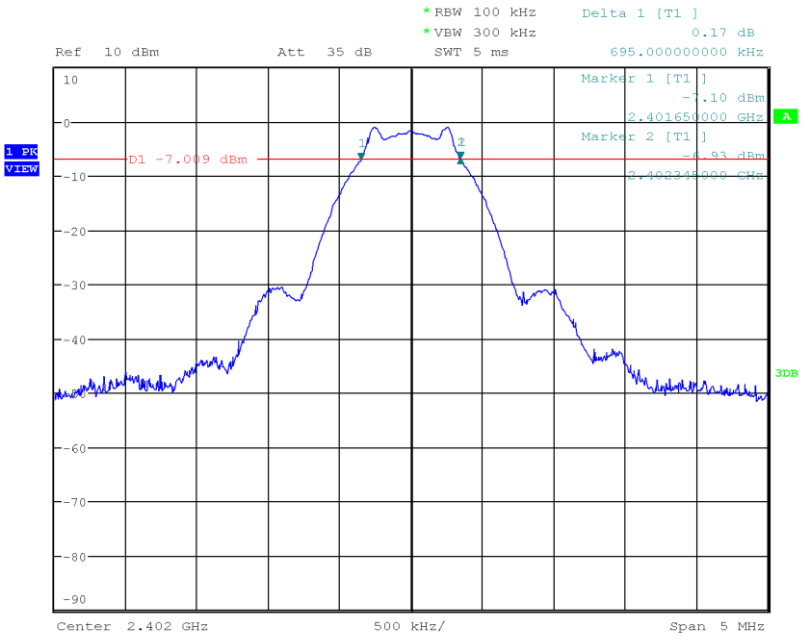

DTS (6 dB) Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.8.1 Option 1
Operational Mode:	GFSK, Channel: 19, 2440 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Lower Frequency [MHz]:	2439.635
Upper Frequency [MHz]:	2440.350
6 dB Bandwidth [kHz]:	715

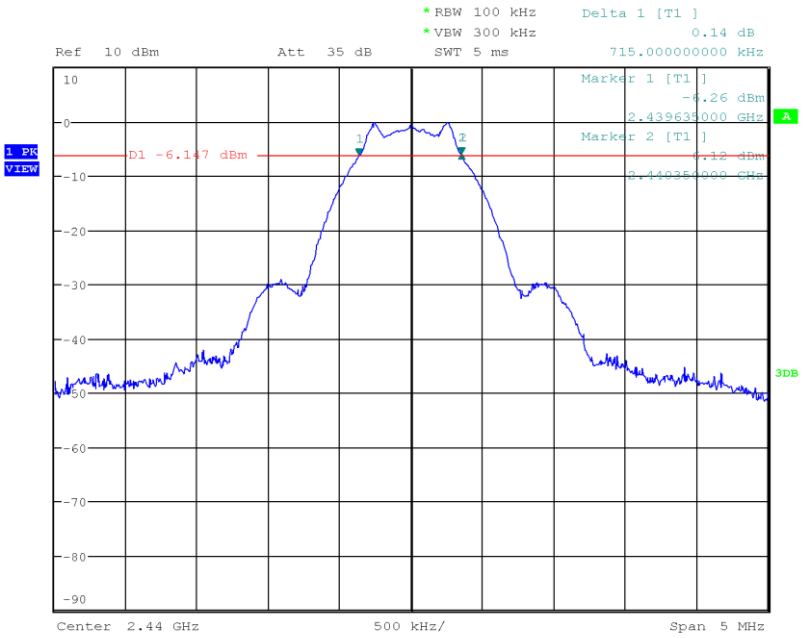

DTS (6 dB) Bandwidth

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.8.1 Option 1
Operational Mode:	GFSK, Channel: 39, 2480 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Lower Frequency [MHz]:	2479.630
Upper Frequency [MHz]:	2480.345
6 dB Bandwidth [kHz]:	715

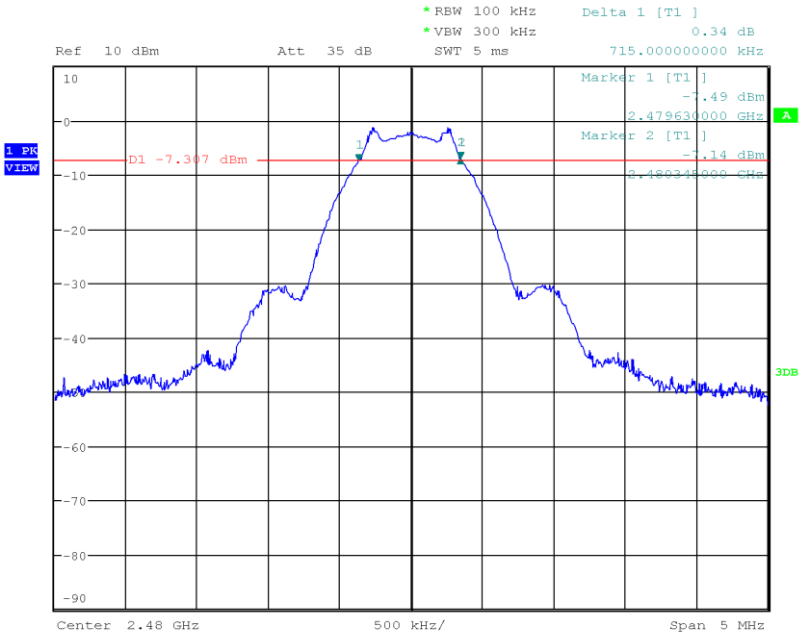

3.3 Test Conditions and Results - Maximum peak conducted output power

3.3.1 Information

Test Information	
Reference	FCC § 15.247(b)(1); ISED RSS-247, Issue 2 (section 5.4)
Measurement Method	ANSI C63.10 11.9.1
Operator	Florian Voigt
Date	2020-04-06

3.3.2 Limits

Limits
1 W (30 dBm)
The conducted output power limit specified above is based on the use of antennas with directional gains that do not exceed 6 dBi. If transmitting antennas of directional gain greater than 6 dBi are used, the conducted output power from the intentional radiator shall be reduced below the stated values in the table, as appropriate, by the amount in dB that the directional gain of the antenna exceeds 6 dBi.

3.3.3 Setup

Test Setup



3.3.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.3.5 Procedure

Test Procedure
1. EUT set to test mode (Communication tester is used if needed) 2. Analyzer resolution bandwidth is set ≥ DTS bandwidth 3. Detector set to peak and max hold 4. Sweep time is set to auto 5. After the trace has stabilized a marker is set to peak of envelope

3.3.6 Results

Test Results				
Channel [MHz]	Power [dBm]	Power [W]	Limit [W]	Verdict
2402	-0.171	0.0010	1.0	PASS
2440	0.879	0.0012	1.0	PASS
2480	-0.200	0.0010	1.0	PASS

3.4 Test Conditions and Results - Power spectral density

3.4.1 Information

Test Information	
Reference	FCC § 15.247(e); ISED RSS-247, Issue 2 (section 5.2)
Measurement Method	ANSI C63.10 11.10.2, 14.3.2
Operator	Florian Voigt
Date	2020-04-06

3.4.2 Limits

Limits
8 dBm / 3 kHz

3.4.3 Setup

Test Setup


3.4.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.4.5 Procedure

Test Procedure
1. EUT set to test mode 2. The analyzer is set to DTS channel center frequency with a span of 1.5 times the DTS bandwidth 3. The RBW is set to 100 kHz with VBW ≥ RBW and the detector is set to peak with max hold 4. After the trace has stabilized a marker is set to the envelope maximum 5. If the power spectral density is above the limit the RBW is reduced (not lower than 3 kHz) and the measurement is repeated 6. If the EUT has more than one transmit chain the procedure is repeated for each transmit chain

3.4.6 Results

Test Results			
Channel [MHz]	PSD [dBm/RBW]	Limit [dBm/3kHz]	Verdict
2402	-0.585	8.0	PASS
2440	0.308	8.0	PASS
2480	-0.790	8.0	PASS
RBW = 100 kHz			

Peak Power Spectral Density

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.10.2
Operational Mode:	GFSK, Channel: 0, 2402 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Peak Frequency [MHz]:	2402.240
Spectral Density [dBm/RBW]:	-0.585
Resolution Bandwidth [kHz]:	100 kHz

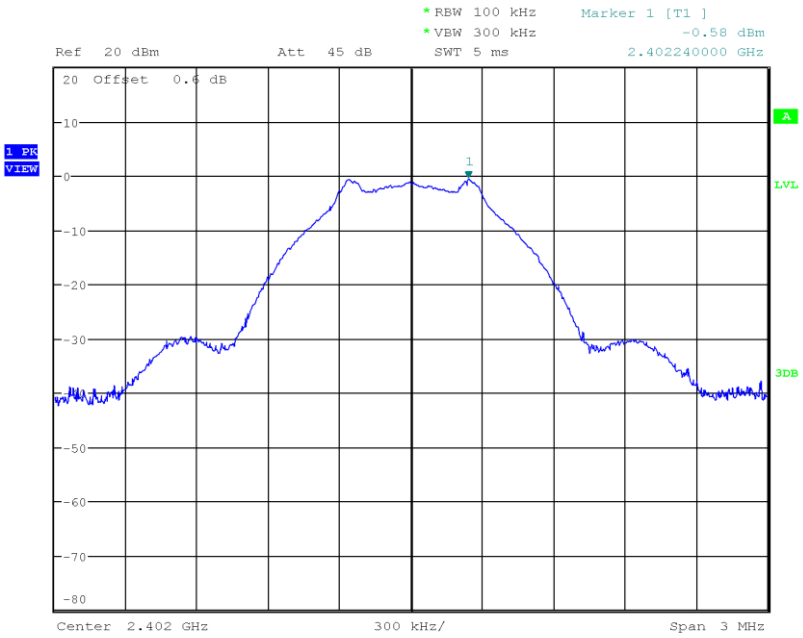

Peak Power Spectral Density

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.10.2
Operational Mode:	GFSK, Channel: 19, 2440 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Peak Frequency [MHz]:	2440.252
Spectral Density [dBm/RBW]:	0.308
Resolution Bandwidth [kHz]:	100 kHz

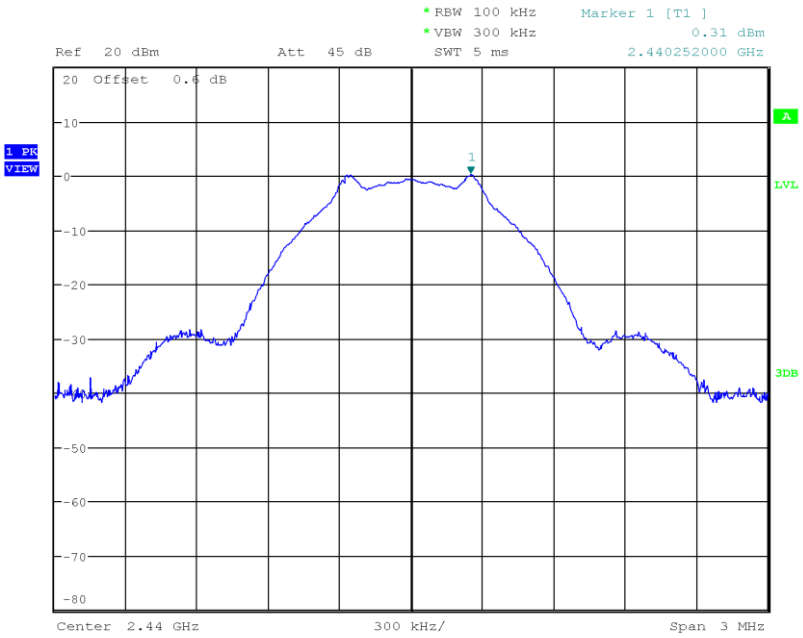

Peak Power Spectral Density

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.10.2
Operational Mode:	GFSK, Channel: 39, 2480 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Peak Frequency [MHz]:	2480.261
Spectral Density [dBm/RBW]:	-0.790
Resolution Bandwidth [kHz]:	100 kHz

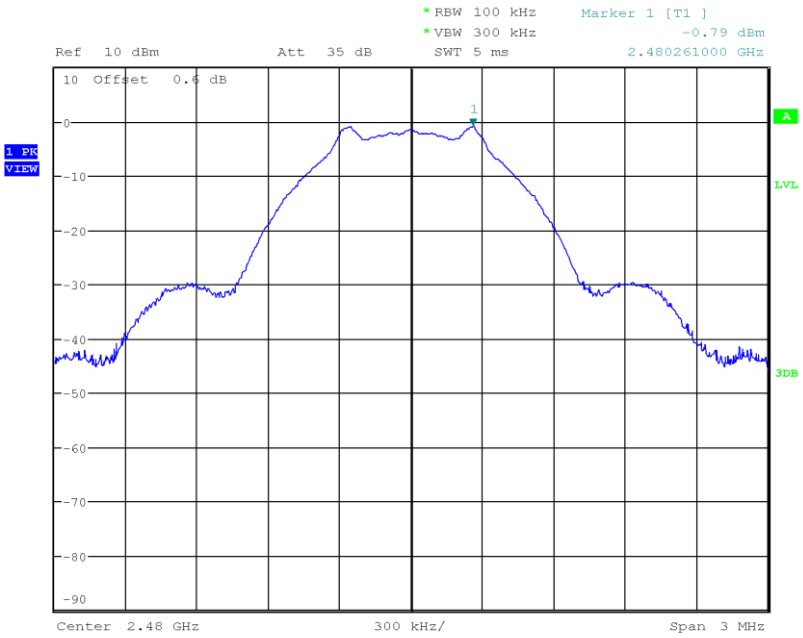

3.5 Test Conditions and Results - Band-edge compliance

3.5.1 Information

Test Information	
Reference	FCC § 15.247(d); ISED RSS-247, Issue 2 (section 5.5)
Measurement Method	ANSI C63.10 11.13
Operator	Florian Voigt
Date	2020-04-06

3.5.2 Limits

Limits	
Power Measurement	Out-of-band attenuation [dB]
Peak	20
RMS	30

3.5.3 Setup

Test Setup



3.5.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.5.5 Procedure

Test Procedure

1. EUT set to test mode (Communication tester is used if needed)
2. Span set around lower band edge and detector is set to peak and max hold
3. Resolution bandwidth is set to 100 kHz
4. Markers are set to peak emission levels within frequency band and outside frequency band
5. Band edge attenuation is determined from level difference

3.5.6 Results

Test Results				
Mode	Channel [MHz]	Out-of-band Attenuation [dB]	Limit [dB]	Verdict
GFSK	2402	-39.34	-20	PASS
GFSK	2480	-39.02	-20	PASS

Emissions in nonrestricted frequency bands at the Band-edge

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 7.8.6, 6.10.4
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Band-edge	Lower
In-band Frequency [MHz]:	2401.76
Max. in-band Level [dBm/100 kHz]:	-0.696
Out-of-band Frequency [MHz]:	2397.856
Max. out-of-band Level [dBm/100 kHz]:	-40.032
Attenuation [dB]:	-39.34

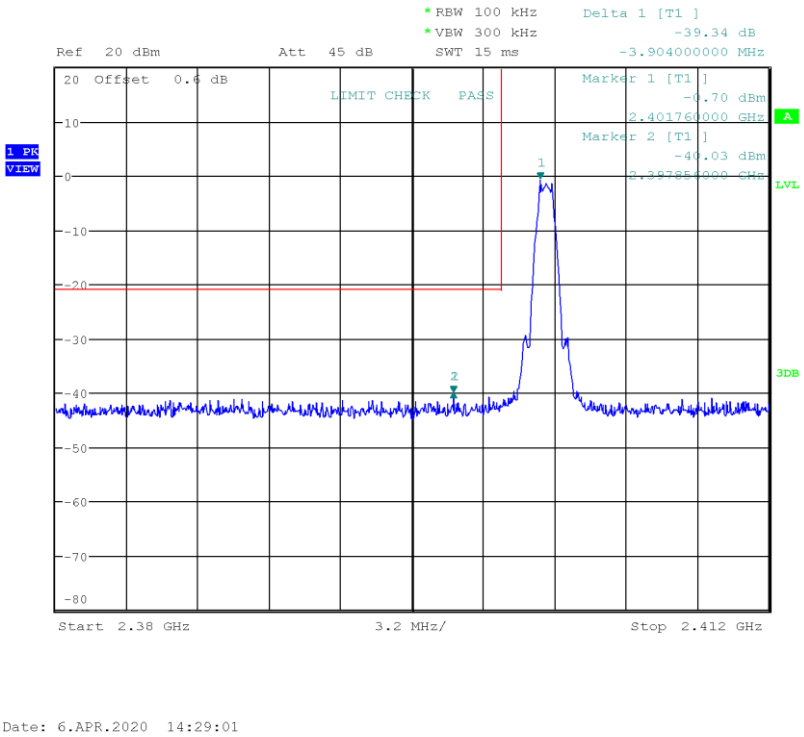

Emissions in nonrestricted frequency bands at the Band-edge

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 7.8.6, 6.10.4
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Band-edge	Upper
In-band Frequency [MHz]:	2480.255
Max. in-band Level [dBm/100 kHz]:	-1.27
Out-of-band Frequency [MHz]:	2496.705
Max. out-of-band Level [dBm/100 kHz]:	-40.288
Attenuation [dB]:	-39.02

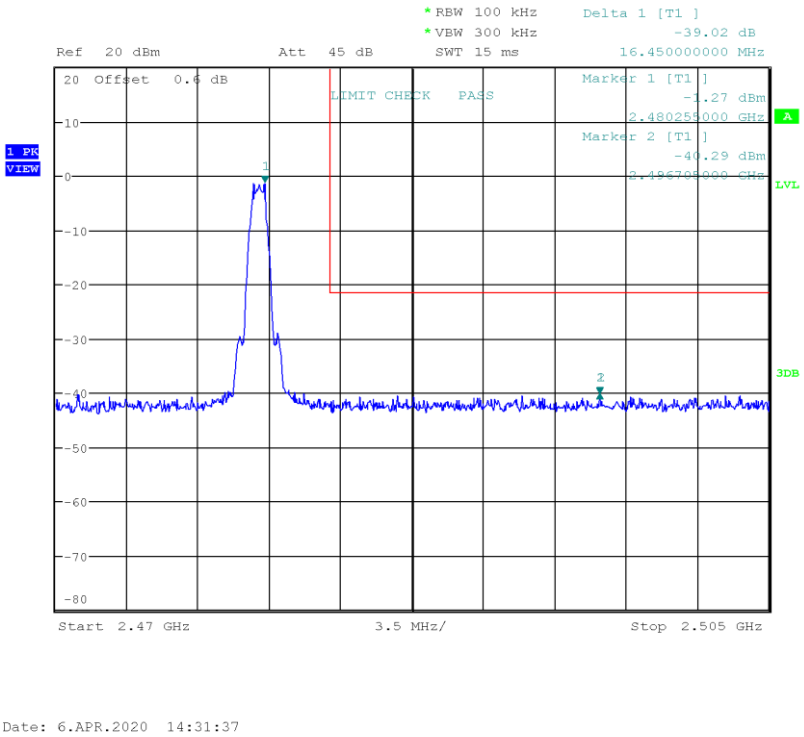

3.6 Test Conditions and Results - Conducted spurious emissions

3.6.1 Information

Test Information	
Reference	FCC § 15.247(d); ISED RSS-247, Issue 2 (section 5.5)
Measurement Method	ANSI C63.10 11.11
Operator	Florian Voigt
Date	2020-04-06

3.6.2 Limits

Limits	
Power Measurement	Out-of-band attenuation [dB]
Peak	20
RMS	30

3.6.3 Setup

Test Setup



3.6.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum analyzer	R&S	FSU43	EF01631	2019-12	2020-12

3.6.5 Procedure

Test Procedure

1. EUT set to test mode (Communication tester is used if needed)
2. Span set around lower band edge and detector is set to peak and max hold
3. Resolution bandwidth is set to 100 kHz
4. Markers are set to peak emission levels within frequency band and outside frequency band
5. Band edge attenuation is determined from level difference

3.6.6 Results

Test Results		
Mode	Channel [MHz]	Verdict
GFSK	2402	PASS
GFSK	2440	PASS
GFSK	2480	PASS

Conducted Spurious Emissions

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.11
Operational Mode:	GFSK, Channel: 0, 2402 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Max. in-band Frequency [MHz]:	2401.7
Max. in-band Level [dBm/100 kHz]:	-1.2
Out-of-band Limit [dBm/100 kHz]:	-21.2

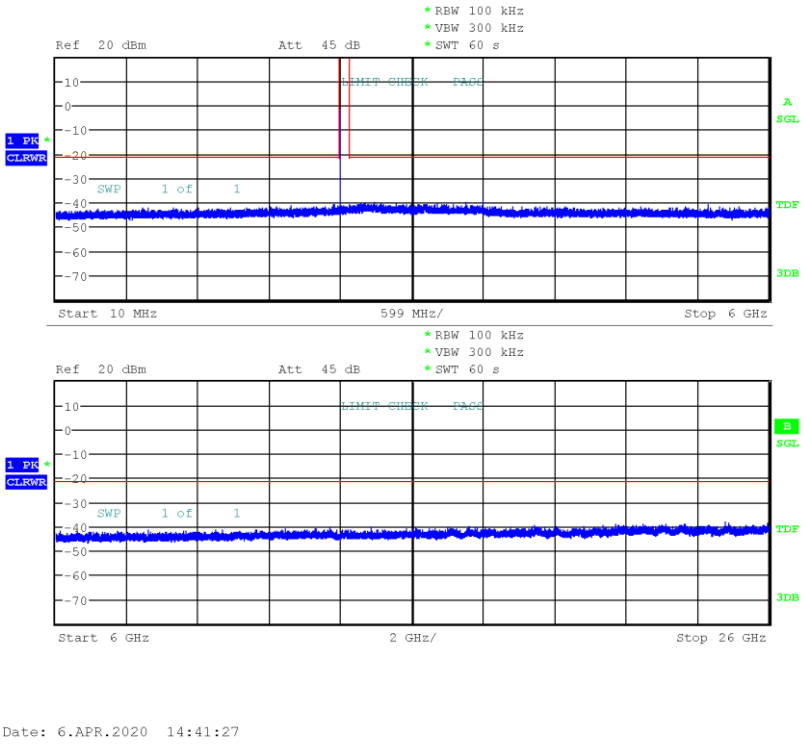

Conducted Spurious Emissions

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.11
Operational Mode:	GFSK, Channel: 19, 2440 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Max. in-band Frequency [MHz]:	2440.2
Max. in-band Level [dBm/100 kHz]:	-0.0
Out-of-band Limit [dBm/100 kHz]:	-20.0

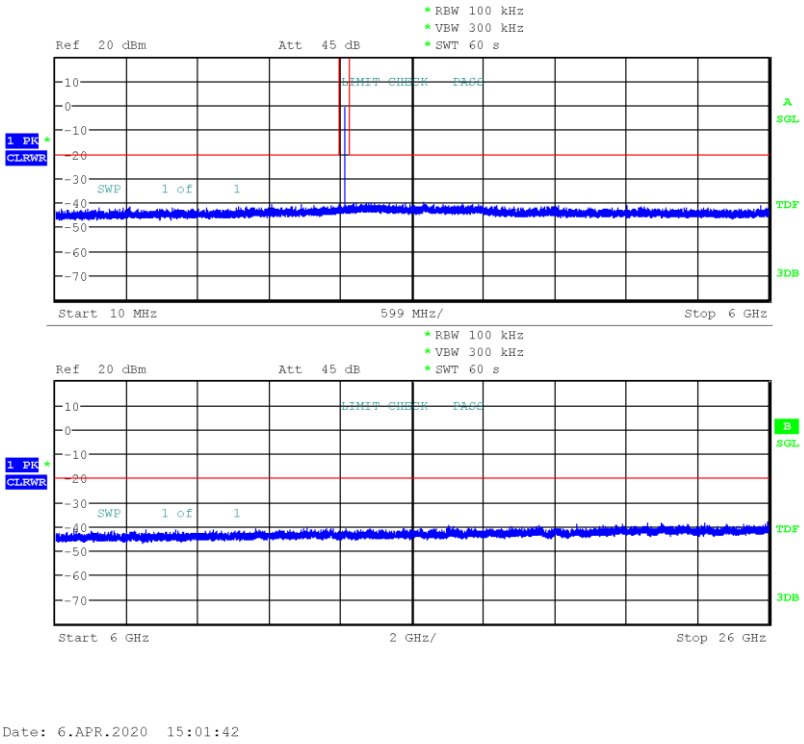

Conducted Spurious Emissions

Project Number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
Model Description:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Sample ID:	28703
Reference Standards:	FCC 15.247, RSS-247
Reference Method:	ANSI C63.10:2013, Section 11.11
Operational Mode:	GFSK, Channel: 39, 2480 MHz
Operating Conditions:	Tnom/Vnom
Operator:	Florian Voigt
Test Site:	Eurofins Product Service GmbH
Test Date:	2020-04-06
Max. in-band Frequency [MHz]:	2479.7
Max. in-band Level [dBm/100 kHz]:	-1.3
Out-of-band Limit [dBm/100 kHz]:	-21.3

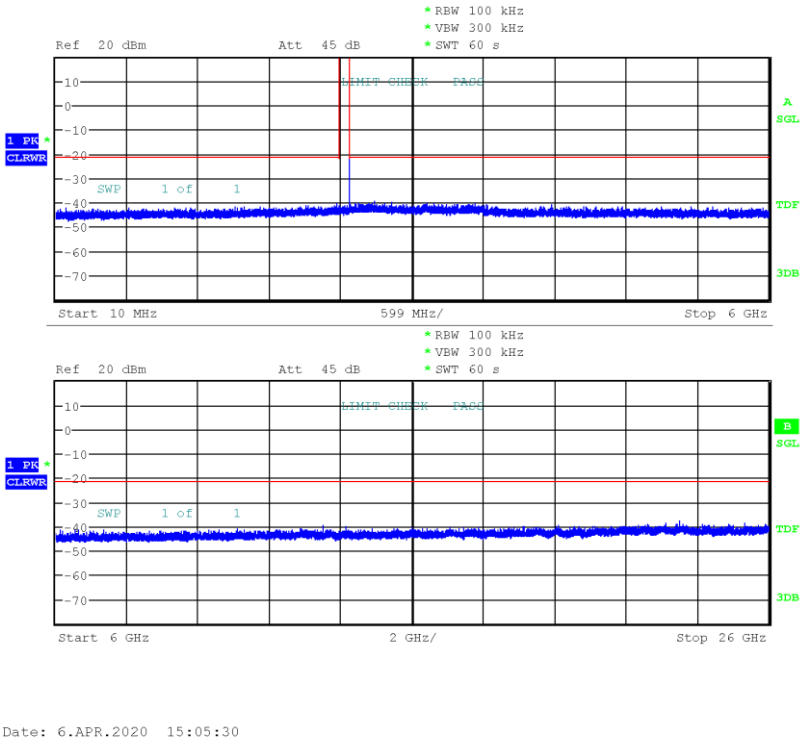

3.7 Test Conditions and Results - Transmitter radiated emissions

3.7.1 Information

Test Information	
Reference	FCC § 15.247(d); FCC § 15.209; ISED RSS-Gen, Issue 5 (section 6.13)
Measurement Method	ANSI C63.10 6.4, 6.5, 6.6, 11.12
Operator	Florian Voigt
Date	2020-04-06 – 2020-04-08

3.7.2 Limits

Limits			
Frequency [MHz]	Detector	Field strength [µV/m]	Measurement distance [m]
0.009 - 0.09	Average	2400/F[kHz]	300
0.09 - 0.110	Quasi-Peak	2400/F[kHz]	300
0.110 - 0.490	Average	2400/F[kHz]	300
0.490 - 1.705	Quasi-Peak	24000/F[kHz]	30
1.705 - 30.0	Quasi-Peak	30	30
30 - 88	Quasi-Peak	100	3
88 - 216	Quasi-Peak	150	3
216 - 960	Quasi-Peak	200	3
960 - 1000	Quasi-Peak	500	3
>1000	Average	500	3

3.7.3 Setup

Test Setup 30 - 1000 MHz

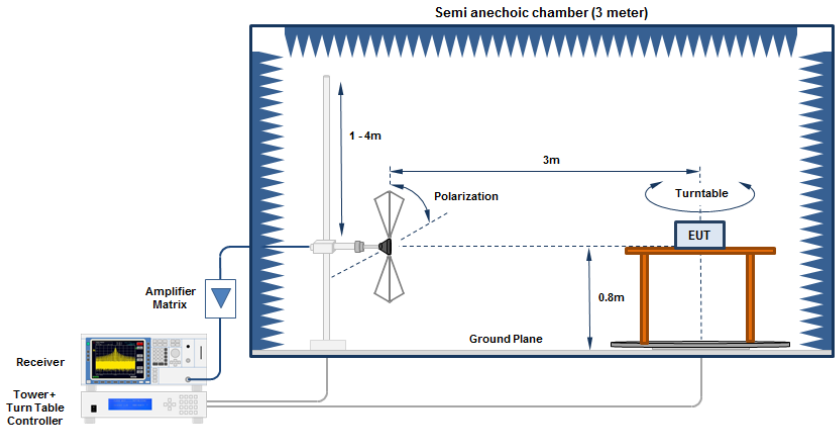

Test Setup > 1 GHz
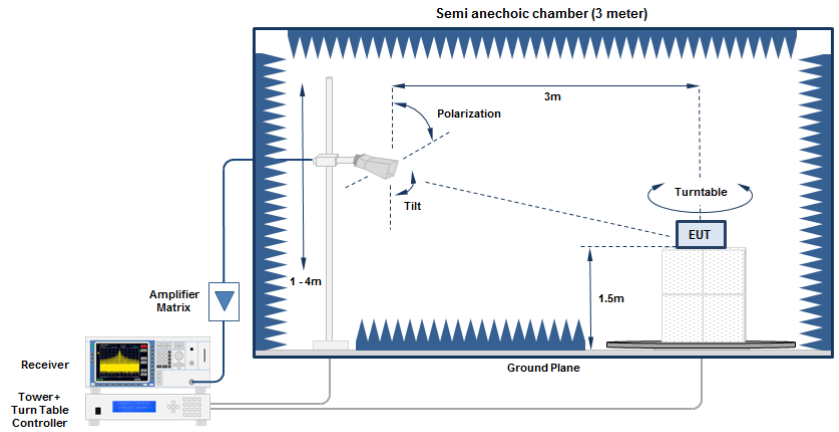

3.7.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2016.1.10

Test Equipment 30 - 1000 MHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00062	2018-07	2021-07
Measurement Receiver	Agilent	N9038A-526/WXP	EF01070	2019-09	2020-09
Antenna	R&S	HK 116	EF00030	2019-04	2022-04
Antenna	R&S	HL 223	EF00187	2019-05	2022-05

Test Equipment > 1 GHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00062	2018-07	2021-07
Measurement Receiver	Agilent	N9038A-526/WXP	EF01070	2019-09	2020-09
Antenna	Schwarzbeck	BBHA 9120D	EF00018	2019-10	2022-10
Antenna	Amplifier Research	AT4560	EF00302	2019-05	2020-05

3.7.5 Procedure

Test Procedure 30 - 1000 MHz
1. EUT is placed on a non conducting support at the center of a turn table 0.8 m above the ground 2. EUT set to test mode 3. The receiver is set to peak detection with max hold 4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m 5. All significant emissions are measured again using the corresponding final detector

Test Procedure > 1 GHz
1. EUT is placed on a non conducting support at the center of a turn table 1.5 m above the ground
2. EUT set to test mode
3. The receiver is set to peak detection with max hold
4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m
5. All significant emissions are measured again using the corresponding final detector

3.7.6 Results

Test Results						
Channel [MHz]	Emission [MHz]	Level [dBµV/m]	Det.	Pol.	Limit [dBµV/m]	Margin [dB]
2402	119.389	28.39	qpk	ver	43.52	-15.13
2402	240	25.86	pk	hor	46.00	-20.14
2402	240	25.33	pk	ver	46.00	-20.67
2402	2378	36.56	RMS	hor	54.00	-17.44
2402	2378	37.81	RMS	ver	54.00	-16.19
2402	4804	43.79	RMS	hor	54.00	-10.21
2402	4804	48.00	RMS	ver	54.00	-06.00
2440	240	27.34	pk	ver	46.00	-18.66
2440	960	29.74	pk	ver	54.00	-24.26
2440	4880	44.78	pk	hor	74.00	-29.22
2440	4881	48.09	pk	ver	74.00	-25.91
2440	4881	45.49	RMS	ver	54.00	-08.51
2440	7319	50.70	pk	ver	74.00	-23.30
2440	7319	47.04	RMS	ver	54.00	-06.96
2440	7321	50.65	pk	hor	74.00	-23.35
2440	7321	46.82	RMS	hor	54.00	-07.18
2480	240	22.80	pk	hor	46.00	-23.20
2480	240	26.89	pk	ver	46.00	-19.11
2480	2483.5	47.95	RMS	hor	54.00	-06.05
2480	2483.5	49.91	RMS	ver	54.00	-04.09
2480	4960	44.18	pk	hor	74.00	-29.82
2480	4960	47.19	pk	ver	74.00	-26.81
2480	4960	44.41	RMS	ver	54.00	-09.59
2480	7441	49.05	pk	hor	74.00	-24.95
2480	7441	44.94	RMS	hor	54.00	-09.06
2480	7441	49.65	pk	ver	74.00	-24.35
2480	7441	45.96	RMS	ver	54.00	-08.04

3.8 Test Conditions and Results - Receiver radiated emissions

3.8.1 Information

Test Information	
Reference	ISED RSS-247, Issue 2 (section 3.1)
Measurement Method	ANSI C63.10 6.5, 6.6, 11.12
Operator	Florian Voigt
Date	2020-04-07

3.8.2 Limits

Limits			
Frequency [MHz]	Detector	Field strength [µV/m]	Measurement distance [m]
30 - 88	Quasi-Peak	100	3
88 - 216	Quasi-Peak	150	3
216 - 960	Quasi-Peak	200	3
960 - 1000	Quasi-Peak	500	3
>1000	Average	500	3

3.8.3 Setup

Test Setup 30 - 1000 MHz

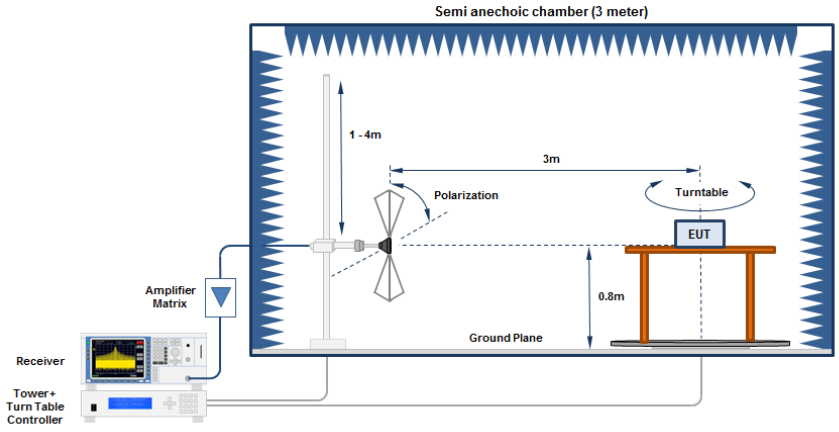

Test Setup > 1 GHz
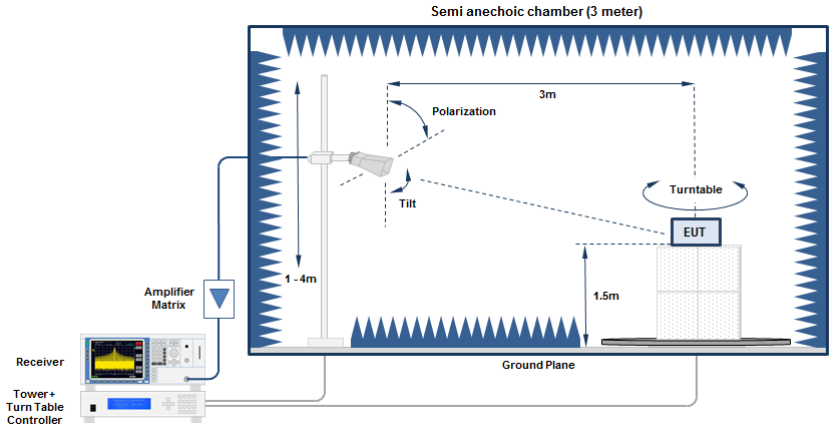

3.8.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2016.1.10

Test Equipment 30 - 1000 MHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00062	2018-07	2021-07
Measurement Receiver	Agilent	N9038A-526/WXP	EF01070	2019-09	2020-09
Antenna	R&S	HK 116	EF00030	2019-04	2022-04
Antenna	R&S	HL 223	EF00187	2019-05	2022-05

Test Equipment > 1 GHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00062	2018-07	2021-07
Measurement Receiver	Agilent	N9038A-526/WXP	EF01070	2019-09	2020-09
Antenna	Schwarzbeck	BBHA 9120D	EF00018	2019-10	2022-10

3.8.5 Procedure

Test Procedure 30 - 1000 MHz
1. EUT is placed on a non conducting support at the center of a turn table 0.8 m above the ground 2. EUT set to test mode 3. The receiver is set to peak detection with max hold 4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m 5. All significant emissions are measured again using the corresponding final detector

Test Procedure > 1 GHz
1. EUT is placed on a non conducting support at the center of a turn table 1.5 m above the ground 2. EUT set to test mode 3. The receiver is set to peak detection with max hold 4. The EUT is rotated through 360° and the height of the antenna is varied from 1 m to 4 m 5. All significant emissions are measured again using the corresponding final detector

3.8.6 Results

Test Results						
Channel [MHz]	Emission [MHz]	Level [dBµV/m]	Det.	Pol.	Limit [dBµV/m]	Margin [dB]
2440	4872	39.33	pk	hor	53.98	-14.65
2440	4872	39.22	pk	ver	53.98	-14.76

ANNEX A Transmitter spurious emissions

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 45

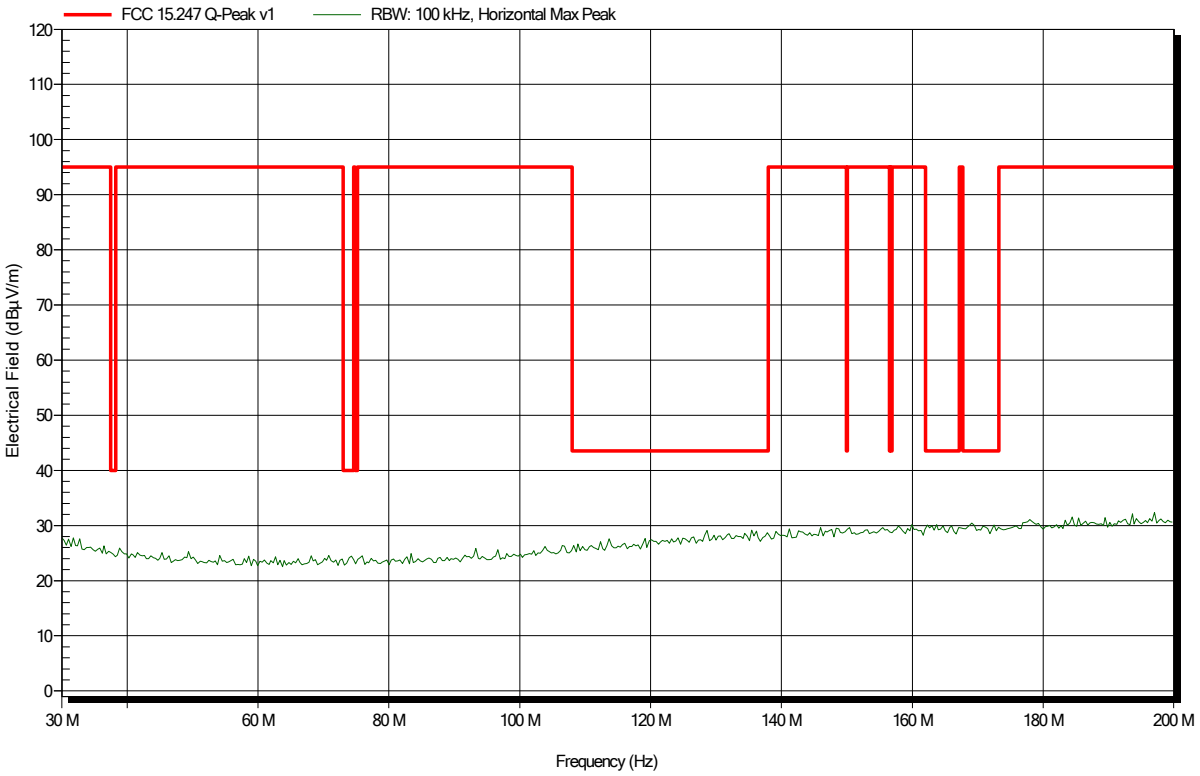

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 43

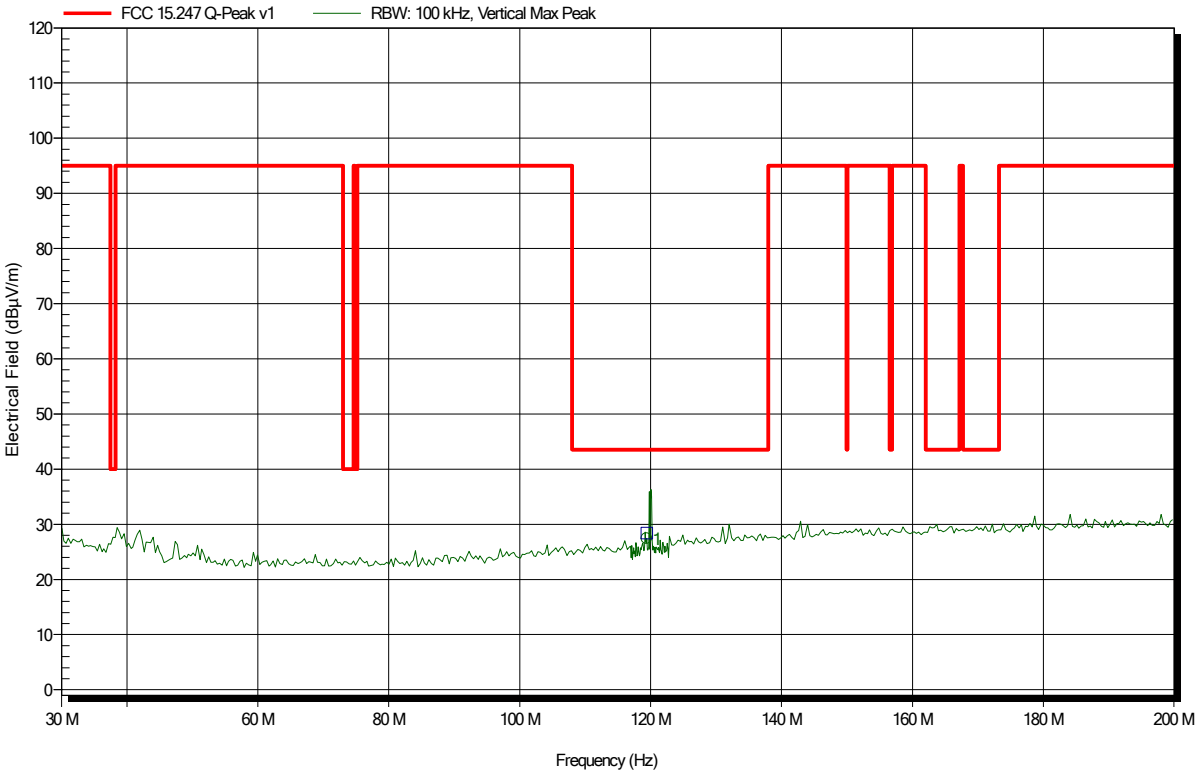

Frequency	Peak	Peak Limit	Peak Difference	Status
119.389 MHz	27.41 dBµV/m	---	---	---

Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
119.389 MHz	28.39 dBµV/m	43.52 dBµV/m	-15.13 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 42

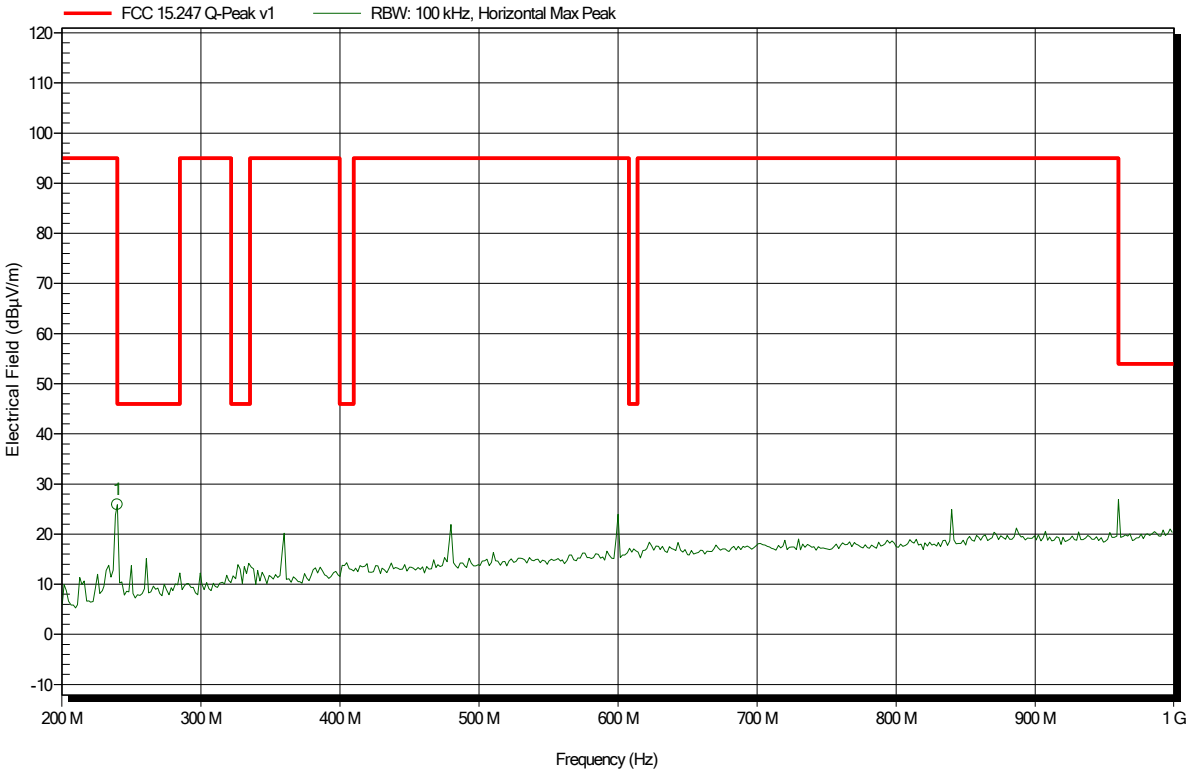

Frequency	Peak	Peak Limit	Peak Difference	Status
240 MHz	25.86 dBµV/m	46 dBµV/m	-20.14 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 38

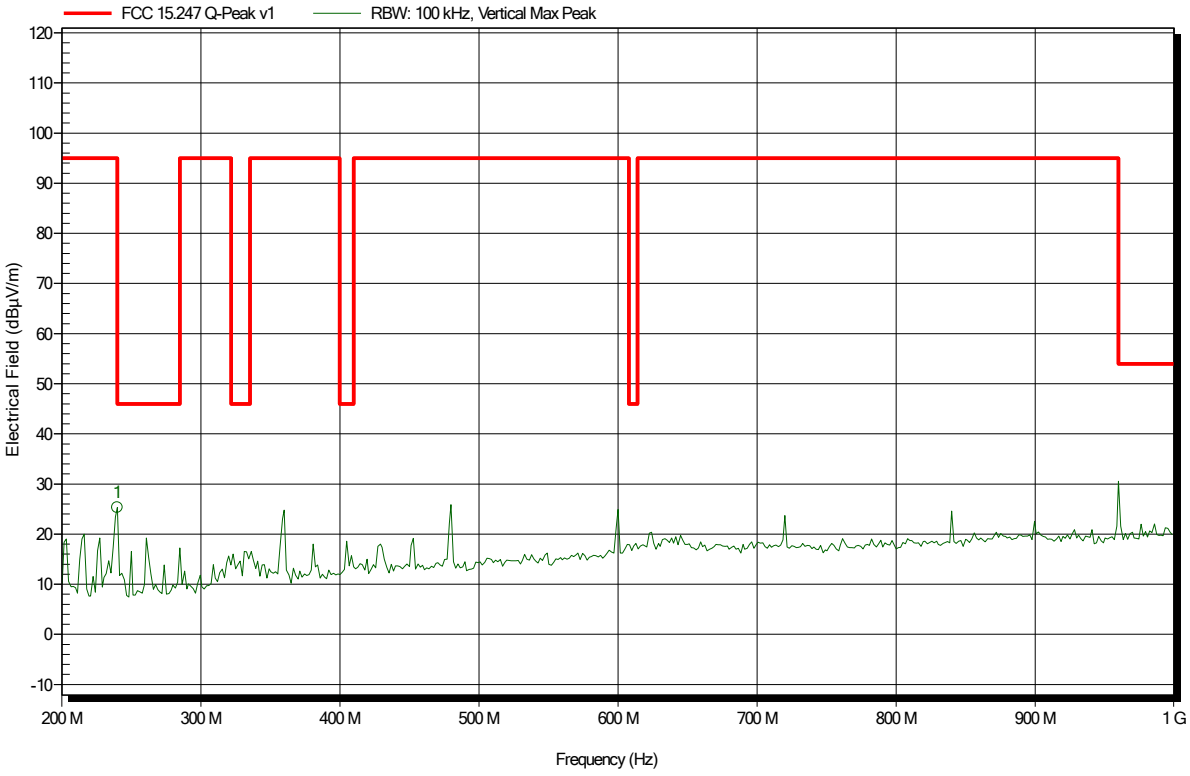

Frequency	Peak	Peak Limit	Peak Difference	Status
240 MHz	25.33 dBµV/m	46 dBµV/m	-20.67 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 14

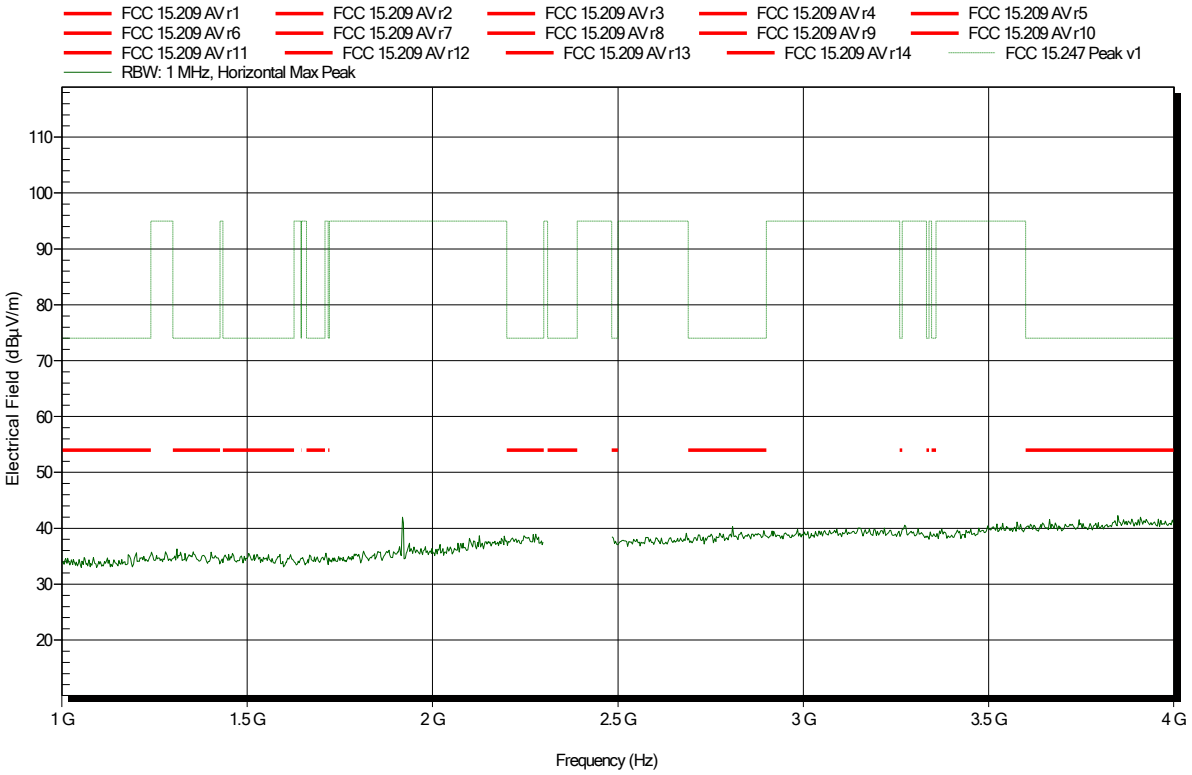

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 6

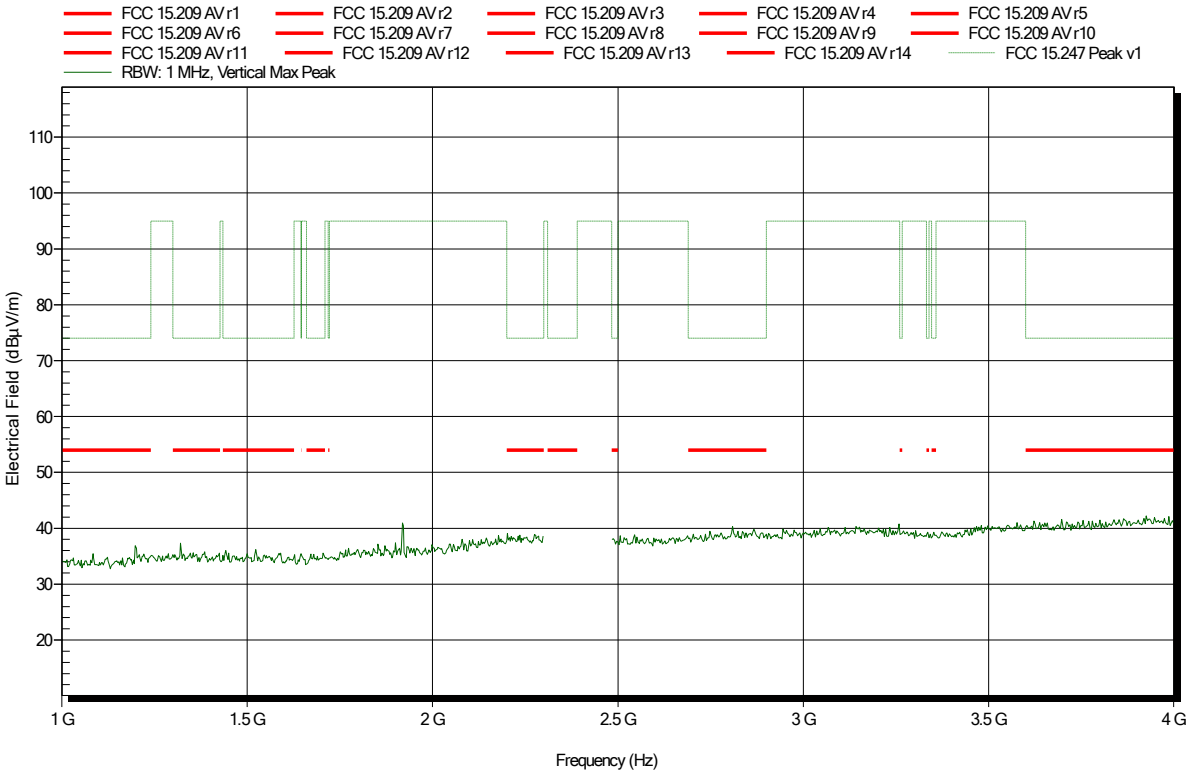

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 15

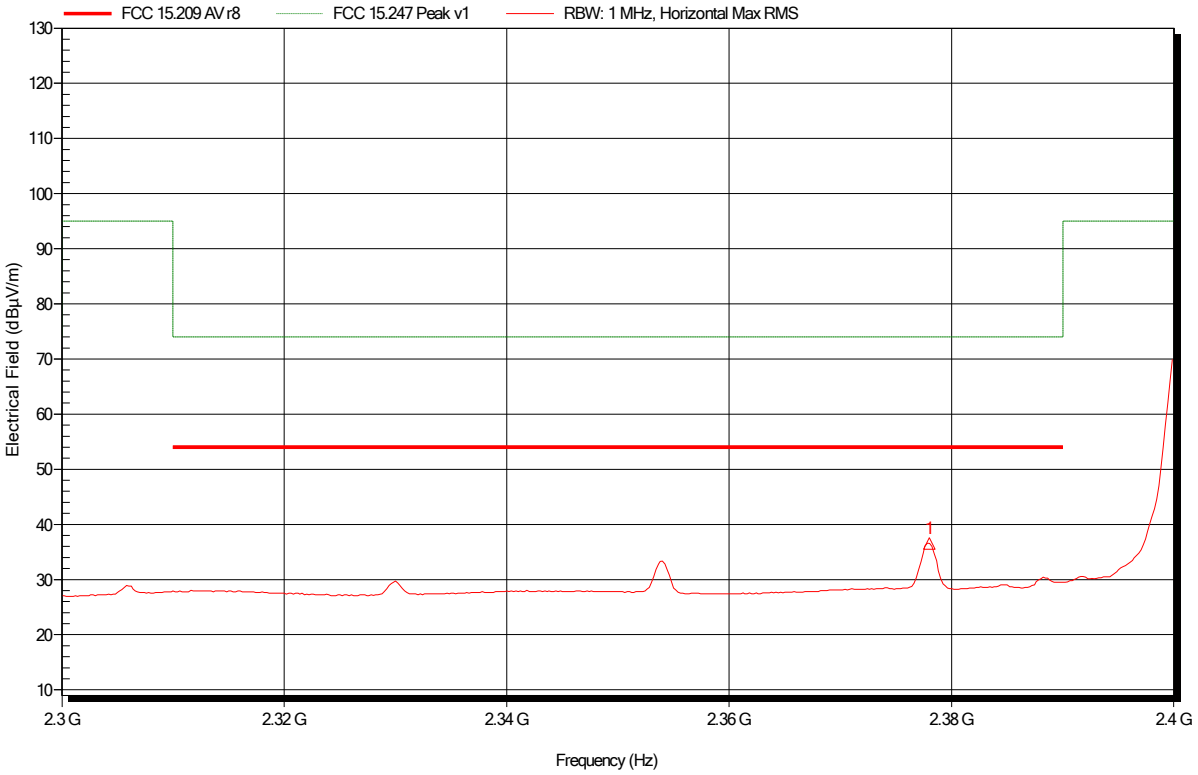

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
2.378 GHz	36.56 dBµV/m	54 dBµV/m	-17.44 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 7

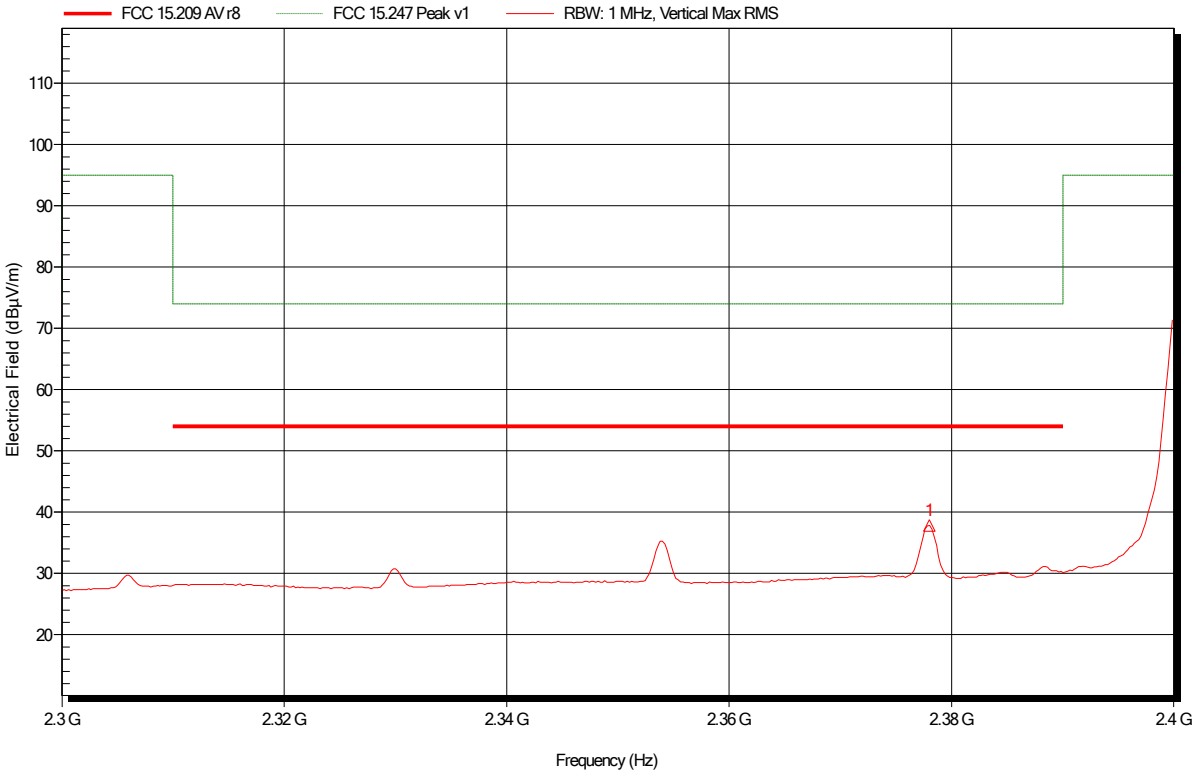

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
2.378 GHz	37.81 dBµV/m	54 dBµV/m	-16.19 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 17

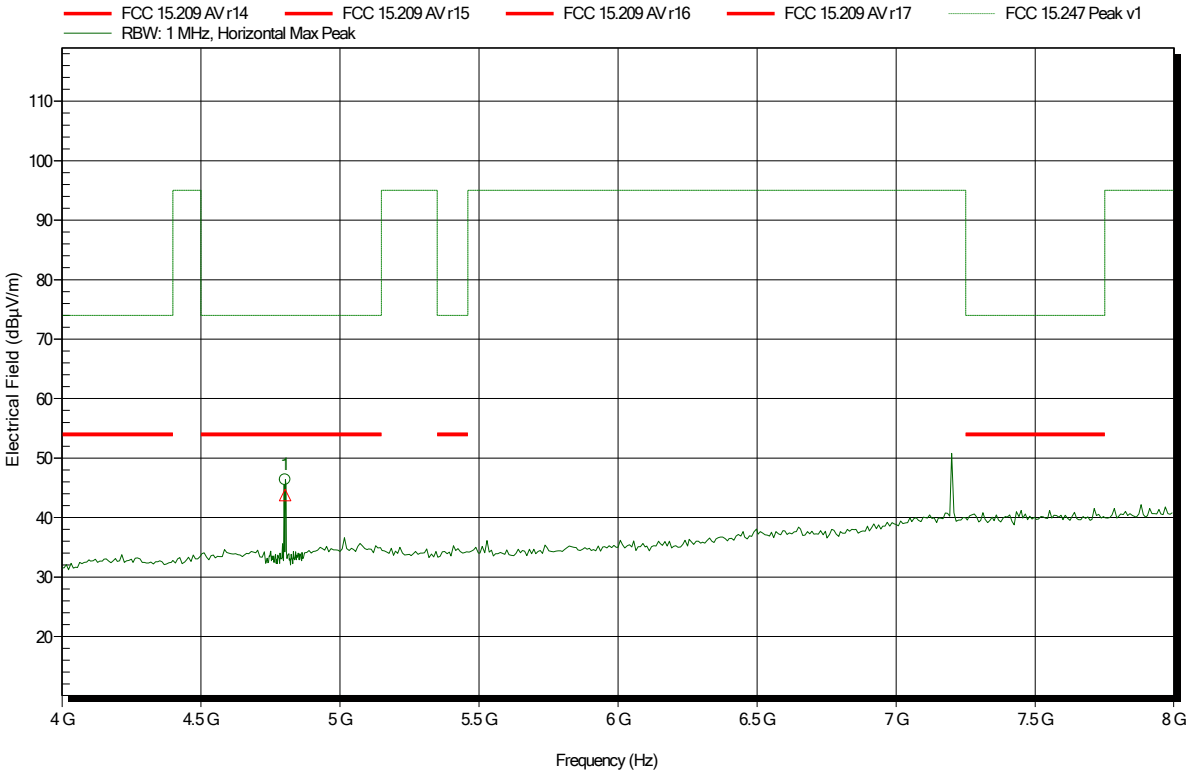

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.804 GHz	46.39 dBµV/m	---	---	---

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
4.804 GHz	43.79 dBµV/m	54 dBµV/m	-10.21 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 28

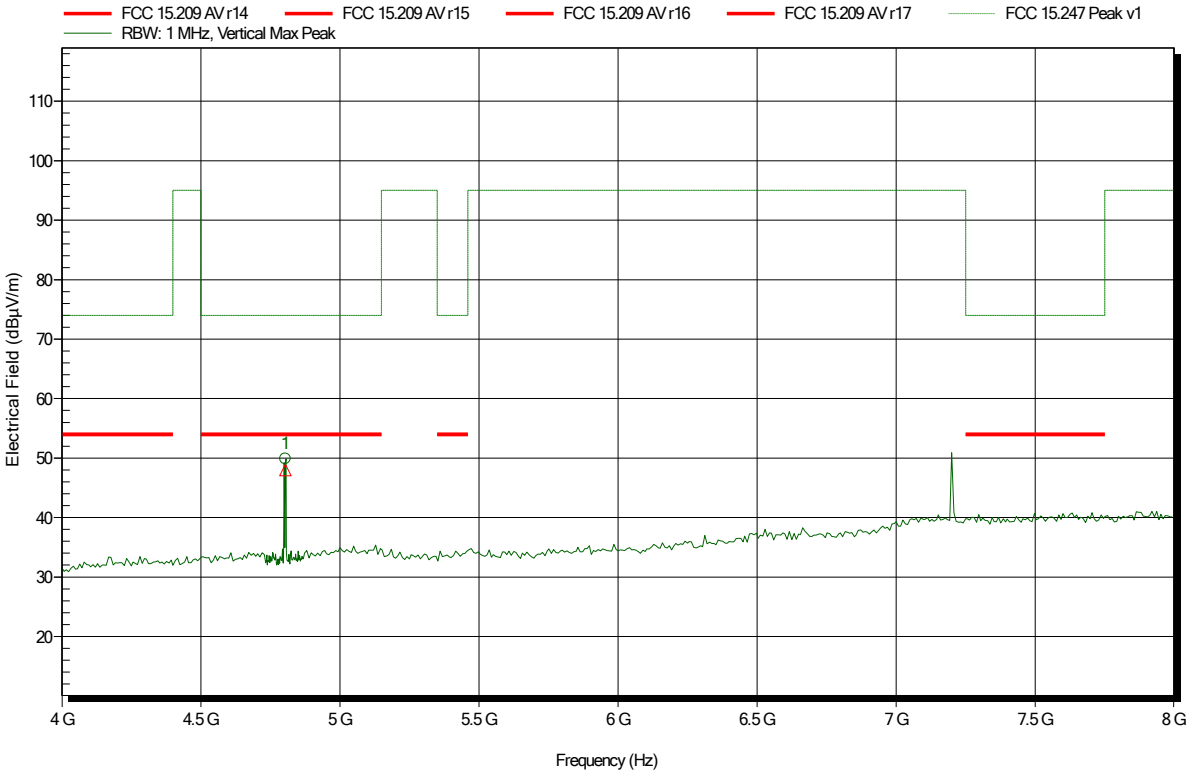

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.804 GHz	49.89 dBµV/m	---	---	---

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
4.804 GHz	48 dBµV/m	54 dBµV/m	-6 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 22

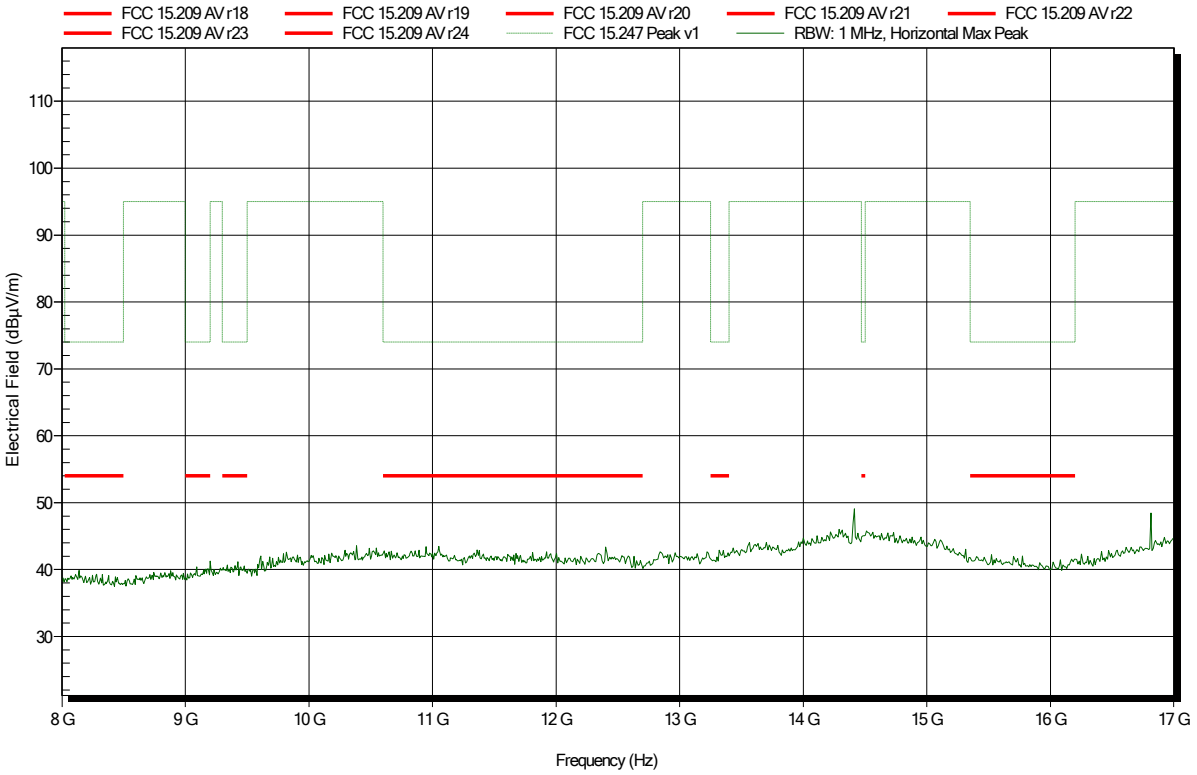

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 23

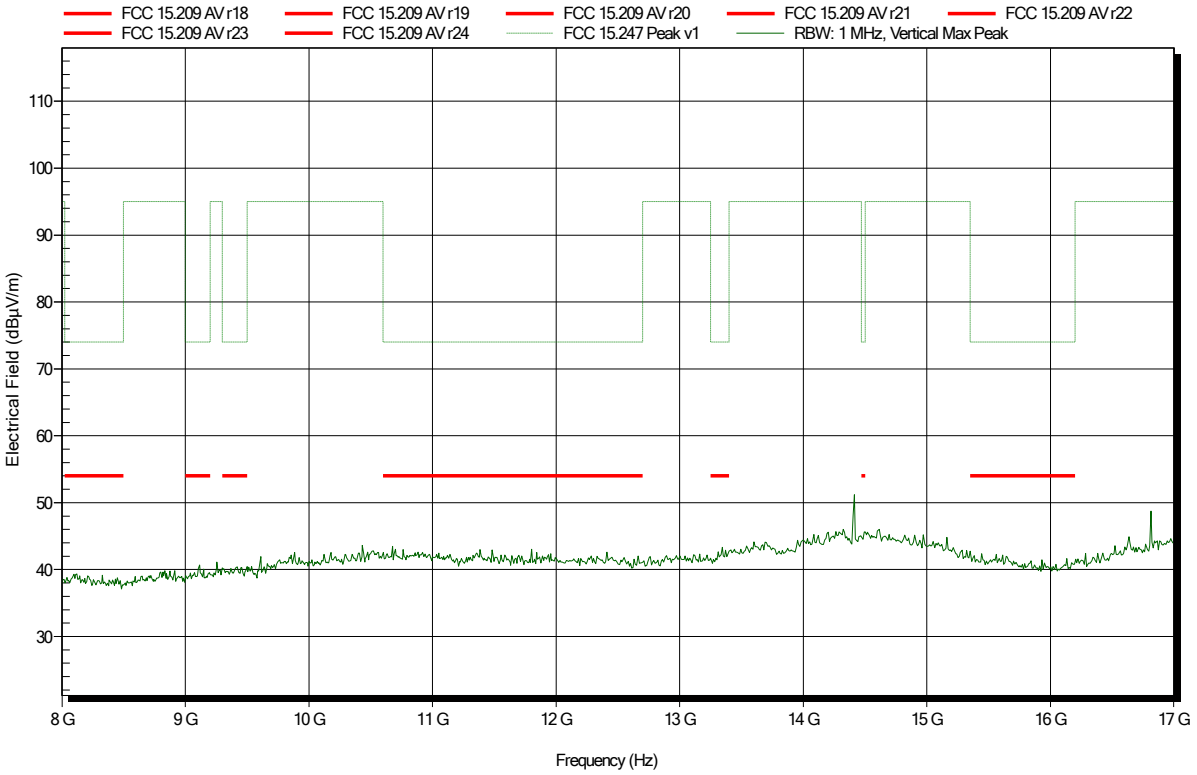

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-08
Note:	

Index 50

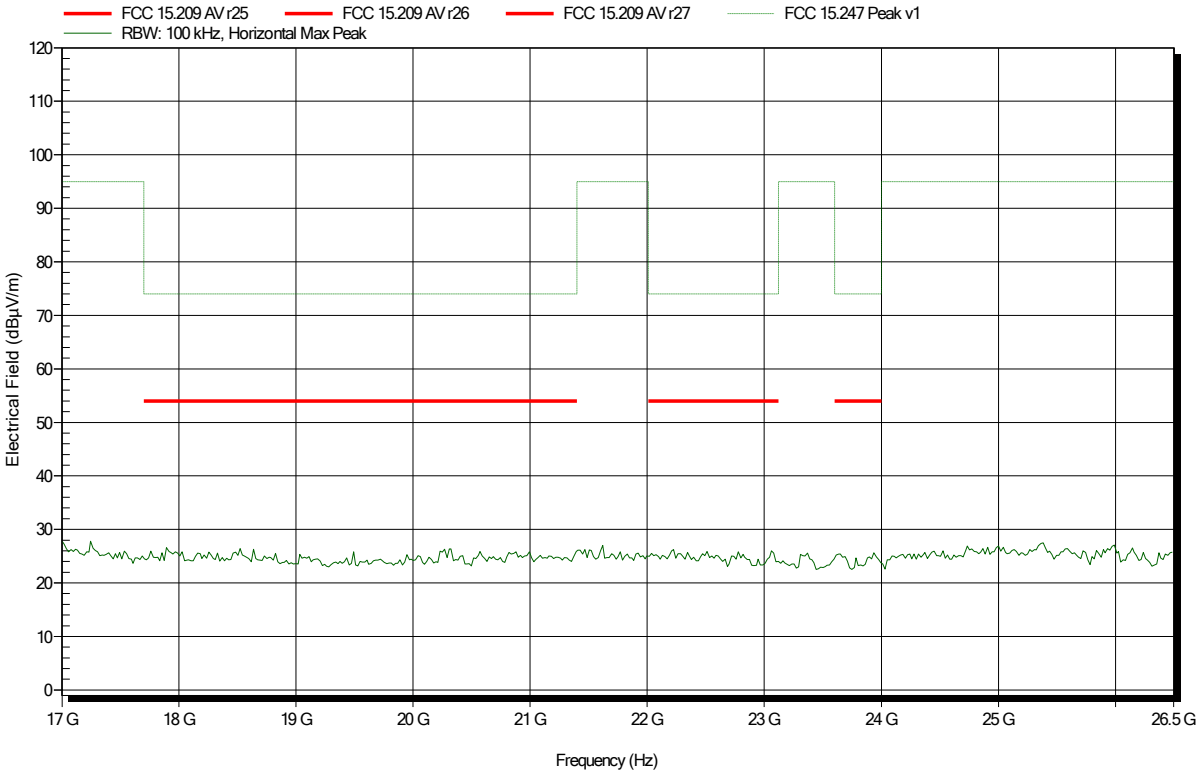

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2402MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 31

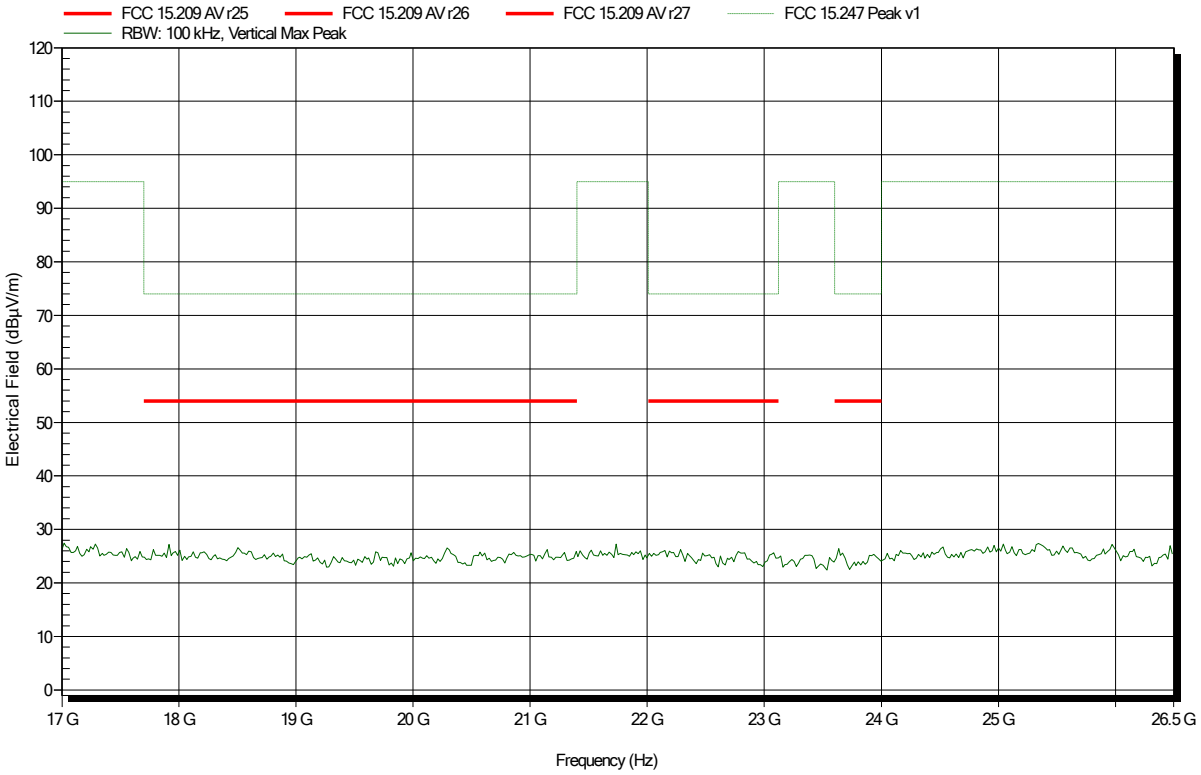

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 46

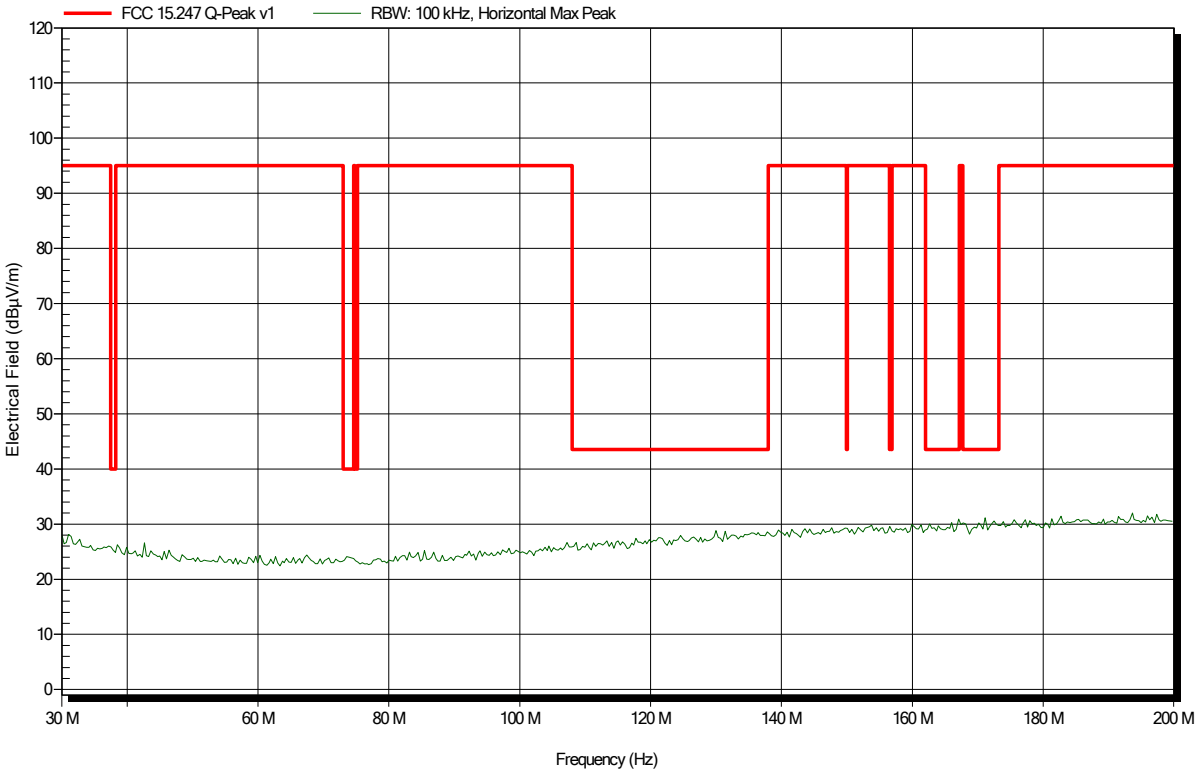

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 44

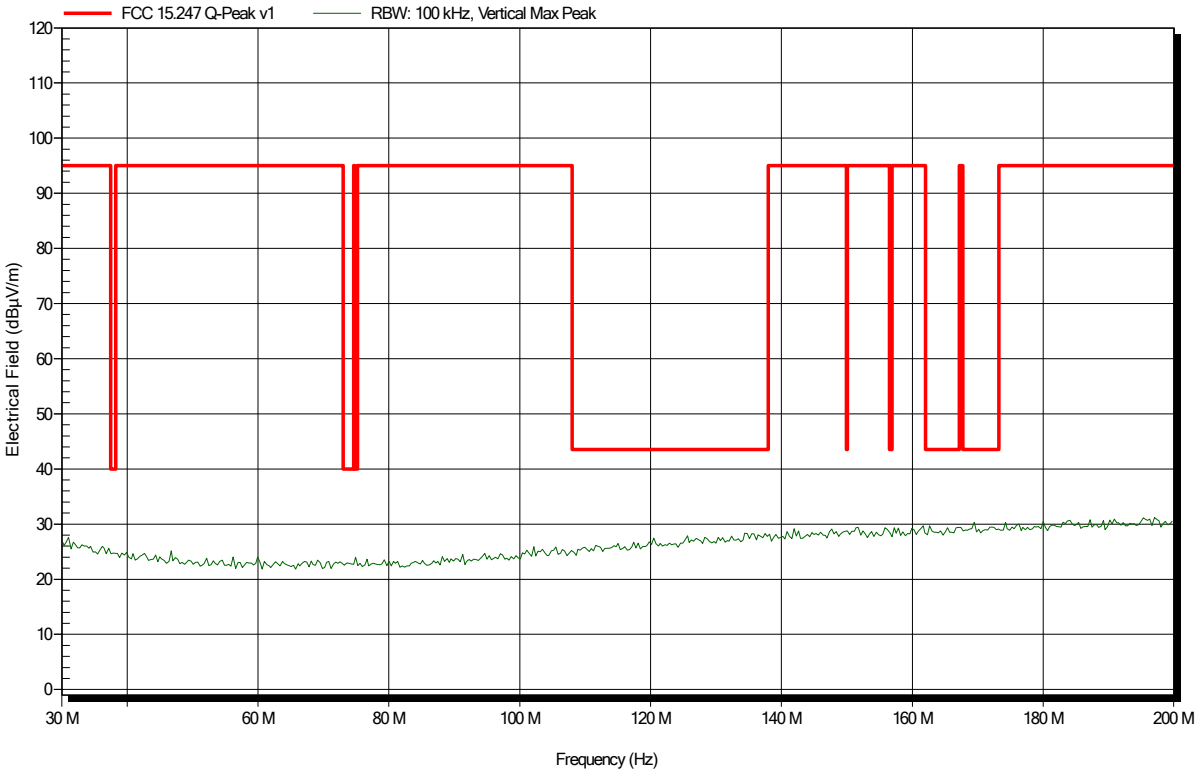

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 41

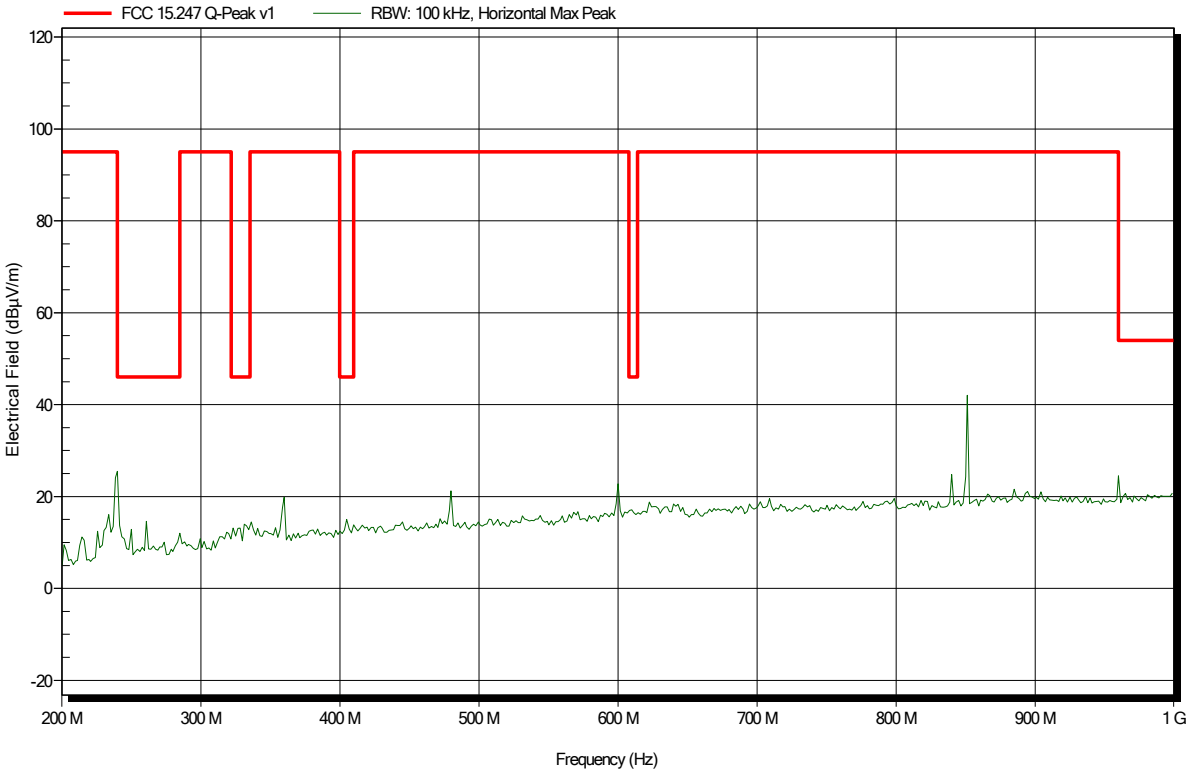

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 37

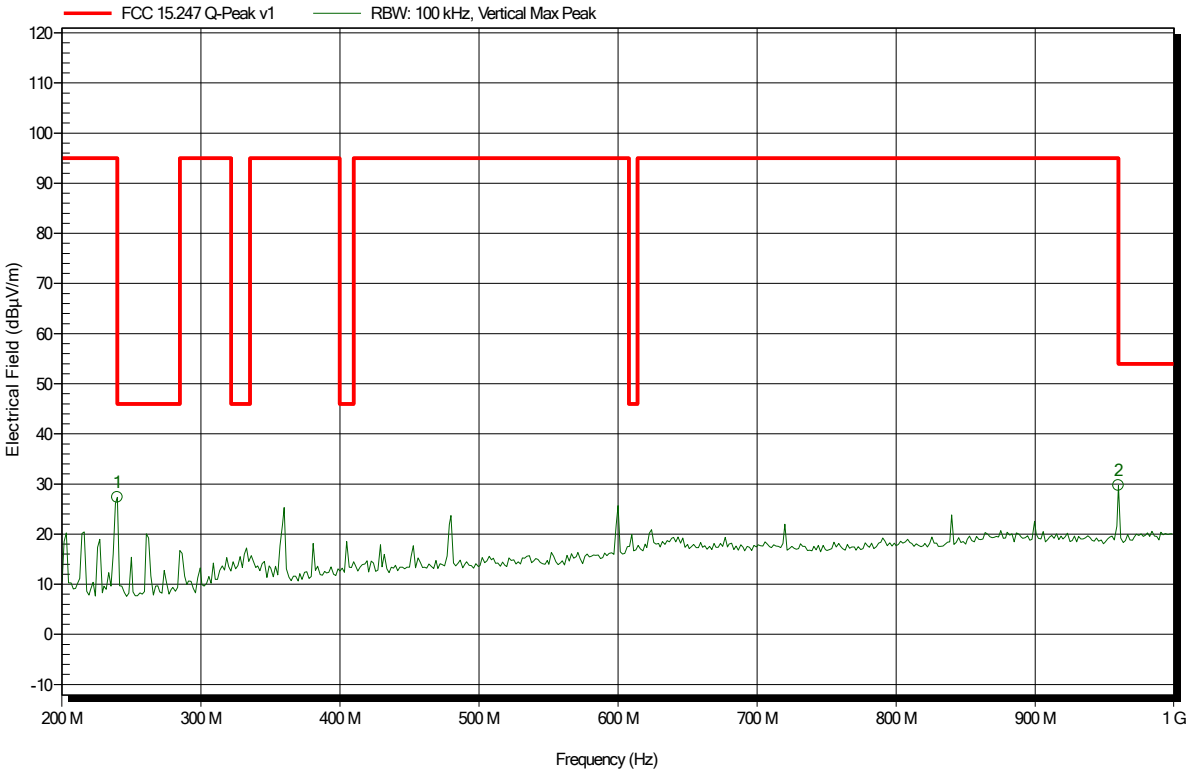

Frequency	Peak	Peak Limit	Peak Difference	Status
240 MHz	27.34 dBµV/m	46 dBµV/m	-18.66 dB	Pass
960 MHz	29.74 dBµV/m	54 dBµV/m	-24.26 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 13

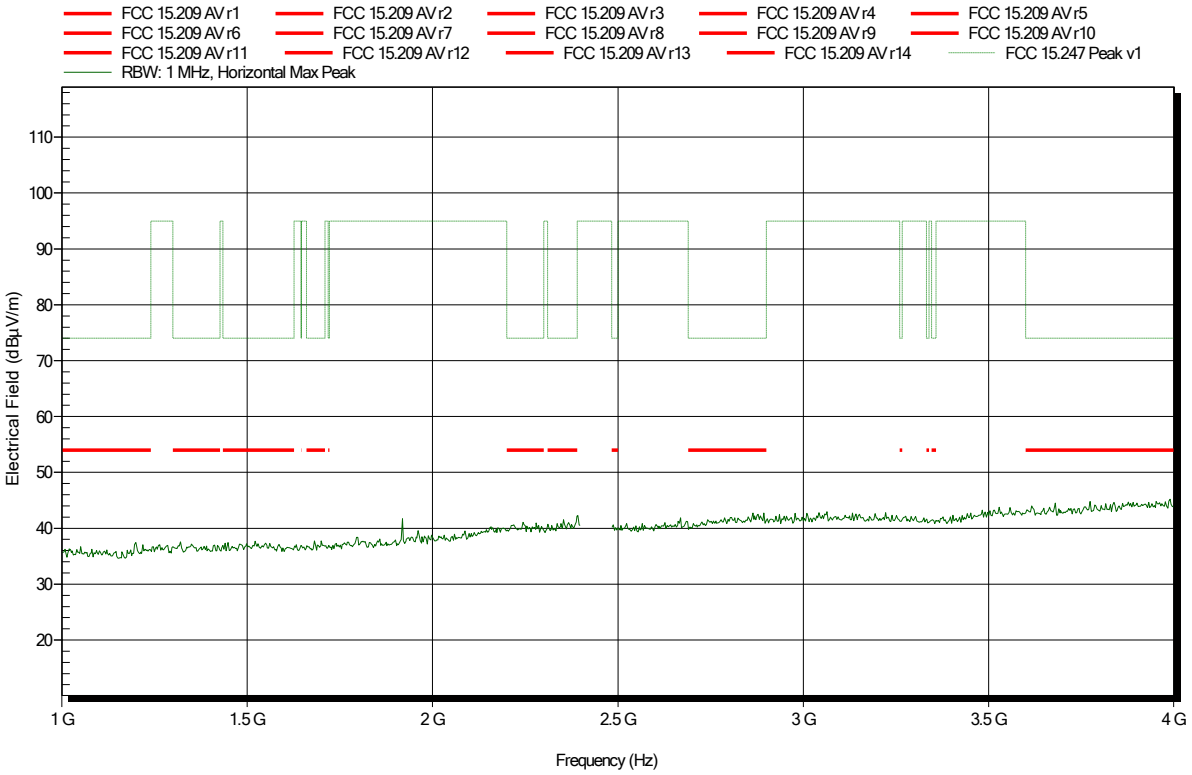

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 8

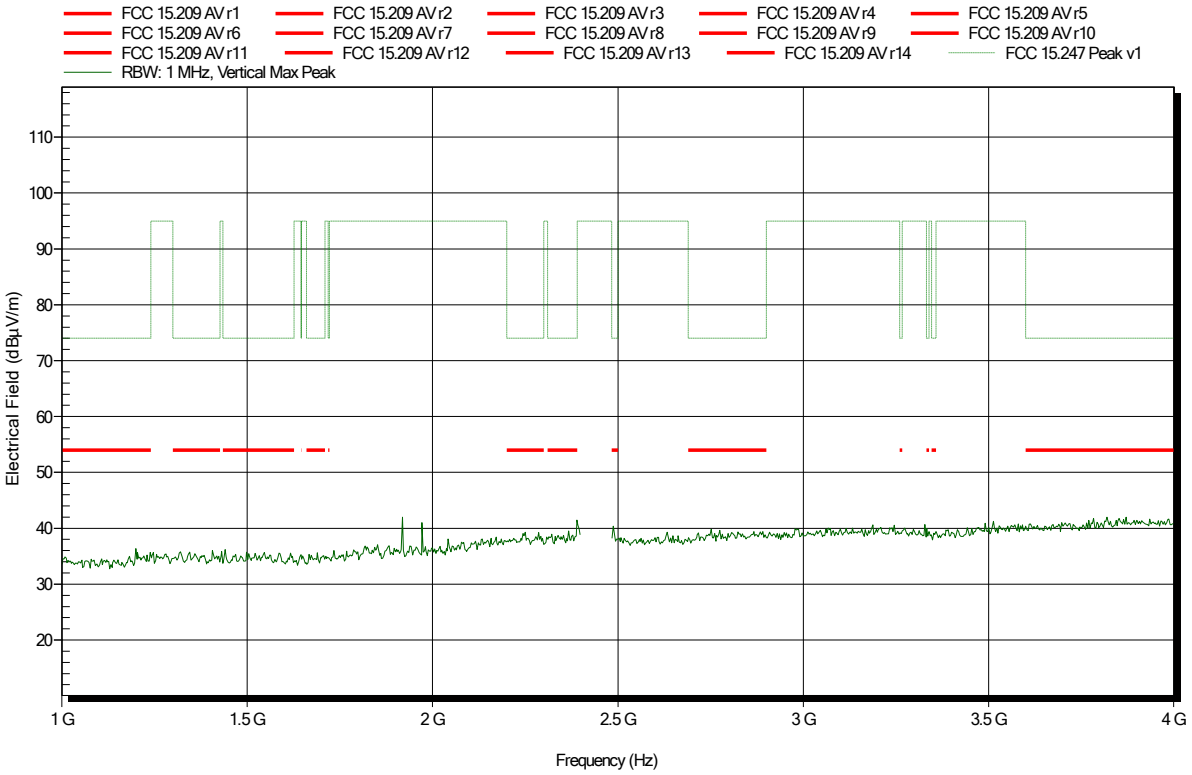

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 18

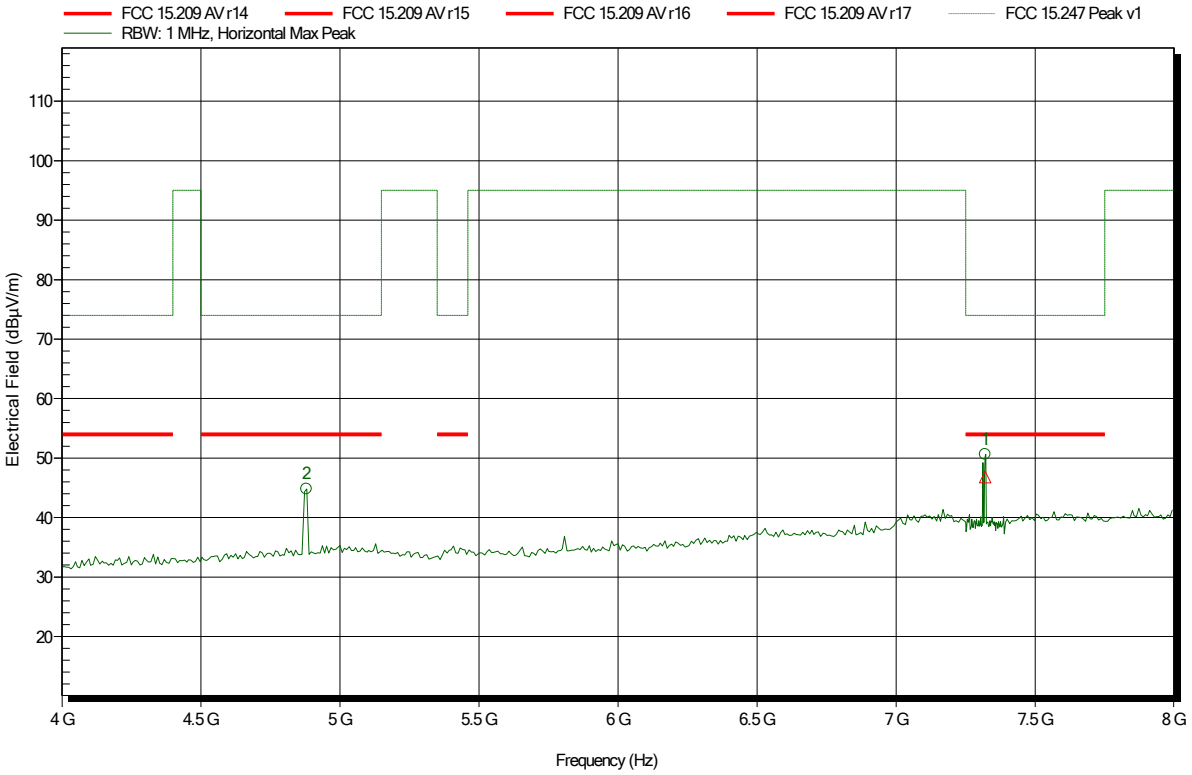

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.88 GHz	44.78 dBµV/m	74 dBµV/m	-29.22 dB	Pass
7.321 GHz	50.65 dBµV/m	74 dBµV/m	-23.35 dB	Pass

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
7.321 GHz	46.82 dBµV/m	54 dBµV/m	-7.18 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 27

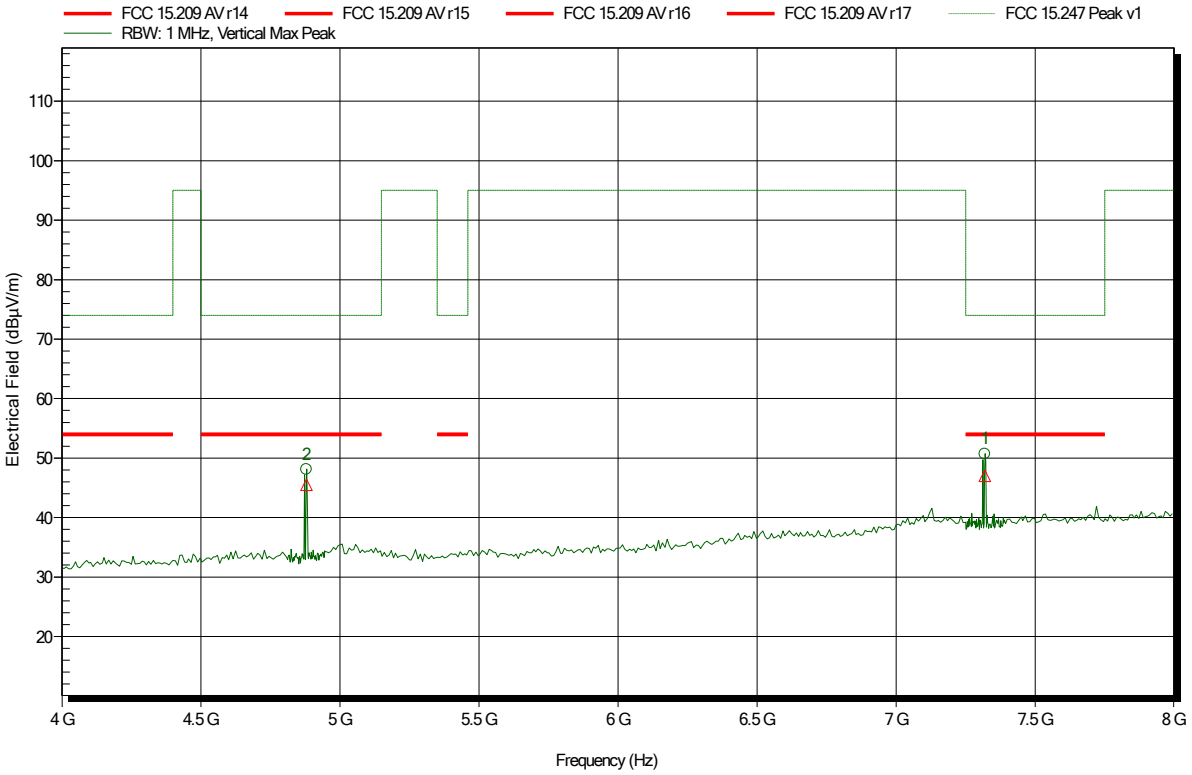

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.881 GHz	48.09 dBµV/m	74 dBµV/m	-25.91 dB	Pass
7.319 GHz	50.7 dBµV/m	74 dBµV/m	-23.3 dB	Pass

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
4.881 GHz	45.49 dBµV/m	54 dBµV/m	-8.51 dB	Pass
7.319 GHz	47.04 dBµV/m	54 dBµV/m	-6.96 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 21

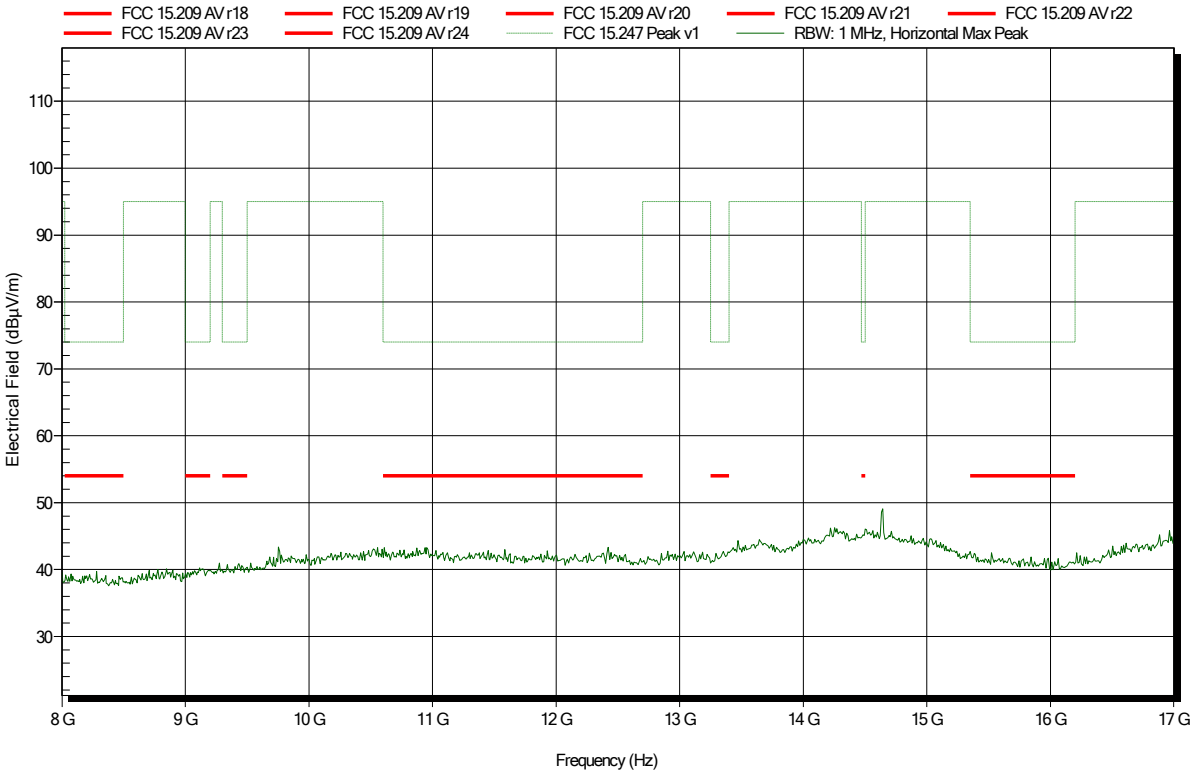

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 24

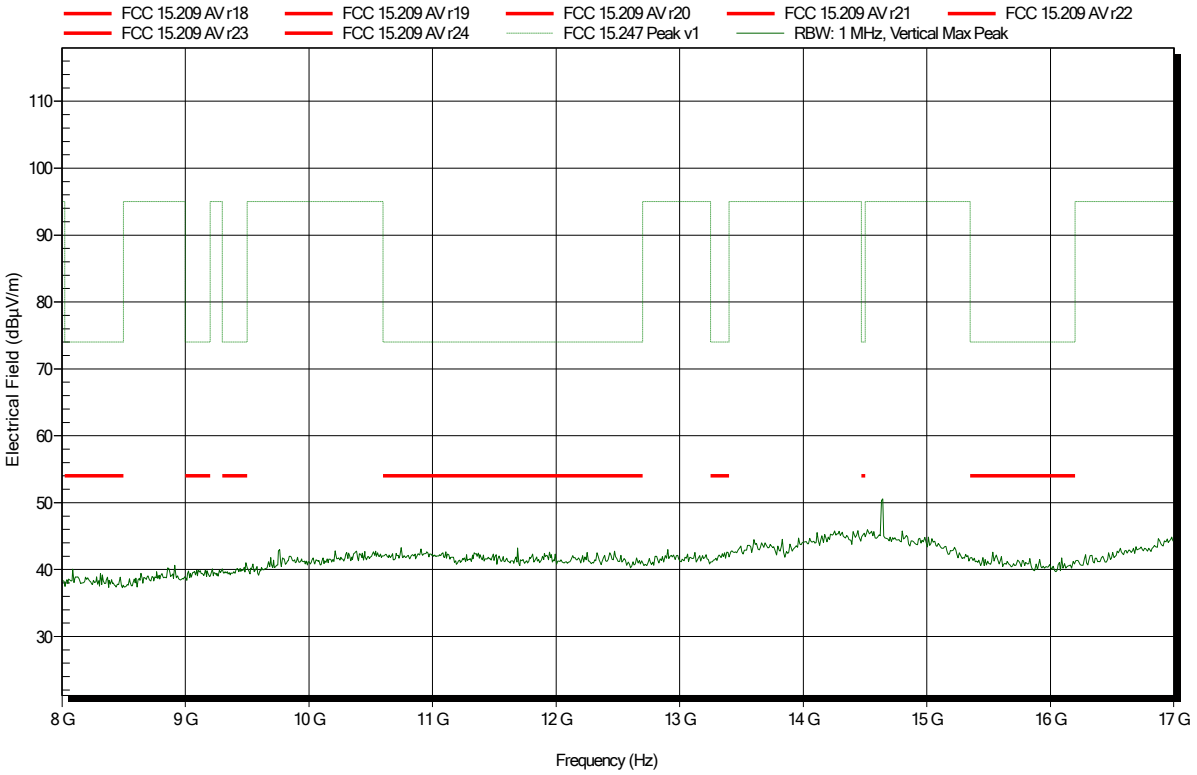

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-08
Note:	

Index 51

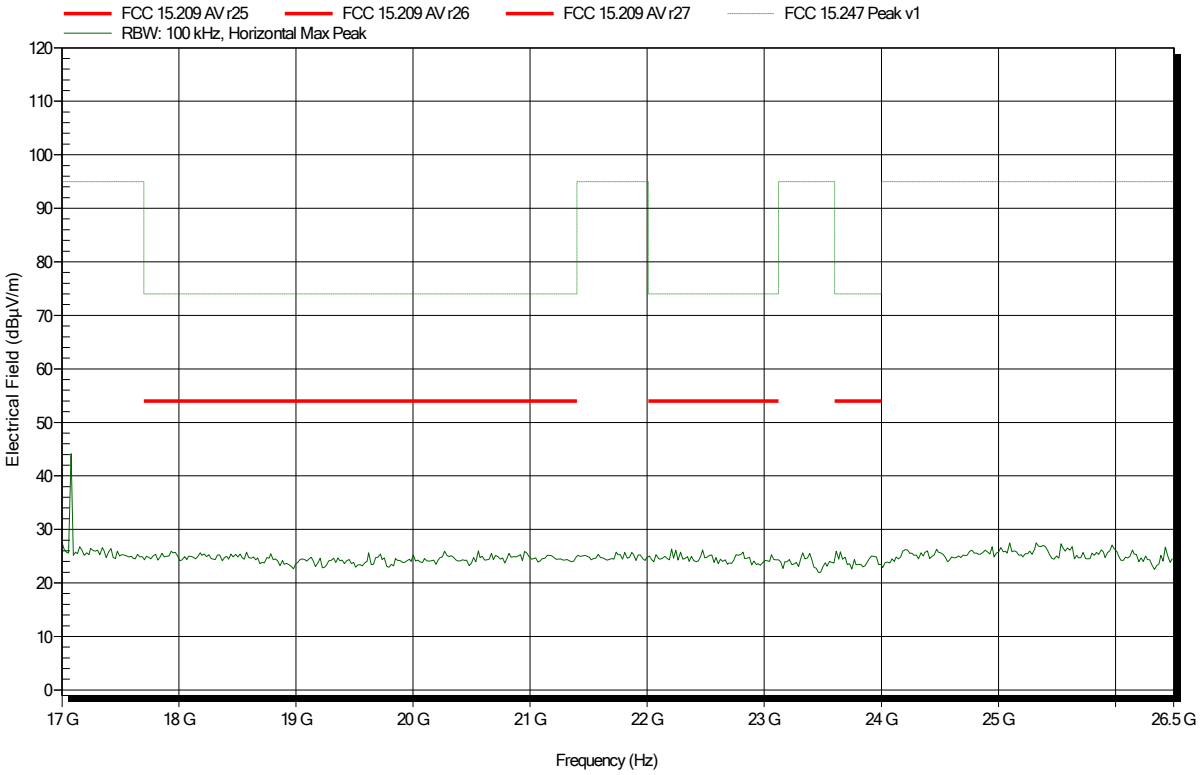

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2440MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 32

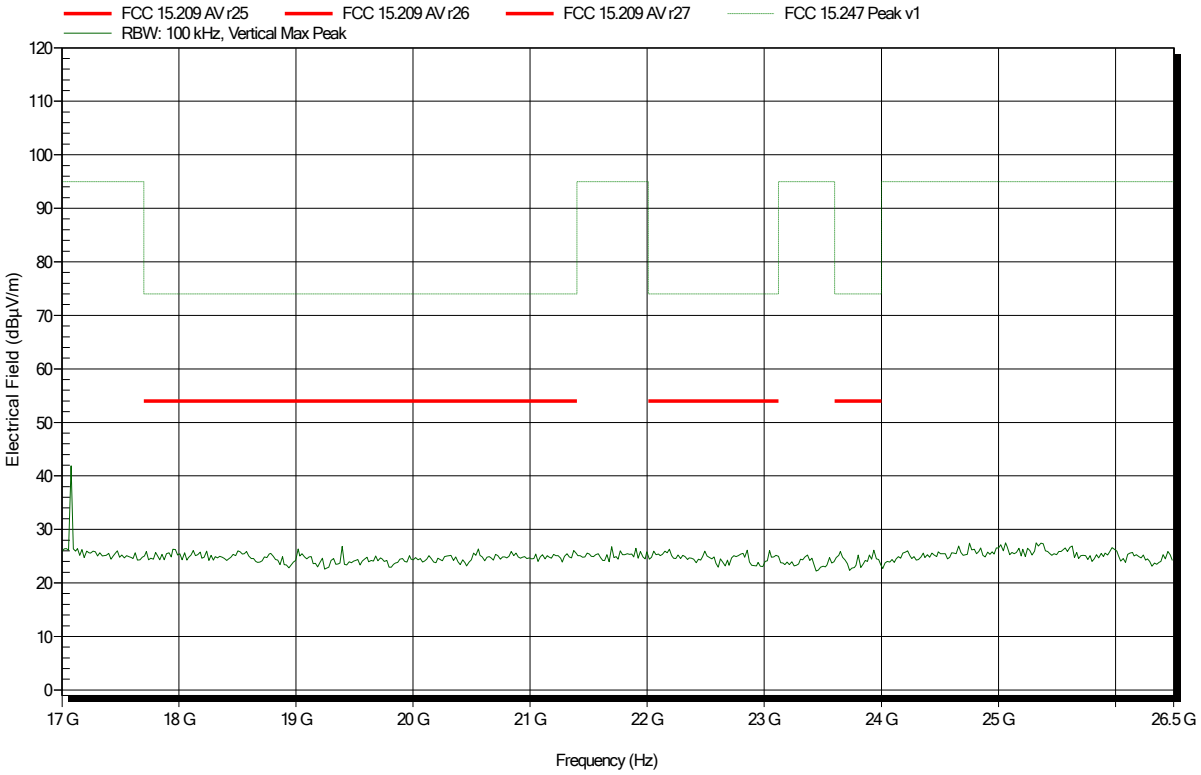

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 49

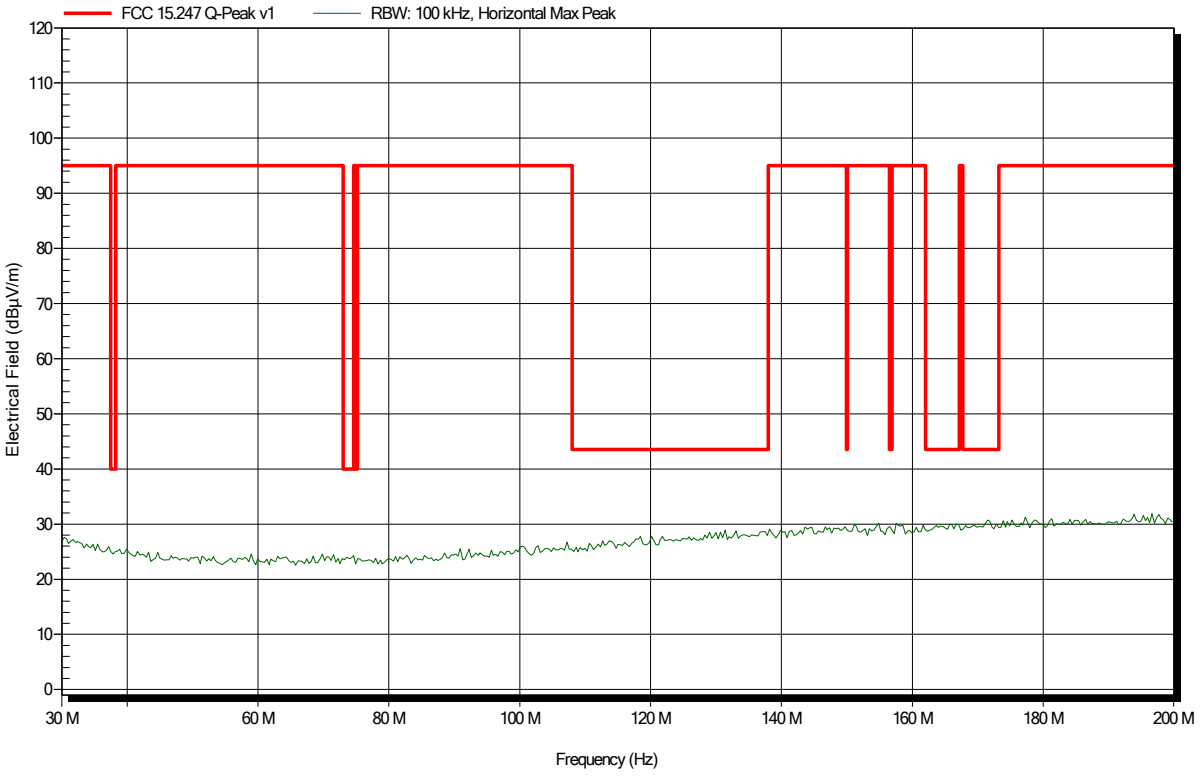

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	HK116, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 48

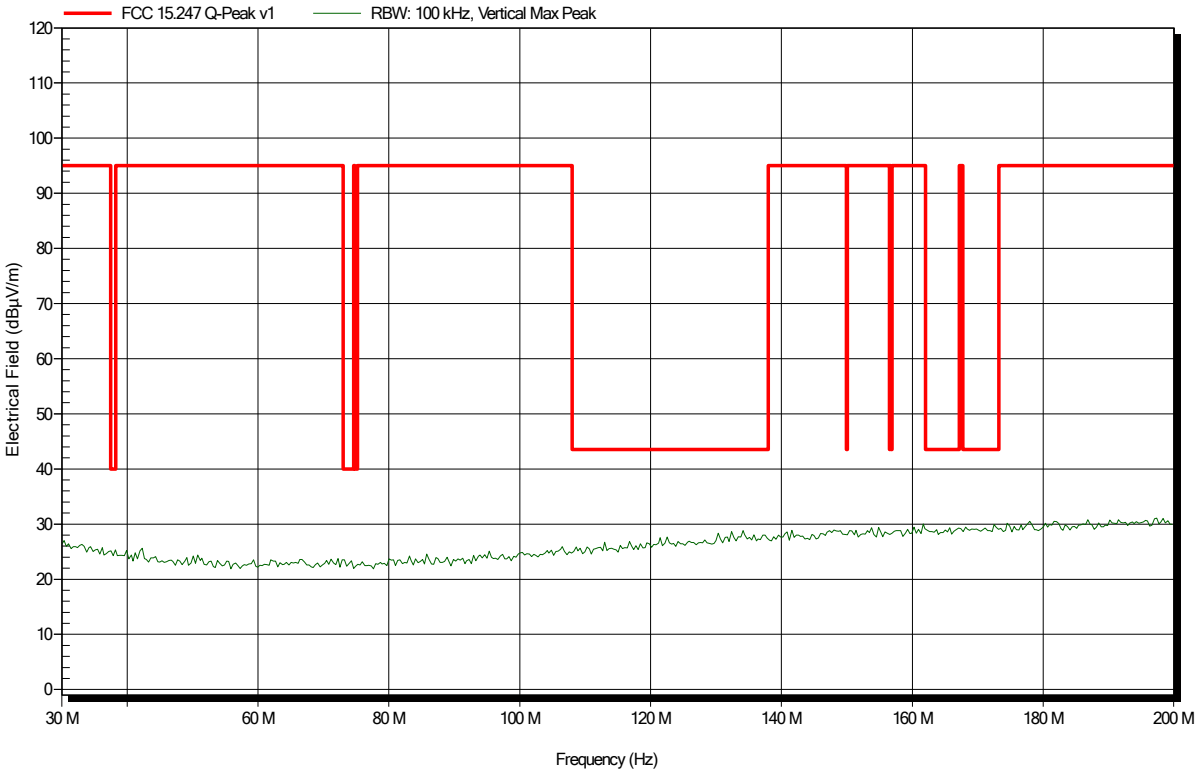

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 40

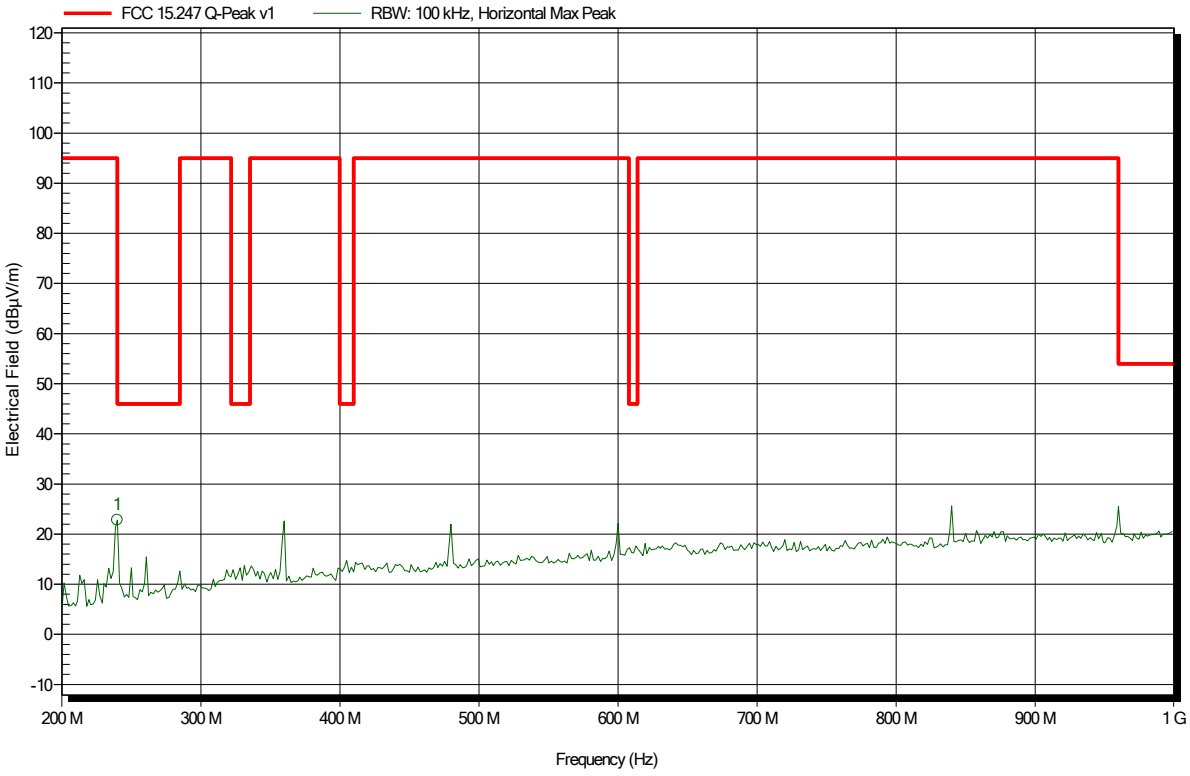

Frequency	Peak	Peak Limit	Peak Difference	Status
240 MHz	22.8 dBµV/m	46 dBµV/m	-23.2 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 39

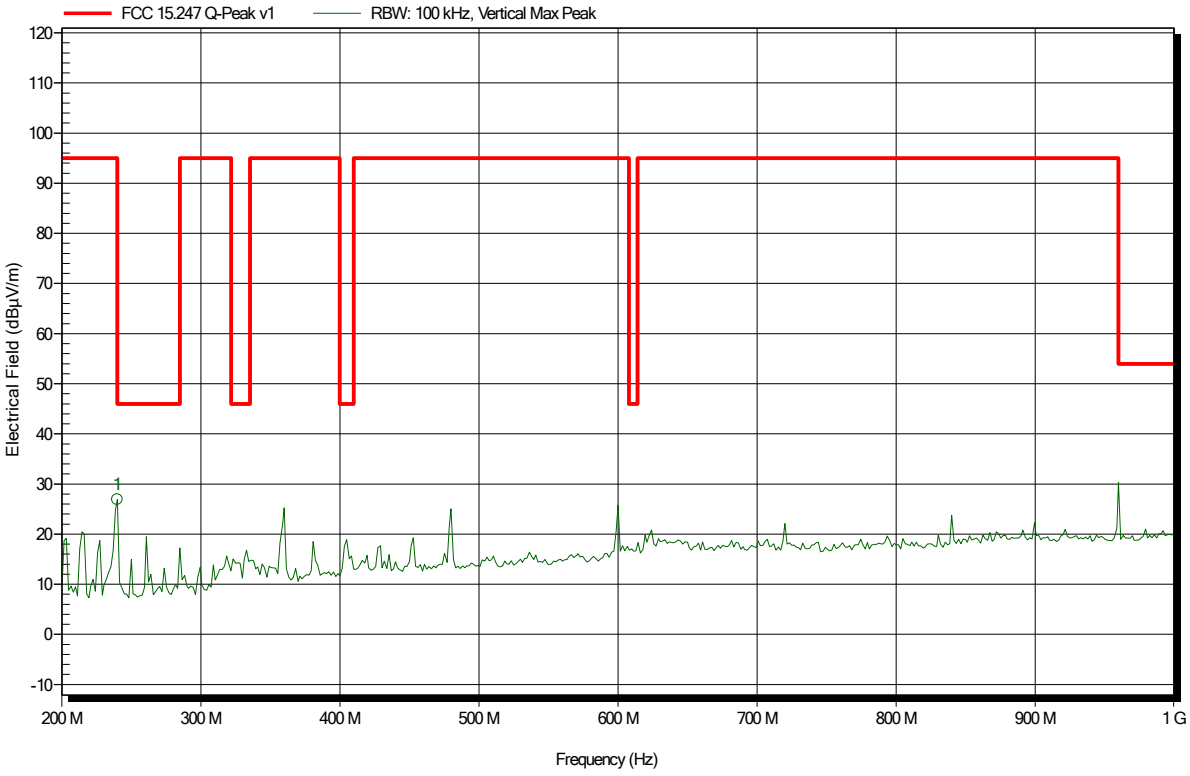

Frequency	Peak	Peak Limit	Peak Difference	Status
240 MHz	26.89 dBµV/m	46 dBµV/m	-19.11 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 12

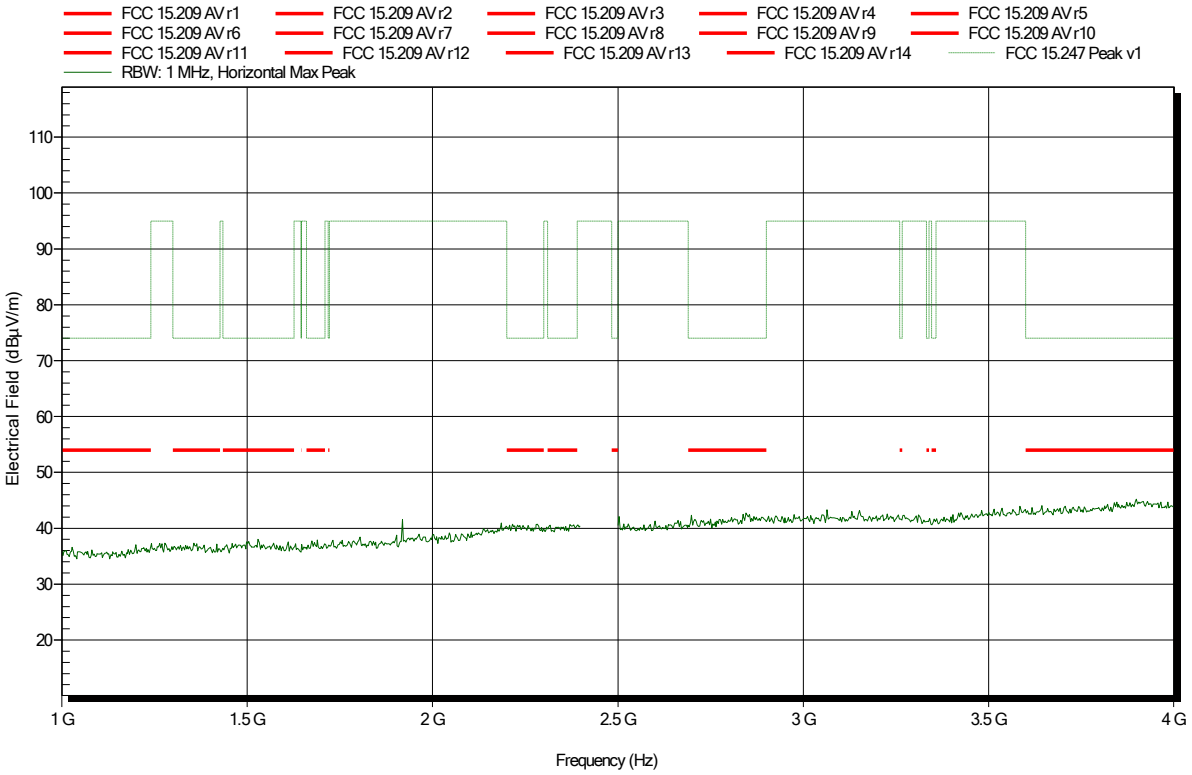

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 9

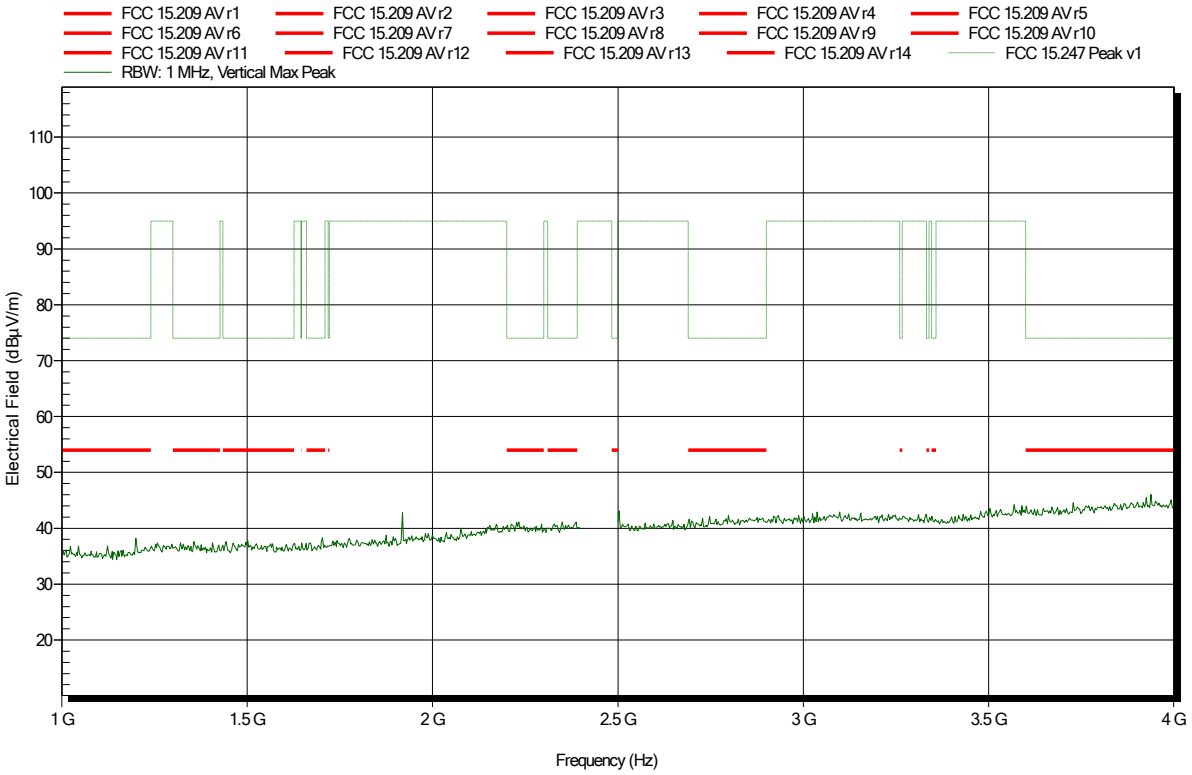

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 11

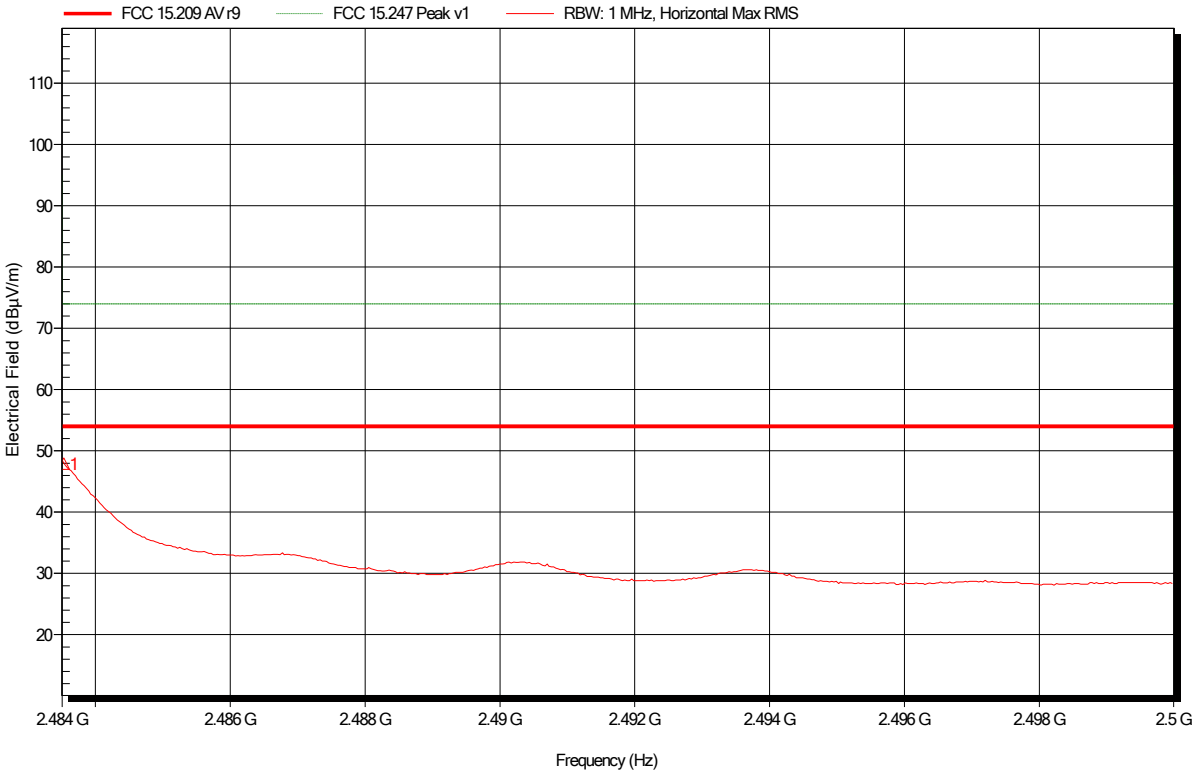

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
2.4835 GHz	47.95 dBµV/m	54 dBµV/m	-6.05 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-06
Note:	

Index 10

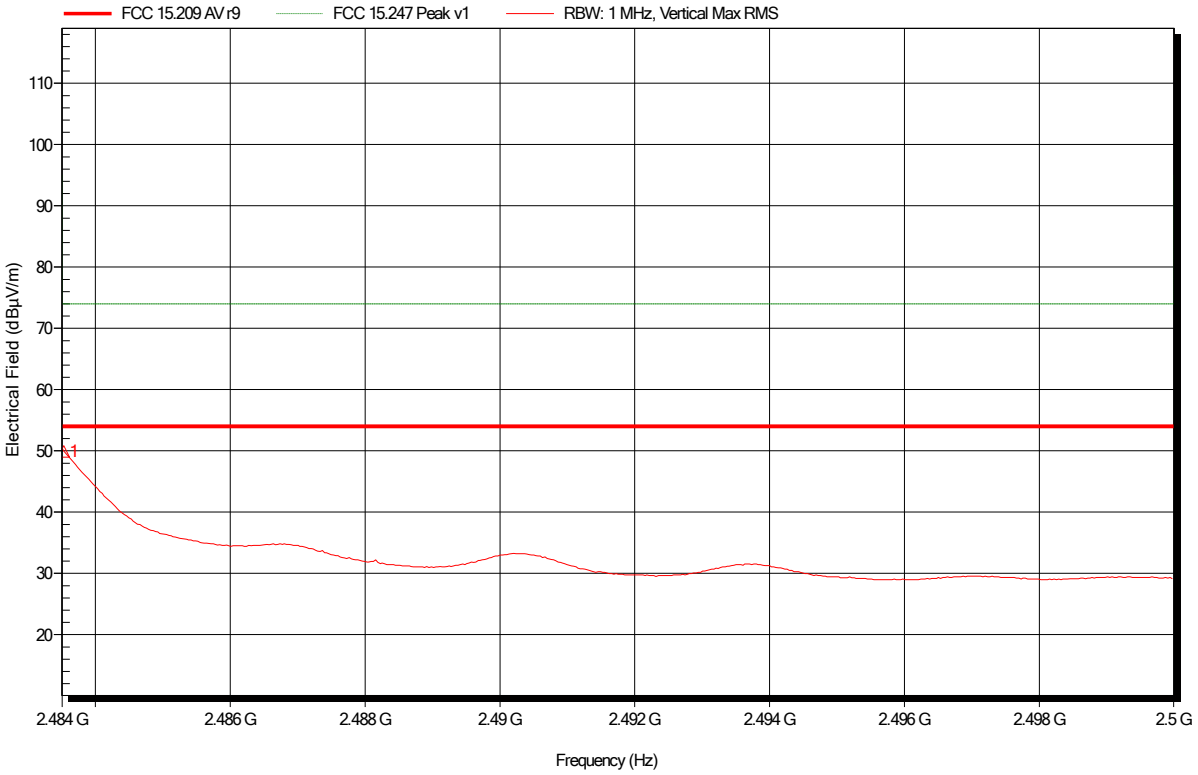

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
2.4835 GHz	49.91 dBµV/m	54 dBµV/m	-4.09 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 19

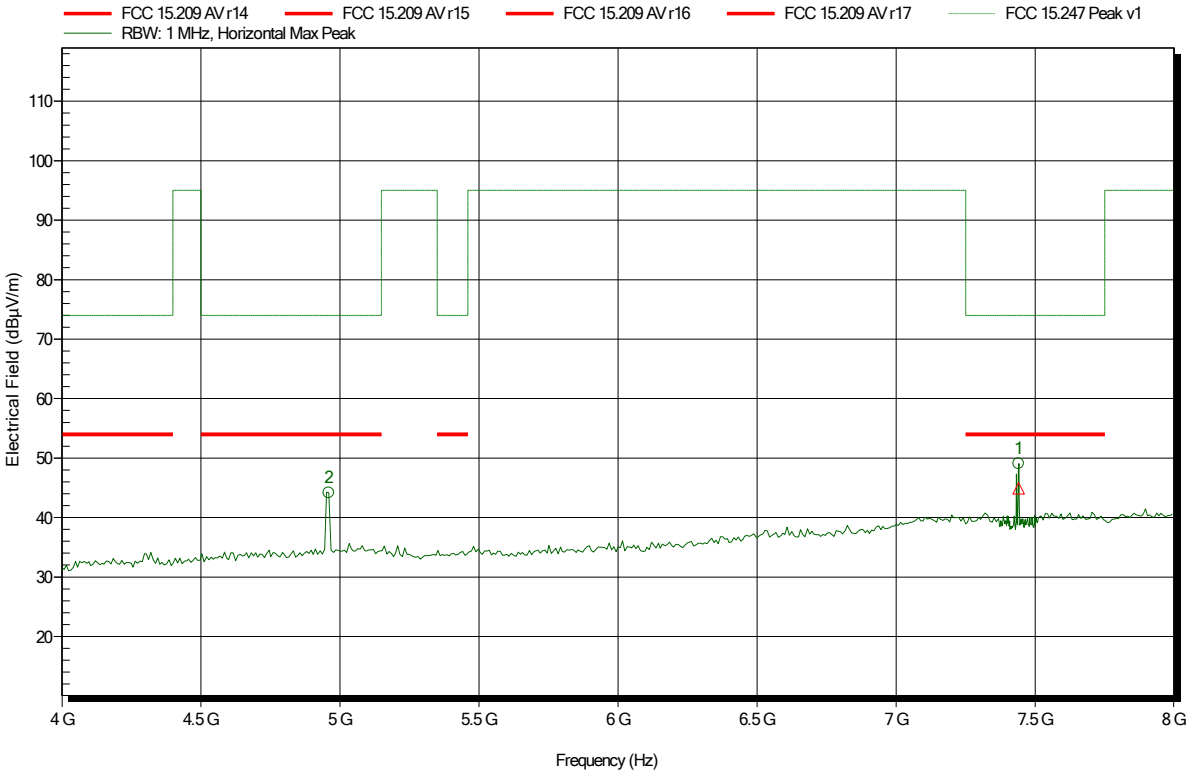

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.96 GHz	44.18 dBµV/m	74 dBµV/m	-29.82 dB	Pass
7.441 GHz	49.05 dBµV/m	74 dBµV/m	-24.95 dB	Pass

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
7.441 GHz	44.94 dBµV/m	54 dBµV/m	-9.06 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 26

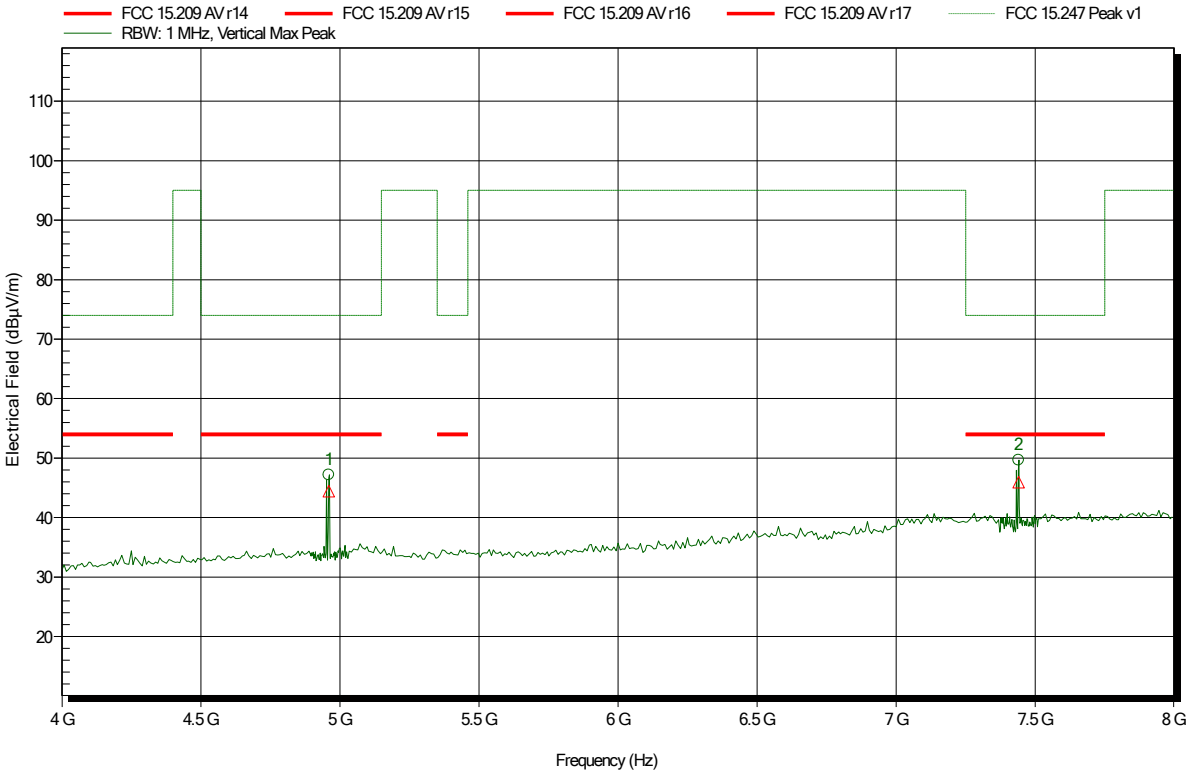

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.96 GHz	47.19 dBµV/m	74 dBµV/m	-26.81 dB	Pass
7.441 GHz	49.65 dBµV/m	74 dBµV/m	-24.35 dB	Pass

Frequency	RMS	RMS Limit	RMS Difference	RMS Status
4.96 GHz	44.41 dBµV/m	54 dBµV/m	-9.59 dB	Pass
7.441 GHz	45.96 dBµV/m	54 dBµV/m	-8.04 dB	Pass

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 20

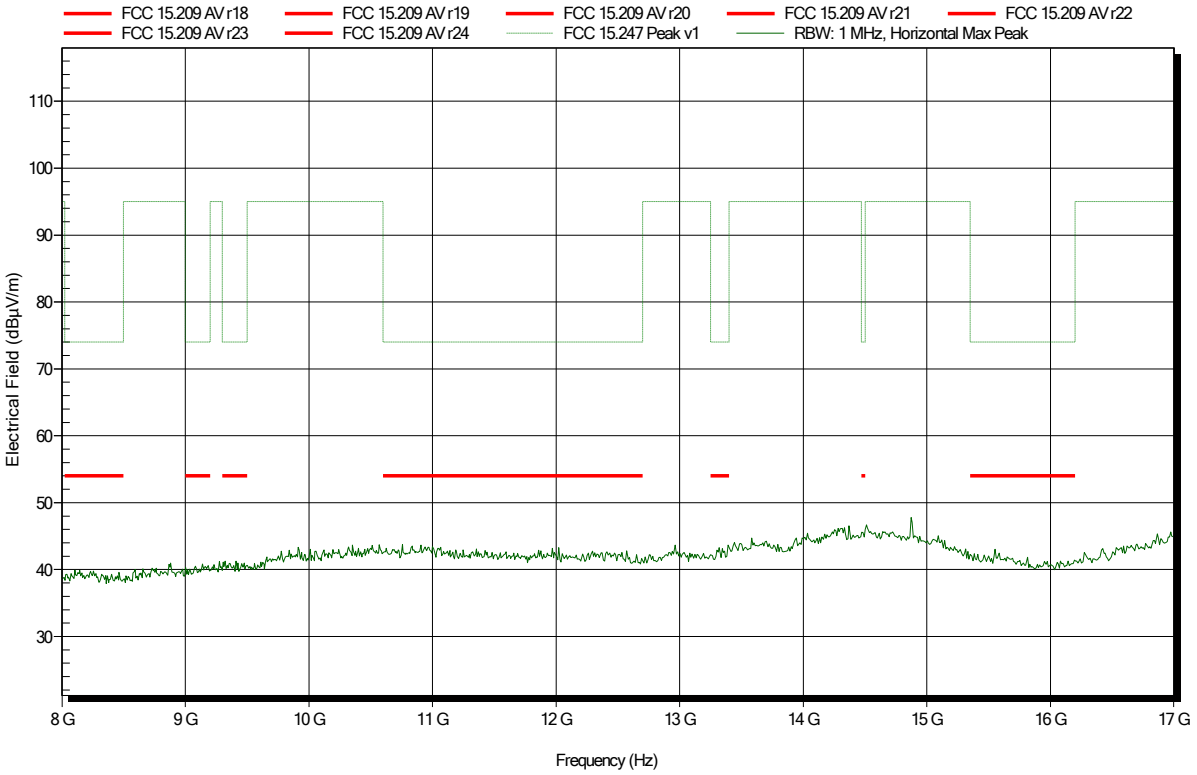

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 25

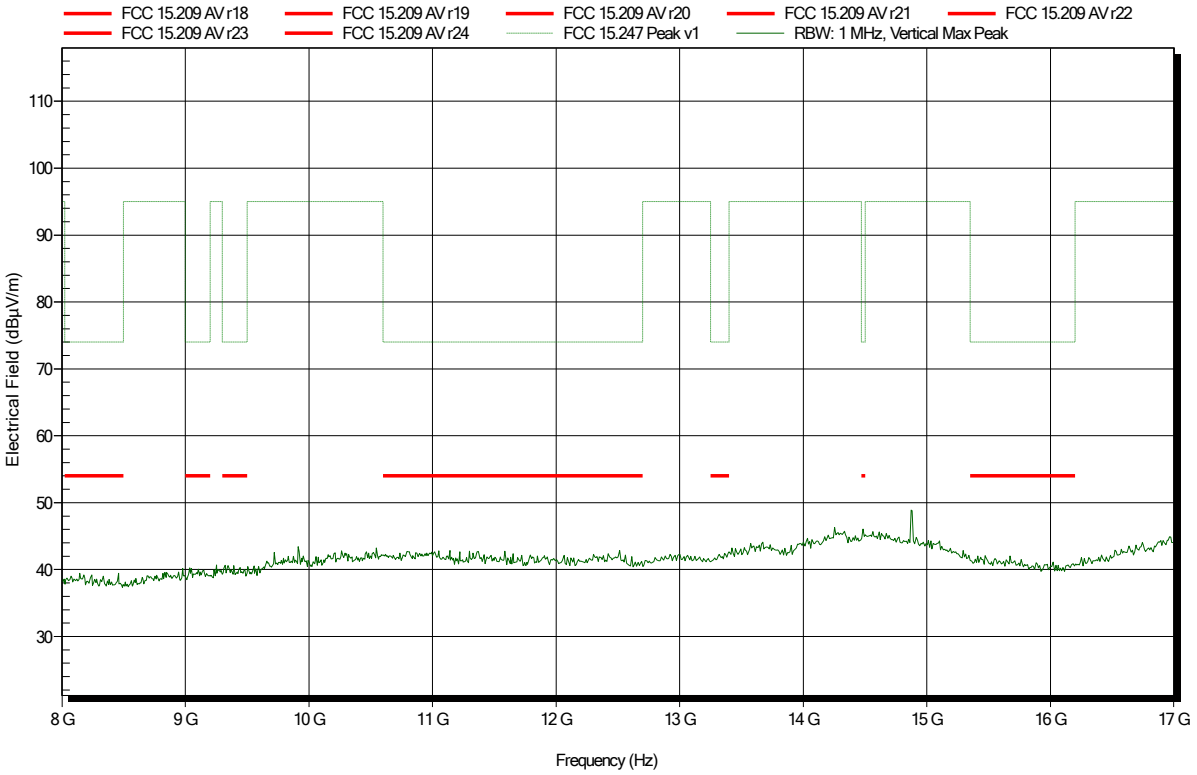

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-08
Note:	

Index 52

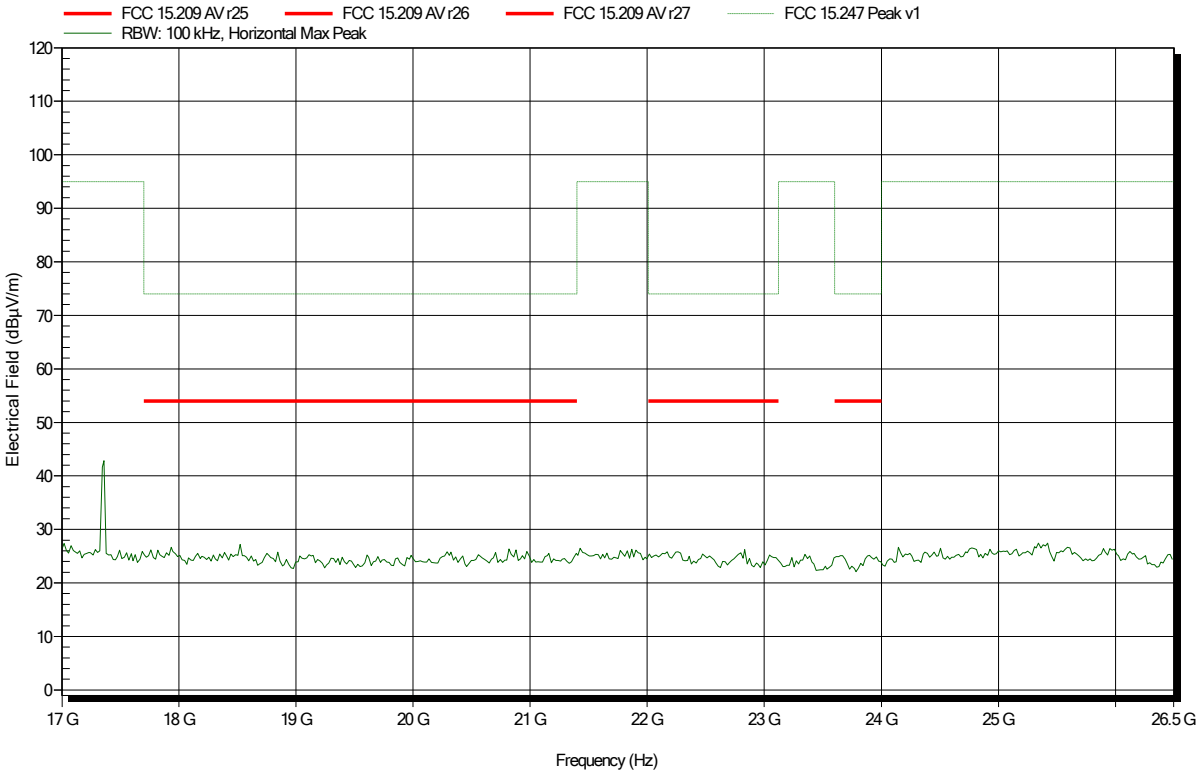

Spurious emissions according to FCC 47 CFR § 15.247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 22.7°C, Vnom: 3.3 VDC
Antenna:	Amplifier Research AT4560, Vertical
Measurement distance:	1 m converted to 3m
Mode:	TX; BTLE, 2480MHz, 2FSK, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 33

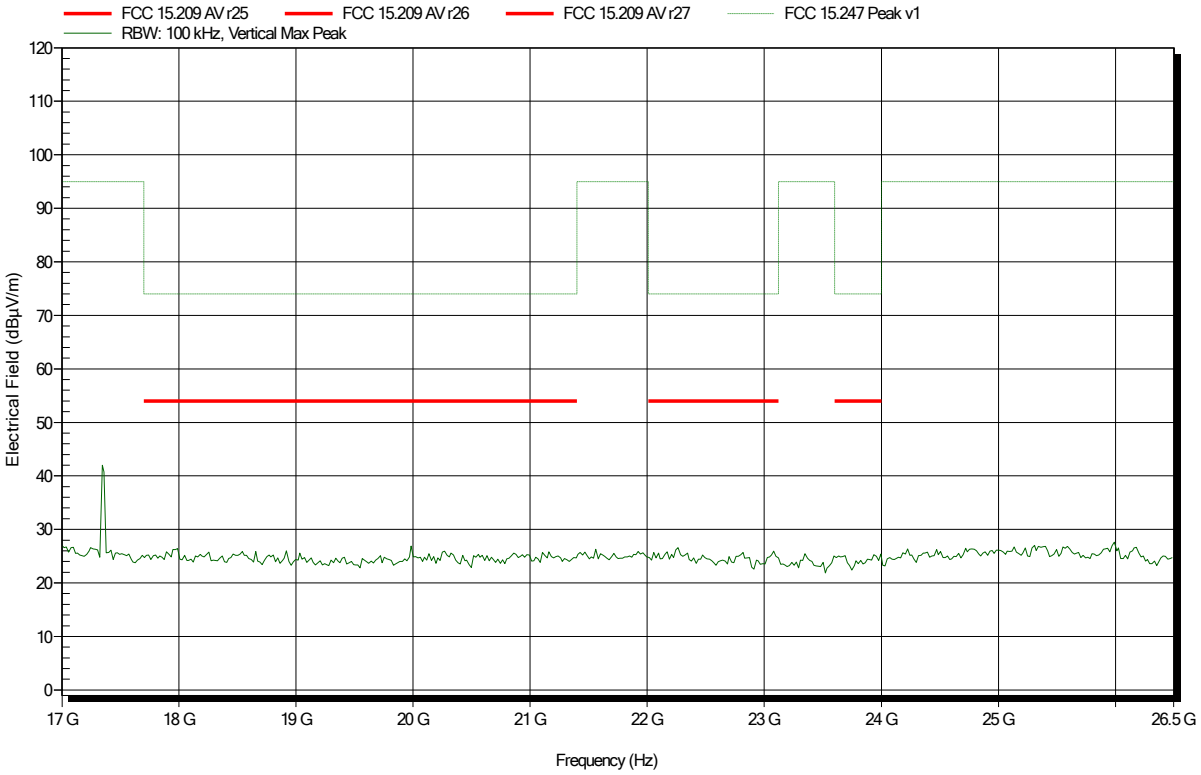

ANNEX B Receiver spurious emissions

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 1

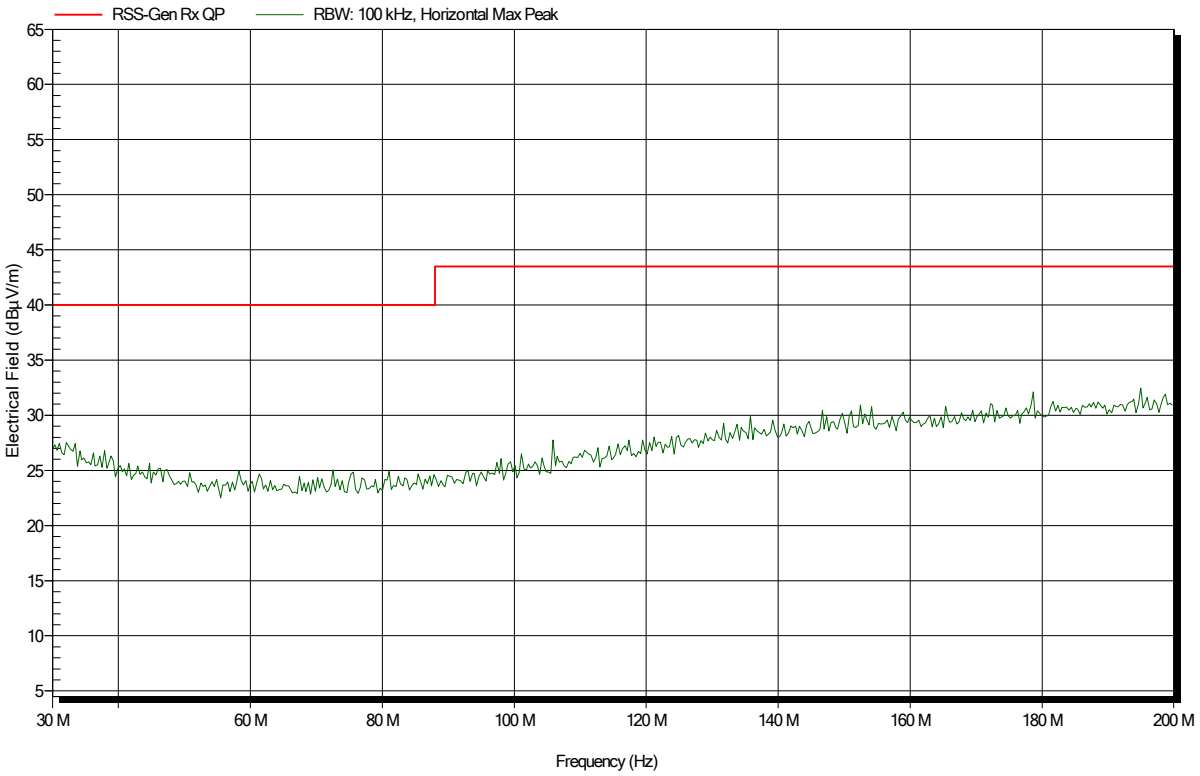

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	HK116, Vertical
Measurement distance:	3 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 2

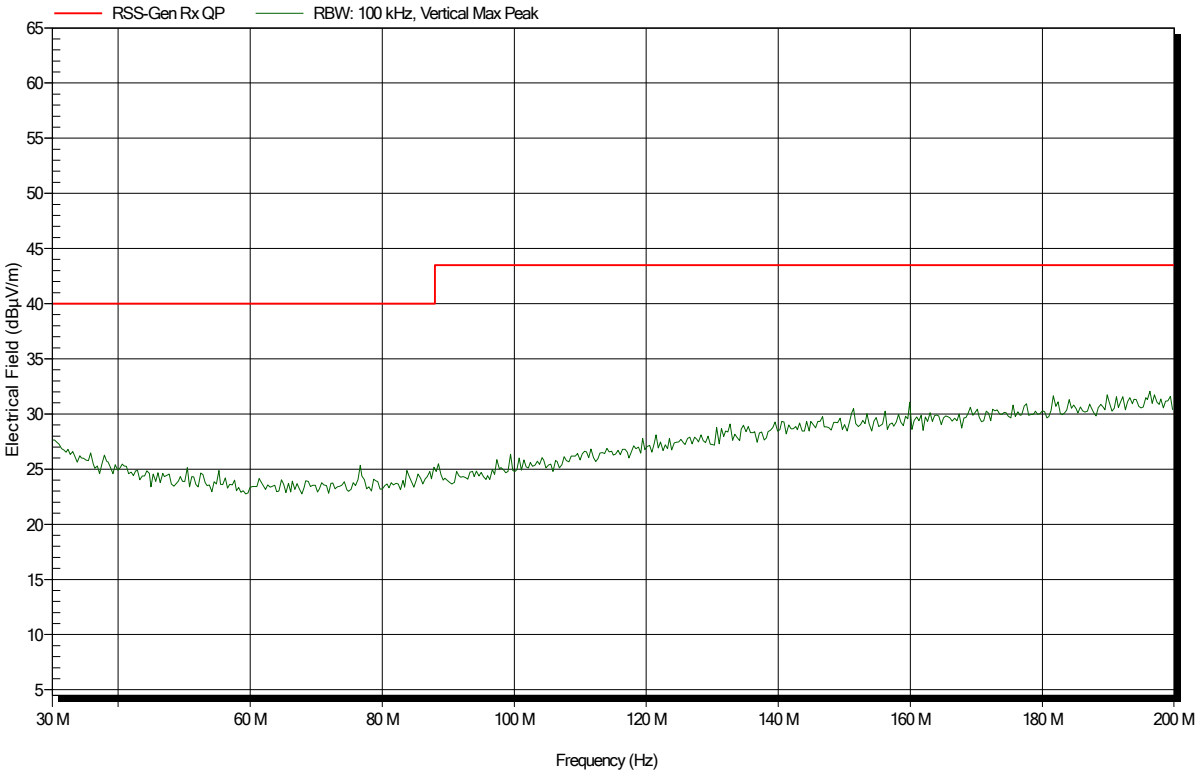

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 4

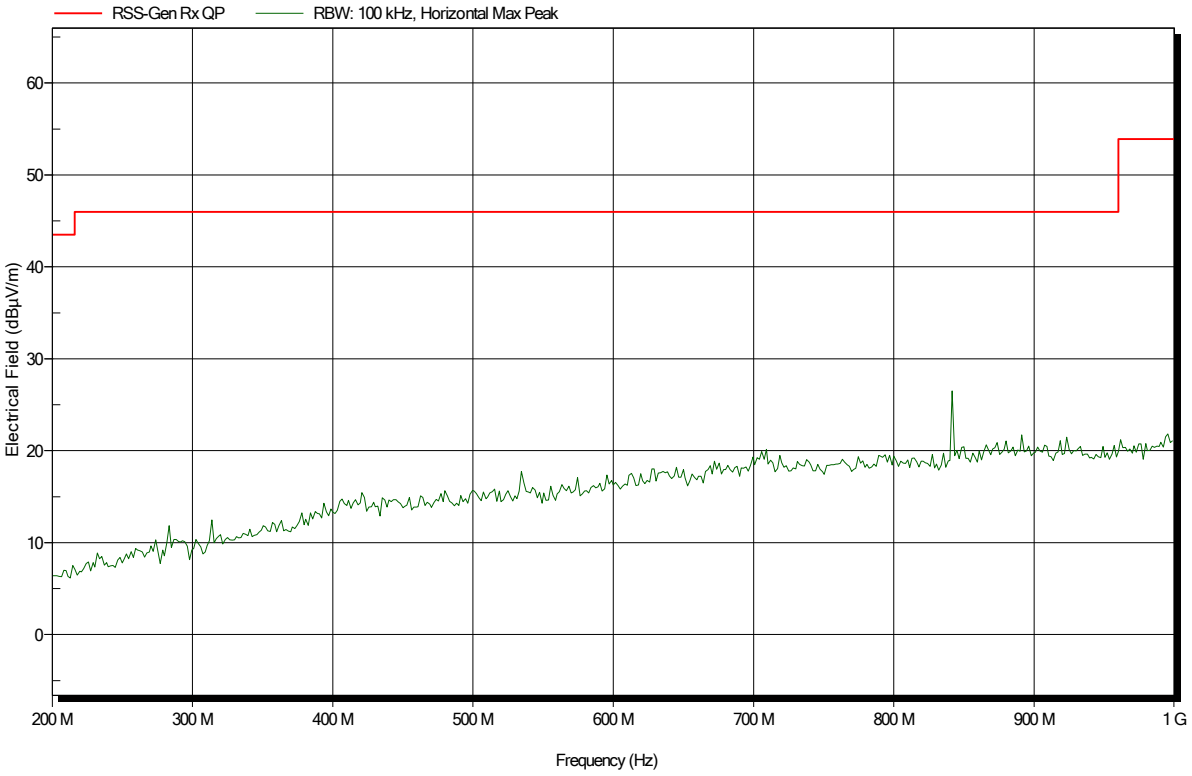

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 3

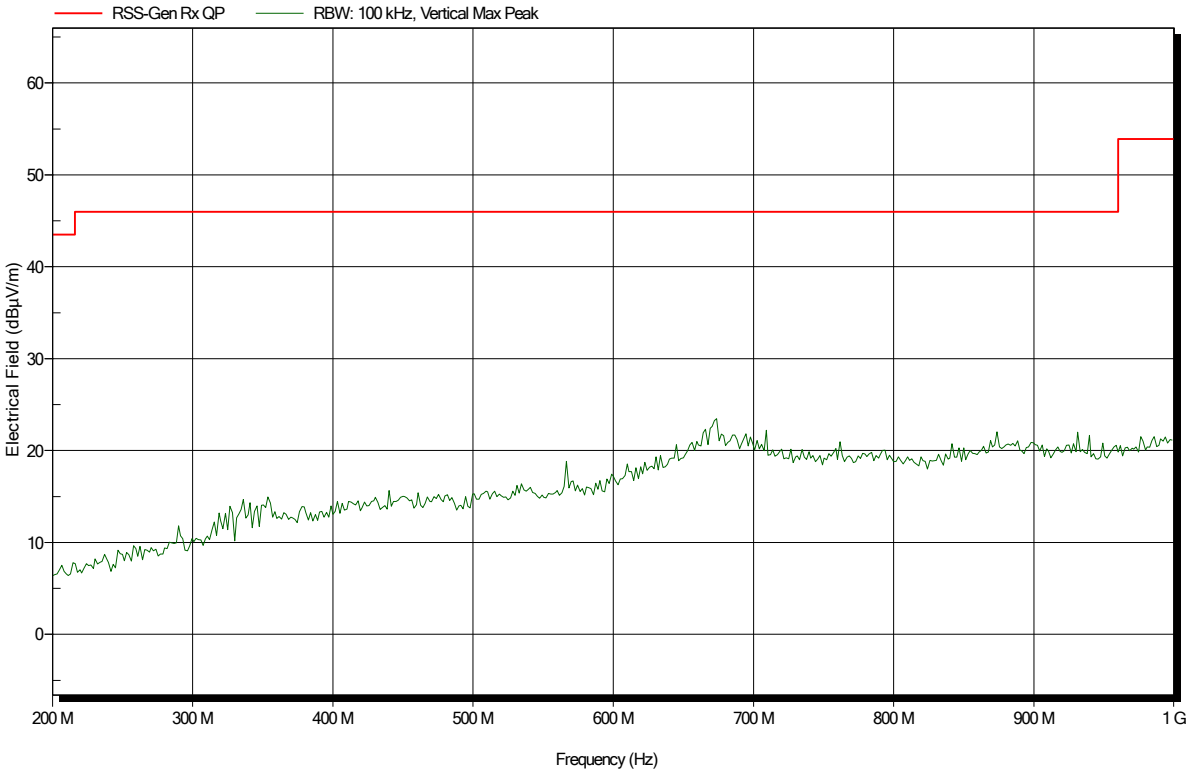

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Measurement software:	RadiMation, version 2015.2.4
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 10

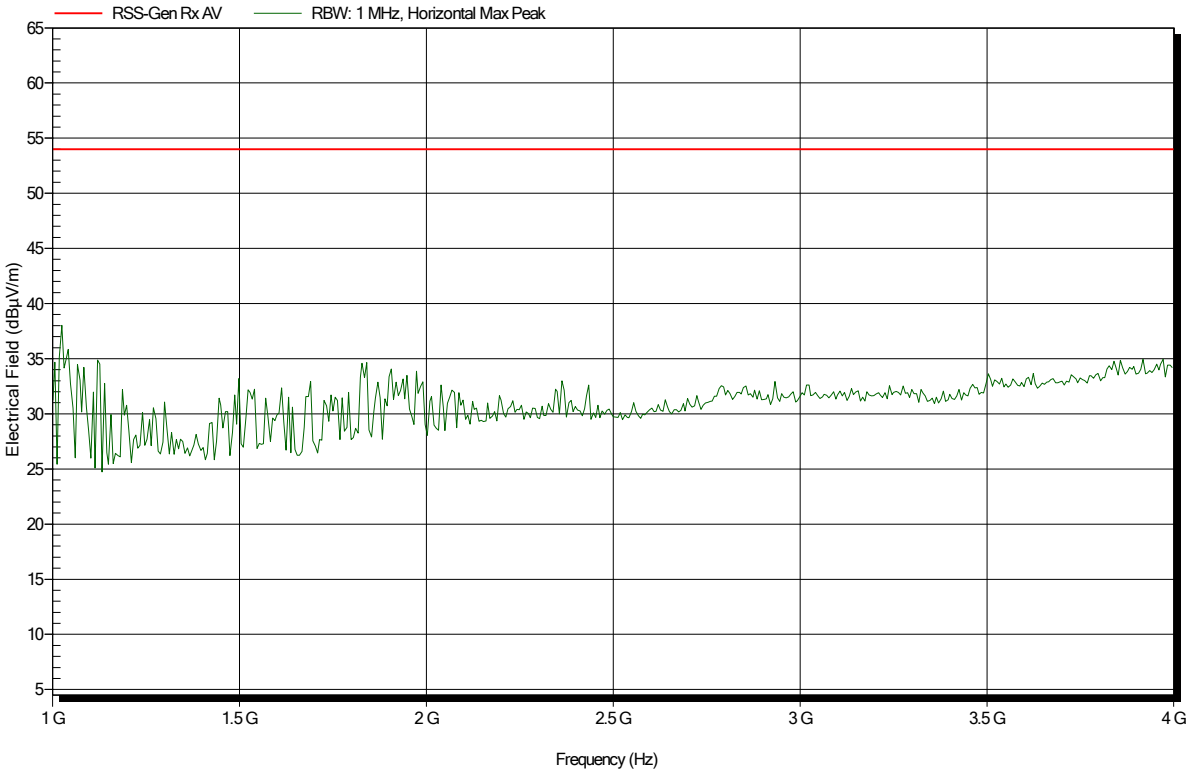

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Measurement software:	RadiMation, version 2015.2.4
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 5

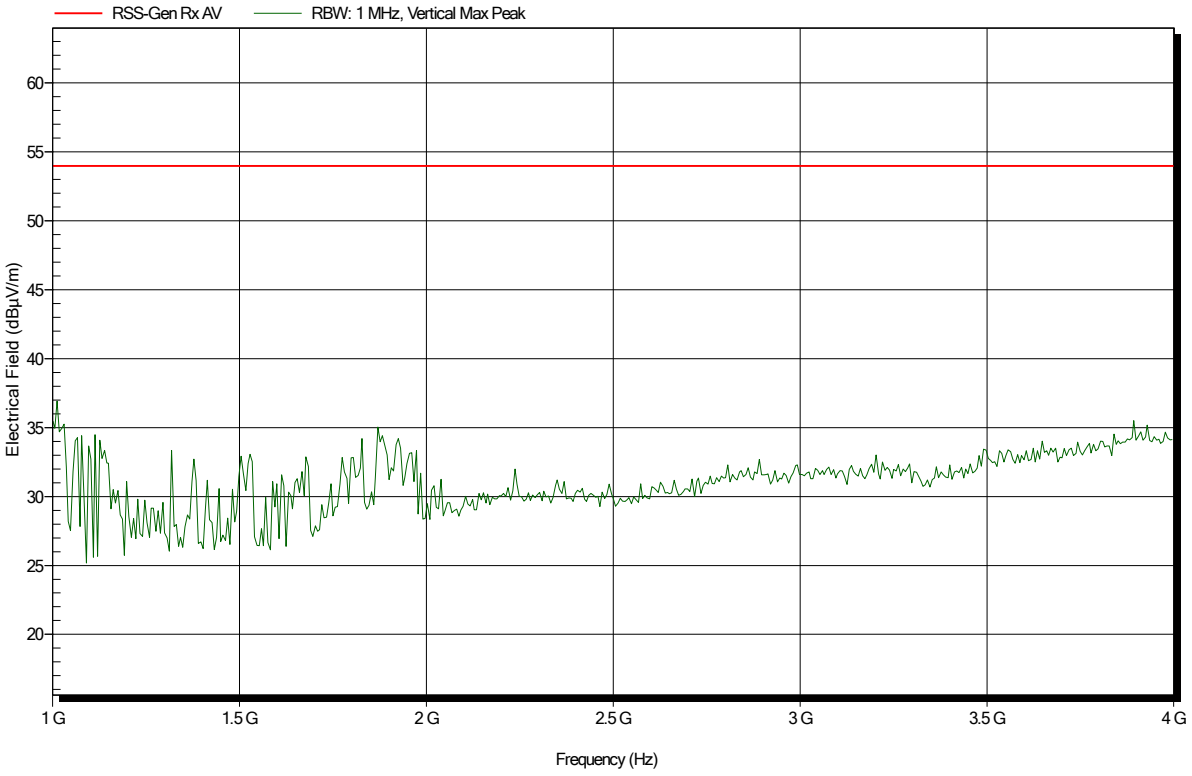

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 9

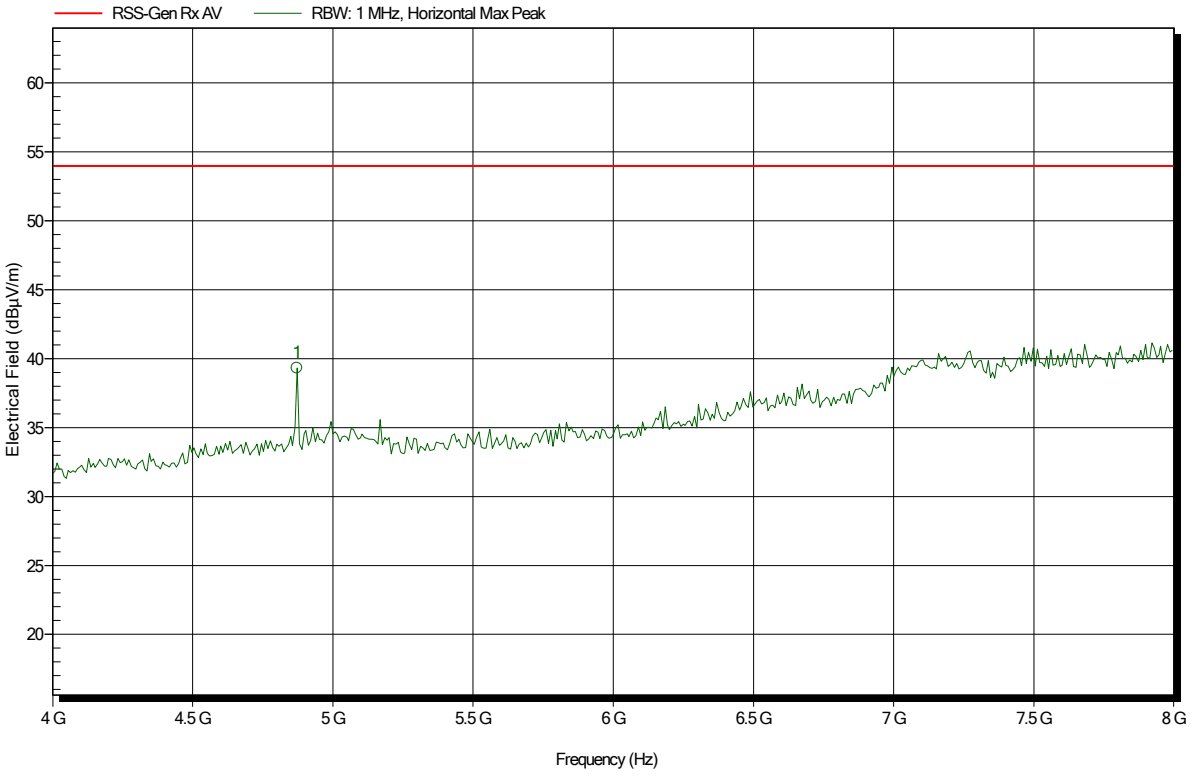

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.872 GHz	39.33 dBµV/m	53.98 dBµV/m	-14.65 dB	Pass

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Operator:	Florian Voigt (supervised)
Measurement software:	RadiMation, version 2015.2.4
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 6

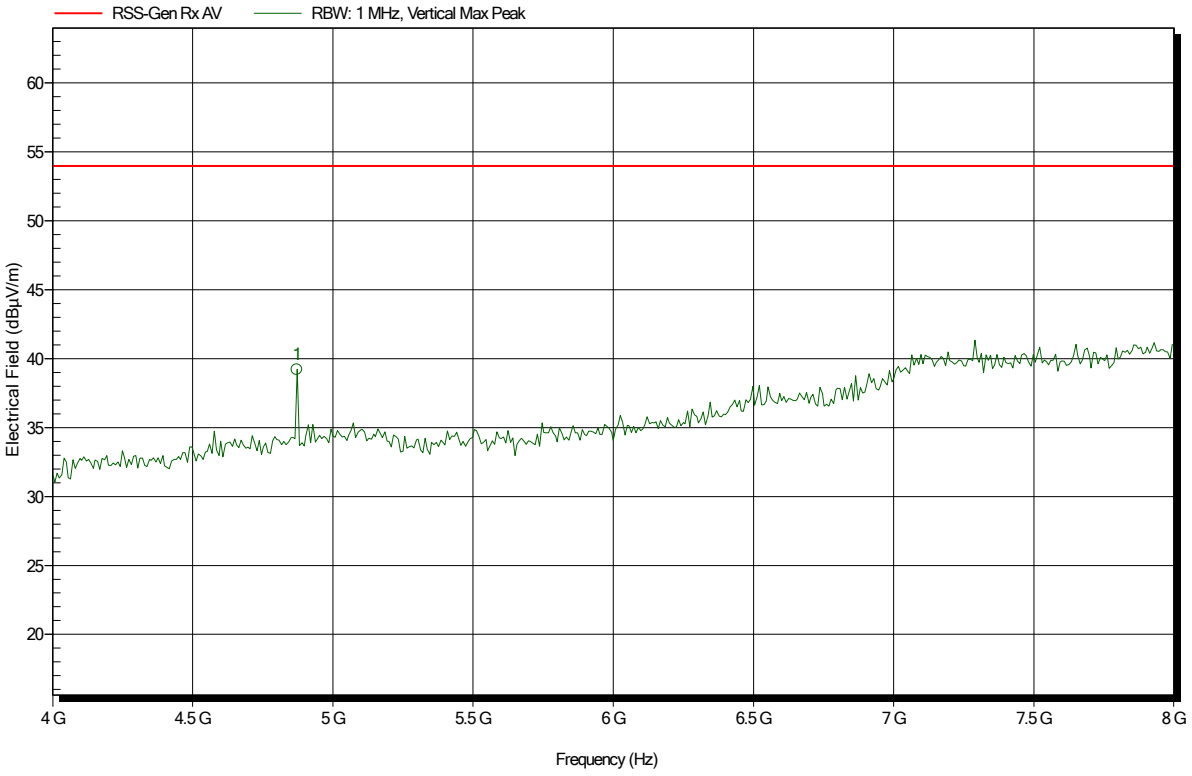

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.872 GHz	39.22 dBµV/m	53.98 dBµV/m	-14.76 dB	Pass

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Measurement software:	RadiMation, version 2015.2.4
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	1 m converted to 3m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	

Index 8

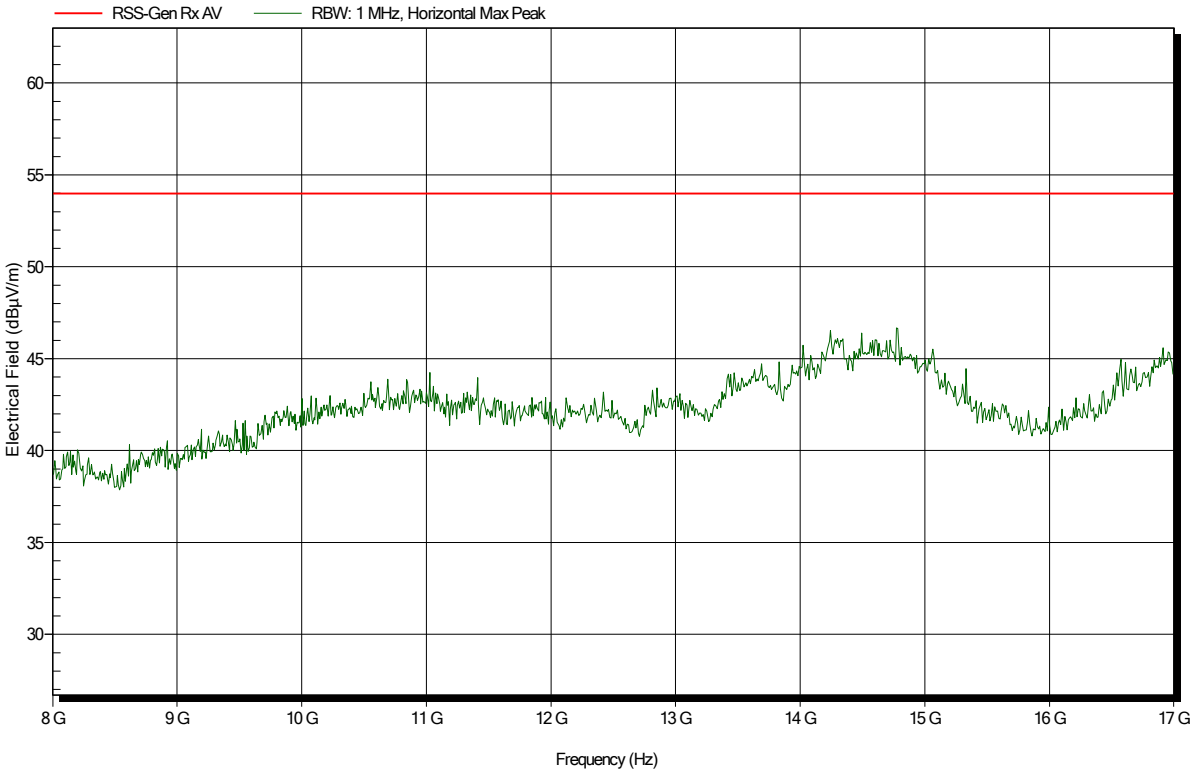

Spurious emissions according to ISED RSS-247

Project number:	G0M-2003-8888
Applicant:	GWA Hygiene GmbH
EUT Name:	Hygiene-Monitoring-System
Model:	NosoEx Point of Care / Drucksensor
Test Site:	Eurofins Product Service GmbH
Measurement software:	RadiMation, version 2015.2.4
Operator:	Florian Voigt (supervised)
Test Conditions:	Tnom: 24.8°C, Vnom: 3.3 VDC
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	1 m converted to 3m
Mode:	RX; BTLE, 2440MHz, 1MBit/s
Test Date:	2020-04-07
Note:	
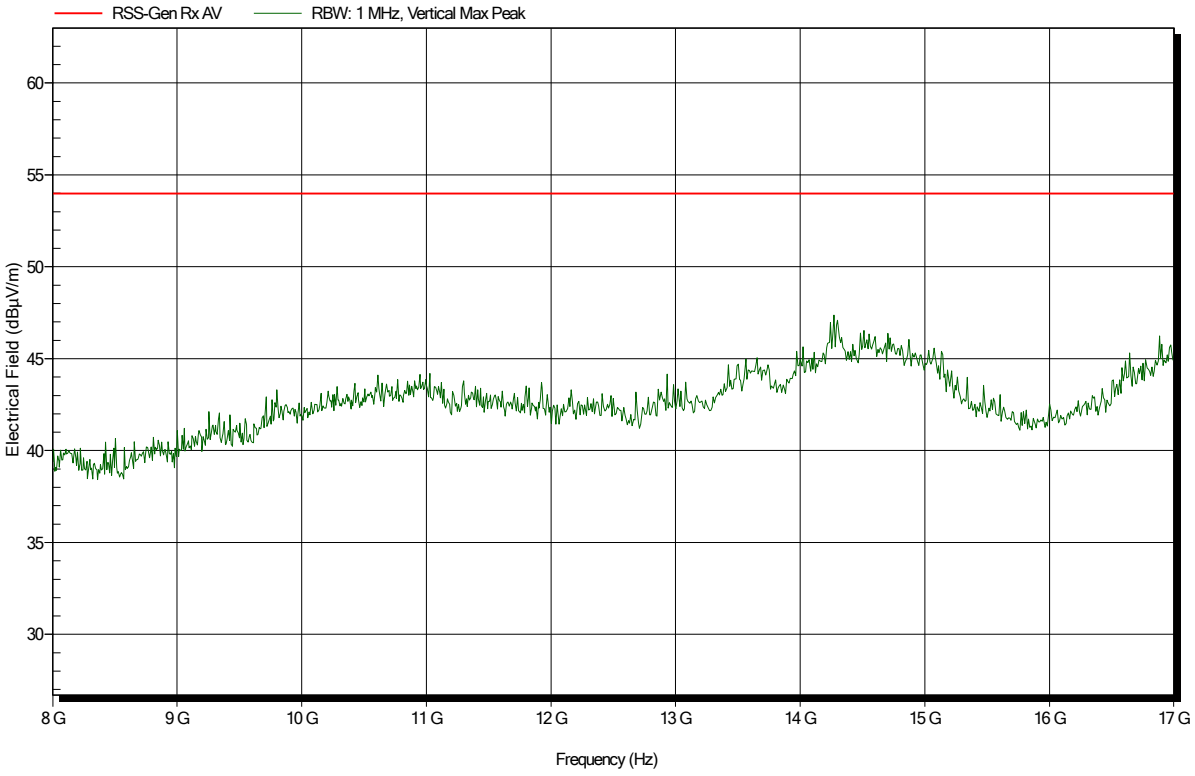
Index 7