

Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2600

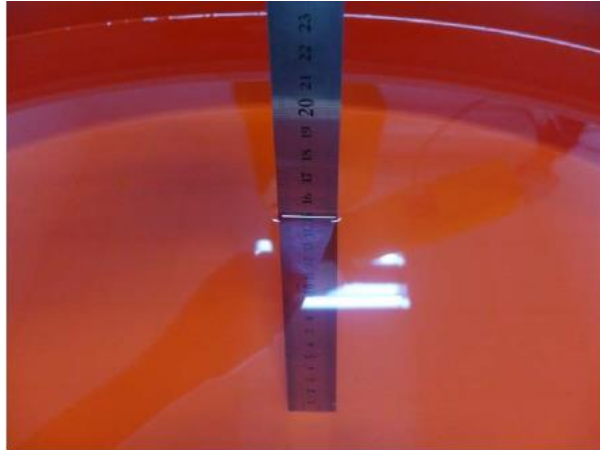

3. Photographs of EUT test position

Photo 2: Horizontal Down 5mm	Photo 3: Horizontal up 5mm
	
Photo 4: Vertical Front 5mm	Photo 5: Vertical Back 5mm
	
Photo 6: Tip mode 5mm	Photo 7: Bottom side 5mm
	

Photo 8: Horizontal Down 90° 5mm	Photo 9: Horizontal Down 180° 5mm
	

4. EUT Constructional Details

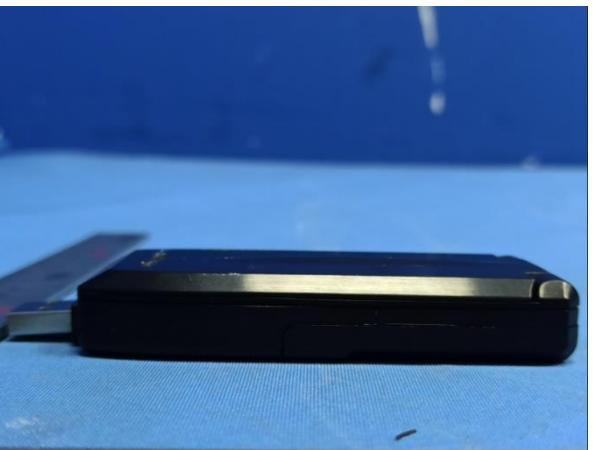
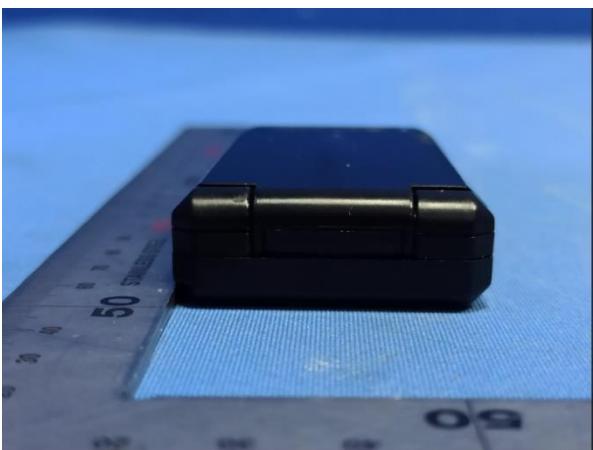
Photo 10: Front View	Photo 11: Back View
	
Photo 12: Left View	Photo 13: Right View
	
Photo 14: Top View	Photo 15: Bottom View
	

Photo 16: Front view with cover open



Photo 17: Left view with cover open with 90°



Photo 18: Left view with cover open with 180°

