

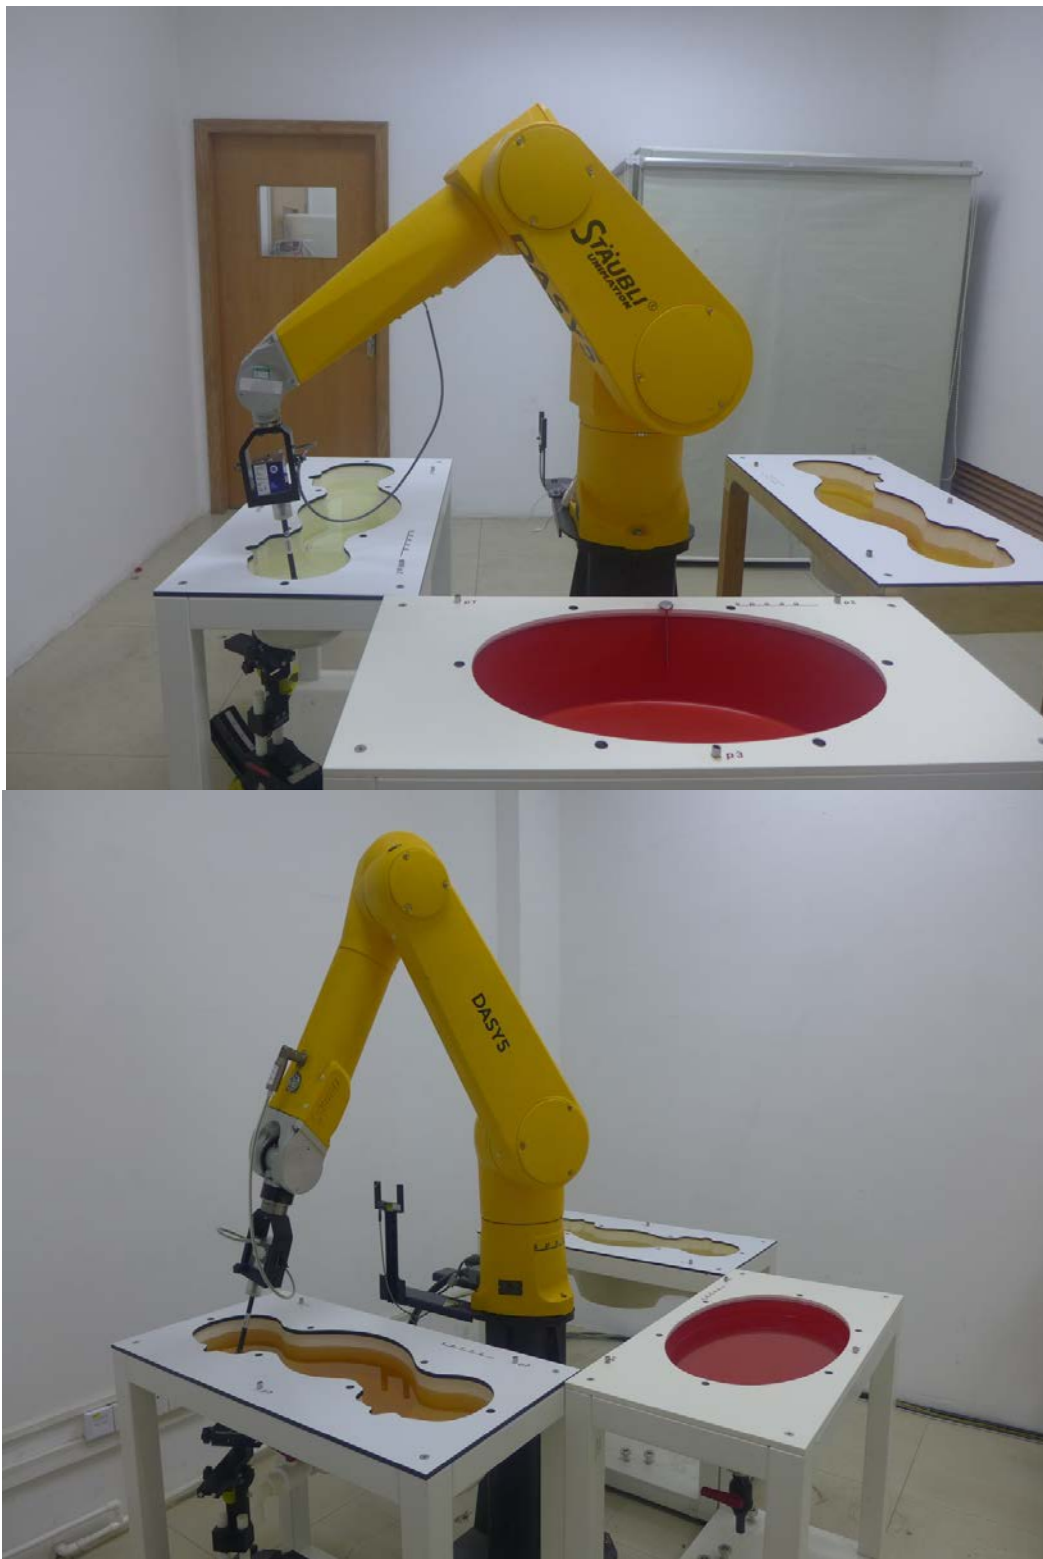


Appendix D

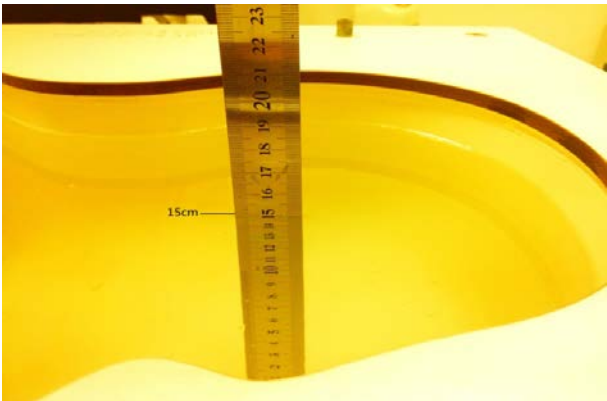
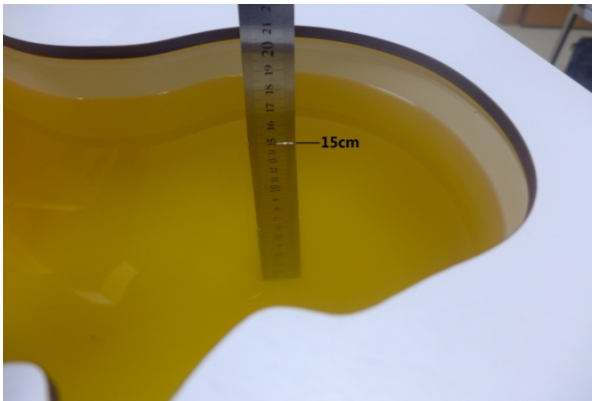
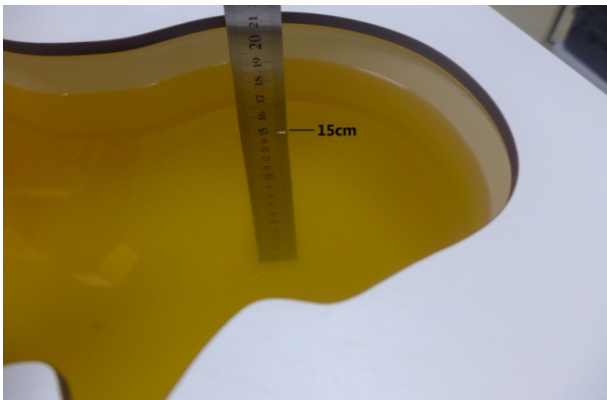
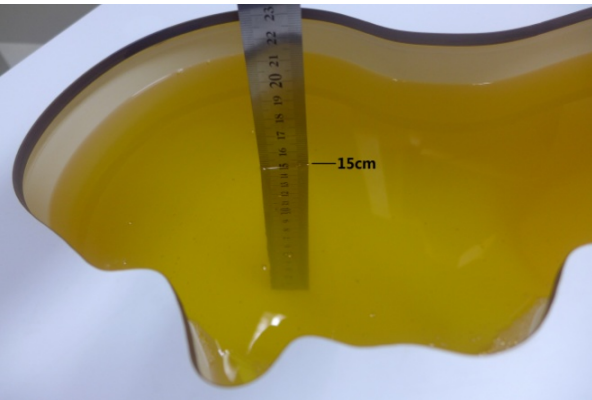
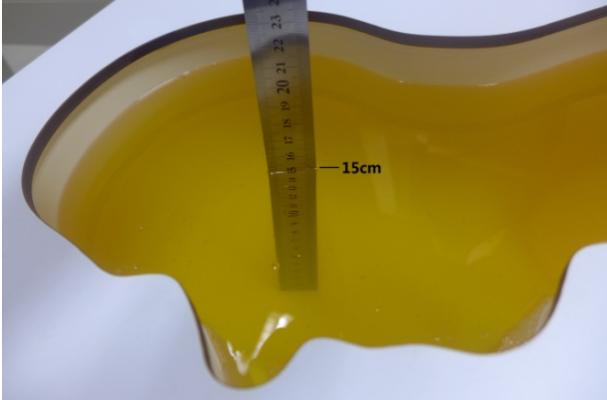
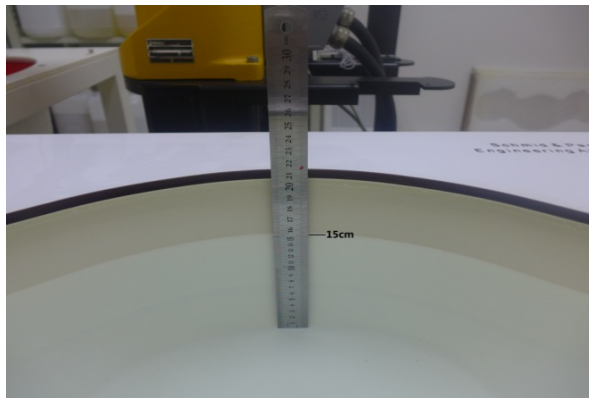
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1750
	
Photo 3: issue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Head 2450
	
Photo 5: Tissue Simulant Liquid for Head 2600	Photo 6: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position

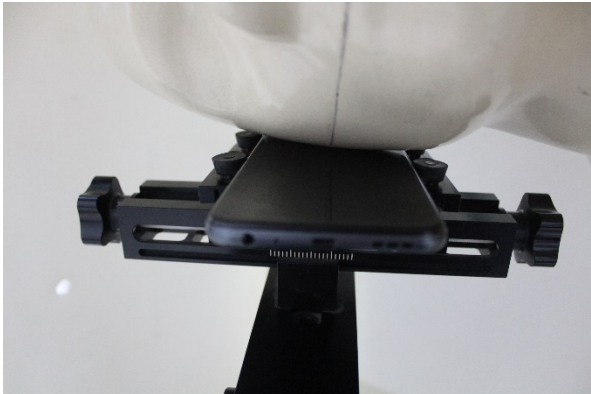
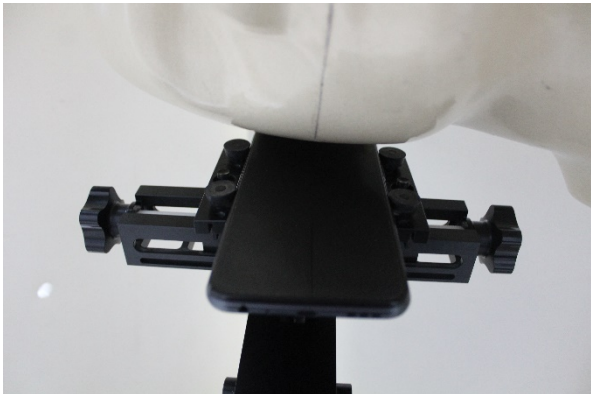
Photo 7: Left cheek	Photo 8: Right cheek
	
Photo 9: Right tilted	Photo 10: Back side 10mm
	
Photo 11: Right side 10mm	Photo 12: Top side 10mm
	

Photo 13: Bottom side 10mm	Photo 14: Back side 15mm
	
Photo 15: Back side 0mm	Photo 16: Top side 0mm
	

4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
	