

PURPOSE

This document is the master of instructions for use for NICCI technology.

SCOPE

n/a

REFERENCES

Ref	Doc ID	Version	Document Title
[1]	LAB-000194	04	NICCI System instructions for use set-up and design specification
[2]	SDS-000056	06* ²	CNAP - Alarms & Messages
[3]	REQ-000036	05	PR00678 Default Parameter
[4]	SDS-000062	01* ¹	UI Integration Manual - User Interaction Specifications

*¹ The IFU contents are according to Polarion baseline 23.07.2019.

*² Every message is listed only once in the IFU (despite the different error codes).

CHANGE HISTORY

Version	Edit Date	Description	Issuer	Reference to the project (DCC, DCP)
01	28 May 2019	First release	I. Sichna	VIENNA
02	27 July 2019	- Update of 'Alarms and messages' according to SDS-000056-05. - Changes in the SW description: - Explanation of grey bars in the pressure parameter field; - Addition of the term 'CO calibration' to the index; - Explanation of the curve icon in the NIBP history table. - Format improvements in chapter 'D2 NICCI Sensor activation'. - Changes in the description of 'NIBP only' mode (chapter new 'E2 NIBP only measurement') - Minor wording/pictures improvements in the chapter 'Setup&start'. - Updates according to LAB-000194-02: - chapter A1-3 (impact of RAC-000498-06). - chapter B3 (impact of REQ-000065-08 and REQ-000036-05) - chapter A4-6: transfer of new/removing/update of warnings/cautions/notes - appendix O (addition of rated range of the sensor cuffs pressure 0-280 mmHg)	I. Sichna	VIENNA

03	13 Aug. 2019	1. Minor wording/pictures improvements in the chapter 'Setup&start'. 2. Appendix O: addition of rated measurement range (20-250mmHg). 3. Update of 'Alarms and messages' according to SDS-000056-06.	I. Sichna	VIENNA
04	5 Sept. 2019	1. Chapter K: update according to LAB-000194-03 (update of cleaning and disinfection agents, impact of REQ-000065-09).	I. Sichna	VIENNA
05	18 Sept. 2019	1. Table 15 (electromagnetic immunity): update of ESD test level and ESD compliance level	I. Sichna	VIENNA
06	17 Dec. 2019	1. Addition of the placeholder for IFU unique identifier on the last page.	I. Sichna	VIENNA
07	27 Jan. 2020	1. Chapter P: update according to LAB-000194-04 (ESD test level and ESD compliance level). 2. Chapter O: update of the weight of the NICCI Upper Arm Cuff.	I. Sichna	DCC-19-062 DCC-19-089



NICCI Technology

Operator's Manual

GETINGE 

NICCI components

Table 1 – NICCI components

NICCI components		Component variants	Article numbers
	NICCI Module	NICCI Module	PC6500
	Connected to the host monitor PulsioFlex PC4000		
	NICCI Mouse*	NICCI Mouse	PC6510
	Connected to the NICCI Module		
	NICCI Upper Arm Cuff*	NICCI Upper Arm Cuff, S	PC6531
		NICCI Upper Arm Cuff, M	PC6532
		NICCI Upper Arm Cuff, L	PC6533
		NICCI Upper Arm Cuff, XL	PC6534
	Connected to the NICCI Module		
	NICCI Sensor*	NICCI Sensor S, single use	PV6550
		NICCI Sensor M, single use	PV6551
		NICCI Sensor L, single use	PV6552
		Connected to the NICCI Mouse	

*Not made with Natural Rubber Latex

NICCI compatibility:

PulsioFlex PC4000 equipped with the software version 6.0 or higher.

About this manual

This manual is an extension to the **PulsioFlex operator's manual** (PC406*) that specifically describes the NICCI technology integrated into the PulsioFlex monitor PC4000. Both manuals need to be considered.

* plus two digit language code according to ISO 639-1



This icon indicates a hazardous situation that, if not avoided, could result in death or serious injury. It may also describe potential serious adverse reactions and safety hazards. Additionally, the **WARNING** is generally used as the signal word.



This icon indicates a hazardous situation that, if not avoided, could result in minor or moderate injury. Additionally, the **CAUTION** is generally used as the signal word.



This icon indicates information considered important, but not hazard-related. The icon indicates items of information for which careful attention must be paid in order to avoid damage to the equipment or inaccurate data as well as operational errors. Additionally, the **NOTE** is generally used as the signal word.



This icon indicates helpful user information.

All figures contained in this manual are examples and are subjects to change without further notice. Some localization rules in the figures may be omitted.

Contents

NICCI components	III
About this manual	IV
Contents	V
List of figures	VII
List of tables	VIII
Frequently used functions	IX
A General information	10
1 Intended Use	10
2 Indications for Use	10
2.1 Intended Patient Population	10
2.2 Intended Body Parts (Interacted With)	10
2.3 Intended User Profile	10
2.4 Intended Use Environment	10
3 Contraindications	10
4  Warnings	10
5  Safety instructions	12
6  Notes	12
7 Additional use	12
B NICCI technology	13
1 Technology principle	13
2 Technology components	13
2.1 NICCI Module	14
2.2 NICCI monitoring units	15
2.2.1 NICCI Sensor	15
2.2.2 NICCI Mouse	16
2.3 NICCI Upper Arm Cuff	16
3 Parameters and ranges of normal values	16
C NICCI setup & start	18
1 Attachment of the NICCI Module to the PulsioFlex Monitor	18
2 Attachment of NICCI monitoring units	18
2.1 Selection of the NICCI Sensor	18
2.2 Attachment of the NICCI Sensor	19
3 Selection and attachment of the NICCI Upper Arm Cuff	20
D NICCI measurement	21
1 Patient data	21
1.1 Entering patient data	21
1.2 NICCI Sensor functions	21
2 NICCI Sensor activation	22
2.1 New NICCI Sensor	22
2.2 Activated NICCI Sensor	23

3	Measurement via PulsioFlex.....	23
4	Measurement via NICCI Module.....	24
E	NIBP measurement modes.....	25
1	NIBP modes for continuous NICCI measurement	25
1.1	NICCI NIBP	25
1.2	Manual NIBP input.....	26
2	NIBP only measurement.....	27
F	End of treatment	28
G	NICCI additional configuration: transmission of blood pressure values to patient monitor	29
H	NICCI graphical user interface: elements and options.....	30
1	Real time pressure curve.....	30
2	Parameter fields	30
2.1	Pressure settings screen	30
2.1.1	Zero AP Out to Patient Monitor subscreen.....	31
2.2	NIBP and Finger Change screen	31
2.2.1	NICCI BP Settings subscreen	32
2.3	Parameters screen.....	33
2.3.1	CO/CI calibration subscreen.....	34
3	Trend curves screen.....	34
I	NICCI Module markings & functions	36
1	Control buttons	36
2	LED status lights.....	36
3	Connector markings	36
J	Alarms and messages	37
1	Parameter alarms	37
2	Parameter alarm limits.....	37
3	Technical alarms	38
4	Physiological alarms.....	41
5	General alarms	41
K	Cleaning & disinfection	43
L	Disposal	43
M	Service & maintenance.....	43
N	Appendix - Accessories & detachable components.....	44
O	Appendix - Technical data & essential performance	45
P	Appendix - Electromagnetic compatibility	47
Q	Appendix - Technical specifications - Near Field Communication.....	50
R	Appendix - Technical specifications - Light source equipment	51
	Symbols.....	53
	Index	54
	Information	55

Q Appendix - Technical specifications - Near Field Communication

The NICCI uses Near Field Communication (NFC) technology to enable communication between the NICCI Mouse and NICCI Sensor without electrical connection.


This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation'.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- *Reorient or relocate the NICCI Mouse, which integrates the receiving antenna.*
- *Increase the separation between the equipment and the NICCI Mouse.*
- *Consult an experienced technician for help.*

Functional description

NFC is an international transmission standard for the wireless exchange of data over the short distances. During operation of the NICCI, the following data is exchanged between the NICCI Mouse and the NICCI Sensor:

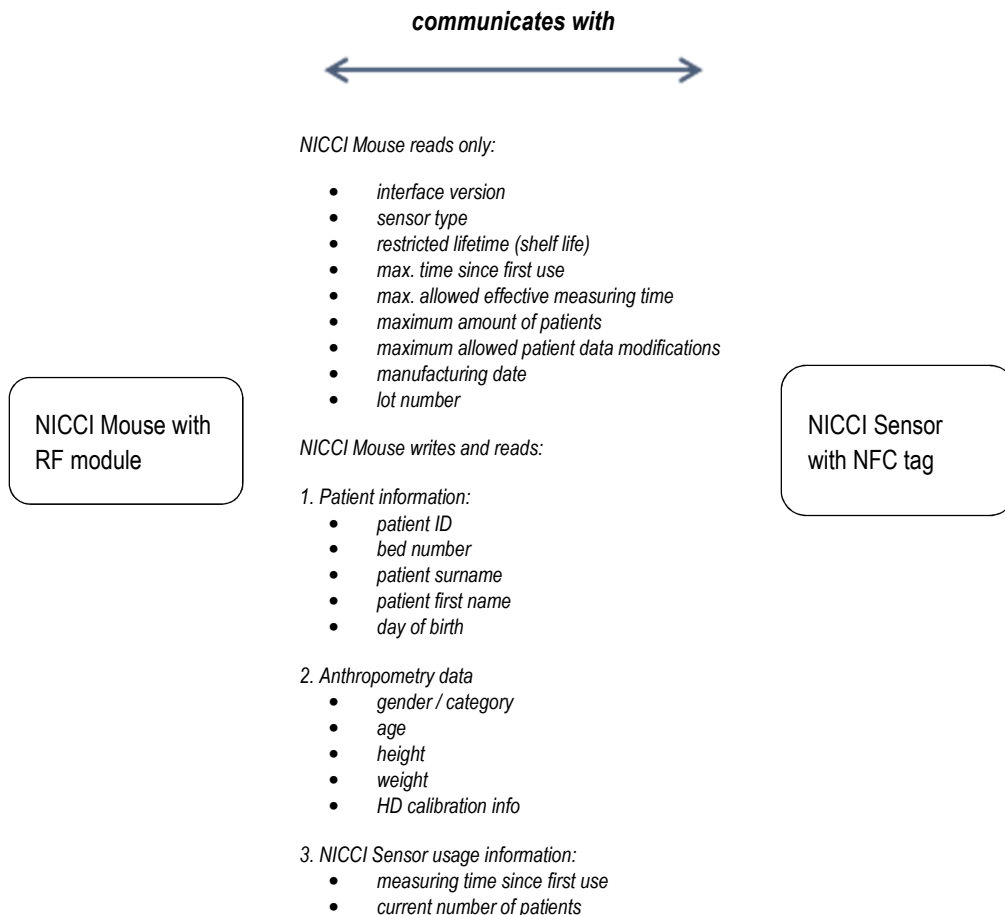

- *current patient data modifications*
- *date of first use*
- *current date of use*

Technical description

In general, a radio frequency module is (usually) a small electronic device used to transmit and receive the radio signals between two devices. The radio frequency module is a part of NICCI Mouse printed circuit board. It contains the NFC reader chip with an integrated antenna, which send and receive the data from a transponder.

When powered on and operating, the radio frequency module has two operating states:

1. The NICCI Sensor with its NFC tag is in the reading distance. The communication between NICCI Mouse and NICCI Sensor is possible.
2. The NICCI Sensor with its NFC tag is not in the reading distance. The communication between NICCI Mouse and NICCI Sensor is not possible.

The user cannot change the wireless communication specification such as operating mode, power level or bandwidth.

Table 18 – Technical data - Radio frequency module

Radio frequency module	
NFC reader chip	NXP CLRC663
NFC tag	NXP ICODE DNA (Type V)
Reading / writing mode	supports ISO/IEC 15693
Reading distance	less than 22 mm (measured from the NICCI Mouse surface)
Operating frequency	13.56 MHz
Operating mode	– operating – power off (no standby mode)
Power output (max.)	1.5 Watt

Restriction of data access

The data stored on the NFC tag is separated into different memory areas in order to restrict access to the violent data via third party devices (e.g. mobile phones):

1. NICCI Sensor information is stored on the NFC tag, is read-only and cannot be changed.
2. Patient information is given through the manual input by the user. In order to read or change the patient data, the radio frequency module inside of the NICCI Mouse uses an authentication key to encode the encrypted patient data on the NFC tag.

R Appendix - Technical specifications - Light source equipment

Table 19 – Technical data - NICCI Mouse LED

NICCI Mouse LED	
Output of optical radiation (max.)	890nm
Variation of output	2,13 W/cm ² (peak) 0,34 W/cm ² (average)
Pulse duration	0.18ms
Pulse interval	0.98ms

Information



PULSION Medical Systems SE

Hans-Riedl-Straße 17

85622 Feldkirchen

GERMANY

Phone: +49 – (0)89 – 45 99 14 – 0

Fax: +49 – (0)89 – 45 99 14 – 18

E-mail: info@pulsion.com

Internet: www.getinge.com

Protected by the following international and U.S. patent(s): <http://patents.getinge.com>.



Getinge is a global provider of innovative solutions for operating rooms, intensive care units, sterilization departments and for life science companies and institutions. Based on our firsthand experience and close partnerships with clinical experts, healthcare professionals and medtech specialists, we are improving the everyday life for people - today and tomorrow.

www.getinge.com



>> Space for IFU unique identifier/revision for commercial version<< · Copyright © >> Space for the issue date for commercial version<< by PULSION Medical Systems SE.