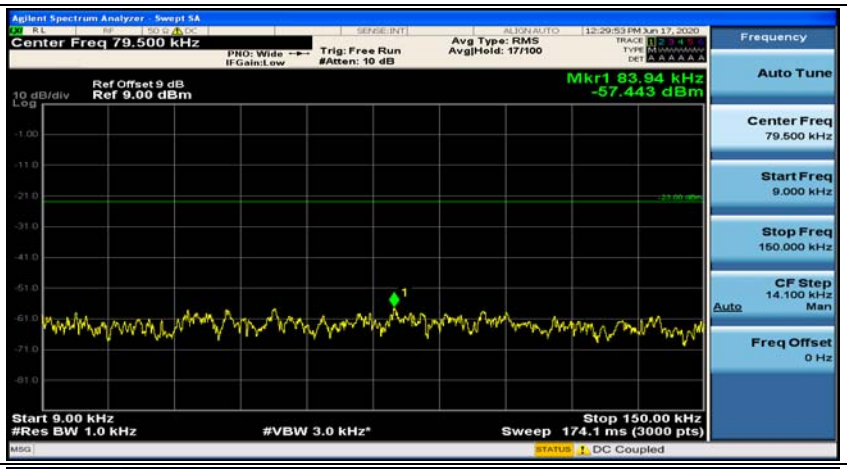
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:29:53 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 83.94 kHz
-57.443 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

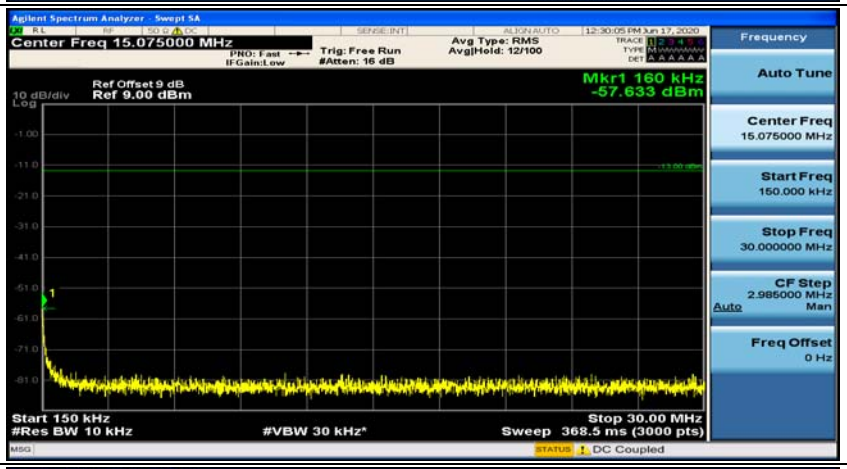
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:30:05 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-57.633 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

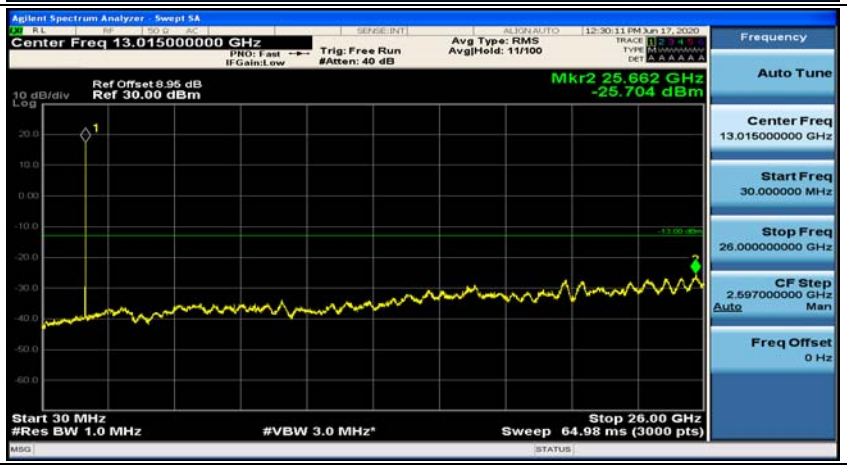
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:30:11 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.662 GHz
-25.704 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#0

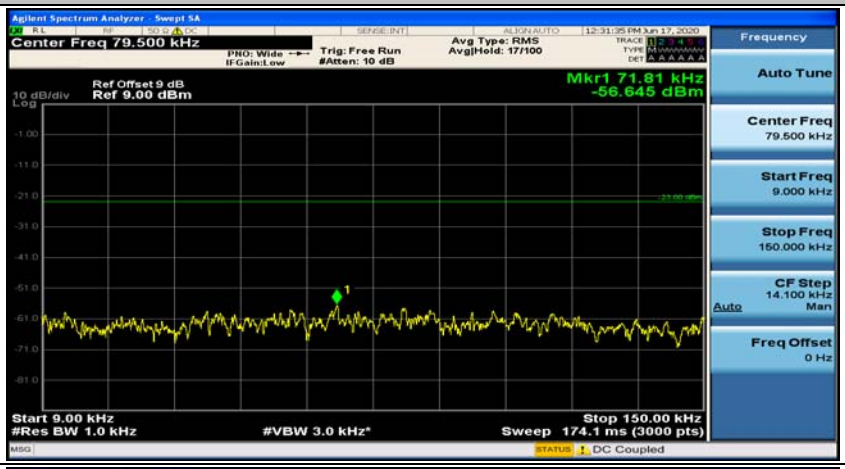

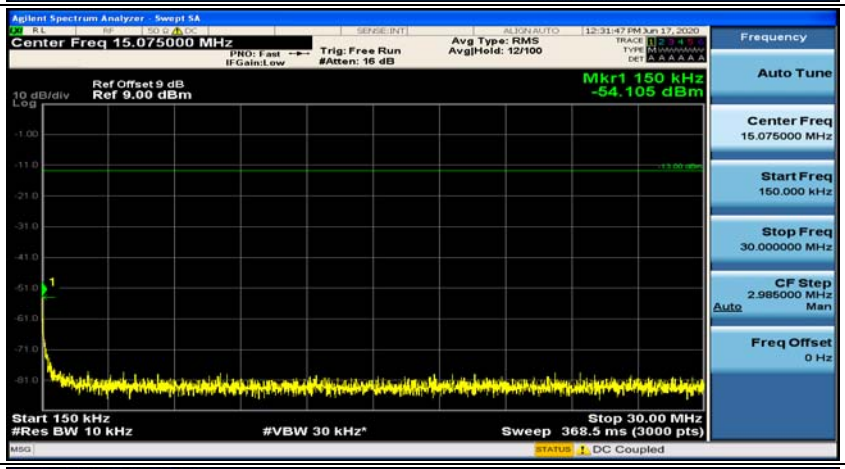

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#37

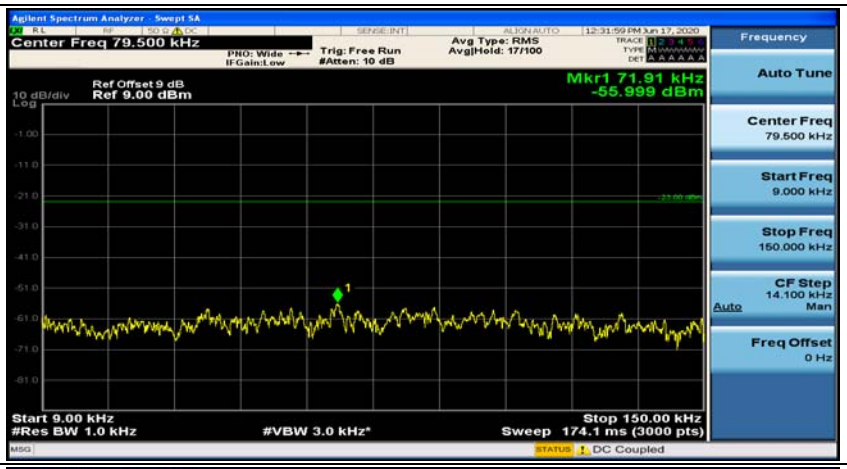

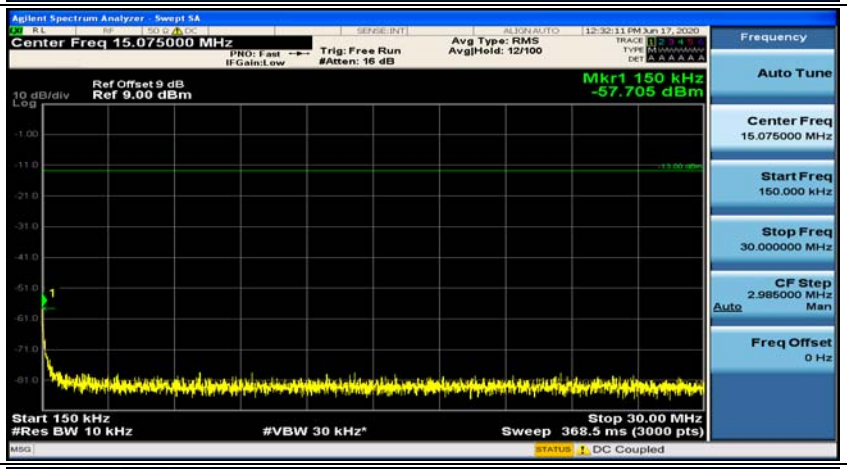

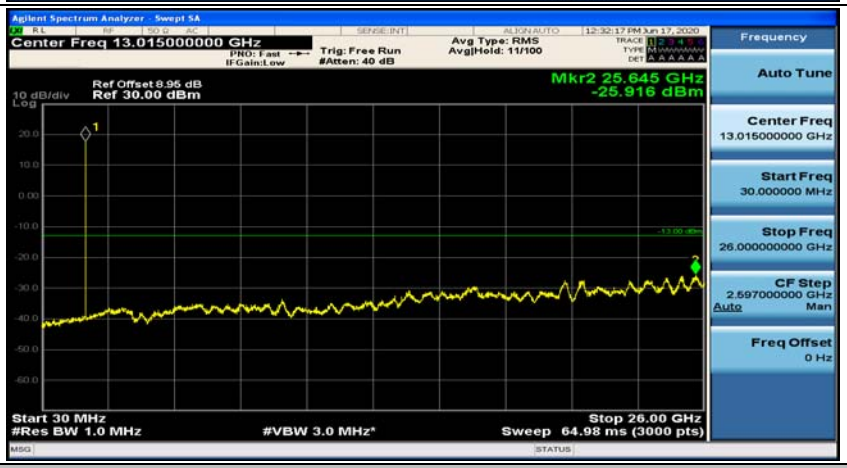

(Channel Bandwidth:15 MHz)_HCH_QPSK_1RB#74

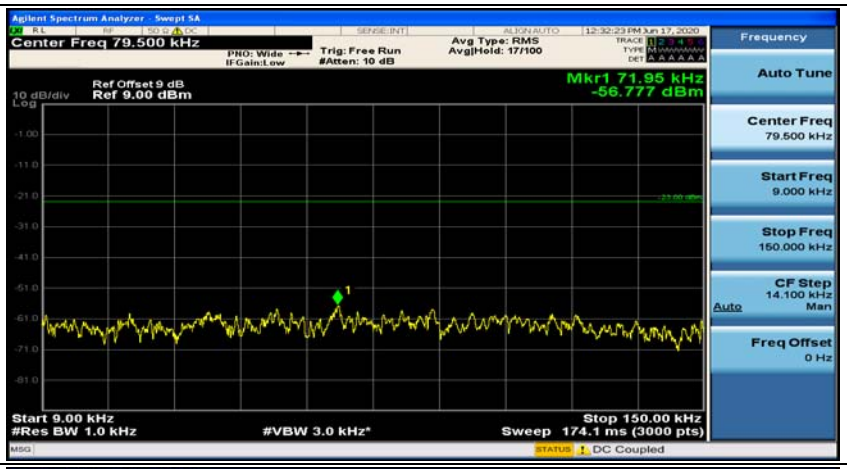
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:32:23 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 71.95 kHz
-56.777 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

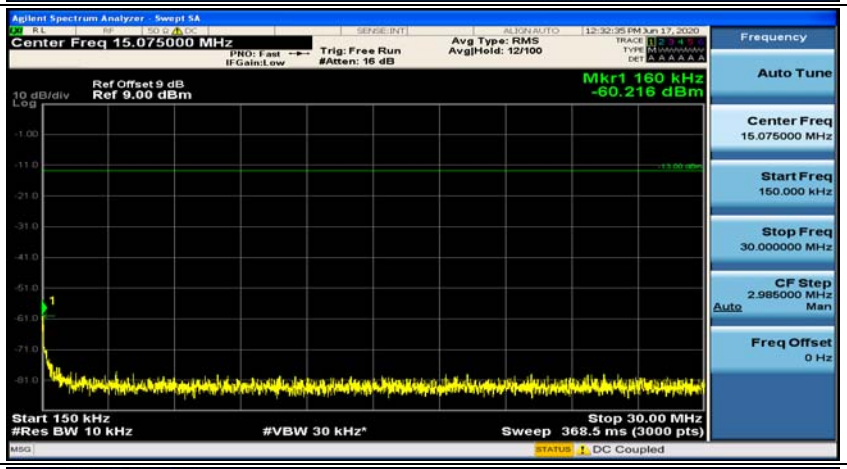
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:32:35 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-60.216 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

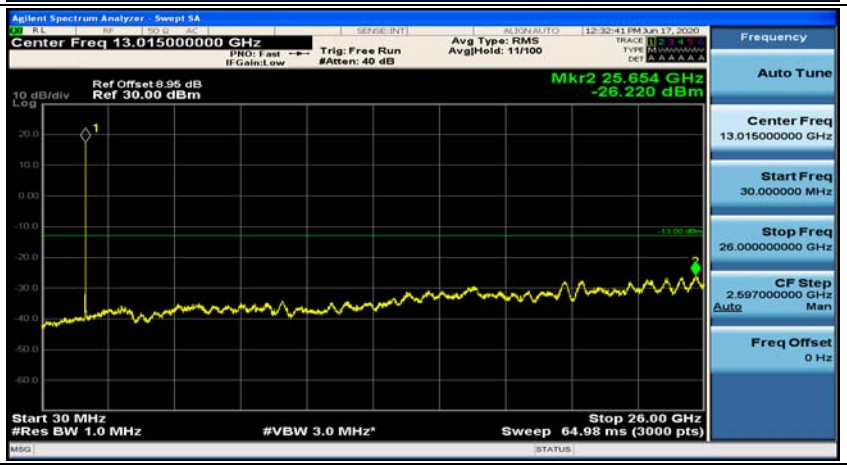
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:32:41 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.654 GHz
-26.220 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#0

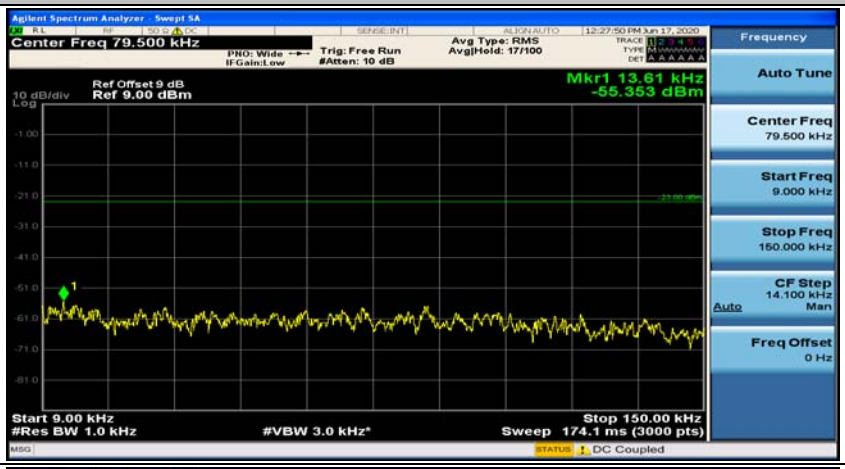

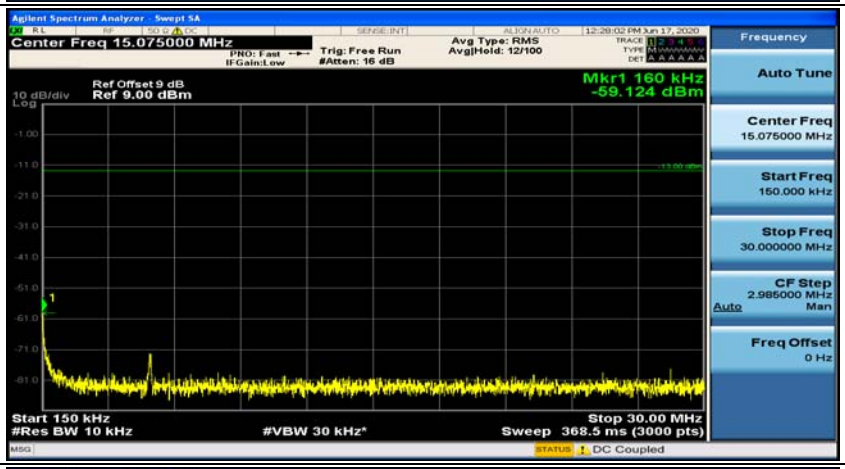

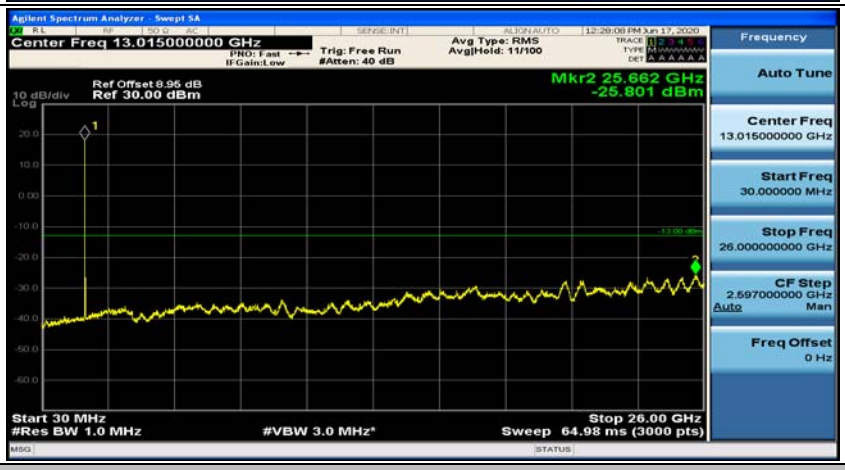

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#37

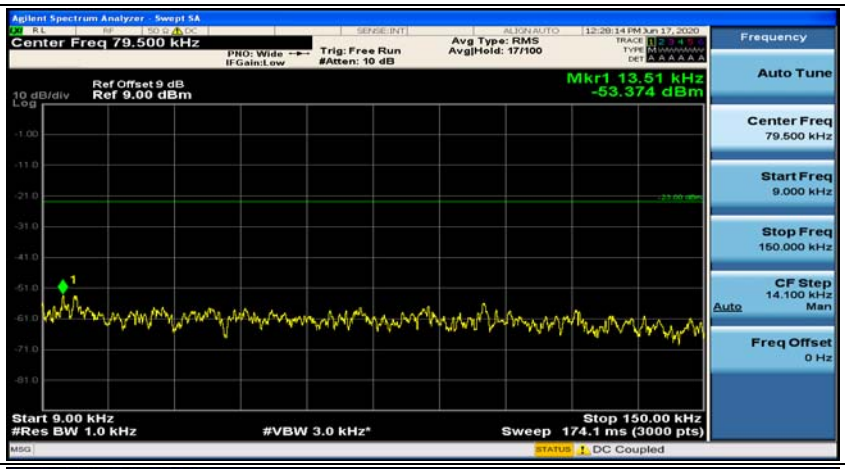

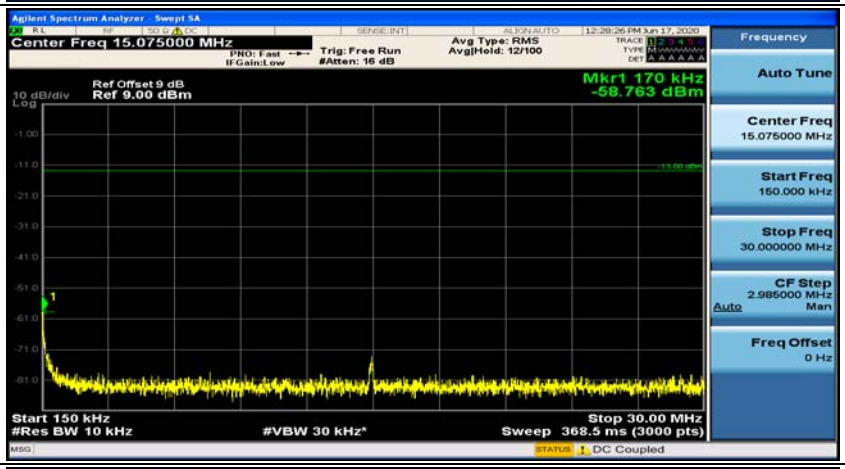

(Channel Bandwidth:15 MHz)_LCH_16QAM_1RB#74

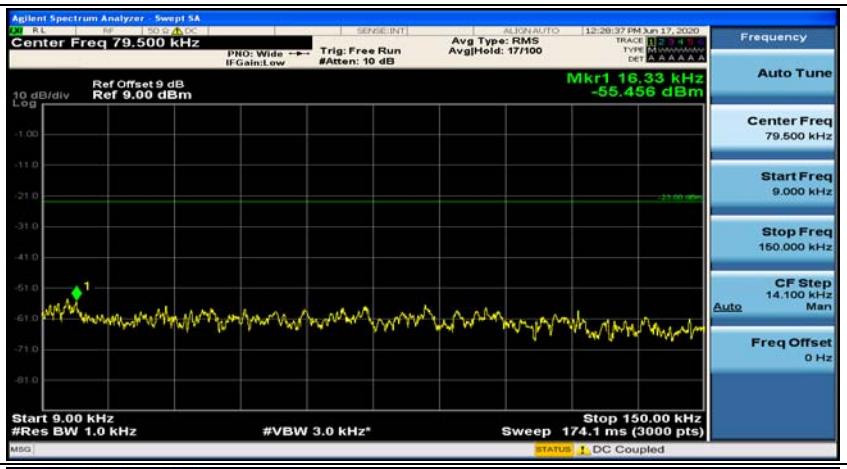
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:28:37 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 16.33 kHz
-55.456 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

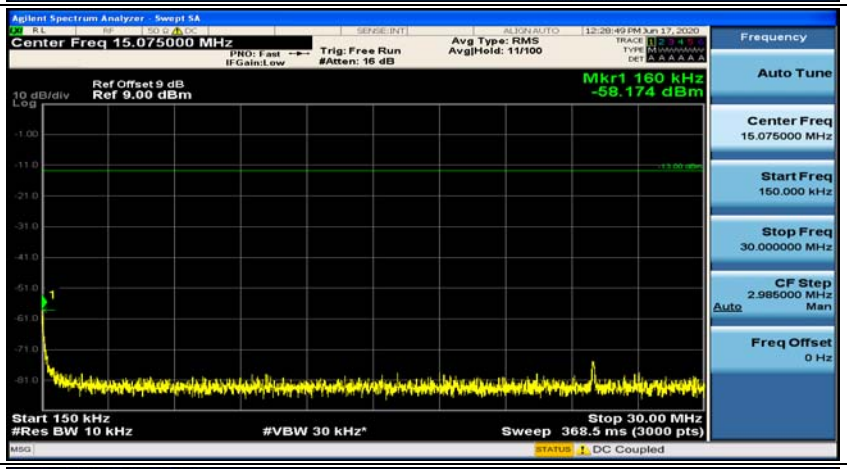
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
12:28:49 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.174 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

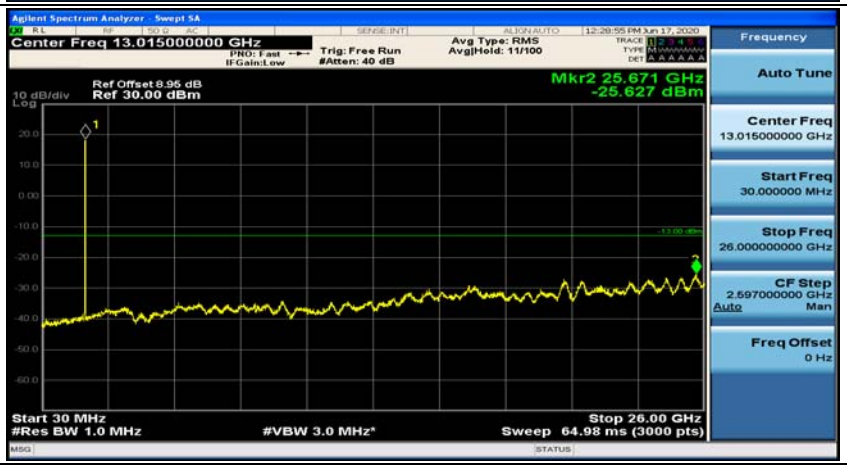
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:28:55 PM Jun 17, 2020
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.671 GHz
-25.627 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#0

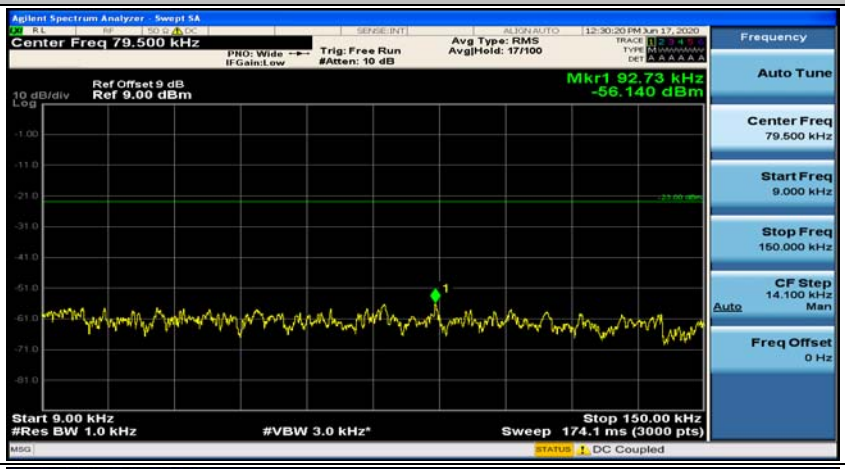

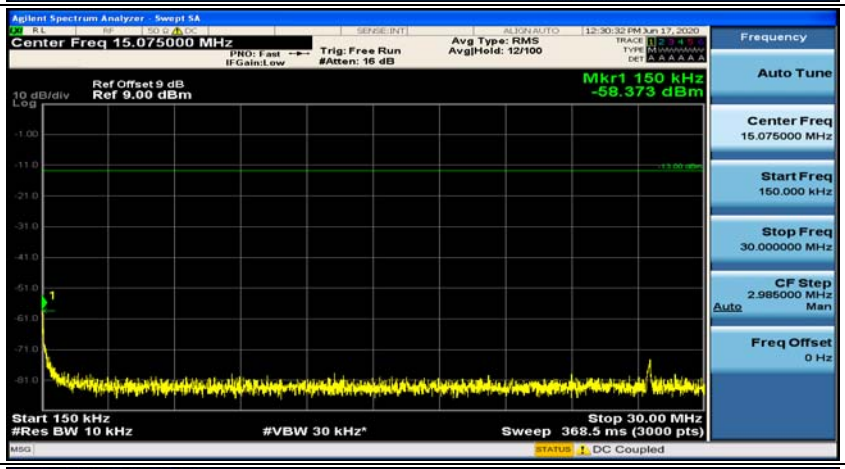

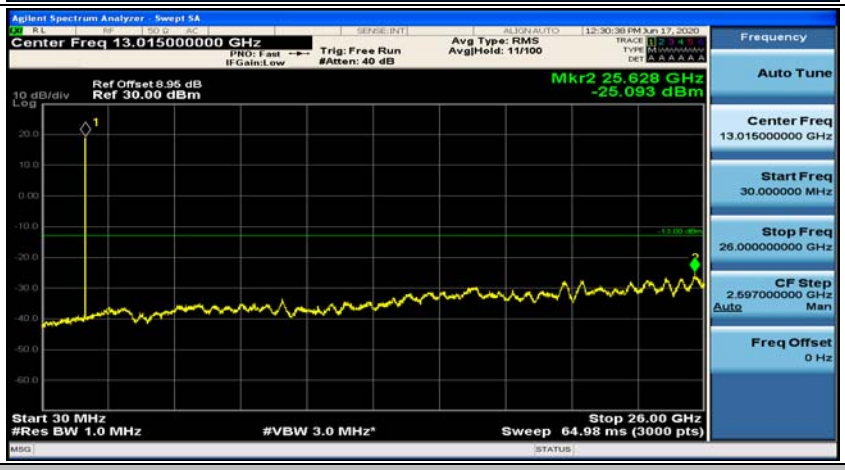

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#37

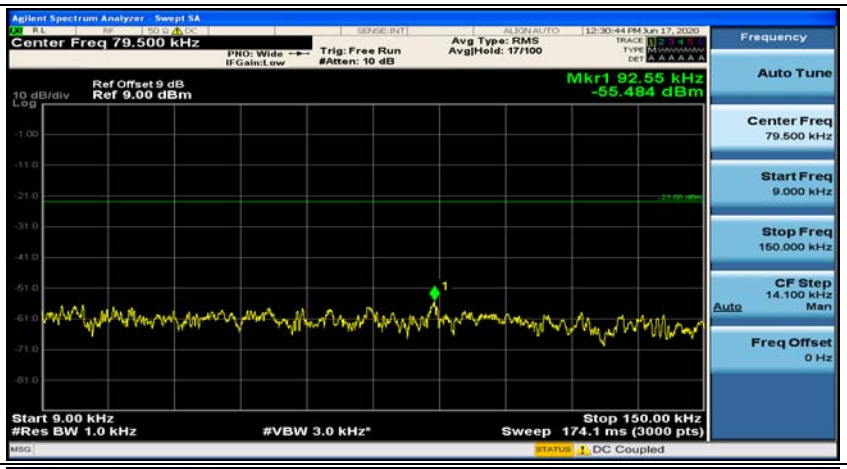

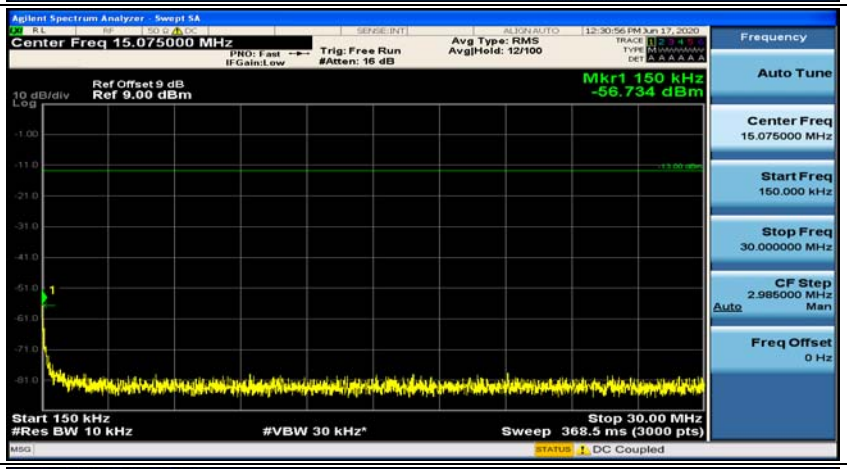

(Channel Bandwidth:15 MHz)_MCH_16QAM_1RB#74

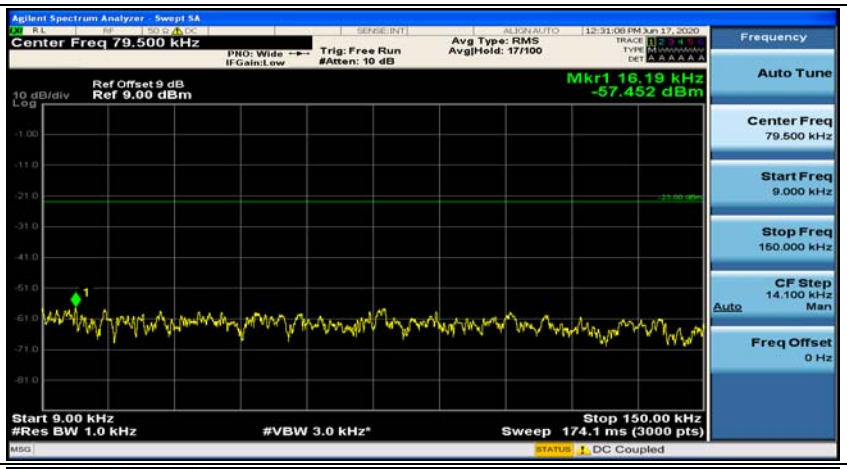
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:31:08 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 16.19 kHz
-57.452 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto Man
Freq Offset
0 Hz

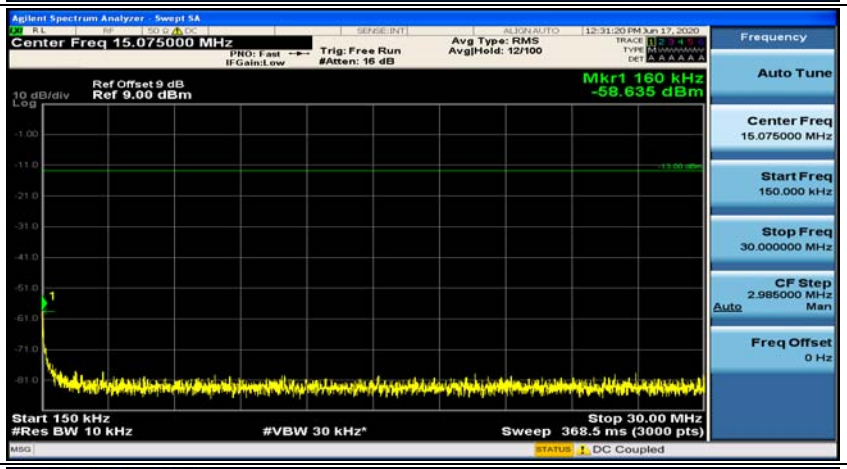
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:31:20 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 160 kHz
-58.635 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto Man
Freq Offset
0 Hz

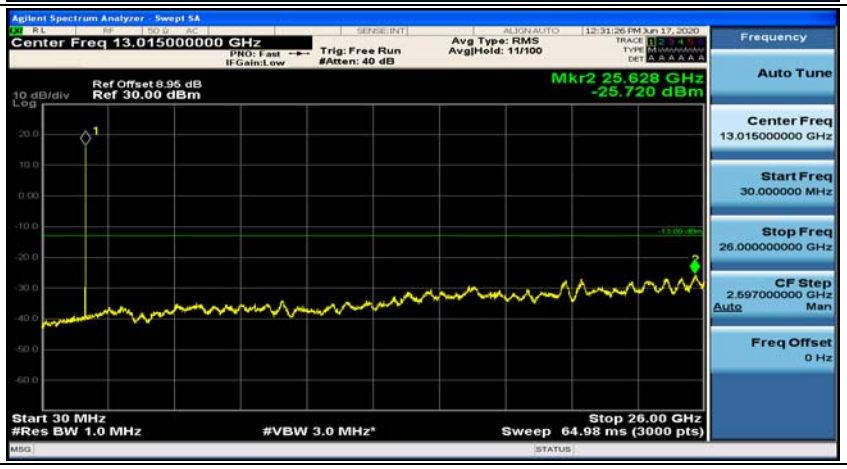
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:31:26 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Log
Mkr2 25.628 GHz
-25.720 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto Man
Freq Offset
0 Hz

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#0

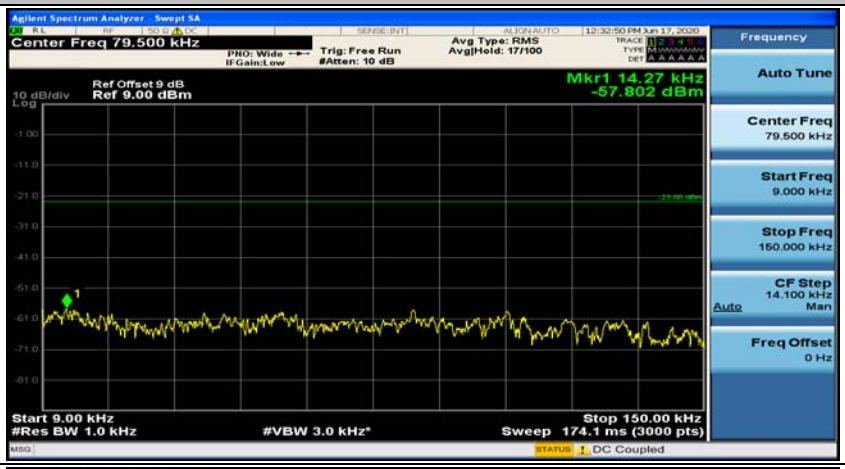

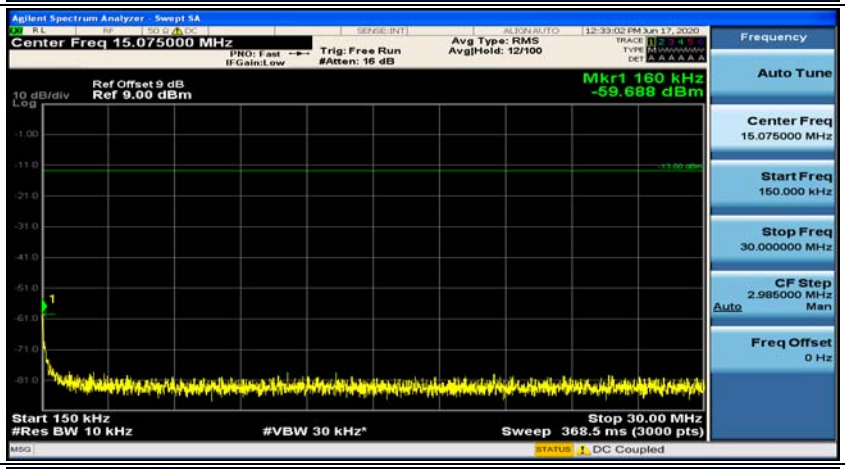

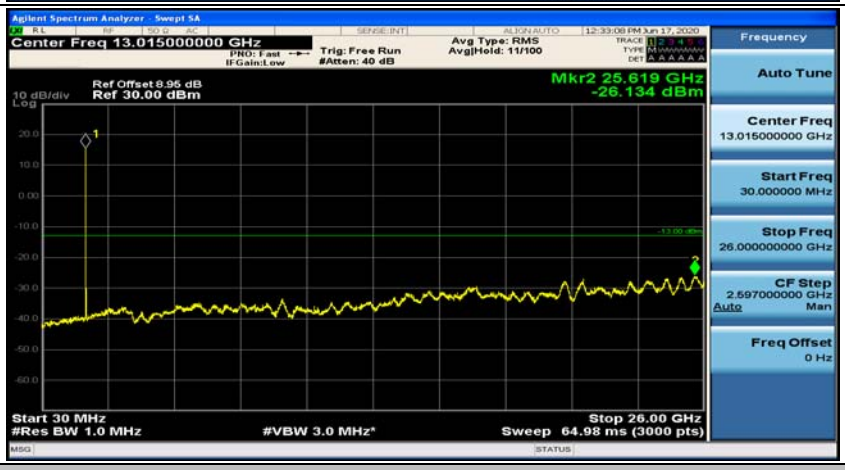

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#37

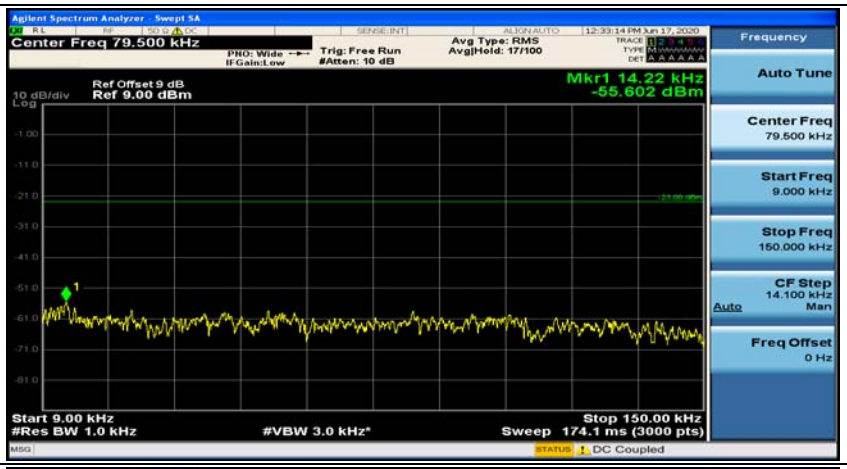

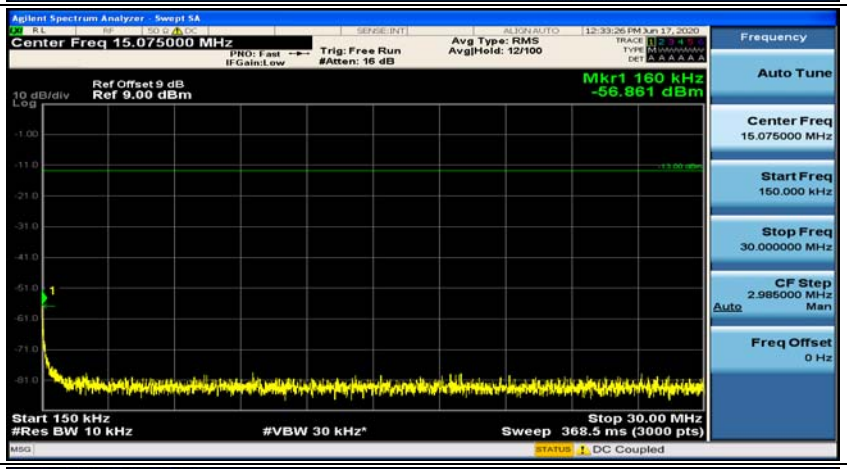

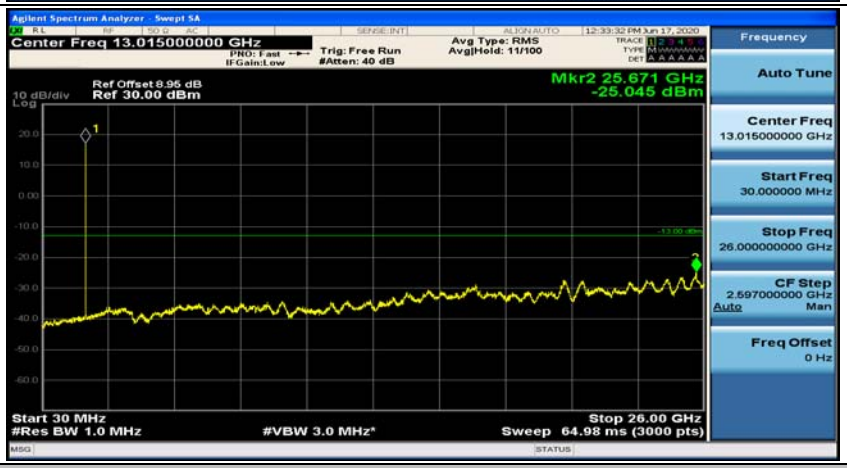

(Channel Bandwidth:15 MHz)_HCH_16QAM_1RB#74

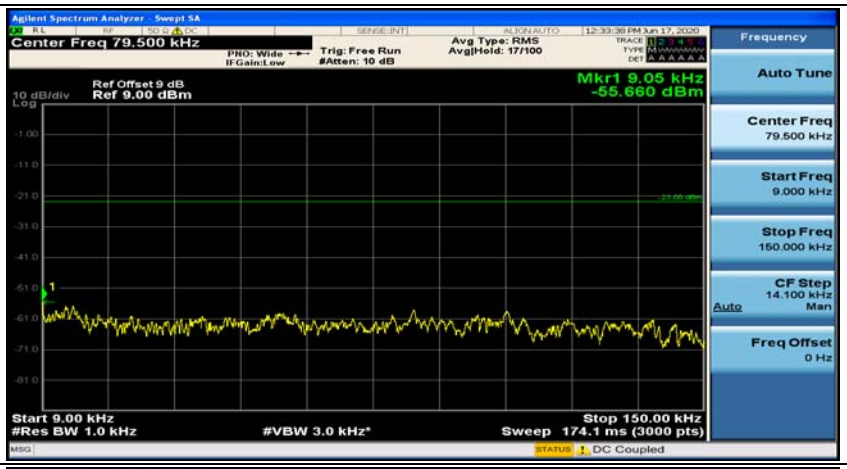
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:33:38 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 9.05 kHz
-55.660 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

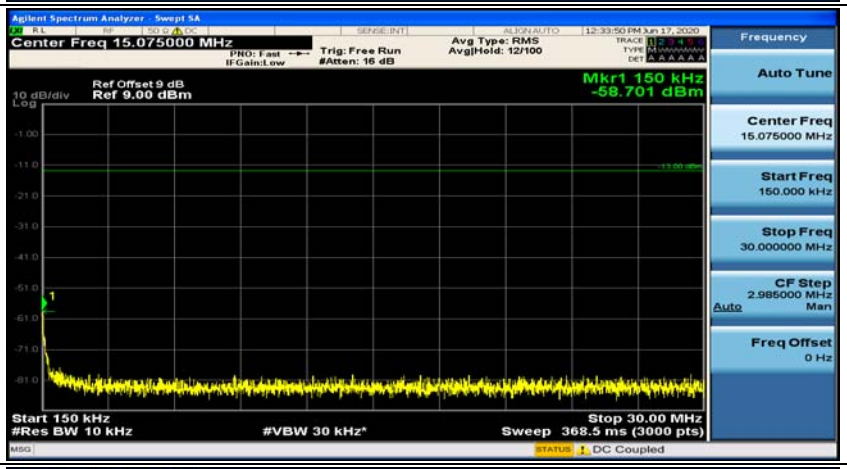
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:33:50 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-58.701 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

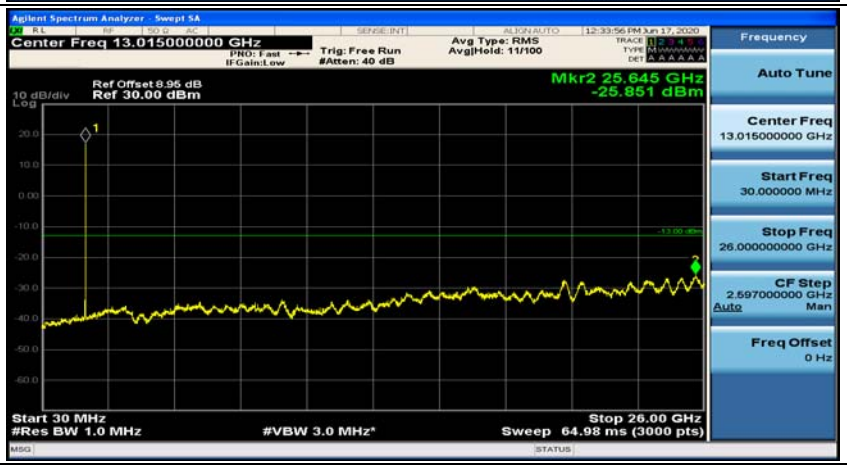
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:33:56 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Log
Mkr2 25.645 GHz
-25.851 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 20 MHz

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#0

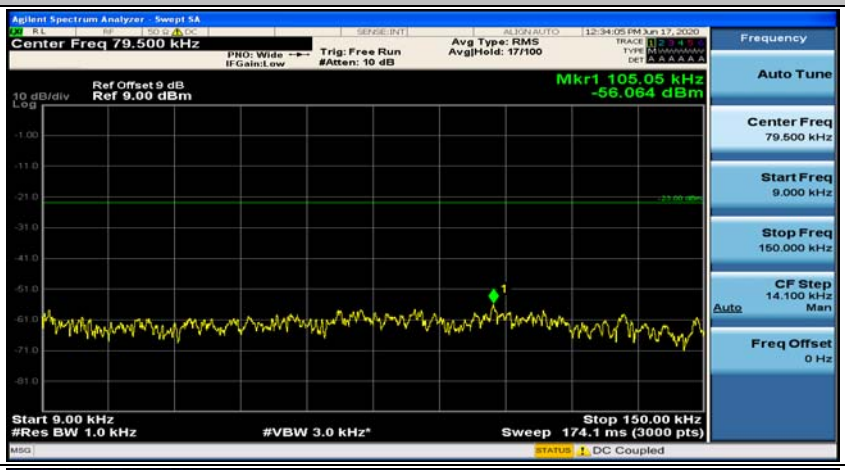

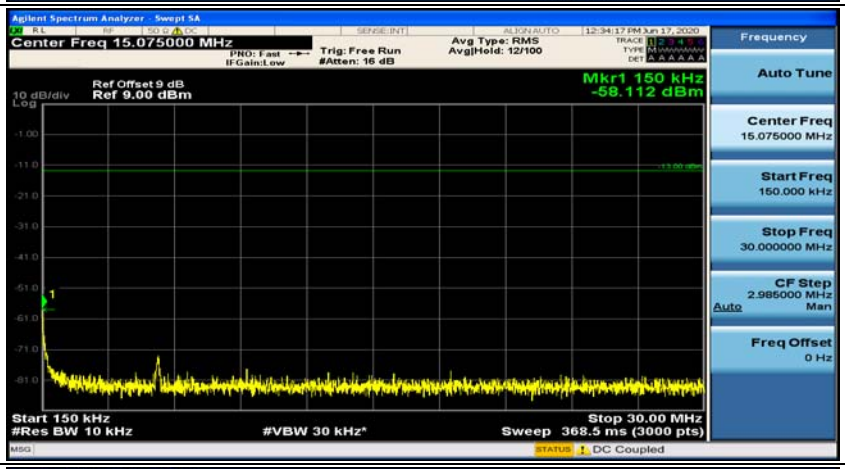

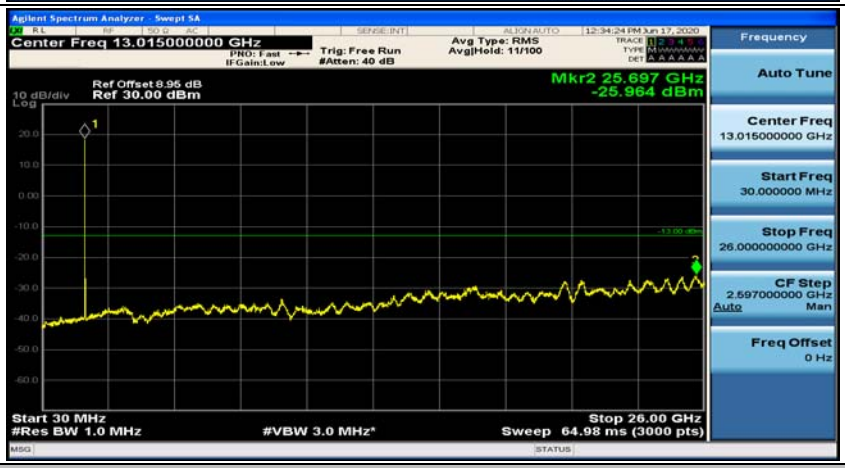

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#49

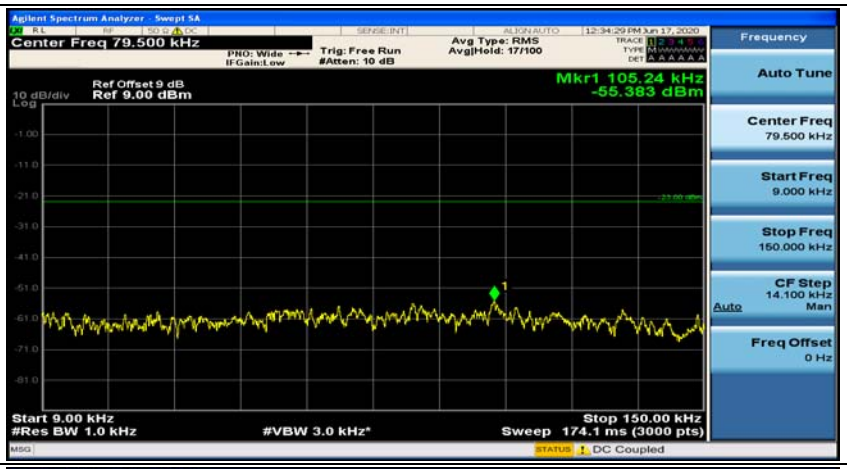

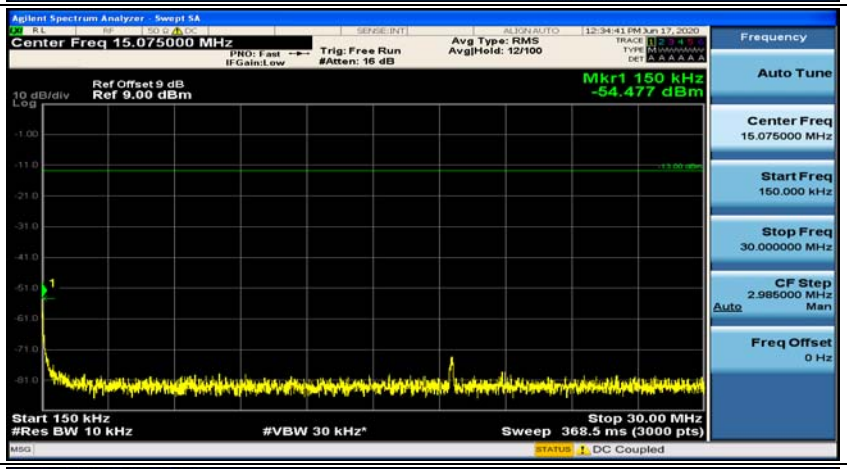

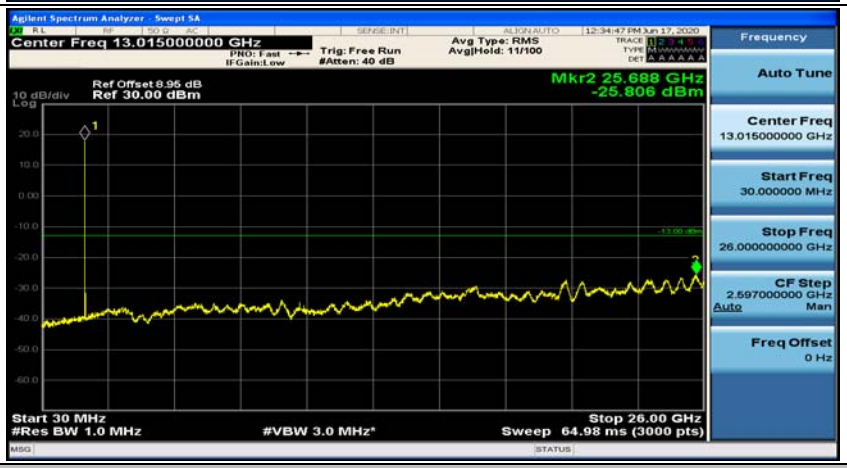

(Channel Bandwidth:20 MHz)_LCH_QPSK_1RB#99

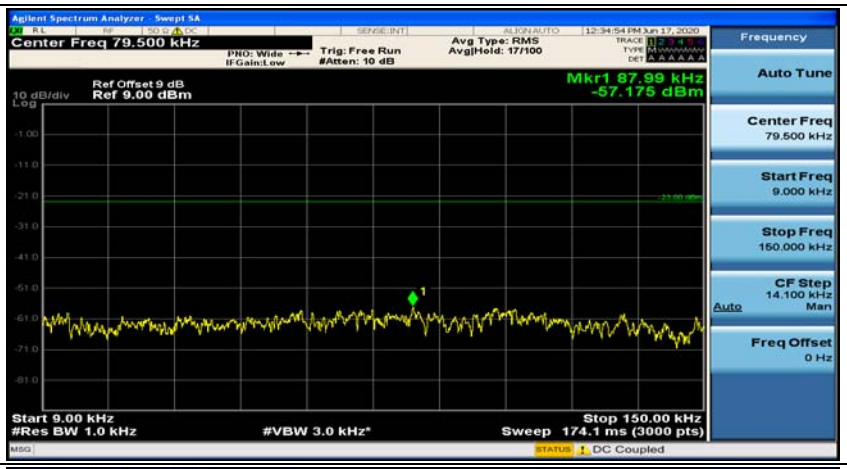
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:34:54 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 87.99 kHz
-57.175 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

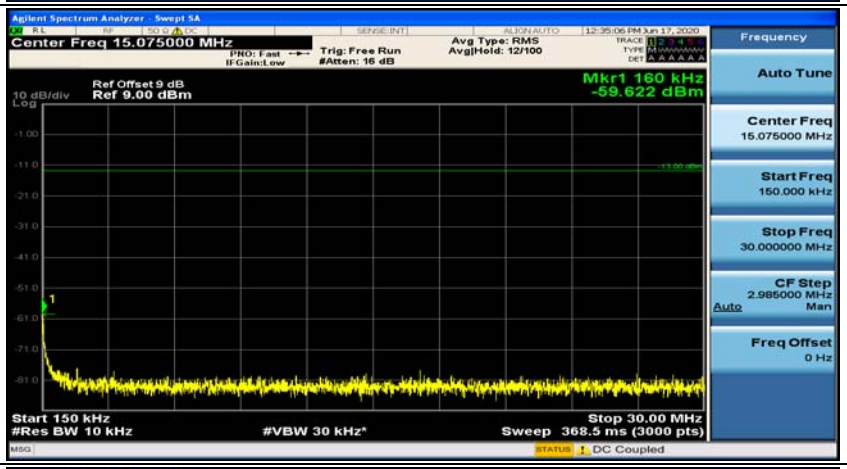
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:35:06 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-59.622 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

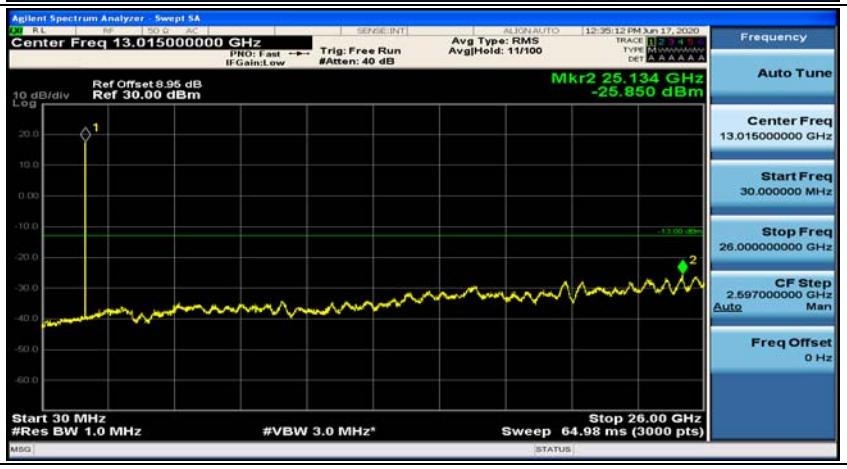
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:35:12 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.134 GHz
-25.850 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#0

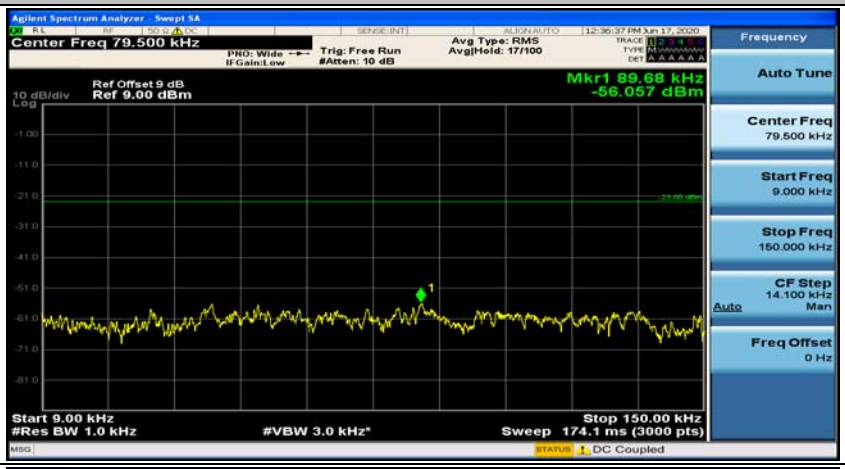

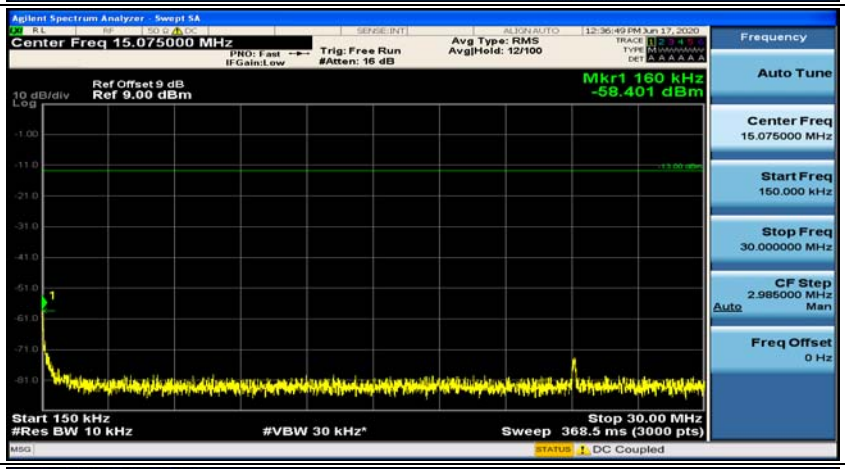

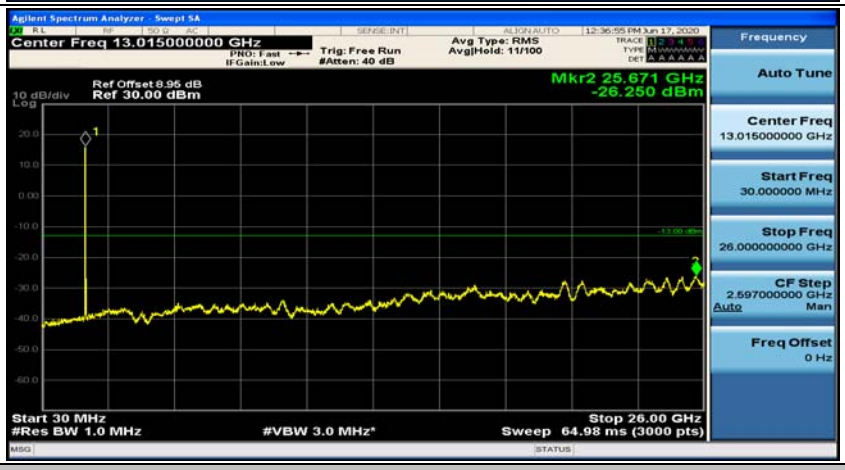

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#49

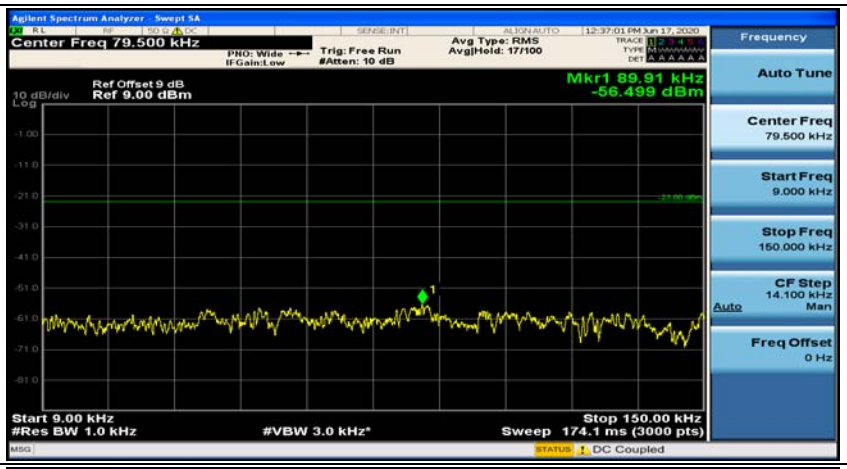

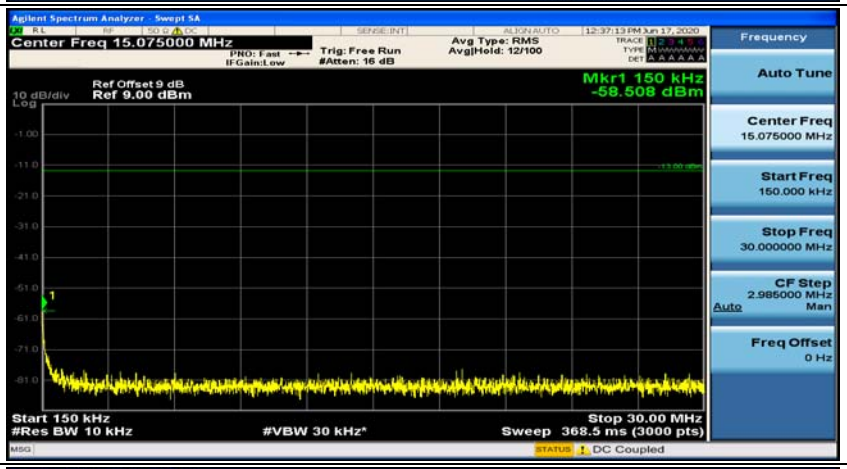

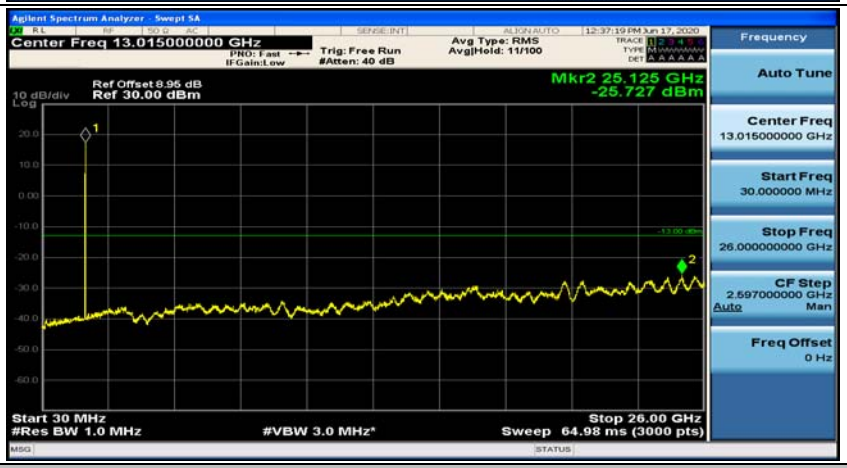

(Channel Bandwidth:20 MHz)_MCH_QPSK_1RB#99

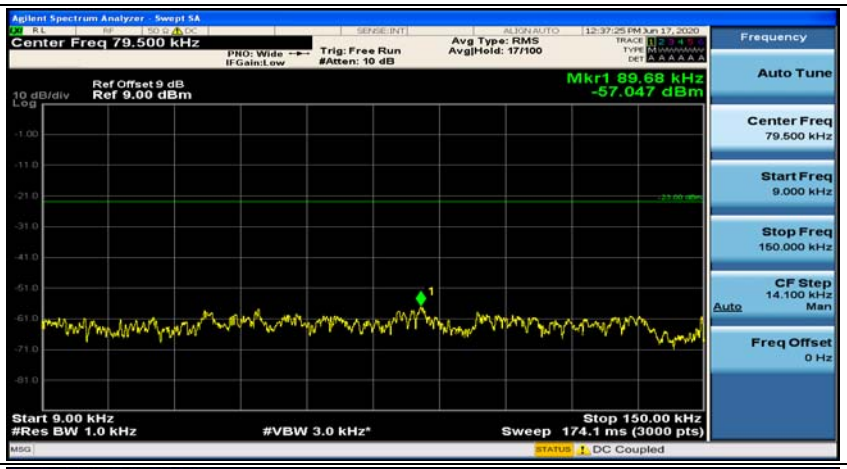
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:37:25 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 89.68 kHz
-57.047 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

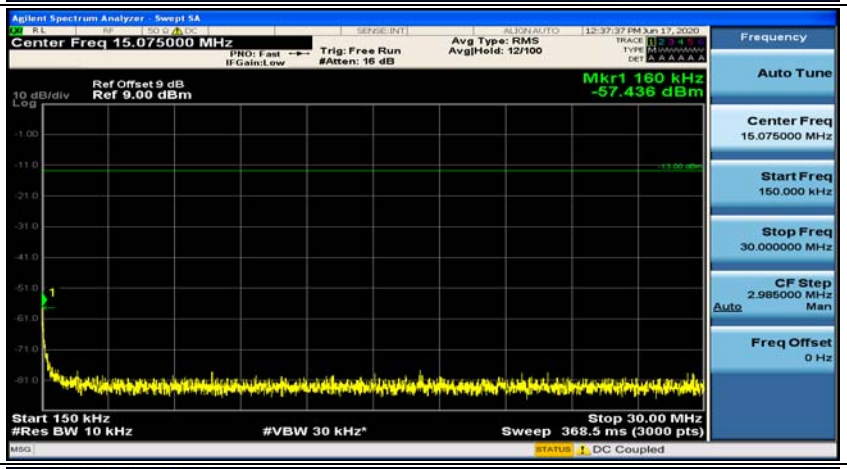
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:37:37 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-57.436 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

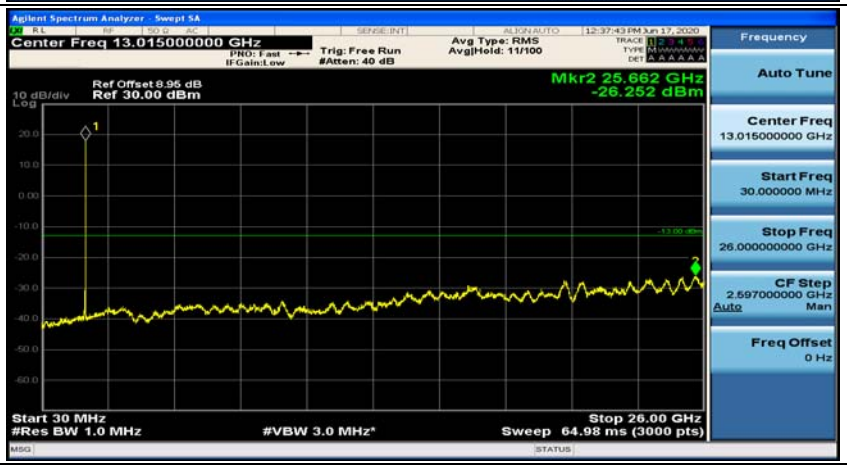
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:37:43 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.662 GHz
-26.252 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#0

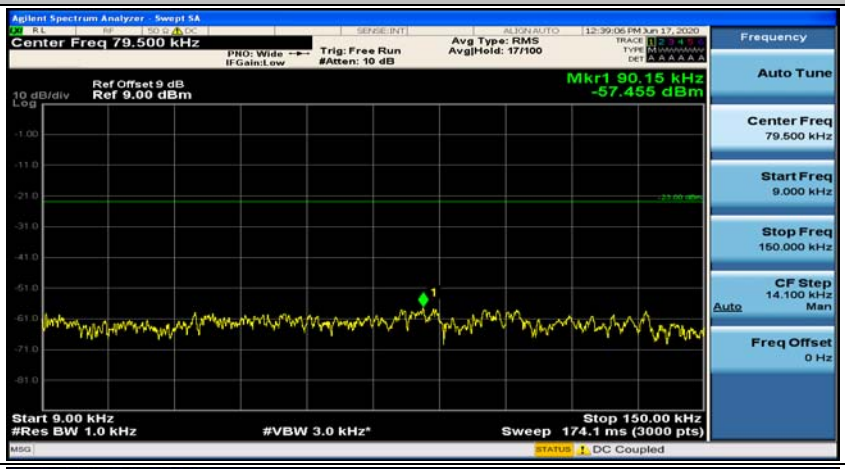

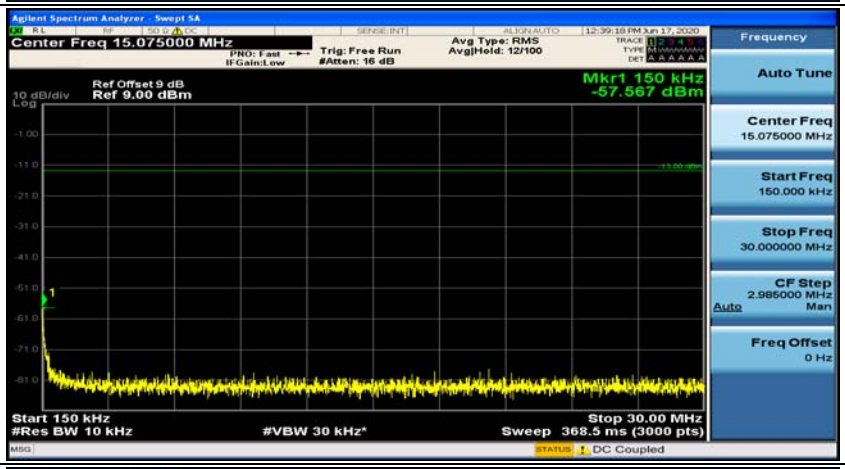

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#49

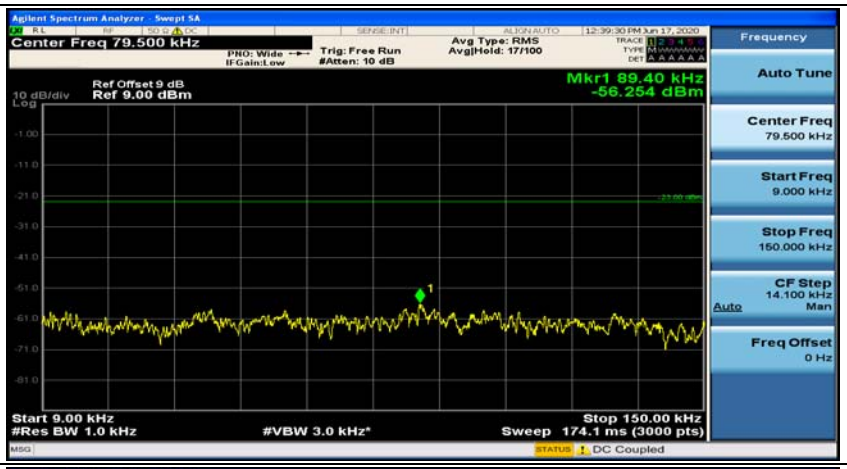

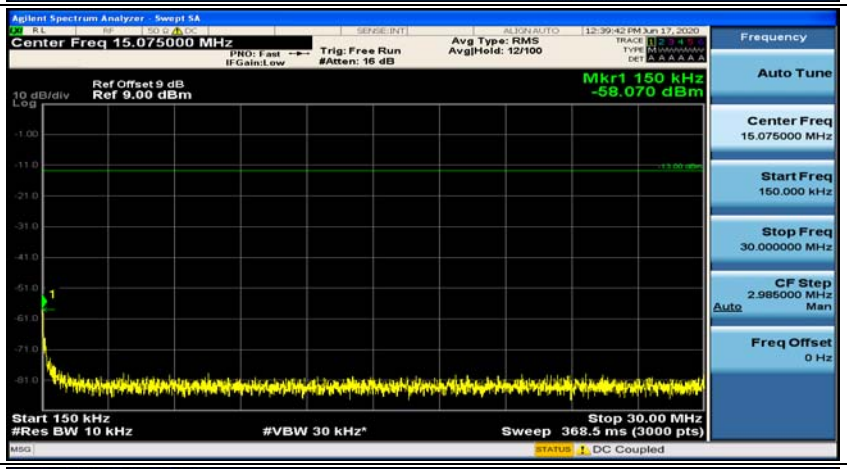

(Channel Bandwidth:20 MHz)_HCH_QPSK_1RB#99

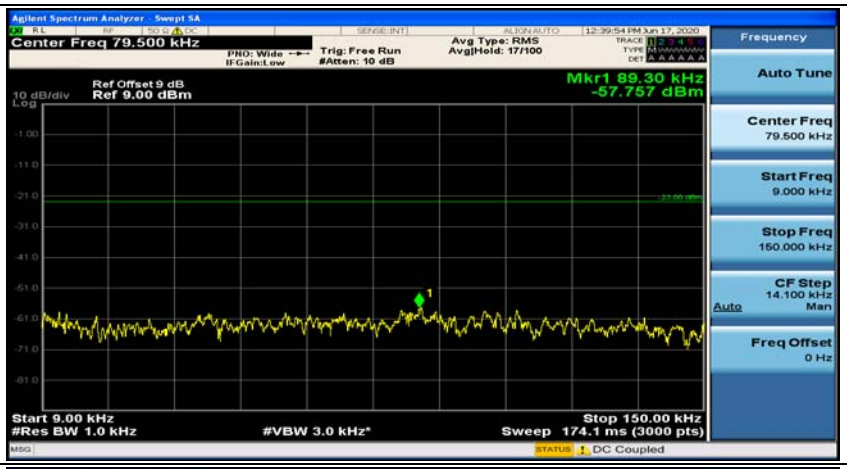
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:39:54 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Log
Mkr1 89.30 kHz
-57.757 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

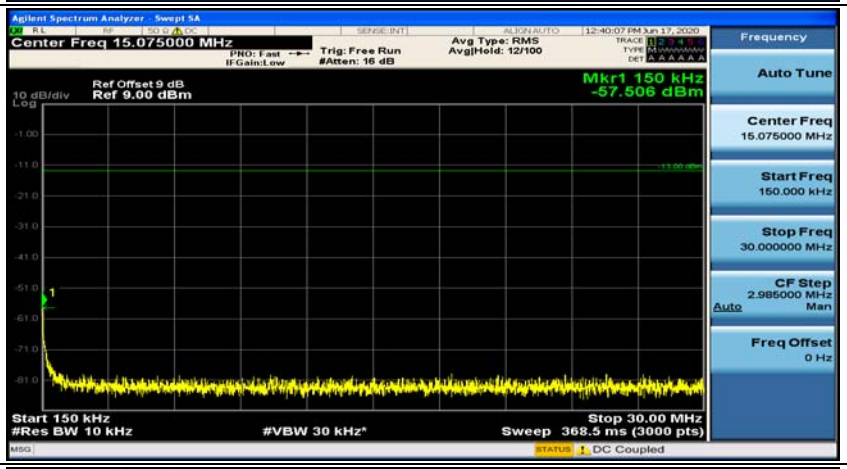
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:40:07 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Log
Mkr1 150 kHz
-57.506 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

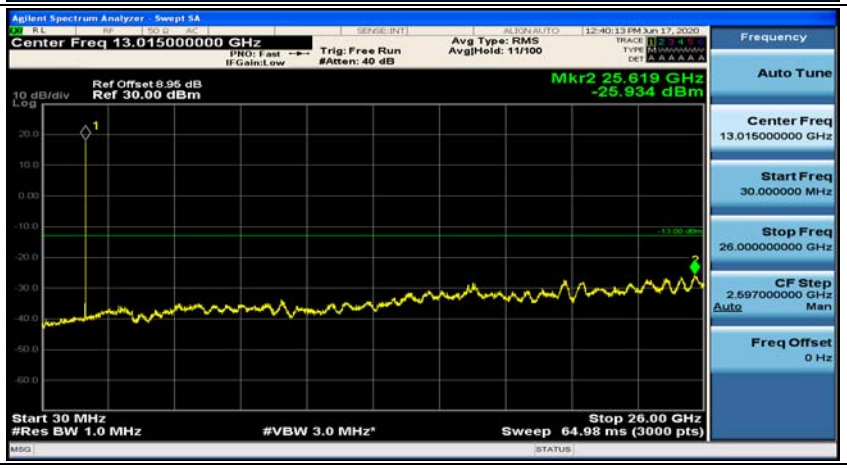
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:40:13 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Log
Mkr2 25.619 GHz
-25.934 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#0

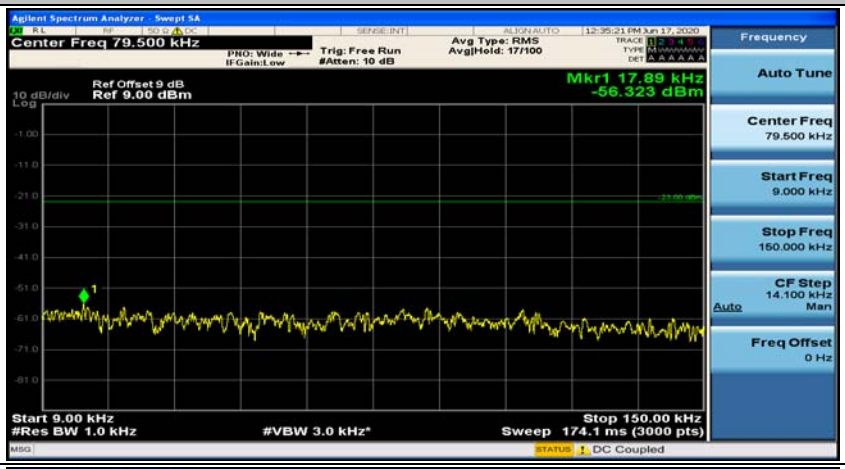

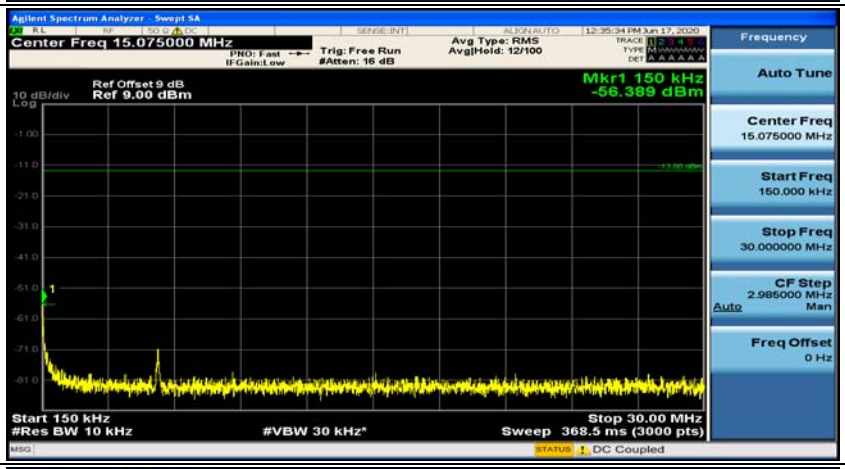

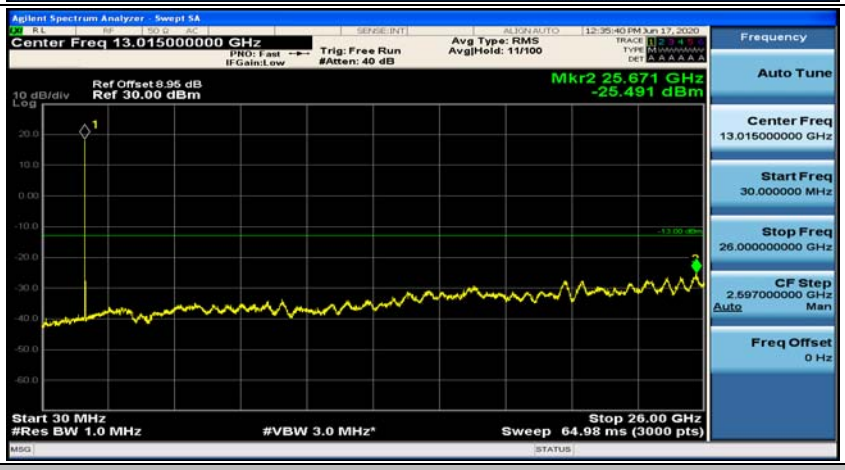

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#49

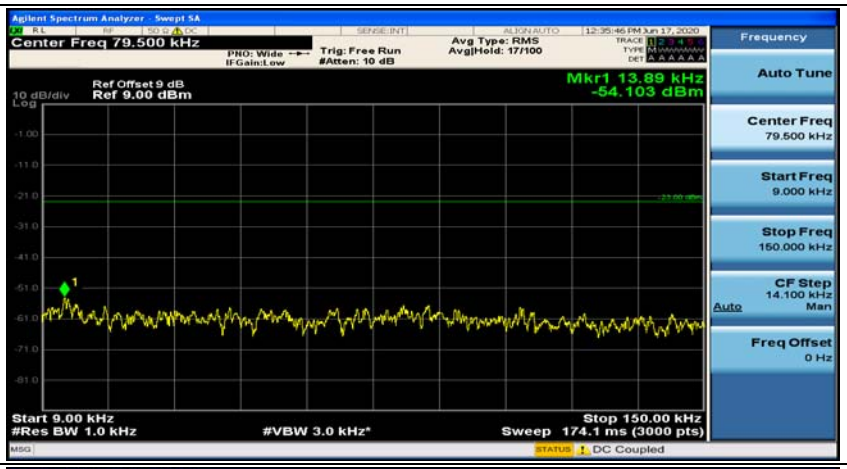

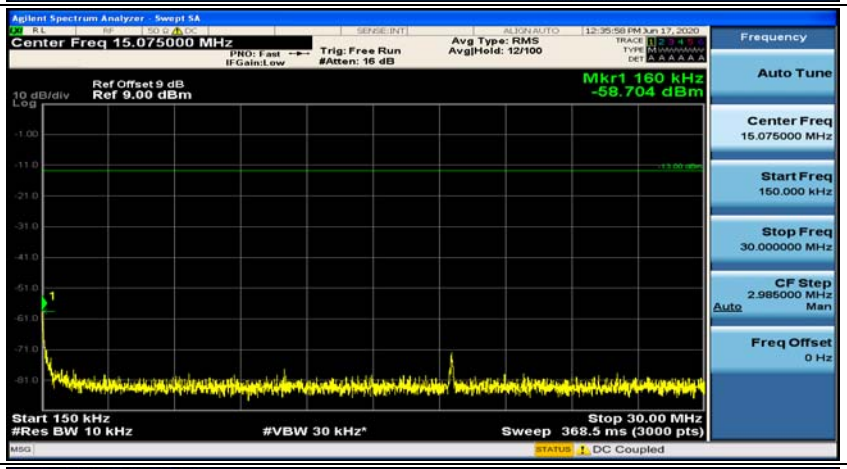

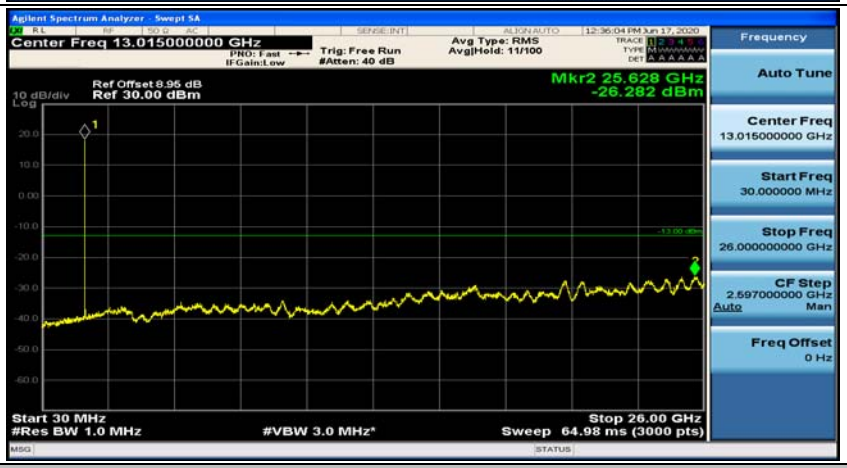

(Channel Bandwidth:20 MHz)_LCH_16QAM_1RB#99

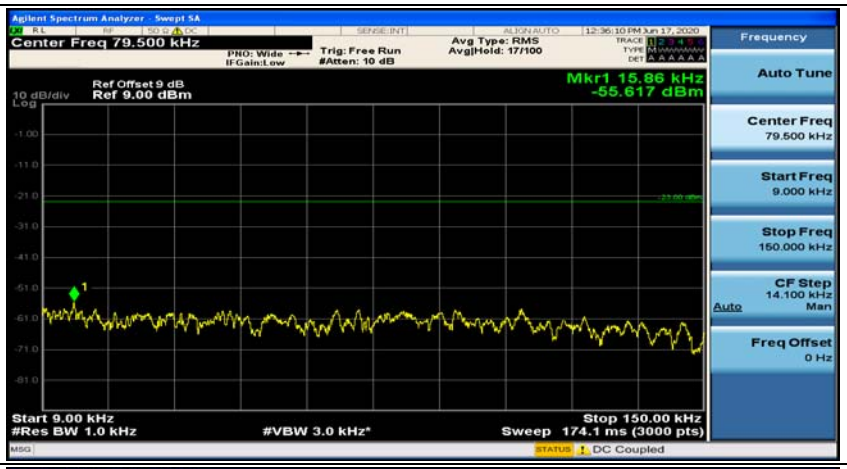
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:36:10 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 15.86 kHz
-55.617 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto Man
Freq Offset
0 Hz

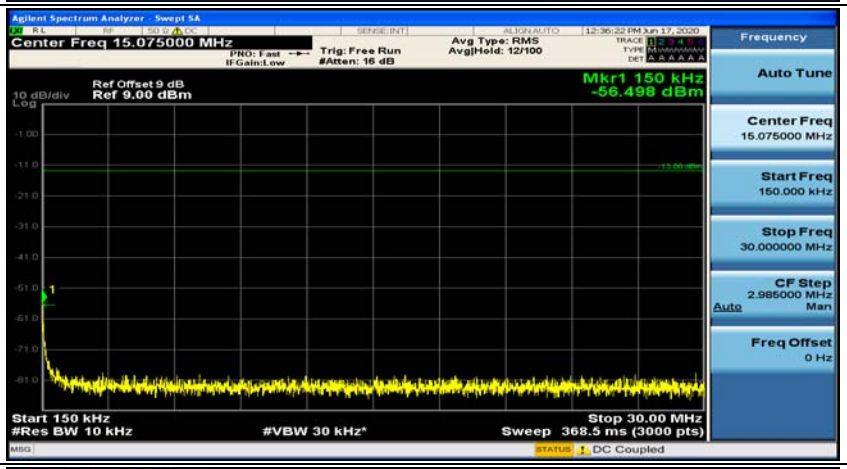
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:36:22 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-56.498 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto Man
Freq Offset
0 Hz

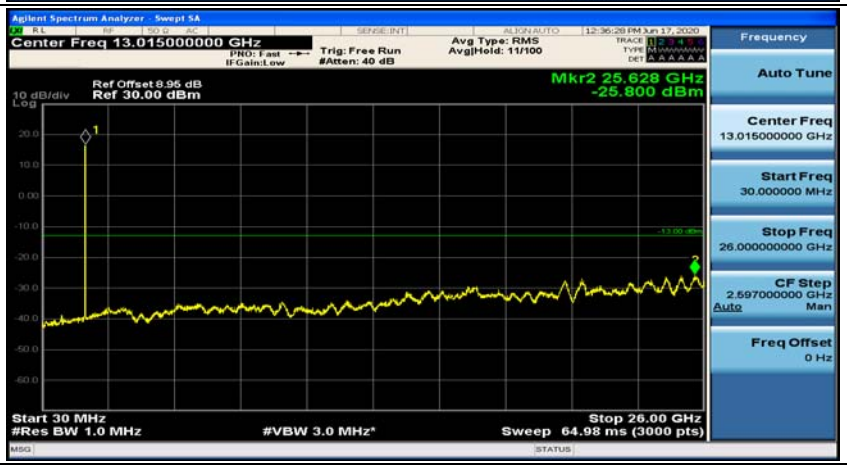
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:36:28 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Log
Mkr2 25.628 GHz
-25.800 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#0

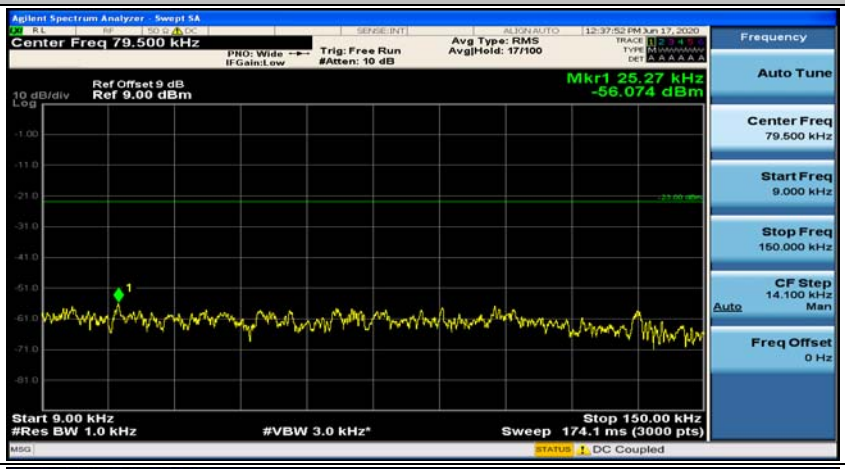

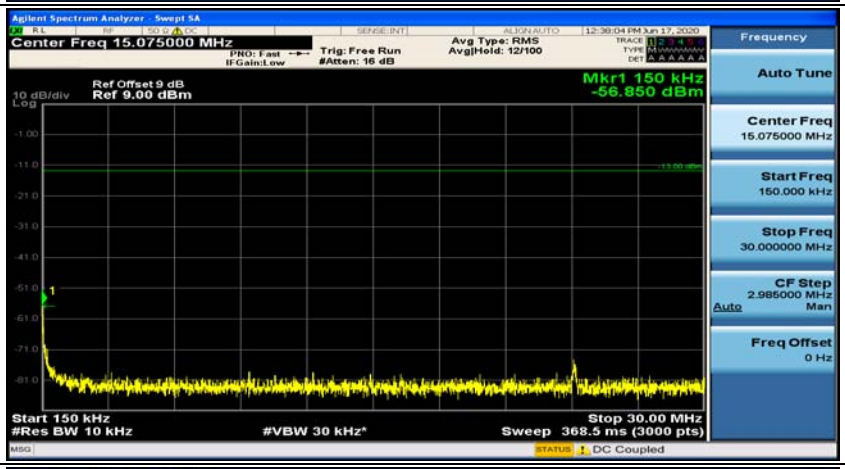

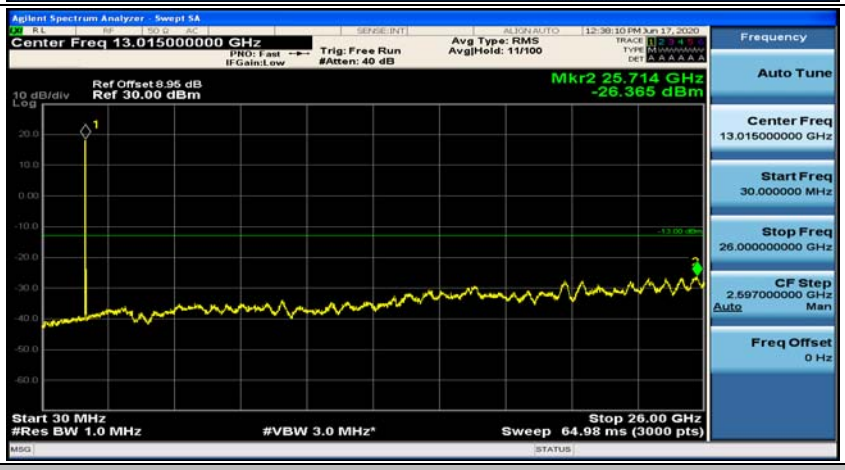

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#49

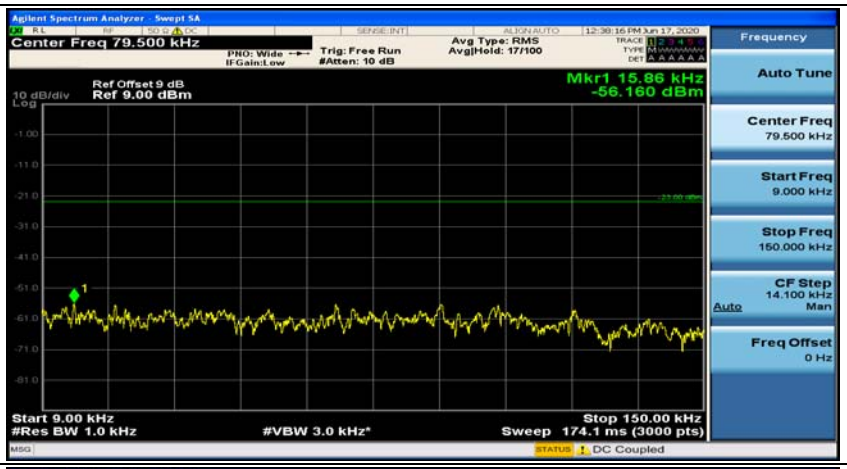

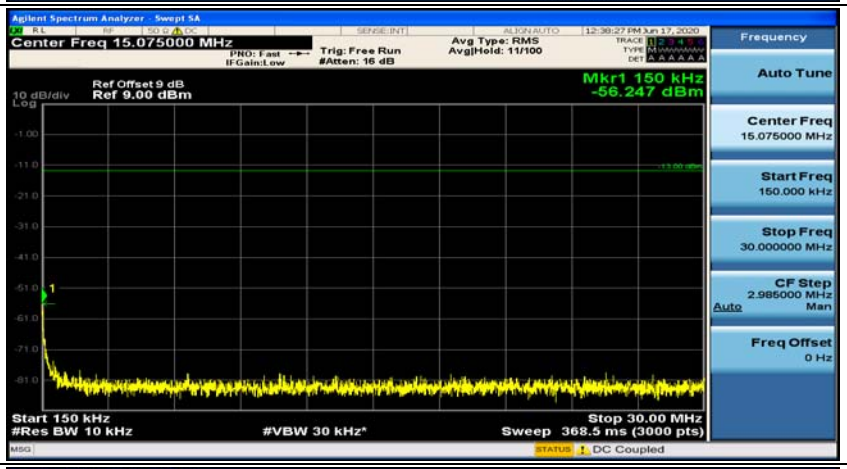

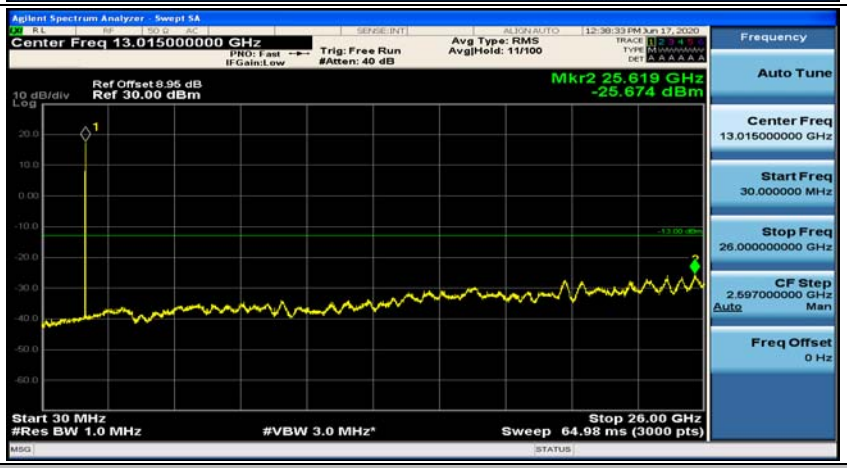

(Channel Bandwidth:20 MHz)_MCH_16QAM_1RB#99

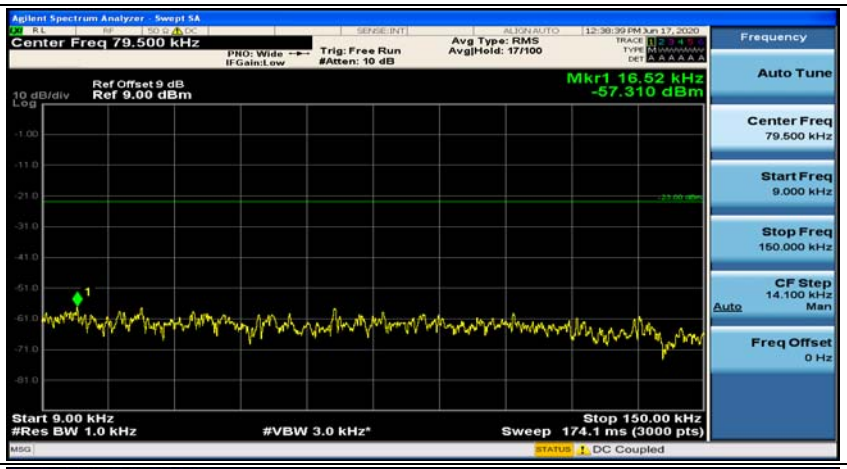
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:38:39 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 16.52 kHz
-57.310 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

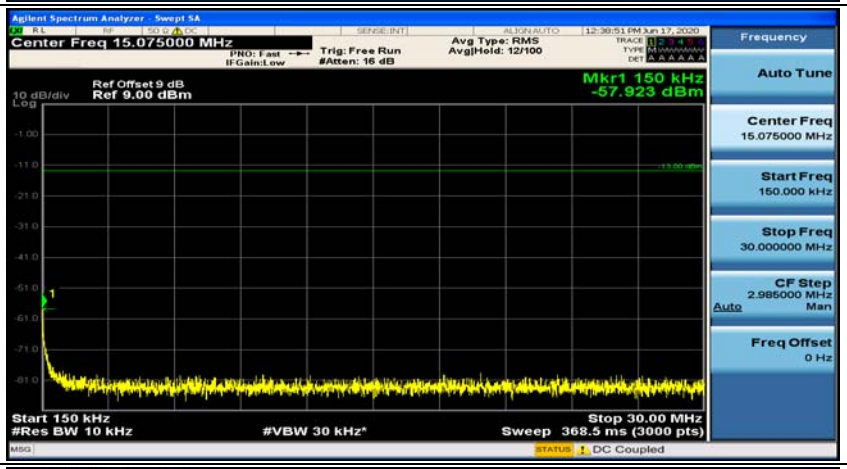
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
12:38:51 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.923 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

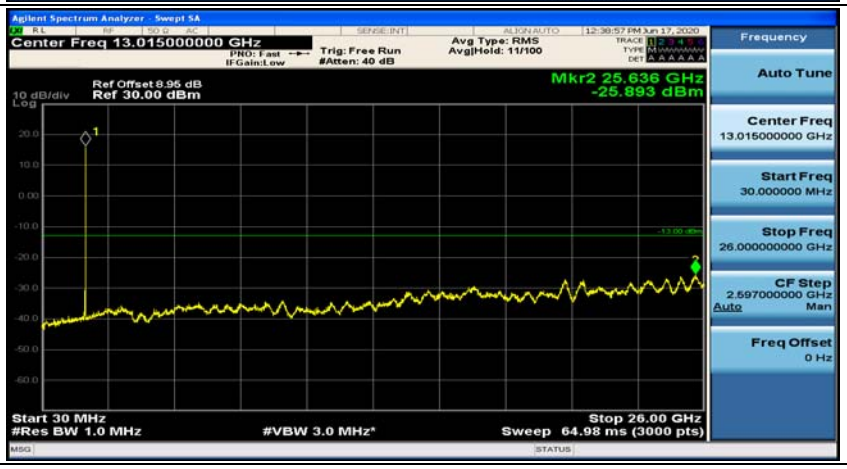
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:38:57 PM Jun 17, 2020
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.636 GHz
-25.893 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#0

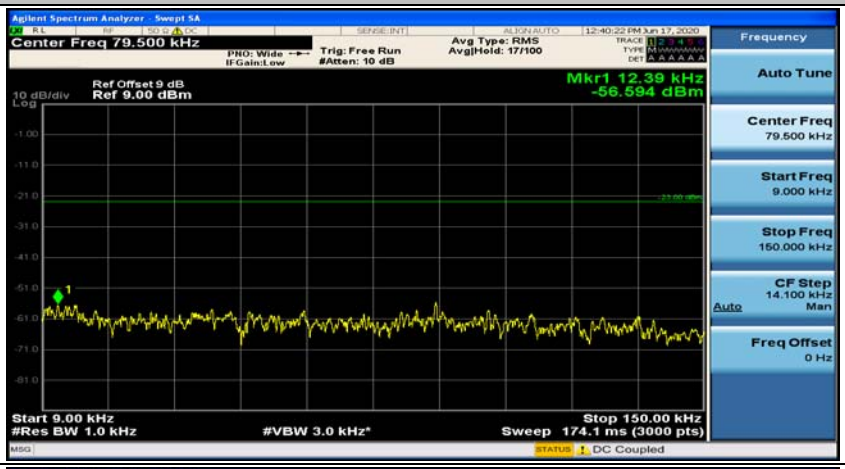

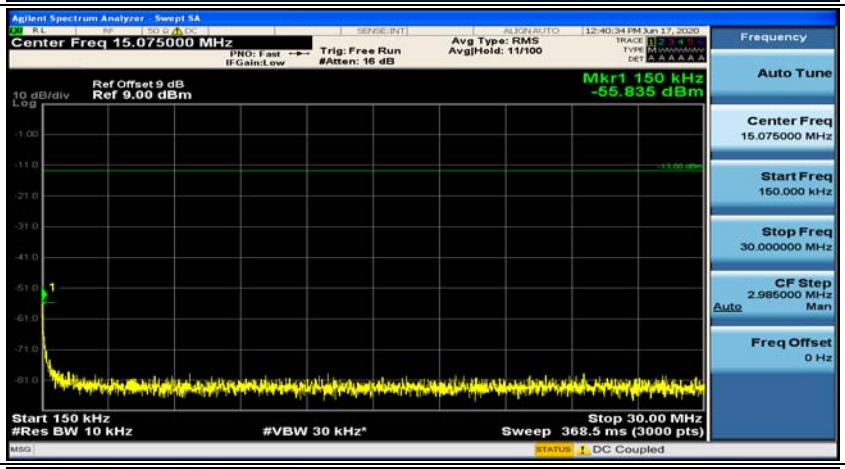

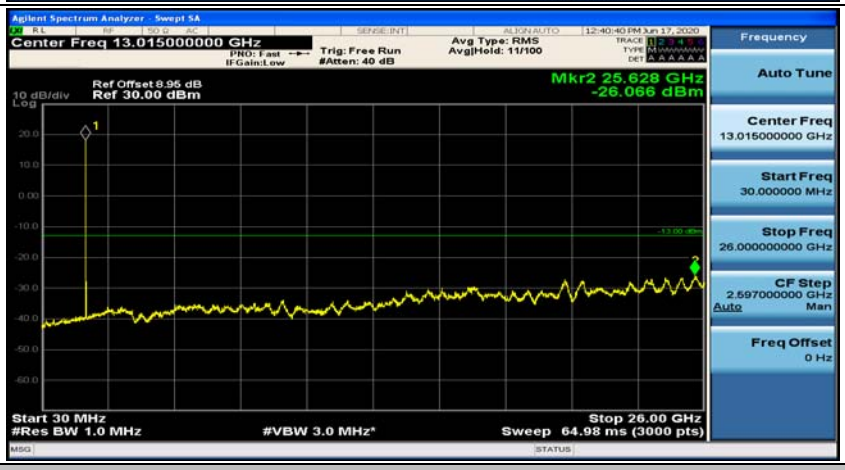

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#49

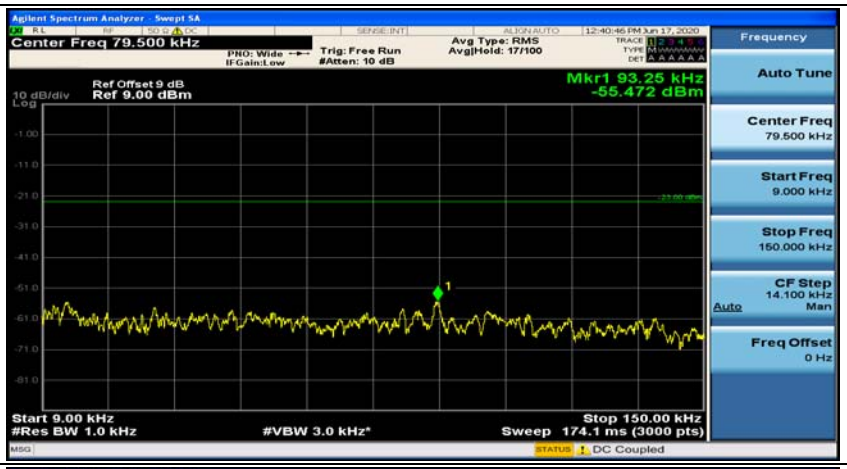

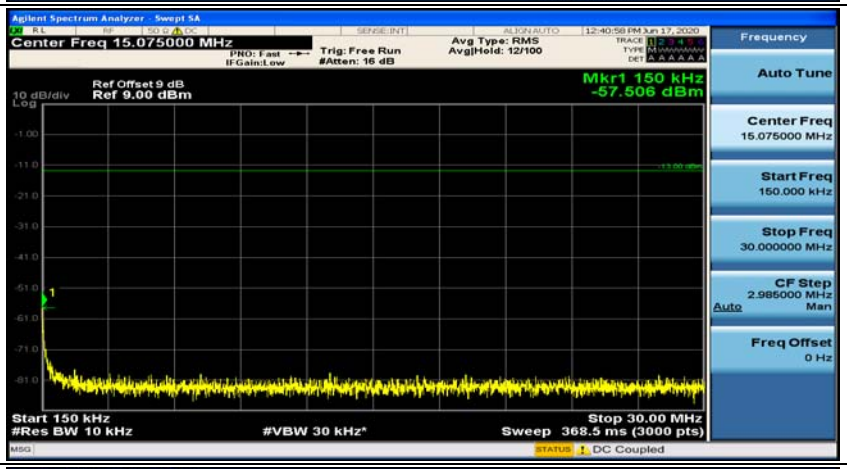

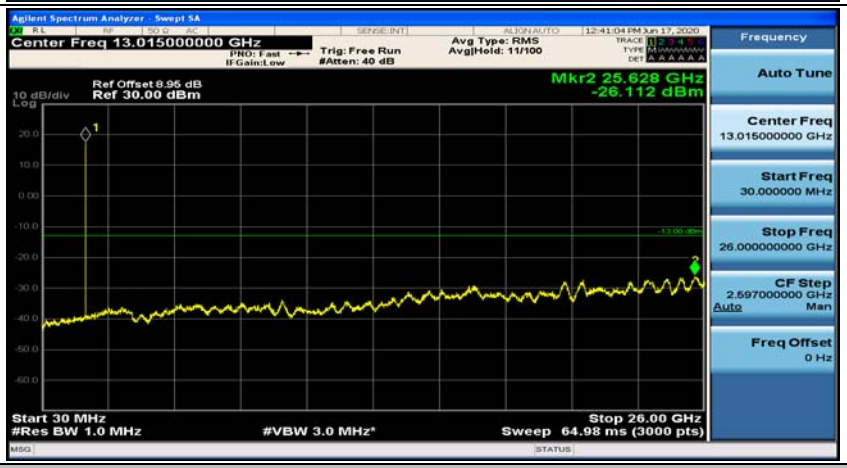

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#99

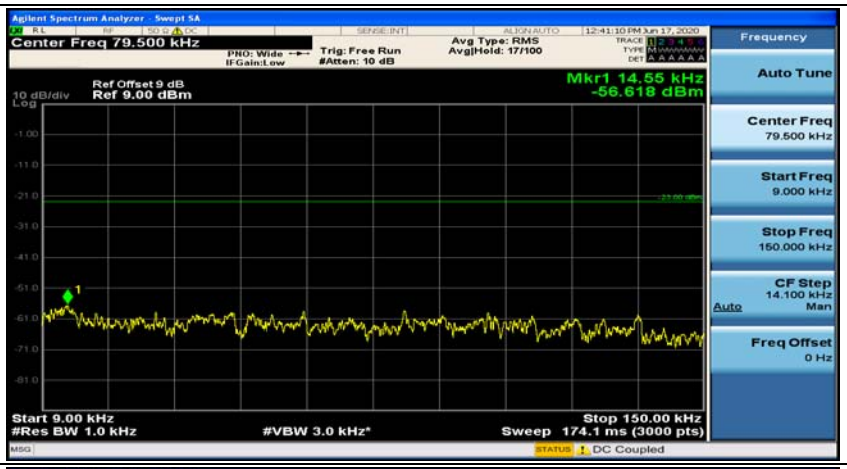
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
12:41:10 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 14.55 kHz
-56.618 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

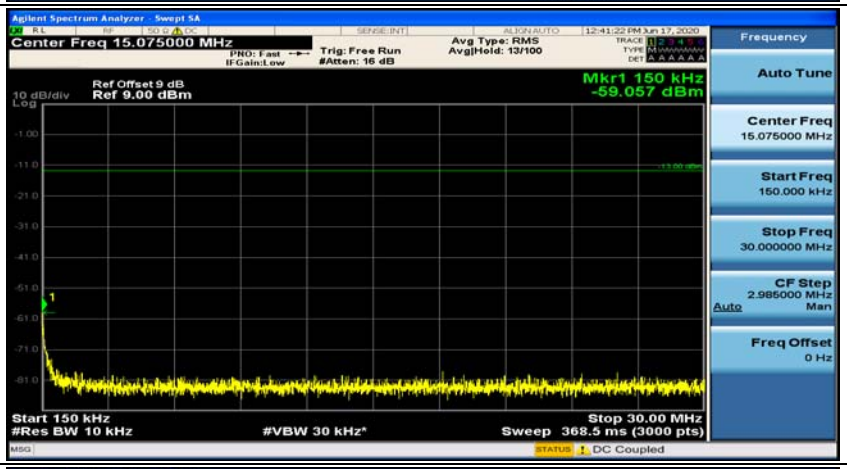
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
12:41:22 PM Jun 17, 2020
Ref Offset 9 dB
10 dB/div Ref 9.00 dBm
Log
Mkr1 150 kHz
-59.057 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

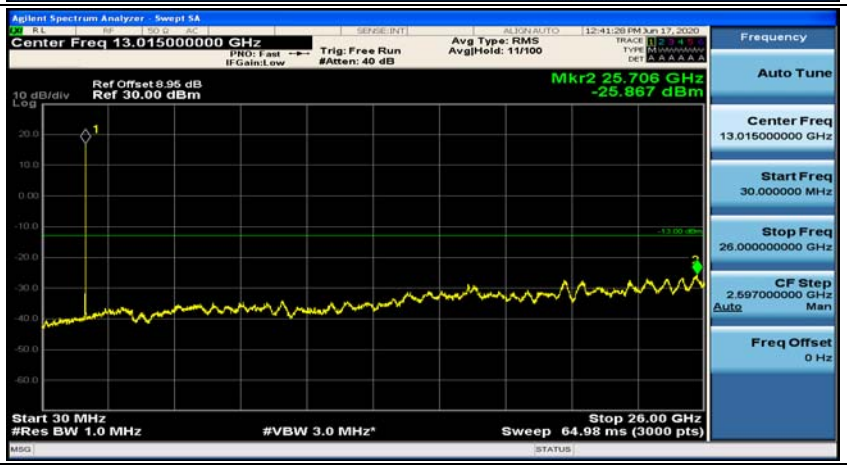
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
12:41:28 PM Jun 17, 2020
Ref Offset 8.95 dB
10 dB/div Ref 30.00 dBm
Log
Mkr2 25.706 GHz
-25.867 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

Appendix F: Frequency Stability

Test Result

Channel Bandwidth: 1.4 MHz

Channel Bandwidth: 1.4 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	3.3	0.001929	± 2.5	PASS
		VN	TN	2.4	0.001403	± 2.5	PASS
		VH	TN	4.44	0.002595	± 2.5	PASS
	MCH	VL	TN	2.09	0.001206	± 2.5	PASS
		VN	TN	0.56	0.000323	± 2.5	PASS
		VH	TN	1.06	0.000612	± 2.5	PASS
	HCH	VL	TN	-0.75	-0.000428	± 2.5	PASS
		VN	TN	-1.96	-0.001117	± 2.5	PASS
		VH	TN	4.23	0.002411	± 2.5	PASS
16QAM	LCH	VL	TN	-1.06	-0.000620	± 2.5	PASS
		VN	TN	0.7	0.000409	± 2.5	PASS
		VH	TN	2.48	0.001450	± 2.5	PASS
	MCH	VL	TN	-0.68	-0.000392	± 2.5	PASS
		VN	TN	-0.43	-0.000248	± 2.5	PASS
		VH	TN	-0.27	-0.000156	± 2.5	PASS
	HCH	VL	TN	2.14	0.001220	± 2.5	PASS
		VN	TN	-1.52	-0.000866	± 2.5	PASS
		VH	TN	2.19	0.001248	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	0.69	0.000403	± 2.5	PASS
		VN	-20	4.92	0.002876	± 2.5	PASS
		VN	-10	2.03	0.001187	± 2.5	PASS
		VN	0	2.6	0.001520	± 2.5	PASS
		VN	10	2.58	0.001508	± 2.5	PASS
		VN	20	2.34	0.001368	± 2.5	PASS
		VN	30	2.79	0.001631	± 2.5	PASS
		VN	40	-1.39	-0.000813	± 2.5	PASS
		VN	50	2.92	0.001707	± 2.5	PASS

	MCH	VN	-30	-0.91	-0.000525	± 2.5	PASS
		VN	-20	3.06	0.001766	± 2.5	PASS
		VN	-10	3.08	0.001778	± 2.5	PASS
		VN	0	1.7	0.000981	± 2.5	PASS
		VN	10	0.31	0.000179	± 2.5	PASS
		VN	20	4.54	0.002620	± 2.5	PASS
		VN	30	4.32	0.002494	± 2.5	PASS
		VN	40	4.88	0.002817	± 2.5	PASS
		VN	50	4.09	0.002361	± 2.5	PASS
	HCH	VN	-30	2.77	0.001579	± 2.5	PASS
		VN	-20	4.95	0.002822	± 2.5	PASS
		VN	-10	4.87	0.002776	± 2.5	PASS
		VN	0	4.46	0.002542	± 2.5	PASS
		VN	10	3.82	0.002178	± 2.5	PASS
		VN	20	0.19	0.000108	± 2.5	PASS
		VN	30	-1.86	-0.001060	± 2.5	PASS
		VN	40	2.82	0.001607	± 2.5	PASS
		VN	50	-1.79	-0.001020	± 2.5	PASS
16QAM	LCH	VN	-30	-0.54	-0.000316	± 2.5	PASS
		VN	-20	3.49	0.002040	± 2.5	PASS
		VN	-10	-0.91	-0.000532	± 2.5	PASS
		VN	0	3.47	0.002028	± 2.5	PASS
		VN	10	1.05	0.000614	± 2.5	PASS
		VN	20	3.59	0.002099	± 2.5	PASS
		VN	30	1.01	0.000590	± 2.5	PASS
		VN	40	4.5	0.002631	± 2.5	PASS
		VN	50	3.89	0.002274	± 2.5	PASS
	MCH	VN	-30	0.24	0.000137	± 2.5	PASS
		VN	-20	-1.01	-0.000576	± 2.5	PASS
		VN	-10	2.67	0.001522	± 2.5	PASS
		VN	0	3.24	0.001847	± 2.5	PASS
		VN	10	0.69	0.000393	± 2.5	PASS
		VN	20	3.19	0.001818	± 2.5	PASS
		VN	30	-0.28	-0.000160	± 2.5	PASS
		VN	40	4.53	0.002582	± 2.5	PASS
		VN	50	4.48	0.002554	± 2.5	PASS
	HCH	VN	-30	3.69	0.002103	± 2.5	PASS
		VN	-20	-0.85	-0.000485	± 2.5	PASS
		VN	-10	-0.84	-0.000479	± 2.5	PASS
		VN	0	3.72	0.002121	± 2.5	PASS
		VN	10	2.14	0.001220	± 2.5	PASS

		VN	20	0.58	0.000331	± 2.5	PASS
		VN	30	-0.3	-0.000171	± 2.5	PASS
		VN	40	4.52	0.002577	± 2.5	PASS
		VN	50	2.63	0.001499	± 2.5	PASS

Channel Bandwidth: 3 MHz

Channel Bandwidth: 3 MHz+							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	4.32	0.002524	± 2.5	PASS
		VN	TN	0.59	0.000345	± 2.5	PASS
		VH	TN	-1.42	-0.000830	± 2.5	PASS
	MCH	VL	TN	-1.17	-0.000675	± 2.5	PASS
		VN	TN	-1.47	-0.000848	± 2.5	PASS
		VH	TN	3.51	0.002026	± 2.5	PASS
	HCH	VL	TN	1.53	0.000873	± 2.5	PASS
		VN	TN	-1.57	-0.000895	± 2.5	PASS
		VH	TN	-0.63	-0.000359	± 2.5	PASS
16QAM	LCH	VL	TN	1.46	0.000853	± 2.5	PASS
		VN	TN	1.33	0.000777	± 2.5	PASS
		VH	TN	4.35	0.002542	± 2.5	PASS
	MCH	VL	TN	0.78	0.000450	± 2.5	PASS
		VN	TN	0.13	0.000075	± 2.5	PASS
		VH	TN	0.94	0.000543	± 2.5	PASS
	HCH	VL	TN	3.12	0.001779	± 2.5	PASS
		VN	TN	4.1	0.002338	± 2.5	PASS
		VH	TN	3.98	0.002270	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	1.64	0.000958	± 2.5	PASS
		VN	-20	4.97	0.002904	± 2.5	PASS
		VN	-10	0.59	0.000345	± 2.5	PASS
		VN	0	0.26	0.000152	± 2.5	PASS
		VN	10	4.43	0.002588	± 2.5	PASS
		VN	20	1.34	0.000783	± 2.5	PASS
		VN	30	-0.75	-0.000438	± 2.5	PASS
		VN	40	-0.58	-0.000339	± 2.5	PASS
		VN	50	0.4	0.000234	± 2.5	PASS
	MCH	VN	-30	3.36	0.001939	± 2.5	PASS

		VN	-20	-1.62	-0.000935	± 2.5	PASS
		VN	-10	2.58	0.001489	± 2.5	PASS
		VN	0	4.73	0.002730	± 2.5	PASS
		VN	10	2.93	0.001691	± 2.5	PASS
		VN	20	2.49	0.001437	± 2.5	PASS
		VN	30	3.4	0.001962	± 2.5	PASS
		VN	40	-1.17	-0.000675	± 2.5	PASS
		VN	50	3.23	0.001864	± 2.5	PASS
	HCH	VN	-30	1.36	0.000776	± 2.5	PASS
		VN	-20	2.73	0.001557	± 2.5	PASS
		VN	-10	4.06	0.002315	± 2.5	PASS
		VN	0	0.68	0.000388	± 2.5	PASS
		VN	10	-1.01	-0.000576	± 2.5	PASS
		VN	20	4.39	0.002504	± 2.5	PASS
		VN	30	1.14	0.000650	± 2.5	PASS
		VN	40	4.31	0.002458	± 2.5	PASS
		VN	50	2.98	0.001699	± 2.5	PASS
16QAM	LCH	VN	-30	4.32	0.002494	± 2.5	PASS
		VN	-20	-1.8	-0.001039	± 2.5	PASS
		VN	-10	2.37	0.001368	± 2.5	PASS
		VN	0	2.72	0.001570	± 2.5	PASS
		VN	10	3.66	0.002113	± 2.5	PASS
		VN	20	-1.04	-0.000600	± 2.5	PASS
		VN	30	1.09	0.000629	± 2.5	PASS
		VN	40	-1.27	-0.000733	± 2.5	PASS
		VN	50	2.38	0.001374	± 2.5	PASS
	MCH	VN	-30	-0.52	-0.000297	± 2.5	PASS
		VN	-20	0.97	0.000553	± 2.5	PASS
		VN	-10	2.11	0.001203	± 2.5	PASS
		VN	0	-0.31	-0.000177	± 2.5	PASS
		VN	10	-1.67	-0.000952	± 2.5	PASS
		VN	20	-0.73	-0.000416	± 2.5	PASS
		VN	30	-0.08	-0.000046	± 2.5	PASS
		VN	40	4.38	0.002498	± 2.5	PASS
		VN	50	2.54	0.001449	± 2.5	PASS
	HCH	VN	-30	1.58	0.000901	± 2.5	PASS
		VN	-20	-1.91	-0.001089	± 2.5	PASS
		VN	-10	1.6	0.000912	± 2.5	PASS
		VN	0	2.72	0.001551	± 2.5	PASS
		VN	10	2.88	0.001642	± 2.5	PASS
		VN	20	3.37	0.001922	± 2.5	PASS

		VN	30	2.02	0.001152	± 2.5	PASS
		VN	40	-0.87	-0.000496	± 2.5	PASS
		VN	50	-1.86	-0.001061	± 2.5	PASS

Channel Bandwidth: 5 MHz

Channel Bandwidth: 5 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	4.41	0.002575	± 2.5	PASS
		VN	TN	3.98	0.002324	± 2.5	PASS
		VH	TN	-0.93	-0.000543	± 2.5	PASS
	MCH	VL	TN	1.44	0.000831	± 2.5	PASS
		VN	TN	3.31	0.001911	± 2.5	PASS
		VH	TN	1.76	0.001016	± 2.5	PASS
	HCH	VL	TN	-1.01	-0.000576	± 2.5	PASS
		VN	TN	1.6	0.000913	± 2.5	PASS
		VH	TN	1.58	0.000902	± 2.5	PASS
16QAM	LCH	VL	TN	3.53	0.002061	± 2.5	PASS
		VN	TN	3.67	0.002143	± 2.5	PASS
		VH	TN	2.45	0.001431	± 2.5	PASS
	MCH	VL	TN	0.85	0.000491	± 2.5	PASS
		VN	TN	-1.09	-0.000629	± 2.5	PASS
		VH	TN	1.65	0.000952	± 2.5	PASS
	HCH	VL	TN	3	0.001712	± 2.5	PASS
		VN	TN	3.54	0.002020	± 2.5	PASS
		VH	TN	-0.69	-0.000394	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	-1.74	-0.001016	± 2.5	PASS
		VN	-20	0.32	0.000187	± 2.5	PASS
		VN	-10	3.77	0.002201	± 2.5	PASS
		VN	0	2.62	0.001530	± 2.5	PASS
		VN	10	3.85	0.002248	± 2.5	PASS
		VN	20	3.48	0.002032	± 2.5	PASS
		VN	30	3.41	0.001991	± 2.5	PASS
		VN	40	2.6	0.001518	± 2.5	PASS
		VN	50	-0.85	-0.000496	± 2.5	PASS
	MCH	VN	-30	1.56	0.000900	± 2.5	PASS
		VN	-20	0.62	0.000358	± 2.5	PASS

		VN	-10	-0.16	-0.000092	± 2.5	PASS
		VN	0	2.75	0.001587	± 2.5	PASS
		VN	10	3.84	0.002216	± 2.5	PASS
		VN	20	-0.64	-0.000369	± 2.5	PASS
		VN	30	4.35	0.002511	± 2.5	PASS
		VN	40	-1.14	-0.000658	± 2.5	PASS
		VN	50	4.79	0.002765	± 2.5	PASS
	HCH	VN	-30	3.39	0.001934	± 2.5	PASS
		VN	-20	4.5	0.002359	± 2.5	PASS
		VN	-10	0.23	0.000121	± 2.5	PASS
		VN	0	0.27	0.000142	± 2.5	PASS
		VN	10	-1.89	-0.000991	± 2.5	PASS
		VN	20	-1.12	-0.000587	± 2.5	PASS
		VN	30	-1.91	-0.001001	± 2.5	PASS
		VN	40	1.18	0.000619	± 2.5	PASS
		VN	50	4.62	0.002422	± 2.5	PASS
16QAM	LCH	VN	-30	2.46	0.001420	± 2.5	PASS
		VN	-20	3.57	0.002061	± 2.5	PASS
		VN	-10	2.53	0.001460	± 2.5	PASS
		VN	0	0.94	0.000543	± 2.5	PASS
		VN	10	3.45	0.001991	± 2.5	PASS
		VN	20	1.37	0.000791	± 2.5	PASS
		VN	30	-1.61	-0.000929	± 2.5	PASS
		VN	40	-1.54	-0.000889	± 2.5	PASS
		VN	50	3.13	0.001807	± 2.5	PASS
	MCH	VN	-30	-0.78	-0.000445	± 2.5	PASS
		VN	-20	-0.23	-0.000131	± 2.5	PASS
		VN	-10	4.18	0.002385	± 2.5	PASS
		VN	0	0.81	0.000462	± 2.5	PASS
		VN	10	2.12	0.001210	± 2.5	PASS
		VN	20	4.12	0.002351	± 2.5	PASS
		VN	30	-0.81	-0.000462	± 2.5	PASS
		VN	40	4	0.002282	± 2.5	PASS
		VN	50	-1.31	-0.000748	± 2.5	PASS
	HCH	VN	-30	2.76	0.001447	± 2.5	PASS
		VN	-20	2.09	0.001096	± 2.5	PASS
		VN	-10	0.94	0.000493	± 2.5	PASS
		VN	0	0.82	0.000430	± 2.5	PASS
		VN	10	1.72	0.000902	± 2.5	PASS
		VN	20	3.85	0.002018	± 2.5	PASS
		VN	30	1.79	0.000938	± 2.5	PASS

		VN	40	-0.1	-0.000052	± 2.5	PASS
		VN	50	1.36	0.000713	± 2.5	PASS

Channel Bandwidth: 10 MHz

Channel Bandwidth: 10 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	3.54	0.002064	± 2.5	PASS
		VN	TN	-0.35	-0.000204	± 2.5	PASS
		VH	TN	-1.21	-0.000706	± 2.5	PASS
	MCH	VL	TN	-0.6	-0.000346	± 2.5	PASS
		VN	TN	3.55	0.002049	± 2.5	PASS
		VH	TN	2.93	0.001691	± 2.5	PASS
	HCH	VL	TN	2.97	0.001697	± 2.5	PASS
		VN	TN	-0.88	-0.000503	± 2.5	PASS
		VH	TN	4.34	0.002480	± 2.5	PASS
16QAM	LCH	VL	TN	4.31	0.002513	± 2.5	PASS
		VN	TN	2.82	0.001644	± 2.5	PASS
		VH	TN	2.06	0.001201	± 2.5	PASS
	MCH	VL	TN	1.49	0.000860	± 2.5	PASS
		VN	TN	-0.59	-0.000341	± 2.5	PASS
		VH	TN	0.93	0.000537	± 2.5	PASS
	HCH	VL	TN	0.62	0.000354	± 2.5	PASS
		VN	TN	0.16	0.000091	± 2.5	PASS
		VH	TN	-1.98	-0.001131	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	1.69	0.000985	± 2.5	PASS
		VN	-20	4.45	0.002595	± 2.5	PASS
		VN	-10	-0.92	-0.000536	± 2.5	PASS
		VN	0	0.35	0.000204	± 2.5	PASS
		VN	10	1.67	0.000974	± 2.5	PASS
		VN	20	4.65	0.002711	± 2.5	PASS
		VN	30	-1.18	-0.000688	± 2.5	PASS
		VN	40	2.87	0.001673	± 2.5	PASS
		VN	50	-0.56	-0.000327	± 2.5	PASS
	MCH	VN	-30	4.59	0.002649	± 2.5	PASS
		VN	-20	2.86	0.001651	± 2.5	PASS
		VN	-10	3.05	0.001760	± 2.5	PASS

		VN	0	4.39	0.002534	± 2.5	PASS
		VN	10	1.63	0.000941	± 2.5	PASS
		VN	20	-1.22	-0.000704	± 2.5	PASS
		VN	30	4.46	0.002574	± 2.5	PASS
		VN	40	1.97	0.001137	± 2.5	PASS
		VN	50	3.05	0.001760	± 2.5	PASS
	HCH	VN	-30	-0.81	-0.000463	± 2.5	PASS
		VN	-20	-0.95	-0.000543	± 2.5	PASS
		VN	-10	0.02	0.000011	± 2.5	PASS
		VN	0	4.1	0.002343	± 2.5	PASS
		VN	10	-0.08	-0.000046	± 2.5	PASS
		VN	20	1.85	0.001057	± 2.5	PASS
		VN	30	-1.99	-0.001137	± 2.5	PASS
		VN	40	1.43	0.000817	± 2.5	PASS
		VN	50	4.44	0.002537	± 2.5	PASS
16QAM	LCH	VN	-30	2.27	0.001310	± 2.5	PASS
		VN	-20	-1.43	-0.000825	± 2.5	PASS
		VN	-10	4.1	0.002367	± 2.5	PASS
		VN	0	-1.14	-0.000658	± 2.5	PASS
		VN	10	4.82	0.002782	± 2.5	PASS
		VN	20	-1.76	-0.001016	± 2.5	PASS
		VN	30	-0.82	-0.000473	± 2.5	PASS
		VN	40	-0.3	-0.000173	± 2.5	PASS
		VN	50	2.14	0.001235	± 2.5	PASS
	MCH	VN	-30	1.58	0.000903	± 2.5	PASS
		VN	-20	-0.92	-0.000526	± 2.5	PASS
		VN	-10	-0.28	-0.000160	± 2.5	PASS
		VN	0	2.79	0.001594	± 2.5	PASS
		VN	10	-1.84	-0.001051	± 2.5	PASS
		VN	20	0.23	0.000131	± 2.5	PASS
		VN	30	2.07	0.001183	± 2.5	PASS
		VN	40	0.56	0.000320	± 2.5	PASS
		VN	50	3.48	0.001989	± 2.5	PASS
	HCH	VN	-30	3.07	0.001754	± 2.5	PASS
		VN	-20	-0.72	-0.000411	± 2.5	PASS
		VN	-10	3.48	0.001989	± 2.5	PASS
		VN	0	-0.28	-0.000160	± 2.5	PASS
		VN	10	0.07	0.000040	± 2.5	PASS
		VN	20	1.67	0.000954	± 2.5	PASS
		VN	30	-1.86	-0.001063	± 2.5	PASS
		VN	40	0.29	0.000166	± 2.5	PASS

		VN	50	2.31	0.001320	± 2.5	PASS

Channel Bandwidth: 15 MHz

Channel Bandwidth: 15 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	3.28	0.001910	± 2.5	PASS
		VN	TN	0.12	0.000070	± 2.5	PASS
		VH	TN	2.28	0.001328	± 2.5	PASS
	MCH	VL	TN	1.95	0.001126	± 2.5	PASS
		VN	TN	-0.07	-0.000040	± 2.5	PASS
		VH	TN	4.38	0.002528	± 2.5	PASS
	HCH	VL	TN	0.39	0.000223	± 2.5	PASS
		VN	TN	2.41	0.001379	± 2.5	PASS
		VH	TN	3.22	0.001843	± 2.5	PASS
16QAM	LCH	VL	TN	2.06	0.001199	± 2.5	PASS
		VN	TN	5	0.002911	± 2.5	PASS
		VH	TN	-0.96	-0.000559	± 2.5	PASS
	MCH	VL	TN	4.29	0.002476	± 2.5	PASS
		VN	TN	4.11	0.002372	± 2.5	PASS
		VH	TN	1.58	0.000912	± 2.5	PASS
	HCH	VL	TN	3.16	0.001808	± 2.5	PASS
		VN	TN	4.52	0.002587	± 2.5	PASS
		VH	TN	3.28	0.001877	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	-1.6	-0.000932	± 2.5	PASS
		VN	-20	4.46	0.002597	± 2.5	PASS
		VN	-10	-0.19	-0.000111	± 2.5	PASS
		VN	0	0.92	0.000536	± 2.5	PASS
		VN	10	0.8	0.000466	± 2.5	PASS
		VN	20	-1.74	-0.001013	± 2.5	PASS
		VN	30	-1.75	-0.001019	± 2.5	PASS
		VN	40	1.24	0.000722	± 2.5	PASS
		VN	50	1.4	0.000815	± 2.5	PASS
	MCH	VN	-30	2.24	0.001293	± 2.5	PASS
		VN	-20	-1.89	-0.001091	± 2.5	PASS
		VN	-10	4.36	0.002517	± 2.5	PASS
		VN	0	4.55	0.002626	± 2.5	PASS

		VN	10	3.92	0.002263	± 2.5	PASS
		VN	20	-0.33	-0.000190	± 2.5	PASS
		VN	30	-0.56	-0.000323	± 2.5	PASS
		VN	40	3.63	0.002095	± 2.5	PASS
		VN	50	1.46	0.000843	± 2.5	PASS
	HCH	VN	-30	-1.55	-0.000887	± 2.5	PASS
		VN	-20	-0.02	-0.000011	± 2.5	PASS
		VN	-10	2.3	0.001316	± 2.5	PASS
		VN	0	4.18	0.002392	± 2.5	PASS
		VN	10	3.05	0.001745	± 2.5	PASS
		VN	20	4.59	0.002627	± 2.5	PASS
		VN	30	4.28	0.002449	± 2.5	PASS
		VN	40	0.41	0.000235	± 2.5	PASS
		VN	50	1.54	0.000881	± 2.5	PASS
16QAM	LCH	VN	-30	0.73	0.000421	± 2.5	PASS
		VN	-20	-1.7	-0.000981	± 2.5	PASS
		VN	-10	0.92	0.000531	± 2.5	PASS
		VN	0	-0.39	-0.000225	± 2.5	PASS
		VN	10	1.67	0.000964	± 2.5	PASS
		VN	20	0.4	0.000231	± 2.5	PASS
		VN	30	2.42	0.001397	± 2.5	PASS
		VN	40	2.67	0.001541	± 2.5	PASS
		VN	50	0.09	0.000052	± 2.5	PASS
	MCH	VN	-30	4.69	0.002684	± 2.5	PASS
		VN	-20	2.79	0.001597	± 2.5	PASS
		VN	-10	-1.02	-0.000584	± 2.5	PASS
		VN	0	4.62	0.002644	± 2.5	PASS
		VN	10	0.44	0.000252	± 2.5	PASS
		VN	20	3.15	0.001803	± 2.5	PASS
		VN	30	0	0.000000	± 2.5	PASS
		VN	40	0.69	0.000395	± 2.5	PASS
		VN	50	3.62	0.002072	± 2.5	PASS
	HCH	VN	-30	2.59	0.001482	± 2.5	PASS
		VN	-20	3.81	0.002180	± 2.5	PASS
		VN	-10	4.79	0.002741	± 2.5	PASS
		VN	0	-1.37	-0.000784	± 2.5	PASS
		VN	10	1.56	0.000893	± 2.5	PASS
		VN	20	4.22	0.002415	± 2.5	PASS
		VN	30	3.1	0.001774	± 2.5	PASS
		VN	40	4.52	0.002587	± 2.5	PASS
		VN	50	0.25	0.000143	± 2.5	PASS

Channel Bandwidth: 20 MHz

Channel Bandwidth: 20 MHz							
Voltage							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VL	TN	4.9	0.002849	± 2.5	PASS
		VN	TN	-0.32	-0.000186	± 2.5	PASS
		VH	TN	4.99	0.002901	± 2.5	PASS
	MCH	VL	TN	0.72	0.000416	± 2.5	PASS
		VN	TN	1.47	0.000848	± 2.5	PASS
		VH	TN	1.47	0.000848	± 2.5	PASS
	HCH	VL	TN	3.79	0.002172	± 2.5	PASS
		VN	TN	3.18	0.001822	± 2.5	PASS
		VH	TN	3.84	0.002201	± 2.5	PASS
16QAM	LCH	VL	TN	0.03	0.000017	± 2.5	PASS
		VN	TN	2.75	0.001599	± 2.5	PASS
		VH	TN	3.1	0.001802	± 2.5	PASS
	MCH	VL	TN	2.78	0.001605	± 2.5	PASS
		VN	TN	4	0.002309	± 2.5	PASS
		VH	TN	1.74	0.001004	± 2.5	PASS
	HCH	VL	TN	2.8	0.001605	± 2.5	PASS
		VN	TN	4.12	0.002361	± 2.5	PASS
		VH	TN	2.1	0.001203	± 2.5	PASS
Temperature							
Modulation	Channel	Voltage [Vdc]	Temperature (℃)	Deviation (Hz)	Deviation (ppm)	Limit (ppm)	Verdict
QPSK	LCH	VN	-30	-1.23	-0.000715	± 2.5	PASS
		VN	-20	3.17	0.001843	± 2.5	PASS
		VN	-10	4.55	0.002645	± 2.5	PASS
		VN	0	0.24	0.000140	± 2.5	PASS
		VN	10	0.02	0.000012	± 2.5	PASS
		VN	20	1.17	0.000680	± 2.5	PASS
		VN	30	-1.89	-0.001099	± 2.5	PASS
		VN	40	-0.8	-0.000465	± 2.5	PASS
		VN	50	3.02	0.001756	± 2.5	PASS
	MCH	VN	-30	-0.45	-0.000260	± 2.5	PASS
		VN	-20	1.53	0.000883	± 2.5	PASS
		VN	-10	0.82	0.000473	± 2.5	PASS
		VN	0	0.32	0.000185	± 2.5	PASS
		VN	10	4.37	0.002522	± 2.5	PASS

		VN	20	4.73	0.002730	± 2.5	PASS
		VN	30	2.07	0.001195	± 2.5	PASS
		VN	40	0.17	0.000098	± 2.5	PASS
		VN	50	-1.9	-0.001097	± 2.5	PASS
	HCH	VN	-30	-1.69	-0.000968	± 2.5	PASS
		VN	-20	-0.01	-0.000006	± 2.5	PASS
		VN	-10	3.97	0.002275	± 2.5	PASS
		VN	0	3.48	0.001994	± 2.5	PASS
		VN	10	3.64	0.002086	± 2.5	PASS
		VN	20	-0.12	-0.000069	± 2.5	PASS
		VN	30	4.89	0.002802	± 2.5	PASS
		VN	40	1.55	0.000888	± 2.5	PASS
		VN	50	4.99	0.002860	± 2.5	PASS
16QAM	LCH	VN	-30	0.21	0.000121	± 2.5	PASS
		VN	-20	2.72	0.001570	± 2.5	PASS
		VN	-10	-0.51	-0.000294	± 2.5	PASS
		VN	0	-0.18	-0.000104	± 2.5	PASS
		VN	10	2.13	0.001229	± 2.5	PASS
		VN	20	2.91	0.001680	± 2.5	PASS
		VN	30	1.84	0.001062	± 2.5	PASS
		VN	40	2.58	0.001489	± 2.5	PASS
		VN	50	1.64	0.000947	± 2.5	PASS
	MCH	VN	-30	3.44	0.001971	± 2.5	PASS
		VN	-20	4.34	0.002487	± 2.5	PASS
		VN	-10	1.88	0.001077	± 2.5	PASS
		VN	0	2.48	0.001421	± 2.5	PASS
		VN	10	-0.81	-0.000464	± 2.5	PASS
		VN	20	2.25	0.001289	± 2.5	PASS
		VN	30	-1.47	-0.000842	± 2.5	PASS
		VN	40	1.75	0.001003	± 2.5	PASS
		VN	50	2.71	0.001553	± 2.5	PASS
	HCH	VN	-30	-0.05	-0.000029	± 2.5	PASS
		VN	-20	3.78	0.002166	± 2.5	PASS
		VN	-10	4.96	0.002842	± 2.5	PASS
		VN	0	-1.26	-0.000722	± 2.5	PASS
		VN	10	3.16	0.001811	± 2.5	PASS
		VN	20	0.03	0.000017	± 2.5	PASS
		VN	30	0.67	0.000384	± 2.5	PASS
		VN	40	4.1	0.002350	± 2.5	PASS
		VN	50	-1.05	-0.000602	± 2.5	PASS