


The FCC ID shall be permanently affixed in the rear side of the equipment

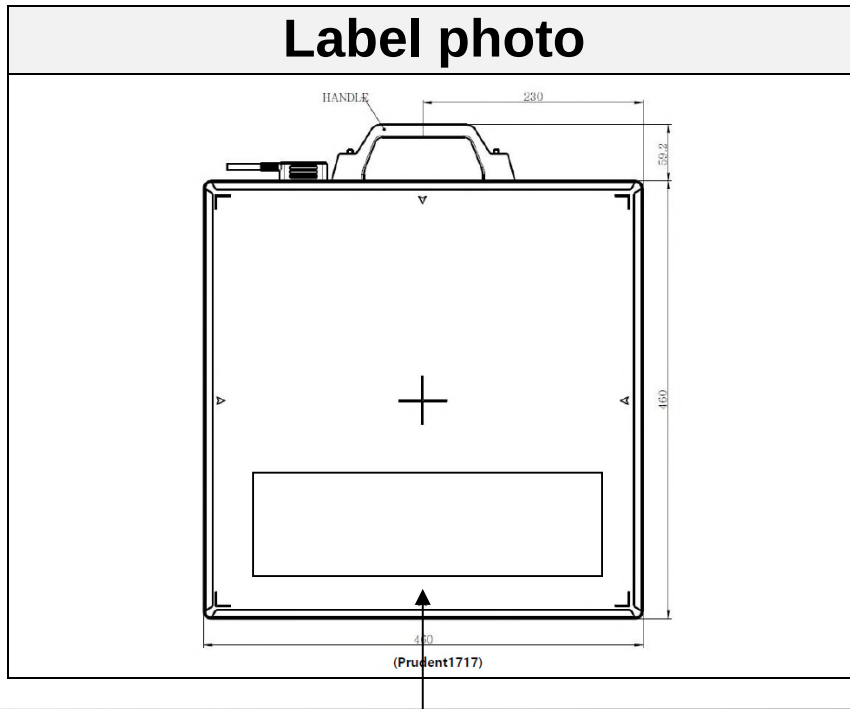

PIXXGEN

Product Name : Flat Panel Digital X-ray Detector
Model Name : Prudent 1717
Serial Number :

- Manufactured Date :
- Specification : 460X460X15 mm
- Weight : 3,9 Kg $\pm 10\%$
- Rating : 18Vd.c., 3.5A
- Battery : DC14.8V, 3300mAh
- Manufacturer : PIXXGEN Corporation

! For use with Charger PIXXGEN Model PICB only

EC REP

CMC Medical Device & Djrugs S.L.

C/Horacio Lengo N° 18, CP 29006, Málaga, Spain.

CE

Tested To comply with
FCC Standards

1370

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful, and (2) this device must accept any interference received, including interference that may cause undesired operation.



FCC ID: 2AWVMPRUDENT1717

PIXXGEN Corporation
MADE IN KOREA

5F, SMART BAY, 123, Beolmal-ro, Dongan-gu,
Anyang-si, Gyeonggi-do, 14056, Korea