

Date: 2025-08-11

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250811 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 42.8$ Ambient

Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.75, 9.37, 9.43); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.44 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.16 W/kg; SAR (8g) = 1.52 W/kg; SAR (10g) = 1.44 W/kg

Smallest distance from peaks to all points 3 dB below = 18.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

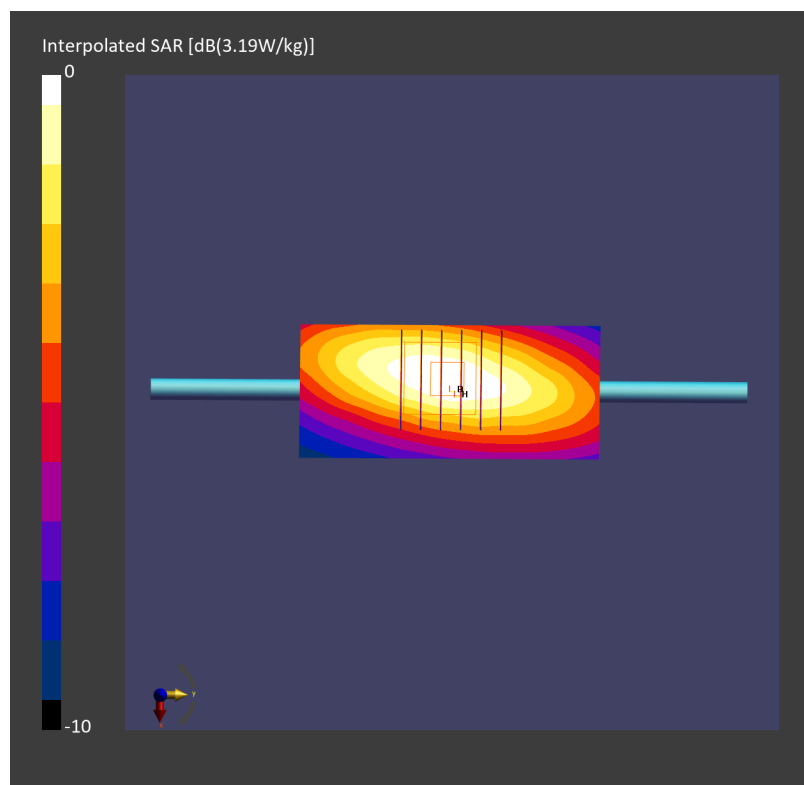

Date: 2025-08-14

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250814 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.888$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(9.46, 9.11, 8.98); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.18 W/kg; SAR (10g) = 1.47 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.57 W/kg; SAR (10g) = 1.50 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.9 %

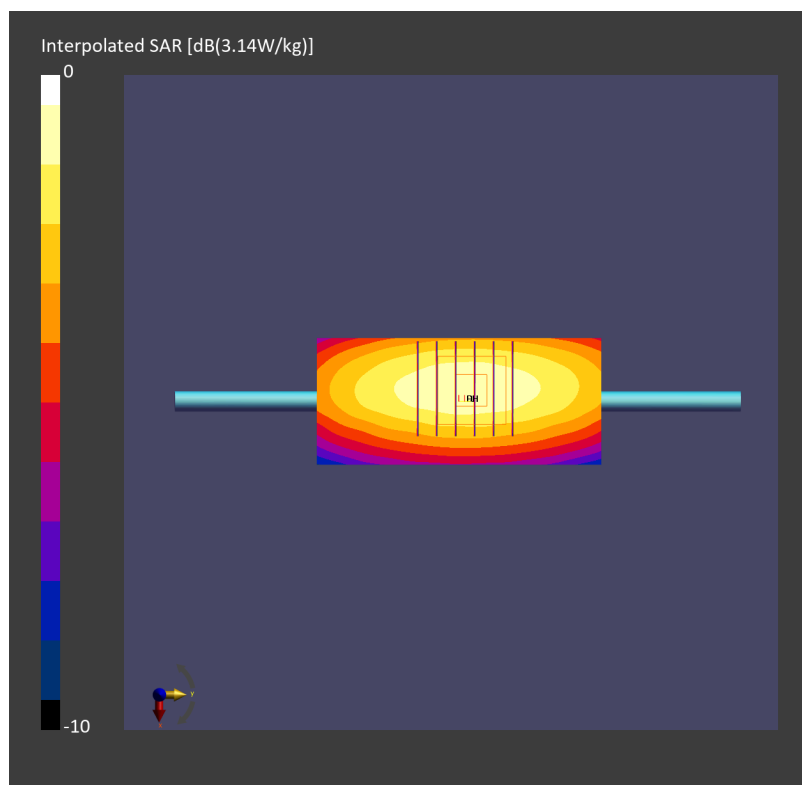

Date: 2025-08-14

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250814 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.896$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(9.6, 9.44, 9.5); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.08 W/kg; SAR (10g) = 1.39 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.07 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.38 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

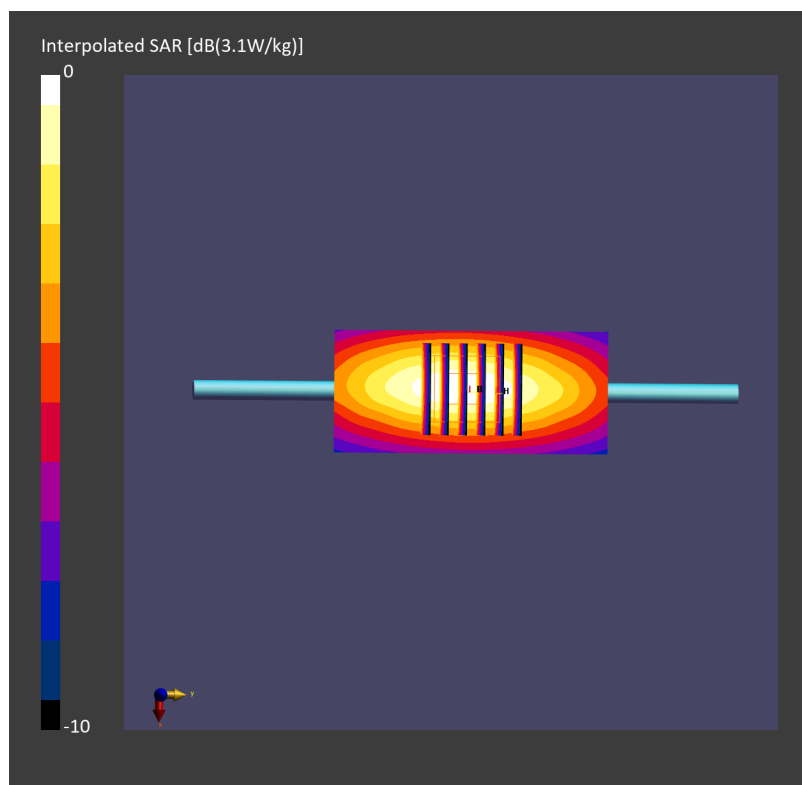

Date: 2025-08-21

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250821 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.893$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.75, 9.37, 9.43); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.06 W/kg; SAR (10g) = 1.38 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 2.06 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.37 W/kg

Smallest distance from peaks to all points 3 dB below = 16.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

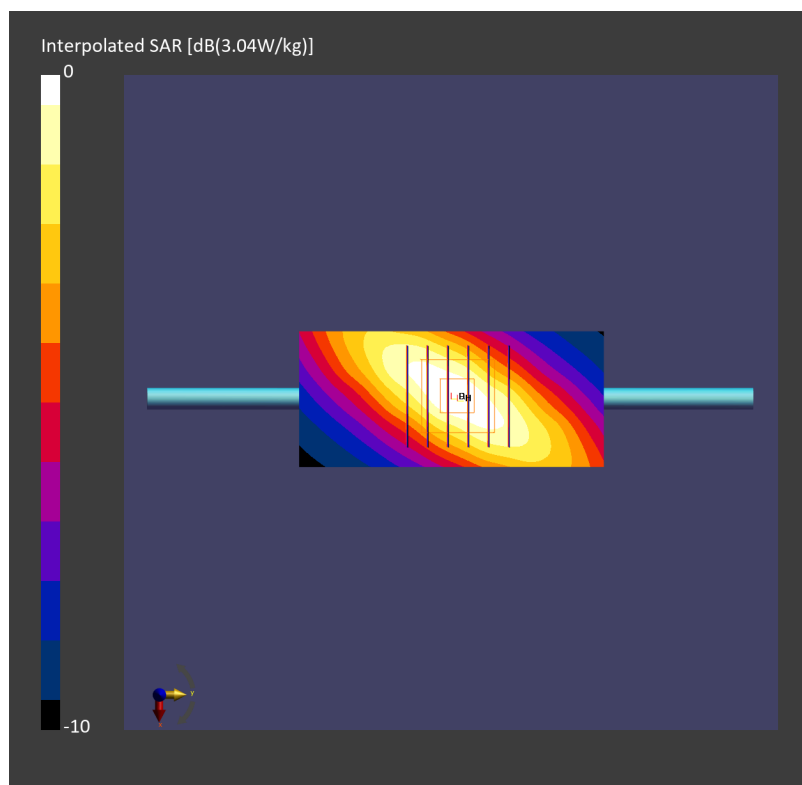

Date: 2025-08-12

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250812 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.925$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(10.0, 9.61, 9.66); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.29 W/kg; SAR (10g) = 1.50 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.29 W/kg; SAR (8g) = 1.59 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

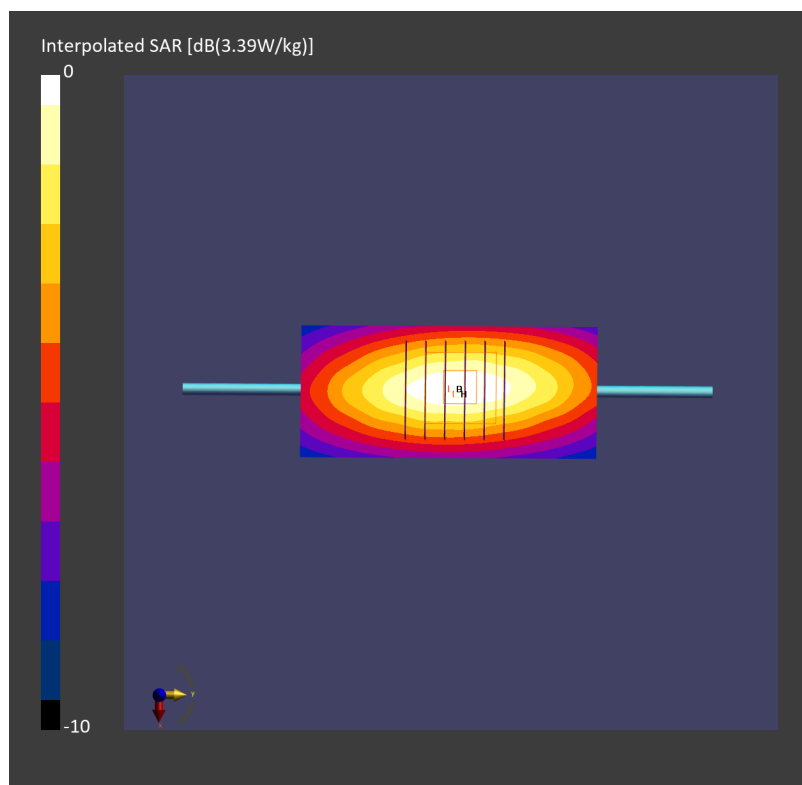

Date: 2025-08-14

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250814 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.922$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(9.11, 8.77, 8.65); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.69 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.82 W/kg; SAR (10g) = 1.74 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

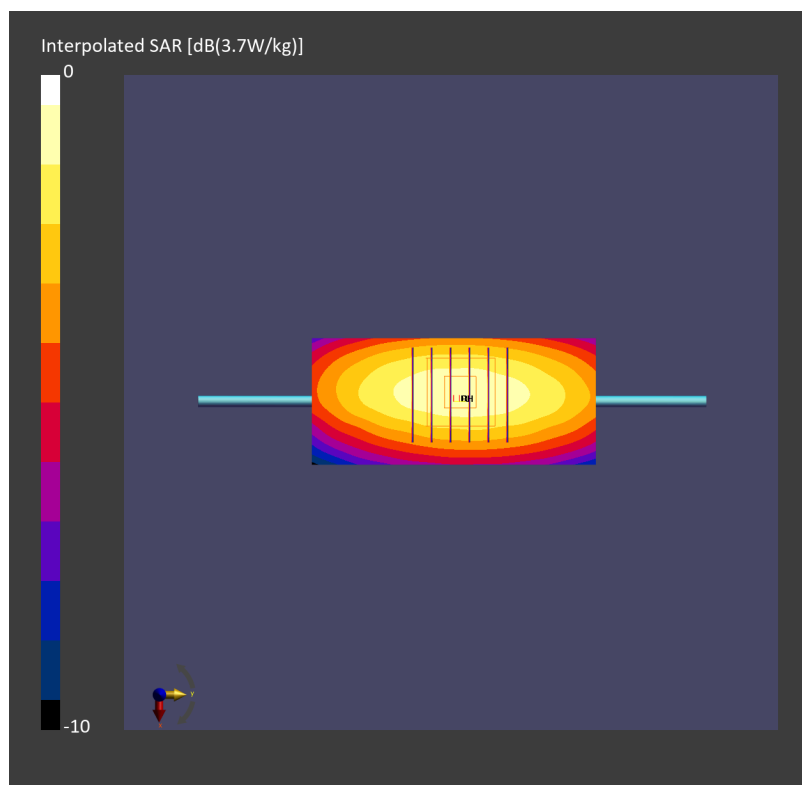

Date: 2025-08-14

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250814 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(9.27, 9.12, 9.17); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.57 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.36 W/kg; SAR (8g) = 1.64 W/kg; SAR (10g) = 1.56 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

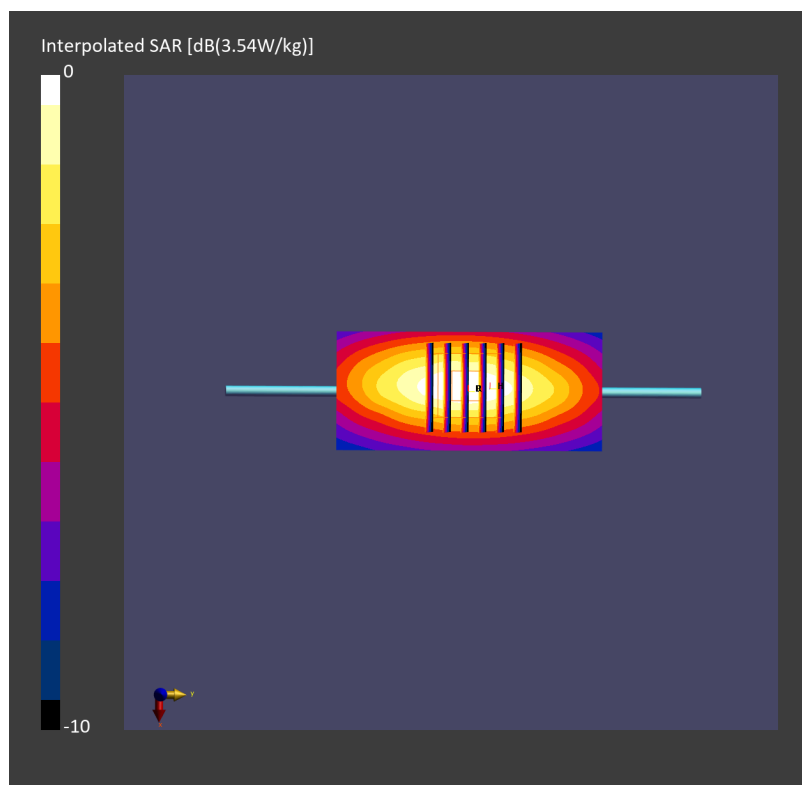

Date: 2025-08-22

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250822 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(10.0, 9.61, 9.66); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.29 W/kg; SAR (10g) = 1.50 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.29 W/kg; SAR (8g) = 1.59 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

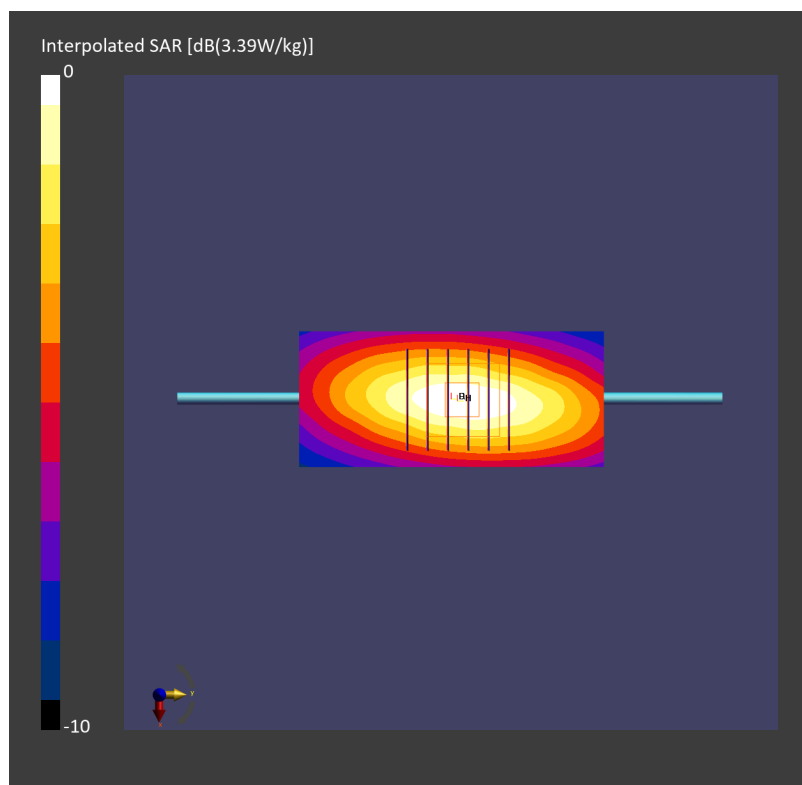

Date: 2025-08-15

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250815 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.9, 7.61, 7.5); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 0.972 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

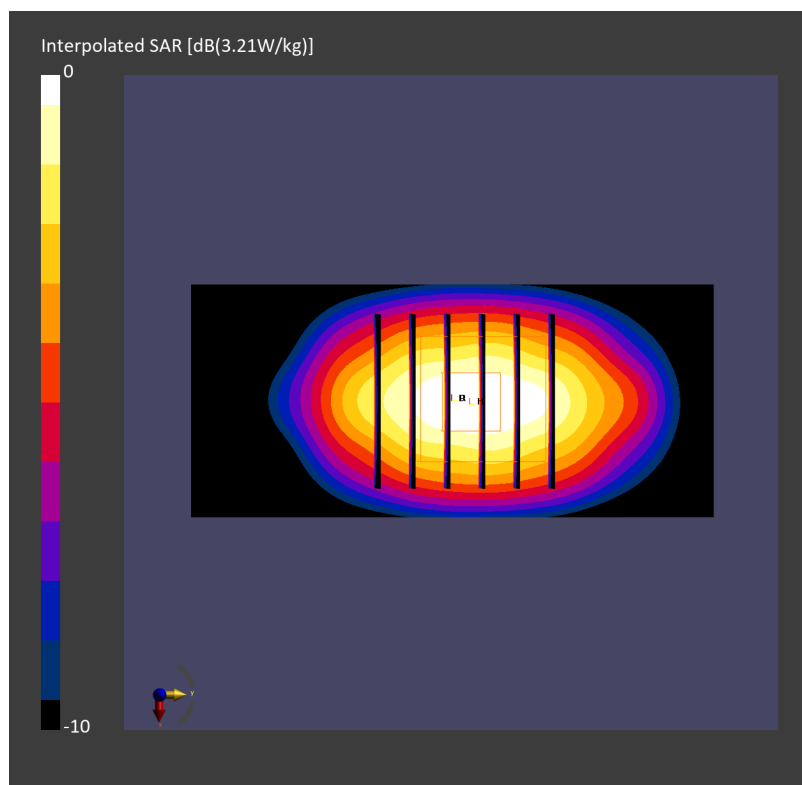

Date: 2025-08-15

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250815 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.72 W/kg; SAR (10g) = 0.926 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.944 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

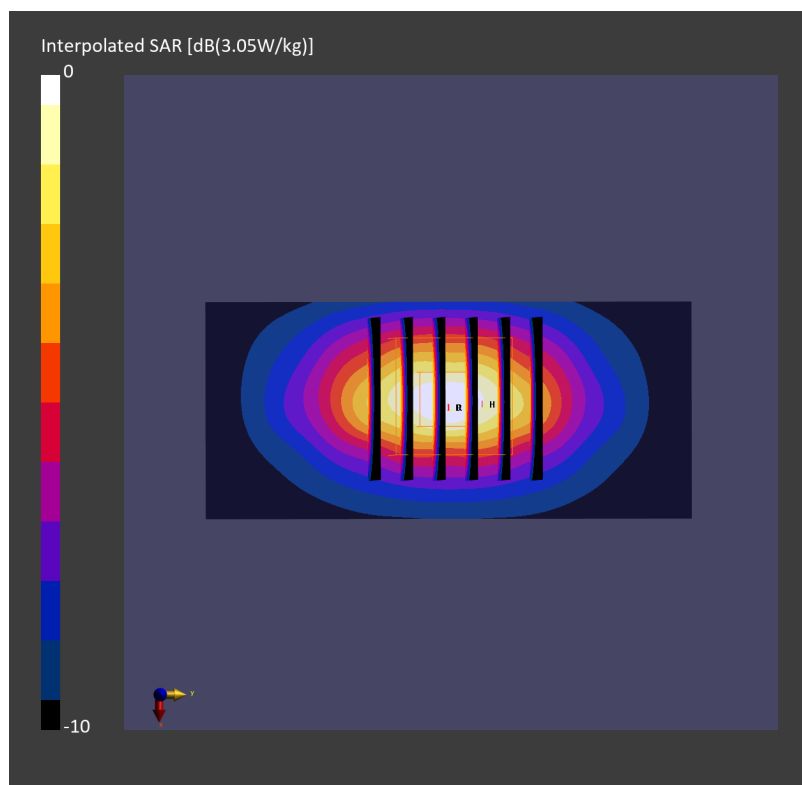

Date: 2025-08-24

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250824 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.38, 8.05, 8.1); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.950 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.969 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.8 %

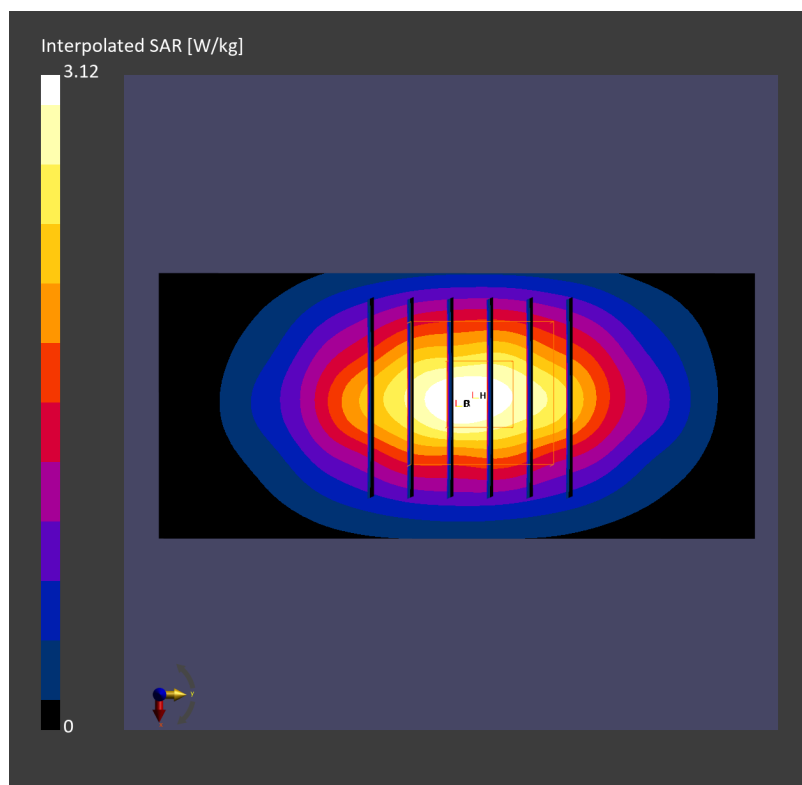

Date: 2025-08-15

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250815 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.67, 7.38, 7.28); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.1 W/kg; SAR (10g) = 5.44 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 10.3 W/kg; SAR (8g) = 6.06 W/kg; SAR (10g) = 5.60 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 86.3 %

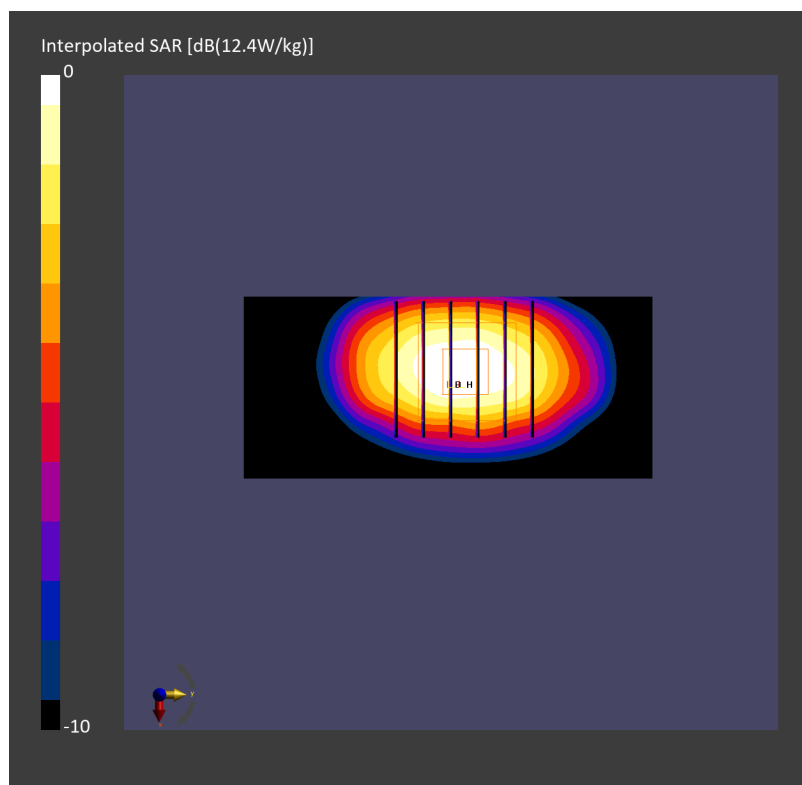

Date: 2025-08-15

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250815 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.979 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.984 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

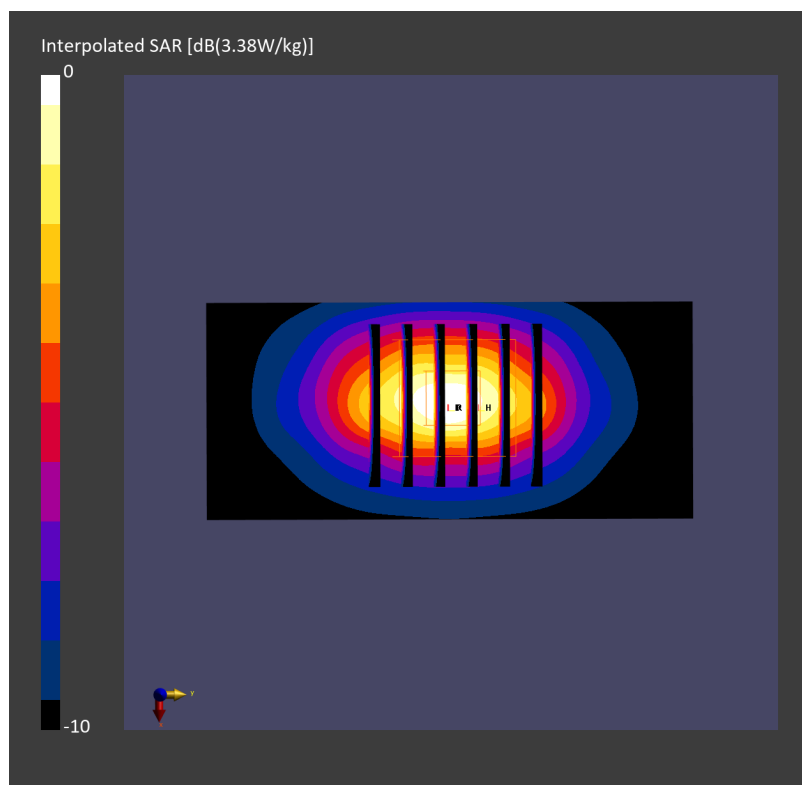

Date: 2025-08-27

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250827 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.94, 7.63, 7.67); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 0.982 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

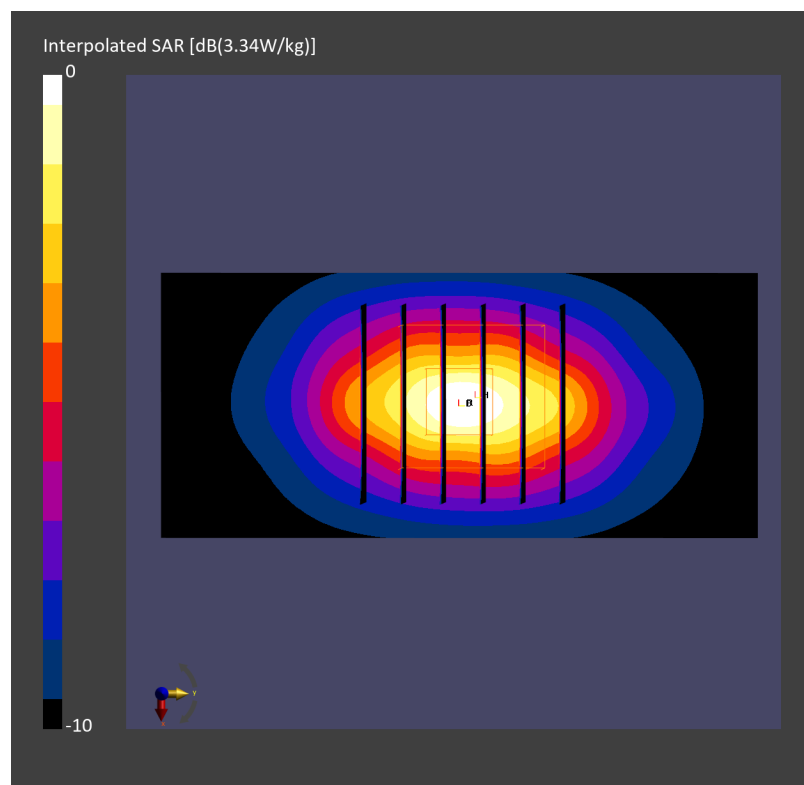

Date: 2025-08-16

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250816 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.67$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.37, 7.09, 6.99); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_0mm; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 11.6 W/kg; SAR (10g) = 5.78 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 12.2 W/kg; SAR (8g) = 6.66 W/kg; SAR (10g) = 6.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

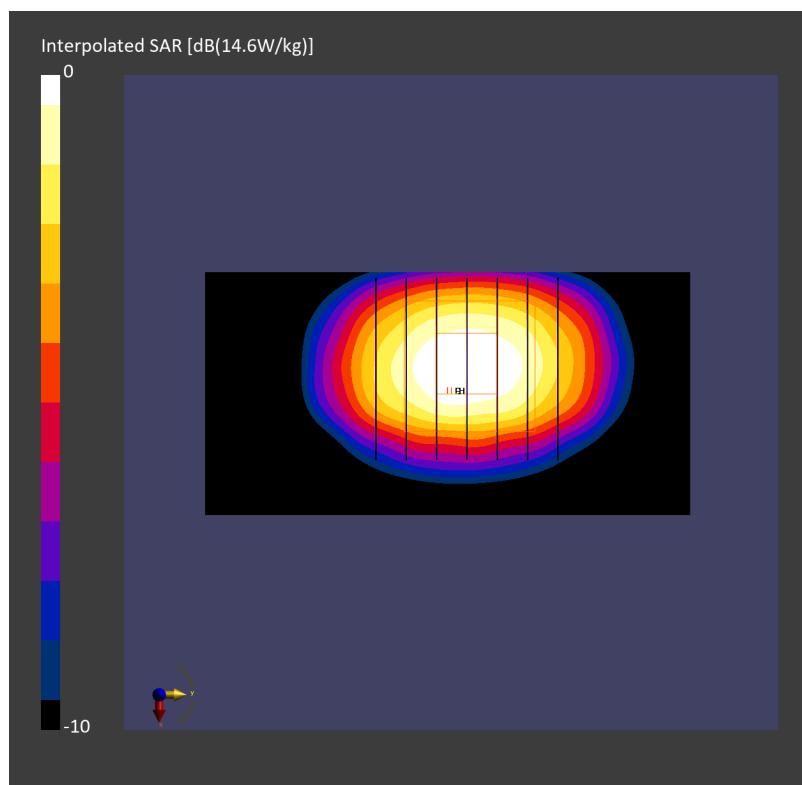

Date: 2025-08-16

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250816 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.67$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.37, 7.25, 7.29); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.15 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.45 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.8 %

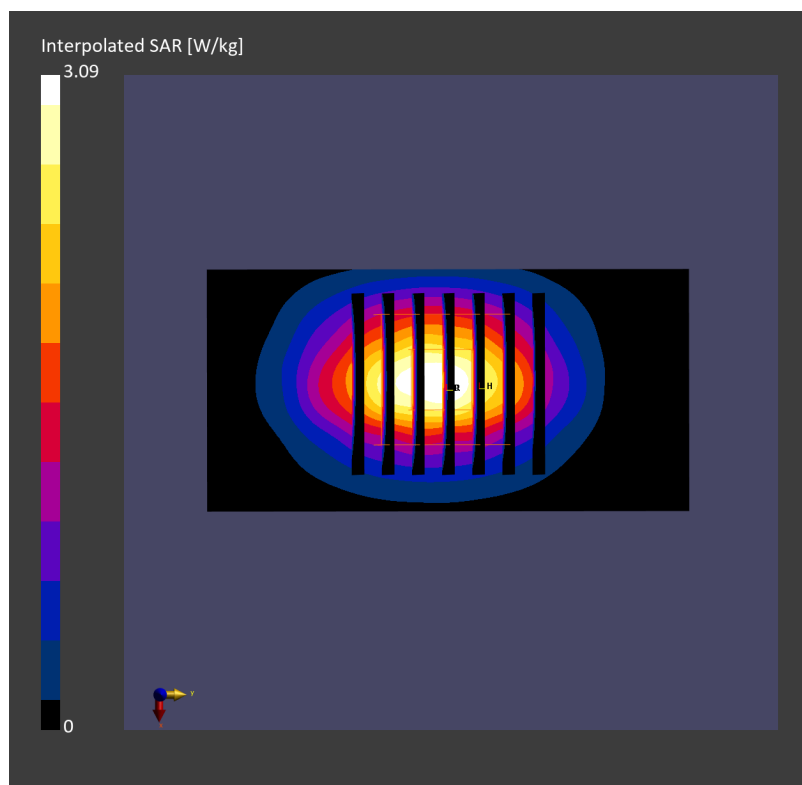

Date: 2025-08-25

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250825 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.66, 7.36, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.0 W/kg; SAR (10g) = 5.66 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 12.0 W/kg; SAR (8g) = 6.38 W/kg; SAR (10g) = 5.81 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

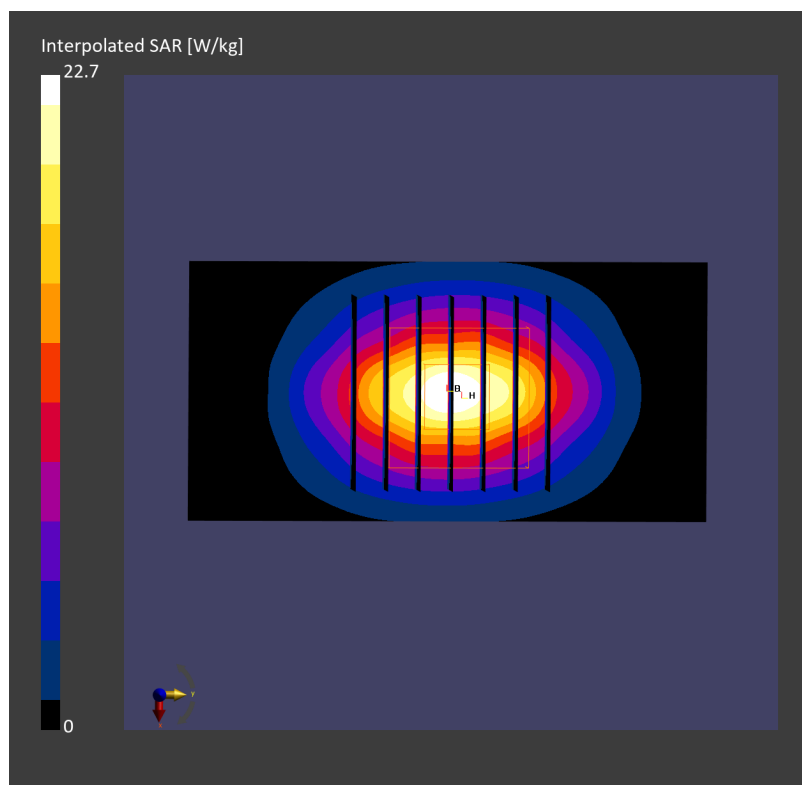

Date: 2025-08-28

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250828 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.64$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.66, 7.36, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 11.2 W/kg; SAR (10g) = 5.27 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 11.2 W/kg; SAR (8g) = 5.96 W/kg; SAR (10g) = 5.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

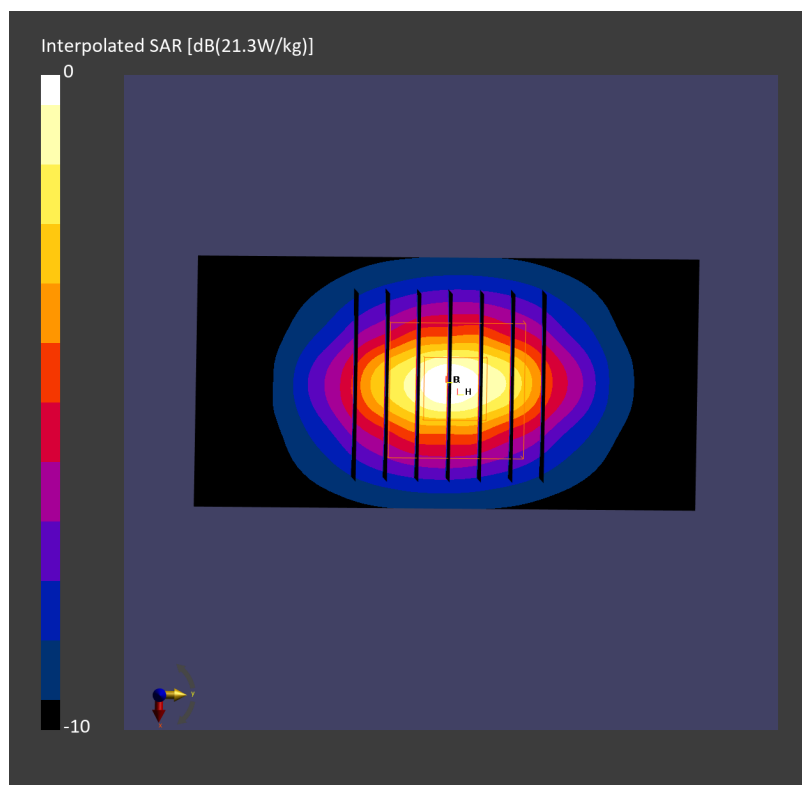

Date: 2025-08-16

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250816 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.01, 6.75, 6.65); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.91 W/kg; SAR (10g) = 1.30 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.91 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.4 %

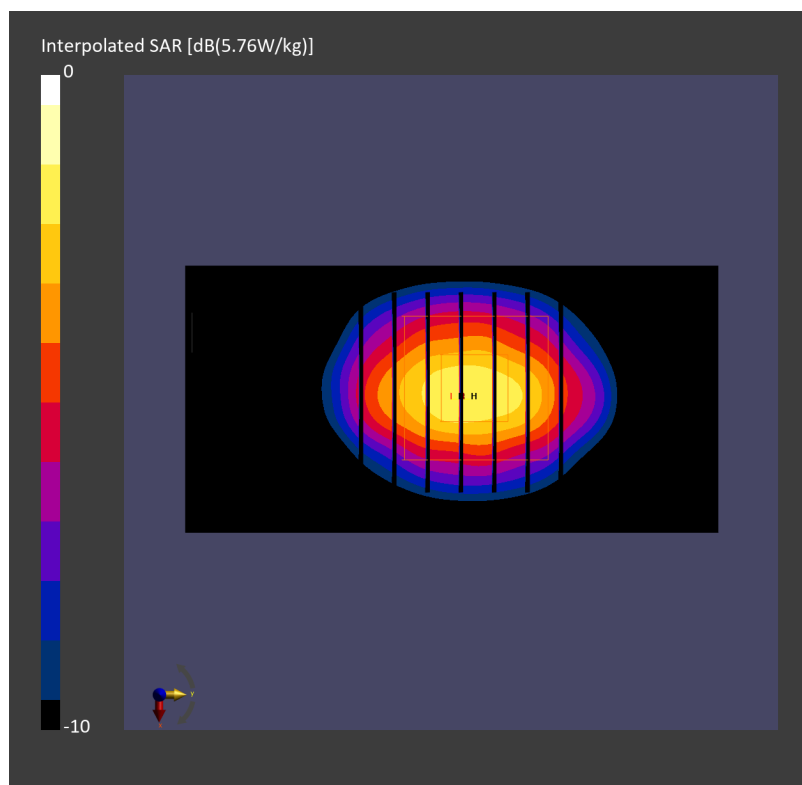

Date: 2025-08-16

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250816 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.97 W/kg; SAR (10g) = 1.33 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 3.04 W/kg; SAR (8g) = 1.51 W/kg; SAR (10g) = 1.36 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.6 %

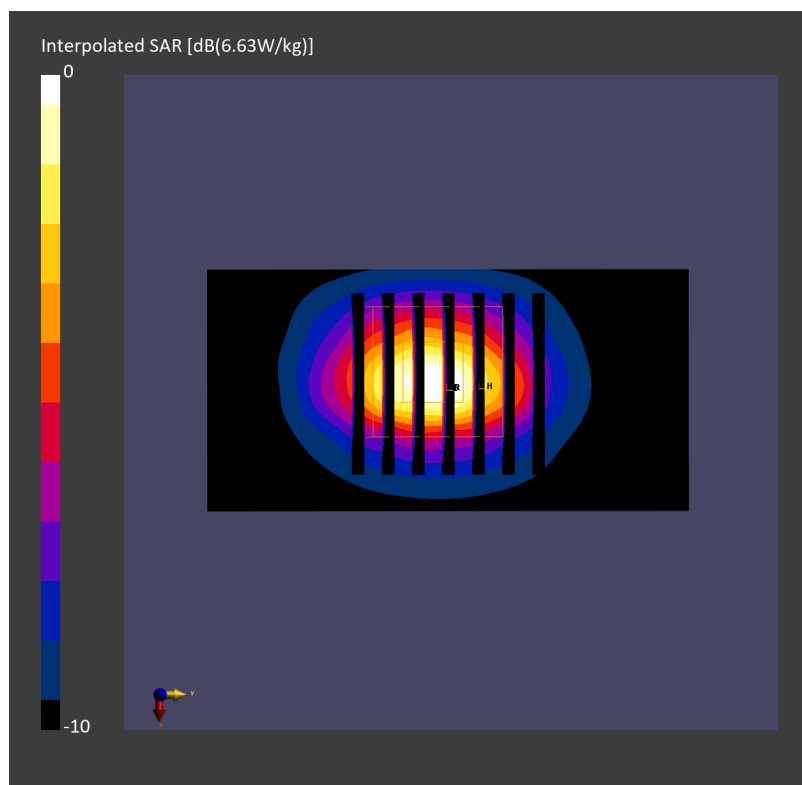

Date: 2025-08-25

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250825 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.65, 7.35, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.1 W/kg; SAR (10g) = 5.82 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.2 W/kg; SAR (8g) = 6.67 W/kg; SAR (10g) = 6.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

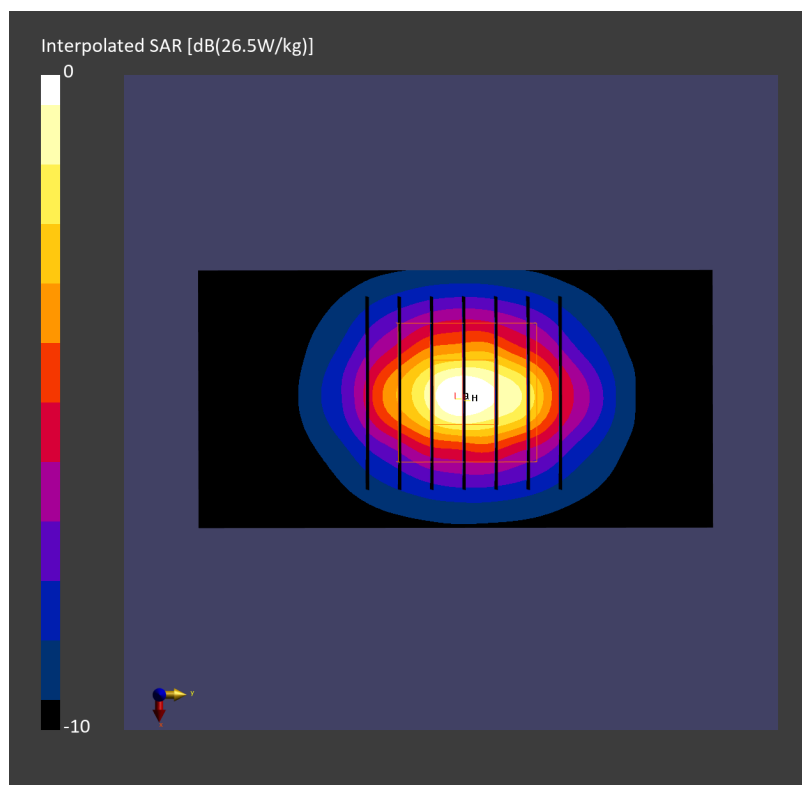

Date: 2025-08-28

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250828 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.65, 7.35, 7.4); Calibrated: 2025-01-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.7 W/kg; SAR (10g) = 6.11 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 13.8 W/kg; SAR (8g) = 6.95 W/kg; SAR (10g) = 6.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

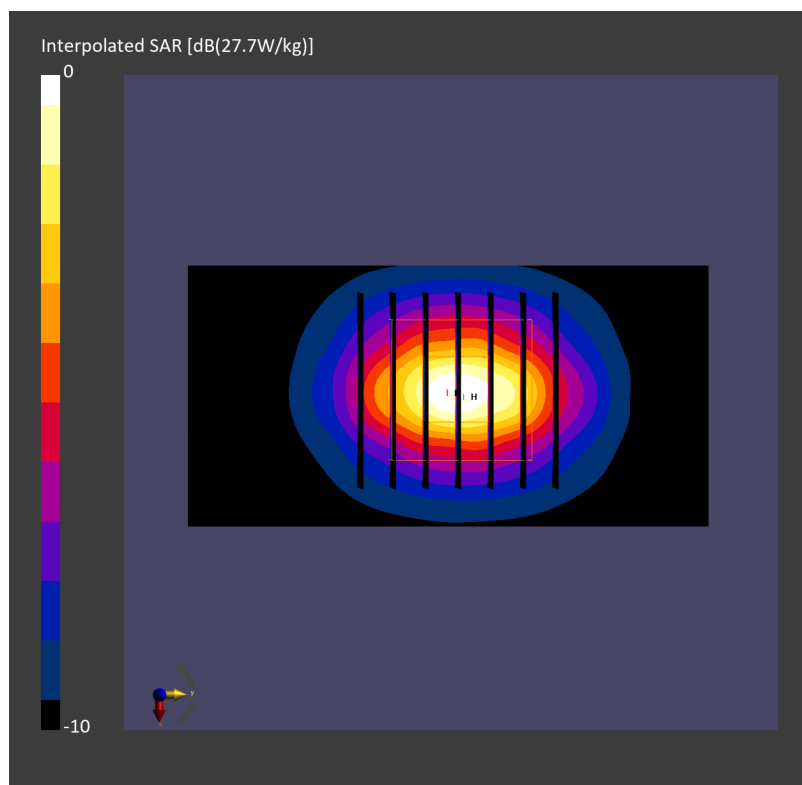

Date: 2025-08-13

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250813 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(6.6, 6.35, 6.26); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.24 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

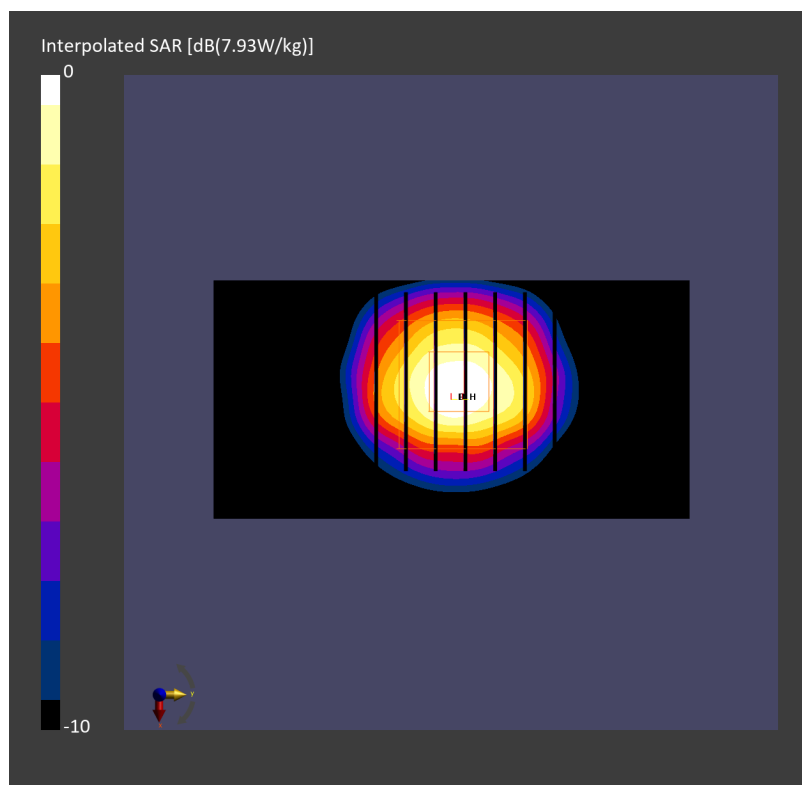

Date: 2025-08-16

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250816 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.31 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.51 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

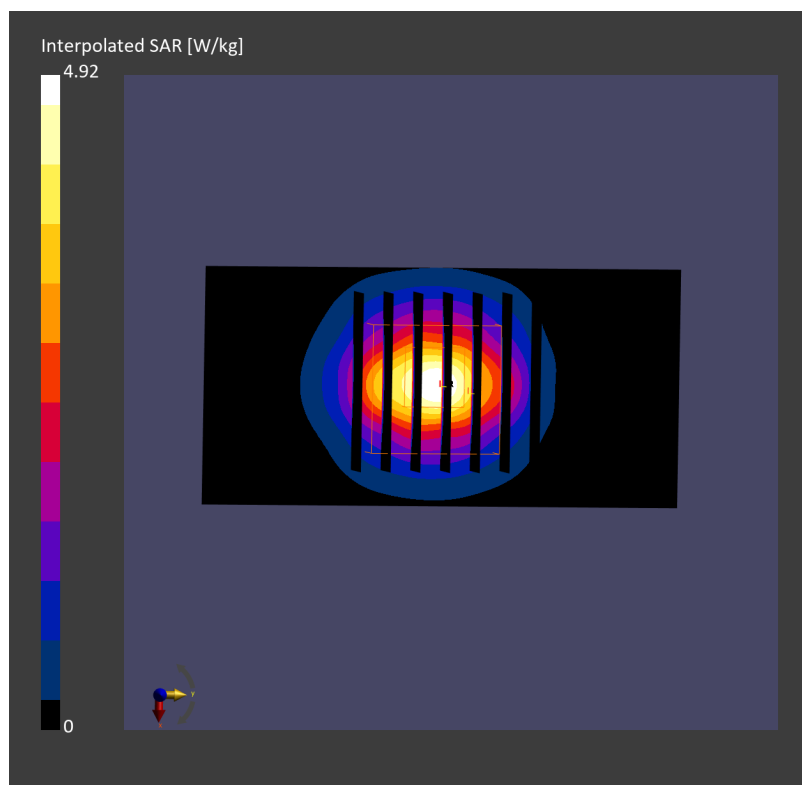

Date: 2025-08-13

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250813 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(6.54, 6.3, 6.21); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1794; Calibrated: 2025-02-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055_for Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.3 W/kg; SAR (10g) = 6.64 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 18.1 W/kg; SAR (8g) = 7.81 W/kg; SAR (10g) = 6.91 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.6 %

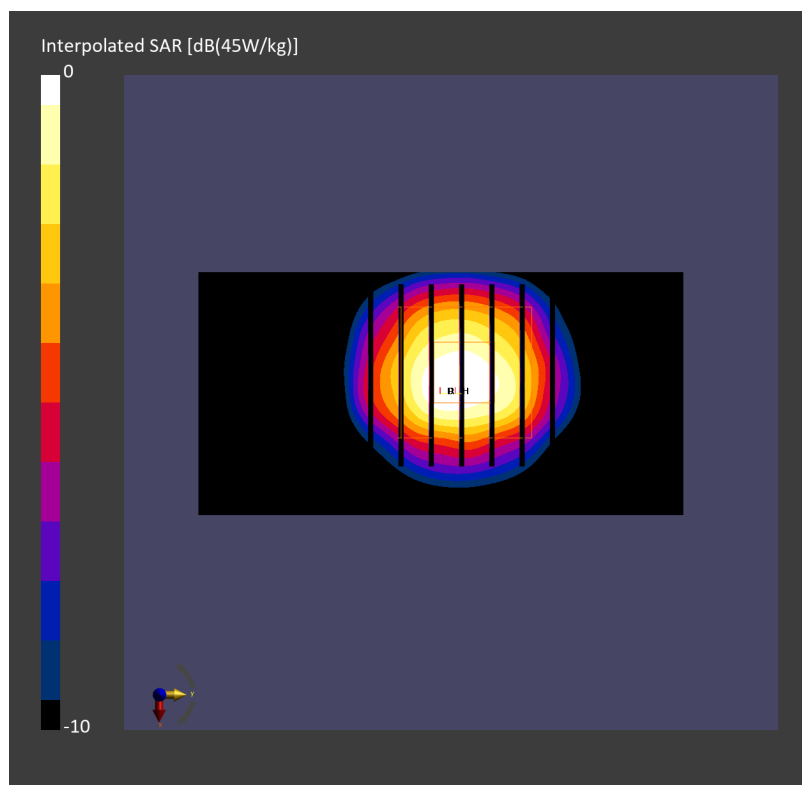

Date: 2025-08-16

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250816 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.56 W/kg; SAR (10g) = 1.35 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.81 W/kg; SAR (8g) = 1.59 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.4 %

