



Moisture analyzer MA X2 - external photographs


1. Device equipped with internal calibration

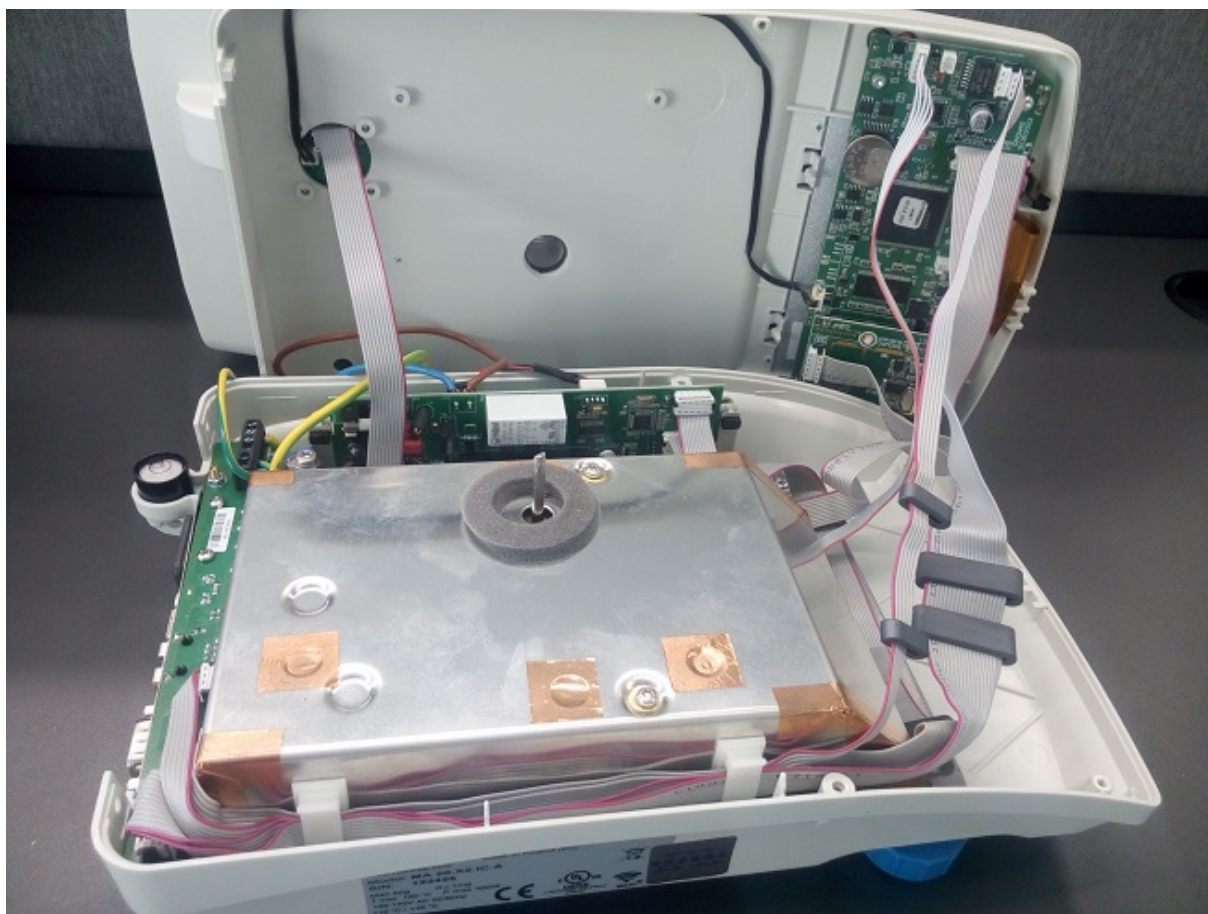


Both parts of housing

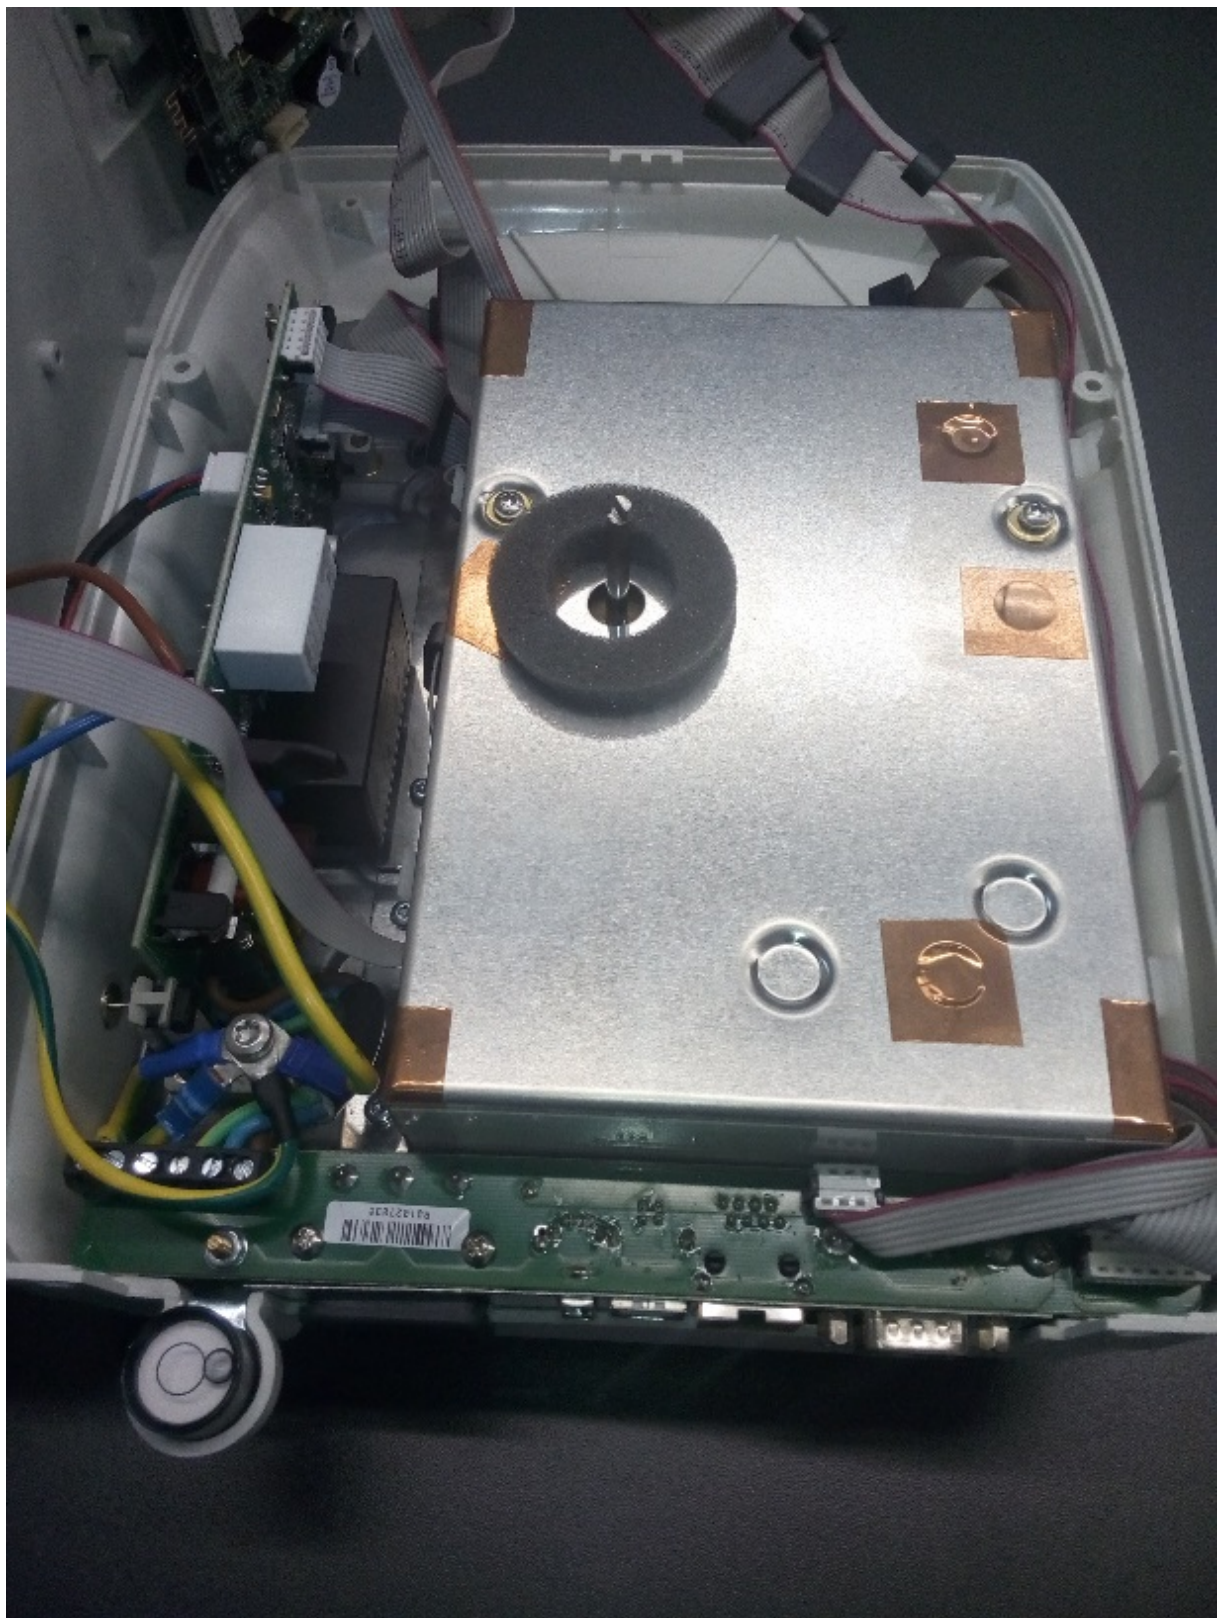

Bottom part

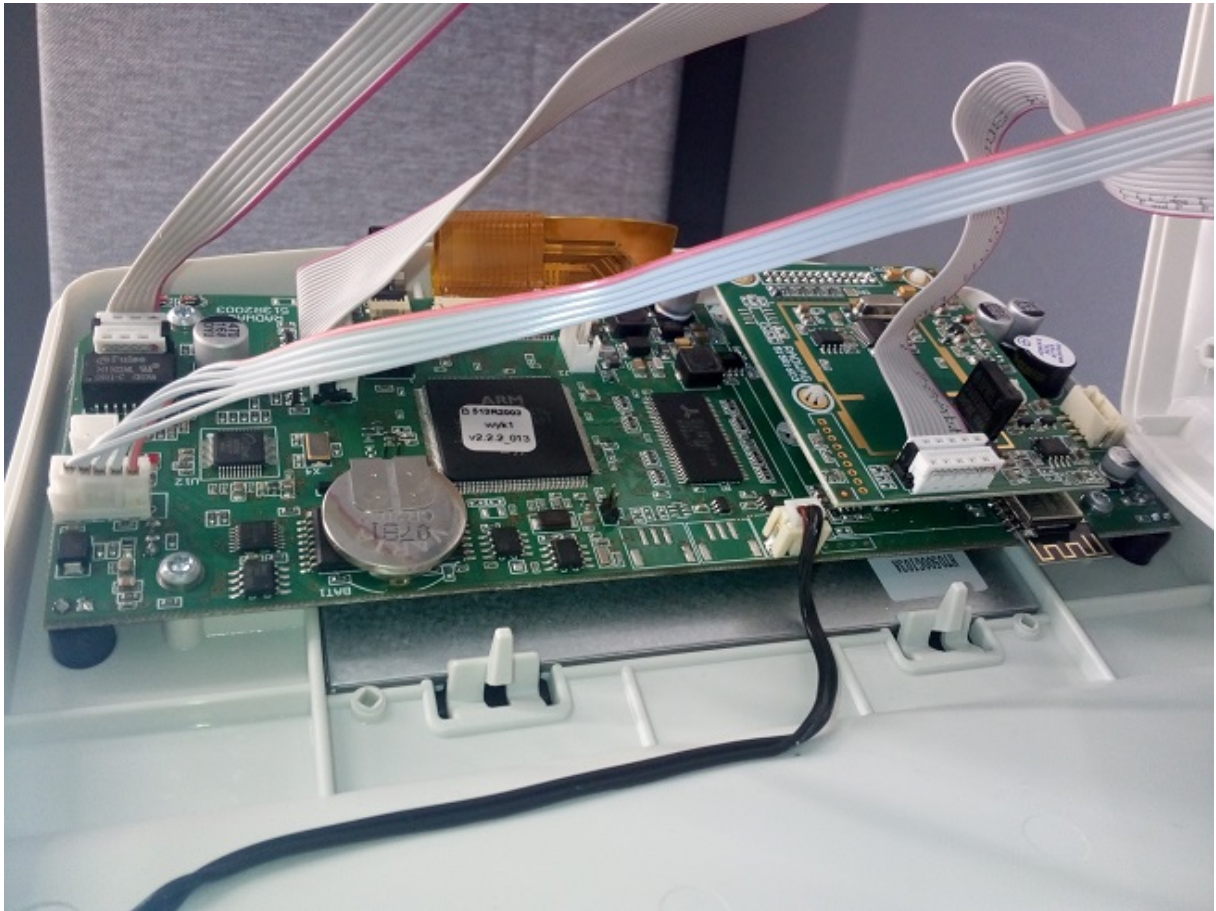


Top part

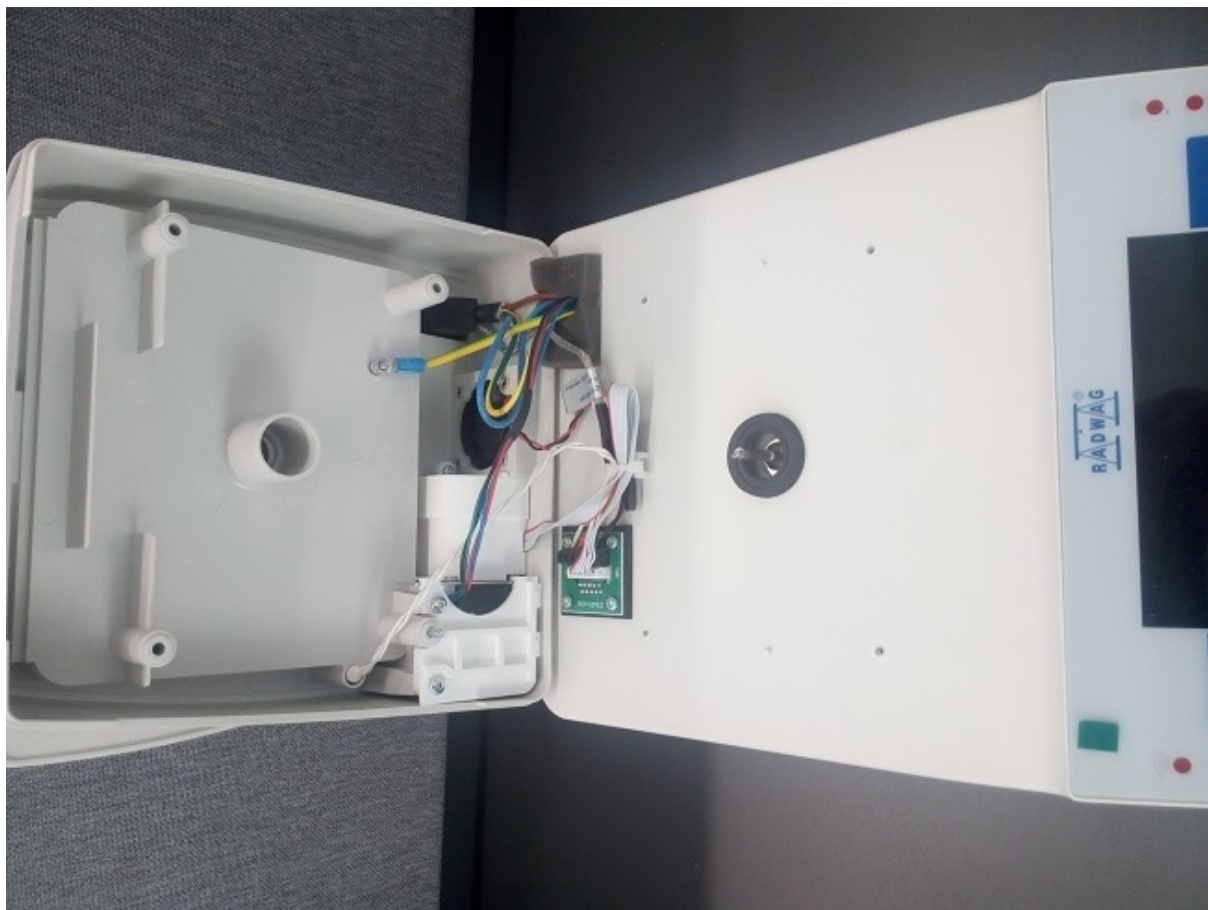


A cooling chamber under the weighing pan

2. Device not equipped with internal calibration

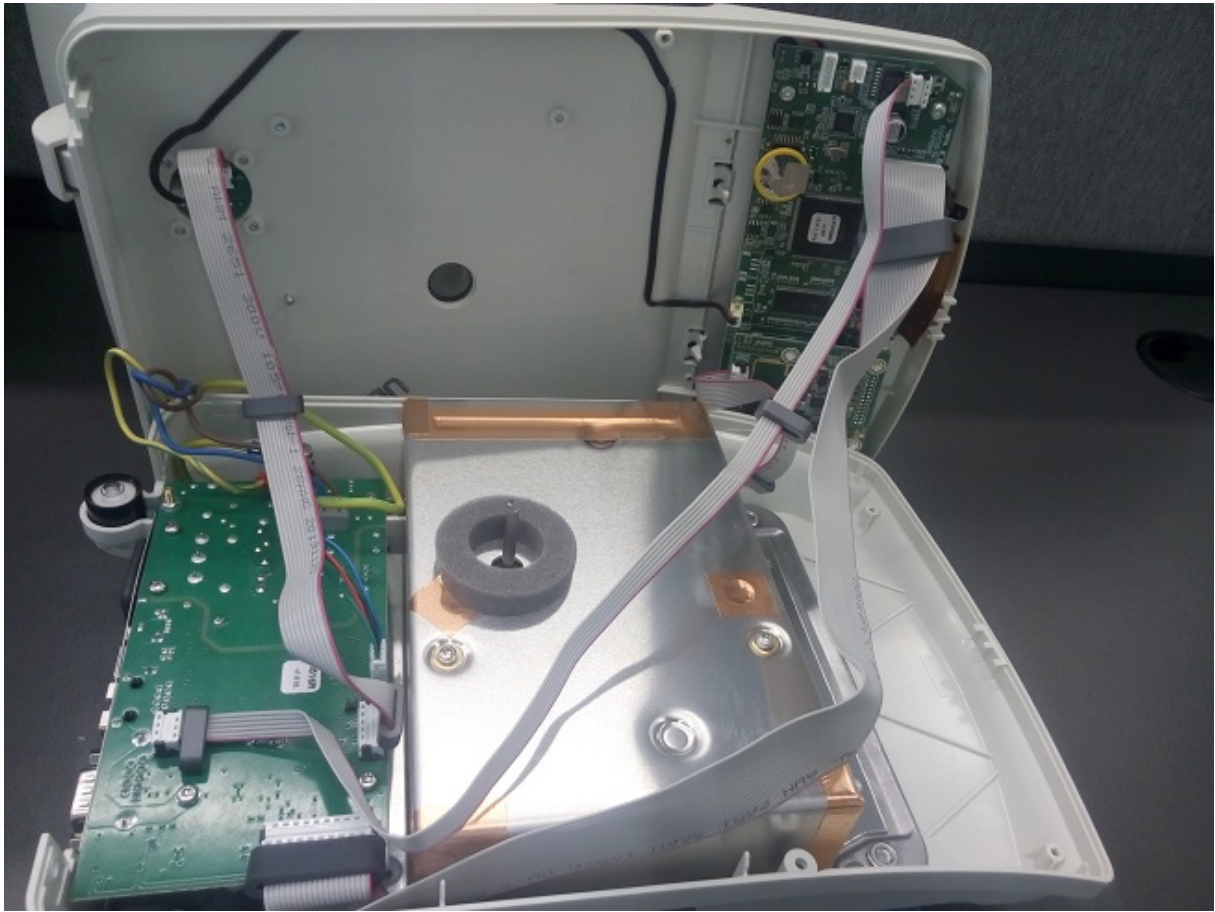


Both parts of housing

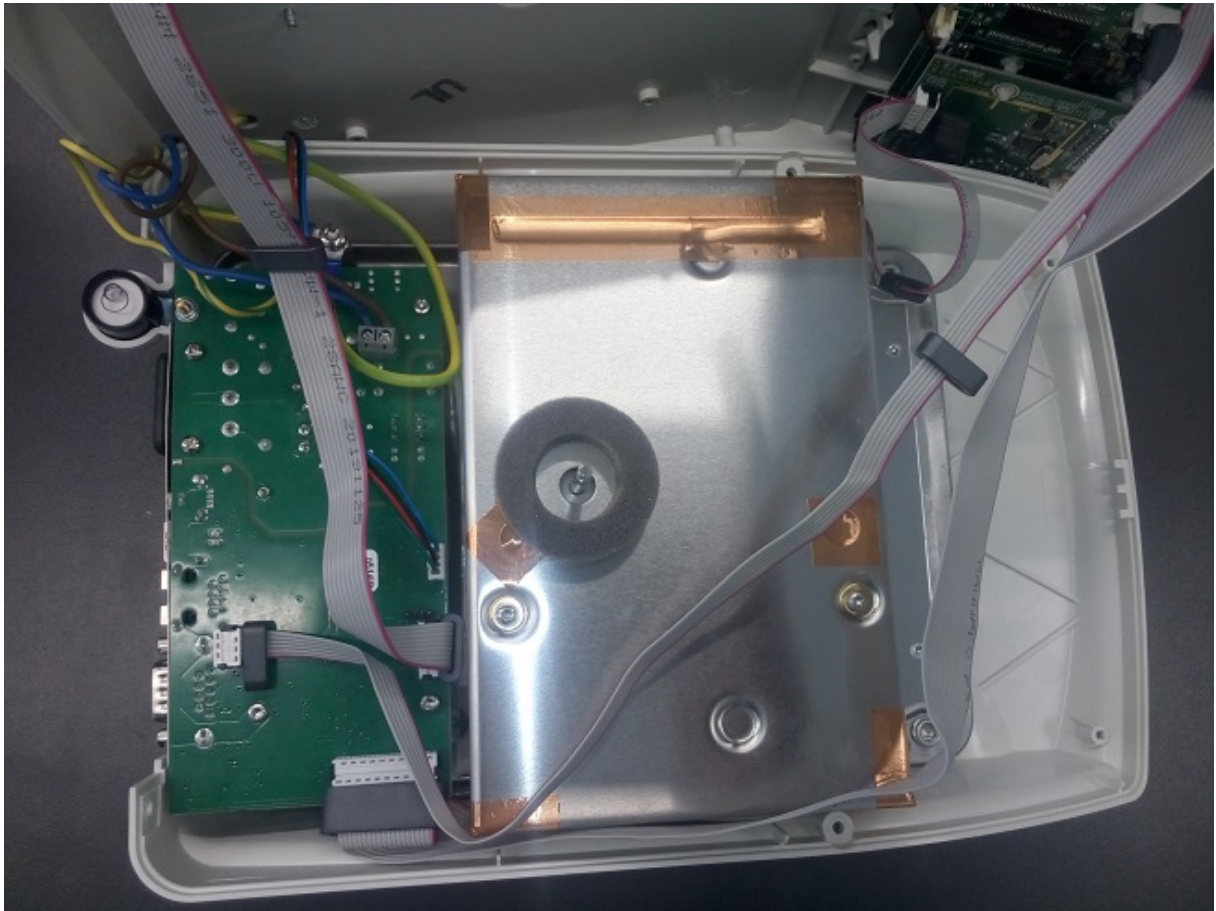

Bottom part



Top part

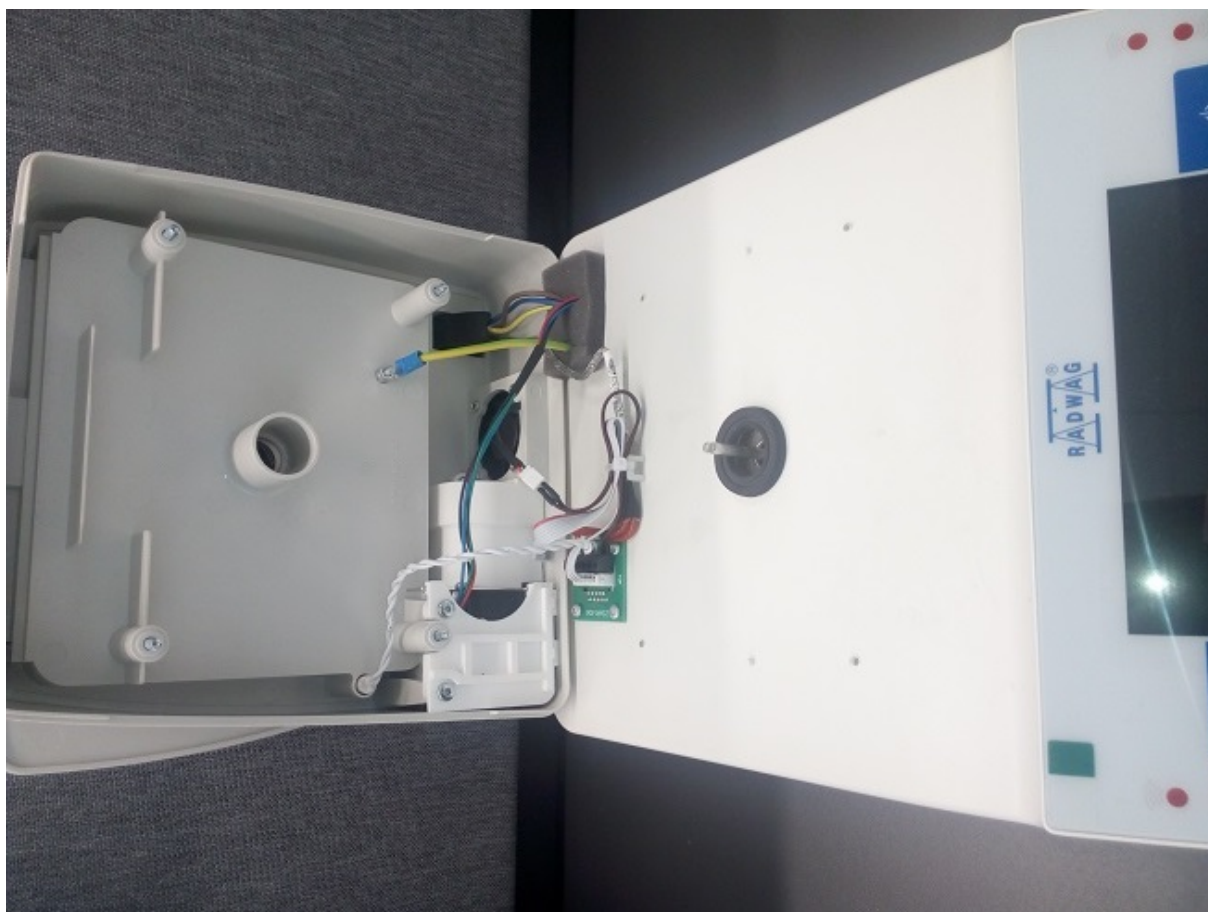

A cooling chamber under the weighing pan