


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

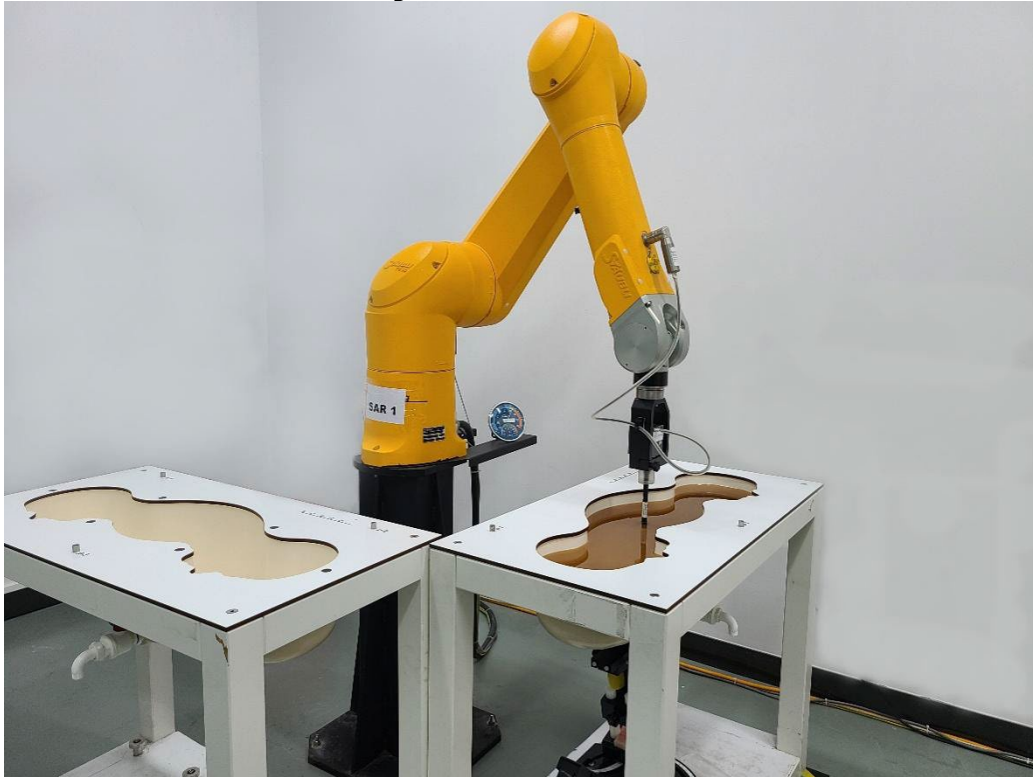

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the liquid level reaching approximately the 10 cm mark. The container has a blue outer rim and a white inner lining.	NA

3. Photographs of EUT test position

Photo 2: Front Side 10mm



Photo 3: Back Side 10mm



Photo 4: Left Side 10mm




Photo 5: Right Side 10mm



Photo 6: Top Side 10mm



Photo 7: Bottom Side 10mm

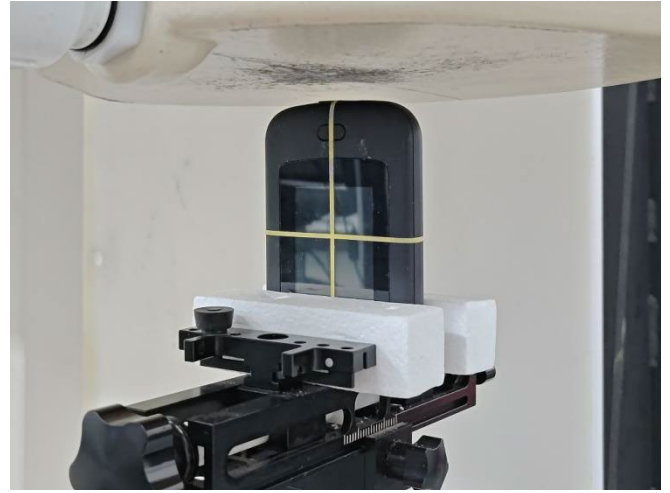

4. EUT Constructional Details

