

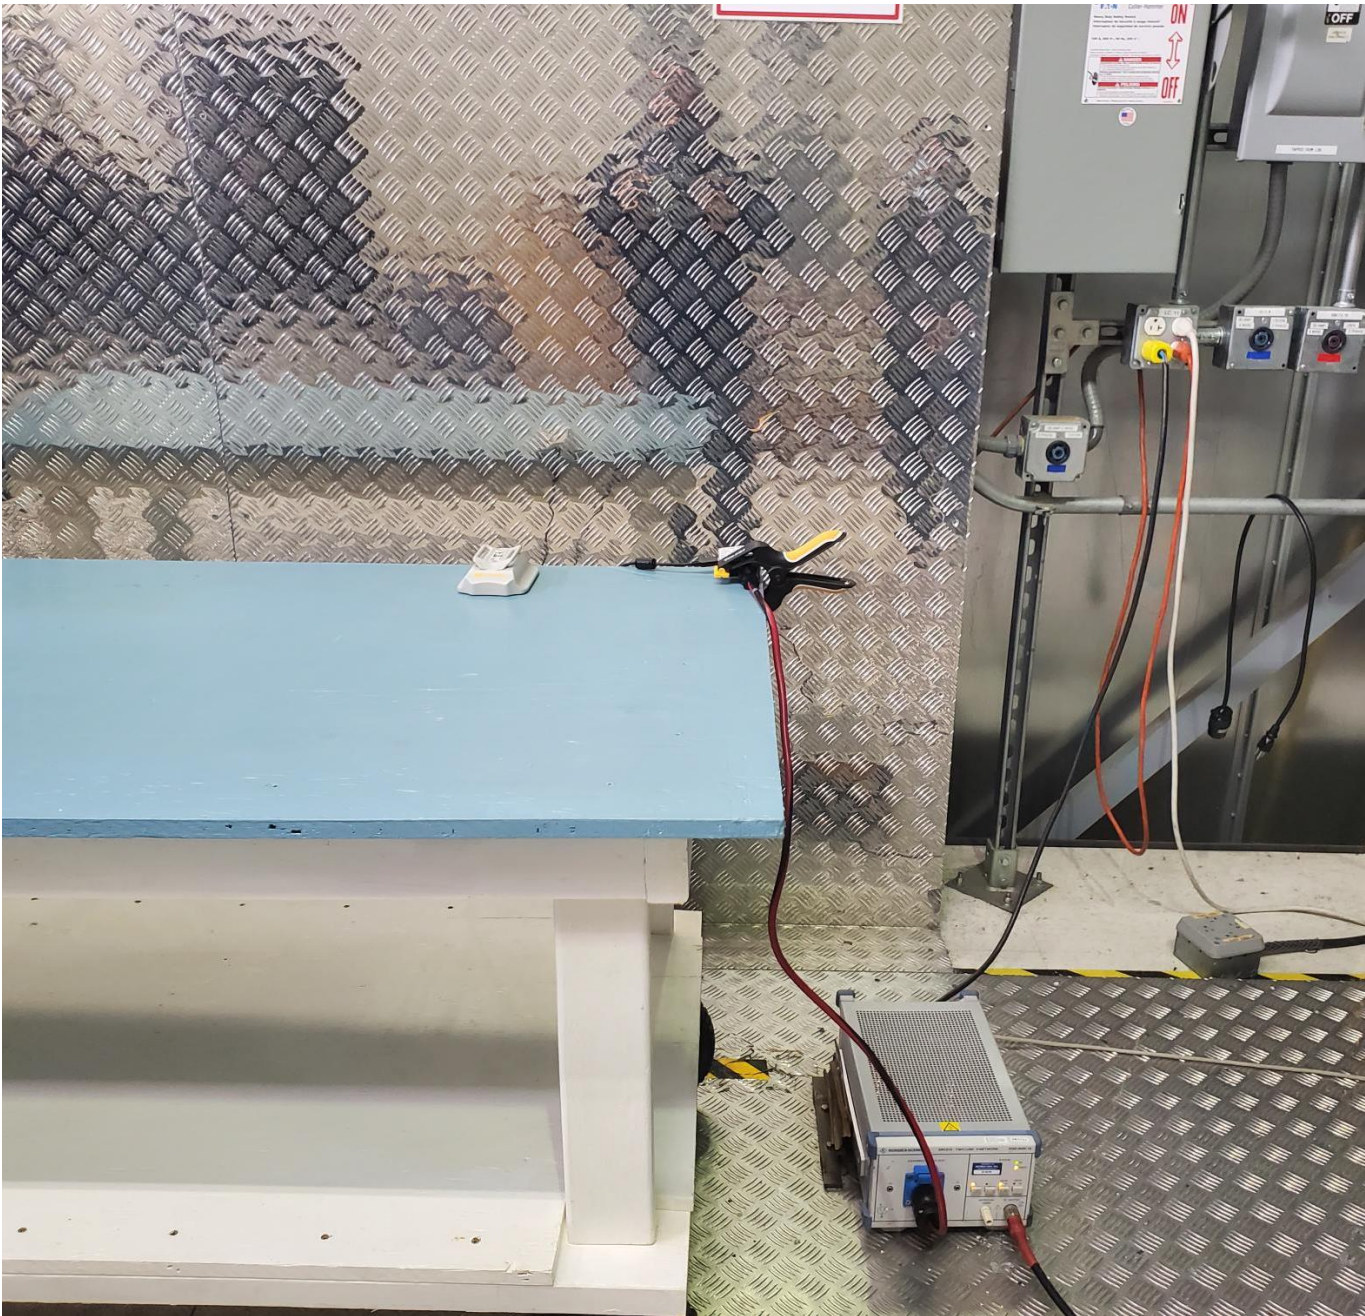


Section 1. Test Setup Photos


1.1 Conducted emissions setup

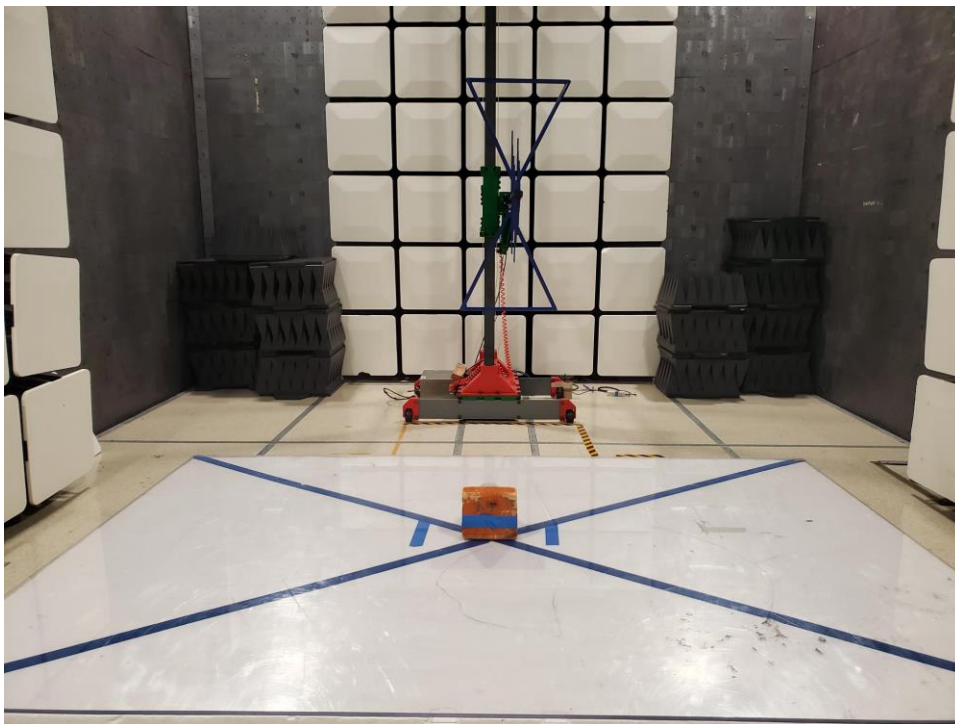

1.2 Radiated emissions 30 MHz – 1 GHz

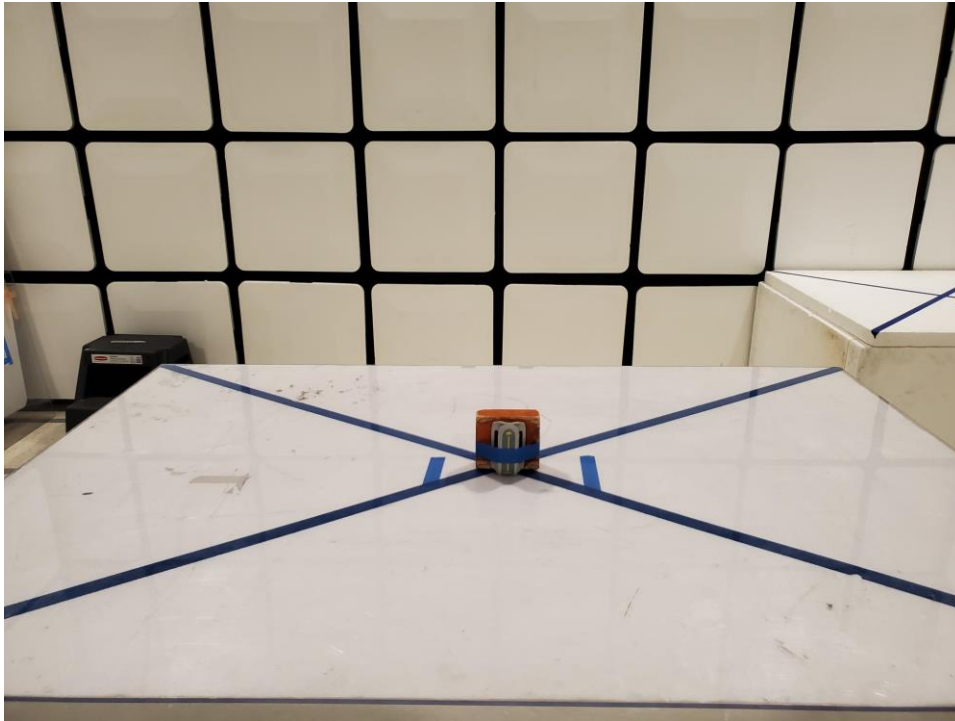

1.3 Radiated emissions 1 to 5 GHz

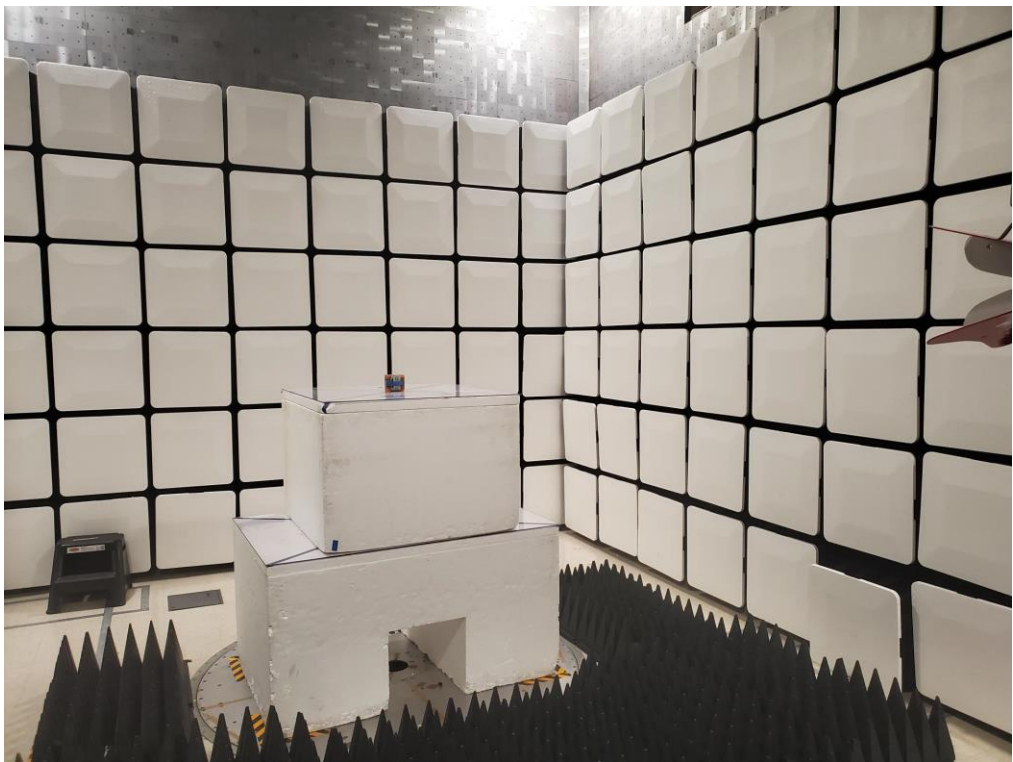

Model: Canary Medical Clinic Wearable Device, Model: 20024-0120

1.4 Wireless bench testing

