


FCC ID Label Location

- *FCC ID Label Placement Location*

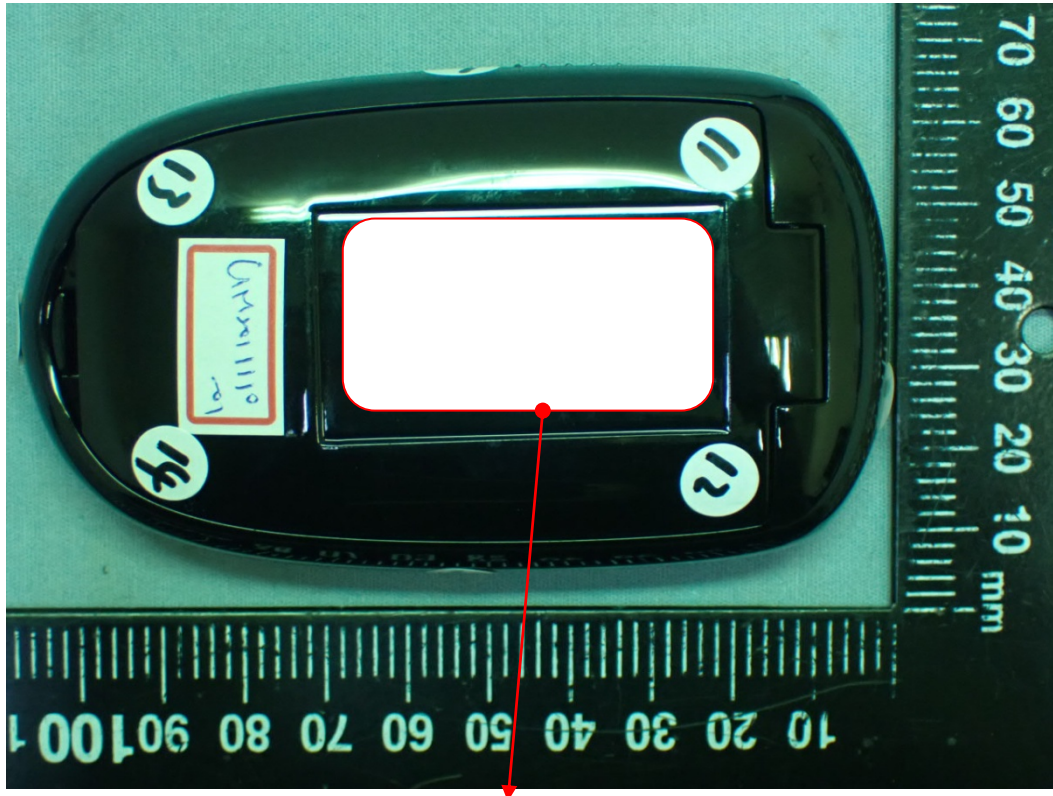

FCC ID Label Placement Location (EUT Bottom View)

- *FCC ID Label Format*

ACEZIN GLUGold
Blood Glucose Meter Model: AM100 plus
FCC ID: 2AYCBAM100PLUS
This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

 Ace Medical Technology Co., Ltd. No.52, Dinghu Rd., Gulshan Dist., Taoyuan City 33378, Taiwan
SN
P/N: M709-000000-XXX VER: 001