




Band2_1.4MHz_16QAM_18607_1RB#5



Band2_1.4MHz_QPSK_18607_6RB#0



Band2_1.4MHz_16QAM_18607_6RB#0

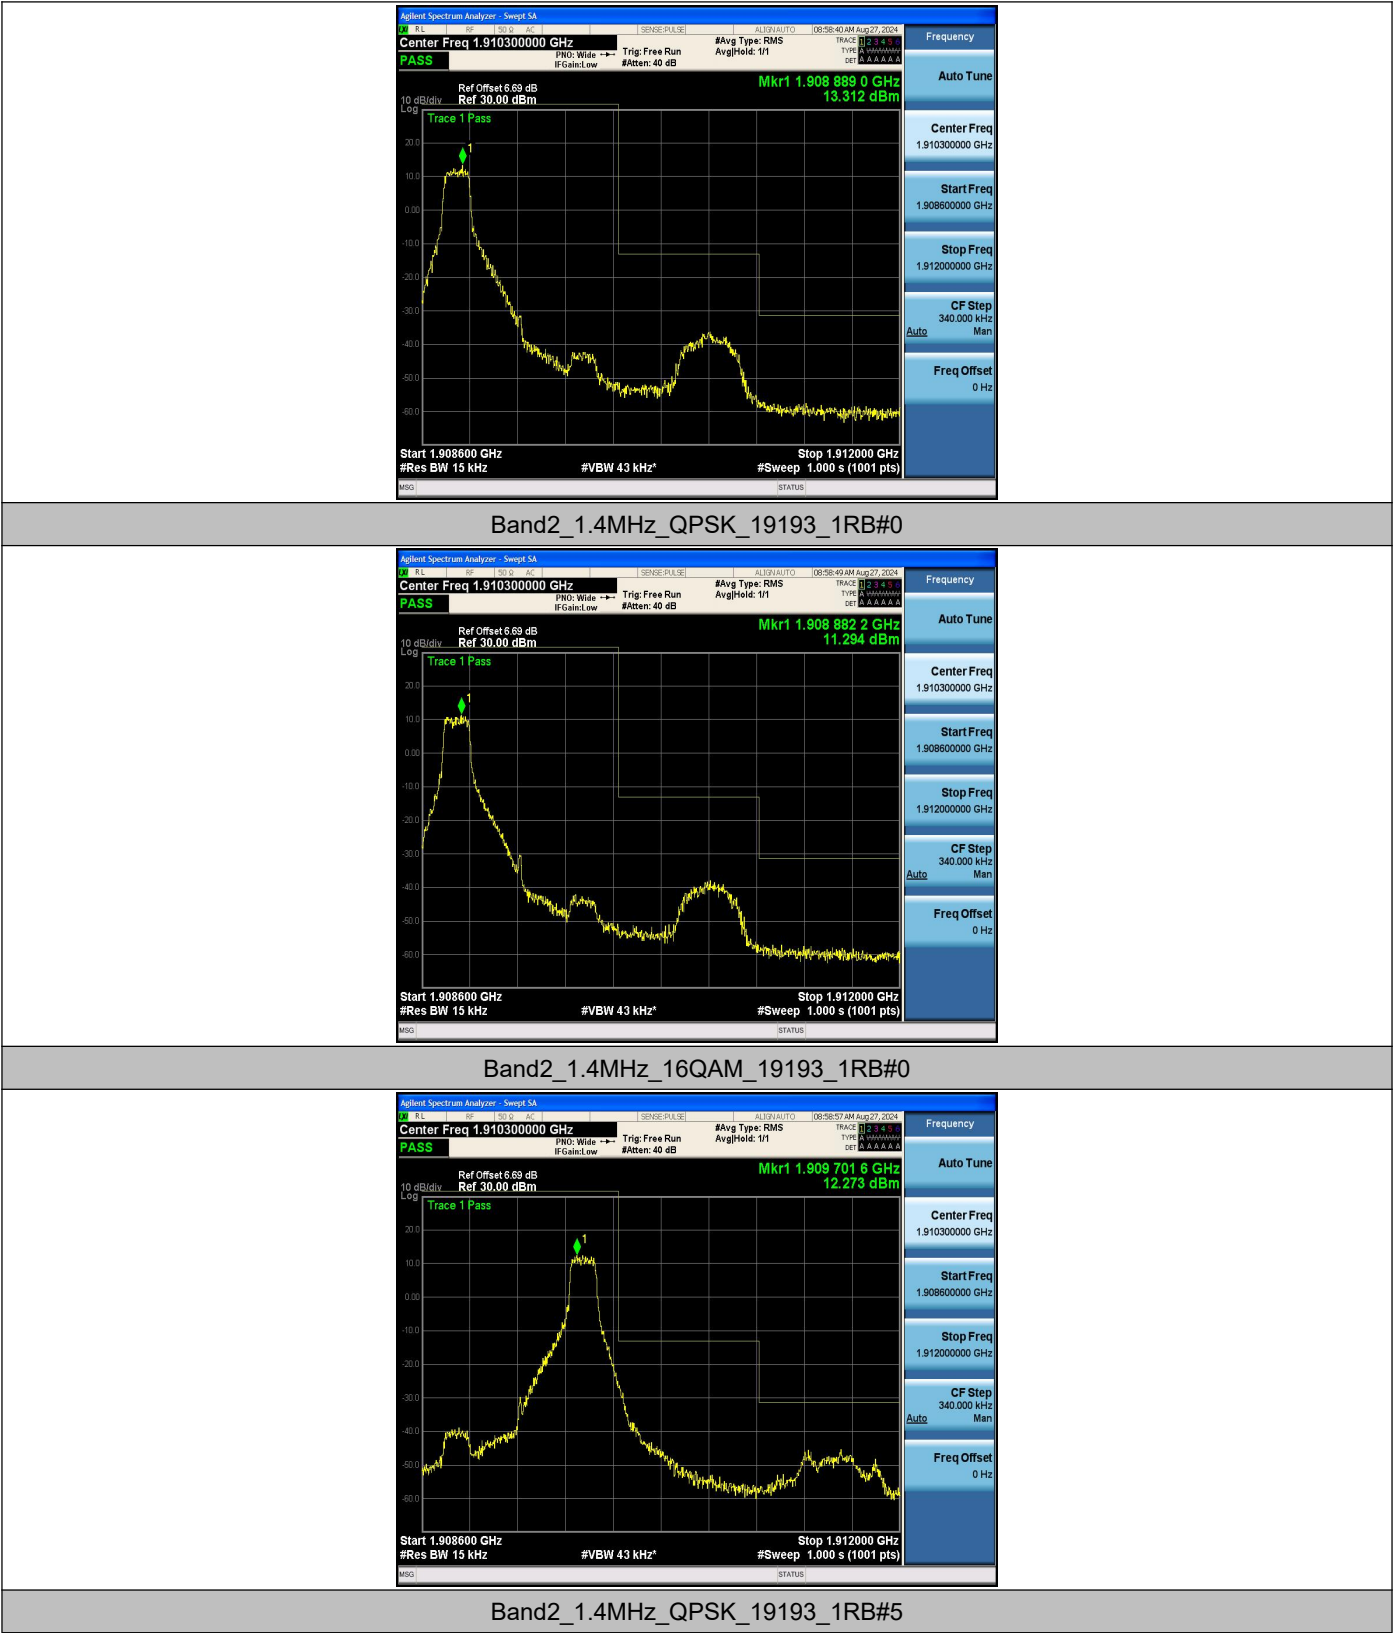

Band2_1.4MHz_16QAM_19193_1RB#0

Agilent Spectrum Analyzer - Swept SA

Center Freq 1.910300000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.908600 GHz

#Res BW 15 kHz

#VBW 43 kHz

Stop 1.912000 GHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq
1.910300000 GHz

Start Freq
1.908600000 GHz

Stop Freq
1.912000000 GHz


CF Step
340.000 kHz
Auto

Freq Offset
0 Hz

Mkr1 1.909 701 8 GHz

12.273 dBm

Band2_1.4MHz_QPSK_19193_1RB#5

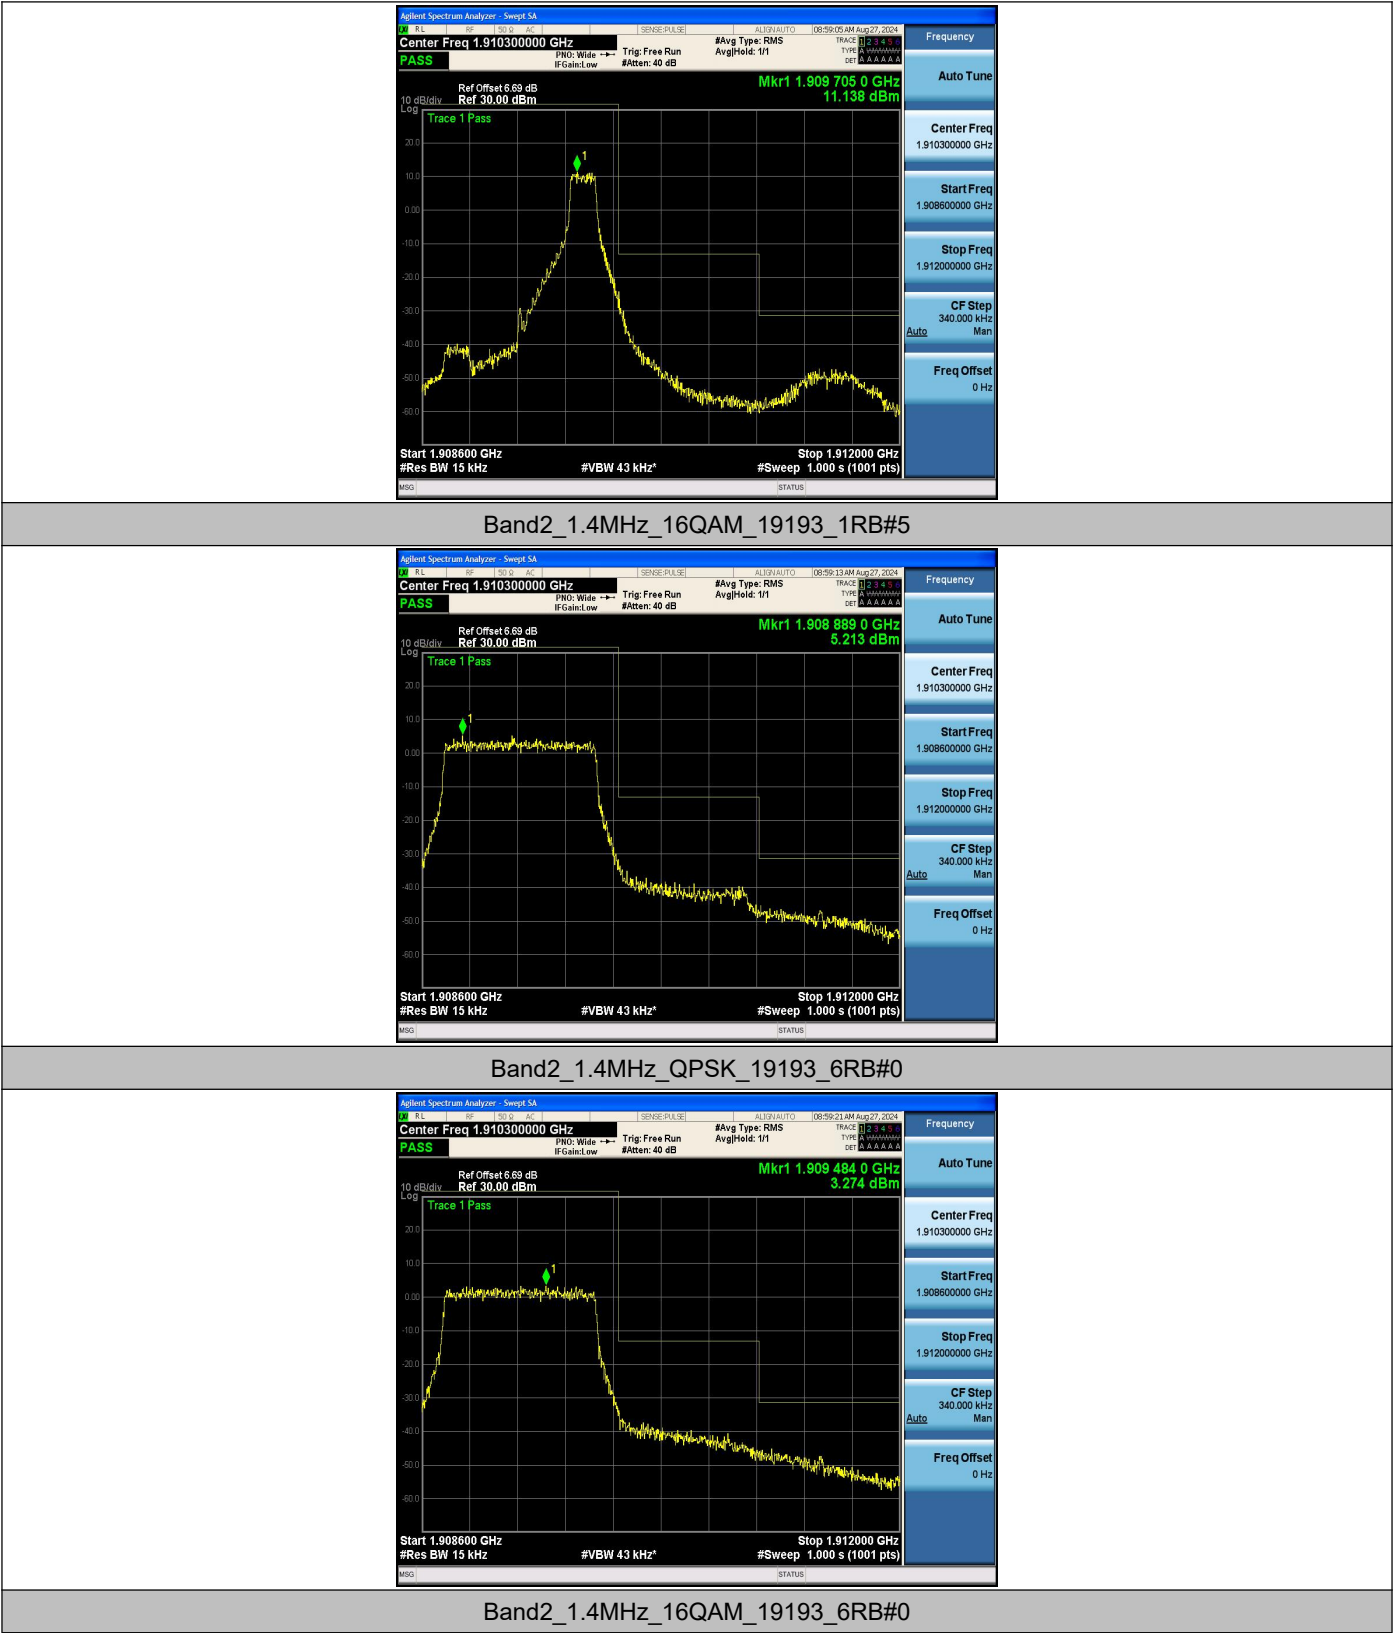

Band2_1.4MHz_QPSK_19193_6RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 1.910300000 GHz

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.908600 GHz

Stop 1.912000 GHz

Res BW 15 kHz

VBW 43 kHz

Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 1.910300000 GHz

Start Freq 1.908600000 GHz

Stop Freq 1.912000000 GHz


CF Step 340.000 kHz

Auto

Freq Offset 0 Hz

Mkr1 1.909 484 0 GHz


3.274 dBm

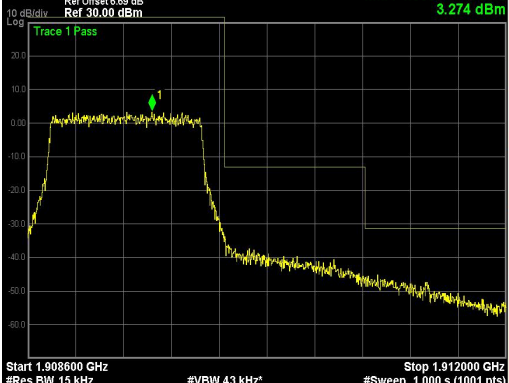

Band2_1.4MHz_16QAM_19193_6RB#0




Band2_3MHz_QPSK_18615_1RB#0

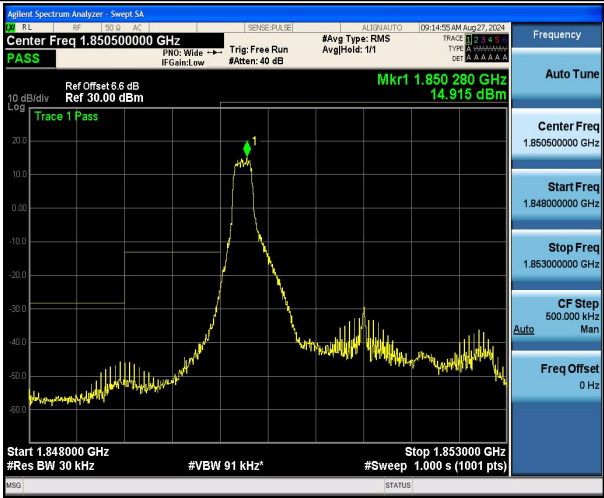


Band2_3MHz_16QAM_18615_1RB#0



Band2_3MHz_QPSK_18615_1RB#14

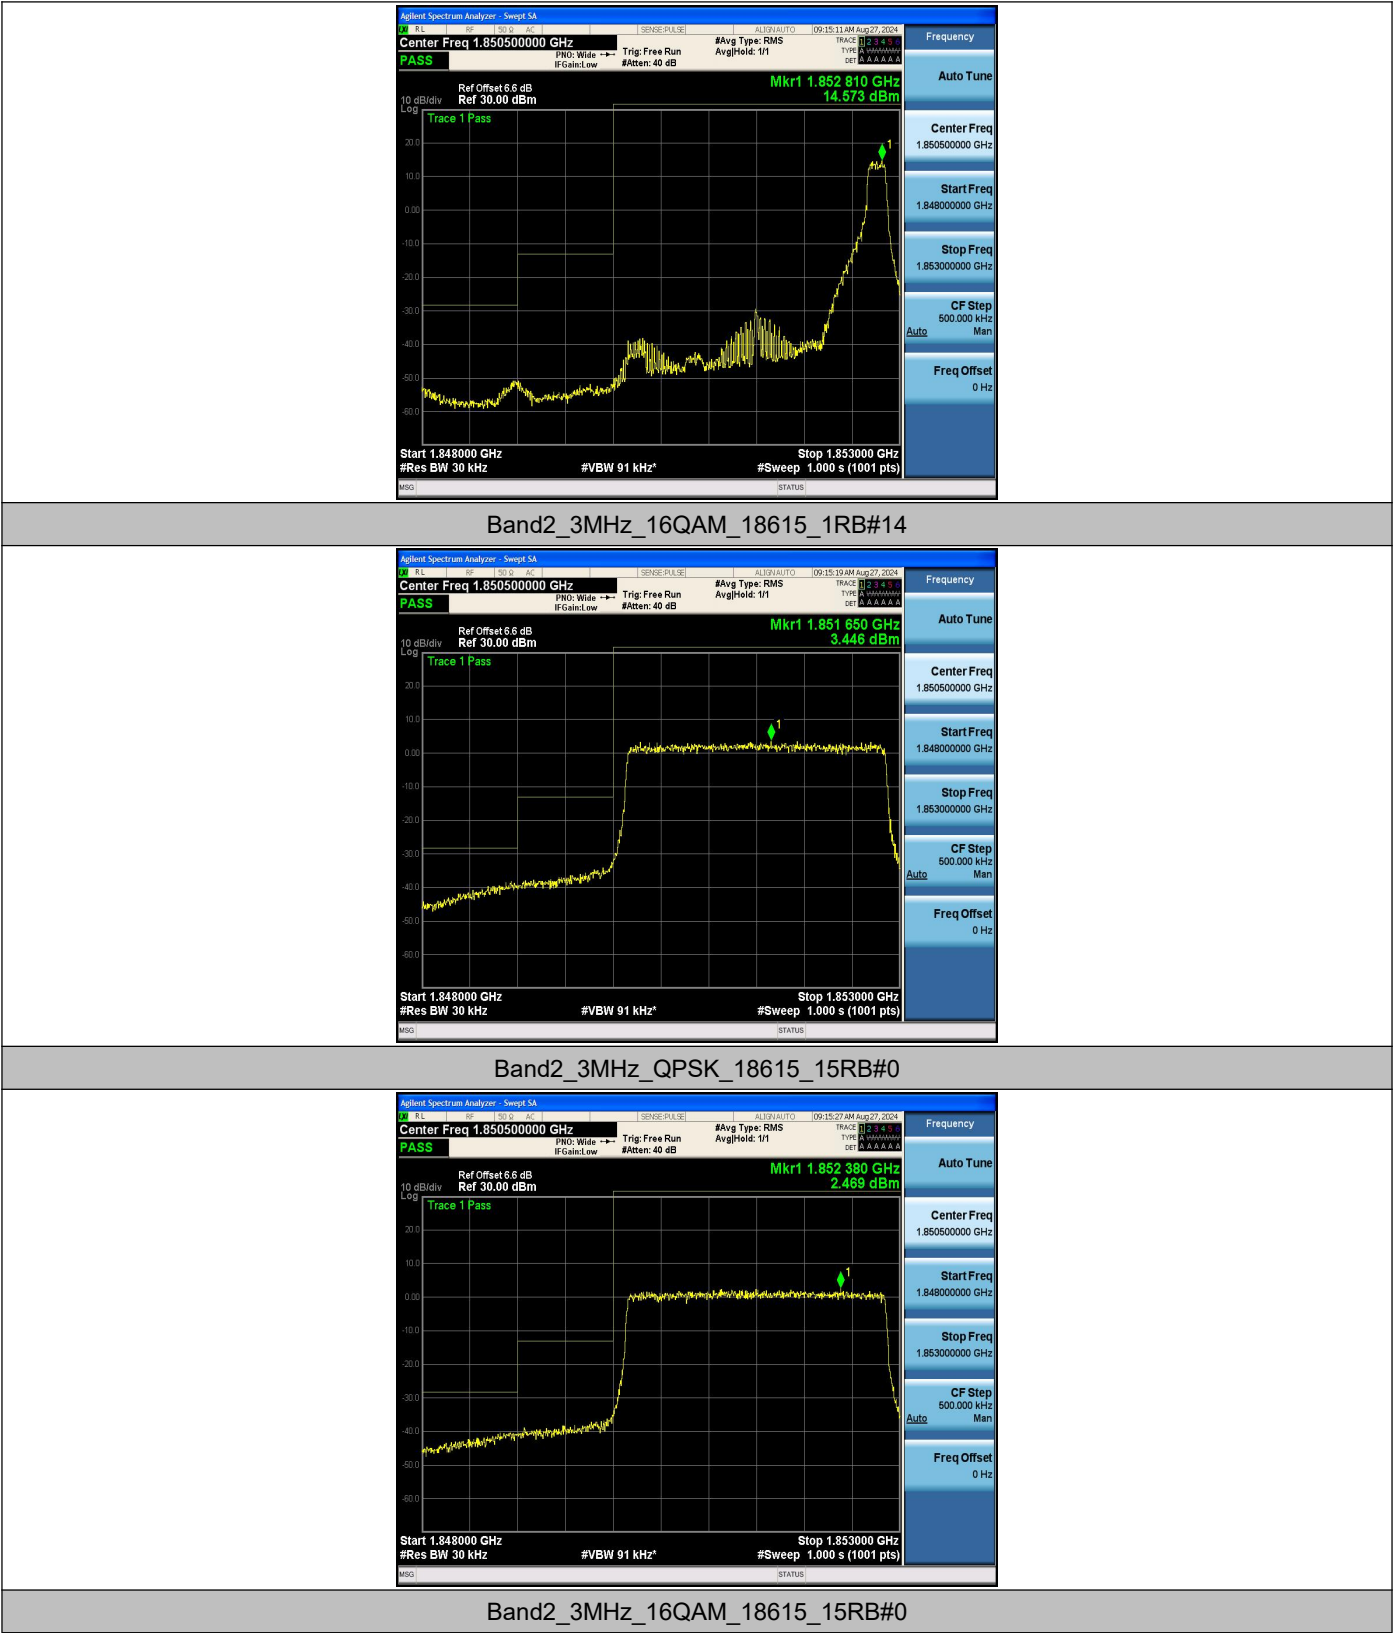

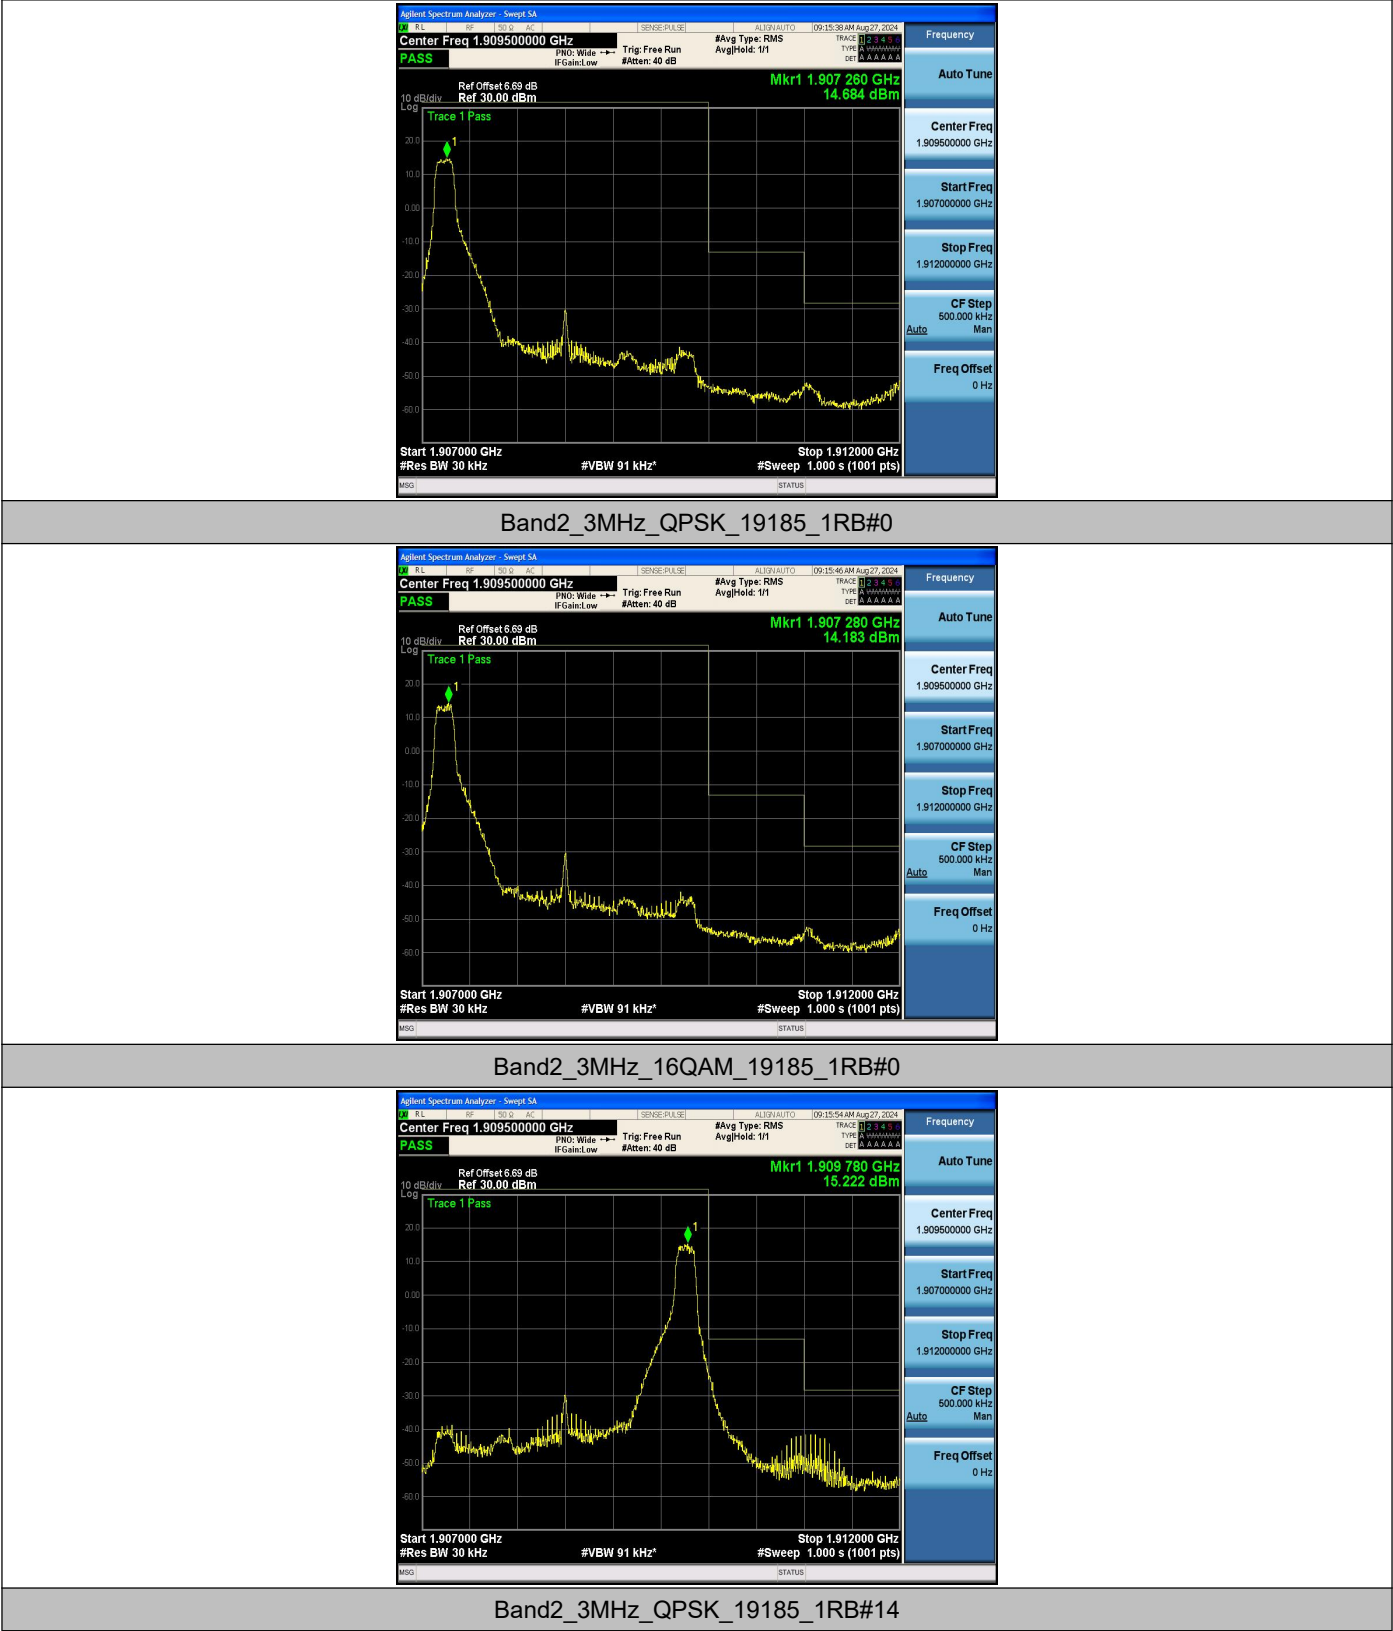

Band2_3MHz_QPSK_19185_1RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 1.909500000 GHz

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.907000 GHz

Stop 1.912000 GHz

Res BW 30 kHz

VBW 91 kHz

Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 1.909500000 GHz

Start Freq 1.907000000 GHz

Stop Freq 1.912000000 GHz


CF Step 500.000 kHz

Auto


Freq Offset 0 Hz


15.222 dBm


Mkr1 1.909 780 GHz

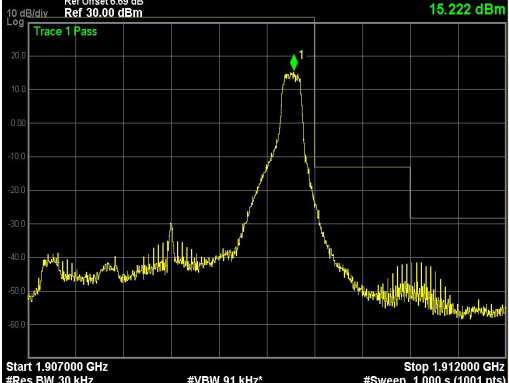

Band2_3MHz_QPSK_19185_1RB#14

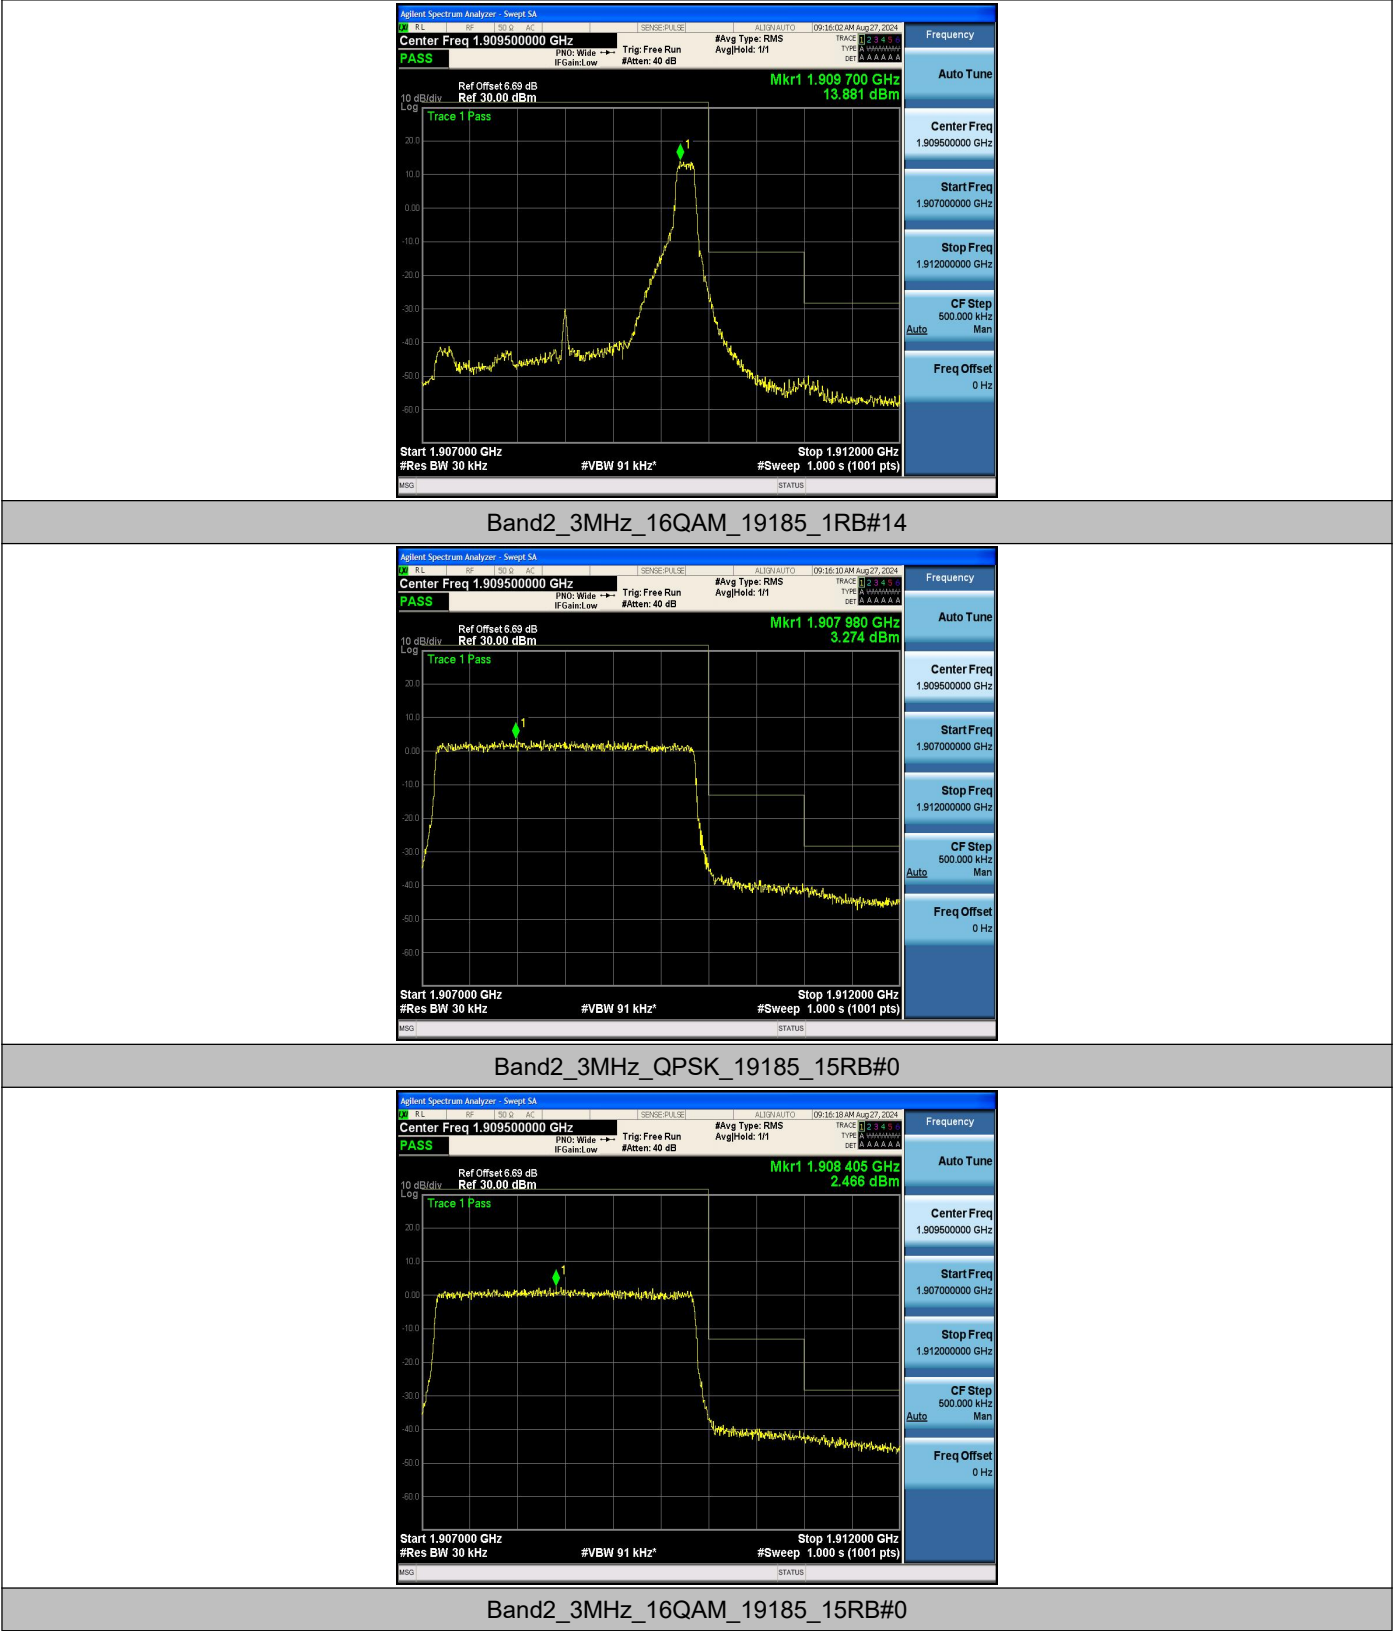

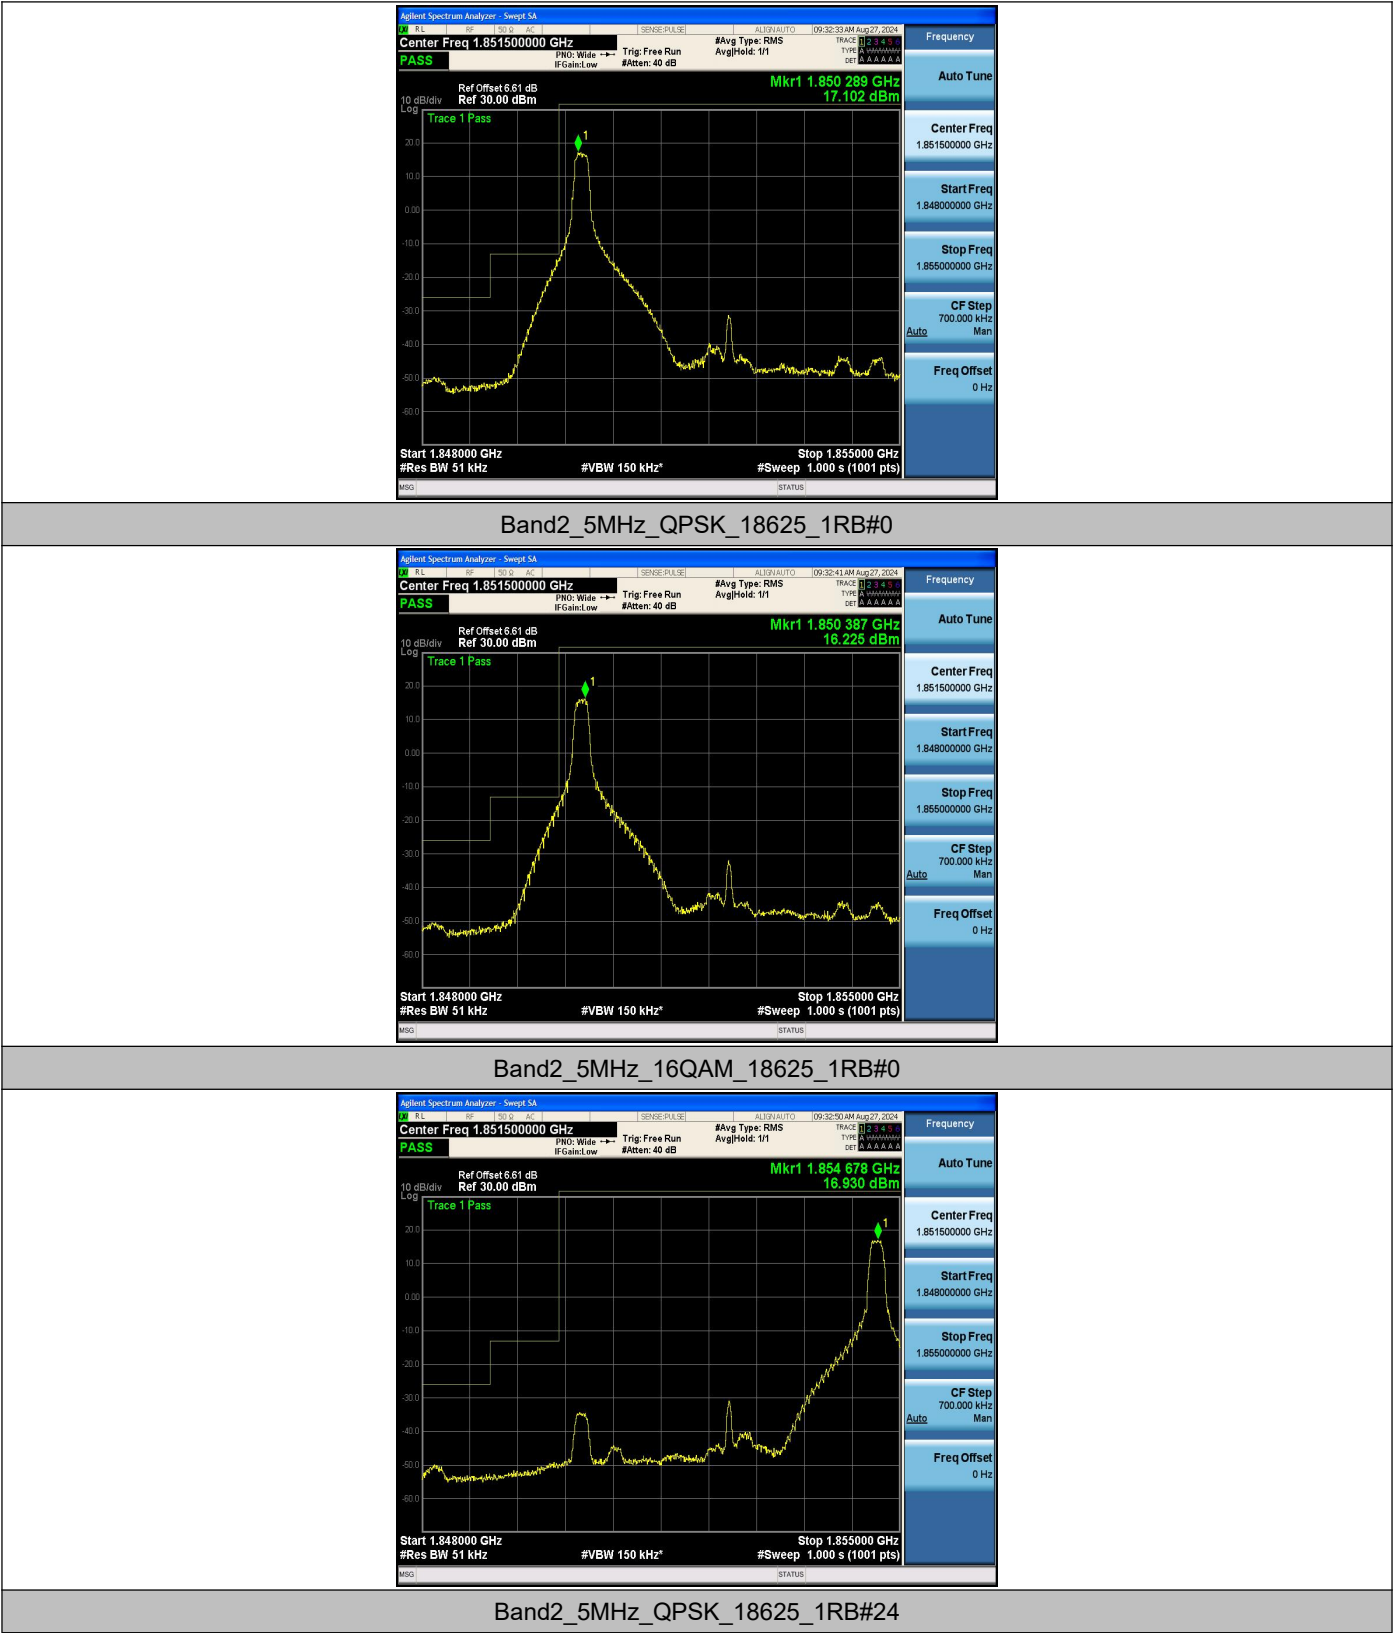

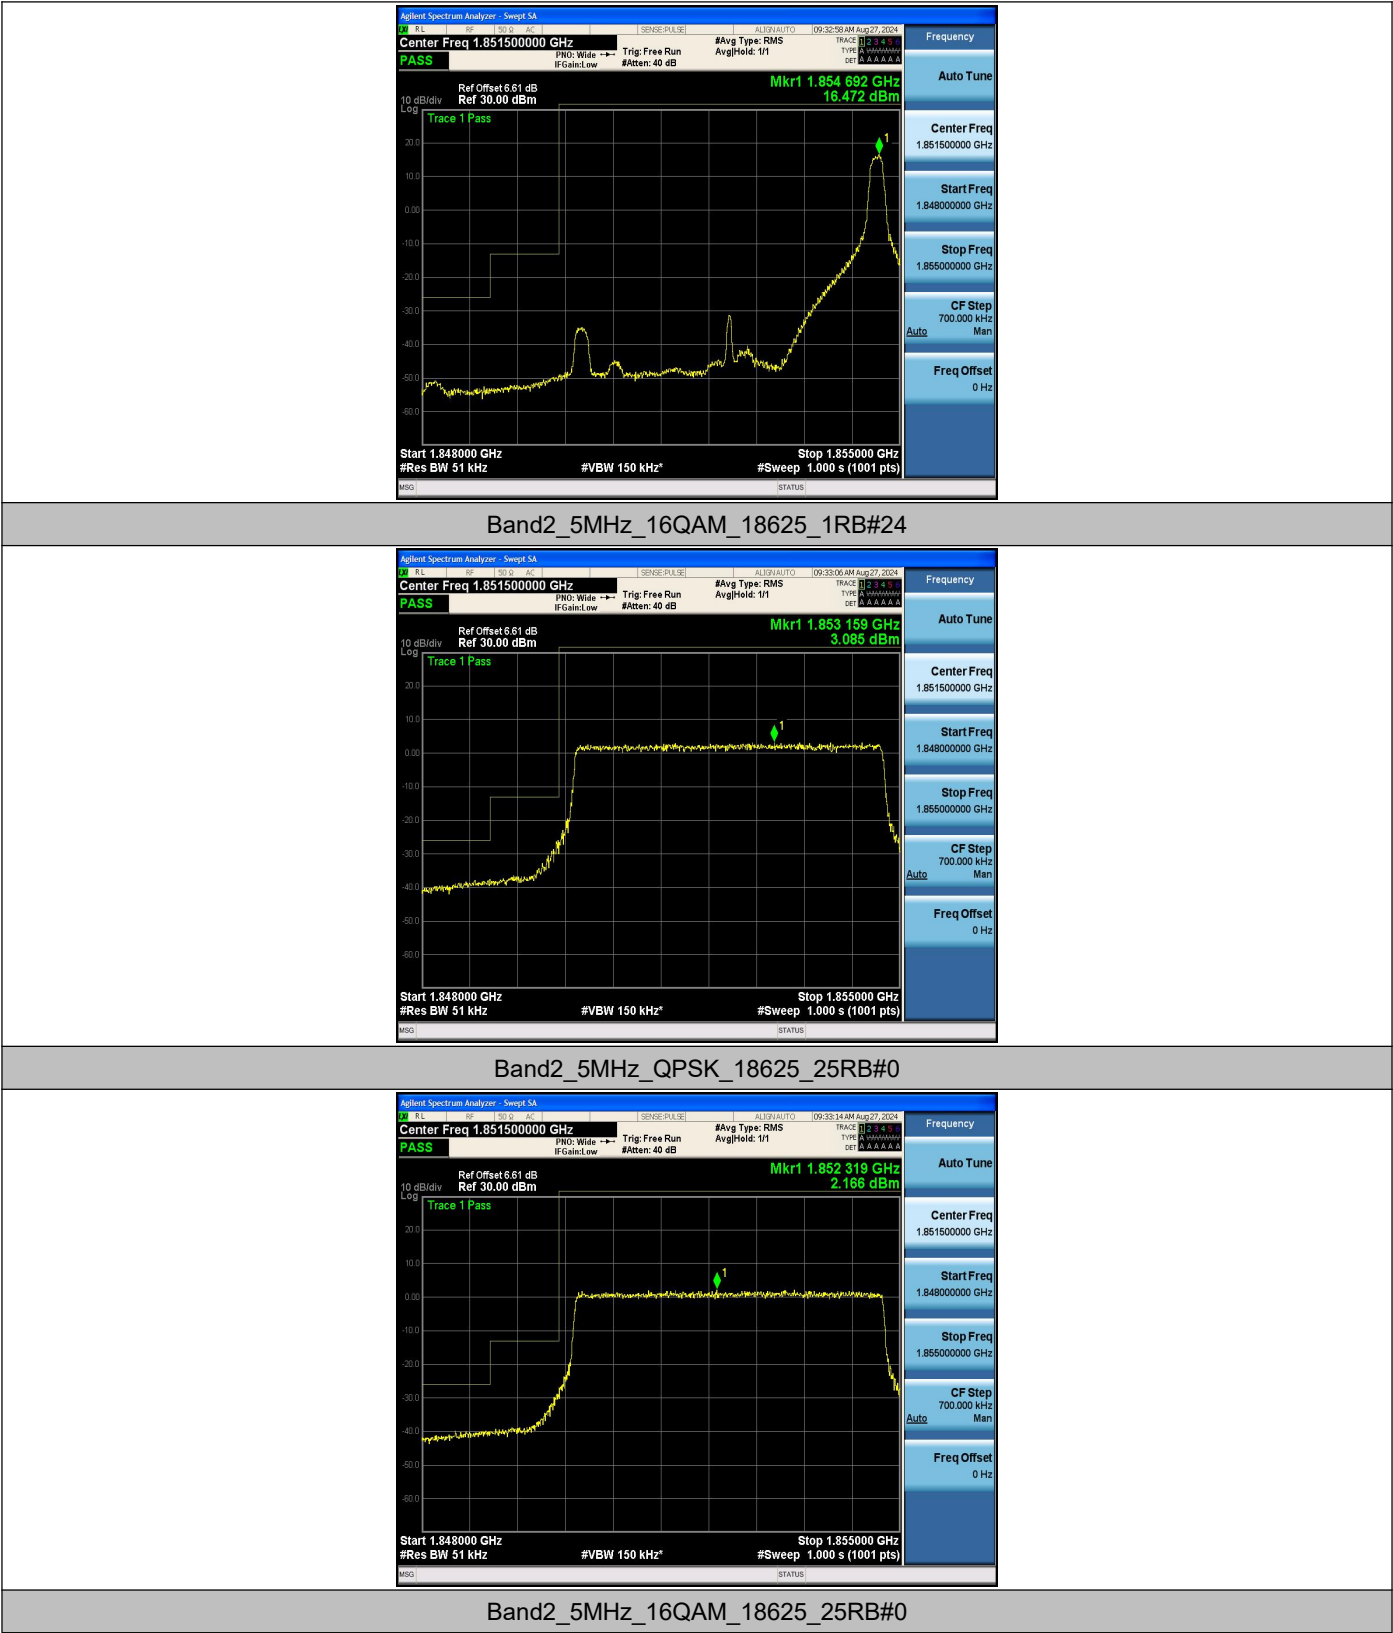



Band2_5MHz_QPSK_19175_1RB#0




Band2_5MHz_16QAM_19175_1RB#0



Band2_5MHz_QPSK_19175_1RB#24




Band2_5MHz_16QAM_19175_1RB#24

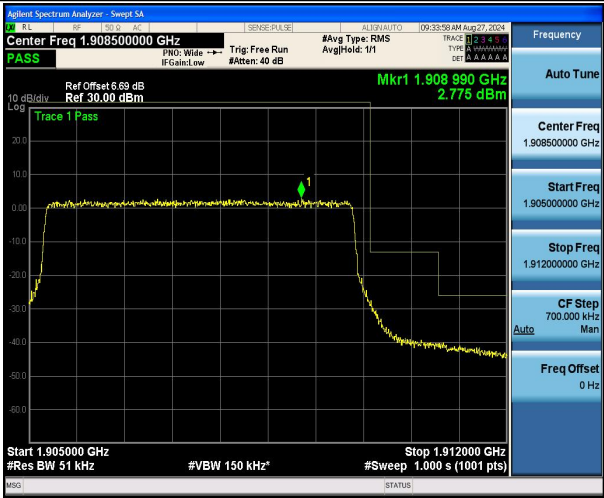



Band2_5MHz_QPSK_19175_25RB#0



Band2_5MHz_16QAM_19175_25RB#0

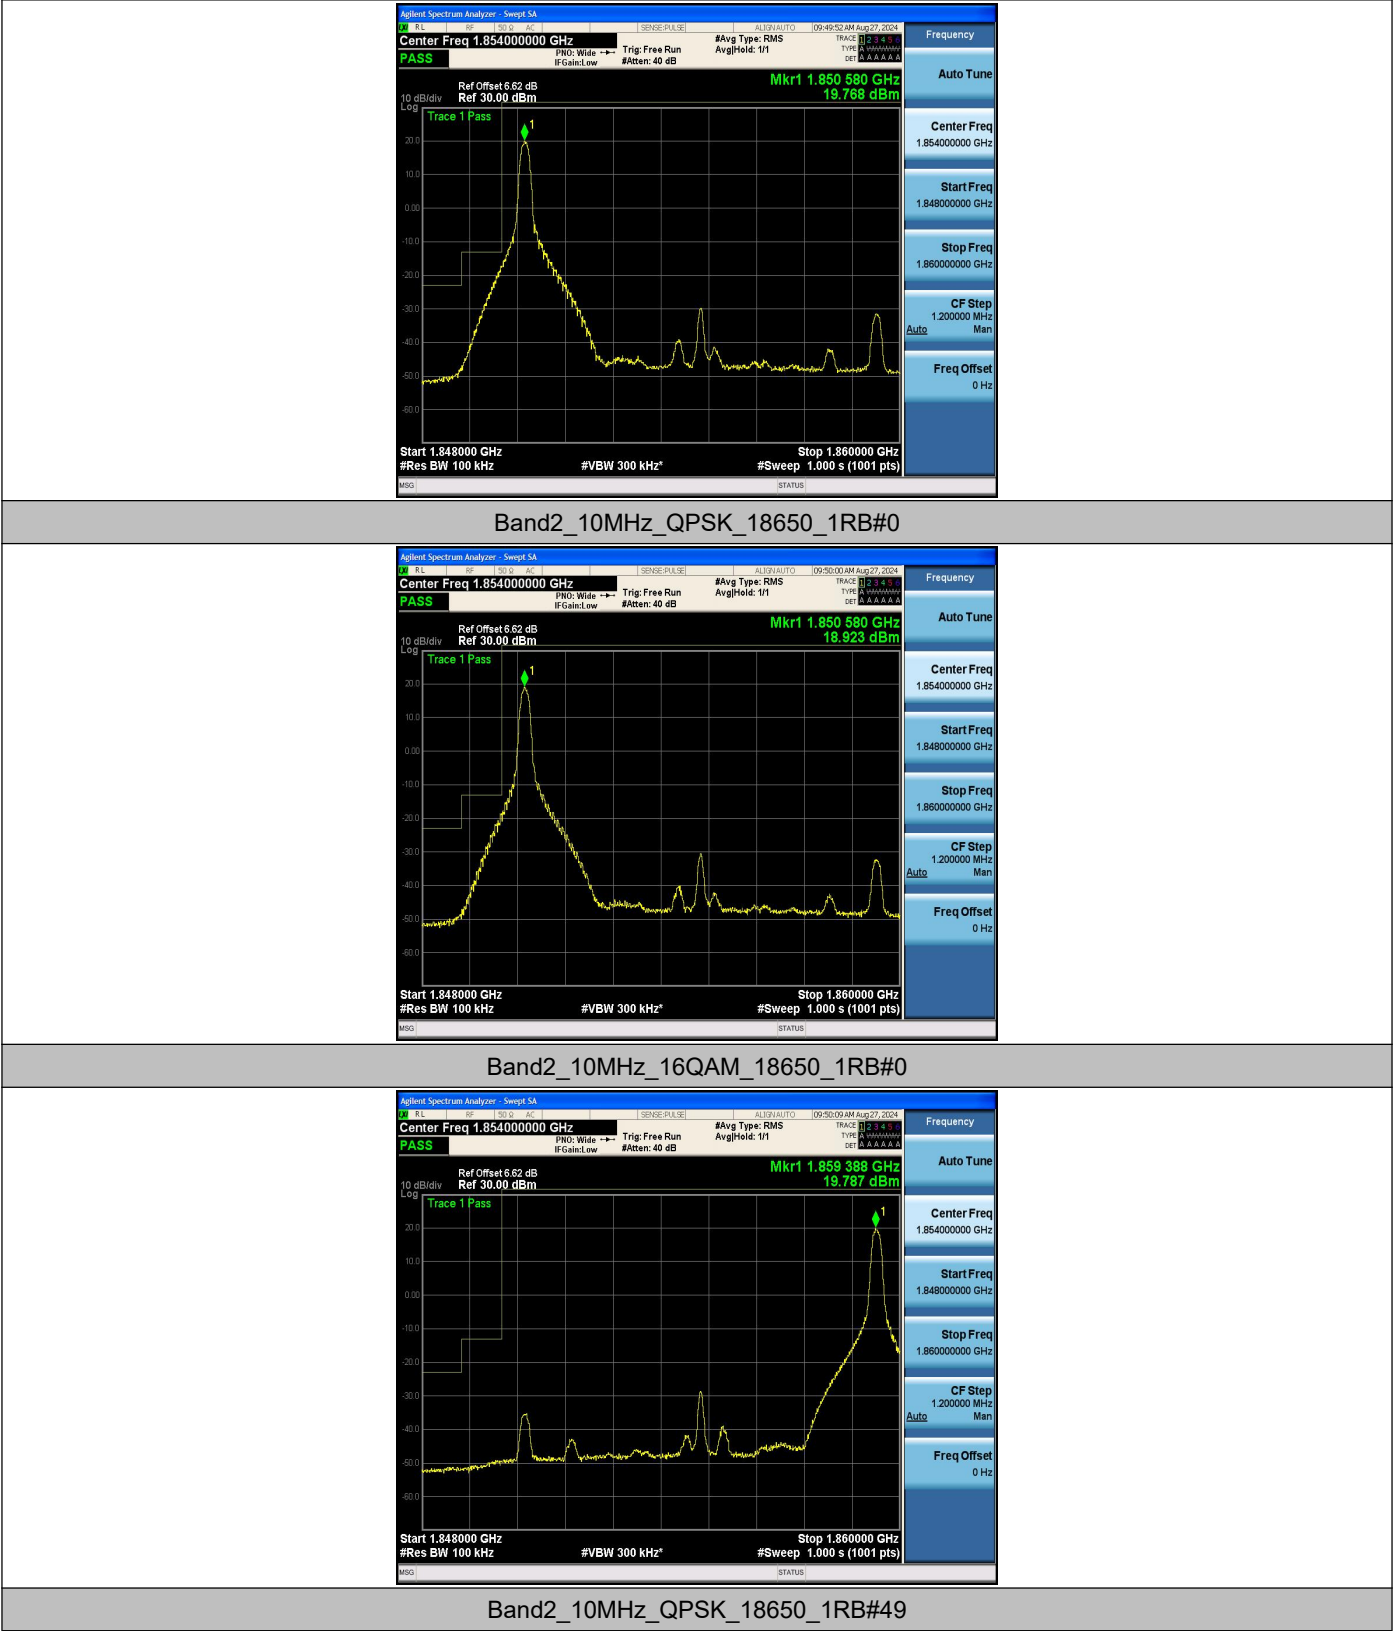

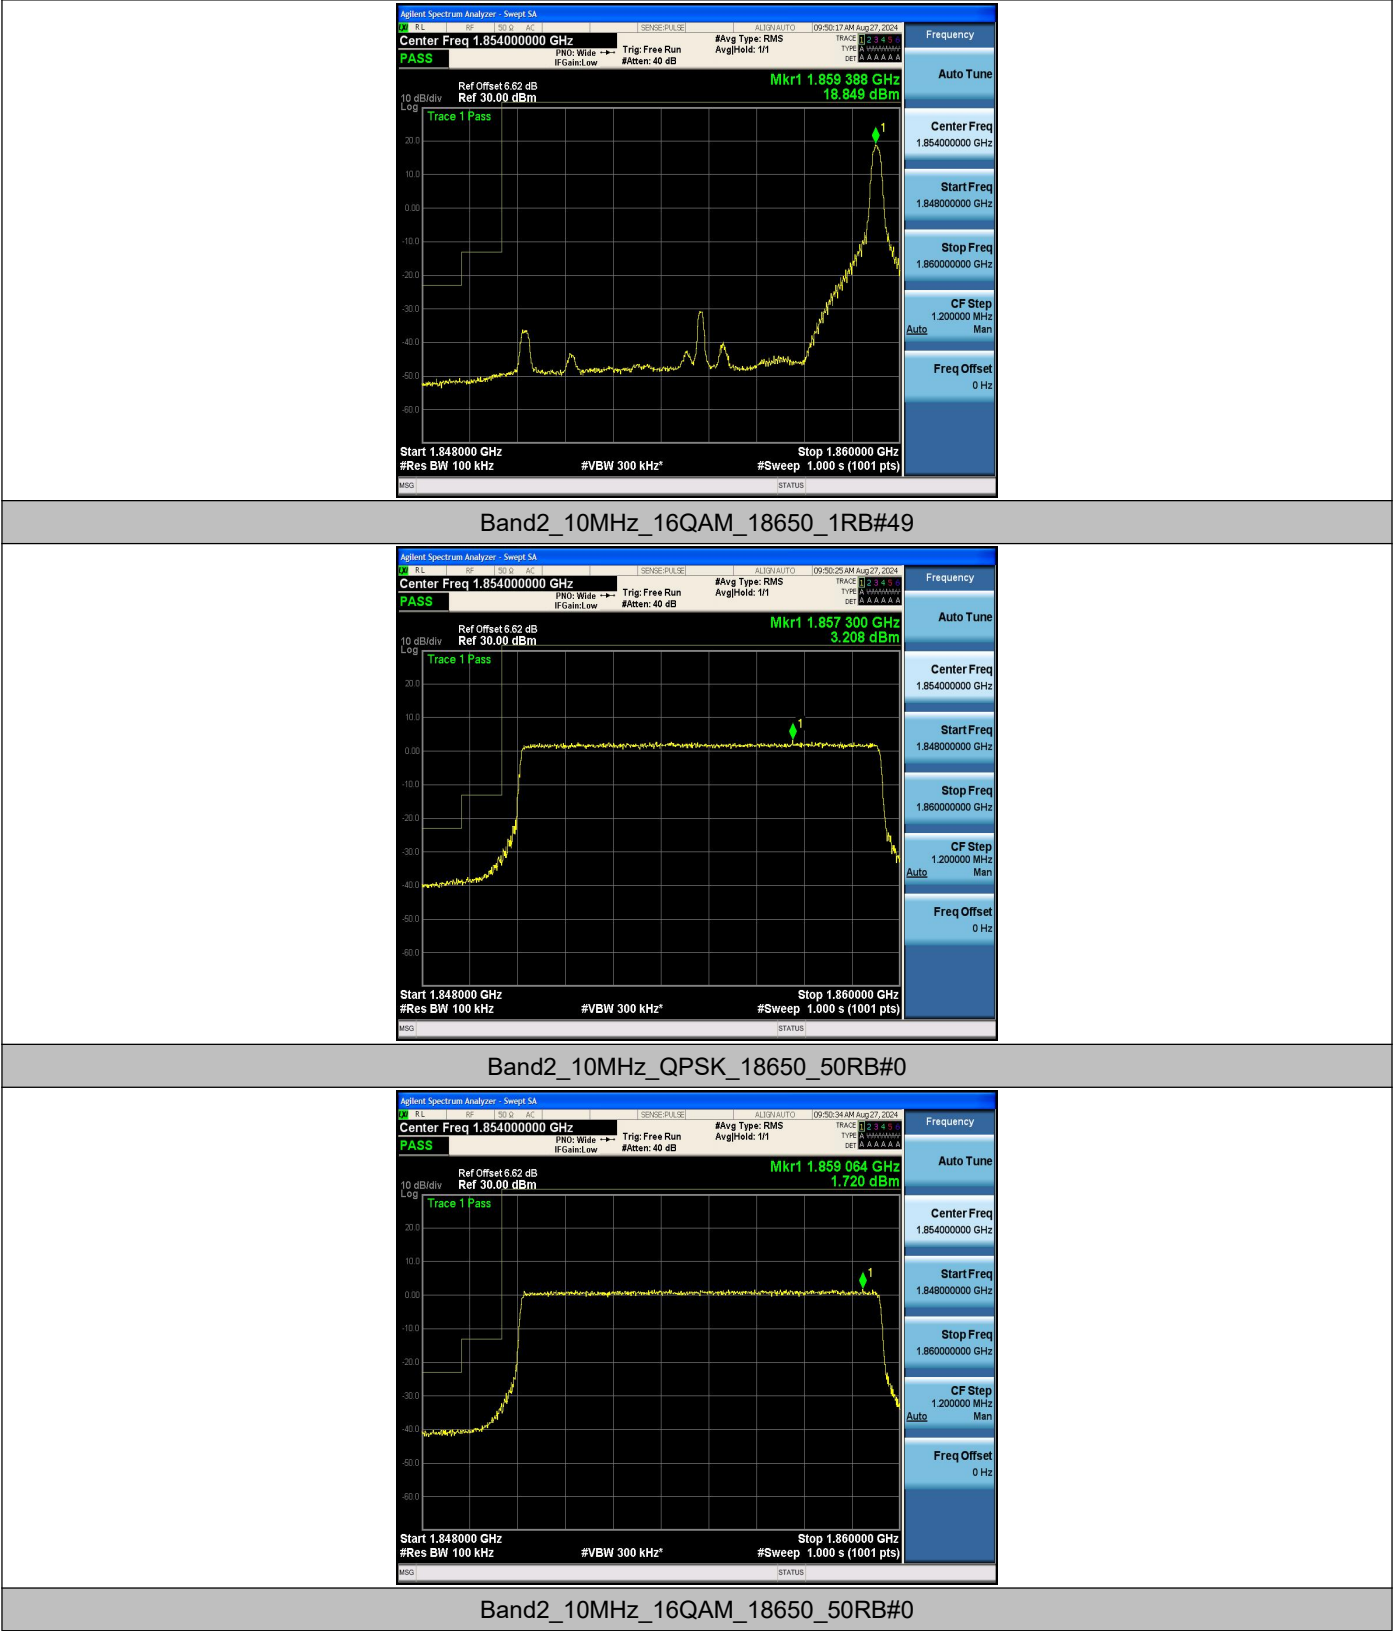

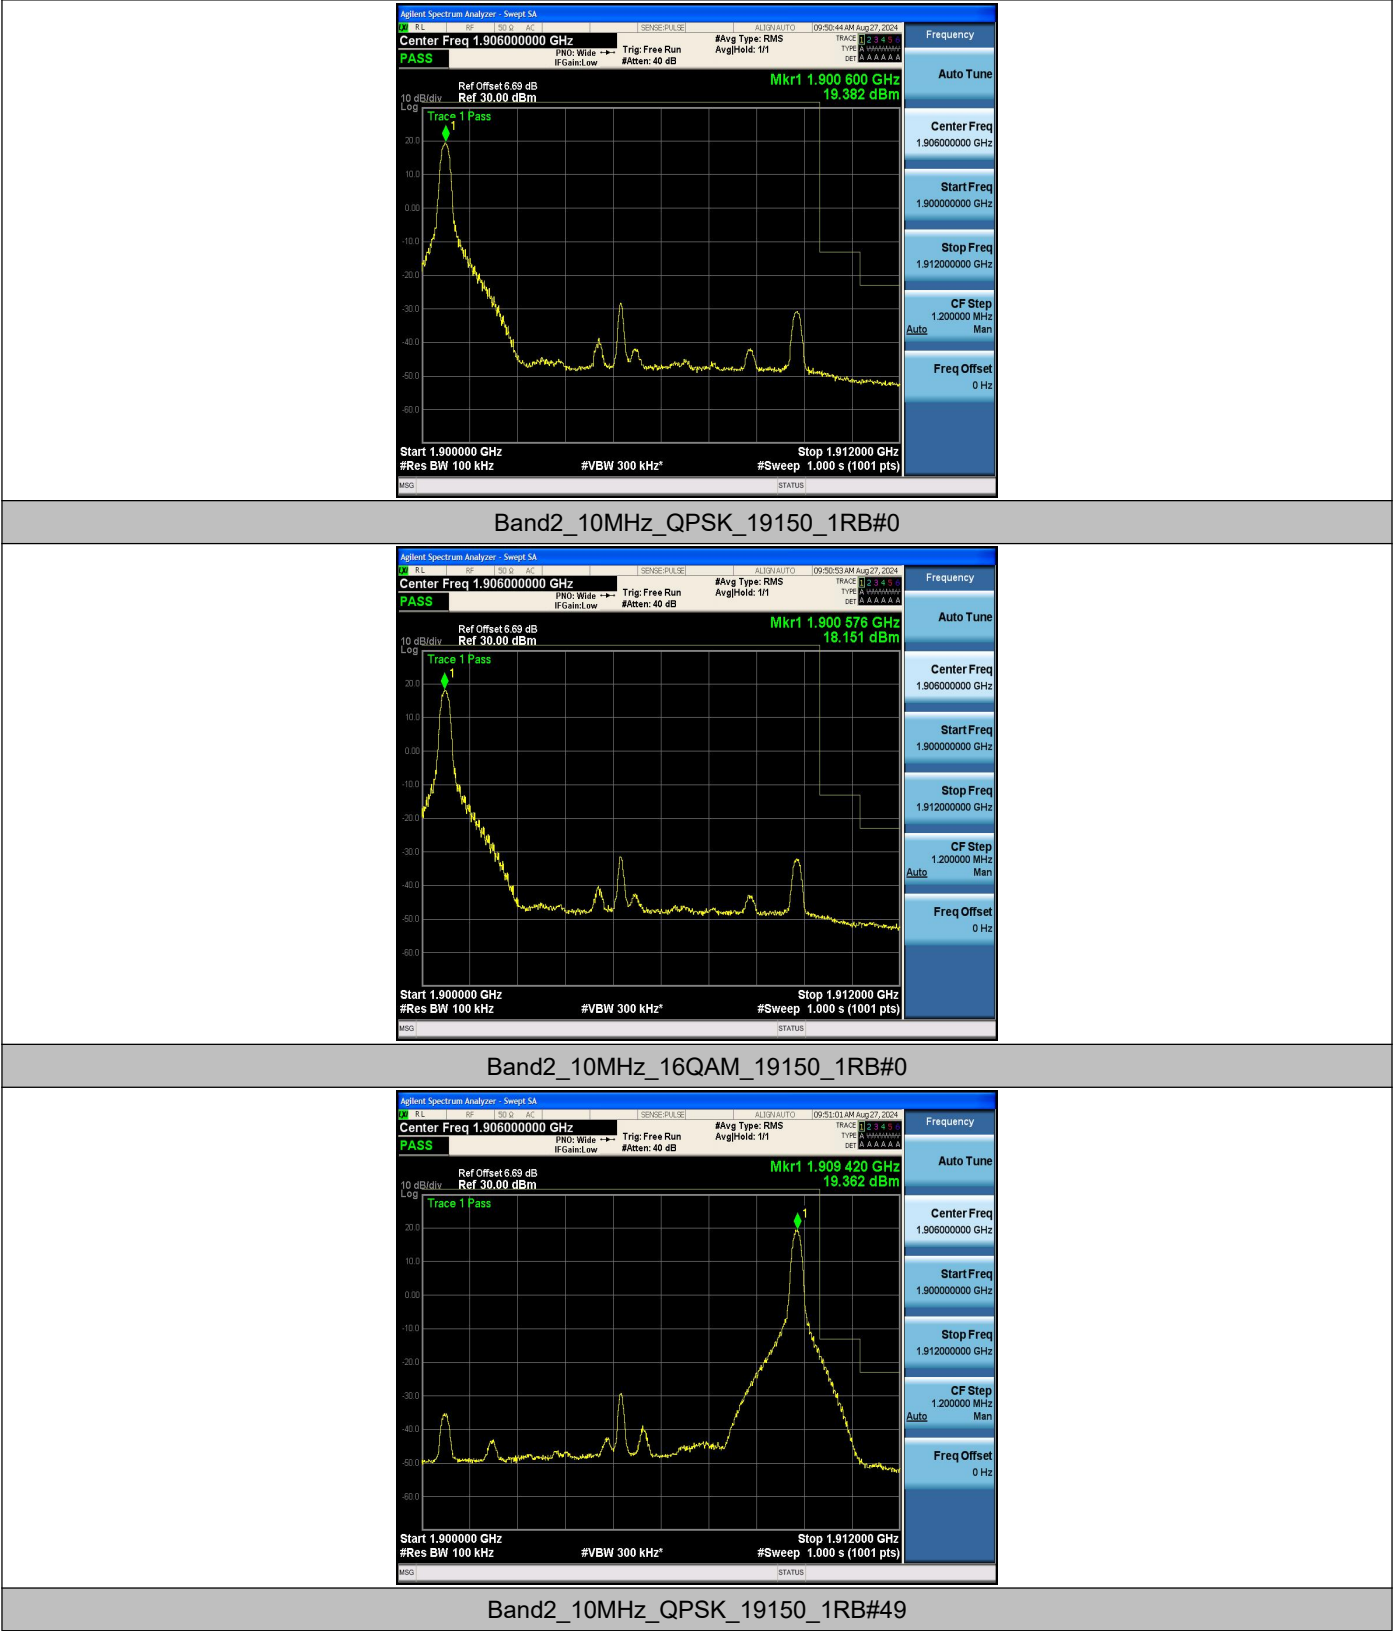

Band2_10MHz_16QAM_19150_1RB#0

Agilent Spectrum Analyzer - Swept SA

Center Freq 1.906000000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.900000 GHz

Stop 1.912000 GHz

#Res BW 100 kHz

#VBW 300 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 1.906000000 GHz

Start Freq 1.900000000 GHz

Stop Freq 1.912000000 GHz


CF Step 1.200000 MHz

Auto


Freq Offset 0 Hz

Mkr1 1.908 420 GHz

19.362 dBm

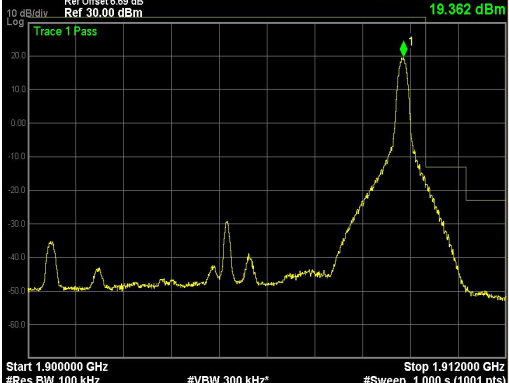

Band2_10MHz_QPSK_19150_1RB#49

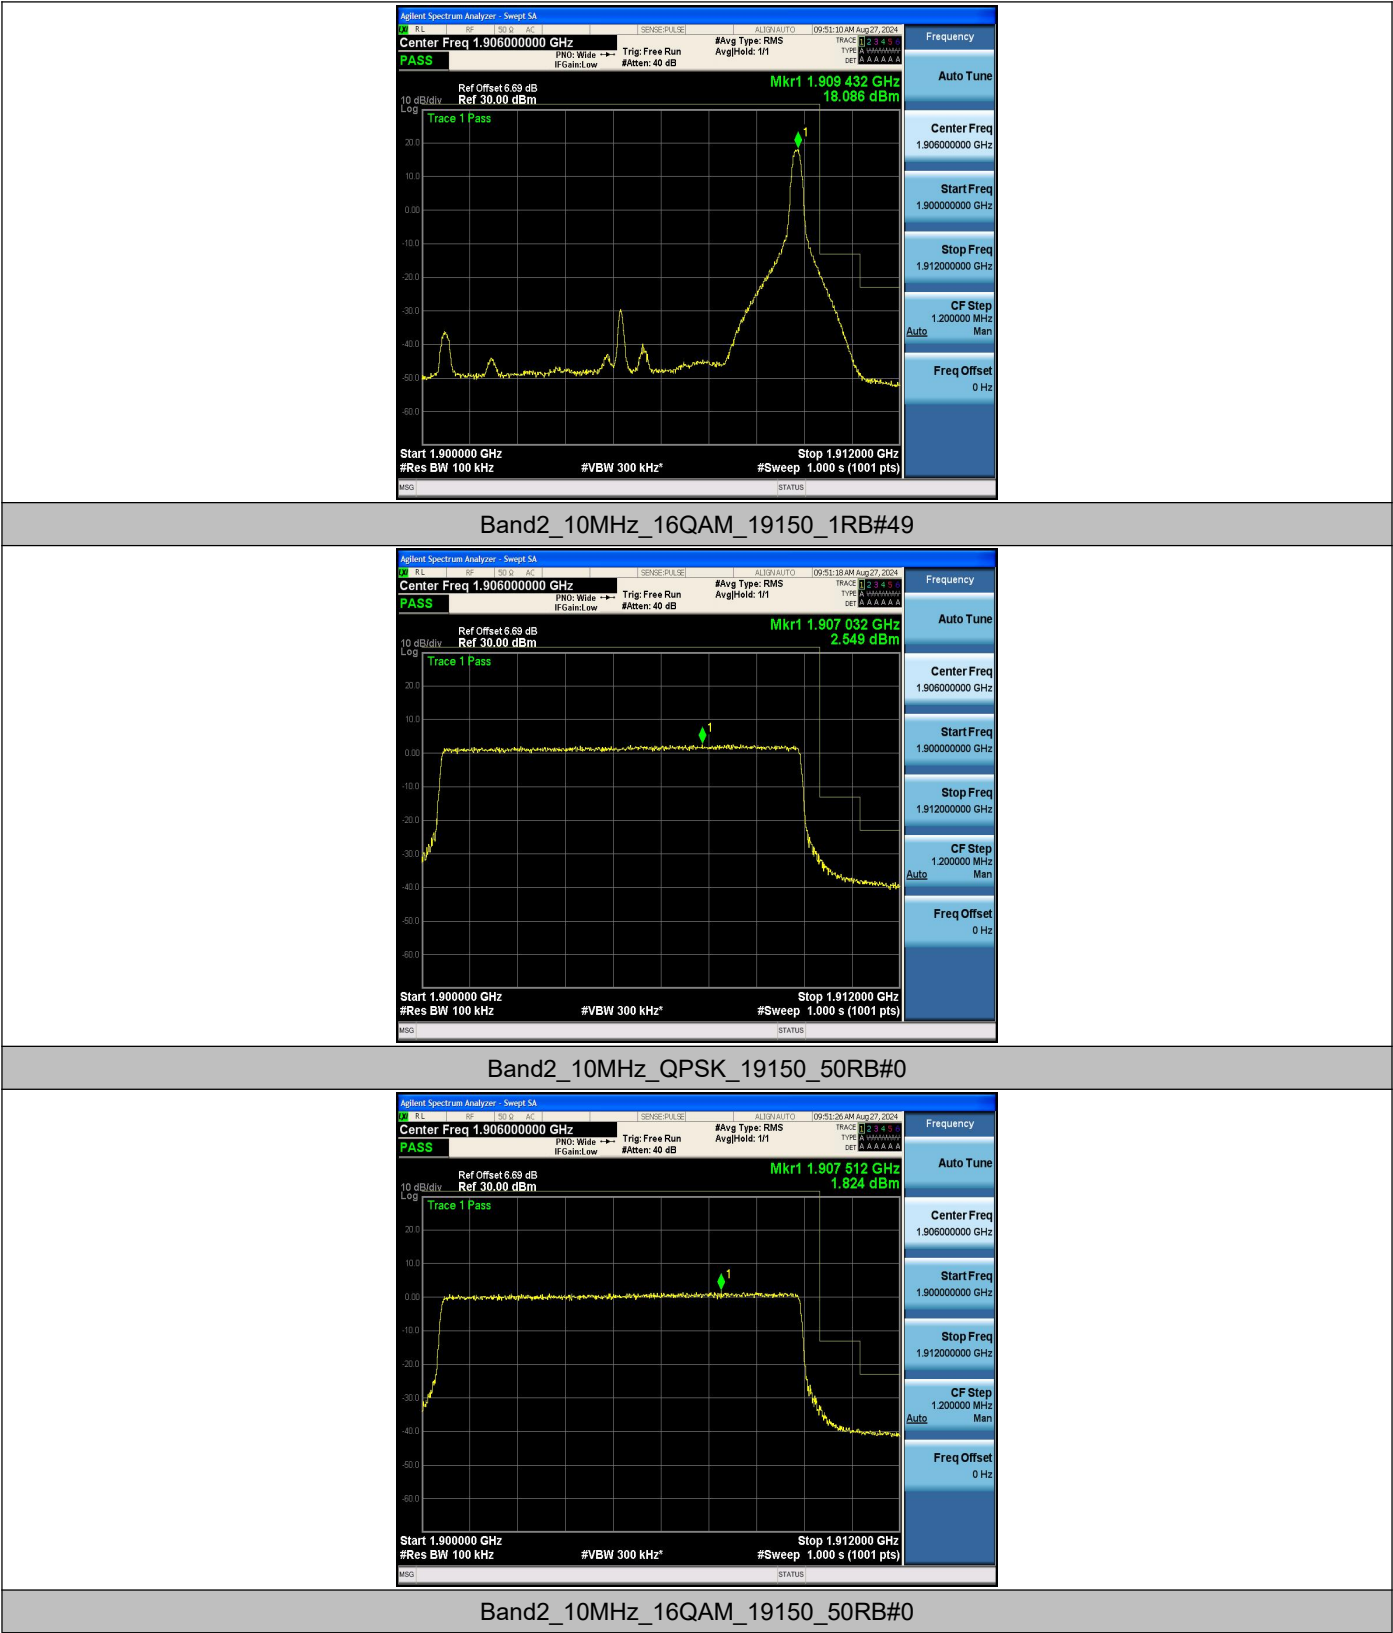

Band2_10MHz_QPSK_19150_50RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 1.906000000 GHz

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.900000 GHz

Stop 1.912000 GHz

#Res BW 100 kHz

#VBW 300 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 1.906000000 GHz

Start Freq 1.900000000 GHz

Stop Freq 1.912000000 GHz


CF Step 1.200000 MHz

Auto

Freq Offset 0 Hz

Mkr1 1.907 512 GHz

1.824 dBm

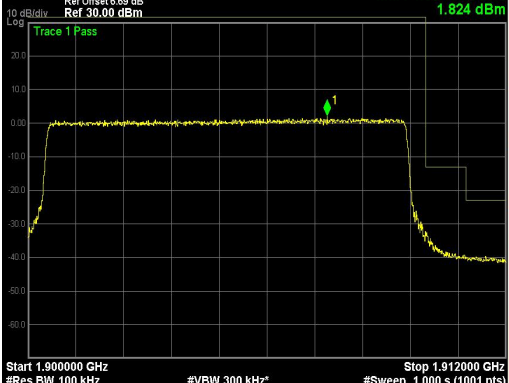

Band2_10MHz_16QAM_19150_50RB#0