

Date: 2026-03-17

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 38.5$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 12.6 W/kg; SAR (10g) = 6.11 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.13 dB
SAR (1g) = 12.8 W/kg; SAR (10g) = 6.06 W/kg
Smallest distance from peaks to all points 3 dB below = 8.8 mm
Ratio of SAR at M2 to SAR at M1 = 76.3 %

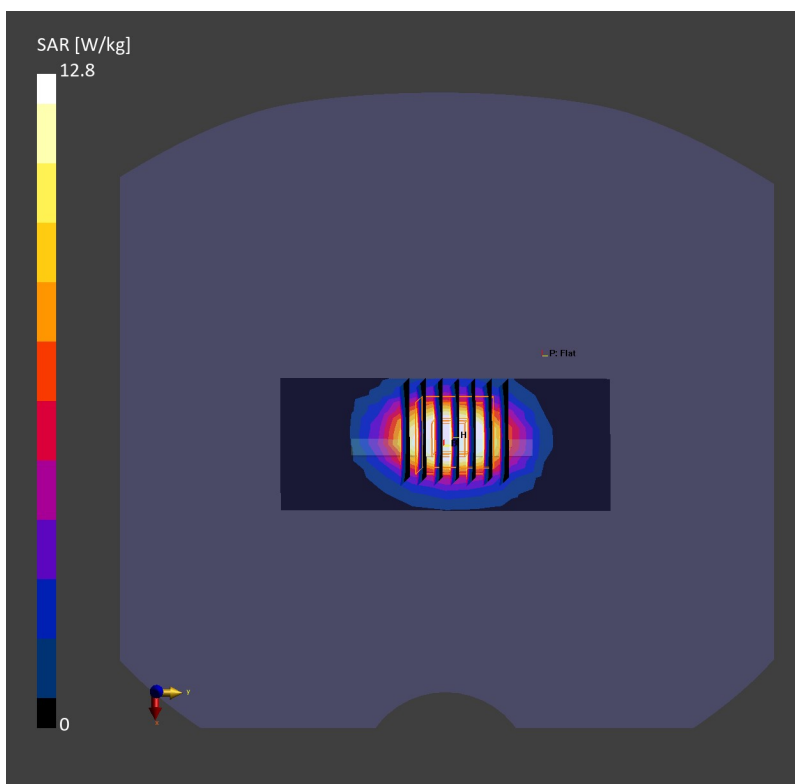

Date: 2026-03-21

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.6$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 12.9 W/kg; SAR (10g) = 6.08 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 13.1 W/kg; SAR (10g) = 6.09 W/kg
Smallest distance from peaks to all points 3 dB below = 9.4 mm
Ratio of SAR at M2 to SAR at M1 = 78.8 %

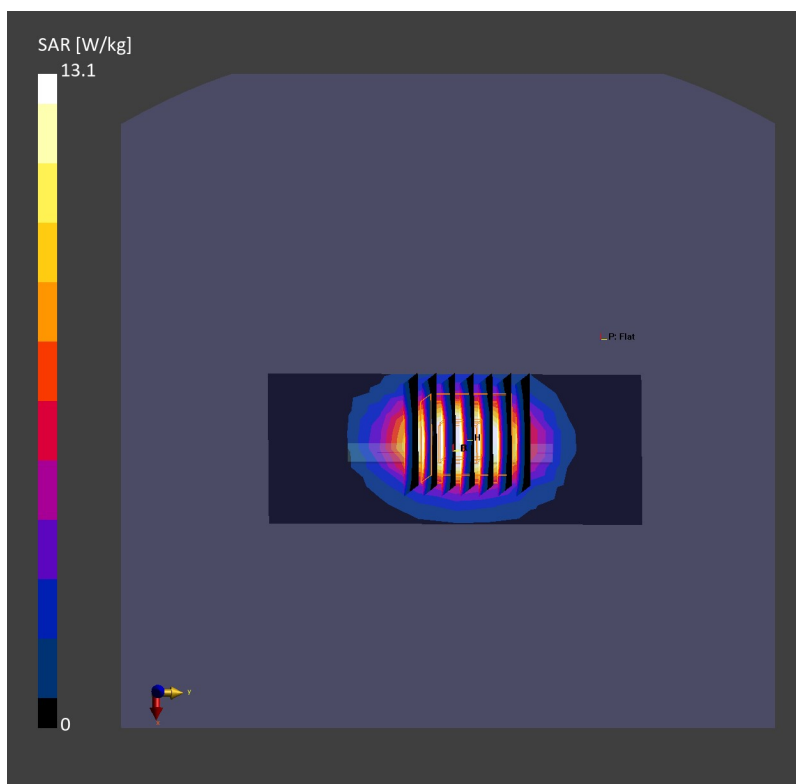

Date: 2026-03-25

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 39.8$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.4 W/kg; SAR (10g) = 6.12 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.03 dB
SAR (1g) = 13.6 W/kg; SAR (10g) = 6.16 W/kg
Smallest distance from peaks to all points 3 dB below = 8.2 mm
Ratio of SAR at M2 to SAR at M1 = 71.2 %

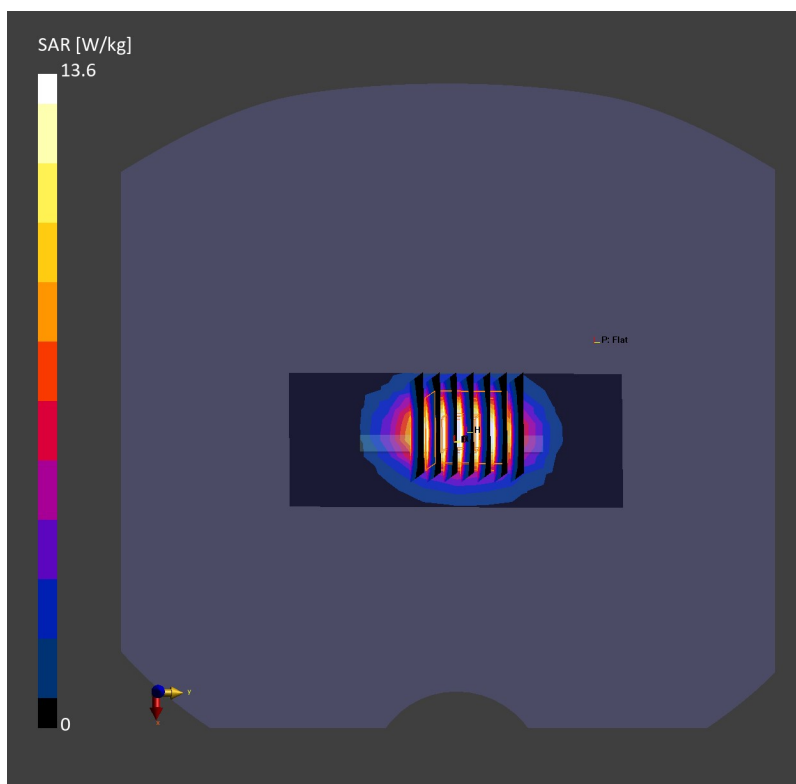

Date: 2026-04-11

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 39.7$
Ambient Temperature: 23.8°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.7 W/kg; SAR (10g) = 6.18 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 13.9 W/kg; SAR (10g) = 6.18 W/kg
Smallest distance from peaks to all points 3 dB below = 8.9 mm
Ratio of SAR at M2 to SAR at M1 = 79.1 %

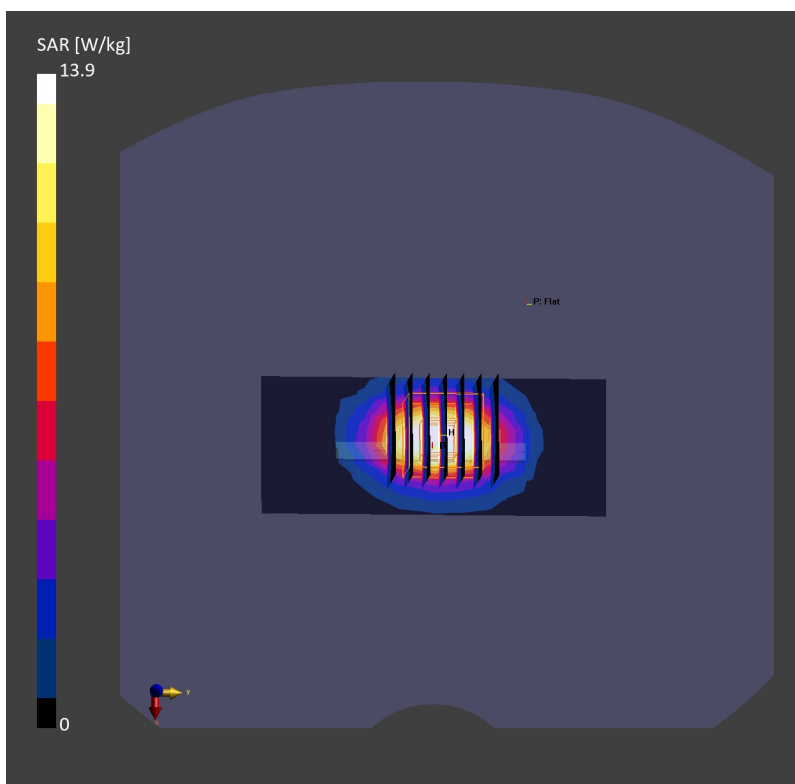

Date: 2026-03-18

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.56$ S/m; $\epsilon_r = 35.9$
Ambient Temperature: 23.7°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.80, 5.57, 5.56); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.74 W/kg; SAR (10g) = 2.23 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.07 dB
SAR (1g) = 8.32 W/kg; SAR (10g) = 2.41 W/kg
Smallest distance from peaks to all points 3 dB below = 8.9 mm
Ratio of SAR at M2 to SAR at M1 = 63.1 %

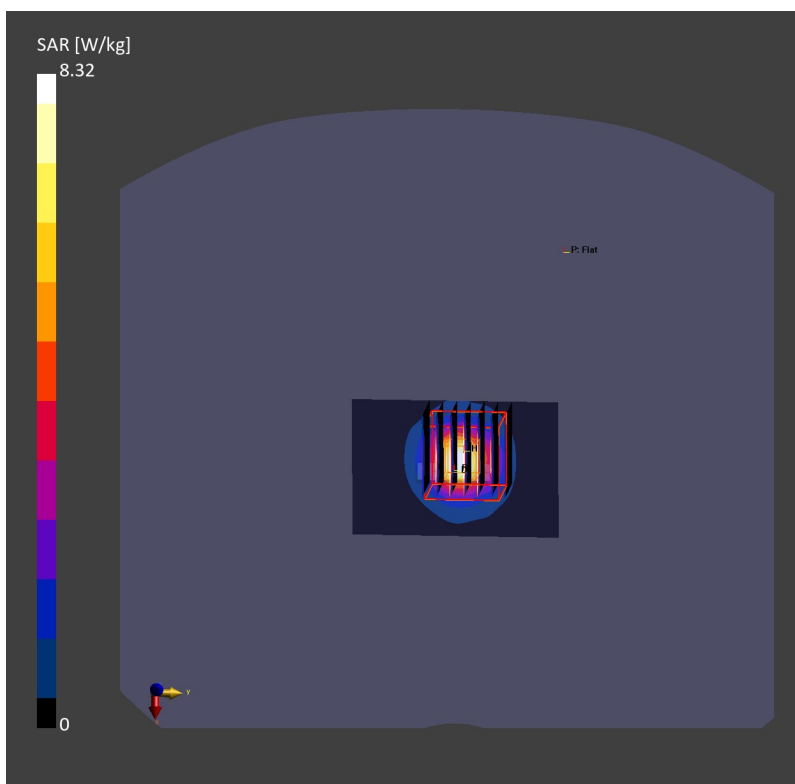

Date: 2026-03-20

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.57$ S/m; $\epsilon_r = 36.6$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.80, 5.57, 5.56); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.76 W/kg; SAR (10g) = 2.13 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 8.26 W/kg; SAR (10g) = 2.26 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 69.6 %

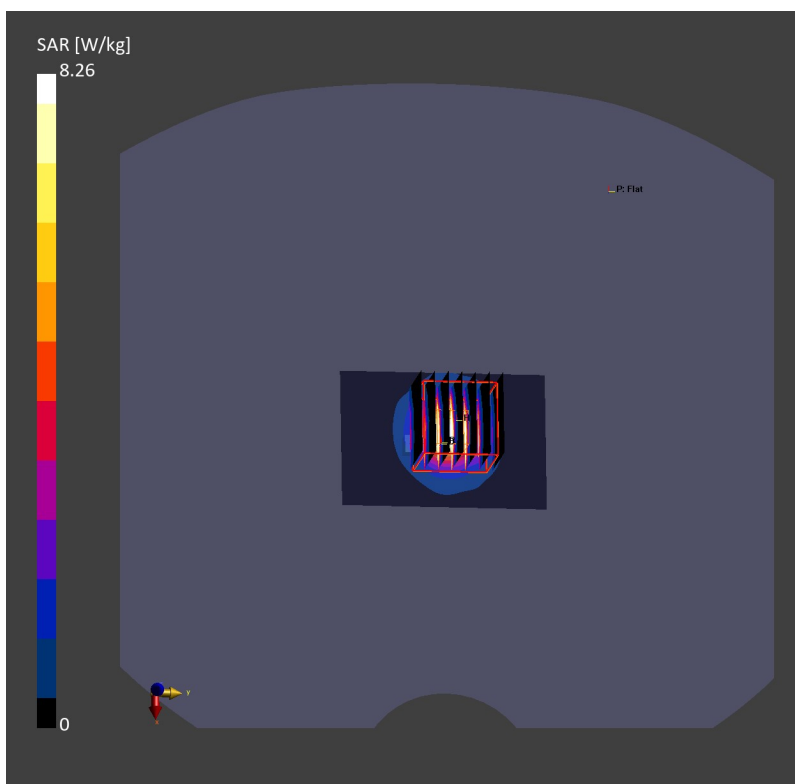

Date: 2026-03-22

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.52$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.80, 5.57, 5.56); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.78 W/kg; SAR (10g) = 2.22 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 8.31 W/kg; SAR (10g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 66.9 %

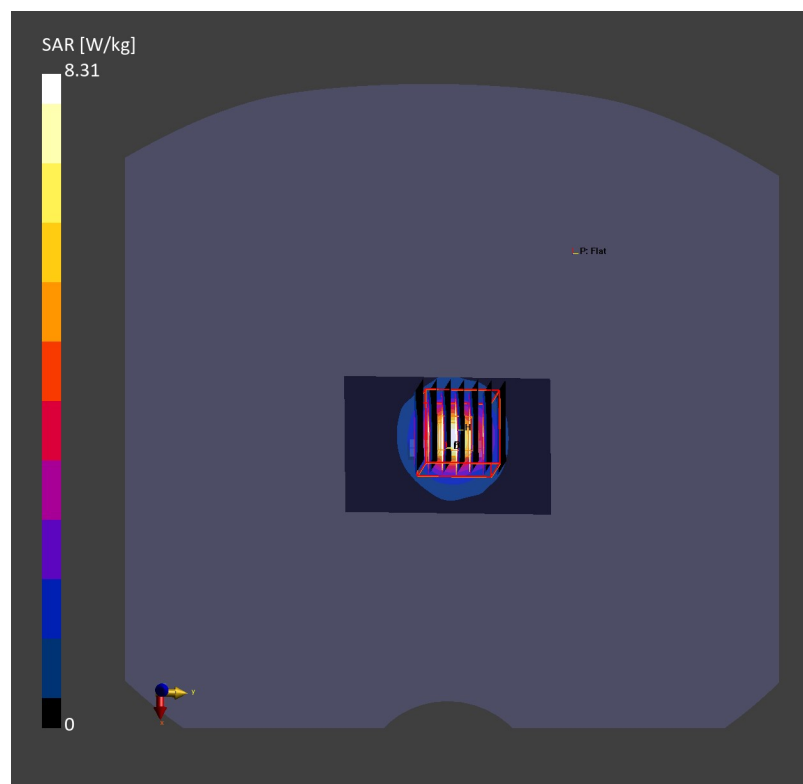

Date: 2026-04-13

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.53$ S/m; $\epsilon_r = 35.6$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.00); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.74 W/kg; SAR (10g) = 2.19 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.11 dB
SAR (1g) = 8.28 W/kg; SAR (10g) = 2.24 W/kg
Smallest distance from peaks to all points 3 dB below = 7.8 mm
Ratio of SAR at M2 to SAR at M1 = 64.2 %

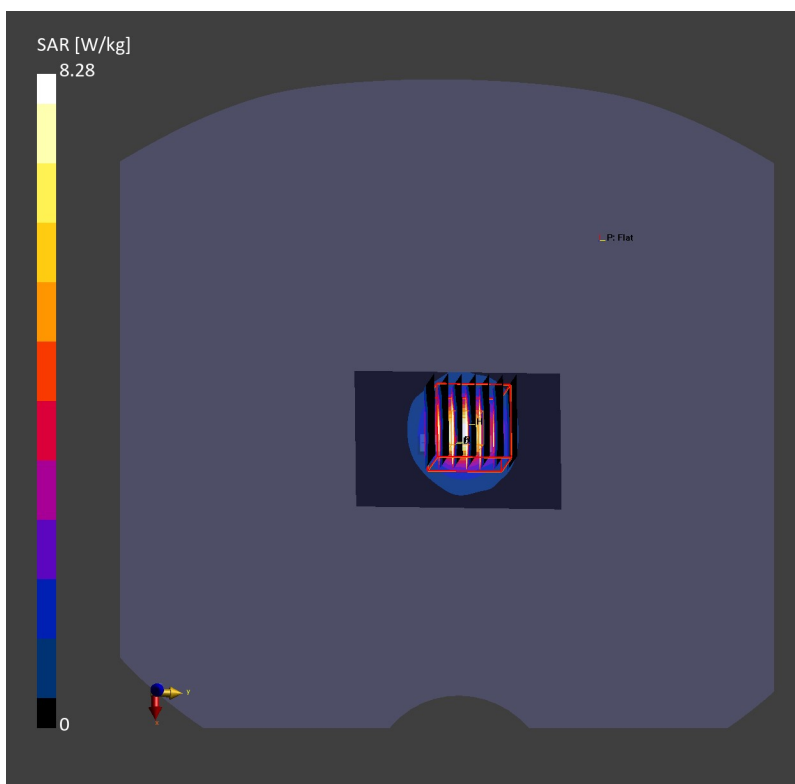

Date: 2026-03-24

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.87$ S/m; $\epsilon_r = 35.0$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.24 W/kg; SAR (10g) = 2.42 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.14 dB
SAR (1g) = 8.27 W/kg; SAR (10g) = 2.49 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 67.9 %

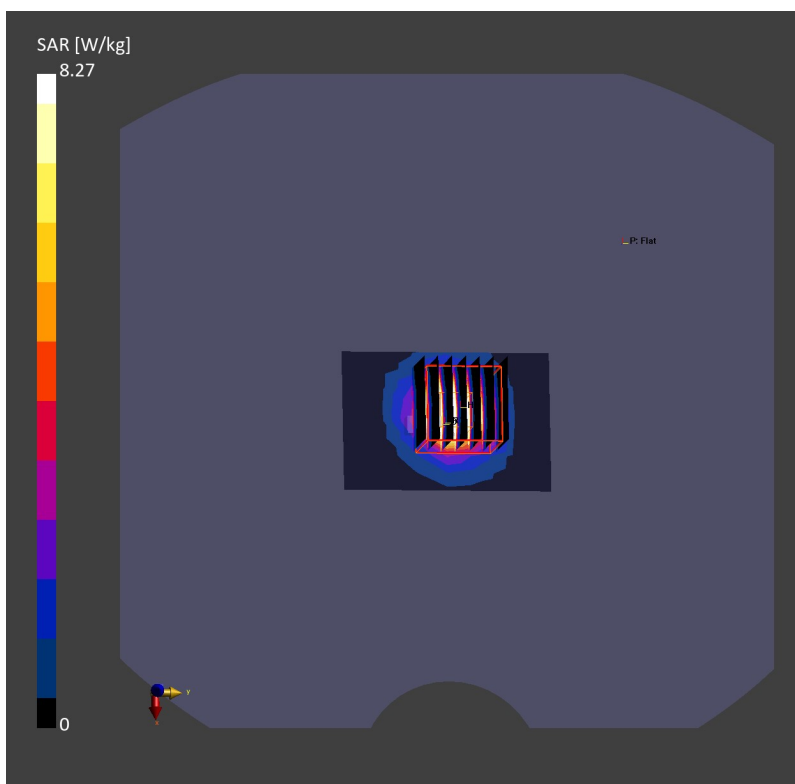

Date: 2026-03-27

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.91$ S/m; $\epsilon_r = 35.3$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.19 W/kg; SAR (10g) = 2.41 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.13 dB
SAR (1g) = 8.23 W/kg; SAR (10g) = 2.46 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 67.5 %

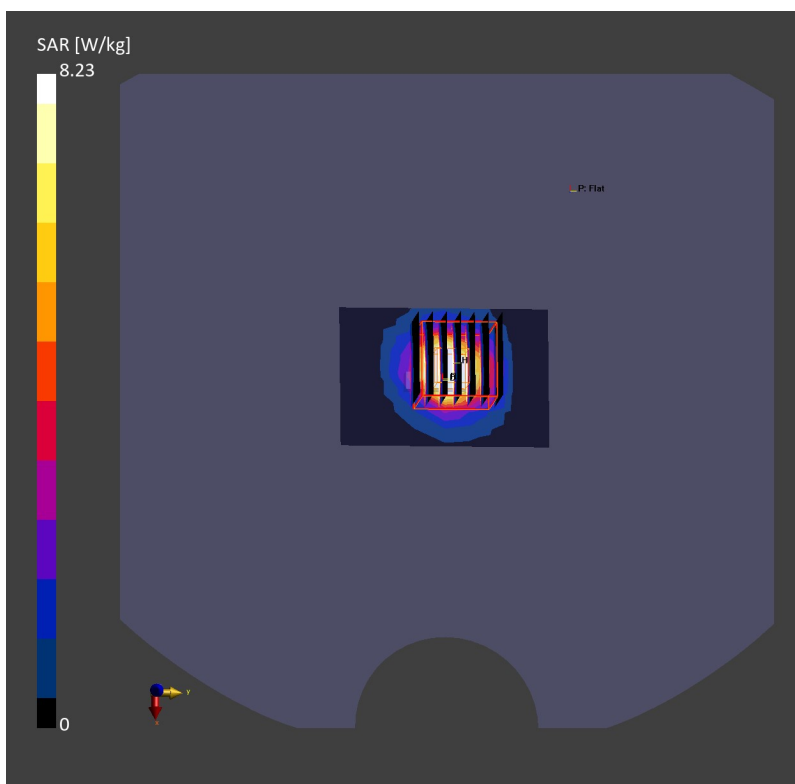

Date: 2026-03-29

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.92$ S/m; $\epsilon_r = 36.1$
Ambient Temperature: 23.7°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.56 W/kg; SAR (10g) = 2.35 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.06 dB
SAR (1g) = 8.19 W/kg; SAR (10g) = 2.43 W/kg
Smallest distance from peaks to all points 3 dB below = 8.2 mm
Ratio of SAR at M2 to SAR at M1 = 71.4 %

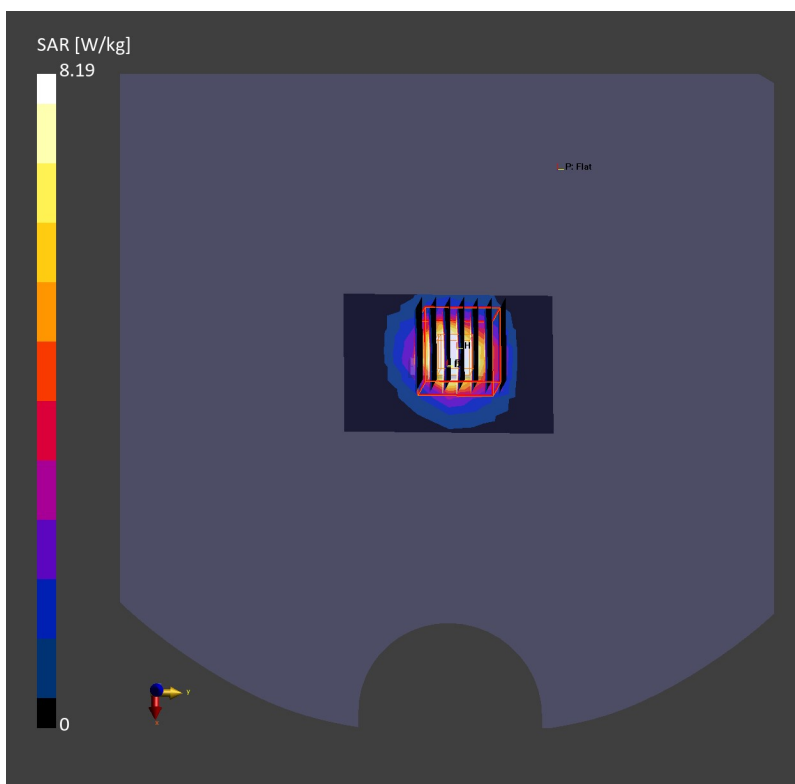

Date: 2026-04-12

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
 Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.9$ S/m; $\epsilon_r = 35.2$
 Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
 SAR (1g) = 8.04 W/kg; SAR (10g) = 2.39 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
 Power Drift = -0.11 dB
 SAR (1g) = 8.14 W/kg; SAR (10g) = 2.35 W/kg
 Smallest distance from peaks to all points 3 dB below = 9.6 mm
 Ratio of SAR at M2 to SAR at M1 = 67.7 %

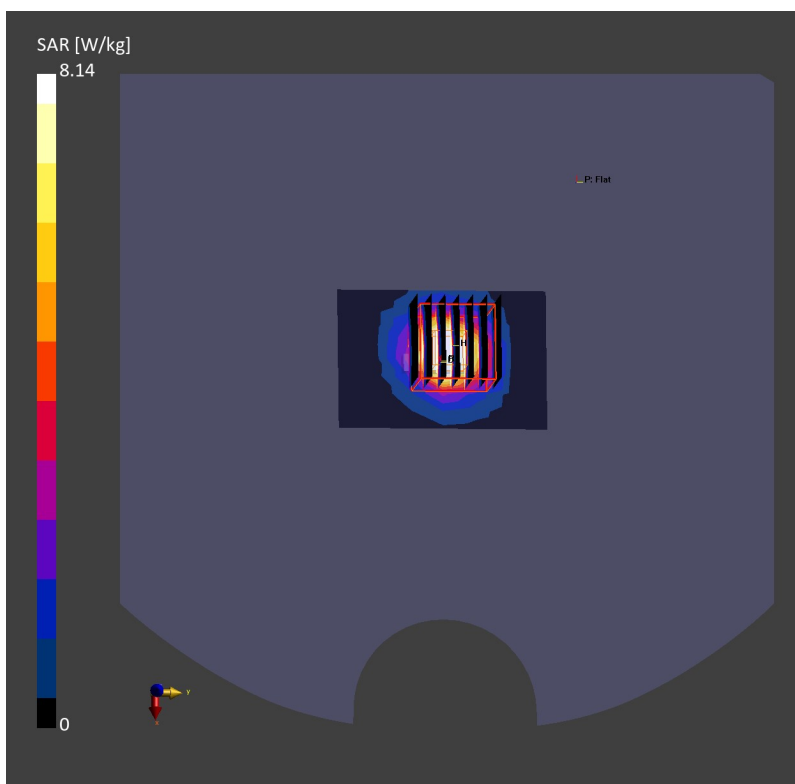

Date: 2026-03-27

System Check_5800MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.07$ S/m; $\epsilon_r = 34.9$
Ambient Temperature: 23.7°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.89 W/kg; SAR (10g) = 2.32 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.07 dB
SAR (1g) = 8.16 W/kg; SAR (10g) = 2.45 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 64.5 %

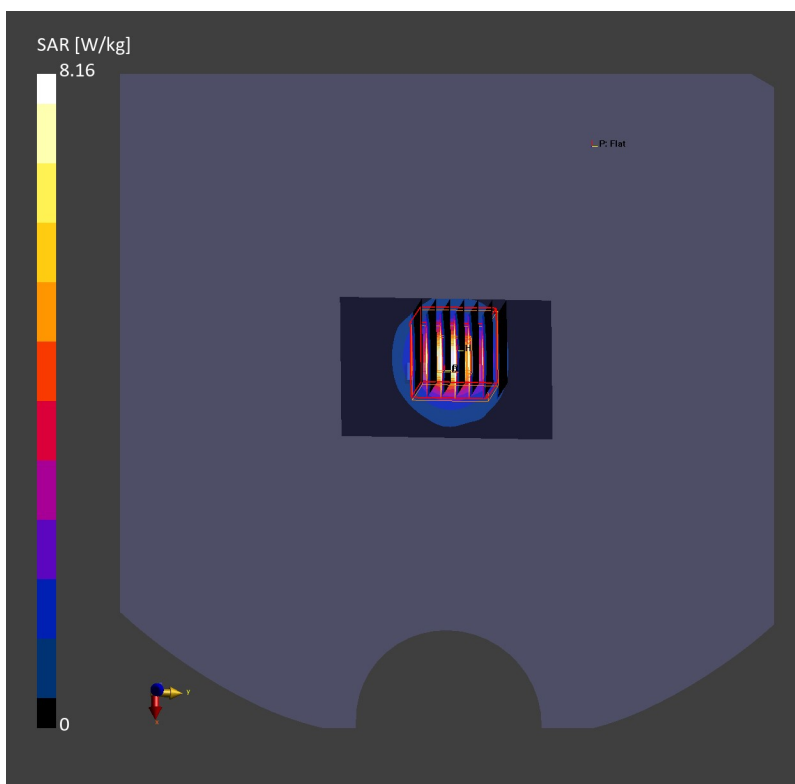

Date: 2026-03-29

System Check_5800MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.11$ S/m; $\epsilon_r = 35.1$
Ambient Temperature: 23.8°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.82 W/kg; SAR (10g) = 2.29 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.06 dB
SAR (1g) = 8.11 W/kg; SAR (10g) = 2.38 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 63.3 %

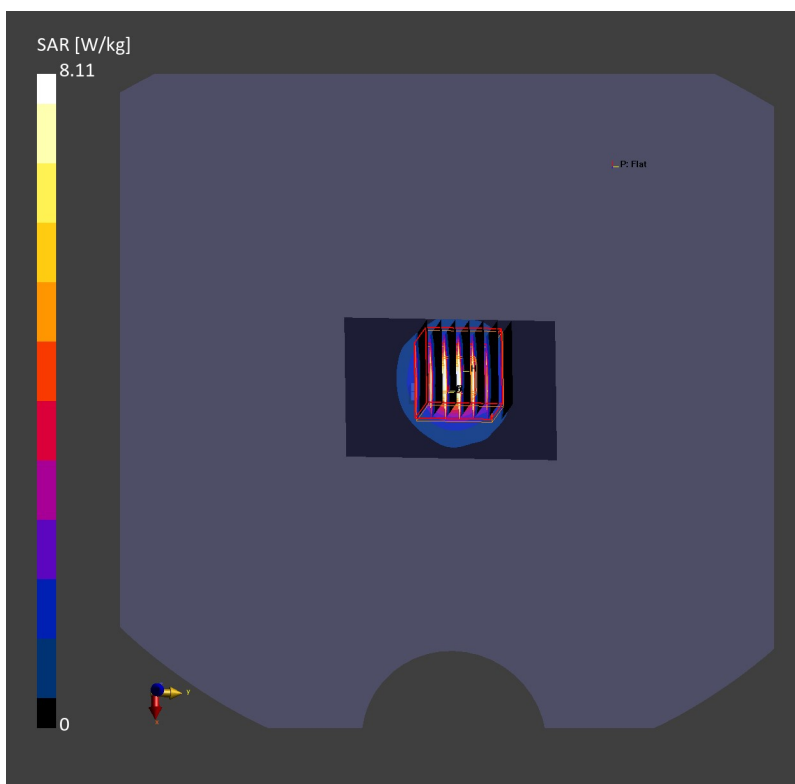

Date: 2026-04-02

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.14$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.76 W/kg; SAR (10g) = 2.21 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.12 dB

SAR (1g) = 8.06 W/kg; SAR (10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 69.5 %

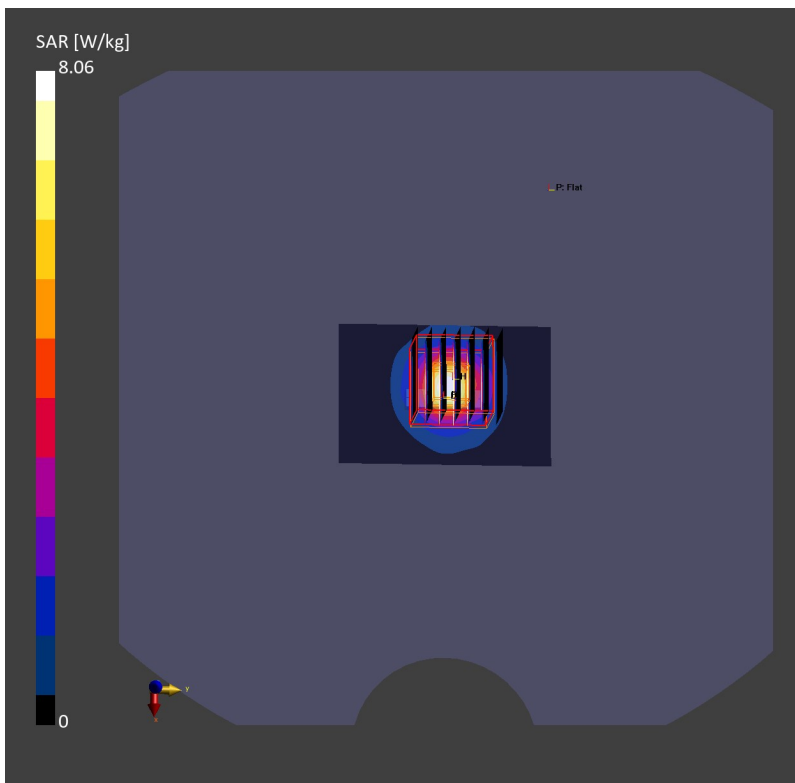

Date: 2026-04-13

System Check_5800MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.16$ S/m; $\epsilon_r = 34.7$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.72 W/kg; SAR (10g) = 2.18 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.05 dB
SAR (1g) = 7.97 W/kg; SAR (10g) = 2.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.5 mm
Ratio of SAR at M2 to SAR at M1 = 67.3 %

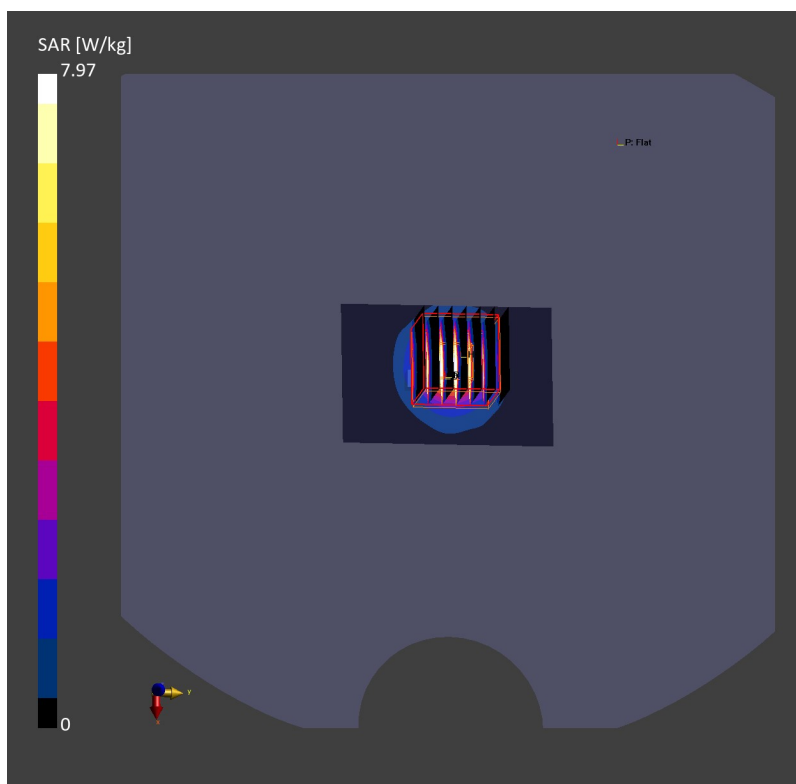

Date: 2026-03-24

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**


Communication System: CW; Frequency: 6500.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f=6500.0$ MHz; $\sigma=5.9$ S/m; $\epsilon_r=34.1$
Ambient Temperature: 23.7°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.58, 5.36, 5.35); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 51.0 mm): Measurement Grid: 6.0 mm x 8.5 mm
SAR (1g) = 27.9 W/kg; SAR (10g) = 5.65 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 30.9 W/kg; SAR (10g) = 5.72 W/kg
Smallest distance from peaks to all points 3 dB below = 5.2 mm
Ratio of SAR at M2 to SAR at M1 = 55.7 %
psAPD (4.0cm², sq) = 137 [W/m²]

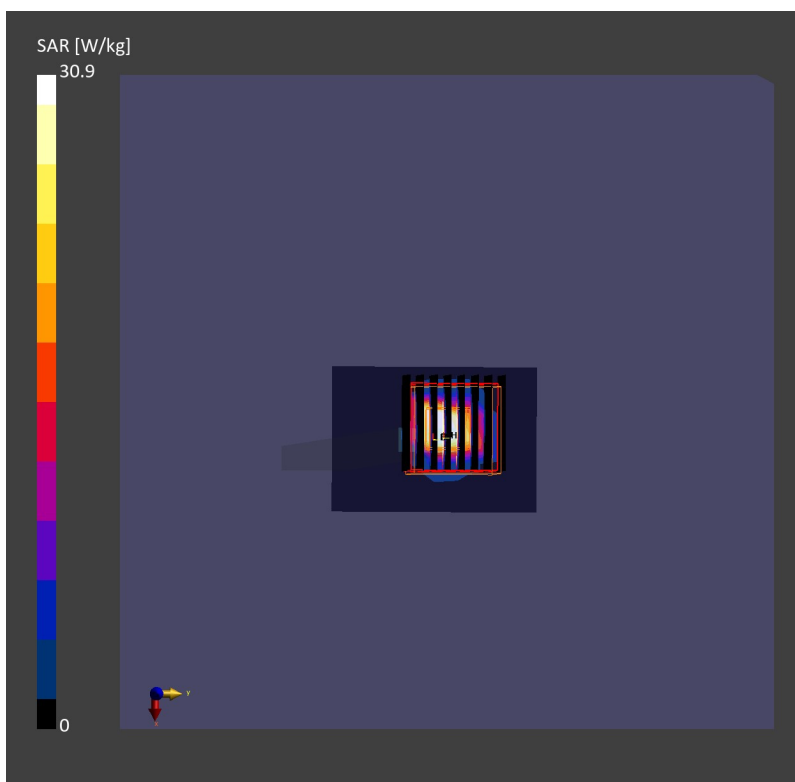

Date: 2026-03-25

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**


Communication System: CW; Frequency: 6500.0 MHz; Duty Cycle: 1:1
 Medium: HSL Medium parameters used: $f = 6500.0$ MHz; $\sigma = 5.82$ S/m; $\epsilon_r = 33.8$
 Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.58, 5.36, 5.35); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 51.0 mm): Measurement Grid: 6.0 mm x 8.5 mm
 SAR (1g) = 27.7 W/kg; SAR (10g) = 5.56 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm
 Power Drift = 0.07 dB
 SAR (1g) = 30.1 W/kg; SAR (10g) = 5.68 W/kg
 Smallest distance from peaks to all points 3 dB below = 6.1 mm
 Ratio of SAR at M2 to SAR at M1 = 58.8 %
 psAPD (4.0cm², sq) = 139 [W/m²]

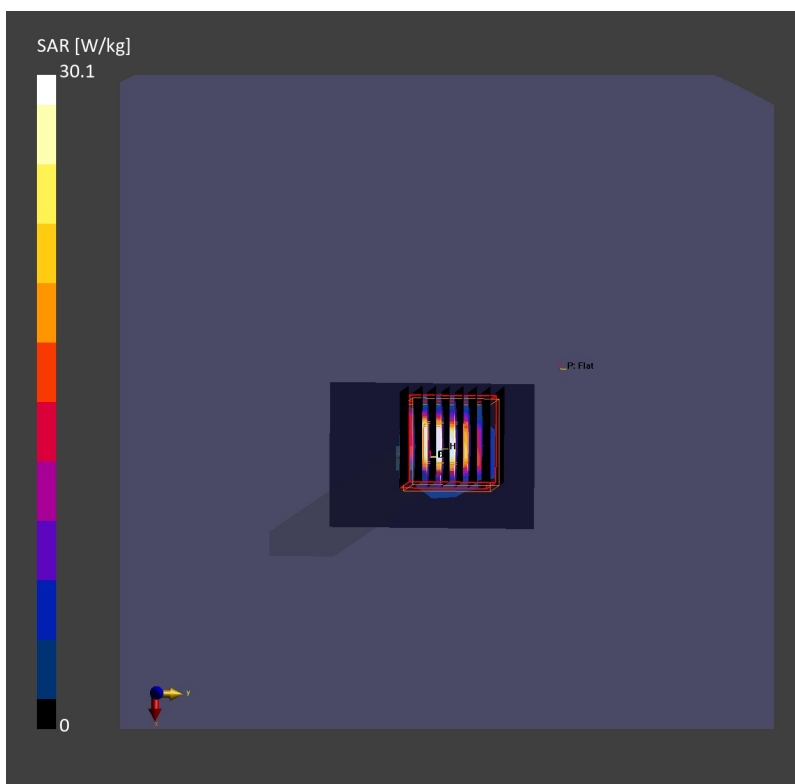

Date: 2026-04-01

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**


Communication System: CW; Frequency: 6500.0 MHz; Duty Cycle: 1:1
 Medium: HSL Medium parameters used: $f = 6500.0$ MHz; $\sigma = 5.91$ S/m; $\epsilon_r = 34.8$
 Ambient Temperature: 23.6°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.68, 5.58, 5.60); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1210; Calibrated: 2025-11-28
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2033; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 51.0 mm): Measurement Grid: 6.0 mm x 8.5 mm
 SAR (1g) = 27.1 W/kg; SAR (10g) = 5.48 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm
 Power Drift = -0.06 dB
 SAR (1g) = 29.9 W/kg; SAR (10g) = 5.53 W/kg
 Smallest distance from peaks to all points 3 dB below = 6.7 mm
 Ratio of SAR at M2 to SAR at M1 = 63.1 %
 psAPD (4.0cm², sq) = 138 [W/m²]

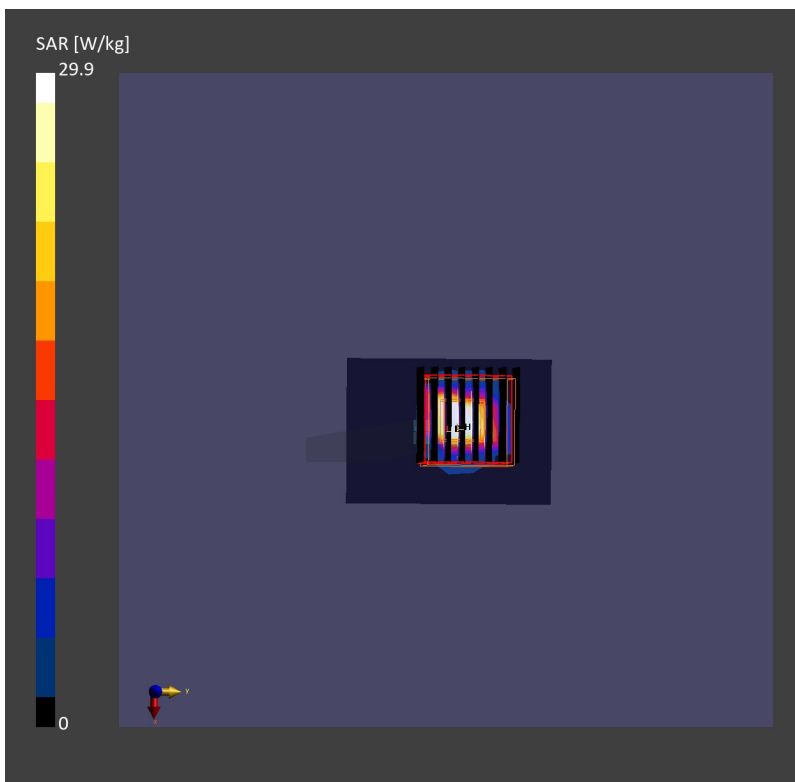

Date: 2026-04-14

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**


Communication System: CW; Frequency: 6500.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 6500.0$ MHz; $\sigma = 5.96$ S/m; $\epsilon_r = 33.5$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.58, 5.36, 5.35); Calibrated: 2025-07-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 51.0 mm): Measurement Grid: 6.0 mm x 8.5 mm
SAR (1g) = 26.9 W/kg; SAR (10g) = 5.43 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 29.7 W/kg; SAR (10g) = 5.49 W/kg
Smallest distance from peaks to all points 3 dB below = 5.3 mm
Ratio of SAR at M2 to SAR at M1 = 59.7 %
psAPD (4.0cm², sq) = 132 [W/m²]

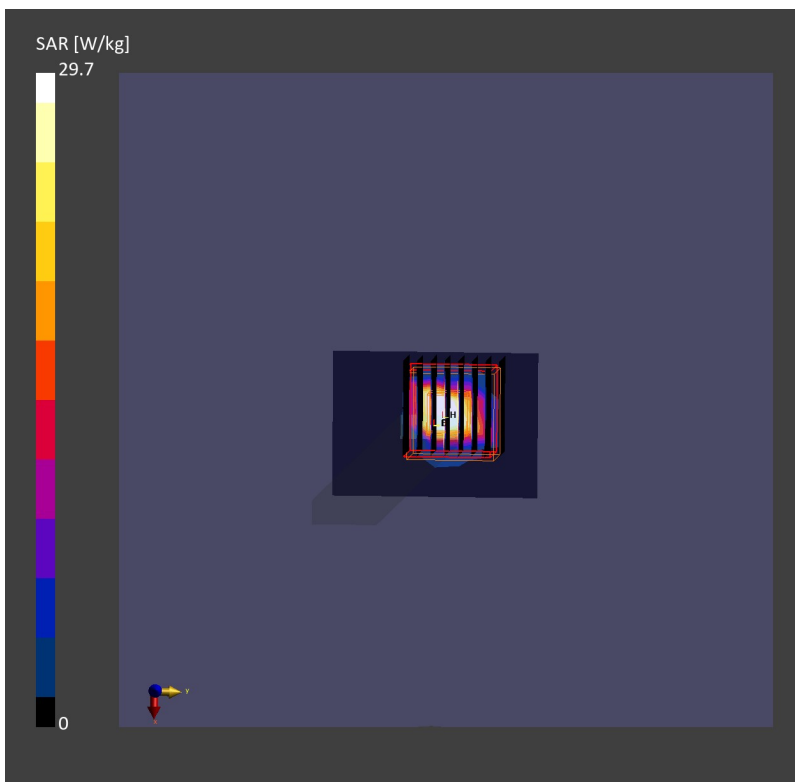

System Check_2450MHz**DUT:D2450V2-SN:924**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.85	40.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-03-25	2026-03-25
psSAR1g [W/Kg]	11.7	13.1
psSAR10g [W/Kg]	5.12	6.26
Power Drift [dB]	-0.03	-0.02

SAR Pattern

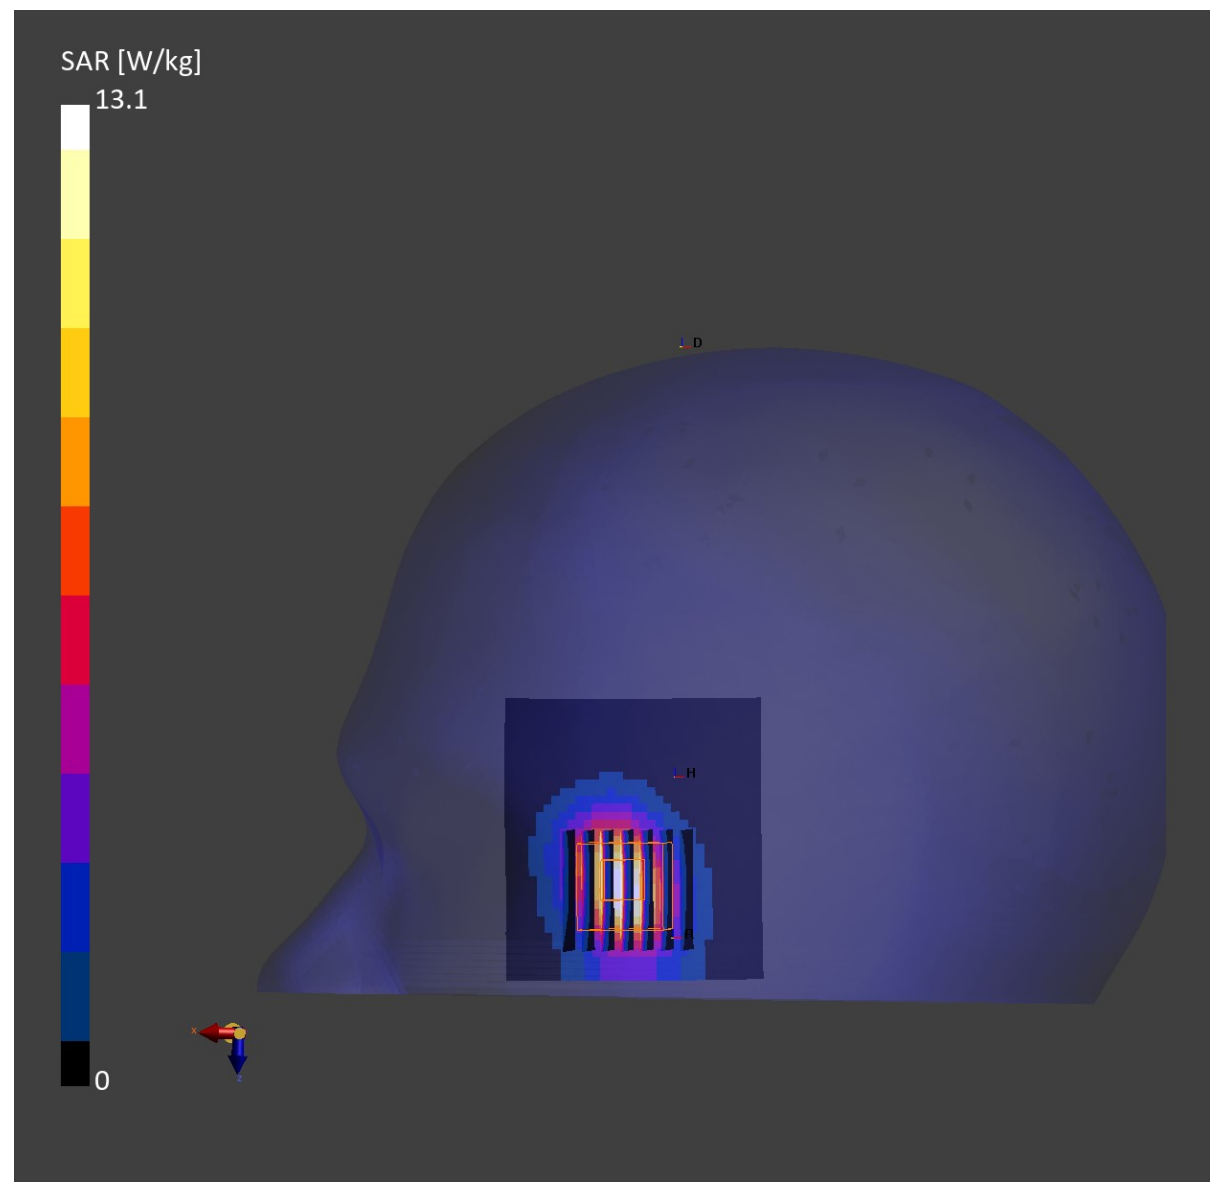

System Check_2450MHz**DUT:D2450V2-SN:924**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.77	38.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-03-27	2026-03-27
psSAR1g [W/Kg]	12.1	13.8
psSAR10g [W/Kg]	5.18	6.29
Power Drift [dB]	0.05	-0.08

SAR Pattern

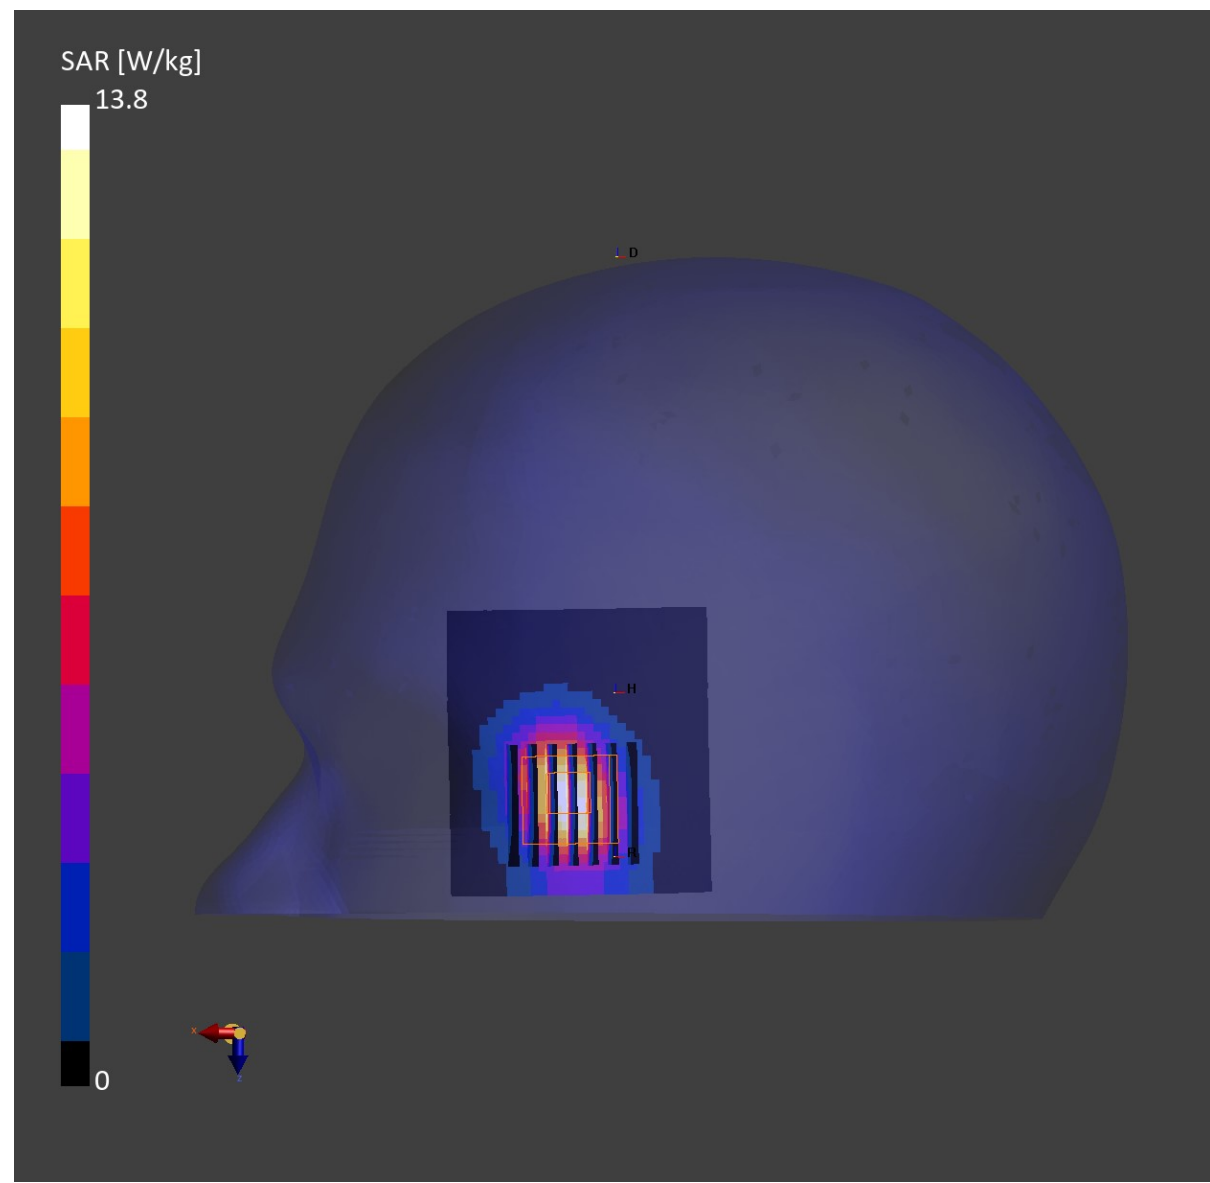

System Check_2450MHz**DUT:D2450V2-SN:924**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.82	38.6

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-03-31	2026-03-31
psSAR1g [W/Kg]	11.2	13.1
psSAR10g [W/Kg]	5.01	6.12
Power Drift [dB]	-0.03	0.12

SAR Pattern

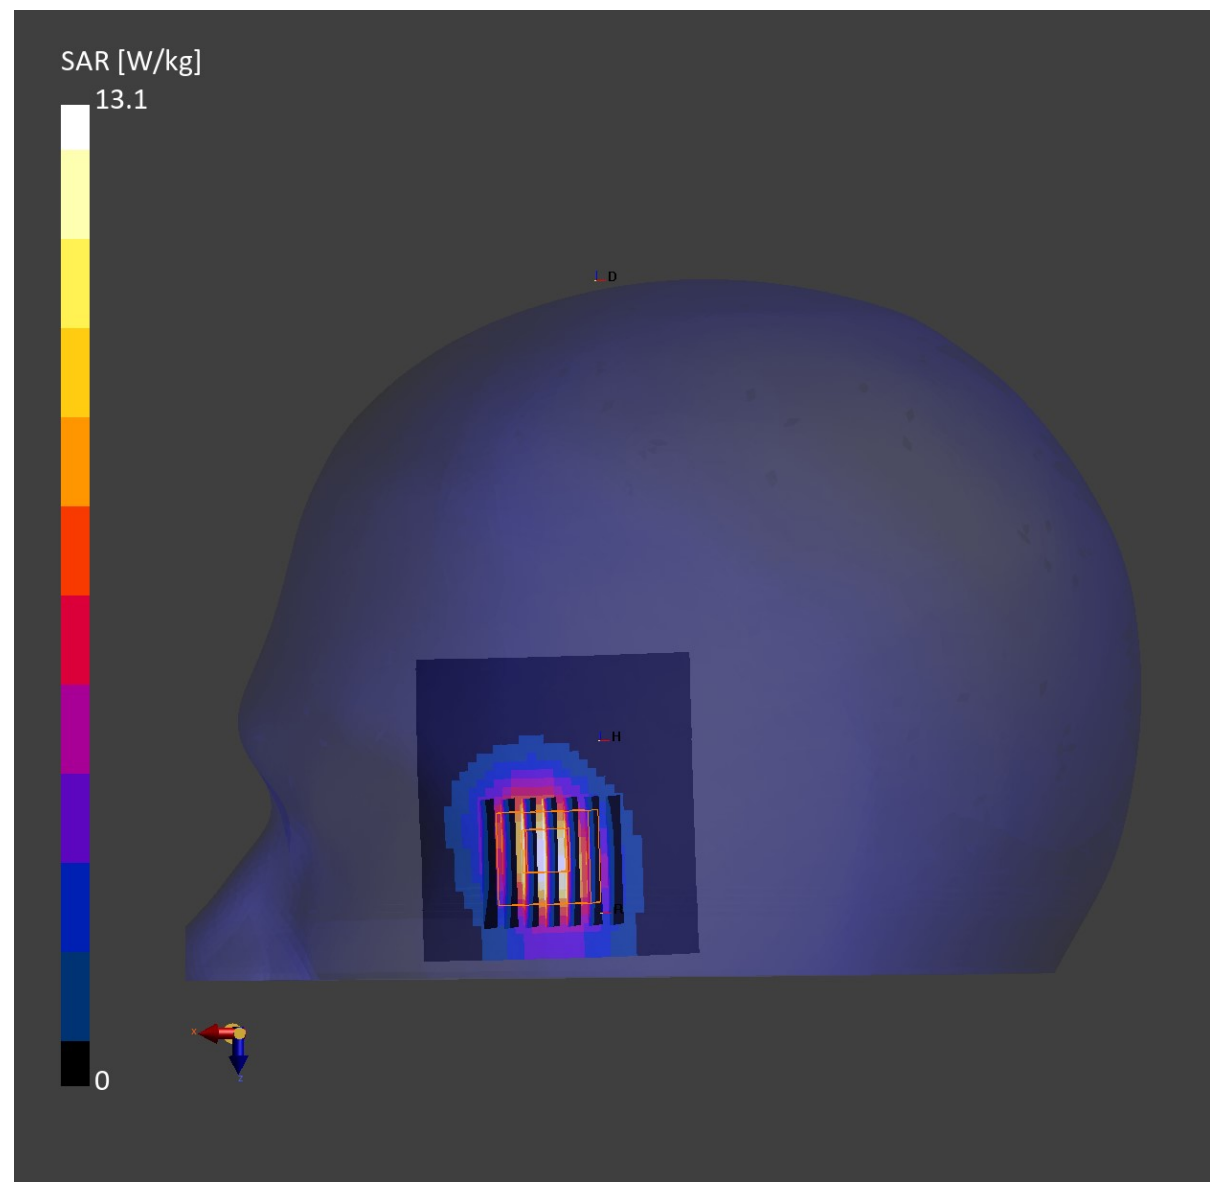

System Check_2450MHz**DUT:D2450V2-SN:924**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 10.00	D2450	CW, 0--	2450.0, 50	7.87	1.78	38.5

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-04-12	2026-04-12
psSAR1g [W/Kg]	10.9	12.5
psSAR10g [W/Kg]	4.91	6.04
Power Drift [dB]	-0.05	0.01

SAR Pattern

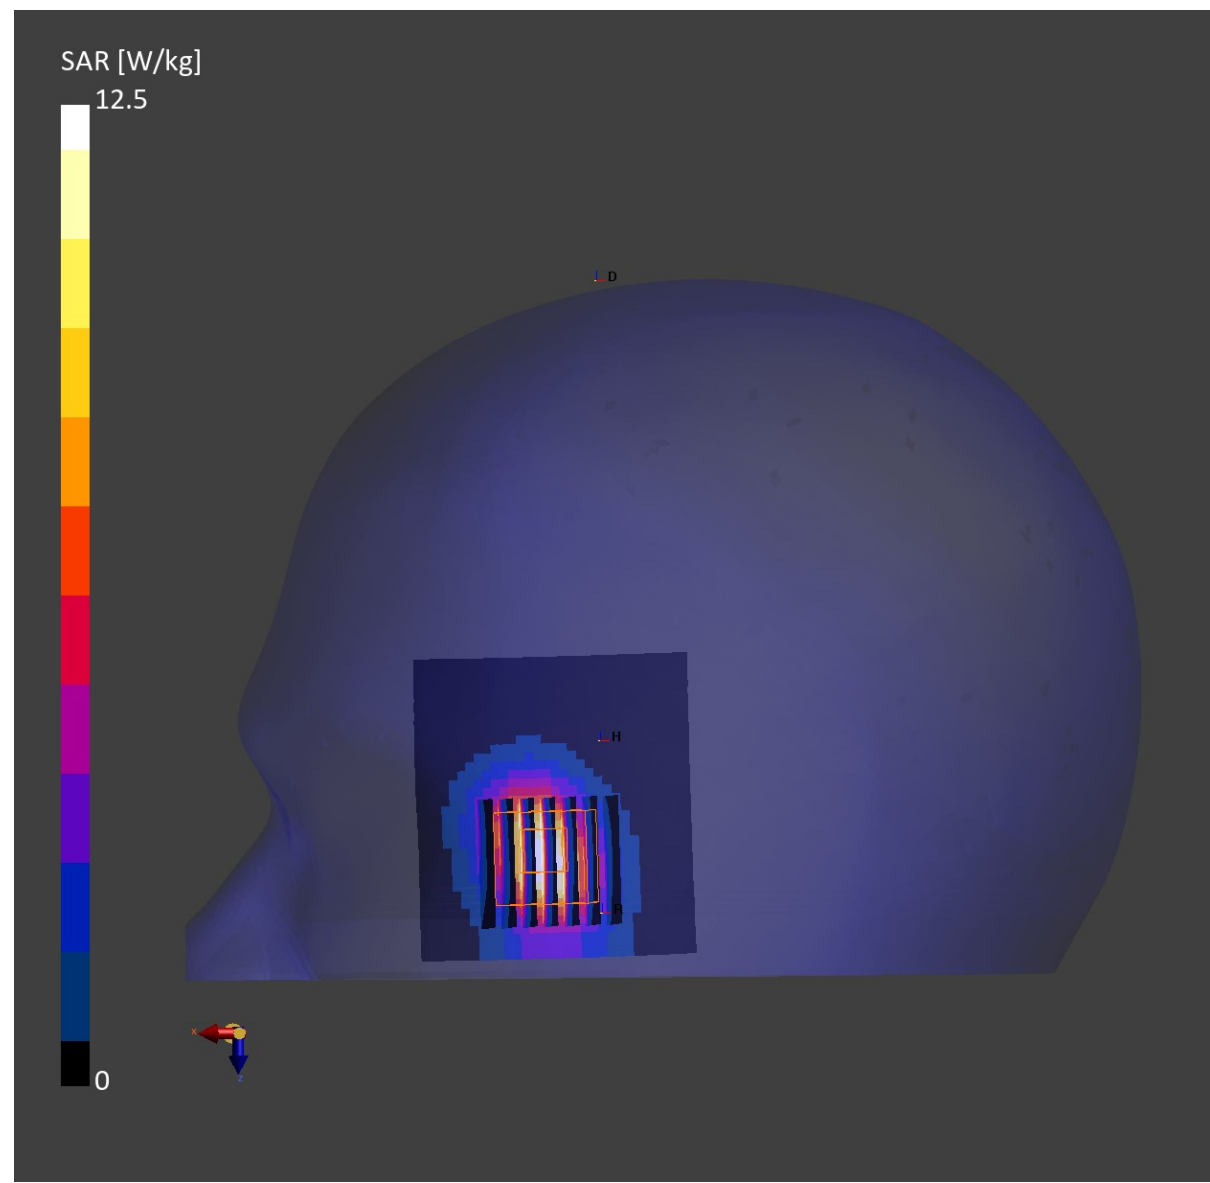

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.20	35.1

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-03-28	2026-03-28
psSAR1g [W/Kg]	1.77	1.79
psSAR10g [W/Kg]	0.611	0.597
Power Drift [dB]	-0.04	0.11

SAR Pattern

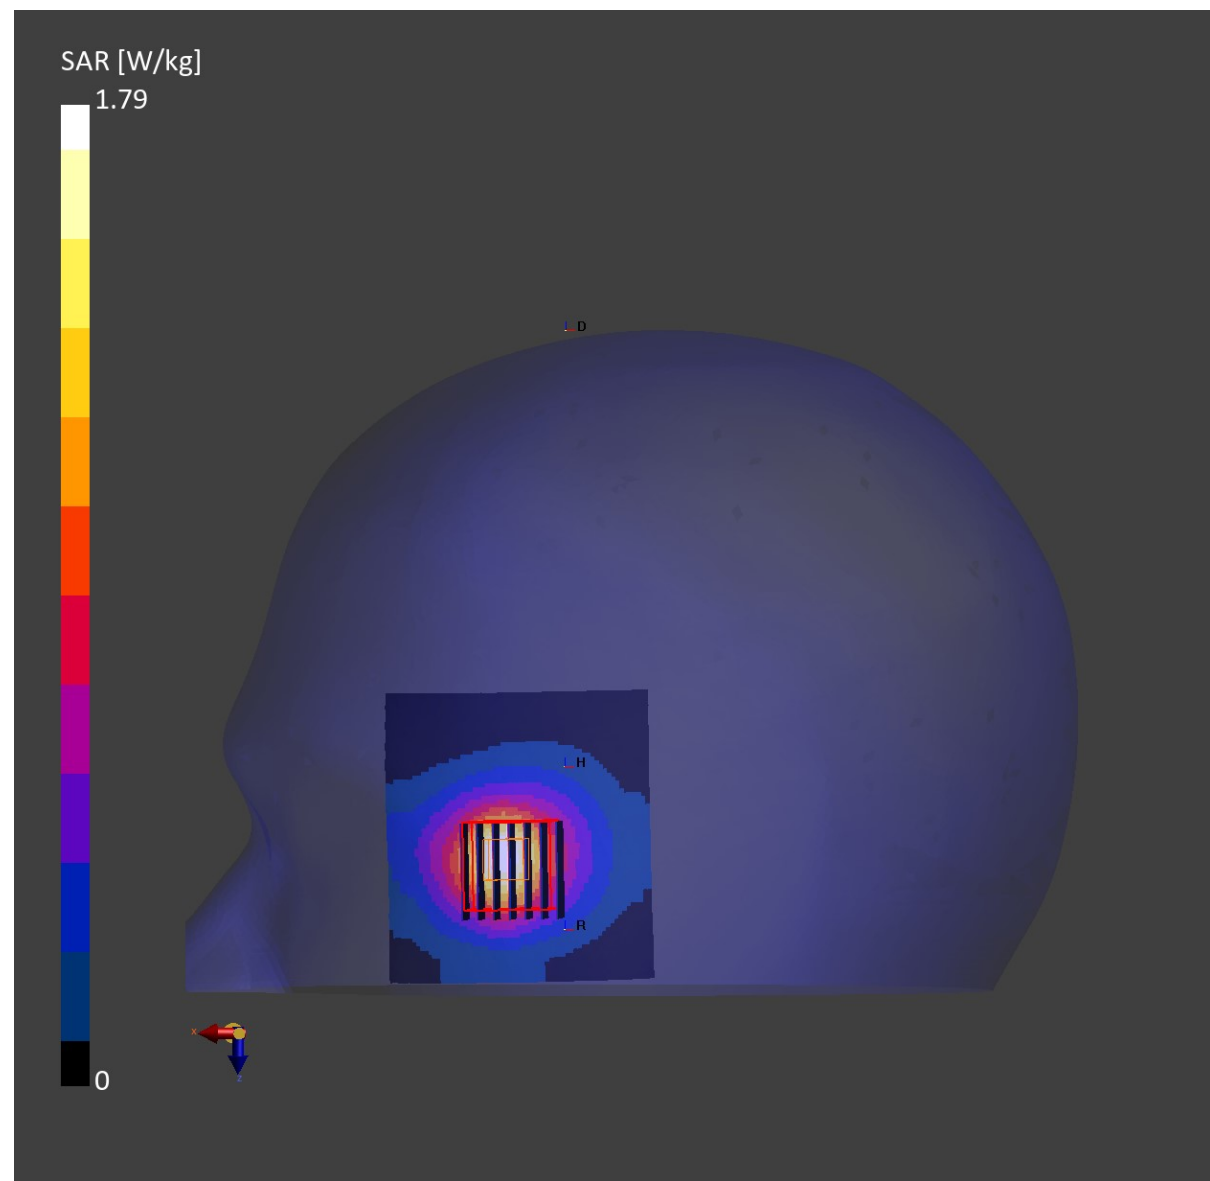

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.24	35.5

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-03-29	2026-03-29
psSAR1g [W/Kg]	1.68	1.72
psSAR10g [W/Kg]	0.601	0.588
Power Drift [dB]	0.15	0.04

SAR Pattern

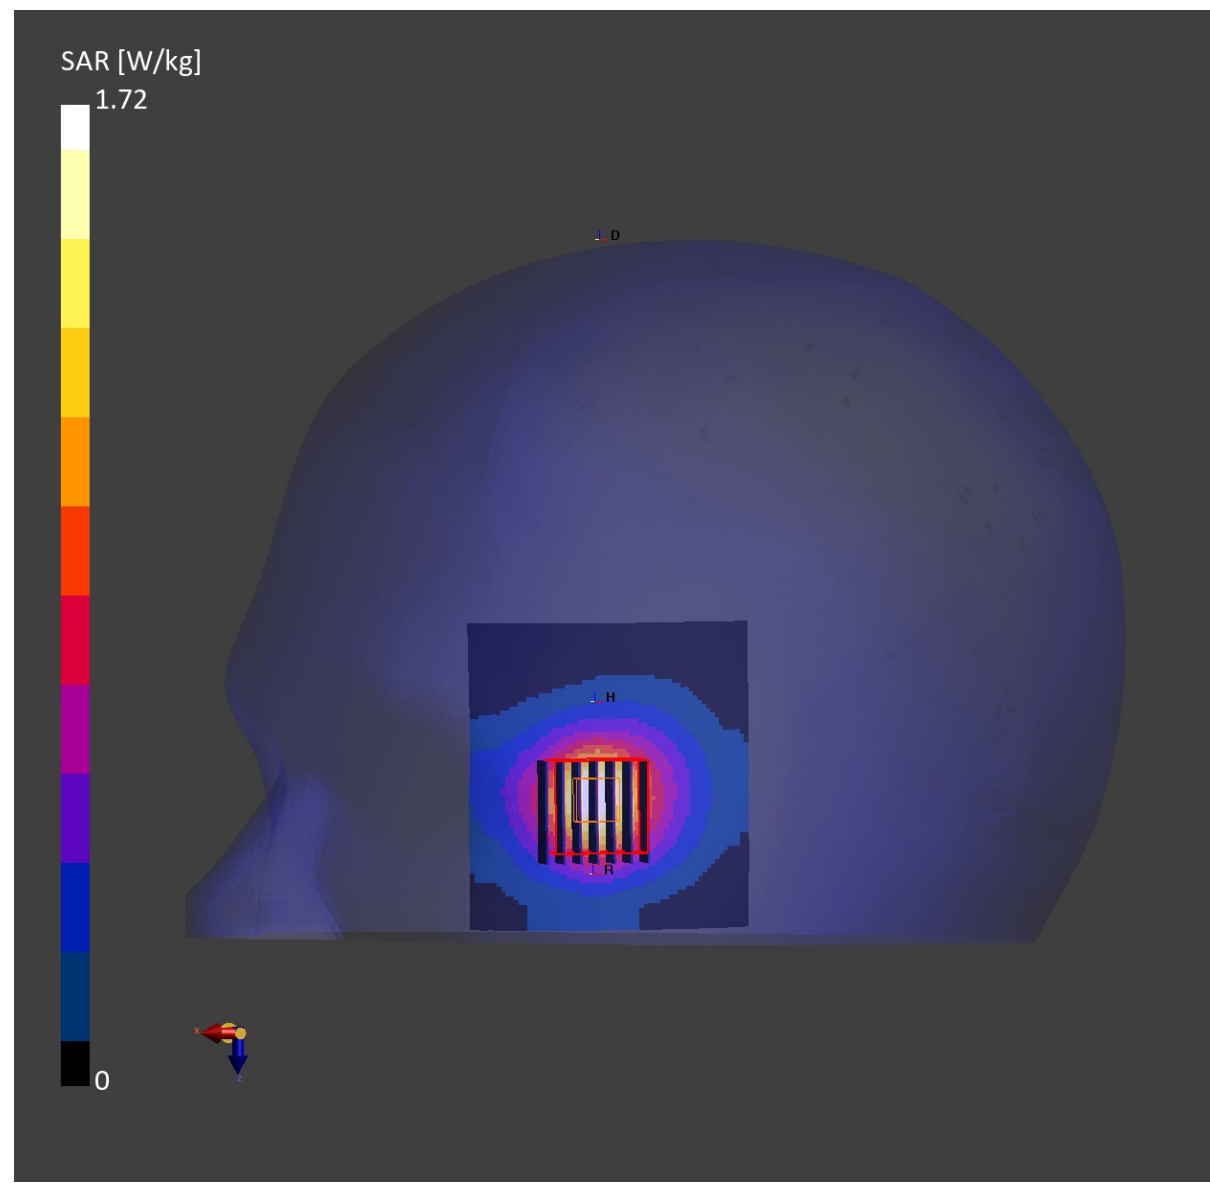

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.14	35.3

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-04-02	2026-04-02
psSAR1g [W/Kg]	1.76	1.77
psSAR10g [W/Kg]	0.605	0.594
Power Drift [dB]	-0.07	0.02

SAR Pattern

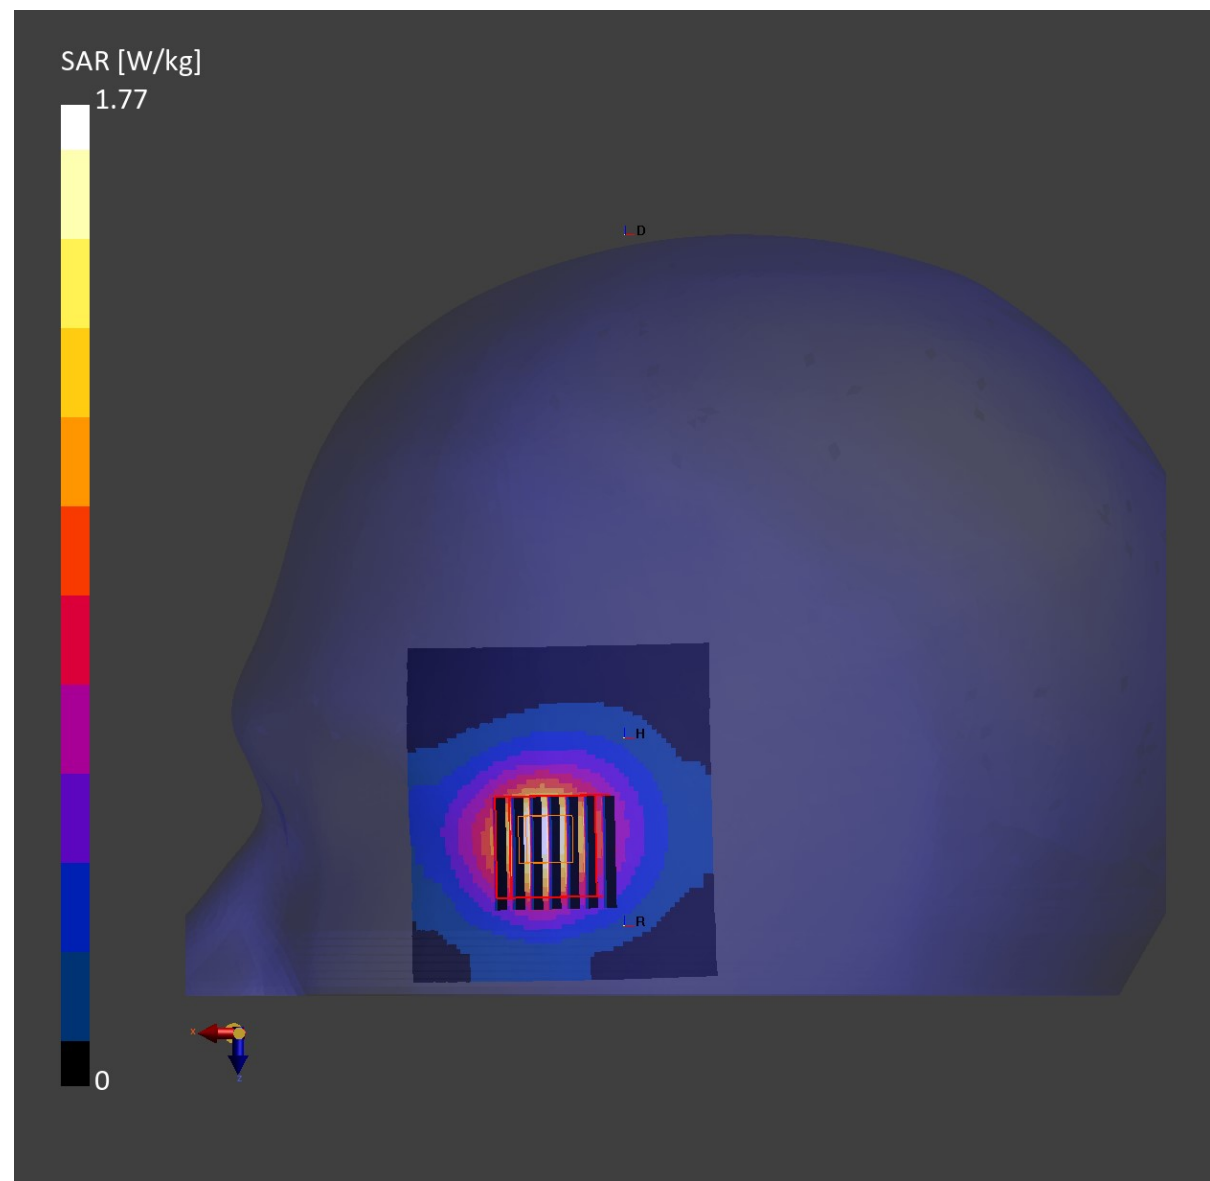

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	158.2 x 77.9 x 8.0		Dipole

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Headstand, HSL	DEFAULT, 25.00	D5GHz	CW, 0--	5800.0, 80	5.52	5.13	35.1

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
SAM-HeadStand V10.0 – 1024	HBBL-600-10000 ,	EX3DV4 – SN7641, 2025-06-26	DAE4 Sn1210, 2025-11-28


Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	71.6 x 65.1	22.0 x 22.0 x 22.0
Grid Steps [mm]	5.0 x 5.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	3.0
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
Scan Method	Measured	Measured

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2026-04-13	2026-04-13
psSAR1g [W/Kg]	1.85	1.86
psSAR10g [W/Kg]	0.614	0.602
Power Drift [dB]	-0.16	-0.09

SAR Pattern

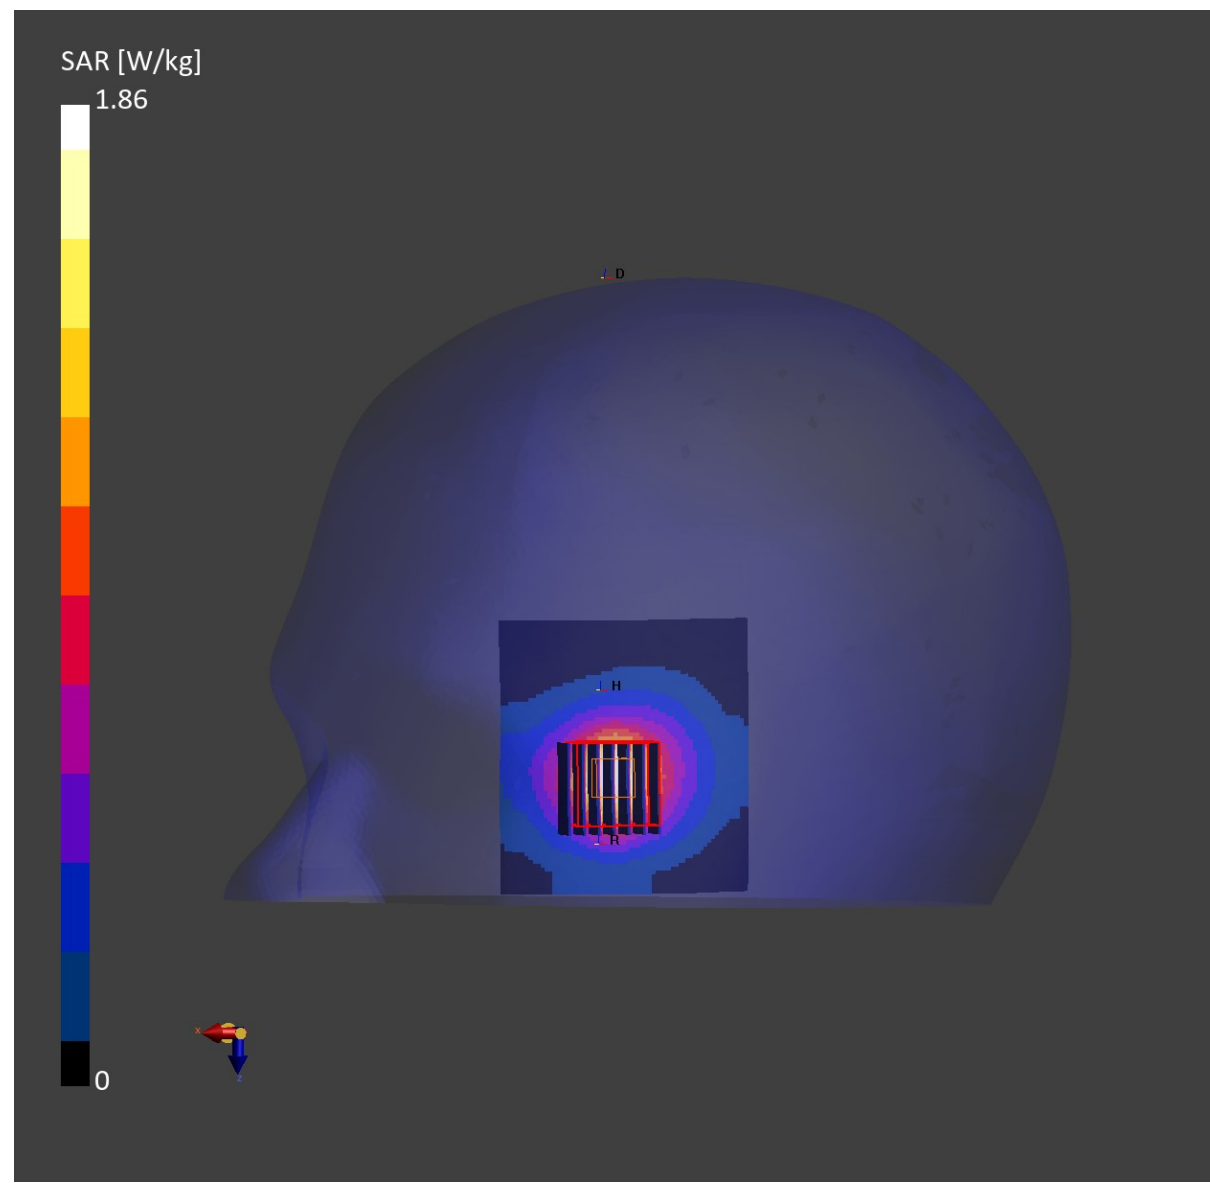

Measurement Report for Device, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	100.0 x 100.0 x 105.0		5G Verification Source

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave	Air -	EUmmWV4 - SN9461_F1-55GHz, 2025-10-15	DAE4 Sn715, 2025-11-28

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2026-04-14
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	151
psPDtot+ [W/m ²]	153
psPDmod+ [W/m ²]	156
E _{max} [V/m]	298
Power Drift [dB]	0.00

