



FCC ID: 2AYQY-ES-2020
Report No.: T201207N01-RP1-2

Page: 1 / 59
Rev.: 00

FCC 47 CFR PART 15 SUBPART C AND ANSI C63.10: 2013

TEST REPORT

For

Electronic Stethoscope

Model: ES-2020

Data Applies To: N/A

Brand: **ibiomedi**

Issued for

Sound Land Corporation

No.32, Keji 1st Rd., Guishan Dist., Taoyuan City 33383, Taiwan

Issued by

Compliance Certification Services Inc.

Tainan Lab.

No.8, Jiucengling, Xinhua Dist.,

Tainan City, Taiwan

Issued Date: June 28, 2021

Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. Ltd. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明，此報告結果僅對測試之樣品負責，同時此樣品僅保留90天。本報告未經本公司書面許可，不可部份複製。

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.tw/Terms-and-Conditions> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.tw/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of client's instruction, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced, except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



Report No.: T201207N01-RP1-2

Page: 2 / 59
Rev.: 00

REVISION HISTORY

Rev.	Issue Date	Revisions	Effect Page	Revised By
00	June 28, 2021	Initial Issue	ALL	Polly Wang



TABLE OF CONTENTS

1. TEST REPORT CERTIFICATION	4
2. TEST RESULT SUMMARY	5
3. EUT DESCRIPTION.....	6
3.1 DESCRIPTION OF EUT & POWER	6
4. DESCRIPTION OF TEST MODES.....	7
5. TEST METHODOLOGY.....	8
6. FACILITIES AND ACCREDITATIONS	8
6.1 FACILITIES.....	8
6.2 EQUIPMENT.....	8
6.3 LABORATORY ACCREDITATIONS LISTINGS	8
6.4 TABLE OF ACCREDITATIONS AND LISTINGS	9
7. CALIBRATION AND UNCERTAINTY	10
7.1 MEASURING INSTRUMENT CALIBRATION.....	11
7.2 MEASUREMENT UNCERTAINTY.....	11
8. SETUP OF EQUIPMENT UNDER TEST	12
8.1 SETUP CONFIGURATION OF EUT.....	12
8.2 SUPPORT EQUIPMENT	13
8.3 EUT OPERATING CONDITION.....	14
9. APPLICABLE LIMITS AND TEST RESULTS	15
9.1 6dB BANDWIDTH	15
9.2 MAXIMUM PEAK OUTPUT POWER.....	19
9.3 DUTY CYCLE	25
9.4 POWER SPECTRAL DENSITY	29
9.5 CONDUCTED SPURIOUS EMISSION	33
9.6 RADIATED EMISSIONS	39
9.7 POWERLINE CONDUCTED EMISSIONS.....	53
10. ANTENNA REQUIREMENT	55
10.1 STANDARD APPLICABLE	55
10.2 ANTENNA CONNECTED CONSTRUCTION	55
APPENDIX I SETUP PHOTOS.....	56

1. TEST REPORT CERTIFICATION

Applicant Sound Land Corporation
No.32, Keji 1st Rd., Guishan Dist., Taoyuan City 33383,
Taiwan

Manufacturer Sound Land Corporation
No.32, Keji 1st Rd., Guishan Dist., Taoyuan City 33383,
Taiwan

Equipment Under Test Electronic Stethoscope

Model Number ES-2020

Data Applies To N/A

Brand Name ibiomed

Date of Test December 31, 2020 ~ January 05, 2021

APPLICABLE STANDARD	
STANDARD	TEST RESULT
FCC Part 15 Subpart C AND ANSI C63.10: 2013	No non-compliance noted

Statements of Conformity
Determining compliance shall be based on the results of the compliance measurement, not taking into account measurement instrumentation uncertainty.

Approved by:



Eric Huang
Section Manager



Report No.: T201207N01-RP1-2

Page: 5 / 59
Rev.: 00

2. TEST RESULT SUMMARY

FCC Standard Section	Report Section	Test Item	Result
15.247(a)	9.1	6dB BANDWIDTH	Pass
15.247(b)	9.2	MAXIMUM PEAK OUTPUT POWER	Pass
-	9.3	DUTY CYCLE	-
15.247(e)	9.4	POWER SPECTRAL DENSITY	Pass
15.247(d)	9.5	CONDUCTED SPURIOUS EMISSION	Pass
15.205(a)	9.6	RADIATED EMISSIONS	Pass
15.207(a)	9.7	POWERLINE CONDUCTED EMISSIONS	N/A
15.203	10	ANTENNA REQUIREMENT	Pass

3. EUT DESCRIPTION

3.1 DESCRIPTION OF EUT & POWER

Product Name	Electronic Stethoscope
Model Number	ES-2020
Data Applies To	N/A
Brand Name	ibiomedi
Received Date	December 07, 2020
Reported Date	January 15, 2021
Operating Frequency Range	DSSS (4.0) Mode: 2402MHz~2480MHz
Transmit Power	GFSK(4.0) Mode: 5.75dBm (3.754mW)
Channel Spacing	GFSK(4.0) Mode: 2 MHz
Channel Number	GFSK(4.0) Mode: 40 Channels
Transmit Data Rate	GFSK(4.0) Mode: 1 Mbps
Type of Modulation	GFSK
Antenna Type	Type: PCB antenna Model: KB64A/B/C Gain: 0.11 dBi Manufacturer: Kirchhoff Technology Co., Ltd
Power Source	DC 3V, 0.1A (Powered by battery)
Firmware Version	ES-2020 V1.00
Software Version	ES-2020 V1.00

REMARK:

1. The sample selected for test was engineering sample that approximated to production product and was provided by manufacturer.
2. This submittal(s) (test report) is intended for FCC ID: **2AYQY-ES-2020** filing to comply with Section 15.207, 15.209 and 15.247 of the FCC Part 15, Subpart C Rules.
3. For more details, please refer to the user manual.

4. DESCRIPTION OF TEST MODES

The EUT is a Electronic Stethoscope .

The RF Chip is manufactured by Kirchhoff Technology Co., Ltd

The antenna peak gain 0.11 dBi (highest gain) were chosen for full testing.

GFSK(4.0) mode

The EUT had been tested under operating condition.

There are three channels have been tested as following:

Channel	Frequency (MHz)
Low	2402
Middle	2442
High	2480

GFSK(4.0) mode: 1Mbps long data rates (worst case) were chosen for full testing.

5. TEST METHODOLOGY

The tests documented in this report were performed in accordance with ANSI C63.10 and FCC CFR 47 15.207, 15.209 and 15.247 and KdB 558074.

6. FACILITIES AND ACCREDITATIONS

6.1 FACILITIES

All measurement facilities used to collect the measurement data are located at No.8, Jiucengling, Xinhua Dist., Tainan City 712, Taiwan (R.O.C.)

The sites are constructed in conformance with the requirements of ANSI C63.7:1992, ANSI C63.10: 2013 and CISPR Publication 22.

6.2 EQUIPMENT

Radiated emissions are measured with one or more of the following types of linearly polarized antennas: tuned dipole, biconical, log periodic, bi-log, and/or ridged waveguide, horn. Spectrum analyzers with preselectors and quasi-peak detectors are used to perform radiated measurements.

Conducted emissions are measured with Line Impedance Stabilization Networks and EMI Test Receivers.

Calibrated wideband preamplifiers, coaxial cables, and coaxial attenuators are also used for making measurements.

All receiving equipment conforms to CISPR Publication 16-1, "Radio Interference Measuring Apparatus and Measurement Methods."

6.3 LABORATORY ACCREDITATIONS LISTINGS

The test facilities used to perform radiated and conducted emissions tests are accredited by Taiwan Accreditation Foundation for the specific scope of accreditation under Lab Code: 1109 to perform Electromagnetic Interference tests according to FCC PART 15 AND CISPR 22 requirements. No part of this report may be used to claim or imply product endorsement by TAF or any agency of the Government. In addition, the test facilities are listed with Federal Communications Commission (registration no: TW1109).



6.4 TABLE OF ACCREDITATIONS AND LISTINGS

Our laboratories are accredited and approved by the following accreditation body according to ISO/IEC 17025.

Taiwan

TAF

The measuring facility of laboratories has been authorized or registered by the following approval agencies.

Canada

Industry Canada (TW1109)

Germany

TUV NORD

Taiwan

BSMI

USA

FCC (TW1109)

Japan

VCCI

Copies of granted accreditation certificates are available for downloading from our web site,

<http://www.ccsrf.com>

6.5 MEASUREMENT EQUIPMENT USED

For §9.6

Chamber 966 Room (Radiation Test)					
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Date	Calibration Due
Active Loop Antenna	ETS-LINDREN	6502	8905-2356	08/02/2019	08/01/2021
Bilog Antenna With 6dB Attenuator	SUNOL SCIENCES & EMC	JB1 & AT-N0681	A070506-1 & AT-N0681	09/14/2020	09/13/2021
Cable	Suhner	SUCOFLEX104PEA	20520/4PEA&O6	01/30/2020	01/29/2021
Double Ridged Guide Horn Antenna	ETS-LINDGREN	3116	00078900	03/26/2020	03/25/2021
EMI Test Receiver	R&S	ESCI	100960	02/11/2020	02/10/2021
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	07/20/2020	07/19/2021
Horn Antenna	Com-Power	AH-118	071032	04/29/2020	04/28/2021
Pre-Amplifier	EMCI	EMC012645	980098	01/30/2020	01/29/2021
Pre-Amplifier	HP	8447F	2443A01683	01/22/2020	01/21/2021
Pre-Amplifier	Com-Power	PAM-840A	461378	07/20/2020	07/19/2021
Type N coaxial cable	Suhner	CHA9513	6	01/21/2020	01/20/2021
Notch Filter	MICRO-TRONICS	BRM50702-01	018	N.C.R	N.C.R
Test S/W	Excel(ccs-o6-2020 v1.1) e3(6.101222)				

For §9.1~9.5

Chamber 966 Room (Conducted Test)					
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Date	Calibration Due
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	07/20/2020	07/19/2021
Power Meter	Anritsu	ML2487A	6K00003888	11/20/2019	05/19/2021
Power Sensor	Anritsu	MA2491A	033265	11/20/2019	05/19/2021
SMA Cable + 10dB Attenuator	CCS	SMA+10dB ATT	SMA/10dB	01/30/2020	01/29/2021
Test S/W	Excel(ccs-o6-2020 v1.1)				

For §9.7

Conducted Emission room #1					
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Date	Calibration Due
-	-	-	-	-	-
-	-	-	-	-	-
-	-	-	-	-	-
-	-	-	-	-	-
-	-	-	-	-	-
Test S/W	-				

7. CALIBRATION AND UNCERTAINTY

7.1 MEASURING INSTRUMENT CALIBRATION

The measuring equipment utilized to perform the tests documented in this report has been calibrated in accordance with the manufacturer's recommendations, and is traceable to recognized national standards.

7.2 MEASUREMENT UNCERTAINTY

Where relevant, the following measurement uncertainty levels have been estimated for tests performed on the apparatus:

PARAMETER	UNCERTAINTY
Radiated Emission, 30 to 200 MHz Test Site : OATS-6	$\pm 3.3456\text{dB}$
Radiated Emission, 200 to 1000 MHz Test Site : OATS-6	$\pm 2.6828\text{dB}$
Radiated Emission, 1 to 8 GHz	$\pm 2.6485\text{dB}$
Radiated Emission, 8 to 18 GHz	$\pm 2.6852\text{dB}$
Radiated Emission, 18 to 26.5 GHz	$\pm 2.6485\text{dB}$
Radiated Emission, 26 to 40 GHz	$\pm 3.0295\text{dB}$
Power Line Conducted Emission	$\pm 1.91\text{dB}$
Band Width	136.49kHz
Peak Output Power MU	$\pm 1.904\text{dB}$
Band Edge MU	$\pm 0.302\text{dBuV}$
Channel Separation MU	361.69Hz
Duty Cycle MU	0.064ms
Frequency Stability MU	0.223kHz


This measurement uncertainty is confidence of approximately 95%, $k=2$

8. SETUP OF EQUIPMENT UNDER TEST


8.1 SETUP CONFIGURATION OF EUT

EMI


【Bluetooth】

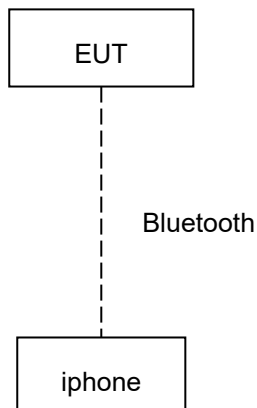

【LINK】

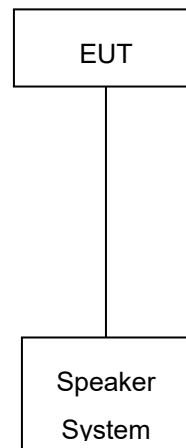

RF

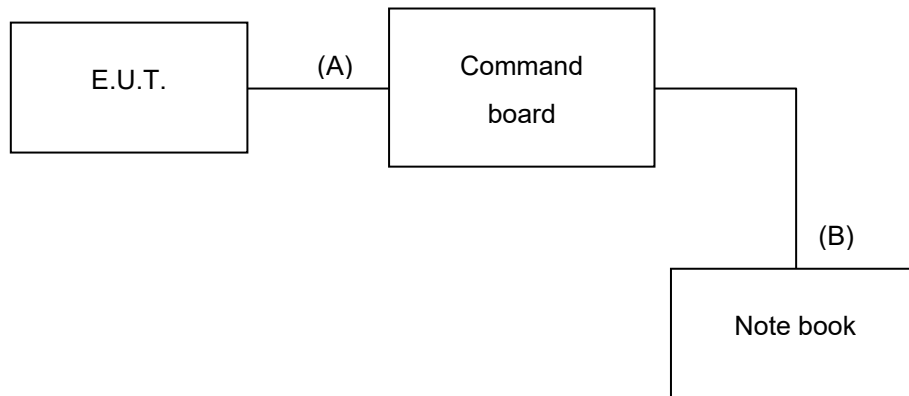

8.2 SUPPORT EQUIPMENT

For EMI test

No.	Product	Manufacturer	Model No.	Certify No.	Signal cable
1	Speaker System	T.C.SATR	TCS2285	DOC	Unshielded, 1.6m.
2	iPhone	Apple	N/A	N/A	N/A

No.	Signal cable description	
A	Audio	Shielded, 1.0m 1 pcs

For RF test

No.	Product	Manufacturer	Model No.	Certify No.	Signal cable
1	Note Book	Acer	Z5WE1	DOC	Unshielded, 1.8m, with 1 core.

No.	Signal cable description	
A	Command cable	Unshielded, 0.2m 1 pcs.
B	USB	Shielded, 0.8m 1 pcs.

Note:

- 1) All the equipment/cables were placed in the worst-case configuration to maximize the emission during the test.
- 2) Grounding was established in accordance with the manufacturer's requirements and conditions for the intended use.
- 3) shd. = shielded; unshd. = unshielded



Report No.: T201207N01-RP1-2

Page: 14 / 59
Rev.: 00

8.3 EUT OPERATING CONDITION

RF Setup

1. Set up all computers like the setup diagram.
2. The "CSR BlueSuite 2.6.4", "Blue Test 3" software was used for testing.
3. Choose Transport "SPI" and Port "USB SPI (1003512)"

TX Mode:

BLE TEST TX :

Channel > 0 (0-39)

Length > 37

Bit pattern > 0

RX Mode:

BLE TEST RX

4. All of the function are under run.
5. Start test.

9. APPLICABLE LIMITS AND TEST RESULTS

9.1 6dB BANDWIDTH

LIMIT

§ 15.207(a) (2) For direct sequence systems, the minimum 6dB bandwidth shall be at least 500kHz

TEST SETUP



TEST PROCEDURE

- a) Set RBW = 100 kHz.
- b) Set the video bandwidth (VBW) ≥ 3 RBW.
- c) Detector = Peak.
- d) Trace mode = max hold.
- e) Sweep = auto couple.
- f) Allow the trace to stabilize.
- g) Measure the maximum width of the emission that is constrained by the frequencies associated with the two outermost amplitude points (upper and lower frequencies) that are attenuated by 6 dB relative to the maximum level measured in the fundamental emission.

TEST RESULTS

No non-compliance noted.

Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31


GFSK(4.0) mode


Channel	Channel Frequency (MHz)	6dB Bandwidth (kHz)	Minimum Limit (kHz)	Pass / Fail
Low	2402	701.00	500	PASS
Middle	2442	697.00	500	PASS
High	2480	698.00	500	PASS

NOTE :

1. At final test to get the worst-case emission at 1Mbps long.
2. The cable assembly insertion loss of 11.1dB (including 10 dB pad and 1.1 dB cable) was entered as an offset in the spectrum analyzer to allow for direct reading of power.

6dB BANDWIDTH (GFSK(4.0) MODE)

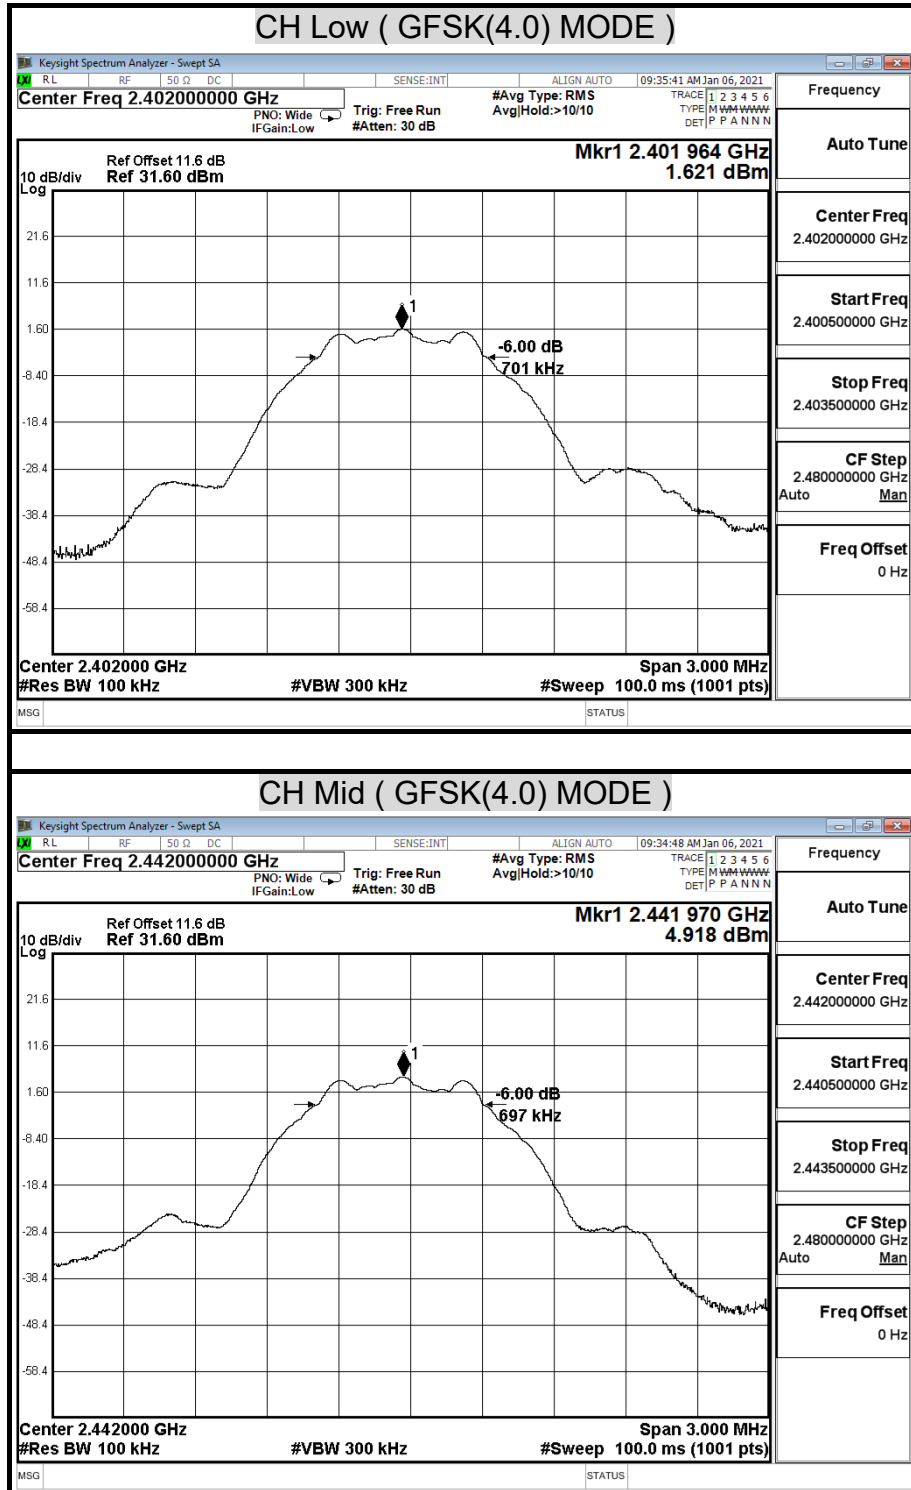

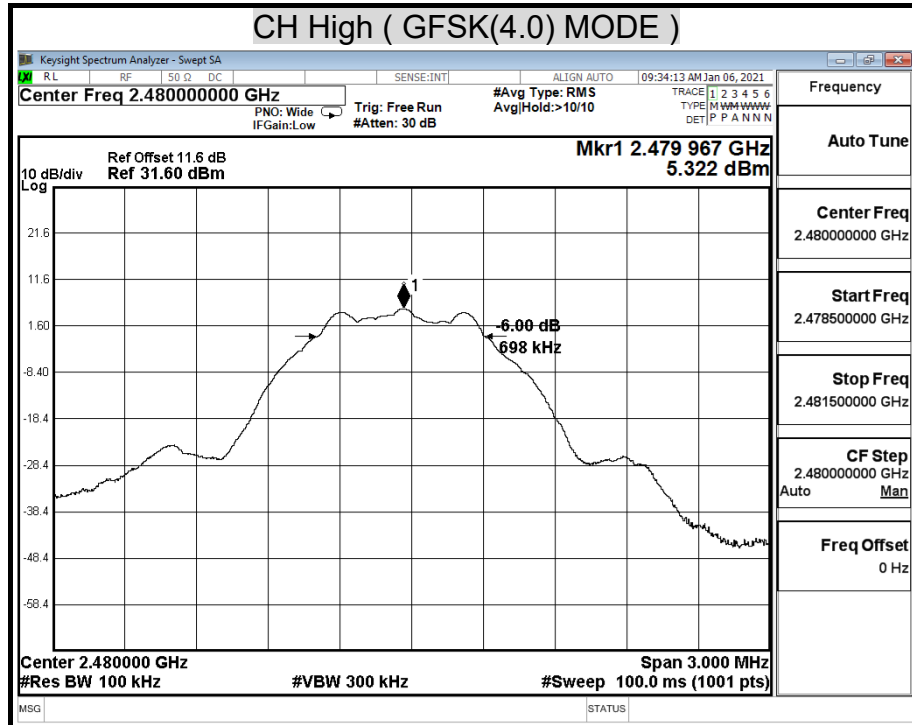

9.2 MAXIMUM PEAK OUTPUT POWER

LIMIT


§ 15.247(b) The maximum peak output power of the intentional radiator shall not exceed the following :

§ 15.247(b) (3) For systems using digital modulation in the 902-928 MHz, 2400-2483.5 MHz, and 5725-5850 MHz bands : 1 watt.

§ 15.247(b) (4) Except as shown in paragraphs (c) of this section , if transmitting antennas of directional gain greater than 6 dBi are used the peak output power from the intentional radiator shall be reduced below the stated values in paragraphs (b)(1) or (b)(2), and (b)(3) of this section , as appropriate, by the amount in dB that the directional gain of the antenna exceeds 6 dBi.

TEST SETUP

For Peak Power

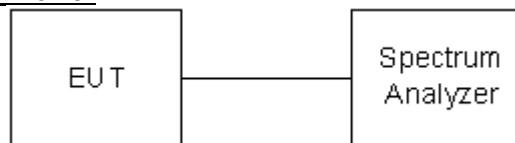

For Average Power





Report No.: T201207N01-RP1-2

Page: 20 / 59
Rev.: 00

TEST PROCEDURE

The tests were performed in accordance with KDB 558074 D01 v05r02 and ANSI C63.10-2013, 11.9.1.1.

9.2.1 Measurement Procedure :

- a) Set the RBW $\geq$ DTS bandwidth.
- b) Set VBW $\geq$ 3 RBW.
- c) Set span $\geq$ 3 x RBW
- d) Sweep time = auto couple.
- e) Detector = peak.
- f) Trace mode = max hold.
- g) Allow trace to fully stabilize.
- h) Use peak marker function to determine the peak amplitude level.

Average Power

The tests were performed in accordance with ANSI C63.11 9.2.3.1.

Connect the EUT to power meter, set the center frequency of the power meter to the channel center frequency.

TEST RESULTS

No non-compliance noted.

Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31

GFSK(4.0) mode

Channel	Channel Frequency (MHz)	Peak Power (dBm)	Peak Power Limit (dBm)	Pass / Fail
Low	2402	2.10	30.00	PASS
Middle	2442	5.37	30.00	PASS
High	2480	5.75	30.00	PASS

NOTE : 1. At final test to get the worst-case emission at 1Mbps long.
2. The cable assembly insertion loss of 11.1dB (including 10 dB pad and 1.1 dB cable) was entered as an offset in the power meter to allow for direct reading of power.



Report No.: T201207N01-RP1-2

Page: 22 / 59
Rev.: 00

Average Power Data


Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31


GFSK(4.0) mode

Channel	Channel Frequency (MHz)	Measure Power (dBm)	10 log (1 / D)	Average Power (dBm)
Low	2402	-0.50	2.109	1.61
Middle	2442	2.85	2.109	4.96
High	2480	3.33	2.109	5.44

Note: *D is duty cycle.

MAXIMUM PEAK OUTPUT POWER (GFSK(4.0) MODE)

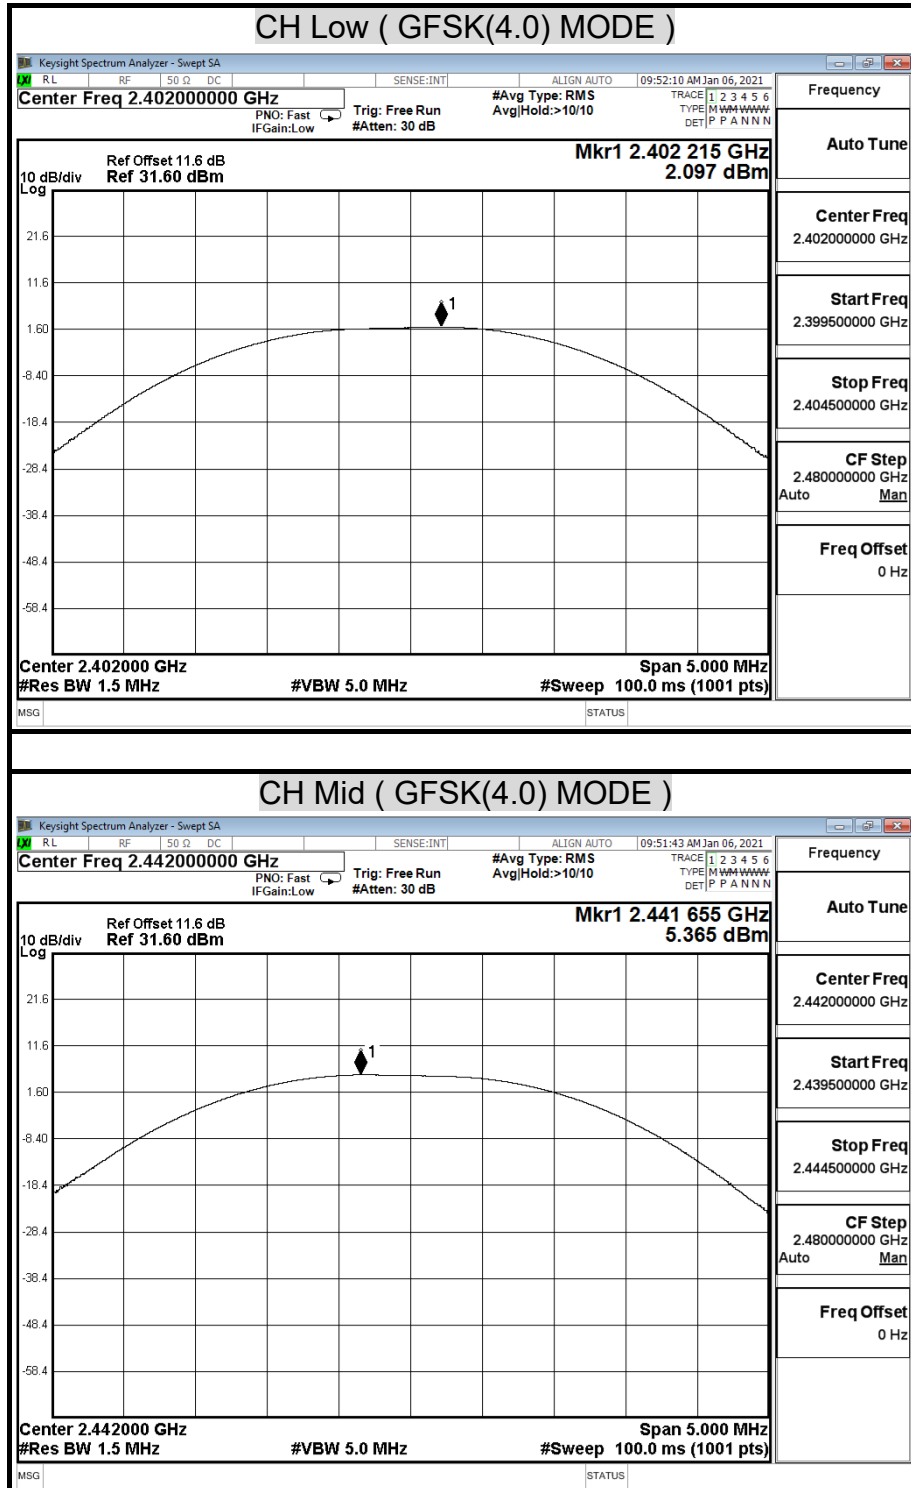

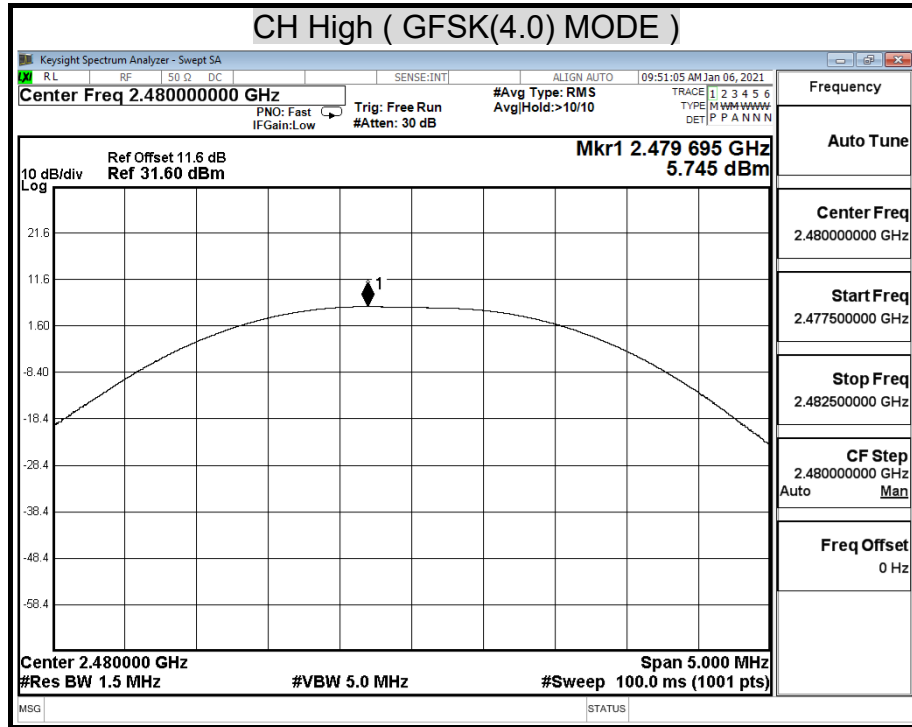

9.3 DUTY CYCLE

LIMIT

Nil (No dedicated limit specified in the Rules)

TEST SETUP



TEST PROCEDURE

1. Place the EUT on the table and set it in transmitting mode.
2. Remove the antenna from the EUT and then connect a low loss RF cable from the antenna port to the spectrum analyzer.
3. The zero-span mode on a spectrum analyzer or EMI receiver if the response time and spacing between bins on the sweep are sufficient to permit accurate measurements of the on and off times of the transmitted signal. Set the center frequency of the instrument to the center frequency of the transmission. Set RBW $\geq$ OBW if possible; otherwise, set RBW to the largest available value. Set VBW $\geq$ RBW. Set detector = peak or average. The zero-span measurement method shall not be used unless both RBW and VBW are $> 50/T$ and the number of sweep points across duration T exceeds 100. (For example, if VBW and/or RBW are limited to 3 MHz, then the zero-span method of measuring duty cycle shall not be used if $T \leq 16.7$ microseconds.)

TEST RESULTS

No non-compliance noted.

Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31


GFSK(4.0) Mode

	us	Times	Ton	Total Ton time(ms)
Ton1	400.000	1	400	
Ton2		0	0	
Ton3			0	0.4
Tp				0.65

Ton	0.4
Tp(Ton+Toff)	0.65
Duty Cycle	0.62
Duty Factor	2.109

TEST PLOT


Duty Cycle

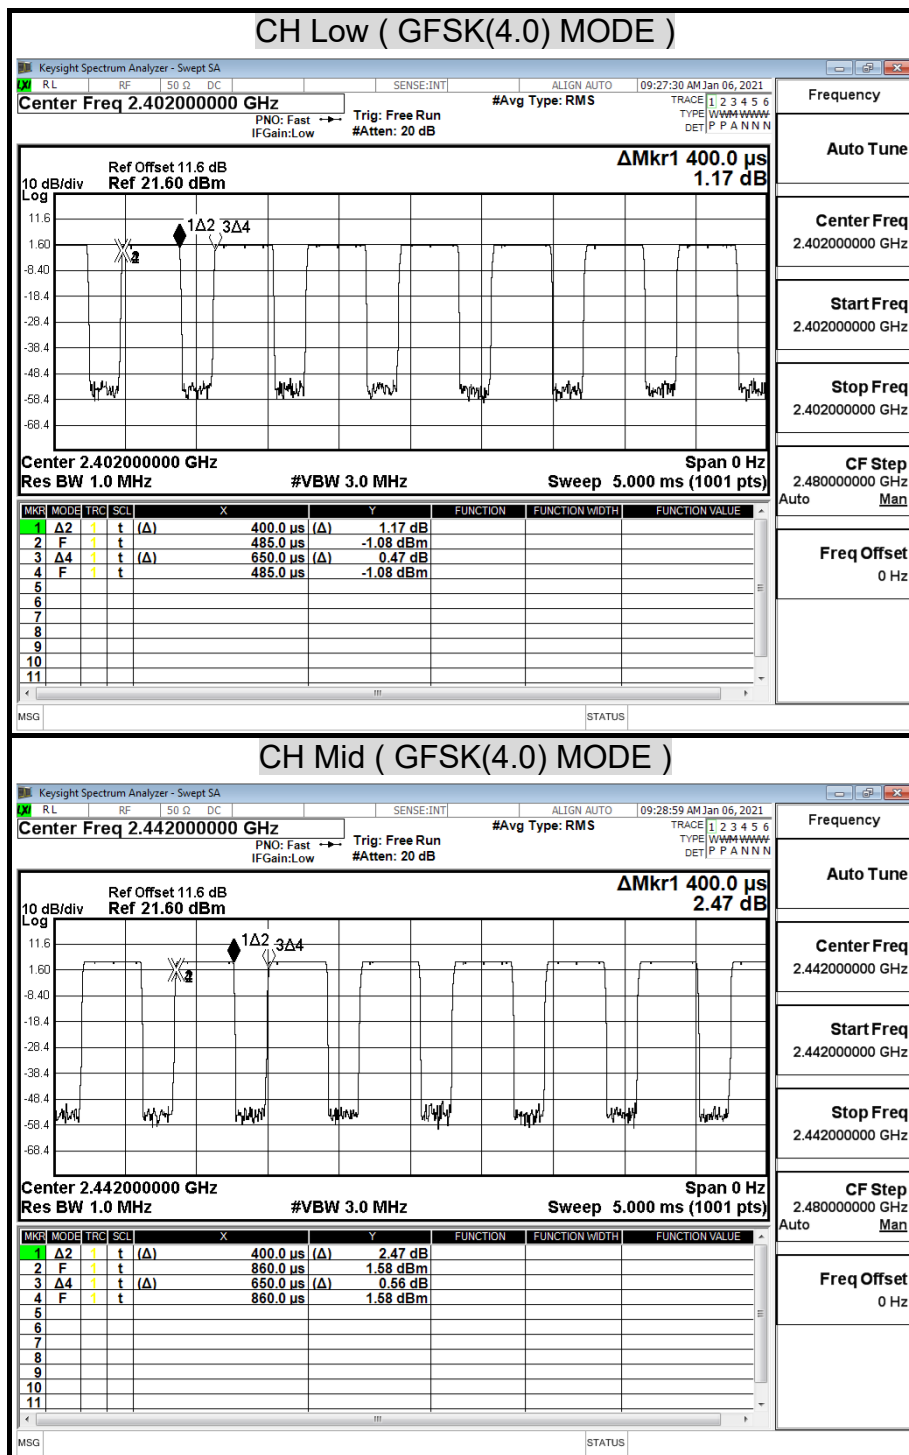



Report No.: T201207N01-RP1-2

Page: 28 / 59
Rev.: 00

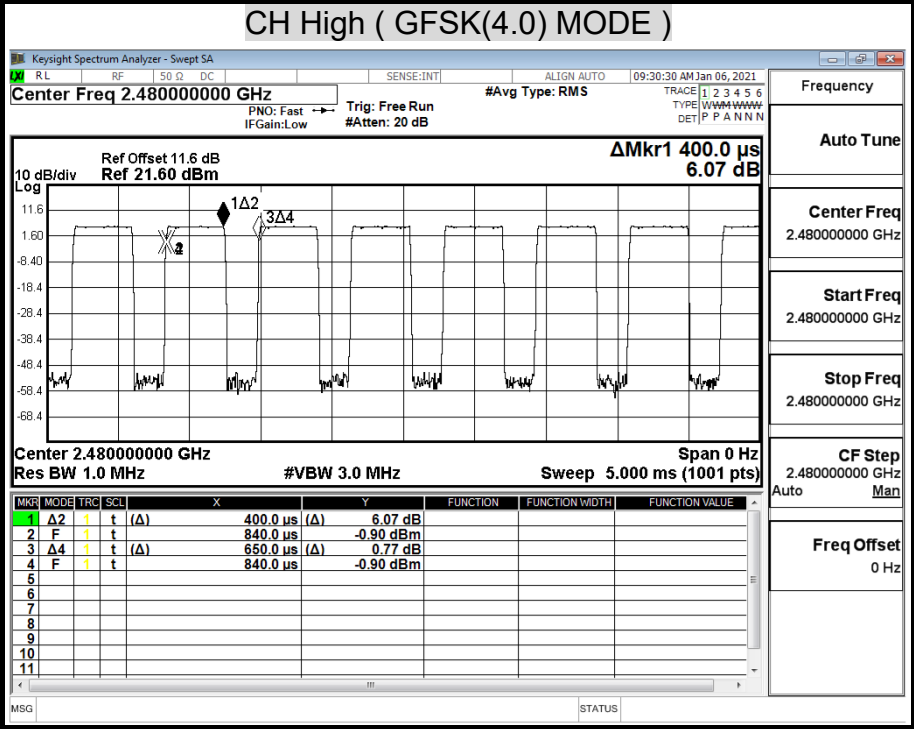


9.4 POWER SPECTRAL DENSITY

LIMIT

§ 15.247(e) For digitally modulated systems, the power spectral density conducted from the intentional radiator to the antenna shall not greater than 8 dBm in any 3 kHz band during any time interval of continuous transmission.

TEST SETUP

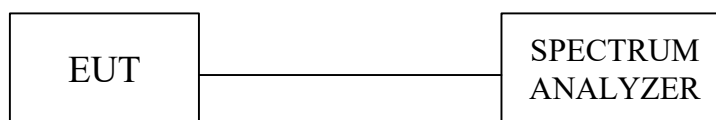

TEST PROCEDURE

The tests were performed in accordance with KDB 8.4 (ANSI C63.10, 11.10.2)

10.2 Method PKPSD (peak PSD):

1. Set analyzer center frequency to DTS channel center frequency.
2. Set the span to 1.5 times the DTS bandwidth.
3. Set the RBW to: $3 \text{ kHz} \leq \text{RBW} \leq 100 \text{ kHz}$.
4. Set the VBW $\geq 3 \text{ RBW}$.
5. Detector = peak.
6. Sweep time = auto couple.
7. Trace mode = max hold.
8. Allow trace to fully stabilize.
9. Use the peak marker function to determine the maximum amplitude level within the RBW.
10. If measured value exceeds limit, reduce RBW (no less than 3 kHz) and repeat.

TEST RESULTS

No non-compliance noted.


Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31


GFSK(4.0) mode

Channel	Frequency (MHz)	PPSD/3kHz (dBm)	Limit (dBm)	Margin (dB)	Result
Low	2402	-13.73	8.00	-21.73	PASS
Middle	2442	-10.32	8.00	-18.32	PASS
High	2480	-9.79	8.00	-17.79	PASS

NOTE : 1. At final test to get the worst-case emission at 1Mbps long.
2. The cable assembly insertion loss of 11.1dB (including 10 dB pad and 1.1 dB cable) was Entered as an offset in the spectrum analyzer to allow for direct reading of power.

POWER SPECTRAL DENSITY (GFSK(4.0) MODE)

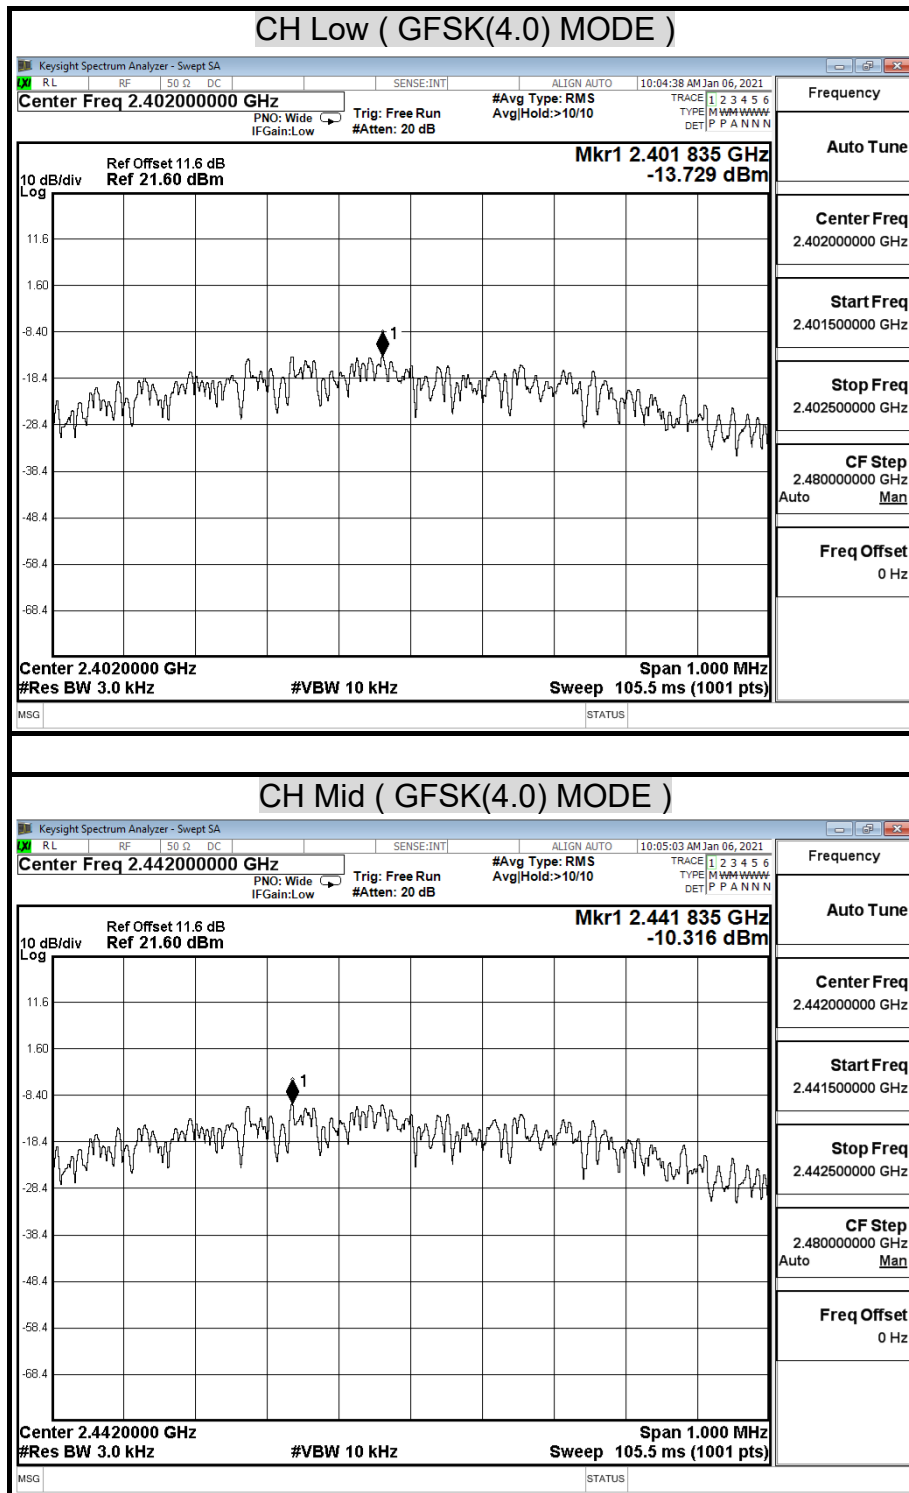

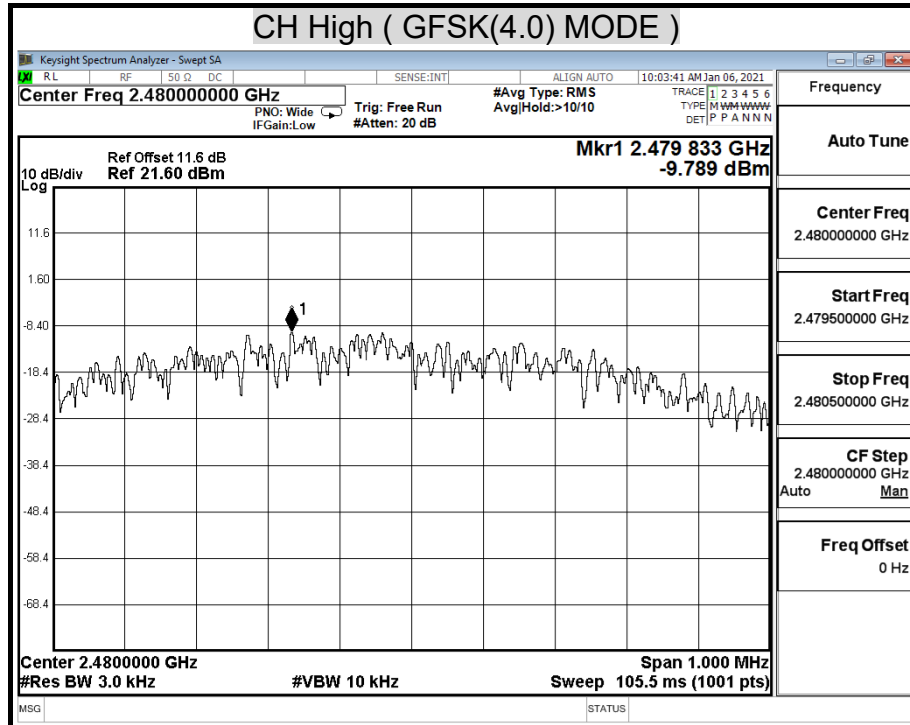

9.5 CONDUCTED SPURIOUS EMISSION

LIMITS

§ 15.247(d) In any 100 kHz bandwidth outside the frequency band in which the spread spectrum intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement. Attenuation below the general limits specified in § 15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in § 15.205(a), must also comply with the radiated emission limits specified in § 15.209(a) (see § 15.205(c)).

TEST SETUP



TEST PROCEDURE

The transmitter output is connected to a spectrum analyzer. The resolution bandwidth is set to 100kHz. The video bandwidth is set to 300kHz.

The spectrum from 30 MHz to 26.5 GHz is investigated with the transmitter set to the lowest, middle, and highest channels in the 2.4 GHz band.


TEST RESULTS


No non-compliance noted.


TEST DATA


Model Name	ES-2020	Test By	Ted Huang
Temp & Humidity	22.5°C, 54%	Test Date	2020/12/31

OUT-OF-BAND SPURIOUS EMISSIONS-CONDUCTED MEASUREMENT

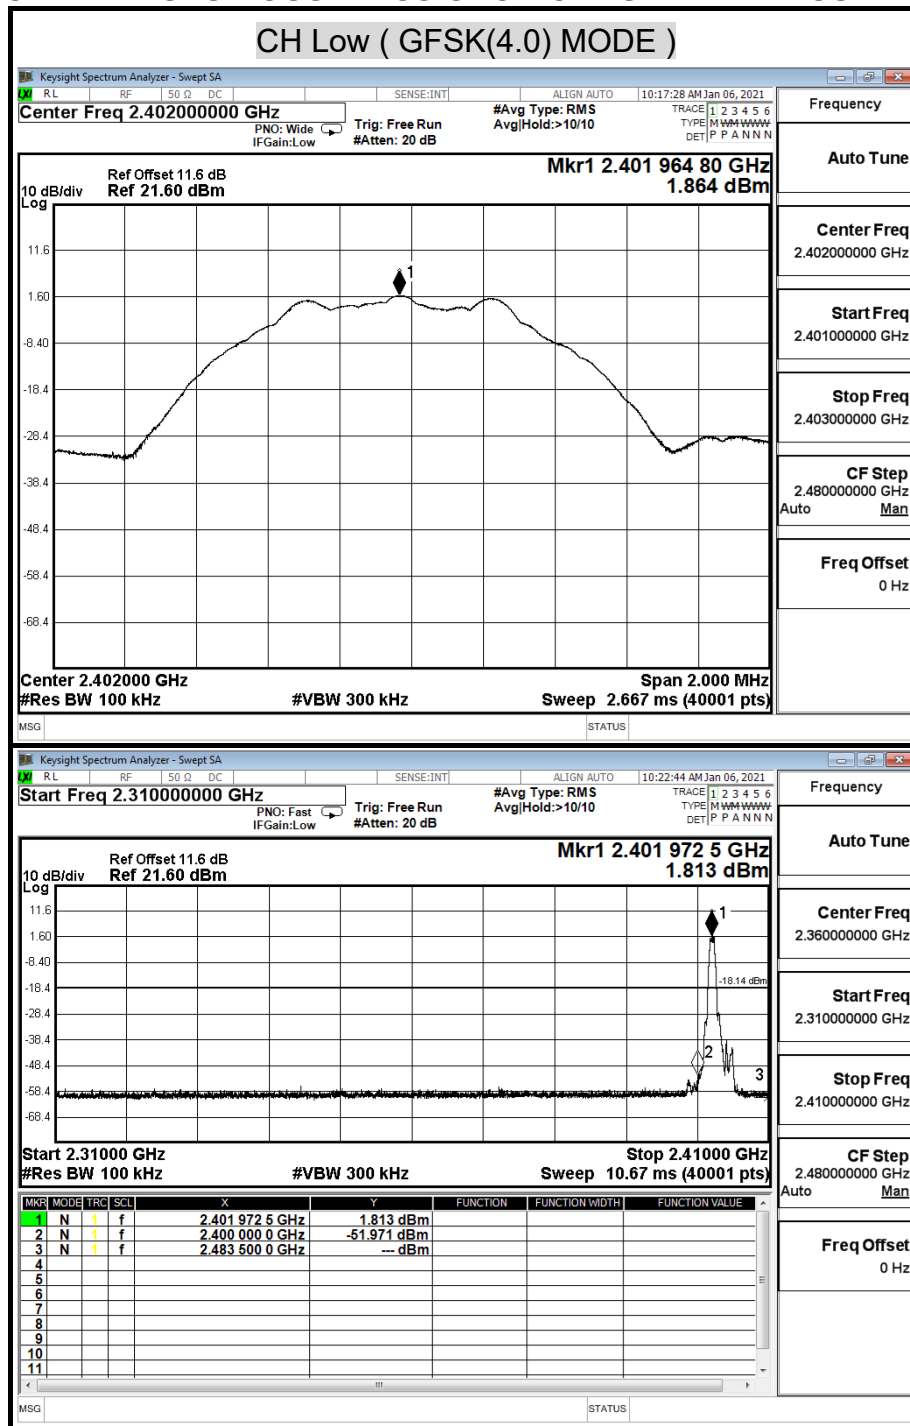

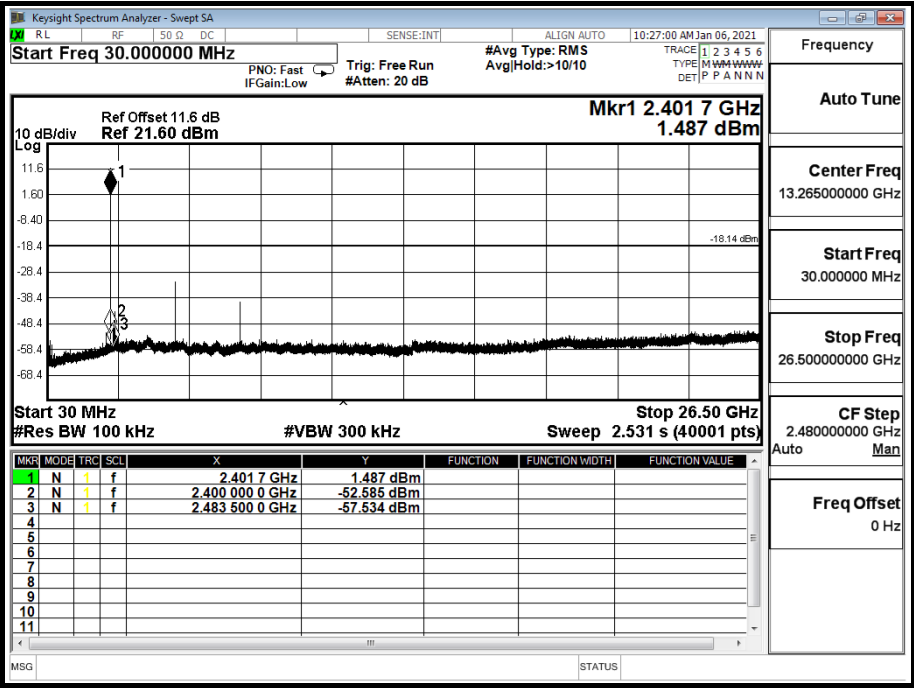

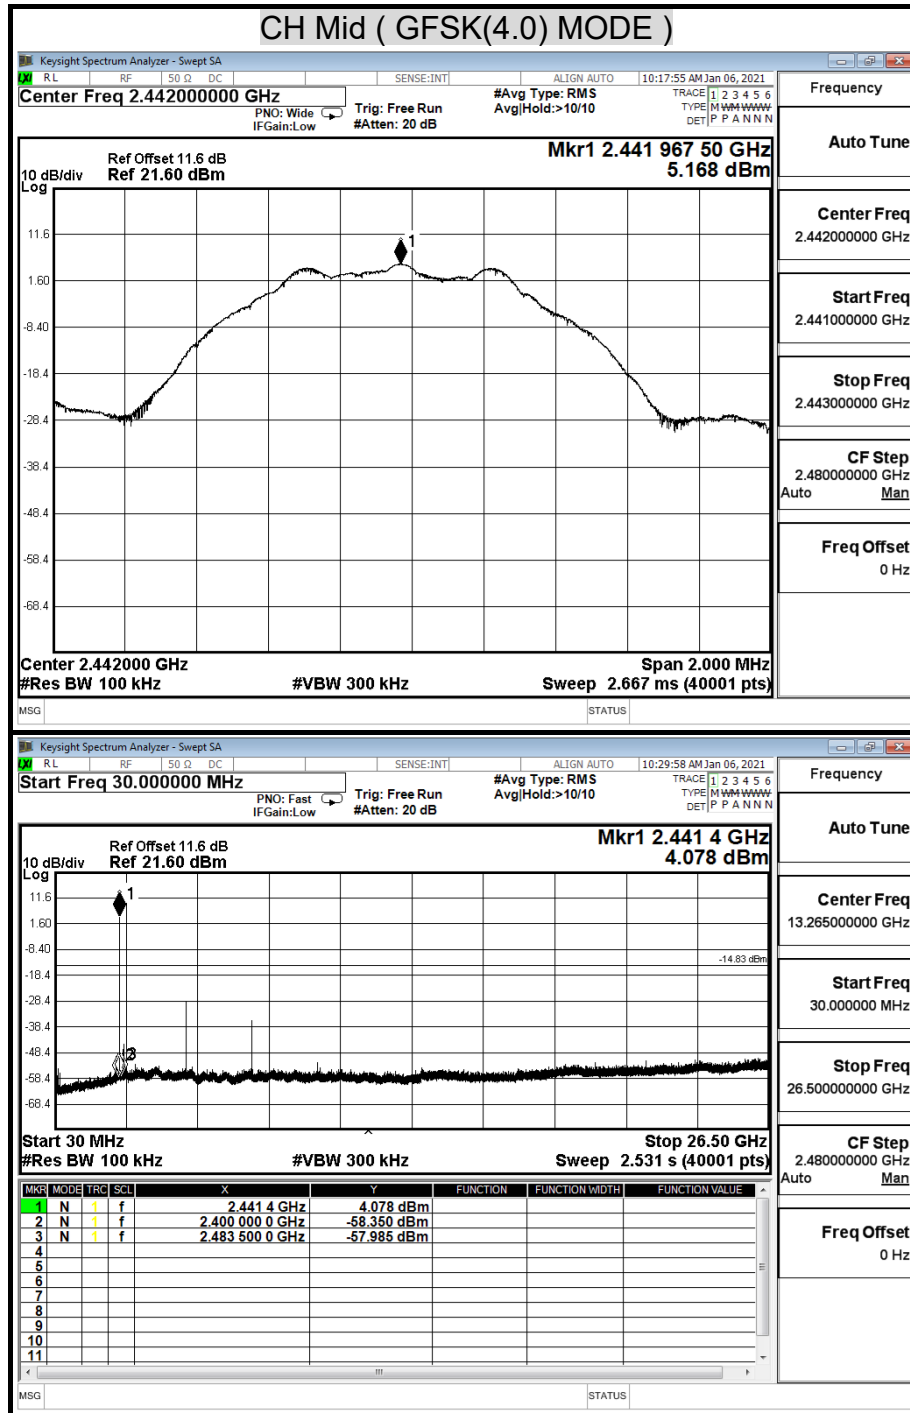


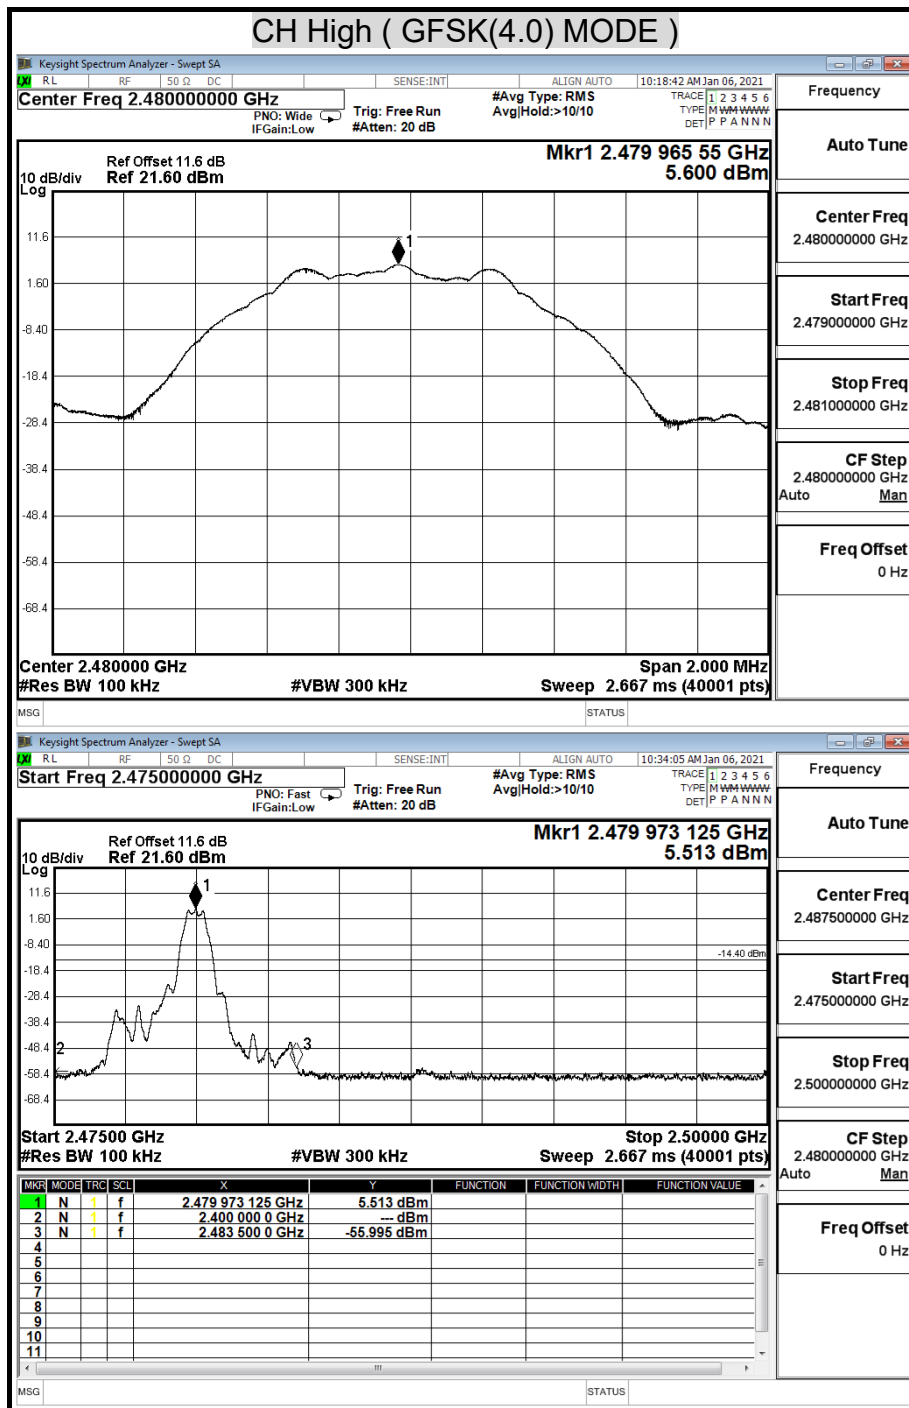



Report No.: T201207N01-RP1-2

Page: 38 / 59
Rev.: 00

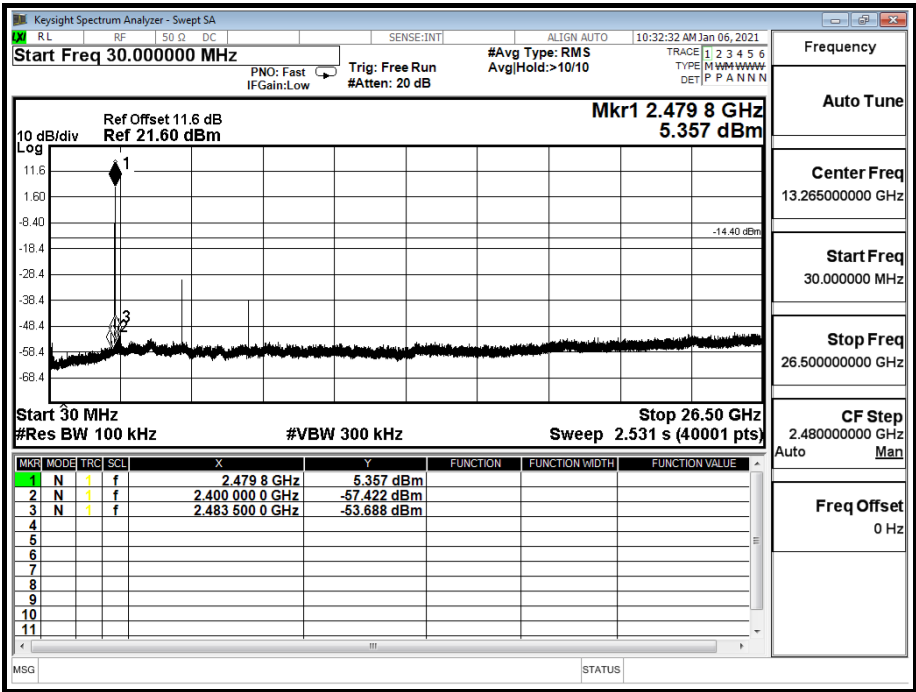

9.6 RADIATED EMISSIONS

9.6.1 TRANSMITTER RADIATED SUPURIOUS EMSSIONS

LIMITS

§ 15.205 (a) Except as shown in paragraph (d) of this section, only spurious emissions are permitted in any of the frequency bands listed below:

MHz	MHz	MHz	GHz
0.090 - 0.110	16.42 - 16.423	399.9 - 410	4.5 - 5.15
¹ 0.495 - 0.505	16.69475 - 16.69525	608 - 614	5.35 - 5.46
2.1735 - 2.1905	16.80425 - 16.80475	960 - 1240	7.25 - 7.75
4.125 - 4.128	25.5 - 25.67	1300 - 1427	8.025 - 8.5
4.17725 - 4.17775	37.5 - 38.25	1435 - 1626.5	9.0 - 9.2
4.20725 - 4.20775	73 - 74.6	1645.5 - 1646.5	9.3 - 9.5
6.215 - 6.218	74.8 - 75.2	1660 - 1710	10.6 - 12.7
6.26775 - 6.26825	108 - 121.94	1718.8 - 1722.2	13.25 - 13.4
6.31175 - 6.31225	123 - 138	2200 - 2300	14.47 - 14.5
8.291 - 8.294	149.9 - 150.05	2310 - 2390	15.35 - 16.2
8.362 - 8.366	156.52475 - 156.52525	2483.5 - 2500	17.7 - 21.4
8.37625 - 8.38675	156.7 - 156.9	2655 - 2900	22.01 - 23.12
8.41425 - 8.41475	162.0125 - 167.17	3260 - 3267	23.6 - 24.0
12.29 - 12.293	167.72 - 173.2	3332 - 3339	31.2 - 31.8
12.51975 - 12.52025	240 - 285	3345.8 - 3338	36.43 - 36.5
12.57675 - 12.57725	322 - 335.4	3600 - 4400	(²)
13.36 - 13.41			

¹ Until February 1, 1999, this restricted band shall be 0.490-0.510 MHz.

² Above 38.6

§ 15.205 (b) Except as provided in paragraphs (d) and (e), the field strength of emissions appearing within these frequency bands shall not exceed the limits shown in Section 15.209. At frequencies equal to or less than 1000 MHz, compliance with the limits in Section 15.209 shall be demonstrated using measurement instrumentation employing a CISPR quasi-peak detector. Above 1000 MHz, compliance with the emission limits in Section 15.209 shall be demonstrated based on the average value of the measured emissions. The provisions in Section 15.35 apply to these measurements.

§ 15.209 (a) Except as provided elsewhere in this Subpart, the emissions from an intentional radiator shall not exceed the field strength levels specified in the following table :

Frequency (MHz)	Field Strength (microvolts/meter)	Measurement Distance (meters)
30 - 88	100 **	3
88 - 216	150 **	3
216 - 960	200 **	3
Above 960	500	3


** Except as provided in paragraph (g), fundamental emissions from intentional radiators operating under this Section shall not be located in the frequency bands 54-72 MHz, 76-88 MHz, 174-216 MHz or 470-806 MHz, However, operation within these frequency bands is permitted under other sections of this Part, e-g, Sections 15.231 and 15.241.

§ 15.209 (b) In the emission table above, the tighter limit applies at the band edges.


TEST SETUP

The diagram below shows the test setup that is utilized to make the measurements for emission from below 1GHz.


9kHz ~ 30MHz

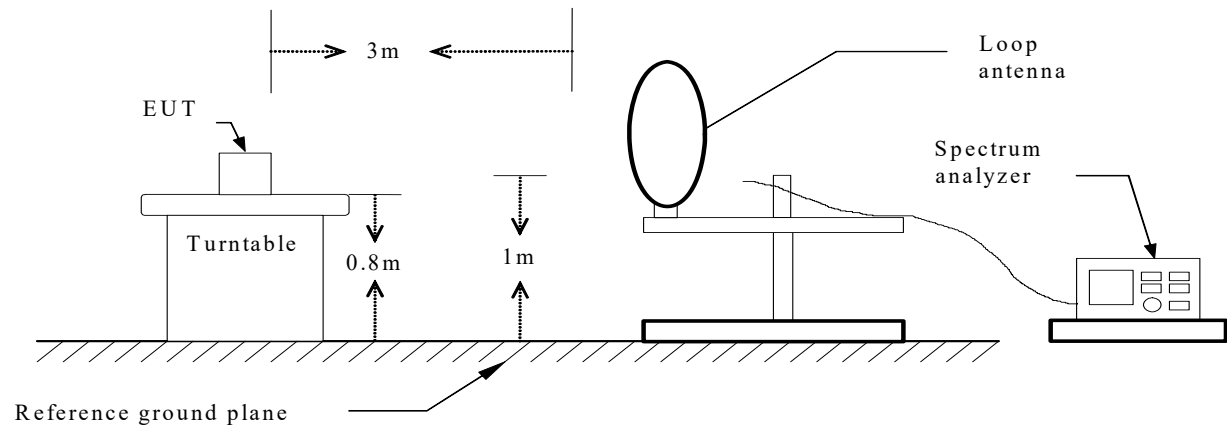

30MHz ~ 1GHz

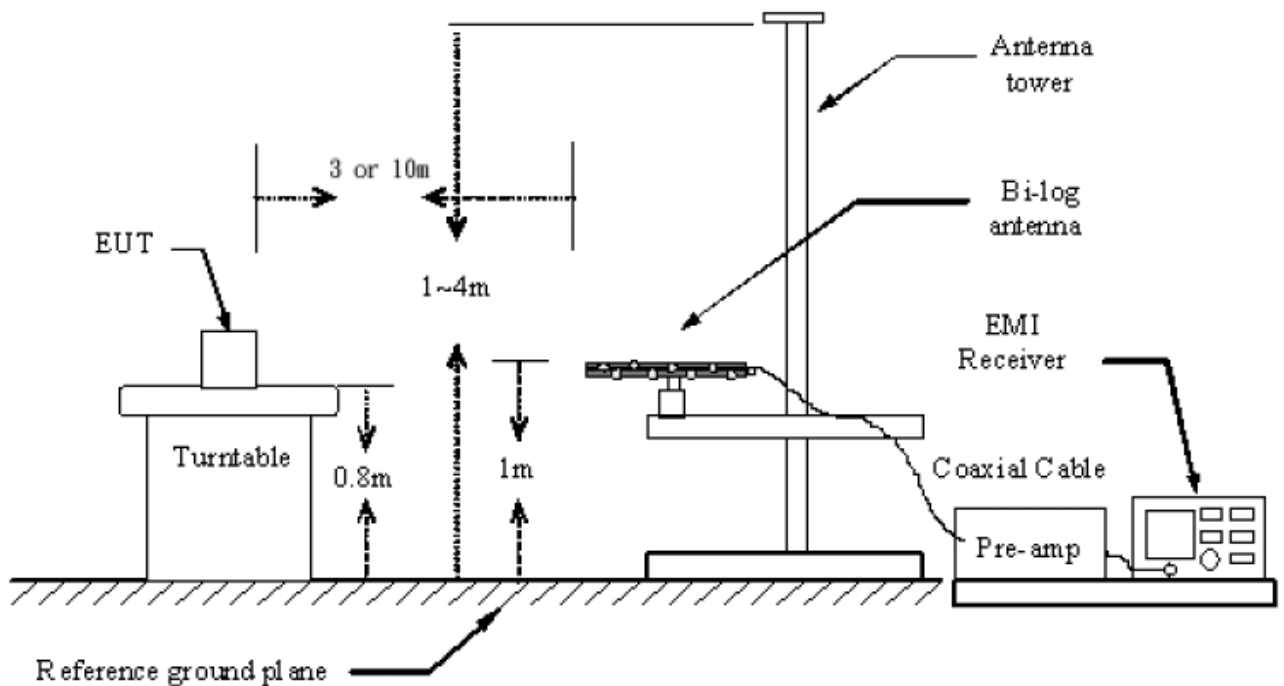

The diagram below shows the test setup that is utilized to make the measurements for emission above 1GHz.

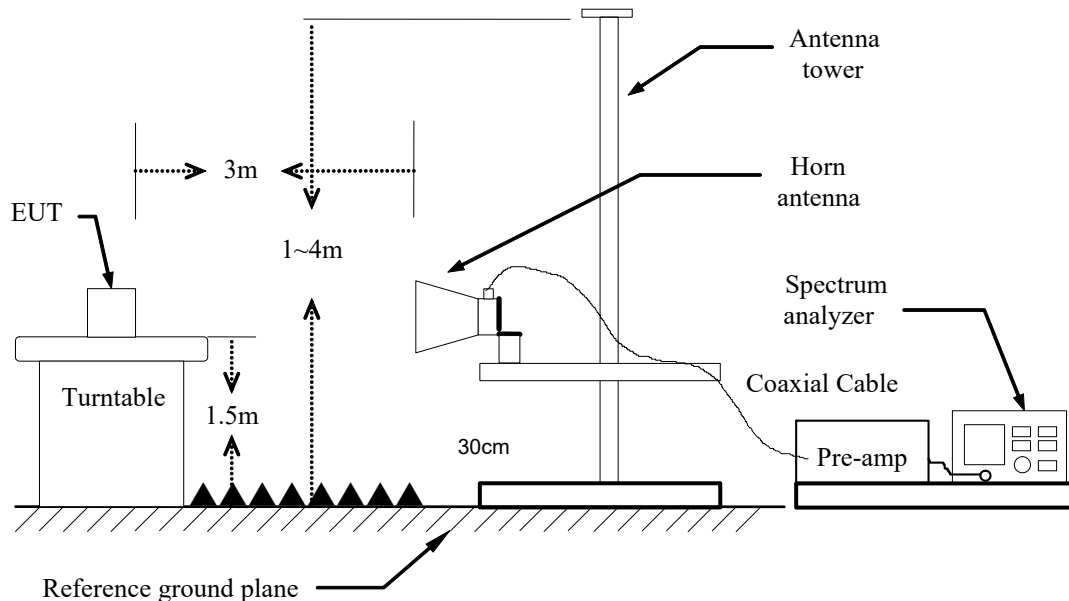

TEST PROCEDURE

- a. The EUT was placed on the top of a rotating table 0.8/1.5 meters above the ground at a 10 meter open area test site. The table was rotated 360 degrees to determine the position of the highest radiation.
- b. While measuring the radiated emission below 1GHz, the EUT was set 3 meters away from the interference-receiving antenna, which was mounted on the top of a variable-height antenna tower. While measuring the radiated emission above 1GHz, the EUT was set 3 meters away from the interference-receiving antenna.
- c. The antenna is a broadband antenna, and its height is varied from one meter to four meters above the ground to determine the maximum value of the field strength. Both horizontal and vertical polarization of the antenna are set to make the measurement.
- d. For each suspected emission, the EUT was arranged to its worst case and then the antenna was tuned to heights from 1 meter to 4 meters and the table was turned from 0 degrees to 360 degrees to find the maximum reading.
- e. The test-receiver system was set to Peak Detect Function and Specified Bandwidth with Maximum Hold Mode.
- f. If the emission level of the EUT in peak mode was 10 dB lower than the limit specified, then testing could be stopped and the peak values of the EUT would be reported. Otherwise the emissions that did not have 10 dB margin would be re-tested one by one using peak, quasi-peak or average method as specified and then reported in a data sheet.
- g. The tests were performed in accordance with 558074 D01 15.247 Meas Guidance v05

NOTE:

1. The resolution bandwidth and video bandwidth of test receiver/spectrum analyzer is 120 KHz for Peak detection (PK) and Quasi-peak detection (QP) at frequency below 1GHz.
2. The resolution bandwidth and video bandwidth of test receiver/spectrum analyzer is 1 MHz for Peak detection and frequency above 1GHz.
3. The resolution bandwidth of test receiver/spectrum analyzer is 1 MHz and the video bandwidth is 10 Hz for Average detection (AV) at frequency above 1GHz.
4. No emission is found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz)


TEST RESULTS

No non-compliance noted.

9.6.2 WORST-CASE RADIATED EMISSION BELOW 1 GHz

Product Name	Electronic Stethoscope	Test Date	2021/01/05
Model Name	ES-2020	Test By	Ted Huang
Test Mode	TX	Temp & Humidity	25.5°C, 53%

Vertical

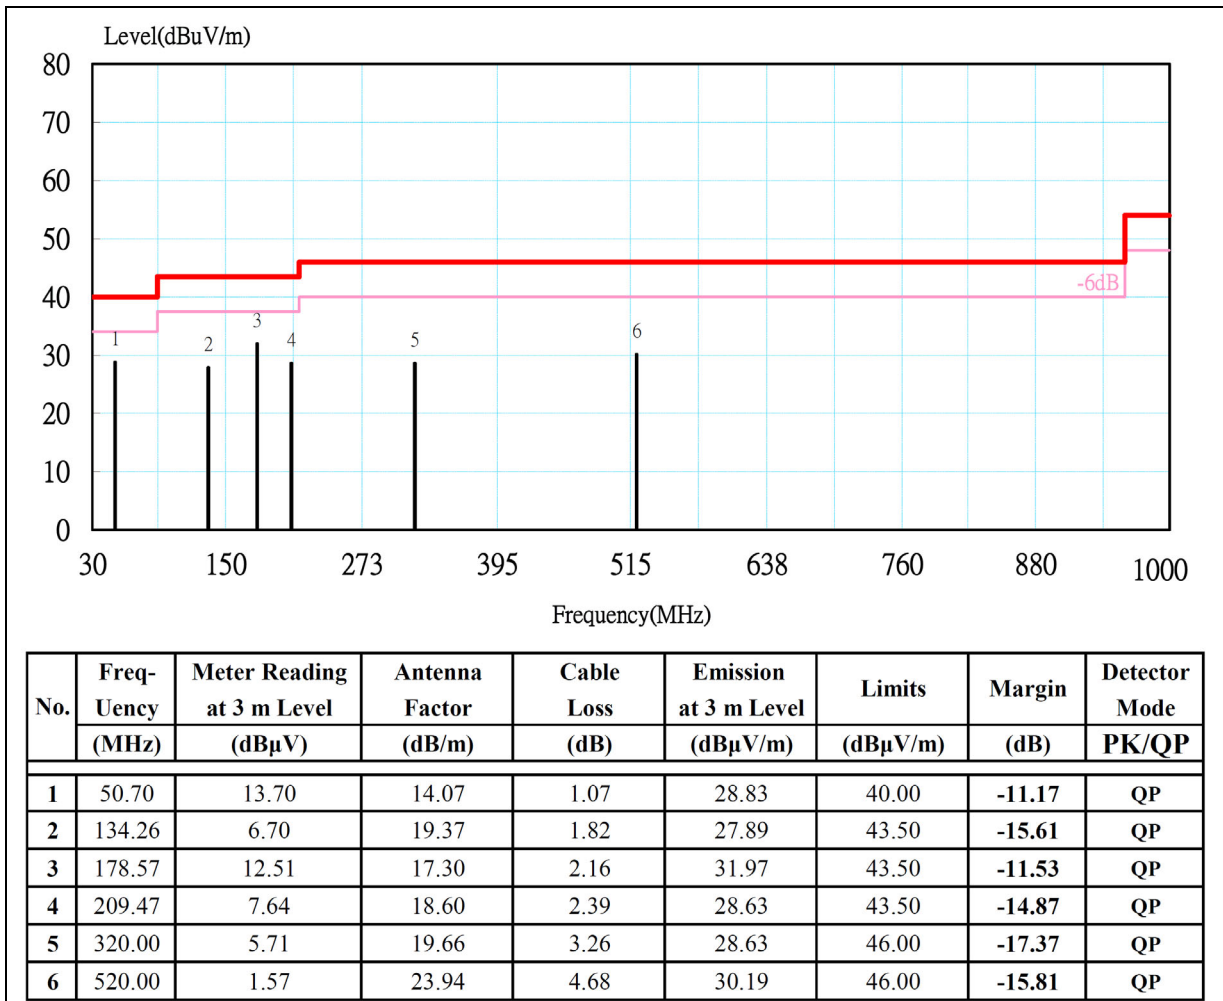


Remark:

- No emission found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz).
- Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using peak/quasi-peak detector mode.
- Quasi-peak test would be performed if the peak result were greater than the quasi-peak limit or as required by the applicant.
- Measurements above show only up to 6 maximum emissions noted, or would be lesser, with " N/A " remark, if no specific emissions from the EUT are recorded (ie: margin>20dB from the applicable limit) and considered that's already beyond the background noise floor.
- Emission at 3m Level=Meter Reading +Antenna Factor +Cable Loss
Margin= Emission at 3m Level -Limits
- That the limit for signals below 1GHz is a QP limit and peak readings are below the QP limit.
- The fundamental signal is not shown in the test data because measurements at fundamental frequency are shown separately and were ignored during the 30 – 1000 MHz scan.

Product Name	Electronic Stethoscope	Test Date	2021/01/05
Model Name	ES-2020	Test By	Ted Huang
Test Mode	TX	Temp & Humidity	25.5°C, 53%

Horizontal

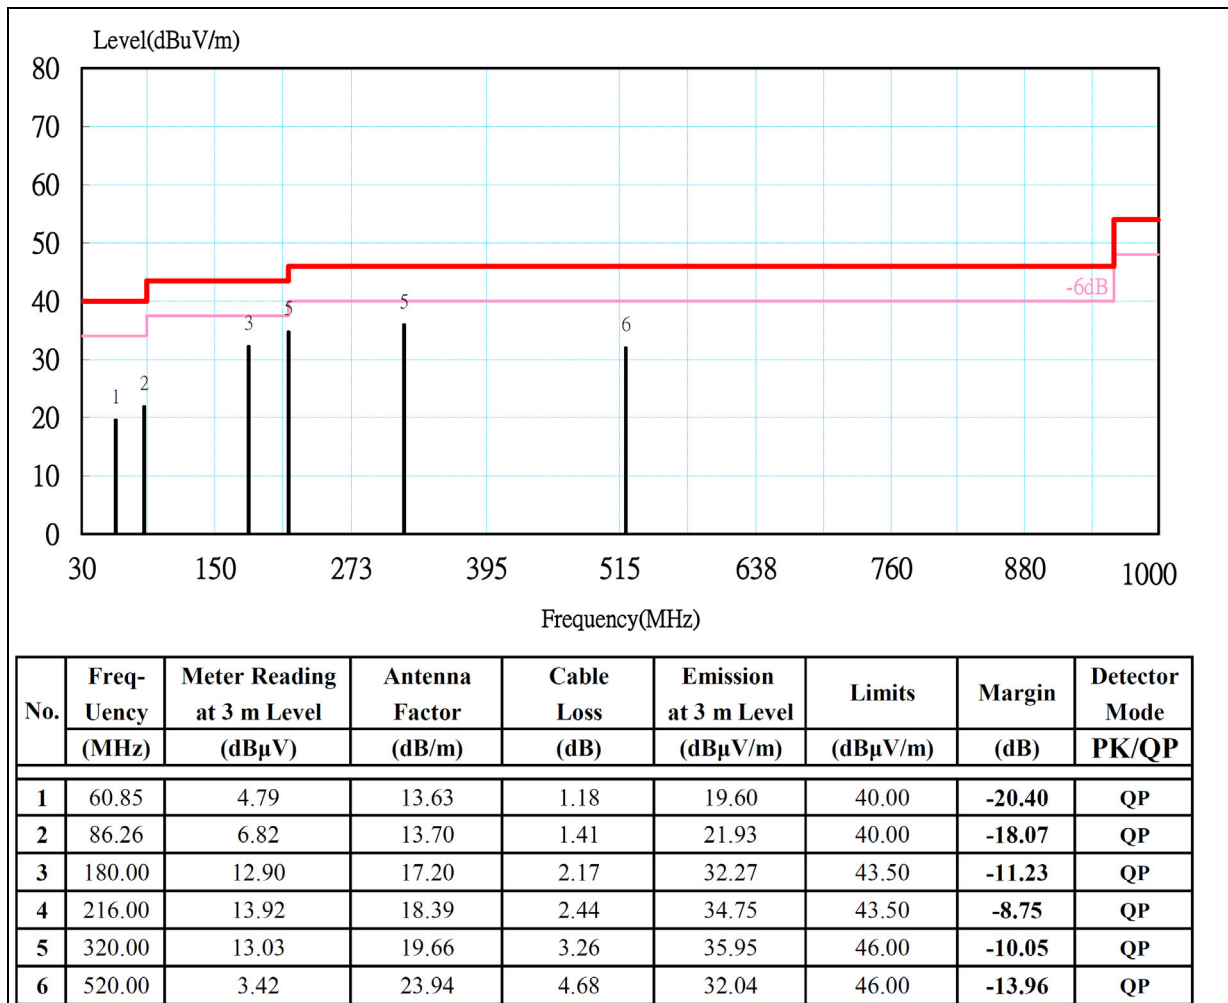

Remark:

- No emission found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz).
- Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using peak/quasi-peak detector mode.
- Quasi-peak test would be performed if the peak result were greater than the quasi-peak limit or as required by the applicant.
- Measurements above show only up to 6 maximum emissions noted, or would be lesser, with "N/A" remark, if no specific emissions from the EUT are recorded (ie: margin>20dB from the applicable limit) and considered that's already beyond the background noise floor.
- Emission at 3m Level=Meter Reading +Antenna Factor +Cable Loss
Margin= Emission at 3m Level -Limits
- That the limit for signals below 1GHz is a QP limit and peak readings are below the QP limit.
- The fundamental signal is not shown in the test data because measurements at fundamental frequency are shown separately and were ignored during the 30 – 1000 MHz scan.

9.6.3 TRANSMITTER RADIATED EMISSION ABOVE 1 GHz

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH Low)	TEMP& Humidity	22.5°C, 54%

Horizontal

TX / GFSK(4.0) mode / CH Low				Measurement Distance at 3m		Horizontal polarity			
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
1288.25	61.62	25.61	2.26	46.18	0.43	43.74	74.00	-30.26	P
1288.25	51.71	25.61	2.26	46.18	0.43	33.83	54.00	-20.17	A
* 4803.76	58.52	33.23	4.30	44.77	0.22	51.51	74.00	-22.49	P
* 4803.76	49.12	33.23	4.30	44.77	0.22	42.11	54.00	-11.89	A
7206.18	54.41	38.68	5.39	44.06	0.27	54.69	74.00	-19.31	P
7206.18	45.68	38.68	5.39	44.06	0.27	45.96	54.00	-8.04	A

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH Low)	TEMP& Humidity	22.5°C, 54%

Vertical

TX / GFSK(4.0) mode / CH Low				Measurement Distance at 3m		Vertical polarity			
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
1279.41	62.60	25.57	2.25	46.19	0.43	44.67	74.00	-29.33	P
1279.41	50.99	25.57	2.25	46.19	0.43	33.06	54.00	-20.94	A
* 4803.98	60.69	33.23	4.30	44.77	0.22	53.68	74.00	-20.32	P
* 4803.98	51.49	33.23	4.30	44.77	0.22	44.48	54.00	-9.52	A
7206.43	57.73	38.68	5.39	44.06	0.27	58.01	74.00	-15.99	P
7206.43	48.68	38.68	5.39	44.06	0.27	48.96	54.00	-5.04	A

REMARK:

1. AF: Antenna Factor, Cable: Cable Loss, Pre-Amp: Preamplifier gain, Filter: 2.4GHz~2.5GHz Filter Insertion Loss
2. Spectrum analyzer setting P(Peak): RBW=1MHz, VBW=1MHz, A(Average): RBW=1MHz, VBW=10Hz
3. The result basic equation calculation is as follow:
Level = Reading + AF + Cable – Preamp + Filter – Dist, Margin = Level-Limit
4. The other emission levels were 20dB below the limit
5. The test limit distance is 3M limit.
6. *=Restricted bands of operation

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH Middle)	TEMP& Humidity	22.5°C, 54%

Horizontal

TX / GFSK(4.0) mode / CH Middle				Measurement Distance at 3m		Horizontal polarity			
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
1770.14	61.55	28.72	2.63	45.63	0.74	48.01	74.00	-25.99	P
1770.14	53.74	28.72	2.63	45.63	0.74	40.20	54.00	-13.80	A
* 4883.65	60.10	33.50	4.35	44.78	0.23	53.40	74.00	-20.60	P
* 4883.65	54.57	33.50	4.35	44.78	0.23	47.87	54.00	-6.13	A
* 7325.30	52.41	39.14	5.44	43.94	0.27	53.32	74.00	-20.68	P
* 7325.30	45.76	39.14	5.44	43.94	0.27	46.67	54.00	-7.33	A

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH Middle)	TEMP& Humidity	22.5°C, 54%

Vertical

TX / GFSK(4.0) mode / CH Middle				Measurement Distance at 3m		Vertical polarity			
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
* 1321.14	65.68	25.75	2.29	46.14	0.44	48.01	74.00	-25.99	P
* 1321.14	51.91	25.75	2.29	46.14	0.44	34.24	54.00	-19.76	A
* 4883.67	61.89	33.50	4.35	44.78	0.23	55.19	74.00	-18.81	P
* 4883.67	55.94	33.50	4.35	44.78	0.23	49.24	54.00	-4.76	A
* 7325.18	56.03	39.14	5.44	43.94	0.27	56.94	74.00	-17.06	P
* 7325.18	47.59	39.14	5.44	43.94	0.27	48.50	54.00	-5.50	A

REMARK:

1. AF: Antenna Factor, Cable: Cable Loss, Pre-Amp: Preamplifier gain, Filter: 2.4GHz~2.5GHz Filter Insertion Loss
2. Spectrum analyzer setting P(Peak): RBW=1MHz, VBW=1MHz, A(Average): RBW=1MHz, VBW=10Hz
3. The result basic equation calculation is as follow:
Level = Reading + AF + Cable – Preamp + Filter – Dist, Margin = Level-Limit
4. The other emission levels were 20dB below the limit
5. The test limit distance is 3M limit.
6. *=Restricted bands of operation

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH High)	TEMP& Humidity	22.5°C, 54%

Horizontal

TX / GFSK(4.0) mode / CH High				Measurement Distance at 3m				Horizontal polarity	
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
1763.27	64.52	28.66	2.63	45.63	0.73	50.91	74.00	-23.09	P
1763.27	53.41	28.66	2.63	45.63	0.73	39.80	54.00	-14.20	A
* 4959.64	60.14	33.76	4.39	44.78	0.24	53.75	74.00	-20.25	P
* 4959.64	52.92	33.76	4.39	44.78	0.24	46.53	54.00	-7.47	A
* 7439.54	53.96	39.57	5.48	43.81	0.27	55.47	74.00	-18.53	P
* 7439.54	46.32	39.57	5.48	43.81	0.27	47.83	54.00	-6.17	A

Product Name	Electronic Stethoscope	Test Date	2020/12/31
Model	ES-2020	Test By	Ted Huang
Test Mode	GFSK(4.0) TX (CH High)	TEMP& Humidity	22.5°C, 54%



Vertical

TX / GFSK(4.0) mode / CH High				Measurement Distance at 3m				Vertical polarity	
Freq.	Reading	AF	Cable Loss	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dBμV)	(dB/m)	(dB)	(dB)	(dB)	(dBμV/m)	(dBμV/m)	(dB)	(P/Q/A)
* 1325.16	61.58	25.77	2.29	46.14	0.44	43.94	74.00	-30.06	P
* 1325.16	50.94	25.77	2.29	46.14	0.44	33.30	54.00	-20.70	A
* 4959.63	59.46	33.76	4.39	44.78	0.24	53.07	74.00	-20.93	P
* 4959.63	52.46	33.76	4.39	44.78	0.24	46.07	54.00	-7.93	A
* 7439.24	57.16	39.57	5.48	43.81	0.27	58.67	74.00	-15.33	P
* 7439.24	47.18	39.57	5.48	43.81	0.27	48.69	54.00	-5.31	A

REMARK:


1. AF: Antenna Factor, Cable: Cable Loss, Pre-Amp: Preamplifier gain, Filter: 2.4GHz~2.5GHz Filter Insertion Loss
2. Spectrum analyzer setting P(Peak): RBW=1MHz, VBW=1MHz, A(Average): RBW=1MHz, VBW=10Hz
3. The result basic equation calculation is as follow:
Level = Reading + AF + Cable – Preamp + Filter – Dist, Margin = Level-Limit
4. The other emission levels were 20dB below the limit
5. The test limit distance is 3M limit.
6. *=Restricted bands of operation

9.6.4 RESTRICTED BAND EDGES

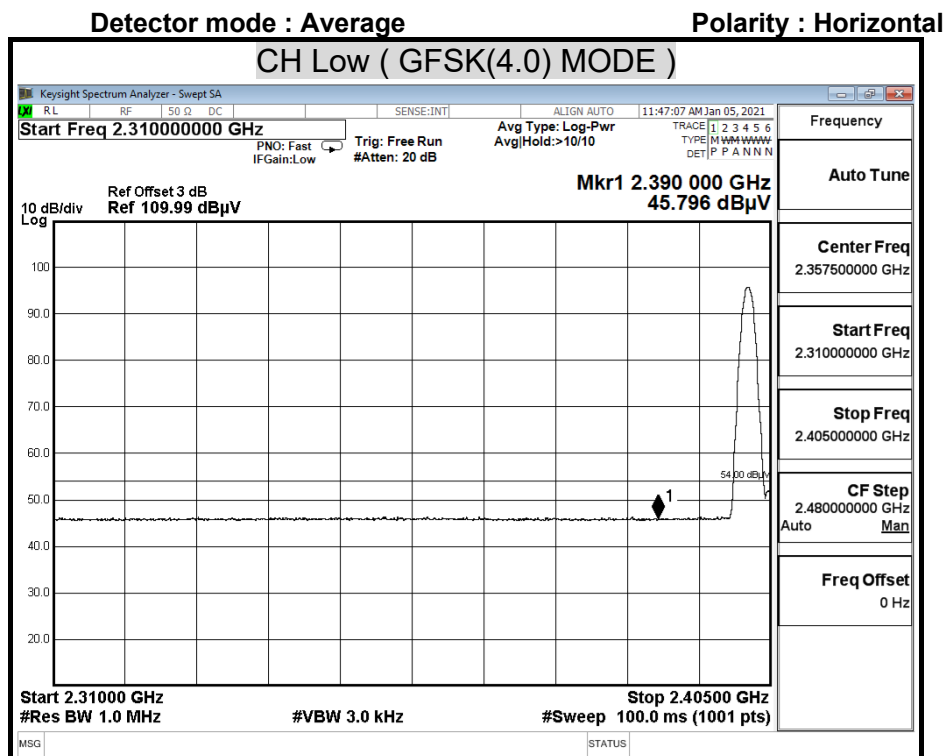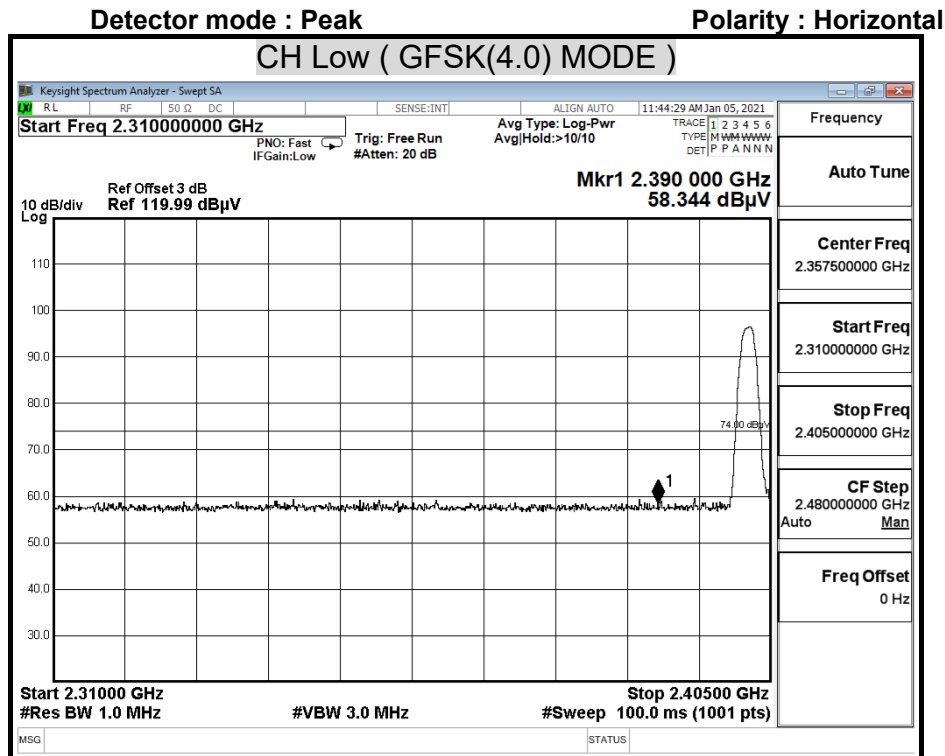


Detector mode : Peak



Polarity : Vertical

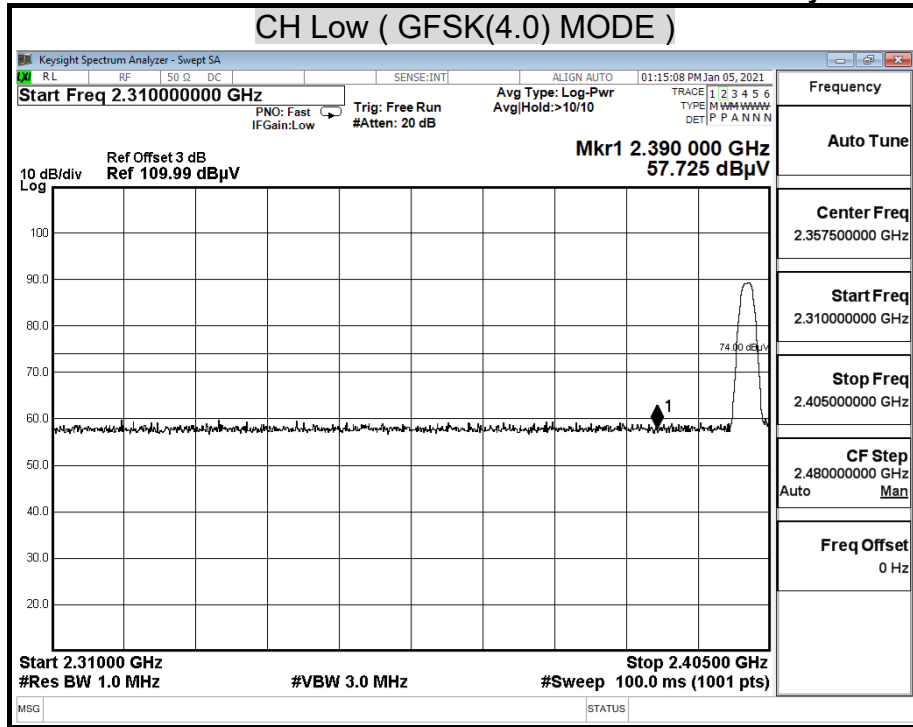

Detector mode : Average


Polarity : Vertical

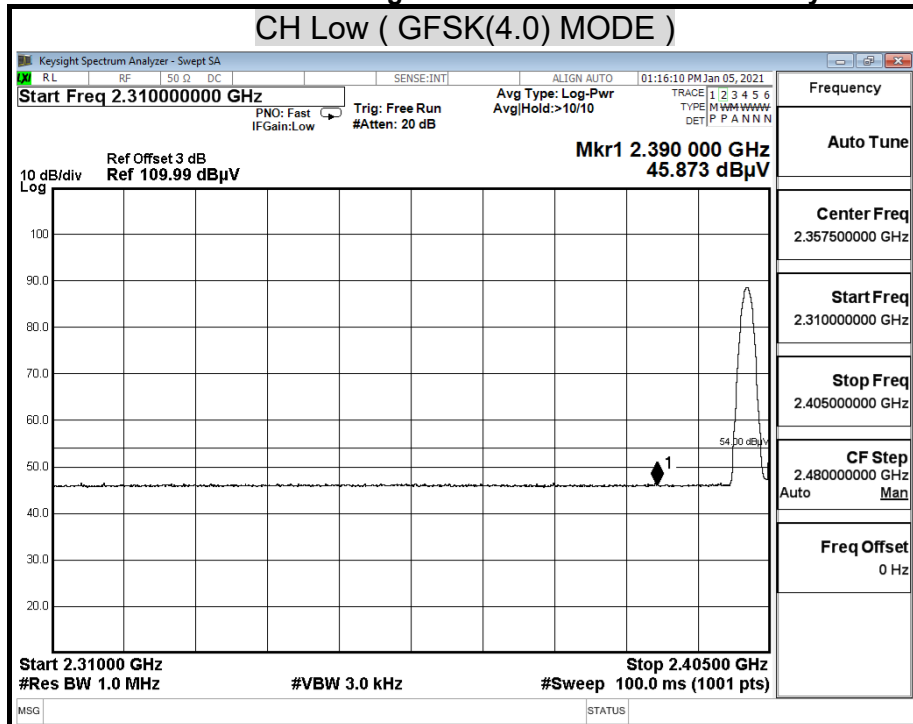

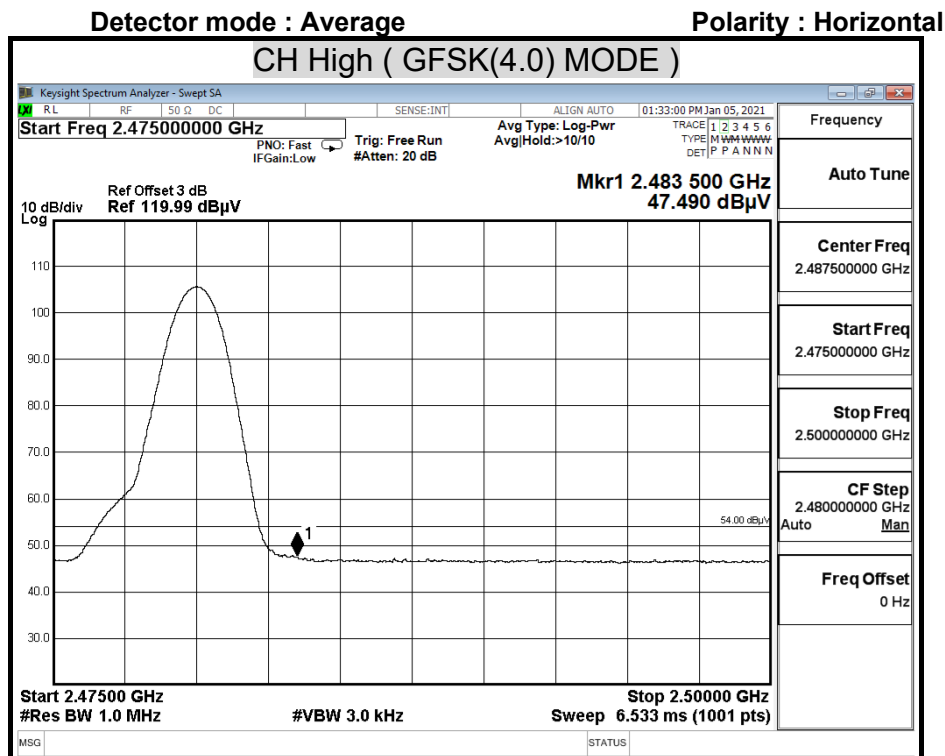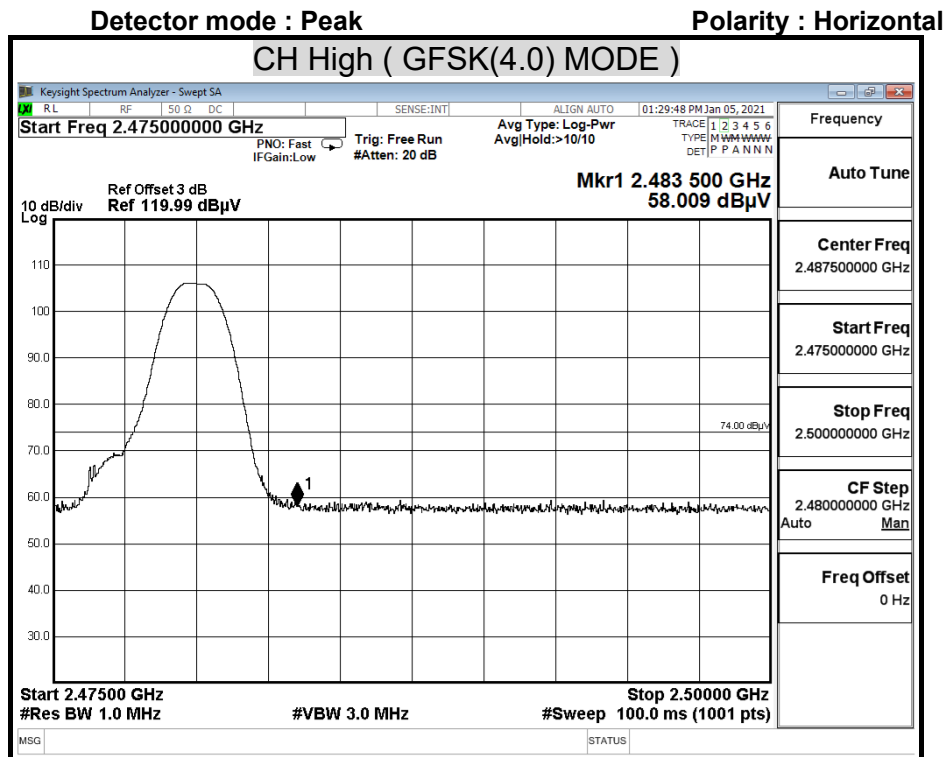


Detector mode : Peak

Polarity : Vertical

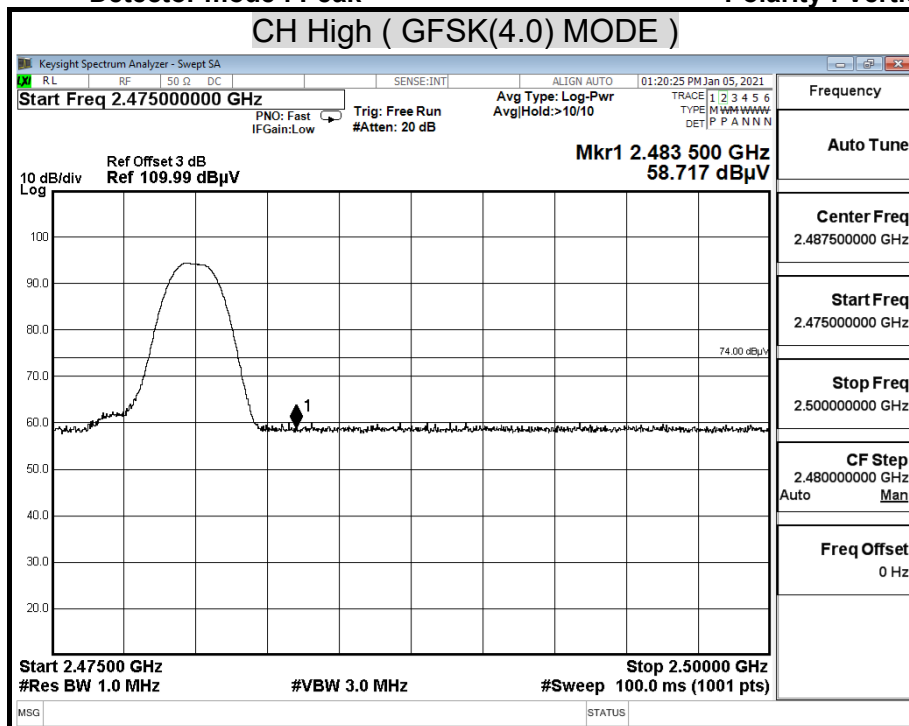

Detector mode : Average

Polarity : Vertical

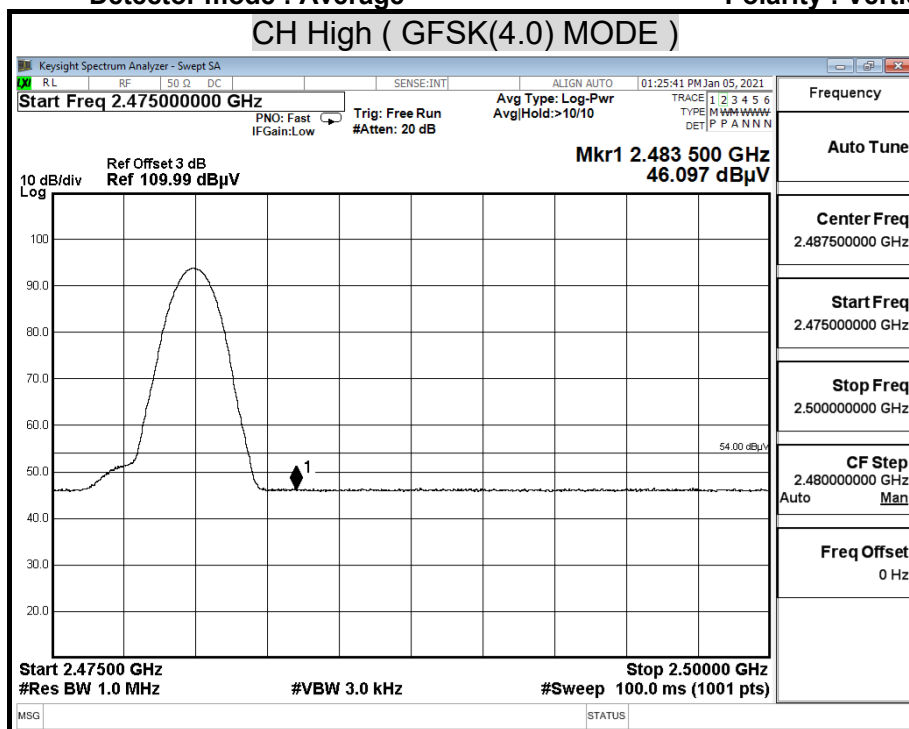

9.7 POWERLINE CONDUCTED EMISSIONS


LIMITS

§ 15.207 (a) Except as shown in paragraph (b) and (c) this section, for an intentional radiator that is designed to be connected to the public utility (AC) power line, the radio frequency voltage that is conducted back onto the AC power line on any frequency or frequencies within the band 150 kHz to 30 MHz shall not exceed the limits in the following table, as measured using a 50 μ H/50 ohms line impedance stabilization network (LISN). Compliance with the provisions of this paragraph shall be based on the measurement of the radio frequency voltage between each power line and ground at the power terminal.

The lower limit applies at the boundary between the frequency ranges.

Frequency of Emission (MHz)	Conducted limit (dB μ v)	
	Quasi-peak	Average
0.15 - 0.5	66 to 56	56 to 46
0.5 - 5	56	46
5 - 30	60	50

TEST SETUP

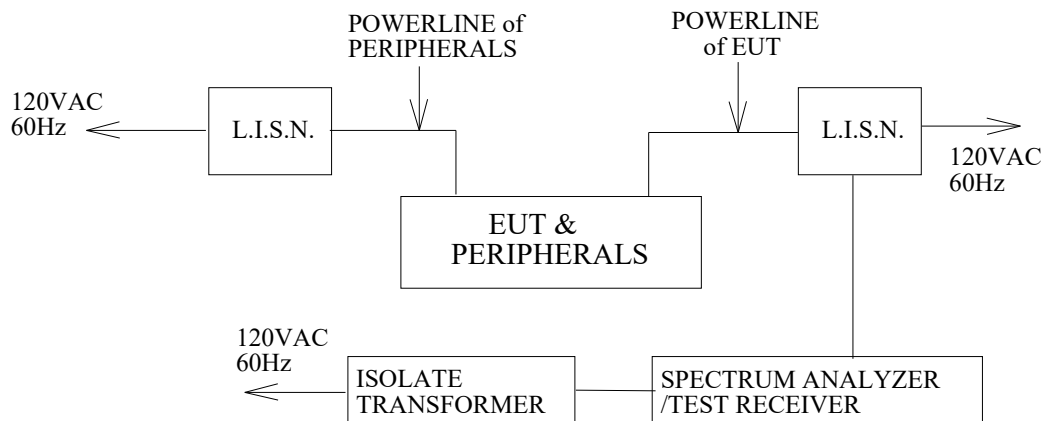

TEST PROCEDURE

The EUT is placed on a non-conducting table 40 cm from the vertical ground plane and 80cm above the horizontal ground plane. The EUT IS CONFIGURED IN ACCORDANCE WITH ANSI C63.10.

The resolution bandwidth is set to 9 kHz for both quasi-peak detection and average detection measurements.

Line conducted data is recorded for both NEUTRAL and LINE.

TEST RESULTS

No non-compliance noted.

✖ This EUT is not connected to AC Source directly. Not applicable for this test.



Report No.: T201207N01-RP1-2

Page: 55 / 59
Rev.: 00

10. ANTENNA REQUIREMENT

10.1 STANDARD APPLICABLE

For intentional device, according to FCC 47 CFR Section 15.203, an intentional radiator shall be designed to ensure that no antenna other than that furnished by the responsible party shall be used with the device.

And according to FCC 47 CFR Section 15.247 (b), if transmitting antennas of directional gain greater than 6dBi are used, the power shall be reduced by the amount in dB that the directional gain of the antenna exceeds 6dBi.

10.2 ANTENNA CONNECTED CONSTRUCTION

Manufacturer: Kirchhoff Technology Co., Ltd
Type: PCB antenna
Model: KB64A/B/C
Gain: 0.11 dBi

=== END of Report ===