



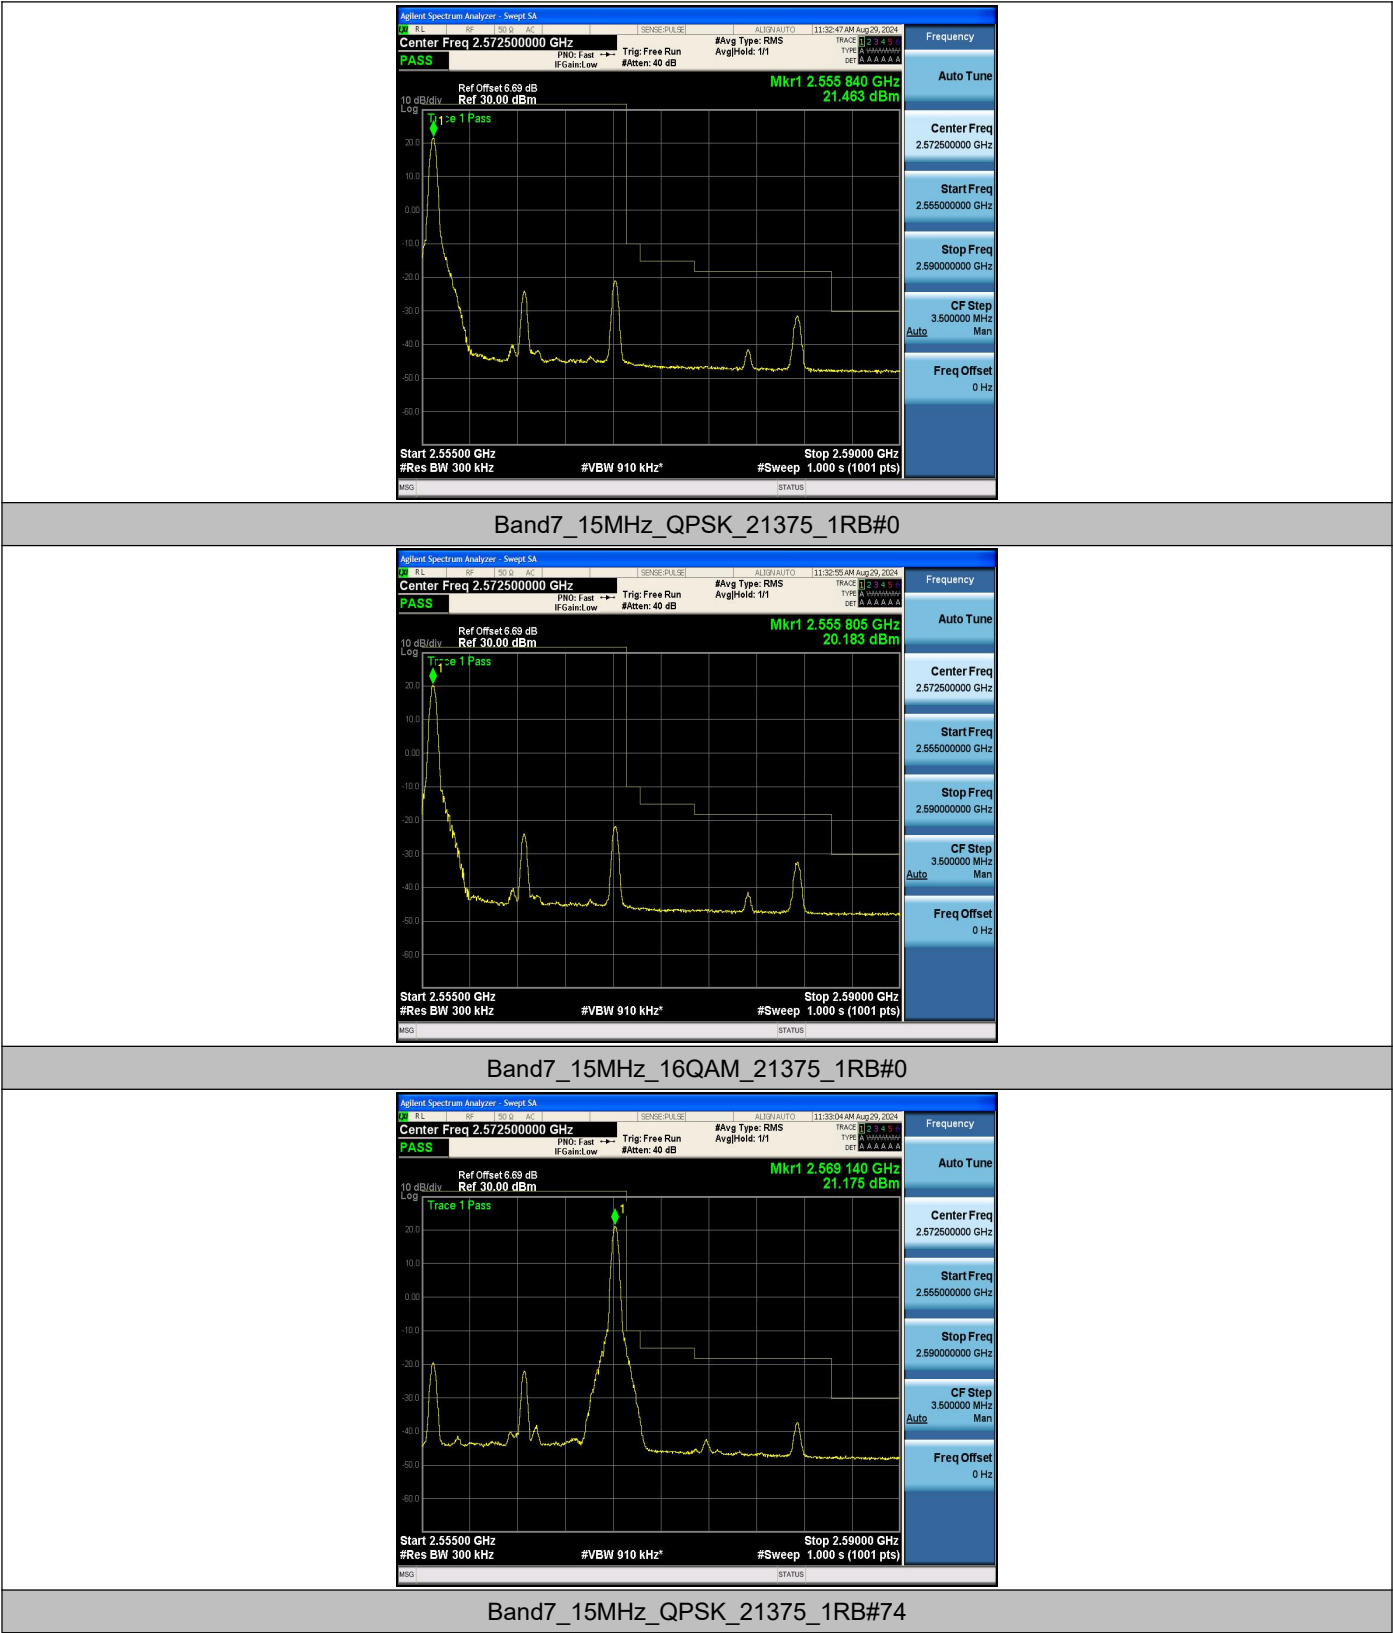

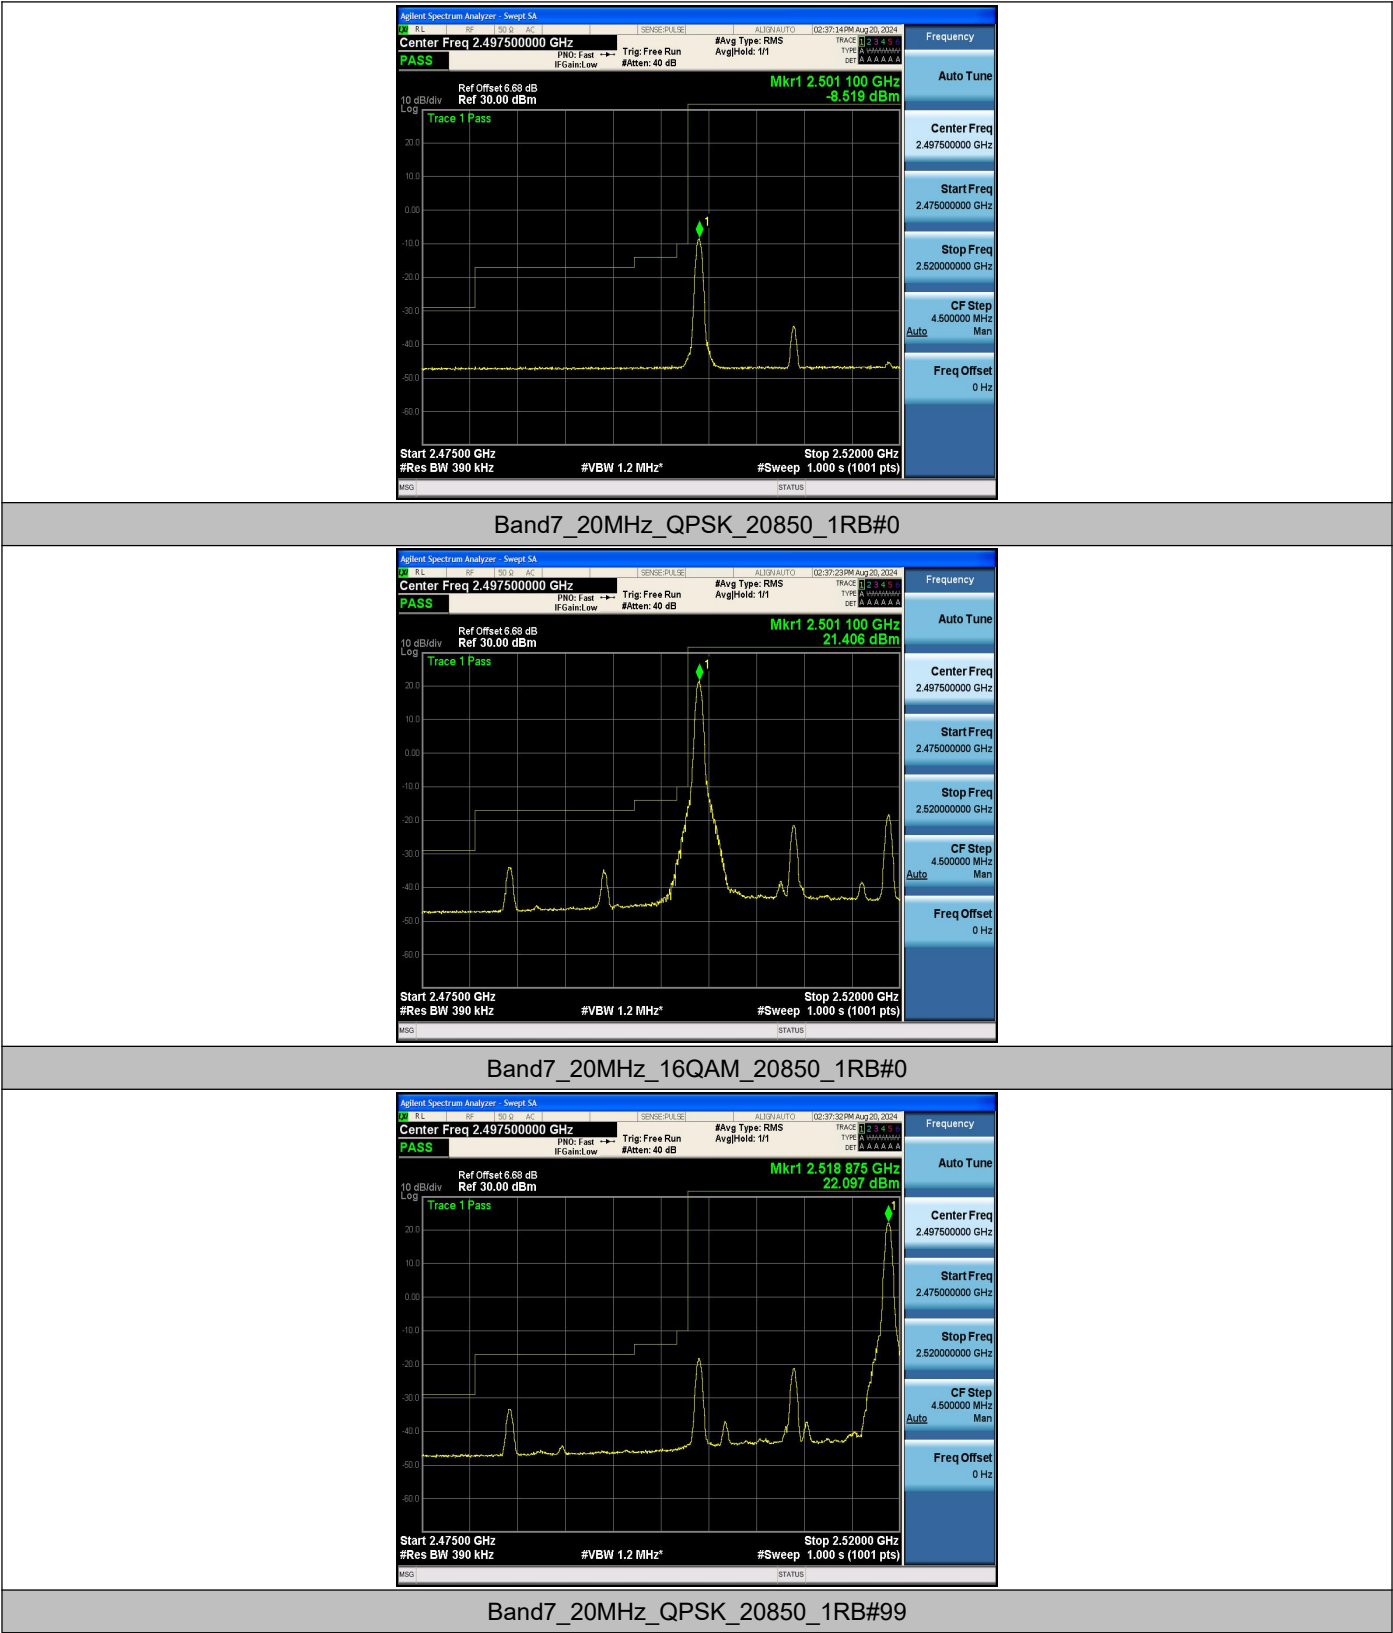

Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.497500000 GHz

PASS

Ref Offset 6.68 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.47500 GHz

Res BW 390 kHz

VBW 1.2 MHz

Stop 2.52000 GHz

Sweep 1.000 s (1001 pts)

Mkr1 2.518 875 GHz

22.097 dBm

Frequency

Auto Tune

Center Freq

2.497500000 GHz

Start Freq

2.475000000 GHz

Stop Freq

2.520000000 GHz

CF Step

4.500000 MHz

Auto

Freq Offset

0 Hz

Band7_20MHz_QPSK_20850_1RB#99



Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.497500000 GHz

PASS

Ref Offset 6.68 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.47500 GHz

#Res BW 390 kHz

#VBW 1.2 MHz

Stop 2.52000 GHz

#Sweep 1.000 s (1001 pts)

SENSE (PLA SE)

ALIST AUTO

02:37:58 PM Aug 20, 2024

TYPE A WWWWWWWW

DET A A A A A A

Trig: Free Run

#Att: 40 dB

#Avg Type: RMS

Avg Hold: 1/1

Mkr1 2.509 200 GHz

4.719 dBm

Frequency

Auto Tune

Center Freq

2.497500000 GHz

Start Freq

2.475000000 GHz

Stop Freq

2.520000000 GHz

CF Step

4.500000 MHz

Auto

Freq Offset

0 Hz

Band7_20MHz_16QAM_20850_100RB#0







Agilent Spectrum Analyzer - Swept SA

Center Freq 2.572500000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.550000 GHz

#Res BW 390 kHz

#VBW 1.2 MHz

Stop 2.595000 GHz

#Sweep 1.000 s (1001 pts)

SENSE (PLA SE)

ALTO AUTO

02:39:25 PM Aug 20, 2024

TYPE A

DEF A

Trig: Free Run

#Att: 40 dB

#Avg Type: RMS

Avg Hold: 1/1

Frequency

Auto Tune

Center Freq

2.572500000 GHz

Start Freq

2.550000000 GHz

Stop Freq

2.595000000 GHz

CF Step

4.500000 MHz

Auto

Man


Freq Offset

0 Hz


Mkr1 2.551 990 GHz

5.165 dBm

Band7_20MHz_16QAM_21350_100RB#0

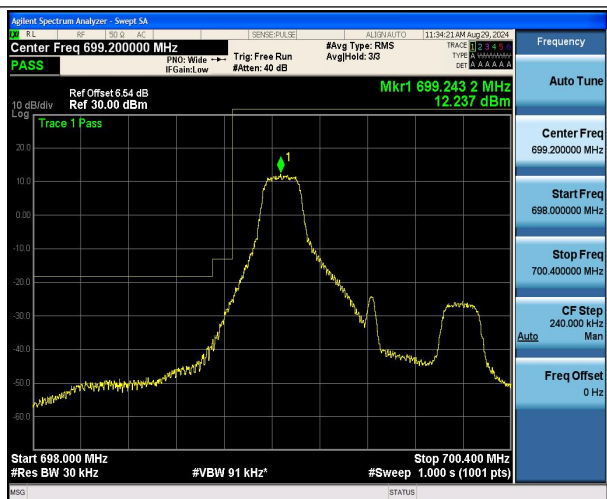


Band12_1.4MHz_QPSK_23017_1RB#0

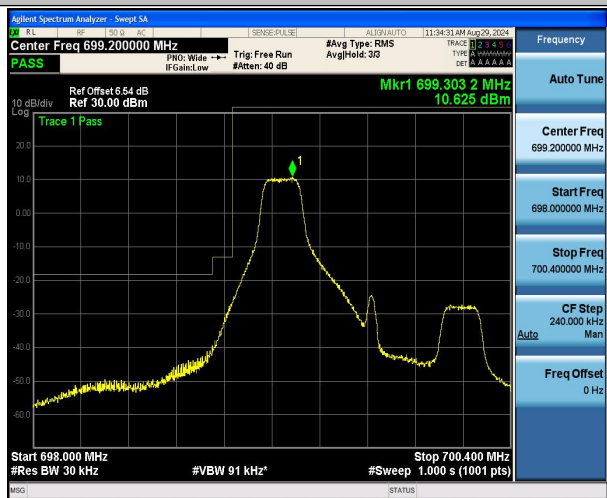


Band12 1.4MHz 16QAM 23017 1RB#0



Band12_1.4MHz_QPSK_23017_1RB#5

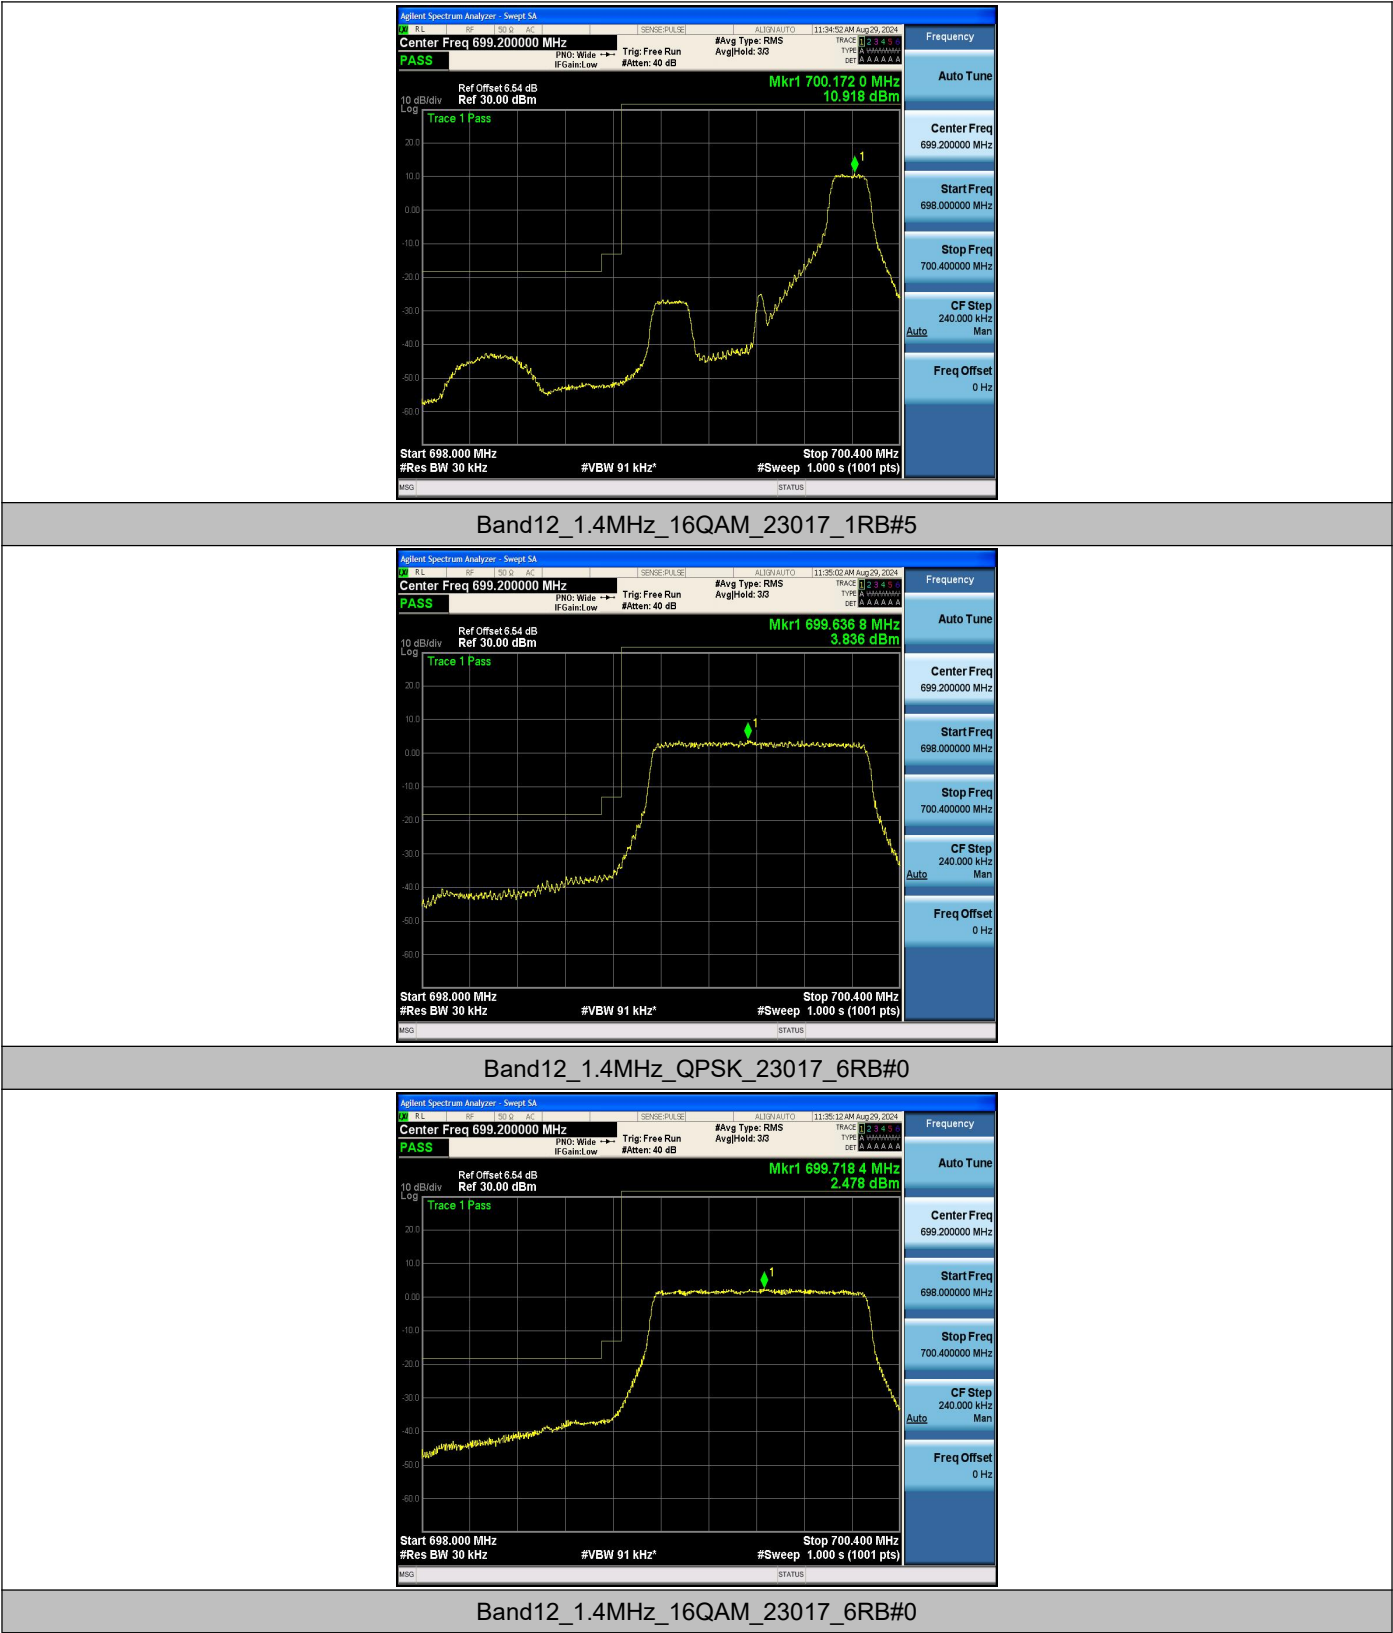

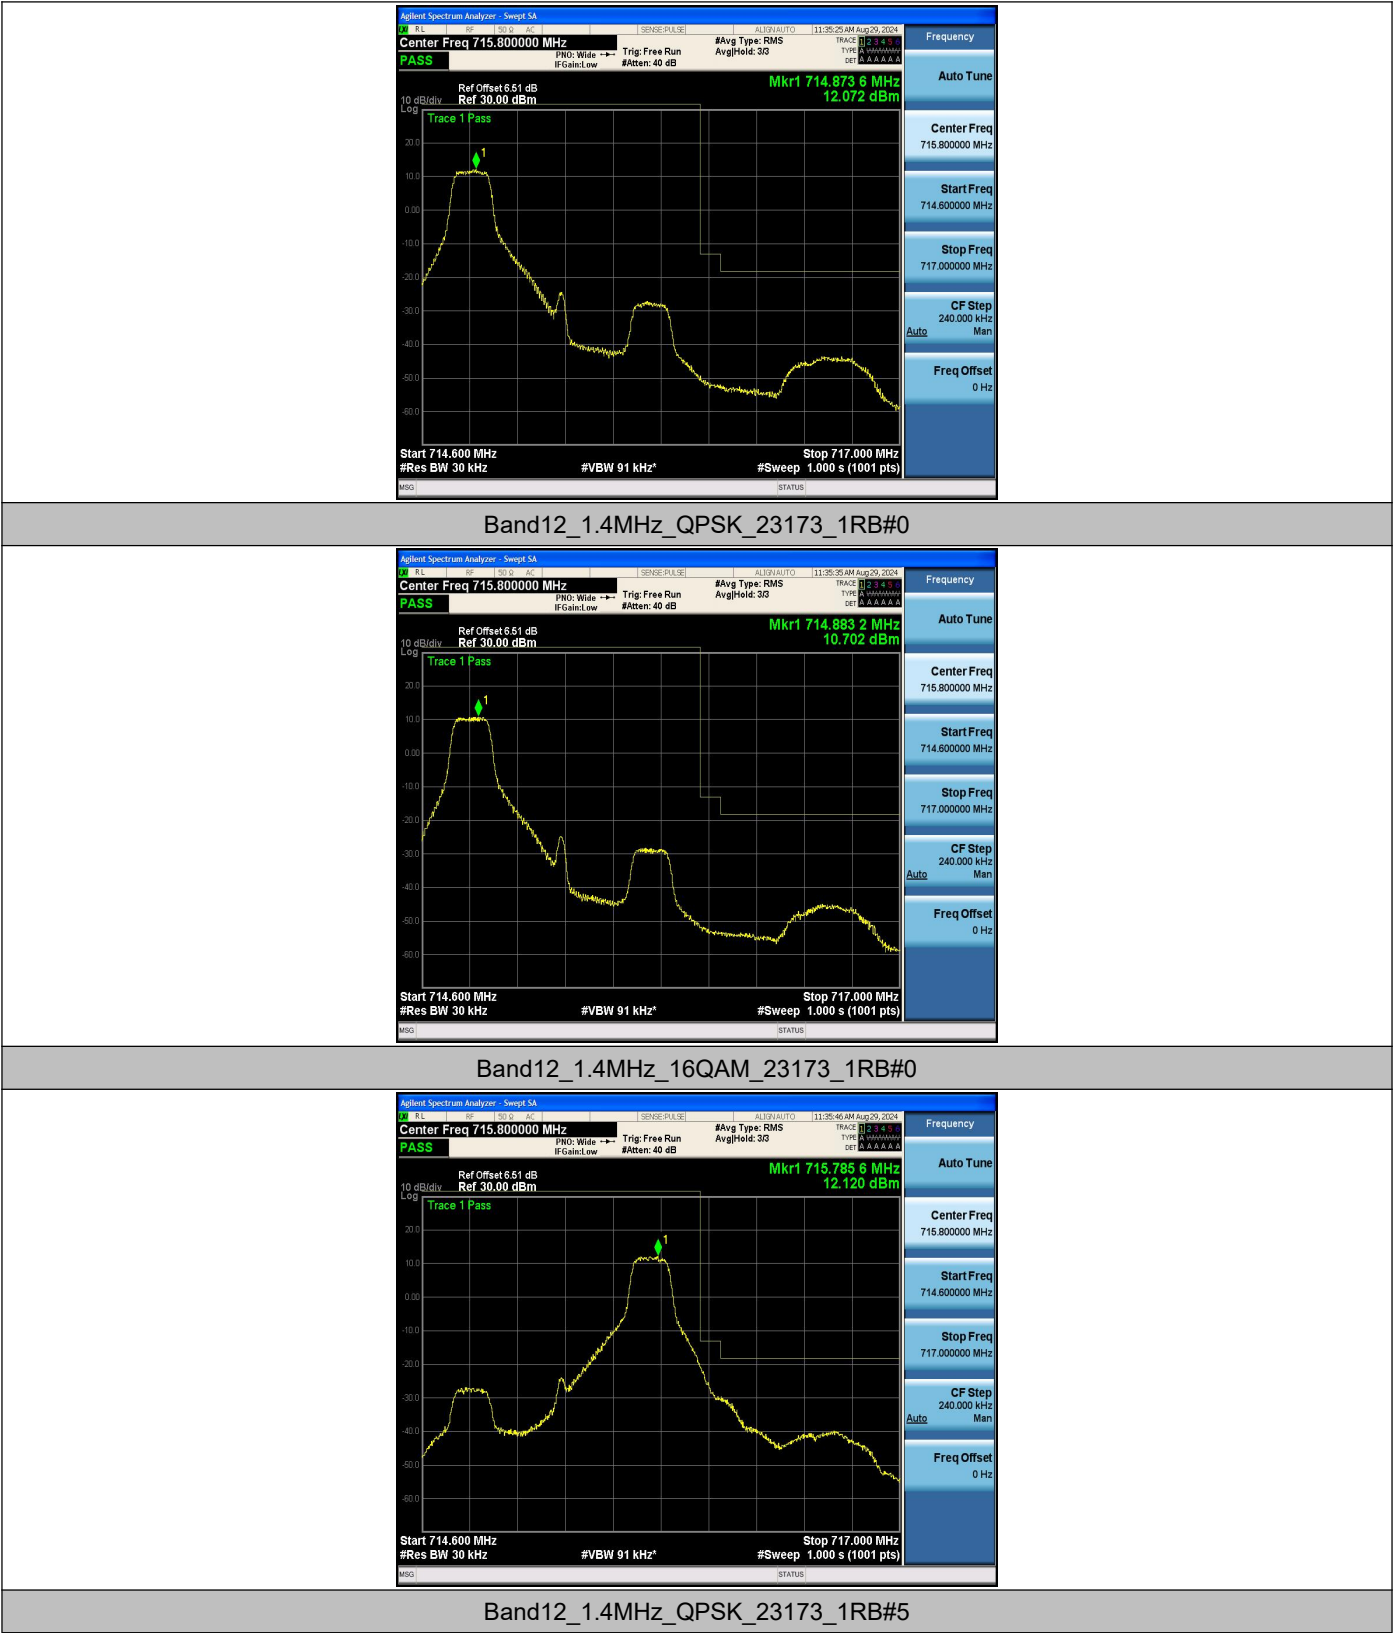

Agilent Spectrum Analyzer - Sweep SA

Center Freq 715.800000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 714.600 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 715.800000 MHz

Start Freq 714.600000 MHz

Stop Freq 717.000000 MHz

CF Step 240.000 kHz


Auto

Freq Offset 0 Hz

Mkr1 715.785 6 MHz

12.120 dBm

Band12_1.4MHz_QPSK_23173_1RB#5

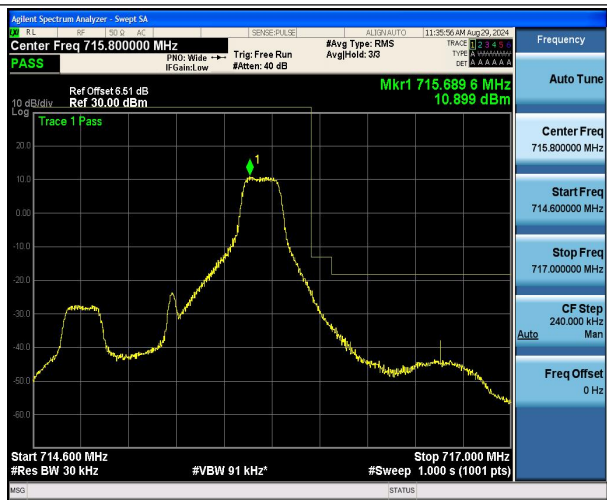


Band12_1.4MHz_16QAM_23173_1RB#5



Band12_1.4MHz_QPSK_23173_6RB#0



Band12_3MHz_QPSK_23025_1RB#0

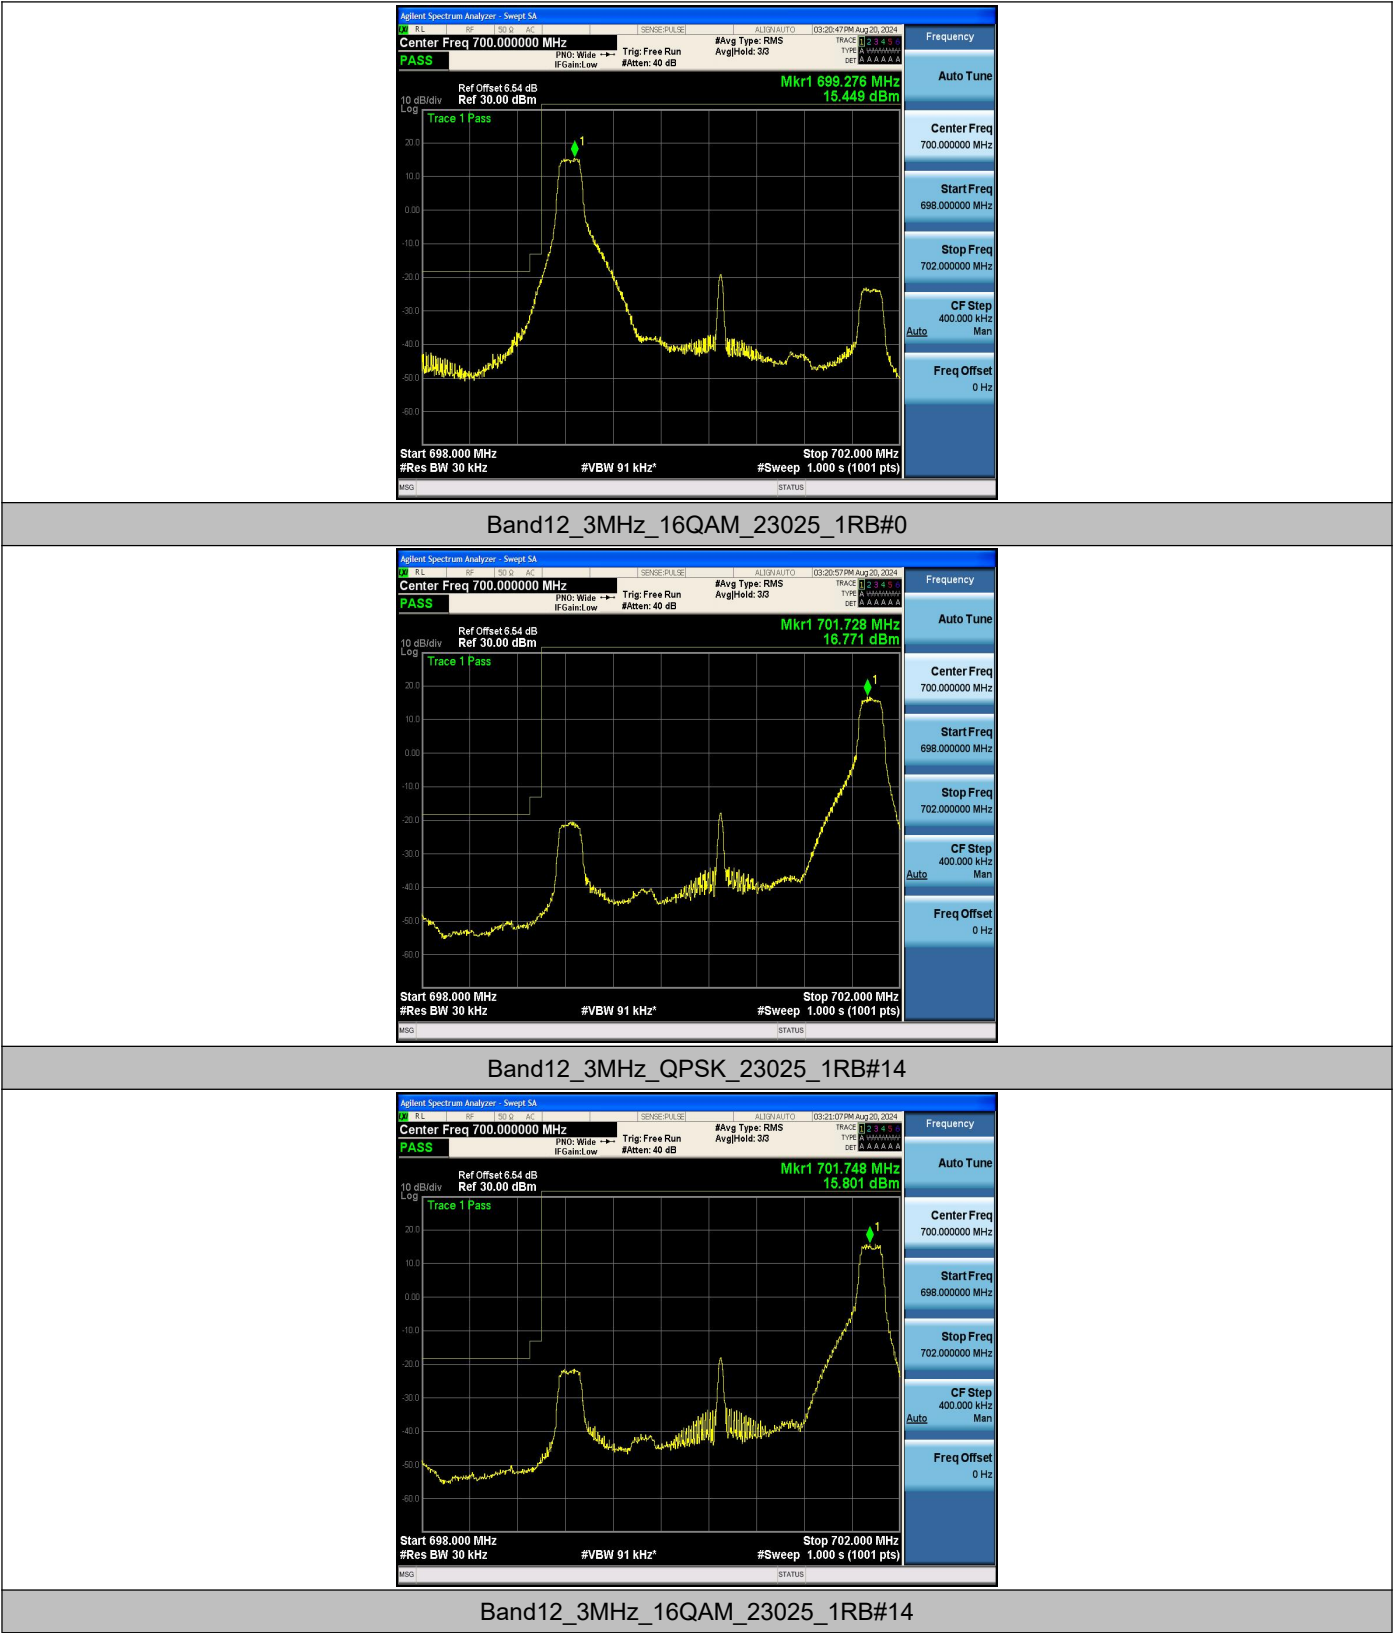



Band12_3MHz_QPSK_23025_15RB#0



Band12_3MHz_16QAM_23025_15RB#0



Band12_3MHz_QPSK_23165_1RB#0



Band12_3MHz_16QAM_23165_1RB#0



Band12_1.4MHz_16QAM_23173_6RB#0



Band12_3MHz_QPSK_23165_1RB#14




Band12_3MHz_16QAM_23165_1RB#14



Band12_3MHz_QPSK_23165_15RB#0



Band12_3MHz_16QAM_23165_15RB#0

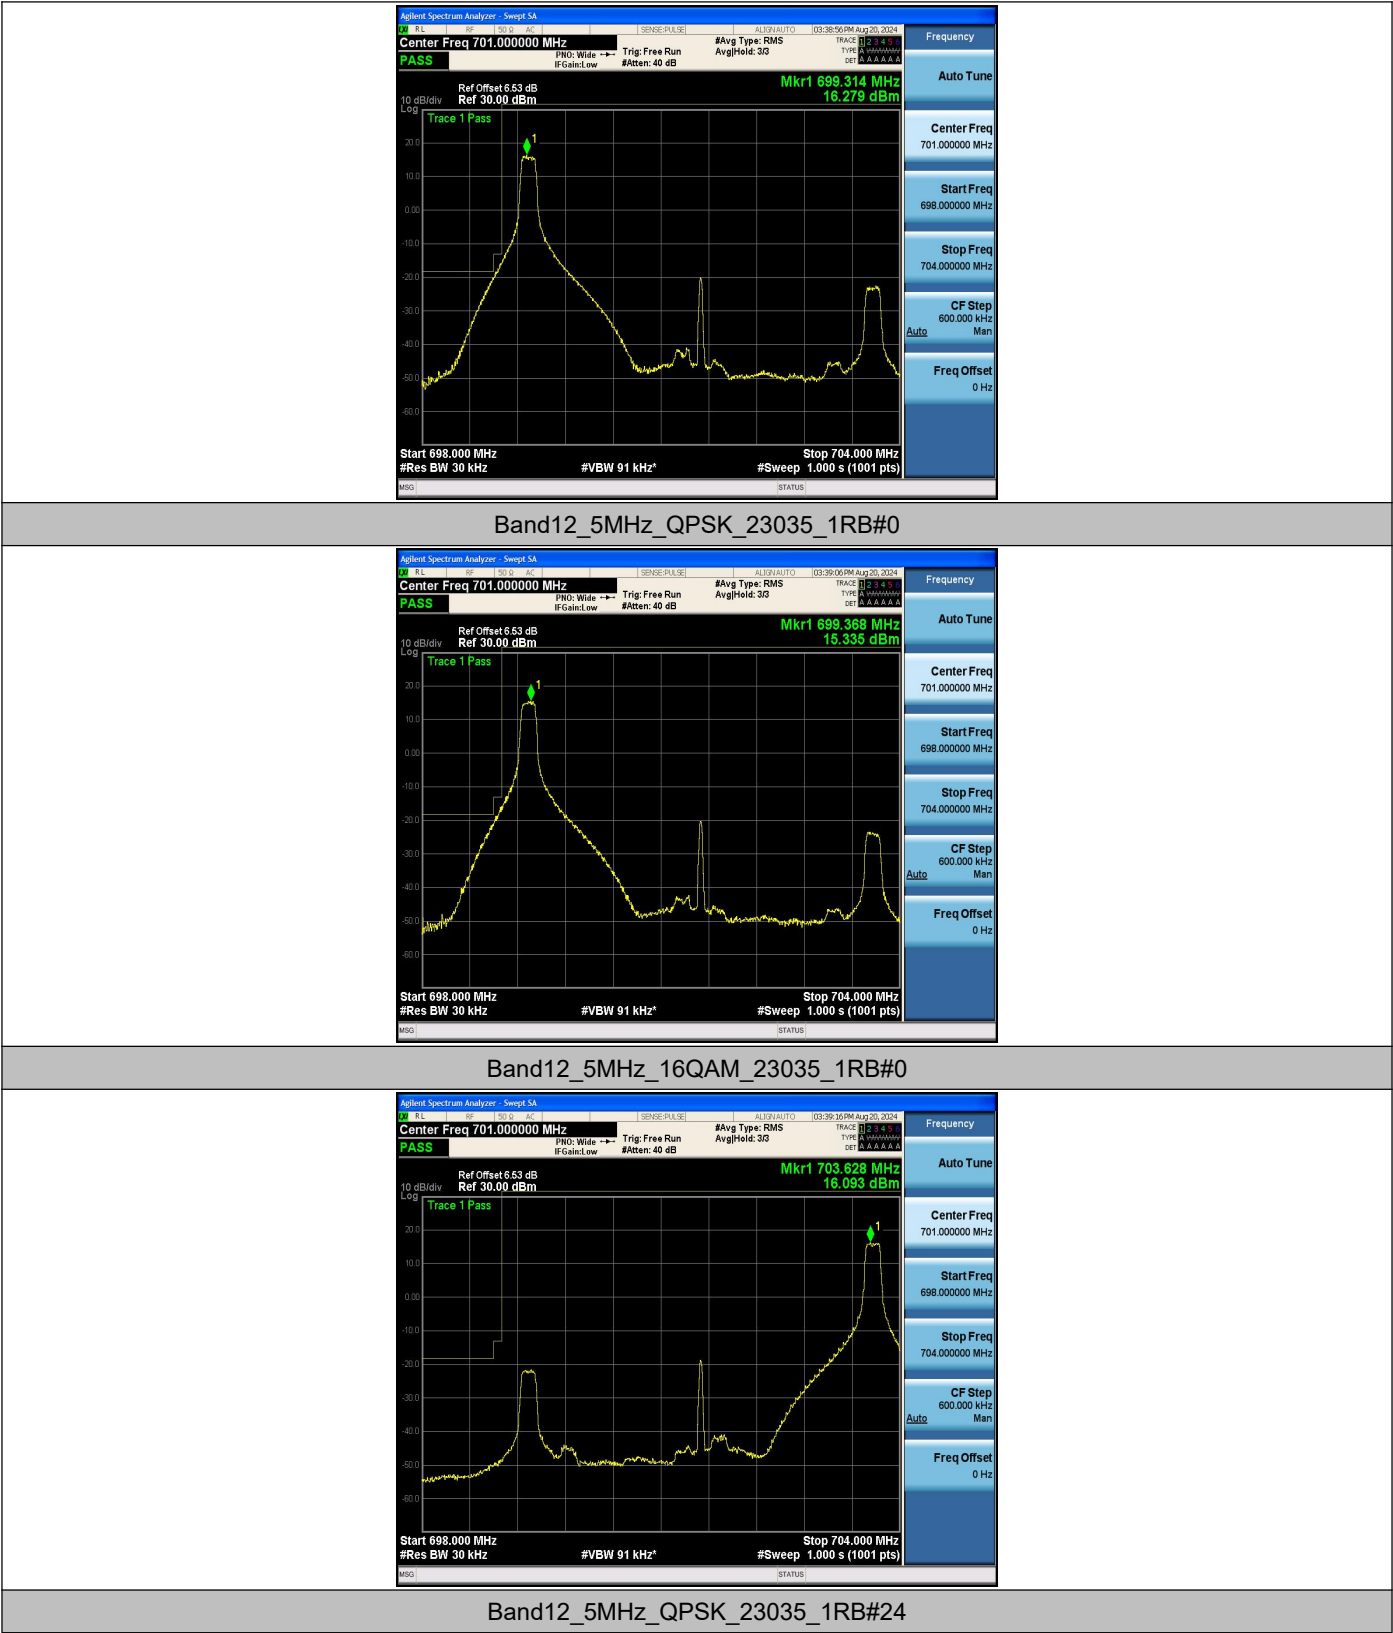

Agilent Spectrum Analyzer - Sweep SA

Center Freq 701.000000 MHz

PASS

Ref Offset 6.53 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 704.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 701.000000 MHz

Start Freq 698.000000 MHz

Stop Freq 704.000000 MHz

CF Step 600.000 kHz


Auto

Man

Freq Offset 0 Hz

Mkr1 703.628 MHz

16.093 dBm

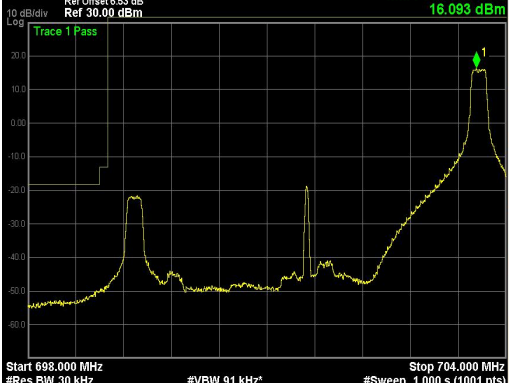

Band12_5MHz_QPSK_23035_1RB#24