



## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.60.10.21.MVGB.A

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 5000             | 36.2 $\pm$ 10 %                         |          | 4.45 $\pm$ 10 %               |          |
| 5100             | 36.1 $\pm$ 10 %                         |          | 4.56 $\pm$ 10 %               |          |
| 5200             | 36.0 $\pm$ 10 %                         | 34.06    | 4.66 $\pm$ 10 %               | 4.70     |
| 5300             | 35.9 $\pm$ 10 %                         |          | 4.76 $\pm$ 10 %               |          |
| 5400             | 35.8 $\pm$ 10 %                         | 33.39    | 4.86 $\pm$ 10 %               | 4.91     |
| 5500             | 35.6 $\pm$ 10 %                         |          | 4.97 $\pm$ 10 %               |          |
| 5600             | 35.5 $\pm$ 10 %                         | 32.77    | 5.07 $\pm$ 10 %               | 5.13     |
| 5700             | 35.4 $\pm$ 10 %                         |          | 5.17 $\pm$ 10 %               |          |
| 5800             | 35.3 $\pm$ 10 %                         | 32.40    | 5.27 $\pm$ 10 %               | 5.34     |
| 5900             | 35.2 $\pm$ 10 %                         |          | 5.38 $\pm$ 10 %               |          |
| 6000             | 35.1 $\pm$ 10 %                         |          | 5.48 $\pm$ 10 %               |          |

## 7.2 MEASUREMENT RESULT

At those frequencies, the target SAR value can not be generic. Hereunder is the target SAR value defined by Satimo, within the uncertainty for the system validation. All SAR values are normalized to 1 W net power. In bracket, the measured SAR is given with the used input power.


| Frequency (MHz) | 1 g SAR (W/kg) |                | 10 g SAR (W/kg) |              |
|-----------------|----------------|----------------|-----------------|--------------|
|                 | required       | measured       | required        | measured     |
| 5200            | 159.00         | 162.34 (16.23) | 56.90           | 55.42 (5.54) |
| 5400            | 166.40         | 168.48 (16.85) | 58.43           | 57.03 (5.70) |
| 5600            | 173.80         | 174.92 (17.49) | 59.97           | 58.63 (5.86) |
| 5800            | 181.20         | 178.89 (17.89) | 61.50           | 59.32 (5.93) |




**SAR REFERENCE WAVEGUIDE CALIBRATION REPORT**

Ref: ACR.60.10.21.MVGB.A


**SAR MEASUREMENT PLOTS @ 5200 MHz**

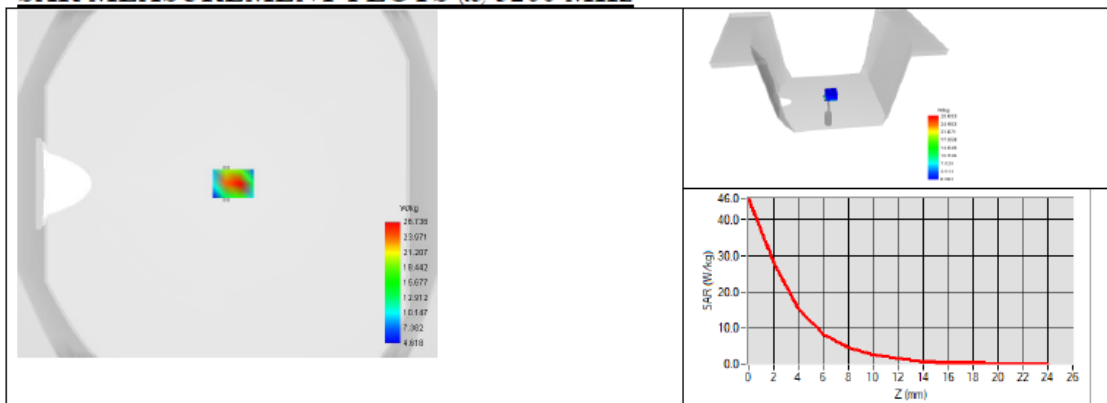

**SAR MEASUREMENT PLOTS @ 5400 MHz**

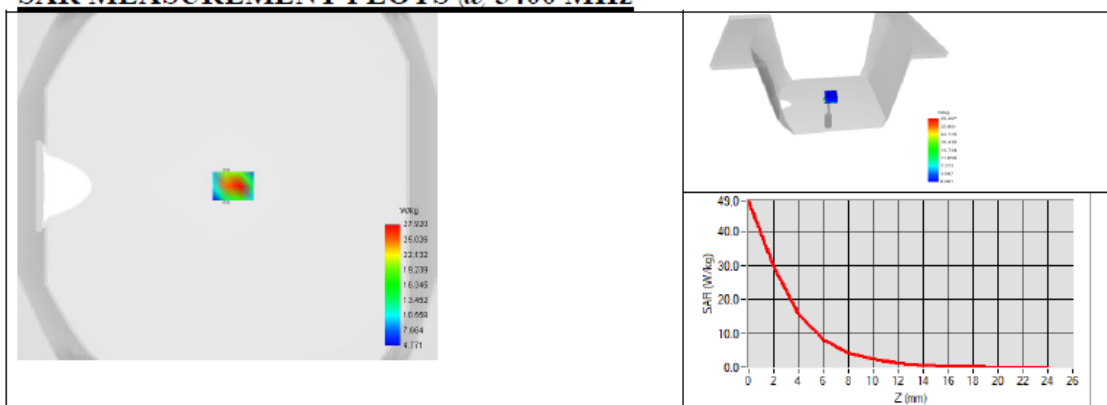

**SAR MEASUREMENT PLOTS @ 5600 MHz**

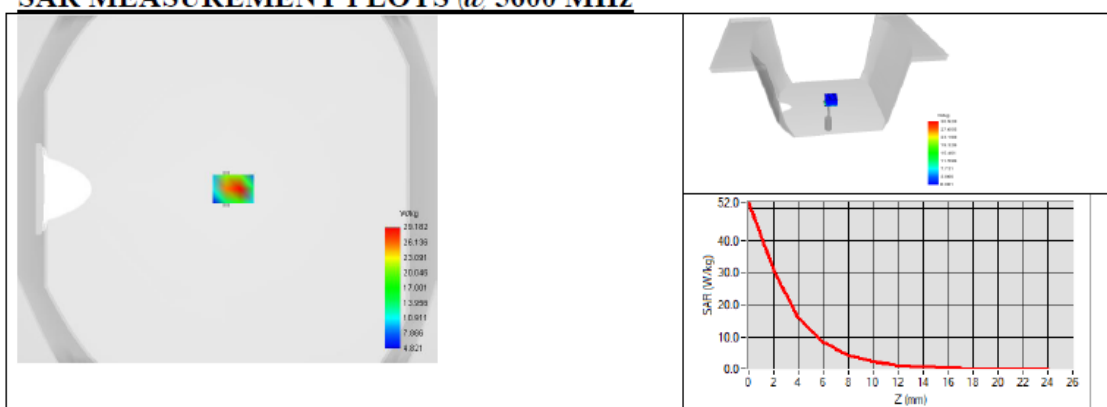




SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.60.10.21.MVGB.A

SAR MEASUREMENT PLOTS @ 5800 MHz

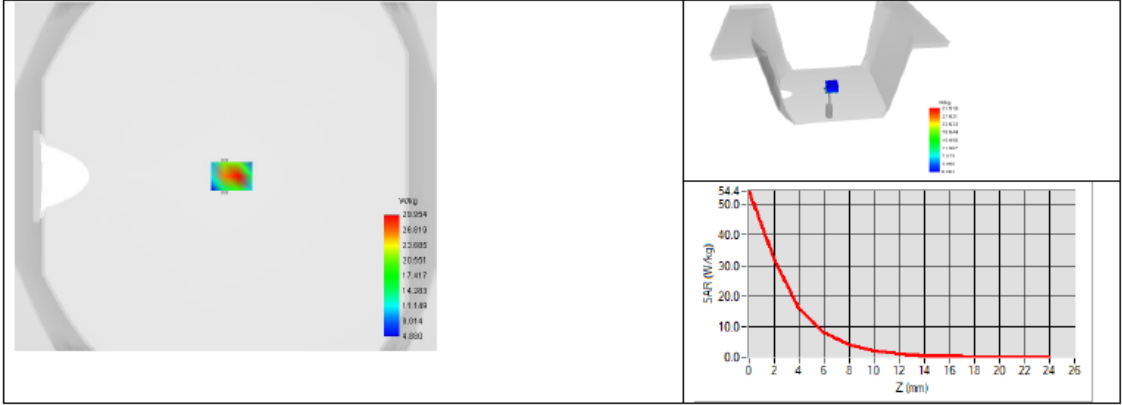



SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref. ACR.60.10.21.MVGB.A

8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| Flat Phantom                       | MVG                     | SN-13/09-SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 05/2019                                       | 05/2022                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2019                                       | 05/2022                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2019                                       | 10/2022                                       |
| Reference Probe                    | MVG                     | EPGO333 SN 41/18   | 05/2020                                       | 05/2021                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2020                                       | 02/2023                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2019                                       | 04/2022                                       |
| Amplifier                          | Aethercomm              | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 05/2019                                       | 05/2022                                       |
| Directional Coupler                | Narda 4216-20           | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44220687           | 05/2020                                       | 05/2023                                       |

### <Justification of the extended calibration>




If dipoles are verified in return loss ( $<-20\text{dB}$ , within 20% of prior calibration for below 3GHz, and  $<-8\text{dB}$ , within 20% of prior calibration for 5GHz to 6GHz), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

### <Head 2450MHz>

| Return Loss (dB) | Delta (%) | Impedance | Delta(ohm) | Date of Measurement |
|------------------|-----------|-----------|------------|---------------------|
| -23.18           | -         | 56.30     | -          | Mar. 01, 2021       |
| -23.39           | 0.91      | 56.342    | 0.042      | Feb. 28, 2022       |
| -26.296          | 13.44     | 54.99     | 1.310      | Feb. 20, 2023       |

The return loss is  $<-20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

Dipole Verification Data

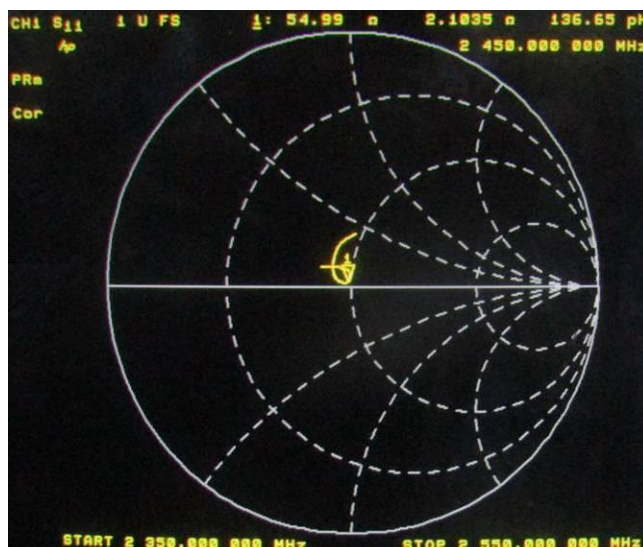
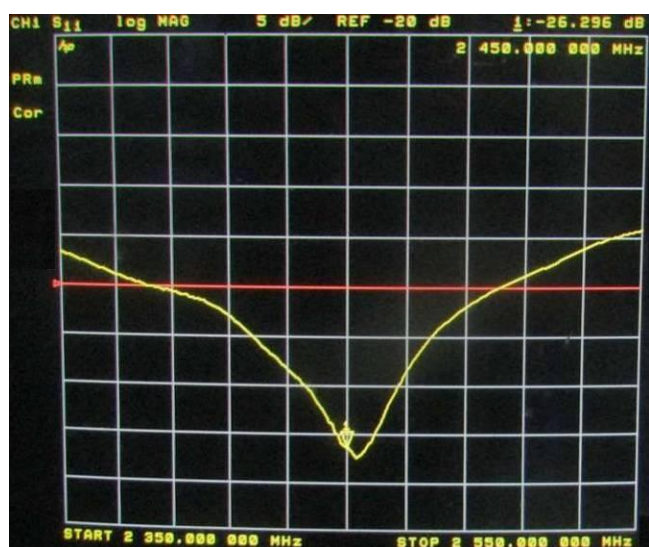
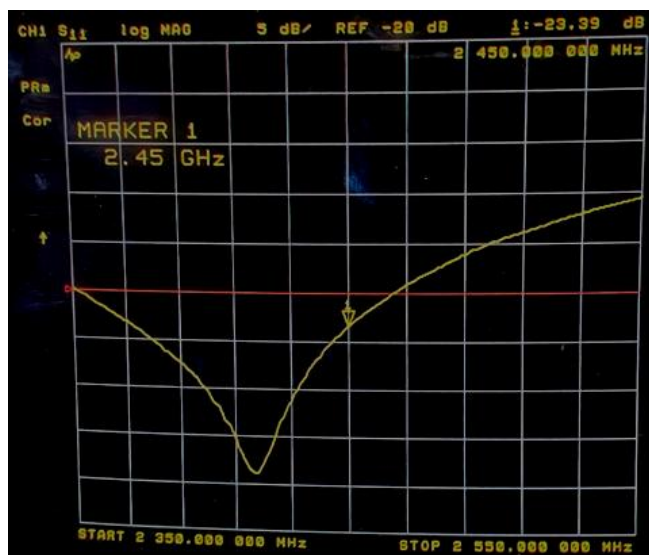


<Head 5200MHz>

| Return Loss (dB) | Delta (%) | Impedance | Delta(ohm) | Date of Measurement |
|------------------|-----------|-----------|------------|---------------------|
| -9.15            | -         | 21.17     | -          | Mar. 01, 2021       |
| -9.1819          | 0.35      | 21.191    | 0.021      | Feb. 28, 2022       |
| -8.317           | 9.10      | 25.673    | 4.503      | Feb. 20, 2023       |

The return loss is <-8dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

Dipole Verification Data

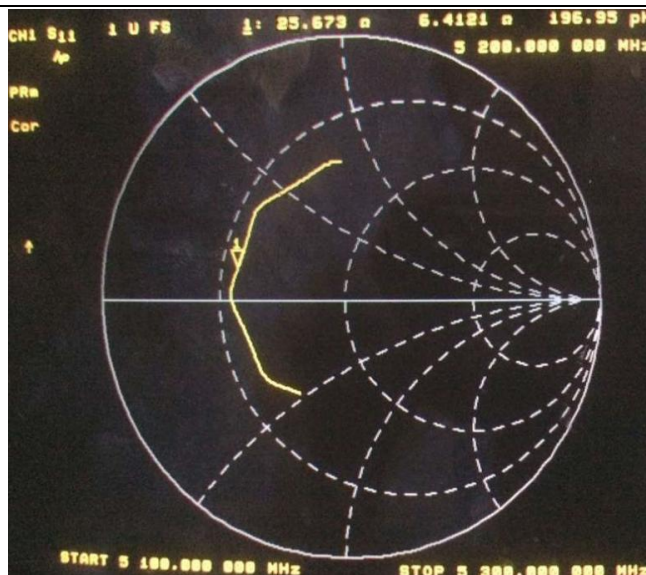
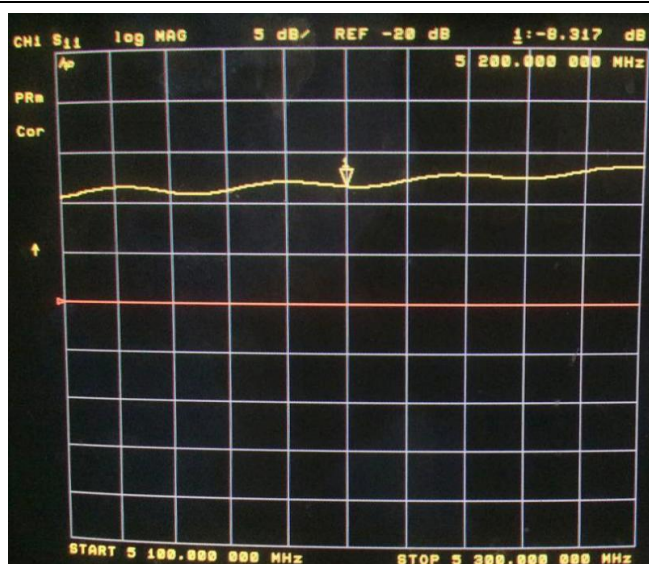
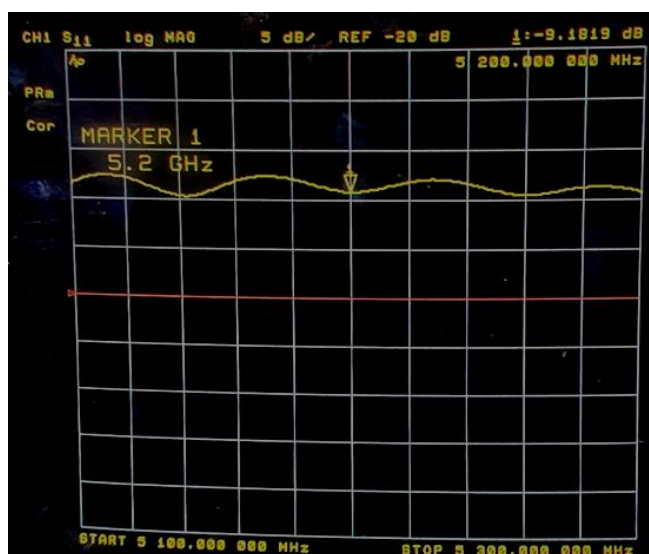


<Head 5800MHz>

| Return Loss (dB) | Delta (%) | Impedance | Delta(ohm) | Date of Measurement |
|------------------|-----------|-----------|------------|---------------------|
| -14.30           | -         | 54.74     | -          | Mar. 01, 2021       |
| -14.349          | 0.34      | 55.115    | 0.375      | Feb. 28, 2022       |
| -12.808          | 10.43     | 55.289    | 0.549      | Feb. 27, 2023       |

The return loss is <-8dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

Dipole Verification Data

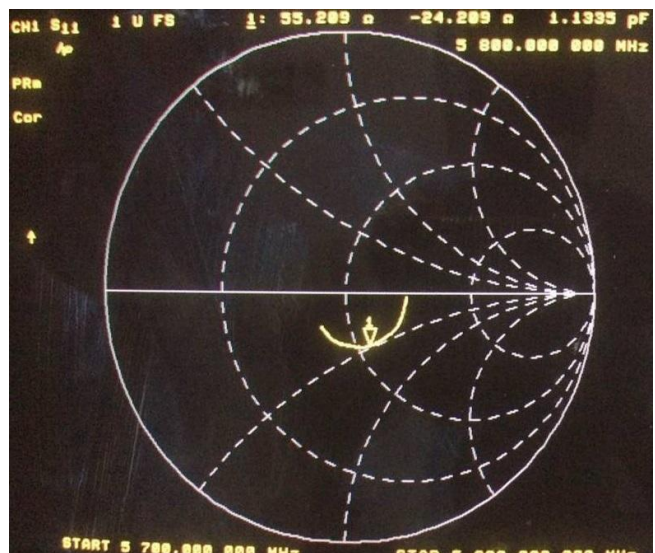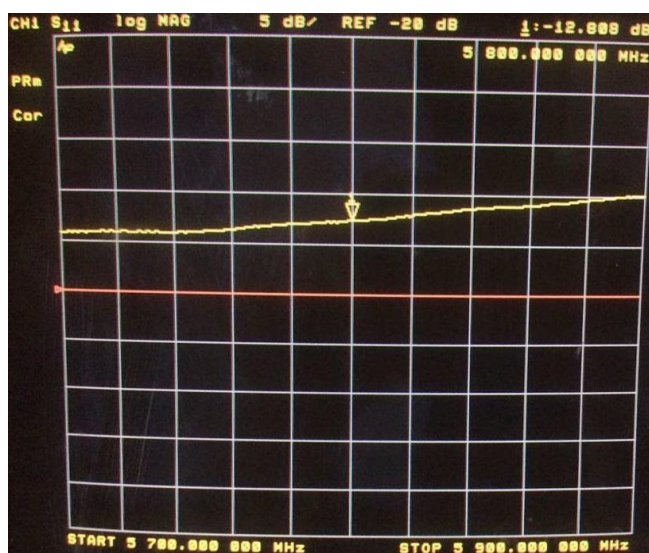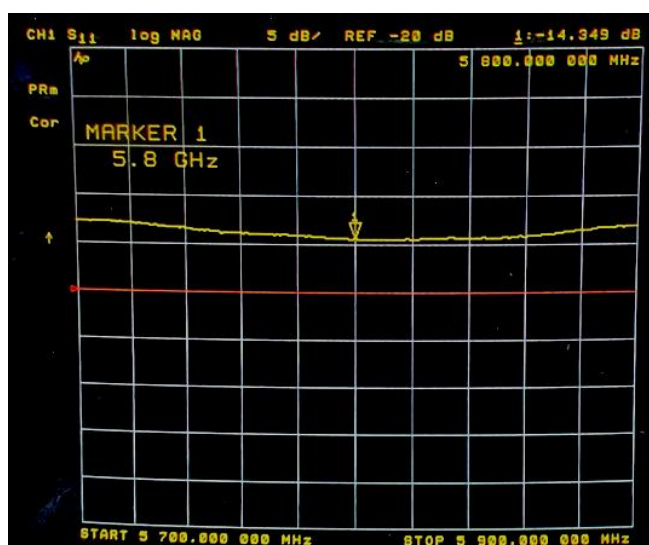

END