

Date: 2026-01-19

**System Check\_Head\_750MHz****DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL\_750\_260119 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.891$  S/m;  $\epsilon_r = 42.9$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(10.72, 10.09, 10.2); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=50mW/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.425 W/kg; SAR (10g) = 0.282 W/kg;


**Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.430 W/kg; SAR (10g) = 0.288 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 86.1 %

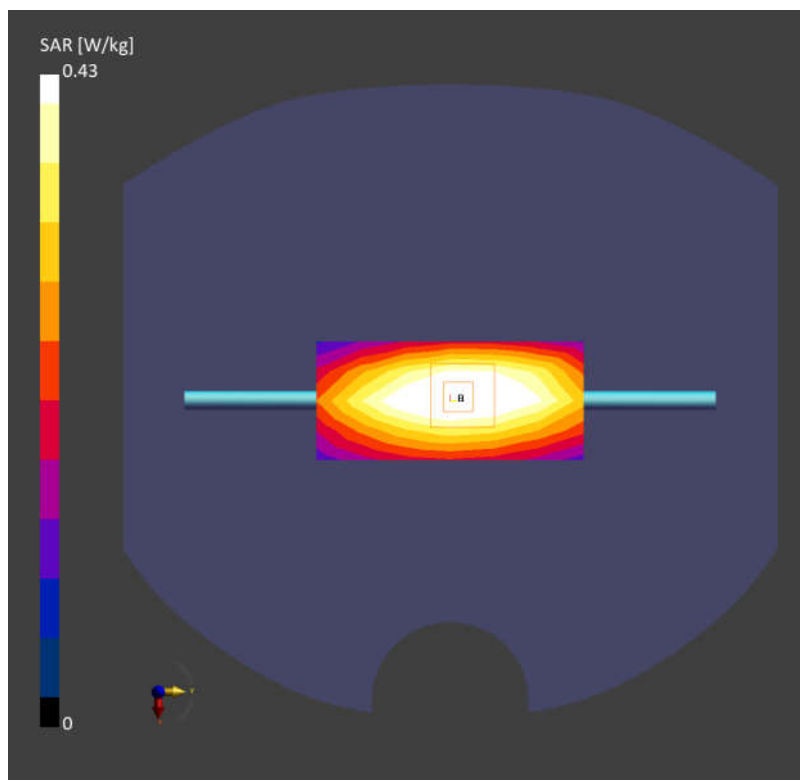

Date: 2026-01-20

**System Check\_Head\_835MHz****DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL\_835\_260120 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.915$  S/m;  $\epsilon_r = 42.6$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(10.4, 9.79, 9.9); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=50mW/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.492 W/kg; SAR (10g) = 0.328 W/kg;


**Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.516 W/kg; SAR (10g) = 0.344 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

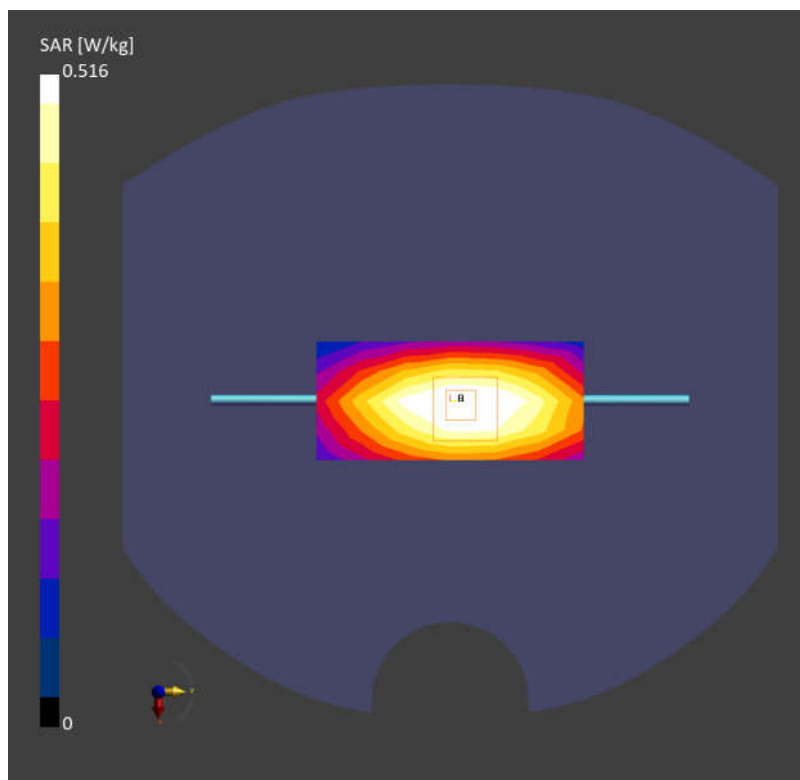

Date: 2026-01-21

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL\_1750\_260121 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.37$  S/m;  $\epsilon_r = 40.7$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(8.3, 7.81, 7.9); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=50mW/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.06 W/kg;


**Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

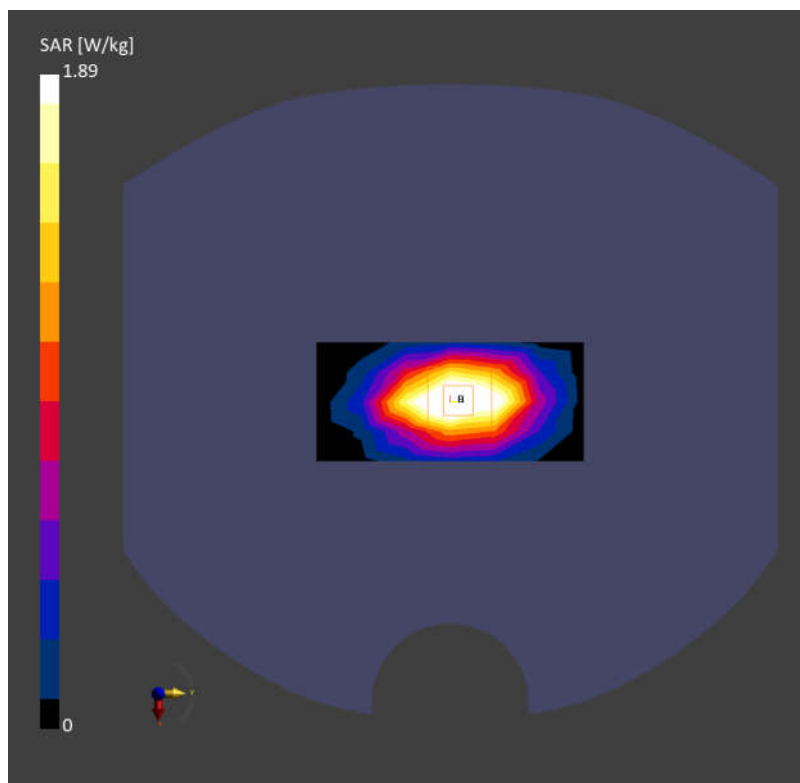

Date: 2026-01-22

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL\_1900\_260122 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.46$  S/m;  $\epsilon_r = 39.2$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(8.09, 7.62, 7.7); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=50mW/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.16 W/kg; SAR (10g) = 1.12 W/kg;

**Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.16 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

