

Measurement Report for 2450.000MHz

Exposure Conditions

Phantom Section, TSL	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	2450.000	6.77	1.69	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 18:35	2025-12-03, 18:45
psSAR1g [W/kg]	5.89	6.07
psSAR10g [W/kg]	2.76	2.84
Power Drift [dB]	-0.02	-0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		81.3
Dist 3dB Peak [mm]		9.9

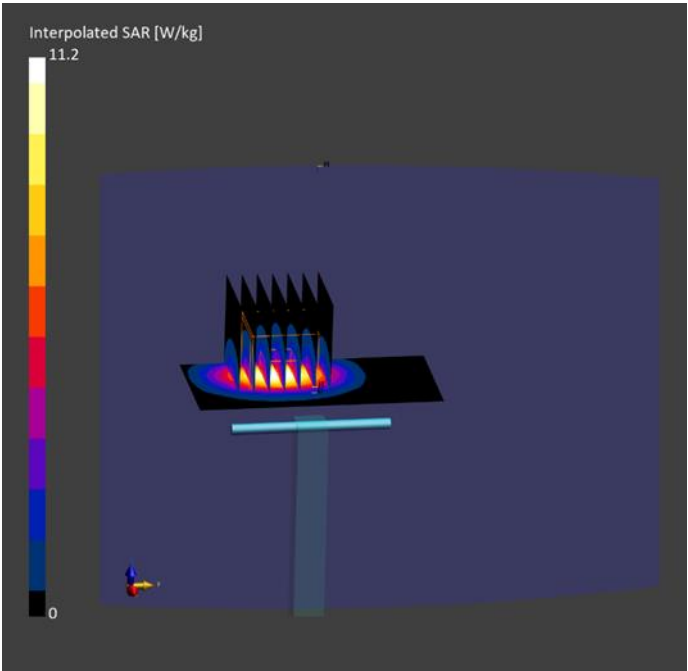

; Name : DAK 3.5 Head 24.1 deg.C 2025-Dec-04 15:27:08						
; Date : 2025-Dec-04 15:27:08						
; Temperature(C) : 24.1						
; Probe : DAK 3.5						
; Network Analyzer : Keysight ENA						
MHz	RefIR	RefII	EpsR	EpsI	Sigma	TanD
2400	0.3889	-0.6417	37.6529	12.4239	1.6588	0.33
2402	0.3885	-0.6418	37.6497	12.4246	1.66	0.33
2402	0.3885	-0.6418	37.6496	12.4247	1.66	0.33
2402	0.3885	-0.6418	37.6495	12.4247	1.6601	0.33
2402	0.3885	-0.6418	37.6493	12.4247	1.6601	0.33
2402	0.3885	-0.6418	37.6491	12.4246	1.6601	0.33
2402	0.3885	-0.6418	37.649	12.4245	1.6602	0.33
2402	0.3884	-0.6418	37.6487	12.4244	1.6602	0.33
2402	0.3884	-0.6419	37.6486	12.4244	1.6602	0.33
2402	0.3884	-0.6419	37.6483	12.4244	1.6603	0.33
2402	0.3884	-0.6419	37.6481	12.4243	1.6603	0.33
2402	0.3884	-0.6419	37.648	12.4243	1.6604	0.33
2402	0.3884	-0.6419	37.6479	12.4243	1.6604	0.33
2402	0.3884	-0.6419	37.6478	12.4243	1.6604	0.33
2402	0.3883	-0.6419	37.6479	12.4243	1.6605	0.33
2402	0.3883	-0.6419	37.6481	12.4243	1.6605	0.33
2412	0.3859	-0.6426	37.6384	12.4296	1.6675	0.3302
2412	0.3859	-0.6426	37.6382	12.4296	1.6675	0.3302
2412	0.3859	-0.6426	37.6378	12.4296	1.6676	0.3302
2412	0.3859	-0.6426	37.6374	12.4295	1.6676	0.3302
2412	0.3858	-0.6426	37.6371	12.4295	1.6676	0.3302
2412	0.3858	-0.6426	37.6367	12.4295	1.6677	0.3302
2412	0.3858	-0.6426	37.6364	12.4296	1.6677	0.3303
2412	0.3858	-0.6426	37.636	12.4297	1.6678	0.3303
2412	0.3858	-0.6426	37.6357	12.4297	1.6678	0.3303
2412	0.3858	-0.6426	37.6355	12.4298	1.6679	0.3303
2412	0.3857	-0.6426	37.6353	12.4298	1.668	0.3303
2412	0.3857	-0.6426	37.635	12.4299	1.668	0.3303
2412	0.3857	-0.6426	37.6349	12.4301	1.6681	0.3303
2412	0.3857	-0.6427	37.6349	12.4302	1.6681	0.3303
2412	0.3857	-0.6426	37.6349	12.4304	1.6682	0.3303
2412	0.3856	-0.6427	37.6351	12.4305	1.6683	0.3303
2412	0.3856	-0.6427	37.6351	12.4305	1.6683	0.3303
2437	0.3786	-0.6445	37.6348	12.4673	1.6899	0.3313
2437	0.3786	-0.6445	37.6349	12.4675	1.69	0.3313

2437	0.3786	-0.6445	37.6352	12.4678	1.6901	0.3313
2437	0.3786	-0.6445	37.6353	12.4679	1.6901	0.3313
2437	0.3785	-0.6445	37.6355	12.4682	1.6902	0.3313
2437	0.3785	-0.6445	37.6356	12.4685	1.6903	0.3313
2437	0.3785	-0.6445	37.6358	12.4686	1.6904	0.3313
2437	0.3785	-0.6445	37.636	12.4686	1.6904	0.3313
2437	0.3784	-0.6445	37.6362	12.4684	1.6904	0.3313
2437	0.3784	-0.6445	37.6363	12.4684	1.6905	0.3313
2437	0.3784	-0.6445	37.6363	12.4683	1.6905	0.3313
2437	0.3784	-0.6446	37.6364	12.4681	1.6905	0.3313
2437	0.3784	-0.6445	37.6364	12.4679	1.6905	0.3313
2437	0.3784	-0.6446	37.6363	12.4676	1.6905	0.3313
2437	0.3784	-0.6446	37.6362	12.4676	1.6906	0.3313
2437	0.3783	-0.6446	37.6362	12.4675	1.6906	0.3313
2440	0.3777	-0.6447	37.6394	12.4721	1.6926	0.3314
2440	0.3777	-0.6448	37.6396	12.4722	1.6927	0.3314
2440	0.3776	-0.6448	37.6398	12.4723	1.6927	0.3314
2440	0.3776	-0.6448	37.64	12.4724	1.6928	0.3314
2440	0.3776	-0.6448	37.6402	12.4723	1.6928	0.3314
2440	0.3776	-0.6448	37.6403	12.4722	1.6929	0.3314
2440	0.3776	-0.6448	37.6405	12.4719	1.6928	0.3313
2440	0.3776	-0.6448	37.6407	12.4716	1.6929	0.3313
2440	0.3775	-0.6448	37.6409	12.4714	1.6929	0.3313
2440	0.3776	-0.6448	37.6409	12.4711	1.6929	0.3313
2440	0.3775	-0.6448	37.641	12.4709	1.6929	0.3313
2440	0.3775	-0.6449	37.6409	12.4707	1.6929	0.3313
2440	0.3775	-0.6449	37.641	12.4706	1.6929	0.3313
2440	0.3775	-0.6449	37.641	12.4705	1.693	0.3313
2440	0.3775	-0.6449	37.6411	12.4706	1.693	0.3313
2440	0.3774	-0.6449	37.6412	12.4708	1.6931	0.3313
2440	0.3774	-0.6449	37.6414	12.4708	1.6931	0.3313
2450	0.3743	-0.6458	37.6752	12.4895	1.702	0.3315
2450	0.3743	-0.6459	37.6747	12.4888	1.7019	0.3315
2450	0.3743	-0.6459	37.6739	12.4882	1.7019	0.3315
2450	0.3742	-0.6459	37.6733	12.4877	1.7019	0.3315
2450	0.3742	-0.6459	37.6725	12.4873	1.7018	0.3315
2450	0.3742	-0.6459	37.6719	12.4869	1.7018	0.3315
2450	0.3742	-0.6459	37.6713	12.4864	1.7018	0.3315
2450	0.3742	-0.6459	37.6709	12.4861	1.7018	0.3315
2450	0.3743	-0.6459	37.6706	12.4858	1.7018	0.3314
2450	0.3743	-0.6459	37.6704	12.4857	1.7018	0.3314
2450	0.3742	-0.6459	37.6702	12.4856	1.7019	0.3314

2450	0.3742	-0.6459	37.6702	12.4856	1.7019	0.3314
2450	0.3742	-0.6459	37.6703	12.4857	1.702	0.3314
2450	0.3741	-0.6459	37.6707	12.4858	1.702	0.3314
2450	0.3741	-0.6459	37.6713	12.486	1.7021	0.3314
2462	0.3711	-0.6474	37.688	12.465	1.707	0.3307
2462	0.371	-0.6474	37.6881	12.4649	1.707	0.3307
2462	0.371	-0.6474	37.6882	12.4648	1.707	0.3307
2462	0.371	-0.6474	37.6883	12.4647	1.707	0.3307
2462	0.371	-0.6475	37.6884	12.4646	1.7071	0.3307
2462	0.371	-0.6475	37.6886	12.4644	1.7071	0.3307
2462	0.371	-0.6475	37.6887	12.4642	1.7071	0.3307
2462	0.3709	-0.6475	37.6888	12.464	1.7071	0.3307
2462	0.3709	-0.6475	37.689	12.4637	1.7071	0.3307
2462	0.3709	-0.6475	37.689	12.4635	1.7071	0.3307
2462	0.3709	-0.6475	37.6889	12.4632	1.7071	0.3307
2462	0.3709	-0.6475	37.6889	12.4629	1.7072	0.3307
2462	0.3709	-0.6475	37.6888	12.4627	1.7072	0.3307
2462	0.3709	-0.6476	37.6886	12.4625	1.7072	0.3307
2462	0.3709	-0.6476	37.6883	12.4622	1.7072	0.3307
2480	0.3667	-0.6495	37.6766	12.4253	1.7139	0.3298
2480	0.3667	-0.6495	37.6764	12.4251	1.7139	0.3298
2480	0.3667	-0.6495	37.6762	12.425	1.714	0.3298
2480	0.3667	-0.6495	37.6761	12.4249	1.714	0.3298
2480	0.3667	-0.6496	37.676	12.4247	1.714	0.3298
2480	0.3667	-0.6495	37.6759	12.4246	1.714	0.3298
2480	0.3666	-0.6495	37.6758	12.4245	1.7141	0.3298
2480	0.3666	-0.6495	37.6758	12.4244	1.7141	0.3298
2480	0.3666	-0.6496	37.6756	12.4242	1.7141	0.3298
2480	0.3666	-0.6496	37.6755	12.424	1.7141	0.3298
2480	0.3666	-0.6496	37.6754	12.4239	1.7142	0.3298
2480	0.3666	-0.6496	37.6753	12.4238	1.7142	0.3298
2480	0.3666	-0.6496	37.6752	12.4237	1.7142	0.3298
2480	0.3665	-0.6496	37.6751	12.4237	1.7143	0.3298
2480	0.3665	-0.6496	37.675	12.4236	1.7143	0.3298
2480	0.3665	-0.6496	37.6749	12.4236	1.7143	0.3298
2480	0.3665	-0.6496	37.6747	12.4236	1.7144	0.3298
2500	0.3621	-0.651	37.6191	12.4078	1.7257	0.3298

Measurement Report for (2450.000MHz)
Exposure Conditions

Phantom Section, TSL	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	2450.000	6.77	1.69	37.7

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 19:47	2025-12-04, 19:57
psSAR1g [W/kg]	5.28	5.45
psSAR10g [W/kg]	2.57	2.62
Power Drift [dB]	-0.05	0.01
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		81.6
Dist 3dB Peak		9.9
[mm]		

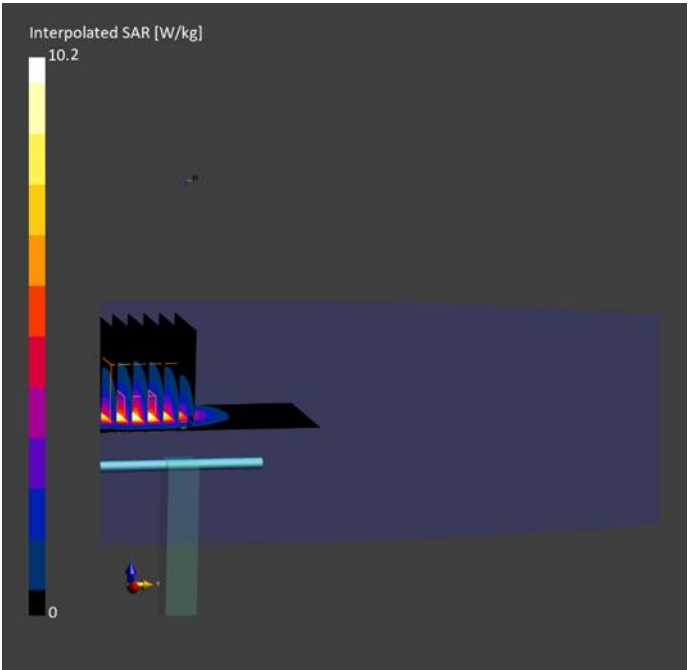

15 Annex E – SAR Plots

Measurement Report for Azena Medical, LLC., FRONT, 2.4 GHz BLE, 2440.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	15.0 x 15.0	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	Y
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 19:08	2025-12-03, 19:52
psSAR1g [W/kg]	0.120	0.124
psSAR10g [W/kg]	0.044	0.047
Power Drift [dB]	0.11	0.20
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only

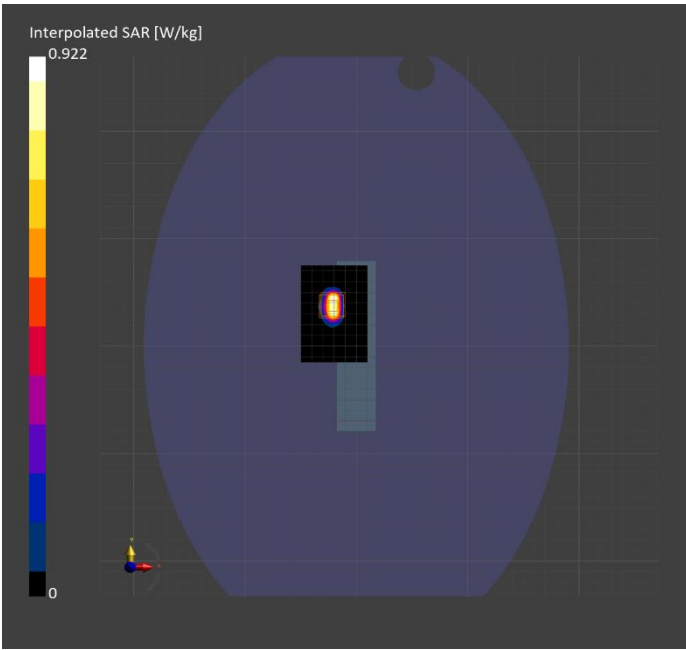

Plot #1

Measurement Report for Azena Medical, LLC., REAR, 2.4 GHz BLE, 2440.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	REAR, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 200.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	All points	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 20:15	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	0.19	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

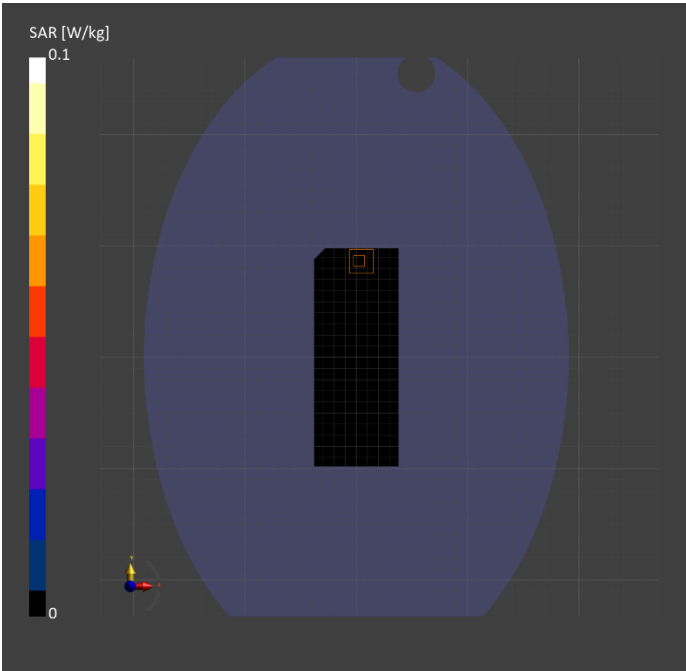

Plot #2

Measurement Report for Azena Medical, LLC., EDGE LEFT, 2.4 GHz BLE, 2402.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE LEFT, 0.00	2402.000	6.77	1.65	39.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 21:52	2025-12-03, 22:16
psSAR1g [W/kg]	0.167	0.184
psSAR10g [W/kg]	0.060	0.059
Power Drift [dB]	0.07	0.16
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only

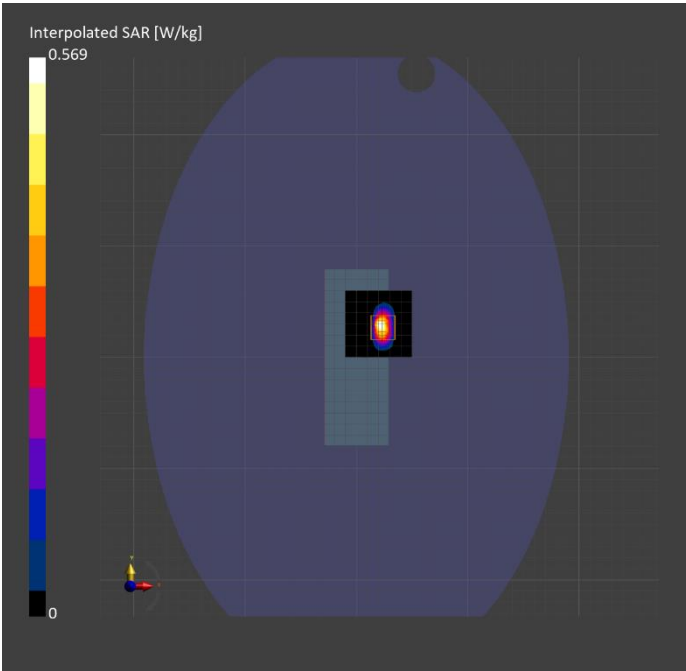

Plot #3

Measurement Report for Azena Medical, LLC., EDGE LEFT, 2.4 GHz BLE, 2440.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE LEFT, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 20:32	2025-12-03, 20:56
psSAR1g [W/kg]	0.136	0.132
psSAR10g [W/kg]	0.043	0.040
Power Drift [dB]	-0.02	0.18
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only

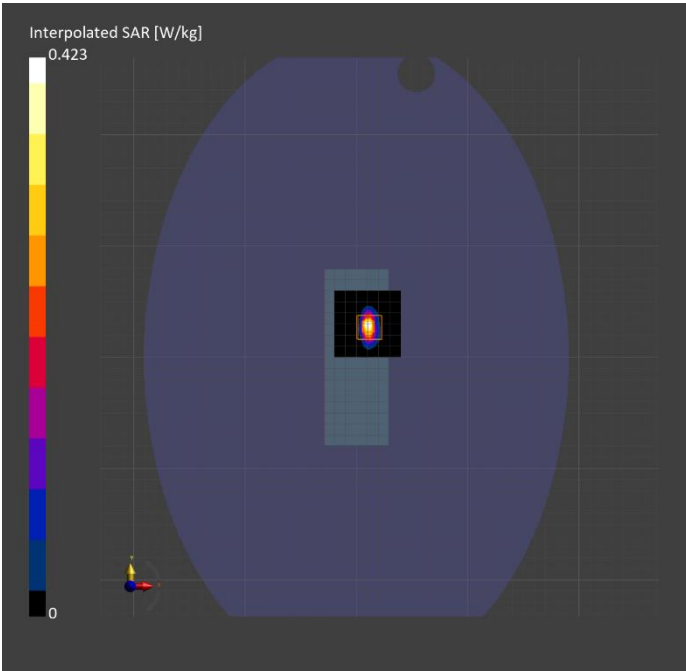

Plot #4

Measurement Report for Azena Medical, LLC., EDGE LEFT, 2.4 GHz BLE, 2480.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE LEFT, 0.00	2480.000	6.77	1.71	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.5 x 3.5 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	Y
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 22:29	2025-12-03, 23:02
psSAR1g [W/kg]	0.054	0.054
psSAR10g [W/kg]	0.017	0.013
Power Drift [dB]	0.18	0.17
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only

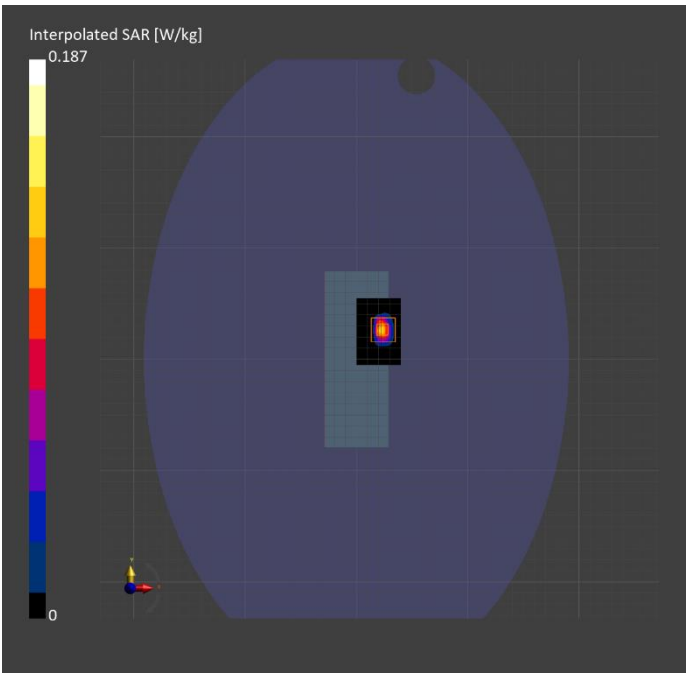

Plot #5

Measurement Report for Azena Medical, LLC., EDGE RIGHT, 2.4 GHz BLE, 2440.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE RIGHT, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	100.0 x 200.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 21:21	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	-0.14	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

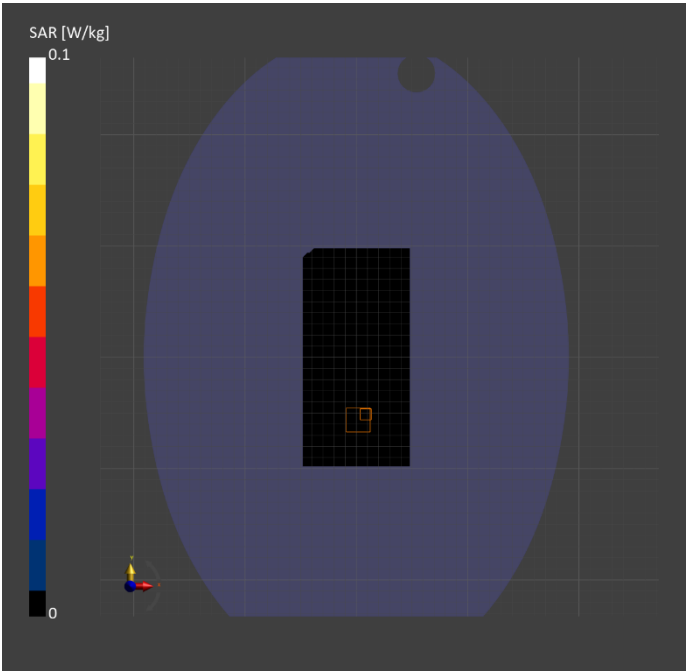

Plot #6

Measurement Report for Azena Medical, LLC., EDGE TOP, 2.4 GHz BLE, 2440.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE TOP, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	100.0 x 80.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 23:24	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	-0.07	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

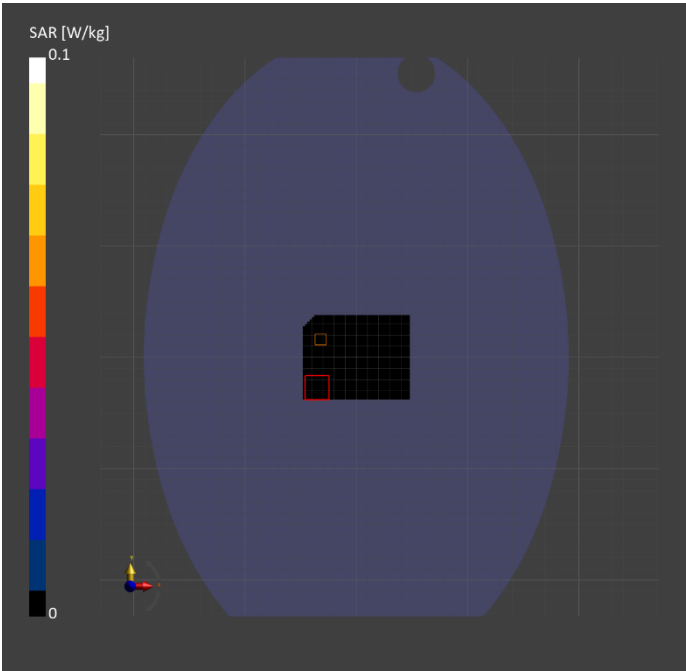

Plot #7

Measurement Report for Azena Medical, LLC., EDGE BOTTOM, 2.4 GHz BLE, 2440.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE BOTTOM, 0.00	2440.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	100.0 x 80.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-03, 23:49	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	0.01	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

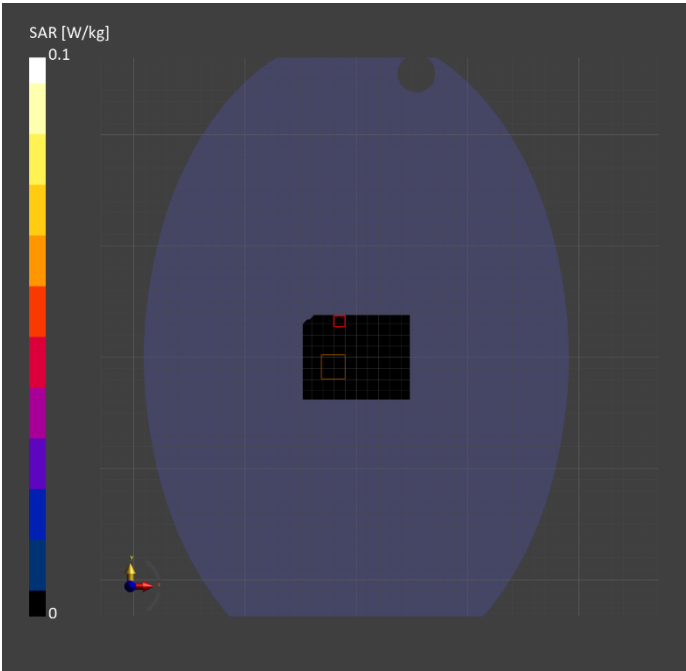

Plot #8

Measurement Report for Azena Medical, LLC., EDGE LEFT, 2.4 GHz BLE, 2402.000MHz (Repeat)
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE LEFT, 0.00	2402.000	6.77	1.66	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	Y
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-05, 02:12	2025-12-05, 02:36
psSAR1g [W/kg]	0.135	0.145
psSAR10g [W/kg]	0.048	0.049
Power Drift [dB]	-0.06	-0.20
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

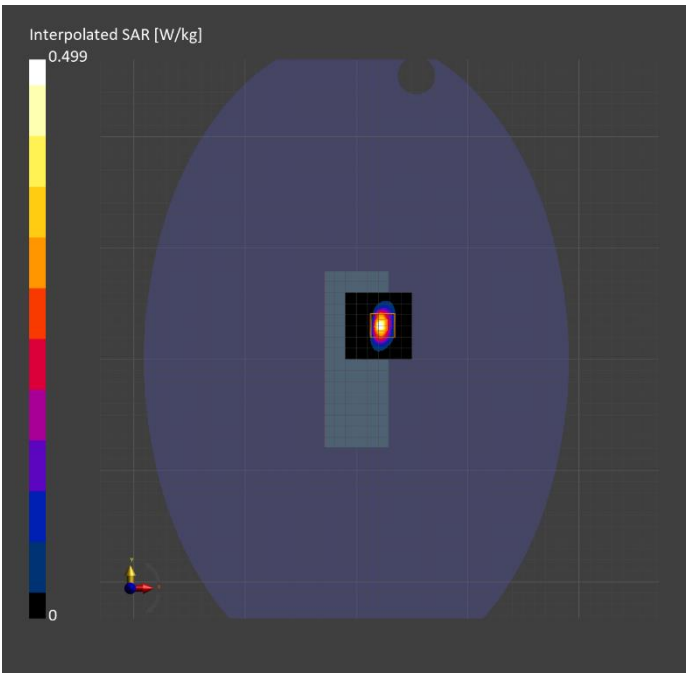

Plot #9

Measurement Report for Azena Medical, LLC., FRONT, WLAN (DSSS) 2.4GHz, 2412.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2412.000	6.77	1.67	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	2.7 x 2.7 x 1.2
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.2
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 21:36	2025-12-04, 22:46
psSAR1g [W/kg]	0.384	0.396
psSAR10g [W/kg]	0.164	0.164
Power Drift [dB]	-0.03	-0.02
Power Scaling	Disabled	Disabled
Scaling Factor		
[dB]		
TSL Correction	Positive only	Positive only

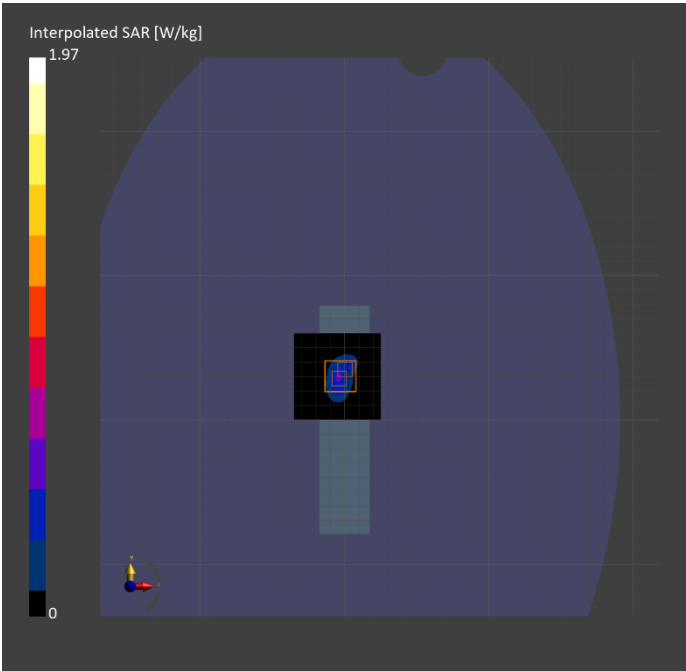

Plot #10

Measurement Report for Azena Medical, LLC., FRONT, WLAN (DSSS) 2.4GHz, 2437.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2437.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	2.6 x 2.6 x 1.2
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.2
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 09:50	2025-12-04, 10:48
psSAR1g [W/kg]	0.286	0.279
psSAR10g [W/kg]	0.116	0.114
Power Drift [dB]	0.08	-0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

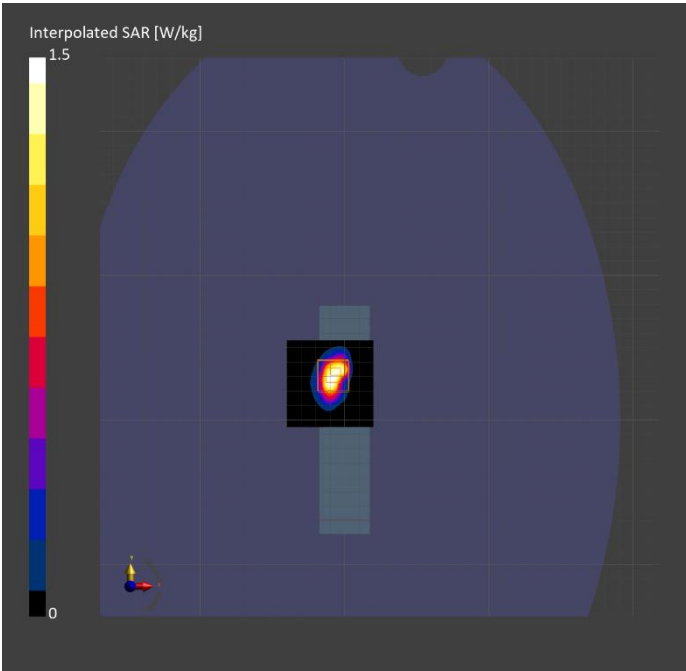

Plot #11

Measurement Report for Azena Medical, LLC., FRONT, WLAN (DSSS) 2.4GHz, 2462.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2462.000	6.77	1.70	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.5 x 3.5 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 17:07	2025-12-04, 17:38
psSAR1g [W/kg]	0.346	0.348
psSAR10g [W/kg]	0.141	0.142
Power Drift [dB]	-0.09	-0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

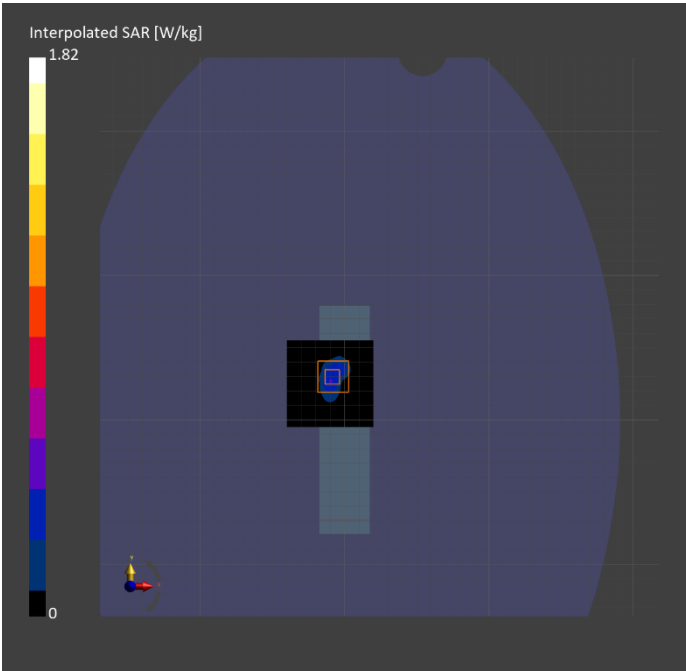

Plot #12

Measurement Report for Azena Medical, LLC., REAR, WLAN (DSSS) 2.4GHz, 2437.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	REAR, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 200.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 20:27	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	0.14	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

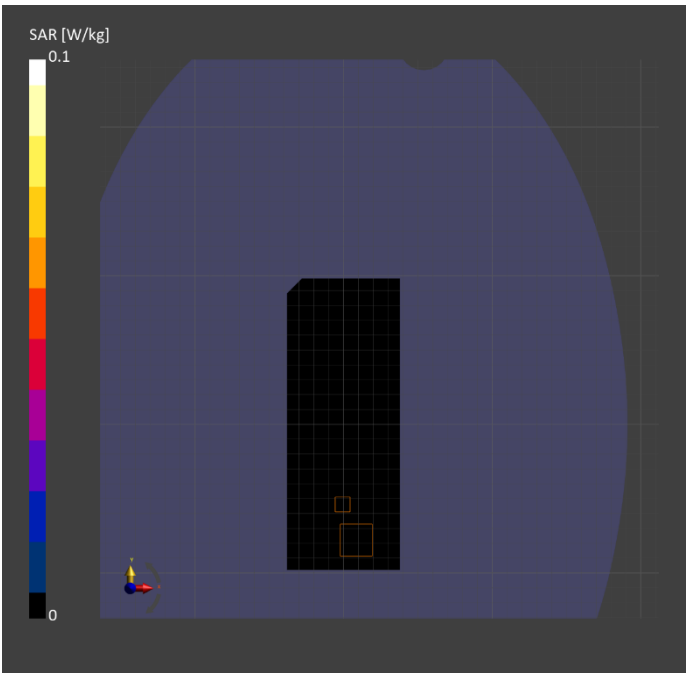

Plot #13

Measurement Report for Azena Medical, LLC., EDGE LEFT, WLAN (DSSS) 2.4GHz, 2437.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE LEFT, 0.00	2437.000	6.77	1.68	39.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-03	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	3.8 x 3.8 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 12:59	2025-12-04, 13:28
psSAR1g [W/kg]	0.263	0.277
psSAR10g [W/kg]	0.094	0.091
Power Drift [dB]	0.05	-0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

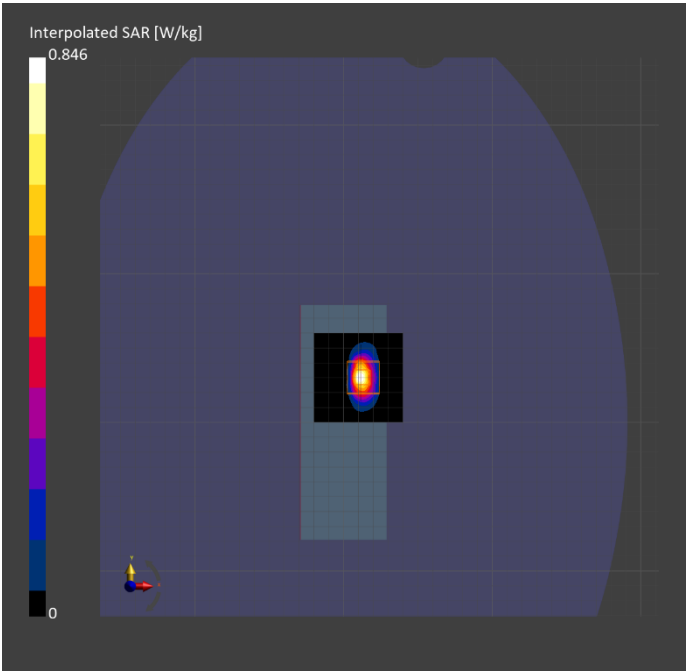

Plot #14

Measurement Report for Azena Medical, LLC., EDGE RIGHT, WLAN (DSSS) 2.4GHz, 2437.000MHz

Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE RIGHT, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	100.0 x 200.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	All points	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 20:52	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	0.20	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

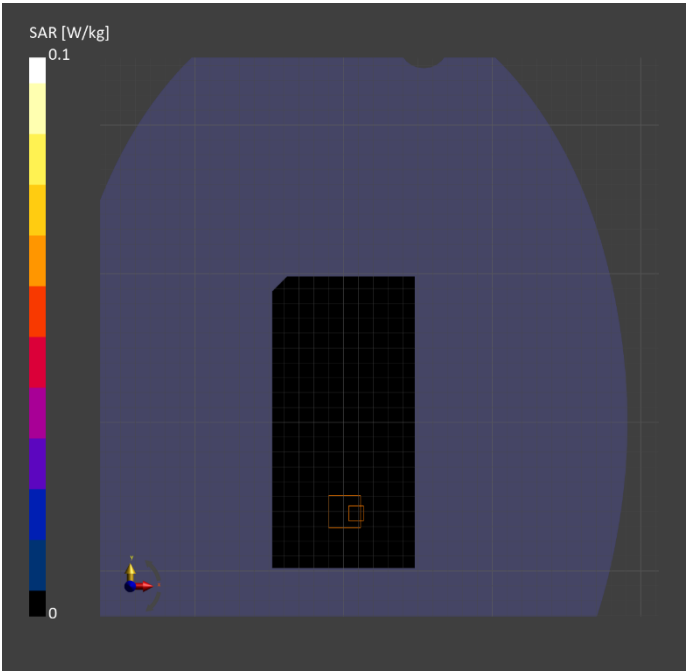

Plot #15

Measurement Report for Azena Medical, LLC., EDGE TOP, WLAN (DSSS) 2.4GHz, 2437.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE TOP, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	100.0 x 80.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 21:08	
psSAR1g [W/kg]	0	
psSAR10g [W/kg]	0	
Power Drift [dB]	-0.15	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

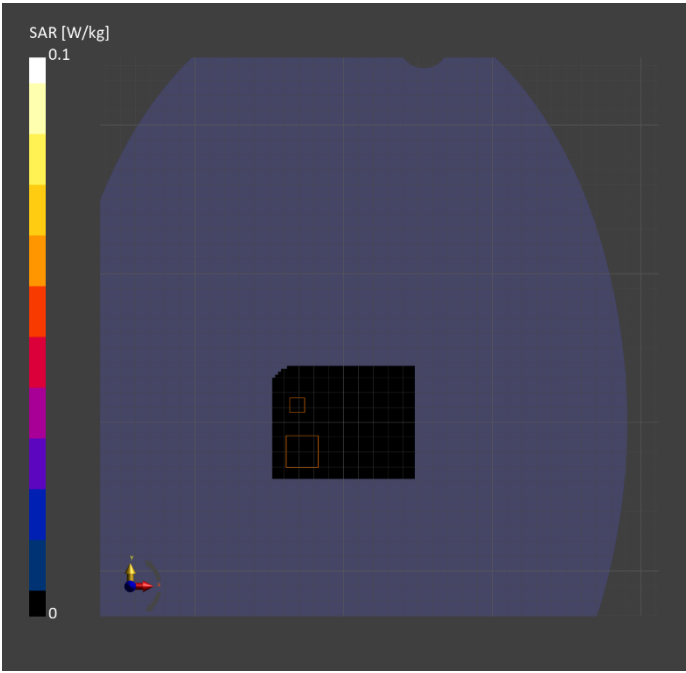

Plot #16

Measurement Report for Azena Medical, LLC., EDGE BOTTOM, WLAN (DSSS) 2.4GHz, 2437.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	EDGE BOTTOM, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	80.0 x 120.0	x x
Grid Steps [mm]	10.0 x 10.0	x x
Sensor Surface [mm]	3.0	
Graded Grid	N/A	
Grading Ratio	N/A	
MAIA	Y	
Surface Detection	Unknown method	
Scan Method	Measured	

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 21:23	
psSAR1g [W/kg]	0.002	
psSAR10g [W/kg]	0	
Power Drift [dB]	-0.17	
Power Scaling	Disabled	
Scaling Factor		
[dB]		
TSL Correction	Positive only	

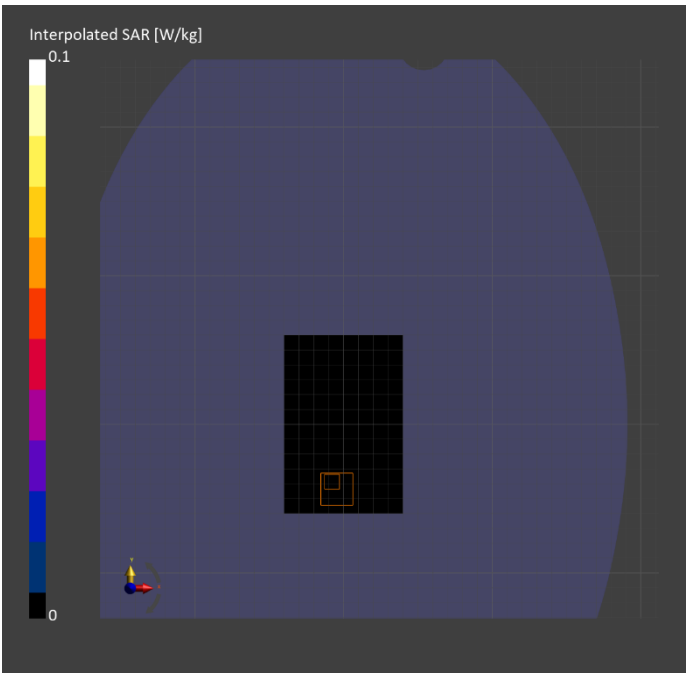

Plot #17

Measurement Report for Azena Medical, LLC., FRONT, WLAN (OFDM) 2.4GHz, 2437.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	2.7 x 2.7 x 1.2
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.2
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-04, 22:59	2025-12-04, 23:54
psSAR1g [W/kg]	0.686	0.696
psSAR10g [W/kg]	0.287	0.291
Power Drift [dB]	0.01	0.15
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

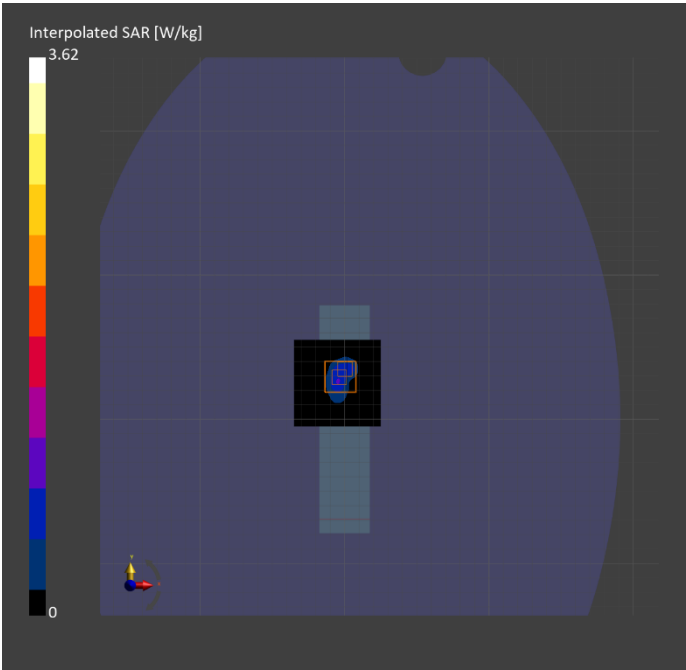

Plot #18

Measurement Report for Azena Medical, LLC., FRONT, WLAN (OFDM) 2.4GHz, 2462.000MHz
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2462.000	6.77	1.71	37.7

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	2.5 x 2.5 x 1.2
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.2
MAIA	Y	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-05, 00:06	2025-12-05, 01:20
psSAR1g [W/kg]	0.325	0.331
psSAR10g [W/kg]	0.132	0.137
Power Drift [dB]	0.05	0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

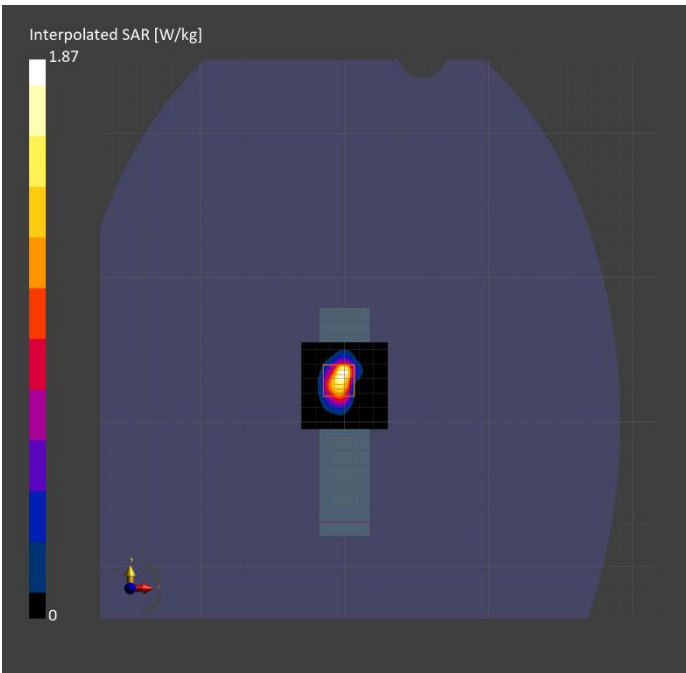

Plot #19

Measurement Report for Azena Medical, LLC., FRONT, WLAN (OFDM) 2.4GHz, 2437.000MHz (Repeat)
Device under Test Properties

Model, Manufacturer	Dimensions [mm]	DUT Type
Vision, Azena Medical, LLC.	158.0 x 35.0 x 58.0	Oral Treatment Device

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	FRONT, 0.00	2437.000	6.77	1.69	37.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2191	HBBL-600-10000 SLAAHU16BC221222-1, 2025-Dec-04	EX3DV4 - SN7783, 2025-03-12	DAE4 Sn1724, 2025-03-14

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	60.0 x 60.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	All points	All points
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2025-12-05, 01:28	2025-12-05, 01:55
psSAR1g [W/kg]	0.700	0.680
psSAR10g [W/kg]	0.294	0.285
Power Drift [dB]	-0.07	-0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only

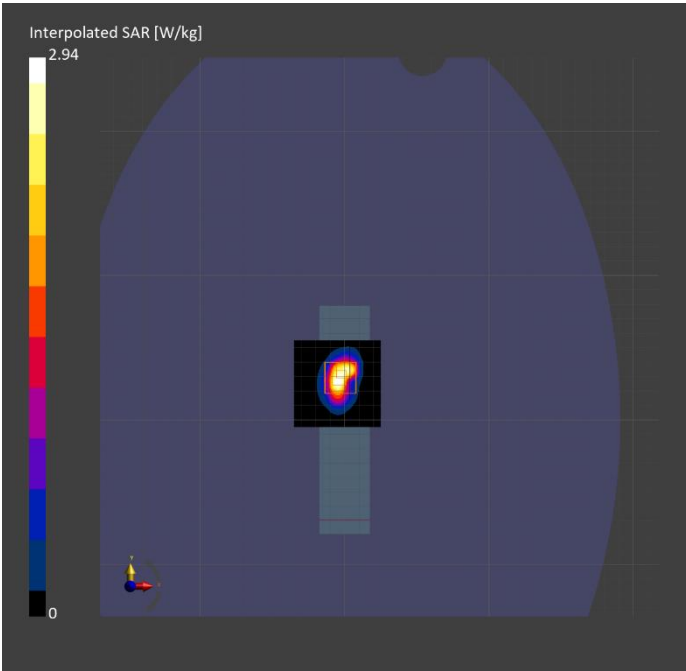

Plot #20

16 Annex F – RF Average Output Power Measurement

Mode	Channel	Frequency (MHz)	Measured Conducted Power (dBm)	Rated Conducted Power (dBm)	Antenna Gain (dBi)	EIRP (dBm)	Rated EIRP (dBm)
BLE 2M (GFSK)	Low	2402	11.11	12.00	3.35	14.46	15.35
	Middle	2440	10.53	11.50	3.35	13.88	14.85
	High	2480	7.30	8.00	3.35	10.65	11.35
802.11b (DSSS)	Low	2412	15.40	15.50	3.35	18.75	18.85
	Middle	2437	12.51	13.00	3.35	15.86	16.35
	High	2462	13.87	14.00	3.35	17.22	17.35
802.11g (OFDM)	Low	2412	14.47	15.00	3.35	17.82	18.35
	Middle	2437	17.08	17.50	3.35	20.43	20.85
	High	2462	14.63	15.00	3.35	17.98	18.35

Note 1: The average output power for tested modes and channels were re-measured at the beginning of SAR testing.

Note 2: The software used to configure the radio was “EspRFTestTool_v4.9_Manual”.

17 Annex G – DUT Test Setup Photographs

Please refer to attached file.

18 Annex H - Informative References

- [1] Federal Communications Commission, "Report and order: Guidelines for evaluating the environmental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- [2] David L. Means Kwok Chan, Robert F. Cleveland, "Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commission, Office of Engineering & Technology, Washington, DC, 1997.
- [3] Thomas Schmid, Oliver Egger, and Niels Kuster, "Automated E-field scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105-113, Jan. 1996.
- [4] Niels Kuster, Ralph Kastle, and Thomas Schmid, "Dosimetric evaluation of mobile communications equipment with known precision", IEEE Transactions on Communications, vol. E80-B, no. 5, pp. 645-652, May 1997.
- [5] CENELEC, "Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1992: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, "Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies", in ICECOM '97, Dubrovnik, October 15-17, 1997, pp. 120-24.
- [8] Katja Pokovic, Thomas Schmid, and Niels Kuster, "E-field probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23-25 June, 1996, pp. 172-175.
- [9] Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard Kuhn, and Niels Kuster, "The dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865-1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, "The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Recipes in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992. Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, "The treatment of uncertainty in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, "Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10.

19 Annex I (Normative) - A2LA Electrical Testing Certificate**Accredited Laboratory**

A2LA has accredited

BAY AREA COMPLIANCE LABORATORIES CORP.

Sunnyvale, CA

for technical competence in the field of

Electrical Testing

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017 General requirements for the competence of testing and calibration laboratories. This laboratory also meets A2LA R222 - Specific Requirements EPA ENERGY STAR Accreditation Program. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

Presented this 13th day of September 2024.

Mr. Trace McInturff, Vice President, Accreditation Services
For the Accreditation Council
Certificate Number 3297.02
Valid to September 30, 2026

For the tests to which this accreditation applies, please refer to the laboratory's Electrical Scope of Accreditation.

Please follow the web link below for a full ISO 17025 scope

[A2LA Scope ~ Cert. 3297-02.pdf](#)

--- END OF REPORT ---