



Appendix D


Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details







1. SAR measurement System

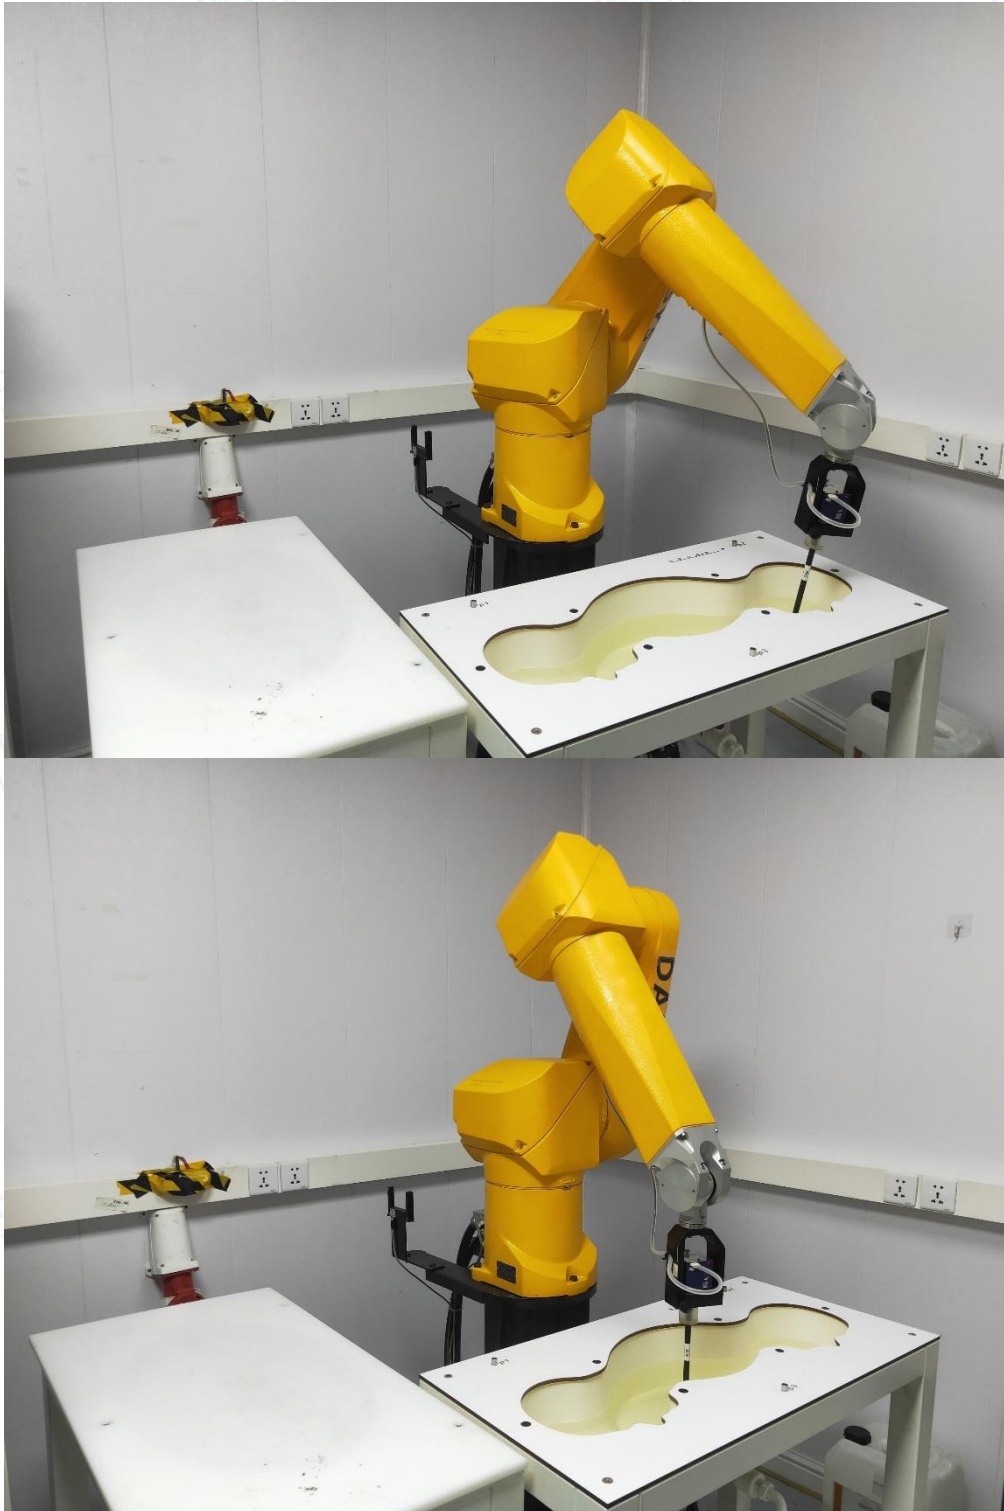



2. Photographs of Tissue Simulate Liquid

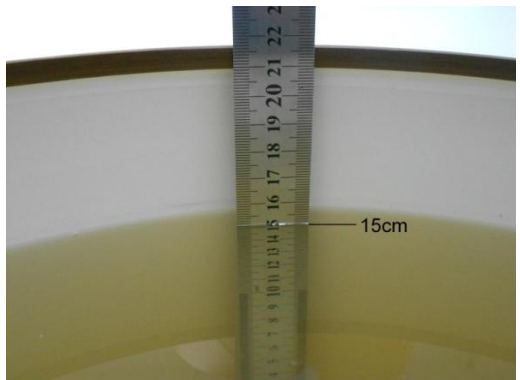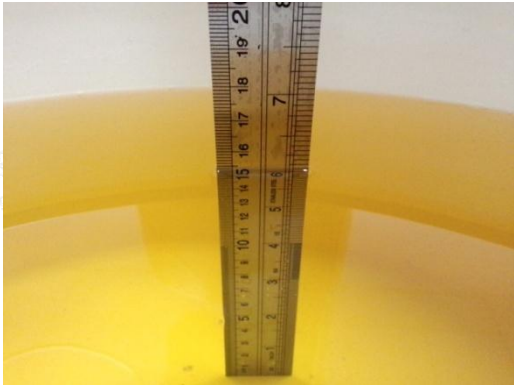Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	
Photo 7: Tissue Simulant Liquid for Head 5000	NA





3. Photographs of EUT test position

Photo 8: Left touch cheek

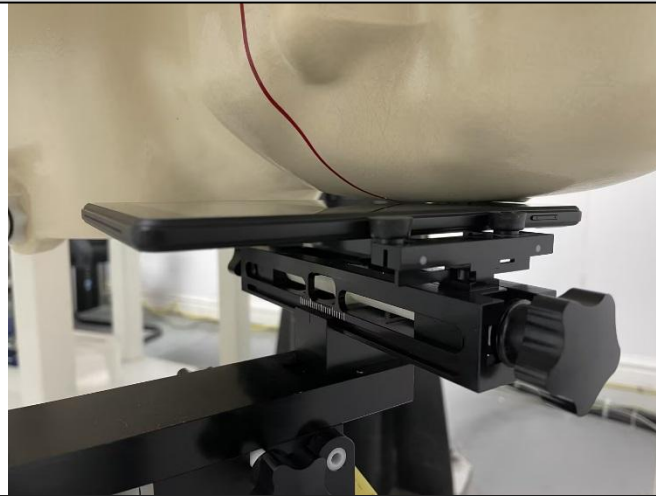


Photo 9: Left tilted 15 degree

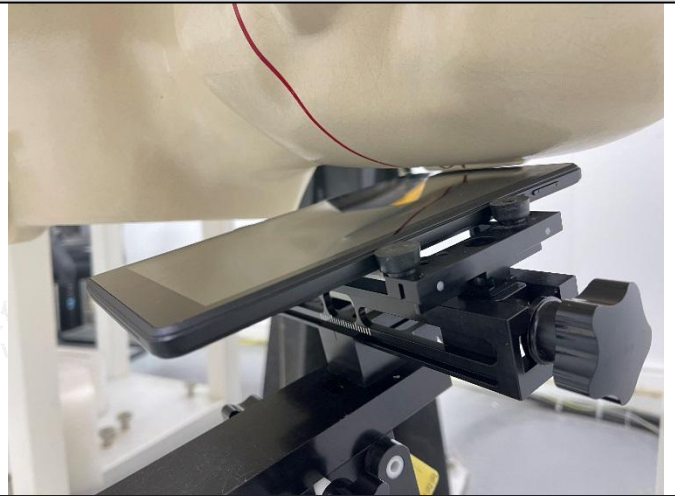


Photo 10: Right touch cheek



Photo 11: Right tilted 15 degree

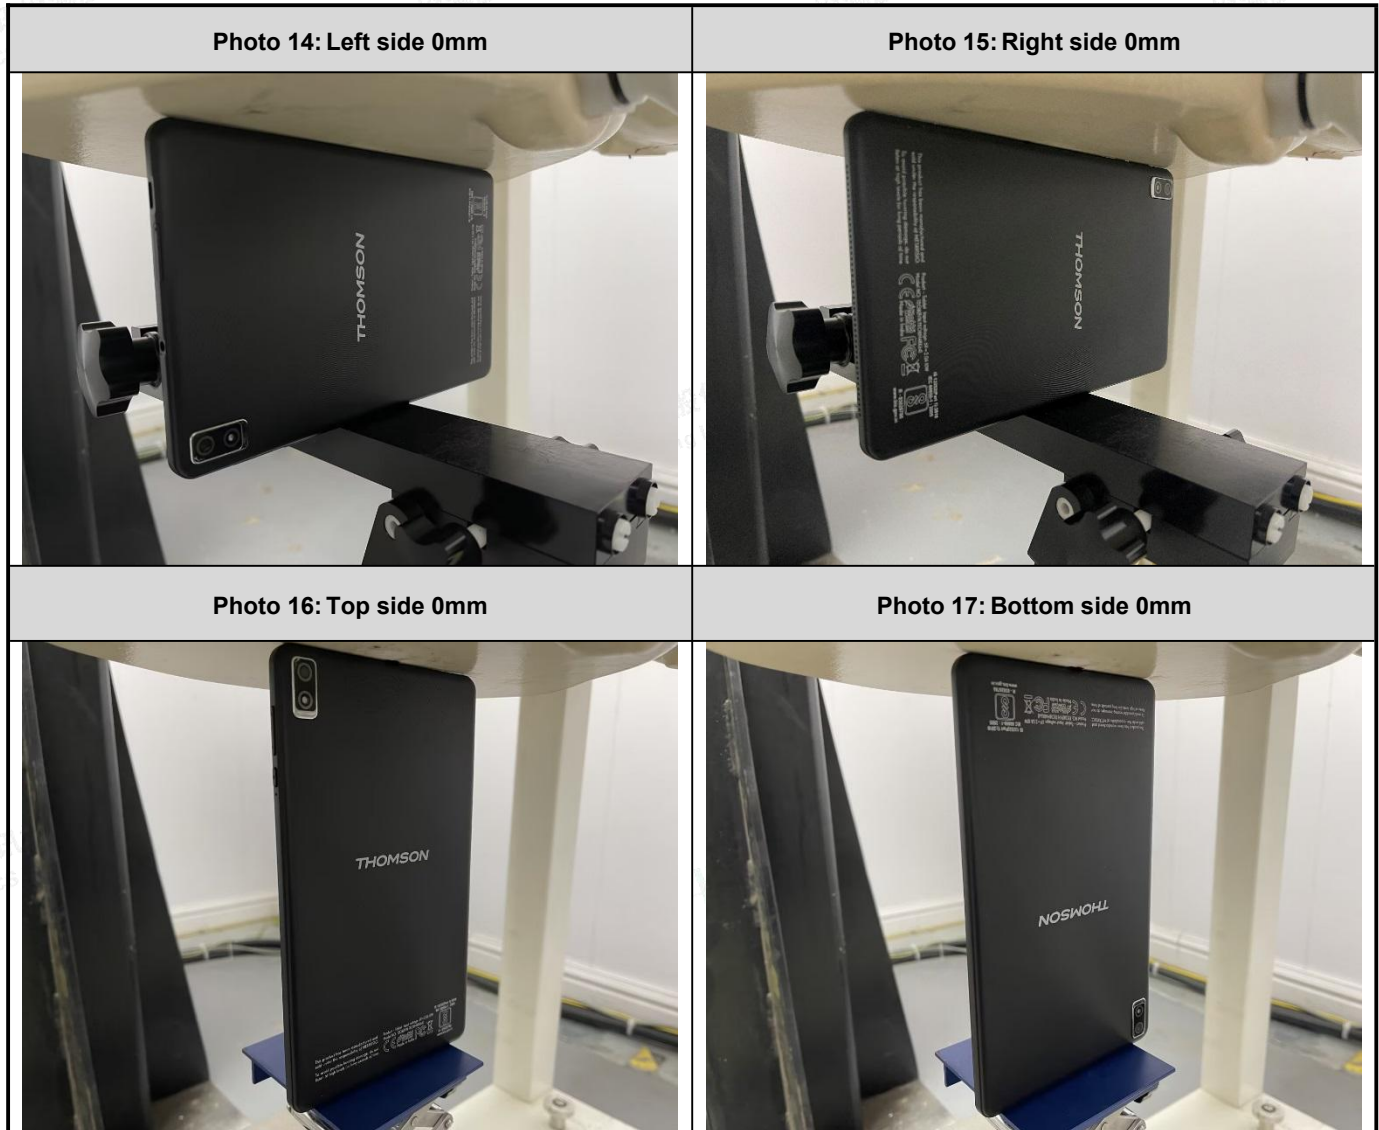


Photo 12: Front side 0mm



Photo 13: Back side 0mm







4. EUT Constructional Details

