



Impedance Plot for SN 29/15 DIP 2G450-393 2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $50.0\Omega + 5.0j\Omega$ (within 5Ω)

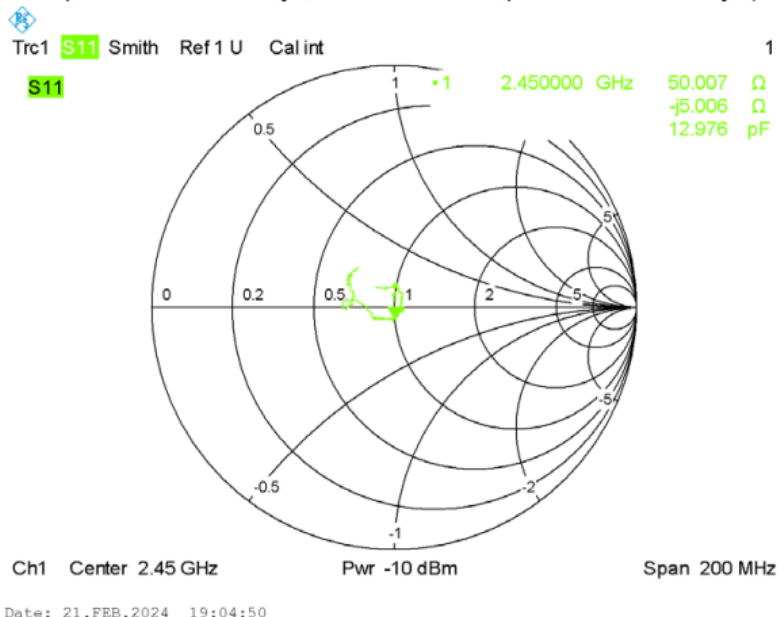

Calibrated return loss: -27.80dB; Measurement return loss: -26.75dB (within 20%)

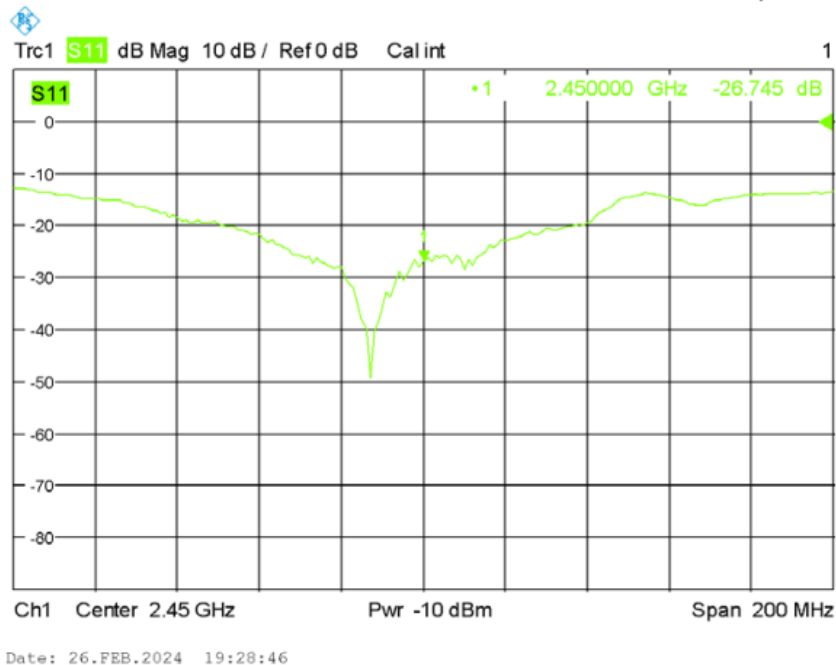

not having not been signed by authorized approver, or having been altered without authorization, or having not been stamped by the "Dedicated Test Report" is deemed to be invalid. Copying or excerpting portion of, or altering the content of the report is not permitted without the written authorization of AGC. The data and results in the report apply only to the tested sample. Any objections to report issued by AGC should be submitted to AGC within 15 days after the issuance of the report. Any inquiry of validity or verification of the test report should be addressed to AGC by agc01@agccert.com.

AGC of Global Compliance (Shenzhen) Co., Ltd

AGC of Global Compliance (Shenzhen) Std & Tech Co., Ltd

+86-755 2523 4088

E-mail: agc@agccert.com

Web: <http://www.agccert.com/>