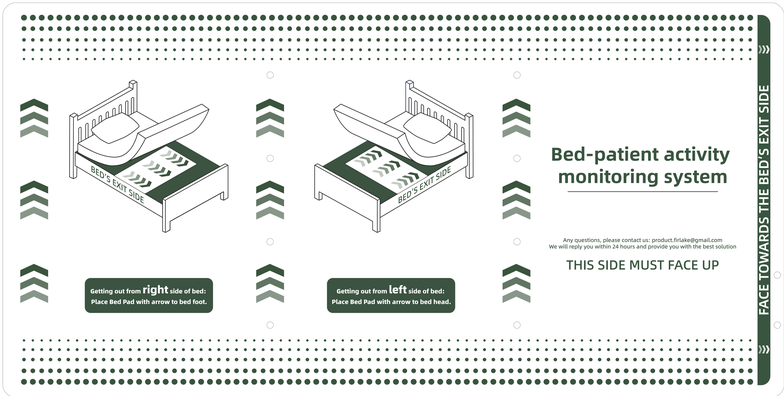
BED'S EXIT SIDE
BED'S EXIT SIDE
Getting out from right side of bed:
Place Bed Pad with arrow to bed foot.
Getting out from left side of bed:
Place Bed Pad with arrow to bed head.
Bed-patient activity monitoring system
Any questions, please contact us: product.firlake@gmail.com
We will reply you within 24 hours and provide you with the best solution
THIS SIDE MUST FACE UP
FACE TOWARDS THE BED'S EXIT SIDE

正面

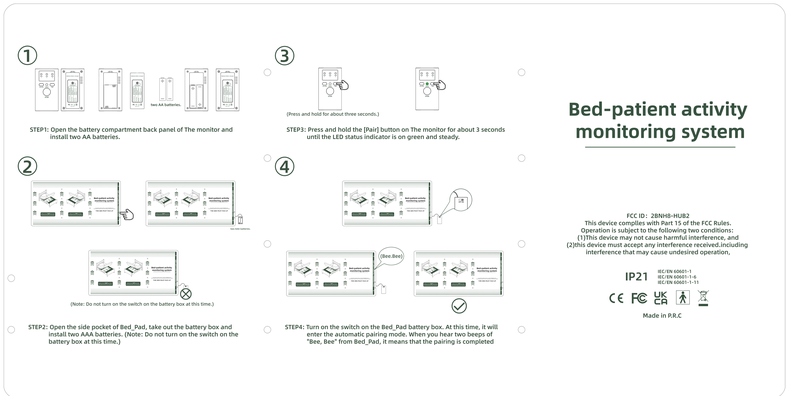
①
Two AA batteries.
STEP1: Open the battery compartment back panel of The monitor and install two AA batteries.
②
Two AAA batteries.
(Note: Do not turn on the switch on the battery box at this time.)
STEP2: Open the side pocket of Bed_Pad, take out the battery box and install two AAA batteries. (Note: Do not turn on the switch on the battery box at this time.)
③
(Press and hold for about three seconds.)
STEP3: Press and hold the [Pair] button on The monitor for about 3 seconds until the LED status indicator is on green and steady.
④
(Bee.Bee)
STEP4: Turn on the switch on the Bed_Pad battery box. At this time, it will enter the automatic pairing mode. When you hear two beeps of "Bee, Bee" from Bed_Pad, it means that the pairing is completed
Bed-patient activity monitoring system
FCC ID: 2BNHB-HUB2
This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1)This device may not cause harmful interference, and
(2)this device must accept any interference received.including interference that may cause undesired operation.
IP21
IEC/EN 60601-1
IEC/EN 60601-1-6
IEC/EN 60601-1-11
Made in P.R.C

背面