

**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D2450V2-806\_Mar25****CALIBRATION CERTIFICATE**Object **D2450V2 - SN: 806**Calibration procedure(s) **QA CAL-05.v12  
Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz**Calibration date **March 13, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature

Issued: March 14, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |                                     |
|-------------------------------------|--------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR         | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation   |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom     |                                     |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 5mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| <b>Frequency</b>                    | 2450MHz $\pm$ 1MHz       |                                     |

## HSL parameters at 2450 MHz

The following parameters and calculations were applied:

|                                           | Temperature         | Permittivity  | Conductivity        |
|-------------------------------------------|---------------------|---------------|---------------------|
| <b>Nominal HSL parameters</b>             | 22.0 °C             | 39.2          | 1.80 mho/m          |
| <b>Measured HSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 37.9 $\pm$ 6% | 1.86 mho/m $\pm$ 6% |
| <b>HSL temperature change during test</b> | < 0.5 °C            |               |                     |

## SAR result with HSL at 2450 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of HSL</b> | Condition          |                               |
|--------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                         | 24 dBm input power | 13.3 W/kg                     |
| SAR for nominal HSL parameters                         | normalized to 1W   | 52.9 W/kg $\pm$ 17.0% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of HSL</b> | Condition          |                               |
|----------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                           | 24 dBm input power | 6.21 W/kg                     |
| SAR for nominal HSL parameters                           | normalized to 1W   | 24.7 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 2450 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 55.5 $\Omega$ + 3.3 j $\Omega$ |
| Return Loss | -24.4 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.162 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole          | Frequency [MHz] | TSL | Power [dBm] |
|-----------------|-----------------|-----|-------------|
| D2450V2 - SN806 | 2450            | HSL | -24         |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0---   | 2450, 0                         | 7.06              | 1.86                   | 37.9             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-03-13    | EX3DV4 - SN7349, 2025-01-10 | DAE4lp Sn1836, 2024-10-28 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 30 x 30 x 30    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.5 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS - 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-03-13          |
| psSAR1g [W/Kg]      | 13.3                |
| psSAR10g [W/Kg]     | 6.21                |
| Power Drift [dB]    | 0.01                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

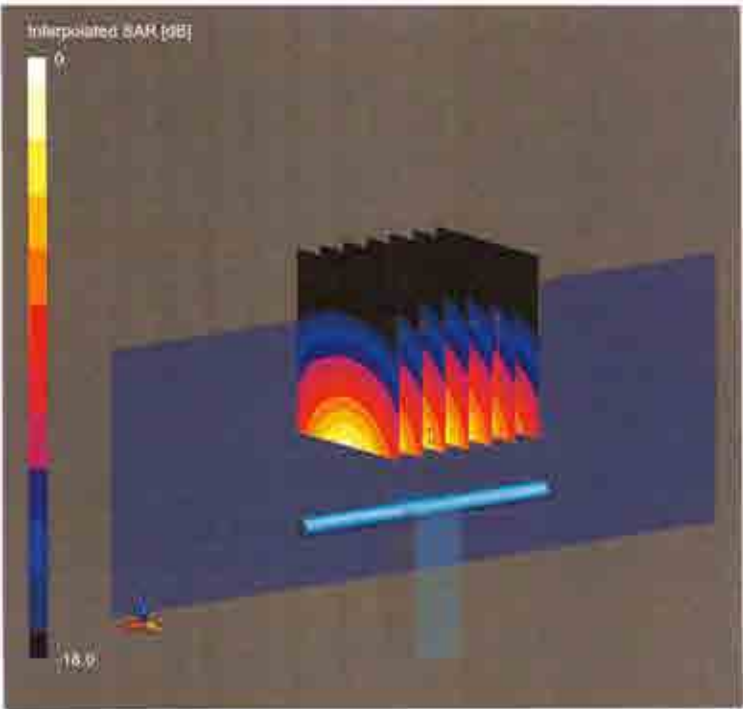

0 dB = 27.7 W/Kg

## Impedance Measurement Plot for HSL

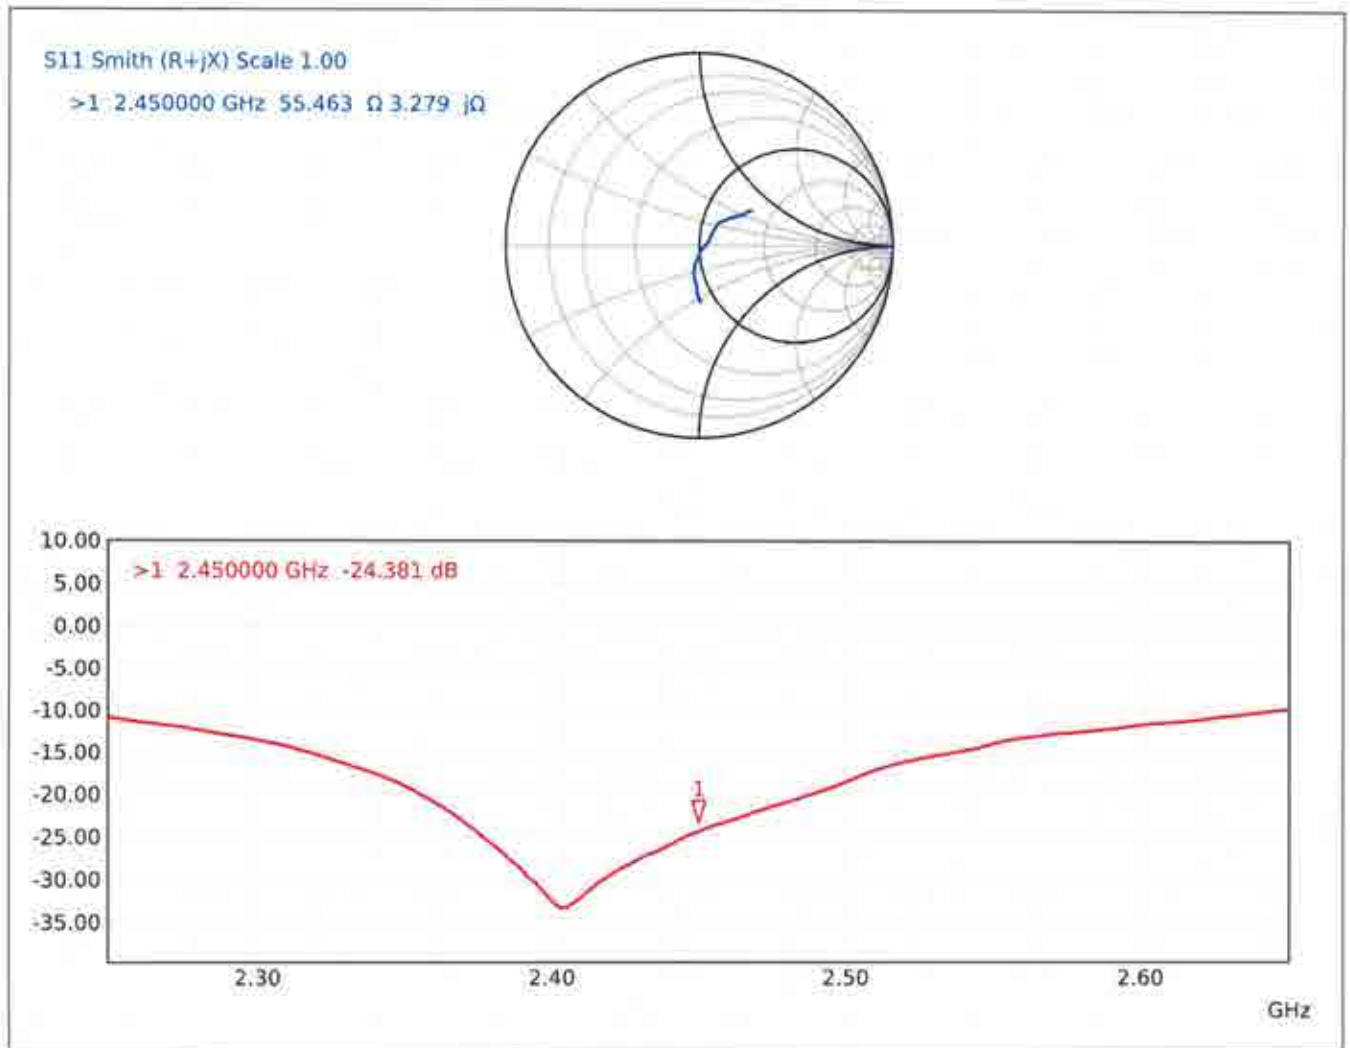

## D2450V2, serial no. 806 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.



### <Justification of the extended calibration>

| D2450V2 – serial no. 806    |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
| 2450MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 03.13.2025<br>(Cal. Report) | -24.381          |           | 55.463               |             | 3.279                     |             |
| 03.12.2026<br>(extended)    | -24.502          | 0.496     | 55.343               | -0.12       | 3.2566                    | -0.0224     |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D2450V2, serial no. 806 (Data of Measurement : 03.12.2026)

2450 MHz - Head

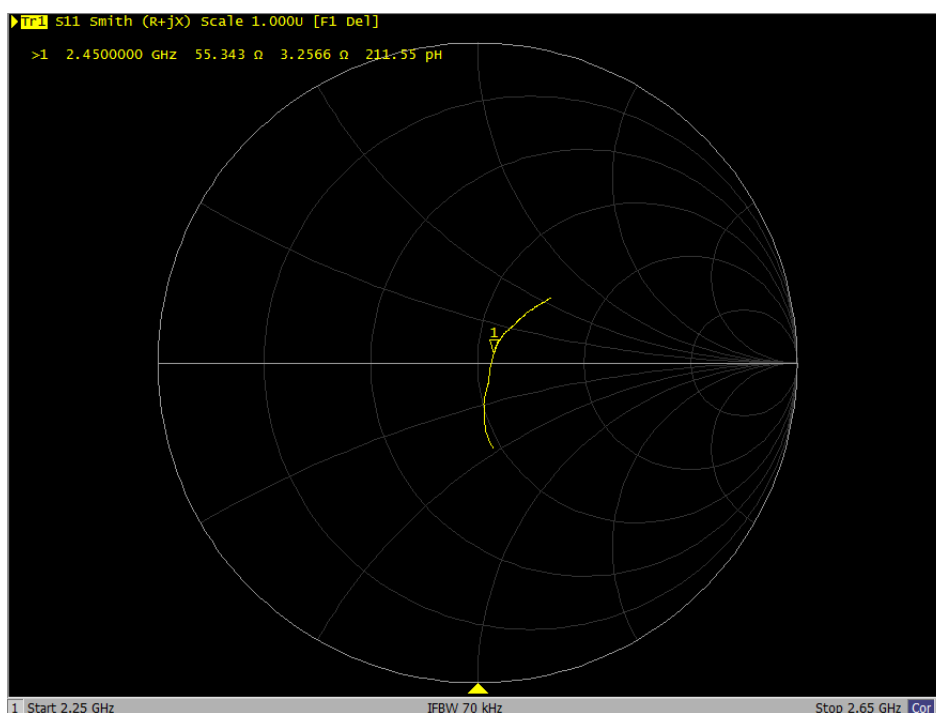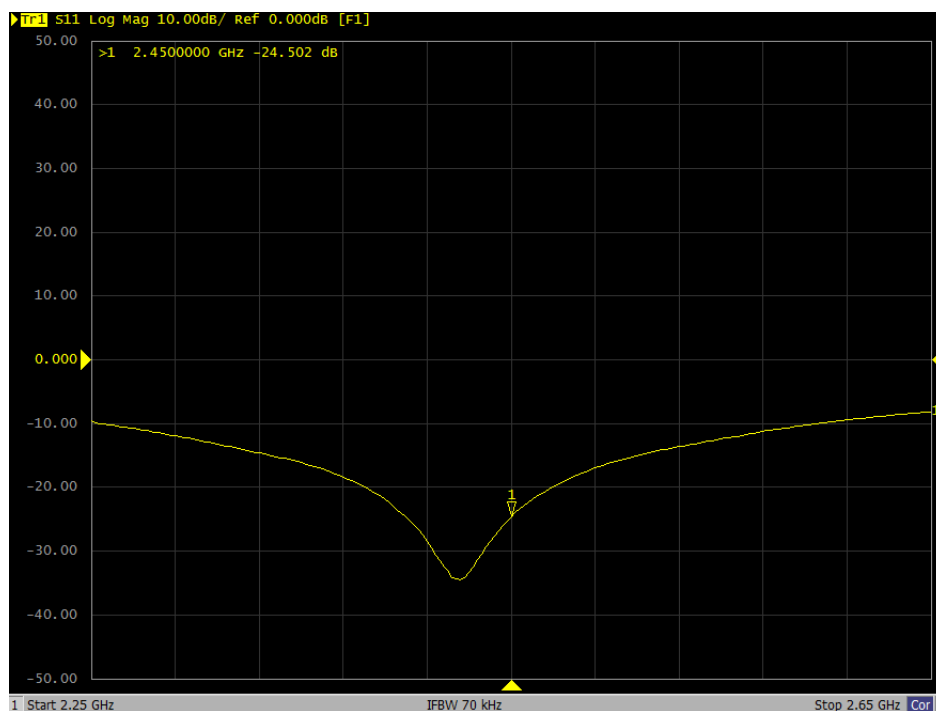



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

Sporton  
Taoyuan City

Certificate No.

D2450V2-929\_Nov25

## CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 929

Calibration procedure(s)

QA CAL-05.v13

Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz

Calibration date

November 12, 2025

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 29-Oct-25 (No. Part of L1407)          | Oct-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 16-Sept-25 (No. OCP-DAK12-1016_Sep25)  | Sep-26        |
| OCP DAK-3.5                 | SN: 1249   | 16-Sept-25 (No. OCP-DAK3.5-1249_Sep25) | Sep-26        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1910   | 11-Mar-25 (No. DAE4ip-1910_Mar25)      | Mar-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch; SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature

Issued: November 12, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |                                     |
|------------------------------|--------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR         | 17.0.2                              |
| Extrapolation                | Advanced Extrapolation   |                                     |
| Phantom                      | Modular Flat Phantom     |                                     |
| Distance Dipole Center - TSL | 10 mm                    | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 5mm, dz = 1.5mm | Graded Ratio = 1.5 mm (Z direction) |
| Frequency                    | 2450MHz $\pm$ 1MHz       |                                     |

## HSL parameters at 2450 MHz

The following parameters and calculations were applied.

|                                    | Temperature         | Permittivity  | Conductivity        |
|------------------------------------|---------------------|---------------|---------------------|
| Nominal HSL parameters             | 22.0 °C             | 39.2          | 1.80 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2) °C | 38.3 $\pm$ 6% | 1.87 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C            |               |                     |

## SAR result with HSL at 2450 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 24 dBm input power | 13.4 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 53.3 W/kg $\pm$ 17.0% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 24 dBm input power | 6.32 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 25.2 W/kg $\pm$ 16.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 2450 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.9 $\Omega$ + 3.4 j $\Omega$ |
| Return Loss | -27.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1,162 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole          | Frequency (MHz) | TSL | Power (dBm) |
|-----------------|-----------------|-----|-------------|
| D2450V2 - SN929 | 2450            | HSL | 24          |

Exposure Conditions

| Phantom Section, TSL | Test Distance (mm) | Band | Group, UID | Frequency (MHz), Channel Number | Conversion Factor | TSL Conductivity (S/m) | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 |      | CW, 0---   | 2450, 0                         | 7.06              | 1.87                   | 38.3             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-11-12    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1910, 2025-03-11 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents (mm)   | 30 x 30 x 30    |
| Grid Steps (mm)     | 5.0 x 5.0 x 1.5 |
| Sensor Surface (mm) | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS = 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-11-12          |
| psSAR1g (W/Kg)      | 13.4                |
| psSAR10g (W/Kg)     | 6.32                |
| Power Drift (dB)    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor (dB) |                     |
| TSL Correction      | Positive / Negative |

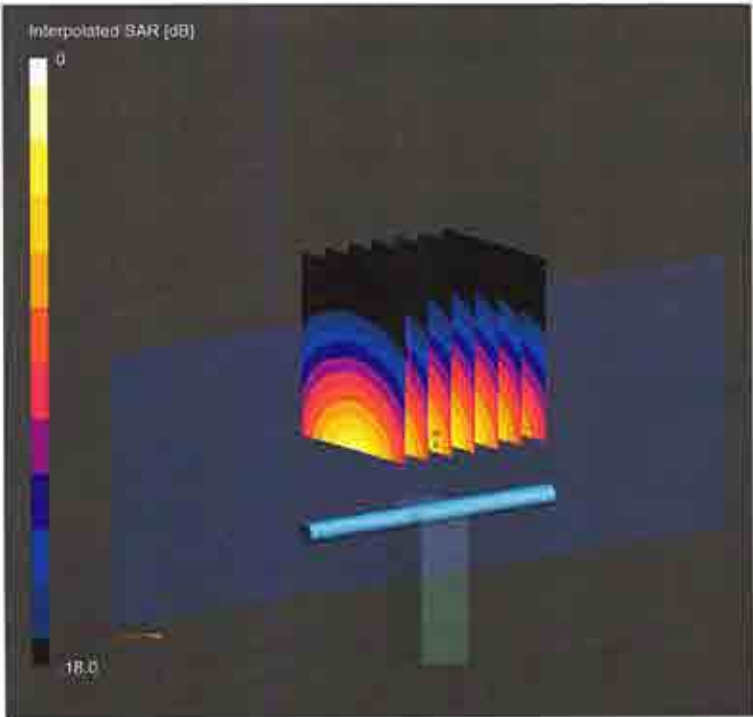

0 dB = 27.2 W/Kg

Impedance Measurement Plot for HSL

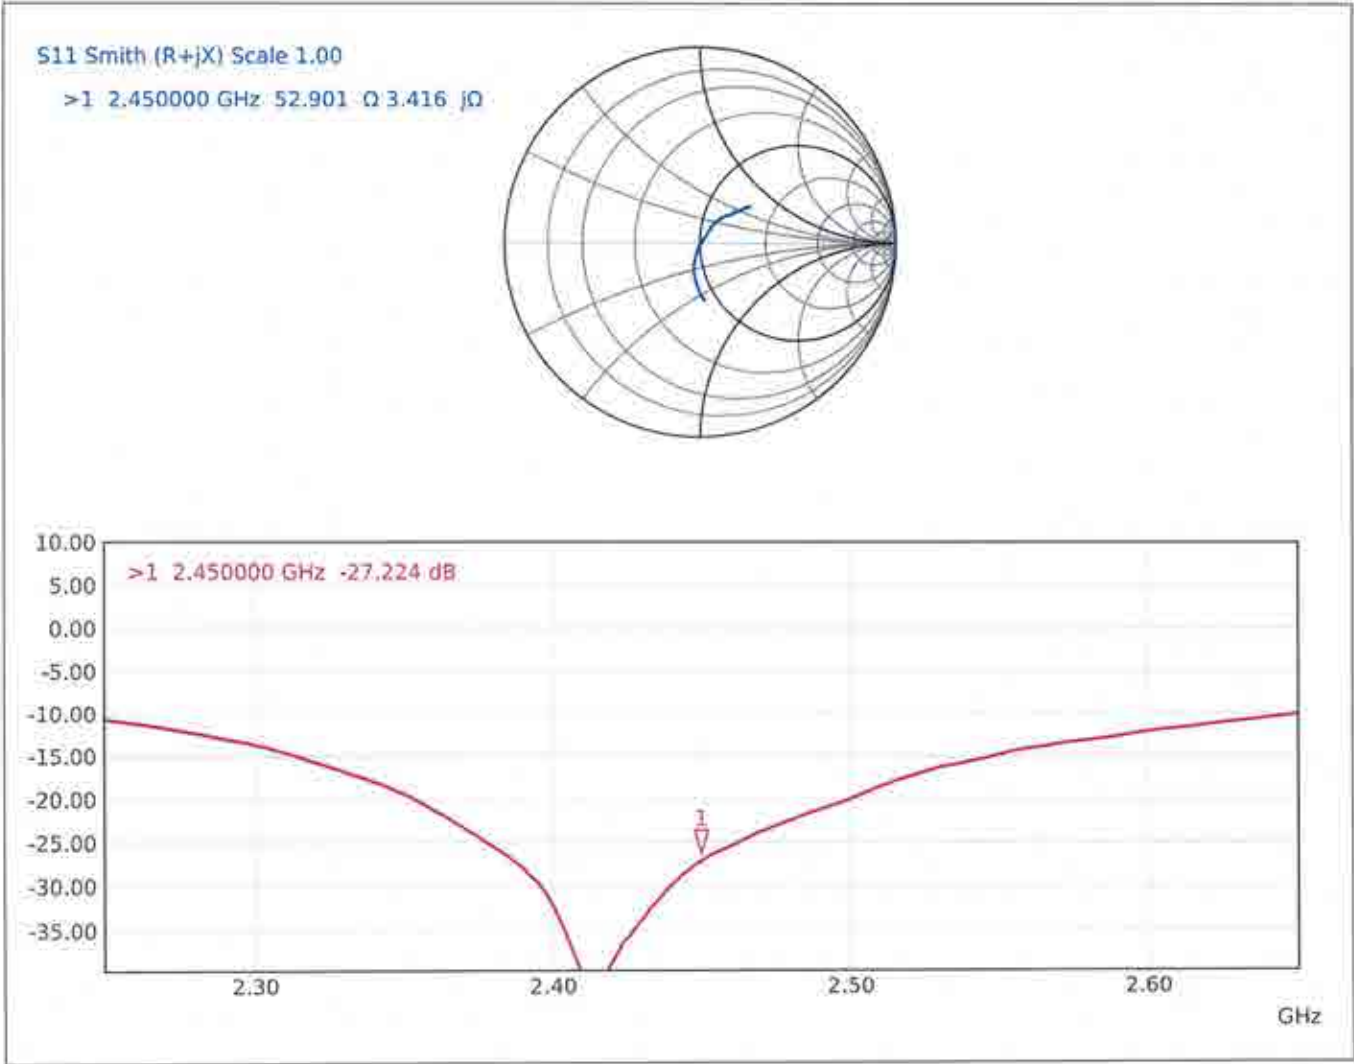

**Calibration Laboratory of****Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland

**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**D6.5GHzV2-1083\_Oct25****CALIBRATION CERTIFICATE**

Object

**D6.5GHzV2 - SN: 1083**

Calibration procedure(s)

**QA CAL-22.v8****Calibration Procedure for SAR Validation Sources between 3 - 10 GHz**

Calibration date

**October 22, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|-----------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 30-Apr-25 (No. 1020-300791789)         | Apr-26        |
| Power Sensor R&S NRP18A     | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40 | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| 3.5mm mismatch combination  | SN: 1152   | 24-Mar-25 (No. 217-04293)              | Mar-26        |
| OCP DAK-12                  | SN: 1016   | 16-Sept-25 (No. OCP-DAK12-1016_Sep25)  | Sep-26        |
| OCP DAK-3.5                 | SN: 1249   | 16-Sept-25 (No. OCP-DAK3.5-1249_Sep25) | Sep-26        |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                      | SN: 1836   | 04-Sept-25 (No. DAE4ip-1836_Sep25)     | Sep-26        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Setup 1                 | SN: 1000   | 27-May-25 (No. 675-ACAD_Source_Box-250527) | May-26          |
| Signal Generator R&S SMB100A | SN: 182081 | 27-May-25 (No. 675-CAL16-S4588-250527)     | May-26          |
| Mismatch; SMA                | SN: 1102   | 24-Apr-25 (No. 675-Mismatch_SMA-250424)    | Apr-26          |
| OCP DAK-12                   | SN: 1029   | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)       | Feb-26          |
| OCP DAK-3.5                  | SN: 1336   | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)      | Dec-25          |

|                                                                                                                 | Name       | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|------------|-----------------------|-----------|
| Calibrated by                                                                                                   | Paulo Pina | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn  | Technical Manager     |           |
| Issued: October 22, 2025                                                                                        |            |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |            |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                            |                                     |
|------------------------------|----------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR           | 17.0.2                              |
| Extrapolation                | Advanced Extrapolation     |                                     |
| Phantom                      | Modular Flat Phantom       |                                     |
| Distance Dipole Center - TSL | 5 mm                       | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 3.4mm, dz = 1.4mm | Graded Ratio = 1.4 mm (Z direction) |
| Frequency                    | 6500MHz $\pm$ 1MHz         |                                     |

## HSL parameters at 6500 MHz

The following parameters and calculations were applied.

|                                    | Temperature        | Permittivity  | Conductivity        |
|------------------------------------|--------------------|---------------|---------------------|
| Nominal HSL parameters             | 22.0 °C            | 34.5          | 6.07 mho/m          |
| Measured HSL parameters            | (22.0 $\pm$ 0.2)°C | 34.9 $\pm$ 6% | 6.22 mho/m $\pm$ 6% |
| HSL temperature change during test | < 0.5 °C           |               |                     |

## SAR result with HSL at 6500 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of HSL | Condition          |                              |
|--------------------------------------------------|--------------------|------------------------------|
| SAR for nominal HSL parameters                   | 20 dBm input power | 30.2 W/kg                    |
| SAR for nominal HSL parameters                   | normalized to 1W   | 302 W/kg $\pm$ 24.7% (k = 2) |

| SAR averaged over 8 cm <sup>3</sup> (8 g) of HSL | Condition          |                               |
|--------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                   | 20 dBm input power | 6.84 W/kg                     |
| SAR for nominal HSL parameters                   | normalized to 1W   | 68.4 W/kg $\pm$ 24.4% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of HSL | Condition          |                               |
|----------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal HSL parameters                     | 20 dBm input power | 5.65 W/kg                     |
| SAR for nominal HSL parameters                     | normalized to 1W   | 56.5 W/kg $\pm$ 24.4% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with HSL at 6500 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 49.6 $\Omega$ – 2.2 j $\Omega$ |
| Return Loss | -32.8 dB                       |

**APD (Absorbed Power Density)**

| APD averaged over 1 cm <sup>3</sup> | Condition          |                               |
|-------------------------------------|--------------------|-------------------------------|
| APD measured                        | 20 dBm input power | 302 W/kg                      |
| APD measured                        | normalized to 1W   | 3020 W/kg $\pm$ 29.2% (k = 2) |

| APD averaged over 4 cm <sup>3</sup> | Condition          |                               |
|-------------------------------------|--------------------|-------------------------------|
| APD measured                        | 20 dBm input power | 137 W/kg                      |
| APD measured                        | normalized to 1W   | 1370 W/kg $\pm$ 28.9% (k = 2) |

\*The reported APD values have been derived using the psSAR1g and psSAR8g.

**General Antenna Parameters and Design**

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole             | Frequency [MHz] | TSL | Power [dBm] |
|--------------------|-----------------|-----|-------------|
| D6.5GHzV2 - SN1083 | 6500            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band     | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|----------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 5                  | CW, 0--- |            | 6500, 0                         | 5.49              | 6.22                   | 34.9             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2025-10-22    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2025-09-04 |

Scans Setup


|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 3.4 x 3.4 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2025-10-22          |
| psSAR1g [W/Kg]      | 30.2                |
| psSAR10g [W/Kg]     | 5.65                |
| Power Drift [dB]    | -0.01               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

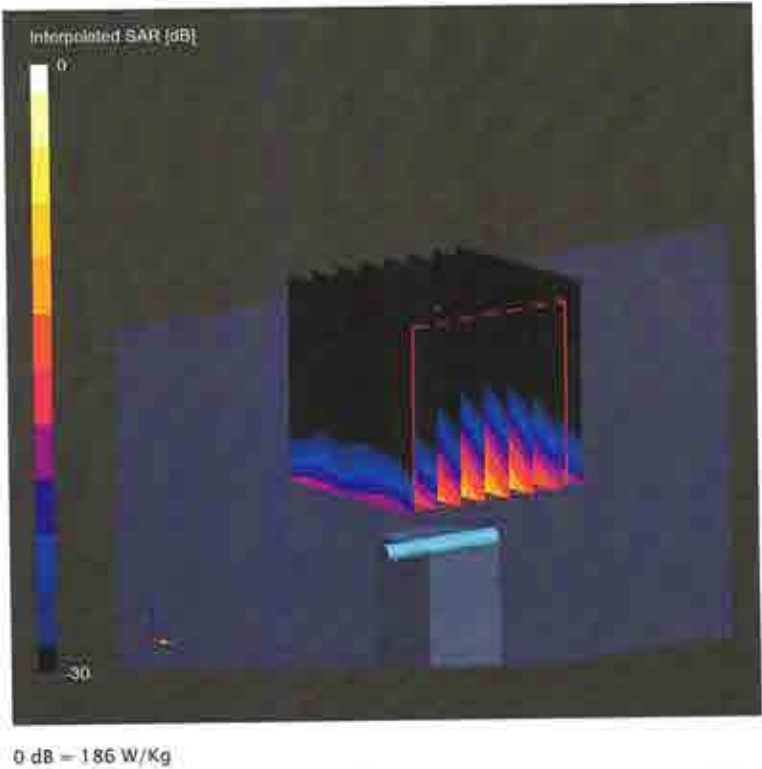

Impedance Measurement Plot for HSL

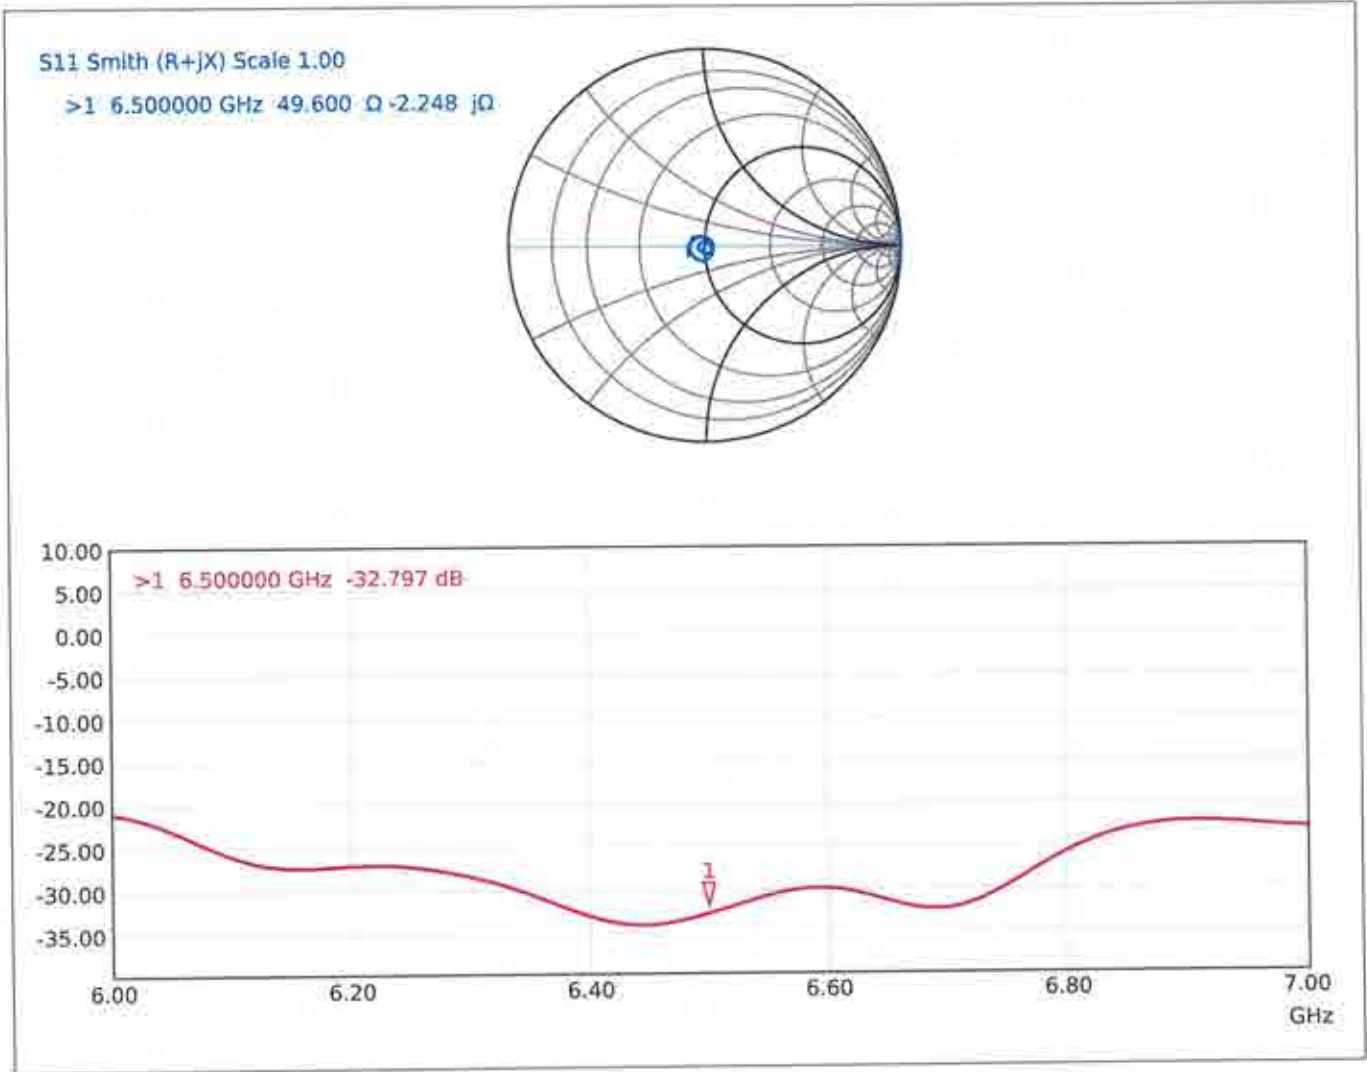



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **Sporton**  
**Taoyuan City**

Certificate No. **D5GHzV2-1171\_Apr24**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1171**

Calibration procedure(s) **QA CAL-22.v7**  
**Calibration Procedure for SAR Validation Sources between 3-10 GHz**

Calibration date: **April 19, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards               | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|---------------------------------|--------------------|-----------------------------------|------------------------|
| Power meter NRP2                | SN: 104778         | 26-Mar-24 (No. 217-04036/04037)   | Mar-25                 |
| Power sensor NRP-Z91            | SN: 103244         | 26-Mar-24 (No. 217-04036)         | Mar-25                 |
| Power sensor NRP-Z91            | SN: 103245         | 26-Mar-24 (No. 217-04037)         | Mar-25                 |
| Reference 20 dB Attenuator      | SN: BH9394 (20k)   | 26-Mar-24 (No. 217-04046)         | Mar-25                 |
| Type-N mismatch combination     | SN: 310982 / 06327 | 26-Mar-24 (No. 217-04047)         | Mar-25                 |
| Reference Probe EX3DV4          | SN: 3503           | 07-Mar-24 (No. EX3-3503_Mar24)    | Mar-25                 |
| DAE4                            | SN: 601            | 30-Jan-24 (No. DAE4-601_Jan24)    | Jan-25                 |
| Secondary Standards             | ID #               | Check Date (in house)             | Scheduled Check        |
| Power meter E4419B              | SN: GB39512475     | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: US37292783     | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A           | SN: MY41093315     | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06         | SN: 100972         | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477     | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

Calibrated by: **Paulo Pina**      Function: **Laboratory Technician**      Signature:

Approved by: **Sven Kühn**      Technical Manager      Signature:

Issued: April 23, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- DASY System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                                                                                              |                                  |
|------------------------------|----------------------------------------------------------------------------------------------|----------------------------------|
| DASY Version                 | DASY52                                                                                       | V52.10.4                         |
| Extrapolation                | Advanced Extrapolation                                                                       |                                  |
| Phantom                      | Modular Flat Phantom V5.0                                                                    |                                  |
| Distance Dipole Center - TSL | 10 mm                                                                                        | with Spacer                      |
| Zoom Scan Resolution         | $dx, dy = 4.0 \text{ mm}$ , $dz = 1.4 \text{ mm}$                                            | Graded Ratio = 1.4 (Z direction) |
| Frequency                    | 5250 MHz $\pm 1 \text{ MHz}$<br>5600 MHz $\pm 1 \text{ MHz}$<br>5800 MHz $\pm 1 \text{ MHz}$ |                                  |

## Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

|                                         | Temperature                 | Permittivity    | Conductivity                  |
|-----------------------------------------|-----------------------------|-----------------|-------------------------------|
| Nominal Head TSL parameters             | 22.0 °C                     | 35.9            | 4.71 mho/m                    |
| Measured Head TSL parameters            | $(22.0 \pm 0.2) \text{ °C}$ | $37.1 \pm 6 \%$ | $4.65 \text{ mho/m} \pm 6 \%$ |
| Head TSL temperature change during test | $< 0.5 \text{ °C}$          | ----            | ----                          |

## SAR result with Head TSL at 5250 MHz

|                                                       |                    |                                                 |
|-------------------------------------------------------|--------------------|-------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                                 |
| SAR measured                                          | 100 mW input power | 7.82 W/kg                                       |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | <b>78.7 W/kg <math>\pm 19.9 \%</math> (k=2)</b> |

|                                                         |                    |                                                 |
|---------------------------------------------------------|--------------------|-------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                                 |
| SAR measured                                            | 100 mW input power | 2.25 W/kg                                       |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | <b>22.7 W/kg <math>\pm 19.5 \%</math> (k=2)</b> |

## Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature                 | Permittivity    | Conductivity                  |
|-----------------------------------------|-----------------------------|-----------------|-------------------------------|
| Nominal Head TSL parameters             | 22.0 °C                     | 35.5            | 5.07 mho/m                    |
| Measured Head TSL parameters            | $(22.0 \pm 0.2) \text{ °C}$ | $36.5 \pm 6 \%$ | $5.05 \text{ mho/m} \pm 6 \%$ |
| Head TSL temperature change during test | $< 0.5 \text{ °C}$          | ----            | ----                          |

## SAR result with Head TSL at 5600 MHz

|                                                       |                    |                                                 |
|-------------------------------------------------------|--------------------|-------------------------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                                 |
| SAR measured                                          | 100 mW input power | 8.10 W/kg                                       |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | <b>81.4 W/kg <math>\pm 19.9 \%</math> (k=2)</b> |

|                                                         |                    |                                                 |
|---------------------------------------------------------|--------------------|-------------------------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                                 |
| SAR measured                                            | 100 mW input power | 2.32 W/kg                                       |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | <b>23.4 W/kg <math>\pm 19.5 \%</math> (k=2)</b> |

## Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.3         | 5.27 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 36.2 ± 6 %   | 5.27 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ----         | ----             |

## SAR result with Head TSL at 5800 MHz

|                                                             |                    |                                 |
|-------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                | 100 mW input power | 7.85 W/kg                       |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | <b>78.9 W/kg ± 19.9 % (k=2)</b> |

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.23 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.4 W/kg ± 19.5 % (k=2)</b> |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL at 5250 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 47.4 $\Omega$ - 7.3 j $\Omega$ |
| Return Loss                          | - 22.0 dB                      |

### Antenna Parameters with Head TSL at 5600 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.9 $\Omega$ - 3.4 j $\Omega$ |
| Return Loss                          | - 26.0 dB                      |

### Antenna Parameters with Head TSL at 5800 MHz

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 54.6 $\Omega$ - 5.6 j $\Omega$ |
| Return Loss                          | - 23.2 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1,206 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1171**

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz

Frequency: 5800 MHz

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.65$  S/m;  $\epsilon_r = 37.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5.05$  S/m;  $\epsilon_r = 36.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.27$  S/m;  $\epsilon_r = 36.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.39, 5.39, 5.39) @ 5250 MHz, ConvF(5, 5, 5) @ 5600 MHz, ConvF(4.86, 4.86, 4.86) @ 5800 MHz; Calibrated: 07.03.2024
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2024
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.37 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 26.3 W/kg

**SAR(1 g) = 7.82 W/kg; SAR(10 g) = 2.25 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 71.3%

Maximum value of SAR (measured) = 17.9 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 72.14 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 29.8 W/kg

**SAR(1 g) = 8.10 W/kg; SAR(10 g) = 2.32 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 68.4%

Maximum value of SAR (measured) = 19.3 W/kg

**Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 70.59 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 30.6 W/kg

**SAR(1 g) = 7.85 W/kg; SAR(10 g) = 2.23 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.5 mm


Ratio of SAR at M2 to SAR at M1 = 66.5%

Maximum value of SAR (measured) = 18.9 W/kg



0 dB = 19.3 W/kg = 12.85 dBW/kg

Impedance Measurement Plot for Head TSL

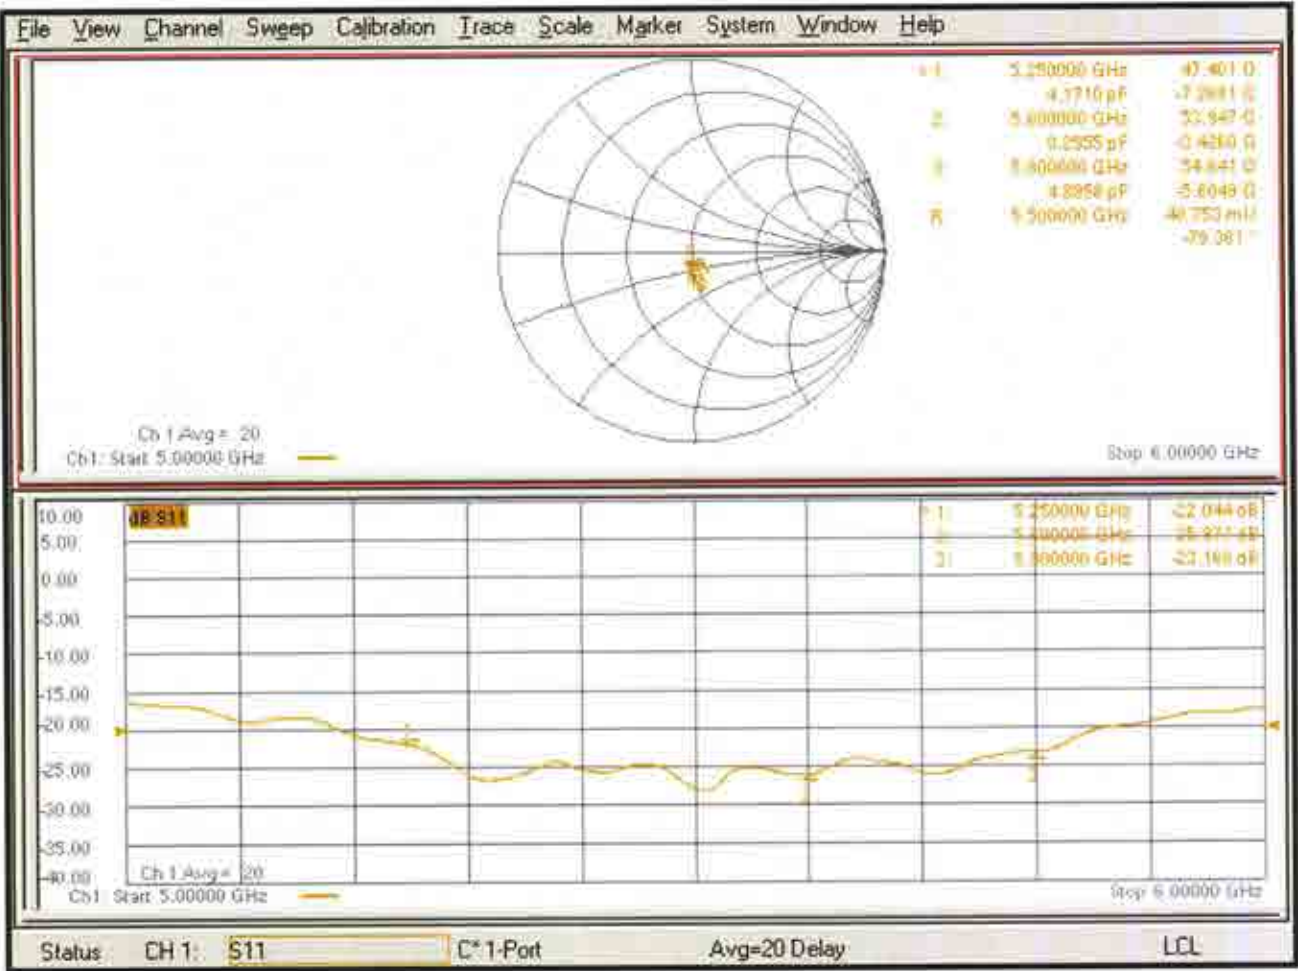

## D5000HzV2, serial no. 1171 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D5000HzV2 – serial no. 1171 |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
| 5250MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 04.19.2024<br>(Cal. Report) | -22.044          |           | 47.401               |             | -7.2681                   |             |
| 04.18.2025<br>(extended)    | -20.138          | 8.646     | 50.939               | 3.538       | -6.2738                   | 0.9943      |
| 04.17.2026<br>(extended)    | -19.602          | 11.078    | 47.593               | 0.192       | -9.1251                   | -1.8570     |
| 5600MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 04.19.2024<br>(Cal. Report) | -25.977          |           | 53.947               |             | -3.4260                   |             |
| 04.18.2025<br>(extended)    | -26.020          | 0.166     | 54.248               | 0.301       | -3.9386                   | -0.5126     |
| 04.17.2026<br>(extended)    | -24.011          | 7.568     | 52.728               | -1.219      | -6.9900                   | -3.5640     |
| 5800MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 04.19.2024<br>(Cal. Report) | -23.168          |           | 54.641               |             | -5.6049                   |             |
| 04.18.2025<br>(extended)    | -23.371          | 0.876     | 51.231               | -3.410      | -6.1356                   | -0.5307     |
| 04.17.2026<br>(extended)    | -23.459          | 1.256     | 56.126               | 1.485       | -4.0473                   | 1.5576      |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.


<Dipole Verification Data> - D5000 V2, serial no. 1171 (Data of Measurement : 04.18.2025)

5000 MHz - Head

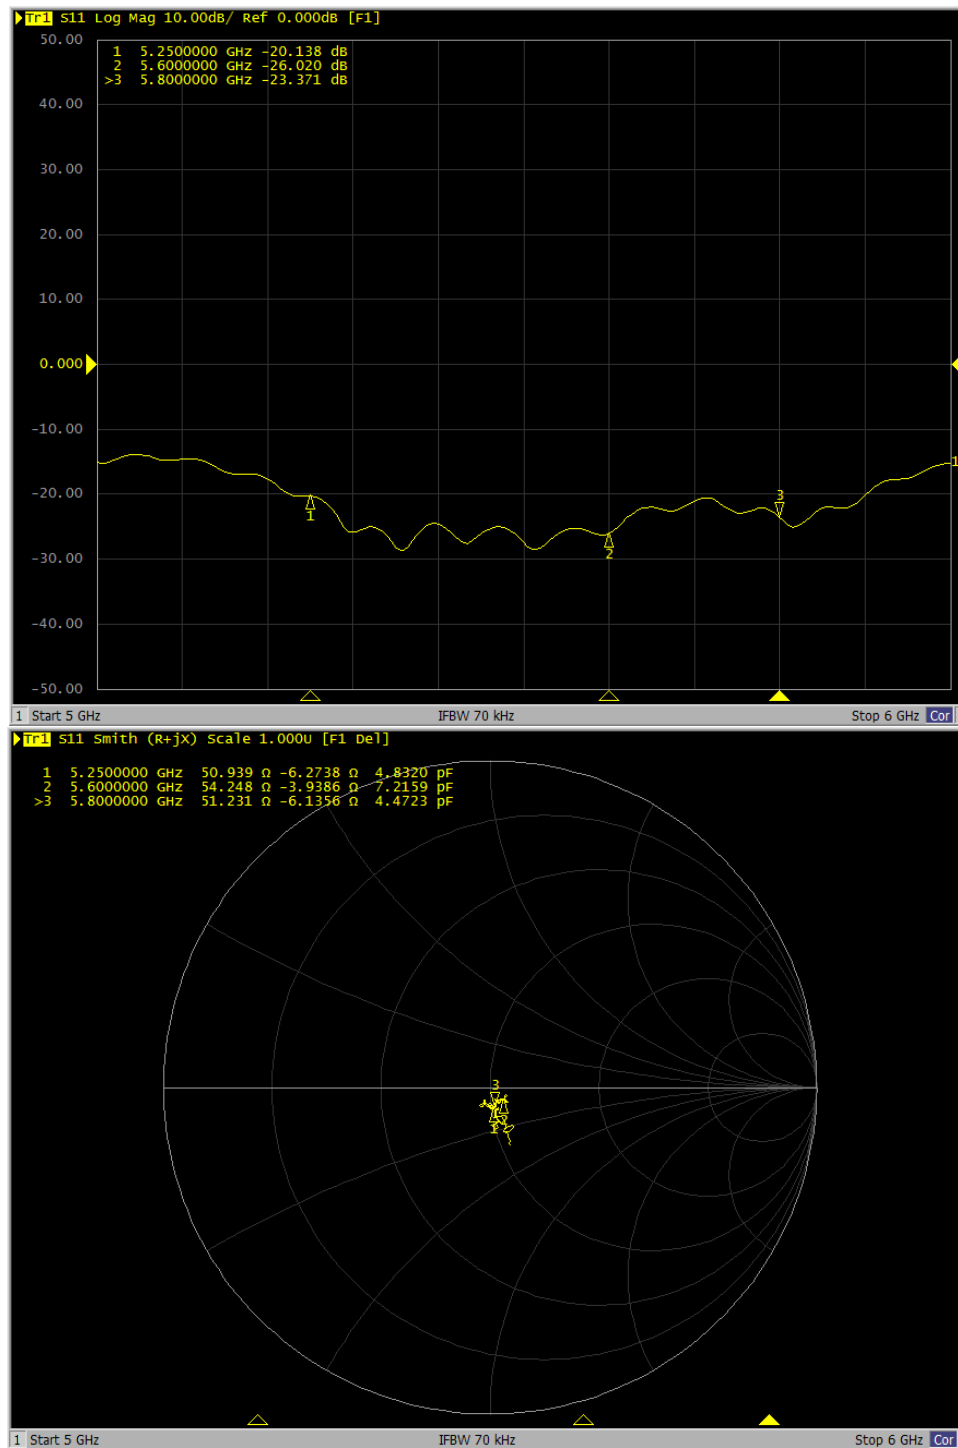

<Dipole Verification Data> - D5000 V2, serial no. 1171 (Data of Measurement : 04.17.2026)

5000 MHz - Head

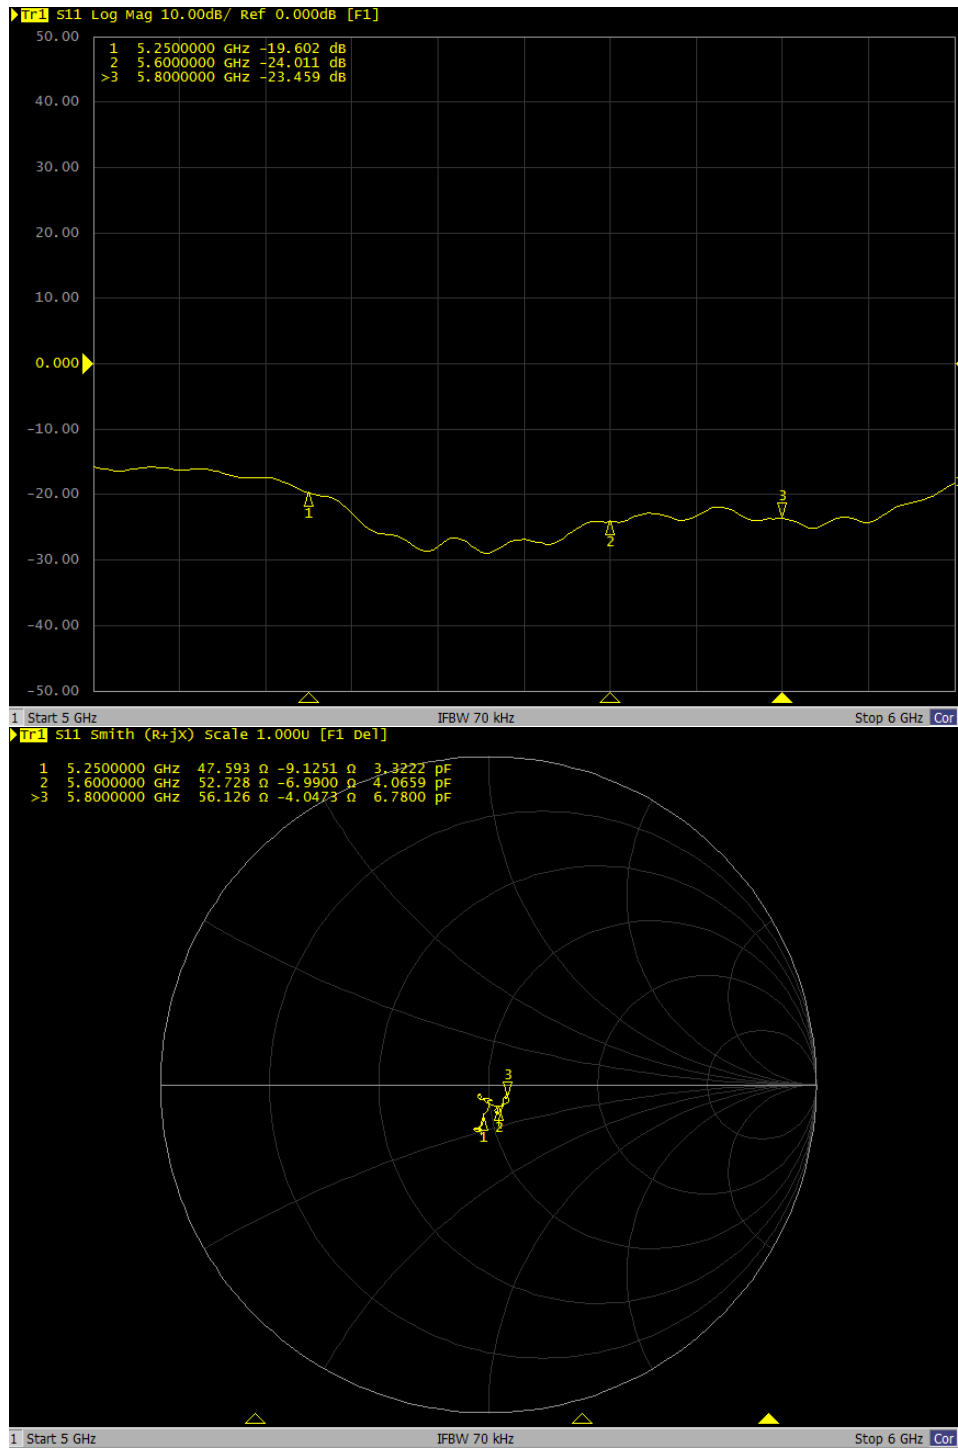

# Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

**Sporton**

Taoyuan City

Certificate No.

**D5GHzV2-1006\_Oct24**

## CALIBRATION CERTIFICATE

Object

D5GHzV2 - SN: 1006

Calibration procedure(s)

QA CAL-22.v7

Calibration Procedure for SAR Validation Sources between 3 - 10 GHz

Calibration date

October 15, 2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)            | Scheduled Cal |
|--------------------------------------------|------------|---------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)             | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 22-Jul-24 (No. 4030A315008547)        | Jul-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)        | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)             | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sep-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sep-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 03-Jun-24 (No. EX3-7349_Jun24)        | Jun-25        |
| DAE4ip                                     | SN: 1836   | 10-Jan-24 (No. DAE4ip-1836_Jan24)     | Jan-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|                                                                                                                 |            |                       |           |
|-----------------------------------------------------------------------------------------------------------------|------------|-----------------------|-----------|
|                                                                                                                 | Name       | Function              | Signature |
| Calibrated by                                                                                                   | Paulo Pina | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn  | Technical Manager     |           |
| Issued: October 15, 2024                                                                                        |            |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |            |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                                                 |                                     |
|------------------------------|-------------------------------------------------|-------------------------------------|
| DASY Version                 | DASY8 Module SAR                                | 16.4.0                              |
| Extrapolation                | Advanced Extrapolation                          |                                     |
| Phantom                      | Modular Flat Phantom                            |                                     |
| Distance Dipole Center - TSL | 10 mm                                           | with spacer                         |
| Zoom Scan Resolution         | dx, dy = 4mm, dz = 1.4mm                        | Graded Ratio = 1.4 mm (Z direction) |
| Frequency                    | 5250MHz ±1MHz<br>5600MHz ±1MHz<br>5800MHz ±1MHz |                                     |

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

|                                         |               |              |                |
|-----------------------------------------|---------------|--------------|----------------|
|                                         | Temperature   | Permittivity | Conductivity   |
| Nominal Head TSL parameters             | 22.0 °C       | 35.9         | 4.71 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 36.2 ±6%     | 4.64 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

SAR result with Head TSL at 5250 MHz

|                                                       |                    |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.06 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 80.6 W/kg ±19.9% (k = 2) |

|                                                         |                    |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.28 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 22.8 W/kg ±19.5% (k = 2) |

### Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.5         | 5.07 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.8 ±6%     | 5.04 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5600 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.34 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 83.4 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.37 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 23.7 W/kg ±19.5% (k = 2) |

### Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 35.3         | 5.27 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 35.6 ±6%     | 5.21 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

### SAR result with Head TSL at 5800 MHz

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 8.06 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 80.6 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.27 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 22.7 W/kg ±19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL at 5250 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 53.0 $\Omega$ – 5.9 j $\Omega$ |
| Return Loss | -23.8 dB                       |

**Antenna Parameters with Head TSL at 5600 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 57.2 $\Omega$ – 6.3 j $\Omega$ |
| Return Loss | -21.0 dB                       |

**Antenna Parameters with Head TSL at 5800 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 55.5 $\Omega$ + 3.2 j $\Omega$ |
| Return Loss | -24.4 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.201 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1006 | 5250            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 5250, 0                         | 5.58              | 4.64                   | 36.2             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-15    | EX3DV6 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-15          |
| psSAR1g [W/Kg]      | 8.06                |
| psSAR10g [W/Kg]     | 2.28                |
| Power Drift [dB]    | -0.09               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

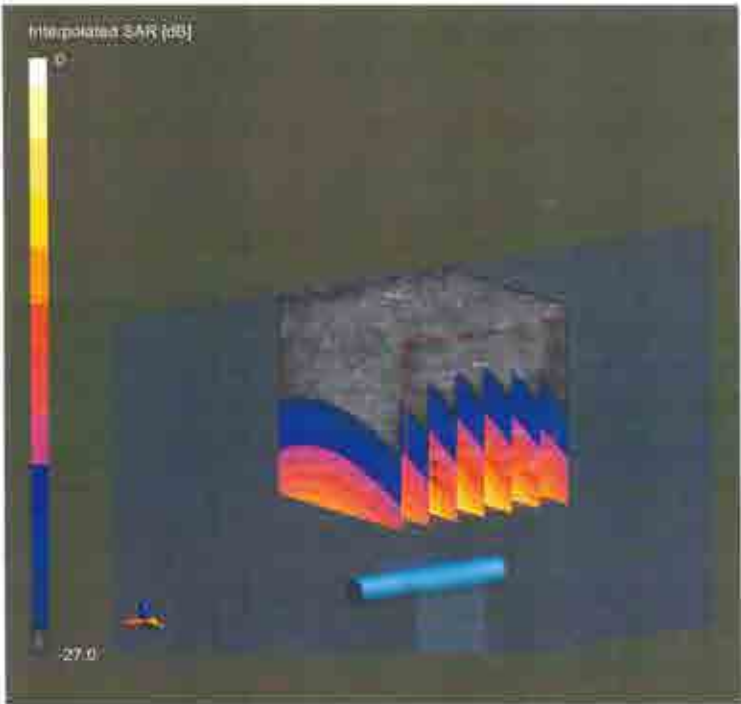

0 dB = 32.5 W/Kg

System Performance Check Report

Summary

| Dipole           | Frequency (MHz) | TSL | Power (dBm) |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1006 | 5600            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance (mm) | Band    | Group, UID | Frequency (MHz), Channel Number | Conversion Factor | TSL Conductivity (S/m) | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 5600, 0                         | 5.03              | 5.04                   | 35.8             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-15    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup

|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents (mm)   | 22 x 22 x 22    |
| Grid Steps (mm)     | 4.0 x 4.0 x 1.4 |
| Sensor Surface (mm) | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-15          |
| psSAR1g (W/Kg)      | 8.34                |
| psSAR10g (W/Kg)     | 2.37                |
| Power Drift (dB)    | -0.02               |
| Power Scaling       | Disabled            |
| Scaling Factor (dB) |                     |
| TSL Correction      | Positive / Negative |

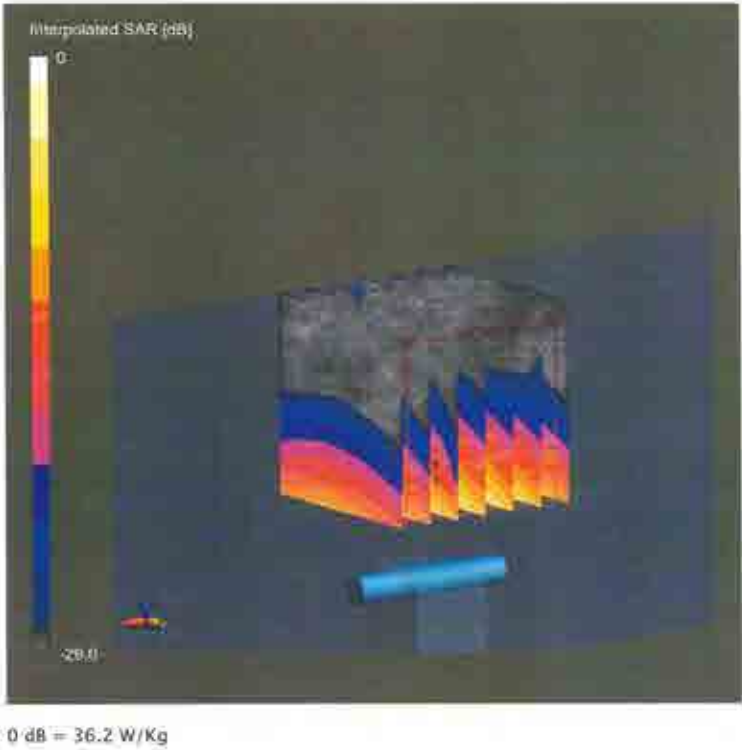

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
|------------------|-----------------|-----|-------------|
| D5GHzV2 - SN1006 | 5800            | HSL | 20          |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat                 | 10                 | CW, 0-- |            | 5800, 0                         | 5.08              | 5.21                   | 35.6             |

Hardware Setup


| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------|--------------------|-----------------------------|---------------------------|
| MFP V8.0 Center | HSL, 2024-10-15    | EX3DV4 - SN7349, 2024-06-03 | DAE4ip Sn1836, 2024-01-10 |

Scans Setup


|                     | Zoom Scan       |
|---------------------|-----------------|
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 4.0 x 4.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     | Zoom Scan           |
|---------------------|---------------------|
| Date                | 2024-10-15          |
| psSAR1g [W/Kg]      | 8.06                |
| psSAR10g [W/Kg]     | 2.27                |
| Power Drift [dB]    | -0.02               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

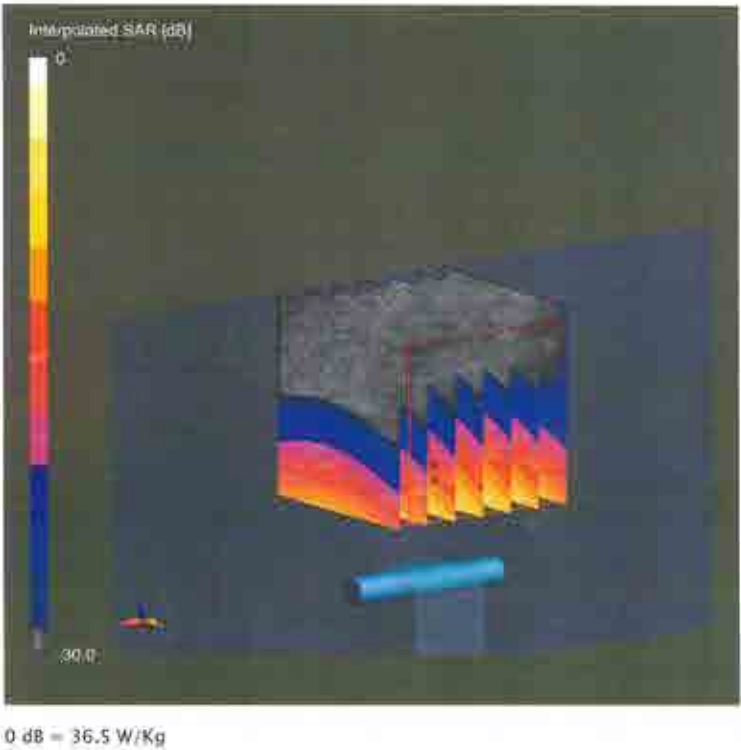

Impedance Measurement Plot for Head TSL

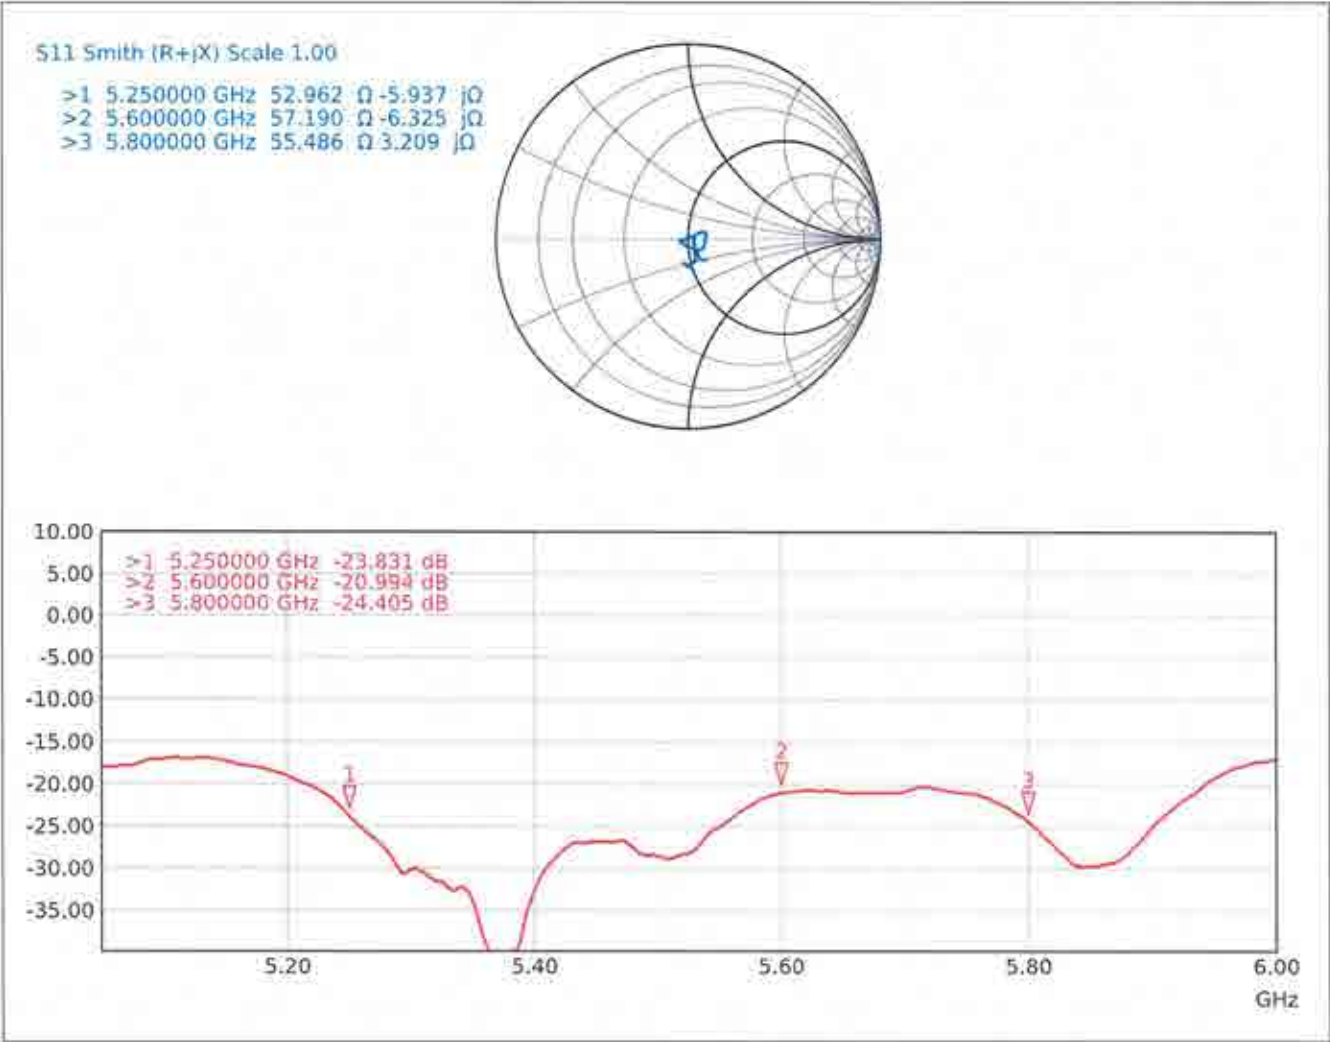

## D5000V2, serial no. 1006 Extended Dipole Calibrations

If dipoles are verified in return loss ( $< -20\text{dB}$ , within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.


### <Justification of the extended calibration>

| D5000V2 – serial no. 1006   |                  |           |                      |             |                           |             |
|-----------------------------|------------------|-----------|----------------------|-------------|---------------------------|-------------|
| 5250MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 10.15.2024<br>(Cal. Report) | -23.831          |           | 52.962               |             | -5.937                    |             |
| 10.14.2025<br>(extended)    | -19.925          | 16.39%    | 57.307               | 4.345       | -9.5184                   | -3.5814     |
| 5600MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 10.15.2024<br>(Cal. Report) | -20.994          |           | 57.190               |             | -6.325                    |             |
| 10.14.2025<br>(extended)    | -18.983          | 9.579%    | 55.998               | -1.192      | -6.4629                   | -0.1379     |
| 5800MHZ                     |                  |           |                      |             |                           |             |
| Date of Measurement         | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (ohm) | Delta (ohm) |
| 10.15.2024<br>(Cal. Report) | -24.405          |           | 55.486               |             | 3.209                     |             |
| 10.14.2025<br>(extended)    | -22.094          | 9.469%    | 55.421               | -0.065      | 6.6866                    | 3.4776      |

The return loss is  $< -20\text{dB}$ , within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data> - D5000V2, serial no. 1006 (Data of Measurement : 10.14.2025)

5000 MHz - Head

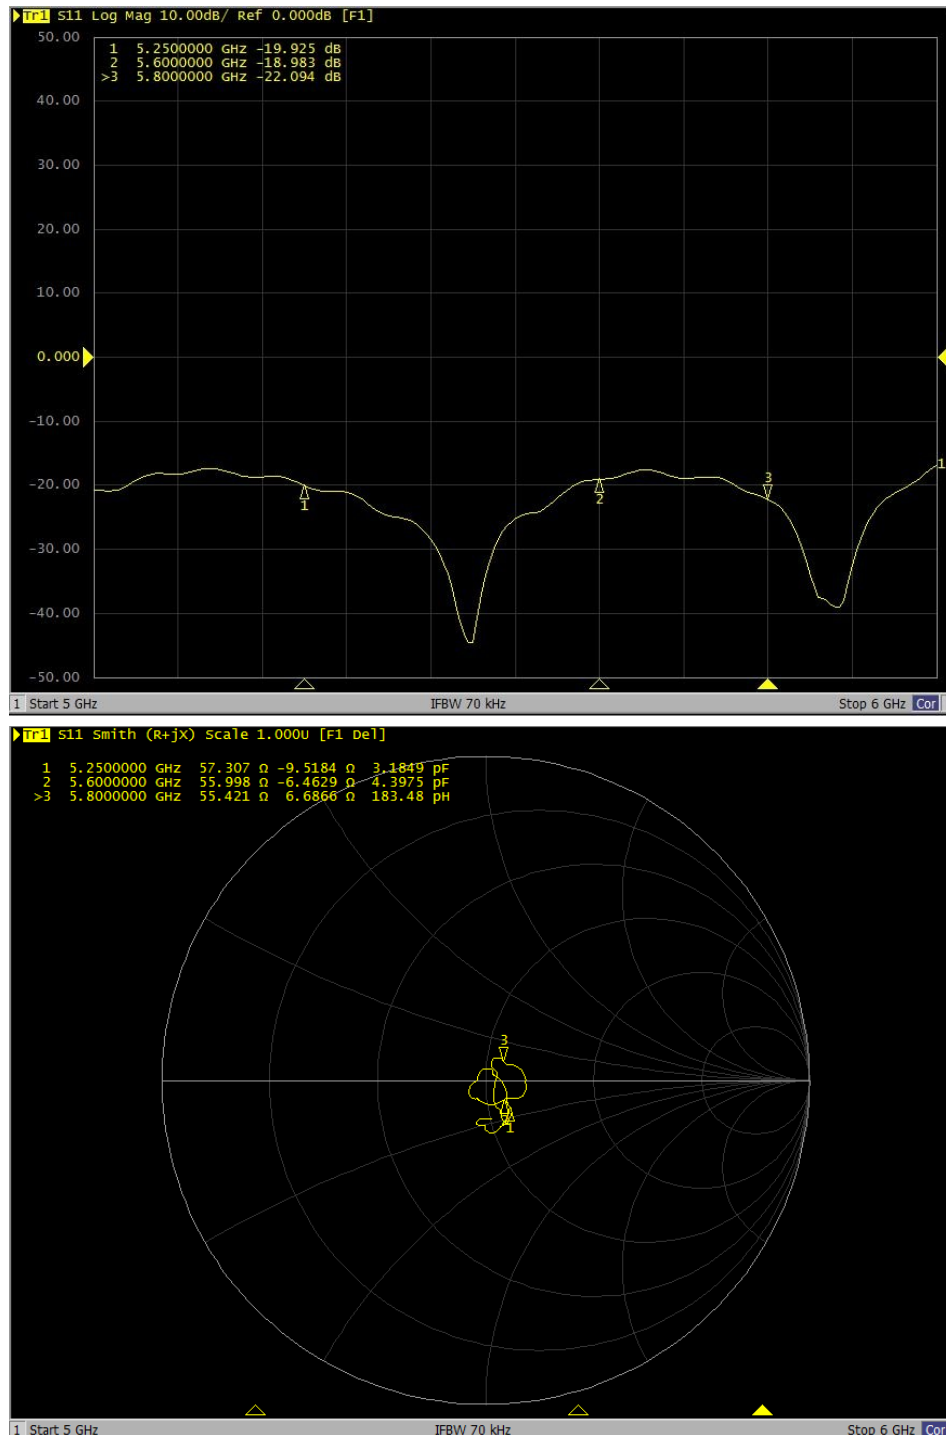



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

Sporton  
Taoyuan City

Certificate No.

5G-Veri10-1052\_Oct25

## CALIBRATION CERTIFICATE

Object 5G Verification Source 10 GHz - SN: 1052

Calibration procedure(s) QA CAL-45.v6  
Calibration procedure for sources in air > 6 GHz

Calibration date October 13, 2025

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID       | Cal Date (Certificate No.)        | Scheduled Cal |
|-------------------------|----------|-----------------------------------|---------------|
| Reference Probe EUMmWV3 | SN: 9374 | 26-Aug-25 (No. Eumm 9374_Aug25)   | Aug-26        |
| DAE4ip                  | SN: 1602 | 06-Nov-24 (No. DAE4ip-1602_Nov24) | Nov-25        |

| Secondary Standards              | ID             | Check Date (in house)                    | Scheduled Check |
|----------------------------------|----------------|------------------------------------------|-----------------|
| Signal Generator R&S SMF100A     | SN: 100184     | 26-Nov-24 (No. 5G-Source-Cal-IHC-202411) | Nov-25          |
| Power Sensor R&S NRP18S-10       | SN: 101258     | 26-Nov-24 (No. 5G-Source-Cal-IHC-202411) | Nov-25          |
| Network Analyzer Keysight E5063A | SN: MY54504221 | 30-Sept-24 (No. 675-CAL18-S4489-Sep24)   | Sep-26          |

|                                                                                                                 | Name           | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|----------------|-----------------------|-----------|
| Calibrated by                                                                                                   | Joanna Lleshaj | Laboratory Technician |           |
| Approved by                                                                                                     | Sven Kühn      | Technical Manager     |           |
| Issued: October 13, 2025                                                                                        |                |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                |                       |           |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

CW Continuous wave

## Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45, Calibration procedure for sources in air above 6 GHz.
- IEC/IEEE 63195-1, "Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (frequency range of 6 GHz to 300 GHz)", May 2022

## Methods Applied and Interpretation of Parameters

- *Coordinate System:* z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- *Measurement Conditions:* (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. The forward power is measured prior and after the measurement with a power sensor. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by far-field measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- *Horn Positioning:* The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- *E-field distribution:* The E-field is measured in two x-y-planes (10mm, 10mm +  $\lambda/4$ ) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm<sup>2</sup> and 4cm<sup>2</sup>) power density values at 10mm in front of the horn.
- *Field polarization:* Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

## Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m<sup>2</sup>) averaged over the surface area of 1 cm<sup>2</sup> and 4cm<sup>2</sup> at the nominal operational frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                |                               |      |
|--------------------------------|-------------------------------|------|
| DASY Version                   | DASY8 Module mmWave           | V3.2 |
| Phantom                        | 5G Phantom                    |      |
| Distance Horn Aperture - plane | 10 mm                         |      |
| Number of measured planes      | 2 (10mm, 10mm + $\lambda/4$ ) |      |
| Frequency                      | 10.0 GHz $\pm$ 10 MHz         |      |

## Calibration Parameters, 10 GHz

### Circular Averaging

| Distance Horn Aperture to Measurement Plane | Prad <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Avg Power Density<br>Avg ( psPDn+, psPDtot+, psPDmod+ )<br>(W/m <sup>2</sup> ) |                  | Uncertainty (k = 2) |
|---------------------------------------------|------------------------|-------------------|---------------------|--------------------------------------------------------------------------------|------------------|---------------------|
|                                             |                        |                   |                     | 1cm <sup>2</sup>                                                               | 4cm <sup>2</sup> |                     |
| 10 mm                                       | 93.3                   | 149               | 1.27 dB             | 57.7                                                                           | 54.1             | 1.28 dB             |

| Distance Horn Aperture to Measurement Plane | Prad <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                  | Uncertainty (k = 2) |
|---------------------------------------------|------------------------|-------------------|---------------------|--------------------------------------------------------------------|------------------|---------------------|
|                                             |                        |                   |                     | 1cm <sup>2</sup>                                                   | 4cm <sup>2</sup> |                     |
| 10 mm                                       | 93.3                   | 149               | 1.27 dB             | 57.5, 57.7, 57.9                                                   | 53.8, 54.1, 54.3 | 1.28 dB             |

### Square Averaging

| Distance Horn Aperture to Measurement Plane | Prad <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Avg Power Density<br>Avg ( psPDn+, psPDtot+, psPDmod+ )<br>(W/m <sup>2</sup> ) |                  | Uncertainty (k = 2) |
|---------------------------------------------|------------------------|-------------------|---------------------|--------------------------------------------------------------------------------|------------------|---------------------|
|                                             |                        |                   |                     | 1cm <sup>2</sup>                                                               | 4cm <sup>2</sup> |                     |
| 10 mm                                       | 93.3                   | 149               | 1.27 dB             | 57.7                                                                           | 54.0             | 1.28 dB             |

| Distance Horn Aperture to Measurement Plane | Prad <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Power Density<br>psPDn+, psPDtot+, psPDmod+<br>(W/m <sup>2</sup> ) |                  | Uncertainty (k = 2) |
|---------------------------------------------|------------------------|-------------------|---------------------|--------------------------------------------------------------------|------------------|---------------------|
|                                             |                        |                   |                     | 1cm <sup>2</sup>                                                   | 4cm <sup>2</sup> |                     |
| 10 mm                                       | 93.3                   | 149               | 1.27 dB             | 57.5, 57.6, 57.9                                                   | 53.7, 54.0, 54.2 | 1.28 dB             |

### Max Power Density

| Distance Horn Aperture to Measurement Plane | Prad <sup>1</sup> (mW) | Max E-field (V/m) | Uncertainty (k = 2) | Max Power Density<br>Sn, Stot,  Stot <br>(W/m <sup>2</sup> ) | Uncertainty (k = 2) |
|---------------------------------------------|------------------------|-------------------|---------------------|--------------------------------------------------------------|---------------------|
| 10 mm                                       | 93.3                   | 149               | 1.27 dB             | 58.9, 59.0, 59.3                                             | 1.28 dB             |


<sup>1</sup> Assessed ohmic and mismatch loss plus numerical offset: 0.30 dB

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.5 $\Omega$ – 1.2 j $\Omega$ |
| Return Loss                          | -29.0 dB                       |

Impedance Measurement Plot

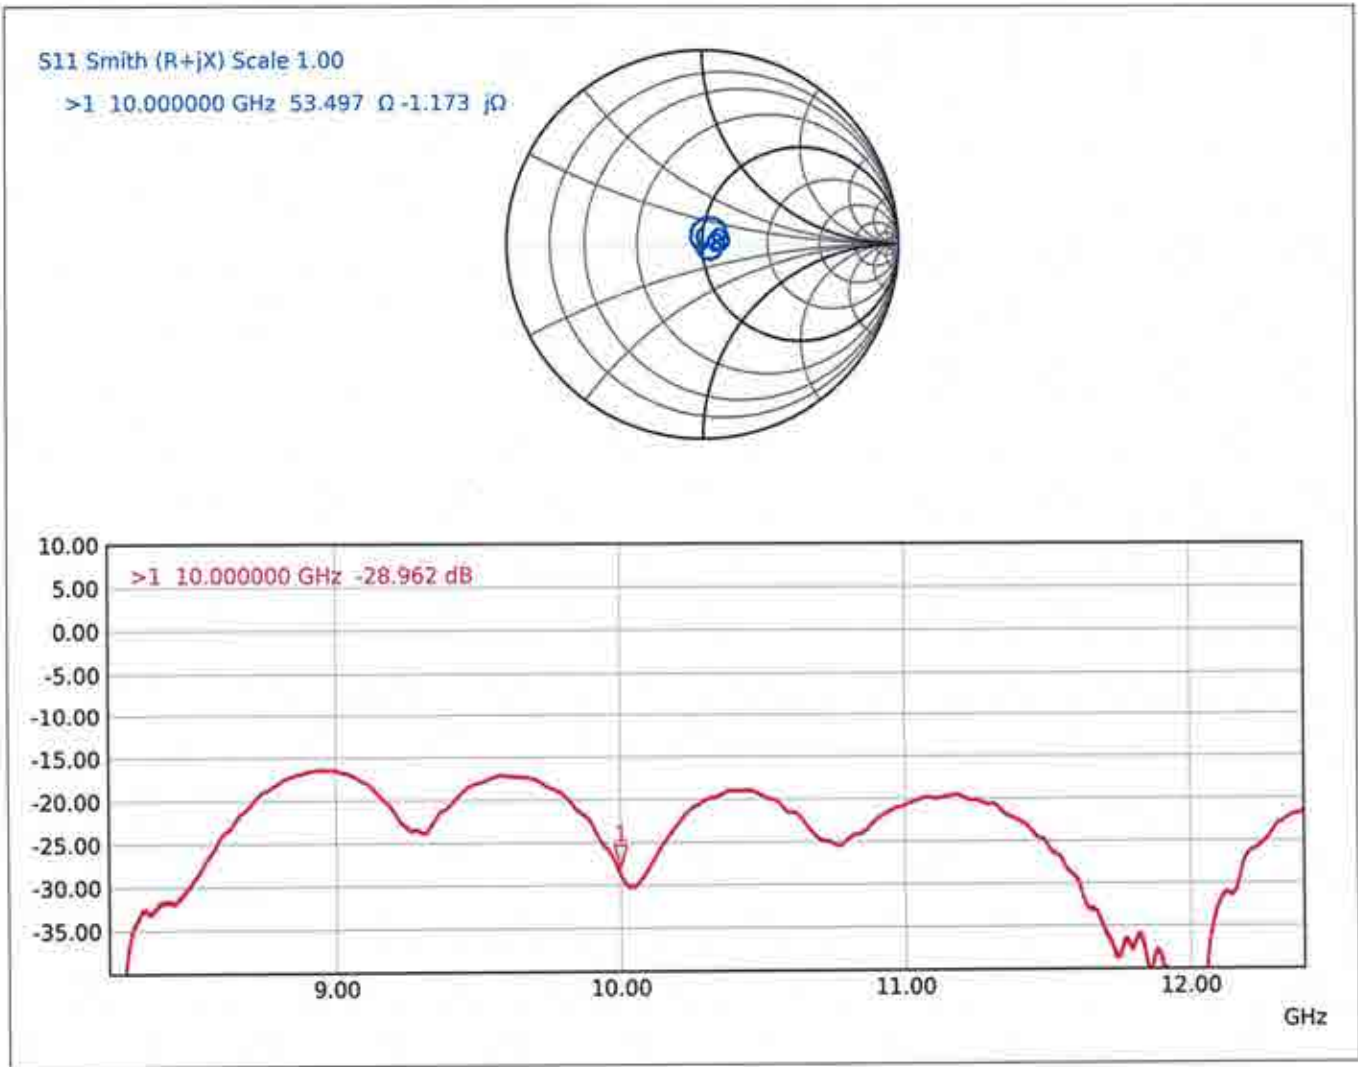

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000.0 (10000.0 MHz)

Device Under Test Properties

| Model, Manufacturer             | Dimensions [mm]       | IMEI     | DUT Type |
|---------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz - | 100.0 x 100.0 x 172.0 | SN: 1052 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, UID | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|------------|---------------------------------|-------------------|
| SG -            | 10.0 mm                      | Validation band | CW, 0-     | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom          | Medium | Probe, Calibration Date               | DAE, Calibration Date       |
|------------------|--------|---------------------------------------|-----------------------------|
| mmWave Phantom - | Air -  | ELmmWV3 - SN9374_FT-55GHz, 2025-08-26 | DAE4lp - SN1602, 2024-11-06 |

Scans Setup

|                     |               |
|---------------------|---------------|
| Sensor Surface [mm] | 10.0          |
| MAIA                | MAIA not used |

Measurement Results

|                                |                    |
|--------------------------------|--------------------|
| Scan Type                      | 5G Scan            |
| Date                           | 2025-10-13         |
| Avg. Area [cm <sup>2</sup> ]   | 1.00               |
| Avg. Type                      | Circular Averaging |
| psPDn+ [W/m <sup>2</sup> ]     | 57.5               |
| psPDtot+ [W/m <sup>2</sup> ]   | 57.7               |
| psPDmod+ [W/m <sup>2</sup> ]   | 57.9               |
| Max(Sn) [W/m <sup>2</sup> ]    | 58.9               |
| Max(Stot) [W/m <sup>2</sup> ]  | 59.0               |
| Max(Stot1) [W/m <sup>2</sup> ] | 59.3               |
| E <sub>max</sub> [V/m]         | 149                |
| Power Drift [dB]               | -0.01              |

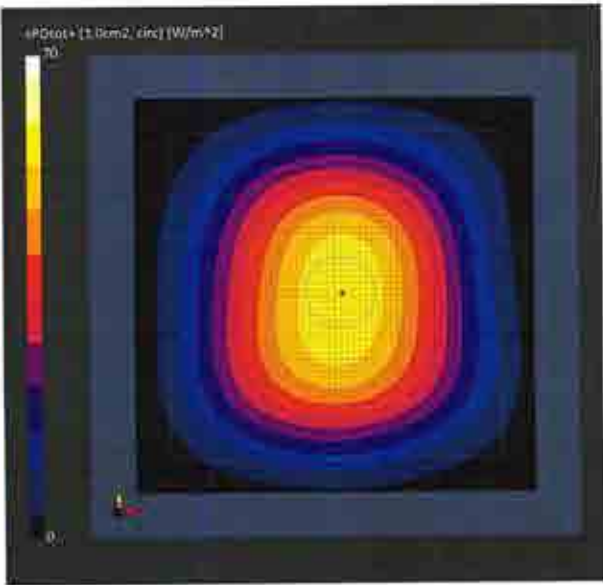

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000.0 (10000.0 MHz)

Device Under Test Properties

| Model, Manufacturer             | Dimensions [mm]       | IMEI     | DUT Type |
|---------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz - | 100.0 x 100.0 x 172.0 | SN: 1052 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, UID | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|------------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW, 0 --   | 10000.0, 10000                  | 1.0               |

Hardware Setup


| Phantom          | Medium | Probe, Calibration Date               | DAE, Calibration Date       |
|------------------|--------|---------------------------------------|-----------------------------|
| mmWave Phantom - | Air -  | E3mmWV3 - SN9374_F1-55GHz, 2025-08-26 | DAE4ip - SN1602, 2024-11-06 |

Scans Setup

|                     |               |
|---------------------|---------------|
| Sensor Surface [mm] | 10.0          |
| MAIA                | MAIA not used |

Measurement Results

|                        |                    |
|------------------------|--------------------|
| Scan Type              | 5G Scan            |
| Date                   | 2025-10-13         |
| Avg. Area [cm²]        | 4.00               |
| Avg. Type              | Circular Averaging |
| psPDn+ [W/m²]          | 53.8               |
| psPDtot+ [W/m²]        | 54.1               |
| psPDmod+ [W/m²]        | 54.3               |
| Max(Sn) [W/m²]         | 58.9               |
| Max(Stot) [W/m²]       | 59.0               |
| Max(IStot) [W/m²]      | 59.3               |
| E <sub>max</sub> [V/m] | 149                |
| Power Drift [dB]       | -0.01              |

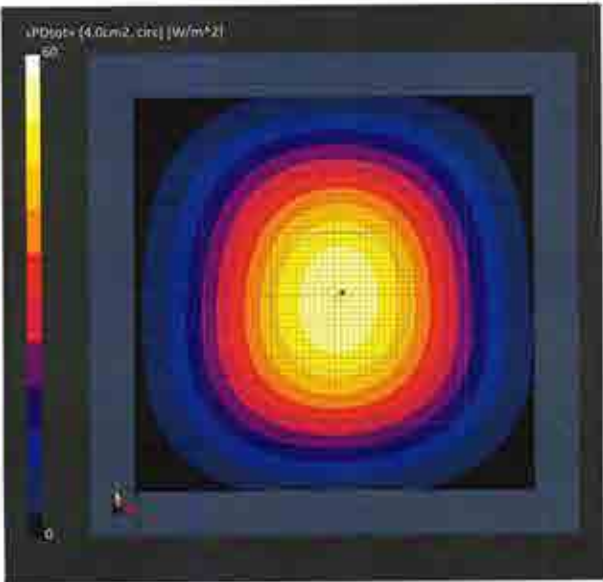

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000.0 (10000.0 MHz)

Device Under Test Properties

| Model, Manufacturer           | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1052 | —        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, UID | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|------------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW, 0—     | 10000.0,10000                   | 1.0               |

Hardware Setup


| Phantom          | Medium | Probe, Calibration Date                | DAE, Calibration Date       |
|------------------|--------|----------------------------------------|-----------------------------|
| mmWave Phantom - | Air -  | EUmmWV3 - SN9374, F1-55GHz, 2025-08-26 | DAE4ip - SN1602, 2024-11-06 |

Scans Setup

|                     |               |
|---------------------|---------------|
| Sensor Surface [mm] | 10.0          |
| MAIA                | MAIA not used |

Measurement Results

|                                |                  |
|--------------------------------|------------------|
| Scan Type                      | 5G Scan          |
| Date                           | 2025-10-13       |
| Avg. Area [cm <sup>2</sup> ]   | 1.00             |
| Avg. Type                      | Square Averaging |
| psPDn+ [W/m <sup>2</sup> ]     | 57.5             |
| psPDtot+ [W/m <sup>2</sup> ]   | 57.6             |
| psPDmod+ [W/m <sup>2</sup> ]   | 57.9             |
| Max(Sn) [W/m <sup>2</sup> ]    | 58.9             |
| Max(Stot) [W/m <sup>2</sup> ]  | 59.0             |
| Max(IStot) [W/m <sup>2</sup> ] | 59.3             |
| E <sub>max</sub> [V/m]         | 149              |
| Power Drift [dB]               | -0.01            |

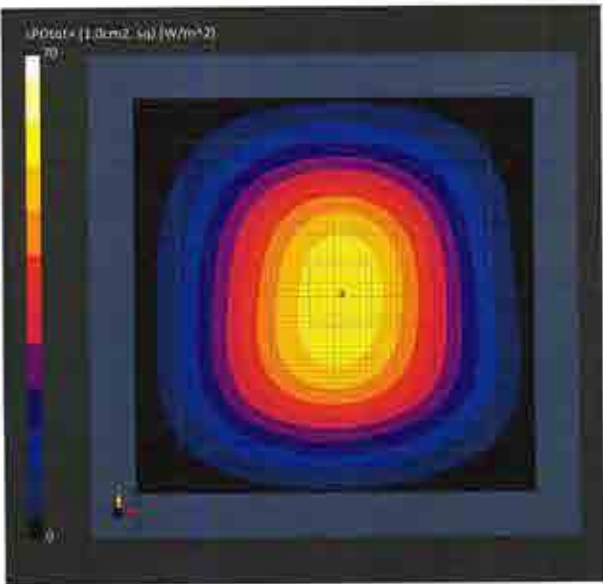

DASY Report

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000.0 (10000.0 MHz)

Device Under Test Properties

| Model, Manufacturer           | Dimensions [mm]       | IMEI     | DUT Type |
|-------------------------------|-----------------------|----------|----------|
| 5G Verification Source 10 GHz | 100.0 x 100.0 x 172.0 | SN: 1052 | -        |

Exposure Conditions

| Phantom Section | Position, Test Distance [mm] | Band            | Group, UID | Frequency [MHz], Channel Number | Conversion Factor |
|-----------------|------------------------------|-----------------|------------|---------------------------------|-------------------|
| 5G -            | 10.0 mm                      | Validation band | CW, 0-     | 10000.0,10000                   | 1.0               |

Hardware Setup


| Phantom          | Medium | Probe, Calibration Date                | DAE, Calibration Date       |
|------------------|--------|----------------------------------------|-----------------------------|
| mmWave Phantom - | Air -  | EDmirWV3 - SN9374_F1-55GHz, 2025-08-26 | DAE4ip - SN1602, 2024-11-08 |

Scans Setup

|                     |               |
|---------------------|---------------|
| Sensor Surface [mm] | 10.0          |
| MAIA                | MAIA not used |

Measurement Results

|                                |                  |
|--------------------------------|------------------|
| Scan Type                      | 5G Scan          |
| Date                           | 2025-10-13       |
| Avg. Area [cm <sup>2</sup> ]   | 4.00             |
| Avg. Type                      | Square Averaging |
| psPDn+ [W/m <sup>2</sup> ]     | 53.7             |
| psPDtot+ [W/m <sup>2</sup> ]   | 54.0             |
| psPDmod+ [W/m <sup>2</sup> ]   | 54.2             |
| Max(Sn) [W/m <sup>2</sup> ]    | 58.9             |
| Max(Stot) [W/m <sup>2</sup> ]  | 59.0             |
| Max(IStot) [W/m <sup>2</sup> ] | 59.3             |
| E <sub>max</sub> [V/m]         | 149              |
| Power Drift [dB]               | -0.01            |

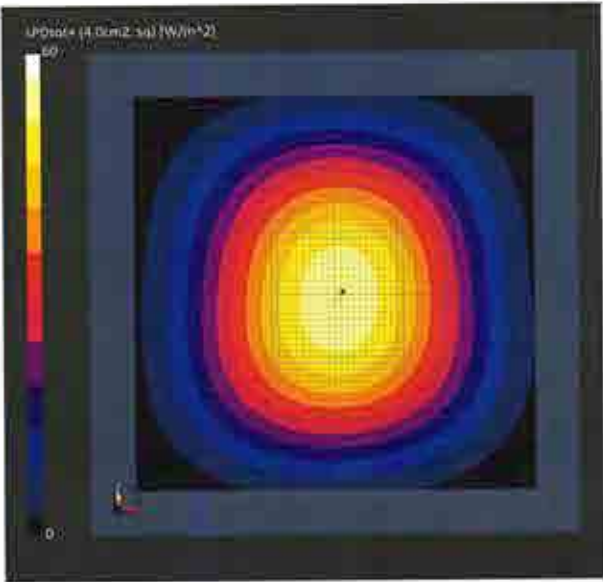



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **Sporton**  
Taoyuan City

Certificate No: DAE4-853\_Sep25

## CALIBRATION CERTIFICATE

Object DAE4 - SD 000 D04 BM - SN: 853

Calibration procedure(s) QA CAL-06.v30  
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: September 09, 2025

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards             | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 0810278        | 15-Aug-25 (No:43873)       | Aug-26                 |
| Secondary Standards           | ID #               | Check Date (in house)      | Scheduled Check        |
| Auto DAE Calibration Unit     | SE UWS 053 AA 1001 | 23-Jan-25 (in house check) | In house check: Jan-26 |
| Calibrator Box V2.1           | SE UMS 006 AA 1002 | 23-Jan-25 (in house check) | In house check: Jan-26 |

Calibrated by: Name Adrian Gehring Function Laboratory Technician Signature

Approved by: Sven Kühn Technical Manager

Issued: September 9, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

**DAE** data acquisition electronics  
**Connector angle** information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1  $\mu$ V full range = -100...+300 mV

Low Range: 1LSB = 61nV full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 402.944 $\pm$ 0.02% (k=2) | 403.599 $\pm$ 0.02% (k=2) | 403.766 $\pm$ 0.02% (k=2) |
| Low Range           | 3.98023 $\pm$ 1.50% (k=2) | 3.97690 $\pm$ 1.50% (k=2) | 4.00374 $\pm$ 1.50% (k=2) |

## Connector Angle

|                                           |                   |
|-------------------------------------------|-------------------|
| Connector Angle to be used in DASY system | 133.5 ° $\pm$ 1 ° |
|-------------------------------------------|-------------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range        | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 199999.90                 | 2.73                         | 0.00      |
| Channel X + Input | 20003.46                  | 0.57                         | 0.00      |
| Channel X - Input | -19999.05                 | 3.32                         | -0.02     |
| Channel Y + Input | 199999.49                 | 2.43                         | 0.00      |
| Channel Y + Input | 20000.86                  | -1.70                        | -0.01     |
| Channel Y - Input | -20002.85                 | -0.17                        | 0.00      |
| Channel Z + Input | 199997.32                 | -0.04                        | -0.00     |
| Channel Z + Input | 20001.26                  | -1.33                        | -0.01     |
| Channel Z - Input | -20003.33                 | -0.82                        | 0.00      |

| Low Range         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 2001.35                   | 0.09                         | 0.00      |
| Channel X + Input | 202.16                    | 0.75                         | 0.37      |
| Channel X - Input | -197.80                   | 0.46                         | -0.23     |
| Channel Y + Input | 2001.35                   | 0.26                         | 0.01      |
| Channel Y + Input | 200.63                    | -0.72                        | -0.36     |
| Channel Y - Input | -198.59                   | -0.22                        | 0.11      |
| Channel Z + Input | 2001.03                   | -0.02                        | -0.00     |
| Channel Z + Input | 200.38                    | -0.92                        | -0.46     |
| Channel Z - Input | -199.24                   | -0.84                        | 0.42      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | -6.15                                        | -7.69                                       |
|           | - 200                          | 10.15                                        | 8.70                                        |
| Channel Y | 200                            | 5.35                                         | 4.96                                        |
|           | - 200                          | -5.32                                        | -5.90                                       |
| Channel Z | 200                            | 0.07                                         | 0.91                                        |
|           | - 200                          | -3.03                                        | -2.80                                       |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | -0.33                       | -2.28                       |
| Channel Y | 200                | 6.00                        | -                           | 0.65                        |
| Channel Z | 200                | 10.19                       | 2.84                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16123            | 16108           |
| Channel Y | 15971            | 16466           |
| Channel Z | 16115            | 15716           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.79               | 0.02                   | 1.61                   | 0.33                      |
| Channel Y | 0.39               | -0.77                  | 1.51                   | 0.42                      |
| Channel Z | 0.22               | -1.54                  | 1.35                   | 0.48                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Sporton**  
Taoyuan City

Certificate No: **DAE4-699\_Feb26**

## CALIBRATION CERTIFICATE

Object **DAE4 - SD.000 D04 BO - SN: 699**

Calibration procedure(s) **QA CAL-06.v30**  
**Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **February 13, 2026**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards             | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 0810278        | 15-Aug-25 (No:43873)       | Aug-26                 |
| Secondary Standards           | ID #               | Check Date (in house)      | Scheduled Check        |
| Auto DAE Calibration Unit     | SE UWS 053 AA 1001 | 23-Jan-26 (in house check) | In house check: Jan-27 |
| Calibrator Box V2.1           | SE UMS 006 AA 1002 | 23-Jan-26 (in house check) | In house check: Jan-27 |

Calibrated by: **Name** **Adrian Gehring** **Function** **Laboratory Technician** **Signature**

Approved by: **Sven Kühn** **Technical Manager**

Issued: February 13, 2026

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|                 |                                                                                         |
|-----------------|-----------------------------------------------------------------------------------------|
| DAE             | data acquisition electronics                                                            |
| Connector angle | information used in DASY system to align probe sensor X to the robot coordinate system. |

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1  $\mu$ V , full range = -100...+300 mV

Low Range: 1LSB = 61 nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 404.780 $\pm$ 0.02% (k=2) | 403.410 $\pm$ 0.02% (k=2) | 404.576 $\pm$ 0.02% (k=2) |
| Low Range           | 3.93354 $\pm$ 1.50% (k=2) | 3.95127 $\pm$ 1.50% (k=2) | 3.97689 $\pm$ 1.50% (k=2) |

## Connector Angle

|                                           |                   |
|-------------------------------------------|-------------------|
| Connector Angle to be used in DASY system | 171.5 ° $\pm$ 1 ° |
|-------------------------------------------|-------------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range |         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|------------|---------|---------------------------|------------------------------|-----------|
| Channel X  | + Input | 199995.30                 | -0.31                        | -0.00     |
| Channel X  | + Input | 20002.17                  | -0.43                        | -0.00     |
| Channel X  | - Input | -19998.37                 | 3.90                         | -0.02     |
| Channel Y  | + Input | 199996.48                 | 0.68                         | 0.00      |
| Channel Y  | + Input | 20000.78                  | -1.85                        | -0.01     |
| Channel Y  | - Input | -20005.47                 | -3.23                        | 0.02      |
| Channel Z  | + Input | 199995.87                 | 0.13                         | 0.00      |
| Channel Z  | + Input | 20000.06                  | -2.57                        | -0.01     |
| Channel Z  | - Input | -20001.49                 | 0.76                         | -0.00     |

| Low Range |         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-----------|---------|---------------------------|------------------------------|-----------|
| Channel X | + Input | 2001.21                   | 0.11                         | 0.01      |
| Channel X | + Input | 201.80                    | 0.56                         | 0.28      |
| Channel X | - Input | -197.99                   | 0.44                         | -0.22     |
| Channel Y | + Input | 2002.02                   | 1.10                         | 0.05      |
| Channel Y | + Input | 200.29                    | -0.83                        | -0.41     |
| Channel Y | - Input | -199.47                   | -0.87                        | 0.44      |
| Channel Z | + Input | 2001.17                   | 0.15                         | 0.01      |
| Channel Z | + Input | 200.90                    | -0.21                        | -0.11     |
| Channel Z | - Input | -199.00                   | -0.38                        | 0.19      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | -1.66                                        | -2.85                                       |
|           | - 200                          | 3.68                                         | 3.02                                        |
| Channel Y | 200                            | 23.39                                        | 23.20                                       |
|           | - 200                          | -24.68                                       | -25.34                                      |
| Channel Z | 200                            | 8.20                                         | 8.06                                        |
|           | - 200                          | -9.68                                        | -9.33                                       |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | -2.01                       | -1.80                       |
| Channel Y | 200                | 7.64                        | -                           | -1.09                       |
| Channel Z | 200                | 3.99                        | 7.42                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16112            | 16319           |
| Channel Y | 16432            | 16440           |
| Channel Z | 16307            | 17302           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.90               | -0.99                  | 1.74                   | 0.42                      |
| Channel Y | -0.67              | -1.76                  | 0.54                   | 0.47                      |
| Channel Z | -0.11              | -0.82                  | 0.82                   | 0.35                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Sporton**  
Taoyuan City

Certificate No: **DAE3-577\_Mar26**

## CALIBRATION CERTIFICATE

Object **DAE3 - SD 000 D03 AA - SN: 577**

Calibration procedure(s) **QA CAL-06.v30**  
**Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **March 13, 2026**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards             | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001 | SN: 0810278        | 15-Aug-25 (No:43873)       | Aug-26                 |
| Secondary Standards           | ID #               | Check Date (in house)      | Scheduled Check        |
| Auto DAE Calibration Unit     | SE UWS 053 AA 1001 | 23-Jan-26 (in house check) | In house check: Jan-27 |
| Calibrator Box V2.1           | SE UMS 006 AA 1002 | 23-Jan-26 (in house check) | In house check: Jan-27 |

Calibrated by: 

| Name           | Function              | Signature |
|----------------|-----------------------|-----------|
| Adrian Gehring | Laboratory Technician |           |

Approved by: 

| Name      | Function          |
|-----------|-------------------|
| Sven Kühn | Technical Manager |

Issued: March 13, 2026

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full-scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal  
High Range: 1LSB = 6.1µV , full range = -100...+300 mV  
Low Range: 1LSB = 61nV , full range = -1.....+3mV  
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                     | Y                     | Z                     |
|---------------------|-----------------------|-----------------------|-----------------------|
| High Range          | 403.594 ± 0.02% (k=2) | 403.579 ± 0.02% (k=2) | 403.883 ± 0.02% (k=2) |
| Low Range           | 3.92875 ± 1.50% (k=2) | 3.94327 ± 1.50% (k=2) | 3.96211 ± 1.50% (k=2) |

Connector Angle

|                                           |               |
|-------------------------------------------|---------------|
| Connector Angle to be used in DASY system | 181.5 ° ± 1 ° |
|-------------------------------------------|---------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range |         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|------------|---------|---------------------------|------------------------------|-----------|
| Channel X  | + Input | 199998.73                 | -0.88                        | -0.00     |
| Channel X  | + Input | 20007.99                  | 2.82                         | 0.01      |
| Channel X  | - Input | -19996.12                 | 3.68                         | -0.02     |
| Channel Y  | + Input | 199997.57                 | -1.72                        | -0.00     |
| Channel Y  | + Input | 20007.54                  | 2.40                         | 0.01      |
| Channel Y  | - Input | -20000.80                 | -0.90                        | 0.00      |
| Channel Z  | + Input | 199996.25                 | -3.13                        | -0.00     |
| Channel Z  | + Input | 20007.25                  | 2.18                         | 0.01      |
| Channel Z  | - Input | -19999.31                 | 0.65                         | -0.00     |

| Low Range |         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-----------|---------|---------------------------|------------------------------|-----------|
| Channel X | + Input | 2004.79                   | 1.16                         | 0.06      |
| Channel X | + Input | 204.92                    | 1.11                         | 0.55      |
| Channel X | - Input | -194.93                   | 1.02                         | -0.52     |
| Channel Y | + Input | 2004.46                   | 0.91                         | 0.05      |
| Channel Y | + Input | 203.53                    | -0.16                        | -0.08     |
| Channel Y | - Input | -196.56                   | -0.46                        | 0.23      |
| Channel Z | + Input | 2003.59                   | 0.07                         | 0.00      |
| Channel Z | + Input | 203.31                    | -0.41                        | -0.20     |
| Channel Z | - Input | -196.88                   | -0.83                        | 0.42      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | -1.22                                        | -3.75                                       |
|           | - 200                          | 5.26                                         | 3.48                                        |
| Channel Y | 200                            | -13.64                                       | -14.09                                      |
|           | - 200                          | 12.82                                        | 12.95                                       |
| Channel Z | 200                            | 3.13                                         | 3.18                                        |
|           | - 200                          | -5.09                                        | -5.38                                       |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | -0.79                       | -3.05                       |
| Channel Y | 200                | 8.18                        | -                           | 0.74                        |
| Channel Z | 200                | 5.96                        | 5.47                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16123            | 15210           |
| Channel Y | 16101            | 16475           |
| Channel Z | 16089            | 12697           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 1.03               | 0.38                   | 1.55                   | 0.28                      |
| Channel Y | -0.09              | -1.15                  | 1.93                   | 0.47                      |
| Channel Z | -0.86              | -1.78                  | 0.16                   | 0.33                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
 Taoyuan City

Certificate No.

**EX-7822\_Sep25**

## CALIBRATION CERTIFICATE

Object

**EX3DV4 - SN:7822**

Calibration procedure(s)

**QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6,  
 QA CAL-25.v8  
 Calibration procedure for dosimetric E-field probes**

Calibration date

**September 11, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Calibration Date (Certificate No.)     | Sched. Cal. |
|-----------------------------|------------|----------------------------------------|-------------|
| Power Sensor R&S NRP-33T    | SN: 100967 | 30-Apr-25 (No. 1020-300791789)         | Apr-26      |
| N-type mismatch combination | SN: L1119  | 26-Mar-25 (No. 217-04292)              | Mar-26      |
| OCP DAK-12                  | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25      |
| OCP DAK-3.5                 | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25      |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26      |
| DAE4                        | SN: 1301   | 07-Nov-24 (No. DAE4-1301_Nov24)        | Nov-25      |

| Secondary Standards | ID        | Check Date (In house)                            | Sched. Check |
|---------------------|-----------|--------------------------------------------------|--------------|
| ACAP 2020 Setup 1   | SN: L1404 | 30-Sept-24 (No. Report_ACAP2020E-Cave_20240930s) | Sep-25       |
| OCP DAK-12          | SN: 1029  | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)             | Feb-26       |
| OCP DAK-3.5         | SN: 1336  | 09-Dec-24 (No. OCP-DAK3.5-1336_Dec24)            | Dec-25       |

Calibrated by **Jeffrey Katzman** Laboratory Technician

Approved by **Sven Kühn** Technical Manager

Signature

Issued: September 11, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

|                        |                                                                                                                                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                    | tissue simulating liquid                                                                                                                       |
| NORM <sub>x,y,z</sub>  | sensitivity in free space                                                                                                                      |
| ConvF                  | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                     |
| DCP                    | diode compression point                                                                                                                        |
| CF                     | crest factor (1/duty_cycle) of the RF signal                                                                                                   |
| A, B, C, D             | modulation dependent linearization parameters                                                                                                  |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |
| Connector Angle        | information used in DASY system to align probe sensor X to the robot coordinate system                                                         |

## Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices – Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart): This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

## Parameters of Probe: EX3DV4 - SN:7822

## Basic Calibration Parameters

|                                                    | Sensor X | Sensor Y | Sensor Z | Unc (k = 2)  |
|----------------------------------------------------|----------|----------|----------|--------------|
| Norm ( $\mu\text{V}/(\text{V/m})^2$ ) <sup>A</sup> | 0.59     | 0.69     | 0.67     | $\pm 10.1\%$ |
| DCP (mV) <sup>B</sup>                              | 109.3    | 105.2    | 105.1    | $\pm 4.7\%$  |

## Calibration Results for Modulation Response

| UID   | Communication System Name      |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C     | D<br>dB | VR<br>mV | Max<br>dev. | Max<br>Unc <sup>E</sup><br>k = 2 |
|-------|--------------------------------|---|---------|------------------------------|-------|---------|----------|-------------|----------------------------------|
| 0     | Continuous Wave                | X | 0.00    | 0.00                         | 1.00  | 0.00    | 143.4    | $\pm 1.2\%$ | $\pm 4.7\%$                      |
|       |                                | Y | 0.00    | 0.00                         | 1.00  |         | 128.5    |             |                                  |
|       |                                | Z | 0.00    | 0.00                         | 1.00  |         | 121.7    |             |                                  |
| 10352 | Pulse (D=10%, T=5 ms)          | X | 0.19    | 59.44                        | 14.38 | 10.00   | 23.0     | $\pm 2.0\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.55    | 70.00                        | 18.25 |         | 24.0     |             |                                  |
|       |                                | Z | 0.41    | 69.98                        | 18.64 |         | 24.0     |             |                                  |
| 10353 | Pulse (D=20%, T=5 ms)          | X | 0.18    | 62.45                        | 14.41 | 6.99    | 46.0     | $\pm 1.7\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.51    | 73.01                        | 18.30 |         | 48.0     |             |                                  |
|       |                                | Z | 0.39    | 72.99                        | 18.68 |         | 48.0     |             |                                  |
| 10354 | Pulse (D=40%, T=5 ms)          | X | 0.17    | 65.46                        | 14.43 | 3.98    | 92.0     | $\pm 1.6\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.48    | 76.02                        | 18.34 |         | 97.0     |             |                                  |
|       |                                | Z | 0.36    | 76.00                        | 18.72 |         | 97.0     |             |                                  |
| 10355 | Pulse (D=60%, T=5 ms)          | X | 0.16    | 67.22                        | 14.45 | 2.22    | 139.0    | $\pm 1.5\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.46    | 77.78                        | 18.37 |         | 145.0    |             |                                  |
|       |                                | Z | 0.34    | 77.76                        | 18.74 |         | 145.0    |             |                                  |
| 10387 | Random (BW=1 MHz, MOD=QPSK)    | X | 0.01    | 64.34                        | 15.40 | 0.37    | 106.0    | $\pm 1.5\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.01    | 74.90                        | 19.65 |         | 112.0    |             |                                  |
|       |                                | Z | 0.00    | 50.03                        | 19.89 |         | 112.0    |             |                                  |
| 10388 | Random (BW=10 MHz, MOD=QPSK)   | X | 0.58    | 64.23                        | 13.69 | 0.00    | 112.0    | $\pm 2.7\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 1.68    | 74.78                        | 17.45 |         | 118.0    |             |                                  |
|       |                                | Z | 1.51    | 74.77                        | 17.78 |         | 119.0    |             |                                  |
| 10396 | Random (BW=100 kHz, MOD=64QAM) | X | 0.00    | 63.17                        | 16.54 | 1.64    | 81.0     | $\pm 3.1\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 0.00    | 73.72                        | 20.95 |         | 85.0     |             |                                  |
|       |                                | Z | 0.00    | 73.71                        | 20.92 |         | 85.0     |             |                                  |
| 10399 | Random (BW=40 MHz, MOD=64QAM)  | X | 1.57    | 63.17                        | 12.86 | 0.00    | 104.0    | $\pm 4.2\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 3.88    | 73.73                        | 17.33 |         | 110.0    |             |                                  |
|       |                                | Z | 3.61    | 73.71                        | 17.63 |         | 110.0    |             |                                  |
| 10414 | Random (BW=40 MHz, HIGH PAR)   | X | 1.96    | 60.91                        | 12.77 | 0.00    | 75.0     | $\pm 2.2\%$ | $\pm 9.6\%$                      |
|       |                                | Y | 4.77    | 71.46                        | 17.33 |         | 80.0     |             |                                  |
|       |                                | Z | 4.43    | 71.44                        | 17.63 |         | 80.0     |             |                                  |

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Linearization parameter uncertainty for maximum specified field strength.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## Parameters of Probe: EX3DV4 - SN:7822

### Sensor Model Parameters

|   | C1<br>fF | C2<br>fF | $\alpha$<br>$V^{-1}$ | T1<br>$ms V^{-2}$ | T2<br>$ms V^{-1}$ | T3<br>ms | T4<br>$V^{-2}$ | T5<br>$V^{-1}$ | T6   |
|---|----------|----------|----------------------|-------------------|-------------------|----------|----------------|----------------|------|
| x | 8.8      | 63.49    | 33.56                | 6.55              | 0.00              | 4.90     | 0.84           | 0.00           | 1.00 |
| y | 10.0     | 73.10    | 34.46                | 3.37              | 0.00              | 4.91     | 0.00           | 0.08           | 1.00 |
| z | 9.7      | 71.26    | 34.70                | 3.37              | 0.00              | 4.90     | 0.00           | 0.03           | 1.00 |

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle                               | 15.7°      |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 12 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 1.4 mm     |

**Note:** Measurement distance from surface can be increased to 3–4 mm for an Area Scan job.

## Parameters of Probe: EX3DV4 - SN:7822

## Calibration Parameter Determined in HSL

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity <sup>F</sup> (S/m) | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unc <sup>H</sup> (k = 2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|--------------------------|
| 750                  | 41.9                               | 0.89                            | 9.16    | 9.01    | 9.31    | 0.37               | 1.27                    | ±11.0%                   |
| 835                  | 41.5                               | 0.90                            | 9.03    | 8.87    | 9.17    | 0.37               | 1.27                    | ±11.0%                   |
| 900                  | 41.5                               | 0.97                            | 8.76    | 8.61    | 8.90    | 0.37               | 1.27                    | ±11.0%                   |
| 1750                 | 40.1                               | 1.37                            | 7.41    | 7.28    | 7.53    | 0.37               | 1.27                    | ±11.0%                   |
| 1900                 | 40.0                               | 1.40                            | 7.24    | 7.11    | 7.35    | 0.37               | 1.27                    | ±11.0%                   |
| 2000                 | 40.0                               | 1.40                            | 7.07    | 6.95    | 7.19    | 0.37               | 1.27                    | ±11.0%                   |
| 2300                 | 39.5                               | 1.67                            | 6.82    | 6.71    | 6.93    | 0.37               | 1.27                    | ±11.0%                   |
| 2450                 | 39.2                               | 1.80                            | 6.61    | 6.49    | 6.71    | 0.37               | 1.27                    | ±11.0%                   |
| 2600                 | 39.0                               | 1.96                            | 6.48    | 6.35    | 6.56    | 0.37               | 1.27                    | ±11.0%                   |
| 3300                 | 38.2                               | 2.71                            | 6.13    | 6.02    | 6.22    | 0.37               | 1.27                    | ±13.1%                   |
| 3500                 | 37.9                               | 2.91                            | 6.07    | 5.97    | 6.17    | 0.37               | 1.27                    | ±13.1%                   |
| 3700                 | 37.7                               | 3.12                            | 6.01    | 5.91    | 6.11    | 0.37               | 1.27                    | ±13.1%                   |
| 3900                 | 37.5                               | 3.32                            | 5.94    | 5.83    | 6.03    | 0.37               | 1.27                    | ±13.1%                   |
| 4100                 | 37.2                               | 3.53                            | 5.85    | 5.75    | 5.94    | 0.37               | 1.27                    | ±13.1%                   |
| 4200                 | 37.1                               | 3.63                            | 5.77    | 5.67    | 5.86    | 0.37               | 1.27                    | ±13.1%                   |
| 4400                 | 36.9                               | 3.84                            | 5.69    | 5.59    | 5.78    | 0.37               | 1.27                    | ±13.1%                   |
| 4600                 | 36.7                               | 4.04                            | 5.57    | 5.48    | 5.66    | 0.37               | 1.27                    | ±13.1%                   |
| 4800                 | 36.4                               | 4.25                            | 5.52    | 5.42    | 5.61    | 0.37               | 1.27                    | ±13.1%                   |
| 4950                 | 36.3                               | 4.40                            | 5.42    | 5.33    | 5.50    | 0.35               | 1.27                    | ±13.1%                   |
| 5250                 | 35.9                               | 4.71                            | 5.16    | 5.07    | 5.24    | 0.32               | 1.27                    | ±13.1%                   |
| 5600                 | 35.5                               | 5.07                            | 4.74    | 4.66    | 4.82    | 0.29               | 1.27                    | ±13.1%                   |
| 5800                 | 35.3                               | 5.27                            | 4.65    | 4.57    | 4.73    | 0.27               | 1.27                    | ±13.1%                   |

<sup>C</sup> Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ±50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4–9 MHz, and ConvF assessed at 13 MHz is 9–19 MHz. Above 5 GHz frequency validity can be extended to ±110 MHz.

<sup>F</sup> The probes are calibrated using tissue simulating liquids (TSL) that deviate for  $\epsilon$  and  $\sigma$  by less than ±5% from the target values (typically better than ±3%) and are valid for TSL with deviations of up to ±10% if SAR correction is applied.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3–6 GHz at any distance larger than half the probe tip diameter from the boundary.

<sup>H</sup> The stated uncertainty is the total calibration uncertainty (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

## Parameters of Probe: EX3DV4 - SN:7822

### Calibration Parameter Determined in HSL

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity <sup>F</sup> (S/m) | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unc <sup>H</sup> (k = 2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|--------------------------|
| 6500                 | 34.5                               | 6.07                            | 4.96    | 4.88    | 5.04    | 0.20               | 1.27                    | ±18.6%                   |

<sup>C</sup> Frequency validity is -600/+700 MHz at 6.5 GHz, ±700 MHz at or above 7 GHz, and ±150 MHz at 9.85 GHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


<sup>F</sup> The probes are calibrated using tissue simulating liquids (TSL) that deviate for  $\epsilon$  and  $\sigma$  by less than ±10% from the target values (typically better than ±6%) and are valid for TSL with deviations of up to ±10%.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz; below ±2% for frequencies between 3–6 GHz; and below ±4% for frequencies between 6–10 GHz at any distance larger than half the probe tip diameter from the boundary.

<sup>H</sup> The stated uncertainty is the total calibration uncertainty (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.



Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide:R22)

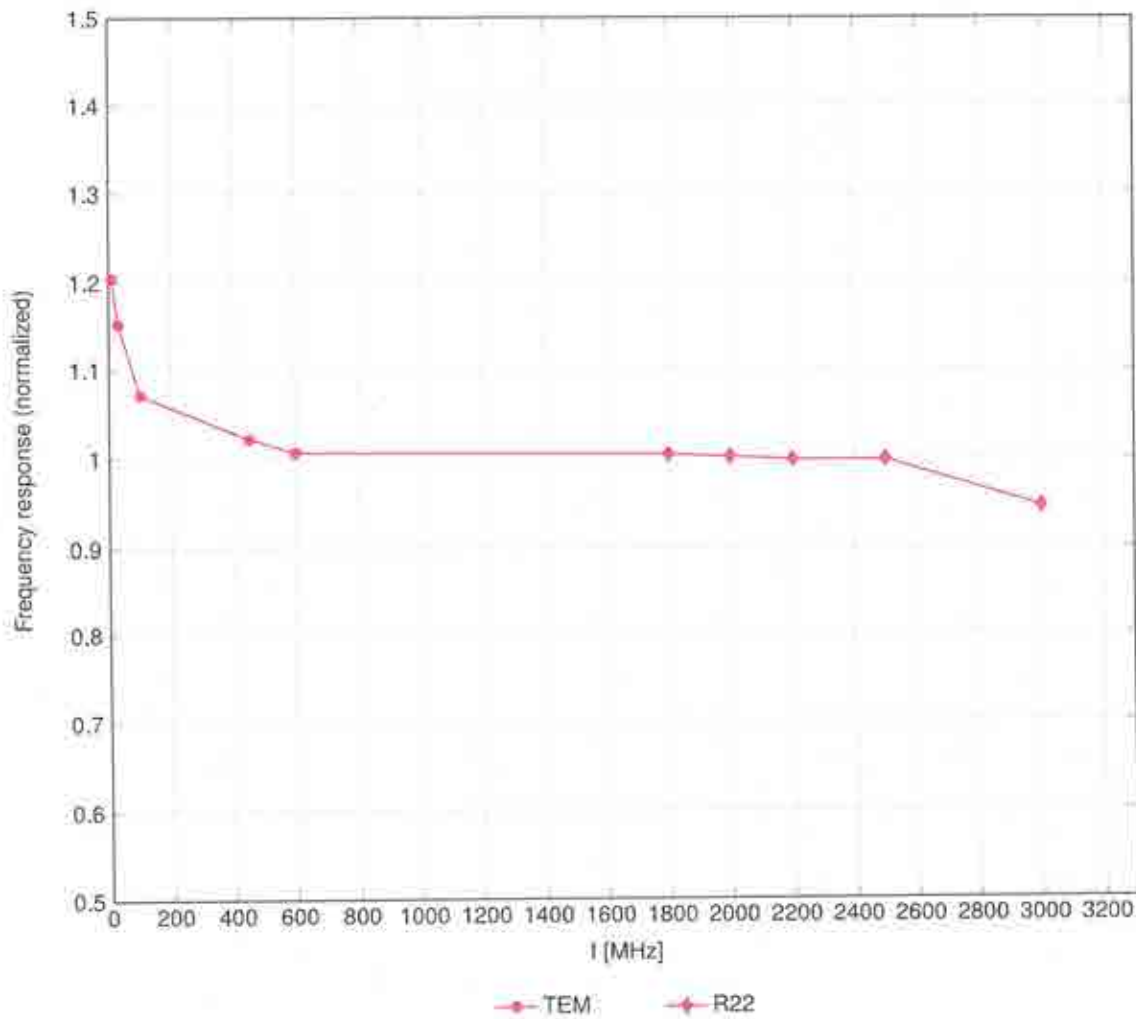

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )



### Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

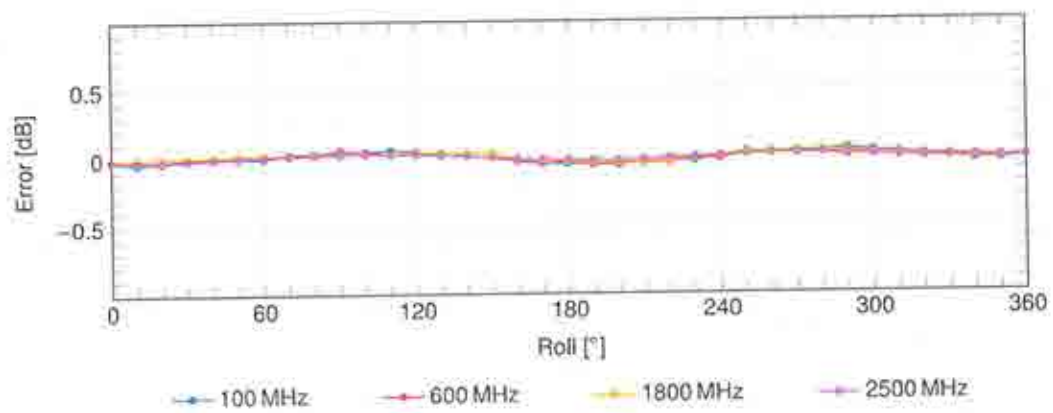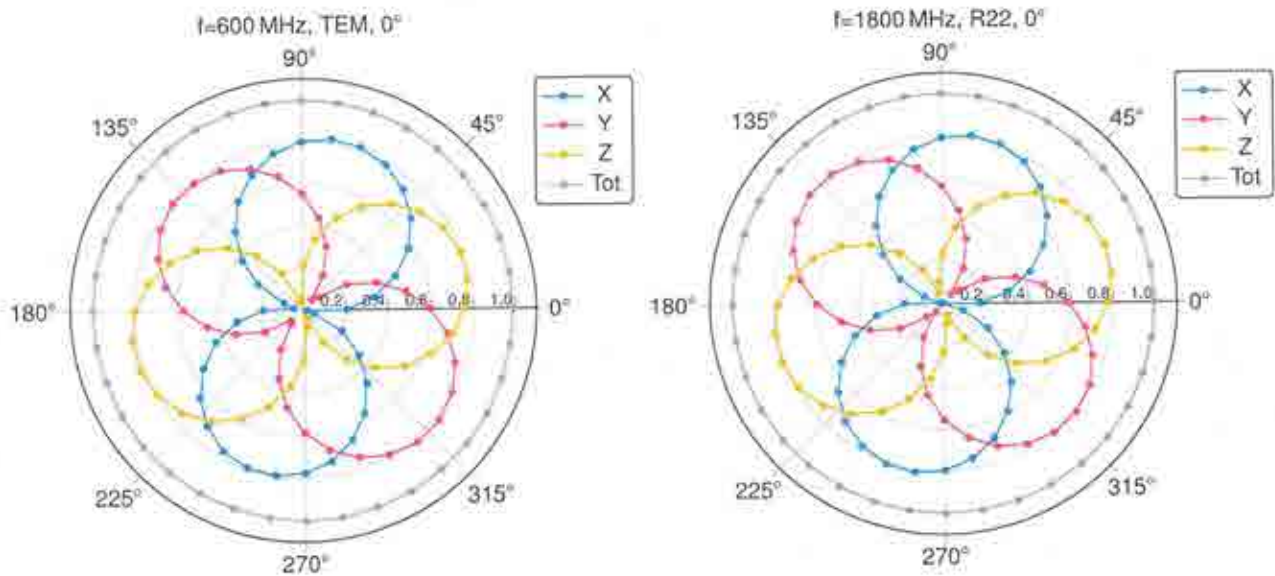

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


Dynamic Range f(SAR<sub>HSL</sub>)

(TEM cell, f<sub>eval</sub> = 1900 MHz)

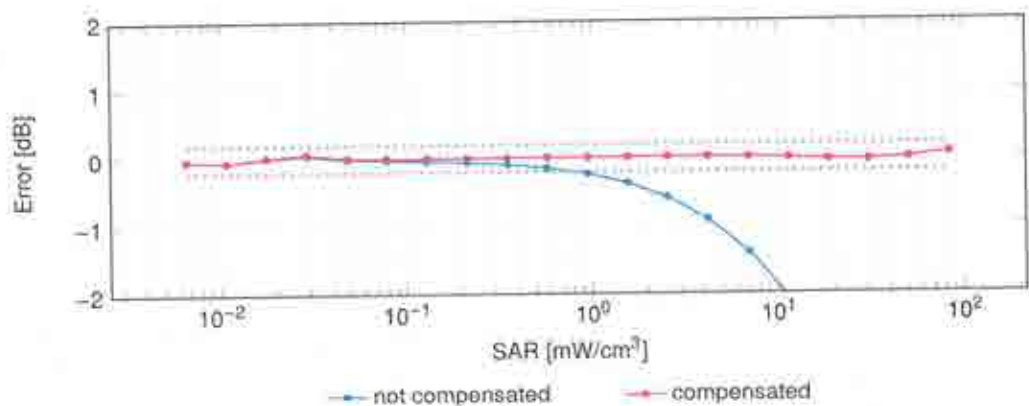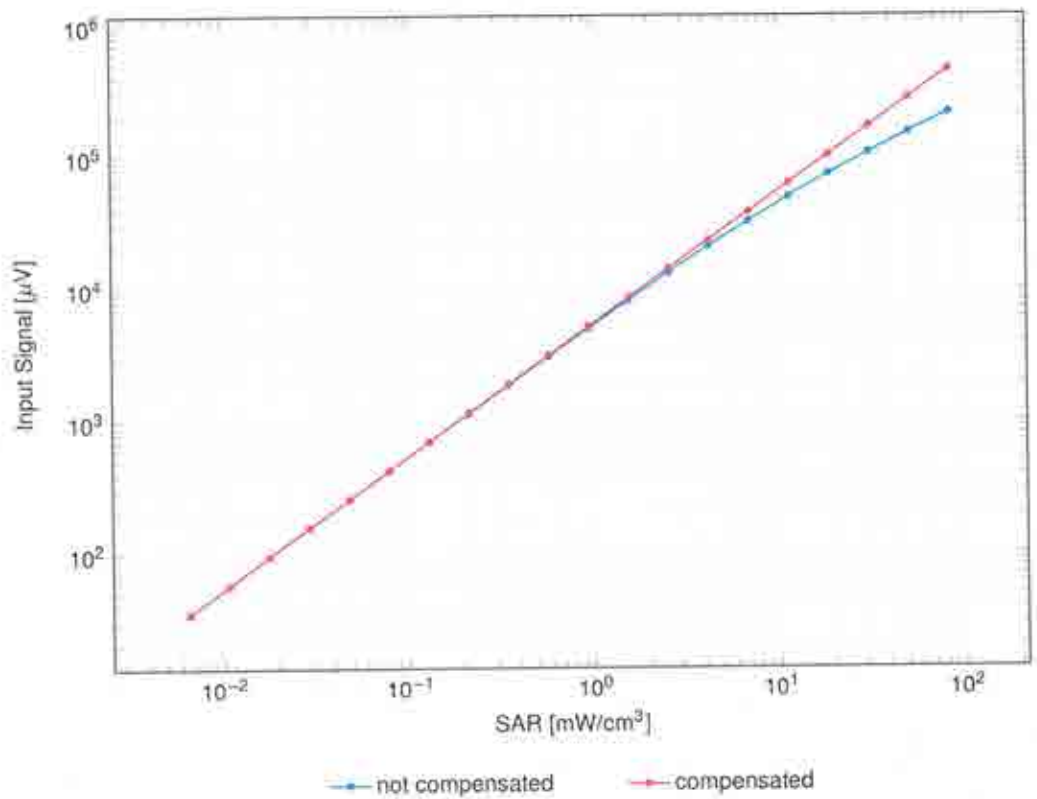


Uncertainty of Linearity Assessment: ±0.6% (k=2)

## Conversion Factor Assessment

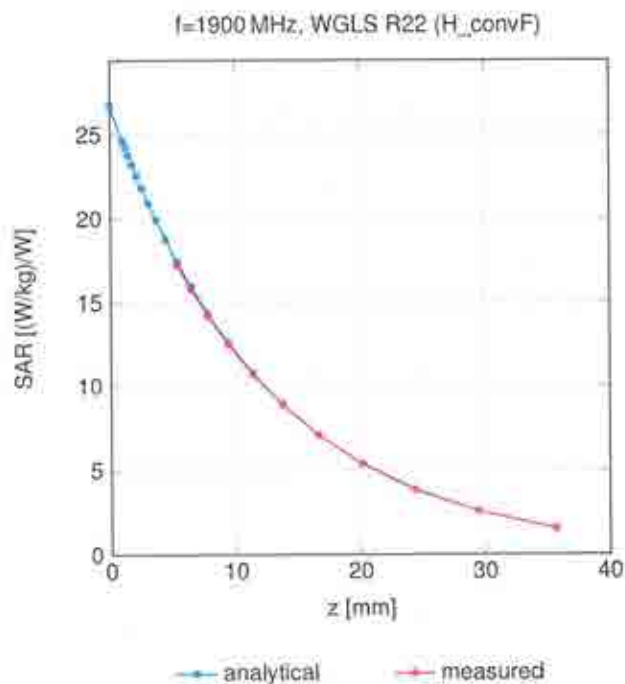

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900\text{ MHz}$

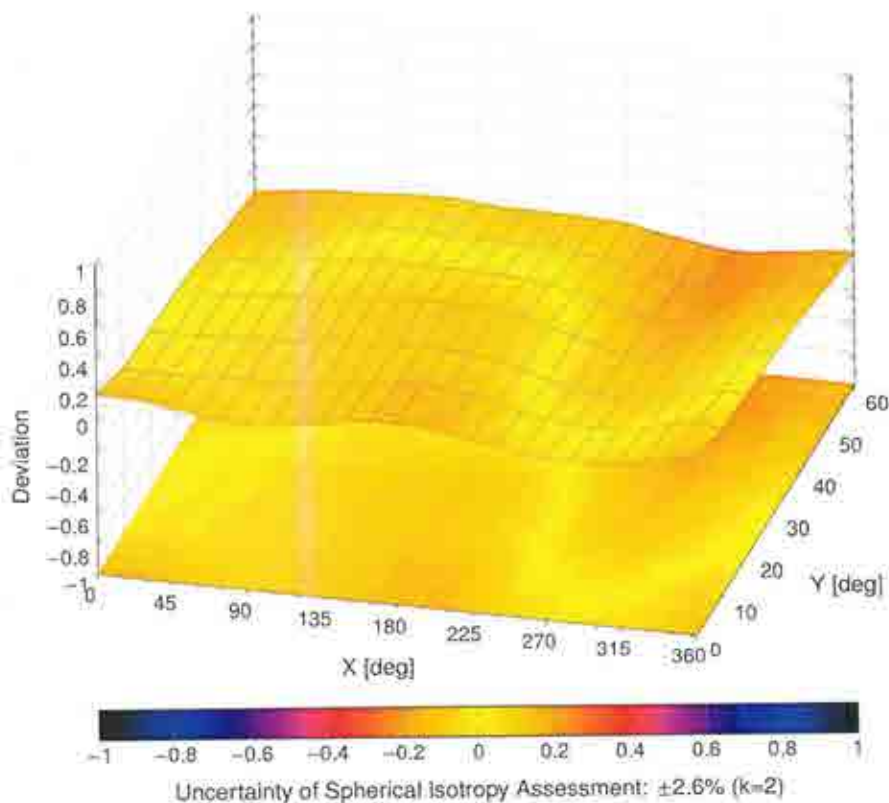

## Appendix: Modulation Calibration Parameters

| UID   | Rev | Communication System Name                      | Group     | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|------------------------------------------------|-----------|----------|------------------------|
| 0     |     | Continuous Wave                                | CW        | 0.00     | ±4.7                   |
| 10010 | CAB | Pulse (D=10%, T=100 ms)                        | Test      | 10.00    | ±9.6                   |
| 10011 | CAC | Ref. 99, RMC, QPSK, 5.0 MHz                    | WCDMA     | 2.91     | ±9.6                   |
| 10012 | CAB | DSSS, DBPSK, 1.0 Mbps, 92.5% DC                | WLAN      | 1.87     | ±9.6                   |
| 10013 | CAB | OFDM, BPSK, 6.0 Mbps, 72.1% DC                 | WLAN      | 9.46     | ±9.6                   |
| 10021 | DAC | Voice, GMSK, 1 slot(s)                         | GSM       | 9.39     | ±9.6                   |
| 10023 | DAC | Data, GMSK, 1 slot(s)                          | GSM       | 9.57     | ±9.6                   |
| 10024 | DAC | Data, GMSK, 2 slot(s)                          | GSM       | 6.56     | ±9.6                   |
| 10025 | DAC | Data, 8PSK, 1 slot(s)                          | GSM       | 12.62    | ±9.6                   |
| 10026 | DAC | Data, 8PSK, 2 slot(s)                          | GSM       | 9.55     | ±9.6                   |
| 10027 | DAC | Data, GMSK, 3 slot(s)                          | GSM       | 4.80     | ±9.6                   |
| 10028 | DAC | Data, GMSK, 4 slot(s)                          | GSM       | 3.55     | ±9.6                   |
| 10029 | DAC | Data, 8PSK, 3 slot(s)                          | GSM       | 7.78     | ±9.6                   |
| 10030 | CAA | BR, DH1, GFSK                                  | Bluetooth | 5.30     | ±9.6                   |
| 10031 | CAA | BR, DH3, GFSK                                  | Bluetooth | 1.87     | ±9.6                   |
| 10032 | CAA | BR, DH5, GFSK                                  | Bluetooth | 1.16     | ±9.6                   |
| 10033 | CAA | EDR, DH1, pi/4-DQPSK                           | Bluetooth | 7.74     | ±9.6                   |
| 10034 | CAA | EDR, DH3, pi/4-DQPSK                           | Bluetooth | 4.53     | ±9.6                   |
| 10035 | CAA | EDR, DH5, pi/4-DQPSK                           | Bluetooth | 3.83     | ±9.6                   |
| 10036 | CAA | EDR, DH1, 8-DPSK                               | Bluetooth | 8.01     | ±9.6                   |
| 10037 | CAA | EDR, DH3, 8-DPSK                               | Bluetooth | 4.77     | ±9.6                   |
| 10038 | CAA | EDR, DH5, 8-DPSK                               | Bluetooth | 4.10     | ±9.6                   |
| 10039 | CAB | RC1, 1xRTT                                     | CDMA2000  | 4.57     | ±9.6                   |
| 10048 | CAA | Full Slot, GFSK, 1 slot(s)                     | DECT      | 13.80    | ±9.6                   |
| 10049 | CAA | Double Slot, GFSK, 2 slot(s)                   | DECT      | 10.79    | ±9.6                   |
| 10056 | CAA | TD-SCDMA, QPSK, 1.6 MHz                        | TD-SCDMA  | 11.01    | ±9.6                   |
| 10058 | DAC | Data: 8PSK, 4 slot(s)                          | GSM       | 6.52     | ±9.6                   |
| 10059 | CAB | DSSS, DQPSK, 2.0 Mbps, 87.4% DC                | WLAN      | 2.12     | ±9.6                   |
| 10060 | CAB | HR-DSSS, DQPSK, 5.5 Mbps, 72.7% DC             | WLAN      | 2.63     | ±9.6                   |
| 10061 | CAB | HR-DSSS, DQPSK, 11.0 Mbps, 57.5% DC            | WLAN      | 3.60     | ±9.6                   |
| 10062 | CAE | OFDM, BPSK, 6.0 Mbps, 89.1% DC                 | WLAN      | 8.68     | ±9.6                   |
| 10063 | CAE | OFDM, BPSK, 9.0 Mbps, 85.3% DC                 | WLAN      | 8.83     | ±9.6                   |
| 10064 | CAE | OFDM, QPSK, 12.0 Mbps, 82.0% DC                | WLAN      | 9.09     | ±9.6                   |
| 10065 | CAE | OFDM, QPSK, 18.0 Mbps, 76.0% DC                | WLAN      | 9.00     | ±9.6                   |
| 10066 | CAE | OFDM, 16QAM, 24.0 Mbps, 70.6% DC               | WLAN      | 9.38     | ±9.6                   |
| 10067 | CAE | OFDM, 16QAM, 36.0 Mbps, 62.9% DC               | WLAN      | 10.12    | ±9.6                   |
| 10068 | CAE | OFDM, 64QAM, 48.0 Mbps, 56.6% DC               | WLAN      | 10.24    | ±9.6                   |
| 10069 | CAE | OFDM, 64QAM, 54.0 Mbps, 54.4% DC               | WLAN      | 10.56    | ±9.6                   |
| 10071 | CAB | OFDM, BPSK, 9.0 Mbps, 85.1% DC                 | WLAN      | 9.83     | ±9.6                   |
| 10072 | CAB | OFDM, QPSK, 12.0 Mbps, 80.1% DC                | WLAN      | 9.62     | ±9.6                   |
| 10073 | CAB | OFDM, QPSK, 18.0 Mbps, 53.1% DC                | WLAN      | 9.94     | ±9.6                   |
| 10074 | CAB | OFDM, 16QAM, 24.0 Mbps, 48.5% DC               | WLAN      | 10.30    | ±9.6                   |
| 10075 | CAB | OFDM, 16QAM, 36.0 Mbps, 42.9% DC               | WLAN      | 10.77    | ±9.6                   |
| 10076 | CAB | OFDM, 64QAM, 48.0 Mbps, 39.5% DC               | WLAN      | 10.94    | ±9.6                   |
| 10077 | CAB | OFDM, 64QAM, 54.0 Mbps, 38.5% DC               | WLAN      | 11.00    | ±9.6                   |
| 10081 | CAB | RC3, 1xRTT                                     | CDMA2000  | 3.97     | ±9.6                   |
| 10097 | CAC | Ref. 5 HSDPA, QPSK, 5.0 MHz                    | WCDMA     | 3.98     | ±9.6                   |
| 10098 | CAC | Ref. 6 HSUPA, Subset 2, QPSK, 5.0 MHz          | WCDMA     | 3.98     | ±9.6                   |
| 10100 | CAF | 20.0 MHz, QPSK, 100% RB                        | LTE-FDD   | 5.67     | ±9.6                   |
| 10101 | CAF | 20.0 MHz, 16QAM, 100% RB                       | LTE-FDD   | 6.42     | ±9.6                   |
| 10102 | CAF | 20.0 MHz, 64QAM, 100% RB                       | LTE-FDD   | 6.60     | ±9.6                   |
| 10103 | CAH | 20.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB  | LTE-TDD   | 9.29     | ±9.6                   |
| 10104 | CAH | 20.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB | LTE-TDD   | 9.97     | ±9.6                   |
| 10105 | CAH | 20.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB | LTE-TDD   | 10.01    | ±9.6                   |
| 10108 | CAH | 10.0 MHz, QPSK, 100% RB                        | LTE-FDD   | 5.80     | ±9.6                   |
| 10109 | CAH | 10.0 MHz, 16QAM, 100% RB                       | LTE-FDD   | 6.43     | ±9.6                   |
| 10110 | CAH | 5.0 MHz, QPSK, 100% RB                         | LTE-FDD   | 5.75     | ±9.6                   |
| 10111 | CAH | 5.0 MHz, 16QAM, 100% RB                        | LTE-FDD   | 6.44     | ±9.6                   |
| 10112 | CAH | 10.0 MHz, 64QAM, 100% RB                       | LTE-FDD   | 6.59     | ±9.6                   |
| 10113 | CAH | 5.0 MHz, 64QAM, 100% RB                        | LTE-FDD   | 6.62     | ±9.6                   |
| 10114 | CAE | HT40 Greenfield, MCS0 (13.5 Mbps), 99.7% DC    | WLAN      | 8.10     | ±9.6                   |
| 10115 | CAE | HT40 Greenfield, MCS4 (81.0 Mbps), 99.7% DC    | WLAN      | 8.46     | ±9.6                   |
| 10116 | CAE | HT40 Greenfield, MCS7 (135.0 Mbps), 99.7% DC   | WLAN      | 8.15     | ±9.6                   |

| UID   | Rev | Communication System Name                     | Group   | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|-----------------------------------------------|---------|----------|------------------------|
| 10117 | CAE | HT40 Mixed, MCS0 (13.5 Mbps), 99.7% DC        | WLAN    | 8.07     | ±9.6                   |
| 10118 | CAE | HT40 Mixed, MCS4 (81.0 Mbps), 99.7% DC        | WLAN    | 8.59     | ±9.6                   |
| 10119 | CAE | HT40 Mixed, MCS7 (135.0 Mbps), 99.7% DC       | WLAN    | 8.13     | ±9.6                   |
| 10140 | CAF | 15.0 MHz, 16QAM, 100% RB                      | LTE-FDD | 6.49     | ±9.6                   |
| 10141 | CAF | 15.0 MHz, 64QAM, 100% RB                      | LTE-FDD | 6.53     | ±9.6                   |
| 10142 | CAF | 3.0 MHz, QPSK, 100% RB                        | LTE-FDD | 5.73     | ±9.6                   |
| 10143 | CAF | 3.0 MHz, 16QAM, 100% RB                       | LTE-FDD | 6.35     | ±9.6                   |
| 10144 | CAF | 3.0 MHz, 64QAM, 100% RB                       | LTE-FDD | 6.65     | ±9.6                   |
| 10145 | CAG | 1.4 MHz, QPSK, 100% RB                        | LTE-FDD | 5.76     | ±9.6                   |
| 10146 | CAG | 1.4 MHz, 16QAM, 100% RB                       | LTE-FDD | 6.41     | ±9.6                   |
| 10147 | CAG | 1.4 MHz, 64QAM, 100% RB                       | LTE-FDD | 6.72     | ±9.6                   |
| 10149 | CAF | 20.0 MHz, 16QAM, 50% RB                       | LTE-FDD | 6.42     | ±9.6                   |
| 10150 | CAF | 20.0 MHz, 64QAM, 50% RB                       | LTE-FDD | 6.60     | ±9.6                   |
| 10151 | CAH | 20.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB  | LTE-TDD | 9.28     | ±9.6                   |
| 10152 | CAH | 20.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB | LTE-TDD | 9.92     | ±9.6                   |
| 10153 | CAH | 20.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB | LTE-TDD | 10.05    | ±9.6                   |
| 10154 | CAH | 10.0 MHz, QPSK, 50% RB                        | LTE-FDD | 5.75     | ±9.6                   |
| 10155 | CAH | 10.0 MHz, 16QAM, 50% RB                       | LTE-FDD | 6.43     | ±9.6                   |
| 10156 | CAH | 5.0 MHz, QPSK, 50% RB                         | LTE-FDD | 5.79     | ±9.6                   |
| 10157 | CAH | 5.0 MHz, 16QAM, 50% RB                        | LTE-FDD | 6.49     | ±9.6                   |
| 10158 | CAH | 10.0 MHz, 64QAM, 50% RB                       | LTE-FDD | 6.62     | ±9.6                   |
| 10159 | CAH | 5.0 MHz, 64QAM, 50% RB                        | LTE-FDD | 6.58     | ±9.6                   |
| 10160 | CAF | 15.0 MHz, QPSK, 50% RB                        | LTE-FDD | 5.82     | ±9.6                   |
| 10161 | CAF | 15.0 MHz, 16QAM, 50% RB                       | LTE-FDD | 6.43     | ±9.6                   |
| 10162 | CAF | 15.0 MHz, 64QAM, 50% RB                       | LTE-FDD | 6.58     | ±9.6                   |
| 10166 | CAG | 1.4 MHz, QPSK, 50% RB                         | LTE-FDD | 5.46     | ±9.6                   |
| 10167 | CAG | 1.4 MHz, 16QAM, 50% RB                        | LTE-FDD | 6.21     | ±9.6                   |
| 10168 | CAG | 1.4 MHz, 64QAM, 50% RB                        | LTE-FDD | 6.79     | ±9.6                   |
| 10169 | CAF | 20.0 MHz, QPSK, 1 RB                          | LTE-FDD | 5.73     | ±9.6                   |
| 10170 | CAF | 20.0 MHz, 16QAM, 1 RB                         | LTE-FDD | 6.52     | ±9.6                   |
| 10171 | AAF | 20.0 MHz, 64QAM, 1 RB                         | LTE-FDD | 6.49     | ±9.6                   |
| 10172 | CAH | 20.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB    | LTE-TDD | 9.21     | ±9.6                   |
| 10173 | CAH | 20.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB   | LTE-TDD | 9.48     | ±9.6                   |
| 10174 | CAH | 20.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB   | LTE-TDD | 10.25    | ±9.6                   |
| 10175 | CAH | 10.0 MHz, QPSK, 1 RB                          | LTE-FDD | 5.72     | ±9.6                   |
| 10176 | CAH | 10.0 MHz, 16QAM, 1 RB                         | LTE-FDD | 6.52     | ±9.6                   |
| 10177 | CAJ | 5.0 MHz, QPSK, 1 RB                           | LTE-FDD | 5.73     | ±9.6                   |
| 10178 | CAH | 5.0 MHz, 16QAM, 1 RB                          | LTE-FDD | 6.52     | ±9.6                   |
| 10179 | CAH | 10.0 MHz, 64QAM, 1 RB                         | LTE-FDD | 6.50     | ±9.6                   |
| 10180 | CAH | 5.0 MHz, 64QAM, 1 RB                          | LTE-FDD | 6.50     | ±9.6                   |
| 10181 | CAF | 15.0 MHz, QPSK, 1 RB                          | LTE-FDD | 5.72     | ±9.6                   |
| 10182 | CAF | 15.0 MHz, 16QAM, 1 RB                         | LTE-FDD | 6.52     | ±9.6                   |
| 10183 | AAE | 15.0 MHz, 64QAM, 1 RB                         | LTE-FDD | 6.50     | ±9.6                   |
| 10184 | CAF | 3.0 MHz, QPSK, 1 RB                           | LTE-FDD | 5.73     | ±9.6                   |
| 10185 | CAF | 3.0 MHz, 16QAM, 1 RB                          | LTE-FDD | 6.51     | ±9.6                   |
| 10186 | AAF | 3.0 MHz, 64QAM, 1 RB                          | LTE-FDD | 6.50     | ±9.6                   |
| 10187 | CAG | 1.4 MHz, QPSK, 1 RB                           | LTE-FDD | 5.73     | ±9.6                   |
| 10188 | CAG | 1.4 MHz, 16QAM, 1 RB                          | LTE-FDD | 6.52     | ±9.6                   |
| 10189 | AAG | 1.4 MHz, 64QAM, 1 RB                          | LTE-FDD | 6.50     | ±9.6                   |
| 10193 | CAE | HT20 Greenfield, MCS0 (6.5 Mbps), 99.4% DC    | WLAN    | 8.09     | ±9.6                   |
| 10194 | CAE | HT20 Greenfield, MCS4 (39.0 Mbps), 99.5% DC   | WLAN    | 8.12     | ±9.6                   |
| 10195 | CAE | HT20 Greenfield, MCS7 (65.0 Mbps), 99.5% DC   | WLAN    | 8.21     | ±9.6                   |
| 10196 | CAE | HT20 Mixed, MCS0 (6.5 Mbps), 99.4% DC         | WLAN    | 8.10     | ±9.6                   |
| 10197 | CAE | HT20 Mixed, MCS4 (39.0 Mbps), 99.5% DC        | WLAN    | 8.13     | ±9.6                   |
| 10198 | CAE | HT20 Mixed, MCS7 (65.0 Mbps), 99.5% DC        | WLAN    | 8.27     | ±9.6                   |
| 10219 | CAE | HT20 Mixed, MCS0 (7.2 Mbps), 99.3% DC         | WLAN    | 8.03     | ±9.6                   |
| 10220 | CAE | HT20 Mixed, MCS4 (43.3 Mbps), 99.4% DC        | WLAN    | 8.13     | ±9.6                   |
| 10221 | CAE | HT20 Mixed, MCS7 (72.2 Mbps), 99.4% DC        | WLAN    | 8.27     | ±9.6                   |
| 10222 | CAE | HT40 Mixed, MCS0 (15.0 Mbps), 99.7% DC        | WLAN    | 8.06     | ±9.6                   |
| 10223 | CAE | HT40 Mixed, MCS4 (90.0 Mbps), 99.7% DC        | WLAN    | 8.48     | ±9.6                   |
| 10224 | CAE | HT40 Mixed, MCS7 (150.0 Mbps), 99.7% DC       | WLAN    | 8.08     | ±9.6                   |
| 10225 | CAC | Ref. 7 HSPA+, 16QAM, 5.0 MHz                  | WCDMA   | 5.97     | ±9.6                   |
| 10226 | CAC | 1.4 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB    | LTE-TDD | 9.49     | ±9.6                   |
| 10227 | CAC | 1.4 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB    | LTE-TDD | 10.26    | ±9.6                   |
| 10228 | CAC | 1.4 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB     | LTE-TDD | 9.22     | ±9.6                   |
| 10229 | CAE | 3.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB    | LTE-TDD | 9.48     | ±9.6                   |

| UID   | Rev | Communication System Name                        | Group    | PAR (dB) | Unc <sup>F</sup> k = 2 |
|-------|-----|--------------------------------------------------|----------|----------|------------------------|
| 10230 | CAE | 3.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB       | LTE-TDD  | 10.25    | ±9.6                   |
| 10231 | CAE | 3.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB        | LTE-TDD  | 9.19     | ±9.6                   |
| 10232 | CAH | 5.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB       | LTE-TDD  | 9.48     | ±9.6                   |
| 10233 | CAH | 5.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB       | LTE-TDD  | 10.25    | ±9.6                   |
| 10234 | CAH | 5.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB        | LTE-TDD  | 9.21     | ±9.6                   |
| 10235 | CAH | 10.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB      | LTE-TDD  | 9.48     | ±9.6                   |
| 10236 | CAH | 10.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB      | LTE-TDD  | 10.25    | ±9.6                   |
| 10237 | CAH | 10.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB       | LTE-TDD  | 9.21     | ±9.6                   |
| 10238 | CAG | 15.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 1 RB      | LTE-TDD  | 9.48     | ±9.6                   |
| 10239 | CAG | 15.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 1 RB      | LTE-TDD  | 10.25    | ±9.6                   |
| 10240 | CAG | 15.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 1 RB       | LTE-TDD  | 9.21     | ±9.6                   |
| 10241 | CAC | 1.4 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 9.82     | ±9.6                   |
| 10242 | CAC | 1.4 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 9.86     | ±9.6                   |
| 10243 | CAC | 1.4 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB      | LTE-TDD  | 9.46     | ±9.6                   |
| 10244 | CAE | 3.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 10.06    | ±9.6                   |
| 10245 | CAE | 3.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 10.06    | ±9.6                   |
| 10246 | CAE | 3.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB      | LTE-TDD  | 9.30     | ±9.6                   |
| 10247 | CAH | 5.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 9.91     | ±9.6                   |
| 10248 | CAH | 5.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 10.09    | ±9.6                   |
| 10249 | CAH | 5.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB      | LTE-TDD  | 9.29     | ±9.6                   |
| 10250 | CAH | 10.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB    | LTE-TDD  | 9.81     | ±9.6                   |
| 10251 | CAH | 10.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB    | LTE-TDD  | 10.17    | ±9.6                   |
| 10252 | CAH | 10.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 9.24     | ±9.6                   |
| 10253 | CAG | 15.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 50% RB    | LTE-TDD  | 9.90     | ±9.6                   |
| 10254 | CAG | 15.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 50% RB    | LTE-TDD  | 10.14    | ±9.6                   |
| 10255 | CAG | 15.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 50% RB     | LTE-TDD  | 9.20     | ±9.6                   |
| 10256 | CAC | 1.4 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.96     | ±9.6                   |
| 10257 | CAC | 1.4 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 10.08    | ±9.6                   |
| 10258 | CAC | 1.4 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB     | LTE-TDD  | 9.34     | ±9.6                   |
| 10259 | CAE | 3.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.98     | ±9.6                   |
| 10260 | CAE | 3.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.97     | ±9.6                   |
| 10261 | CAE | 3.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB     | LTE-TDD  | 9.24     | ±9.6                   |
| 10262 | CAH | 5.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.83     | ±9.6                   |
| 10263 | CAH | 5.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 10.16    | ±9.6                   |
| 10264 | CAH | 5.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB     | LTE-TDD  | 9.23     | ±9.6                   |
| 10265 | CAH | 10.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB   | LTE-TDD  | 9.92     | ±9.6                   |
| 10266 | CAH | 10.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB   | LTE-TDD  | 10.07    | ±9.6                   |
| 10267 | CAH | 10.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.30     | ±9.6                   |
| 10268 | CAG | 15.0 MHz, 16QAM, UL/DL CFG: 1, SSC: 4, 100% RB   | LTE-TDD  | 10.06    | ±9.6                   |
| 10269 | CAG | 15.0 MHz, 64QAM, UL/DL CFG: 1, SSC: 4, 100% RB   | LTE-TDD  | 10.13    | ±9.6                   |
| 10270 | CAG | 15.0 MHz, QPSK, UL/DL CFG: 1, SSC: 4, 100% RB    | LTE-TDD  | 9.58     | ±9.6                   |
| 10274 | CAC | Rel. 6 HSUPA Subset 2, beta_d 0, QPSK, 5.0 MHz   | WCDMA    | 4.87     | ±9.6                   |
| 10275 | CAC | Rel. 6 HSUPA Subset 2, beta_d 15, QPSK, 5.0 MHz  | WCDMA    | 3.96     | ±9.6                   |
| 10290 | AAB | RC1, SO55, Full frame rate, 1xRTT                | CDMA2000 | 3.91     | ±9.6                   |
| 10291 | AAB | RC3, SO55, Full frame rate, 1xRTT                | CDMA2000 | 3.46     | ±9.6                   |
| 10292 | AAB | RC3, SO32, Full frame rate, SCH0 disabled, 1xRTT | CDMA2000 | 3.39     | ±9.6                   |
| 10293 | AAB | RC3, SO3, Full frame rate, 1xRTT                 | CDMA2000 | 3.50     | ±9.6                   |
| 10295 | AAB | RC3, SO3, 1/8 frame rate, 1xRTT                  | CDMA2000 | 12.49    | ±9.6                   |
| 10297 | AAE | 20.0 MHz, QPSK, 50% RB                           | LTE-FDD  | 5.81     | ±9.6                   |
| 10298 | AAE | 3.0 MHz, QPSK, 50% RB                            | LTE-FDD  | 5.72     | ±9.6                   |
| 10299 | AAE | 3.0 MHz, 16QAM, 50% RB                           | LTE-FDD  | 6.39     | ±9.6                   |
| 10300 | AAE | 3.0 MHz, 64QAM, 50% RB                           | LTE-FDD  | 6.60     | ±9.6                   |
| 10301 | AAA | PUSC, 29:18, QPSK, 5.0 ms, 18 TRAF SYM           | WiMAX    | 12.03    | ±9.6                   |
| 10302 | AAA | PUSC, 29:18, QPSK, 5.0 ms, 15 TRAF SYM           | WiMAX    | 12.57    | ±9.6                   |
| 10303 | AAA | PUSC, 31:15, 64QAM, 5.0 ms, 15 TRAF SYM          | WiMAX    | 12.52    | ±9.6                   |
| 10304 | AAA | PUSC, 29:18, 64QAM, 5.0 ms, 18 TRAF SYM          | WiMAX    | 11.86    | ±9.6                   |
| 10305 | AAA | PUSC, 31:15, 64QAM, 10.0 ms, 15 TRAF SYM         | WiMAX    | 15.24    | ±9.6                   |
| 10306 | AAA | PUSC, 29:18, 64QAM, 10.0 ms, 18 TRAF SYM         | WiMAX    | 14.67    | ±9.6                   |
| 10307 | AAA | PUSC, 29:18, QPSK, 10.0 ms, 18 TRAF SYM          | WiMAX    | 14.49    | ±9.6                   |
| 10308 | AAA | PUSC, 29:18, 16QAM, 10.0 ms, 18 TRAF SYM         | WiMAX    | 14.46    | ±9.6                   |
| 10309 | AAA | AMC 2x3, 29:18, 16QAM, 10.0 ms, 18 TRAF SYM      | WiMAX    | 14.58    | ±9.6                   |
| 10310 | AAA | AMC 2x3, 29:18, QPSK, 10.0 ms, 18 TRAF SYM       | WiMAX    | 14.57    | ±9.6                   |
| 10311 | AAE | 15.0 MHz, QPSK, 100% RB                          | LTE-FDD  | 6.06     | ±9.6                   |
| 10315 | AAB | DSSS, DBPSK, 1.0 Mbps, 95.0% DC                  | WLAN     | 1.71     | ±9.6                   |
| 10316 | AAB | OFDM, BPSK, 6.0 Mbps, 95.9% DC                   | WLAN     | 8.36     | ±9.6                   |
| 10317 | AAE | OFDM, BPSK, 6.0 Mbps, 95.9% DC                   | WLAN     | 8.36     | ±9.6                   |

| UID   | Rev | Communication System Name                                   | Group    | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|-------------------------------------------------------------|----------|----------|------------------------|
| 10352 | AAA | Pulse (D=10%, T=5 ms)                                       | Generic  | 10.00    | ±9.6                   |
| 10353 | AAA | Pulse (D=20%, T=5 ms)                                       | Generic  | 6.99     | ±9.6                   |
| 10354 | AAA | Pulse (D=40%, T=5 ms)                                       | Generic  | 3.98     | ±9.6                   |
| 10355 | AAA | Pulse (D=60%, T=5 ms)                                       | Generic  | 2.22     | ±9.6                   |
| 10356 | AAA | Pulse (D=80%, T=5 ms)                                       | Generic  | 0.97     | ±9.6                   |
| 10387 | AAA | Random (BW=1 MHz, MOD=QPSK)                                 | Generic  | 5.10     | ±9.6                   |
| 10388 | AAA | Random (BW=10 MHz, MOD=QPSK)                                | Generic  | 5.22     | ±9.6                   |
| 10398 | AAA | Random (BW=100 kHz, MOD=64QAM)                              | Generic  | 6.27     | ±9.6                   |
| 10399 | AAA | Random (BW=40 MHz, MOD=64QAM)                               | Generic  | 6.27     | ±9.6                   |
| 10400 | AAF | VHT20, MCS5 (52.0 Mbps), 99.0% DC                           | WLAN     | 8.37     | ±9.6                   |
| 10401 | AAF | VHT40, MCS5 (108.0 Mbps), 96.7% DC                          | WLAN     | 8.60     | ±9.6                   |
| 10402 | AAF | VHT80, MCS5 (234.0 Mbps), 99.0% DC                          | WLAN     | 8.53     | ±9.6                   |
| 10403 | AAB | Rev. 0, 1xEV-DO                                             | CDMA2000 | 3.76     | ±9.6                   |
| 10404 | AAB | Rev. A, 1xEV-DO                                             | CDMA2000 | 3.77     | ±9.6                   |
| 10406 | AAB | RC3, SC32, Full frame rate, SCH0 enabled, 1xRTT             | CDMA2000 | 5.22     | ±9.6                   |
| 10410 | AAH | 10.0 MHz, QPSK, UL/DL CFG: 0, SSC: 4, 1 RB                  | LTE-TDD  | 7.82     | ±9.6                   |
| 10414 | AAA | Random (BW=40 MHz, HIGH PAR)                                | Generic  | 8.54     | ±9.6                   |
| 10415 | AAA | DSSS, DBPSK, 1.0 Mbps, 99.9% DC                             | WLAN     | 1.54     | ±9.6                   |
| 10416 | AAA | OFDM, BPSK, 6.0 Mbps, 99.9% DC                              | WLAN     | 8.23     | ±9.6                   |
| 10417 | AAD | OFDM, BPSK, 6.0 Mbps, 99.9% DC                              | WLAN     | 8.23     | ±9.6                   |
| 10418 | AAA | OFDM (LTF), BPSK, 6.0 Mbps, 99.8% DC                        | WLAN     | 8.14     | ±9.6                   |
| 10419 | AAA | OFDM (STF), BPSK, 6.0 Mbps, 99.8% DC                        | WLAN     | 8.19     | ±9.6                   |
| 10422 | AAD | HT20 Greenfield, MCS0 (7.2 Mbps), 99.3% DC                  | WLAN     | 8.32     | ±9.6                   |
| 10423 | AAD | HT20 Greenfield, MCS4 (43.3 Mbps), 99.3% DC                 | WLAN     | 8.47     | ±9.6                   |
| 10424 | AAD | HT20 Greenfield, MCS7 (72.2 Mbps), 99.3% DC                 | WLAN     | 8.40     | ±9.6                   |
| 10425 | AAD | HT40 Greenfield, MCS0 (15.0 Mbps), 99.2% DC                 | WLAN     | 8.41     | ±9.6                   |
| 10426 | AAD | HT40 Greenfield, MCS4 (90.0 Mbps), 99.2% DC                 | WLAN     | 8.45     | ±9.6                   |
| 10427 | AAD | HT40 Greenfield, MCS7 (150.0 Mbps), 99.2% DC                | WLAN     | 8.41     | ±9.6                   |
| 10430 | AAE | 5.0 MHz, 64-QAM, 100% RB                                    | LTE-FDD  | 8.28     | ±9.6                   |
| 10431 | AAE | 10.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 8.38     | ±9.6                   |
| 10432 | AAD | 15.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 8.34     | ±9.6                   |
| 10433 | AAD | 20.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 8.34     | ±9.6                   |
| 10434 | AAB | BS Test Model 1, 64 DPCH, 64QAM, 5.0 MHz (DL)               | WCDMA    | 8.60     | ±9.6                   |
| 10435 | AAG | 20.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 7.82     | ±9.6                   |
| 10447 | AAE | 5.0 MHz, 64-QAM, 100% RB                                    | LTE-FDD  | 7.56     | ±9.6                   |
| 10448 | AAE | 10.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 7.53     | ±9.6                   |
| 10449 | AAD | 15.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 7.51     | ±9.6                   |
| 10450 | AAD | 20.0 MHz, 64-QAM, 100% RB                                   | LTE-FDD  | 7.48     | ±9.6                   |
| 10451 | AAB | BS Test Model 1, 64 DPCH, Clipping 44%, 64QAM, 5.0 MHz (DL) | WCDMA    | 7.59     | ±9.6                   |
| 10456 | AAD | VHT160, MCS5 (58.5 Mbps), 99.0% DC                          | WLAN     | 8.63     | ±9.6                   |
| 10457 | AAB | Rel. 5 DC-HSDPA, QPSK, 10.0 MHz                             | WCDMA    | 8.62     | ±9.6                   |
| 10458 | AAA | Rev. B, 2 carriers, 1xEV-DO                                 | CDMA2000 | 6.55     | ±9.6                   |
| 10459 | AAA | Rev. B, 3 carriers, 1xEV-DO                                 | CDMA2000 | 8.25     | ±9.6                   |
| 10460 | AAB | Rel. 99, AMR, QPSK, 5.0 MHz                                 | WCDMA    | 2.39     | ±9.6                   |
| 10461 | AAC | 1.4 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                   | LTE-TDD  | 7.82     | ±9.6                   |
| 10462 | AAC | 1.4 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.30     | ±9.6                   |
| 10463 | AAC | 1.4 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.56     | ±9.6                   |
| 10464 | AAD | 3.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                   | LTE-TDD  | 7.82     | ±9.6                   |
| 10465 | AAD | 3.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.32     | ±9.6                   |
| 10466 | AAD | 3.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.57     | ±9.6                   |
| 10467 | AAG | 5.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                   | LTE-TDD  | 7.82     | ±9.6                   |
| 10468 | AAG | 5.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.32     | ±9.6                   |
| 10469 | AAG | 5.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 8.56     | ±9.6                   |
| 10470 | AAG | 10.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 7.82     | ±9.6                   |
| 10471 | AAG | 10.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.32     | ±9.6                   |
| 10472 | AAG | 10.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.57     | ±9.6                   |
| 10473 | AAF | 15.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 1 RB                  | LTE-TDD  | 7.82     | ±9.6                   |
| 10474 | AAF | 15.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.32     | ±9.6                   |
| 10475 | AAF | 15.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.57     | ±9.6                   |
| 10477 | AAG | 20.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.32     | ±9.6                   |
| 10478 | AAG | 20.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 1 RB                 | LTE-TDD  | 8.57     | ±9.6                   |
| 10479 | AAC | 1.4 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB                 | LTE-TDD  | 7.74     | ±9.6                   |
| 10480 | AAC | 1.4 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB                | LTE-TDD  | 8.18     | ±9.6                   |
| 10481 | AAC | 1.4 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB                | LTE-TDD  | 8.45     | ±9.6                   |
| 10482 | AAD | 3.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB                 | LTE-TDD  | 7.71     | ±9.6                   |
| 10483 | AAD | 3.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB                | LTE-TDD  | 8.39     | ±9.6                   |

| UID   | Rev | Communication System Name                      | Group   | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|------------------------------------------------|---------|----------|------------------------|
| 10484 | AAD | 3.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 8.47     | ±9.6                   |
| 10485 | AAG | 5.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB    | LTE-TDD | 7.59     | ±9.6                   |
| 10486 | AAG | 5.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 8.38     | ±9.6                   |
| 10487 | AAG | 5.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 8.60     | ±9.6                   |
| 10488 | AAG | 10.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 7.70     | ±9.6                   |
| 10489 | AAG | 10.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.31     | ±9.6                   |
| 10490 | AAG | 10.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.54     | ±9.6                   |
| 10491 | AAF | 15.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 7.74     | ±9.6                   |
| 10492 | AAF | 15.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.41     | ±9.6                   |
| 10493 | AAF | 15.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.55     | ±9.6                   |
| 10494 | AAG | 20.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 50% RB   | LTE-TDD | 7.74     | ±9.6                   |
| 10495 | AAG | 20.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.37     | ±9.6                   |
| 10496 | AAG | 20.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 50% RB  | LTE-TDD | 8.54     | ±9.6                   |
| 10497 | AAC | 1.4 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB   | LTE-TDD | 7.67     | ±9.6                   |
| 10498 | AAC | 1.4 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.40     | ±9.6                   |
| 10499 | AAC | 1.4 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.68     | ±9.6                   |
| 10500 | AAD | 3.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB   | LTE-TDD | 7.67     | ±9.6                   |
| 10501 | AAD | 3.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.44     | ±9.6                   |
| 10502 | AAD | 3.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.52     | ±9.6                   |
| 10503 | AAG | 5.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB   | LTE-TDD | 7.72     | ±9.6                   |
| 10504 | AAG | 5.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.31     | ±9.6                   |
| 10505 | AAG | 5.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 8.54     | ±9.6                   |
| 10506 | AAG | 10.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 7.74     | ±9.6                   |
| 10507 | AAG | 10.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.36     | ±9.6                   |
| 10508 | AAG | 10.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.55     | ±9.6                   |
| 10509 | AAF | 15.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 7.99     | ±9.6                   |
| 10510 | AAF | 15.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.49     | ±9.6                   |
| 10511 | AAF | 15.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.51     | ±9.6                   |
| 10512 | AAG | 20.0 MHz, QPSK, UL/DL CFG: 0, SSC: 7, 100% RB  | LTE-TDD | 7.74     | ±9.6                   |
| 10513 | AAG | 20.0 MHz, 16QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.42     | ±9.6                   |
| 10514 | AAG | 20.0 MHz, 64QAM, UL/DL CFG: 0, SSC: 7, 100% RB | LTE-TDD | 8.45     | ±9.6                   |
| 10515 | AAA | DSSS, DQPSK, 2.0 Mbps, 99.0% DC                | WLAN    | 1.58     | ±9.6                   |
| 10516 | AAA | HR-DSSS, DQPSK, 5.5 Mbps, 99.2% DC             | WLAN    | 1.57     | ±9.6                   |
| 10517 | AAA | HR-DSSS, DQPSK, 11.0 Mbps, 99.0% DC            | WLAN    | 1.58     | ±9.6                   |
| 10518 | AAD | OFDM, BPSK, 9.0 Mbps, 98.9% DC                 | WLAN    | 8.23     | ±9.6                   |
| 10519 | AAD | OFDM, QPSK, 12.0 Mbps, 99.0% DC                | WLAN    | 8.39     | ±9.6                   |
| 10520 | AAD | OFDM, QPSK, 18.0 Mbps, 99.0% DC                | WLAN    | 8.12     | ±9.6                   |
| 10521 | AAD | OFDM, 16QAM, 24.0 Mbps, 99.0% DC               | WLAN    | 7.97     | ±9.6                   |
| 10522 | AAD | OFDM, 16QAM, 36.0 Mbps, 99.0% DC               | WLAN    | 8.45     | ±9.6                   |
| 10523 | AAD | OFDM, 64QAM, 48.0 Mbps, 99.0% DC               | WLAN    | 8.08     | ±9.6                   |
| 10524 | AAD | OFDM, 64QAM, 54.0 Mbps, 99.0% DC               | WLAN    | 8.27     | ±9.6                   |
| 10525 | AAD | VHT20, MCS0 (6.5 Mbps), 98.9% DC               | WLAN    | 8.36     | ±9.6                   |
| 10526 | AAD | VHT20, MCS1 (13.0 Mbps), 99.0% DC              | WLAN    | 8.42     | ±9.6                   |
| 10527 | AAD | VHT20, MCS2 (19.5 Mbps), 99.0% DC              | WLAN    | 8.21     | ±9.6                   |
| 10528 | AAD | VHT20, MCS3 (26.0 Mbps), 99.0% DC              | WLAN    | 8.36     | ±9.6                   |
| 10529 | AAD | VHT20, MCS4 (39.0 Mbps), 99.0% DC              | WLAN    | 8.36     | ±9.6                   |
| 10531 | AAD | VHT20, MCS6 (58.5 Mbps), 99.0% DC              | WLAN    | 8.43     | ±9.6                   |
| 10532 | AAD | VHT20, MCS7 (65.0 Mbps), 99.0% DC              | WLAN    | 8.29     | ±9.6                   |
| 10533 | AAD | VHT20, MCS8 (78.0 Mbps), 99.0% DC              | WLAN    | 8.38     | ±9.6                   |
| 10534 | AAD | VHT40, MCS0 (13.5 Mbps), 98.9% DC              | WLAN    | 8.45     | ±9.6                   |
| 10535 | AAD | VHT40, MCS1 (27.0 Mbps), 98.8% DC              | WLAN    | 8.45     | ±9.6                   |
| 10536 | AAD | VHT40, MCS2 (40.5 Mbps), 98.8% DC              | WLAN    | 8.32     | ±9.6                   |
| 10537 | AAD | VHT40, MCS3 (54.0 Mbps), 98.7% DC              | WLAN    | 8.44     | ±9.6                   |
| 10538 | AAD | VHT40, MCS4 (81.0 Mbps), 98.5% DC              | WLAN    | 8.54     | ±9.6                   |
| 10540 | AAD | VHT40, MCS6 (121.5 Mbps), 98.3% DC             | WLAN    | 8.39     | ±9.6                   |
| 10541 | AAD | VHT40, MCS7 (135.0 Mbps), 98.3% DC             | WLAN    | 8.46     | ±9.6                   |
| 10542 | AAD | VHT40, MCS8 (162.0 Mbps), 98.1% DC             | WLAN    | 8.65     | ±9.6                   |
| 10543 | AAD | VHT40, MCS9 (180.0 Mbps), 98.0% DC             | WLAN    | 8.65     | ±9.6                   |
| 10544 | AAD | VHT80, MCS0 (29.3 Mbps), 99.0% DC              | WLAN    | 8.47     | ±9.6                   |
| 10545 | AAD | VHT80, MCS1 (58.5 Mbps), 99.0% DC              | WLAN    | 8.55     | ±9.6                   |
| 10546 | AAD | VHT80, MCS2 (87.8 Mbps), 99.0% DC              | WLAN    | 8.35     | ±9.6                   |
| 10547 | AAD | VHT80, MCS3 (117.0 Mbps), 99.0% DC             | WLAN    | 8.49     | ±9.6                   |
| 10548 | AAD | VHT80, MCS4 (175.5 Mbps), 99.0% DC             | WLAN    | 8.37     | ±9.6                   |
| 10550 | AAD | VHT80, MCS6 (263.3 Mbps), 99.0% DC             | WLAN    | 8.38     | ±9.6                   |
| 10551 | AAD | VHT80, MCS7 (292.5 Mbps), 99.0% DC             | WLAN    | 8.50     | ±9.6                   |
| 10552 | AAD | VHT80, MCS8 (351.0 Mbps), 99.0% DC             | WLAN    | 8.42     | ±9.6                   |

| UID   | Rev | Communication System Name               | Group | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|-----------------------------------------|-------|----------|------------------------|
| 10553 | AAE | VHT80, MCS9 (390.0 Mbps), 99.0% DC      | WLAN  | 8.45     | ±9.6                   |
| 10554 | AAE | VHT160, MCS0 (58.5 Mbps), 99.0% DC      | WLAN  | 8.48     | ±9.6                   |
| 10555 | AAE | VHT160, MCS1 (117.0 Mbps), 99.0% DC     | WLAN  | 8.47     | ±9.6                   |
| 10556 | AAE | VHT160, MCS2 (175.5 Mbps), 99.0% DC     | WLAN  | 8.50     | ±9.6                   |
| 10557 | AAE | VHT160, MCS3 (234.0 Mbps), 99.0% DC     | WLAN  | 8.52     | ±9.6                   |
| 10558 | AAE | VHT160, MCS4 (351.0 Mbps), 99.0% DC     | WLAN  | 8.81     | ±9.6                   |
| 10560 | AAE | VHT160, MCS6 (526.5 Mbps), 99.0% DC     | WLAN  | 8.73     | ±9.6                   |
| 10561 | AAE | VHT160, MCS7 (585.0 Mbps), 99.0% DC     | WLAN  | 8.56     | ±9.6                   |
| 10562 | AAE | VHT160, MCS8 (702.0 Mbps), 99.0% DC     | WLAN  | 8.69     | ±9.6                   |
| 10563 | AAE | VHT160, MCS9 (780.0 Mbps), 99.0% DC     | WLAN  | 8.77     | ±9.6                   |
| 10564 | AAA | OFDM, BPSK, 9.0 Mbps, 98.9% DC          | WLAN  | 8.25     | ±9.6                   |
| 10565 | AAA | OFDM, QPSK, 12.0 Mbps, 99.0% DC         | WLAN  | 8.45     | ±9.6                   |
| 10566 | AAA | OFDM, QPSK, 18.0 Mbps, 99.0% DC         | WLAN  | 8.13     | ±9.6                   |
| 10567 | AAA | OFDM, 16QAM, 24.0 Mbps, 99.0% DC        | WLAN  | 8.00     | ±9.6                   |
| 10568 | AAA | OFDM, 16QAM, 36.0 Mbps, 99.0% DC        | WLAN  | 8.37     | ±9.6                   |
| 10569 | AAA | OFDM, 64QAM, 48.0 Mbps, 99.0% DC        | WLAN  | 8.10     | ±9.6                   |
| 10570 | AAA | OFDM, 64QAM, 54.0 Mbps, 99.0% DC        | WLAN  | 8.30     | ±9.6                   |
| 10571 | AAA | DSSS, DQPSK, 1.0 Mbps, 90.0% DC         | WLAN  | 1.99     | ±9.6                   |
| 10572 | AAA | DSSS, DQPSK, 2.0 Mbps, 90.0% DC         | WLAN  | 1.99     | ±9.6                   |
| 10573 | AAA | HR-DSSS, DQPSK, 5.5 Mbps, 90.1% DC      | WLAN  | 1.98     | ±9.6                   |
| 10574 | AAA | HR-DSSS, DQPSK, 11.0 Mbps, 90.3% DC     | WLAN  | 1.98     | ±9.6                   |
| 10575 | AAA | OFDM, BPSK, 6.0 Mbps, 89.9% DC          | WLAN  | 8.59     | ±9.6                   |
| 10576 | AAA | OFDM, BPSK, 9.0 Mbps, 89.9% DC          | WLAN  | 8.60     | ±9.6                   |
| 10577 | AAA | OFDM, QPSK, 12.0 Mbps, 90.0% DC         | WLAN  | 8.70     | ±9.6                   |
| 10578 | AAA | OFDM, QPSK, 18.0 Mbps, 90.0% DC         | WLAN  | 8.49     | ±9.6                   |
| 10579 | AAA | OFDM, 16QAM, 24.0 Mbps, 90.0% DC        | WLAN  | 8.36     | ±9.6                   |
| 10580 | AAA | OFDM, 16QAM, 36.0 Mbps, 90.0% DC        | WLAN  | 8.76     | ±9.6                   |
| 10581 | AAA | OFDM, 64QAM, 48.0 Mbps, 90.0% DC        | WLAN  | 8.35     | ±9.6                   |
| 10582 | AAA | OFDM, 64QAM, 54.0 Mbps, 90.0% DC        | WLAN  | 8.67     | ±9.6                   |
| 10583 | AAD | OFDM, BPSK, 6.0 Mbps, 89.9% DC          | WLAN  | 8.59     | ±9.6                   |
| 10584 | AAD | OFDM, BPSK, 9.0 Mbps, 89.9% DC          | WLAN  | 8.60     | ±9.6                   |
| 10585 | AAD | OFDM, QPSK, 12.0 Mbps, 90.0% DC         | WLAN  | 8.70     | ±9.6                   |
| 10586 | AAD | OFDM, QPSK, 18.0 Mbps, 90.0% DC         | WLAN  | 8.49     | ±9.6                   |
| 10587 | AAD | OFDM, 16QAM, 24.0 Mbps, 90.0% DC        | WLAN  | 8.36     | ±9.6                   |
| 10588 | AAD | OFDM, 16QAM, 36.0 Mbps, 90.0% DC        | WLAN  | 8.76     | ±9.6                   |
| 10589 | AAD | OFDM, 64QAM, 48.0 Mbps, 90.0% DC        | WLAN  | 8.35     | ±9.6                   |
| 10590 | AAD | OFDM, 64QAM, 54.0 Mbps, 90.0% DC        | WLAN  | 8.67     | ±9.6                   |
| 10591 | AAD | HT20 Mixed, MCS0 (6.5 Mbps), 89.9% DC   | WLAN  | 8.63     | ±9.6                   |
| 10592 | AAD | HT20 Mixed, MCS1 (13.0 Mbps), 90.0% DC  | WLAN  | 8.79     | ±9.6                   |
| 10593 | AAD | HT20 Mixed, MCS2 (19.5 Mbps), 90.0% DC  | WLAN  | 8.64     | ±9.6                   |
| 10594 | AAD | HT20 Mixed, MCS3 (26.0 Mbps), 90.0% DC  | WLAN  | 8.74     | ±9.6                   |
| 10595 | AAD | HT20 Mixed, MCS4 (39.0 Mbps), 90.0% DC  | WLAN  | 8.74     | ±9.6                   |
| 10596 | AAD | HT20 Mixed, MCS5 (52.0 Mbps), 90.0% DC  | WLAN  | 8.71     | ±9.6                   |
| 10597 | AAD | HT20 Mixed, MCS6 (58.5 Mbps), 90.0% DC  | WLAN  | 8.72     | ±9.6                   |
| 10598 | AAD | HT20 Mixed, MCS7 (65.0 Mbps), 90.0% DC  | WLAN  | 8.50     | ±9.6                   |
| 10599 | AAD | HT40 Mixed, MCS0 (13.5 Mbps), 89.9% DC  | WLAN  | 8.79     | ±9.6                   |
| 10600 | AAD | HT40 Mixed, MCS1 (27.0 Mbps), 89.7% DC  | WLAN  | 8.88     | ±9.6                   |
| 10601 | AAD | HT40 Mixed, MCS2 (40.5 Mbps), 89.6% DC  | WLAN  | 8.82     | ±9.6                   |
| 10602 | AAD | HT40 Mixed, MCS3 (54.0 Mbps), 89.4% DC  | WLAN  | 8.94     | ±9.6                   |
| 10603 | AAD | HT40 Mixed, MCS4 (81.0 Mbps), 89.2% DC  | WLAN  | 9.03     | ±9.6                   |
| 10604 | AAD | HT40 Mixed, MCS5 (108.0 Mbps), 88.9% DC | WLAN  | 8.76     | ±9.6                   |
| 10605 | AAD | HT40 Mixed, MCS6 (121.5 Mbps), 88.8% DC | WLAN  | 8.97     | ±9.6                   |
| 10606 | AAD | HT40 Mixed, MCS7 (135.0 Mbps), 88.7% DC | WLAN  | 8.82     | ±9.6                   |
| 10607 | AAD | VHT20, MCS0 (6.5 Mbps), 89.9% DC        | WLAN  | 8.64     | ±9.6                   |
| 10608 | AAD | VHT20, MCS1 (13.0 Mbps), 90.0% DC       | WLAN  | 8.77     | ±9.6                   |
| 10609 | AAD | VHT20, MCS2 (19.5 Mbps), 90.0% DC       | WLAN  | 8.57     | ±9.6                   |
| 10610 | AAD | VHT20, MCS3 (26.0 Mbps), 90.0% DC       | WLAN  | 8.78     | ±9.6                   |
| 10611 | AAD | VHT20, MCS4 (39.0 Mbps), 90.0% DC       | WLAN  | 8.70     | ±9.6                   |
| 10612 | AAD | VHT20, MCS5 (52.0 Mbps), 90.0% DC       | WLAN  | 8.77     | ±9.6                   |
| 10613 | AAD | VHT20, MCS6 (58.5 Mbps), 90.0% DC       | WLAN  | 8.94     | ±9.6                   |
| 10614 | AAD | VHT20, MCS7 (65.0 Mbps), 90.0% DC       | WLAN  | 8.59     | ±9.6                   |
| 10615 | AAD | VHT20, MCS8 (78.0 Mbps), 90.0% DC       | WLAN  | 8.82     | ±9.6                   |
| 10616 | AAD | VHT40, MCS0 (13.5 Mbps), 89.9% DC       | WLAN  | 8.82     | ±9.6                   |
| 10617 | AAD | VHT40, MCS1 (27.0 Mbps), 89.7% DC       | WLAN  | 8.81     | ±9.6                   |
| 10618 | AAD | VHT40, MCS2 (40.5 Mbps), 89.6% DC       | WLAN  | 8.58     | ±9.6                   |
| 10619 | AAD | VHT40, MCS3 (54.0 Mbps), 89.4% DC       | WLAN  | 8.86     | ±9.6                   |

| UID   | Rev | Communication System Name                  | Group     | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|--------------------------------------------|-----------|----------|------------------------|
| 10620 | AAD | VHT40, MCS4 (81.0 Mbps), 89.2% DC          | WLAN      | 8.87     | ±9.6                   |
| 10621 | AAD | VHT40, MCS5 (108.0 Mbps), 88.9% DC         | WLAN      | 8.77     | ±9.6                   |
| 10622 | AAD | VHT40, MCS6 (121.5 Mbps), 88.8% DC         | WLAN      | 8.66     | ±9.6                   |
| 10623 | AAD | VHT40, MCS7 (135.0 Mbps), 88.6% DC         | WLAN      | 8.82     | ±9.6                   |
| 10624 | AAD | VHT40, MCS8 (162.0 Mbps), 88.4% DC         | WLAN      | 8.96     | ±9.6                   |
| 10625 | AAD | VHT40, MCS9 (180.0 Mbps), 88.2% DC         | WLAN      | 8.96     | ±9.6                   |
| 10626 | AAD | VHT80, MCS0 (29.3 Mbps), 90.0% DC          | WLAN      | 8.83     | ±9.6                   |
| 10627 | AAD | VHT80, MCS1 (58.5 Mbps), 90.0% DC          | WLAN      | 8.88     | ±9.6                   |
| 10628 | AAD | VHT80, MCS2 (87.8 Mbps), 90.0% DC          | WLAN      | 8.71     | ±9.6                   |
| 10629 | AAD | VHT80, MCS3 (117.0 Mbps), 90.0% DC         | WLAN      | 8.85     | ±9.6                   |
| 10630 | AAD | VHT80, MCS4 (175.5 Mbps), 90.0% DC         | WLAN      | 8.72     | ±9.6                   |
| 10631 | AAD | VHT80, MCS5 (234.0 Mbps), 90.0% DC         | WLAN      | 8.81     | ±9.6                   |
| 10632 | AAD | VHT80, MCS6 (263.3 Mbps), 90.0% DC         | WLAN      | 8.74     | ±9.6                   |
| 10633 | AAD | VHT80, MCS7 (292.5 Mbps), 90.0% DC         | WLAN      | 8.83     | ±9.6                   |
| 10634 | AAD | VHT80, MCS8 (351.0 Mbps), 90.0% DC         | WLAN      | 8.80     | ±9.6                   |
| 10635 | AAD | VHT80, MCS9 (390.0 Mbps), 90.0% DC         | WLAN      | 8.81     | ±9.6                   |
| 10636 | AAE | VHT160, MCS0 (58.5 Mbps), 90.0% DC         | WLAN      | 8.83     | ±9.6                   |
| 10637 | AAE | VHT160, MCS1 (117.0 Mbps), 90.0% DC        | WLAN      | 8.79     | ±9.6                   |
| 10638 | AAE | VHT160, MCS2 (175.5 Mbps), 90.0% DC        | WLAN      | 8.86     | ±9.6                   |
| 10639 | AAE | VHT160, MCS3 (234.0 Mbps), 90.0% DC        | WLAN      | 8.85     | ±9.6                   |
| 10640 | AAE | VHT160, MCS4 (351.0 Mbps), 90.0% DC        | WLAN      | 8.98     | ±9.6                   |
| 10641 | AAE | VHT160, MCS5 (468.0 Mbps), 90.0% DC        | WLAN      | 9.06     | ±9.6                   |
| 10642 | AAE | VHT160, MCS6 (526.5 Mbps), 90.0% DC        | WLAN      | 9.06     | ±9.6                   |
| 10643 | AAE | VHT160, MCS7 (585.0 Mbps), 90.0% DC        | WLAN      | 8.89     | ±9.6                   |
| 10644 | AAE | VHT160, MCS8 (702.0 Mbps), 90.0% DC        | WLAN      | 9.05     | ±9.6                   |
| 10645 | AAE | VHT160, MCS9 (780.0 Mbps), 90.0% DC        | WLAN      | 9.11     | ±9.6                   |
| 10646 | AAH | 5.0 MHz, QPSK, UL/DL CFG: 2, SSC: 4, 1 RB  | LTE-TDD   | 11.96    | ±9.6                   |
| 10647 | AAG | 20.0 MHz, QPSK, UL/DL CFG: 2, SSC: 7, 1 RB | LTE-TDD   | 11.96    | ±9.6                   |
| 10648 | AAA | RC8, SO75, 1xAdvanced                      | CDMA2000  | 3.45     | ±9.6                   |
| 10670 | AAA | LE, Test, GFSK                             | Bluetooth | 2.19     | ±9.6                   |
| 10671 | AAC | ET20, MCS0 (8.8 Mbps), 90.0% DC            | WLAN      | 9.09     | ±9.6                   |
| 10672 | AAC | ET20, MCS1 (17.0 Mbps), 90.0% DC           | WLAN      | 8.57     | ±9.6                   |
| 10673 | AAC | ET20, MCS2 (26.0 Mbps), 90.0% DC           | WLAN      | 8.78     | ±9.6                   |
| 10674 | AAC | ET20, MCS3 (34.0 Mbps), 90.0% DC           | WLAN      | 8.74     | ±9.6                   |
| 10675 | AAC | ET20, MCS4 (52.0 Mbps), 90.0% DC           | WLAN      | 8.90     | ±9.6                   |
| 10676 | AAC | ET20, MCS5 (69.0 Mbps), 90.0% DC           | WLAN      | 8.77     | ±9.6                   |
| 10677 | AAC | ET20, MCS6 (77.0 Mbps), 90.0% DC           | WLAN      | 8.73     | ±9.6                   |
| 10678 | AAC | ET20, MCS7 (86.0 Mbps), 90.0% DC           | WLAN      | 8.78     | ±9.6                   |
| 10679 | AAC | ET20, MCS8 (103.0 Mbps), 90.0% DC          | WLAN      | 8.89     | ±9.6                   |
| 10680 | AAC | ET20, MCS9 (115.0 Mbps), 90.0% DC          | WLAN      | 8.80     | ±9.6                   |
| 10681 | AAC | ET20, MCS10 (122.0 Mbps), 90.0% DC         | WLAN      | 8.62     | ±9.6                   |
| 10682 | AAC | ET20, MCS11 (135.0 Mbps), 90.0% DC         | WLAN      | 8.83     | ±9.6                   |
| 10683 | AAC | ET20, MCS0 (8.6 Mbps), 100.0% DC           | WLAN      | 8.42     | ±9.6                   |
| 10684 | AAC | ET20, MCS1 (17.0 Mbps), 100.0% DC          | WLAN      | 8.26     | ±9.6                   |
| 10685 | AAC | ET20, MCS2 (26.0 Mbps), 100.0% DC          | WLAN      | 8.33     | ±9.6                   |
| 10686 | AAC | ET20, MCS3 (34.0 Mbps), 100.0% DC          | WLAN      | 8.28     | ±9.6                   |
| 10687 | AAC | ET20, MCS4 (52.0 Mbps), 100.0% DC          | WLAN      | 8.45     | ±9.6                   |
| 10688 | AAC | ET20, MCS5 (69.0 Mbps), 100.0% DC          | WLAN      | 8.29     | ±9.6                   |
| 10689 | AAC | ET20, MCS6 (77.0 Mbps), 100.0% DC          | WLAN      | 8.55     | ±9.6                   |
| 10690 | AAC | ET20, MCS7 (86.0 Mbps), 100.0% DC          | WLAN      | 8.29     | ±9.6                   |
| 10691 | AAC | ET20, MCS8 (103.0 Mbps), 100.0% DC         | WLAN      | 8.25     | ±9.6                   |
| 10692 | AAC | ET20, MCS9 (115.0 Mbps), 100.0% DC         | WLAN      | 8.29     | ±9.6                   |
| 10693 | AAC | ET20, MCS10 (122.0 Mbps), 100.0% DC        | WLAN      | 8.25     | ±9.6                   |
| 10694 | AAC | ET20, MCS11 (135.0 Mbps), 100.0% DC        | WLAN      | 8.57     | ±9.6                   |
| 10695 | AAC | ET40, MCS0 (17.2 Mbps), 89.8% DC           | WLAN      | 8.78     | ±9.6                   |
| 10696 | AAC | ET40, MCS1 (34.0 Mbps), 89.8% DC           | WLAN      | 8.91     | ±9.6                   |
| 10697 | AAC | ET40, MCS2 (52.0 Mbps), 89.7% DC           | WLAN      | 8.61     | ±9.6                   |
| 10698 | AAC | ET40, MCS3 (69.0 Mbps), 89.7% DC           | WLAN      | 8.89     | ±9.6                   |
| 10699 | AAC | ET40, MCS4 (103.0 Mbps), 89.9% DC          | WLAN      | 8.82     | ±9.6                   |
| 10700 | AAC | ET40, MCS5 (138.0 Mbps), 89.8% DC          | WLAN      | 8.73     | ±9.6                   |
| 10701 | AAC | ET40, MCS6 (155.0 Mbps), 89.8% DC          | WLAN      | 8.86     | ±9.6                   |
| 10702 | AAC | ET40, MCS7 (172.0 Mbps), 89.8% DC          | WLAN      | 8.70     | ±9.6                   |
| 10703 | AAC | ET40, MCS8 (207.0 Mbps), 89.8% DC          | WLAN      | 8.82     | ±9.6                   |
| 10704 | AAC | ET40, MCS9 (229.0 Mbps), 89.8% DC          | WLAN      | 8.56     | ±9.6                   |
| 10705 | AAC | ET40, MCS10 (258.0 Mbps), 89.8% DC         | WLAN      | 8.69     | ±9.6                   |
| 10706 | AAC | ET40, MCS11 (267.0 Mbps), 89.8% DC         | WLAN      | 8.66     | ±9.6                   |

| UID   | Rev | Communication System Name                        | Group         | PAR (dB) | Unc <sup>E</sup> $k = 2$ |
|-------|-----|--------------------------------------------------|---------------|----------|--------------------------|
| 10707 | AAC | ET40, MCS0 (17.2 Mbps), 99.8% DC                 | WLAN          | 8.32     | ±9.6                     |
| 10708 | AAC | ET40, MCS1 (34.0 Mbps), 99.7% DC                 | WLAN          | 8.55     | ±9.6                     |
| 10709 | AAC | ET40, MCS2 (52.0 Mbps), 99.7% DC                 | WLAN          | 8.33     | ±9.6                     |
| 10710 | AAC | ET40, MCS3 (69.0 Mbps), 99.7% DC                 | WLAN          | 8.29     | ±9.6                     |
| 10711 | AAC | ET40, MCS4 (103.0 Mbps), 99.8% DC                | WLAN          | 8.39     | ±9.6                     |
| 10712 | AAC | ET40, MCS5 (138.0 Mbps), 99.8% DC                | WLAN          | 8.67     | ±9.6                     |
| 10713 | AAC | ET40, MCS6 (155.0 Mbps), 99.8% DC                | WLAN          | 8.33     | ±9.6                     |
| 10714 | AAC | ET40, MCS7 (172.0 Mbps), 99.8% DC                | WLAN          | 8.26     | ±9.6                     |
| 10715 | AAC | ET40, MCS8 (207.0 Mbps), 99.8% DC                | WLAN          | 8.45     | ±9.6                     |
| 10716 | AAC | ET40, MCS9 (229.0 Mbps), 99.8% DC                | WLAN          | 8.30     | ±9.6                     |
| 10717 | AAC | ET40, MCS10 (258.0 Mbps), 99.8% DC               | WLAN          | 8.48     | ±9.6                     |
| 10718 | AAC | ET40, MCS11 (267.0 Mbps), 99.8% DC               | WLAN          | 8.24     | ±9.6                     |
| 10719 | AAC | ET80, MCS0 (36.0 Mbps), 90.0% DC                 | WLAN          | 8.81     | ±9.6                     |
| 10720 | AAC | ET80, MCS1 (72.1 Mbps), 90.0% DC                 | WLAN          | 8.87     | ±9.6                     |
| 10721 | AAC | ET80, MCS2 (108.1 Mbps), 90.0% DC                | WLAN          | 8.76     | ±9.6                     |
| 10722 | AAC | ET80, MCS3 (144.1 Mbps), 90.0% DC                | WLAN          | 8.55     | ±9.6                     |
| 10723 | AAC | ET80, MCS4 (216.2 Mbps), 90.0% DC                | WLAN          | 8.70     | ±9.6                     |
| 10724 | AAC | ET80, MCS5 (288.2 Mbps), 90.0% DC                | WLAN          | 8.90     | ±9.6                     |
| 10725 | AAC | ET80, MCS6 (324.4 Mbps), 90.0% DC                | WLAN          | 8.74     | ±9.6                     |
| 10726 | AAC | ET80, MCS7 (360.3 Mbps), 90.0% DC                | WLAN          | 8.72     | ±9.6                     |
| 10727 | AAC | ET80, MCS8 (432.4 Mbps), 90.0% DC                | WLAN          | 8.66     | ±9.6                     |
| 10728 | AAC | ET80, MCS9 (480.4 Mbps), 90.0% DC                | WLAN          | 8.65     | ±9.6                     |
| 10729 | AAC | ET80, MCS10 (540.4 Mbps), 90.0% DC               | WLAN          | 8.64     | ±9.6                     |
| 10730 | AAC | ET80, MCS11 (72.0 Mbps), 90.0% DC                | WLAN          | 8.67     | ±9.6                     |
| 10731 | AAC | ET80, MCS0 (36.0 Mbps), 100.0% DC                | WLAN          | 8.42     | ±9.6                     |
| 10732 | AAC | ET80, MCS1 (72.1 Mbps), 100.0% DC                | WLAN          | 8.46     | ±9.6                     |
| 10733 | AAC | ET80, MCS2 (108.1 Mbps), 100.0% DC               | WLAN          | 8.40     | ±9.6                     |
| 10734 | AAC | ET80, MCS3 (144.1 Mbps), 100.0% DC               | WLAN          | 8.25     | ±9.6                     |
| 10735 | AAC | ET80, MCS4 (216.2 Mbps), 100.0% DC               | WLAN          | 8.33     | ±9.6                     |
| 10736 | AAC | ET80, MCS5 (288.2 Mbps), 100.0% DC               | WLAN          | 8.27     | ±9.6                     |
| 10737 | AAC | ET80, MCS6 (324.4 Mbps), 100.0% DC               | WLAN          | 8.36     | ±9.6                     |
| 10738 | AAC | ET80, MCS7 (360.3 Mbps), 100.0% DC               | WLAN          | 8.42     | ±9.6                     |
| 10739 | AAC | ET80, MCS8 (432.4 Mbps), 100.0% DC               | WLAN          | 8.29     | ±9.6                     |
| 10740 | AAC | ET80, MCS9 (480.4 Mbps), 100.0% DC               | WLAN          | 8.48     | ±9.6                     |
| 10741 | AAC | ET80, MCS10 (540.4 Mbps), 100.0% DC              | WLAN          | 8.40     | ±9.6                     |
| 10742 | AAC | ET80, MCS11 (600.5 Mbps), 100.0% DC              | WLAN          | 8.43     | ±9.6                     |
| 10743 | AAC | ET160, MCS0 (72.0 Mbps), 88.2% DC                | WLAN          | 8.94     | ±9.6                     |
| 10744 | AAC | ET160, MCS1 (144.0 Mbps), 87.1% DC               | WLAN          | 9.16     | ±9.6                     |
| 10745 | AAC | ET160, MCS2 (216.0 Mbps), 87.4% DC               | WLAN          | 8.93     | ±9.6                     |
| 10746 | AAC | ET160, MCS3 (282.0 Mbps), 87.1% DC               | WLAN          | 9.11     | ±9.6                     |
| 10747 | AAC | ET160, MCS4 (432.0 Mbps), 87.4% DC               | WLAN          | 9.04     | ±9.6                     |
| 10748 | AAC | ET160, MCS5 (576.0 Mbps), 86.8% DC               | WLAN          | 8.93     | ±9.6                     |
| 10749 | AAC | ET160, MCS6 (649.0 Mbps), 86.7% DC               | WLAN          | 8.90     | ±9.6                     |
| 10750 | AAC | ET160, MCS7 (721.0 Mbps), 86.7% DC               | WLAN          | 8.79     | ±9.6                     |
| 10751 | AAC | ET160, MCS8 (865.0 Mbps), 86.3% DC               | WLAN          | 8.82     | ±9.6                     |
| 10752 | AAC | ET160, MCS9 (961.0 Mbps), 86.3% DC               | WLAN          | 8.81     | ±9.6                     |
| 10753 | AAC | ET160, MCS10 (1081.0 Mbps), 86.7% DC             | WLAN          | 9.00     | ±9.6                     |
| 10754 | AAC | ET160, MCS11 (1201.0 Mbps), 86.7% DC             | WLAN          | 8.94     | ±9.6                     |
| 10755 | AAC | ET160, MCS0 (72.0 Mbps), 98.0% DC                | WLAN          | 8.64     | ±9.6                     |
| 10756 | AAC | ET160, MCS1 (144.0 Mbps), 96.8% DC               | WLAN          | 8.77     | ±9.6                     |
| 10757 | AAC | ET160, MCS2 (216.0 Mbps), 97.1% DC               | WLAN          | 8.77     | ±9.6                     |
| 10758 | AAC | ET160, MCS3 (282.0 Mbps), 96.8% DC               | WLAN          | 8.69     | ±9.6                     |
| 10759 | AAC | ET160, MCS4 (432.0 Mbps), 97.1% DC               | WLAN          | 8.58     | ±9.6                     |
| 10760 | AAC | ET160, MCS5 (576.0 Mbps), 96.5% DC               | WLAN          | 8.49     | ±9.6                     |
| 10761 | AAC | ET160, MCS6 (649.0 Mbps), 96.3% DC               | WLAN          | 8.58     | ±9.6                     |
| 10762 | AAC | ET160, MCS7 (721.0 Mbps), 96.3% DC               | WLAN          | 8.49     | ±9.6                     |
| 10763 | AAC | ET160, MCS8 (865.0 Mbps), 95.9% DC               | WLAN          | 8.53     | ±9.6                     |
| 10764 | AAC | ET160, MCS9 (961.0 Mbps), 95.9% DC               | WLAN          | 8.54     | ±9.6                     |
| 10765 | AAC | ET160, MCS10 (1081.0 Mbps), 96.3% DC             | WLAN          | 8.54     | ±9.6                     |
| 10766 | AAC | ET160, MCS11 (1201.0 Mbps), 96.3% DC             | WLAN          | 8.51     | ±9.6                     |
| 10767 | AAG | CP-OFDM, 5.0 MHz, QPSK, 15 kHz, 99.9% DC, 1 RB   | 5G NR FR1 TDD | 7.99     | ±9.6                     |
| 10768 | AAE | CP-OFDM, 10.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB | 5G NR FR1 TDD | 8.01     | ±9.6                     |
| 10769 | AAD | CP-OFDM, 15.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB | 5G NR FR1 TDD | 8.01     | ±9.6                     |
| 10770 | AAE | CP-OFDM, 20.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB | 5G NR FR1 TDD | 8.02     | ±9.6                     |
| 10771 | AAD | CP-OFDM, 25.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB | 5G NR FR1 TDD | 8.02     | ±9.6                     |
| 10772 | AAE | CP-OFDM, 30.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB | 5G NR FR1 TDD | 8.23     | ±9.6                     |

| UID   | Rev | Communication System Name                            | Group         | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|------------------------------------------------------|---------------|----------|------------------------|
| 10773 | AAF | CP-OFDM, 40.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 8.03     | ±9.6                   |
| 10774 | AAE | CP-OFDM, 50.0 MHz, QPSK, 15 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 8.02     | ±9.6                   |
| 10775 | AAF | CP-OFDM, 5.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB    | 5G NR FR1 TDD | 8.31     | ±9.6                   |
| 10776 | AAE | CP-OFDM, 10.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.30     | ±9.6                   |
| 10777 | AAC | CP-OFDM, 15.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.30     | ±9.6                   |
| 10778 | AAE | CP-OFDM, 20.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10779 | AAC | CP-OFDM, 25.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.42     | ±9.6                   |
| 10780 | AAE | CP-OFDM, 30.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.38     | ±9.6                   |
| 10781 | AAF | CP-OFDM, 40.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.38     | ±9.6                   |
| 10782 | AAE | CP-OFDM, 50.0 MHz, QPSK, 15 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.43     | ±9.6                   |
| 10783 | AAG | CP-OFDM, 5.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB   | 5G NR FR1 TDD | 8.31     | ±9.6                   |
| 10784 | AAE | CP-OFDM, 10.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.29     | ±9.6                   |
| 10785 | AAD | CP-OFDM, 15.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.40     | ±9.6                   |
| 10786 | AAE | CP-OFDM, 20.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.35     | ±9.6                   |
| 10787 | AAD | CP-OFDM, 25.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.44     | ±9.6                   |
| 10788 | AAE | CP-OFDM, 30.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.39     | ±9.6                   |
| 10789 | AAF | CP-OFDM, 40.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.37     | ±9.6                   |
| 10790 | AAE | CP-OFDM, 50.0 MHz, QPSK, 15 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.39     | ±9.6                   |
| 10791 | AAG | CP-OFDM, 5.0 MHz, QPSK, 30 kHz, 99.9% DC, 1 RB       | 5G NR FR1 TDD | 7.83     | ±9.6                   |
| 10792 | AAE | CP-OFDM, 10.0 MHz, QPSK, 30 kHz, 99.9% DC, 1 RB      | 5G NR FR1 TDD | 7.92     | ±9.6                   |
| 10793 | AAD | CP-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.95     | ±9.6                   |
| 10794 | AAE | CP-OFDM, 20.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.82     | ±9.6                   |
| 10795 | AAD | CP-OFDM, 25.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.84     | ±9.6                   |
| 10796 | AAE | CP-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.82     | ±9.6                   |
| 10797 | AAF | CP-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 8.01     | ±9.6                   |
| 10798 | AAE | CP-OFDM, 50.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.89     | ±9.6                   |
| 10799 | AAF | CP-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.93     | ±9.6                   |
| 10801 | AAF | CP-OFDM, 80.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.89     | ±9.6                   |
| 10802 | AAE | CP-OFDM, 90.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.87     | ±9.6                   |
| 10803 | AAF | CP-OFDM, 100.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB    | 5G NR FR1 TDD | 7.93     | ±9.6                   |
| 10805 | AAE | CP-OFDM, 10.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10806 | AAD | CP-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.37     | ±9.6                   |
| 10809 | AAE | CP-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10810 | AAF | CP-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10812 | AAF | CP-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.35     | ±9.6                   |
| 10817 | AAG | CP-OFDM, 5.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB   | 5G NR FR1 TDD | 8.35     | ±9.6                   |
| 10818 | AAE | CP-OFDM, 10.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10819 | AAD | CP-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.33     | ±9.6                   |
| 10820 | AAE | CP-OFDM, 20.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.30     | ±9.6                   |
| 10821 | AAD | CP-OFDM, 25.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10822 | AAE | CP-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10823 | AAF | CP-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.36     | ±9.6                   |
| 10824 | AAE | CP-OFDM, 50.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.39     | ±9.6                   |
| 10825 | AAF | CP-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10827 | AAF | CP-OFDM, 80.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.42     | ±9.6                   |
| 10828 | AAE | CP-OFDM, 90.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.43     | ±9.6                   |
| 10829 | AAF | CP-OFDM, 100.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB | 5G NR FR1 TDD | 8.40     | ±9.6                   |
| 10830 | AAE | CP-OFDM, 10.0 MHz, QPSK, 60 kHz, 99.9% DC, 1 RB      | 5G NR FR1 TDD | 7.63     | ±9.6                   |
| 10831 | AAD | CP-OFDM, 15.0 MHz, QPSK, 60 kHz, 99.9% DC, 1 RB      | 5G NR FR1 TDD | 7.73     | ±9.6                   |
| 10832 | AAE | CP-OFDM, 20.0 MHz, QPSK, 60 kHz, 99.9% DC, 1 RB      | 5G NR FR1 TDD | 7.74     | ±9.6                   |
| 10833 | AAD | CP-OFDM, 25.0 MHz, QPSK, 60 kHz, 99.9% DC, 1 RB      | 5G NR FR1 TDD | 7.70     | ±9.6                   |
| 10834 | AAE | CP-OFDM, 30.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.75     | ±9.6                   |
| 10835 | AAF | CP-OFDM, 40.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.70     | ±9.6                   |
| 10836 | AAE | CP-OFDM, 50.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.66     | ±9.6                   |
| 10837 | AAF | CP-OFDM, 60.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.68     | ±9.6                   |
| 10839 | AAF | CP-OFDM, 80.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.70     | ±9.6                   |
| 10840 | AAE | CP-OFDM, 90.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB     | 5G NR FR1 TDD | 7.87     | ±9.6                   |
| 10841 | AAF | CP-OFDM, 100.0 MHz, QPSK, 60 kHz, 100.0% DC, 1 RB    | 5G NR FR1 TDD | 7.71     | ±9.6                   |
| 10843 | AAD | CP-OFDM, 15.0 MHz, QPSK, 60 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.49     | ±9.6                   |
| 10844 | AAE | CP-OFDM, 20.0 MHz, QPSK, 60 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10846 | AAE | CP-OFDM, 30.0 MHz, QPSK, 60 kHz, 100.0% DC, 50% RB   | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10854 | AAE | CP-OFDM, 10.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10855 | AAD | CP-OFDM, 15.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.36     | ±9.6                   |
| 10856 | AAE | CP-OFDM, 20.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.37     | ±9.6                   |
| 10857 | AAD | CP-OFDM, 25.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.35     | ±9.6                   |
| 10858 | AAE | CP-OFDM, 30.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB  | 5G NR FR1 TDD | 8.36     | ±9.6                   |

| UID   | Rev | Communication System Name                                 | Group         | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|-----------------------------------------------------------|---------------|----------|------------------------|
| 10859 | AAF | CP-OFDM, 40.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB       | 5G NR FR1 TDD | 8.34     | ±9.6                   |
| 10860 | AAE | CP-OFDM, 50.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB       | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10861 | AAF | CP-OFDM, 60.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB       | 5G NR FR1 TDD | 8.40     | ±9.6                   |
| 10863 | AAF | CP-OFDM, 80.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB       | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10864 | AAE | CP-OFDM, 90.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB       | 5G NR FR1 TDD | 8.37     | ±9.6                   |
| 10865 | AAF | CP-OFDM, 100.0 MHz, QPSK, 60 kHz, 100.0% DC, 100% RB      | 5G NR FR1 TDD | 8.41     | ±9.6                   |
| 10866 | AAF | DFT-s-OFDM, 100.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB      | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10868 | AAF | DFT-s-OFDM, 100.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB   | 5G NR FR1 TDD | 5.89     | ±9.6                   |
| 10868 | AAE | DFT-s-OFDM, 100.0 MHz, QPSK, 120 kHz, 100.0% DC, 1 RB     | 5G NR FR2 TDD | 5.75     | ±9.6                   |
| 10870 | AAE | DFT-s-OFDM, 100.0 MHz, QPSK, 120 kHz, 100.0% DC, 100% RB  | 5G NR FR2 TDD | 5.86     | ±9.6                   |
| 10871 | AAE | DFT-s-OFDM, 100.0 MHz, 16QAM, 120 kHz, 100.0% DC, 1 RB    | 5G NR FR2 TDD | 5.75     | ±9.6                   |
| 10872 | AAE | DFT-s-OFDM, 100.0 MHz, 16QAM, 120 kHz, 100.0% DC, 100% RB | 5G NR FR2 TDD | 6.52     | ±9.6                   |
| 10873 | AAE | DFT-s-OFDM, 100.0 MHz, 64QAM, 120 kHz, 100.0% DC, 1 RB    | 5G NR FR2 TDD | 6.61     | ±9.6                   |
| 10874 | AAE | DFT-s-OFDM, 100.0 MHz, 64QAM, 120 kHz, 100.0% DC, 100% RB | 5G NR FR2 TDD | 6.65     | ±9.6                   |
| 10875 | AAE | CP-OFDM, 100.0 MHz, QPSK, 120 kHz, 100.0% DC, 1 RB        | 5G NR FR2 TDD | 7.78     | ±9.6                   |
| 10876 | AAE | CP-OFDM, 100.0 MHz, QPSK, 120 kHz, 100.0% DC, 100% RB     | 5G NR FR2 TDD | 6.39     | ±9.6                   |
| 10877 | AAE | CP-OFDM, 100.0 MHz, 16QAM, 120 kHz, 100.0% DC, 1 RB       | 5G NR FR2 TDD | 7.95     | ±9.6                   |
| 10878 | AAE | CP-OFDM, 100.0 MHz, 16QAM, 120 kHz, 100.0% DC, 100% RB    | 5G NR FR2 TDD | 8.41     | ±9.6                   |
| 10879 | AAE | CP-OFDM, 100.0 MHz, 64QAM, 120 kHz, 100.0% DC, 1 RB       | 5G NR FR2 TDD | 8.12     | ±9.6                   |
| 10880 | AAE | CP-OFDM, 100.0 MHz, 64QAM, 120 kHz, 100.0% DC, 100% RB    | 5G NR FR2 TDD | 8.38     | ±9.6                   |
| 10881 | AAE | DFT-s-OFDM, 50.0 MHz, QPSK, 120 kHz, 100.0% DC, 1 RB      | 5G NR FR2 TDD | 6.75     | ±9.6                   |
| 10882 | AAE | DFT-s-OFDM, 50.0 MHz, QPSK, 120 kHz, 100.0% DC, 100% RB   | 5G NR FR2 TDD | 6.96     | ±9.6                   |
| 10883 | AAE | DFT-s-OFDM, 50.0 MHz, 16QAM, 120 kHz, 100.0% DC, 1 RB     | 5G NR FR2 TDD | 6.57     | ±9.6                   |
| 10884 | AAE | DFT-s-OFDM, 50.0 MHz, 16QAM, 120 kHz, 100.0% DC, 100% RB  | 5G NR FR2 TDD | 6.53     | ±9.6                   |
| 10885 | AAE | DFT-s-OFDM, 50.0 MHz, 64QAM, 120 kHz, 100.0% DC, 1 RB     | 5G NR FR2 TDD | 6.61     | ±9.6                   |
| 10886 | AAE | DFT-s-OFDM, 50.0 MHz, 64QAM, 120 kHz, 100.0% DC, 100% RB  | 5G NR FR2 TDD | 6.65     | ±9.6                   |
| 10887 | AAE | CP-OFDM, 50.0 MHz, QPSK, 120 kHz, 99.9% DC, 1 RB          | 5G NR FR2 TDD | 7.78     | ±9.6                   |
| 10888 | AAE | CP-OFDM, 50.0 MHz, QPSK, 120 kHz, 100.0% DC, 100% RB      | 5G NR FR2 TDD | 8.35     | ±9.6                   |
| 10889 | AAE | CP-OFDM, 50.0 MHz, 16QAM, 120 kHz, 100.0% DC, 1 RB        | 5G NR FR2 TDD | 8.02     | ±9.6                   |
| 10890 | AAE | CP-OFDM, 50.0 MHz, 16QAM, 120 kHz, 100.0% DC, 100% RB     | 5G NR FR2 TDD | 8.40     | ±9.6                   |
| 10891 | AAE | CP-OFDM, 50.0 MHz, 64QAM, 120 kHz, 100.0% DC, 1 RB        | 5G NR FR2 TDD | 8.13     | ±9.6                   |
| 10892 | AAE | CP-OFDM, 50.0 MHz, 64QAM, 120 kHz, 100.0% DC, 100% RB     | 5G NR FR2 TDD | 8.41     | ±9.6                   |
| 10897 | AAE | DFT-s-OFDM, 5.0 MHz, QPSK, 30 kHz, 99.9% DC, 1 RB         | 5G NR FR1 TDD | 5.66     | ±9.6                   |
| 10898 | AAC | DFT-s-OFDM, 10.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.67     | ±9.6                   |
| 10899 | AAB | DFT-s-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.67     | ±9.6                   |
| 10900 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.66     | ±9.6                   |
| 10901 | AAB | DFT-s-OFDM, 25.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10902 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10903 | AAD | DFT-s-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10904 | AAC | DFT-s-OFDM, 50.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10905 | AAD | DFT-s-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10906 | AAD | DFT-s-OFDM, 80.0 MHz, QPSK, 30 kHz, 100.0% DC, 1 RB       | 5G NR FR1 TDD | 5.68     | ±9.6                   |
| 10907 | AAE | DFT-s-OFDM, 5.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB      | 5G NR FR1 TDD | 5.78     | ±9.6                   |
| 10908 | AAC | DFT-s-OFDM, 10.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.93     | ±9.6                   |
| 10909 | AAB | DFT-s-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.96     | ±9.6                   |
| 10910 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.83     | ±9.6                   |
| 10911 | AAB | DFT-s-OFDM, 25.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.93     | ±9.6                   |
| 10912 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.84     | ±9.6                   |
| 10913 | AAD | DFT-s-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.84     | ±9.6                   |
| 10914 | AAC | DFT-s-OFDM, 50.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.85     | ±9.6                   |
| 10915 | AAD | DFT-s-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.83     | ±9.6                   |
| 10916 | AAD | DFT-s-OFDM, 80.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB     | 5G NR FR1 TDD | 5.87     | ±9.6                   |
| 10917 | AAD | DFT-s-OFDM, 100.0 MHz, QPSK, 30 kHz, 100.0% DC, 50% RB    | 5G NR FR1 TDD | 5.94     | ±9.6                   |
| 10918 | AAE | DFT-s-OFDM, 5.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB     | 5G NR FR1 TDD | 5.86     | ±9.6                   |
| 10919 | AAC | DFT-s-OFDM, 10.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.86     | ±9.6                   |
| 10920 | AAB | DFT-s-OFDM, 15.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.87     | ±9.6                   |
| 10921 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.84     | ±9.6                   |
| 10922 | AAB | DFT-s-OFDM, 25.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.82     | ±9.6                   |
| 10923 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.84     | ±9.6                   |
| 10924 | AAD | DFT-s-OFDM, 40.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.95     | ±9.6                   |
| 10925 | AAC | DFT-s-OFDM, 50.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.95     | ±9.6                   |
| 10926 | AAD | DFT-s-OFDM, 60.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.84     | ±9.6                   |
| 10927 | AAD | DFT-s-OFDM, 80.0 MHz, QPSK, 30 kHz, 100.0% DC, 100% RB    | 5G NR FR1 TDD | 5.94     | ±9.6                   |
| 10928 | AAD | DFT-s-OFDM, 5.0 MHz, QPSK, 15 kHz, 1 RB                   | 5G NR FR1 FDD | 5.52     | ±9.6                   |
| 10929 | AAD | DFT-s-OFDM, 10.0 MHz, QPSK, 15 kHz, 1 RB                  | 5G NR FR1 FDD | 5.52     | ±9.6                   |
| 10930 | AAC | DFT-s-OFDM, 15.0 MHz, QPSK, 15 kHz, 1 RB                  | 5G NR FR1 FDD | 5.52     | ±9.6                   |

| UID   | Rev | Communication System Name                   | Group         | PAR (dB) | Unc <sup>E</sup> k = 2 |
|-------|-----|---------------------------------------------|---------------|----------|------------------------|
| 10931 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 15 kHz, 1 RB    | 5G NR FR1 FDD | 5.51     | ±9.6                   |
| 10932 | AAC | DFT-s-OFDM, 25.0 MHz, QPSK, 15 kHz, 1 RB    | 5G NR FR1 FDD | 5.51     | ±9.6                   |
| 10933 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 15 kHz, 1 RB    | 5G NR FR1 FDD | 5.51     | ±9.6                   |
| 10934 | AAC | DFT-s-OFDM, 40.0 MHz, QPSK, 15 kHz, 1 RB    | 5G NR FR1 FDD | 5.51     | ±9.6                   |
| 10935 | AAD | DFT-s-OFDM, 50.0 MHz, QPSK, 15 kHz, 1 RB    | 5G NR FR1 FDD | 5.51     | ±9.6                   |
| 10936 | AAD | DFT-s-OFDM, 5.0 MHz, QPSK, 15 kHz, 50% RB   | 5G NR FR1 FDD | 5.90     | ±9.6                   |
| 10937 | AAD | DFT-s-OFDM, 10.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.77     | ±9.6                   |
| 10938 | AAC | DFT-s-OFDM, 15.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.90     | ±9.6                   |
| 10939 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.82     | ±9.6                   |
| 10940 | AAC | DFT-s-OFDM, 25.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.89     | ±9.6                   |
| 10941 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.83     | ±9.6                   |
| 10942 | AAC | DFT-s-OFDM, 40.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.85     | ±9.6                   |
| 10943 | AAD | DFT-s-OFDM, 50.0 MHz, QPSK, 15 kHz, 50% RB  | 5G NR FR1 FDD | 5.95     | ±9.6                   |
| 10944 | AAD | DFT-s-OFDM, 5.0 MHz, QPSK, 15 kHz, 100% RB  | 5G NR FR1 FDD | 5.81     | ±9.6                   |
| 10945 | AAD | DFT-s-OFDM, 10.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.85     | ±9.6                   |
| 10946 | AAC | DFT-s-OFDM, 15.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.83     | ±9.6                   |
| 10947 | AAC | DFT-s-OFDM, 20.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.87     | ±9.6                   |
| 10948 | AAC | DFT-s-OFDM, 25.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.94     | ±9.6                   |
| 10949 | AAC | DFT-s-OFDM, 30.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.87     | ±9.6                   |
| 10950 | AAC | DFT-s-OFDM, 40.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.94     | ±9.6                   |
| 10951 | AAD | DFT-s-OFDM, 50.0 MHz, QPSK, 15 kHz, 100% RB | 5G NR FR1 FDD | 5.92     | ±9.6                   |
| 10978 | AAA | BDR, 1.0 MHz, 76.7% DC                      | ULLA          | 1.16     | ±9.6                   |
| 10979 | AAA | HDR4, 2.0 MHz, 25.1% DC                     | ULLA          | 8.58     | ±9.6                   |
| 10980 | AAA | HDR8, 4.0 MHz, 16.5% DC                     | ULLA          | 10.32    | ±9.6                   |
| 10981 | AAA | HDRp4, 2.0 MHz, 89.0% DC                    | ULLA          | 3.19     | ±9.6                   |
| 10982 | AAA | HDRp8, 4.0 MHz, 90.3% DC                    | ULLA          | 3.43     | ±9.6                   |
| 11013 | AAB | EHT320, MCS1 (272.0 Mbps), 100.0% DC        | WLAN          | 8.47     | ±9.6                   |
| 11014 | AAB | EHT320, MCS2 (408.0 Mbps), 100.0% DC        | WLAN          | 8.45     | ±9.6                   |
| 11015 | AAB | EHT320, MCS3 (544.0 Mbps), 100.0% DC        | WLAN          | 8.44     | ±9.6                   |
| 11016 | AAB | EHT320, MCS4 (817.0 Mbps), 100.0% DC        | WLAN          | 8.44     | ±9.6                   |
| 11017 | AAB | EHT320, MCS5 (1089.0 Mbps), 100.0% DC       | WLAN          | 8.41     | ±9.6                   |
| 11018 | AAB | EHT320, MCS6 (1225.0 Mbps), 100.0% DC       | WLAN          | 8.40     | ±9.6                   |
| 11019 | AAB | EHT320, MCS7 (1361.0 Mbps), 100.0% DC       | WLAN          | 8.29     | ±9.6                   |
| 11020 | AAB | EHT320, MCS8 (1633.0 Mbps), 100.0% DC       | WLAN          | 8.27     | ±9.6                   |
| 11021 | AAB | EHT320, MCS9 (1815.0 Mbps), 100.0% DC       | WLAN          | 8.46     | ±9.6                   |
| 11022 | AAB | EHT320, MCS10 (2042.0 Mbps), 100.0% DC      | WLAN          | 8.36     | ±9.6                   |
| 11023 | AAB | EHT320, MCS11 (2269.0 Mbps), 100.0% DC      | WLAN          | 8.09     | ±9.6                   |
| 11024 | AAB | EHT320, MCS12 (2450.0 Mbps), 100.0% DC      | WLAN          | 8.42     | ±9.6                   |
| 11025 | AAB | EHT320, MCS13 (2722.0 Mbps), 100.0% DC      | WLAN          | 8.37     | ±9.6                   |
| 11026 | AAB | EHT320, MCS0 (136.0 Mbps), 100.0% DC        | WLAN          | 8.39     | ±9.6                   |

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

**Sporton**  
Taoyuan City

Certificate No.

**EX-7700\_Jan26**

## CALIBRATION CERTIFICATE

Object

**EX3DV4 - SN:7700**

Calibration procedure(s)

QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6,  
QA CAL-25.v8, QA CAL-48.v2  
Calibration procedure for dosimetric E-field probes

Calibration date

**January 26, 2026**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID         | Calibration Date (Certificate No.)     | Sched. Cal. |
|-----------------------------|------------|----------------------------------------|-------------|
| Power Sensor R&S NRP40T     | SN: 101861 | 29-Apr-25 (No. 2025-001450)            | Apr-26      |
| N-type mismatch combination | SN: L1119  | 26-Mar-25 (No. 217-04292)              | Mar-26      |
| OCP DAK-12                  | SN: 1016   | 16-Sept-25 (No. OCP-DAK12-1016_Sep25)  | Sep-26      |
| OCP DAK-3,5                 | SN: 1249   | 16-Sept-25 (No. OCP-DAK3.5-1249_Sep25) | Sep-26      |
| Reference Probe EX3DV4      | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26      |
| DAE4                        | SN: 1301   | 22-Jan-26 (No. DAE4-1301_Jan26)        | Jan-27      |

| Secondary Standards | ID        | Check Date (in house)                 | Sched. Check |
|---------------------|-----------|---------------------------------------|--------------|
| ACAP 2020 Setup 1   | SN: L1404 | 01-Oct-25 (No. IHCK_ACAP2020-1_Oct25) | Oct-26       |
| OCP DAK-12          | SN: 1029  | 27-Feb-25 (No. OCP-DAK12-1029_Feb25)  | Feb-26       |
| OCP DAK-3,5         | SN: 1336  | 10-Dec-25 (No. OCP-DAK3.5-1336_Dec25) | Dec-26       |

Calibrated by

Name

Joanna Lleshaj

Function

Laboratory Technician

Signature

Approved by

Sven Kühn

Technical Manager

Issued: January 27, 2026

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

## Glossary

|                        |                                                                                                                                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                    | tissue simulating liquid                                                                                                                       |
| NORM <sub>x,y,z</sub>  | sensitivity in free space                                                                                                                      |
| ConvF                  | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                     |
| DCP                    | diode compression point                                                                                                                        |
| CF                     | crest factor (1/duty_cycle) of the RF signal                                                                                                   |
| A, B, C, D             | modulation dependent linearization parameters                                                                                                  |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |
| Connector Angle        | information used in DASY system to align probe sensor X to the robot coordinate system                                                         |

## Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices – Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

## Parameters of Probe: EX3DV4 - SN:7700

## Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k = 2) |
|-----------------------------------------------------------|----------|----------|----------|-------------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.63     | 0.64     | 0.67     | ±10.1%      |
| DCP (mV) <sup>B</sup>                                     | 106.4    | 105.7    | 105.4    | ±4.7%       |

## Calibration Results for Modulation Response

| UID   | Communication System Name      |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C     | D<br>dB | VR<br>mV | Max<br>dev. | Max<br>Unc <sup>E</sup><br>k = 2 |
|-------|--------------------------------|---|---------|------------------------------|-------|---------|----------|-------------|----------------------------------|
| 0     | Continuous Wave                | X | 0.00    | 0.00                         | 1.00  | 0.00    | 129.4    | ±2.0%       | ±4.7%                            |
|       |                                | Y | 0.00    | 0.00                         | 1.00  |         | 137.4    |             |                                  |
|       |                                | Z | 0.00    | 0.00                         | 1.00  |         | 135.4    |             |                                  |
| 10352 | Pulse (D=10%, T=5 ms)          | X | 0.81    | 69.92                        | 17.76 | 10.00   | 23.0     | ±1.7%       | ±9.6%                            |
|       |                                | Y | 0.28    | 60.15                        | 15.10 |         | 24.0     |             |                                  |
|       |                                | Z | 0.58    | 69.94                        | 18.35 |         | 24.0     |             |                                  |
| 10353 | Pulse (D=20%, T=5 ms)          | X | 0.76    | 72.93                        | 17.79 | 6.99    | 47.0     | ±1.3%       | ±9.6%                            |
|       |                                | Y | 0.26    | 63.16                        | 15.17 |         | 48.0     |             |                                  |
|       |                                | Z | 0.54    | 72.95                        | 18.40 |         | 48.0     |             |                                  |
| 10354 | Pulse (D=40%, T=5 ms)          | X | 0.71    | 75.94                        | 17.83 | 3.98    | 93.0     | ±1.2%       | ±9.6%                            |
|       |                                | Y | 0.23    | 66.17                        | 15.24 |         | 95.0     |             |                                  |
|       |                                | Z | 0.50    | 75.96                        | 18.46 |         | 97.0     |             |                                  |
| 10355 | Pulse (D=60%, T=5 ms)          | X | 0.68    | 77.71                        | 17.86 | 2.22    | 139.0    | ±1.2%       | ±9.6%                            |
|       |                                | Y | 0.22    | 67.93                        | 15.29 |         | 143.0    |             |                                  |
|       |                                | Z | 0.48    | 77.72                        | 18.50 |         | 145.0    |             |                                  |
| 10387 | Random (BW=1 MHz, MOD=QPSK)    | X | 0.01    | 74.83                        | 19.16 | 0.20    | 107.0    | ±1.4%       | ±9.6%                            |
|       |                                | Y | 0.00    | 65.05                        | 17.05 |         | 110.0    |             |                                  |
|       |                                | Z | 0.01    | 74.84                        | 19.91 |         | 112.0    |             |                                  |
| 10388 | Random (BW=10 MHz, MOD=QPSK)   | X | 1.59    | 74.71                        | 17.41 | 0.00    | 113.0    | ±2.4%       | ±9.6%                            |
|       |                                | Y | 0.56    | 64.93                        | 14.31 |         | 116.0    |             |                                  |
|       |                                | Z | 1.62    | 74.72                        | 17.53 |         | 118.0    |             |                                  |
| 10396 | Random (BW=100 kHz, MOD=64QAM) | X | 0.00    | 73.65                        | 20.01 | 1.52    | 80.0     | ±3.2%       | ±9.6%                            |
|       |                                | Y | 0.00    | 63.87                        | 18.49 |         | 82.0     |             |                                  |
|       |                                | Z | 0.02    | 73.67                        | 21.37 |         | 84.0     |             |                                  |
| 10399 | Random (BW=40 MHz, MOD=64QAM)  | X | 3.73    | 73.65                        | 17.31 | 0.00    | 105.0    | ±3.7%       | ±9.6%                            |
|       |                                | Y | 1.68    | 63.87                        | 12.91 |         | 108.0    |             |                                  |
|       |                                | Z | 3.71    | 73.67                        | 17.38 |         | 110.0    |             |                                  |
| 10414 | Random (BW=40 MHz, HIGH PAR)   | X | 4.44    | 71.39                        | 17.30 | 0.00    | 75.0     | ±1.7%       | ±9.6%                            |
|       |                                | Y | 1.96    | 61.61                        | 12.81 |         | 78.0     |             |                                  |
|       |                                | Z | 4.52    | 71.40                        | 17.38 |         | 80.0     |             |                                  |

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Linearization parameter uncertainty for maximum specified field strength.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## Parameters of Probe: EX3DV4 - SN:7700

### Sensor Model Parameters

|   | C1<br>fF | C2<br>fF | $\alpha$<br>$V^{-1}$ | T1<br>$ms V^{-2}$ | T2<br>$ms V^{-1}$ | T3<br>ms | T4<br>$V^{-2}$ | T5<br>$V^{-1}$ | T6   |
|---|----------|----------|----------------------|-------------------|-------------------|----------|----------------|----------------|------|
| x | 8.9      | 64.60    | 33.42                | 3.03              | 0.00              | 4.90     | 0.39           | 0.00           | 1.00 |
| y | 7.9      | 57.28    | 33.97                | 3.73              | 0.00              | 4.90     | 0.43           | 0.00           | 1.00 |
| z | 9.9      | 72.50    | 34.24                | 3.10              | 0.00              | 4.90     | 0.00           | 0.02           | 1.00 |

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle                               | -70.6°     |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 12 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 1.4 mm     |

**Note:** Measurement distance from surface can be increased to 3–4 mm for an *Area Scan* job.

## Parameters of Probe: EX3DV4 - SN:7700

## Calibration Parameter Determined in HSL

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity <sup>F</sup> (S/m) | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unc <sup>H</sup> (k = 2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|--------------------------|
| 750                  | 41.9                               | 0.89                            | 9.98    | 9.68    | 9.75    | 0.39               | 1.27                    | ±11.0%                   |
| 835                  | 41.5                               | 0.90                            | 9.97    | 9.66    | 9.74    | 0.39               | 1.27                    | ±11.0%                   |
| 900                  | 41.5                               | 0.97                            | 9.55    | 9.25    | 9.33    | 0.38               | 1.27                    | ±11.0%                   |
| 1750                 | 40.1                               | 1.37                            | 8.26    | 8.00    | 8.07    | 0.37               | 1.27                    | ±11.0%                   |
| 1900                 | 40.0                               | 1.40                            | 8.08    | 7.83    | 7.89    | 0.37               | 1.27                    | ±11.0%                   |
| 2000                 | 40.0                               | 1.40                            | 7.82    | 7.58    | 7.64    | 0.37               | 1.27                    | ±11.0%                   |
| 2300                 | 39.5                               | 1.67                            | 7.76    | 7.52    | 7.57    | 0.37               | 1.27                    | ±11.0%                   |
| 2450                 | 39.2                               | 1.80                            | 7.46    | 7.23    | 7.29    | 0.37               | 1.27                    | ±11.0%                   |
| 2600                 | 39.0                               | 1.96                            | 7.62    | 7.39    | 7.44    | 0.36               | 1.27                    | ±11.0%                   |
| 3300                 | 38.2                               | 2.71                            | 6.80    | 6.59    | 6.64    | 0.36               | 1.27                    | ±13.1%                   |
| 3500                 | 37.9                               | 2.91                            | 6.73    | 6.52    | 6.57    | 0.35               | 1.27                    | ±13.1%                   |
| 3700                 | 37.7                               | 3.12                            | 6.87    | 6.66    | 6.71    | 0.35               | 1.27                    | ±13.1%                   |
| 3900                 | 37.5                               | 3.32                            | 6.84    | 6.63    | 6.68    | 0.35               | 1.27                    | ±13.1%                   |
| 4100                 | 37.2                               | 3.53                            | 6.64    | 6.43    | 6.48    | 0.35               | 1.27                    | ±13.1%                   |
| 5250                 | 35.9                               | 4.71                            | 5.66    | 5.49    | 5.53    | 0.31               | 1.27                    | ±13.1%                   |
| 5600                 | 35.5                               | 5.07                            | 5.27    | 5.11    | 5.15    | 0.28               | 1.27                    | ±13.1%                   |
| 5800                 | 35.3                               | 5.27                            | 5.21    | 5.05    | 5.09    | 0.26               | 1.27                    | ±13.1%                   |

<sup>C</sup> Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2); else it is restricted to ±50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4–8 MHz, and ConvF assessed at 13 MHz is 9–19 MHz. Above 5 GHz frequency validity can be extended to ±110 MHz.

<sup>F</sup> The probes are calibrated using tissue simulating liquids (TSL) that deviate for  $\epsilon$  and  $\sigma$  by less than ±5% from the target values (typically better than ±3%) and are valid for TSL with deviations of up to ±10% if SAR correction is applied.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3–6 GHz at any distance larger than half the probe tip diameter from the boundary.

<sup>H</sup> The stated uncertainty is the total calibration uncertainty (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

**Parameters of Probe: EX3DV4 - SN:7700****Calibration Parameter Determined in HSL**

| <b>f (MHz)<sup>C</sup></b> | <b>Relative Permittivity<sup>F</sup></b> | <b>Conductivity<sup>F</sup> (S/m)</b> | <b>ConvF X</b> | <b>ConvF Y</b> | <b>ConvF Z</b> | <b>Alpha<sup>G</sup></b> | <b>Depth<sup>G</sup> (mm)</b> | <b>Unc<sup>H</sup> (k = 2)</b> |
|----------------------------|------------------------------------------|---------------------------------------|----------------|----------------|----------------|--------------------------|-------------------------------|--------------------------------|
| 6500                       | 34.5                                     | 6.07                                  | 5.68           | 5.50           | 5.54           | 0.20                     | 1.27                          | ±18.6%                         |

<sup>C</sup> Frequency validity is -600/+700 MHz at 6.5 GHz, ±700 MHz at or above 7 GHz, and ±150 MHz at 9.85 GHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


<sup>F</sup> The probes are calibrated using tissue simulating liquids (TSL) that deviate for  $\epsilon$  and  $\sigma$  by less than ±10% from the target values (typically better than ±6%) and are valid for TSL with deviations of up to ±10%.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz; below ±2% for frequencies between 3–6 GHz; and below ±4% for frequencies between 6–10 GHz at any distance larger than half the probe tip diameter from the boundary.



<sup>H</sup> The stated uncertainty is the total calibration uncertainty (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1526:2020.

## Frequency Response of E-Field

(TEM-Cell:ifl110 EXX, Waveguide:R22)

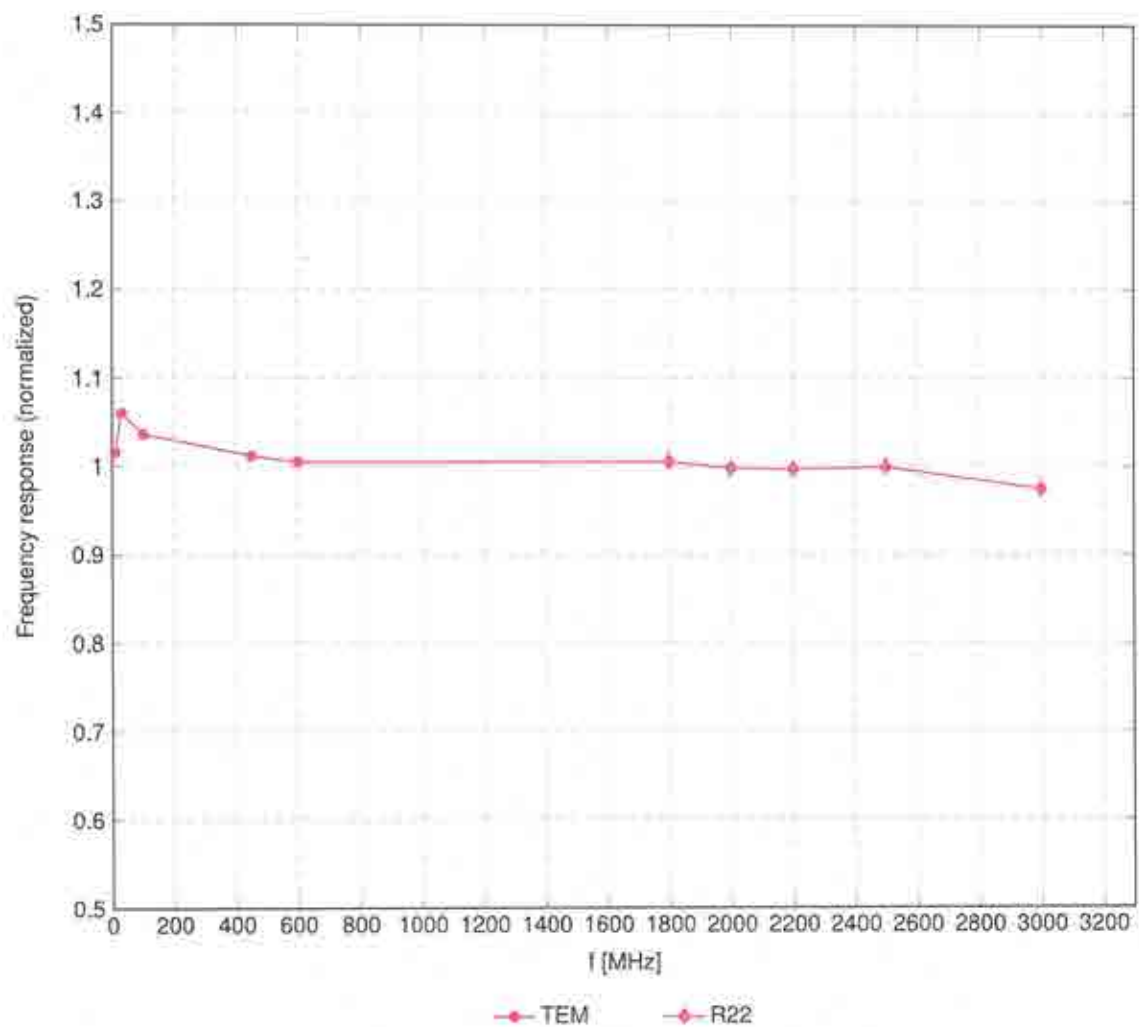

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

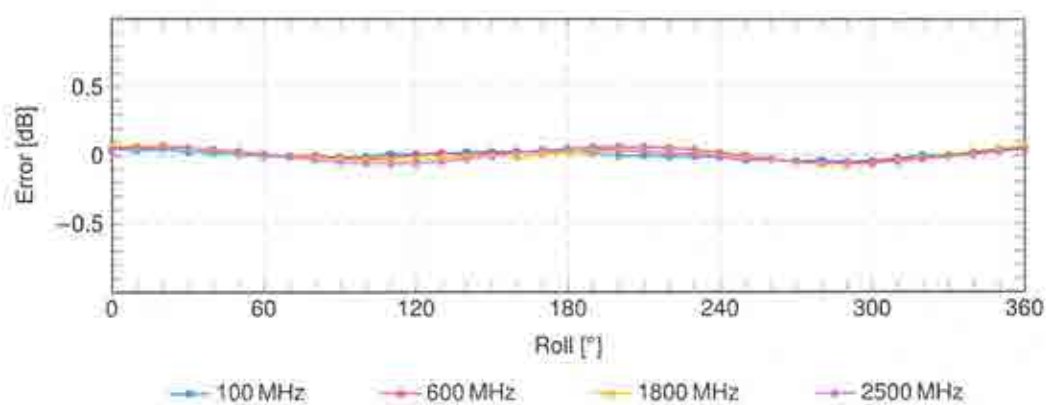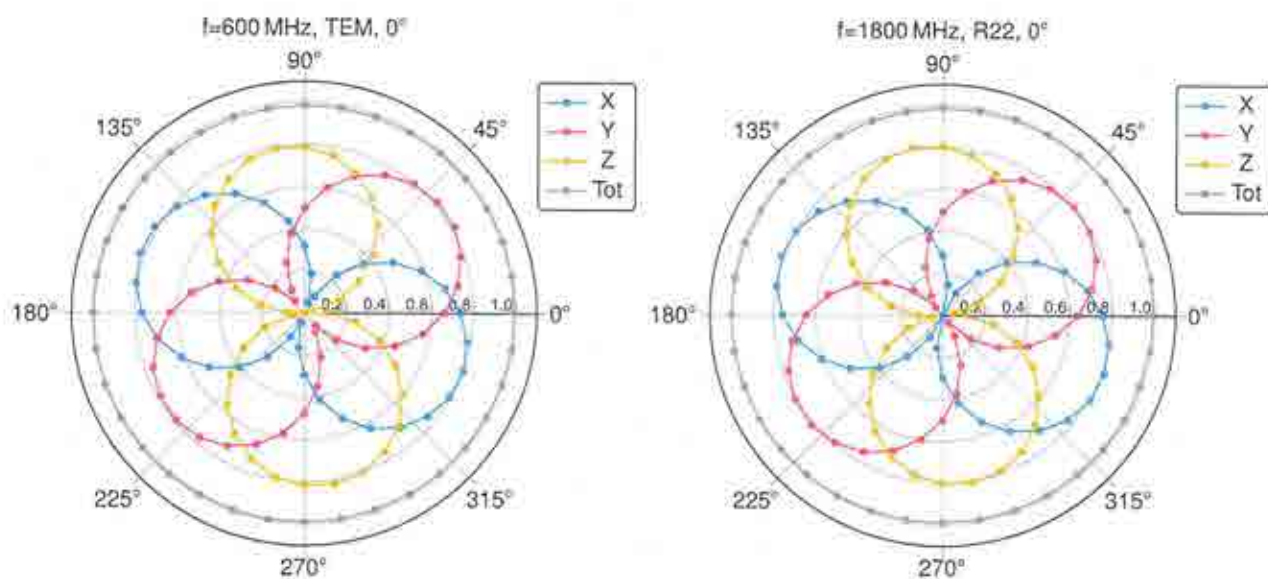Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$ Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )