

ollivia

User Manual

TheOllier S1 Beauty Device

Please read this manual carefully before using TheOllier S1 to ensure safe and proper operation.
Keep this manual for future reference.
If the illustrations in this manual differ from the actual product, please follow the actual product.

- Model : Ollier.S1
- Homepage : www.ollivia.kr



Table of Contents

1) Please Read Before Use

- Precautions Before Use 03

2) Introducing TheOllier S1

- Product Overview 05
- Components and Part Names . . . 06
- Device Controls 08
- LCD Display Indicators 09

3) User Guide

- UDM Key Functions 11
- Using the UDM Mode 12
- HFU Key Functions 15
- Using the HFU Mode 16

5) Charging Instructions

- Charging the Battery 19

6) Storage & Care Tips

- Main Unit Care 20
- Safety Precautions 21

7) Warranty & Service

- Warranty and Service Policy 23

8) INFORMATION


- Manufacturer Information 24

This manual is a general guide. Some components or images may differ from the actual product. The contents may be revised for product improvement without prior notice.

✱ **Please follow these instructions for your safety.**

Please read this manual carefully before using the product, and keep it for future reference.

Failure to follow the safety instructions may result in adverse effects, for which the company assumes no liability.

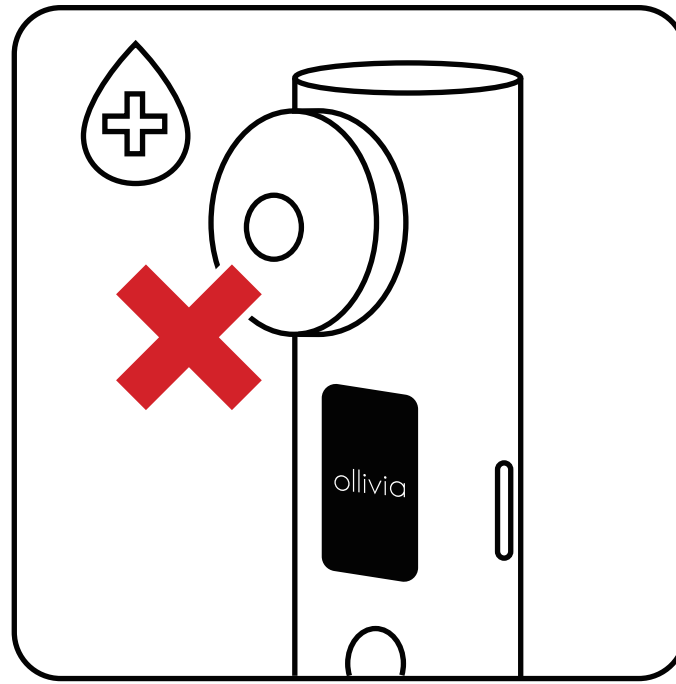


1. This product is not a medical device.




2. Remove the protective film from the head before use.




3. Do not use this device if you are underage, pregnant, or breastfeeding.

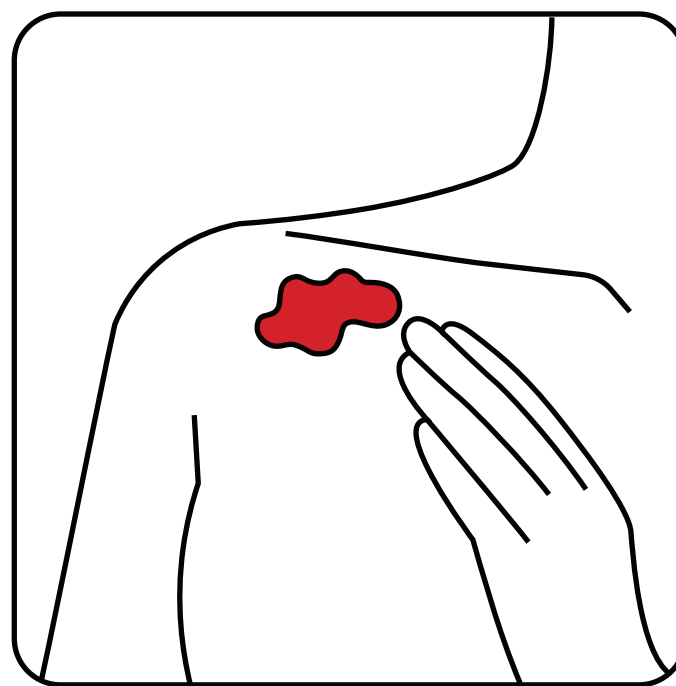

4. Do not use the device on areas with wounds, infections, boils, or other skin conditions.

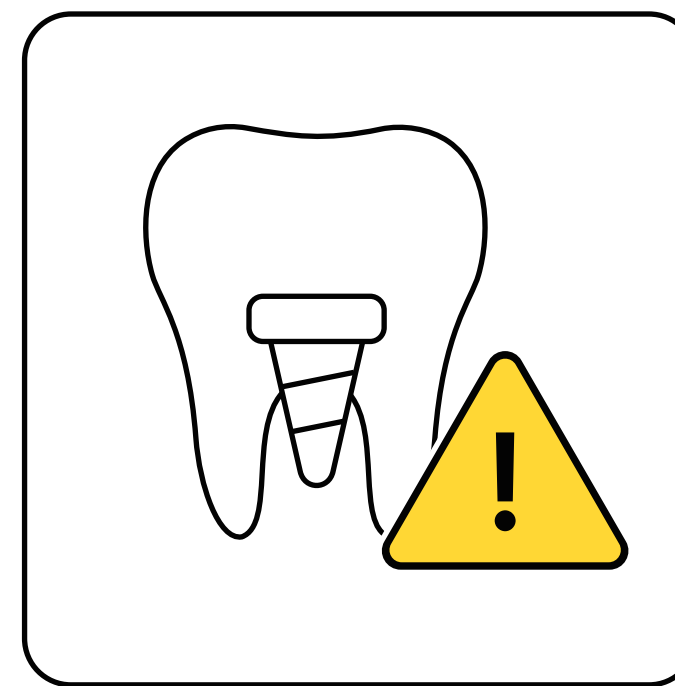

5. For dental treatments such as implants, nerve therapy, or orthodontics, consult a medical professional before use.

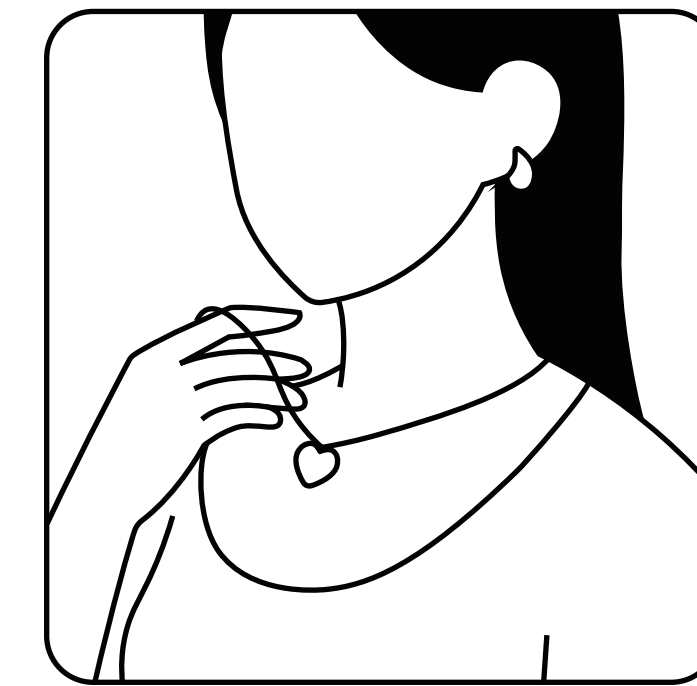


6. Remove all metal accessories such as necklaces and earrings before using the device.


❖ **Please follow these instructions for your safety.**

Please read this manual carefully before using the product, and keep it for future reference.


Failure to follow the safety instructions may result in adverse effects, for which the company assumes no liability.

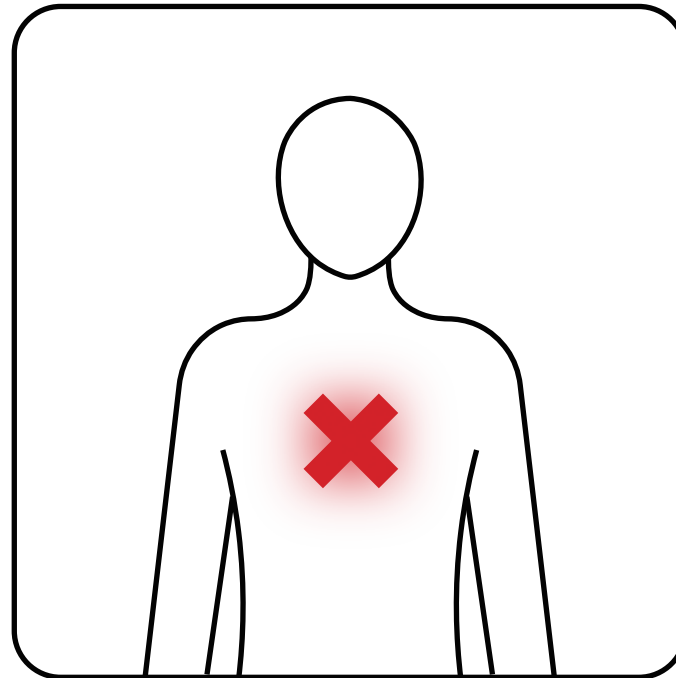


7. This device is intended for facial use only.
Do not apply it to other areas of the body.

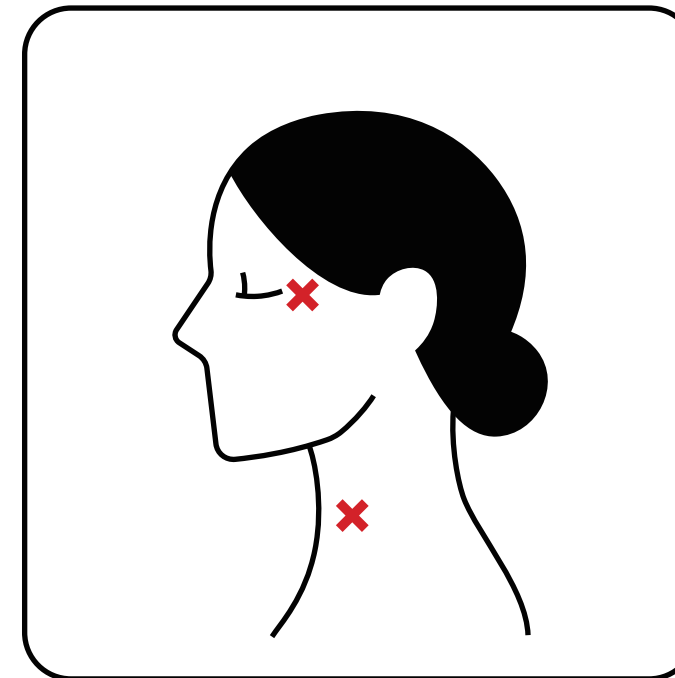


8. Do not use on or around the eyes,
or over the thyroid gland.

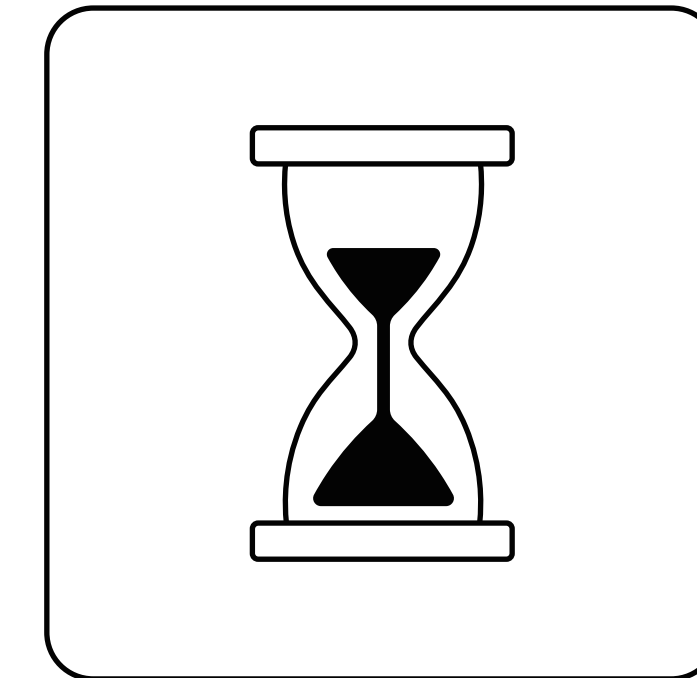


9. Do not leave the device on one area of the skin for too long,
as it may cause irritation.

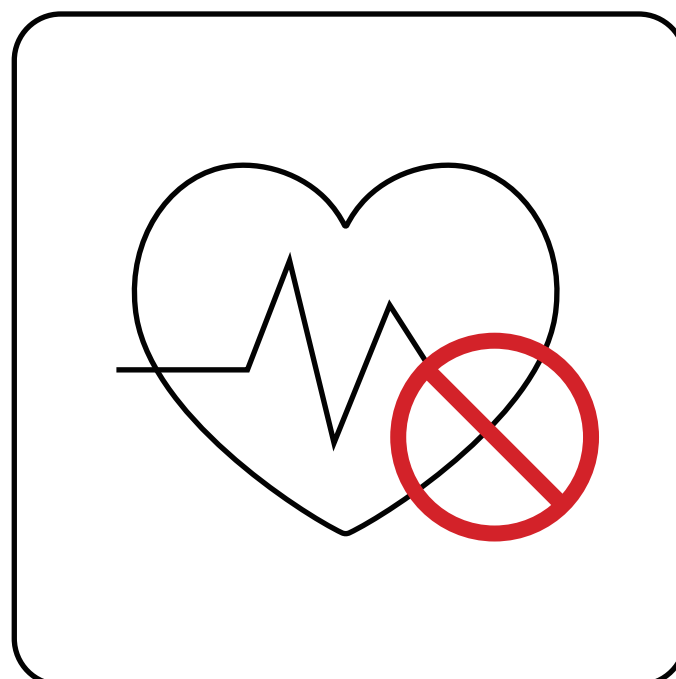

10. Do not use the device if you have a pacemaker,
implanted medical devices, or a history of serious illness,
or if you are currently receiving medical treatment.

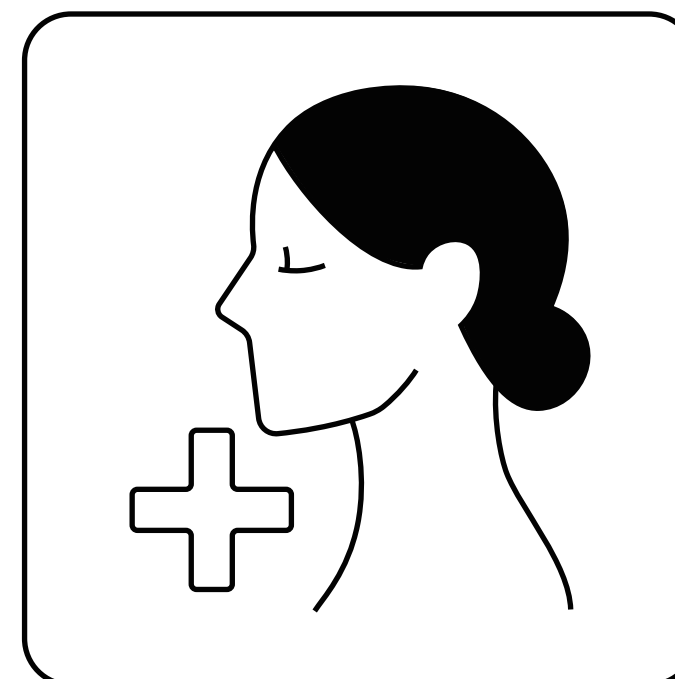

11. For all cosmetic procedures,
consult a medical professional before use.

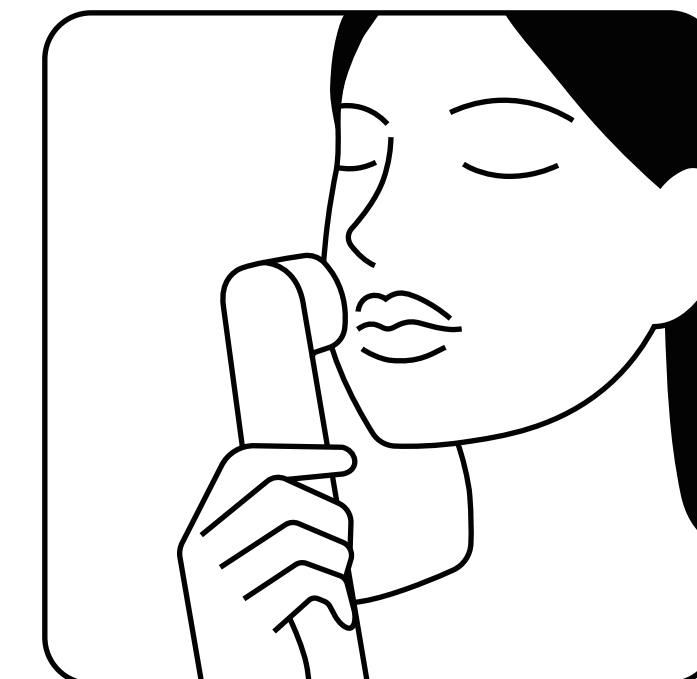

12. Prolonged use on a single area may cause irritation.
Adjust intensity according to your skin sensitivity.

Product Overview


Ollivia TheOllier S1 is a premium beauty device that incorporates core technologies commonly found in professional aesthetic equipment. Utilizing HIFU and UDM ultrasound technologies, it delivers precise energy deep into the skin to improve elasticity, hydration, radiance, and provide anti-aging effects. Its system also supports superficial lymphatic care, providing a professional-grade skincare experience as part of your daily routine.

◆ Effects of TheOllier S1 Treatment

*The effectiveness of this product has been verified through clinical data.

Skin tightening & firming

Improves sagging contours
by enhancing skin elasticity from within.

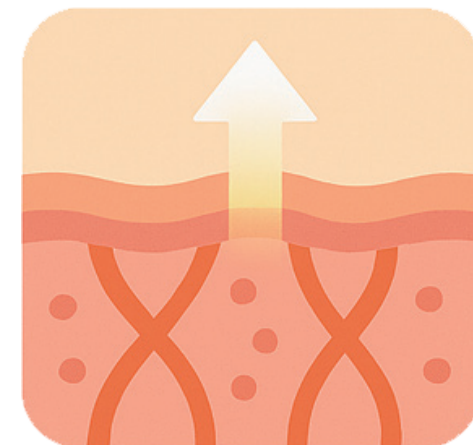


Enhanced surface & deep hydration

Delivers long-lasting moisture deep into the skin,
leaving it soft, hydrated, and free from tightness.




Radiance boost & wrinkle care

Used with the gel, hyaluronic acid is absorbed evenly,
boosting hydration, firmness, and smoothing wrinkles.

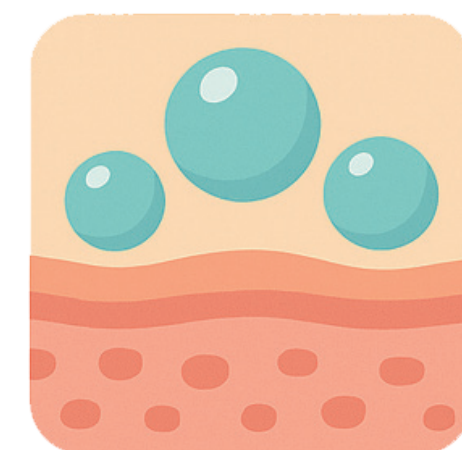

Lymphatic Massage

Raises muscle and tissue temperature,
boosting circulation and lymphatic flow.

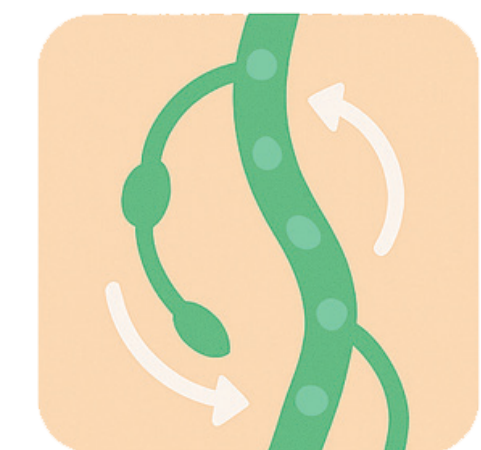




Components and Part Names

Product specifications and components may change without prior notice to improve performance or functionality.


Model Name	Ollier.S1 (WOO-S200WV)	Product Name	TheOllier S1
Product Dimensions	W48 x H198 x D57 mm	Product / Head Weight	Approx. 275g/47g(UDM), 26g(HFU)
Rated Voltage	DC 5V2A	Battery	2400mAh
KC CODE	R-R-TWAY-Ollier-S1	LCD	1.14inch (135 x 240 px)
Charging Cable	C-TYPE	Run Time	Approx. 150 min *Based on Level 5, per full charge
Charging Time	Approx. 180 min *From fully discharged to fully charged	Date	Specified separately
Mfr / Dist.	Thatway Inc. / Beautyway Inc.	Support Center	+82 031-8067-6453
Service Center	+82 031-8067-6453		

Components and Part Names

◆ Package Contents

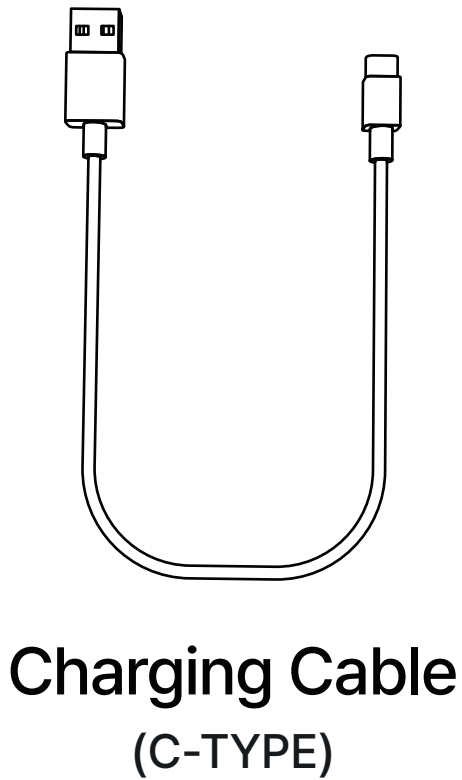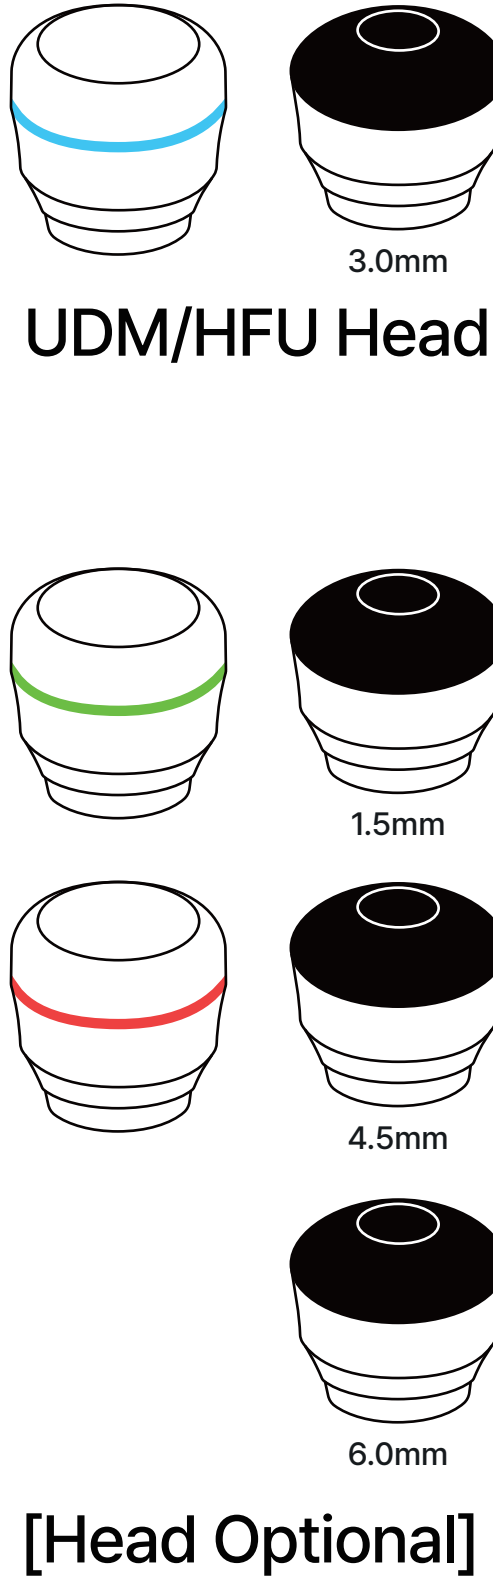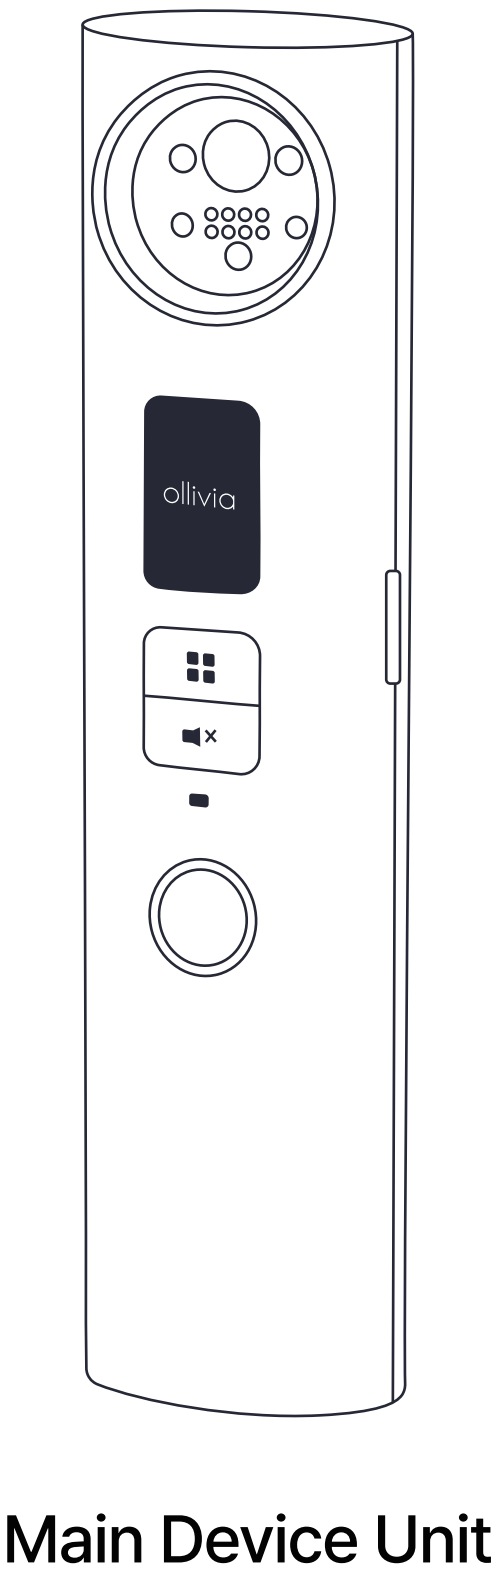


◆ Device Components

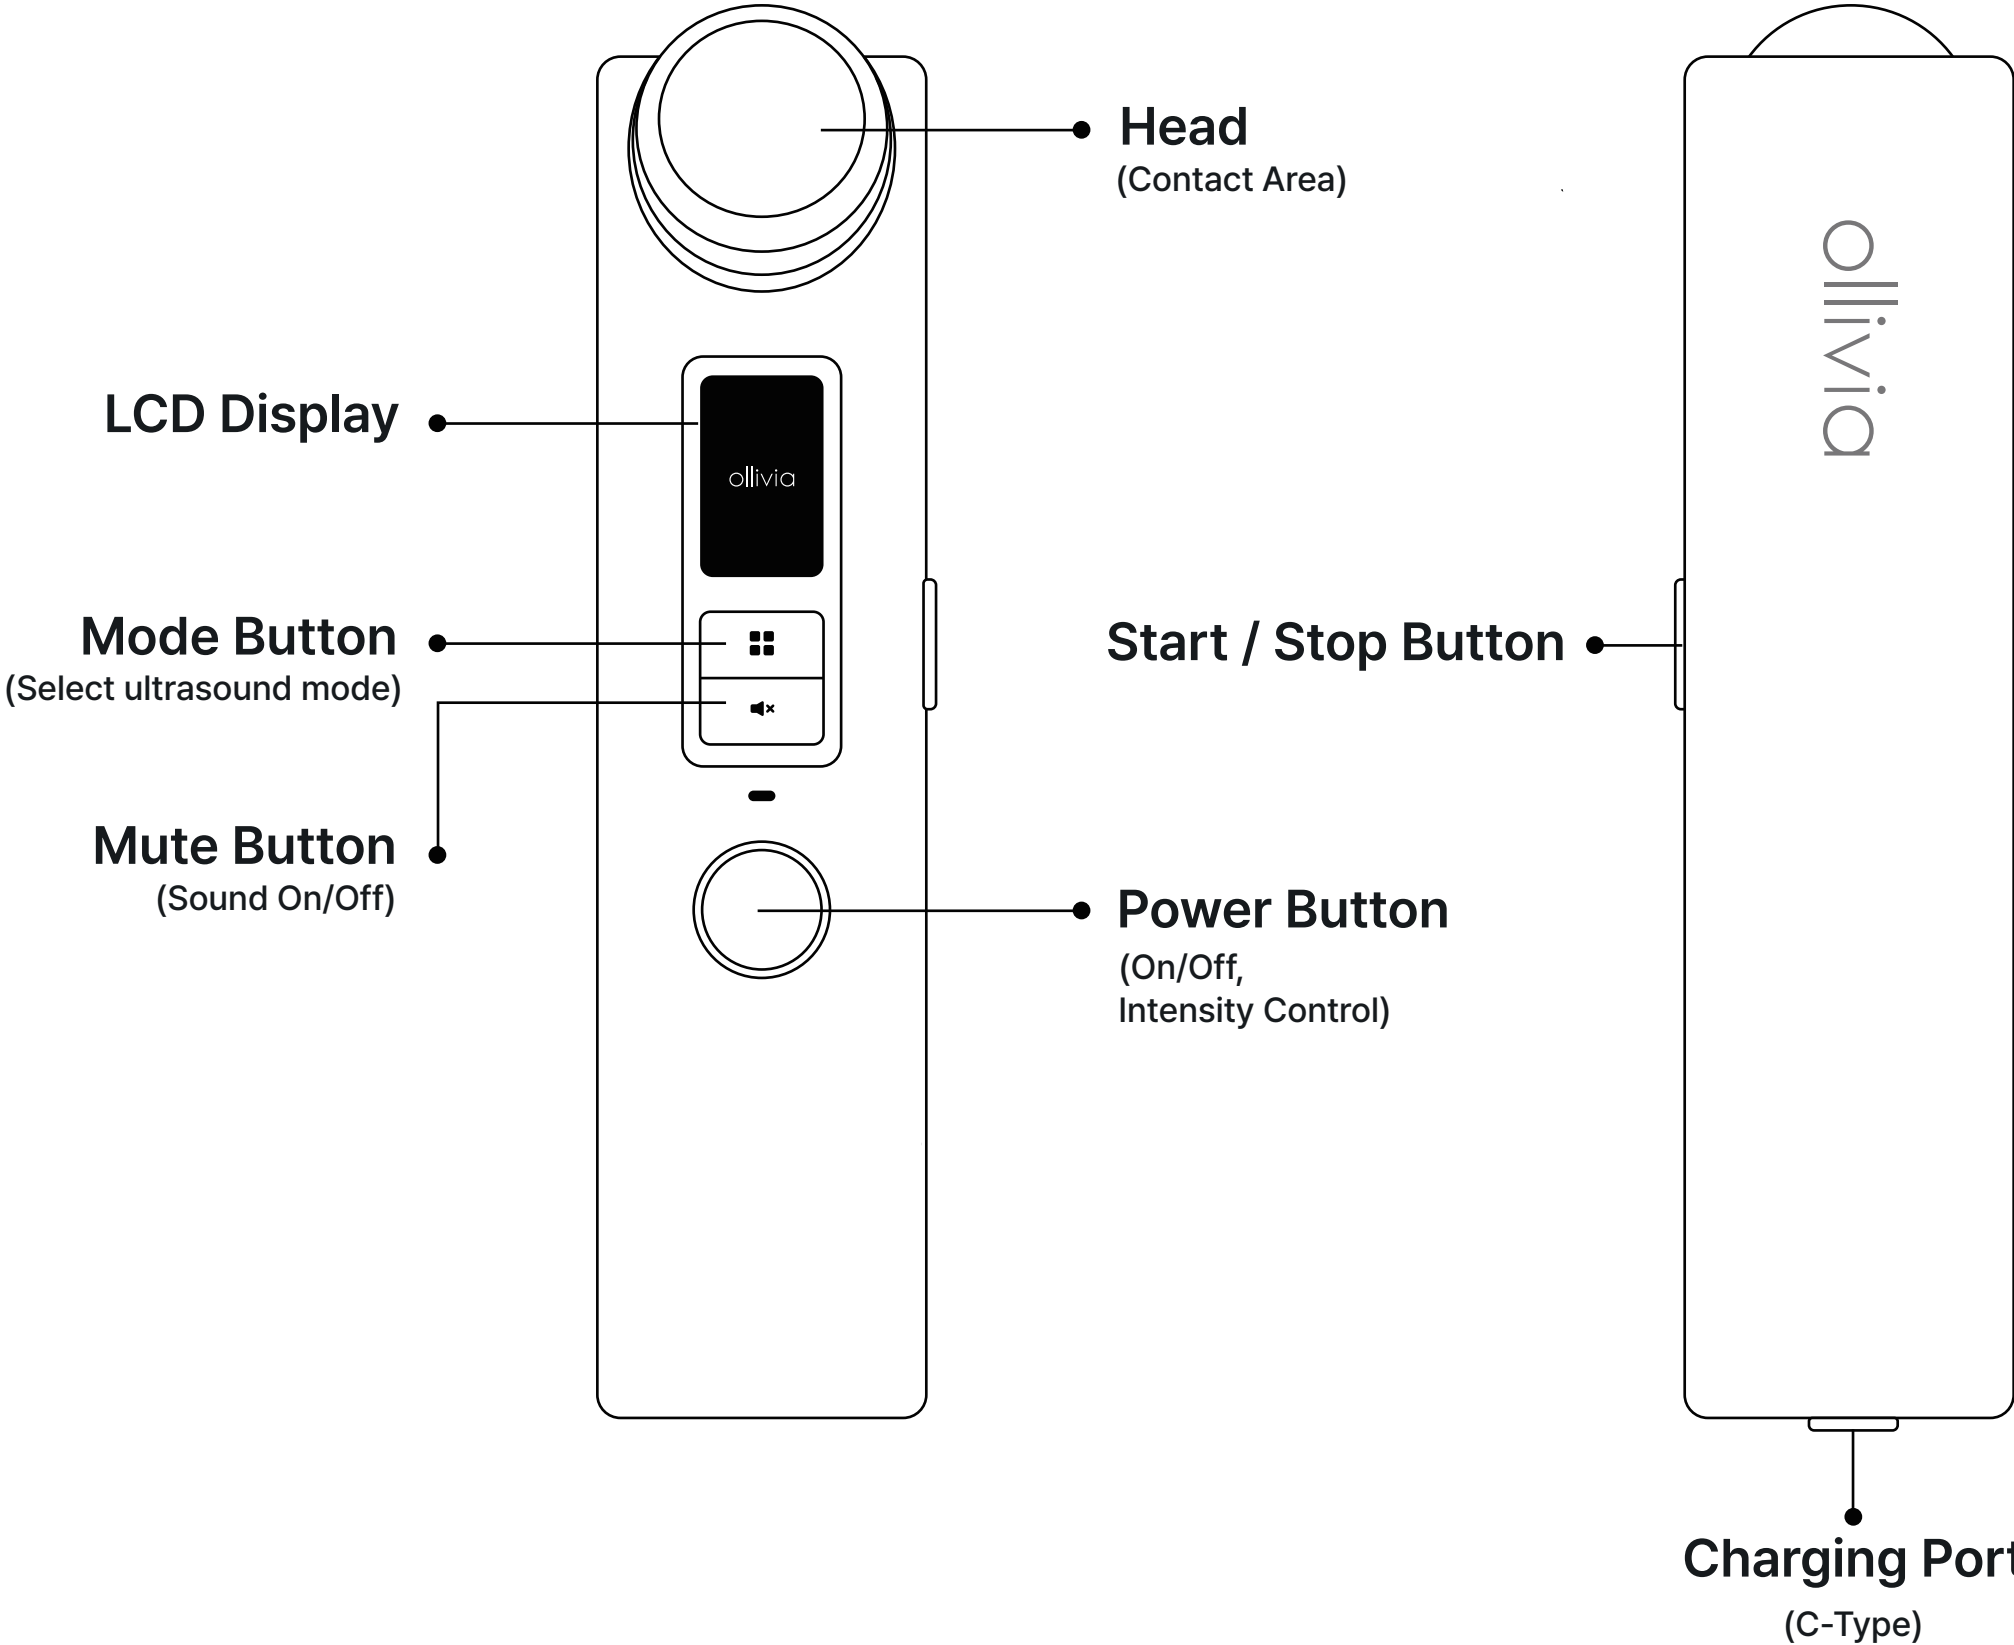

Device Controls

◆ How to Use

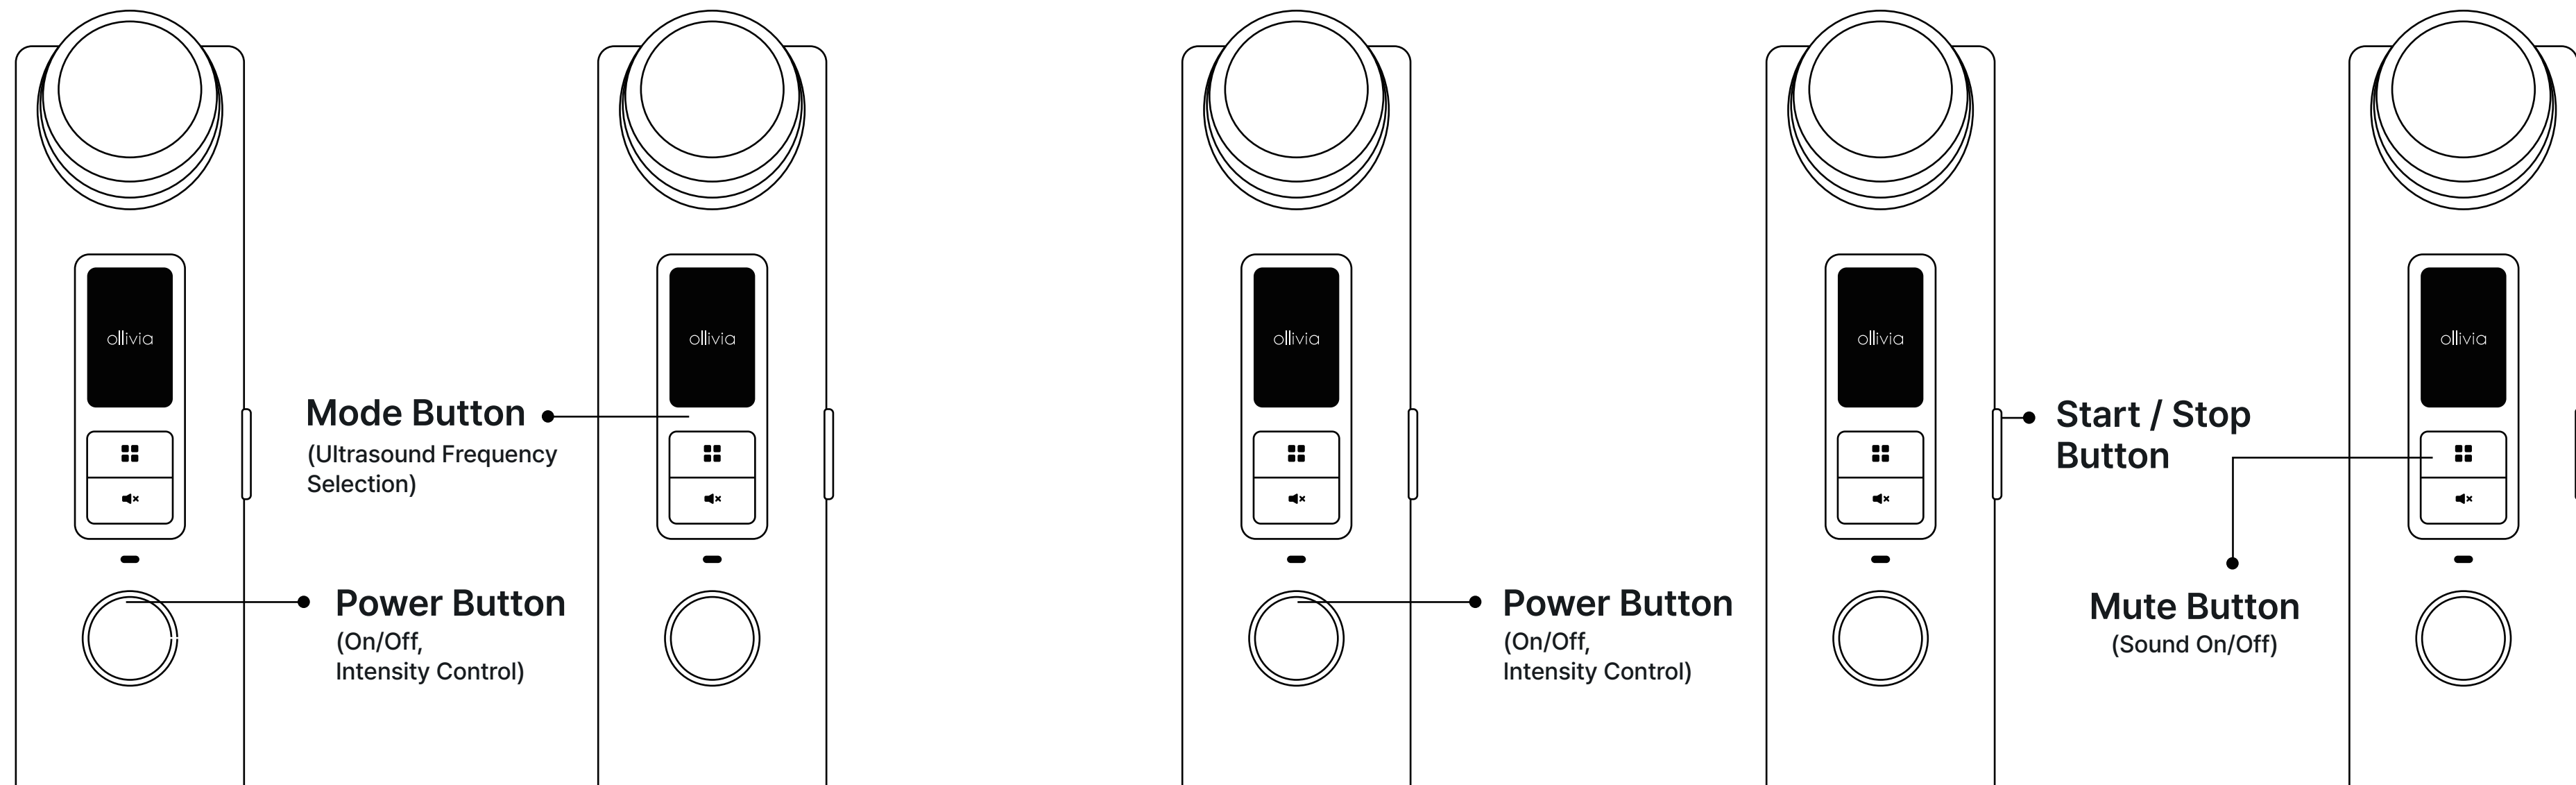

1 Power ON

Press and hold the Power Button for 3 seconds to turn the device on.

3 Mode Selection

Press the Mode Button [⋮] briefly to select the ultrasound mode.

4 Intensity Adjustment

Press the Power Button briefly to adjust the intensity from Step 1 to Step 5.

5 Start Operation

Press the Side Button briefly to start the operation.

7 SOUND ON/OFF

Press the Mute Button [🔊×] to turn the sound ON or OFF (mute).


2 Power OFF

Press and hold the Power Button for 3 seconds to turn the device off.

6 Pause Operation

While operating, press the Side Button briefly to pause the treatment.


LCD Display Indicators

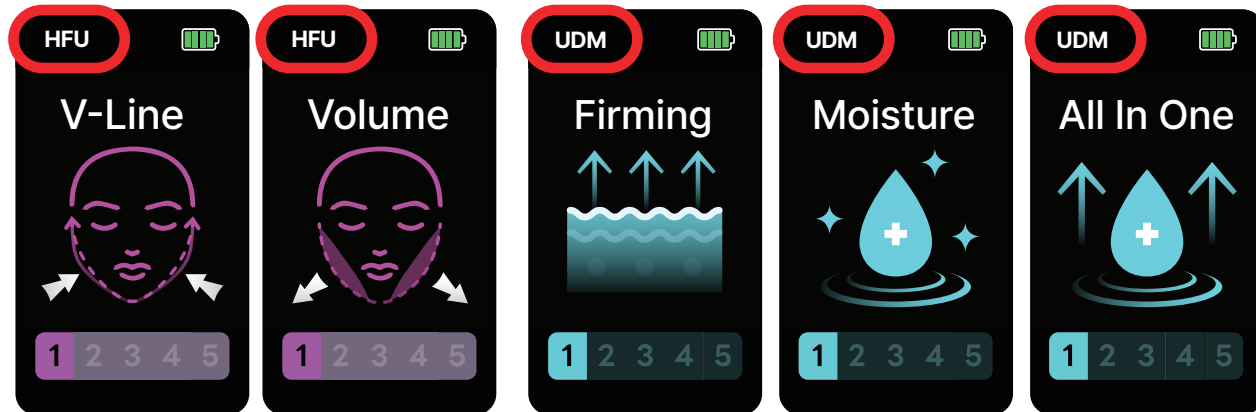

1 Frequency Indicator

Shows the selected treatment mode (HFU or UDM)

HFU: V-Line Care, Volume Care / UDM: Firming Care, Moisture Care, All In One Care

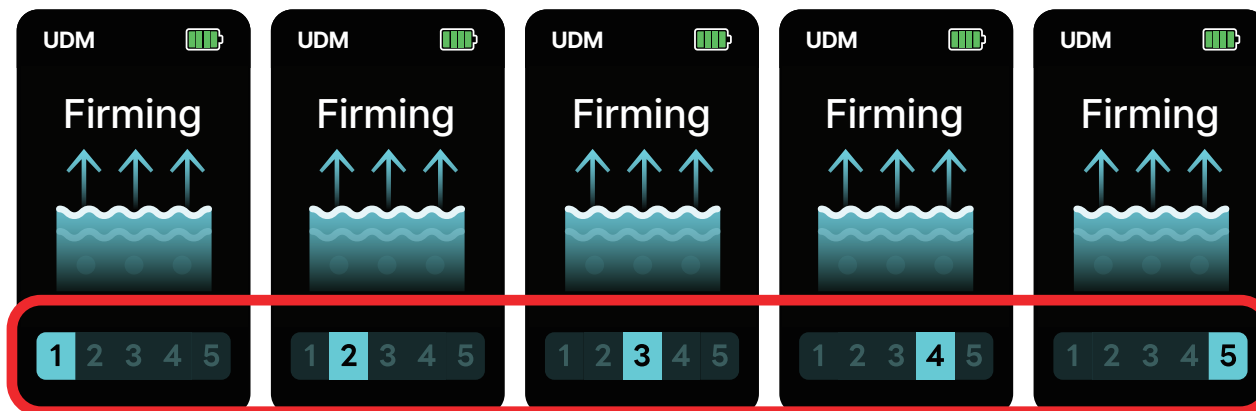


2 Intensity Level Indicator

The selected intensity level (1 to 5) is shown

Step 1 : The gentlest setting. Recommended for sensitive skin or first-time users.

Step 2 : Low intensity. Suitable for delicate or sensitive areas. **Step 4** : High intensity. Ideal for targeted care and skin firming.

Step 3 : Medium intensity. Standard setting ideal for daily care. **Step 5** : The highest setting. Recommended for intensive lifting and firming.

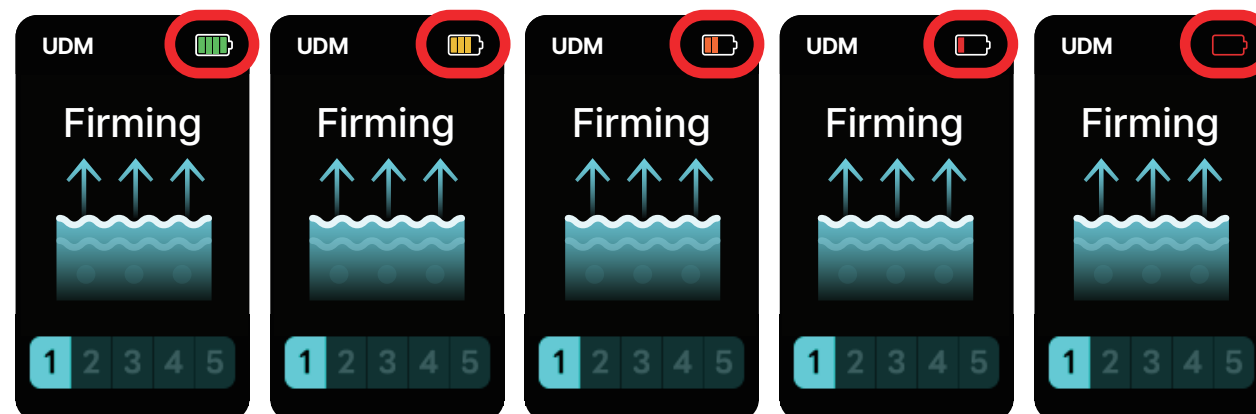


3 Battery Level Indicator

All functions support five intensity levels (Step 1 to Step 5)

 Full : Fully charged  High : Sufficient battery remaining  Mid : Approximately 50% remaining

 Low : Low battery  Empty : Battery depleted

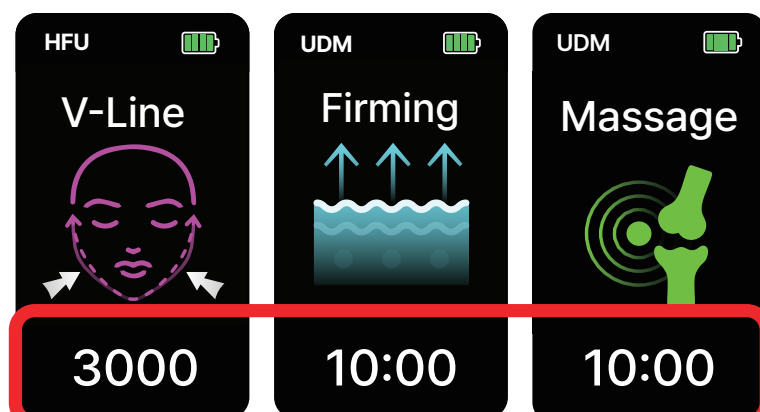


4 Treatment Time Indicator

The remaining time or shot count is displayed depending on the mode

HFU: Shows remaining shots (default: 3000 shots)

UDM: Displays remaining time (default: 10 minutes)

LCD Display Indicators

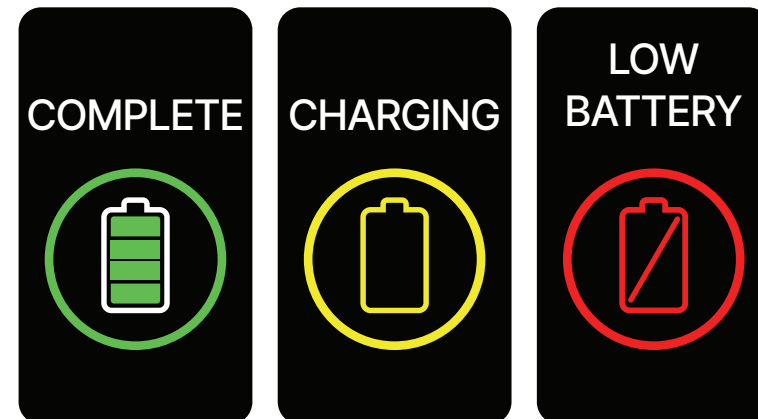

5 Charging Status Indicator

The battery status (Charging, Complete, or Low Battery) is displayed when charging via C-type



6 Gyroscope Function Indicator

The gyroscope icon appears based on the tilt or orientation of the device.


◆ HFU Mode

Operation stops automatically if no movement is detected for more than 10 seconds.

❖ Refer to the HFU gyro angle image on page 16


◆ UDM Mode

The device automatically shuts down after 1 minute of inactivity.

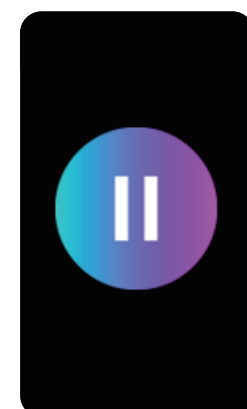

7 Pause Status Indicator

The "Pause" icon appears when the device is in a paused state.

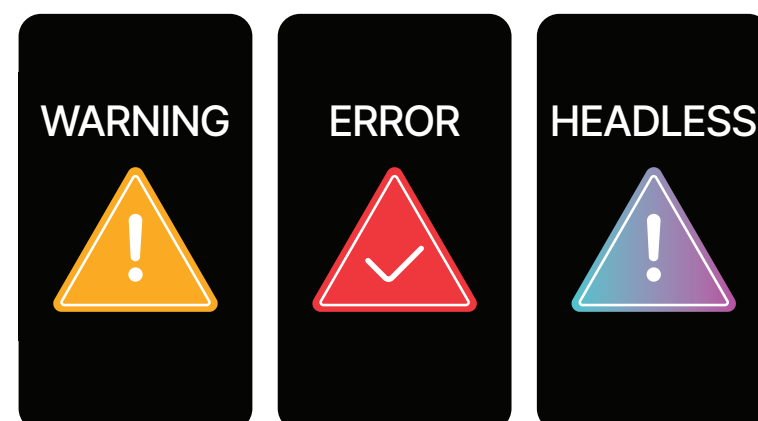

8 System Alert Indicator


A system-wide alert icon notifies the user of abnormal device conditions.

- Warning: If a risk or malfunction is detected, stop use immediately and refer to the safety instructions.
- Error: If an internal error occurs, turn off the device and restart. If the issue persists, contact customer support.
- Head Not Detected: If the treatment head is not properly attached, reattach it securely and try again.

UDM Key Functions

◆ Ultrasonic Dynamic Massage (UDM)

The UDM function of TheOllier S1 delivers precise and gentle energy to multiple skin layers by alternately emitting 3MHz and 10MHz frequencies. It helps stimulate collagen production, improve skin elasticity, and support deep hydration and radiance.

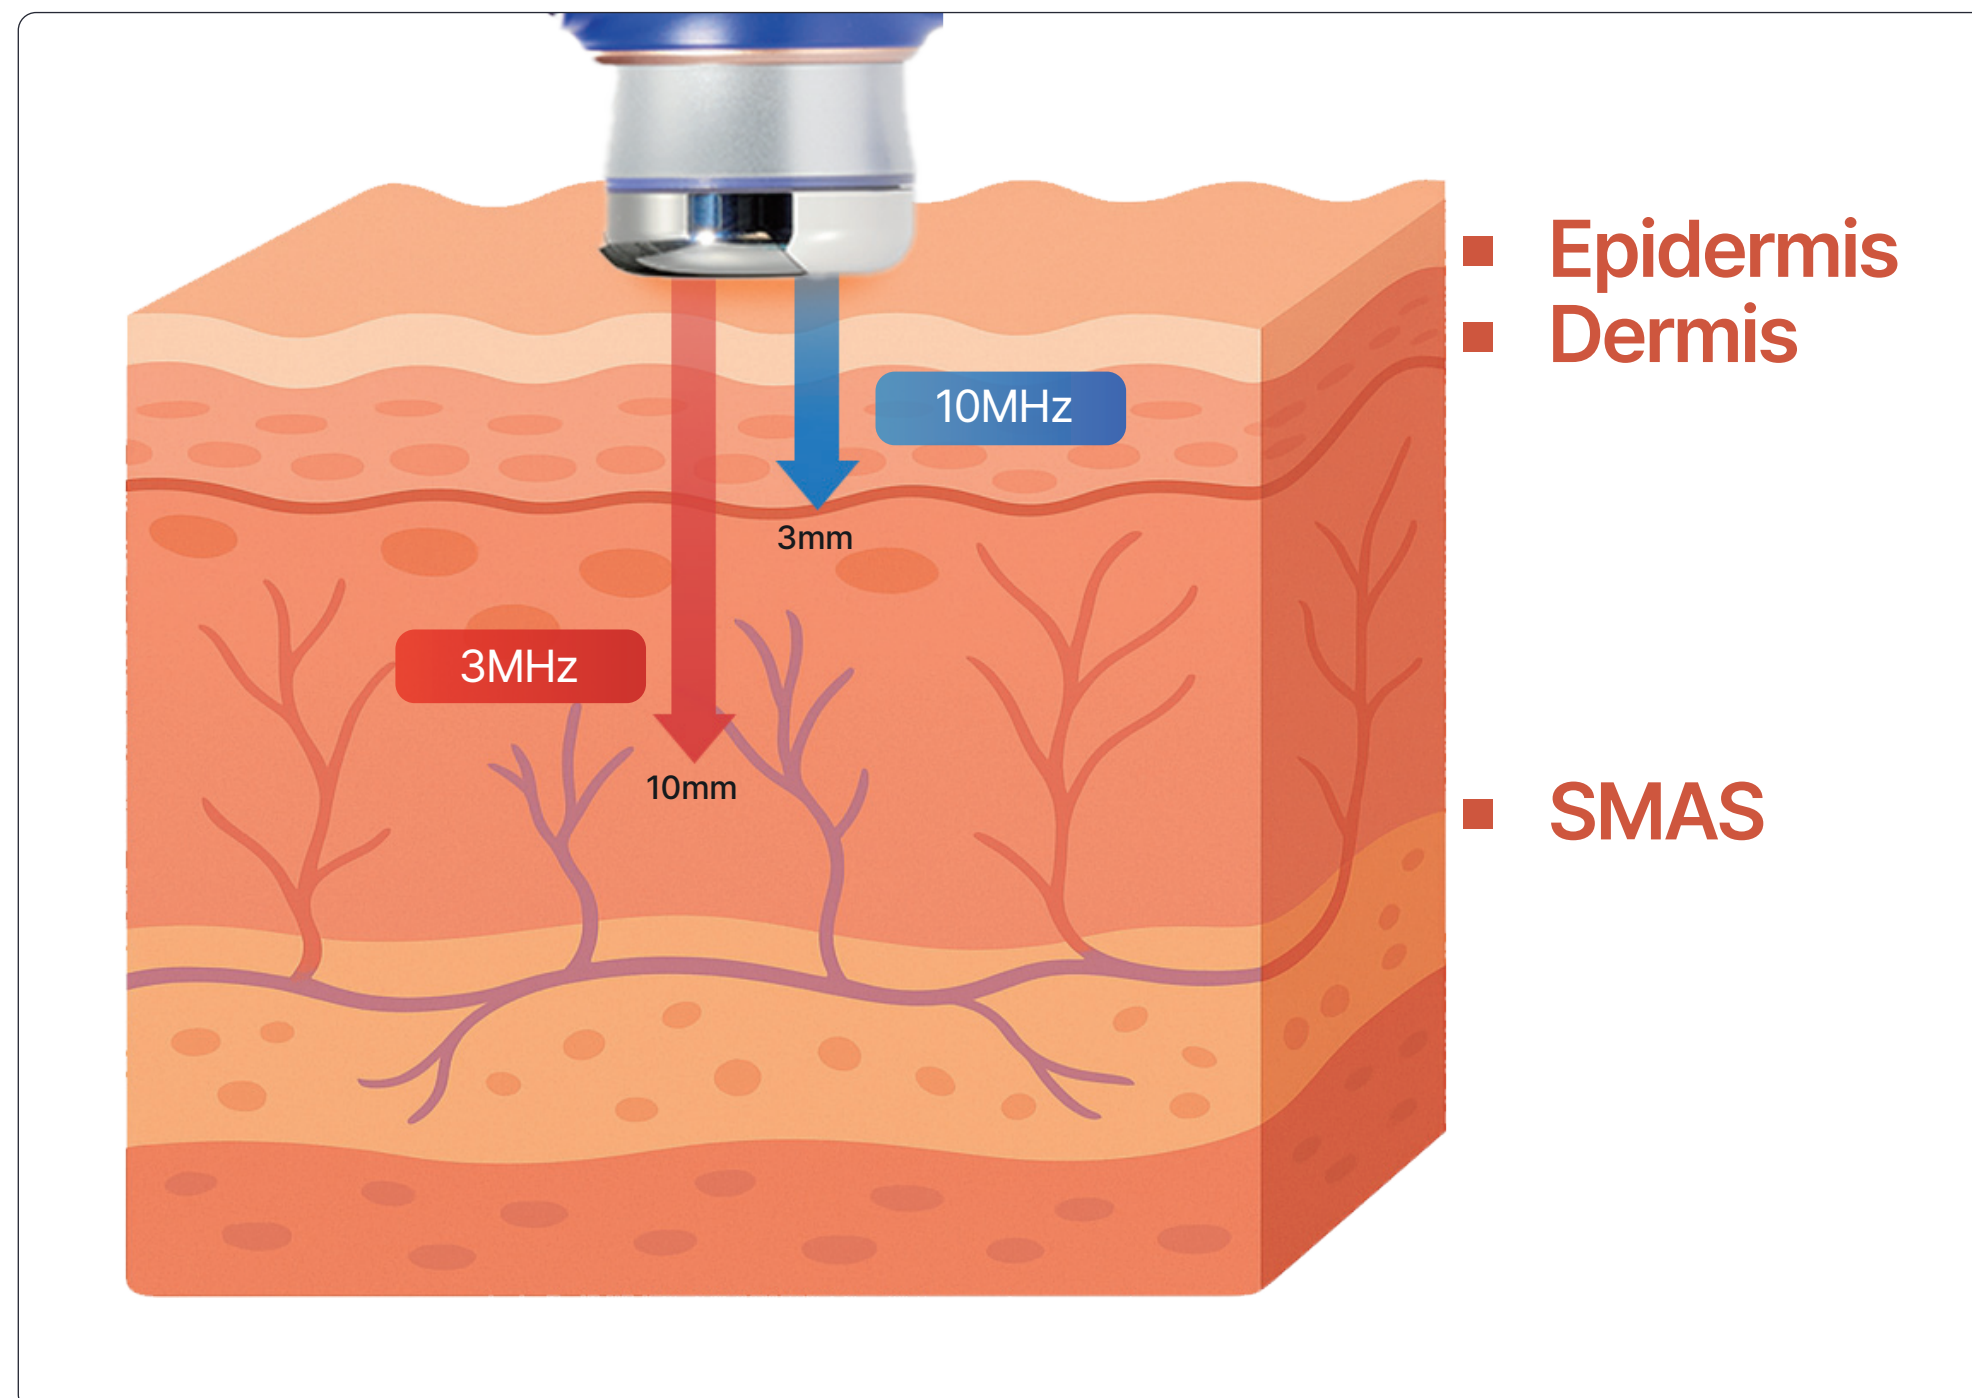

3MHz	10MHz	3MHz+10MHz
- Firming - Lifting Care	- Moisture Glow - Soothing Care	- Firming / Lifting Care - Moisture Glow / Soothing Care
3MHz		10MHz
Vibration		
3 million vibrations per second (3 MHz)		10 million vibrations per second (10 MHz)


Please check the following before use!

- If you normally wear glasses, be sure to remove them before using the device.
- Remove the protective sticker from the treatment head before use.
- Do not use the device near the thyroid gland or around the eyes.

Using the UDM Mode


Ensure you understand the UDM usage guidelines and precautions before treatment.

*Note Before Using UDM Mode

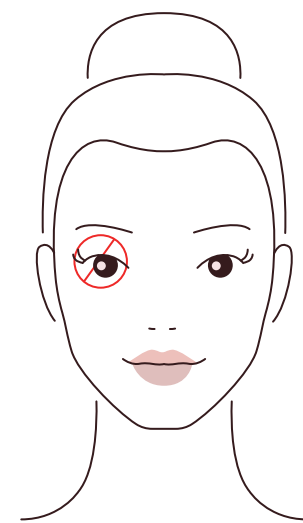

Prohibited Areas of Use

Do not use the device around the eyes.

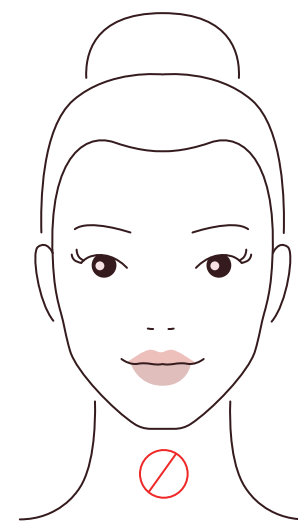


Prohibited Areas of Use

Do not use the device over the thyroid area.



Pre-Treatment

Cleanse the skin thoroughly before use.




Usage Frequency

Recommended daily use:
10 minutes



Accessory Precaution

Remove metal accessories before use (e.g. necklace, earrings).

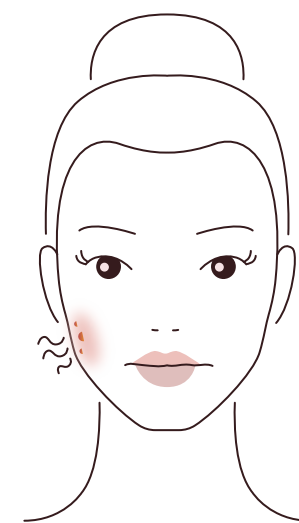


Intensity Adjustment

If you experience discomfort or skin irritation, reduce the intensity level.


UDM Mode (Frequency Setting)

Three frequency options are available.

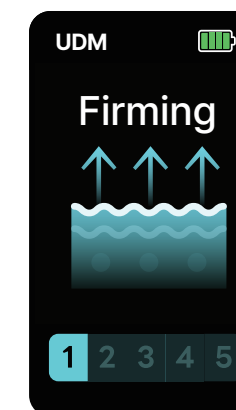

3MHz

Firming Care · Lifting Care · Anti-Aging Care
Blemish Care / Trouble Care · Swelling Care / De-Puffing Care
3 million vibrations per second / Penetrates up to 10mm

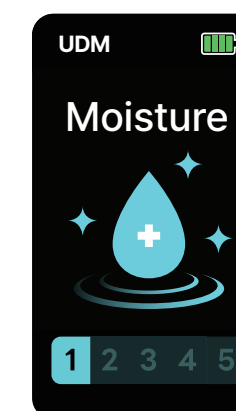

10MHz

Moisture Glow Care · Soothing Care · Hydration Care
Pore Care · Redness Care · Brightening Care
10 million vibrations per second / Penetrates up to 3mm









3MHz + 10MHz

Lymphatic Circulation · Skin Regeneration
Optimal Combination: Dual-Frequency Ultrasound
(Recommended for Use)

Using the UDM Mode

◆ How to

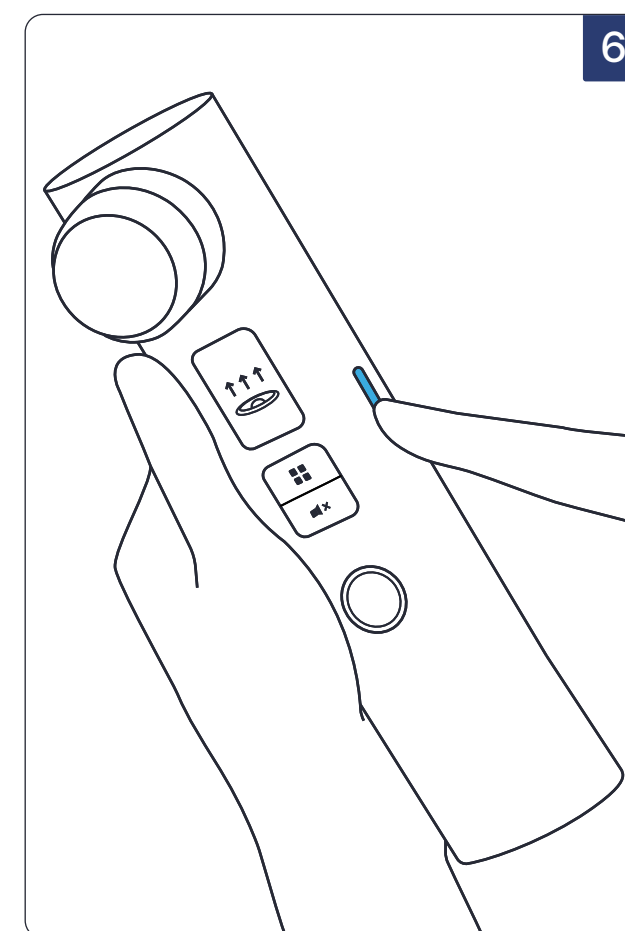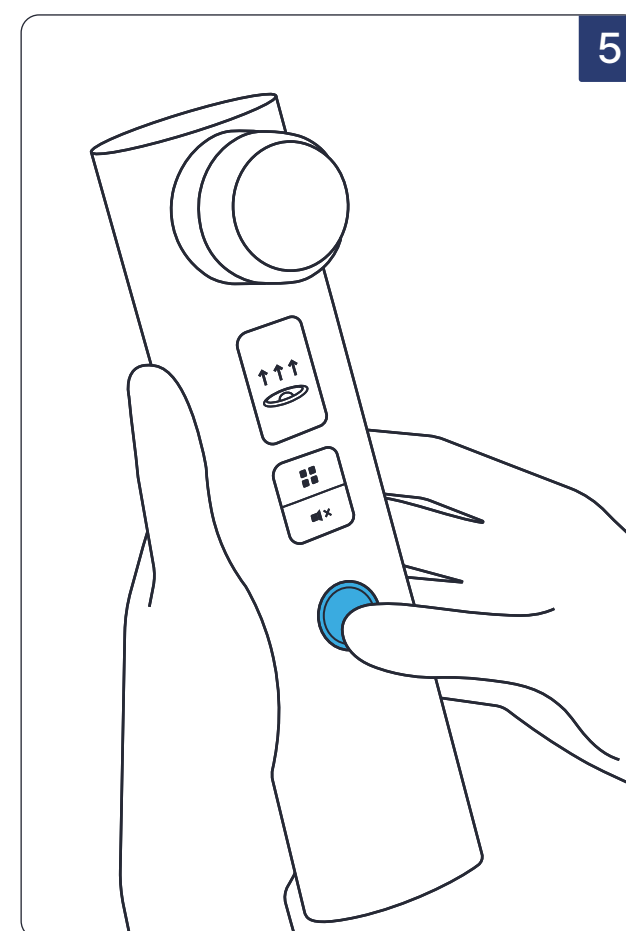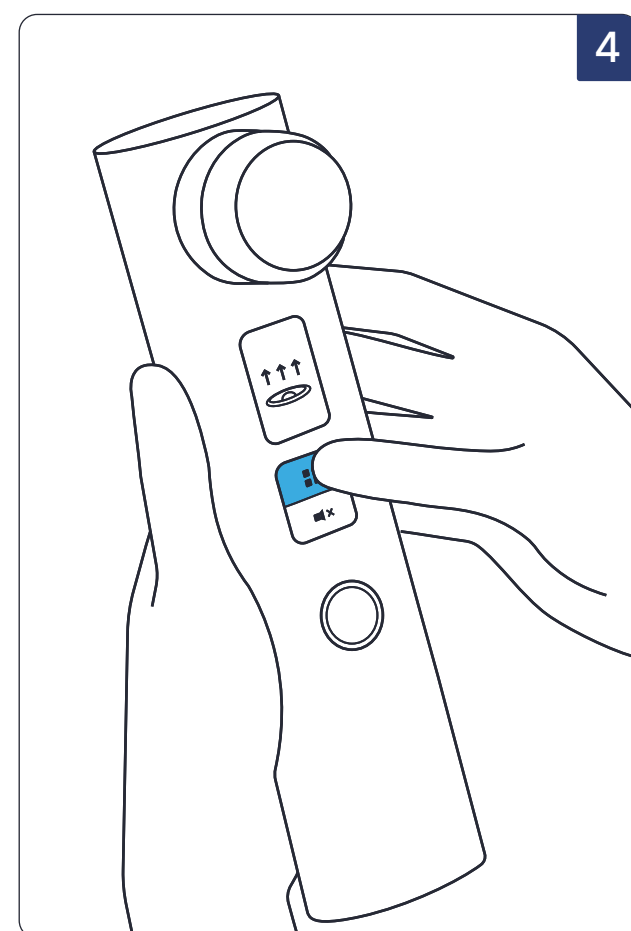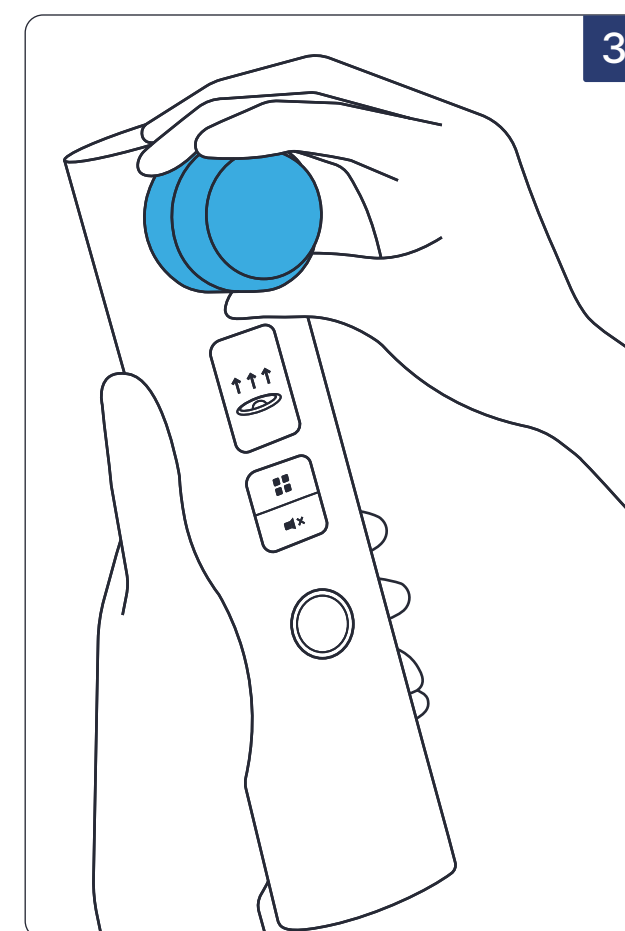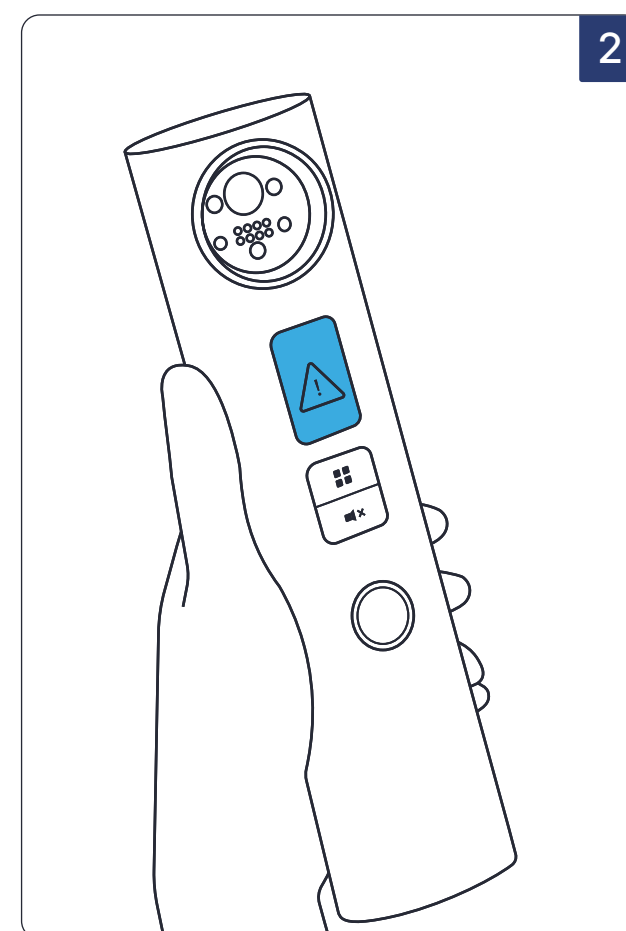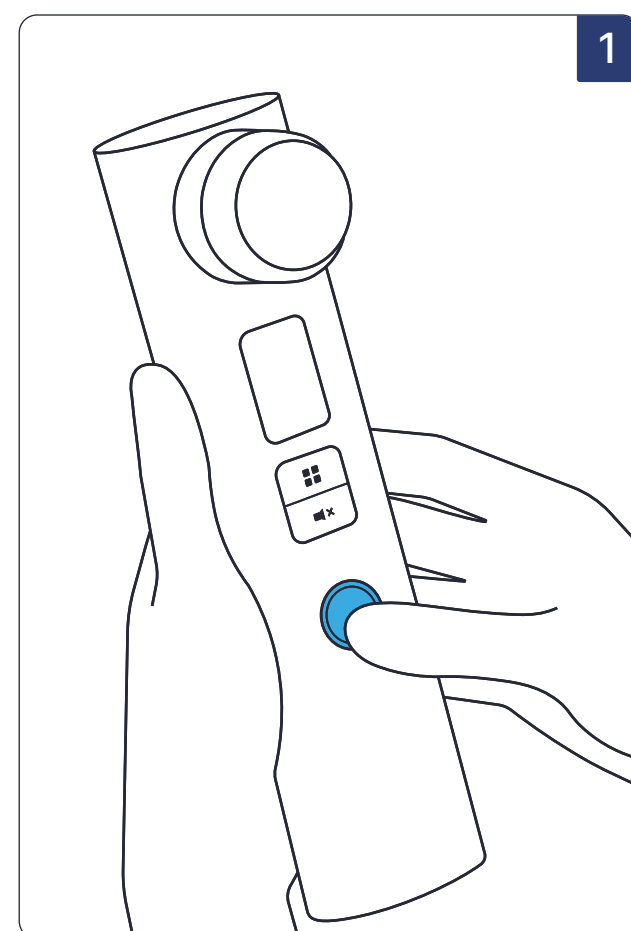

1 Power On/Off

Press and hold the Power Button to turn on the ollivia the Ollier S1
Press and hold again to power it off.

2 Head Detection Warning

If the UDM head is not attached when the device is powered on,
the LCD screen will display a "Head Not Detected" message.

3 Attaching the UDM Head

Once the UDM head is attached,
the UDM function will be automatically activated.

4 Mode Selection

Press the [■] to select one of the three available UDM modes.

5 Intensity Adjustment

Press the Intensity Button to select the desired level (1 to 5).
Level 3 is commonly recommended for most users.
If skin irritation is felt, reduce to a lower intensity level.

6 Start and Pause

Press the Side Button briefly to start operation.
To pause during operation, press the button again.

Using the UDM Mode

◆ Recommended UDM Routine (Full Face Application)

Please read all safety precautions before using the device.




STEP 01

Apply Gel

Generously apply gel or ampoule to the treatment area.

Tip. For enhanced results, use with Ivilro Ollier Steam Booster Water Gel

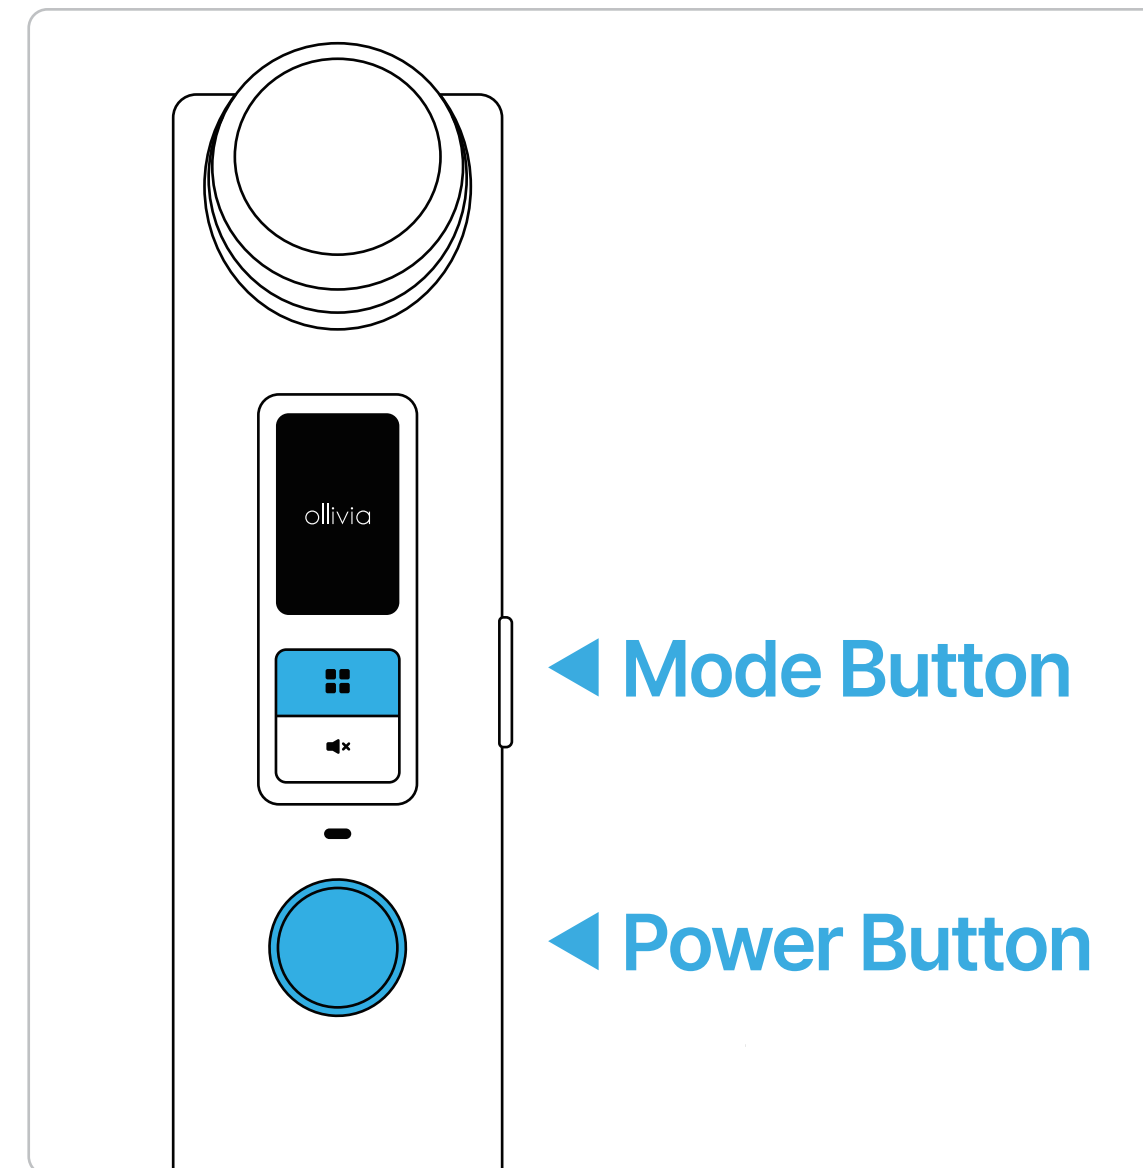


STEP 02

Set Frequency & Intensity

Use the mode button [⌘] and power button to select the desired frequency and intensity.

Recommended mode : All-in-One Care
Recommended intensity: Step 1-3

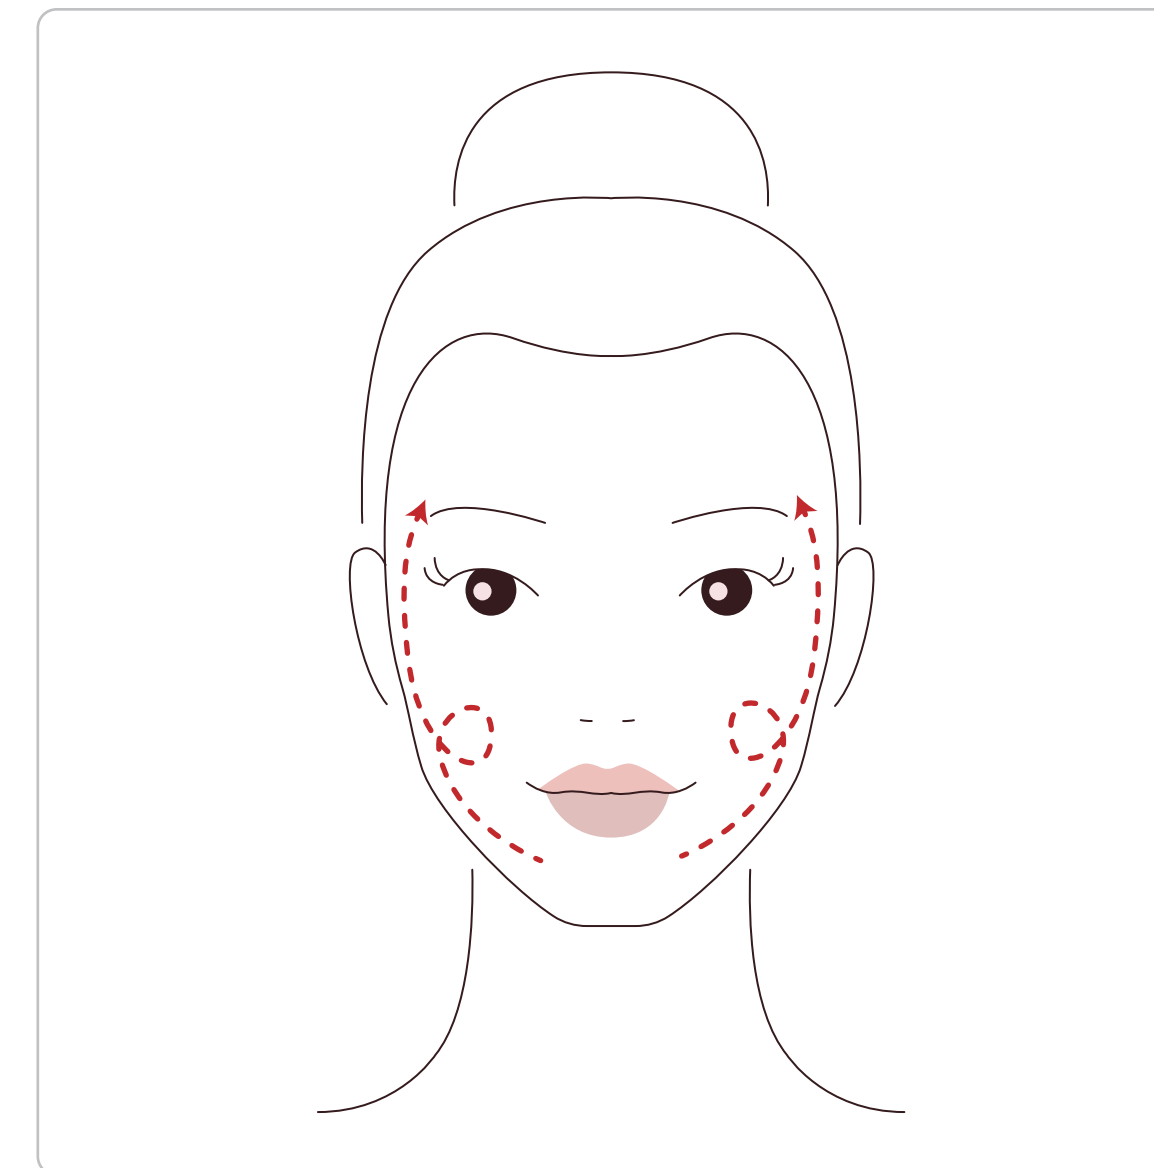


STEP 03

Full-Face Treatment

Start from the jawline or concern areas, then move across the cheeks, eyes, and forehead. Glide the device gently for 10 minutes to boost absorption and improve glow and elasticity.

Tip. Use liquid-type skincare products instead of thick creams.

Scan the QR code below to view detailed video instructions for using TheOllier S1 device.

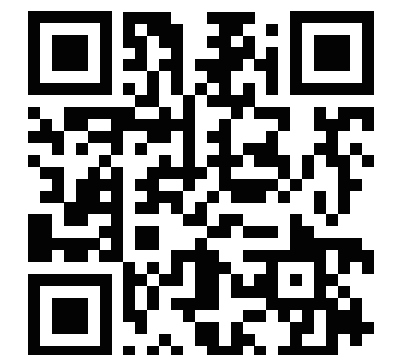

[How to Scan]

Open the camera app on your smartphone. Point the camera at the QR code, and a link will automatically appear. Tap the link to view the user manual.


[If Scanning Fails]

If the QR code is not recognized, adjust the lighting or refocus your camera, then try again.

HFU Key Functions

◆ High Focused Ultrasound(HFU)

HFU delivers focused ultrasound to the dermis, creating thermal points for collagen regeneration. It firms sagging contours non-invasively, without cuts or irritation.

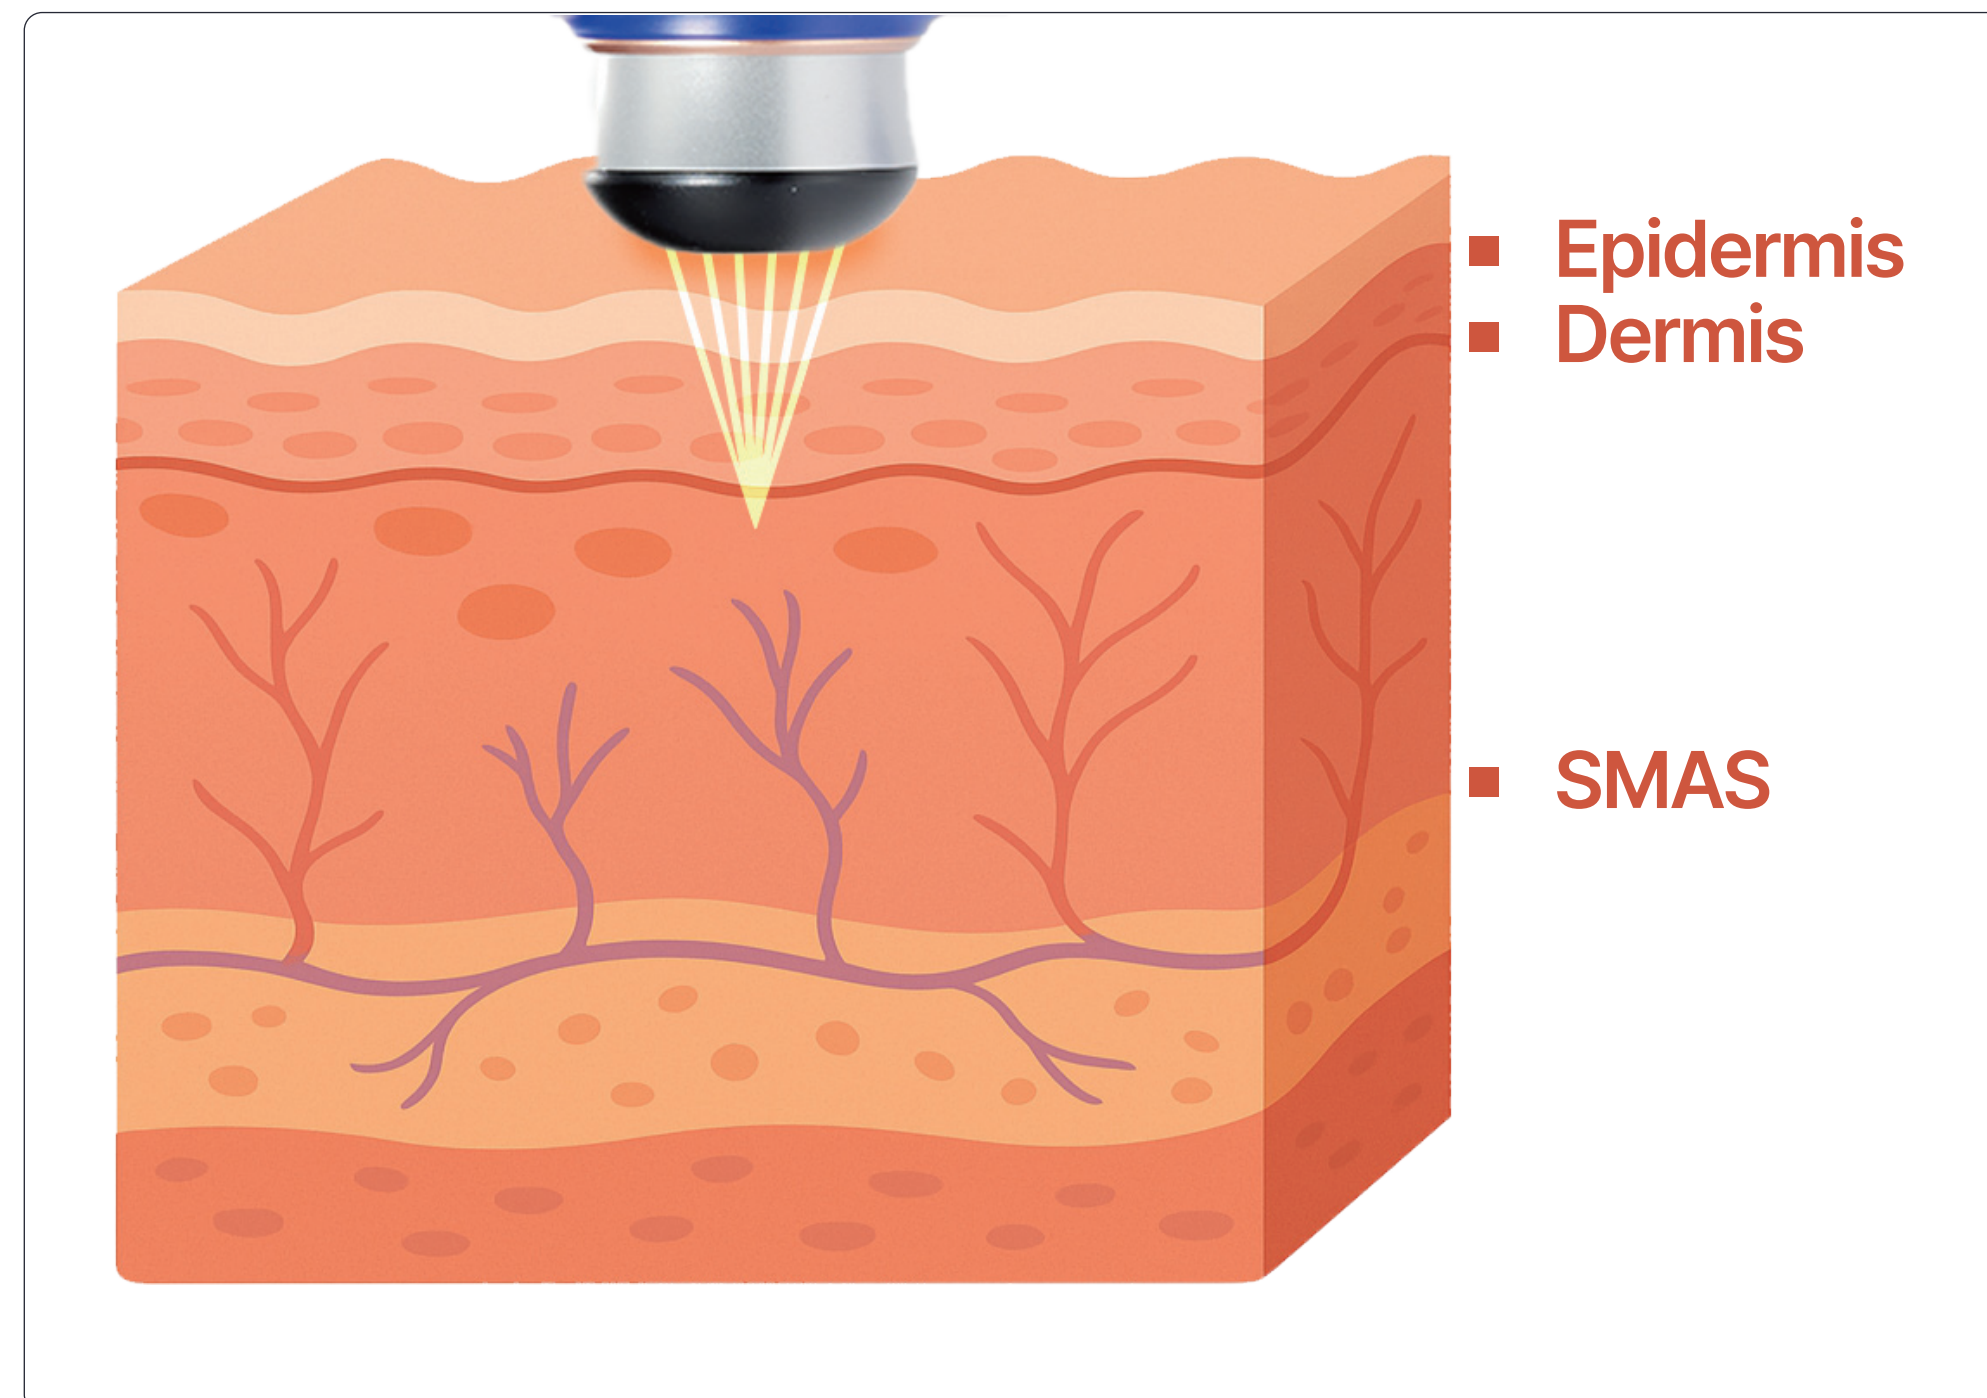

Recommended Shots per Session

3,000 shots/session

3,000 shots

3.0 mm

The 3.0mm depth directly targets the layer where collagen and elastin are produced, helping to improve skin elasticity, refine texture, and reduce fine lines.


Please Note

- Remove glasses before use if you normally wear them.
- Be sure to remove the sticker from the treatment head before using the device.
- Do not use the device over the thyroid area or around the eyes.

Using the HFU Mode


Please read all safety instructions carefully before using the HFU mode.

***Please read before using the HFU mode.**

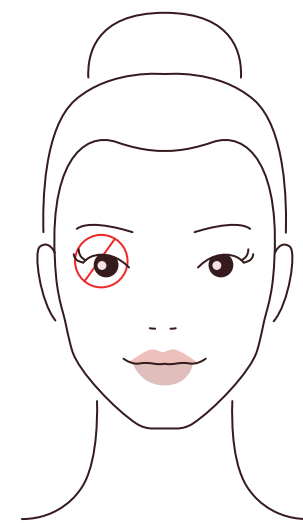

Prohibited Areas of Use

Do not use the device around the eyes.

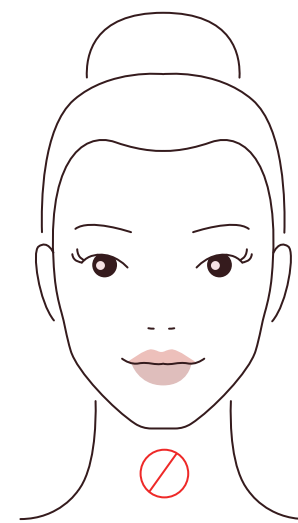


Prohibited Areas of Use

Do not use the device over the thyroid area.



Pre-Treatment

Cleanse the skin thoroughly before use.




Usage Frequency

Recommended usage:
once per week
with 3,000 shots per session.



Accessory Precaution

Remove metal accessories
before use
(e.g., necklaces, earrings).

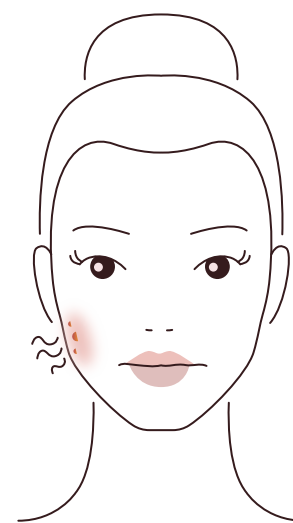

Intensity Adjustment

If you experience discomfort
or skin irritation,
reduce the intensity level.

HFU Mode (Frequency Setting)

Available in two treatment modes.

HFU uses high-intensity focused ultrasound. Excessive use may reduce subcutaneous fat and cause volume loss in the face. Recommended usage: once per week.



V-Line Mode

Skin firming, contour lifting, collagen production, and pore tightening
Precisely targets the 3.0mm dermal layer



Volume Care Mode

Promotes collagen remodeling
and restores inner skin firmness and density.







Consistent HFU energy at any angle (Angle-less Design)

Consistent output at any angle
with no wrist strain for flexible HFU care.

**Ergonomic
360° design**

Using the HFU Mode

◆ How to

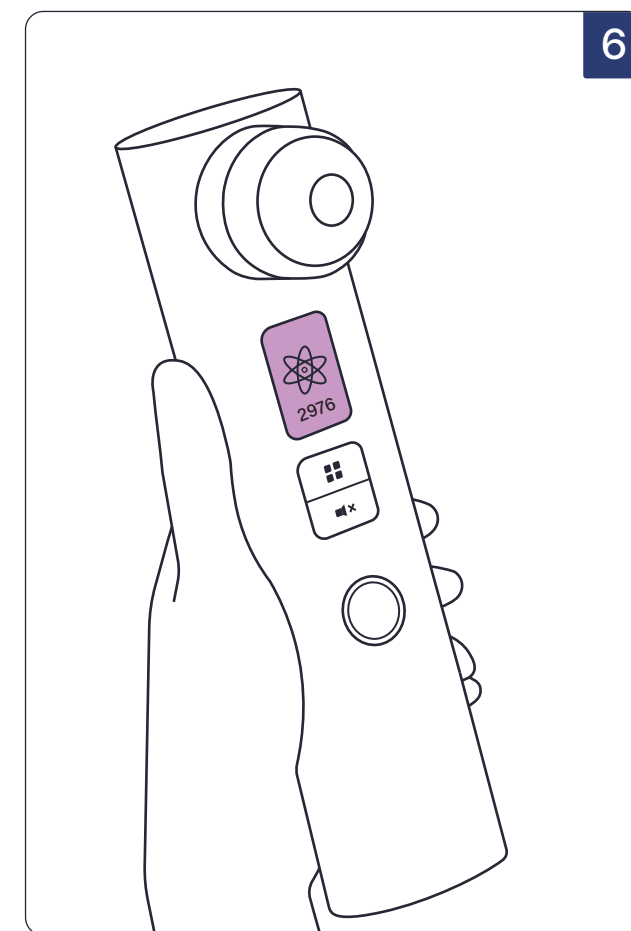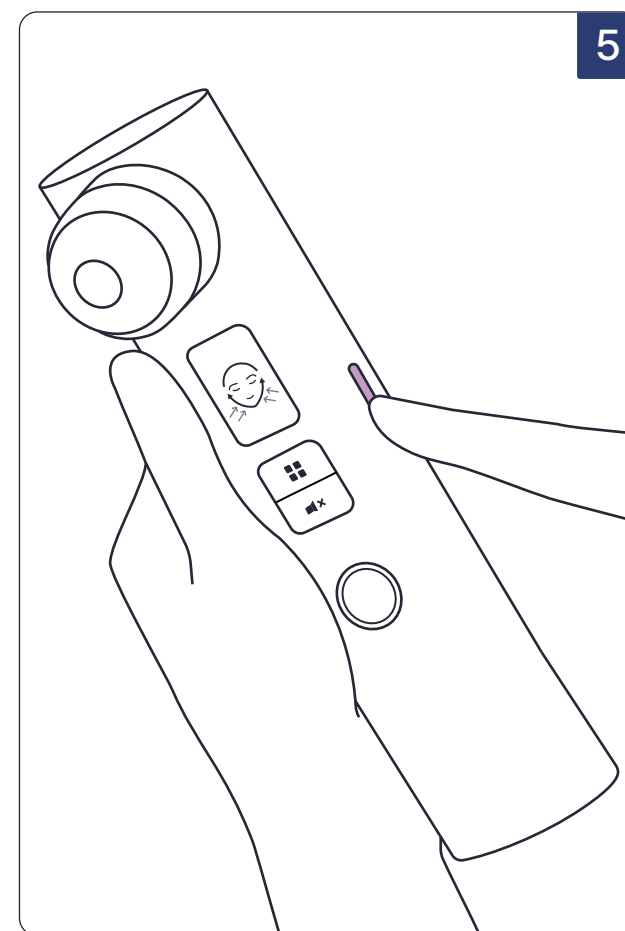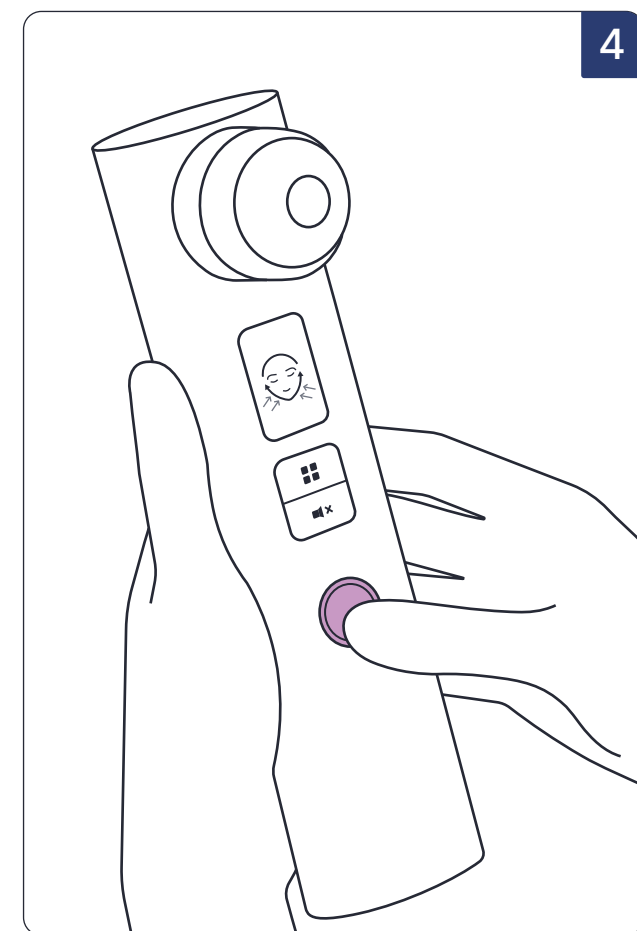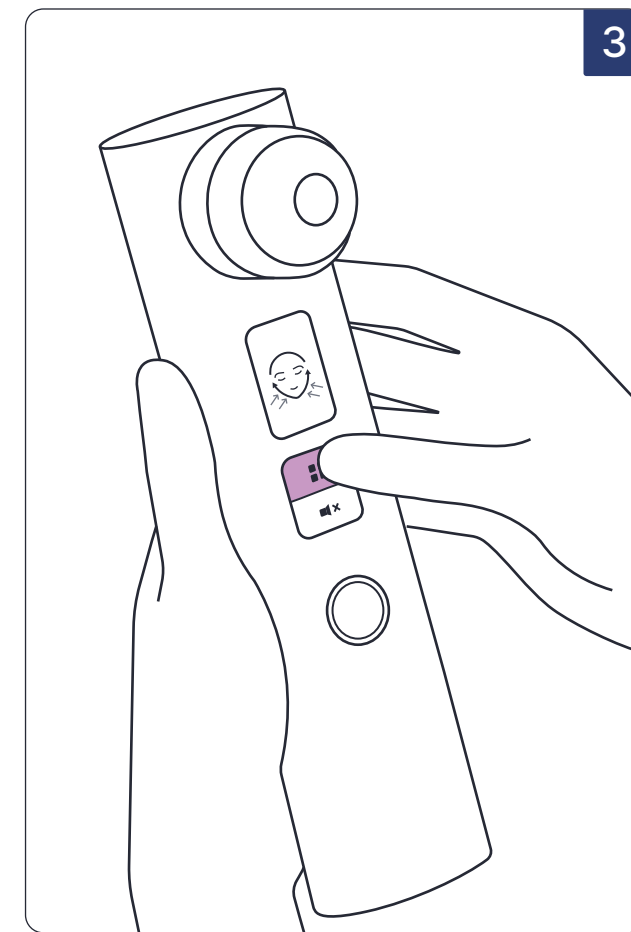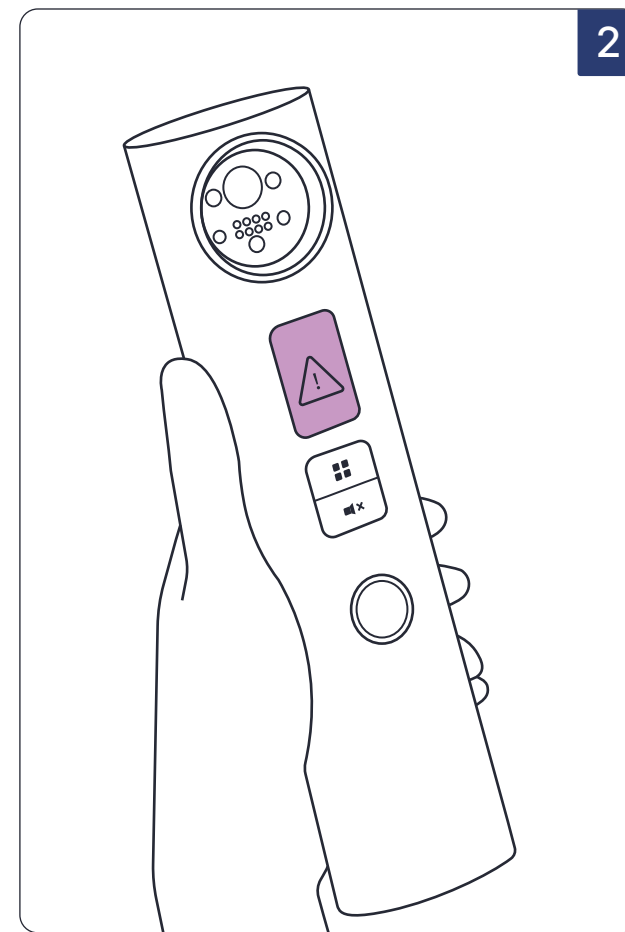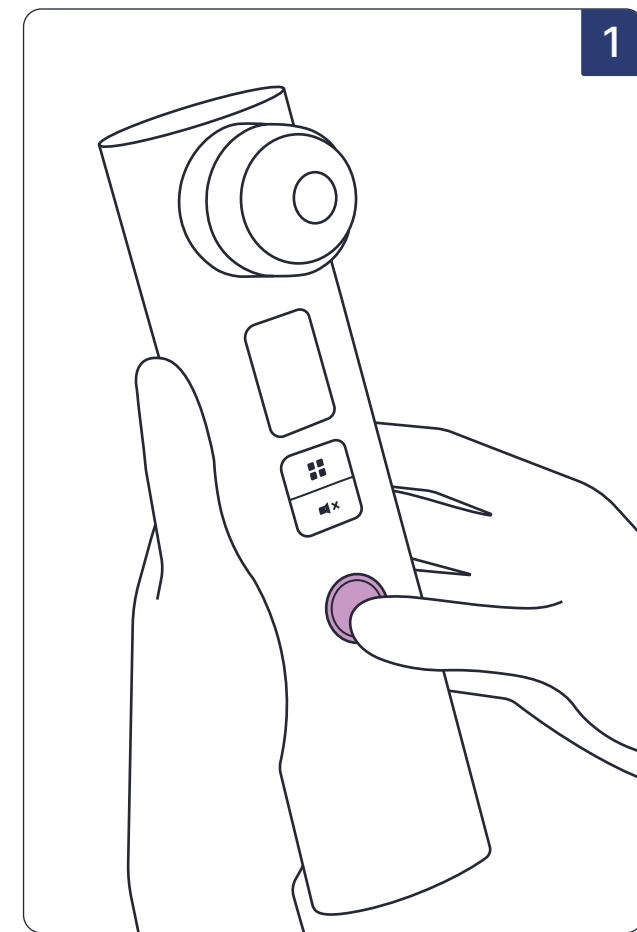

1 Power On/Off

Press and hold the Power Button to turn on the ollivia TheOllier S1. Press and hold again to power it off.

2 Head Detection Warning

If the HFU head is not attached when the device is powered on, the LCD screen will display a "Head Not Detected" message.

3 Mode Selection

Press the [■] to select one of the three available HFU modes.

4 Intensity Adjustment

Press the Intensity Button to select the desired level (1 to 5). Level 1 is recommended by default. If skin irritation is felt, reduce to a lower intensity level.

5 Start and Pause

Press the Side Button briefly to start operation. To pause during operation, press the button again.

6 360° Angle-Free Design

Enjoy smooth and uninterrupted use at any angle.

Using the HFU Mode

◆ Recommended HFU Usage (Full-Face Application)

Please read all safety precautions before using the device.




STEP 01

Apply Gel

Generously apply gel or ampoule to the treatment area.

Tip. For enhanced results, use with Aivillo Ollier Steam Booster Water Gel

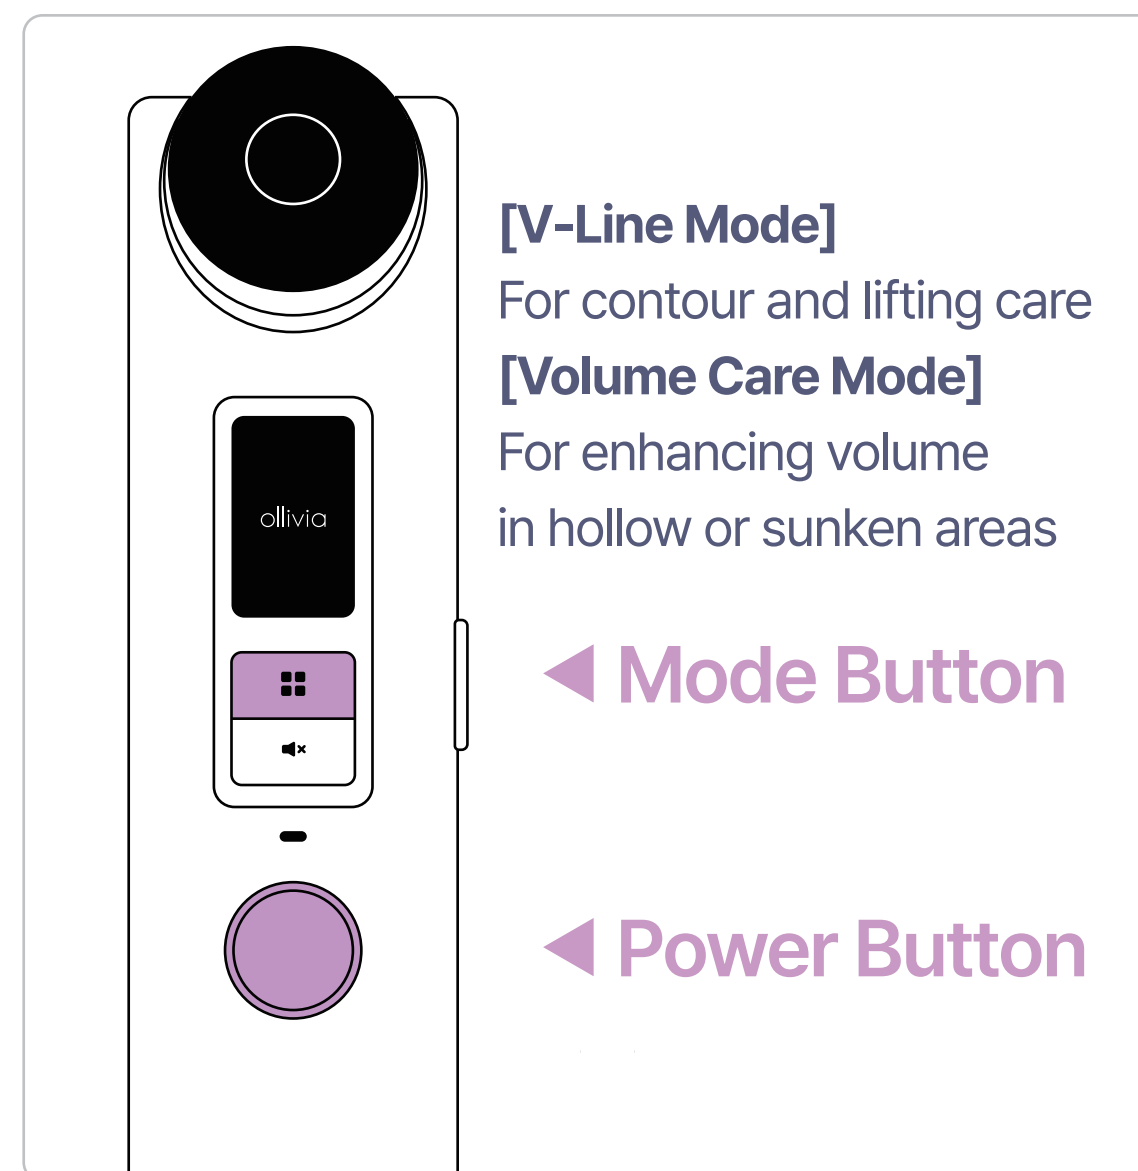


STEP 02

Set Frequency & Intensity

Use the mode button [■] and power button to select the desired frequency and intensity.

Use 3.0 MHz frequency
Recommended intensity: Step 1-3

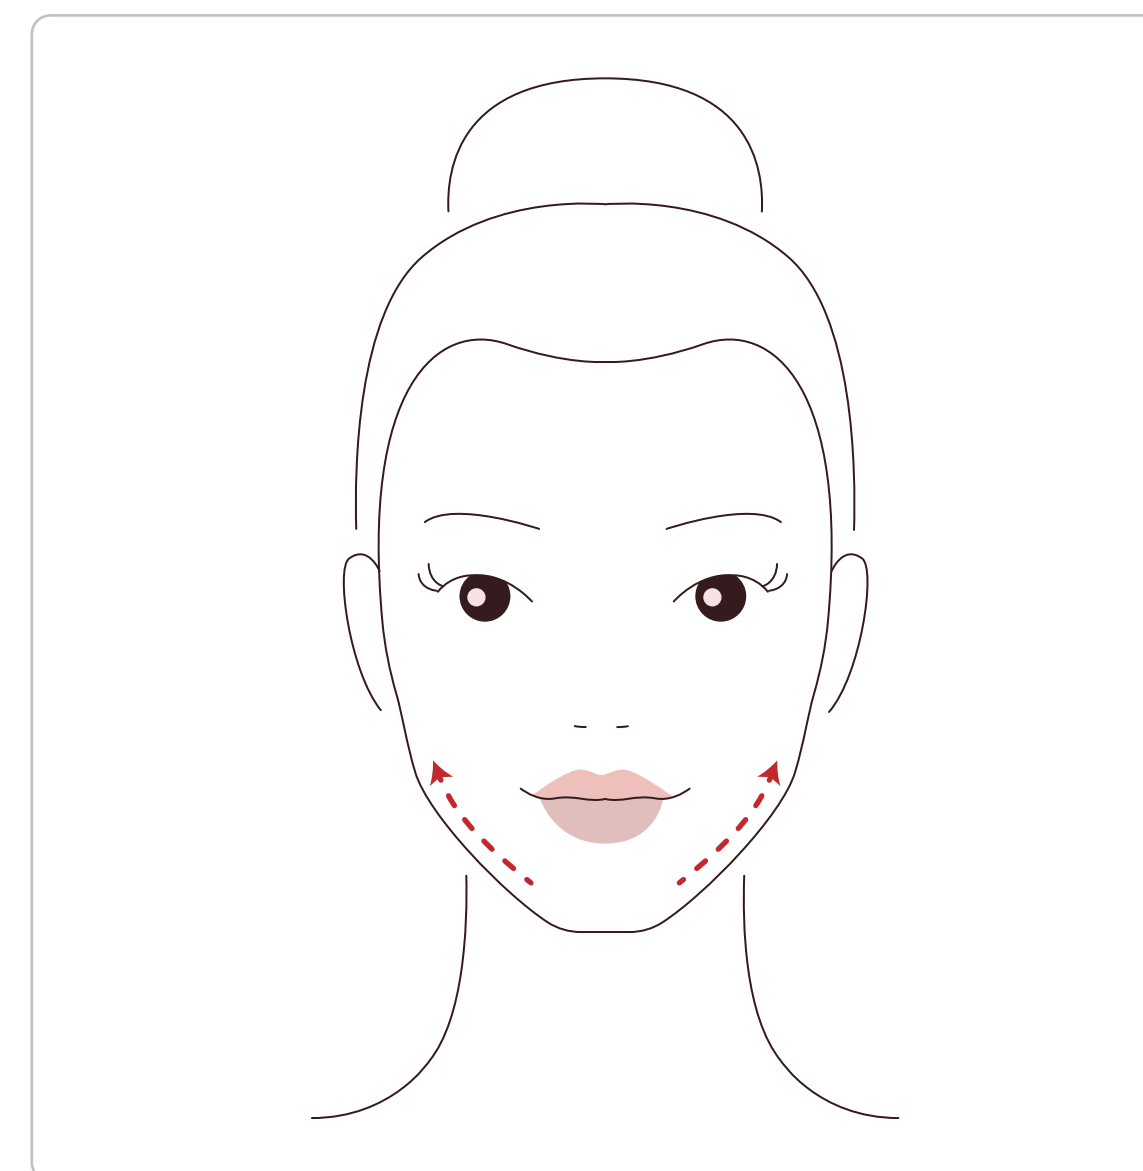

STEP 03

Full-Face Treatment

Apply gel to the desired area for contouring, lifting, or volume care, then gently glide the device over the skin.

Tip. Use lightweight skincare products rather than heavy creams.

Scan the QR code below to view detailed video instructions for using TheOllier S1 device.



[How to Scan]


Open the camera app on your smartphone. Point the camera at the QR code, and a link will automatically appear. Tap the link to view the user manual.

[If Scanning Fails]

If the QR code is not recognized, adjust the lighting or refocus your camera, then try again.

Charging Instructions

◆ Charging the Battery

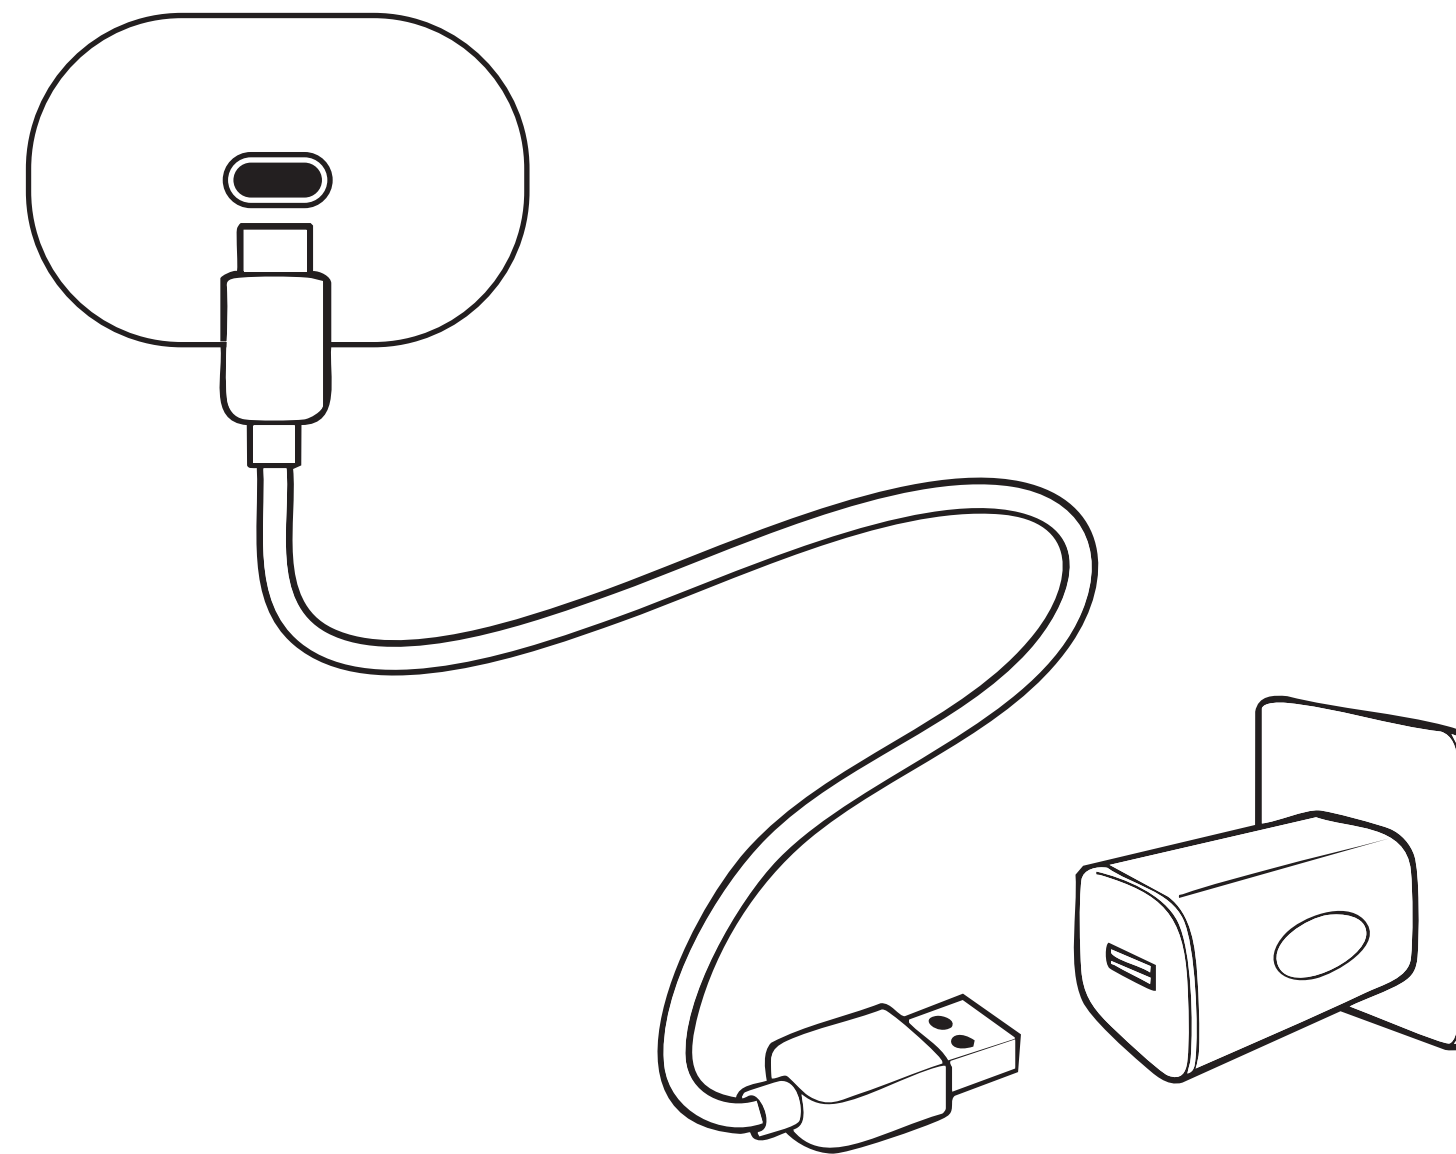

For more stable care, fully charge the battery before use.

1. Connect the USB-C cable to the charger.
2. Insert the cable into the port at the bottom of the device to begin charging.

Caution

- Use only a certified adapter with a KC mark or a DC adapter rated 5V, 2.0A or higher. Non-certified adapters may cause safety issues.
- Connecting the charging cable while powered on will turn off the device. Turn it back on to use.
- Ensure the device and USB-C port are completely dry. Moisture or debris may cause electric shock or damage to the device.
- Do not charge the device with wet hands or in areas with moisture. Ensure it is stored in a safe place, away from impact or drops. Avoid charging in humid environments like bathrooms or near sinks. Moisture can pose safety risks and damage the device.
- Do not bend or pull the cable with excessive force.

Main Unit Care

◆ Main Device Care Instructions

If cosmetics or dust remain on the device after use, gently wipe the main body and head with a dry tissue or soft cloth. After cleaning, store the device in a cool and dry place, away from direct sunlight.

Do Not Use Strong Chemicals or Alcohol

The HFU head contains built-in coolant and is a precision component. Its black film is made of a special material, not ordinary film.



- ❖ Not eligible for exchange/refund due to user negligence.
- ❖ Take extra care to keep the device away from water.

- ⊘ Do not twist the head to detach it. Only detach it in the correct direction to avoid damage.
- ⊘ If cosmetics or moisture enter the head-device connection, gently wipe with a dry tissue before reuse.
- ⊘ Wiping with rough cloths or strong force may cause scratches. Such damage is not covered by exchange or refund.
- ⊘ Avoid getting moisture or cosmetics inside the device.
- ⊘ If the head is not recognized properly, gently wipe its bottom with a dry tissue and try again.
- ⊘ With long-term use, minor wrinkles or changes may appear on the HFU head surface. This is normal and does not affect performance.

We are not responsible for any issues caused by failure to follow the recommended guidelines.

◆ Device Care Instructions

- After use, turn off the device and gently wipe off any residue.
Use a soft dry cloth and store in a cool, dry place.
- Store in a cool, dry place away from direct sunlight or humidity.
Avoid airtight or high-temperature environments for long-term storage.
- Avoid dropping or impacting the device. Do not disassemble or repair it.
Keep it away from strong magnetic fields or electromagnetic interference.
- If not in use for an extended period, fully charge the device,
turn it off, and periodically check its operation.
- Loss of the head excludes the device from warranty or service,
regardless of the warranty period.
Store and use carefully to prevent safety risks or malfunctions.
- Keep the device out of children's reach.
Ensure they do not play with or put it in their mouths.
- Using HFU on sensitive areas like eyes, ears, or lymph nodes
may cause serious issues such as vision or hearing loss. Use with caution.
- Avoid exposing the head to sharp objects.
Clean the main body with a soft dry cloth.
Alcohol or strong chemicals may cause discoloration or damage.
- For more detailed care and A/S information,
please refer to the manufacturer's warranty policy.

◆ Charging Instructions & Battery Precautions

- Do not expose the battery to high temperatures or fire. Risk of explosion or fire.
- The battery is non-replaceable and built-in. Do not disassemble or attempt to replace it.
- If the battery emits an odor, heat, discoloration, or swelling,
stop use immediately and contact customer support.
- Strong impact may damage the battery. Do not touch it with wet hands or immerse it in water.
- Leaving the device unused for long periods may cause complete discharge.
Fully charge every 2–3 months or maintain 60–70% battery level to extend battery life.
- Overcharging (continuous connection to the charger)
may raise the device temperature and degrade battery performance.
- Do not use the device while charging.
Avoid pulling or swinging it by the cable to prevent fire or damage.
- Battery-related damage may not be covered under warranty.
Use and store the device properly for safety.

We are not responsible for any issues caused by failure to follow the recommended guidelines.

◆ Precautions Before Using the Device

- This product is not a medical device. Please read and follow the precautions below.
- Before first use, read the user manual carefully. For detailed information, scan the QR code provided under our eco-friendly policy.
- Remove the protective film from the device and head, and fully charge before use.
- Do not use on children, pregnant or nursing individuals, or areas with wounds, infections, or skin conditions.
- Consult a medical professional if you are undergoing dental treatments such as implants or orthodontics.
- Those with medical concerns (e.g., pacemakers, organ transplants, serious illness, outpatient treatment) or cosmetic surgery should consult a physician before use.
- This device is intended for facial use only. Do not use it on other body parts.
- Adjust the intensity (Step 1–5) based on skin sensitivity. Avoid eyes, eye area, and thyroid region.
- Using HFU on sensitive areas like eyes, ears, or lymph nodes may cause serious issues such as vision or hearing problems. Use with caution.
- Insufficient gel may cause irritation. Always apply enough gel or ampoule and ensure full contact between the skin and device.
- Do not hold the device in one spot for too long to avoid irritation. Never detach or replace the head while the power is on.
- Do not press or shake the device forcefully. Unauthorized modification or repair voids warranty—even within the warranty period. Please use our designated service center.
- If malfunction or abnormality is suspected, stop use immediately and contact customer support.

Warranty and Service Policy

✳ Caution

The warranty period is one year from the date of purchase.

Valid only within the warranty period. Contact your seller or our service center for support.

✳ Within Warranty Period

Within 1 year from purchase: free maintenance is available (product registration required).

If a defect occurs in the main body due to manufacturing issues, free repair will be provided.

However, failure to register the product may result in exclusion from free service.

✳ After Warranty Period

After the warranty period, paid repair is available for products not discontinued. Discontinued products may not be serviceable.

✳ Exceptions

Even within the warranty period, the following cases are subject to paid repair.

- | | |
|---|---|
| 1) Loss or theft of the product | 5) Damage due to improper storage (heat, humidity, direct sunlight) |
| 2) Damage caused by user negligence (e.g., drops, impact ...) | 6) Damage from fire, flooding, salt, or natural disasters |
| 3) Unauthorized disassembly or modification | 7) Failure to follow usage guidelines outlined in the manual, |
| 4) Repairs done by unauthorized personnel or centers | resulting in malfunction or damage |

Information

◆ Where to Buy

Beautyway Co., Ltd.

D-810, 357 Guseong-ro, Giheung-gu, Yongin-si, Gyeonggi-do, Republic of Korea

A/S +82 031-8067-6453

 ollivia.official

 ollivia.official

FCC Compliance Statement

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions:

(1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

FCC Interference Statement

This equipment complies with Class B digital device limits under FCC Part 15, intended to reduce interference in residential settings.

It may emit radio frequency energy, which could interfere with communications if not properly installed or used.

Although interference is unlikely, it is not guaranteed. If it occurs, try turning the device off and on, adjusting the antenna, increasing distance, using a different outlet, or consulting a technician.

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC Caution

Any unauthorized changes or modifications may void the user's right to operate this device.

This transmitter must not be used with other antennas or transmitters. Co-located operation is strictly prohibited.