


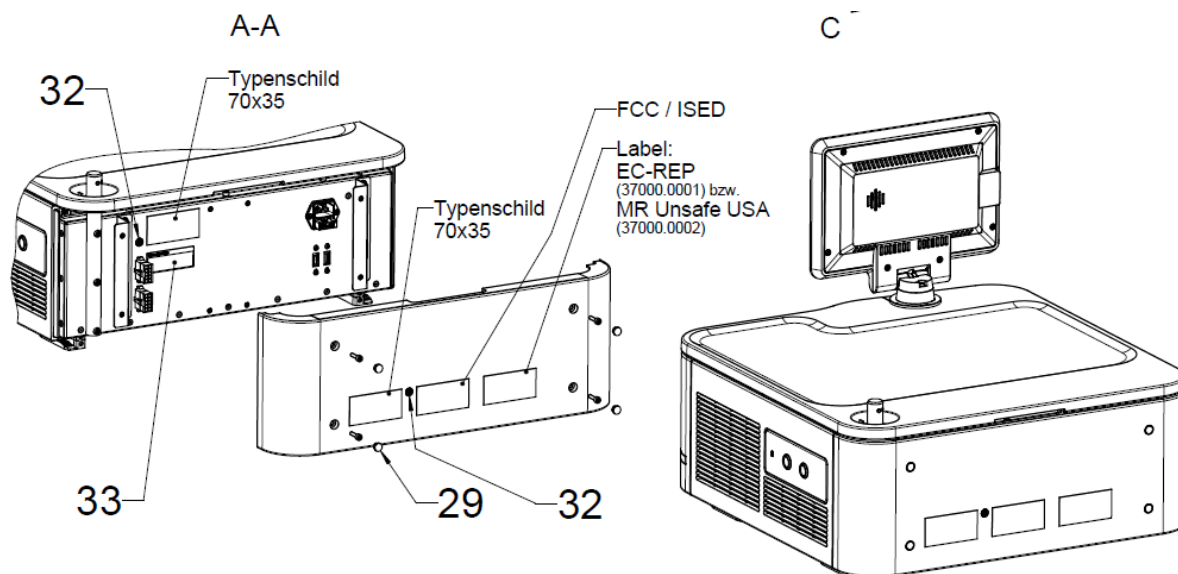

STORZ MEDICAL

Handpiece R-SW (37700.0001)

IC: 35173-37700

FCC ID: 2BTGO-37700

This device complies with part 15 of the FCC Rules.

Operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.