

Appendix B.1 Calibration certificate for Probe

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **SGS Korea (Dymstec)**

Certificate No: **EX3-3986_Mar18**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:3986**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6**
Calibration procedure for dosimetric E-field probes

Calibration date: **March 23, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02525)	Apr-18
Reference 20 dB Attenuator	SN: S5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013 Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660 Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293674	06-Apr-18 (in house check Jun-18)	In house check: Jun-18
Power sensor E4412A	SN: MY41419081	06-Apr-18 (in house check Jun-18)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-18 (in house check Jun-18)	In house check: Jun-18
RF generator HP 8648C	SN: US3542U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

	Name	Function	Signature
Calibrated by:	Michael Weber	Laboratory Technician	
Approved by:	Ketja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			Issued: March 24, 2018

Certificate No: EX3-3986_Mar18

Page 1 of 39

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization β	β rotation around an axis that is in the plane normal to probe axis (at measurement center). i.e., $\beta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization $\beta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:3986

March 23, 2018

Probe EX3DV4

SN:3986

Manufactured: November 11, 2013
Calibrated: March 23, 2018

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3986

March 23, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^{2/3}$) ^A	0.51	0.52	0.48	$\pm 10.1 \%$
DCP (mV) ^B	99.1	99.4	100.9	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	141.4	$\pm 2.5 \%$
		Y	0.0	0.0	1.0		146.1	
		Z	0.0	0.0	1.0		160.0	

Note: For details on UID parameters see Appendix.

Sensor Model Parameters

	C1 fF	C2 fF	α V^{-1}	T1 $\text{ms}\cdot\text{V}^{-2}$	T2 $\text{ms}\cdot\text{V}^{-1}$	T3 ms	T4 V^{-2}	T5 V^{-1}	T6
X	46.81	354.7	36.48	14.62	0.777	5.068	0.000	0.528	1.009
Y	53.35	398.5	35.69	21.23	0.578	5.100	1.142	0.403	1.008
Z	41.48	312.6	36.19	10.59	0.731	5.056	0.028	0.504	1.007

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter; uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value

EX3DV4- SN:3986

March 23, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
750	41.9	0.89	11.55	11.55	11.55	0.40	0.99	± 12.0 %
835	41.5	0.90	10.88	10.88	10.88	0.41	0.93	± 12.0 %
900	41.5	0.97	10.56	10.56	10.56	0.45	0.86	± 12.0 %
1750	40.1	1.37	9.13	9.13	9.13	0.46	0.80	± 12.0 %
1900	40.0	1.40	8.84	8.84	8.84	0.41	0.80	± 12.0 %
1950	40.0	1.40	8.47	8.47	8.47	0.38	0.80	± 12.0 %
2300	39.5	1.67	8.39	8.39	8.39	0.34	0.80	± 12.0 %
2450	39.2	1.80	7.98	7.98	7.98	0.30	0.95	± 12.0 %
2600	39.0	1.96	7.70	7.70	7.70	0.34	0.89	± 12.0 %
3700	37.7	3.12	7.55	7.55	7.55	0.25	1.25	± 13.1 %
5200	36.0	4.66	5.32	5.32	5.32	0.40	1.80	± 13.1 %
5300	35.9	4.76	5.20	5.20	5.20	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.94	4.94	4.94	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.91	4.91	4.91	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3986

March 23, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
750	55.5	0.96	11.34	11.34	11.34	0.62	0.81	± 12.0 %
835	55.2	0.97	10.83	10.83	10.83	0.53	0.80	± 12.0 %
1750	53.4	1.49	8.87	8.87	8.87	0.36	0.91	± 12.0 %
1900	53.3	1.52	8.39	8.39	8.39	0.45	0.80	± 12.0 %
2450	52.7	1.95	7.99	7.99	7.99	0.31	0.80	± 12.0 %
2600	52.5	2.16	7.85	7.85	7.85	0.25	0.80	± 12.0 %
3700	51.0	3.55	7.21	7.21	7.21	0.30	1.25	± 13.1 %
5200	49.0	5.30	4.75	4.75	4.75	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.58	4.58	4.58	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.09	4.09	4.09	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.24	4.24	4.24	0.50	1.90	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^e At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3986

March 23, 2018

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

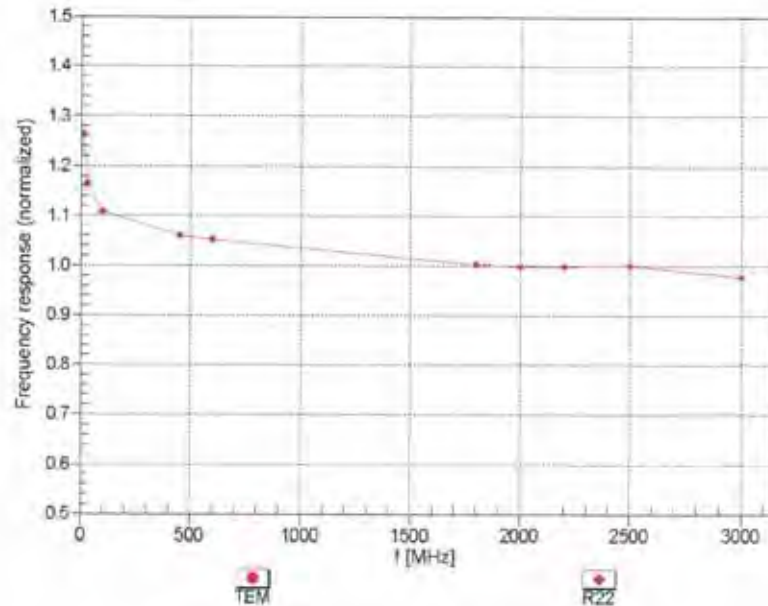


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:3986

March 23, 2018

Receiving Pattern (ϕ), $\theta = 0^\circ$

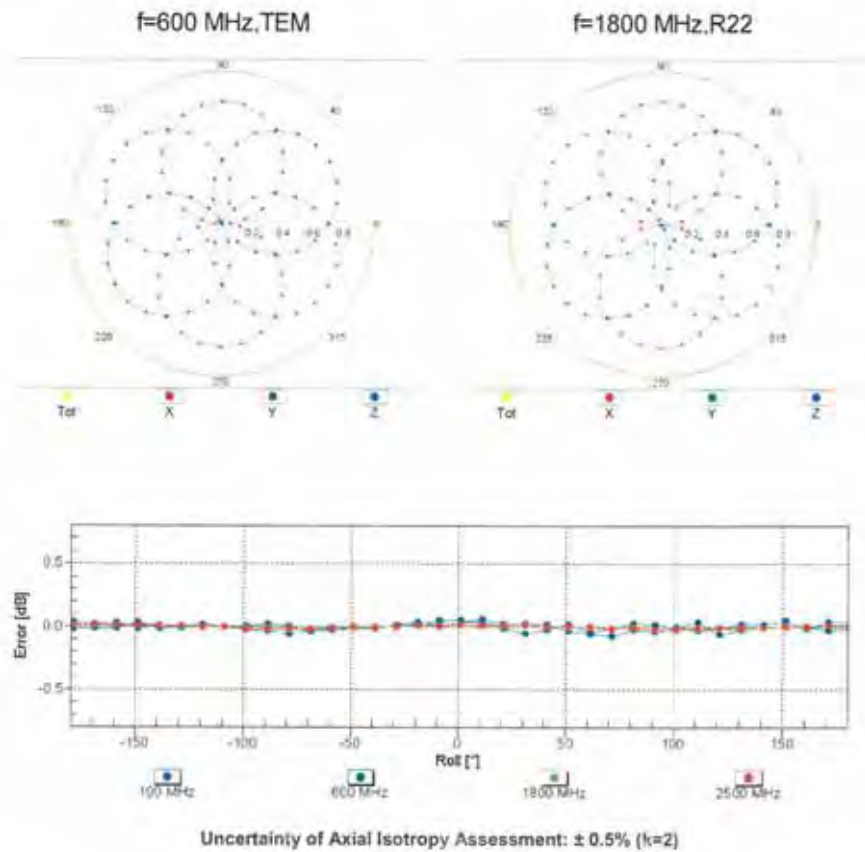


Certificate No: EX3-3986_Mar18

Page 8 of 39

EX3DV4--SN:3986

March 23, 2018

Dynamic Range $f(SAR_{head})$ (TEM cell, $f_{eval} = 1900$ MHz)

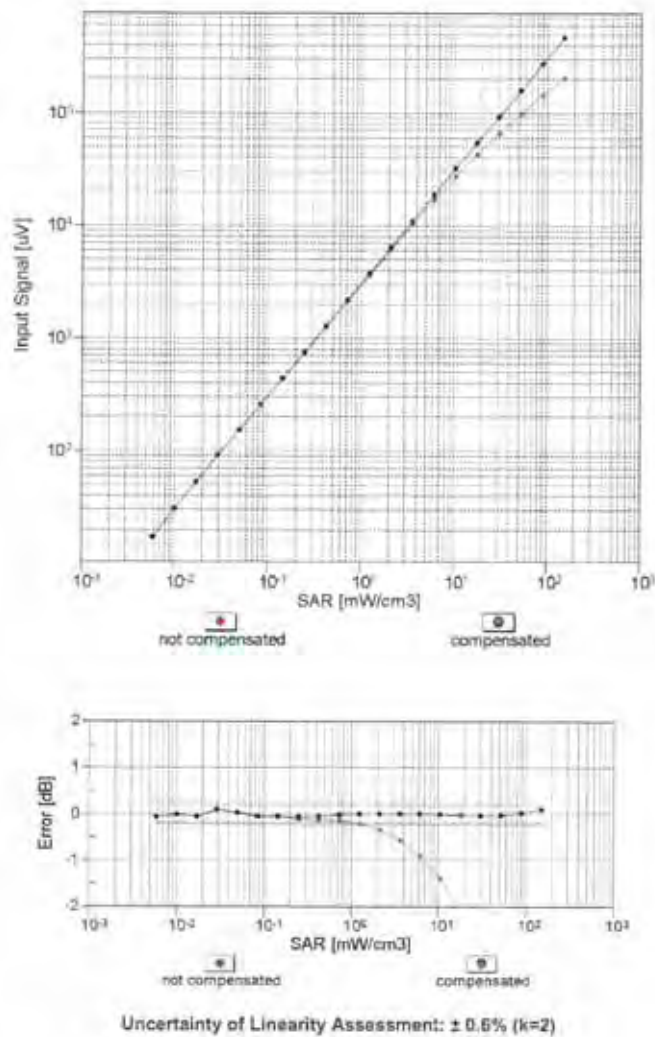

Certificate No: EX3-3986_Mar18

Page 9 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)


RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)


EX3DV4-SN:3986

March 23, 2018

Conversion Factor Assessment

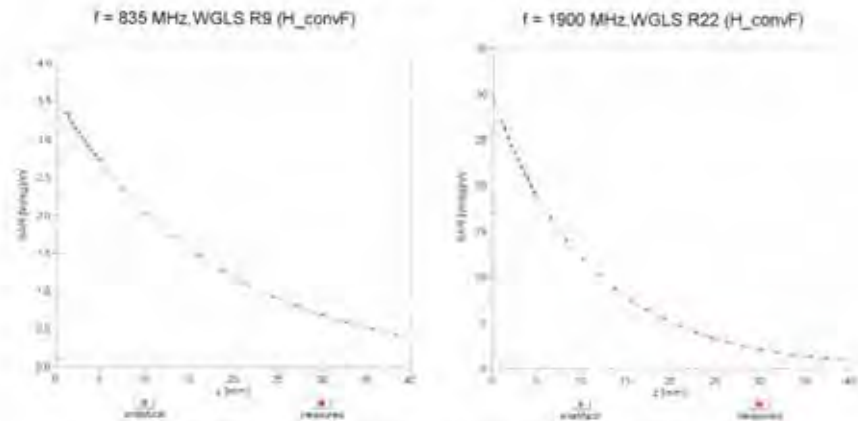

Deviation from Isotropy in Liquid Error (ϕ , θ), $f = 900$ MHz

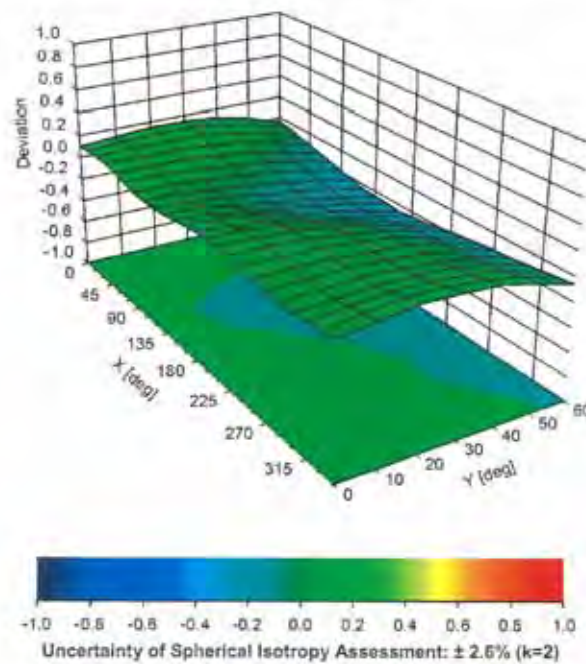

Certificate No: EX3-3986_Mar18

Page 10 of 39

EX3DV4- SN:3986

March 23, 2018

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	131.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:3986

March 23, 2018

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB μ V	C	D dB	VR mV	Max Unc ^E (% $\pm$ 2)
0	CW	X	0.00	0.00	1.00	0.00	141.4	$\pm$ 2.5 %
		Y	0.00	0.00	1.00		146.1	
		Z	0.00	0.00	1.00		160.0	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	X	2.70	67.23	11.23	10.00	20.0	$\pm$ 9.6 %
		Y	4.89	74.21	14.29		20.0	
		Z	2.17	64.62	9.55		20.0	
10011- CAB	UMTS-FDD (WCDMA)	X	0.90	65.80	14.00	0.00	150.0	$\pm$ 9.6 %
		Y	1.09	68.79	16.05		150.0	
		Z	0.91	67.06	14.60		150.0	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	1.11	63.36	14.74	0.41	150.0	$\pm$ 9.6 %
		Y	1.21	64.76	15.90		150.0	
		Z	1.07	63.69	15.01		150.0	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	4.82	66.57	16.99	1.46	150.0	$\pm$ 9.6 %
		Y	4.95	66.84	17.28		150.0	
		Z	4.72	66.67	17.01		150.0	
10021- DAC	GSM-FDD (TDMA, GMSK)	X	100.00	114.18	27.62	9.39	50.0	$\pm$ 9.6 %
		Y	100.00	116.58	28.81		50.0	
		Z	100.00	111.02	25.96		50.0	
10023- DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	100.00	113.90	27.54	9.57	50.0	$\pm$ 9.6 %
		Y	100.00	116.36	28.75		50.0	
		Z	100.00	110.70	25.87		50.0	
10024- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	100.00	112.03	25.58	6.56	60.0	$\pm$ 9.6 %
		Y	100.00	114.80	27.14		60.0	
		Z	100.00	108.84	23.82		60.0	
10025- DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	4.41	70.99	26.27	12.57	50.0	$\pm$ 9.6 %
		Y	10.51	100.04	40.62		50.0	
		Z	4.19	69.91	25.53		50.0	
10026- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	10.12	93.76	33.13	9.56	60.0	$\pm$ 9.6 %
		Y	23.67	115.77	41.03		60.0	
		Z	8.72	91.03	32.14		60.0	
10027- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	100.00	111.33	24.50	4.80	80.0	$\pm$ 9.6 %
		Y	100.00	115.07	26.56		80.0	
		Z	100.00	107.81	22.56		80.0	
10028- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	100.00	111.15	23.73	3.55	100.0	$\pm$ 9.6 %
		Y	100.00	116.48	26.51		100.0	
		Z	100.00	106.78	21.41		100.0	
10029- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	6.36	83.11	27.90	7.80	80.0	$\pm$ 9.6 %
		Y	10.84	95.59	32.95		80.0	
		Z	5.47	80.67	26.98		80.0	
10030- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	X	100.00	109.99	24.20	5.30	70.0	$\pm$ 9.6 %
		Y	100.00	113.44	26.12		70.0	
		Z	100.00	106.49	22.28		70.0	
10031- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	X	100.00	104.21	19.51	1.88	100.0	$\pm$ 9.6 %
		Y	100.00	116.37	25.07		100.0	
		Z	100.00	94.03	14.91		100.0	

Certificate No: EX3-3986_Mar18

Page 12 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10032-CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	100.00	99.46	16.78	1.17	100.0	± 9.6 %
		Y	100.00	121.68	26.19		100.0	
		Z	0.19	60.00	3.97		100.0	
10033-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)	X	20.12	101.92	27.33	5.30	70.0	± 9.6 %
		Y	100.00	129.51	35.25		70.0	
		Z	16.86	98.44	25.65		70.0	
10034-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	X	3.34	78.01	18.12	1.88	100.0	± 9.6 %
		Y	15.09	100.48	26.22		100.0	
		Z	3.11	77.28	17.17		100.0	
10035-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	X	1.99	72.33	15.63	1.17	100.0	± 9.6 %
		Y	4.95	85.50	21.44		100.0	
		Z	1.85	71.92	14.80		100.0	
10036-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	X	35.27	110.83	29.79	5.30	70.0	± 9.6 %
		Y	100.00	129.90	35.44		70.0	
		Z	30.95	107.63	28.20		70.0	
10037-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	X	3.07	77.01	17.72	1.88	100.0	± 9.6 %
		Y	13.32	98.72	25.69		100.0	
		Z	2.77	75.94	16.65		100.0	
10038-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	X	2.02	72.78	15.92	1.17	100.0	± 9.6 %
		Y	5.16	86.46	21.88		100.0	
		Z	1.90	72.49	15.16		100.0	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	1.42	68.69	13.64	0.00	150.0	± 9.6 %
		Y	2.19	74.47	17.04		150.0	
		Z	1.34	68.80	13.02		150.0	
10042-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Halfrate)	X	100.00	109.42	24.64	7.78	50.0	± 9.6 %
		Y	100.00	111.97	26.00		50.0	
		Z	100.00	106.15	22.90		50.0	
10044-CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	X	0.05	119.56	13.75	0.00	150.0	± 9.6 %
		Y	0.01	115.38	8.32		150.0	
		Z	0.15	126.77	0.97		150.0	
10048-CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	X	55.33	105.11	26.75	13.80	25.0	± 9.6 %
		Y	100.00	118.73	30.94		25.0	
		Z	12.40	82.49	19.54		25.0	
10049-CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	X	100.00	113.46	27.69	10.79	40.0	± 9.6 %
		Y	100.00	116.03	28.83		40.0	
		Z	16.24	87.92	20.17		40.0	
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	27.47	102.48	27.85	9.03	50.0	± 9.6 %
		Y	100.00	126.07	34.81		50.0	
		Z	21.11	96.88	25.47		50.0	
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.85	77.78	24.95	6.55	100.0	± 9.6 %
		Y	7.19	86.29	28.65		100.0	
		Z	4.24	75.84	24.21		100.0	
10059-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	X	1.16	64.57	15.41	0.61	110.0	± 9.6 %
		Y	1.31	66.62	16.90		110.0	
		Z	1.11	64.87	15.67		110.0	
10060-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	X	23.02	113.04	29.10	1.30	110.0	± 9.6 %
		Y	100.00	137.46	35.70		110.0	
		Z	100.00	135.33	34.04		110.0	

Certificate No: EX3-3986_Mar18

Page 13 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10061-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	3.38	82.65	22.74	2.04	110.0	± 9.6 %
		Y	13.03	105.96	30.66		110.0	
		Z	3.24	83.48	23.13		110.0	
10062-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	X	4.61	66.49	16.38	0.49	100.0	± 9.6 %
		Y	4.74	66.77	16.64		100.0	
		Z	4.51	66.62	16.42		100.0	
10063-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	X	4.63	66.60	16.49	0.72	100.0	± 9.6 %
		Y	4.76	66.89	16.77		100.0	
		Z	4.53	66.72	16.52		100.0	
10064-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	X	4.91	66.88	16.73	0.86	100.0	± 9.6 %
		Y	5.07	67.19	17.01		100.0	
		Z	4.79	66.96	16.74		100.0	
10065-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	X	4.79	66.78	16.83	1.21	100.0	± 9.6 %
		Y	4.95	67.14	17.15		100.0	
		Z	4.67	66.85	16.84		100.0	
10066-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	X	4.81	66.83	17.01	1.46	100.0	± 9.6 %
		Y	4.97	67.20	17.35		100.0	
		Z	4.69	66.88	17.01		100.0	
10067-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	X	5.11	67.02	17.48	2.04	100.0	± 9.6 %
		Y	5.27	67.32	17.78		100.0	
		Z	4.98	67.11	17.48		100.0	
10068-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	X	5.16	67.09	17.71	2.55	100.0	± 9.6 %
		Y	5.34	67.50	18.08		100.0	
		Z	5.02	67.09	17.67		100.0	
10069-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	X	5.24	67.10	17.90	2.67	100.0	± 9.6 %
		Y	5.42	67.45	18.25		100.0	
		Z	5.10	67.12	17.86		100.0	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	4.92	66.67	17.31	1.99	100.0	± 9.6 %
		Y	5.06	66.97	17.62		100.0	
		Z	4.82	66.76	17.32		100.0	
10072-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	X	4.91	67.02	17.54	2.30	100.0	± 9.6 %
		Y	5.06	67.40	17.89		100.0	
		Z	4.79	67.07	17.53		100.0	
10073-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	4.98	67.21	17.88	2.83	100.0	± 9.6 %
		Y	5.14	67.60	18.25		100.0	
		Z	4.86	67.26	17.87		100.0	
10074-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	4.97	67.13	18.05	3.30	100.0	± 9.6 %
		Y	5.12	67.52	18.44		100.0	
		Z	4.86	67.18	18.02		100.0	
10075-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	5.01	67.27	18.37	3.82	90.0	± 9.6 %
		Y	5.18	67.76	18.84		90.0	
		Z	4.89	67.26	18.31		90.0	
10076-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	X	5.03	67.06	18.49	4.15	90.0	± 9.6 %
		Y	5.17	67.49	18.92		90.0	
		Z	4.92	67.09	18.45		90.0	
10077-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	5.06	67.14	18.59	4.30	90.0	± 9.6 %
		Y	5.19	67.54	19.01		90.0	
		Z	4.95	67.18	18.56		90.0	

Certificate No: EX3-3986_Mar18

Page 14 of 39

EX3DV4- SN:3986

March 23, 2018

10081-CAB	CDMA2000 (1xRTT, RC3)	X	0.68	63.73	10.66	0.00	150.0	± 9.6 %
		Y	0.93	67.49	13.59		150.0	
		Z	0.59	63.29	9.69		150.0	
10082-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	X	0.79	60.00	4.67	4.77	80.0	± 9.6 %
		Y	0.92	60.00	5.04		80.0	
		Z	0.70	60.00	4.16		80.0	
10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	100.00	112.11	25.63	6.56	60.0	± 9.6 %
		Y	100.00	114.87	27.19		60.0	
		Z	100.00	108.94	23.89		60.0	
10097-CAB	UMTS-FDD (HSDPA)	X	1.70	66.76	14.94	0.00	150.0	± 9.6 %
		Y	1.87	68.18	16.07		150.0	
		Z	1.72	67.77	15.33		150.0	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	1.66	66.69	14.90	0.00	150.0	± 9.6 %
		Y	1.83	68.15	16.04		150.0	
		Z	1.68	67.71	15.29		150.0	
10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	10.19	93.89	33.17	9.56	60.0	± 9.6 %
		Y	23.93	115.99	41.09		60.0	
		Z	8.78	91.16	32.18		60.0	
10100-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	2.95	69.45	16.13	0.00	150.0	± 9.6 %
		Y	3.27	71.06	17.02		150.0	
		Z	2.96	70.05	16.46		150.0	
10101-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	3.13	67.04	15.58	0.00	150.0	± 9.6 %
		Y	3.30	67.84	16.11		150.0	
		Z	3.08	67.29	15.73		150.0	
10102-CAD	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	3.24	67.04	15.70	0.00	150.0	± 9.6 %
		Y	3.40	67.76	16.18		150.0	
		Z	3.19	67.30	15.85		150.0	
10103-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.59	76.41	20.71	3.98	65.0	± 9.6 %
		Y	8.06	79.57	22.09		65.0	
		Z	6.02	75.62	20.42		65.0	
10104-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	6.34	73.88	20.46	3.98	65.0	± 9.6 %
		Y	7.49	76.67	21.80		65.0	
		Z	5.86	73.12	20.14		65.0	
10105-CAD	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	6.10	73.00	20.39	3.98	65.0	± 9.6 %
		Y	6.84	74.65	21.33		65.0	
		Z	5.54	71.87	19.88		65.0	
10108-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	2.57	68.71	15.94	0.00	150.0	± 9.6 %
		Y	2.86	70.25	16.85		150.0	
		Z	2.55	69.36	16.30		150.0	
10109-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	2.78	66.85	15.44	0.00	150.0	± 9.6 %
		Y	2.96	67.69	16.04		150.0	
		Z	2.73	67.20	15.61		150.0	
10110-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	2.07	67.75	15.46	0.00	150.0	± 9.6 %
		Y	2.33	69.35	16.51		150.0	
		Z	2.04	68.49	15.80		150.0	
10111-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	2.48	67.57	15.63	0.00	150.0	± 9.6 %
		Y	2.68	68.51	16.39		150.0	
		Z	2.46	68.28	15.88		150.0	

Certificate No: EX3-3986_Mar18

Page 15 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10112-CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	2.91	66.88	15.52	0.00	150.0	± 9.6 %
		Y	3.08	67.63	16.08		150.0	
		Z	2.86	67.24	15.69		150.0	
10113-CAE	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	2.64	67.77	15.80	0.00	150.0	± 9.6 %
		Y	2.84	68.59	16.50		150.0	
		Z	2.62	68.48	16.04		150.0	
10114-CAC	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	5.05	67.00	16.30	0.00	150.0	± 9.6 %
		Y	5.15	67.21	16.46		150.0	
		Z	4.97	67.08	16.35		150.0	
10115-CAC	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	5.34	67.13	16.37	0.00	150.0	± 9.6 %
		Y	5.48	67.46	16.59		150.0	
		Z	5.22	67.13	16.39		150.0	
10116-CAC	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	5.14	67.18	16.31	0.00	150.0	± 9.6 %
		Y	5.26	67.44	16.50		150.0	
		Z	5.05	67.26	16.37		150.0	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	5.01	66.85	16.24	0.00	150.0	± 9.6 %
		Y	5.13	67.14	16.44		150.0	
		Z	4.94	66.96	16.31		150.0	
10118-CAC	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	X	5.42	67.34	16.49	0.00	150.0	± 9.6 %
		Y	5.56	67.63	16.68		150.0	
		Z	5.30	67.33	16.50		150.0	
10119-CAC	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	X	5.12	67.13	16.30	0.00	150.0	± 9.6 %
		Y	5.23	67.37	16.48		150.0	
		Z	5.04	67.22	16.36		150.0	
10140-CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	3.27	67.04	15.61	0.00	150.0	± 9.6 %
		Y	3.44	67.76	16.10		150.0	
		Z	3.21	67.30	15.76		150.0	
10141-CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	3.40	67.18	15.80	0.00	150.0	± 9.6 %
		Y	3.56	67.82	16.26		150.0	
		Z	3.34	67.45	15.96		150.0	
10142-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	1.83	67.56	14.97	0.00	150.0	± 9.6 %
		Y	2.11	69.43	16.29		150.0	
		Z	1.80	68.38	15.21		150.0	
10143-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	2.31	68.03	15.13	0.00	150.0	± 9.6 %
		Y	2.58	69.39	16.26		150.0	
		Z	2.29	68.79	15.22		150.0	
10144-CAD	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	2.09	65.80	13.53	0.00	150.0	± 9.6 %
		Y	2.34	67.09	14.67		150.0	
		Z	1.99	65.95	13.29		150.0	
10145-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	1.03	63.33	10.34	0.00	150.0	± 9.6 %
		Y	1.39	66.71	13.06		150.0	
		Z	0.85	62.09	8.88		150.0	
10146-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	1.72	65.13	10.99	0.00	150.0	± 9.6 %
		Y	2.71	70.12	13.96		150.0	
		Z	1.26	62.27	8.55		150.0	
10147-CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	2.00	66.90	12.00	0.00	150.0	± 9.6 %
		Y	3.59	73.77	15.64		150.0	
		Z	1.36	63.03	9.07		150.0	

Certificate No: EX3-3986_Mar18

Page 16 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10149-CAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	2.79	66.91	15.48	0.00	150.0	± 9.6 %
		Y	2.97	67.75	16.09		150.0	
		Z	2.74	67.27	15.66		150.0	
10150-CAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	2.92	66.94	15.56	0.00	150.0	± 9.6 %
		Y	3.09	67.68	16.12		150.0	
		Z	2.87	67.30	15.74		150.0	
10151-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.91	78.83	21.75	3.98	65.0	± 9.6 %
		Y	9.10	83.26	23.61		65.0	
		Z	6.42	78.46	21.62		65.0	
10152-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	5.88	73.85	20.15	3.98	65.0	± 9.6 %
		Y	7.12	77.01	21.70		65.0	
		Z	5.39	73.09	19.76		65.0	
10153-CAD	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	6.28	74.91	20.98	3.98	65.0	± 9.6 %
		Y	7.52	77.91	22.44		65.0	
		Z	5.80	74.26	20.66		65.0	
10154-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	2.11	68.15	15.72	0.00	150.0	± 9.6 %
		Y	2.38	69.82	16.80		150.0	
		Z	2.09	68.95	16.08		150.0	
10155-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	2.49	67.59	15.64	0.00	150.0	± 9.6 %
		Y	2.68	68.52	16.40		150.0	
		Z	2.47	68.31	15.90		150.0	
10156-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	1.66	67.45	14.61	0.00	150.0	± 9.6 %
		Y	1.98	69.71	16.23		150.0	
		Z	1.62	68.21	14.73		150.0	
10157-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	1.91	66.13	13.40	0.00	150.0	± 9.6 %
		Y	2.20	67.84	14.83		150.0	
		Z	1.80	66.22	13.05		150.0	
10158-CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	2.65	67.83	15.84	0.00	150.0	± 9.6 %
		Y	2.84	68.65	16.54		150.0	
		Z	2.63	68.56	16.10		150.0	
10159-CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	2.01	66.56	13.68	0.00	150.0	± 9.6 %
		Y	2.32	68.34	15.14		150.0	
		Z	1.90	66.65	13.32		150.0	
10160-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	2.61	67.99	15.82	0.00	150.0	± 9.6 %
		Y	2.82	69.04	16.54		150.0	
		Z	2.59	68.61	16.13		150.0	
10161-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	2.81	66.87	15.48	0.00	150.0	± 9.6 %
		Y	2.99	67.62	16.06		150.0	
		Z	2.76	67.27	15.64		150.0	
10162-CAD	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	2.92	67.04	15.60	0.00	150.0	± 9.6 %
		Y	3.09	67.72	16.15		150.0	
		Z	2.87	67.47	15.78		150.0	
10166-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	3.47	69.17	18.96	3.01	150.0	± 9.6 %
		Y	3.81	70.43	19.57		150.0	
		Z	3.32	69.20	18.91		150.0	
10167-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	4.17	71.70	19.26	3.01	150.0	± 9.6 %
		Y	4.95	74.10	20.30		150.0	
		Z	3.97	71.73	19.16		150.0	

Certificate No: EX3-3986_Mar18

Page 17 of 39

EX3DV4- SN:3986

March 23, 2018

10166-CAE	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	4.68	74.17	20.72	3.01	150.0	± 9.6 %
		Y	5.55	76.55	21.67		150.0	
		Z	4.51	74.52	20.78		150.0	
10169-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	2.83	68.23	18.56	3.01	150.0	± 9.6 %
		Y	3.36	71.24	19.95		150.0	
		Z	2.69	67.88	18.31		150.0	
10170-CAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	3.76	73.65	20.76	3.01	150.0	± 9.6 %
		Y	5.32	79.50	22.99		150.0	
		Z	3.57	73.35	20.55		150.0	
10171-AAD	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	3.09	69.54	17.93	3.01	150.0	± 9.6 %
		Y	4.12	74.08	19.82		150.0	
		Z	2.90	69.06	17.58		150.0	
10172-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	8.86	92.27	28.98	6.02	65.0	± 9.6 %
		Y	28.53	115.21	36.10		65.0	
		Z	6.18	86.36	26.81		65.0	
10173-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	16.23	99.50	29.35	6.02	65.0	± 9.6 %
		Y	100.00	130.73	37.53		65.0	
		Z	11.50	94.15	27.45		65.0	
10174-CAD	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	12.78	93.95	27.05	6.02	65.0	± 9.6 %
		Y	63.47	120.59	34.43		65.0	
		Z	8.63	88.09	24.90		65.0	
10175-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	2.80	67.92	18.30	3.01	150.0	± 9.6 %
		Y	3.31	70.87	19.68		150.0	
		Z	2.65	67.56	18.04		150.0	
10176-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	3.77	73.67	20.77	3.01	150.0	± 9.6 %
		Y	5.33	79.52	23.00		150.0	
		Z	3.57	73.37	20.56		150.0	
10177-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	2.82	68.07	18.40	3.01	150.0	± 9.6 %
		Y	3.34	71.05	19.78		150.0	
		Z	2.67	67.71	18.14		150.0	
10178-CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	3.73	73.45	20.65	3.01	150.0	± 9.6 %
		Y	5.24	79.20	22.85		150.0	
		Z	3.54	73.17	20.45		150.0	
10179-CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	3.39	71.45	19.20	3.01	150.0	± 9.6 %
		Y	4.65	76.59	21.24		150.0	
		Z	3.19	71.03	18.90		150.0	
10180-CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	3.09	69.47	17.88	3.01	150.0	± 9.6 %
		Y	4.10	73.98	19.76		150.0	
		Z	2.90	69.00	17.53		150.0	
10181-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	2.82	68.05	18.39	3.01	150.0	± 9.6 %
		Y	3.33	71.03	19.77		150.0	
		Z	2.67	67.69	18.13		150.0	
10182-CAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	3.72	73.43	20.64	3.01	150.0	± 9.6 %
		Y	5.23	79.17	22.84		150.0	
		Z	3.53	73.15	20.44		150.0	
10183-AAC	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	3.08	69.45	17.87	3.01	150.0	± 9.6 %
		Y	4.09	73.95	19.75		150.0	
		Z	2.89	68.98	17.52		150.0	

Certificate No: EX3-3986_Mar18

Page 18 of 39

EX3DV4- SN:3986

March 23, 2018

10184-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	2.83	68.10	18.41	3.01	150.0	± 9.6 %
		Y	3.35	71.08	19.80		150.0	
		Z	2.68	67.73	18.15		150.0	
10185-CAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	3.74	73.50	20.68	3.01	150.0	± 9.6 %
		Y	5.26	79.26	22.88		150.0	
		Z	3.55	73.22	20.48		150.0	
10186-AAD	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	3.10	69.51	17.90	3.01	150.0	± 9.6 %
		Y	4.11	74.03	19.78		150.0	
		Z	2.90	69.04	17.56		150.0	
10187-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	2.84	68.15	18.48	3.01	150.0	± 9.6 %
		Y	3.36	71.13	19.86		150.0	
		Z	2.69	67.80	18.23		150.0	
10188-CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	3.86	74.17	21.07	3.01	150.0	± 9.6 %
		Y	5.50	80.16	23.33		150.0	
		Z	3.67	73.90	20.87		150.0	
10189-AAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	3.16	69.92	18.18	3.01	150.0	± 9.6 %
		Y	4.23	74.59	20.11		150.0	
		Z	2.97	69.44	17.84		150.0	
10193-CAC	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	4.44	66.39	15.97	0.00	150.0	± 9.6 %
		Y	4.56	66.64	16.21		150.0	
		Z	4.36	66.57	16.03		150.0	
10194-CAC	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	X	4.61	66.70	16.09	0.00	150.0	± 9.6 %
		Y	4.74	66.97	16.33		150.0	
		Z	4.51	66.85	16.17		150.0	
10195-CAC	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	4.65	66.73	16.11	0.00	150.0	± 9.6 %
		Y	4.78	67.00	16.34		150.0	
		Z	4.55	66.88	16.18		150.0	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	4.44	66.44	15.98	0.00	150.0	± 9.6 %
		Y	4.57	66.72	16.24		150.0	
		Z	4.35	66.60	16.04		150.0	
10197-CAC	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	4.62	66.72	16.11	0.00	150.0	± 9.6 %
		Y	4.76	67.00	16.34		150.0	
		Z	4.53	66.86	16.18		150.0	
10198-CAC	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	4.65	66.75	16.12	0.00	150.0	± 9.6 %
		Y	4.79	67.02	16.35		150.0	
		Z	4.55	66.89	16.19		150.0	
10219-CAC	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	4.39	66.45	15.94	0.00	150.0	± 9.6 %
		Y	4.52	66.73	16.20		150.0	
		Z	4.30	66.62	16.00		150.0	
10220-CAC	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	4.61	66.69	16.10	0.00	150.0	± 9.6 %
		Y	4.75	66.97	16.33		150.0	
		Z	4.52	66.83	16.16		150.0	
10221-CAC	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	X	4.66	66.68	16.11	0.00	150.0	± 9.6 %
		Y	4.79	66.94	16.34		150.0	
		Z	4.56	66.82	16.18		150.0	
10222-CAC	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	4.99	66.85	16.23	0.00	150.0	± 9.6 %
		Y	5.11	67.15	16.44		150.0	
		Z	4.91	66.95	16.30		150.0	

Certificate No: EX3-3986_Mar18

Page 19 of 39

EX3DV4- SN:3986

March 23, 2018

10223-CAC	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	X	5.30	67.09	16.37	0.00	150.0	± 9.6 %
		Y	5.41	67.32	16.54		150.0	
		Z	5.20	67.18	16.44		150.0	
10224-CAC	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	X	5.03	66.96	16.21	0.00	150.0	± 9.6 %
		Y	5.15	67.26	16.42		150.0	
		Z	4.95	67.06	16.28		150.0	
10225-CAB	UMTS-FDD (HSPA+)	X	2.70	65.71	14.94	0.00	150.0	± 9.6 %
		Y	2.84	66.27	15.54		150.0	
		Z	2.63	66.03	14.97		150.0	
10226-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	17.72	101.23	29.97	6.02	65.0	± 9.6 %
		Y	100.00	130.99	37.69		65.0	
		Z	12.50	95.78	28.07		65.0	
10227-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	16.73	98.61	28.53	6.02	65.0	± 9.6 %
		Y	100.00	128.39	36.36		65.0	
		Z	12.03	93.63	26.72		65.0	
10228-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	10.51	96.09	30.34	6.02	65.0	± 9.6 %
		Y	56.61	129.39	39.92		65.0	
		Z	7.74	91.20	28.60		65.0	
10229-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	16.37	99.62	29.40	6.02	65.0	± 9.6 %
		Y	100.00	130.72	37.54		65.0	
		Z	11.59	94.28	27.50		65.0	
10230-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	15.42	97.09	28.00	6.02	65.0	± 9.6 %
		Y	100.00	128.20	36.23		65.0	
		Z	11.10	92.17	26.18		65.0	
10231-CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	9.94	94.88	29.86	6.02	65.0	± 9.6 %
		Y	50.39	126.82	39.17		65.0	
		Z	7.35	90.08	28.13		65.0	
10232-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	16.34	99.61	29.39	6.02	65.0	± 9.6 %
		Y	100.00	130.73	37.54		65.0	
		Z	11.57	94.26	27.50		65.0	
10233-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	15.38	97.06	27.99	6.02	65.0	± 9.6 %
		Y	100.00	128.22	36.24		65.0	
		Z	11.06	92.14	26.17		65.0	
10234-CAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	9.49	93.80	29.39	6.02	65.0	± 9.6 %
		Y	45.29	124.35	38.40		65.0	
		Z	7.04	89.09	27.66		65.0	
10235-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	16.37	99.65	29.41	6.02	65.0	± 9.6 %
		Y	100.00	130.75	37.55		65.0	
		Z	11.59	94.30	27.51		65.0	
10236-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	15.58	97.25	28.04	6.02	65.0	± 9.6 %
		Y	100.00	128.16	36.22		65.0	
		Z	11.20	92.30	26.22		65.0	
10237-CAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	9.96	94.96	29.89	6.02	65.0	± 9.6 %
		Y	51.22	127.19	39.27		65.0	
		Z	7.35	90.13	28.15		65.0	
10238-CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	16.30	99.59	29.38	6.02	65.0	± 9.6 %
		Y	100.00	130.75	37.54		65.0	
		Z	11.55	94.23	27.49		65.0	

Certificate No: EX3-3986_Mar18

Page 20 of 39

EX3DV4- SN:3986

March 23, 2018

10239- CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	15.33	97.02	27.98	6.02	65.0	± 9.6 %
		Y	100.00	128.24	36.25		65.0	
		Z	11.02	92.10	26.16		65.0	
10240- CAD	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	9.93	94.91	29.88	6.02	65.0	± 9.6 %
		Y	50.92	127.09	39.24		65.0	
		Z	7.34	90.09	28.14		65.0	
10241- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	8.09	81.11	25.41	6.98	65.0	± 9.6 %
		Y	10.68	86.56	27.75		65.0	
		Z	7.50	80.51	25.00		65.0	
10242- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	7.59	79.76	24.78	6.98	65.0	± 9.6 %
		Y	9.17	83.24	26.38		65.0	
		Z	6.85	78.62	24.14		65.0	
10243- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	6.17	76.50	24.29	6.98	65.0	± 9.6 %
		Y	7.04	78.99	25.60		65.0	
		Z	5.59	75.36	23.65		65.0	
10244- CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.22	76.53	18.78	3.98	65.0	± 9.6 %
		Y	9.70	83.29	21.88		65.0	
		Z	4.79	72.83	16.53		65.0	
10245- CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	6.01	75.72	18.40	3.98	65.0	± 9.6 %
		Y	9.27	82.28	21.46		65.0	
		Z	4.63	72.08	16.15		65.0	
10246- CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.91	79.07	19.83	3.98	65.0	± 9.6 %
		Y	11.56	89.71	24.25		65.0	
		Z	4.85	76.64	18.40		65.0	
10247- CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	5.13	74.06	18.53	3.98	65.0	± 9.6 %
		Y	6.95	78.87	21.05		65.0	
		Z	4.50	72.63	17.51		65.0	
10248- CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	5.08	73.39	18.23	3.98	65.0	± 9.6 %
		Y	6.79	77.94	20.66		65.0	
		Z	4.44	71.93	17.18		65.0	
10249- CAD	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	7.34	82.89	22.24	3.98	65.0	± 9.6 %
		Y	13.07	92.40	25.99		65.0	
		Z	6.62	82.00	21.62		65.0	
10250- CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	6.07	76.65	21.32	3.98	65.0	± 9.6 %
		Y	7.67	80.57	23.19		65.0	
		Z	5.57	76.00	20.91		65.0	
10251- CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	5.70	74.26	19.93	3.98	65.0	± 9.6 %
		Y	7.06	77.72	21.71		65.0	
		Z	5.19	73.43	19.41		65.0	
10252- CAD	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	7.33	82.13	22.98	3.98	65.0	± 9.6 %
		Y	10.80	88.75	25.62		65.0	
		Z	6.80	81.87	22.82		65.0	
10253- CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	5.75	73.31	19.89	3.98	65.0	± 9.6 %
		Y	6.88	76.25	21.41		65.0	
		Z	5.30	72.62	19.51		65.0	
10254- CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	6.12	74.29	20.64	3.98	65.0	± 9.6 %
		Y	7.27	77.13	22.08		65.0	
		Z	5.66	73.66	20.29		65.0	

Certificate No: EX3-3986_Mar18

Page 21 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10255-CAD	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.55	78.08	21.68	3.98	65.0	± 9.6 %
		Y	8.49	82.29	23.51		65.0	
		Z	6.08	77.71	21.52		65.0	
10256-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	4.63	71.83	15.72	3.98	65.0	± 9.6 %
		Y	7.77	79.22	19.37		65.0	
		Z	3.35	67.67	13.01		65.0	
10257-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	4.45	70.89	15.21	3.98	65.0	± 9.6 %
		Y	7.29	77.85	18.75		65.0	
		Z	3.26	66.98	12.57		65.0	
10258-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	4.19	73.45	16.69	3.98	65.0	± 9.6 %
		Y	8.43	83.93	21.48		65.0	
		Z	3.15	68.94	14.53		65.0	
10259-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	5.51	75.06	19.55	3.98	65.0	± 9.6 %
		Y	7.23	79.45	21.80		65.0	
		Z	4.94	74.01	18.80		65.0	
10260-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	5.52	74.74	19.42	3.98	65.0	± 9.6 %
		Y	7.18	78.97	21.62		65.0	
		Z	4.95	73.66	18.65		65.0	
10261-CAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	6.88	81.53	22.18	3.98	65.0	± 9.6 %
		Y	10.97	89.28	25.35		65.0	
		Z	6.29	80.92	21.74		65.0	
10262-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	6.05	76.59	21.27	3.98	65.0	± 9.6 %
		Y	7.66	80.51	23.15		65.0	
		Z	5.55	75.92	20.86		65.0	
10263-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	5.69	74.23	19.92	3.98	65.0	± 9.6 %
		Y	7.05	77.70	21.70		65.0	
		Z	5.18	73.41	19.40		65.0	
10264-CAD	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	7.24	81.90	22.87	3.98	65.0	± 9.6 %
		Y	10.76	88.49	25.51		65.0	
		Z	6.71	81.61	22.69		65.0	
10265-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	5.87	73.85	20.15	3.98	65.0	± 9.6 %
		Y	7.11	77.01	21.71		65.0	
		Z	5.39	73.09	19.77		65.0	
10266-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	6.27	74.89	20.97	3.98	65.0	± 9.6 %
		Y	7.51	77.90	22.43		65.0	
		Z	5.80	74.24	20.65		65.0	
10267-CAD	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.90	78.78	21.73	3.98	65.0	± 9.6 %
		Y	9.07	83.20	23.59		65.0	
		Z	6.40	78.40	21.60		65.0	
10268-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	6.48	73.71	20.50	3.98	65.0	± 9.6 %
		Y	7.55	76.25	21.75		65.0	
		Z	6.02	73.03	20.20		65.0	
10269-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	6.45	73.28	20.37	3.98	65.0	± 9.6 %
		Y	7.45	75.69	21.58		65.0	
		Z	6.00	72.62	20.06		65.0	
10270-CAD	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.63	75.84	20.71	3.98	65.0	± 9.6 %
		Y	8.01	78.85	22.05		65.0	
		Z	6.17	75.38	20.54		65.0	

Certificate No: EX3-3986_Mar18

Page 22 of 39

EX3DV4-SN.3986

March 23, 2018

10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	2.48	65.99	14.80	0.00	150.0	± 9.6 %
		Y	2.61	66.64	15.45		150.0	
		Z	2.44	66.48	14.91		150.0	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	1.47	66.73	14.65	0.00	150.0	± 9.6 %
		Y	1.68	68.76	16.06		150.0	
		Z	1.47	67.69	15.06		150.0	
10277-CAA	PHS (QPSK)	X	2.32	61.94	7.59	9.03	50.0	± 9.6 %
		Y	2.63	63.26	8.69		50.0	
		Z	2.06	60.99	6.58		50.0	
10278-CAA	PHS (QPSK, BW 884MHz, Rolloff 0.5)	X	5.06	73.13	15.91	9.03	50.0	± 9.6 %
		Y	12.53	87.52	22.04		50.0	
		Z	3.78	68.67	13.19		50.0	
10279-CAA	PHS (QPSK, BW 884MHz, Rolloff 0.38)	X	5.20	73.44	16.09	9.03	50.0	± 9.6 %
		Y	12.80	87.76	22.18		50.0	
		Z	3.89	68.96	13.38		50.0	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	1.17	66.14	12.16	0.00	150.0	± 9.6 %
		Y	1.66	70.46	15.07		150.0	
		Z	1.03	65.62	11.24		150.0	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	0.66	63.57	10.55	0.00	150.0	± 9.6 %
		Y	0.91	67.19	13.43		150.0	
		Z	0.58	63.11	9.57		150.0	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	0.79	66.46	12.40	0.00	150.0	± 9.6 %
		Y	1.30	73.15	16.54		150.0	
		Z	0.75	66.83	11.80		150.0	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	1.16	71.44	15.16	0.00	150.0	± 9.6 %
		Y	2.41	82.34	20.58		150.0	
		Z	1.60	75.90	16.08		150.0	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	10.03	86.00	24.00	9.03	50.0	± 9.6 %
		Y	12.55	91.91	27.07		50.0	
		Z	11.15	86.76	23.45		50.0	
10297-AAC	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	2.58	68.81	16.01	0.00	150.0	± 9.6 %
		Y	2.87	70.35	16.91		150.0	
		Z	2.57	69.47	16.37		150.0	
10298-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	1.35	65.89	12.76	0.00	150.0	± 9.6 %
		Y	1.73	68.98	15.02		150.0	
		Z	1.22	65.64	12.10		150.0	
10299-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	2.41	68.80	13.81	0.00	150.0	± 9.6 %
		Y	3.51	73.26	16.22		150.0	
		Z	1.89	66.17	11.78		150.0	
10300-AAC	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	1.80	64.35	10.90	0.00	150.0	± 9.6 %
		Y	2.37	67.11	12.76		150.0	
		Z	1.46	62.68	9.26		150.0	
10301-AAA	IEEE 802.16e WiMAX (29.18, 5ms, 10MHz, QPSK, PUSC)	X	4.74	65.49	17.34	4.17	50.0	± 9.6 %
		Y	5.08	66.54	18.09		50.0	
		Z	4.70	66.13	17.61		50.0	
10302-AAA	IEEE 802.16e WiMAX (29.18, 5ms, 10MHz, QPSK, PUSC, 3 CTRL symbols)	X	5.22	66.09	18.04	4.96	50.0	± 9.6 %
		Y	5.47	66.76	18.59		50.0	
		Z	5.07	66.14	17.97		50.0	

Certificate No: EX3-3986_Mar18

Page 23 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10303-AAA	IEEE 802.16e WiMAX (31:15, 5ms, 10MHz, 64QAM, PUSC)	X	4.98	65.77	17.88	4.96	50.0	± 9.6 %
		Y	5.24	66.50	18.49		50.0	
		Z	4.83	65.80	17.79		50.0	
10304-AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, 64QAM, PUSC)	X	4.77	65.58	17.35	4.17	50.0	± 9.6 %
		Y	5.02	66.24	17.89		50.0	
		Z	4.63	65.67	17.30		50.0	
10305-AAA	IEEE 802.16e WiMAX (31:15, 10ms, 10MHz, 64QAM, PUSC, 15 symbols)	X	4.63	68.59	19.90	6.02	35.0	± 9.6 %
		Y	4.88	69.47	20.83		35.0	
		Z	4.52	68.82	19.72		35.0	
10306-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 64QAM, PUSC, 18 symbols)	X	4.84	67.16	19.33	6.02	35.0	± 9.6 %
		Y	5.06	67.80	20.03		35.0	
		Z	4.71	67.32	19.20		35.0	
10307-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, PUSC, 18 symbols)	X	4.76	67.41	19.32	6.02	35.0	± 9.6 %
		Y	5.00	68.17	20.09		35.0	
		Z	4.62	67.51	19.17		35.0	
10308-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, PUSC)	X	4.74	67.66	19.48	6.02	35.0	± 9.6 %
		Y	4.98	68.42	20.25		35.0	
		Z	4.62	67.79	19.34		35.0	
10309-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, AMC 2x3, 18 symbols)	X	4.90	67.37	19.47	6.02	35.0	± 9.6 %
		Y	5.14	68.11	20.22		35.0	
		Z	4.78	67.48	19.32		35.0	
10310-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, AMC 2x3, 18 symbols)	X	4.80	67.26	19.32	6.02	35.0	± 9.6 %
		Y	5.02	67.92	20.03		35.0	
		Z	4.67	67.43	19.20		35.0	
10311-AAC	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	2.93	68.13	15.71	0.00	150.0	± 9.6 %
		Y	3.24	69.60	16.54		150.0	
		Z	2.93	68.70	16.04		150.0	
10313-AAA	iDEN 1:3	X	3.90	73.75	16.24	6.99	70.0	± 9.6 %
		Y	8.85	83.91	20.06		70.0	
		Z	3.14	71.69	15.18		70.0	
10314-AAA	iDEN 1:6	X	6.31	83.38	22.66	10.00	30.0	± 9.6 %
		Y	18.89	101.35	28.57		30.0	
		Z	6.05	82.79	22.10		30.0	
10315-AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	1.01	63.14	14.57	0.17	150.0	± 9.6 %
		Y	1.09	64.45	15.70		150.0	
		Z	0.98	63.59	14.92		150.0	
10316-AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	X	4.50	66.46	16.12	0.17	150.0	± 9.6 %
		Y	4.63	66.75	16.39		150.0	
		Z	4.41	66.59	16.17		150.0	
10317-AAC	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	X	4.50	66.46	16.12	0.17	150.0	± 9.6 %
		Y	4.63	66.75	16.39		150.0	
		Z	4.41	66.59	16.17		150.0	
10400-AAD	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	4.59	66.74	16.08	0.00	150.0	± 9.6 %
		Y	4.74	67.04	16.32		150.0	
		Z	4.49	66.88	16.15		150.0	
10401-AAD	IEEE 802.11ac WiFi (40MHz, 64-QAM, 99pc duty cycle)	X	5.32	67.00	16.30	0.00	150.0	± 9.6 %
		Y	5.40	67.14	16.43		150.0	
		Z	5.21	67.00	16.31		150.0	

Certificate No: EX3-3986_Mar18

Page 24 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10402-AAD	IEEE 802.11ac WiFi (80MHz, 64-QAM, 99pc duty cycle)	X	5.56	67.25	16.29	0.00	150.0	± 9.6 %
		Y	5.68	67.55	16.49		150.0	
		Z	5.47	67.30	16.33		150.0	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	1.17	66.14	12.16	0.00	115.0	± 9.6 %
		Y	1.66	70.46	15.07		115.0	
		Z	1.03	65.62	11.24		115.0	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	1.17	66.14	12.16	0.00	115.0	± 9.6 %
		Y	1.66	70.46	15.07		115.0	
		Z	1.03	65.62	11.24		115.0	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	46.77	113.74	29.04	0.00	100.0	± 9.6 %
		Y	100.00	120.68	30.10		100.0	
		Z	100.00	121.56	29.86		100.0	
10410-AAD	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9, Subframe Conf=4)	X	100.00	124.09	31.23	3.23	80.0	± 9.6 %
		Y	100.00	122.11	30.71		80.0	
		Z	100.00	122.65	30.11		80.0	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	0.94	62.29	13.96	0.00	150.0	± 9.6 %
		Y	0.99	63.27	14.93		150.0	
		Z	0.91	62.78	14.34		150.0	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	4.44	66.43	16.04	0.00	150.0	± 9.6 %
		Y	4.56	66.68	16.27		150.0	
		Z	4.36	66.59	16.11		150.0	
10417-AAB	IEEE 802.11a/n WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	4.44	66.43	16.04	0.00	150.0	± 9.6 %
		Y	4.56	66.68	16.27		150.0	
		Z	4.36	66.59	16.11		150.0	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	4.43	66.59	16.05	0.00	150.0	± 9.6 %
		Y	4.55	66.83	16.28		150.0	
		Z	4.35	66.78	16.15		150.0	
10419-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preamble)	X	4.45	66.54	16.06	0.00	150.0	± 9.6 %
		Y	4.57	66.78	16.28		150.0	
		Z	4.37	66.72	16.14		150.0	
10422-AAB	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	4.57	66.54	16.08	0.00	150.0	± 9.6 %
		Y	4.69	66.78	16.30		150.0	
		Z	4.48	66.70	16.15		150.0	
10423-AAB	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	4.73	66.84	16.19	0.00	150.0	± 9.6 %
		Y	4.87	67.12	16.42		150.0	
		Z	4.62	66.98	16.25		150.0	
10424-AAB	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	X	4.65	66.79	16.16	0.00	150.0	± 9.6 %
		Y	4.79	67.07	16.39		150.0	
		Z	4.55	66.94	16.23		150.0	
10425-AAB	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	5.26	67.12	16.36	0.00	150.0	± 9.6 %
		Y	5.37	67.36	16.54		150.0	
		Z	5.16	67.18	16.41		150.0	
10426-AAB	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	X	5.27	67.17	16.39	0.00	150.0	± 9.6 %
		Y	5.37	67.37	16.54		150.0	
		Z	5.18	67.26	16.45		150.0	

Certificate No: EX3-3986_Mar18

Page 25 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2016

10427-AAB	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	5.28	67.13	16.36	0.00	150.0	± 9.6 %
		Y	5.39	67.36	16.53		150.0	
		Z	5.17	67.16	16.39		150.0	
10430-AAB	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	4.18	70.80	18.04	0.00	150.0	± 9.6 %
		Y	4.29	70.89	18.24		150.0	
		Z	4.25	71.95	18.43		150.0	
10431-AAB	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	4.10	66.93	15.97	0.00	150.0	± 9.6 %
		Y	4.27	67.25	16.31		150.0	
		Z	4.00	67.16	16.03		150.0	
10432-AAB	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	4.41	66.83	16.09	0.00	150.0	± 9.6 %
		Y	4.56	67.12	16.35		150.0	
		Z	4.31	67.01	16.16		150.0	
10433-AAB	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	4.66	66.83	16.18	0.00	150.0	± 9.6 %
		Y	4.81	67.11	16.41		150.0	
		Z	4.57	66.97	16.25		150.0	
10434-AAA	W-CDMA (BS Test Model 1, 64 DPCH)	X	4.28	71.62	17.95	0.00	150.0	± 9.6 %
		Y	4.41	71.57	18.25		150.0	
		Z	4.39	72.94	18.33		150.0	
10435-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	123.85	31.12	3.23	80.0	± 9.6 %
		Y	100.00	121.91	30.61		80.0	
		Z	100.00	122.38	29.98		80.0	
10447-AAB	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.37	66.79	15.14	0.00	150.0	± 9.6 %
		Y	3.58	67.35	15.75		150.0	
		Z	3.26	67.04	15.07		150.0	
10448-AAB	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.95	66.71	15.83	0.00	150.0	± 9.6 %
		Y	4.10	67.04	16.17		150.0	
		Z	3.85	66.95	15.90		150.0	
10449-AAB	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	4.23	66.65	15.98	0.00	150.0	± 9.6 %
		Y	4.37	66.96	16.25		150.0	
		Z	4.14	66.84	16.06		150.0	
10450-AAB	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.43	66.59	16.03	0.00	150.0	± 9.6 %
		Y	4.55	66.88	16.27		150.0	
		Z	4.35	66.75	16.10		150.0	
10451-AAA	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	X	3.24	66.85	14.66	0.00	150.0	± 9.6 %
		Y	3.49	67.60	15.43		150.0	
		Z	3.10	66.96	14.45		150.0	
10456-AAB	IEEE 802.11ac WiFi (160MHz, 64-QAM, 99pc duty cycle)	X	6.14	67.69	16.54	0.00	150.0	± 9.6 %
		Y	6.23	67.92	16.68		150.0	
		Z	6.09	67.82	16.62		150.0	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	3.72	65.07	15.74	0.00	150.0	± 9.6 %
		Y	3.79	65.31	15.99		150.0	
		Z	3.66	65.26	15.82		150.0	
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	3.88	70.67	17.18	0.00	150.0	± 9.6 %
		Y	4.04	70.81	17.70		150.0	
		Z	3.90	71.61	17.29		150.0	
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	5.04	68.54	18.12	0.00	150.0	± 9.6 %
		Y	5.09	68.03	18.09		150.0	
		Z	5.02	69.30	18.32		150.0	

Certificate No: EX3-3986_Mar16

Page 26 of 39

EX3DV4- SN:3986

March 23, 2018

10460-AAA	UMTS-FDD (WCDMA, AMR)	X	0.77	66.27	14.61	0.00	150.0	± 9.6 %
		Y	0.96	69.93	17.08		150.0	
		Z	0.80	68.22	15.57		150.0	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	128.15	33.18	3.29	80.0	± 9.6 %
		Y	100.00	128.48	33.65		80.0	
		Z	100.00	126.48	31.96		80.0	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.72	76.43	15.54	3.23	80.0	± 9.6 %
		Y	100.00	107.67	23.93		80.0	
		Z	1.15	62.81	9.58		80.0	
10463-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.64	65.14	10.79	3.23	80.0	± 9.6 %
		Y	95.50	103.01	21.87		80.0	
		Z	0.87	60.00	7.65		80.0	
10464-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.33	31.71	3.23	80.0	± 9.6 %
		Y	100.00	126.00	32.34		80.0	
		Z	100.00	122.97	30.19		80.0	
10465-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.06	71.95	13.94	3.23	80.0	± 9.6 %
		Y	100.00	106.97	23.59		80.0	
		Z	1.05	61.96	9.11		80.0	
10466-AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.46	63.94	10.22	3.23	80.0	± 9.6 %
		Y	18.76	87.35	18.09		80.0	
		Z	0.87	60.00	7.60		80.0	
10467-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.65	31.85	3.23	80.0	± 9.6 %
		Y	100.00	126.28	32.46		80.0	
		Z	100.00	123.35	30.35		80.0	
10468-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.38	73.00	14.33	3.23	80.0	± 9.6 %
		Y	100.00	107.17	23.68		80.0	
		Z	1.08	62.19	9.24		80.0	
10469-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.46	63.98	10.23	3.23	80.0	± 9.6 %
		Y	19.59	87.76	18.20		80.0	
		Z	0.87	60.00	7.60		80.0	
10470-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.69	31.86	3.23	80.0	± 9.6 %
		Y	100.00	126.32	32.47		80.0	
		Z	100.00	123.36	30.35		80.0	
10471-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.34	72.85	14.27	3.23	80.0	± 9.6 %
		Y	100.00	107.10	23.64		80.0	
		Z	1.07	62.13	9.20		80.0	
10472-AAC	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.45	63.91	10.19	3.23	80.0	± 9.6 %
		Y	19.04	87.45	18.10		80.0	
		Z	0.87	60.00	7.58		80.0	
10473-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.65	31.84	3.23	80.0	± 9.6 %
		Y	100.00	126.28	32.45		80.0	
		Z	100.00	123.32	30.33		80.0	
10474-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.30	72.75	14.23	3.23	80.0	± 9.6 %
		Y	100.00	107.10	23.65		80.0	
		Z	1.06	62.11	9.19		80.0	
10475-AAC	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.44	63.88	10.18	3.23	80.0	± 9.6 %
		Y	18.53	87.21	18.04		80.0	
		Z	0.86	60.00	7.58		80.0	

Certificate No: EX3-3986_Mar18

Page 27 of 39

EX3DV4- SN:3986

March 23, 2018

10477-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.05	71.92	13.91	3.23	80.0	± 9.6 %
		Y	100.00	106.89	23.55		80.0	
		Z	1.04	61.90	9.07		80.0	
10478-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.44	63.82	10.14	3.23	80.0	± 9.6 %
		Y	17.65	86.71	17.89		80.0	
		Z	0.87	60.00	7.57		80.0	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	12.13	93.77	25.48	3.23	80.0	± 9.6 %
		Y	23.81	104.28	26.95		80.0	
		Z	14.46	96.25	25.53		80.0	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	10.36	85.51	20.93	3.23	80.0	± 9.6 %
		Y	31.61	100.68	25.78		80.0	
		Z	6.75	79.70	18.25		80.0	
10481-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	7.38	80.27	18.84	3.23	80.0	± 9.6 %
		Y	21.55	94.30	23.62		80.0	
		Z	4.33	73.65	15.73		80.0	
10482-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.78	70.99	16.08	2.23	80.0	± 9.6 %
		Y	6.04	81.91	20.93		80.0	
		Z	2.41	69.87	15.10		80.0	
10483-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.95	75.15	17.41	2.23	80.0	± 9.6 %
		Y	9.71	84.52	21.33		80.0	
		Z	3.09	69.23	14.26		80.0	
10484-AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.48	73.59	16.82	2.23	80.0	± 9.6 %
		Y	8.36	82.19	20.58		80.0	
		Z	2.87	68.10	13.79		80.0	
10485-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.25	73.11	18.00	2.23	80.0	± 9.6 %
		Y	5.68	81.42	21.68		80.0	
		Z	3.16	73.67	17.95		80.0	
10486-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.06	68.85	15.68	2.23	80.0	± 9.6 %
		Y	4.35	73.76	18.36		80.0	
		Z	2.79	68.32	15.05		80.0	
10487-AAC	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.05	68.45	15.50	2.23	80.0	± 9.6 %
		Y	4.27	73.09	18.08		80.0	
		Z	2.77	67.84	14.82		80.0	
10488-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.53	72.37	18.49	2.23	80.0	± 9.6 %
		Y	5.10	77.92	21.01		80.0	
		Z	3.38	72.75	18.63		80.0	
10489-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.41	68.87	17.05	2.23	80.0	± 9.6 %
		Y	4.18	71.77	18.66		80.0	
		Z	3.25	68.98	16.98		80.0	
10490-AAC	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.50	68.71	16.99	2.23	80.0	± 9.6 %
		Y	4.24	71.40	18.51		80.0	
		Z	3.33	68.79	16.91		80.0	
10491-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.74	70.85	18.03	2.23	80.0	± 9.6 %
		Y	4.85	74.73	19.87		80.0	
		Z	3.56	70.96	18.10		80.0	
10492-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.76	68.15	17.08	2.23	80.0	± 9.6 %
		Y	4.37	70.33	18.30		80.0	
		Z	3.57	68.12	17.02		80.0	

Certificate No: EX3-3986_Mar18

Page 28 of 39

EX3DV4- SN-3986

March 23, 2018

10493-AAC	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.82	68.02	17.03	2.23	80.0	± 9.6 %
		Y	4.42	70.10	18.22		80.0	
		Z	3.63	67.98	16.97		80.0	
10494-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.06	72.33	18.48	2.23	80.0	± 9.6 %
		Y	5.56	77.11	20.60		80.0	
		Z	3.87	72.49	18.59		80.0	
10495-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.79	68.51	17.27	2.23	80.0	± 9.6 %
		Y	4.45	70.90	18.55		80.0	
		Z	3.60	68.46	17.23		80.0	
10496-AAC	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.87	68.26	17.20	2.23	80.0	± 9.6 %
		Y	4.49	70.43	18.39		80.0	
		Z	3.68	68.20	17.15		80.0	
10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.85	65.78	12.75	2.23	80.0	± 9.6 %
		Y	4.52	77.28	18.35		80.0	
		Z	1.37	62.97	10.69		80.0	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.46	60.79	9.22	2.23	80.0	± 9.6 %
		Y	2.58	66.94	13.16		80.0	
		Z	1.24	60.00	8.02		80.0	
10499-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.42	60.33	8.83	2.23	80.0	± 9.6 %
		Y	2.44	65.98	12.58		80.0	
		Z	1.26	60.00	7.87		80.0	
10500-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.31	72.52	18.10	2.23	80.0	± 9.6 %
		Y	5.16	79.14	21.14		80.0	
		Z	3.21	73.08	18.16		80.0	
10501-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.24	68.98	16.26	2.23	80.0	± 9.6 %
		Y	4.25	72.83	18.42		80.0	
		Z	3.04	68.89	15.93		80.0	
10502-AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.29	68.82	16.14	2.23	80.0	± 9.6 %
		Y	4.29	72.54	18.24		80.0	
		Z	3.07	68.67	15.76		80.0	
10503-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.48	72.16	18.39	2.23	80.0	± 9.6 %
		Y	5.02	77.66	20.89		80.0	
		Z	3.33	72.51	18.51		80.0	
10504-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.39	68.77	16.98	2.23	80.0	± 9.6 %
		Y	4.15	71.67	18.60		80.0	
		Z	3.23	68.86	16.91		80.0	
10505-AAC	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.48	68.61	16.93	2.23	80.0	± 9.6 %
		Y	4.21	71.30	18.46		80.0	
		Z	3.31	68.68	16.84		80.0	
10506-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.02	72.18	18.41	2.23	80.0	± 9.6 %
		Y	5.51	76.93	20.52		80.0	
		Z	3.84	72.32	18.50		80.0	
10507-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.77	68.45	17.23	2.23	80.0	± 9.6 %
		Y	4.43	70.83	18.51		80.0	
		Z	3.59	68.39	17.19		80.0	

EX3DV4- SN:3986

March 23, 2018

10508-AAC	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.85	68.18	17.15	2.23	80.0	± 9.6 %
		Y	4.47	70.36	18.34		80.0	
		Z	3.66	68.12	17.11		80.0	
10509-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.35	70.93	17.92	2.23	80.0	± 9.6 %
		Y	5.45	74.34	19.50		80.0	
		Z	4.16	70.93	17.97		80.0	
10510-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.26	68.19	17.24	2.23	80.0	± 9.6 %
		Y	4.86	70.17	18.29		80.0	
		Z	4.05	68.03	17.18		80.0	
10511-AAC	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.31	67.95	17.18	2.23	80.0	± 9.6 %
		Y	4.87	69.78	18.17		80.0	
		Z	4.11	67.80	17.12		80.0	
10512-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.55	72.44	18.38	2.23	80.0	± 9.6 %
		Y	6.09	76.91	20.33		80.0	
		Z	4.35	72.47	18.44		80.0	
10513-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.14	68.44	17.33	2.23	80.0	± 9.6 %
		Y	4.79	70.65	18.49		80.0	
		Z	3.94	68.25	17.28		80.0	
10514-AAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.17	68.03	17.22	2.23	80.0	± 9.6 %
		Y	4.75	70.03	18.28		80.0	
		Z	3.27	67.86	17.16		80.0	
10515-AAC	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	0.90	62.42	13.98	0.00	150.0	± 9.6 %
		Y	0.96	63.49	15.01		150.0	
		Z	0.88	62.96	14.39		150.0	
10516-AAC	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle)	X	0.46	67.31	14.81	0.00	150.0	± 9.6 %
		Y	0.72	74.97	19.43		150.0	
		Z	0.55	71.70	16.89		150.0	
10517-AAC	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)	X	0.73	63.87	14.23	0.00	150.0	± 9.6 %
		Y	0.82	65.90	15.90		150.0	
		Z	0.72	64.87	14.90		150.0	
10518-AAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	4.43	66.50	16.01	0.00	150.0	± 9.6 %
		Y	4.56	66.75	16.25		150.0	
		Z	4.35	66.68	16.09		150.0	
10519-AAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)	X	4.61	66.73	16.13	0.00	150.0	± 9.6 %
		Y	4.75	67.00	16.37		150.0	
		Z	4.51	66.87	16.19		150.0	
10520-AAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)	X	4.46	66.67	16.04	0.00	150.0	± 9.6 %
		Y	4.61	66.98	16.30		150.0	
		Z	4.37	66.82	16.11		150.0	
10521-AAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)	X	4.40	66.66	16.02	0.00	150.0	± 9.6 %
		Y	4.54	66.98	16.29		150.0	
		Z	4.30	66.80	16.09		150.0	
10522-AAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)	X	4.46	66.77	16.12	0.00	150.0	± 9.6 %
		Y	4.60	67.04	16.36		150.0	
		Z	4.36	66.93	16.20		150.0	

Certificate No: EX3-3986_Mar18

Page 30 of 39

EX3DV4- SN:3986

March 23, 2018

10523-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle)	X	4.34	66.64	15.97	0.00	150.0	± 9.6 %
		Y	4.47	66.91	16.20		150.0	
		Z	4.26	66.85	16.07		150.0	
10524-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	X	4.40	66.68	16.08	0.00	150.0	± 9.6 %
		Y	4.54	66.96	16.33		150.0	
		Z	4.30	66.86	16.17		150.0	
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	4.39	65.74	15.68	0.00	150.0	± 9.6 %
		Y	4.52	66.01	15.92		150.0	
		Z	4.32	65.93	15.78		150.0	
10526-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	4.55	66.09	15.82	0.00	150.0	± 9.6 %
		Y	4.70	66.39	16.06		150.0	
		Z	4.46	66.25	15.91		150.0	
10527-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)	X	4.47	66.04	15.76	0.00	150.0	± 9.6 %
		Y	4.62	66.36	16.01		150.0	
		Z	4.39	66.22	15.85		150.0	
10528-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle)	X	4.49	66.06	15.79	0.00	150.0	± 9.6 %
		Y	4.63	66.38	16.04		150.0	
		Z	4.40	66.23	15.88		150.0	
10529-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)	X	4.49	66.06	15.79	0.00	150.0	± 9.6 %
		Y	4.63	66.38	16.04		150.0	
		Z	4.40	66.23	15.88		150.0	
10531-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)	X	4.47	66.15	15.79	0.00	150.0	± 9.6 %
		Y	4.63	66.50	16.06		150.0	
		Z	4.38	66.29	15.87		150.0	
10532-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle)	X	4.34	65.99	15.72	0.00	150.0	± 9.6 %
		Y	4.49	66.36	16.00		150.0	
		Z	4.25	66.15	15.80		150.0	
10533-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)	X	4.50	66.11	15.78	0.00	150.0	± 9.6 %
		Y	4.65	66.42	16.03		150.0	
		Z	4.41	66.30	15.88		150.0	
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	5.03	66.18	15.88	0.00	150.0	± 9.6 %
		Y	5.16	66.48	16.08		150.0	
		Z	4.95	66.29	15.95		150.0	
10535-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	5.10	66.37	15.96	0.00	150.0	± 9.6 %
		Y	5.22	66.63	16.15		150.0	
		Z	5.01	66.45	16.03		150.0	
10536-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle)	X	4.97	66.31	15.91	0.00	150.0	± 9.6 %
		Y	5.09	66.61	16.12		150.0	
		Z	4.89	66.43	15.99		150.0	
10537-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)	X	5.03	66.28	15.90	0.00	150.0	± 9.6 %
		Y	5.15	66.57	16.10		150.0	
		Z	4.94	66.38	15.98		150.0	
10538-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)	X	5.11	66.29	15.95	0.00	150.0	± 9.6 %
		Y	5.25	66.61	16.16		150.0	
		Z	5.02	66.38	16.01		150.0	
10540-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	X	5.05	66.31	15.97	0.00	150.0	± 9.6 %
		Y	5.17	66.60	16.17		150.0	
		Z	4.95	66.36	16.02		150.0	

Certificate No: EX3-3986_Mar18

Page 31 of 39

EX30V4- SN:3986

March 23, 2018

10541-AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)	X	5.02	66.18	15.90	0.00	150.0	± 9.6 %
		Y	5.15	66.48	16.11		150.0	
		Z	4.93	66.26	15.95		150.0	
10542-AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)	X	5.18	66.26	15.96	0.00	150.0	± 9.6 %
		Y	5.30	66.54	16.15		150.0	
		Z	5.09	66.35	16.02		150.0	
10543-AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	X	5.25	66.29	16.00	0.00	150.0	± 9.6 %
		Y	5.38	66.57	16.18		150.0	
		Z	5.15	66.36	16.05		150.0	
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	5.35	66.31	15.88	0.00	150.0	± 9.6 %
		Y	5.45	66.59	16.07		150.0	
		Z	5.28	66.38	15.94		150.0	
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	5.54	66.73	16.05	0.00	150.0	± 9.6 %
		Y	5.65	66.98	16.21		150.0	
		Z	5.46	66.81	16.11		150.0	
10546-AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	X	5.41	66.49	15.94	0.00	150.0	± 9.6 %
		Y	5.53	66.82	16.15		150.0	
		Z	5.32	66.53	15.98		150.0	
10547-AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	X	5.48	66.54	15.96	0.00	150.0	± 9.6 %
		Y	5.60	66.86	16.16		150.0	
		Z	5.40	66.60	16.01		150.0	
10548-AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	X	5.71	67.42	16.37	0.00	150.0	± 9.6 %
		Y	5.85	67.78	16.59		150.0	
		Z	5.59	67.37	16.37		150.0	
10550-AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	X	5.44	66.54	15.98	0.00	150.0	± 9.6 %
		Y	5.55	66.81	16.15		150.0	
		Z	5.37	66.64	16.05		150.0	
10551-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	X	5.44	66.56	15.95	0.00	150.0	± 9.6 %
		Y	5.56	66.86	16.14		150.0	
		Z	5.34	66.56	15.98		150.0	
10552-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	X	5.36	66.37	15.86	0.00	150.0	± 9.6 %
		Y	5.47	66.66	16.05		150.0	
		Z	5.29	66.46	15.93		150.0	
10553-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	X	5.44	66.40	15.91	0.00	150.0	± 9.6 %
		Y	5.56	66.70	16.10		150.0	
		Z	5.36	66.45	15.96		150.0	
10554-AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	X	5.76	66.67	15.98	0.00	150.0	± 9.6 %
		Y	5.85	66.94	16.15		150.0	
		Z	5.70	66.72	16.02		150.0	
10555-AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	X	5.89	66.97	16.10	0.00	150.0	± 9.6 %
		Y	5.98	67.24	16.28		150.0	
		Z	5.81	66.99	16.14		150.0	
10556-AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	X	5.91	67.02	16.12	0.00	150.0	± 9.6 %
		Y	6.00	67.29	16.30		150.0	
		Z	5.84	67.06	16.17		150.0	
10557-AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	X	5.87	66.91	16.09	0.00	150.0	± 9.6 %
		Y	5.98	67.21	16.28		150.0	
		Z	5.79	66.94	16.13		150.0	

Certificate No: EX3-3986_Mar18

Page 32 of 39

EX3DV4- SN:3986

March 23, 2018

10558-AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	X	5.92	67.06	16.18	0.00	150.0	± 9.6 %
		Y	6.03	67.38	16.38		150.0	
		Z	5.83	67.08	16.21		150.0	
10560-AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	X	5.91	66.92	16.15	0.00	150.0	± 9.6 %
		Y	6.03	67.24	16.34		150.0	
		Z	5.83	66.95	16.18		150.0	
10561-AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 99pc duty cycle)	X	5.84	66.89	16.17	0.00	150.0	± 9.6 %
		Y	5.94	67.19	16.36		150.0	
		Z	5.76	66.93	16.21		150.0	
10562-AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	X	5.95	67.23	16.34	0.00	150.0	± 9.6 %
		Y	6.08	67.60	16.57		150.0	
		Z	5.84	67.19	16.34		150.0	
10563-AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	X	6.10	67.31	16.34	0.00	150.0	± 9.6 %
		Y	6.38	68.10	16.76		150.0	
		Z	5.92	67.08	16.25		150.0	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	4.76	66.58	16.17	0.46	150.0	± 9.6 %
		Y	4.89	66.84	16.41		150.0	
		Z	4.67	66.71	16.22		150.0	
10565-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle)	X	4.98	67.03	16.51	0.46	150.0	± 9.6 %
		Y	5.13	67.30	16.73		150.0	
		Z	4.88	67.15	16.56		150.0	
10566-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle)	X	4.82	66.86	16.31	0.46	150.0	± 9.6 %
		Y	4.96	67.16	16.56		150.0	
		Z	4.71	66.97	16.36		150.0	
10567-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle)	X	4.85	67.27	16.68	0.46	150.0	± 9.6 %
		Y	4.99	67.55	16.90		150.0	
		Z	4.75	67.42	16.76		150.0	
10568-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle)	X	4.73	66.62	16.07	0.46	150.0	± 9.6 %
		Y	4.87	66.93	16.33		150.0	
		Z	4.62	66.72	16.10		150.0	
10569-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle)	X	4.81	67.39	16.76	0.46	150.0	± 9.6 %
		Y	4.94	67.61	16.95		150.0	
		Z	4.73	67.60	16.87		150.0	
10570-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle)	X	4.84	67.22	16.68	0.46	150.0	± 9.6 %
		Y	4.98	67.46	16.89		150.0	
		Z	4.74	67.38	16.76		150.0	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	1.10	63.80	14.95	0.46	130.0	± 9.6 %
		Y	1.21	65.51	16.29		130.0	
		Z	1.06	64.12	15.22		130.0	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	1.11	64.33	15.29	0.46	130.0	± 9.6 %
		Y	1.24	66.20	16.70		130.0	
		Z	1.07	64.73	15.61		130.0	
10573-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	X	1.44	79.67	20.19	0.46	130.0	± 9.6 %
		Y	15.56	118.71	32.74		130.0	
		Z	2.54	90.27	23.90		130.0	
10574-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)	X	1.18	69.56	17.92	0.46	130.0	± 9.6 %
		Y	1.50	73.90	20.41		130.0	
		Z	1.19	71.21	18.87		130.0	

Certificate No: EX3-3986_Mar18

Page 33 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	4.55	66.38	16.23	0.46	130.0	± 9.6 %
		Y	4.68	66.67	16.50		130.0	
		Z	4.45	66.51	16.27		130.0	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	4.58	66.56	16.30	0.46	130.0	± 9.6 %
		Y	4.71	66.83	16.56		130.0	
		Z	4.48	66.70	16.35		130.0	
10577-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle)	X	4.77	66.84	16.47	0.46	130.0	± 9.6 %
		Y	4.92	67.13	16.73		130.0	
		Z	4.66	66.96	16.51		130.0	
10578-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle)	X	4.67	67.00	16.57	0.46	130.0	± 9.6 %
		Y	4.82	67.30	16.83		130.0	
		Z	4.57	67.13	16.63		130.0	
10579-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle)	X	4.43	66.23	15.84	0.46	130.0	± 9.6 %
		Y	4.59	66.63	16.18		130.0	
		Z	4.32	66.29	15.85		130.0	
10580-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle)	X	4.48	66.29	15.88	0.46	130.0	± 9.6 %
		Y	4.63	66.65	16.19		130.0	
		Z	4.36	66.36	15.88		130.0	
10581-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle)	X	4.57	67.03	16.51	0.46	130.0	± 9.6 %
		Y	4.72	67.35	16.78		130.0	
		Z	4.47	67.19	16.58		130.0	
10582-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle)	X	4.37	65.99	15.62	0.46	130.0	± 9.6 %
		Y	4.53	66.39	15.97		130.0	
		Z	4.25	66.03	15.62		130.0	
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	4.55	66.38	16.23	0.46	130.0	± 9.6 %
		Y	4.68	66.67	16.50		130.0	
		Z	4.45	66.51	16.27		130.0	
10584-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	4.58	66.56	16.30	0.46	130.0	± 9.6 %
		Y	4.71	66.83	16.56		130.0	
		Z	4.48	66.70	16.35		130.0	
10585-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	X	4.77	66.84	16.47	0.46	130.0	± 9.6 %
		Y	4.92	67.13	16.73		130.0	
		Z	4.66	66.96	16.51		130.0	
10586-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)	X	4.67	67.00	16.57	0.46	130.0	± 9.6 %
		Y	4.82	67.30	16.83		130.0	
		Z	4.57	67.13	16.63		130.0	
10587-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	X	4.43	66.23	15.84	0.46	130.0	± 9.6 %
		Y	4.59	66.63	16.18		130.0	
		Z	4.32	66.29	15.85		130.0	
10588-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	X	4.48	66.29	15.88	0.46	130.0	± 9.6 %
		Y	4.63	66.65	16.19		130.0	
		Z	4.36	66.36	15.88		130.0	
10589-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	X	4.57	67.03	16.51	0.46	130.0	± 9.6 %
		Y	4.72	67.35	16.78		130.0	
		Z	4.47	67.19	16.58		130.0	
10590-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)	X	4.37	65.99	15.62	0.46	130.0	± 9.6 %
		Y	4.53	66.39	15.97		130.0	
		Z	4.25	66.03	15.62		130.0	

Certificate No: EX3-3986_Mar18

Page 34 of 39

EX3DV4- SN:3986

March 23, 2018

10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	4.70	66.46	16.34	0.46	130.0	± 9.6 %
		Y	4.83	66.72	16.59		130.0	
		Z	4.61	66.59	16.39		130.0	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	4.85	66.79	16.48	0.46	130.0	± 9.6 %
		Y	4.99	67.06	16.72		130.0	
		Z	4.74	66.90	16.52		130.0	
10593-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	X	4.77	66.68	16.34	0.46	130.0	± 9.6 %
		Y	4.92	66.99	16.61		130.0	
		Z	4.66	66.78	16.38		130.0	
10594-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	X	4.83	66.86	16.51	0.46	130.0	± 9.6 %
		Y	4.97	67.15	16.76		130.0	
		Z	4.72	66.97	16.55		130.0	
10595-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle)	X	4.79	66.81	16.40	0.46	130.0	± 9.6 %
		Y	4.94	67.11	16.66		130.0	
		Z	4.68	66.92	16.45		130.0	
10596-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	X	4.73	66.80	16.40	0.46	130.0	± 9.6 %
		Y	4.88	67.11	16.67		130.0	
		Z	4.61	66.90	16.44		130.0	
10597-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	X	4.67	66.69	16.27	0.46	130.0	± 9.6 %
		Y	4.83	67.03	16.56		130.0	
		Z	4.56	66.77	16.30		130.0	
10598-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle)	X	4.66	66.93	16.54	0.46	130.0	± 9.6 %
		Y	4.81	67.26	16.82		130.0	
		Z	4.56	67.03	16.58		130.0	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	5.38	67.00	16.57	0.46	130.0	± 9.6 %
		Y	5.49	67.24	16.76		130.0	
		Z	5.28	67.05	16.61		130.0	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	5.51	67.43	16.76	0.46	130.0	± 9.6 %
		Y	5.63	67.69	16.96		130.0	
		Z	5.40	67.45	16.78		130.0	
10601-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.39	67.16	16.64	0.46	130.0	± 9.6 %
		Y	5.52	67.43	16.85		130.0	
		Z	5.29	67.22	16.68		130.0	
10602-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	X	5.50	67.23	16.59	0.46	130.0	± 9.6 %
		Y	5.60	67.42	16.76		130.0	
		Z	5.43	67.38	16.67		130.0	
10603-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	X	5.57	67.51	16.87	0.46	130.0	± 9.6 %
		Y	5.70	67.77	17.06		130.0	
		Z	5.49	67.67	16.96		130.0	
10604-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	X	5.41	67.07	16.63	0.46	130.0	± 9.6 %
		Y	5.49	67.21	16.77		130.0	
		Z	5.37	67.32	16.77		130.0	
10605-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	X	5.50	67.32	16.76	0.46	130.0	± 9.6 %
		Y	5.60	67.52	16.93		130.0	
		Z	5.40	67.38	16.79		130.0	
10606-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	X	5.23	66.61	16.25	0.46	130.0	± 9.6 %
		Y	5.38	66.99	16.53		130.0	
		Z	5.14	66.66	16.28		130.0	

Certificate No: EX3-3986_Mar18

Page 35 of 39

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3986

March 23, 2018

10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	4.54	65.77	15.96	0.46	130.0	± 9.6 %
		Y	4.67	66.05	16.22		130.0	
		Z	4.45	65.93	16.03		130.0	
10608-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.72	66.16	16.13	0.46	130.0	± 9.6 %
		Y	4.87	66.47	16.38		130.0	
		Z	4.61	66.29	16.19		130.0	
10609-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	X	4.61	65.99	15.95	0.46	130.0	± 9.6 %
		Y	4.76	66.33	16.23		130.0	
		Z	4.50	66.12	16.01		130.0	
10610-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle)	X	4.66	66.16	16.12	0.46	130.0	± 9.6 %
		Y	4.81	66.48	16.39		130.0	
		Z	4.56	66.29	16.18		130.0	
10611-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	X	4.57	65.96	15.96	0.46	130.0	± 9.6 %
		Y	4.73	66.30	16.25		130.0	
		Z	4.47	66.09	16.02		130.0	
10612-AAB	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	X	4.58	66.10	16.00	0.46	130.0	± 9.6 %
		Y	4.74	66.46	16.29		130.0	
		Z	4.47	66.22	16.06		130.0	
10613-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	X	4.58	65.97	15.88	0.46	130.0	± 9.6 %
		Y	4.75	66.36	16.19		130.0	
		Z	4.46	66.05	15.91		130.0	
10614-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	X	4.53	66.17	16.12	0.46	130.0	± 9.6 %
		Y	4.68	66.54	16.41		130.0	
		Z	4.43	66.30	16.18		130.0	
10615-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	X	4.57	65.78	15.73	0.46	130.0	± 9.6 %
		Y	4.73	66.13	16.03		130.0	
		Z	4.46	65.89	15.77		130.0	
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	5.19	66.24	16.18	0.46	130.0	± 9.6 %
		Y	5.32	66.54	16.40		130.0	
		Z	5.10	66.30	16.22		130.0	
10617-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	5.26	66.43	16.24	0.46	130.0	± 9.6 %
		Y	5.38	66.68	16.43		130.0	
		Z	5.16	66.50	16.29		130.0	
10618-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	X	5.15	66.43	16.26	0.46	130.0	± 9.6 %
		Y	5.27	66.72	16.47		130.0	
		Z	5.06	66.54	16.32		130.0	
10619-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	X	5.16	66.22	16.09	0.46	130.0	± 9.6 %
		Y	5.29	66.54	16.32		130.0	
		Z	5.06	66.29	16.13		130.0	
10620-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.25	66.26	16.16	0.46	130.0	± 9.6 %
		Y	5.39	66.60	16.40		130.0	
		Z	5.15	66.32	16.20		130.0	
10621-AAB	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	X	5.25	66.42	16.36	0.46	130.0	± 9.6 %
		Y	5.38	66.69	16.56		130.0	
		Z	5.16	66.49	16.41		130.0	
10622-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle)	X	5.27	66.57	16.43	0.46	130.0	± 9.6 %
		Y	5.38	66.83	16.62		130.0	
		Z	5.16	66.60	16.46		130.0	

Certificate No: EX3-3986_Mar18

Page 36 of 39

EX3DV4- SN:3986

March 23, 2018

10623-AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)	X	5.14	66.09	16.05	0.46	130.0	± 9.6 %
		Y	5.27	66.39	16.28		130.0	
		Z	5.04	66.11	16.07		130.0	
10624-AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle)	X	5.33	66.29	16.22	0.46	130.0	± 9.6 %
		Y	5.46	66.58	16.44		130.0	
		Z	5.23	66.35	16.26		130.0	
10625-AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)	X	5.66	67.17	16.71	0.46	130.0	± 9.6 %
		Y	5.84	67.59	16.99		130.0	
		Z	5.44	66.88	16.58		130.0	
10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	5.50	66.31	16.14	0.46	130.0	± 9.6 %
		Y	5.60	66.59	16.34		130.0	
		Z	5.42	66.36	16.18		130.0	
10627-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	5.73	66.88	16.39	0.46	130.0	± 9.6 %
		Y	5.83	67.12	16.56		130.0	
		Z	5.65	66.95	16.44		130.0	
10628-AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle)	X	5.52	66.37	16.07	0.46	130.0	± 9.6 %
		Y	5.64	66.72	16.30		130.0	
		Z	5.42	66.36	16.07		130.0	
10629-AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle)	X	5.59	66.42	16.09	0.46	130.0	± 9.6 %
		Y	5.73	66.81	16.34		130.0	
		Z	5.50	66.46	16.12		130.0	
10630-AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)	X	6.00	67.84	16.80	0.46	130.0	± 9.6 %
		Y	6.17	68.30	17.09		130.0	
		Z	5.83	67.66	16.72		130.0	
10631-AAB	IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)	X	5.91	67.69	16.92	0.46	130.0	± 9.6 %
		Y	6.08	68.11	17.17		130.0	
		Z	5.78	67.63	16.91		130.0	
10632-AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)	X	5.71	66.96	16.57	0.46	130.0	± 9.6 %
		Y	5.80	67.18	16.72		130.0	
		Z	5.64	67.08	16.65		130.0	
10633-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle)	X	5.58	66.54	16.19	0.46	130.0	± 9.6 %
		Y	5.71	66.88	16.41		130.0	
		Z	5.49	66.58	16.22		130.0	
10634-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle)	X	5.57	66.57	16.26	0.46	130.0	± 9.6 %
		Y	5.70	66.91	16.48		130.0	
		Z	5.48	66.61	16.30		130.0	
10635-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle)	X	5.44	65.88	15.64	0.46	130.0	± 9.6 %
		Y	5.58	66.27	15.91		130.0	
		Z	5.34	65.85	15.63		130.0	
10636-AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 90pc duty cycle)	X	5.91	66.67	16.23	0.46	130.0	± 9.6 %
		Y	6.01	66.96	16.43		130.0	
		Z	5.84	66.72	16.27		130.0	
10637-AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 90pc duty cycle)	X	6.07	67.06	16.41	0.46	130.0	± 9.6 %
		Y	6.16	67.32	16.59		130.0	
		Z	5.98	67.07	16.43		130.0	
10638-AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 90pc duty cycle)	X	6.06	67.02	16.37	0.46	130.0	± 9.6 %
		Y	6.16	67.31	16.56		130.0	
		Z	5.98	67.06	16.40		130.0	

Certificate No: EX3-3986_Mar18

Page 37 of 39

EX3DV4- SN:3986

March 23, 2018

10639-AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 90pc duty cycle)	X	6.04	66.97	16.38	0.46	130.0	± 9.6 %
		Y	6.15	67.28	16.59		130.0	
		Z	5.95	66.98	16.40		130.0	
10640-AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 90pc duty cycle)	X	6.04	66.97	16.32	0.46	130.0	± 9.6 %
		Y	6.16	67.32	16.55		130.0	
		Z	5.94	66.96	16.33		130.0	
10641-AAC	IEEE 802.11ac WiFi (160MHz, MCS5, 90pc duty cycle)	X	6.09	66.91	16.31	0.46	130.0	± 9.6 %
		Y	6.19	67.16	16.49		130.0	
		Z	6.01	66.94	16.34		130.0	
10642-AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 90pc duty cycle)	X	6.13	67.15	16.61	0.46	130.0	± 9.6 %
		Y	6.24	67.45	16.80		130.0	
		Z	6.04	67.18	16.64		130.0	
10643-AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 90pc duty cycle)	X	5.97	66.83	16.34	0.46	130.0	± 9.6 %
		Y	6.07	67.13	16.54		130.0	
		Z	5.89	66.86	16.36		130.0	
10644-AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 90pc duty cycle)	X	6.11	67.26	16.57	0.46	130.0	± 9.6 %
		Y	6.26	67.69	16.85		130.0	
		Z	5.98	67.16	16.54		130.0	
10645-AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 90pc duty cycle)	X	6.32	67.54	16.67	0.46	130.0	± 9.6 %
		Y	6.68	68.52	17.21		130.0	
		Z	6.11	67.19	16.52		130.0	
10646-AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	X	17.67	108.27	36.87	9.30	60.0	± 9.6 %
		Y	91.41	147.18	47.97		60.0	
		Z	13.46	103.16	35.12		60.0	
10647-AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	X	15.60	106.13	36.35	9.30	60.0	± 9.6 %
		Y	73.20	142.93	47.10		60.0	
		Z	11.75	100.79	34.51		60.0	
10648-AAA	CDMA2000 (1x Advanced)	X	0.56	61.86	9.06	0.00	150.0	± 9.6 %
		Y	0.72	64.26	11.38		150.0	
		Z	0.47	61.12	7.87		150.0	
10652-AAB	LTE-TDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.54	66.63	16.31	2.23	80.0	± 9.6 %
		Y	3.94	68.07	17.28		80.0	
		Z	3.41	66.77	16.27		80.0	
10653-AAB	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	4.07	66.04	16.52	2.23	80.0	± 9.6 %
		Y	4.40	67.14	17.24		80.0	
		Z	3.93	66.03	16.48		80.0	
10654-AAB	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	4.08	65.70	16.54	2.23	80.0	± 9.6 %
		Y	4.35	66.75	17.22		80.0	
		Z	3.93	65.66	16.50		80.0	
10655-AAB	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.12	65.68	16.58	2.23	80.0	± 9.6 %
		Y	4.41	66.75	17.25		80.0	
		Z	3.99	65.60	16.53		80.0	
10658-AAA	Pulse Waveform (200Hz, 10%)	X	32.44	97.69	23.28	10.00	50.0	± 9.6 %
		Y	100.00	114.08	27.89		50.0	
		Z	9.00	80.27	17.37		50.0	
10659-AAA	Pulse Waveform (200Hz, 20%)	X	100.00	108.89	24.37	6.99	60.0	± 9.6 %
		Y	100.00	111.59	25.86		60.0	
		Z	100.00	105.69	22.63		60.0	

Certificate No: EX3-3986_Mar18

Page 38 of 39

EX3DV4- SN:3986

March 23, 2018

10660- AAA	Pulse Waveform (200Hz, 40%)	X	100.00	106.27	21.90	3.98	80.0	± 9.6 %
		Y	100.00	111.14	24.46		80.0	
		Z	100.00	101.79	19.57		80.0	
10661- AAA	Pulse Waveform (200Hz, 60%)	X	100.00	103.27	19.47	2.22	100.0	± 9.6 %
		Y	100.00	112.90	24.00		100.0	
		Z	100.00	95.17	15.70		100.0	
10662- AAA	Pulse Waveform (200Hz, 80%)	X	0.78	66.77	7.35	0.97	120.0	± 9.6 %
		Y	100.00	115.10	23.19		120.0	
		Z	45.90	215.26	10.66		120.0	

* Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **DT&C (Dymstec)**

Certificate No: **EX3-3933_Sep17**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:3933**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6**
 Calibration procedure for dosimetric E-field probes

Calibration date: **September 28, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MTE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02525)	Apr-18
Reference 20 dB Attenuator	SN: S5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Reference Probe ES3DV2	SN: 3013	31-Dec-16 (No. ES3-3013_Dec16)	Dec-17
DAE4	SN: 660	7-Dec-16 (No. DAE4-660_Dec16)	Dec-17
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	09-Apr-16 (in house check Jun-16)	in house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	in house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	in house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	in house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	in house check: Oct-17

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			Issued: September 28, 2017

Certificate No: EX3-3933_Sep17

Page 1 of 11

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerisches Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
 Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}:** Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM (no uncertainty required).

EX3DV4 – SN:3933

September 28, 2017

Probe EX3DV4

SN:3933

Manufactured: July 24, 2013
Calibrated: September 28, 2017

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3933

September 28, 2017

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3933

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu V/(V/m)^2$) ^A	0.47	0.52	0.18	$\pm 10.1 \%$
DCP (mV) ^B	98.6	98.1	89.2	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	153.6	$\pm 3.5 \%$
		Y	0.0	0.0	1.0		143.6	
		Z	0.0	0.0	1.0		155.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3933

September 28, 2017

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3933

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
750	41.9	0.89	11.05	11.05	11.05	0.43	0.80	± 12.0 %
835	41.5	0.90	10.55	10.55	10.55	0.39	0.80	± 12.0 %
900	41.5	0.97	10.31	10.31	10.31	0.45	0.80	± 12.0 %
1750	40.1	1.37	9.32	9.32	9.32	0.36	0.80	± 12.0 %
1900	40.0	1.40	8.95	8.95	8.95	0.33	0.80	± 12.0 %
2300	39.5	1.67	8.34	8.34	8.34	0.22	0.97	± 12.0 %
2450	39.2	1.80	7.98	7.98	7.98	0.34	0.86	± 12.0 %
2600	39.0	1.96	7.72	7.72	7.72	0.41	0.84	± 12.0 %
3500	37.9	2.91	7.68	7.68	7.68	0.25	1.25	± 13.1 %
5200	36.0	4.66	5.60	5.60	5.60	0.35	1.80	± 13.1 %
5300	35.9	4.76	5.36	5.36	5.36	0.35	1.80	± 13.1 %
5500	35.6	4.96	5.20	5.20	5.20	0.40	1.80	± 13.1 %
5600	35.5	5.07	5.00	5.00	5.00	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.95	4.95	4.95	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3933

September 28, 2017

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3933

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^U (mm)	Unc (k=2)
750	55.5	0.96	10.86	10.86	10.86	0.36	0.93	± 12.0 %
835	55.2	0.97	10.60	10.60	10.60	0.42	0.80	± 12.0 %
900	55.0	1.05	10.63	10.63	10.63	0.31	1.06	± 12.0 %
1750	53.4	1.49	8.87	8.87	8.87	0.45	0.80	± 12.0 %
1900	53.3	1.52	8.50	8.50	8.50	0.42	0.80	± 12.0 %
2300	52.9	1.81	8.26	8.26	8.26	0.37	0.94	± 12.0 %
2450	52.7	1.95	8.02	8.02	8.02	0.38	0.89	± 12.0 %
2600	52.5	2.16	7.79	7.79	7.79	0.40	0.86	± 12.0 %
3500	51.3	3.31	7.40	7.40	7.40	0.30	1.20	± 13.1 %
5200	49.0	5.30	5.25	5.25	5.25	0.35	1.90	± 13.1 %
5300	48.9	5.42	4.94	4.94	4.94	0.40	1.90	± 13.1 %
5500	48.6	5.65	4.64	4.64	4.64	0.40	1.90	± 13.1 %
5600	48.5	5.77	4.47	4.47	4.47	0.40	1.90	± 13.1 %
5800	48.2	6.00	4.56	4.56	4.56	0.40	1.90	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3933

September 28, 2017

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

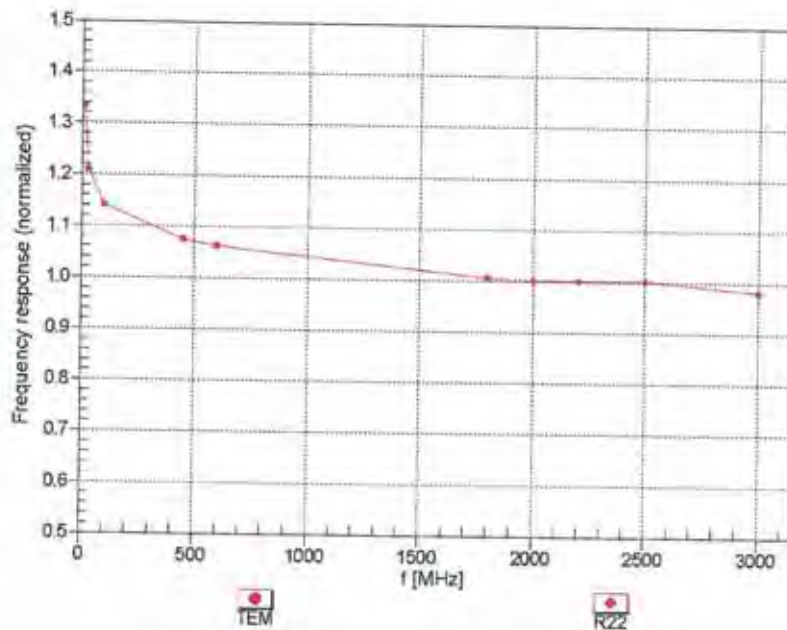


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:3933

September 28, 2017



Receiving Pattern (ϕ), $\theta = 0^\circ$

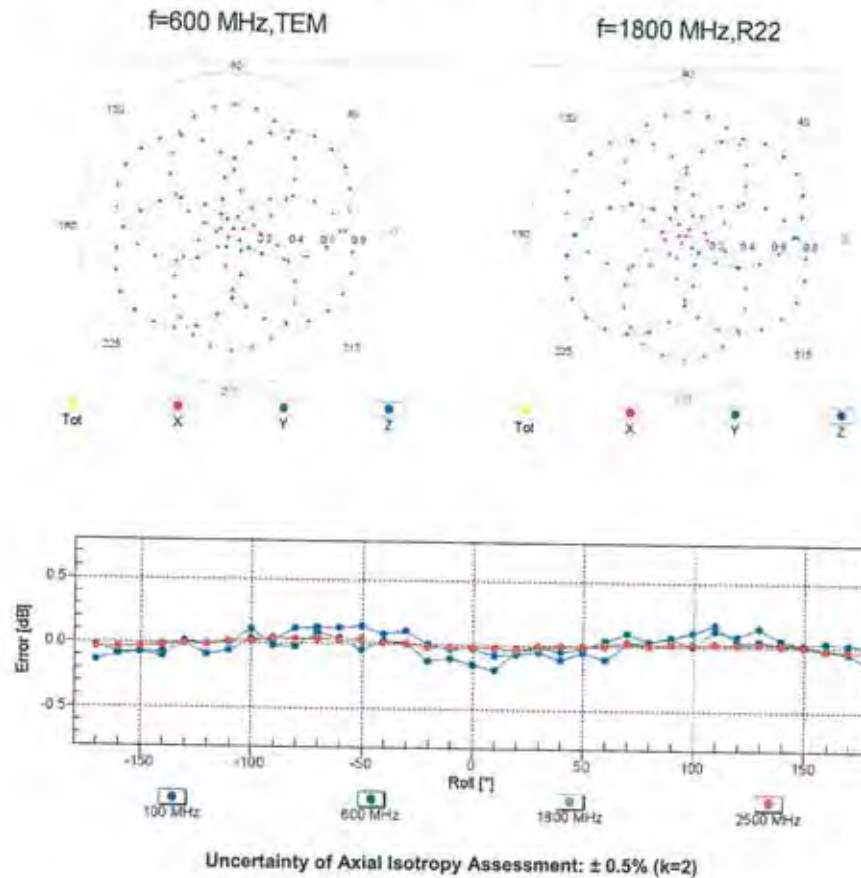

EX3DV4- SN:3933

September 28, 2017

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

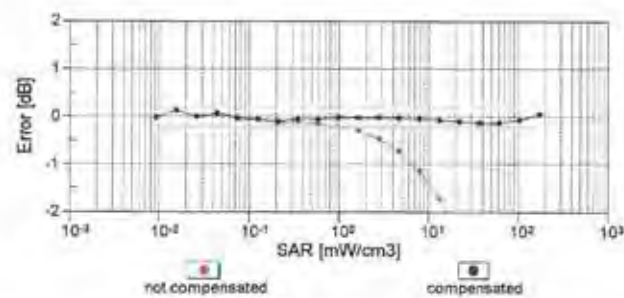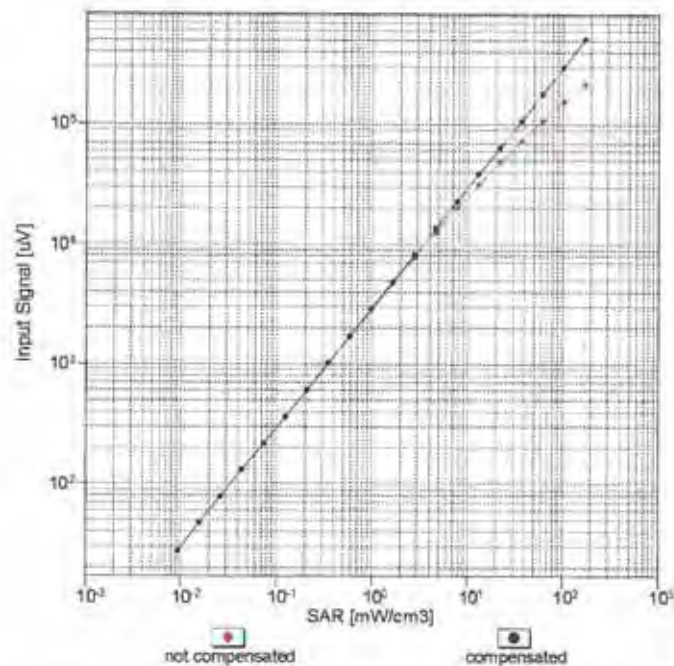

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


Certificate No: EX3-3933_Sep17

Page 9 of 11


EX3DV4-SN:3933

September 28, 2017

Conversion Factor Assessment

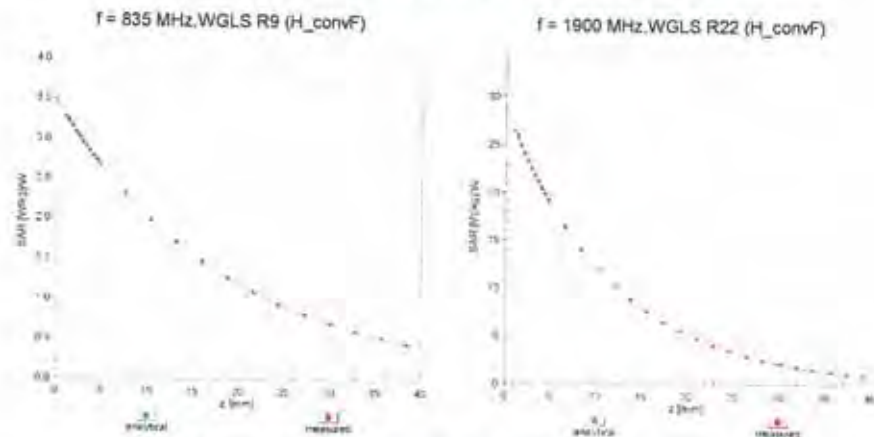

Deviation from Isotropy in Liquid Error (ϕ , θ), f = 900 MHz

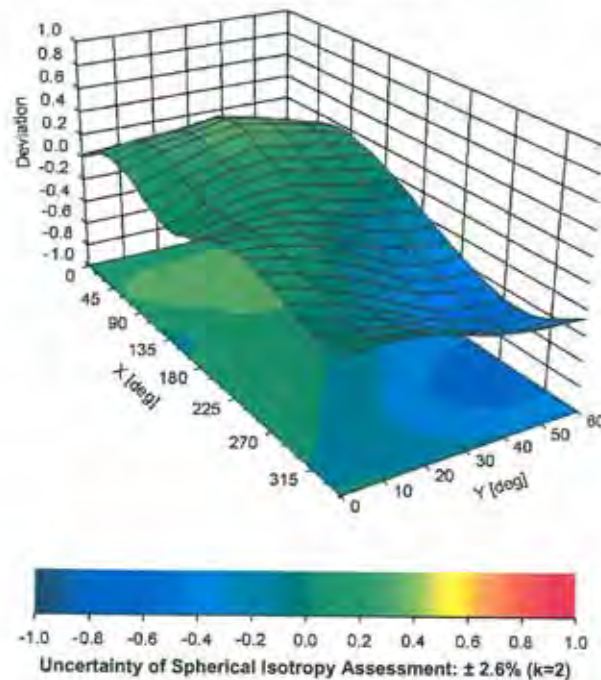

Certificate No: EX3-3933_Sep17

Page 10 of 11

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

EX3DV4- SN:3933

September 28, 2017

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3933

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	79.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Appendix B.2 Calibration certificate for DAE

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland




S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS Korea (Dymstec)**

Certificate No.: **DAE4-1430_Mar18**

CALIBRATION CERTIFICATE			
Object	DAE4 - SD 000 D04 BM - SN: 1430		
Calibration procedure(s)	QA CAL-06.v29 Calibration procedure for the data acquisition electronics (DAE)		
Calibration date:	March 16, 2018		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Kethley Multimeter Type 2001	SN: 0810278	31-Aug-17 (No.21092)	Aug-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	BE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-18
Calibrator Box V2.1	BE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-18
Calibrated by:	Name Eric Hainfeld	Function Laboratory Technician	Signature 
Approved by:	Name Sven Kühn	Function Deputy Manager	Signature 
			Issued: March 16, 2018
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: DAE4-1430_Mar18

Page 1 of 5

Report File No : F690501/RF-SAR002635

Date of Issue : 2018-08-10

(All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.)

RTT5041-76(2015.10.01) (2)

A4 (210mm x 297mm)

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
 - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
 - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
 - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
 - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - **Input resistance:** Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
 - **Power consumption:** Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 μ V , full range = -100...+300 mV
 Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.959 $\pm$ 0.02% (k=2)	404.146 $\pm$ 0.02% (k=2)	403.980 $\pm$ 0.02% (k=2)
Low Range	3.99758 $\pm$ 1.50% (k=2)	3.98046 $\pm$ 1.50% (k=2)	3.99960 $\pm$ 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	253.5 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (μ V)	Difference (μ V)	Error (%)
Channel X + Input	200037.67	1.03	0.00
Channel X + Input	20008.52	2.84	0.01
Channel X - Input	-20002.92	2.42	-0.01
Channel Y + Input	200036.34	-0.34	-0.00
Channel Y + Input	20005.28	-0.38	-0.00
Channel Y - Input	-20006.82	-1.47	0.01
Channel Z + Input	200036.68	-0.06	-0.00
Channel Z + Input	20006.80	1.23	0.01
Channel Z - Input	-20005.79	-0.34	0.00

Low Range	Reading (μ V)	Difference (μ V)	Error (%)
Channel X + Input	2001.84	-0.01	-0.00
Channel X + Input	201.87	0.11	0.06
Channel X - Input	-197.89	0.22	-0.11
Channel Y + Input	2001.53	-0.21	-0.01
Channel Y + Input	201.11	-0.63	-0.31
Channel Y - Input	-198.97	-0.75	0.38
Channel Z + Input	2001.92	0.14	0.01
Channel Z + Input	200.37	-1.29	-0.64
Channel Z - Input	-199.63	-1.14	0.57

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μ V)	Low Range Average Reading (μ V)
Channel X	200	3.16	1.29
	- 200	-0.35	-2.25
Channel Y	200	-20.12	-20.62
	- 200	20.02	19.66
Channel Z	200	-17.77	-18.32
	- 200	16.34	15.89

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μ V)	Channel Y (μ V)	Channel Z (μ V)
Channel X	200	-	1.73	-4.53
Channel Y	200	7.47	-	2.84
Channel Z	200	9.65	5.62	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16014	15513
Channel Y	16217	15103
Channel Z	15851	15866

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec
Input 10M Ω

	Average (μ V)	min. Offset (μ V)	max. Offset (μ V)	Std. Deviation (μ V)
Channel X	0.72	-0.74	2.59	0.52
Channel Y	-1.12	-2.10	-0.08	0.45
Channel Z	-0.44	-1.66	1.28	0.65

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (k Ω m)	Measuring (M Ω m)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Appendix B.3 Calibration certificate for Dipole

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates.

Accreditation No.: **SCS 0108**

Client **SGS Korea (Dymstec)**

Certificate No: **D750V3-1085_Mar17**

CALIBRATION CERTIFICATE

Object **D750V3 - SN:1085**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz



Calibration date: **March 15, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given in the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5056 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047 2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX30V4	SN: 7349	31-Dec-16 (No. EX3-2349, Dec16)	Dec-17
DAE4	SN: 601	04-Jan-17 (No. DAE4-601_Jan17)	Jan-18

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: 0807480704	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
RF generator R&S SMT 06	SN: 100972	15-Jun-15 (in house check Oct-16)	in house check: Oct-16
Network Analyzer HP 8753E	SN: US37390565	16-Oct-01 (in house check Oct-16)	in house check: Oct-17

Calibrated by: **Johannes Kurika** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature



Issued: March 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D750V3-1085_Mar17**

Page 1 of 8

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
 ConvF sensitivity in TSL / NORM x,y,z
 N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.9 $\pm$ 6 %	0.91 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.29 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.43 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	54.6 $\pm$ 6 %	0.99 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.23 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.68 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.46 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.72 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$53.0 \Omega + 1.1 j\Omega$
Return Loss	- 30.1 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$50.1 \Omega - 3.2 j\Omega$
Return Loss	- 29.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.032 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 06, 2013

DASY5 Validation Report for Head TSL

Date: 15.03.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1085

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.91 \text{ S/m}$; $\epsilon_r = 40.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.17, 10.17, 10.17); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 59.18 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 3.18 W/kg

SAR(1 g) = 2.12 W/kg; SAR(10 g) = 1.38 W/kg

Maximum value of SAR (measured) = 2.84 W/kg

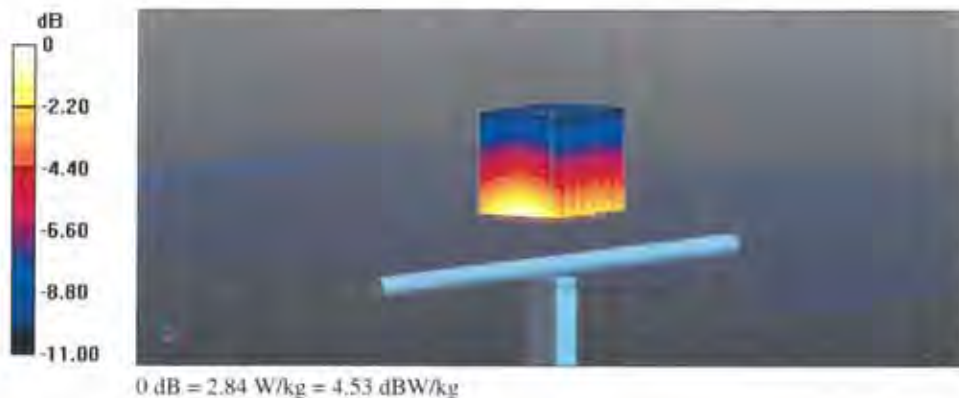

Impedance Measurement Plot for Head TSL

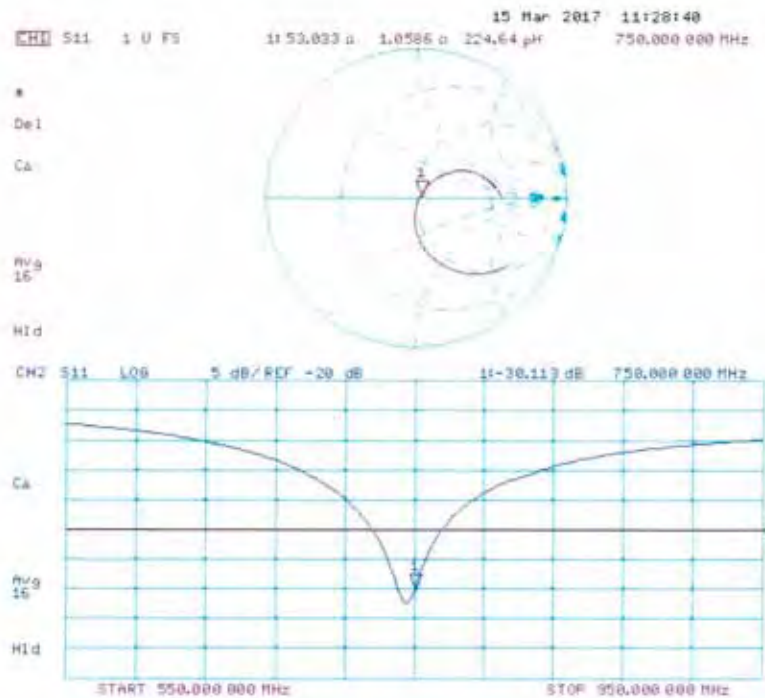

DASY5 Validation Report for Body TSL

Date: 15.03.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1085

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.99 \text{ S/m}$; $\epsilon_r = 54.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.99, 9.99, 9.99); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.23 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 3.35 W/kg

SAR(1 g) = 2.23 W/kg; SAR(10 g) = 1.46 W/kg

Maximum value of SAR (measured) = 2.97 W/kg

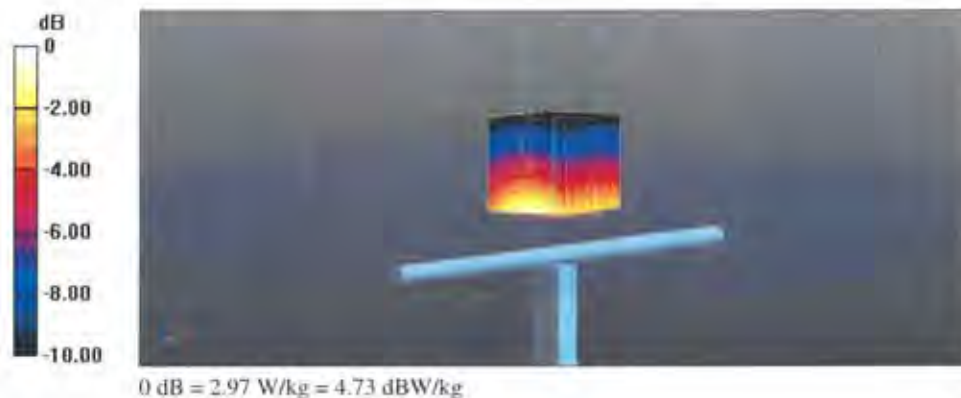

Impedance Measurement Plot for Body TSL

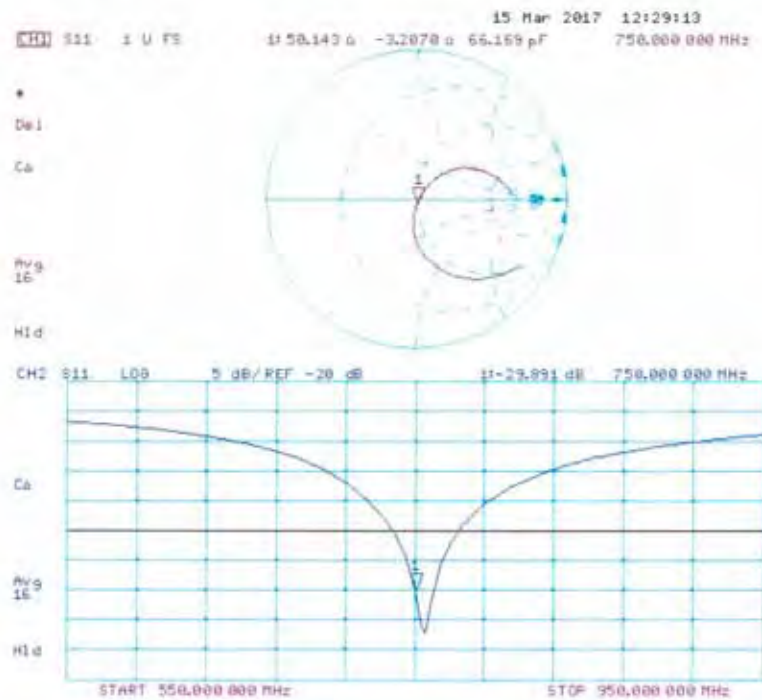

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS Korea (Dymstec)**

Certificate No: **D835V2-490_Jun18**

CALIBRATION CERTIFICATE

Object **D835V2 - SN:490**

Calibration procedure(s) **QA CAL-05.v10
 Calibration procedure for dipole validation kits above 700 MHz**



Calibration date: **June 01, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3) °C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 00327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8481A	SN: US37292785	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	in house check: Oct-18
Network Analyzer HP 6753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	in house check: Oct-18

Calibrated by:	Name: Aeton Kasirali	Function: Laboratory Technician	Signature: 
Approved by:	Name: Katja Pokovic	Function: Technical Manager	Signature: 

Issued: June 1, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-490_Jun18

Page 1 of 8

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1:

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.8 $\pm$ 6 %	0.92 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	-----	-----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.29 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.53 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.03 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	54.6 $\pm$ 6 %	0.99 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	-----	-----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.45 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.63 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.60 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.31 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.4 Ω - 2.5 j Ω
Return Loss	- 29.4 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω - 5.5 j Ω
Return Loss	- 24.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.384 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 19, 2003

DASY5 Validation Report for Head TSL

Date: 01.06.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:490

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.92$ S/m; $\epsilon_r = 40.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.9, 9.9, 9.9) @ 835 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 62.02 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 3.62 W/kg

SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.53 W/kg

Maximum value of SAR (measured) = 3.18 W/kg

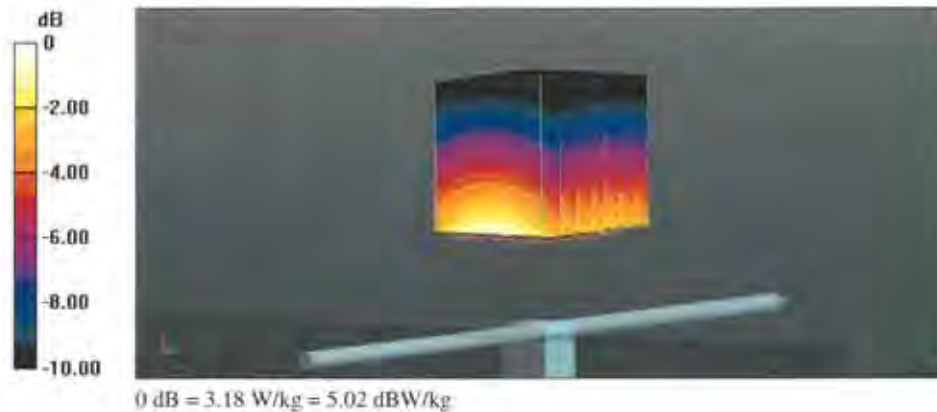

Impedance Measurement Plot for Head TSL

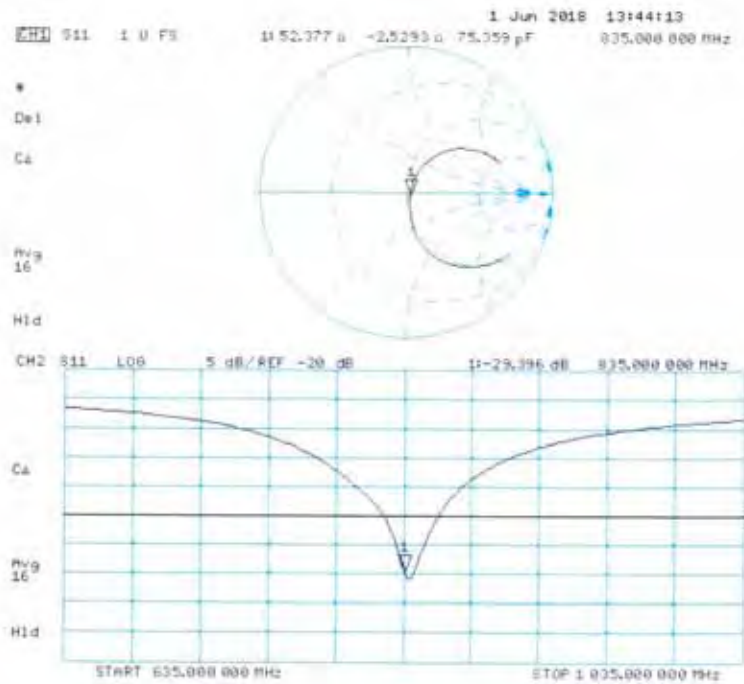

DASY5 Validation Report for Body TSL

Date: 01.06.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:490

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.99$ S/m; $\epsilon_r = 54.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.05, 10.05, 10.05) @ 835 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 61.08 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 3.64 W/kg

SAR(1 g) = 2.45 W/kg; SAR(10 g) = 1.6 W/kg

Maximum value of SAR (measured) = 3.25 W/kg



Impedance Measurement Plot for Body TSL

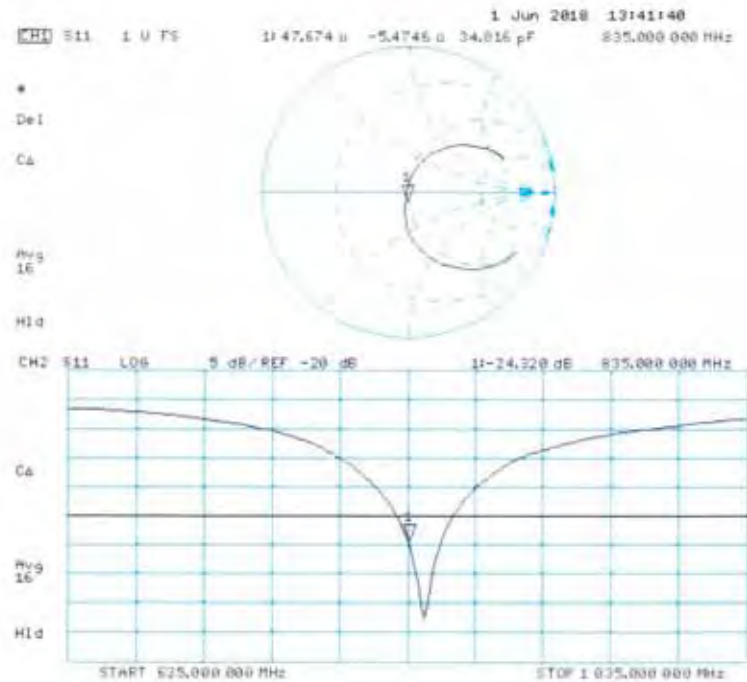

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS Korea (Dymstec)**

Certificate No: **D1750V2-1116_Jul17**

CALIBRATION CERTIFICATE

Object **D1750V2 - SN:1116**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz



Calibration date: **July 21, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18
DAE4	SN: 601	28-Mar-17 (No. DAE4-601_Mar17)	Mar-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
Power sensor HP 8481A	SN: US37282783	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
Power sensor HP 8481A	SN: MY41082317	07-Oct-15 (in house check Oct-16)	in house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	in house check: Oct-16
Network Analyzer HP 8753E	SN: US37300585	18-Oct-01 (in house check Oct-16)	in house check: Oct-17

Calibrated by: **Name: Michael Weber** **Function: Laboratory Technician**

Signature

Approved by: **Katja Pukovic** **Technical Manager**

Issued: July 24, 2017.

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D1750V2-1116_Jul17**

Page 1 of 8

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.0 $\pm$ 6 %	1.35 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.13 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.6 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.81 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.3 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.4	1.49 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.3 $\pm$ 6 %	1.49 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.21 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	36.8 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.90 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	19.6 W/kg $\pm$ 16.5 % (k=2)

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.0 $\pm$ 6 %	1.35 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.13 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.6 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.81 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.3 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.4	1.49 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.3 $\pm$ 6 %	1.49 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.21 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	36.8 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.90 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	19.6 W/kg $\pm$ 16.5 % (k=2)

DASY5 Validation Report for Head TSL

Date: 21.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1116

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 39$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.73, 8.73, 8.73); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.0 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.13 W/kg; SAR(10 g) = 4.81 W/kg

Maximum value of SAR (measured) = 14.0 W/kg

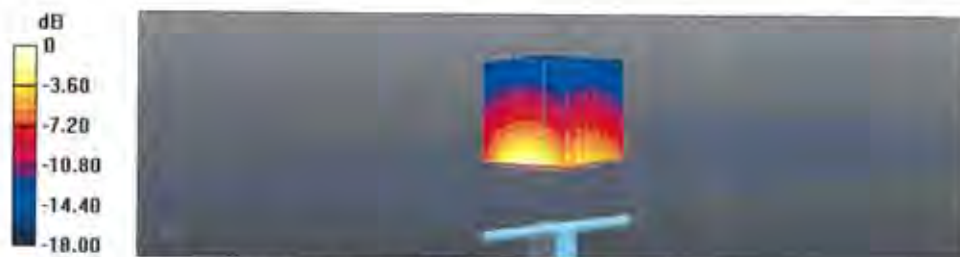

Impedance Measurement Plot for Head TSL

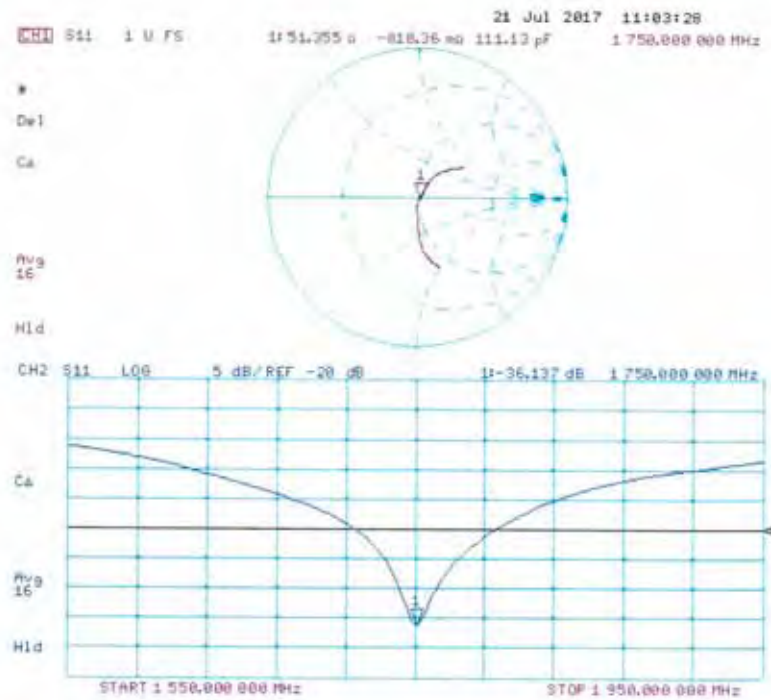

DASY5 Validation Report for Body TSL

Date: 20.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1116

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.49$ S/m; $\epsilon_r = 53.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.46, 8.46, 8.46); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.60 V/m; Power Drift = -0.08 dB


Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 9.21 W/kg; SAR(10 g) = 4.9 W/kg

Maximum value of SAR (measured) = 13.7 W/kg

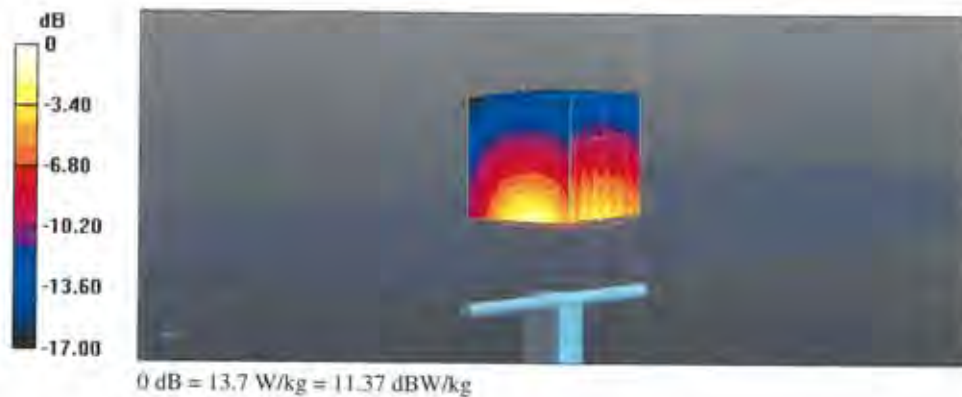

Impedance Measurement Plot for Body TSL

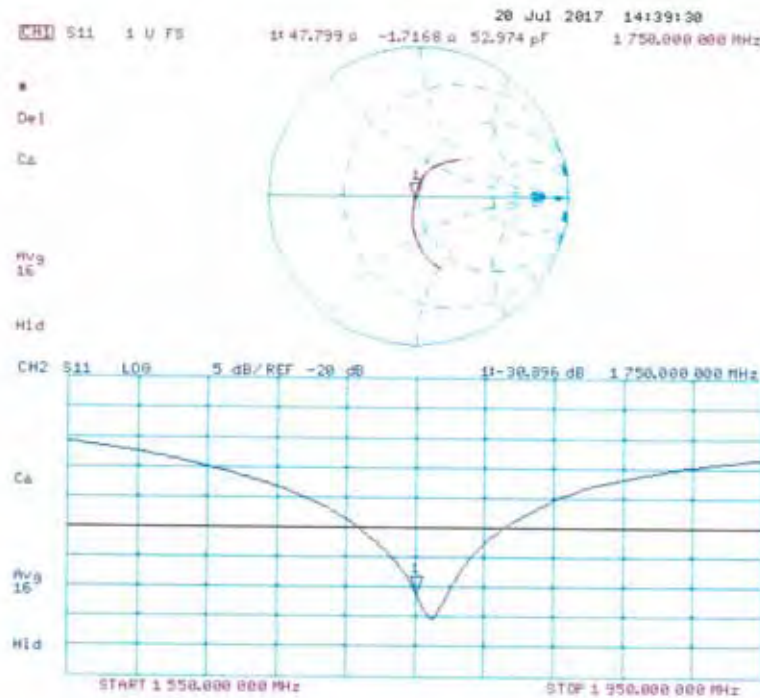

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**


Client **SGS Korea (Dymtec)**

Certificate No: **D1900V2-5d033_May18**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN:5d033**

Calibration procedure(s) **QA CAL-05.v10**
Calibration procedure for dipole validation kits above 700 MHz



Calibration date: **May 28, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combinator	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349, Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name Manu Sert	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature 

Issued: May 29, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D1900V2-5d033_May18**

Page 1 of 6

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	41.2 $\pm$ 6 %	1.35 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.69 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	39.9 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.9 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	55.3 $\pm$ 6 %	1.46 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.81 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.5 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.26 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.5 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$52.8 \Omega + 4.2 j\Omega$
Return Loss	- 26.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$46.6 \Omega + 3.3 j\Omega$
Return Loss	- 26.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1,204 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 17, 2003

DASY5 Validation Report for Head TSL

Date: 25.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d033

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 55.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.15, 8.15, 8.15) @ 1900 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.8 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.81 W/kg; SAR(10 g) = 5.26 W/kg

Maximum value of SAR (measured) = 14.7 W/kg

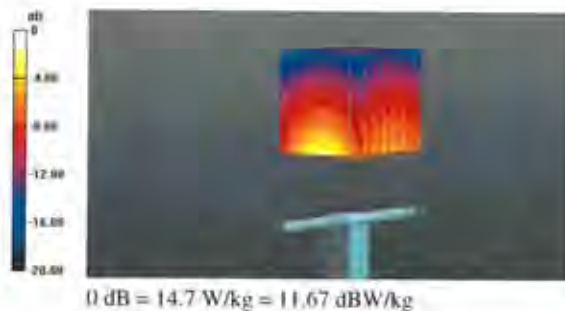

Impedance Measurement Plot for Head TSL

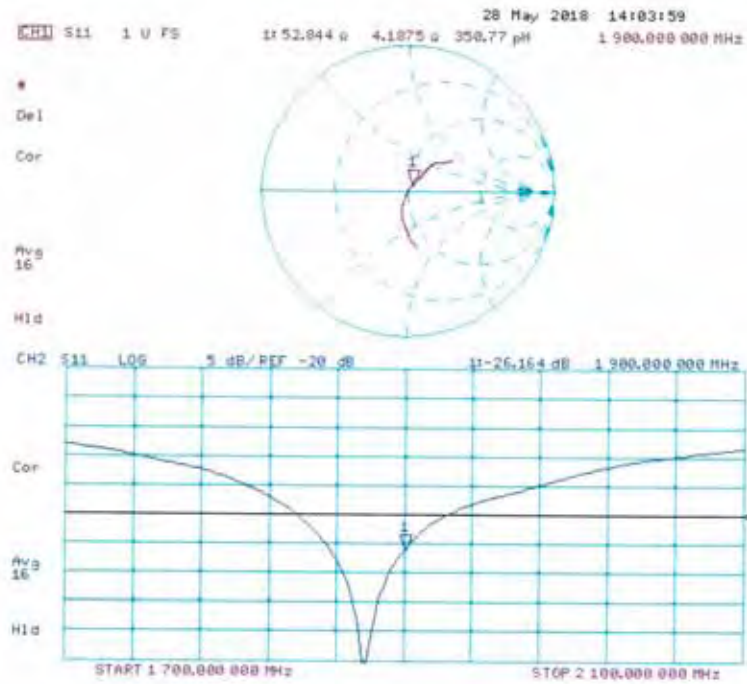

DASY5 Validation Report for Body TSL

Date: 25.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d033

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 55.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.15, 8.15, 8.15) @ 1900 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.8 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.81 W/kg; SAR(10 g) = 5.26 W/kg

Maximum value of SAR (measured) = 14.7 W/kg

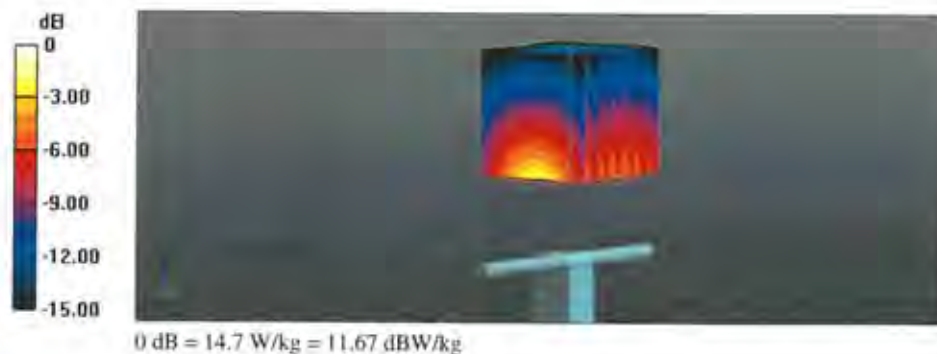

Impedance Measurement Plot for Body TSL

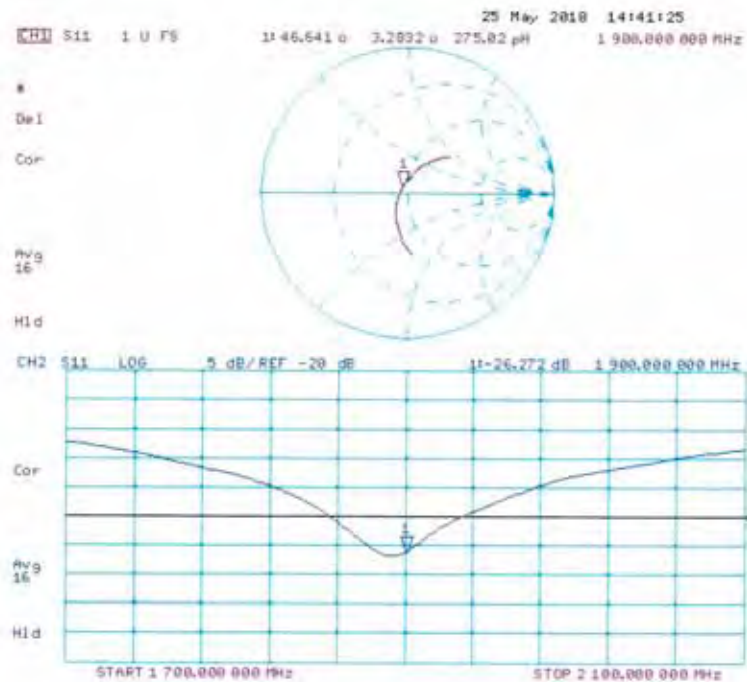

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **DT&C (Dymstec)**

Certificate No: **D2300V2-1028_Nov17**

CALIBRATION CERTIFICATE			
Object	D2300V2 - SN:1028		
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz		
Calibration date:	November 15, 2017		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards:	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8461A	SN: US37292783	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8461A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	in house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	in house check: Oct-18
Calibrated by:	Name Michael Weber	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature 
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: D2300V2-1028_Nov17

Page 1 of 8

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2300 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.3 $\pm$ 6 %	1.70 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	48.8 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.92 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.9	1.81 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.9 $\pm$ 6 %	1.85 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	11.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	46.9 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.73 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.7 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.6 Ω - 2.7 j Ω
Return Loss	- 31.1 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.0 Ω - 2.5 j Ω
Return Loss	- 24.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.167 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 30, 2009

DASY5 Validation Report for Head TSL

Date: 15.11.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1028

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: $f = 2300$ MHz; $\sigma = 1.7$ S/m; $\epsilon_r = 38.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.31, 8.31, 8.31); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 112.9 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 24.4 W/kg

SAR(1 g) = 12.4 W/kg; SAR(10 g) = 5.92 W/kg

Maximum value of SAR (measured) = 19.8 W/kg

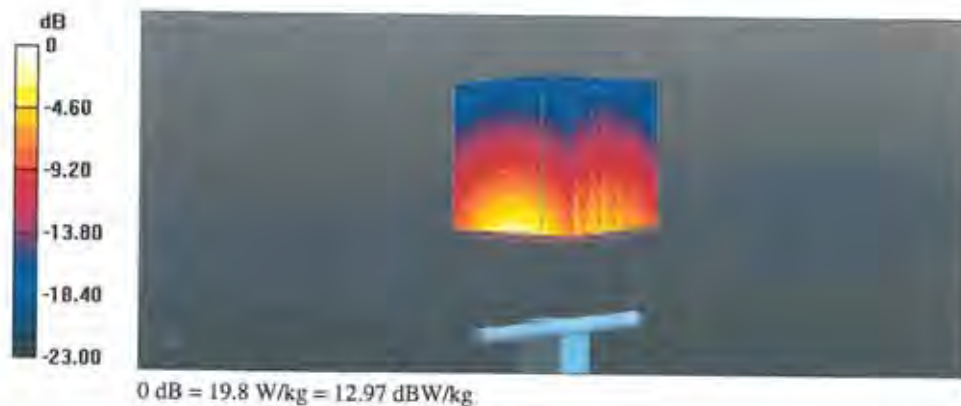

Impedance Measurement Plot for Head TSL

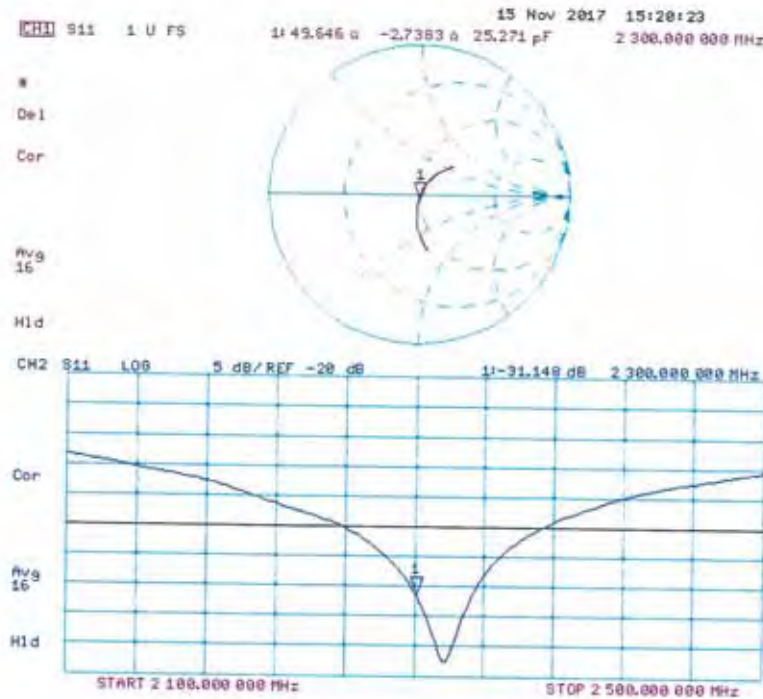

DASY5 Validation Report for Body TSL

Date: 15.11.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1028

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: $f = 2300$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 51.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.22, 8.22, 8.22); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.0 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 22.8 W/kg

SAR(1 g) = 11.9 W/kg; SAR(10 g) = 5.73 W/kg

Maximum value of SAR (measured) = 18.2 W/kg

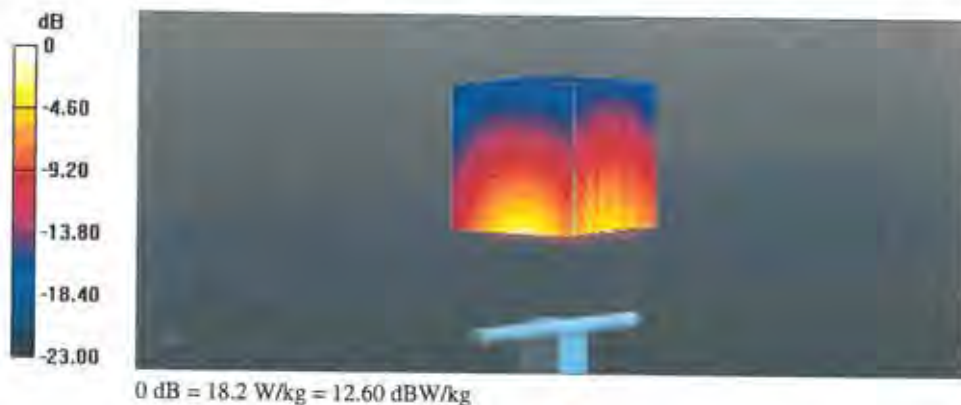

Impedance Measurement Plot for Body TSL

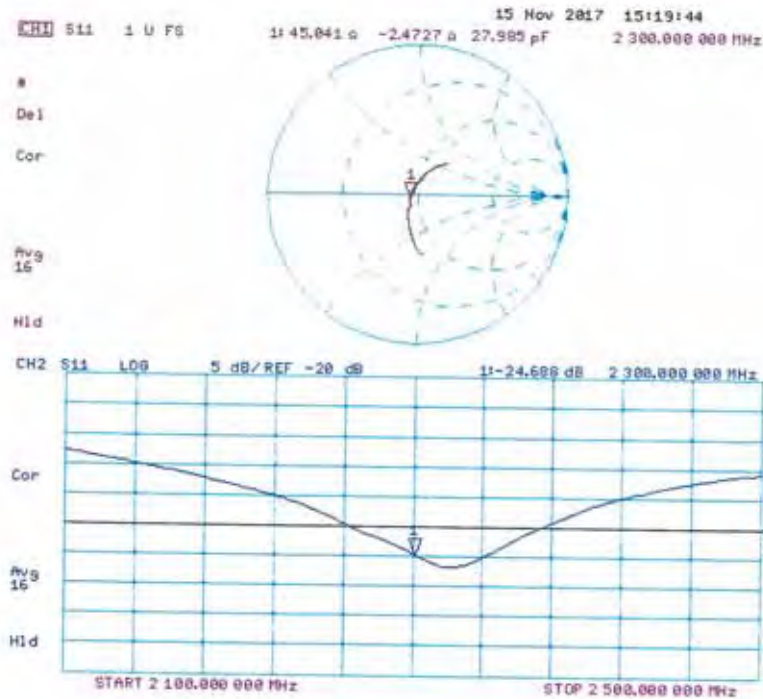

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**


Client **SGS Korea (Dymstec)**

Certificate No: **D2450V2-734_May18**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN:734**

Calibration procedure(s) **QA CAL-05.v10**
Calibration procedure for dipole validation kits above 700 MHz



Calibration date: **May 30, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical) for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-16 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-16 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-16 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-16 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047-2 / 06327	04-Apr-16 (No. 217-02663)	Apr-19
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: 0837460704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 6481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 6481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by: **Name: Mariu Seitz** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

Issued: May 31, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D2450V2-734_May18**

Page 1 of 8

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zughausstrasse 41, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di tarature
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.2 $\pm$ 6 %	1.85 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	51.4 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.08 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.0 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	52.3 $\pm$ 6 %	1.99 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.5 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.4 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.86 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.3 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.8 \Omega + 9.2 j\Omega$
Return Loss	- 20.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$50.1 \Omega + 8.6 j\Omega$
Return Loss	- 21.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.152 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 07, 2003

DASY5 Validation Report for Head TSL

Date: 30.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.88, 7.88, 7.88) @ 2450 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 115.5 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 25.8 W/kg

SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.08 W/kg

Maximum value of SAR (measured) = 21.4 W/kg

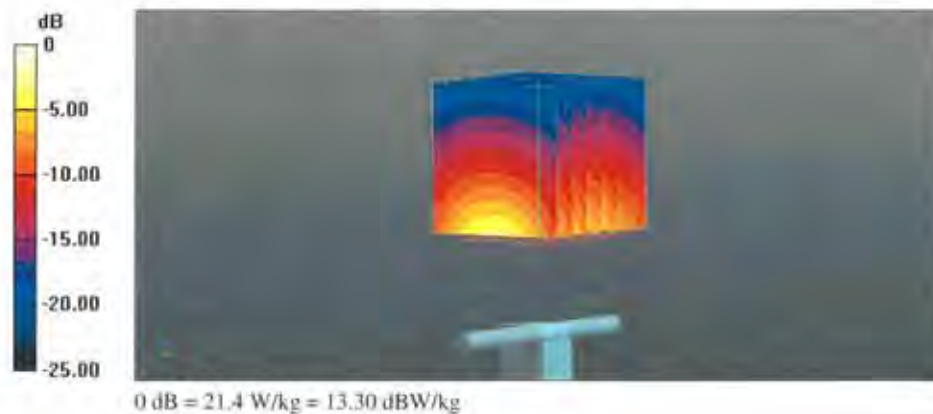

Impedance Measurement Plot for Head TSL

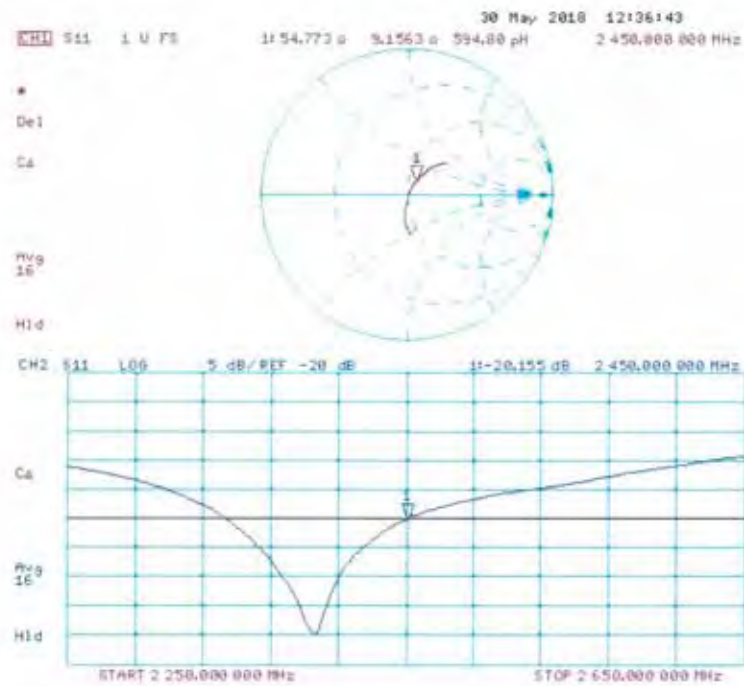

DASY5 Validation Report for Body TSL

Date: 29.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 52.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.01, 8.01, 8.01) @ 2450 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.3 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 24.6 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 5.86 W/kg

Maximum value of SAR (measured) = 20.5 W/kg

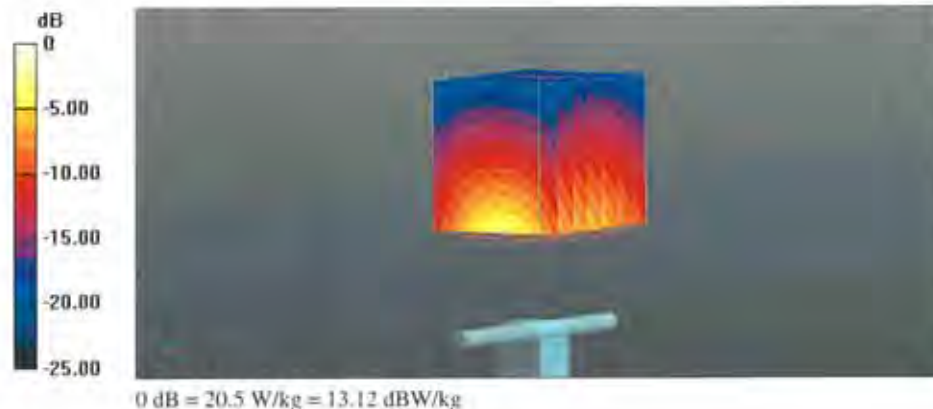

Impedance Measurement Plot for Body TSL

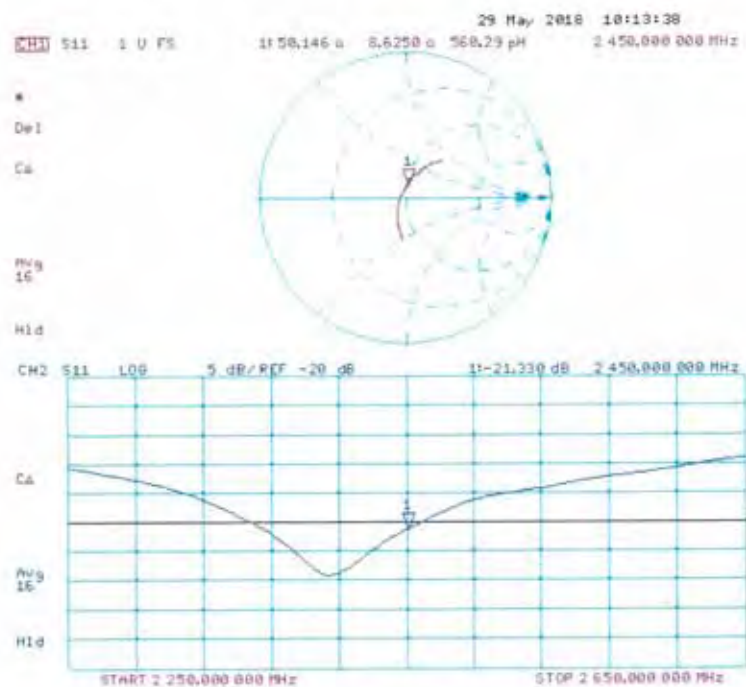

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**


Client **SGS Korea (Dymstec)**

Certificate No: **D2600V2-1038_May17**

CALIBRATION CERTIFICATE

Object **D2600V2 - SN:1038**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz



Calibration date **May 30, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&PE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX30V4	SN: 7460	19-May-17 (No. EX3-7460, May17)	May-18
DAE4	SN: 601	28-Mar-17 (No. DAE4-601, Mar17)	Mar-18

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
Power sensor HP 8461A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	in house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	in house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	in house check: Oct-17

Calibrated by: **Name: Johannes Kurikka** **Function: Laboratory Technician**

Signature

Approved by: **Name: Katja Pokovic** **Function: Technical Manager**

Issued: May 31, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D2600V2-1038_May17**

Page 1 of 8

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates.

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConVF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	37.3 $\pm$ 6 %	2.05 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	57.1 W/kg $\pm$ 17.0 % (k=2)
SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.46 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.4 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.5	2.16 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	52.0 $\pm$ 6 %	2.22 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	54.4 W/kg $\pm$ 17.0 % (k=2)
SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.12 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.3 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.2 Ω - 6.3 j Ω
Return Loss	- 23.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	44.5 Ω - 5.0 j Ω
Return Loss	- 22.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.148 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 03, 2009

DASY5 Validation Report for Head TSL

Date: 30.05.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1038

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.05$ S/m; $\epsilon_r = 37.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7460; ConvF(7.61, 7.61, 7.61); Calibrated: 19.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 115.7 V/m; Power Drift = -0.08 dB


Peak SAR (extrapolated) = 32.1 W/kg

SAR(1 g) = 14.7 W/kg; SAR(10 g) = 6.46 W/kg

Maximum value of SAR (measured) = 24.5 W/kg

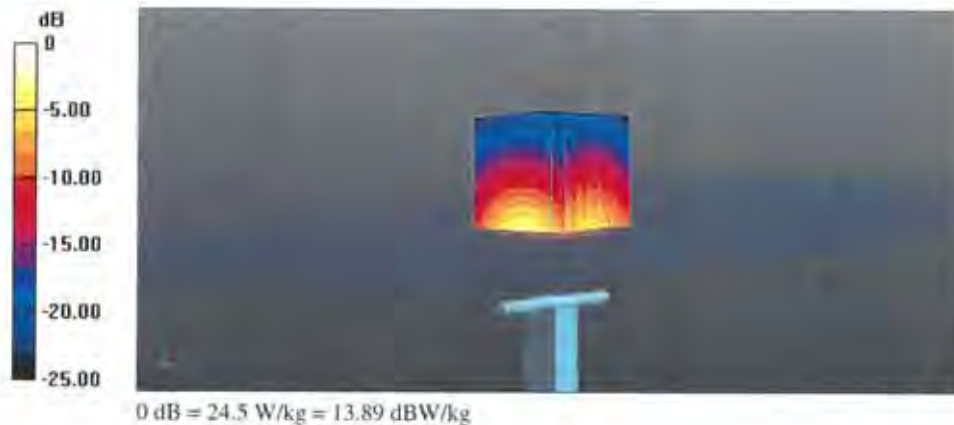

Impedance Measurement Plot for Head TSL

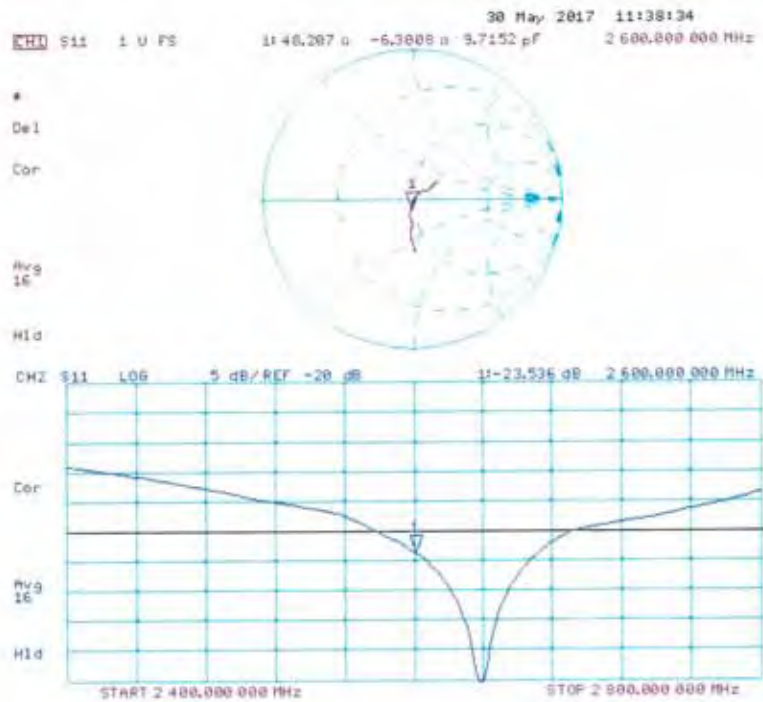

DASY5 Validation Report for Body TSL

Date: 30.05.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1038

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.22$ S/m; $\epsilon_r = 52$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7460; ConvF(7.71, 7.71, 7.71); Calibrated: 19.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.6 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 29.5 W/kg

SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.12 W/kg

Maximum value of SAR (measured) = 22.2 W/kg

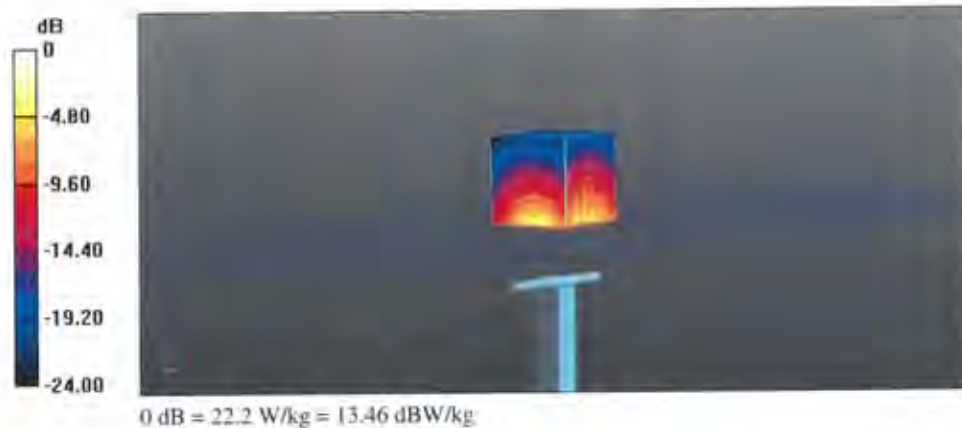

Impedance Measurement Plot for Body TSL

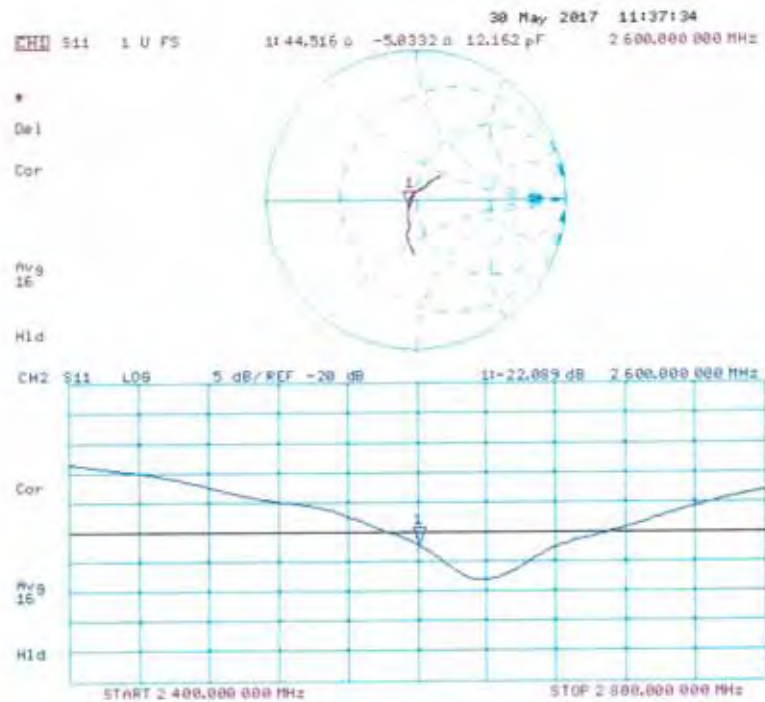

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS Korea (Dymstec)**

Certificate No: **D5GHzV2-1130_May18**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1130**

Calibration procedure(s) **QA CAL-22.v3**
Calibration procedure for dipole validation kits between 3-6 GHz

Calibration date: **May 25, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-18
Power sensor NRP-Z91	SN: 100244	04-Apr-18 (No. 217-02672)	Apr-18
Power sensor NRP-Z91	SN: 100245	04-Apr-18 (No. 217-02673)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20%)	04-Apr-18 (No. 217-02682)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-18
Reference Probe EX3DV4	SN: 3503	30-Dec-17 (No. EX3-3503_Dec17)	Dec-18
DAE4	SN: 601	25-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37460704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by: **Manu Seitz** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Issued: May 25, 2018

Certificate No: D5GHzV2-1130_May18

Page 1 of 14

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz $\pm$ 1 MHz 5300 MHz $\pm$ 1 MHz 5600 MHz $\pm$ 1 MHz 5800 MHz $\pm$ 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	36.2 $\pm$ 6 %	4.52 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.75 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.5 W/kg $\pm$ 19.9 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.23 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.3 W/kg $\pm$ 19.5 % (k=2)

Head TSL parameters at 5300 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	36.1 $\pm$ 6 %	4.63 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5300 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.31 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.1 W / kg $\pm$ 19.9 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.8 W/kg $\pm$ 19.5 % (k=2)

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.7 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.53 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	85.3 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	5.15 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.0 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.6 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.0 ± 6 %	5.41 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.45 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	73.9 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.09 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.7 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5300 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.42 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.8 ± 6 %	5.54 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5300 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.66 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	76.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.15 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.3 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.3 ± 6 %	5.95 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	8.08 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	80.1 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.26 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.4 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	45.9 ± 6 %	6.22 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.63 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.7 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.11 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.9 W/kg ± 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	53.4 Ω - 9.7 j Ω
Return Loss	- 20.0 dB

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	52.1 Ω - 4.3 j Ω
Return Loss	- 26.6 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	58.5 Ω - 2.9 j Ω
Return Loss	- 21.6 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	56.8 Ω - 0.8 j Ω
Return Loss	- 23.9 dB

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	51.6 Ω - 8.6 j Ω
Return Loss	- 21.3 dB

Antenna Parameters with Body TSL at 5300 MHz

Impedance, transformed to feed point	51.0 Ω - 4.0 j Ω
Return Loss	- 27.9 dB

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	57.9 Ω - 3.2 j Ω
Return Loss	- 22.0 dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	55.9 Ω - 2.5 j Ω
Return Loss	- 24.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.206 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 08, 2011

DASY5 Validation Report for Head TSL

Date: 25.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1130

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: $f = 5200$ MHz; $\sigma = 4.52$ S/m; $\epsilon_r = 36.2$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5300$ MHz; $\sigma = 4.63$ S/m; $\epsilon_r = 36.1$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5600$ MHz; $\sigma = 4.94$ S/m; $\epsilon_r = 35.7$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5800$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 35.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.75, 5.75, 5.75) @ 5200 MHz, ConvF(5.5, 5.5, 5.5) @ 5300 MHz, ConvF(5.05, 5.05, 5.05) @ 5600 MHz, ConvF(4.96, 4.96, 4.96) @ 5800 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.29 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 27.9 W/kg

SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.23 W/kg

Maximum value of SAR (measured) = 17.6 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 74.92 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 30.2 W/kg

SAR(1 g) = 8.31 W/kg; SAR(10 g) = 2.38 W/kg

Maximum value of SAR (measured) = 18.9 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm


Reference Value = 75.83 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 32.1 W/kg


SAR(1 g) = 8.53 W/kg; SAR(10 g) = 2.45 W/kg

Maximum value of SAR (measured) = 19.7 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
 Reference Value = 73.55 V/m; Power Drift = -0.09 dB
 Peak SAR (extrapolated) = 32.8 W/kg
SAR(1 g) = 8.3 W/kg; SAR(10 g) = 2.36 W/kg
 Maximum value of SAR (measured) = 19.6 W/kg

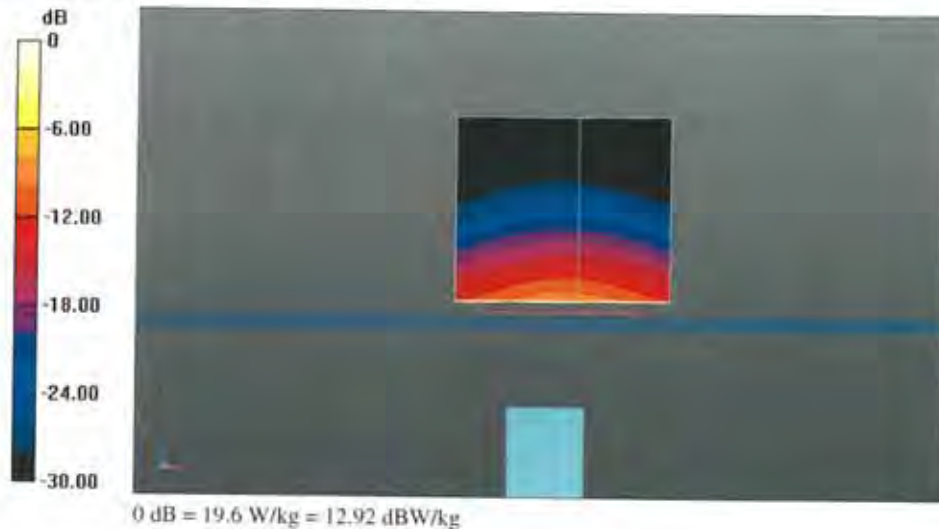

Impedance Measurement Plot for Head TSL

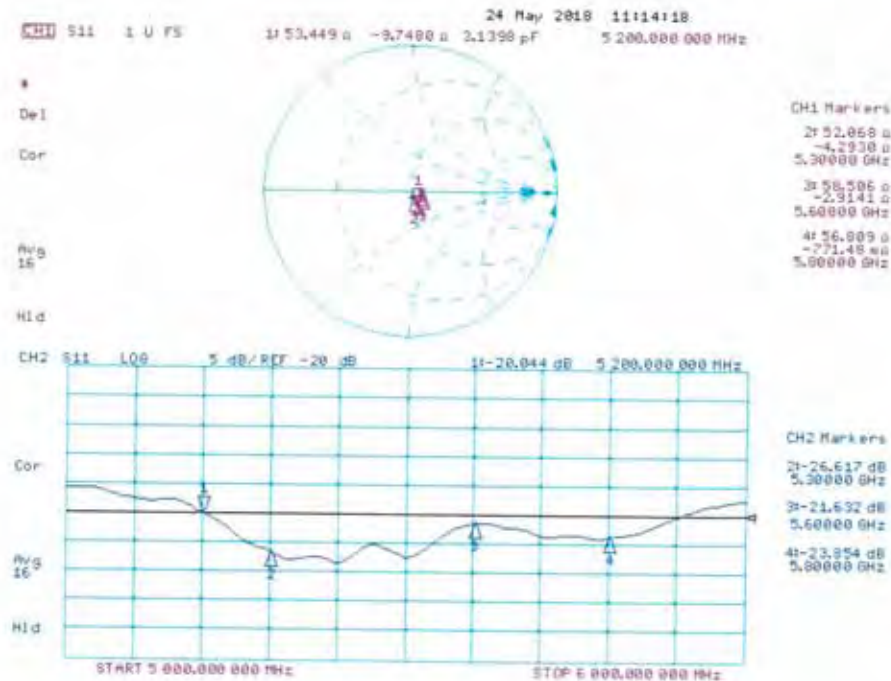

DASY5 Validation Report for Body TSL

Date: 24.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1130

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz

Medium parameters used: $f = 5200$ MHz; $\sigma = 5.41$ S/m; $\epsilon_r = 47$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5300$ MHz; $\sigma = 5.54$ S/m; $\epsilon_r = 46.8$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5600$ MHz; $\sigma = 5.95$ S/m; $\epsilon_r = 46.3$; $\rho = 1000$ kg/m³,

Medium parameters used: $f = 5800$ MHz; $\sigma = 6.22$ S/m; $\epsilon_r = 45.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.35, 5.35, 5.35) @ 5200 MHz, ConvF(5.15, 5.15, 5.15) @ 5300 MHz, ConvF(4.65, 4.65, 4.65) @ 5600 MHz, ConvF(4.53, 4.53, 4.53) @ 5800 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.61 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 27.6 W/kg

SAR(1 g) = 7.45 W/kg; SAR(10 g) = 2.09 W/kg

Maximum value of SAR (measured) = 17.5 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.51 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 29.9 W/kg

SAR(1 g) = 7.66 W/kg; SAR(10 g) = 2.15 W/kg

Maximum value of SAR (measured) = 17.9 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm


Reference Value = 68.63 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 33.8 W/kg


SAR(1 g) = 8.08 W/kg; SAR(10 g) = 2.26 W/kg

Maximum value of SAR (measured) = 19.5 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,
dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
 Reference Value = 66.70 V/m; Power Drift = -0.08 dB
 Peak SAR (extrapolated) = 33.0 W/kg
SAR(1 g) = 7.63 W/kg; SAR(10 g) = 2.11 W/kg
 Maximum value of SAR (measured) = 18.6 W/kg

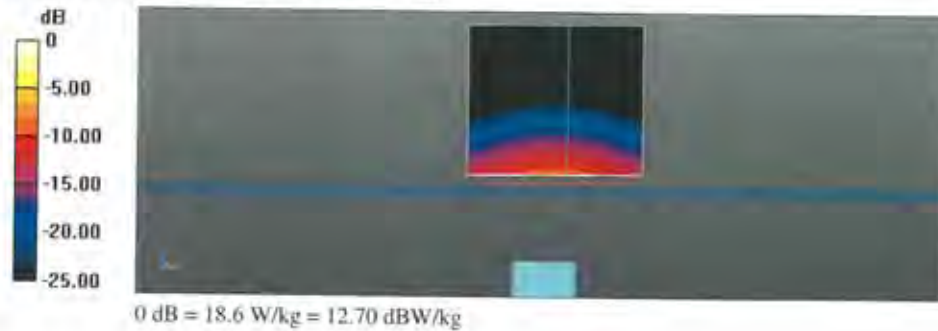

Impedance Measurement Plot for Body TSL

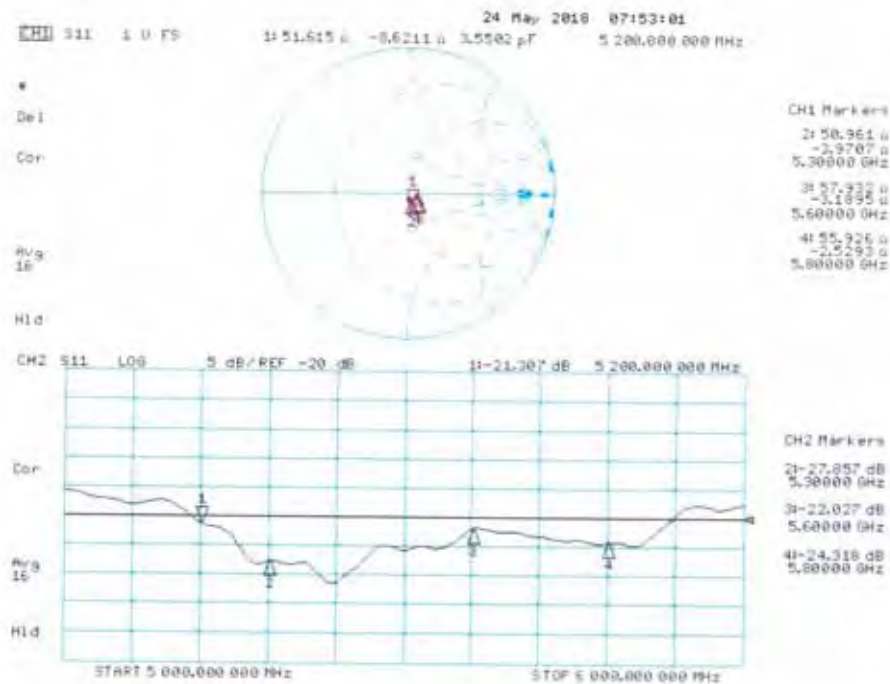

-THE END-