# FCC SAR TEST REPORT

**Test File No : F690501/RF-SAR002241-A2**

| | |
|---|---|
| **Equipment Under Test** | Digital Camera |
| **Model No.** | NX500 |
| **Applicant** | Samsung Electronics Co., Ltd. |
| **Address of Applicant** | 129, Samsung-ro, Yeongtong-gu Suwon-si, Gyeonggi-do, 443-742 Korea, Republic of |
| **FCC ID** | A3LNX500 |
| **Device Category** | Portable Device |
| **Exposure Category** | General Population/Uncontrolled Exposure |
| **Standards** | FCC 47 CFR Part 2 (2.1093)<br>IEEE 1528, 2003<br>ANSI/IEEE C95.1, C95.3 |
| **Date of Receipt** | 2014-12-19 |
| **Date of Test(s)** | 2014-12-30 |
| **Date of Issue** | 2015-01-15 |

In the configuration tested, the EUT complied with the standards specified above.

**Remarks:**

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.
This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Korea Co., Ltd. or testing done by SGS Korea Co., Ltd. in connection with distribution or use of the product described in this report must be approved by SGS Korea Co., Ltd. in writing.

**Report prepared by /**
**Changhyun Song**
**Test Engineer**

**Approved by /**
**Nicky You**
**Technical Manager**

## Revision history

| Revision | Date of issue | Revisions | Revised By |
|---|---|---|---|
| - | January 09, 2015 | Initial issue | - |
| A1 | January 13, 2015 | Updated report<br>1. Added to note about BT and WLAN transmit simultaneously on the page 20.<br>2. Added to SAR test exclusion of Bluetooth.<br>3. Removed the IC ID. | Changhyun Song |
| A2 | January 15, 2015 | Updated report<br>1. Revised to note on the page 20. | Changhyun Song |

# Contents

1 Testing Laboratory 4
2 Details of Applicant 4
3 Description of EUT(s) 4
4 The Highest Reported SAR Values 4
5 Test Methodology 5
6 Test Environment 5
7 Specific Absorption Rate (SAR) 6
7.1 Introduction 6
7.2 SAR Definition 6
7.3 Test Standards and Limits 6
8 The SAR Measurement System 8
9 System Components 9
9.1 Probe 9
9.2 ELI Phantom 9
9.3 Device Holder 10
10 SAR Measurement Procedures 11
10.1 Normal SAR Measurement Procedure 11
11 SAR System Verification 13
12 Tissue Simulant Fluid for the Frequency Band 14
13 Test System Validation 15
14 Instruments List 16
15 FCC Power Measurement Procedures 17
16 Measured and Reported SAR 17
17 Maximum Output Power Specifications 17
18 RF Conducted Power Measurement 18
19 SAR Test configuration 19
19.1 UMPC Mini-Tablet Devices 19
19.2 IEEE 802.11 Transmitters 19
20 Transmit Antenna Separation Distances 20
20.1 UMPC mini-tablet transmitter for SAR Testing 20
21 SAR Test Exclusions Applied 20
22 SAR Data Summary 21
23 SAR Measurement Variability 22
23.1 Measurement Variability 22
23.2 Measurement Uncertainty 22
Appendixes List 23
Appendixes A.1 24
Appendixes A.2 25
Appendixes B.1 26
Appendixes C.1 27
Appendixes C.2 38
Appendixes C.3 45
END 50

## 1. Testing Laboratory

| | |
|---|---|
| **Company Name** | SGS Korea Co., Ltd. (Gunpo Laboratory) |
| **Address** | Wireless Div. 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, 435-040 Republic of Korea |
| **Telephone** | +82 +31 428 5700 |
| **FAX** | +82 +31 427 2371 |
| **Homepage** | All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx |

## 2. Details of Manufacturer

| | |
|---|---|
| **Applicant** | Samsung Electronics Co., Ltd. |
| **Address** | 129, Samsung-ro, Yeongtong-gu, Suwon-city, Gyeonggi-do, 443-742 Korea, Republic of |
| **Contact Person** | Yongwook –Park |
| **Email** | Yongwook.park@samsung.com |
| **Phone No.** | +82 +31 277 7695 |

## 3. Description of EUT(s)

| | | |
|---|---|---|
| **EUT Type** | Digital Camera | |
| **Model** | NX500 | |
| **Serial Number** | DV3-276 | |
| **Mode of Operation** | WLAN | |
| **Duty Cycle** | 1 (WLAN) | |
| **Body worn Accessory** | None | |
| **Tx Frequency Range** | 2412 ㎒ ~ 2462 ㎒ (WLAN 802.11b/g/n)<br>2402 ㎒ ~ 2480 ㎒ (Bluetooth) | |
| **Battery Type** | DC 7.6 V (Li-ion Battery) | |
| **Antenna Information** | Manufacturer | Partron |
| | Type | FPCB |
| | Peak Antenna Gain | |
| | 2400 MHz ~ 2484 MHz | 1.32 dBi |

## 4. The Highest Reported SAR Values

| Exposure Class | Band & Mode | Highest Reported SAR 1g Body (W/kg) |
|---|---|---|
| **DTS** | 2.4 GHz WLAN | 0.24 |
| **DSS** | Bluetooth | N/A |
| Simultaneous SAR per KDB 690783 D01v01r03 | | N/A |

## 5. Test Methodology

ANSI C95.1–1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz. It specifies the maximum exposure limit of 1.6 W/kg as averaged over any 1 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

Test tests documented in this report were performed in accordance with IEEE Standard 1528-2003 & IEEE 1528a-2005 and the following published KDB procedures.

In additions;

| | | |
|---|---|---|
| ☒ | **KDB 865664 D01v01r03** | **SAR Measurement Requirements for 100 MHz to 6 GHz** |
| ☐ | **KDB 447498 D01v05r02** | **Mobile and Portable Devices RF Exposure Procedures and Equipment Authorization Policies** |
| ☐ | KDB 447498 D02v02 | SAR Measurement Procedures for USB Dongle Transmitters |
| ☒ | **KDB 248227 D01v01r02** | **SAR Measurement Procedures for 802.11a,b,g Transmitters** |
| ☐ | KDB 615223 D01v01 | 802.16e/WiMax SAR Measurement Guidance |
| ☐ | KDB 616217 D04v01r01 | SAR Evaluation Considerations for Laptop, Notebook, Netbook and Tablet Computers |
| ☐ | KDB 643646 D01v01r01 | SAR Test Reduction Considerations for Occupational PTT Radios |
| ☐ | KDB 648474 D03v01r02 | Evaluation and Approval Considerations for Handsets with Specific Wireless Charging Battery Covers |
| ☐ | KDB 648474 D04v01r02 | SAR Evaluation Considerations for Wireless Handsets |
| ☐ | KDB 680106 D01v02 | RF Exposure Considerations for Low Power Consumer Wireless Power Transfer Applications |
| ☐ | KDB 941225 D01v03 | SAR Measurement Procedures for 3G Devices (CDMA 2000 / Ev-Do, WCDMA/HSDPA/HSPA |
| ☐ | KDB 941225 D05v02r03 | SAR Evaluation Considerations for LTE Devices |
| ☐ | KDB 941225 D06v02 | SAR Evaluation Procedures for Portable Devices with Wireless Router Capabilities |
| ☒ | **KDB 941225 D07v01r01** | **SAR Evaluation Procedures for UMPC Mini-Tablet Devices** |

## 6. Testing Environment

| | |
|---|---|
| Ambient temperature | 18°C ~ 25°C |
| Relative humidity | 30% ~ 70% |
| Liquid temperature of during the test | <± 2°C |
| Ambient noise & Reflection | < 0.012 W/kg |

# 7. Specific Absorption Rate (SAR)

## 7.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled

## 7.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{\mathbf{d}}{\mathbf{dt}}\left(\frac{\mathbf{dW}}{\mathbf{dm}}\right) = \frac{\mathbf{d}}{\mathbf{dt}}\left(\frac{\mathbf{dW}}{\boldsymbol{\rho}\mathbf{dv}}\right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = \mathbf{C}\left(\frac{\boldsymbol{\delta}\mathbf{T}}{\boldsymbol{\delta}\mathbf{t}}\right)$$

Where: C is the specific head capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\boldsymbol{\sigma}|\mathbf{E}|^2}{\boldsymbol{\rho}}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the RMS electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

## 7.3 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 ㎑ to 300 ㎓," ANSI/IEEE C95.3–2003, Copyright 2003 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the

frequency range from 100 ㎑ to 6 ㎓. Portable devices that transmit at frequencies above 6 ㎓ are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 ㎓ should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.

| Human Exposure | Uncontrolled Environment General Population | Controlled Environment Occupational |
|---|---|---|
| **Partial Peak SAR** (Partial) | 1.60 m W/g | 8.00 m W/g |
| **Partial Average SAR** (Whole Body) | 0.08 m W/g | 0.40 m W/g |
| **Partial Peak SAR** (Hands/Feet/Ankle/Wrist) | 4.00 m W/g | 20.00 m W/g |

1. The spatial Peak value of the SAR averaged over any 1g gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
2. The spatial Average value of the SAR averaged over the whole body.
3. The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

## 8. The SAR Measurement System

A block diagram of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (SPEAG DASY 5 professional system). The model EX3DV4 field probe is used to determine the internal electric fields. The SAR can be obtained from the equation SAR= $\sigma$ ($|Ei|^2$)/ $\rho$ where $\sigma$ and $\rho$ are the conductivity and mass density of the tissue-simulant.

The DASY 5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Staubli TX family) with controller, teach pendant and software. An arm extension is for accommodating the data acquisition electronics (DAE).
- A dosimeter probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- Data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

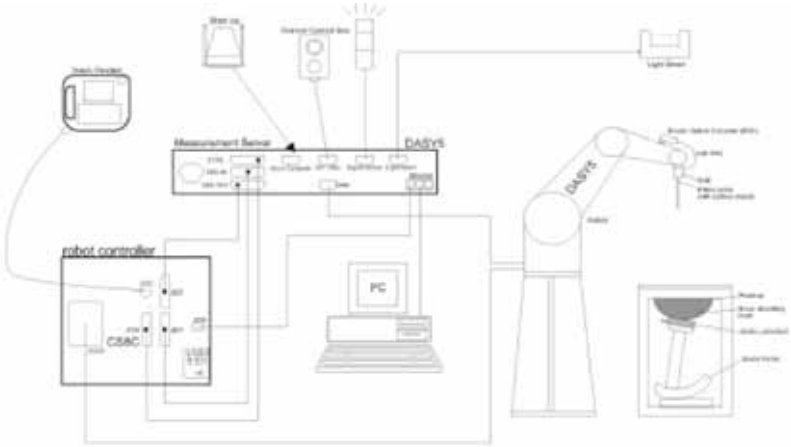


Fig a. The microwave circuit arrangement used for SAR system verification

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows7
- DASY 5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The ELI phantom enabling testing flat usage.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

# 9. System Components

## 9.1 Probe

**Construction** : Symmetrical design with triangular core.
Built-in shielding against static charges.
PEEK enclosure material (resistant to organic solvents, e.g., DGBE)

**Calibration** : Basic Broad Band Calibration in air Conversion Factors (CF) for HSL 835 and HSL1900.
Additional CF-Calibration for other liquids and frequencies upon request.

**Frequency** : 10 ㎒ to 6 ㎓; Linearity: ± 0.2 ㏈ (30 ㎒ to 6 ㎓)

**Directivity** : ± 0.3 ㏈ in HSL (rotation around probe axis)
± 0.5 ㏈ in tissue material (rotation normal to probe axis)

**Dynamic Range** : 10μW/g to > 100 m W/g;
Linearity: ± 0.2 ㏈(noise: typically < 1 μW/g)

**Dimensions** : Overall length: 337 ㎜ (Tip length: 20 ㎜)
Tip diameter: 2.5 ㎜ (Body diameter: 12 ㎜)
Distance from probe tip to dipole centers: 1 ㎜

**Application** : High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 ㎓ with precision of better 30%

**Construction** : Symmetrical design with triangular core.
Built-in shielding against static charges.
PEEK enclosure material (resistant to organic solvents, e.g., DGBE)

EX3DV4 E-Field Probe

**NOTE:**

1. The Probe parameters have been calibrated by the SPEAG. Please reference “APPENDIX C” for the Calibration Certification Report.

## 9.2 ELI Phantom

Construction : Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 ㎒ to 6 ㎓. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG dosimetric probes and dipoles.

ELI V5.0 has the same shell geometry and is manufactured from the same material as ELI4, but has reinforced top structure

ELI Phantom

Shell Thickness : 2.0 mm ± 0.2 mm

Dimensions : Major axis: 600 ㎜
Minor axis: 400 ㎜

### 9.3 Device Holder

Construction: : In combination with the Twin SAM PhantomV4.0/V4.0C or Twin SAM, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

Device Holder

Construction: : Simple but effective and easy-to-use extension for Mounting Device that facilitates the testing of larger devices according to IEC 62209-2 (a.q.. laptops, Cameras, etc.). It is lightweight and fits easily on the upper part of the Mounting Device in place of the phone positioned.

Device Holder

# 10. SAR Measurement Procedures

## 10.1 Normal SAR Measurement Procedure

**Step 1: Power Reference Measurement**

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2 ㎜. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties.

**Step 2 and 3: Area Scan & Zoom Scan Procedures**

The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

1. The extraction of the measured data (grid and values) from the Zoom Scan.
2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
3. The generation of a high-resolution mesh within the measured volume
4. The interpolation of all measured values from the measurement grid to the high-resolution grid
5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
6. The calculation of the averaged SAR within masses of 1 g and 10 g.

**Step 4: Power drift measurement**

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

< Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01v01r03 >

| | | | ≤ 3 GHz | > 3 GHz |
|---|---|---|---|---|
| Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface | | | 5 ± 1 mm | ½·δ·ln(2) ± 0.5 mm |
| Maximum probe angle from probe axis to phantom surface normal at the measurement location | | | 30° ± 1° | 20° ± 1° |
| Maximum area scan spatial resolution: $\Delta x_{Area}$, $\Delta y_{Area}$ | | | ≤ 2 GHz: ≤ 15 mm<br>2 – 3 GHz: ≤ 12 mm | 3 – 4 GHz: ≤ 12 mm<br>4 – 6 GHz: ≤ 10 mm |
| | | | When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be ≤ the corresponding x or y dimension of the test device with at least one measurement point on the test device. | |
| Maximum zoom scan spatial resolution: $\Delta x_{Zoom}$, $\Delta y_{Zoom}$ | | | ≤ 2 GHz: ≤ 8 mm<br>2 – 3 GHz: ≤ 5 mm* | 3 – 4 GHz: ≤ 5 mm*<br>4 – 6 GHz: ≤ 4 mm* |
| Maximum zoom scan spatial resolution, normal to phantom surface | uniform grid: $\Delta z_{Zoom}(n)$ | | ≤ 5 mm | 3 – 4 GHz: ≤ 4 mm<br>4 – 5 GHz: ≤ 3 mm<br>5 – 6 GHz: ≤ 2 mm |
| | graded grid | $\Delta z_{Zoom}(1)$: between 1st two points closest to phantom surface | ≤ 4 mm | 3 – 4 GHz: ≤ 3 mm<br>4 – 5 GHz: ≤ 2.5 mm<br>5 – 6 GHz: ≤ 2 mm |
| | | $\Delta z_{Zoom}(n>1)$: between subsequent points | ≤ 1.5·$\Delta z_{Zoom}(n-1)$ | |
| Minimum zoom scan volume | x, y, z | | ≥ 30 mm | 3 – 4 GHz: ≥ 28 mm<br>4 – 5 GHz: ≥ 25 mm<br>5 – 6 GHz: ≥ 22 mm |

Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.

* When zoom scan is required and the *reported* SAR from the area scan based *1-g SAR estimation* procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.

## 11. SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. 1. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within +/- 10% from the target SAR values. These tests were done at 2450 MHz. The tests were conducted on the same days as the measurement of the DUT. The obtained results from the system accuracy verification are displayed in the table 1. (SAR values are normalized to 1W forward power delivered to the dipole). During the tests, the ambient temperature of the laboratory was in the range (22 ± 2) ° C, the relative humidity was in the range (55 ± 5) % R.H and the liquid depth above the ear reference points was ≥ 15 cm ± 5 mm (frequency ≤ 3 GHz) or ≥ 10 cm ± 5 mm (frequency > 3 G Hz)in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.

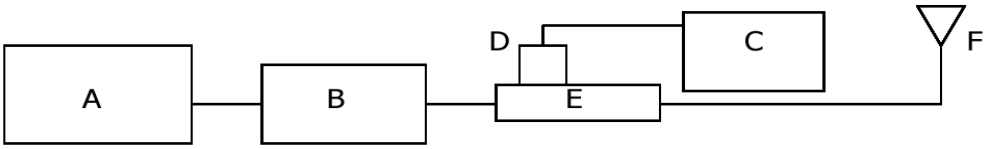


Fig 1. The microwave circuit arrangement used for SAR system verification

A. Agilent Model E8247C Signal Generator
B. EMPOWER Model 2001-BBS3Q7ECK Amplifier
C. Agilent Model E4419B Power Meter
D. Agilent Model 9300H Power Sensor
E. Agilent Model 86205A Directional RF Bridges
F. Reference dipole Antenna

Photo of the dipole Antenna

| Verification Kit | Probe S/N | Tissue | Target SAR 1 g from Calibration Certificate (1 W) | Measured SAR 1 g (0.1 W) | Normalized SAR 1 g (1 W) | Deviation (%) | Date | Liquid Temp. (°C) |
|---|---|---|---|---|---|---|---|---|
| D2450V2 S/N: 734 | 3986 | 2450 MHz Body | 49.8 W/kg | 5.11 | 51.1 | **2.61** | 2014-12-30 | 21.3 |

Table1. Results system verification

## 12. Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this simulant fluid were measured by using the Speag Model DAK-3.5 Dielectric Probe in conjunction with Agilent E5071C Network Analyzer(300 ㎑ - 6 ㎓) by using a procedure detailed in Section V.

| f (㎒) | Tissue type | Limits / Measured | Dielectric Parameters | | |
|---|---|---|---|---|---|
| | | | Permittivity | Conductivity | Simulated Tissue Temp(℃) |
| 2450 | Body | Measured, 2014-12-30 | 52.61 | 1.93 | 21.3 |
| | | *Target Tissue* | *52.70* | *1.95* | 21.0 ~ 23.0 |
| | | Deviation (%) | **-0.17** | **-1.03** | - |
| 2412 | | Measured, 2014-12-30 | 52.72 | 1.88 | 21.3 |
| | | Deviation (%) | **0.04** | **-3.59** | - |
| 2462 | | Measured, 2014-12-30 | 52.58 | 1.94 | 21.3 |
| | | Deviation (%) | **-0.23** | **-0.51** | - |

The composition of the brain & muscle tissue simulating liquid

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

| Ingredients (% by weight) | Frequency (㎒) | | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|
| | 450 | | 835 | | 915 | | 1900 | | 2450 | |
| Tissue Type | Head | Body | Head | Body | Head | Body | Head | Body | Head | Body |
| Water | 38.56 | 51.16 | 41.45 | 52.4 | 41.05 | 56.0 | 54.9 | 40.4 | 62.7 | 73.2 |
| Salt (NaCl) | 3.95 | 1.49 | 1.45 | 1.4 | 1.35 | 0.76 | 0.18 | 0.5 | 0.5 | 0.04 |
| Sugar | 56.32 | 46.78 | 56.0 | 45.0 | 56.5 | 41.76 | 0.0 | 58.0 | 0.0 | 0.0 |
| HEC | 0.98 | 0.52 | 1.0 | 1.0 | 1.0 | 1.21 | 0.0 | 1.0 | 0.0 | 0.0 |
| Bactericide | 0.19 | 0.05 | 0.1 | 0.1 | 0.1 | 0.27 | 0.0 | 0.1 | 0.0 | 0.0 |
| Triton X-100 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 36.8 | 0.0 |
| DGBE | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 0.0 | 44.92 | 0.0 | 0.0 | 26.7 |
| Dielectric Constant | 43.42 | 58.0 | 42.54 | 56.1 | 42.0 | 56.8 | 39.9 | 54.0 | 39.8 | 52.5 |
| Conductivity (S/m) | 0.85 | 0.83 | 0.91 | 0.95 | 1.0 | 1.07 | 1.42 | 1.45 | 1.88 | 1.78 |

Salt: 99 $^{+}$% Pure Sodium Chloride Sugar: 98 $^{+}$% Pure Sucrose

Water: De-ionized, 16 MΩ$^{+}$ resistivity HEC: Hydroxyethyl Cellulose

DGBE: 99 $^{+}$% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1, 3, 3-tetramethylbutyl)phenyl]ether

Simulating Liquids for 5 ㎓, Manufactured by SPEAG

| Ingredients | (% by weight) |
|---|---|
| Water | 78 |
| Mineral Oil | 11 |
| Emulsifiers | 9 |
| Additives and Salt | 2 |

## 13. Test System Validation

Per FCC KDB 865664 D01v01r03, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the require tissue-equivalent media for system validation, according to the procedures outlined in IEEE 1528-2003 and FCC KDB 865664 D01v01r03. Since frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probe and tissue dielectric parameters has been included.

| *f* (MHz) | Date | Probe S/N | Probe Cal point | Tissue Type | Dielectric Parameters | | CW Validation | | | Modulated Validation | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | | | | | Permittivity | Conductivity | Sensitivity | Probe Linearity | Probe Isotropy | Mod. Type | Duty Factor | PAR |
| 2450 | 06/24/2014 | 3986 | 2450 | Body | 51.92 | 1.89 | PASS | PASS | PASS | OFDM | N/A | PASS |

< SAR System Validation Summary>

Note

All measurement were performed using probes calibrated for CW signal only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r03. SAR system were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to KDB 865664 D01v01r03.

## 14. Instruments List

| | | | | | |
|---|---|---|---|---|---|
| **Test Platform** | SPEAG DASY5 Professional | | | | |
| **Location** | SGS Korea Co., Ltd. 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, E&E Lab | | | | |
| **Manufacture** | SPEAG | | | | |
| **Description** | SAR Test System (Frequency range 300 ㎒ - 6 ㎓) | | | | |
| **Software Reference** | DASY52: 52.8.7(1137)<br>SEMCAD X: 14.6.10(7164) | | | | |
| **Hardware Reference** | | | | | |
| **Equipment** | **Type** | **Serial Number** | **Cal Date** | **Cal Interval** | **Cal Due** |
| Robot | TX90XL | F13/5S7KC1/A/01 | N/A | N/A | N/A |
| Software | DASY5 V52 | - | N/A | N/A | N/A |
| Phantom | ELI Phantom | TP-1244 | N/A | N/A | N/A |
| 2450 ㎒ System Validation Dipole | D2450V2 | 734 | 2014-05-20 | Biennial | 2016-05-20 |
| Dosimetric E-Field Probe | EX3DV4 | 3986 | 2014-03-21 | Annual | 2015-03-21 |
| Data acquisition Electronics | DAE4 | 1430 | 2014-03-24 | Annual | 2015-03-24 |
| Network Analyzer | E5071C | MY46111535 | 2014-07-04 | Annual | 2015-07-04 |
| Dielectric Assessment Kit | DAK-3.5 | 1107 | 2014-01-19 | Annual | 2015-01-19 |
| Power Meter | E4419B | GB43311715 | 2014-06-25 | Annual | 2015-06-25 |
| Power Sensor | E9300H | MY41495314 | 2014-07-02 | Annual | 2015-07-02 |
| | | MY41495307 | 2014-07-02 | Annual | 2015-07-02 |
| Signal Generator | E8247C | MY43321024 | 2014-06-25 | Annual | 2015-06-25 |
| Power Amplifier | 2001-BBS3Q7ECK | 1032 D/C 0336 | 2014-12-24 | Annual | 2015-12-24 |
| Directional RF Bridges | 86205A | MY31402302 | 2014-07-03 | Annual | 2015-07-03 |
| LP Filter | LA-30N | N/A | 2014-07-01 | Annual | 2015-07-01 |
| Attenuator | 8491B | 50566 | 2014-07-01 | Annual | 2015-07-01 |
| Hygro- Thermometer | 98585 | 130188 | 2014-06-30 | Annual | 2015-06-30 |
| Digital Thermometer | DTM3000 | 3027 | 2014-07-02 | Annual | 2015-07-02 |
| Spectrum Analyzer | E4445A | MY44020523 | 2014-06-25 | Annual | 2015-06-25 |

## 15. FCC Power Measurement Procedures

The SAR measurement Software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5 % occurred, the tests were repeated.

## 16. Measured and Reported SAR

Per FCC KDB Publication 447498 D01v05r02, When SAR is not measured at the maximum power level allowed for production units, the results must be scaled to the maximum tune-up tolerance limit according to the power applied to the individual channels tested to determine compliance. For simultaneous transmission, the measured aggregate SAR must be scaled according to the sum of the differences between the maximum tune-up tolerance and actual power used to test each transmitter. When SAR is measured at or scaled to the maximum tune-up tolerance limit, the results are referred to as reported SAR. Test highest reported SAR results are identified on the grant of equipment authorization according to procedures in KDB 690783 D01v01r03.

## 17. Maximum Output Power Specifications

This device operates using the following maximum output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB Publication 447498 D01v05r02.

| Average power for Production | | | | |
|---|---|---|---|---|
| **Mode** | **Nominal & Maximum** | **802.11b** | **802.11g** | **802.11n HT20** |
| WLAN | **Maximum** | **15.0** | **11.0** | **10.0** |
| | Nominal | 13.5 | 9.5 | 8.5 |
| Bluetooth | **Nominal & Maximum** | **GFSK** | **DPSK** | **8DPSK** |
| | **Maximum** | **6.0** | **3.0** | **3.0** |
| | Nominal | 4.5 | 1.5 | 1.5 |
| Tune-up Tolerance: -1.5 dB / + 1.5 dB | | | | |

## 18. RF Conducted Power Measurement

IEEE 802.11b Average RF Power

| Mode | Frequency | Channel | 802.11b (2.4 GHz) Conducted Power (dBm) | | | |
|---|---|---|---|---|---|---|
| | | | Data Rate (Mbps) | | | |
| | | | 1 | 2 | 5.5 | 11 |
| 802.11b | 2412 | 1 | 14.29 | 14.05 | 13.54 | 13.51 |
| | 2437 | 6 | 14.73 | 14.66 | 13.63 | 13.51 |
| | 2462 | 11 | 14.34 | 14.16 | 13.82 | 13.76 |

IEEE 802.11g Average RF Power

| Mode | Frequency | Channel | 802.11g (2.4 GHz) Conducted Power (dBm) | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|
| | | | Data Rate (Mbps) | | | | | | | |
| | | | 6 | 9 | 12 | 18 | 24 | 36 | 48 | 54 |
| 802.11g | 2412 | 1 | 10.54 | 10.28 | 10.09 | 9.78 | 9.65 | 8.89 | 8.71 | 8.51 |
| | 2437 | 6 | 10.66 | 10.34 | 10.17 | 10.05 | 9.89 | 8.80 | 8.80 | 8.59 |
| | 2462 | 11 | 10.70 | 10.18 | 10.14 | 9.98 | 8.47 | 8.85 | 8.78 | 8.56 |

IEEE 802.11n Average RF Power 20 MHz Bandwidth

| Mode | Frequency | Channel | 802.11n (2.4 GHz) Conducted Power (dBm) | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|
| | | | Data Rate (Mbps) | | | | | | | |
| | | | MCS0 | MCS1 | MCS2 | MCS3 | MCS4 | MCS5 | MCS6 | MCS7 |
| 802.11n | 2412 | 1 | 9.53 | 9.01 | 8.94 | 8.91 | 8.24 | 7.74 | 7.68 | 7.63 |
| | 2437 | 6 | 9.38 | 8.99 | 8.86 | 8.48 | 8.14 | 8.13 | 7.83 | 7.72 |
| | 2462 | 11 | 9.36 | 8.86 | 8.60 | 8.18 | 8.09 | 8.06 | 7.95 | 7.86 |

Bluetooth

| Channel | Frequency (MHz) | GFSK (dBm) | PI/4DQPSK (dBm) | 8DPSK (dBm) |
|---|---|---|---|---|
| Low | 2402 | 5.32 | 2.19 | 2.19 |
| Middle | 2441 | 5.38 | 2.31 | 2.31 |
| High | 2480 | 5.27 | 2.13 | 2.12 |

# 19. SAR Test Configuration

## 19.1 UMPC Mini-Tablet Devices

Per FCC KDB 941225 D07v01, the test procedures are applicable to devices with a display and overall diagonal dimension ≤ 20 cm(~7.9”). A composite test separation distance of 5 mm is applied to test UMPC mini-tablet transmitters and to maintain RF exposure conservativeness for the interactive operations associated with this type of devices.

Per FCC KDB 941225 D07v01, UMPC mini-tablet devices must be tested for 1-g SAR on all surfaces and side edges with a transmitting antenna located at ≤ 25 mm from that surface or edge, at 5 mm separation from a flat phantom, for the data modes, wireless technologies and frequency bands supported by the device to determine SAR compliance. When 1-g SAR is tested at 5 mm, 10-g SAR is not required

## 19.2 IEEE 802.11 Transmitters

802.11 a/b/g and 4.9 ㎓ operating modes are tested independently according to the service requirements in each frequency band. 802.11 b/g modes are tested on channel 1, 6, and 11. 802.11a is tested for UNII operations on channels 36 and 48 in the 5.15 ~ 5.25 ㎓ band, channels 52 and 64 in the 5.25 ~ 5.35 ㎓ band, channels 104, 116, 124 and 136 in the 5.470 ~ 5.725 ㎓ band, and channels 149 and 161 in the 5.8 ㎓ band. When 5.8 ㎓ §15.247 is also available, channels 149, 157 and 165 should be tested instead of the UNII channels. 802.11g mode was evaluated only if the output power was 0.25 ㏈ higher than the 802.11b mode.

| Mode | | GHz | Channel | Turbo Channel | “Default Test Channels” | | | |
|---|---|---|---|---|---|---|---|---|
| | | | | | §15.247 | | UNII | |
| | | | | | 802.11b | 802.11g | | |
| 802.11 b/g | | 2.412 | 1# | | √ | ∇ | | |
| | | 2.437 | 6 | 6 | √ | ∇ | | |
| | | 2.462 | 11# | | √ | ∇ | | |
| 802.11a | UNII | 5.18 | 36 | 42 (5.21 GHz) | | | √ | |
| | | 5.20 | 40 | | | | | * |
| | | 5.22 | 44 | | | | | * |
| | | 5.24 | 48 | 50 (5.25 GHz) | | | √ | |
| | | 5.26 | 52 | | | | √ | |
| | | 5.28 | 56 | 58 (5.29 GHz) | | | | * |
| | | 5.30 | 60 | | | | | * |
| | | 5.32 | 64 | | | | √ | |
| | | 5.500 | 100 | Unknown | | | | * |
| | | 5.520 | 104 | | | | √ | |
| | | 5.540 | 108 | | | | | * |
| | | 5.560 | 112 | | | | | * |
| | | 5.580 | 116 | | | | √ | |
| | | 5.600 | 120 | | | | | * |
| | | 5.620 | 124 | | | | √ | |
| | | 5.640 | 128 | | | | | * |
| | | 5.660 | 132 | | | | | * |
| | | 5.680 | 136 | | | | √ | |
| | | 5.700 | 140 | | | | | * |
| | UNII or §15.247 | 5.745 | 149 | | √ | | √ | |
| | | 5.765 | 153 | 152 (5.76 GHz) | | * | | * |
| | | 5.785 | 157 | | √ | | | * |
| | | 5.805 | 161 | 160 (5.80 GHz) | | * | √ | |
| | §15.247 | 5.825 | 165 | | √ | | | |

- √ = “default test channels”
- * = possible 802.11a channels with maximum average output > the “default test channels”
- ∇ = possible 802.11g channels with maximum average output ¼ dB ≥ the “default test channels”
- # = when output power is reduced for channel 1 and/or 11 to meet restricted band requirements the highest output channels closest to each of these channels should be tested

## 20. Transmit Antenna Separation Distances

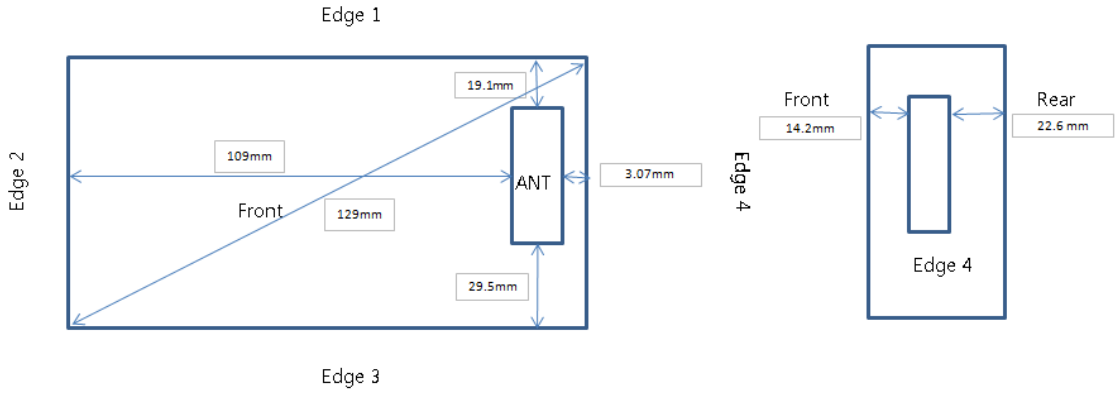


### 20.1 UMPC mini-tablet transmitter for SAR Testing

| Mode | Test Position | | | | | |
|---|---|---|---|---|---|---|
| | Front | Rear | Edge 1 | Edge 2 | Edge 3 | Edge 4 |
| WLAN | O | O | O | X | X | O |

Note:

- SAR is not required because the distance from the antenna to the edge is > 25 mm as per KDB 941225 D07v01r01 SAR Evaluation Procedures for UMPC Mini-Tablet Devices.
- BT and WLAN cannot transmit simultaneously.

## 21. SAR Test Exclusions Applied

Per FCC KDB 447498 D01v05, the SAR exclusion threshold for distances < 50 ㎜ is defined by the following equation:

$$\frac{\text{Max Power of Channel (mW)}}{\text{Test Separation Distance (mm)}} * \sqrt{\text{Frequency(GHz)}} \leq 3.0$$

Based on the maximum tune-up tolerance limit of Bluetooth the antenna to use separation distance,

**<u>Bluetooth SAR was not required</u>: [4/5 * √2.480] = 1.3＜3.0**

## 22. SAR Data Summary

| | |
|---|---|
| Ambient Temperature (°C) | 23.4 |
| Liquid Temperature (°C) | 21.3 |
| Date | 2014-12-30 |

### 802.11b Body SAR

| Test Mode | EUT Position | Traffic Channel | | Distance (㎜) | Power(dBm) | | 1-g SAR (W/kg) | | 1 g SAR Limits (W/kg) |
|---|---|---|---|---|---|---|---|---|---|
| | | Frequency (㎒) | Channel | | Measured Power | Tune-Up Limit | Measured SAR | Scaled SAR | |
| 802.11b | Front | 2437 | 6 | 5 | 14.73 | 15.00 | 0.126 | 0.134 | 1.6 |
| | Rear | 2437 | 6 | 5 | 14.73 | 15.00 | 0.119 | 0.127 | |
| | Edge1 | 2437 | 6 | 5 | 14.73 | 15.00 | 0.165 | 0.176 | |
| | Edge4 | 2437 | 6 | 5 | 14.73 | 15.00 | 0.228 | **0.243** | |

General Notes

1. The test data reported are the worst-case SAR values according to test procedures specified in IEEE 1528-2013, FCC KDB Publication 865664 D01v01r03 and FCC KDB Publication 447498 D01v05r02.
2. All modes of operation were investigated, and worst-case results are reported.
3. The EUT is tested 2nd hot-spot peak, if it is less than 2 dB below the highest peak.
4. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
5. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB Publication 447498 D01v05r02.
6. For 2.4 GHz, justification for reduced test configuration for WIFI channels per KDB Publication 248227 and April 2010 FCC/TCB Meeting Notes: Highest average RF output power channel for the lowest data rate were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers were not greater than 0.25 dB than that of the corresponding channel in the lowest data rate IEEE 802.11b modes.
7. Since the maximum extrapolated peak SAR of the zoom scan for the maximum output channel was ≤ 1.6 W/kg and the reported 1g averaged SAR was < 0.8 W/kg, SAR testing on other default channels was not required.
8. According to KDB248227 D01v01, when the maximum average output channel in each frequency band is not include in the “default test channels”, the maximum average output power channel should be tested instead of an adjacent “default test channels”.
9. WLAN transmission was verified using a spectrum analyzer.

# 23. SAR Measurement Variability

## 23.1 Measurement Variability

Per FCC KDB Publication 865664 D01v01r03, SAR measurement variability was assessed for each frequency band, which was determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media were required for SAR measurements in a frequency band, the variability measurement procedures were applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium. These additional measurements were repeated after the completion of all measurements requiring the same head or body tissue-equivalent medium in a frequency band. The test device was returned to ambient conditions (normal room temperature) with the battery fully charged before it was re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

SAR Measurement Variability was assessed using the following procedures for each frequency band:

1. When the original highest measured SAR is ≥ 0.80 W/kg, the measurement was repeated once.
2. A second repeated measurement was preformed only if the ratio of largest to smallest SAR for the original and first repeated measurements was > 1.20 or when the original or repeated measurement was ≥ 1.45 W/kg (~ 10% from the 1-g SAR limit).
3. A third repeated measurement was performed only if the original, first or second repeated measurement was ≥ 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.
4. **Repeated measurements are not required when the original highest measured SAR is < 0.80 W/kg**

Note: All measured SAR values were < 0.8 W/kg. Therefore, no SAR measurement variability analysis was required.

## 23.2 Measurement Uncertainty

The measured SAR was < 1.5 W/kg for all frequency bands. Therefore, per KDB Publication 865664 D01v01r03, the extended measurement uncertainty analysis per IEEE 1528-2003 was not required.

# Appendixes List

| | |
|---|---|
| **Appendix A** | A.1 Verification Test Plots for 2450 MHz<br>A.2 SAR Test Plots for 802.11b Mode |
| **Appendix B** | B.1 Uncertainty Analysis |
| **Appendix C** | C.1 Calibration certificate for Probe<br>C.2 Calibration certificate for DAE<br>C.3 Calibration certificate for Dipole |

## Appendix A.1

**Verification Test Plots for 2450 MHz**

Date: 2014-12-30

Test Laboratory : SGS Korea (Gunpo Laboratory)
File Name: 2450MHz Verification.da53:0

Input Power : 100 mW

Ambient Temp : 23.4 ℃ Tissue Temp : 21.3 ℃

**DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN:734**

Communication System: UID 0, CW (0); Frequency: 2450 MHz;Duty Cycle: 1:1
Medium parameters used: f = 2450 MHz; $\sigma$ = 1.926 S/m; $\varepsilon_r$ = 52.614; $\rho$ = 1000 kg/m$^3$
Phantom section: Flat Section

DASY52 Configuration:
- Probe: EX3DV4 - SN3986; ConvF(7.6, 7.6, 7.6); Calibrated: 2014-03-21;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1430; Calibrated: 2014-03-24
- Phantom: ELI v4.0; Type: QDOVA002AA; Serial: TP:1244
- DASY52 52.8.7(1137)SEMCAD X 14.6.10(7164)

**Verification/2450MHz Verification/Area Scan (91x91x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm
Maximum value of SAR (interpolated) = 7.92 W/kg

**Verification/2450MHz Verification/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 55.364 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 10.4 W/kg
**SAR(1 g) = 5.11 W/kg; SAR(10 g) = 2.38 W/kg**
Maximum value of SAR (measured) = 7.76 W/kg

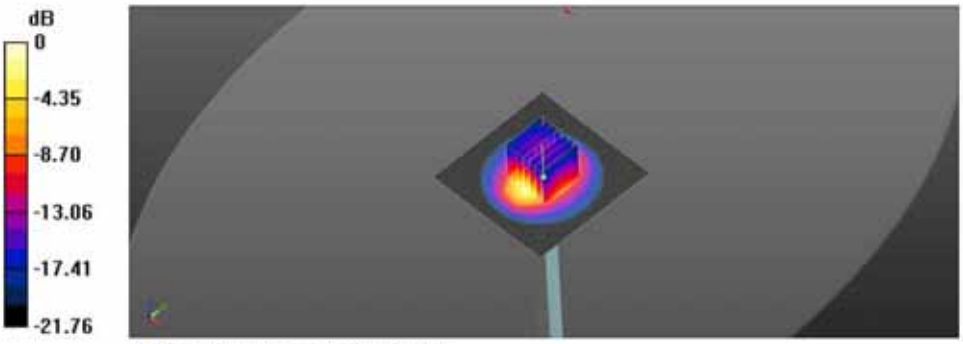


0 dB = 7.76 W/kg = 8.90 dBW/kg

**Appendix A.2**

**SAR Test Plots for 802.11b Mode**

Date: 2014-12-30

Test Laboratory : SGS Korea (Gunpo Laboratory)
File Name: 2.45GHz_WLAN_802.11b_1Mbps_Edge4_CH6.da53:0

Ambient Temp : 23.4 ℃ Tissue Temp : 21.3 ℃

**DUT: NX500; Type: Digital Camera; Serial: DV3-276**

Communication System: UID 0, WLAN 2.45GHz (0); Frequency: 2437 MHz;Duty Cycle: 1:1
Medium parameters used: f = 2437 MHz; $\sigma$ = 1.91 S/m; $\varepsilon_r$ = 52.644; $\rho$ = 1000 kg/m$^3$
Phantom section: Flat Section

DASY52 Configuration:
- Probe: EX3DV4 - SN3986; ConvF(7.6, 7.6, 7.6); Calibrated: 2014-03-21;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1430; Calibrated: 2014-03-24
- Phantom: ELI v4.0; Type: QDOVA002AA; Serial: TP:1244
- DASY52 52.8.7(1137)SEMCAD X 14.6.10(7164)

**WLAN/2.45GHz_WLAN_802.11b_1Mbps_Edge4_CH6/Area Scan (131x141x1):**
Interpolated grid: dx=1.000 mm, dy=1.000 mm
Maximum value of SAR (interpolated) = 0.334 W/kg

**WLAN/2.45GHz_WLAN_802.11b_1Mbps_Edge4_CH6/Zoom Scan (7x7x7)/Cube 0:**
Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 9.020 V/m; Power Drift = -0.12 dB
Peak SAR (extrapolated) = 0.466 W/kg
**SAR(1 g) = 0.228 W/kg; SAR(10 g) = 0.107 W/kg**
Maximum value of SAR (measured) = 0.342 W/kg

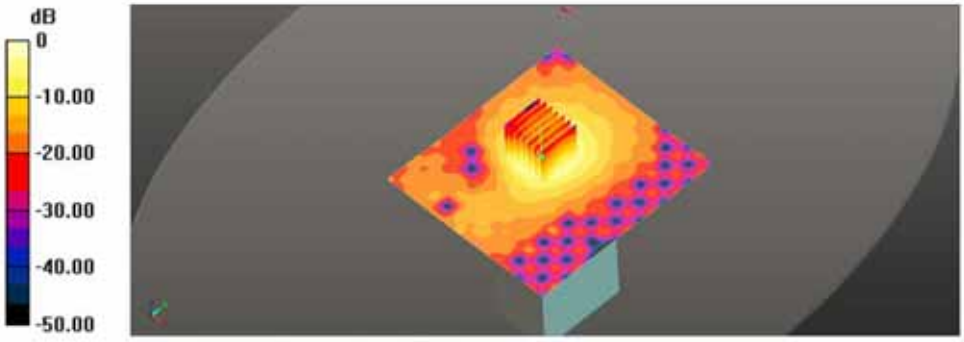


0 dB = 0.342 W/kg = -4.66 dBW/kg

## Appendix B.1 Uncertainty Analysis DASY5 #3

Measurement uncertainty for 300 MHz to 3 GHz averaged over 1 gram

| a | b | c | d | e = f(d,k) | g | i = cxg/e | k |
|---|---|---|---|---|---|---|---|
| Uncertainty Component | Section in P1528 | Tol (%) | Prob . Dist. | Div. | Ci (1g) | 1g ui (%) | Vi (Veff) |
| Probe calibration | E.2.1 | 6.55 | N | 1 | 1 | 6.55 | ∞ |
| Axial isotropy | E.2.2 | 4.7 | R | 1.73 | 0.71 | 1.92 | ∞ |
| hemispherical isotropy | E.2.2 | 9.6 | R | 1.73 | 0.71 | 3.92 | ∞ |
| Boundary effect | E.2.3 | 1.0 | R | 1.73 | 1 | 0.58 | ∞ |
| Linearity | E.2.4 | 4.7 | R | 1.73 | 1 | 2.71 | ∞ |
| System detection limit | E.2.5 | 0.3 | R | 1.73 | 1 | 0.14 | ∞ |
| Readout electronics | E.2.6 | 0.3 | N | 1 | 1 | 0.30 | ∞ |
| Response time | E.2.7 | 0.5 | R | 1.73 | 1 | 0.29 | ∞ |
| Integration time | E.2.8 | 2.6 | R | 1.73 | 1 | 1.50 | ∞ |
| RF ambient Condition -Noise | E.6.1 | 3 | R | 1.73 | 1 | 1.73 | ∞ |
| RF ambient Condition - reflections | E.6.1 | 3 | R | 1.73 | 1 | 1.73 | ∞ |
| Probe positioning- mechanical tolerance | E.6.2 | 1.5 | R | 1.73 | 1 | 0.87 | ∞ |
| Probe positioning- with respect to phantom | E.6.3 | 2.9 | R | 1.73 | 1 | 1.67 | ∞ |
| Max. SAR evaluation | E.5.2 | 1.0 | R | 1.73 | 1 | 0.58 | ∞ |
| Test sample positioning | E.4.2 | 1.35 | N | 1 | 1 | 1.35 | 9 |
| Device holder uncertainty | E.4.1 | 3.6 | N | 1 | 1 | 3.60 | 4 |
| Output power variation -SAR drift measurement | 6.6.3 | 5 | R | 1.73 | 1 | 2.89 | ∞ |
| Phantom uncertainty (shape and thickness tolerances) | E.3.1 | 4 | R | 1.73 | 1 | 2.31 | ∞ |
| Liquid conductivity – deviation from target values | E.3.2 | 5 | R | 1.73 | 0.64 | 1.85 | ∞ |
| Liquid conductivity - measurement uncertainty | E.3.2 | 0.38 | N | 1 | 0.64 | 0.24 | 9 |
| Liquid permittivity – deviation from target values | E.3.3 | 5 | R | 1.73 | 0.6 | 1.73 | ∞ |
| Liquid permittivity – deviation from target values | E.3.3 | 0.27 | N | 1 | 0.6 | 0.16 | 9 |
| Combined standard uncertainty | | | | RSS | | 10.83 | 324 |
| Expanded uncertainty (95% CONFIDENCE INTERVAL) | | | | *k*=2 | | **21.66** | |

**Appendix C.1 Calibration certificate for Probe**

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
Servizio svizzero di taratura
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 108**

Client **SGS (Dymstec)**

Certificate No: **EX3-3986_Mar14**

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | EX3DV4 - SN:3986 |
| Calibration procedure(s) | QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6<br>Calibration procedure for dosimetric E-field probes |
| Calibration date: | March 21, 2014 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration |
|---|---|---|---|
| Power meter E4419B | GB41293874 | 04-Apr-13 (No. 217-01733) | Apr-14 |
| Power sensor E4412A | MY41498087 | 04-Apr-13 (No. 217-01733) | Apr-14 |
| Reference 3 dB Attenuator | SN: S5054 (3c) | 04-Apr-13 (No. 217-01737) | Apr-14 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735) | Apr-14 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738) | Apr-14 |
| Reference Probe ES3DV2 | SN: 3013 | 30-Dec-13 (No. ES3-3013_Dec13) | Dec-14 |
| DAE4 | SN: 660 | 13-Dec-13 (No. DAE4-660_Dec13) | Dec-14 |
| | | | |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check |
| RF generator HP 8648C | US3642U01700 | 4-Aug-99 (in house check Apr-13) | In house check: Apr-16 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by: | Jeton Kastrati | Laboratory Technician | |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: March 21, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3986_Mar14 Page 1 of 11

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
**S** Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 108**

## Glossary:

| | |
|---|---|
| TSL | tissue simulating liquid |
| NORMx,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORMx,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C, D | modulation dependent linearization parameters |
| Polarization φ | φ rotation around probe axis |
| Polarization ϑ | ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., ϑ = 0 is normal to probe axis |
| Connector Angle | information used in DASY system to align probe sensor X to the robot coordinate system |

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

## Methods Applied and Interpretation of Parameters:

- *NORMx,y,z:* Assessed for E-field polarization ϑ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the $E^2$-field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)x,y,z = NORMx,y,z * frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- *DCPx,y,z:* DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- *PAR:* PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- *Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D* are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. *VR* is the maximum calibration range expressed in RMS voltage across the diode.
- *ConvF and Boundary Effect Parameters:* Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z * ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORMx* (no uncertainty required).

# Probe EX3DV4

## SN:3986

Manufactured: November 11, 2013
Calibrated: March 21, 2014

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

## Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|---|---|---|---|
| Norm ($\mu V/(V/m)^2$)[A] | 0.53 | 0.53 | 0.49 | ± 10.1 % |
| DCP (mV)[B] | 96.5 | 99.2 | 103.3 | |

## Modulation Calibration Parameters

| UID | Communication System Name | | A dB | B dB√μV | C | D dB | VR mV | Unc[E] (k=2) |
|---|---|---|---|---|---|---|---|---|
| 0 | CW | X | 0.0 | 0.0 | 1.0 | 0.00 | 147.4 | ±3.8 % |
| | | Y | 0.0 | 0.0 | 1.0 | | 147.9 | |
| | | Z | 0.0 | 0.0 | 1.0 | | 141.5 | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

[A] The uncertainties of NormX,Y,Z do not affect the $E^2$-field uncertainty inside TSL (see Pages 5 and 6).
[B] Numerical linearization parameter: uncertainty not required.
[E] Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4– SN:3986 March 21, 2014

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

## Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) [C] | Relative Permittivity [F] | Conductivity (S/m) [F] | ConvF X | ConvF Y | ConvF Z | Alpha [G] | Depth [G] (mm) | Unct. (k=2) |
|---|---|---|---|---|---|---|---|---|
| 835 | 41.5 | 0.90 | 10.24 | 10.24 | 10.24 | 0.31 | 1.03 | ± 12.0 % |
| 900 | 41.5 | 0.97 | 10.05 | 10.05 | 10.05 | 0.49 | 0.78 | ± 12.0 % |
| 1750 | 40.1 | 1.37 | 8.66 | 8.66 | 8.66 | 0.36 | 0.88 | ± 12.0 % |
| 1900 | 40.0 | 1.40 | 8.45 | 8.45 | 8.45 | 0.53 | 0.73 | ± 12.0 % |
| 2450 | 39.2 | 1.80 | 7.66 | 7.66 | 7.66 | 0.49 | 0.71 | ± 12.0 % |
| 5200 | 36.0 | 4.66 | 5.15 | 5.15 | 5.15 | 0.40 | 1.80 | ± 13.1 % |
| 5300 | 35.9 | 4.76 | 4.88 | 4.88 | 4.88 | 0.40 | 1.80 | ± 13.1 % |
| 5500 | 35.6 | 4.96 | 5.02 | 5.02 | 5.02 | 0.40 | 1.80 | ± 13.1 % |
| 5600 | 35.5 | 5.07 | 4.81 | 4.81 | 4.81 | 0.40 | 1.80 | ± 13.1 % |
| 5800 | 35.3 | 5.27 | 4.70 | 4.70 | 4.70 | 0.45 | 1.80 | ± 13.1 % |

[C] Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
[F] At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
[G] Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

## Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) [C] | Relative Permittivity [F] | Conductivity (S/m) [F] | ConvF X | ConvF Y | ConvF Z | Alpha [G] | Depth [G] (mm) | Unct. (k=2) |
|---|---|---|---|---|---|---|---|---|
| 835 | 55.2 | 0.97 | 10.26 | 10.26 | 10.26 | 0.28 | 1.17 | ± 12.0 % |
| 1750 | 53.4 | 1.49 | 8.27 | 8.27 | 8.27 | 0.41 | 0.83 | ± 12.0 % |
| 1900 | 53.3 | 1.52 | 7.99 | 7.99 | 7.99 | 0.29 | 1.07 | ± 12.0 % |
| 2450 | 52.7 | 1.95 | 7.60 | 7.60 | 7.60 | 0.80 | 0.58 | ± 12.0 % |
| 5200 | 49.0 | 5.30 | 4.83 | 4.83 | 4.83 | 0.40 | 1.90 | ± 13.1 % |
| 5300 | 48.9 | 5.42 | 4.49 | 4.49 | 4.49 | 0.45 | 1.90 | ± 13.1 % |
| 5500 | 48.6 | 5.65 | 4.25 | 4.25 | 4.25 | 0.50 | 1.90 | ± 13.1 % |
| 5600 | 48.5 | 5.77 | 3.99 | 3.99 | 3.99 | 0.50 | 1.90 | ± 13.1 % |
| 5800 | 48.2 | 6.00 | 4.18 | 4.18 | 4.18 | 0.50 | 1.90 | ± 13.1 % |

[C] Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
[F] At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
[G] Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4– SN:3986

March 21, 2014

## Frequency Response of E-Field
(TEM-Cell:ifi110 EXX, Waveguide: R22)

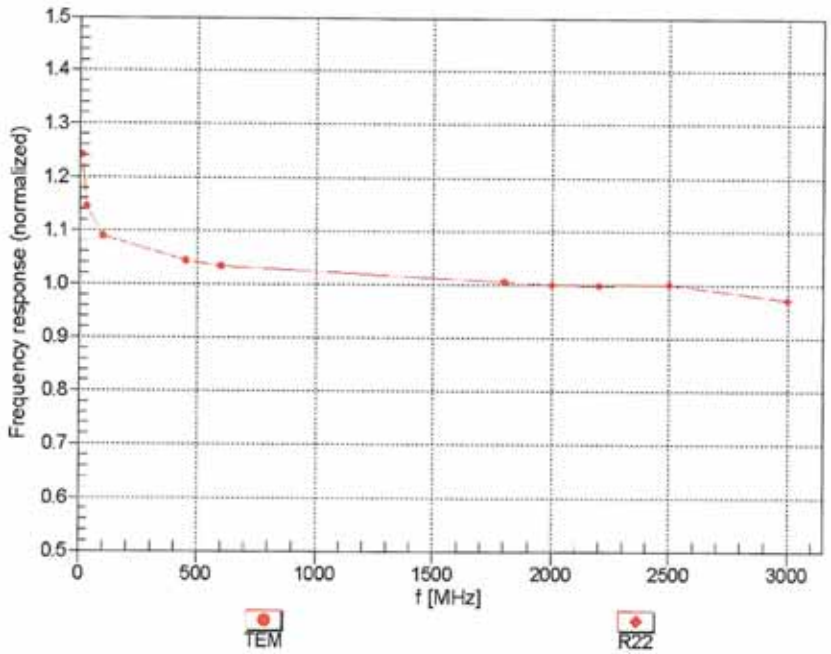


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

EX3DV4– SN:3986

March 21, 2014

## Receiving Pattern (ϕ), ϑ = 0°

f=600 MHz,TEM

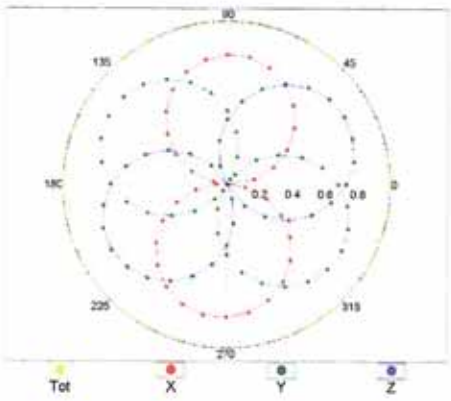


f=1800 MHz,R22

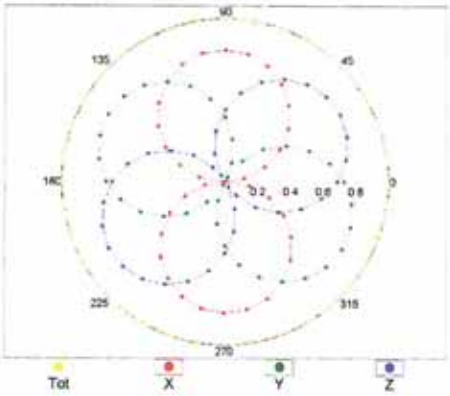


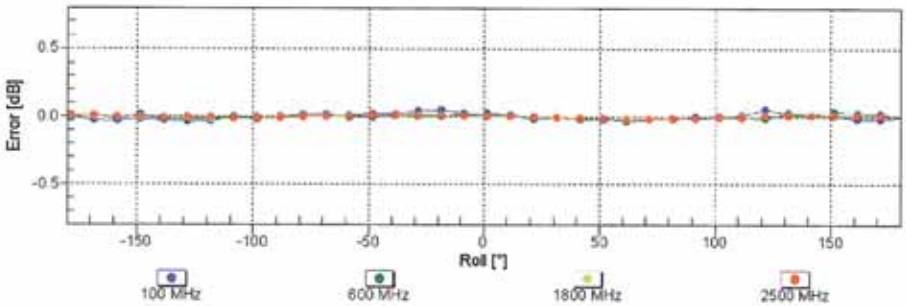


**Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)**

EX3DV4– SN:3986

March 21, 2014

## Dynamic Range f(SAR$_{head}$)
(TEM cell , $f_{eval}$= 1900 MHz)

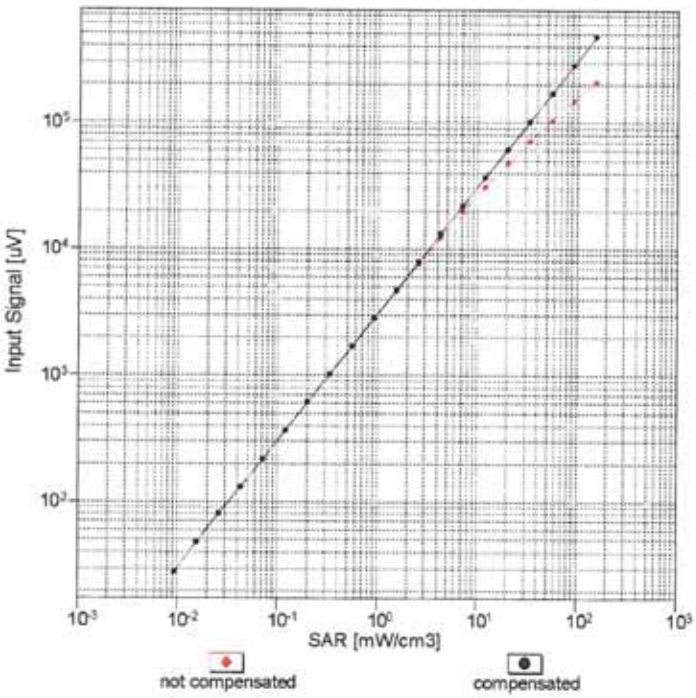


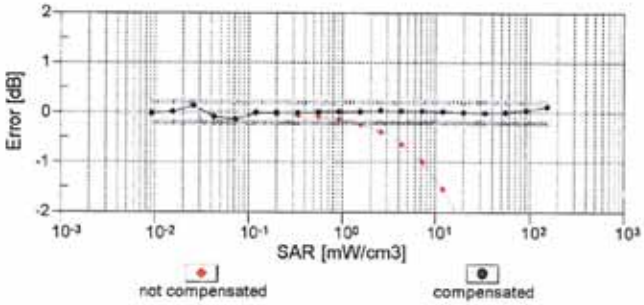


**Uncertainty of Linearity Assessment: ± 0.6% (k=2)**

EX3DV4– SN:3986 March 21, 2014

## Conversion Factor Assessment

f = 835 MHz,WGLS R9 (H_convF)

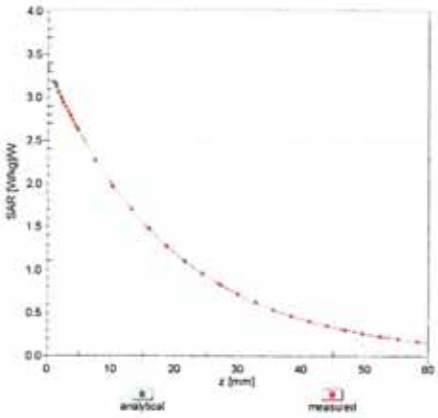


f = 1750 MHz,WGLS R22 (H_convF)

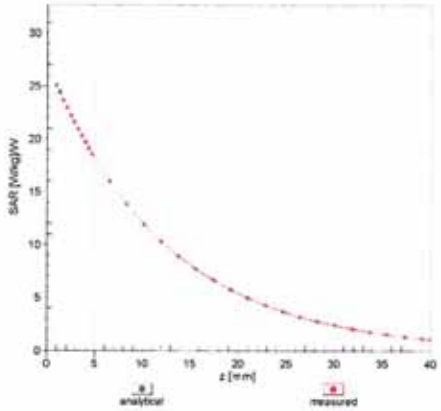


## Deviation from Isotropy in Liquid

Error (ϕ, ϑ), f = 900 MHz

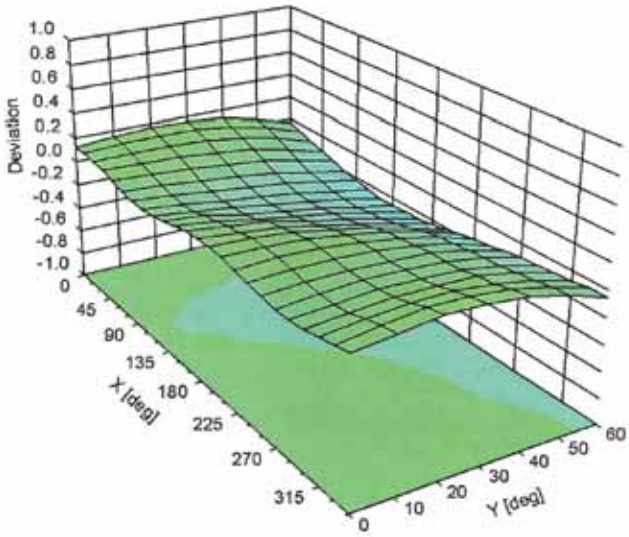





Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: EX3-3986_Mar14 Page 10 of 11

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3986

## Other Probe Parameters

| | |
|---|---|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | -48.4 |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 9 mm |
| Tip Diameter | 2.5 mm |
| Probe Tip to Sensor X Calibration Point | 1 mm |
| Probe Tip to Sensor Y Calibration Point | 1 mm |
| Probe Tip to Sensor Z Calibration Point | 1 mm |
| Recommended Measurement Distance from Surface | 2 mm |

**Appendix C.2 Calibration certificate for DAE**

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
**S** Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 108**

기술책임자
2014. 4. 14

**Client** SGS (Dymstec)

**Certificate No:** DAE4-1430_Mar14

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | DAE4 - SD 000 D04 BM - SN: 1430 |
| Calibration procedure(s) | QA CAL-06.v26<br>Calibration procedure for the data acquisition electronics (DAE) |
| Calibration date: | March 24, 2014 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|---|---|---|---|
| Keithley Multimeter Type 2001 | SN: 0810278 | 01-Oct-13 (No:13976) | Oct-14 |
| **Secondary Standards** | **ID #** | **Check Date (in house)** | **Scheduled Check** |
| Auto DAE Calibration Unit | SE UWS 053 AA 1001 | 07-Jan-14 (in house check) | In house check: Jan-15 |
| Calibrator Box V2.1 | SE UMS 006 AA 1002 | 07-Jan-14 (in house check) | In house check: Jan-15 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by: | Dominique Steffen | Technician | |
| Approved by: | Fin Bomholt | Deputy Technical Manager | |

Issued: March 25, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-1430_Mar14 Page 1 of 5

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
Servizio svizzero di taratura
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 108**

## Glossary

| | |
|---|---|
| DAE | data acquisition electronics |
| Connector angle | information used in DASY system to align probe sensor X to the robot coordinate system. |

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement*: Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

| | | | | |
|---|---|---|---|---|
| High Range: | 1LSB = | 6.1μV , | full range = | -100...+300 mV |
| Low Range: | 1LSB = | 61nV , | full range = | -1.....+3mV |

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X | Y | Z |
|---|---|---|---|
| **High Range** | 403.950 ± 0.02% (k=2) | 404.143 ± 0.02% (k=2) | 403.973 ± 0.02% (k=2) |
| **Low Range** | 3.97294 ± 1.50% (k=2) | 3.99734 ± 1.50% (k=2) | 4.00643 ± 1.50% (k=2) |

## Connector Angle

| | |
|---|---|
| **Connector Angle** to be used in DASY system | 254.0 ° ± 1 ° |

## Appendix

### 1. DC Voltage Linearity

| High Range | | Reading (µV) | Difference (µV) | Error (%) |
|---|---|---|---|---|
| Channel X | + Input | 199995.26 | -0.92 | -0.00 |
| Channel X | + Input | 20003.82 | 3.11 | 0.02 |
| Channel X | - Input | -19999.17 | 1.44 | -0.01 |
| Channel Y | + Input | 199994.65 | -1.91 | -0.00 |
| Channel Y | + Input | 19999.91 | -0.83 | -0.00 |
| Channel Y | - Input | -20001.83 | -1.16 | 0.01 |
| Channel Z | + Input | 199994.72 | -1.73 | -0.00 |
| Channel Z | + Input | 20001.46 | 0.71 | 0.00 |
| Channel Z | - Input | -20000.90 | -0.27 | 0.00 |

| Low Range | | Reading (µV) | Difference (µV) | Error (%) |
|---|---|---|---|---|
| Channel X | + Input | 2001.18 | 0.31 | 0.02 |
| Channel X | + Input | 201.88 | 0.59 | 0.29 |
| Channel X | - Input | -197.92 | 0.76 | -0.38 |
| Channel Y | + Input | 2000.80 | -0.09 | -0.00 |
| Channel Y | + Input | 198.76 | -2.42 | -1.20 |
| Channel Y | - Input | -199.79 | -1.20 | 0.60 |
| Channel Z | + Input | 2000.76 | -0.07 | -0.00 |
| Channel Z | + Input | 200.49 | -0.54 | -0.27 |
| Channel Z | - Input | -199.64 | -0.83 | 0.42 |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Common mode Input Voltage (mV) | High Range Average Reading (µV) | Low Range Average Reading (µV) |
|---|---|---|---|
| Channel X | 200 | 2.92 | 1.46 |
| | - 200 | -0.09 | -1.62 |
| Channel Y | 200 | -20.26 | -21.22 |
| | - 200 | 19.18 | 18.82 |
| Channel Z | 200 | -17.60 | -17.79 |
| | - 200 | 16.06 | 16.42 |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) |
|---|---|---|---|---|
| Channel X | 200 | - | 0.93 | -3.25 |
| Channel Y | 200 | 8.25 | - | 3.38 |
| Channel Z | 200 | 10.05 | 5.15 | - |

## 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | High Range (LSB) | Low Range (LSB) |
|---|---|---|
| Channel X | 16008 | 15788 |
| Channel Y | 16252 | 15331 |
| Channel Z | 15839 | 16937 |

## 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec
Input 10MΩ

| | Average (μV) | min. Offset (μV) | max. Offset (μV) | Std. Deviation (μV) |
|---|---|---|---|---|
| Channel X | 0.39 | -0.47 | 1.25 | 0.32 |
| Channel Y | -2.53 | -3.25 | -1.50 | 0.31 |
| Channel Z | -1.18 | -2.35 | -0.28 | 0.41 |

## 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

## 7. Input Resistance (Typical values for information)

| | Zeroing (kOhm) | Measuring (MOhm) |
|---|---|---|
| Channel X | 200 | 200 |
| Channel Y | 200 | 200 |
| Channel Z | 200 | 200 |

## 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|---|---|
| Supply (+ Vcc) | +7.9 |
| Supply (- Vcc) | -7.6 |

## 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|---|---|---|---|
| Supply (+ Vcc) | +0.01 | +6 | +14 |
| Supply (- Vcc) | –0.01 | -8 | -9 |

**Appendix C.3 Calibration certificate for Dipole**

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 108**

기술책임자

**Client** SGS (Dymstec)

**Certificate No: D2450V2-734_May14** 2014.6.2

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | D2450V2 - SN: 734 |
| Calibration procedure(s) | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |
| Calibration date: | May 20, 2014 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|---|---|---|---|
| Power meter EPM-442A | GB37480704 | 09-Oct-13 (No. 217-01827) | Oct-14 |
| Power sensor HP 8481A | US37292783 | 09-Oct-13 (No. 217-01827) | Oct-14 |
| Power sensor HP 8481A | MY41092317 | 09-Oct-13 (No. 217-01828) | Oct-14 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 03-Apr-14 (No. 217-01918) | Apr-15 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 03-Apr-14 (No. 217-01921) | Apr-15 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Dec-13 (No. ES3-3205_Dec13) | Dec-14 |
| DAE4 | SN: 601 | 30-Apr-14 (No. DAE4-601_Apr14) | Apr-15 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---|---|---|---|
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-13) | In house check: Oct-16 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by: | Claudio Leubler | Laboratory Technician | |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: May 21, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-734_May14 Page 1 of 8

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
Servizio svizzero di taratura
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 108**

**Glossary:**

| | |
|---|---|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

**Calibration is Performed According to the Following Standards:**

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|---|---|---|
| **DASY Version** | DASY5 | V52.8.8 |
| **Extrapolation** | Advanced Extrapolation | |
| **Phantom** | Modular Flat Phantom | |
| **Distance Dipole Center - TSL** | 10 mm | with Spacer |
| **Zoom Scan Resolution** | dx, dy, dz = 5 mm | |
| **Frequency** | 2450 MHz ± 1 MHz | |

## Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---|---|---|
| **Nominal Head TSL parameters** | 22.0 °C | 39.2 | 1.80 mho/m |
| **Measured Head TSL parameters** | (22.0 ± 0.2) °C | 38.5 ± 6 % | 1.83 mho/m ± 6 % |
| **Head TSL temperature change during test** | < 0.5 °C | ---- | ---- |

## SAR result with Head TSL

| **SAR averaged over 1 $cm^3$ (1 g) of Head TSL** | Condition | |
|---|---|---|
| SAR measured | 250 mW input power | 13.2 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | **52.2 W/kg ± 17.0 % (k=2)** |

| **SAR averaged over 10 $cm^3$ (10 g) of Head TSL** | condition | |
|---|---|---|
| SAR measured | 250 mW input power | 6.11 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | **24.3 W/kg ± 16.5 % (k=2)** |

## Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---|---|---|
| **Nominal Body TSL parameters** | 22.0 °C | 52.7 | 1.95 mho/m |
| **Measured Body TSL parameters** | (22.0 ± 0.2) °C | 50.8 ± 6 % | 2.03 mho/m ± 6 % |
| **Body TSL temperature change during test** | < 0.5 °C | ---- | ---- |

## SAR result with Body TSL

| **SAR averaged over 1 $cm^3$ (1 g) of Body TSL** | Condition | |
|---|---|---|
| SAR measured | 250 mW input power | 12.8 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | **49.8 W/kg ± 17.0 % (k=2)** |

| **SAR averaged over 10 $cm^3$ (10 g) of Body TSL** | condition | |
|---|---|---|
| SAR measured | 250 mW input power | 5.90 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | **23.2 W/kg ± 16.5 % (k=2)** |

## Appendix

### Antenna Parameters with Head TSL

| | |
|---|---|
| Impedance, transformed to feed point | 53.3 Ω + 4.2 jΩ |
| Return Loss | - 25.7 dB |

### Antenna Parameters with Body TSL

| | |
|---|---|
| Impedance, transformed to feed point | 50.1 Ω + 5.2 jΩ |
| Return Loss | - 25.8 dB |

### General Antenna Parameters and Design

| | |
|---|---|
| Electrical Delay (one direction) | 1.152 ns |

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

| | |
|---|---|
| Manufactured by | SPEAG |
| Manufactured on | May 07, 2003 |

## DASY5 Validation Report for Head TSL

Date: 20.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 734**

Communication System: UID 0 - CW; Frequency: 2450 MHz
Medium parameters used: f = 2450 MHz; $\sigma$ = 1.83 S/m; $\varepsilon_r$ = 38.5; $\rho$ = 1000 kg/m$^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 101.3 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 27.4 W/kg
**SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.11 W/kg**
Maximum value of SAR (measured) = 17.4 W/kg

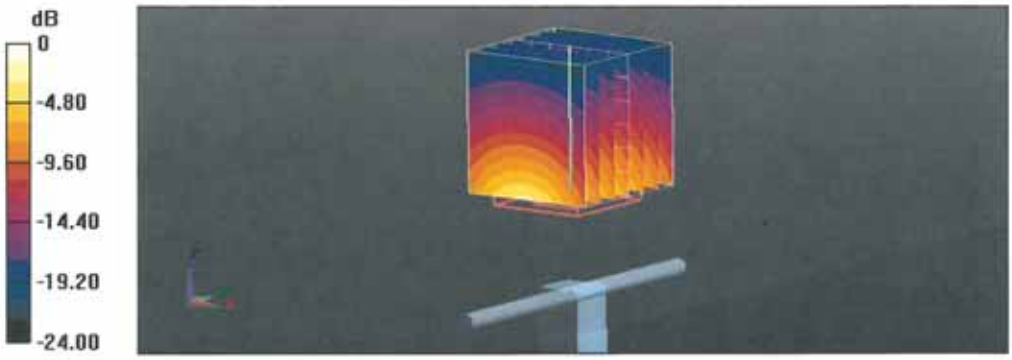


0 dB = 17.4 W/kg = 12.41 dBW/kg

**Impedance Measurement Plot for Head TSL**

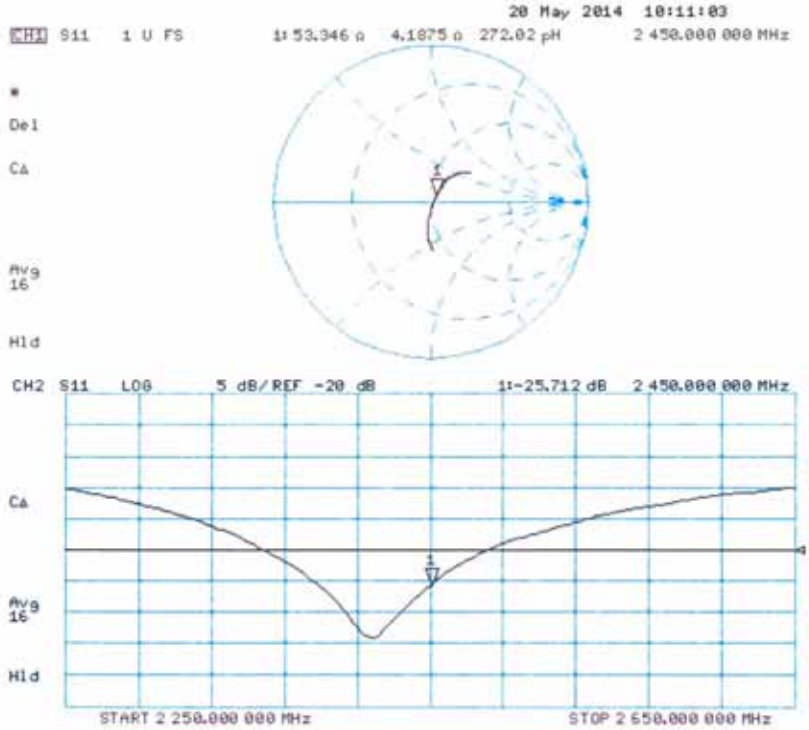

**DASY5 Validation Report for Body TSL**

Date: 20.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 734**

Communication System: UID 0 - CW; Frequency: 2450 MHz
Medium parameters used: f = 2450 MHz; $\sigma$ = 2.03 S/m; $\varepsilon_r$ = 50.8; $\rho$ = 1000 kg/m$^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.35, 4.35, 4.35); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**
Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 94.69 V/m; Power Drift = 0.00 dB
Peak SAR (extrapolated) = 27.0 W/kg
**SAR(1 g) = 12.8 W/kg; SAR(10 g) = 5.9 W/kg**
Maximum value of SAR (measured) = 17.1 W/kg

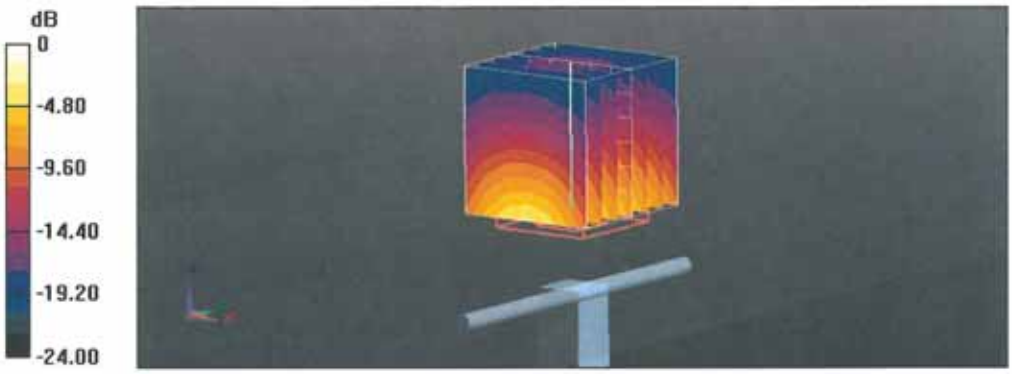


0 dB = 17.1 W/kg = 12.33 dBW/kg

**Impedance Measurement Plot for Body TSL**

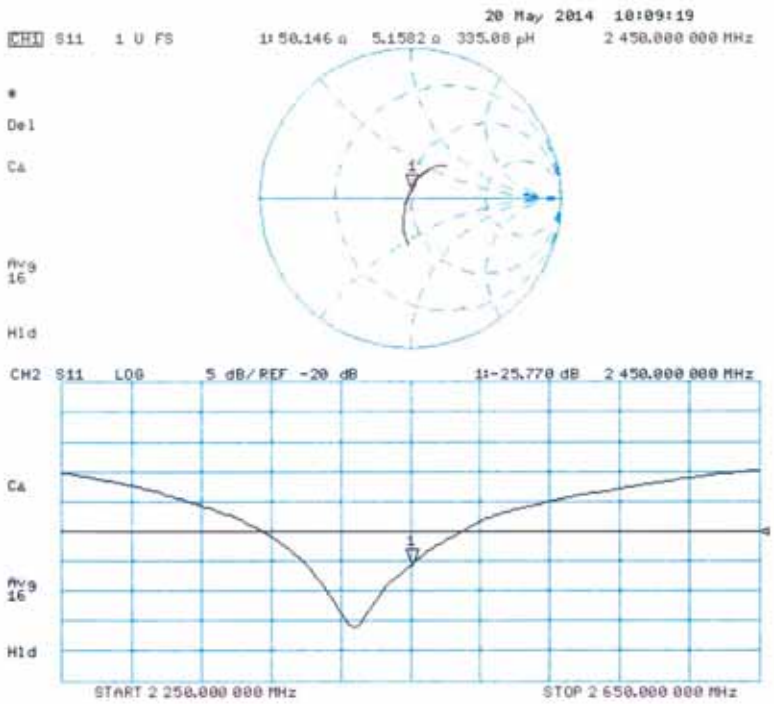




**-THE END-**