

Appendix B: Tissue Stimulating Liquids, System Checks and System Validation

B.1. SAR System Check

Prior to SAR assessment, the system is verified to $\pm 10\%$ of the SAR measurement on the reference dipole at the time of calibration by the calibration facility. Full system validation status and result summary can be found in Section B.3.

Table 1 System Check Results (SAR)

System	Frequency (MHz)	Tissue Type	Date	Amb. Temp. (°C)	Tissue Temp (°C)	Input Power (dBm)	Verification Source SN	Probe SN	DAE SN	Measured 1g SAR (W/Kg)	1W Target 1g SAR (W/Kg)	1W Normalized 1g SAR (W/Kg)	1g SAR Deviation	Measured 10g SAR (W/Kg)	1W Target 10g SAR (W/Kg)	1W Normalized 10g SAR (W/Kg)	10g SAR Deviation
Gamma	13	Head	06/26/2025	22.9	22.5	24.5	1041	7836	1839	0.126	0.457	0.447	-2.17%	0.077	0.296	0.273	-7.70%
Delta	750	Head	06/18/2025	22.5	22.7	17	1235	7853	1844	0.419	8.690	8.360	-3.80%	0.274	5.690	5.467	-3.92%
Delta	750	Head	07/01/2025	23.5	22.7	17	1235	7853	1844	0.413	8.690	8.240	-5.17%	0.270	5.690	5.387	-5.32%
Delta	835	Head	06/18/2025	22.5	22.7	17	4d311	7853	1844	0.499	9.820	9.956	1.39%	0.324	6.370	6.465	1.49%
Delta	835	Head	06/20/2025	22.9	22.1	17	4d311	7853	1844	0.495	9.820	9.877	0.58%	0.323	6.370	6.445	1.17%
Gamma	835	Head	06/27/2025	22.5	23.1	17	4d311	7836	1839	0.518	9.820	10.335	5.25%	0.338	6.370	6.744	5.87%
Delta	1750	Head	06/23/2025	23.1	22.2	17	1205	7857	1844	1.900	36.500	37.910	3.86%	1.010	19.200	20.152	4.96%
Delta	1750	Head	06/27/2025	22.5	23.1	17	1205	7857	1844	1.760	36.500	35.117	-3.79%	0.938	19.200	18.716	-2.52%
Delta	1900	Head	06/25/2025	22.7	21.9	17	5d252	7857	1844	2.030	39.800	40.504	1.77%	1.050	21.000	20.950	-0.24%
Gamma	1900	Head	06/27/2025	22.5	23.1	17	5d252	7836	1839	1.980	39.800	39.506	-0.74%	1.040	21.000	20.751	-1.19%
Gamma	2450	Head	06/16/2025	23.3	22.2	17	1112	7836	1839	2.430	50.600	48.485	-4.18%	1.140	23.700	22.746	-4.03%
Beta	2450	Head	07/10/2025	22.7	21.3	17	1112	7859	1905	2.420	50.600	48.285	-4.57%	1.140	23.700	22.746	-4.03%
Gamma	2600	Head	06/23/2025	23.1	21.9	17	1215	7836	1839	2.570	55.300	51.278	-7.27%	1.160	24.900	23.145	-7.05%
Gamma	5250	Head	06/17/2025	22.9	21.9	17	1396	7836	1839	3.760	77.900	75.022	-3.69%	1.080	22.400	21.549	-3.80%
Gamma	5250	Head	06/23/2025	23.1	21.9	17	1396	7836	1839	3.800	77.900	75.820	-2.67%	1.090	22.400	21.748	-2.91%
Gamma	5250	Head	07/08/2025	22.2	22.4	17	1396	7836	1839	3.670	77.900	73.226	-6.00%	1.040	22.400	20.751	-7.36%
Gamma	5250	Head	07/10/2025	22.7	22	17	1396	7836	1839	3.820	77.900	76.219	-2.16%	1.100	22.400	21.948	-2.02%
Gamma	5600	Head	06/17/2025	22.9	21.9	17	1396	7836	1839	4.050	81.100	80.808	-0.36%	1.150	23.300	22.946	-1.52%
Gamma	5600	Head	06/23/2025	23.1	21.9	17	1396	7836	1839	4.100	81.100	81.806	0.87%	1.170	23.300	23.345	0.19%
Gamma	5600	Head	07/10/2025	22.7	22	17	1396	7836	1839	4.130	81.100	82.404	1.61%	1.170	23.300	23.345	0.19%
Gamma	5750	Head	06/17/2025	22.9	21.9	17	1396	7836	1839	3.750	80.100	74.822	-6.59%	1.070	22.800	21.349	-6.36%
Gamma	5750	Head	06/23/2025	23.1	21.9	17	1396	7836	1839	3.800	80.100	75.820	-5.34%	1.090	22.800	21.748	-4.61%
Gamma	5750	Head	07/10/2025	22.7	22	17	1396	7836	1839	3.840	80.100	76.618	-4.35%	1.090	22.800	21.748	-4.61%

B.2. Dielectric Parameters of the TSL

Table 2 SAR Tissue Dielectric Parameters

Date	Tissue Type	Liquid Temp (°C)	Frequency (MHz)	Conductivity Measured (σ)	Conductivity Target (σ)	Deviation	Permittivity measured (εr)	Permittivity Target (εr)	Deviation
6/16/2025	Head	22.2	2300	1.70	1.67	2.27%	39.2	39.5	-0.69%
6/16/2025	Head	22.2	2310	1.71	1.68	2.19%	39.2	39.4	-0.56%
6/16/2025	Head	22.2	2320	1.72	1.68	2.13%	39.2	39.4	-0.64%
6/16/2025	Head	22.2	2350	1.74	1.71	1.76%	39.1	39.4	-0.62%
6/16/2025	Head	22.2	2400	1.78	1.76	1.44%	39.0	39.3	-0.61%
6/16/2025	Head	22.2	2450	1.82	1.80	1.03%	39.0	39.2	-0.60%
6/16/2025	Head	22.2	2480	1.84	1.83	0.54%	38.9	39.2	-0.67%
6/17/2025	Head	21.9	5150	4.38	4.60	-4.91%	34.3	36.0	-4.78%
6/17/2025	Head	21.9	5200	4.43	4.66	-4.82%	34.2	36.0	-4.85%
6/17/2025	Head	21.9	5250	4.49	4.71	-4.68%	34.1	35.9	-4.99%
6/17/2025	Head	21.9	5300	4.54	4.76	-4.65%	34.1	35.9	-5.03%
6/17/2025	Head	21.9	5350	4.59	4.81	-4.46%	34.0	35.8	-5.19%
6/17/2025	Head	21.9	5500	4.75	4.96	-4.34%	33.7	35.6	-5.38%
6/17/2025	Head	21.9	5550	4.81	5.01	-4.15%	33.6	35.6	-5.49%
6/17/2025	Head	21.9	5600	4.86	5.07	-4.04%	33.5	35.5	-5.57%
6/17/2025	Head	21.9	5650	4.92	5.12	-3.86%	33.5	35.5	-5.68%
6/17/2025	Head	21.9	5700	4.98	5.17	-3.71%	33.4	35.4	-5.76%
6/17/2025	Head	21.9	5750	5.03	5.22	-3.60%	33.3	35.4	-5.82%
6/17/2025	Head	21.9	5800	5.09	5.27	-3.41%	33.2	35.3	-5.98%
6/17/2025	Head	21.9	5850	5.14	5.32	-3.41%	33.1	35.3	-6.01%
6/17/2025	Head	21.9	5900	5.20	5.38	-3.31%	33.0	35.2	-6.16%
6/17/2025	Head	21.9	5985	5.29	5.46	-3.14%	32.9	35.1	-6.30%
6/18/2025	Head	22.4	680	0.87	0.89	-1.20%	40.6	42.3	-3.90%
6/18/2025	Head	22.4	695	0.88	0.89	-0.80%	40.6	42.2	-3.85%
6/18/2025	Head	22.4	700	0.88	0.89	-0.95%	40.5	42.2	-3.92%
6/18/2025	Head	22.4	710	0.88	0.89	-0.28%	40.5	42.1	-3.82%
6/18/2025	Head	22.4	750	0.90	0.89	0.52%	40.4	41.9	-3.69%
6/18/2025	Head	22.4	770	0.90	0.89	1.20%	40.4	41.8	-3.48%
6/18/2025	Head	22.4	785	0.91	0.89	1.56%	40.3	41.7	-3.43%
6/18/2025	Head	22.4	800	0.91	0.90	1.69%	40.2	41.7	-3.45%
6/18/2025	Head	22.4	815	0.92	0.90	2.56%	40.2	41.6	-3.36%
6/18/2025	Head	22.4	835	0.93	0.90	3.03%	40.2	41.5	-3.25%
6/18/2025	Head	22.4	850	0.93	0.92	1.62%	40.1	41.5	-3.31%
6/18/2025	Head	22.4	875	0.94	0.94	-0.06%	40.0	41.5	-3.51%
6/18/2025	Head	22.4	900	0.95	0.97	-1.97%	40.0	41.5	-3.70%
6/18/2025	Head	22.4	935	0.96	0.99	-2.52%	39.9	41.5	-3.76%
6/20/2025	Head	22.1	890	0.91	0.90	1.29%	41.6	41.7	-0.28%
6/20/2025	Head	22.1	815	0.92	0.90	1.95%	41.5	41.6	-0.18%
6/20/2025	Head	22.1	835	0.92	0.90	2.41%	41.5	41.5	-0.07%
6/20/2025	Head	22.1	850	0.93	0.92	1.05%	41.4	41.5	-0.16%
6/20/2025	Head	22.1	875	0.94	0.94	-0.51%	41.3	41.5	-0.39%
6/23/2025	Head	22.2	1710	1.33	1.35	-1.64%	39.2	40.1	-2.33%
6/23/2025	Head	22.2	1750	1.35	1.37	-1.36%	39.2	40.1	-2.31%
6/23/2025	Head	22.2	1790	1.38	1.39	-1.33%	39.1	40.0	-2.29%
6/23/2025	Head	22.3	5150	4.33	4.60	-5.92%	33.8	36.0	-6.32%
6/23/2025	Head	22.3	5200	4.38	4.66	-5.81%	33.7	36.0	-6.41%
6/23/2025	Head	22.3	5250	4.44	4.71	-5.70%	33.6	35.9	-6.54%
6/23/2025	Head	22.3	5300	4.49	4.76	-5.66%	33.5	35.9	-6.60%
6/23/2025	Head	22.3	5350	4.54	4.81	-5.55%	33.4	35.8	-6.76%
6/23/2025	Head	22.3	5500	4.69	4.96	-5.41%	33.2	35.6	-6.96%
6/23/2025	Head	22.3	5550	4.75	5.01	-5.28%	33.1	35.6	-7.08%
6/23/2025	Head	22.3	5600	4.80	5.07	-5.15%	33.0	35.5	-7.15%
6/23/2025	Head	22.3	5650	4.86	5.12	-4.99%	32.9	35.5	-7.29%
6/23/2025	Head	22.3	5700	4.92	5.17	-4.88%	32.8	35.4	-7.37%
6/23/2025	Head	22.3	5750	4.97	5.22	-4.78%	32.7	35.4	-7.44%
6/23/2025	Head	22.3	5800	5.03	5.27	-4.63%	32.6	35.3	-7.56%
6/23/2025	Head	22.3	5850	5.08	5.32	-4.64%	32.6	35.3	-7.65%
6/23/2025	Head	22.3	5900	5.13	5.38	-4.55%	32.5	35.2	-7.77%
6/23/2025	Head	22.3	5985	5.22	5.46	-4.41%	32.3	35.1	-7.93%
6/23/2025	Head	21.9	2500	1.85	1.85	-0.15%	38.2	39.1	-2.27%
6/23/2025	Head	21.9	2550	1.89	1.91	-1.13%	38.2	39.1	-2.32%
6/23/2025	Head	21.9	2600	1.93	1.96	-1.75%	38.1	39.0	-2.32%
6/23/2025	Head	21.9	2650	1.97	2.02	-2.56%	38.0	38.9	-2.43%
6/23/2025	Head	21.9	2680	1.99	2.05	-2.72%	38.0	38.9	-2.42%
6/23/2025	Head	21.9	2700	2.01	2.07	-3.12%	37.9	38.9	-2.45%
6/25/2025	Head	21.9	1850	1.43	1.40	1.85%	39.3	40.0	-1.81%
6/25/2025	Head	21.9	1880	1.44	1.40	3.04%	39.3	40.0	-1.86%
6/25/2025	Head	21.9	1900	1.45	1.40	3.76%	39.2	40.0	-1.95%
6/25/2025	Head	21.9	1920	1.47	1.40	4.71%	39.2	40.0	-2.05%
6/25/2025	Head	21.9	1950	1.49	1.40	6.28%	39.1	40.0	-2.13%
6/26/2025	Head	22.5	12	0.69	0.75	-7.91%	53.7	55.0	-2.32%
6/26/2025	Head	22.5	13	0.69	0.75	-7.89%	53.4	55.0	-2.90%
6/26/2025	Head	22.5	14	0.69	0.75	-7.67%	53.0	55.0	-3.58%
6/27/2025	Head	23.1	1710	1.33	1.35	-1.40%	38.6	40.1	-3.86%
6/27/2025	Head	23.1	1750	1.35	1.37	-1.44%	38.5	40.1	-3.88%
6/27/2025	Head	23.1	1790	1.37	1.39	-1.51%	38.5	40.0	-3.87%
6/27/2025	Head	23.1	815	0.94	0.90	4.36%	40.9	41.6	-1.58%
6/27/2025	Head	23.1	835	0.94	0.90	4.88%	40.9	41.5	-1.47%
6/27/2025	Head	23.1	850	0.95	0.92	3.52%	40.9	41.5	-1.56%
6/27/2025	Head	23.1	1850	1.41	1.40	0.92%	38.8	40.0	-2.95%
6/27/2025	Head	23.1	1880	1.43	1.40	2.06%	38.8	40.0	-2.97%
6/27/2025	Head	23.1	1900	1.44	1.40	2.80%	38.8	40.0	-3.03%
6/27/2025	Head	23.1	1920	1.45	1.40	3.70%	38.8	40.0	-3.12%
7/1/2025	Head	22.7	680	0.87	0.89	-1.19%	40.5	42.3	-4.14%
7/1/2025	Head	22.7	695	0.88	0.89	-0.72%	40.5	42.2	-4.09%
7/1/2025	Head	22.7	700	0.88	0.89	-0.85%	40.4	42.2	-4.15%
7/1/2025	Head	22.7	710	0.89	0.89	-0.16%	40.4	42.1	-4.03%
7/1/2025	Head	22.7	750	0.90	0.89	0.60%	40.3	41.9	-3.91%
7/1/2025	Head	22.7	770	0.90	0.89	1.30%	40.2	41.8	-3.74%
7/1/2025	Head	22.7	785	0.91	0.89	1.67%	40.2	41.7	-3.69%
7/1/2025	Head	22.7	800	0.92	0.90	2.01%	40.2	41.7	-3.67%
7/8/2025	Head	22.4	5150	4.26	4.60	-5.20%	34.3	36.0	-4.91%
7/8/2025	Head	22.4	5200	4.42	4.65	-5.07%	34.2	36.0	-4.98%
7/8/2025	Head	22.4	5250	4.47	4.71	-4.95%	34.1	35.9	-5.11%
7/8/2025	Head	22.4	5300	4.53	4.76	-4.89%	34.0	35.9	-5.16%
7/8/2025	Head	22.4	5350	4.58	4.81	-4.75%	33.9	35.8	-5.33%
7/10/2025	Head	21.3	2400	1.76	1.76	0.21%	38.6	39.3	-1.85%
7/10/2025	Head	21.3	2450	1.79	1.80	-0.36%	38.5	39.2	-1.85%
7/10/2025	Head	21.3	2480	1.82	1.83	-0.86%	38.4	39.2	-1.92%
7/10/2025	Head	21.3	2500	1.83	1.85	-1.19%	38.4	39.1	-1.93%
7/10/2025	Head	21.3	2550	1.87	1.91	-2.23%	38.3	39.1	-1.96%
7/10/2025	Head	21.3	2600	1.91	1.96	-2.73%	38.3	39.0	-1.94%
7/10/2025	Head	22.0	5150	4.42	4.60	-3.95%	35.1	36.0	-2.51%
7/10/2025	Head	22.0	5200	4.49	4.66	-3.56%	35.0	36.0	-2.64%
7/10/2025	Head	22.0	5250	4.54	4.71	-3.53%	35.0	35.9	-2.71%
7/10/2025	Head	22.0	5300	4.60	4.76	-3.40%	34.8	35.9	-2.93%
7/10/2025	Head	22.0	5350	4.64	4.81	-3.54%	34.7	35.8	-3.05%
7/10/2025	Head	22.0	5500	4.81	4.96	-3.04%	34.5	35.6	-3.18%
7/10/2025	Head	22.0	5550	4.86	5.01	-3.10%	34.4	35.6	-3.33%
7/10/2025	Head	22.0	5600	4.93	5.07	-2.70%	34.3	35.5	-3.41%
7/10/2025	Head	22.0	5650	4.97	5.12	-2.77%	34.2	35.5	-3.60%
7/10/2025	Head	22.0	5700	5.04	5.17	-2.38%	34.1	35.4	-3.65%
7/10/2025	Head	22.0	5750	5.09	5.22	-2.54%	34.0	35.4	-3.81%
7/10/2025	Head	22.0	5800	5.16	5.27	-2.12%	33.9	35.3	-3.83%
7/10/2025	Head	22.0	5850	5.20	5.32	-2.32%	33.8	35.3	-4.01%

The above measured tissue parameters were used in the DASY software. The DASY software was used to perform interpolation to determine the dielectric parameters at the SAR test device frequencies (per KDB Publication 865664 D01v01r04 and IEEE 1528-2013 6.6.1.2). The tissue parameters listed in the SAR test plots may slightly differ from the table above due to significant digit rounding in the software.

The SAR values were compensated for deviations between the measured and required tissue dielectric properties, as described in IEEE 1528-2013. The SAR values were applied to only scale up the measured SAR values, and not downward, per KDB Publication 865664 D01v04r04.

B.3. System Validation

Per FCC KDB Publication 865664 D02 Section 2.3 a) states “SAR system validation status and system verification results should be documented in a separate section of the SAR report, or as an attachment, to confirm measurement accuracy.”

The SAR systems used for evaluating this device were validated against its performance specifications prior to the SAR measurements.

Reference dipoles were used with the required tissue-equivalent media for system validation, according to the procedures outlined in FCC KDB Publication 865664 D01 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point.

Per FCC KDB 865664 D02, “the validation status should be documented according to the validation date(s), measurement frequencies, SAR probes, calibrated signal type(s) and tissue dielectric parameters.” A tabulated summary of the system validation status is provided accordingly:

Table 3 System Validation

System	Frequency (MHz)	Date	Probe	DAE	Probe CalF		Cond. (σ)	Perm (ϵ_r)	CW Validation			Mod Validation		
					Freq (MHz)	Tissue Type			Sensitivity	Probe Linearity	Probe Isotropy	Mod Type	Duty Factor	PAR
Gamma	13	11/26/2024	7836	1839	13	Head	0.703	54.138	PASS	PASS	PASS	N/A	N/A	N/A
Delta	750	11/18/2024	7853	1844	750	Head	0.906	43.8	PASS	PASS	PASS	N/A	N/A	N/A
Delta	835	11/18/2024	7853	1844	835	Head	0.936	43.6	PASS	PASS	PASS	GMSK	PASS	N/A
Gamma	835	11/20/2024	7836	1839	835	Head	0.938	41.455	PASS	PASS	PASS	GMSK	PASS	N/A
Delta	1750	06/23/2025	7857	1844	1750	Head	1.35	39.153	PASS	PASS	PASS	N/A	N/A	N/A
Delta	1900	06/23/2025	7857	1844	1900	Head	1.44	38.91	PASS	PASS	PASS	GMSK	PASS	N/A
Gamma	1900	11/19/2024	7836	1839	1900	Head	1.448	39.323	PASS	PASS	PASS	GMSK	PASS	N/A
Gamma	2450	11/21/2024	7836	1839	2450	Head	1.824	38.955	PASS	PASS	PASS	OFDM	N/A	PASS
Beta	2450	05/21/2025	7859	1905	2450	Head	1.72	37.8	PASS	PASS	PASS	OFDM	N/A	PASS
Gamma	2600	11/21/2024	7836	1839	2600	Head	1.945	38.718	PASS	PASS	PASS	TDD	PASS	N/A
Gamma	5250	11/21/2024	7836	1839	5250	Head	4.494	34.126	PASS	PASS	PASS	OFDM	N/A	PASS
Gamma	5600	11/22/2024	7836	1839	5600	Head	4.866	33.528	PASS	PASS	PASS	OFDM	N/A	PASS
Gamma	5750	11/22/2024	7836	1839	5750	Head	5.038	33.263	PASS	PASS	PASS	OFDM	N/A	PASS

NOTE: The probes have been calibrated for both CW and modulated signals. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01 for scenarios when CW probe calibrations are used with other signal types.

SAR systems were additionally validated for modulated signals with a periodic duty cycle or with a high PAR (peak to average ratio) >5 dB, such as OFDM according to FCC KDB Publication 865664 D01 v01r04.

B.4. Sample TSL Compositions

TSL recipes are proprietary to SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer data sheets are provided below.

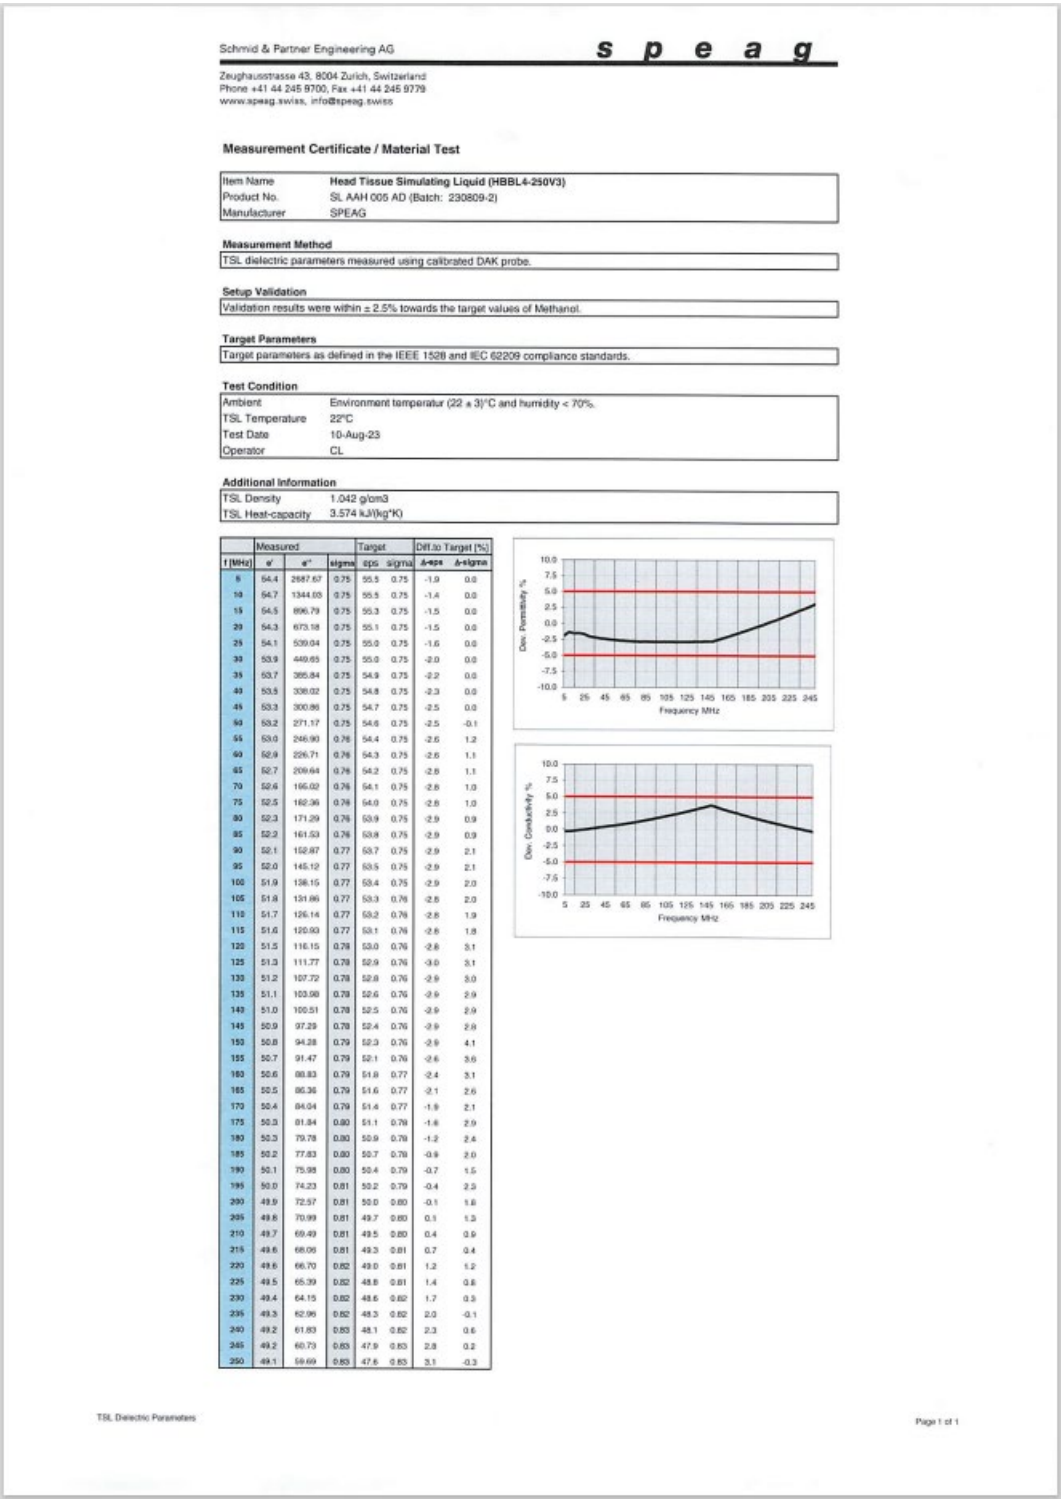


Figure 1 - Head TSL Calibration Certificate Example (4 – 250 MHz)

Measurement Certificate / Material Test

Item Name Head Tissue Simulating Liquid (HBL600-10000V6)
Product No. SL AAH U16 BC (Batch: 230912-5)
Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated DAK probe.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient Condition 22°C ; 30% humidity

TSL Temperature 22°C

Test Date 14-Sep-23

Operator CL



Additional Information

TSL Density

TSL Heat-capacity

Results

f [MHz]	Measured			Target		Diff. to Target [%]	
	e'	e''	sigma	eps	sigma	Δ-eps	Δ-sigma
600	44.7	25.6	0.86	42.7	0.88	4.6	-2.5
750	44.2	21.7	0.90	41.9	0.89	5.4	0.7
800	44.0	20.7	0.92	41.7	0.90	5.6	2.5
825	44.0	20.3	0.93	41.6	0.91	5.8	2.6
835	44.0	20.1	0.94	41.5	0.91	5.9	3.1
850	43.9	19.9	0.94	41.5	0.92	5.8	2.6
900	43.8	19.2	0.96	41.5	0.97	5.5	-1.0
1400	42.8	15.2	1.18	40.6	1.18	5.4	0.0
1450	42.7	15.0	1.21	40.5	1.20	5.4	0.8
1600	42.4	14.4	1.29	40.3	1.28	5.2	0.4
1625	42.4	14.4	1.30	40.3	1.30	5.3	0.1
1640	42.4	14.3	1.31	40.3	1.31	5.3	0.3
1650	42.4	14.3	1.31	40.2	1.31	5.4	-0.2
1700	42.3	14.2	1.34	40.2	1.34	5.3	-0.2
1750	42.2	14.1	1.37	40.1	1.37	5.3	-0.1
1800	42.1	14.0	1.40	40.0	1.40	5.3	0.0
1810	42.1	13.9	1.41	40.0	1.40	5.3	0.7
1825	42.1	13.9	1.42	40.0	1.40	5.3	1.4
1850	42.1	13.9	1.43	40.0	1.40	5.3	2.1
1900	42.0	13.8	1.46	40.0	1.40	5.0	4.3
1950	41.9	13.7	1.49	40.0	1.40	4.7	6.4
2000	41.8	13.7	1.52	40.0	1.40	4.5	8.6
2050	41.8	13.6	1.55	39.9	1.44	4.7	7.3
2100	41.7	13.6	1.59	39.8	1.49	4.7	6.8
2150	41.6	13.6	1.62	39.7	1.53	4.7	5.7
2200	41.6	13.5	1.66	39.6	1.58	4.9	5.2
2250	41.5	13.5	1.69	39.6	1.62	4.9	4.2
2300	41.4	13.5	1.73	39.5	1.67	4.9	3.8
2350	41.4	13.5	1.77	39.4	1.71	5.1	3.4
2400	41.3	13.6	1.81	39.3	1.76	5.1	3.1
2450	41.2	13.6	1.85	39.2	1.80	5.1	2.8
2500	41.2	13.6	1.89	39.1	1.85	5.3	1.9
2550	41.1	13.6	1.93	39.1	1.91	5.2	1.1
2600	41.0	13.6	1.97	39.0	1.96	5.1	0.3

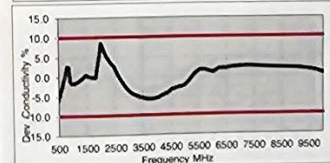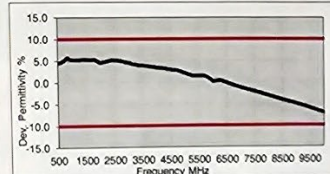

3500	39.4	14.1	2.75	37.9	2.91	3.9	-5.5
3700	39.1	14.3	2.94	37.7	3.12	3.7	-5.8
5200	36.6	16.0	4.62	36.0	4.66	1.7	-0.8
5250	36.5	16.1	4.69	35.9	4.71	1.6	-0.3
5300	36.4	16.2	4.78	35.9	4.78	1.5	0.1
5500	36.2	16.4	5.03	35.6	4.96	1.5	1.3
5600	36.1	16.5	5.14	35.5	5.07	1.5	1.5
5700	35.9	16.5	5.25	35.4	5.17	1.2	1.4
5800	35.7	16.6	5.34	35.3	5.27	1.2	1.4
6000	35.1	16.5	5.52	35.1	5.48	0.2	0.9
6500	34.4	17.1	6.19	34.5	6.07	-0.1	1.9
7000	33.5	17.5	6.81	33.9	6.65	-1.3	2.4
7500	32.6	17.8	7.41	33.3	7.24	-2.1	2.4
8000	31.7	18.0	8.01	32.7	7.84	-3.1	2.2
8500	30.8	18.2	8.62	32.1	8.45	-4.1	2.0
9000	30.0	18.5	9.24	31.5	9.08	-4.9	1.9
9500	29.1	18.8	9.85	31.0	9.71	-5.9	1.4
10000	28.2	18.7	10.41	30.4	10.36	-7.0	0.5

TSL Dielectric Parameters

Figure 2 - Head TSL Calibration Certificate Example (600 – 10000 MHz)