

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	17.89, 16.89,18.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-26	22.9	22.5	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.691	53.4	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.126	-2.17
psSAR10g	0.077	-7.70
Peak SAR (Extrapolated)	0.245	-7.75
psAPD (4.0 cm², sq)	N/A	N/A

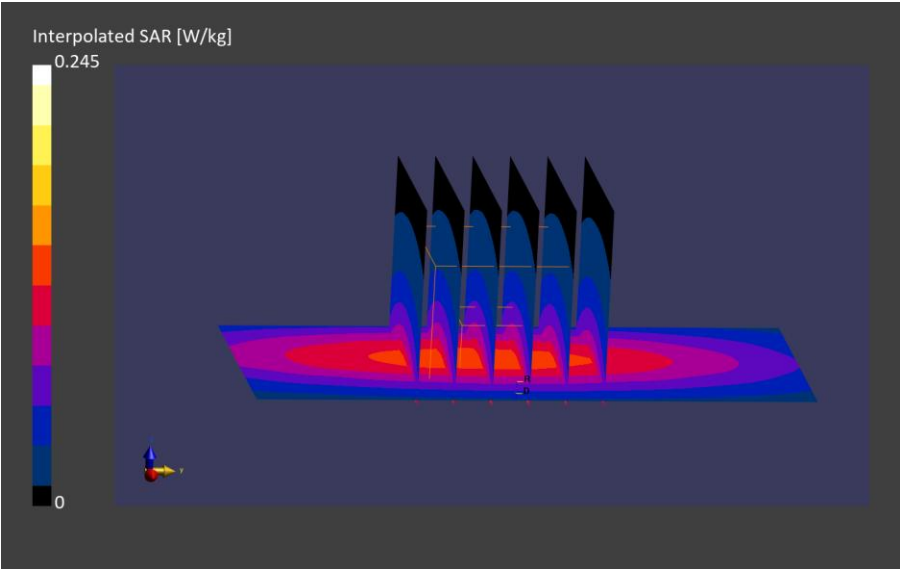

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-18	22.5	22.7	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.898	40.4	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.419	-3.8
psSAR10g	0.274	-3.92
Peak SAR (Extrapolated)	0.668	5.78
psAPD (4.0 cm², sq)	N/A	N/A

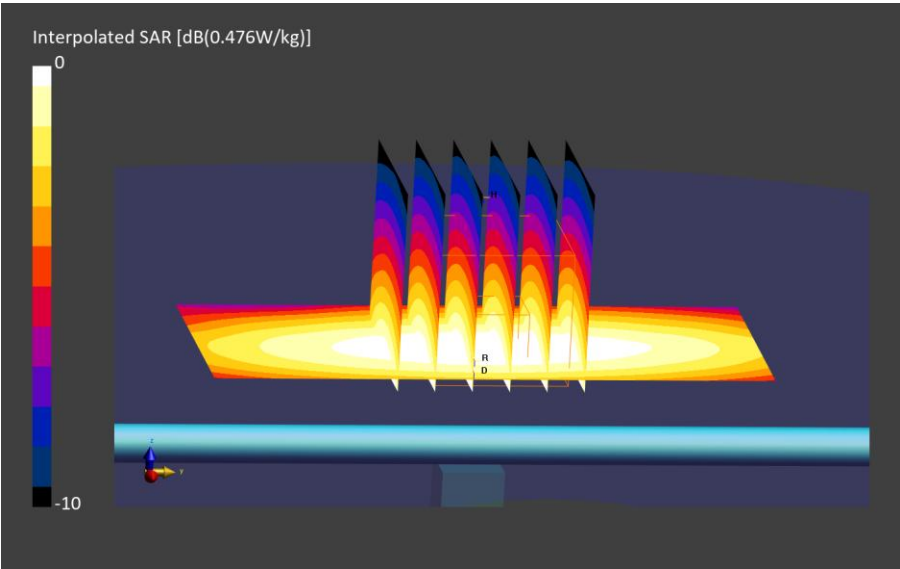

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-01	23.5	22.7	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.899	40.3	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.413	-5.17
psSAR10g	0.270	-5.32
Peak SAR (Extrapolated)	0.635	0.55
psAPD (4.0 cm², sq)	N/A	N/A

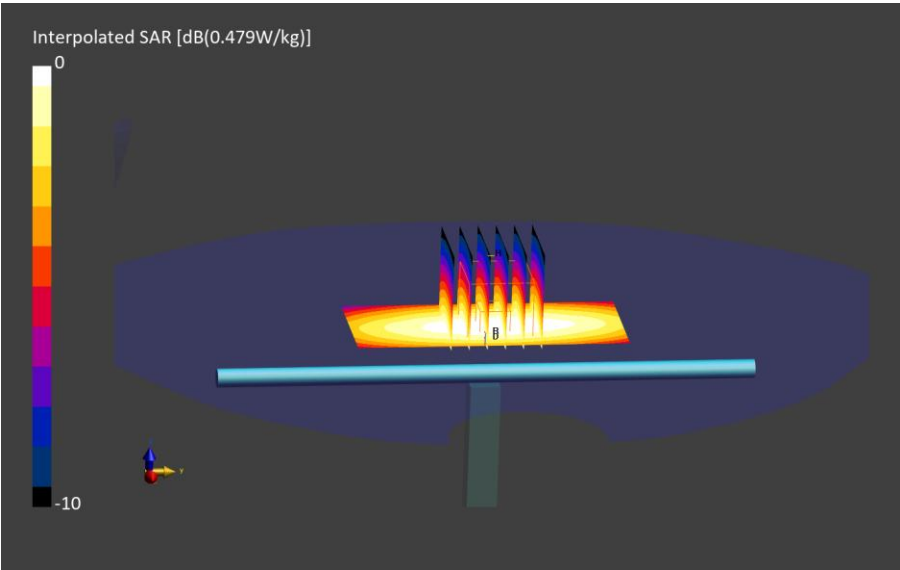

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.21, 8.83, 8.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-18	22.5	22.7	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.927	40.2	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.499	1.39
psSAR10g	0.324	1.49
Peak SAR (Extrapolated)	0.767	8.54
psAPD (4.0 cm², sq)	N/A	N/A

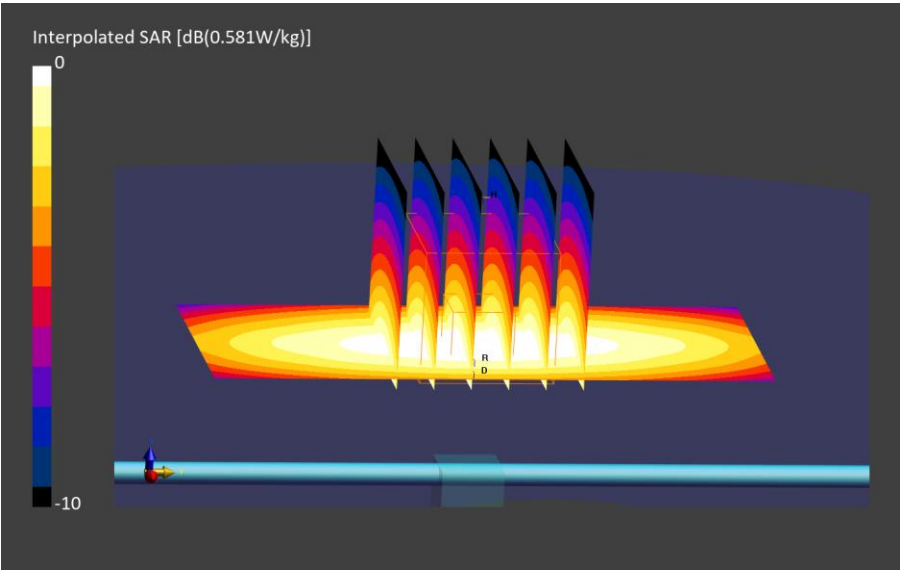

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.21, 8.83,8.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-20	22.9	22.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.922	41.5	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.495	0.58
psSAR10g	0.323	1.17
Peak SAR (Extrapolated)	0.780	10.38
psAPD (4.0 cm², sq)	N/A	N/A

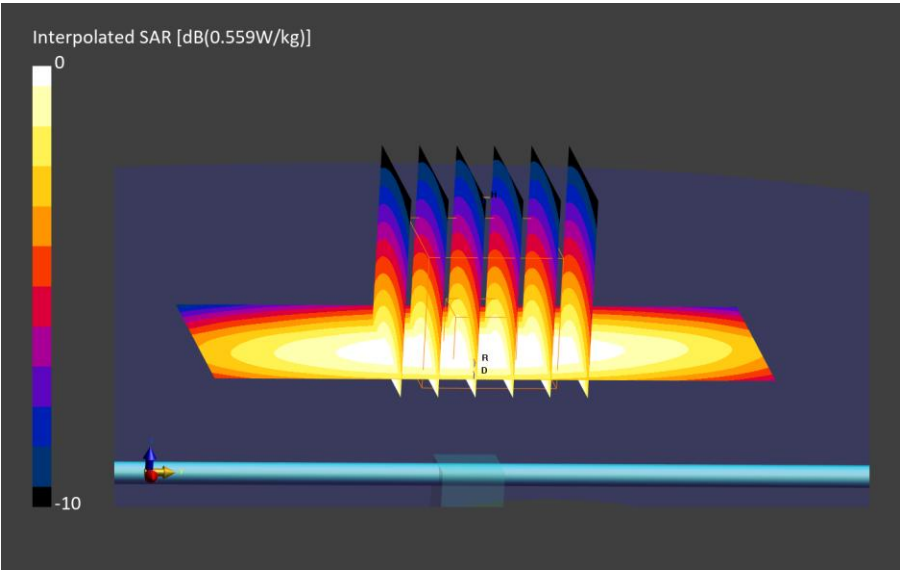

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	8.85, 8.65,9.28

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-27	22.5	23.1	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.944	40.9	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.518	5.25
psSAR10g	0.338	5.87
Peak SAR (Extrapolated)	0.785	11.08
psAPD (4.0 cm², sq)	N/A	N/A

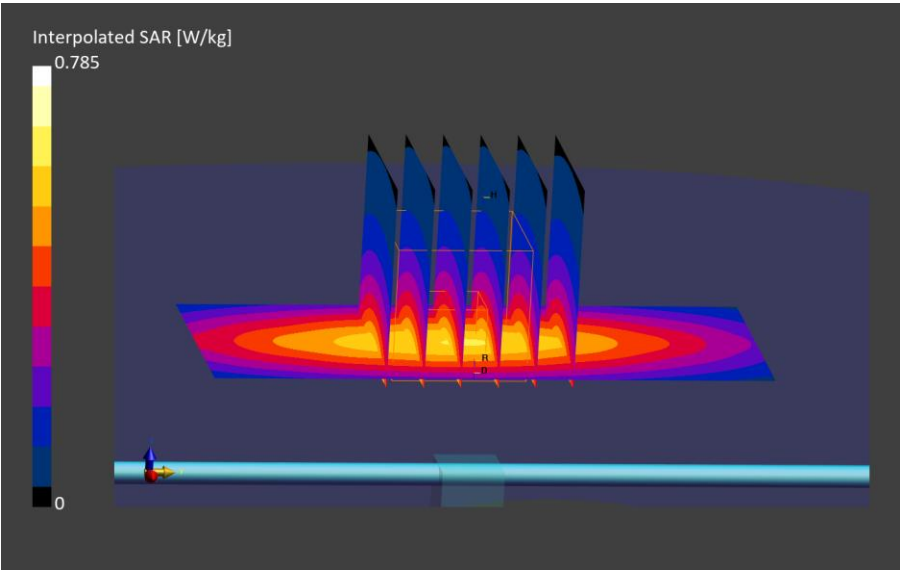

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.09, 7.69, 7.42

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-23	23.1	22.2	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.35	39.2	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.90	3.86
psSAR10g	1.01	4.96
Peak SAR (Extrapolated)	3.49	7.3
psAPD (4.0 cm², sq)	N/A	N/A

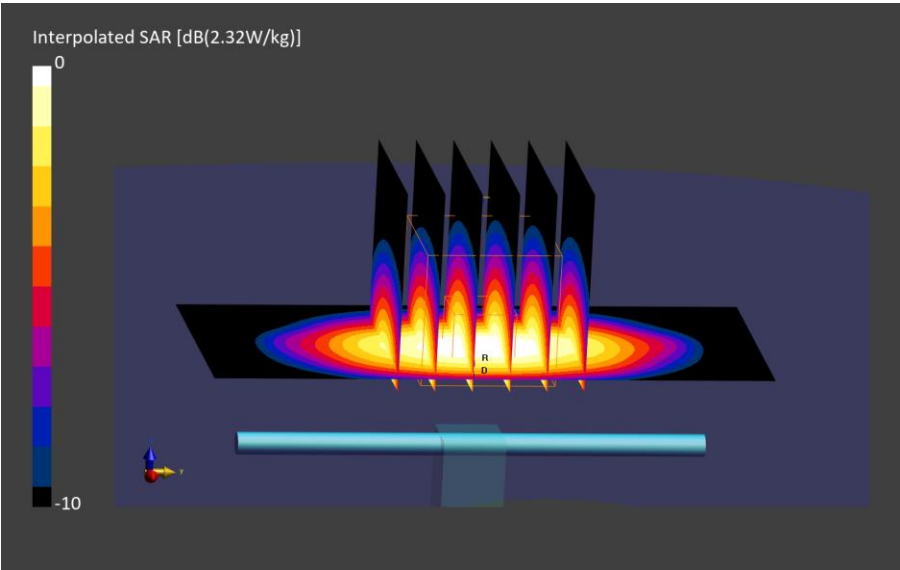

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.09, 7.69, 7.42

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-27	22.5	23.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.35	38.5	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.76	-3.79
psSAR10g	0.938	-2.52
Peak SAR (Extrapolated)	3.24	-0.39
psAPD (4.0 cm², sq)	N/A	N/A

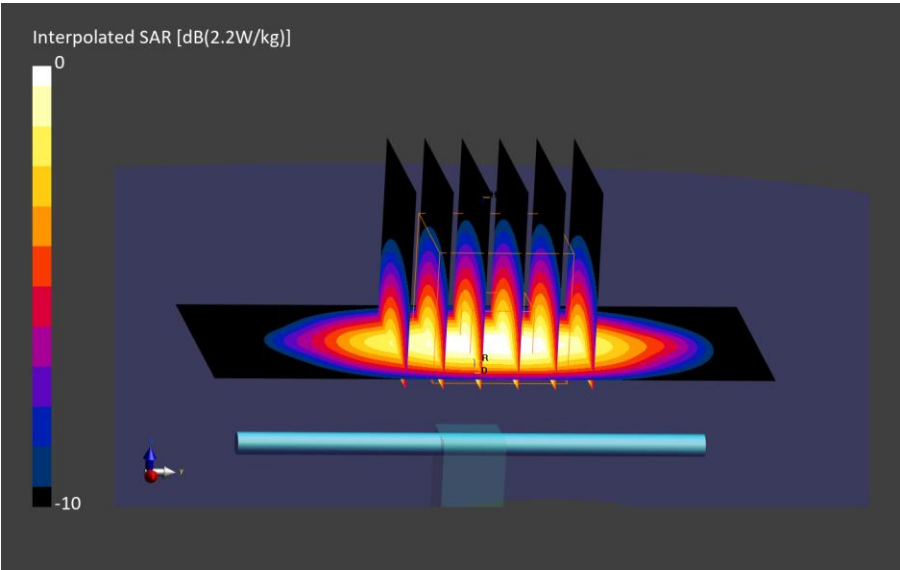

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	6.86, 7.44, 7.18

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-25	22.7	21.9	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.45	39.2	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.03	1.77
psSAR10g	1.05	-0.24
Peak SAR (Extrapolated)	3.80	5.16
psAPD (4.0 cm², sq)	N/A	N/A

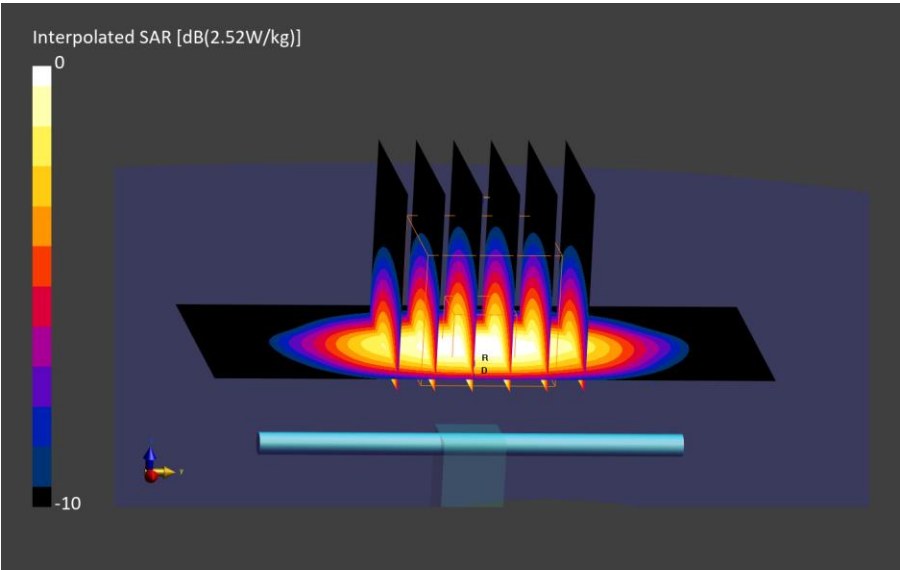

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.4, 7.24,7.76

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-27	22.5	23.1	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.44	38.8	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.98	-0.74
psSAR10g	1.04	-1.19
Peak SAR (Extrapolated)	3.57	-1.21
psAPD (4.0 cm², sq)	N/A	N/A

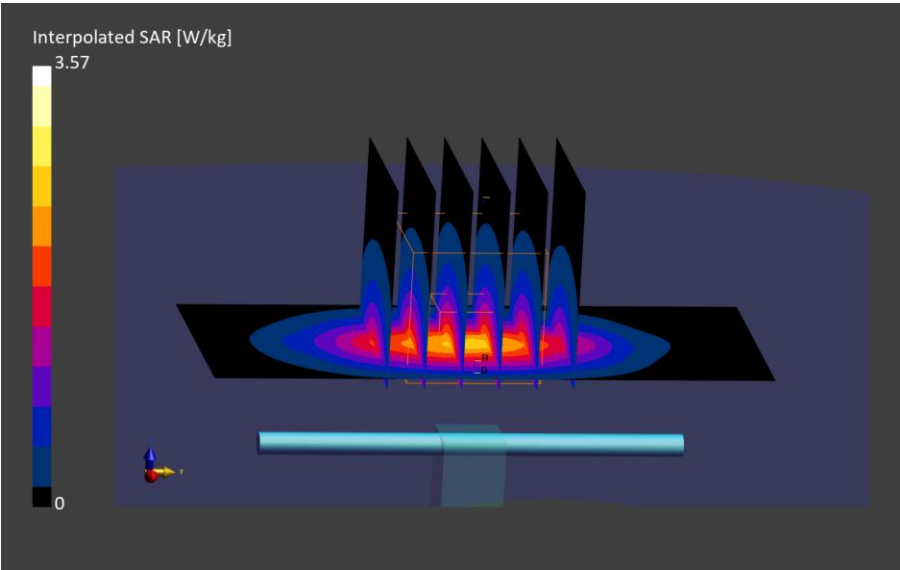

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.02, 6.86, 7.36

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-16	23.3	22.2	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.82	39.0	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.43	-4.18
psSAR10g	1.14	-4.03
Peak SAR (Extrapolated)	4.76	-8.85
psAPD (4.0 cm², sq)	N/A	N/A

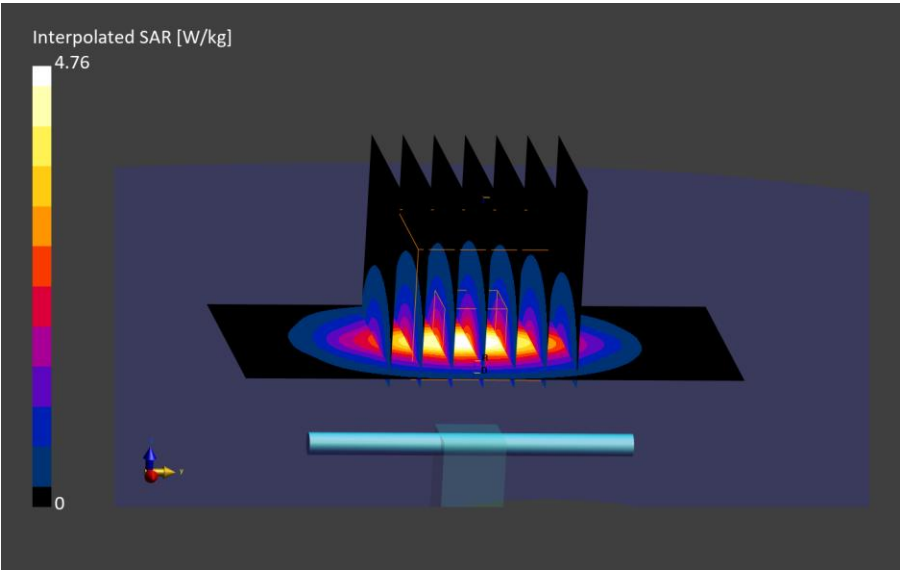

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.72, 7.08,6.68

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-10	22.7	21.3	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.79	38.5	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.42	-4.57
psSAR10g	1.14	-4.03
Peak SAR (Extrapolated)	4.74	-9.24
psAPD (4.0 cm², sq)	N/A	N/A

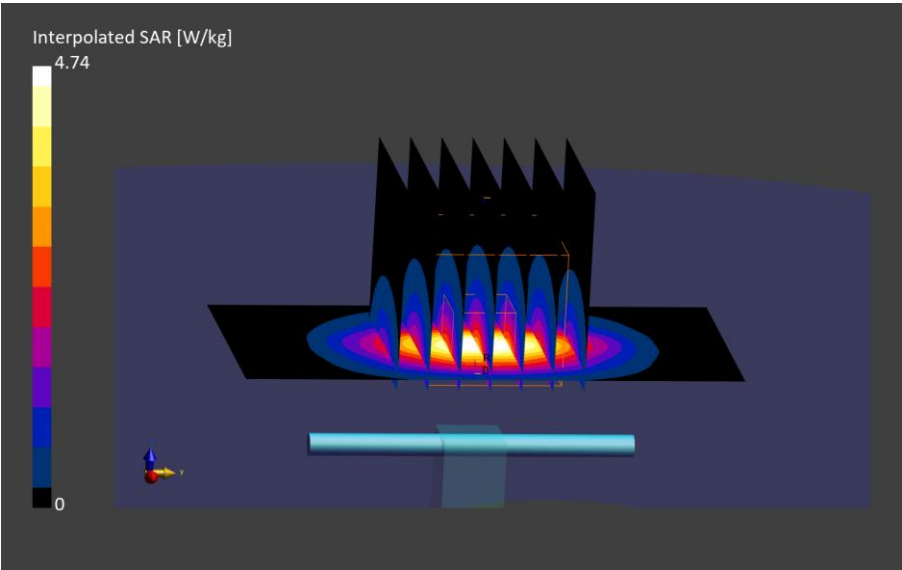

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	7.09, 6.93, 7.44

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-23	23.1	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.93	38.1	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.57	-7.27
psSAR10g	1.16	-7.05
Peak SAR (Extrapolated)	5.20	-12.15
psAPD (4.0 cm², sq)	N/A	N/A

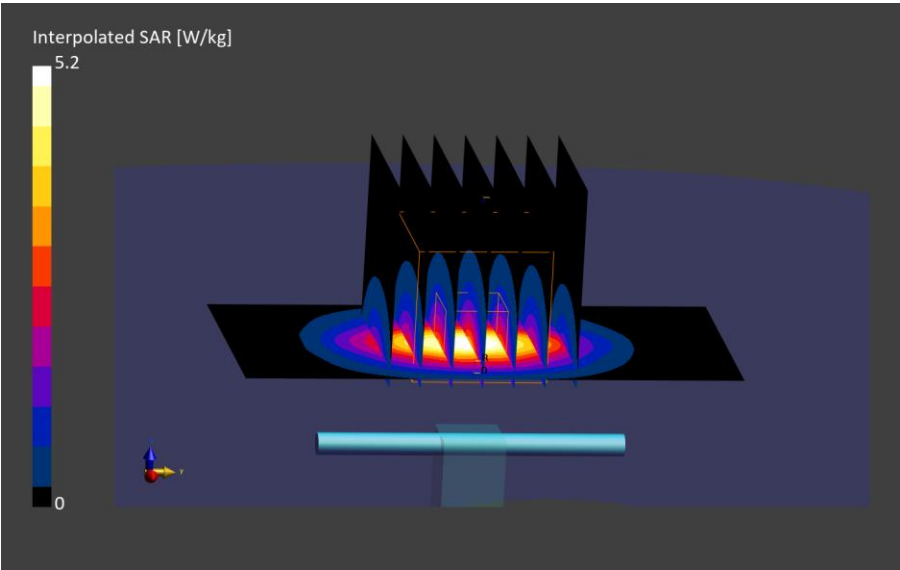

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHZV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.28, 5.16, 5.54

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-17	22.9	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.49	34.1	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 36.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.76	-3.69
psSAR10g	1.08	-3.8
Peak SAR (Extrapolated)	14.8	-4.8
psAPD (4.0 cm², sq)	N/A	N/A

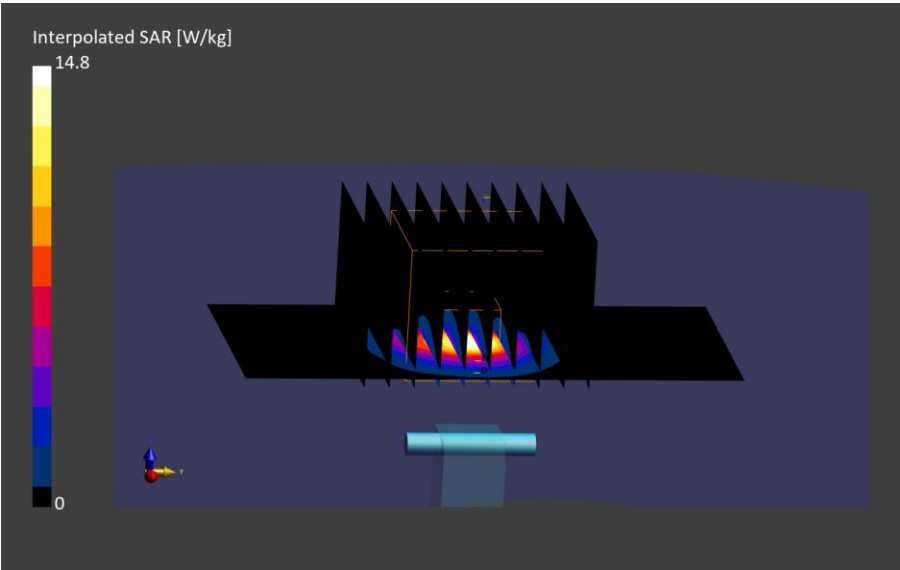

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.28, 5.16, 5.54

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-23	23.1	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.44	33.6	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.80	-2.67
psSAR10g	1.09	-2.91
Peak SAR (Extrapolated)	15.0	-3.52
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.28, 5.16, 5.54

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-08	22.2	22.4	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.47	34.1	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.67	-6
psSAR10g	1.04	-7.36
Peak SAR (Extrapolated)	14.6	-6.09
psAPD (4.0 cm², sq)	N/A	N/A

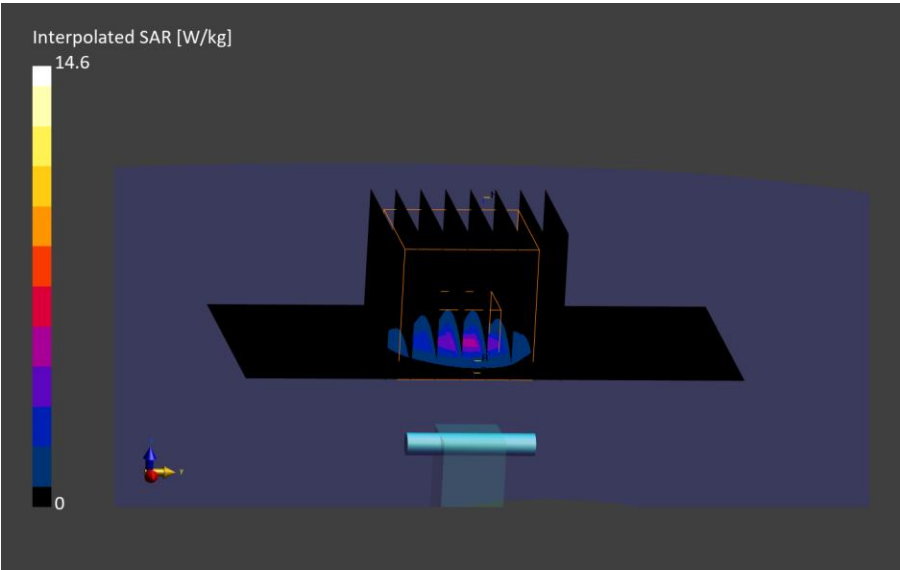

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHZV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.28, 5.16, 5.54

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-10	22.7	22	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.54	35.0	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.82	-2.16
psSAR10g	1.10	-2.02
Peak SAR (Extrapolated)	15.2	-2.23
psAPD (4.0 cm², sq)	N/A	N/A

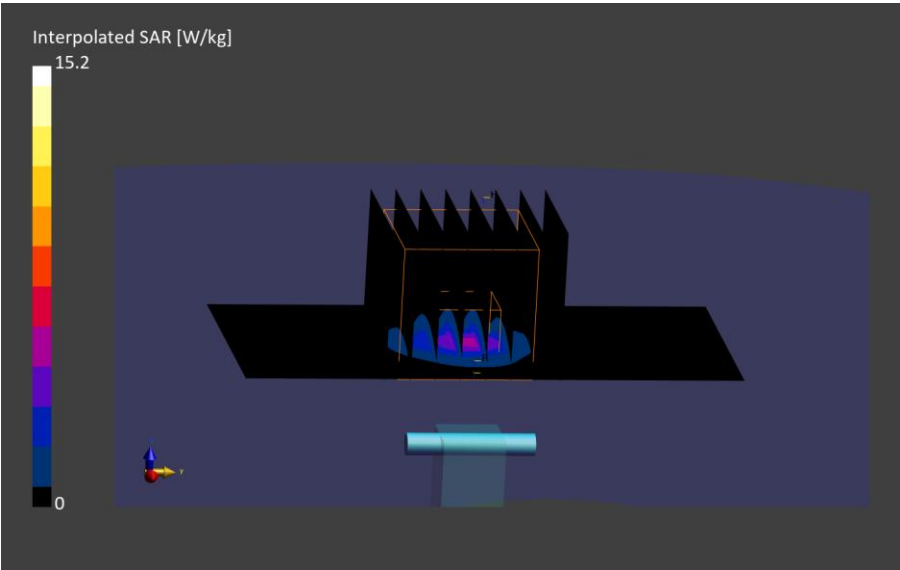

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	4.81, 4.7,5.04

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-17	22.9	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.86	33.5	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 36.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.05	-0.36
psSAR10g	1.15	-1.52
Peak SAR (Extrapolated)	17.3	1.58
psAPD (4.0 cm², sq)	N/A	N/A

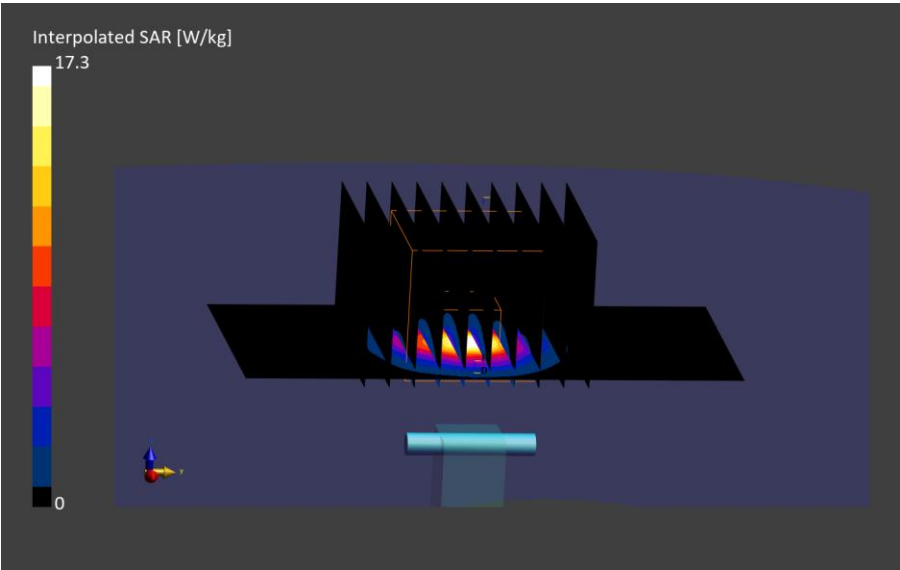

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	4.81, 4.7,5.04

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-23	23.1	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.80	33.0	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.10	0.87
psSAR10g	1.17	0.19
Peak SAR (Extrapolated)	17.5	2.76
psAPD (4.0 cm², sq)	N/A	N/A

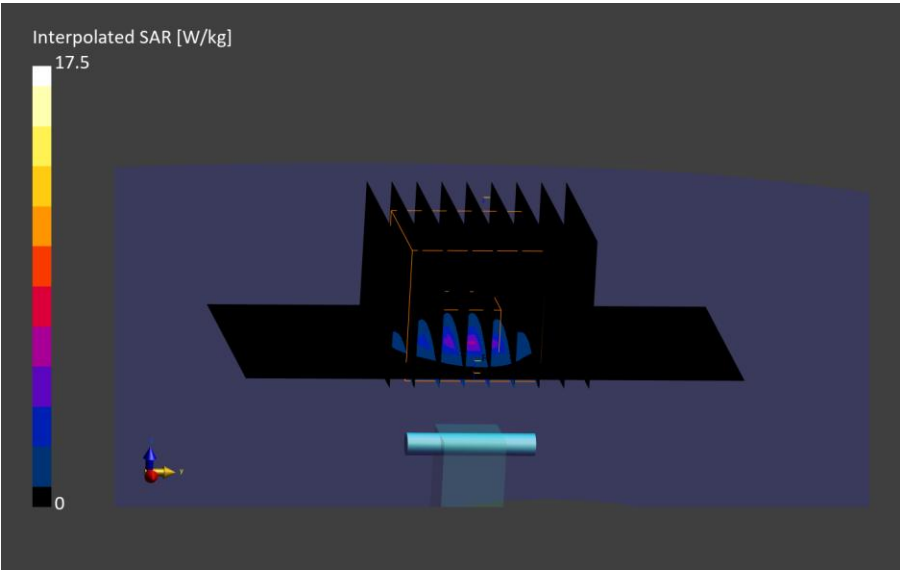

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	4.81, 4.7,5.04

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-10	22.7	22	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.93	34.3	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.13	1.61
psSAR10g	1.17	0.19
Peak SAR (Extrapolated)	17.8	4.52
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	4.98, 4.87, 5.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-17	22.9	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.03	33.3	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 36.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.75	-6.59
psSAR10g	1.07	-6.36
Peak SAR (Extrapolated)	16.5	-1.17
psAPD (4.0 cm², sq)	N/A	N/A

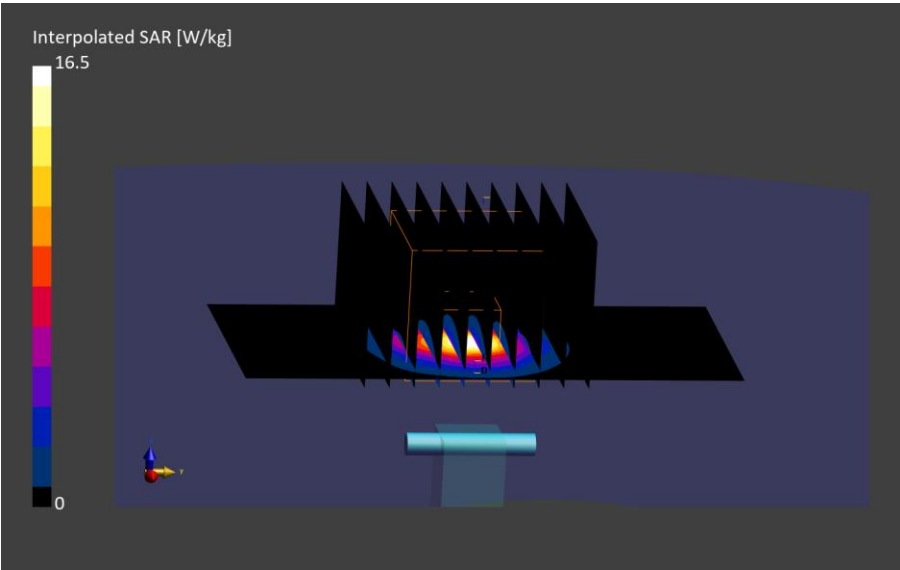

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	4.98, 4.87, 5.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-06-23	23.1	21.9	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.97	32.7	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.80	-5.34
psSAR10g	1.09	-4.61
Peak SAR (Extrapolated)	16.7	0.03
psAPD (4.0 cm², sq)	N/A	N/A

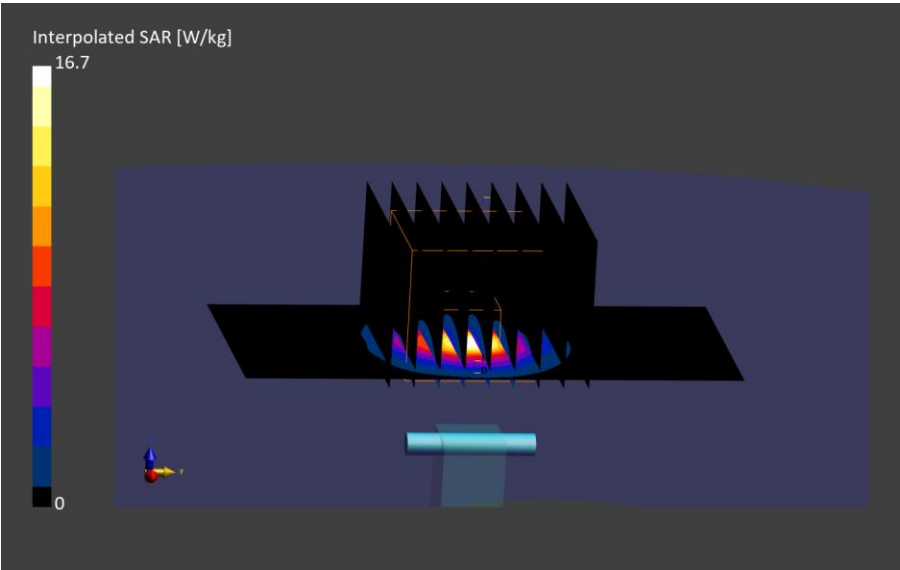

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	4.98, 4.87, 5.22

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-07-10	22.7	22	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.09	34.0	EX3DV4 – SN7836, 2024-09-12	DAE4ip Sn1839, 2024-09-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.84	-4.35
psSAR10g	1.09	-4.61
Peak SAR (Extrapolated)	17.0	1.83
psAPD (4.0 cm², sq)	N/A	N/A

