



HCT Co., Ltd.

2-6, 73, 74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, Republic of Korea

Tel. +82 31 645 6300 Fax. +82 31 645 6401

Appendix A: Test Setup Photo

FCC ID
A3LSMA376B

File No.

HCT-RF-2512-FC041-P	HCT-RF-2512-FC042-P	HCT-RF-2512-FC043-P
HCT-RF-2512-FC044-P	HCT-RF-2512-FC045-P	HCT-RF-2512-FC046-P
HCT-RF-2512-FC047-P	HCT-RF-2512-FC048-P	HCT-RF-2512-FC049-P
HCT-RF-2512-FC050-P	HCT-RF-2512-FC051-P	HCT-RF-2512-FC052-P
HCT-RF-2512-FC053-P	HCT-RF-2512-FC054-P	HCT-RF-2512-FC055-P

REVISION HISTORY

The revision history for this document is shown in table.

Revision No.	Date of Issue	Description
0	December 17, 2025	Initial Release

File No.	HCT-RF-2512-FC041-P	HCT-RF-2512-FC042-P	HCT-RF-2512-FC043-P	HCT-RF-2512-FC044-P	HCT-RF-2512-FC045-P
	HCT-RF-2512-FC046-P	HCT-RF-2512-FC047-P	HCT-RF-2512-FC048-P	HCT-RF-2512-FC049-P	HCT-RF-2512-FC050-P
	HCT-RF-2512-FC051-P	HCT-RF-2512-FC052-P	HCT-RF-2512-FC053-P	HCT-RF-2512-FC054-P	HCT-RF-2512-FC055-P

1. Radiated Test Setup Photo



File No.	HCT-RF-2512-FC041-P	HCT-RF-2512-FC042-P	HCT-RF-2512-FC043-P	HCT-RF-2512-FC044-P	HCT-RF-2512-FC045-P
	HCT-RF-2512-FC046-P	HCT-RF-2512-FC047-P	HCT-RF-2512-FC048-P	HCT-RF-2512-FC049-P	HCT-RF-2512-FC050-P
	HCT-RF-2512-FC051-P	HCT-RF-2512-FC052-P	HCT-RF-2512-FC053-P	HCT-RF-2512-FC054-P	HCT-RF-2512-FC055-P



File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

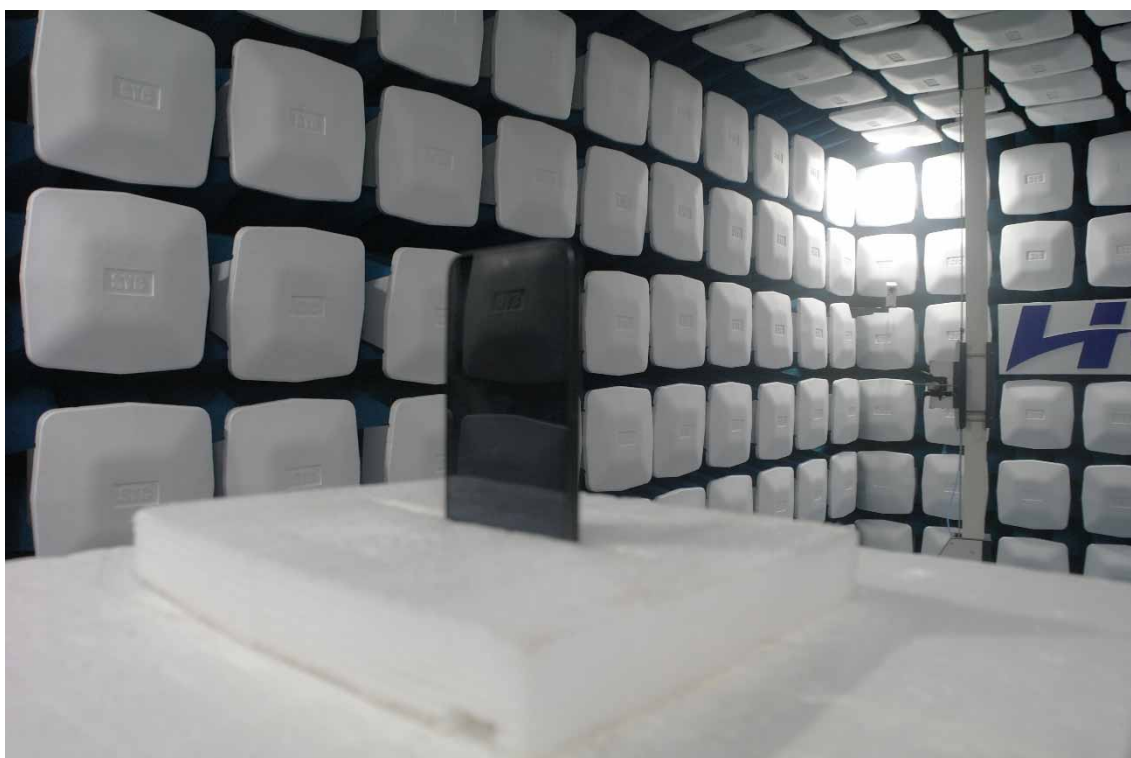

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

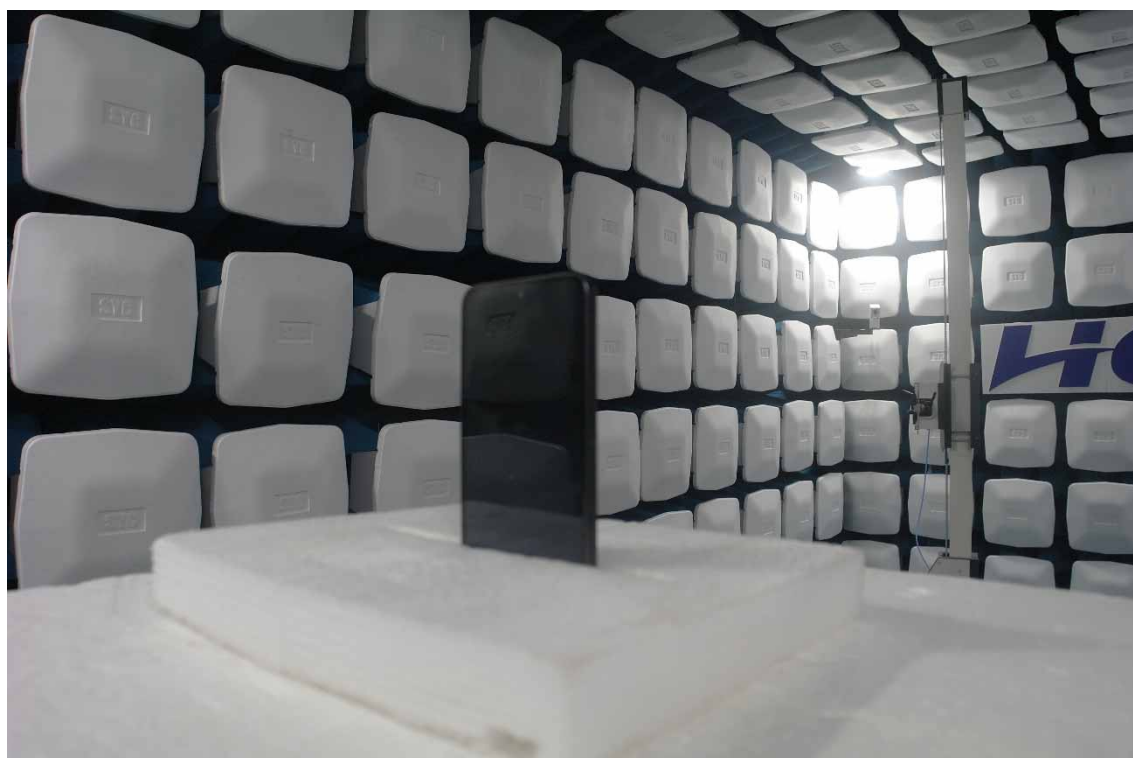

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

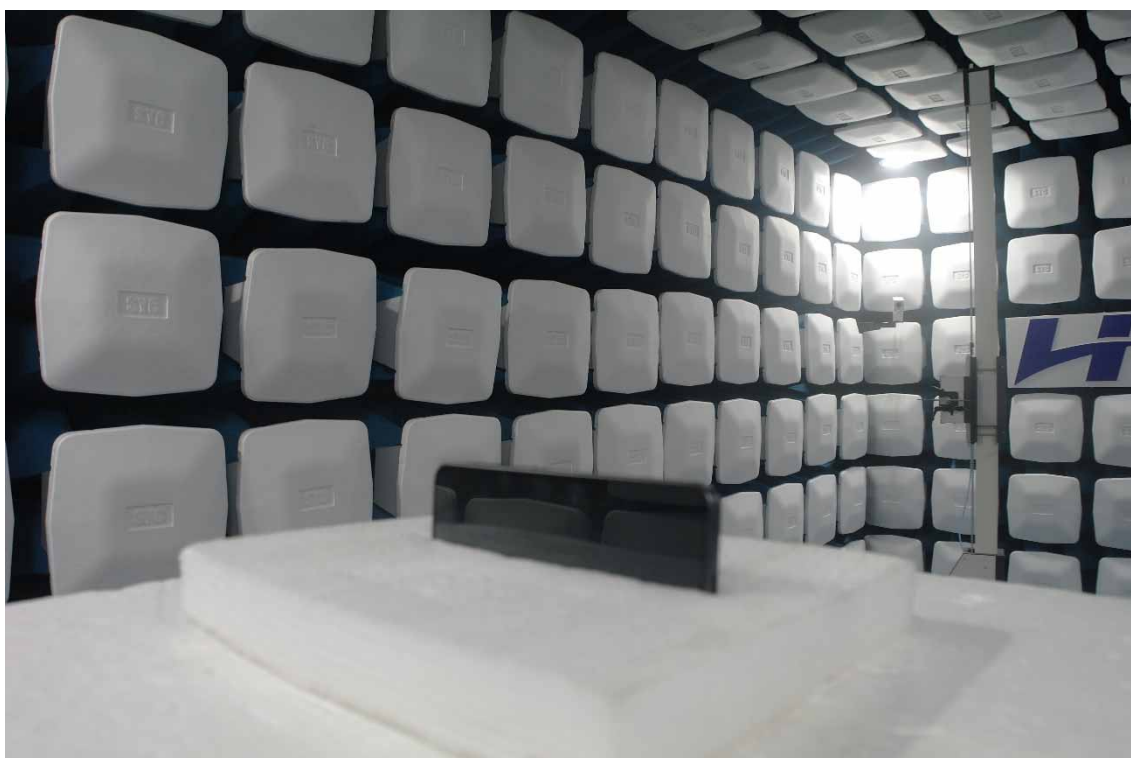

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

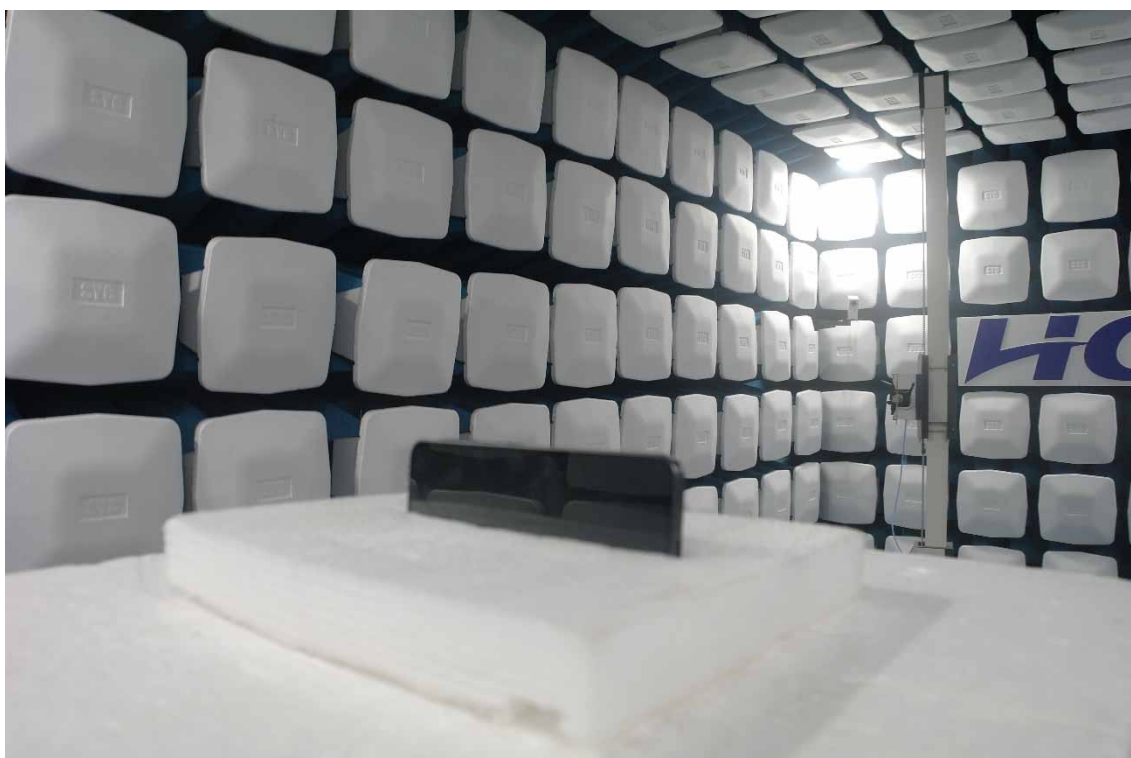

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

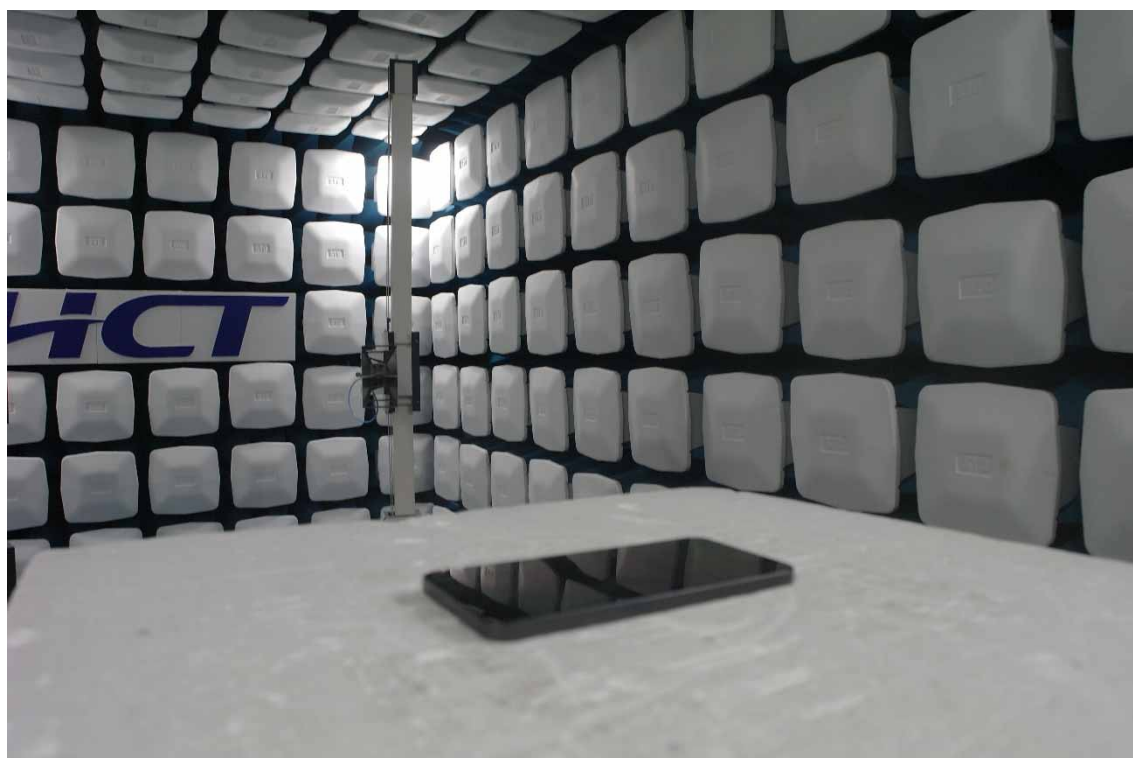

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

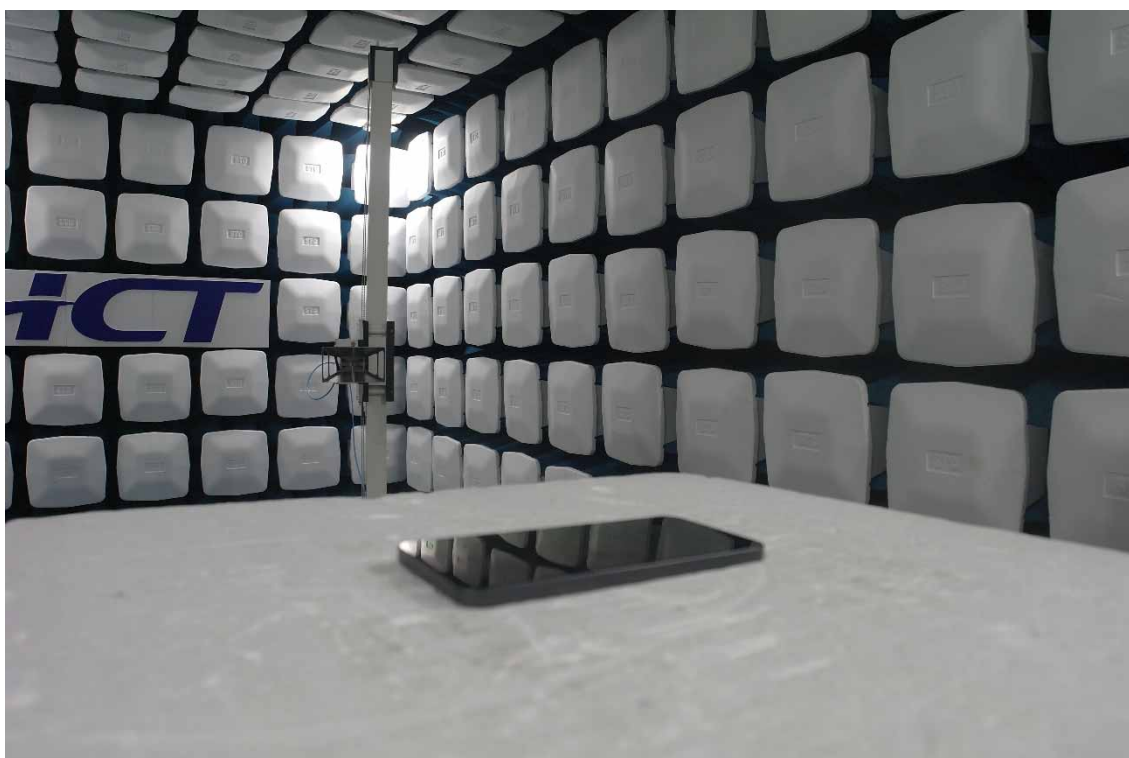

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

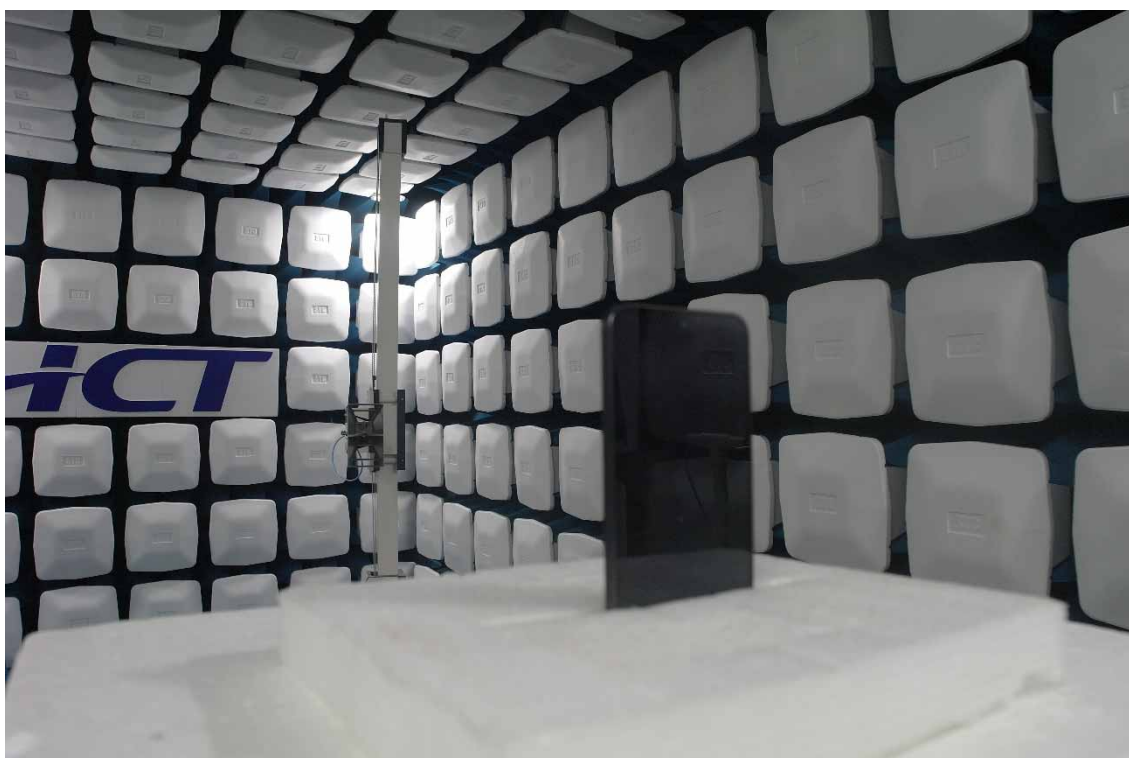

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

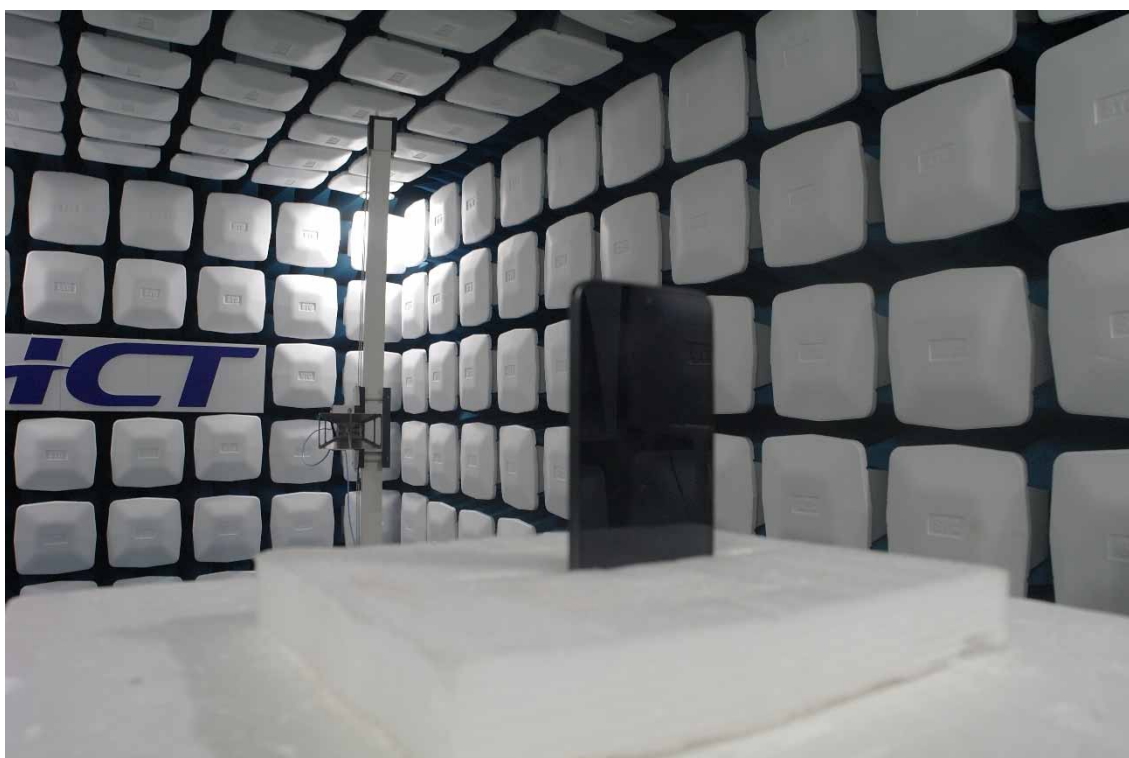

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

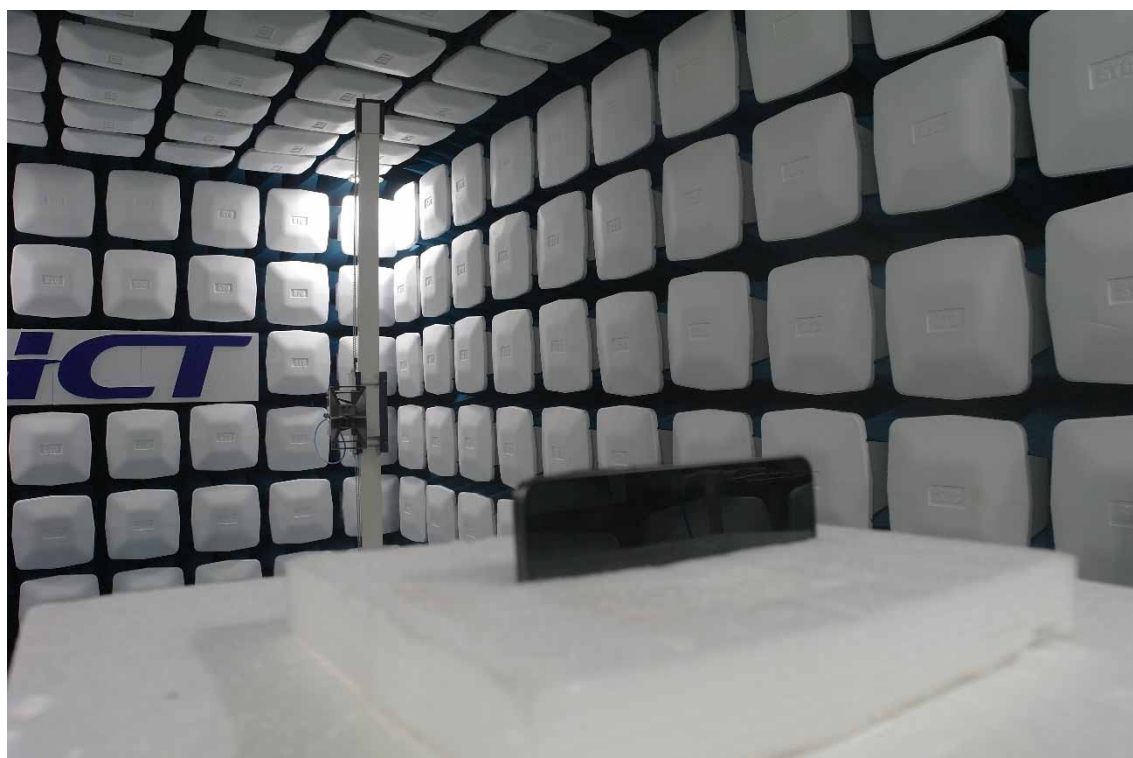

File
No.


HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P

HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

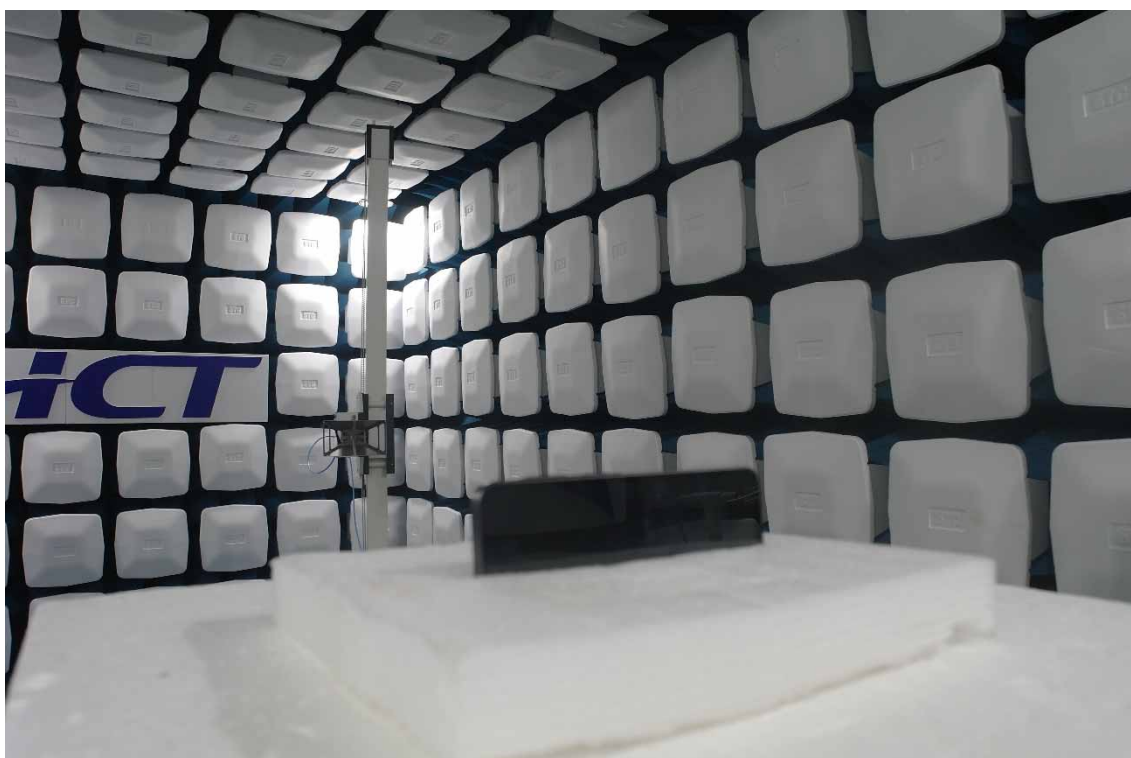

File
No.

HCT-RF-2512-FC041-P
HCT-RF-2512-FC046-P
HCT-RF-2512-FC051-P


HCT-RF-2512-FC042-P
HCT-RF-2512-FC047-P
HCT-RF-2512-FC052-P

HCT-RF-2512-FC043-P
HCT-RF-2512-FC048-P
HCT-RF-2512-FC053-P

HCT-RF-2512-FC044-P
HCT-RF-2512-FC049-P
HCT-RF-2512-FC054-P

HCT-RF-2512-FC045-P
HCT-RF-2512-FC050-P
HCT-RF-2512-FC055-P

2. Conducted Test Setup Photo

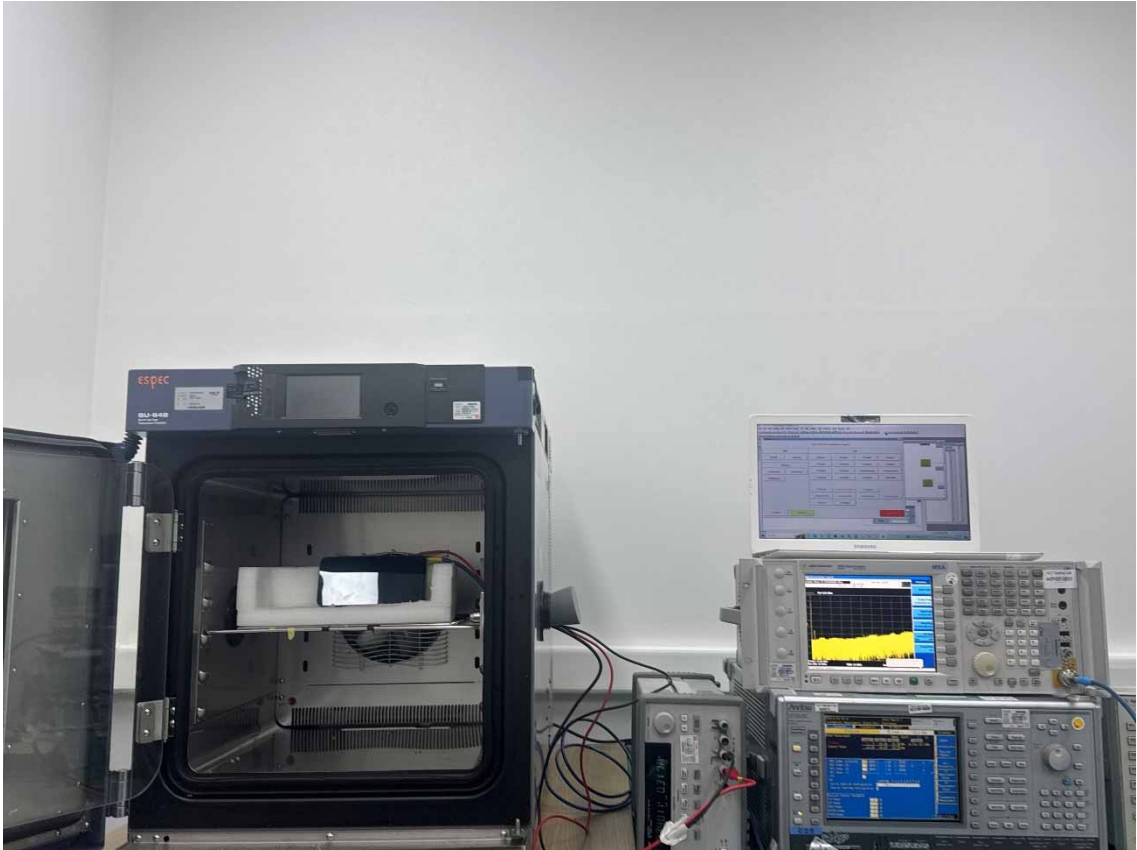

End of Report

File No.	HCT-RF-2512-FC041-P	HCT-RF-2512-FC042-P	HCT-RF-2512-FC043-P	HCT-RF-2512-FC044-P	HCT-RF-2512-FC045-P
	HCT-RF-2512-FC046-P	HCT-RF-2512-FC047-P	HCT-RF-2512-FC048-P	HCT-RF-2512-FC049-P	HCT-RF-2512-FC050-P
	HCT-RF-2512-FC051-P	HCT-RF-2512-FC052-P	HCT-RF-2512-FC053-P	HCT-RF-2512-FC054-P	HCT-RF-2512-FC055-P