

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 1750.000 MHz; Type: D1750V2 - SN1150

Communication System: UID: 0, CW; Frequency: 1750.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

f = 1750.000 MHz; cond = 1.35 S/m; perm = 39.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/05/2025; Ambient Temp: 21.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7659; ConvF:(8.68,8.33,8.44); 2025-04-07

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; 2025-04-10

Phantom: Twin-SAM V8.0; Serial: 1966

Measurement SW: DASY Module SAR V16.4.0.5005

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.58 W/kg

SAR(1 g) = 3.65 W/kg; SAR(10 g) = 1.95 W/kg

Deviation (1 g) = 0.27%; Deviation (10 g) = 0.52%

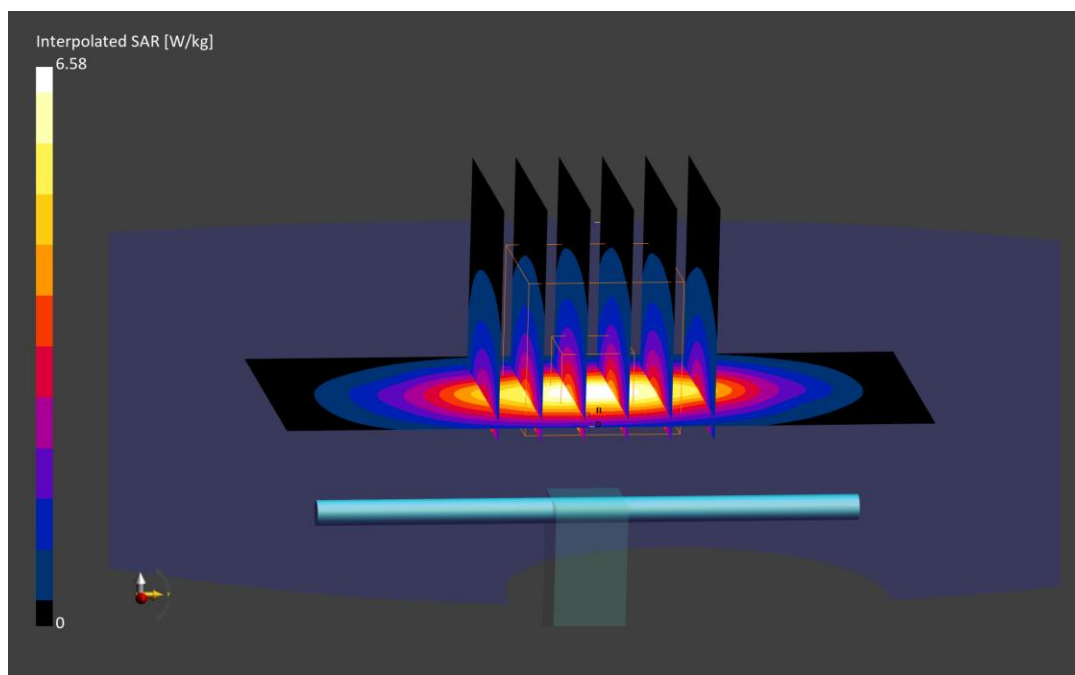

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

$f = 2450.000$ MHz; $\text{cond} = 1.84$ S/m; $\text{perm} = 39.7$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 05/21/2025; Ambient Temp: 20.5°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7410; ConvF:(7.07,6.98,7.38); 2024-12-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1213; 2024-12-04

Phantom: Twin-SAM V8.0; Serial: 1978

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 96.0): Measurement grid: $dx=10.0$ mm, $dy=12.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.1 W/kg

SAR(1 g) = 5.45 W/kg; SAR(10 g) = 2.55 W/kg

Deviation (1 g) = 4.81%; Deviation (10 g) = 4.51%

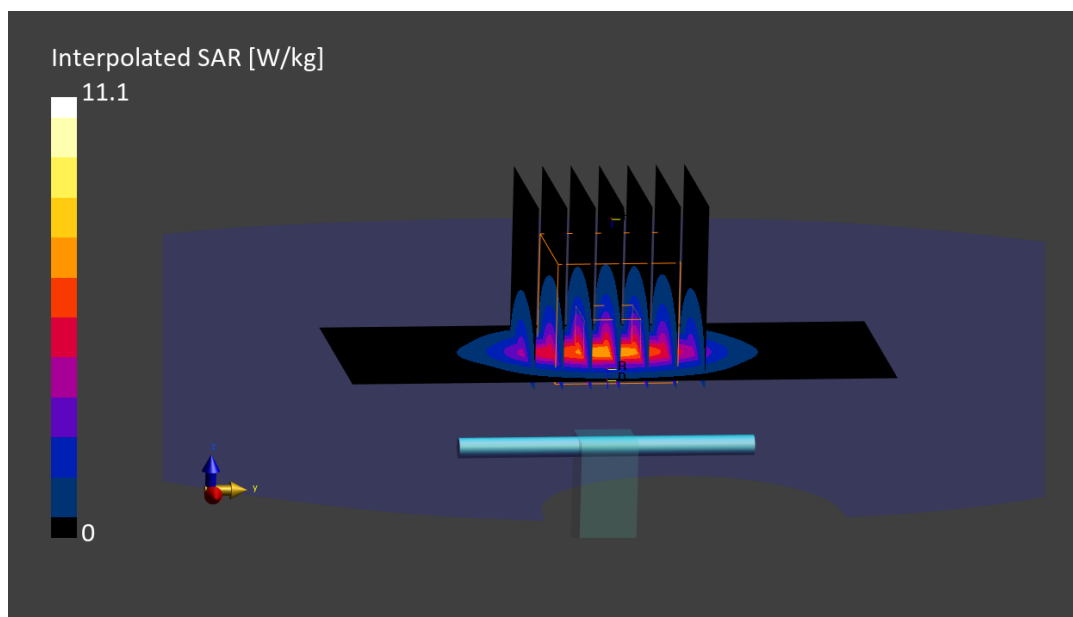

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

$f = 2450.000$ MHz; $\text{cond} = 1.79$ S/m; $\text{perm} = 38.0$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 05/27/2025; Ambient Temp: 21.5°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7406; ConvF:(7.24,6.85,7.63); 2024-07-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; 2024-07-08

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 5.03 W/kg; SAR(10 g) = 2.34 W/kg

Deviation (1 g) = -3.27%; Deviation (10 g) = -4.10%

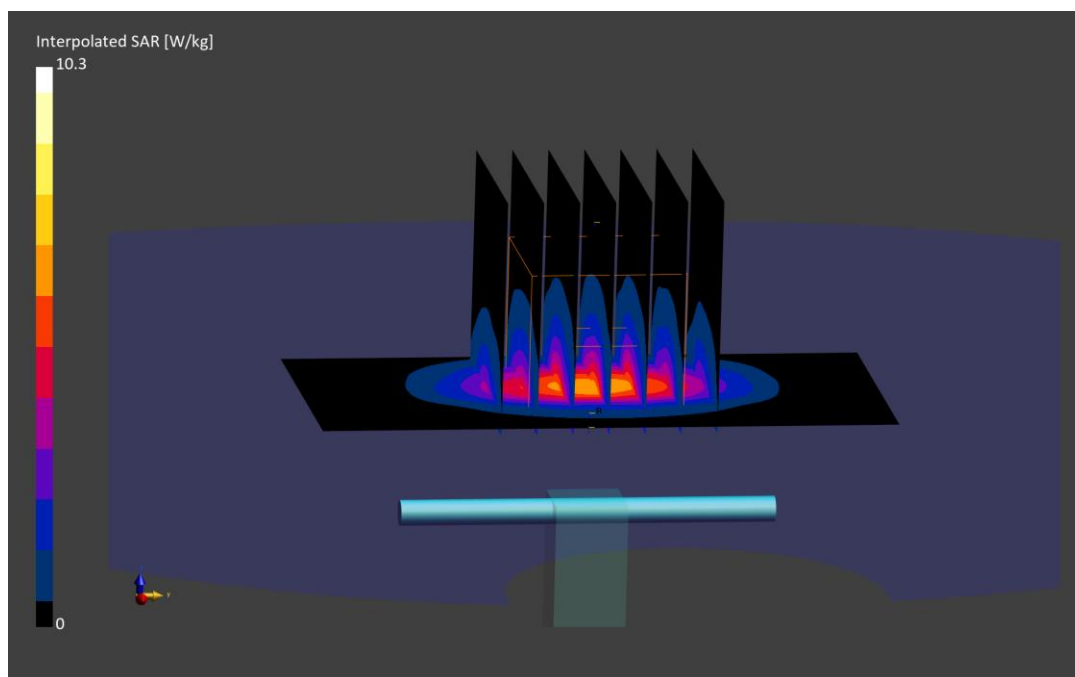

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

$f = 2450.000$ MHz; $\text{cond} = 1.84$ S/m; $\text{perm} = 38.4$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 05/29/2025; Ambient Temp: 21.9°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN7406; ConvF:(7.24,6.85,7.63); 2024-07-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; 2024-07-08

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.7 W/kg

SAR(1 g) = 5.27 W/kg; SAR(10 g) = 2.46 W/kg

Deviation (1 g) = 1.35%; Deviation (10 g) = 0.82%

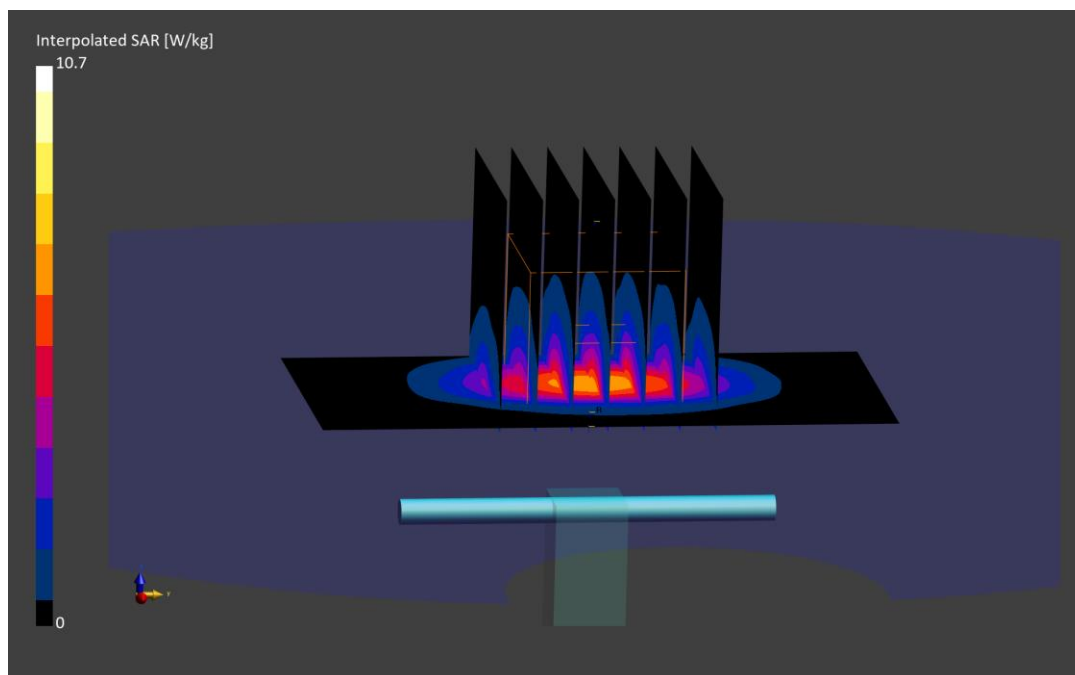

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN719

Communication System: UID: 0, CW; Frequency: 2450.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 2450.000$ MHz; $\text{cond} = 1.81$ S/m; $\text{perm} = 38.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/02/2025; Ambient Temp: 22.9°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7406; ConvF:(7.24,6.85,7.63); 2024-07-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1677; 2024-07-08
Phantom: Twin-SAM V5.0; Serial: 1800
Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

SAR(1 g) = 5.24 W/kg; SAR(10 g) = 2.44 W/kg

Deviation (1 g) = 0.38%; Deviation (10 g) = -0.81%

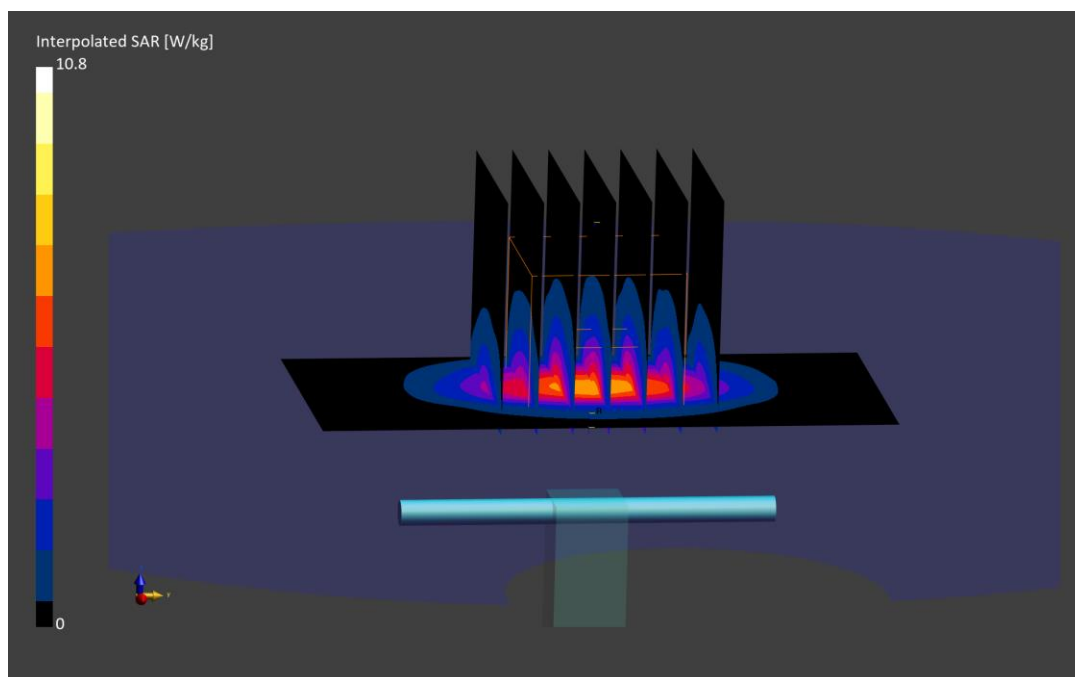

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
f = 2600.000 MHz; cond = 1.96 S/m; perm = 39.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/21/2025; Ambient Temp: 20.5°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7410; ConvF:(6.92,6.83,7.23); 2024-12-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1213; 2024-12-04

Phantom: Twin-SAM V8.0; Serial: 1978

Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 96.0): Measurement grid: dx=10.0 mm, dy=12.0 mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.7 W/kg

SAR(1 g) = 6.15 W/kg; SAR(10 g) = 2.76 W/kg

Deviation (1 g) = 9.04%; Deviation (10 g) = 9.52%

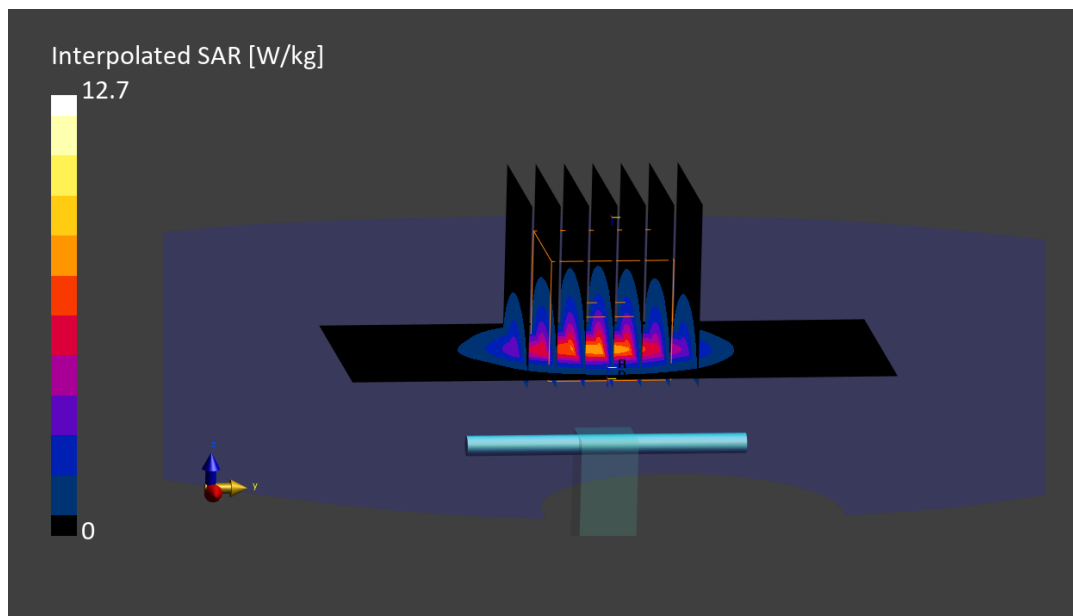

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 2600.000$ MHz; $\text{cond} = 1.91$ S/m; $\text{perm} = 37.7$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/27/2025; Ambient Temp: 21.5°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7406; ConvF:(7.28,6.89,7.67); 2024-07-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1677; 2024-07-08
Phantom: Twin-SAM V5.0; Serial: 1800
Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.40 W/kg; SAR(10 g) = 2.43 W/kg

Deviation (1 g) = -4.26%; Deviation (10 g) = -3.57%

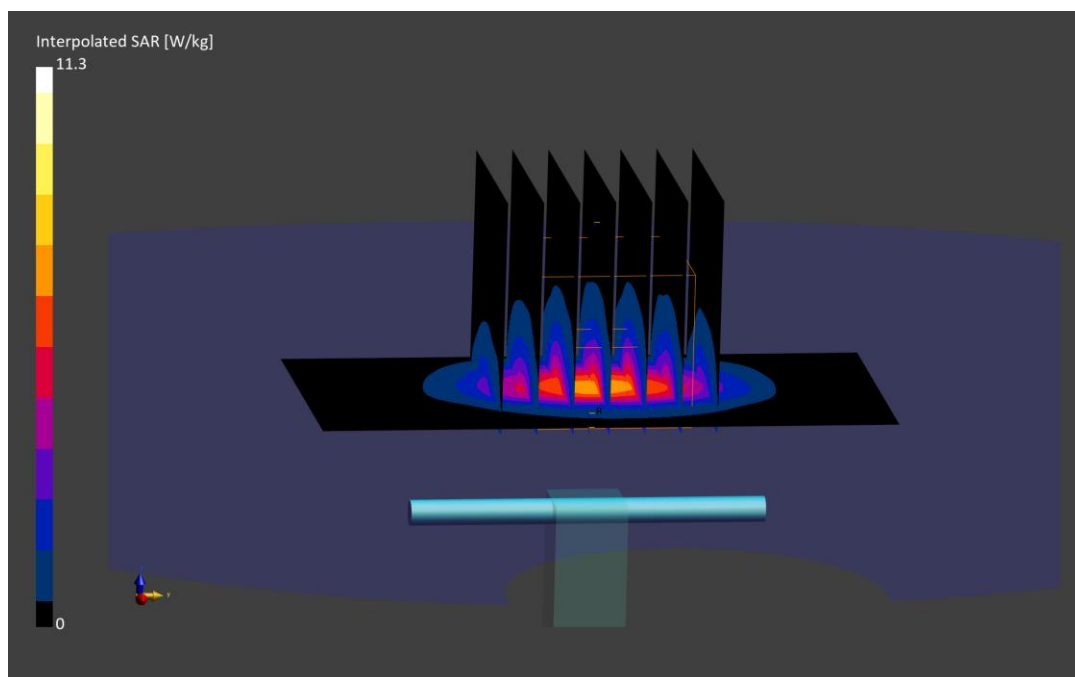

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

f = 2600.000 MHz; cond = 1.95 S/m; perm = 40.7; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 05/29/2025; Ambient Temp: 21.1°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7410; ConvF:(6.92,6.83,7.23); 2024-12-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1213; 2024-12-04

Phantom: Twin-SAM V8.0; Serial: 1978

Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 96.0): Measurement grid: dx=10.0 mm, dy=12.0 mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.2 W/kg

SAR(1 g) = 5.99 W/kg; SAR(10 g) = 2.72 W/kg

Deviation (1 g) = 6.02%; Deviation (10 g) = 7.09%

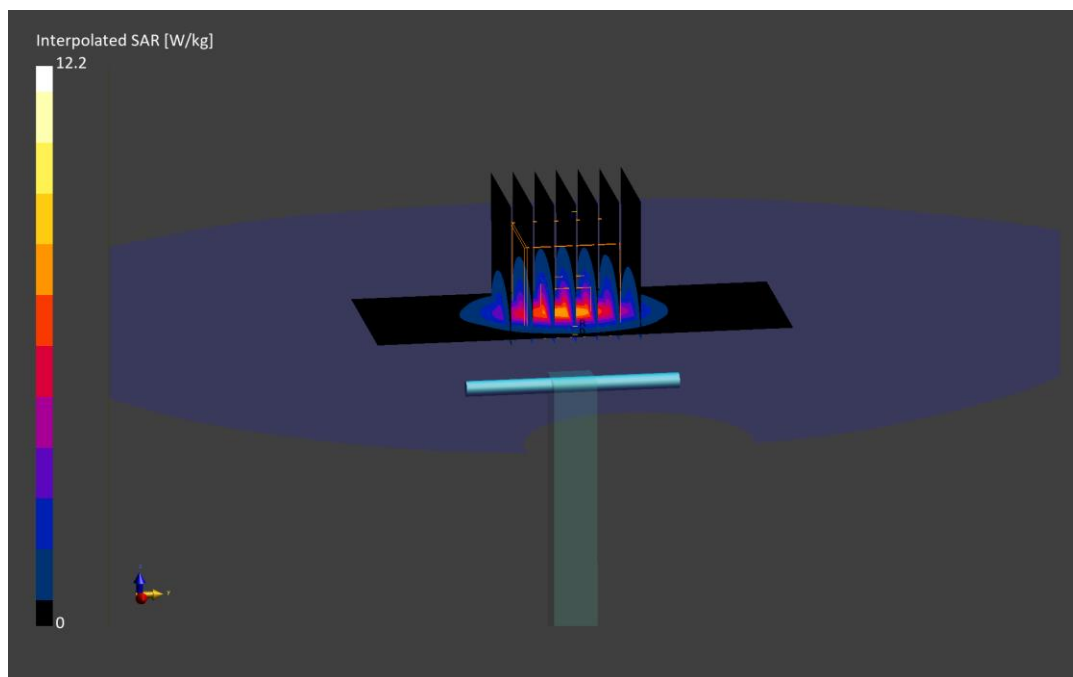

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 2600.000$ MHz; $\text{cond} = 1.94$ S/m; $\text{perm} = 38.3$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/02/2025; Ambient Temp: 22.9°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7406; ConvF:(7.28,6.89,7.67); 2024-07-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1677; 2024-07-08
Phantom: Twin-SAM V5.0; Serial: 1800
Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $\text{dx}=10.0$ mm, $\text{dy}=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $\text{dx}=5.0$ mm, $\text{dy}=5.0$ mm, $\text{dz}=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.35 W/kg; SAR(10 g) = 2.43 W/kg

Deviation (1 g) = -5.31%; Deviation (10 g) = -4.33%

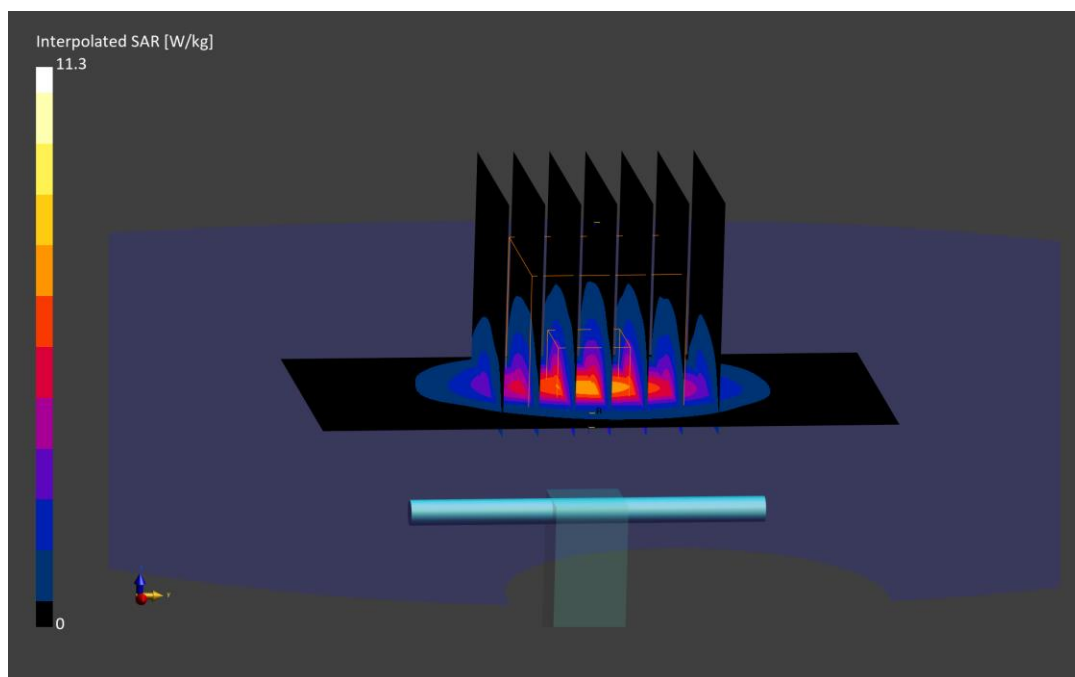

ELEMENT

DUT: Dipole 2600.000 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.000 MHz

Medium: Head Simulating Liquid; Medium parameters used:

f = 2600.000 MHz; cond = 1.93 S/m; perm = 37.3; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/02/2025; Ambient Temp: 20.2°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7410; ConvF:(6.92,6.83,7.23); 2024-12-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1213; 2024-12-04

Phantom: Twin-SAM V8.0; Serial: 1978

Measurement SW: DASY Module SAR V16.4.0.5005

2600.0 MHz System Verification at 20.0 dBm (100 mW)

Area Scan (40.0 x 96.0): Measurement grid: dx=10.0 mm, dy=12.0 mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

SAR(1 g) = 5.59 W/kg; SAR(10 g) = 2.53 W/kg

Deviation (1 g) = -1.06%; Deviation (10 g) = -0.39%

