

System Performance Check Report for D1750V2 – SN1125

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.000	TSL Permittivity	40.4
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.35
Conversion Factor	8.2	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7314 2025-06-03	Phantom	Twin-SAM V5.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1671 2025-08-13	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.45	3.37
psSAR10g [W/Kg]	1.83	1.81
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		9.9
M2/M1 [%]		83.6

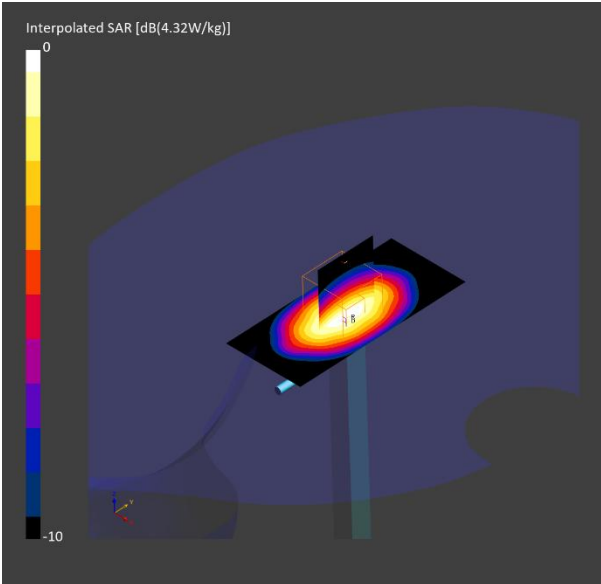

System Performance Check Report for D5GHzV2 - SN1325

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5250.000	TSL Permittivity	37.4
Group / UID	CW / 0-	TSL Conductivity [S/m]	4.65
Conversion Factor	5.84	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7314 2025-06-03	Phantom	Twin-SAM V5.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1671 2025-08-13	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.92	7.23
psSAR10g [W/Kg]	2.01	2.11
Power Drift [dB]		0.03
Dist 3dB Peak [mm]		7.2
M2/M1 [%]		64.4

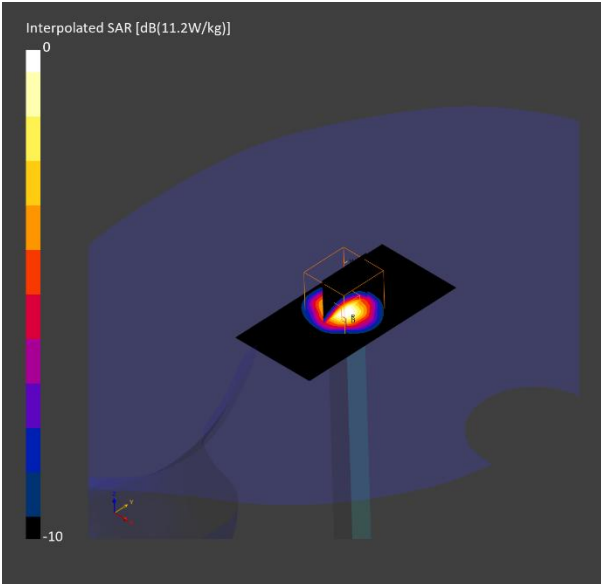

System Performance Check Report for D2450V2 - SN939

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.000	TSL Permittivity	39.0
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.76
Conversion Factor	7.42	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7314 2025-06-03	Phantom	Twin-SAM V5.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1671 2025-08-13	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	4.92	4.81
psSAR10g [W/Kg]	2.32	2.29
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		9.3
M2/M1 [%]		82.8

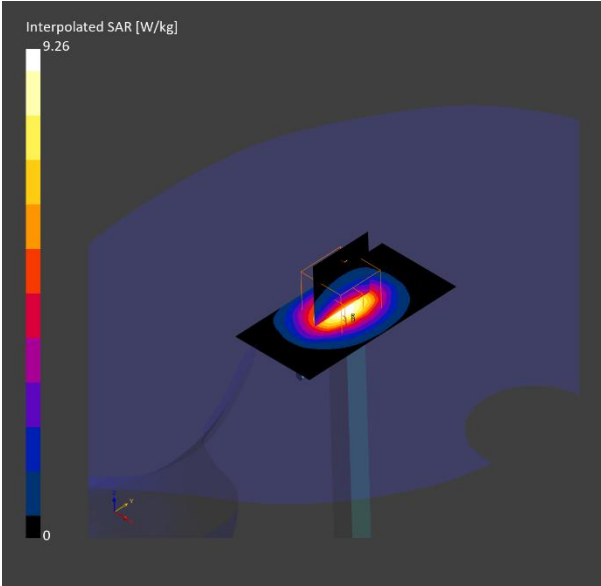

20260313_SystemPerformanceCheck D1750V2 SN1125

Frequency: 1750 MHz; Communication System Channel Number: 0; Duty Cycle: 1:1

Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.324$ S/m; $\epsilon_r = 39.804$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Electronics: DAE4 Sn1591; Calibrated: 2026-02-13
- Probe: EX3DV4 - SN7652; ConvF(8.35, 8.23, 8.5) @ 1750 MHz; Calibrated: 2025-04-22
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (Middle); Phantom section: Flat Section ; Type: QD 000 P40 CD
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Configuration/1750MHz/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 5.14 W/kg

Configuration/1750MHz/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 67.44 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 6.01 W/kg

SAR(1 g) = 3.41 W/kg; SAR(10 g) = 1.81 W/kg

Smallest distance from peaks to all points 3 dB below = 11.2 mm

Ratio of SAR at M2 to SAR at M1 = 56.2%

Maximum value of SAR (measured) = 5.16 W/kg

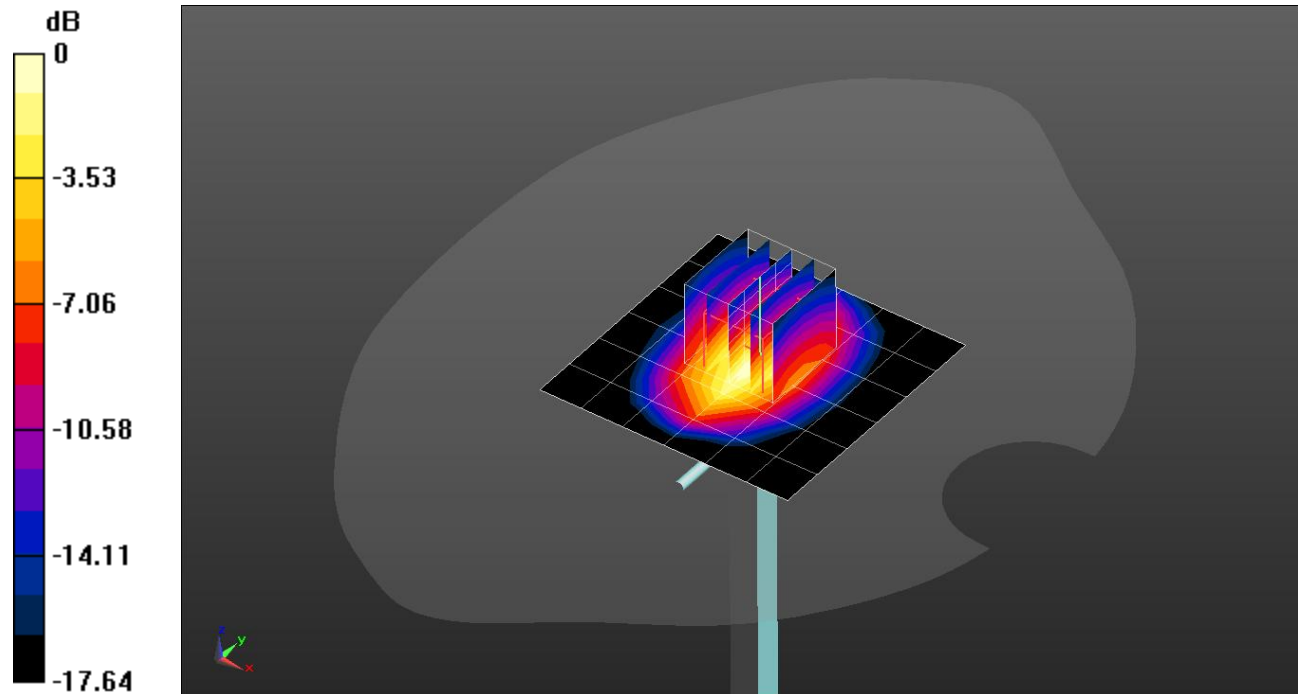

0 dB = 5.16 W/kg = 7.13 dBW/kg

20260324_SystemPerformanceCheck D835V2 SN4d194

Frequency: 835 MHz; Communication System Channel Number: 0; Duty Cycle: 1:1

Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 835$ MHz; $\sigma = 0.901$ S/m; $\epsilon_r = 43.548$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Electronics: DAE4 Sn1591; Calibrated: 2/13/2026
- Probe: EX3DV4 - SN7652; ConvF(9.63, 9.49, 9.81) @ 835 MHz; Calibrated: 4/22/2025
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (Middle); Phantom section: Flat Section ; Type: QD 000 P40 CD
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Configuration/Pin=100 mW/Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 1.29 W/kg

Configuration/Pin=100 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 40.27 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 1.49 W/kg

SAR(1 g) = 1.03 W/kg; SAR(10 g) = 0.682 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 68.9%

Maximum value of SAR (measured) = 1.35 W/kg

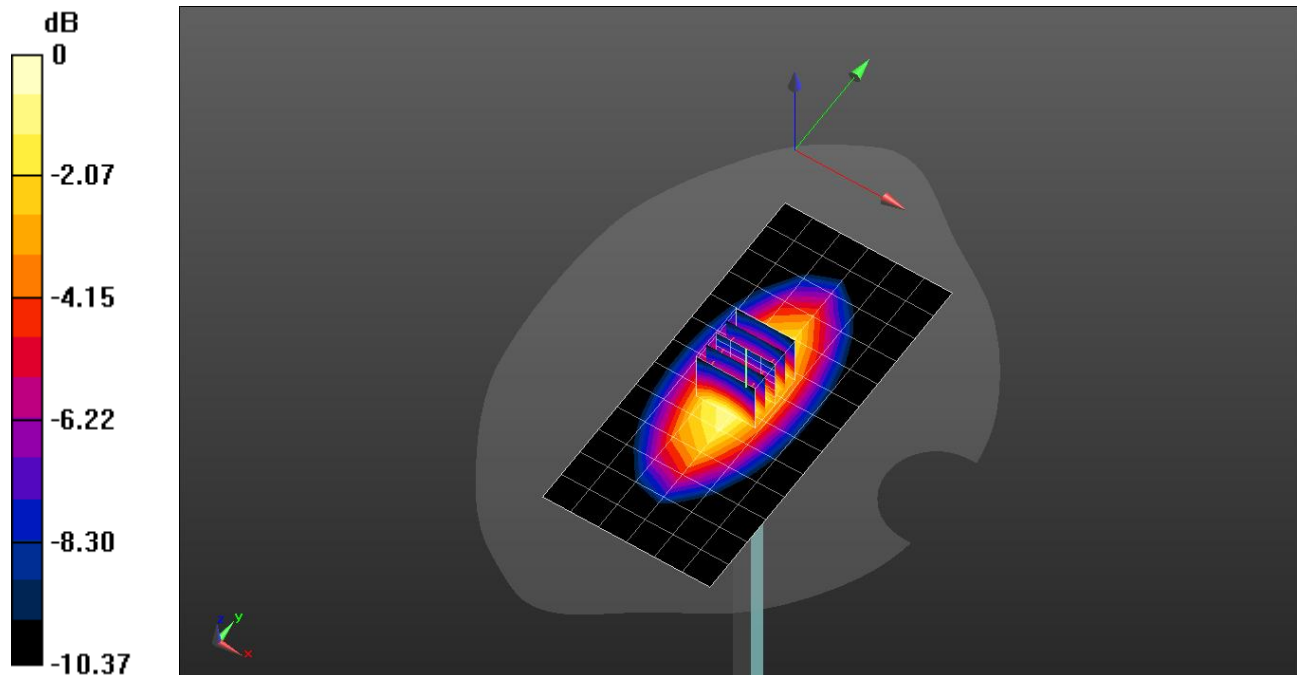

0 dB = 1.35 W/kg = 1.30 dBW/kg

20260331_SystemPerformanceCheck D1750V2 SN1125

Frequency: 1750 MHz; Communication System Channel Number: 0; Duty Cycle: 1:1

Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.341$ S/m; $\epsilon_r = 40.342$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Electronics: DAE4 Sn1447; Calibrated: 3/13/2026
- Probe: EX3DV4 - SN7330; ConvF(8.41, 8, 7.77) @ 1750 MHz; Calibrated: 1/22/2026
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (Right); Phantom section: Flat Section ; Type: QD 000 P40 CD
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Configuration/1750MHz/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 3.77 W/kg

Configuration/1750MHz/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 50.26 V/m; Power Drift = 0.13 dB


Peak SAR (extrapolated) = 5.86 W/kg

SAR(1 g) = 3.39 W/kg; SAR(10 g) = 1.83 W/kg

Smallest distance from peaks to all points 3 dB below = 11.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.4%

Maximum value of SAR (measured) = 5.07 W/kg

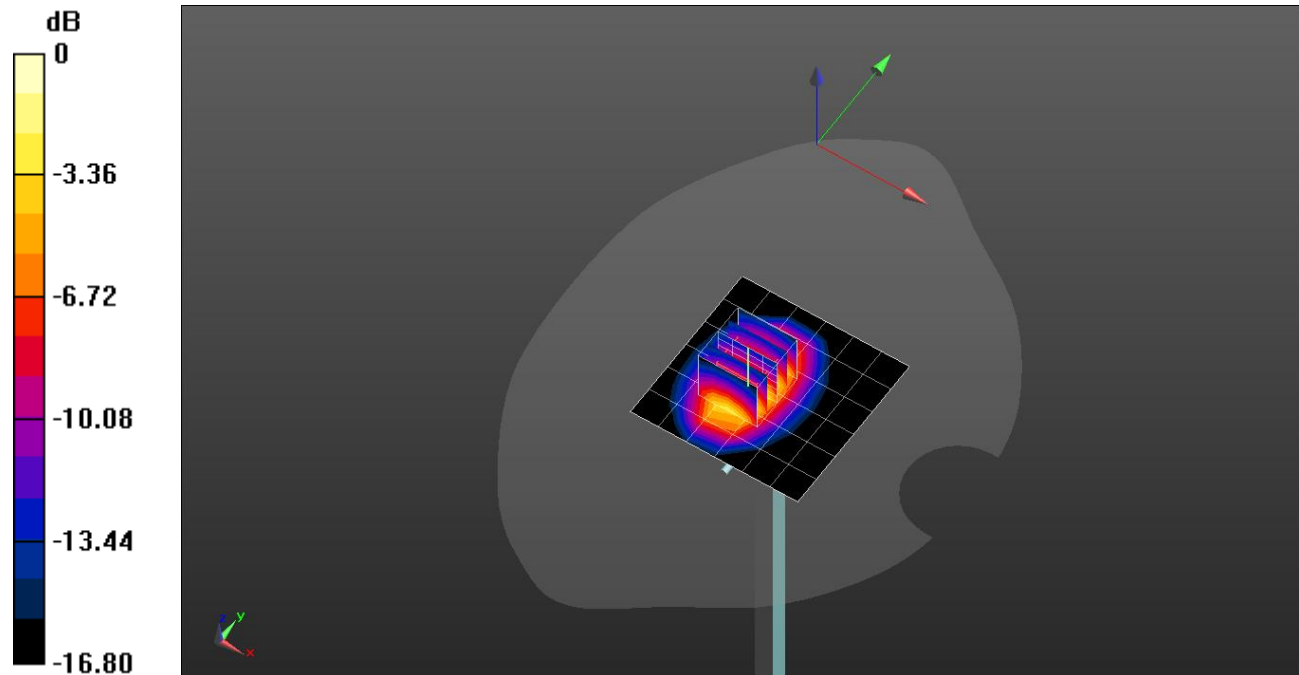

0 dB = 5.07 W/kg = 7.05 dBW/kg

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.000	TSL Permittivity	40.8
Group / UID	CW / 0-	TSL Conductivity [S/m]	0.910
Conversion Factor	8.89	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7545 2025-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1343 2025-07-09	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.857	0.862
psSAR10g [W/Kg]	0.562	0.558
Power Drift [dB]		-0.03
Dist 3dB Peak [mm]		19.0
M2/M1 [%]		87.8

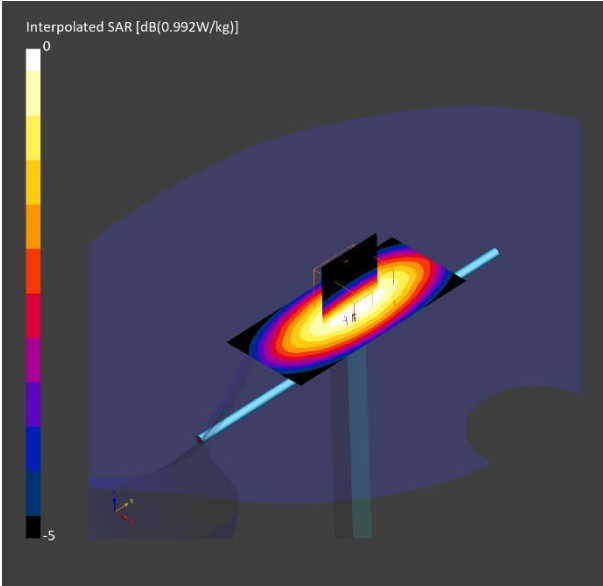

System Performance Check Report for D750V3 - SN1205

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	750.000	TSL Permittivity	41.1
Group / UID	CW / 0-	TSL Conductivity [S/m]	0.907
Conversion Factor	9.39	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7545 2025-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1343 2025-07-09	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.904	0.932
psSAR10g [W/Kg]	0.607	0.614
Power Drift [dB]		-0.01
Dist 3dB Peak [mm]		22.2
M2/M1 [%]		89.2

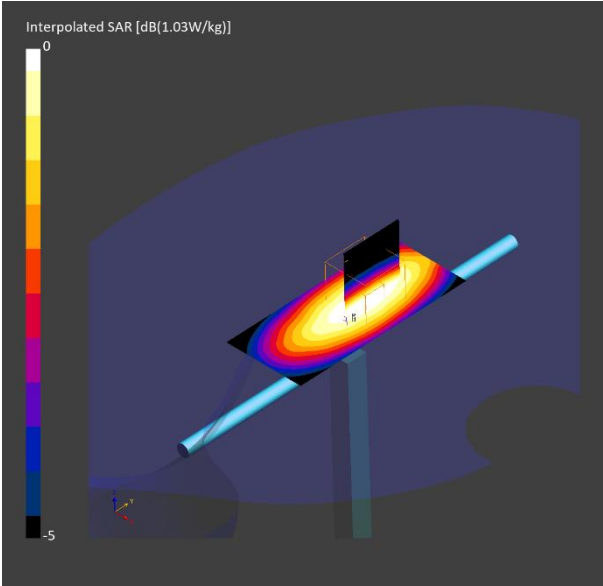

SystemPerformancecheck 2600_SN1178

Frequency: 2600 MHz; Communication System Channel Number: 0; Duty Cycle: 1:1

Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 2600$ MHz; $\sigma = 1.923$ S/m; $\epsilon_r = 39.146$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Electronics: DAE4 Sn1540; Calibrated: 2026-01-08
- Probe: EX3DV4 - SN7313; ConvF(6.91, 7.39, 7.76) @ 2600 MHz; Calibrated: 2025-10-29
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Phantom section: Flat Section ; Type: QD 000 P40 CD
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

system/2600MHz/Area Scan (6x9x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 7.41 W/kg

system/2600MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 75.30 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.78 W/kg; SAR(10 g) = 2.63 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 49.3%

Maximum value of SAR (measured) = 9.64 W/kg

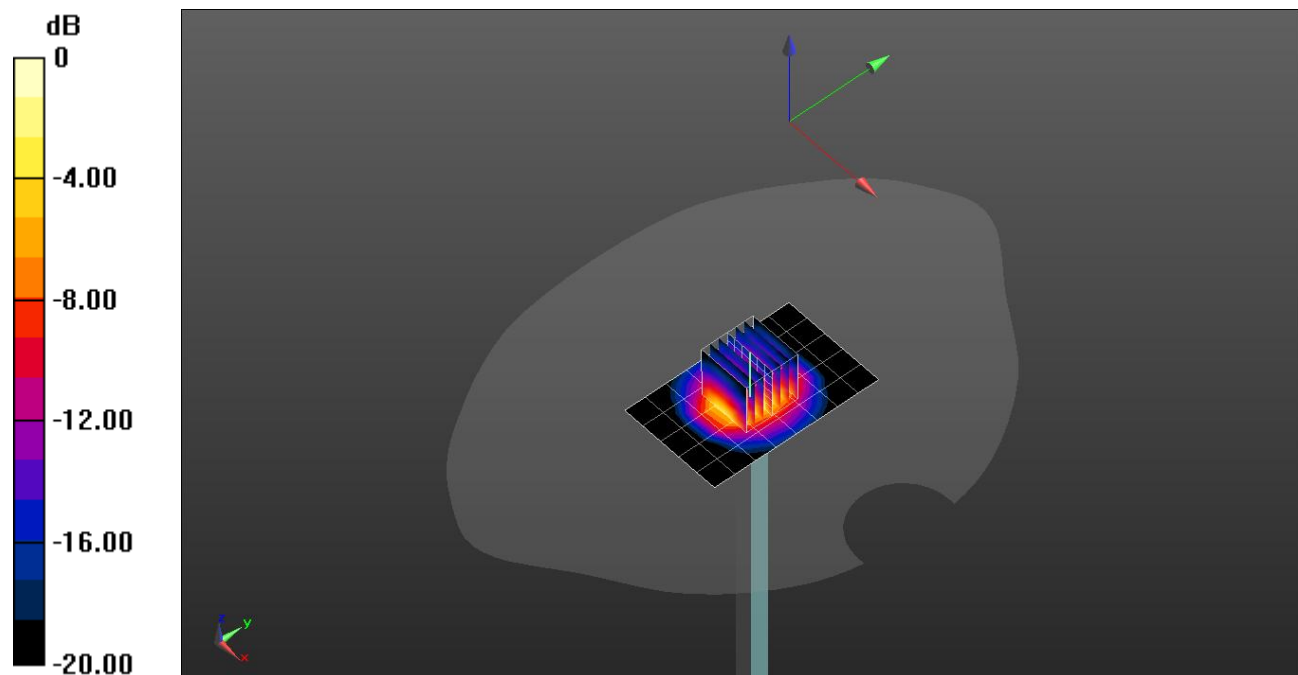

0 dB = 9.64 W/kg = 9.84 dBW/kg

System Performance Check Report for D1900V2 - SN5d190
Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.000	TSL Permittivity	40.5
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.45
Conversion Factor	8.05	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN3871 2025-08-22	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1668 2025-09-17	TSL Type	HBBL-600-10000
Software Version	17.0.4.7034		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.70	3.69
psSAR10g [W/Kg]	1.95	2.03
Power Drift [dB]		0.00
Dist 3dB Peak [mm]		9.9
M2/M1 [%]		86.3

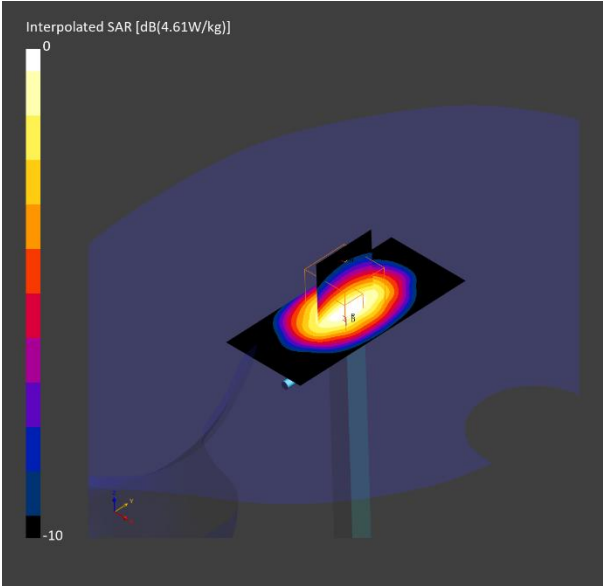

System Performance Check Report for D1750V2 - SN1125

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.000	TSL Permittivity	39.2
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.36
Conversion Factor	8.31	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN3871 2025-08-22	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1668 2025-09-17	TSL Type	HBBL-600-10000
Software Version	17.0.4.7034		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.18	3.36
psSAR10g [W/Kg]	1.73	1.83
Power Drift [dB]		-0.13
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		84.9

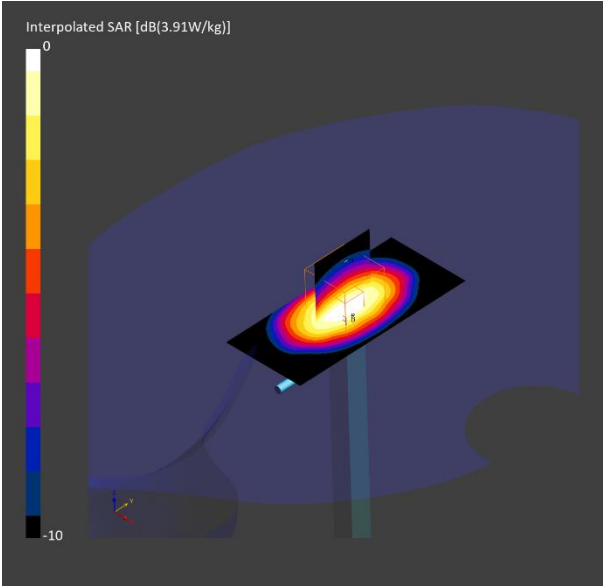

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.000	TSL Permittivity	42.4
Group / UID	CW / 0-	TSL Conductivity [S/m]	0.925
Conversion Factor	10.13	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7330 2026-01-22	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1917 2025-09-10	TSL Type	HBBL-600-10000
Software Version	17.0.4.7034		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.863	0.868
psSAR10g [W/Kg]	0.565	0.578
Power Drift [dB]		-0.15
Dist 3dB Peak [mm]		16.4
M2/M1 [%]		88.5

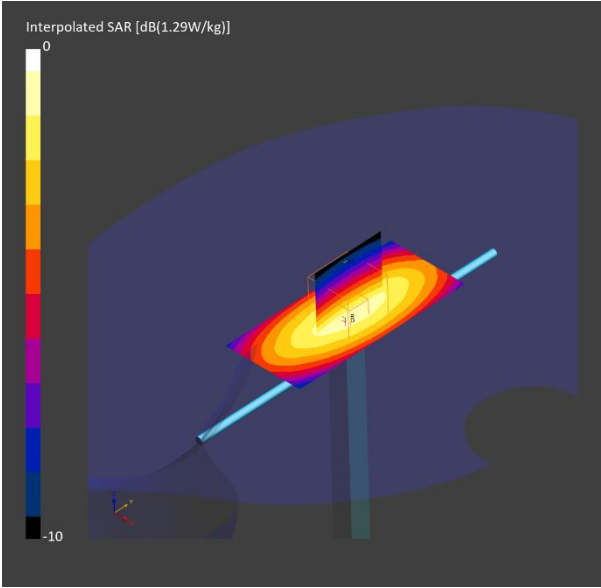

System Performance Check Report for CLA-13 - SN1015

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	13.000	TSL Permittivity	54.8
Group / UID	CW / 0-	TSL Conductivity [S/m]	0.735
Conversion Factor	15.11	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-10-29	Phantom	ELI V6.0 (20deg probe tilt)
DAE Calibration Date	DAE4ip Sn1917 2025-09-10	TSL Type	HBBL-600-10000
Software Version	17.0.4.7034		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.053	0.051
psSAR10g [W/Kg]	0.043	0.032
Power Drift [dB]		-0.02
Dist 3dB Peak [mm]		15.6
M2/M1 [%]		74.1

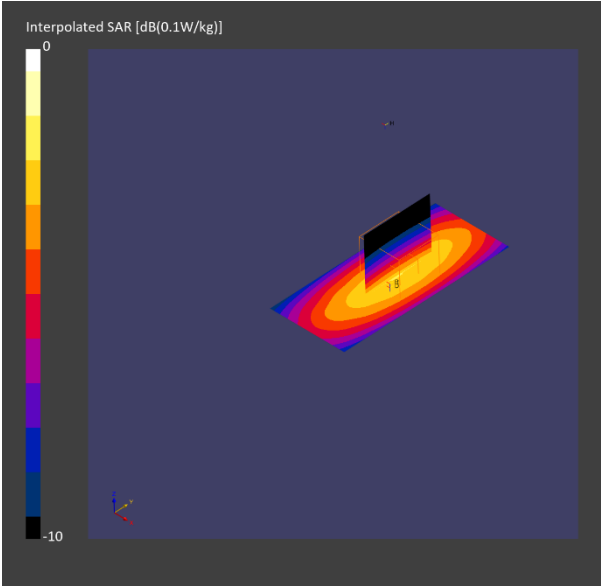

System Performance Check Report for D1640V2 - SN334

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1640.000	TSL Permittivity	39.1
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.28
Conversion Factor	7.49	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2025-10-20	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1670 2025-08-13	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.19	3.21
psSAR10g [W/Kg]	1.75	1.78
Power Drift [dB]		-0.05
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		83.5

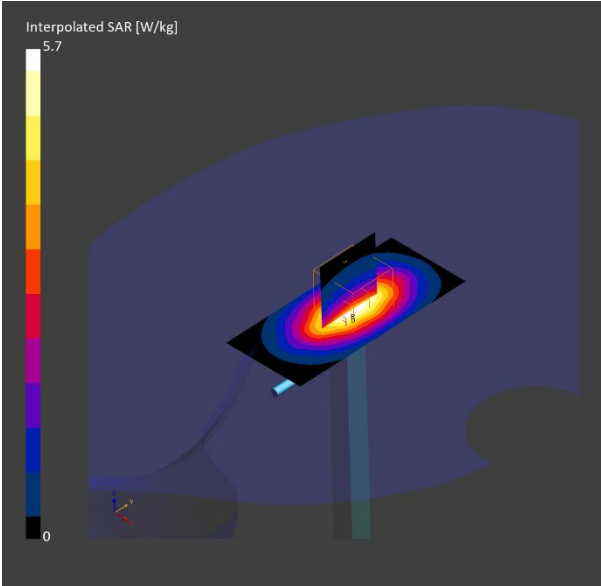

System Performance Check Report for D1900V2 - SN5d190

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.000	TSL Permittivity	38.6
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.42
Conversion Factor	7.26	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2025-10-20	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1670 2025-08-13	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	4.15	4.21
psSAR10g [W/Kg]	2.15	2.24
Power Drift [dB]		-0.02
Dist 3dB Peak [mm]		9.9
M2/M1 [%]		83.8

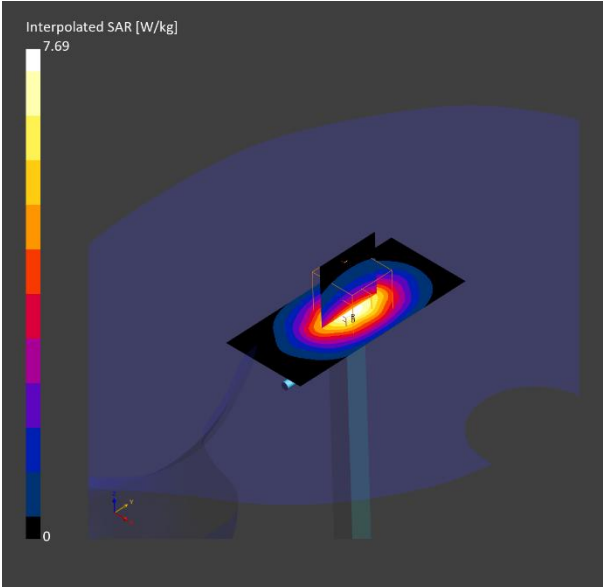

System Performance Check Report for D6.5GHzV2 - SN1010

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	6500.000	TSL Permittivity	33.8
Group / UID	CW / 0--	TSL Conductivity [S/m]	6.21
Conversion Factor	5.04	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2025-10-20	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1670 2025-08-13	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	24.0	27.6
psSAR10g [W/Kg]	4.83	5.44
psAPD (1.0cm², sq.) [W/m²]	N/A	276
psAPD (4.0cm², sq.) [W/m²]	N/A	131
Power Drift [dB]		0.08
Dist 3dB Peak [mm]		4.9
M2/M1 [%]		52.5

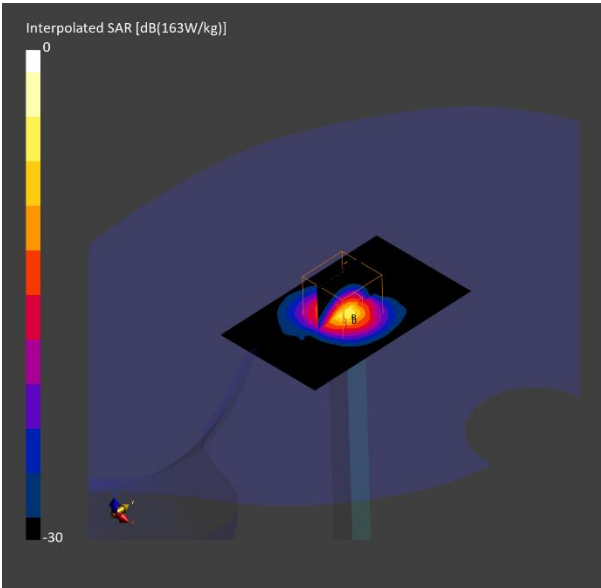

System Performance Check Report for D8GHzV2 - SN1012

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	8000.000	TSL Permittivity	32.0
Group / UID	CW / 0--	TSL Conductivity [S/m]	8.03
Conversion Factor	5.73	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7376 2025-07-29	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4ip Sn1667 2025-09-16	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	52.0 x 91.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	6.5 x 6.5	2.7 x 2.7 x 1.3
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	26.6	27.9
psSAR10g [W/Kg]	5.17	4.96
psAPD (1.0cm², sq.) [W/m²]	N/A	279
psAPD (4.0cm², sq.) [W/m²]	N/A	120
Power Drift [dB]		-0.06
Dist 3dB Peak [mm]		4.4
M2/M1 [%]		43.3

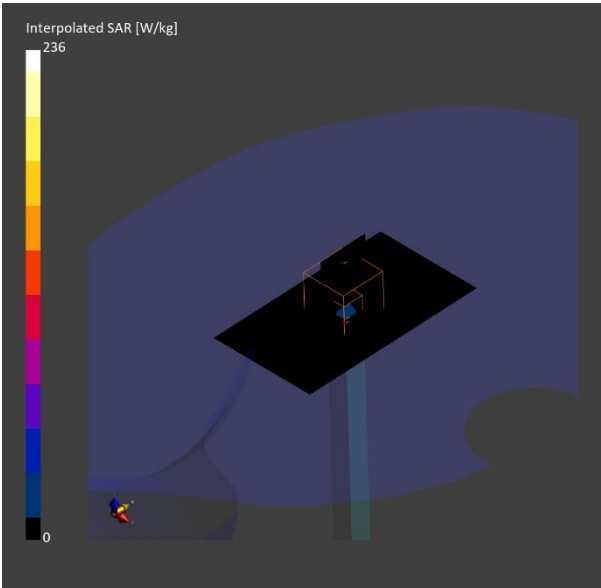

System Performance Check Report for D2300V2 - SN1090

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2300.000	TSL Permittivity	39.5
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.68
Conversion Factor	7.33	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2026-01-22	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1468 2026-02-03	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.07	5.08
psSAR10g [W/Kg]	2.43	2.49
Power Drift [dB]		0.05
Dist 3dB Peak [mm]		9.5
M2/M1 [%]		81.9

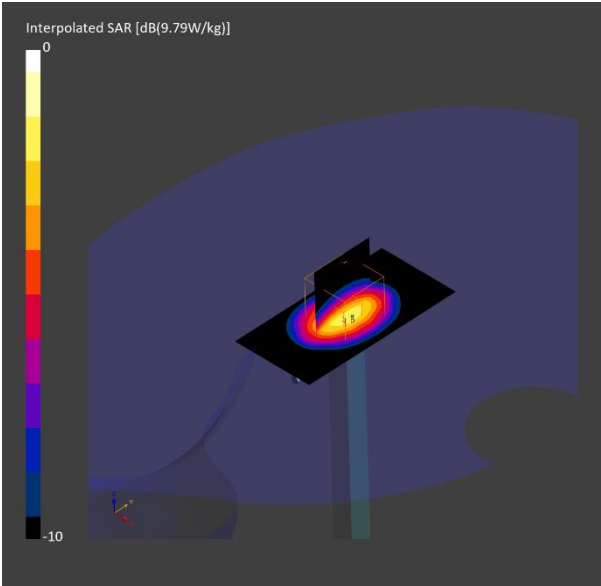

System Performance Check Report for D2600V2 - SN1097

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2600.000	TSL Permittivity	38.2
Group / UID	CW / 0-	TSL Conductivity [S/m]	1.95
Conversion Factor	7.04	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2026-01-22	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1468 2026-02-03	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.50	5.47
psSAR10g [W/Kg]	2.53	2.58
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		9.9
M2/M1 [%]		84.1

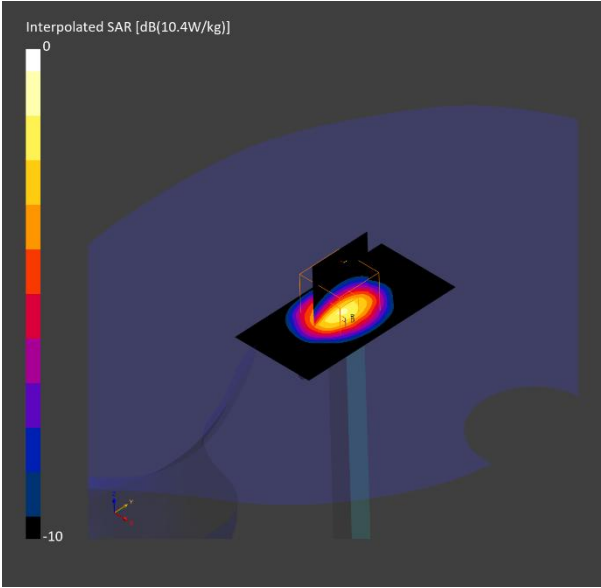

System Performance Check Report for D3500V2 - SN1075

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	3500.000	TSL Permittivity	37.1
Group / UID	CW / 0-	TSL Conductivity [S/m]	2.89
Conversion Factor	6.24	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-10-29	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1468 2026-02-03	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.13	6.19
psSAR10g [W/Kg]	2.40	2.49
Power Drift [dB]		0.02
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		79.1

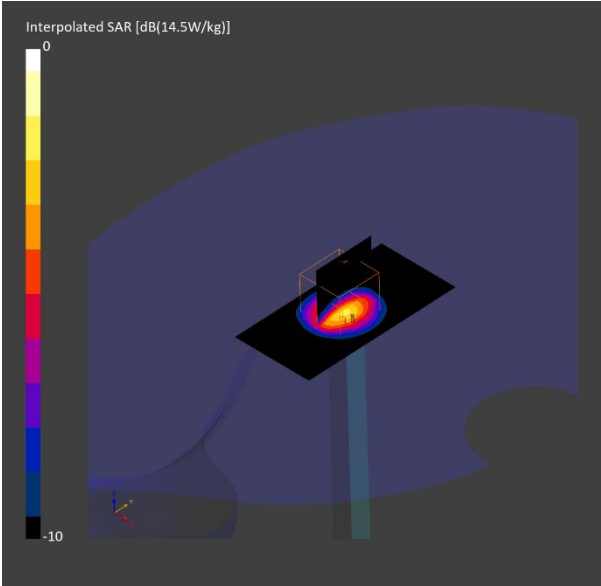

System Performance Check Report for D3700V2 - SN1036

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	3700.000	TSL Permittivity	37.4
Group / UID	CW / 0-	TSL Conductivity [S/m]	3.19
Conversion Factor	6.4	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7651 2026-01-19	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2025-07-09	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.09	6.38
psSAR10g [W/Kg]	2.33	2.63
Power Drift [dB]		0.02
Dist 3dB Peak [mm]		8.6
M2/M1 [%]		81.9

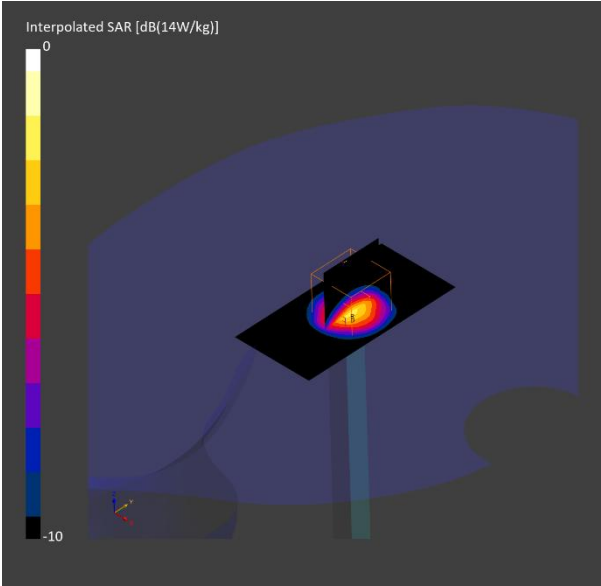

System Performance Check Report for D3900V2 - SN1069

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	3900.000	TSL Permittivity	36.4
Group / UID	CW / 0-	TSL Conductivity [S/m]	3.44
Conversion Factor	6.34	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7651 2026-01-19	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2025-07-09	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.45	6.65
psSAR10g [W/Kg]	2.26	2.48
Power Drift [dB]		-0.06
Dist 3dB Peak [mm]		8.3
M2/M1 [%]		78.1

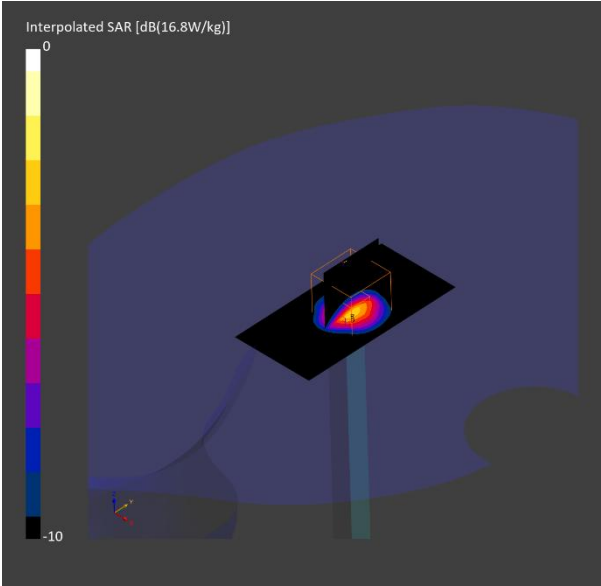

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.000	TSL Permittivity	42.3
Group / UID	CW / 0-	TSL Conductivity [S/m]	0.926
Conversion Factor	9.59	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7651 2026-01-19	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2025-07-09	TSL Type	HBBL-600-10000
Software Version	17.0.2.6775		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.925	0.988
psSAR10g [W/Kg]	0.618	0.649
Power Drift [dB]		-0.02
Dist 3dB Peak [mm]		> 15.0
M2/M1 [%]		89.0

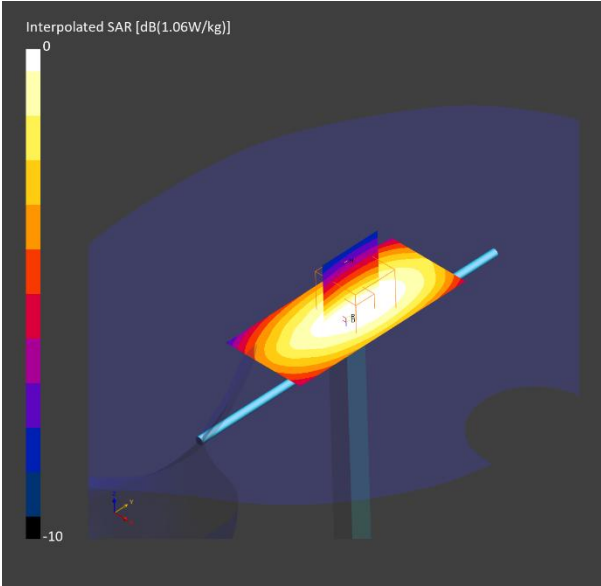

Validation band: CW, FRONT
Room Ambient Temperature: 23.0°C

Exposure Conditions

Band	Validation band	Phantom Section / TSL	5G / Air
Frequency [MHz] / Channel Number	10000.0 / 10000	Test Distance [mm]	10.00
Group / UID	CW / 0--	Conversion Factor	1.0

DASY Configuration

Probe Calibration Date	EUmmWV4 - SN9536_F1-55GHz 2026-02-16	Phantom	mmWave
DAE Calibration Date	DAE4ip Sn1667 2025-09-16	TSL Type	Air
Software Version	3.2.2.2358		

Scan Setup

	Area Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

	5G Scan
Avg. Area [cm²]	4.00
psPDn+ [W/m²]	52.7
psPDtot+ [W/m²]	53.8
psPDmod+ [W/m²]	54.1
E _{max} [V/m]	146
Power Drift [dB]	0.09

