



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No: **D5GHzV2-1191_Sep16**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1191**

Calibration procedure(s) **QA CAL-22.v2**
Calibration procedure for dipole validation kits between 3-6 GHz

BNV
09-28-2016

Calibration date: **September 21, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 3503	30-Jun-16 (No. EX3-3503_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by: **Leif Klysner** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature
Leif Klysner
Katja Pokovic

Issued: September 22, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz $\pm$ 1 MHz 5600 MHz $\pm$ 1 MHz 5750 MHz $\pm$ 1 MHz	

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.5 $\pm$ 6 %	4.59 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.96 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	78.9 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg $\pm$ 19.5 % (k=2)

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.0 ± 6 %	4.93 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.6 W / kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.41 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.8 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.8 ± 6 %	5.08 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5750 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.99 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.4 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.4 ± 6 %	5.52 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.74 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	77.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.17 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.8 ± 6 %	6.00 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.96 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	79.2 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.24 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.2 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.5 ± 6 %	6.21 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5750 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.65 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	76.1 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.14 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.2 W/kg ± 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	55.7 Ω - 4.3 j Ω
Return Loss	- 23.4 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	58.3 Ω - 3.2 j Ω
Return Loss	- 21.8 dB

Antenna Parameters with Head TSL at 5750 MHz

Impedance, transformed to feed point	58.1 Ω + 4.8 j Ω
Return Loss	- 21.2 dB

Antenna Parameters with Body TSL at 5250 MHz

Impedance, transformed to feed point	56.1 Ω - 3.7 j Ω
Return Loss	- 23.4 dB

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	58.9 Ω - 1.7 j Ω
Return Loss	- 21.7 dB

Antenna Parameters with Body TSL at 5750 MHz

Impedance, transformed to feed point	59.5 Ω + 6.9 j Ω
Return Loss	- 19.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.204 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 28, 2003

DASY5 Validation Report for Head TSL

Date: 21.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1191

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz
Medium parameters used: $f = 5250$ MHz; $\sigma = 4.59$ S/m; $\epsilon_r = 34.5$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5600$ MHz; $\sigma = 4.93$ S/m; $\epsilon_r = 34$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5750$ MHz; $\sigma = 5.08$ S/m; $\epsilon_r = 33.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.42, 5.42, 5.42); Calibrated: 30.06.2016, ConvF(4.89, 4.89, 4.89); Calibrated: 30.06.2016, ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.49 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 28.6 W/kg

SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.29 W/kg

Maximum value of SAR (measured) = 18.2 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.34 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 32.9 W/kg

SAR(1 g) = 8.45 W/kg; SAR(10 g) = 2.41 W/kg

Maximum value of SAR (measured) = 20.0 W/kg


Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.15 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 32.3 W/kg


SAR(1 g) = 7.99 W/kg; SAR(10 g) = 2.27 W/kg

Maximum value of SAR (measured) = 19.3 W/kg

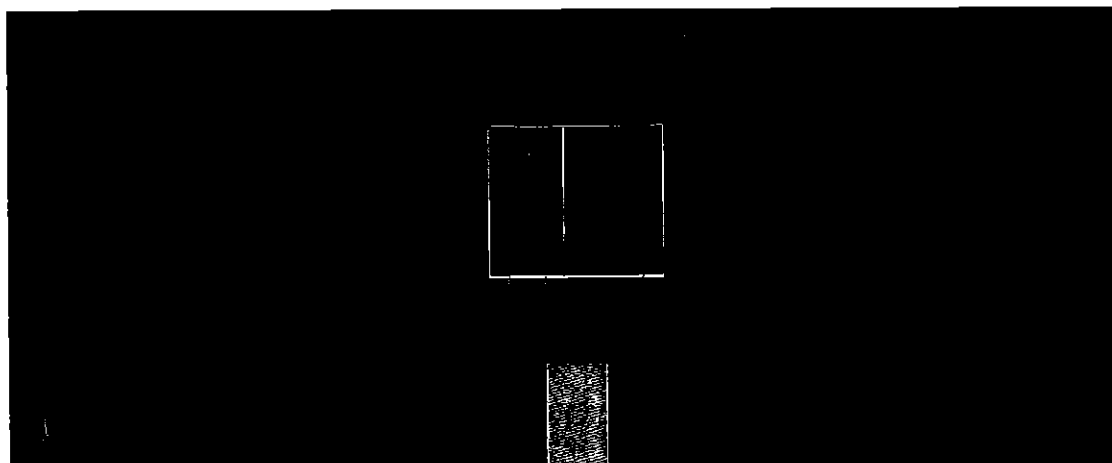

0 dB = 18.2 W/kg = 12.60 dBW/kg

Impedance Measurement Plot for Head TSL

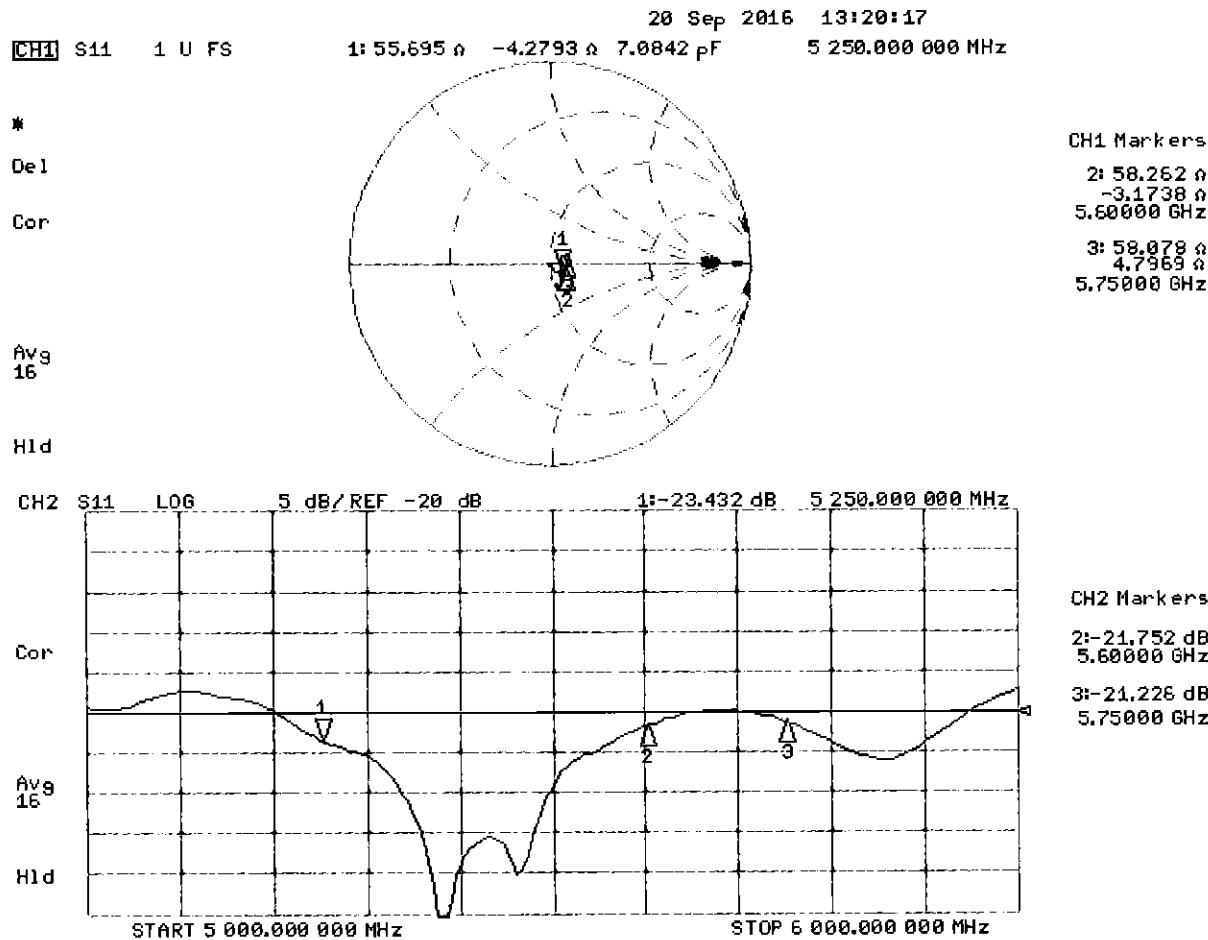

DASY5 Validation Report for Body TSL

Date: 20.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1191

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz
Medium parameters used: $f = 5250$ MHz; $\sigma = 5.52$ S/m; $\epsilon_r = 47.4$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5600$ MHz; $\sigma = 6$ S/m; $\epsilon_r = 46.8$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5750$ MHz; $\sigma = 6.21$ S/m; $\epsilon_r = 46.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016, ConvF(4.35, 4.35, 4.35); Calibrated: 30.06.2016, ConvF(4.3, 4.3, 4.3); Calibrated: 30.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.49 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 29.1 W/kg

SAR(1 g) = 7.74 W/kg; SAR(10 g) = 2.17 W/kg

Maximum value of SAR (measured) = 17.7 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.85 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 32.5 W/kg

SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.24 W/kg

Maximum value of SAR (measured) = 18.8 W/kg



Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.21 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 32.7 W/kg

SAR(1 g) = 7.65 W/kg; SAR(10 g) = 2.14 W/kg

Maximum value of SAR (measured) = 18.5 W/kg

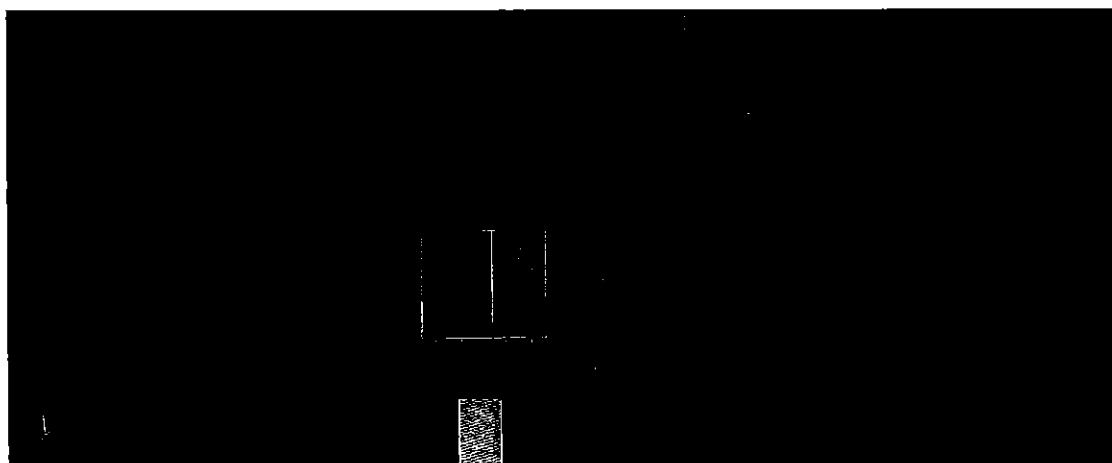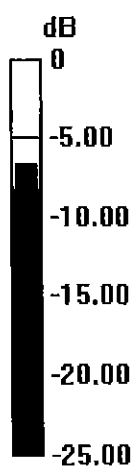


0 dB = 17.7 W/kg = 12.48 dBW/kg

Impedance Measurement Plot for Body TSL

20 Sep 2016 13:19:13
 CH1 S11 1 U FS 1: 56.143 Ω -3.6992 Ω 8.1950 pF 5 250.000 000 MHz


*
 Del
 Cor
 Avg
 16
 H1d

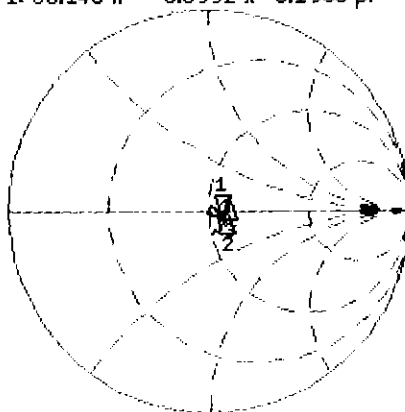

CH1 Markers
 2: 58.887 Ω
 -1.6504 Ω
 5.60000 GHz
 3: 59.510 Ω
 6.9121 Ω
 5.75000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1: -23.406 dB 5 250.000 000 MHz

Cor
 Avg
 16
 H1d

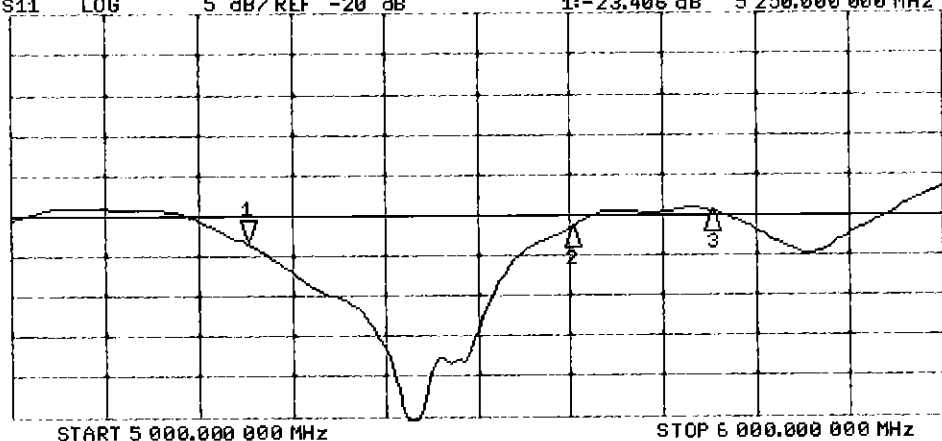

CH2 Markers
 2: -21.616 dB
 5.60000 GHz
 3: -19.400 dB
 5.75000 GHz



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No: **D1765V2-1008_May16**

CALIBRATION CERTIFICATE

Object **D1765V2 - SN:1008**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

*BNV
05/23/16*

Calibration date: **May 11, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	31-Dec-15 (No. EX3-7349_Dec15)	Dec-16
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by: **Michael Weber** Name: **Michael Weber** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

M. Weber

Katja Pokovic

Issued: May 17, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.8 $\pm$ 6 %	1.36 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.10 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.7 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.81 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.3 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.4	1.50 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.8 $\pm$ 6 %	1.50 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.30 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	37.3 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	19.8 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.8 Ω - 6.0 j Ω
Return Loss	- 24.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.8 Ω - 6.8 j Ω
Return Loss	- 21.6 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.211 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 06, 2005

DASY5 Validation Report for Head TSL

Date: 11.05.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1765 MHz; Type: D1765V2; Serial: D1765V2 - SN: 1008

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 39.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.54, 8.54, 8.54); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.4 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 9.1 W/kg; SAR(10 g) = 4.81 W/kg

Maximum value of SAR (measured) = 13.7 W/kg

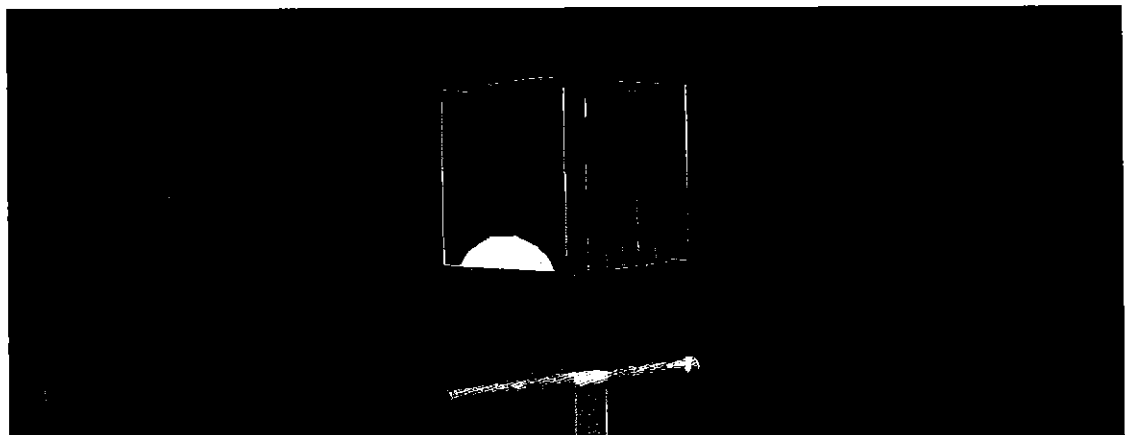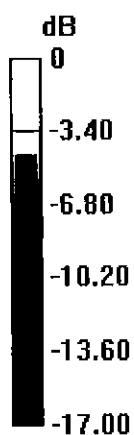

0 dB = 13.7 W/kg = 11.37 dBW/kg

Impedance Measurement Plot for Head TSL

11 May 2016 13:10:14
[CH1] S11 1 U FS 1: 48.842 Ω -6.0117 Ω 15.128 pF 1 750.000 000 MHz


*

De1

Cor

Avg
16

H1d

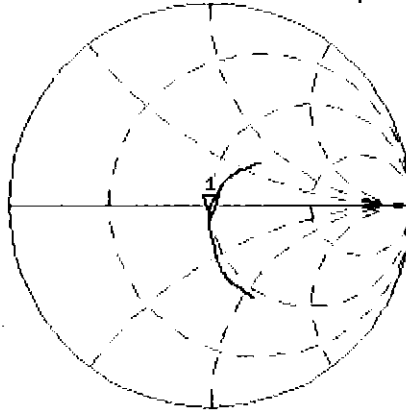


CH2 S11 LOG 5 dB/REF -20 dB 1:-24.177 dB 1 750.000 000 MHz

De1

Cor

Avg
16

H1d

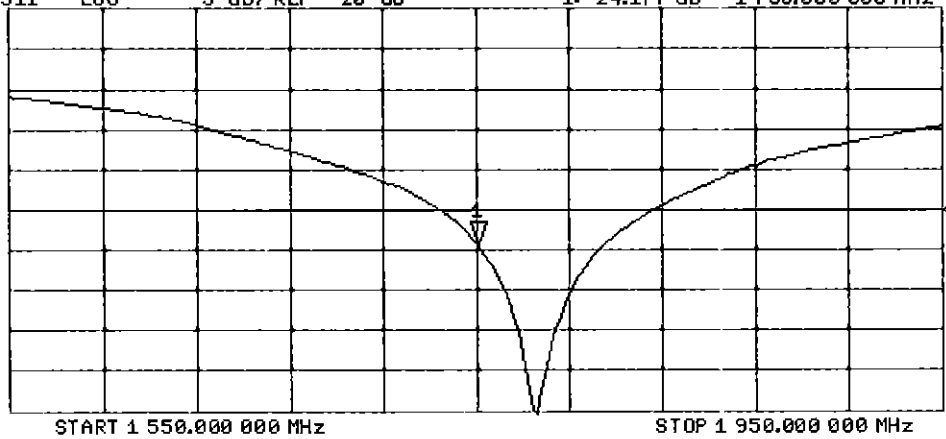

DASY5 Validation Report for Body TSL

Date: 11.05.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1765 MHz; Type: D1765V2; Serial: D1765V2 - SN: 1008

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.5$ S/m; $\epsilon_r = 53.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.25, 8.25, 8.25); Calibrated: 31.12.2015;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 100.9 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 16.4 W/kg

SAR(1 g) = 9.3 W/kg; SAR(10 g) = 4.94 W/kg

Maximum value of SAR (measured) = 14.0 W/kg

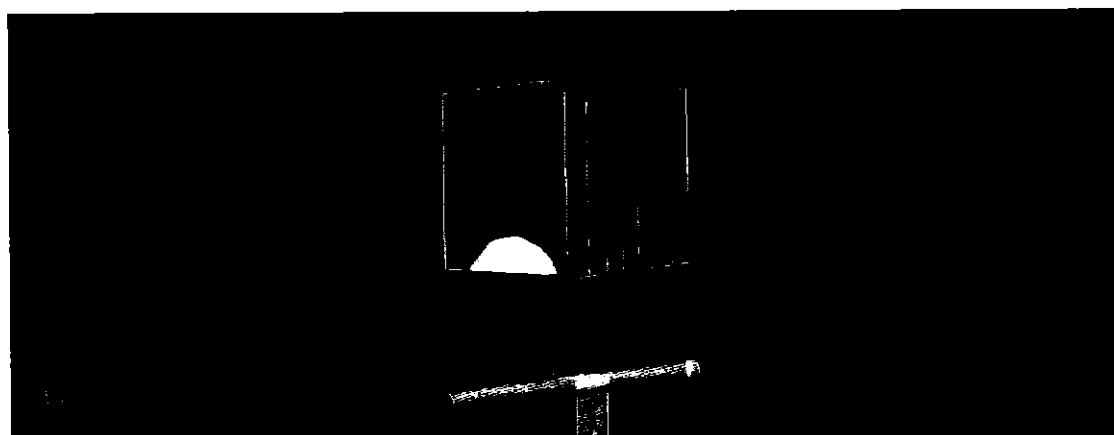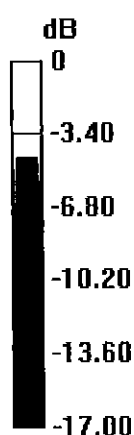


0 dB = 14.0 W/kg = 11.46 dBW/kg

Impedance Measurement Plot for Body TSL

11 May 2016 13:08:31
 [CH1] S11 1 U FS 1: 45.803 Ω -6.7695 Ω 13.435 pF 1 750.000 000 MHz

*
 Del
 Cor

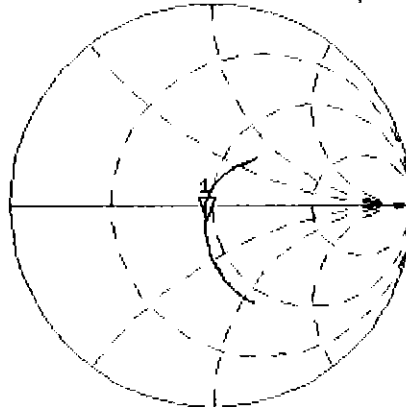

Avg
 16

H1d


CH2 S11 LOG 5 dB/REF -20 dB 1:-21.625 dB 1 750.000 000 MHz

Del

Cor

Avg
 16

H1d

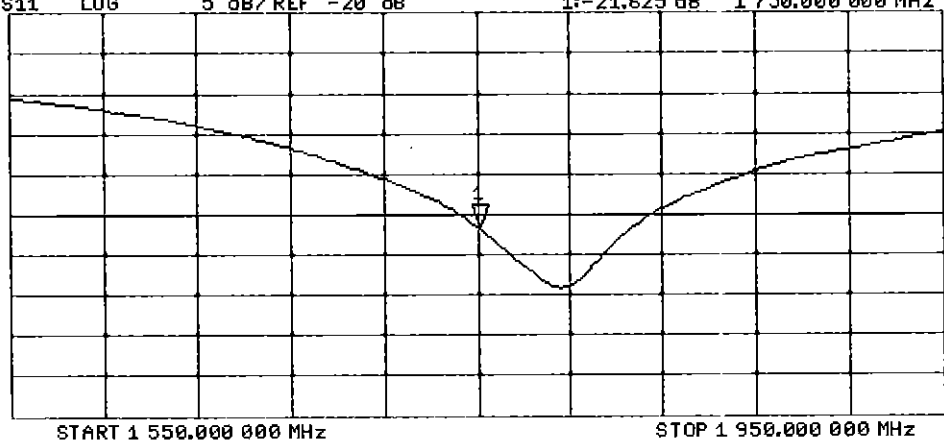



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No: **D2600V2-1071_Sep16**

CALIBRATION CERTIFICATE

Object **D2600V2 - SN:1071**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

BNV
 09-28-2016

Calibration date: **September 13, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	15-Jun-16 (No. EX3-7349_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by: **Jeton Kastrati** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

Issued: September 13, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	37.3 $\pm$ 6 %	2.05 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	56.3 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.3 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.5	2.16 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.1 $\pm$ 6 %	2.22 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	54.2 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.20 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.5 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.9 Ω - 6.7 j Ω
Return Loss	- 23.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.1 Ω - 2.1 j Ω
Return Loss	- 26.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.153 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 17, 2013

DASY5 Validation Report for Head TSL

Date: 13.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1071

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.05$ S/m; $\epsilon_r = 37.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.56, 7.56, 7.56); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 115.1 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 30.4 W/kg

SAR(1 g) = 14.5 W/kg; SAR(10 g) = 6.45 W/kg

Maximum value of SAR (measured) = 24.6 W/kg

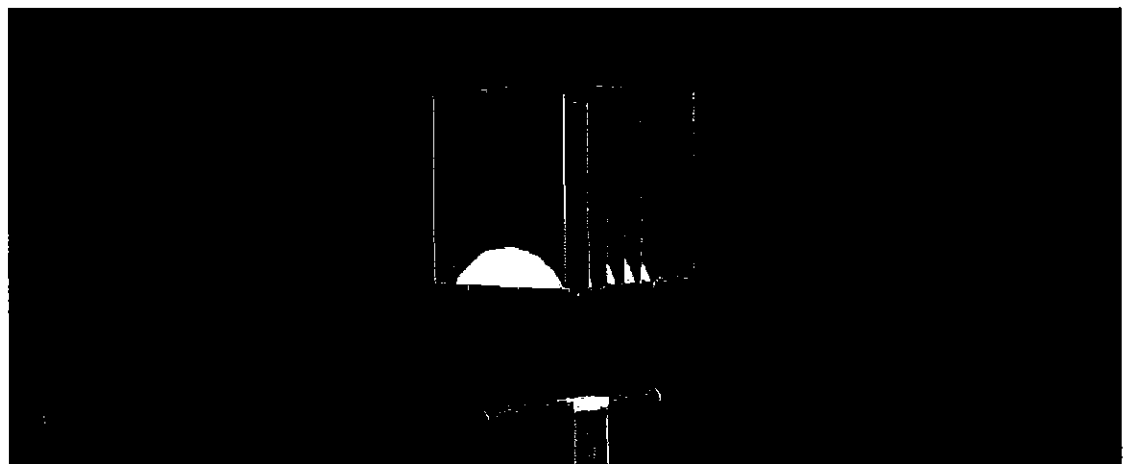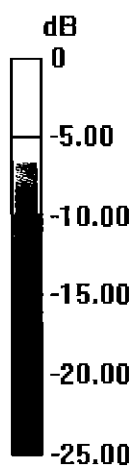


0 dB = 24.6 W/kg = 13.91 dBW/kg

Impedance Measurement Plot for Head TSL

12 Sep 2016 13:13:44
CH1 S11 1 U FS 4: 43.902 Ω -6.6523 Ω 9.2018 pF 2 600.000 000 MHz


*
De l
CA

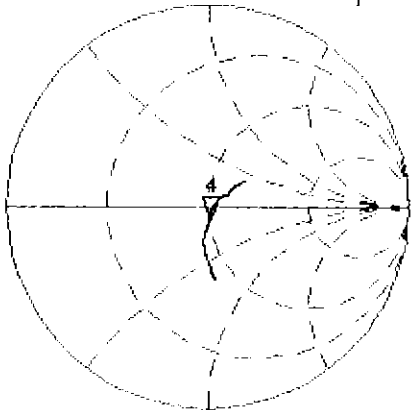

Avg
16
H1 d

CH2 S11 LOG 5 dB/ REF -20 dB 4:-23.548 dB 2 600.000 000 MHz

CA
Avg
16
H1 d

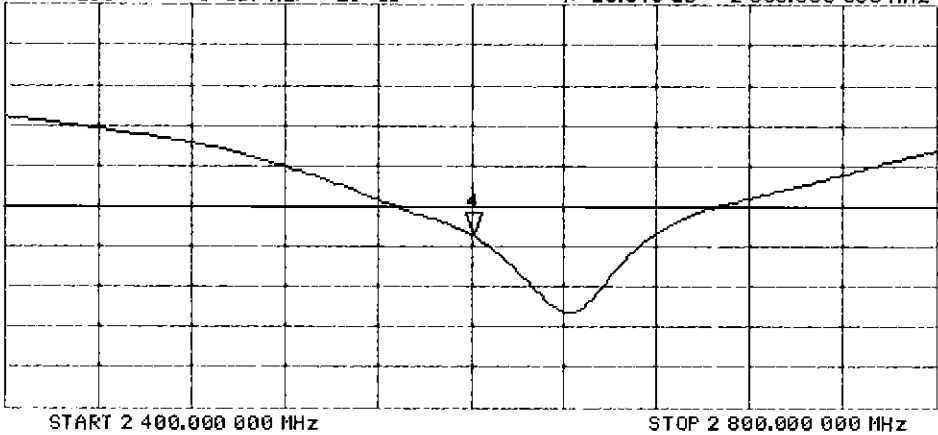

DASY5 Validation Report for Body TSL

Date: 13.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN:1071

Communication System: UID 0 - CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.22$ S/m; $\epsilon_r = 51.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.48, 7.48, 7.48); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.7 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 28.3 W/kg

SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.2 W/kg

Maximum value of SAR (measured) = 23.3 W/kg




0 dB = 23.3 W/kg = 13.67 dBW/kg

Impedance Measurement Plot for Body TSL

12 Sep 2016 13:13:09
[CH1] S11 1 U FS 4: 46.078 Ω -2.0762 Ω 29.484 pF 2 600.000 000 MHz

*
De I
Ca

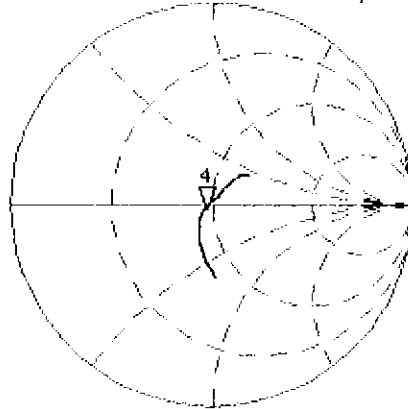

Avg
16


H1 d

CH2 S11 LOG 5 dB/REF -20 dB 4:-26.721 dB 2 600.000 000 MHz

Ca

Avg
16

H1 d

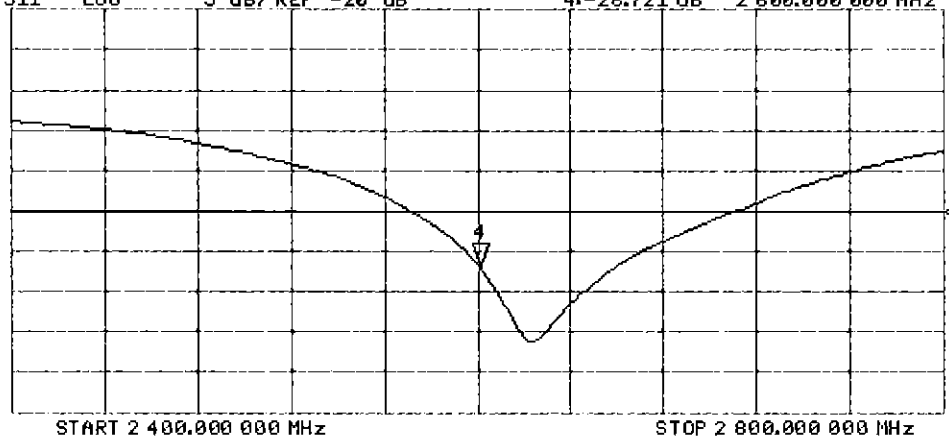



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No: **D5GHzV2-1237_Aug16**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN:1237**

Calibration procedure(s) **QA CAL-22.v2**
Calibration procedure for dipole validation kits between 3-6 GHz

✓PN
8/9/16

Calibration date: **August 02, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 3503	30-Jun-16 (No. EX3-3503_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by: **Claudio Leubler** Name: **Claudio Leubler** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Name: **Katja Pokovic** Function: **Technical Manager**

Signature

Issued: August 4, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz $\pm$ 1 MHz 5600 MHz $\pm$ 1 MHz 5750 MHz $\pm$ 1 MHz	

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.4 $\pm$ 6 %	4.52 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.00 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.2 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.7 W/kg $\pm$ 19.5 % (k=2)

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.9 ± 6 %	4.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.43 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.3 W / kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.42 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.9 W/kg ± 19.5 % (k=2)

Head TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.7 ± 6 %	5.02 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5750 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.25 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.2 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.1 ± 6 %	5.42 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.54 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	74.8 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.12 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.0 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.5 ± 6 %	5.88 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.76 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	77.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.17 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.5 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.2 ± 6 %	6.11 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5750 MHz

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.60 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.4 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.11 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.9 W/kg ± 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	48.6 Ω - 2.5 j Ω
Return Loss	- 30.7 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	50.9 Ω + 1.5 j Ω
Return Loss	- 35.3 dB

Antenna Parameters with Head TSL at 5750 MHz

Impedance, transformed to feed point	53.8 Ω + 5.8 j Ω
Return Loss	- 23.5 dB

Antenna Parameters with Body TSL at 5250 MHz

Impedance, transformed to feed point	47.0 Ω - 3.9 j Ω
Return Loss	- 25.9 dB

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	51.5 Ω + 3.9 j Ω
Return Loss	- 27.7 dB

Antenna Parameters with Body TSL at 5750 MHz

Impedance, transformed to feed point	53.8 Ω + 0.3 j Ω
Return Loss	- 28.6 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.193 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 04, 2015

DASY5 Validation Report for Head TSL

Date: 02.08.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1237

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used: $f = 5250$ MHz; $\sigma = 4.52$ S/m; $\epsilon_r = 34.4$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5600$ MHz; $\sigma = 4.86$ S/m; $\epsilon_r = 33.9$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5750$ MHz; $\sigma = 5.02$ S/m; $\epsilon_r = 33.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.42, 5.42, 5.42); Calibrated: 30.06.2016; ConvF(4.89, 4.89, 4.89); Calibrated: 30.06.2016, ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016,
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 74.10 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 29.5 W/kg

SAR(1 g) = 8 W/kg; SAR(10 g) = 2.3 W/kg

Maximum value of SAR (measured) = 18.3 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.55 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 32.9 W/kg

SAR(1 g) = 8.43 W/kg; SAR(10 g) = 2.42 W/kg

Maximum value of SAR (measured) = 19.7 W/kg


Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 72.23 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 33.6 W/kg

SAR(1 g) = 8.25 W/kg; SAR(10 g) = 2.35 W/kg

Maximum value of SAR (measured) = 18.3 W/kg

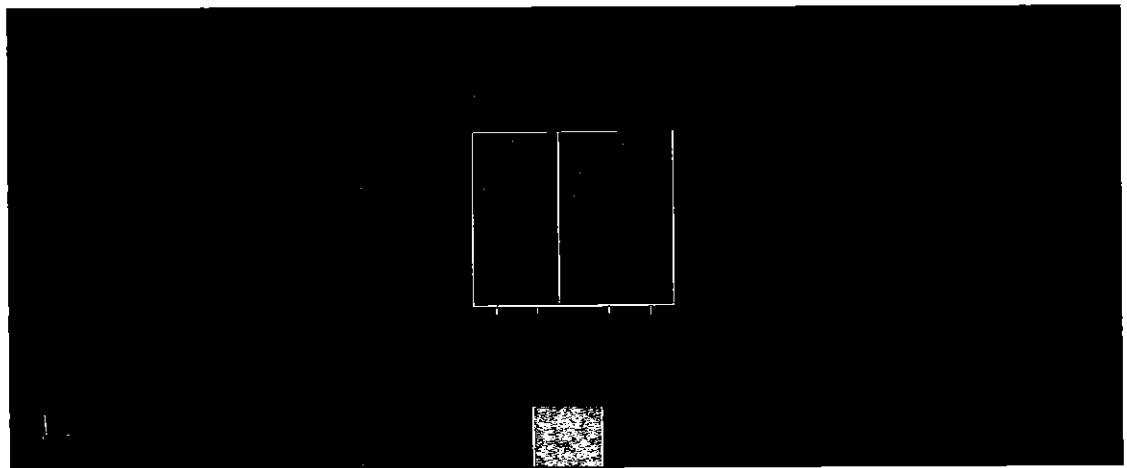


0 dB = 18.3 W/kg = 12.62 dBW/kg

Impedance Measurement Plot for Head TSL

2 Aug 2016 08:52:20
 [CH1] S11 1 U FS 1: 48.623 Ω -2.5332 Ω 11.967 pF 5 250.000 000 MHz


*
 Del
 Cor
 Avg
 16
 H1d

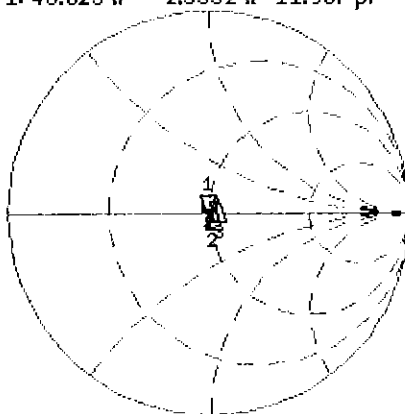

CH1 Markers
 2: 50.867 Ω
 1.4961 Ω
 5.60000 GHz
 3: 53.785 Ω
 5.8164 Ω
 5.75000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1: -30.691 dB 5 250.000 000 MHz

Cor
 Avg
 16
 H1d

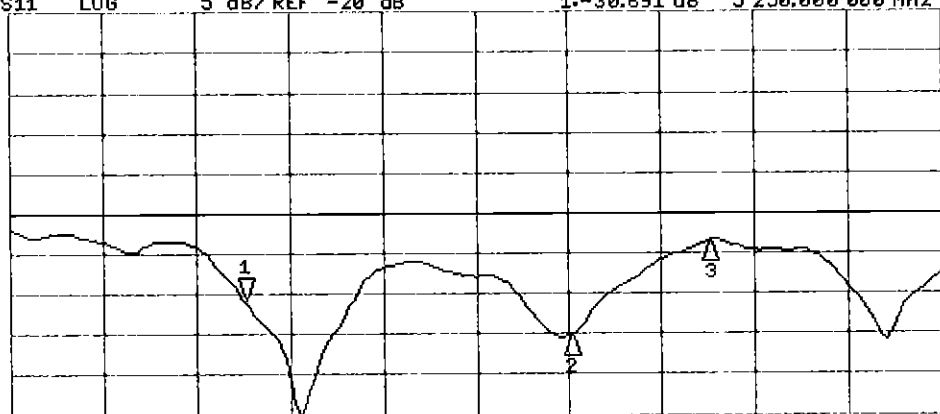

CH2 Markers
 2: -35.297 dB
 5.60000 GHz
 3: -23.501 dB
 5.75000 GHz

DASY5 Validation Report for Body TSL

Date: 02.08.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1237

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used: $f = 5250$ MHz; $\sigma = 5.42$ S/m; $\epsilon_r = 47.1$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5600$ MHz; $\sigma = 5.88$ S/m; $\epsilon_r = 46.5$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5750$ MHz; $\sigma = 6.11$ S/m; $\epsilon_r = 46.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016, ConvF(4.35, 4.35, 4.35); Calibrated: 30.06.2016, ConvF(4.3, 4.3, 4.3); Calibrated: 30.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAB4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.19 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 28.4 W/kg

SAR(1 g) = 7.54 W/kg; SAR(10 g) = 2.12 W/kg

Maximum value of SAR (measured) = 17.3 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.80 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 31.9 W/kg

SAR(1 g) = 7.76 W/kg; SAR(10 g) = 2.17 W/kg

Maximum value of SAR (measured) = 18.3 W/kg



Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.31 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 32.6 W/kg

SAR(1 g) = 7.6 W/kg; SAR(10 g) = 2.11 W/kg

Maximum value of SAR (measured) = 18.4 W/kg

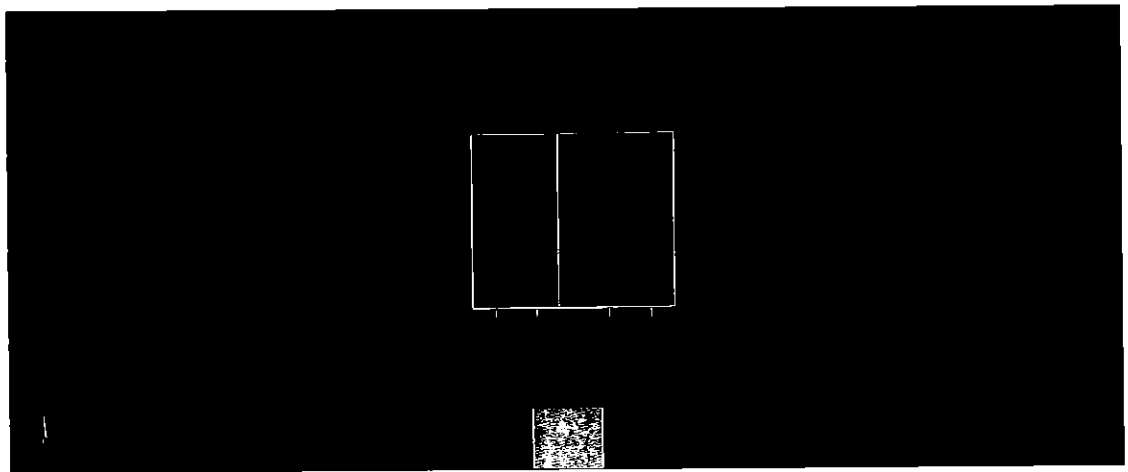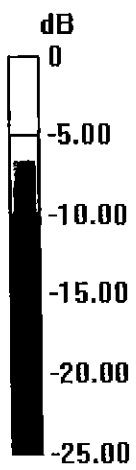


0 dB = 17.3 W/kg = 12.38 dBW/kg

Impedance Measurement Plot for Body TSL

2 Aug 2016 08:49:13
 CH1 S11 1 U FS 1: 46.998 Ω -3.8984 Ω 7.7763 pF 5 250.000 000 MHz


*
 Del
 Cor
 Avg
 16
 H1d

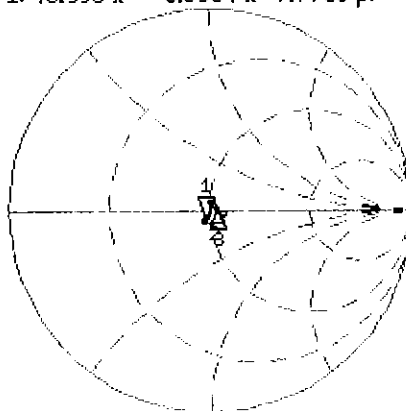

CH1 Markers
 2: 51.525 Ω
 3.8945 Ω
 5.60000 GHz
 3: 53.848 Ω
 0.2930 Ω
 5.75000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1: -25.900 dB 5 250.000 000 MHz

Cor
 Avg
 16
 H1d

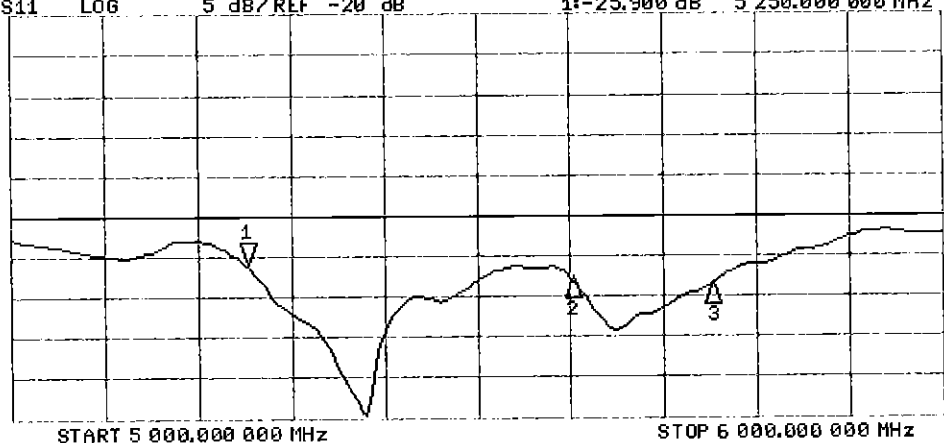

CH2 Markers
 2: -27.699 dB
 5.60000 GHz
 3: -28.596 dB
 5.75000 GHz



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **PC Test**

Certificate No: **D750V3-1003_Jan17**

CALIBRATION CERTIFICATE

Object **D750V3 - SN:1003**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

BNV
01/26/2017

Calibration date: **January 11, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	31-Dec-16 (No. EX3-7349_Dec16)	Dec-17
DAE4	SN: 601	04-Jan-17 (No. DAE4-601_Jan17)	Jan-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by: **Jeton Kastrati** Name Function
Laboratory Technician

Signature
[Signature]

Approved by: **Katja Pokovic** Technical Manager

Issued: January 11, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	41.6 $\pm$ 6 %	0.89 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.10 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.39 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.43 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	54.2 $\pm$ 6 %	0.96 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.21 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.79 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.45 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.78 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.3 Ω - 1.4 j Ω
Return Loss	- 27.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.4 Ω - 6.0 j Ω
Return Loss	- 24.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.034 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	January 21, 2009

DASY5 Validation Report for Head TSL

Date: 11.01.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1003

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.89 \text{ S/m}$; $\epsilon_r = 41.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.17, 10.17, 10.17); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 59.38 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.20 W/kg


SAR(1 g) = 2.1 W/kg; SAR(10 g) = 1.36 W/kg

Maximum value of SAR (measured) = 2.82 W/kg

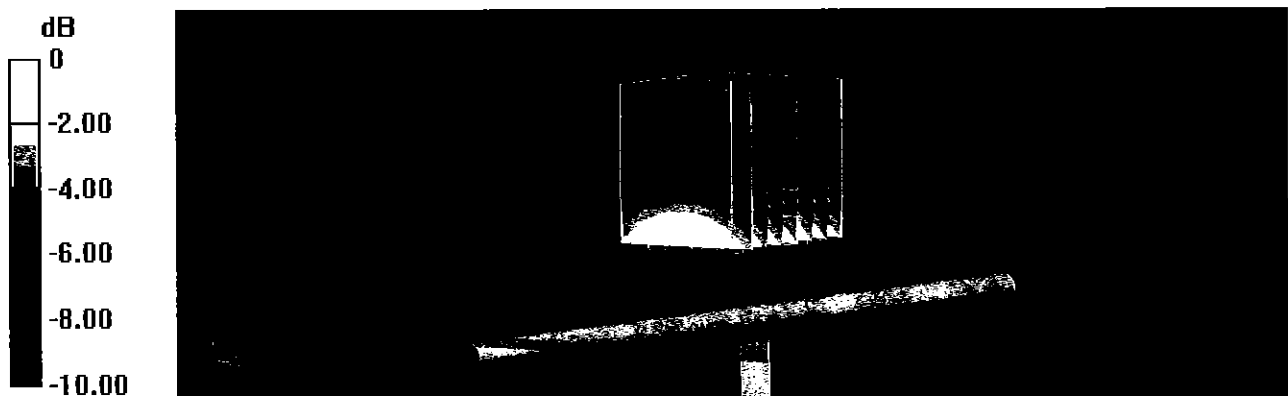

0 dB = 2.82 W/kg = 4.50 dBW/kg

Impedance Measurement Plot for Head TSL

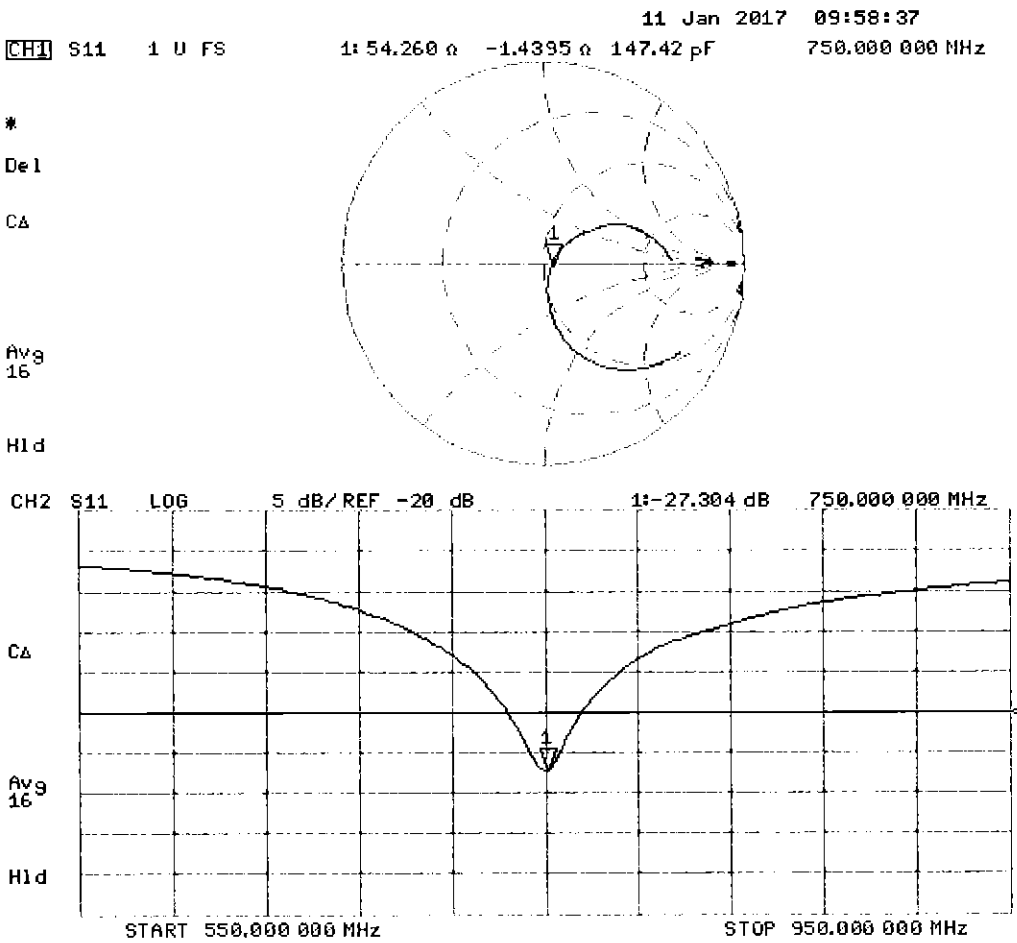

DASY5 Validation Report for Body TSL

Date: 10.01.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1003

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.96 \text{ S/m}$; $\epsilon_r = 54.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.99, 9.99, 9.99); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.01.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 58.22 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 3.40 W/kg

SAR(1 g) = 2.21 W/kg; SAR(10 g) = 1.45 W/kg

Maximum value of SAR (measured) = 2.98 W/kg

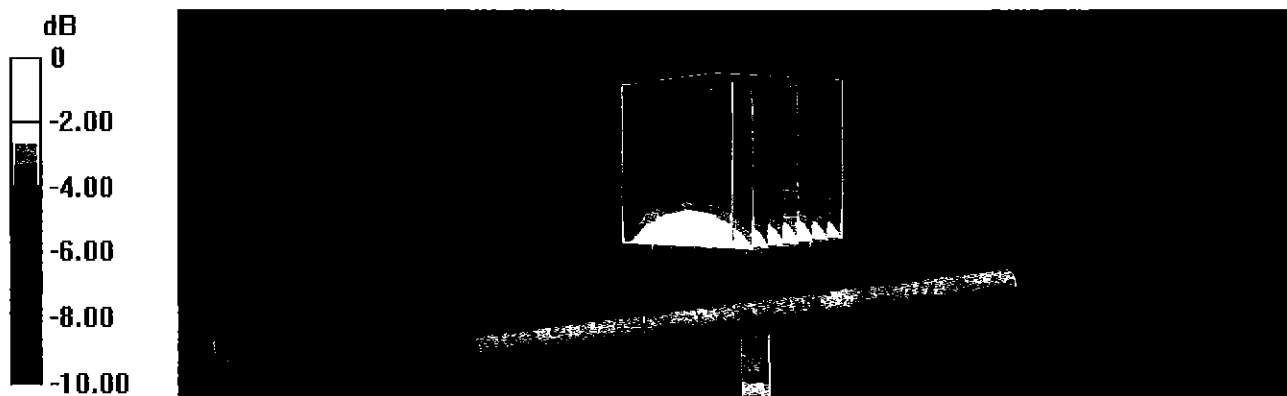

Impedance Measurement Plot for Body TSL

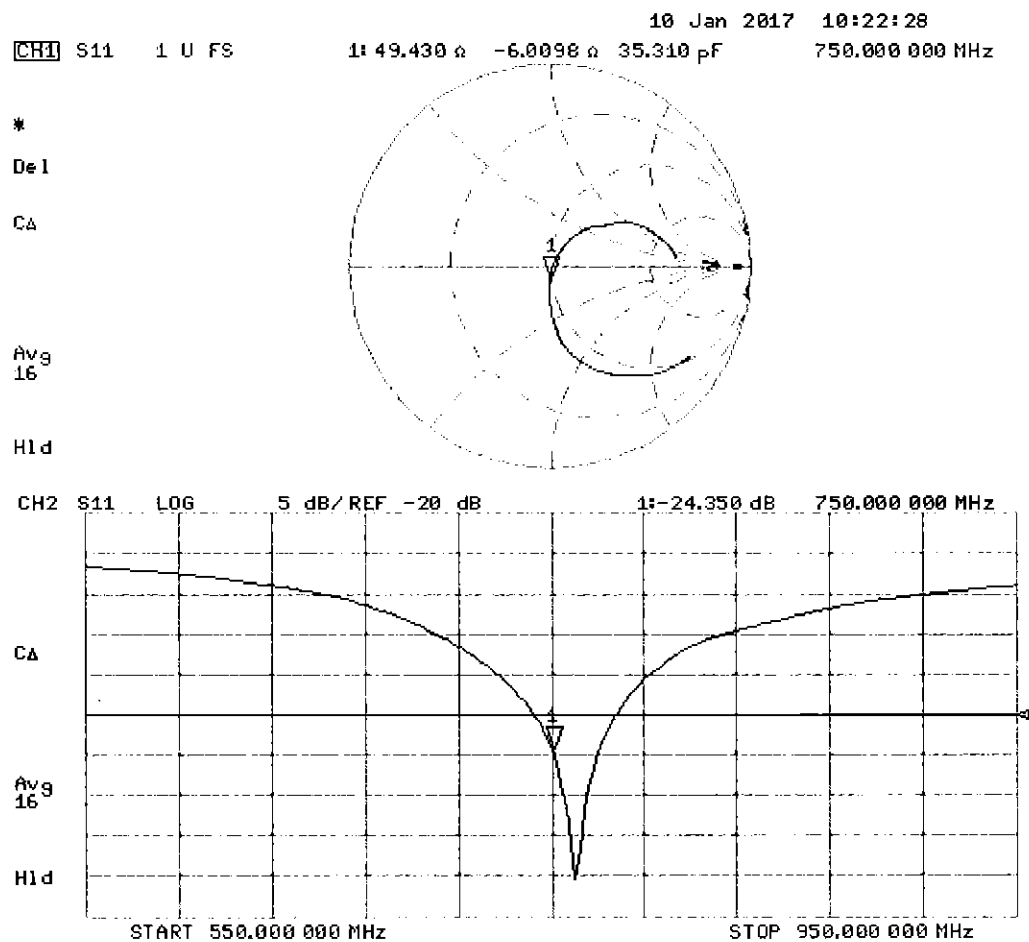

APPENDIX D: SAR TISSUE SPECIFICATIONS

Measurement Procedure for Tissue verification:

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity ϵ' can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\epsilon_r\epsilon_0}{[\ln(b/a)]^2} \int_a^b \int_a^b \int_0^\pi \cos\phi' \frac{\exp[-j\omega r(\mu_0\epsilon_r'\epsilon_0)^{1/2}]}{r} d\phi' d\rho' d\rho$$

where Y is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$, ω is the angular frequency, and $j = \sqrt{-1}$.

Table D-I
Composition of the Tissue Equivalent Matter

Frequency (MHz)	750	750	835	835	1750	1750	1900	1900	2300-2600	2300-2600	5200-5800	5200-5800
Tissue	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Ingredients (% by weight)												
Bactericide	See page 2-3	See page 2	0.1	0.1					See page 4		See page 5	
DGBE					47	31	44.92	29.44		26.7		
HEC			1	1								
NaCl			1.45	0.94	0.4	0.2	0.18	0.39		0.1		
Sucrose			57	44.9								20
Polysorbate (Tween) 80												
Water			40.45	53.06	52.6	68.8	54.9	70.17		73.2		80

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset	APPENDIX D: Page 1 of 5		

2 Composition / Information on ingredients

The Item is composed of the following ingredients:

H ₂ O	Water, 35 – 58%
Sucrose	Sugar, white, refined, 40 – 60%
NaCl	Sodium Chloride, 0 – 6%
Hydroxyethyl-cellulose	Medium Viscosity (CAS# 9004-62-0), <0.3%
Preventol-D7	Preservative: aqueous preparation, (CAS# 55965-84-9), containing 5-chloro-2-methyl-3(2H)-isothiazolone and 2-methyl-3(2H)-isothiazolone, 0.1 – 0.7%
Relevant for safety; Refer to the respective Safety Data Sheet*.	

Figure D-1

Composition of 750 MHz Head and Body Tissue Equivalent Matter

Note: 750MHz liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL750V2)
Product No.	SL AAM 075 AA (Charge: 150223-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	25-Feb-15
Operator	IEN

Additional Information

TSL Density	1.212 g/cm ³
TSL Heat-capacity	3.006 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
600	57.3	24.76	0.83	56.1	0.95	2.2	-13.2
625	57.1	24.43	0.85	56.0	0.95	1.8	-11.0
650	56.8	24.09	0.87	55.9	0.96	1.5	-8.8
675	56.5	23.80	0.89	55.8	0.96	1.2	-6.7
700	56.2	23.51	0.92	55.7	0.96	0.9	-4.6
725	56.0	23.28	0.94	55.6	0.96	0.6	-2.4
750	55.7	23.06	0.96	55.5	0.96	0.4	-0.1
775	55.5	22.87	0.99	55.4	0.97	0.1	2.1
800	55.2	22.68	1.01	55.3	0.97	-0.2	4.4
825	55.0	22.52	1.03	55.2	0.98	-0.5	5.7
838	54.9	22.44	1.05	55.2	0.98	-0.6	6.3
850	54.8	22.36	1.06	55.2	0.99	-0.7	7.0
875	54.5	22.24	1.08	55.1	1.02	-1.0	6.2
900	54.3	22.12	1.11	55.0	1.05	-1.3	5.5
925	54.1	22.01	1.13	55.0	1.06	-1.6	6.5
950	53.9	21.89	1.16	54.9	1.08	-2.0	7.6
975	53.6	21.81	1.18	54.9	1.09	-2.3	8.8
1000	53.4	21.73	1.21	54.8	1.10	-2.7	10.1

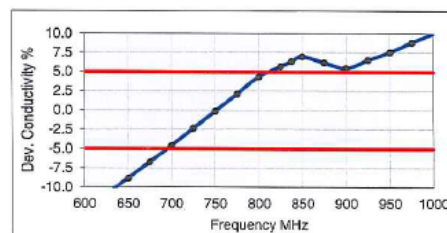
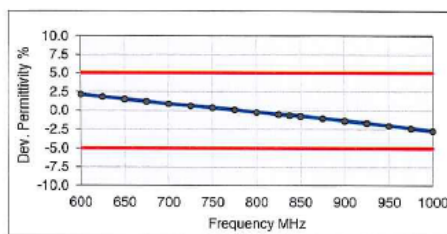


Figure D-2
750MHz Body Tissue Equivalent Matter

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset			APPENDIX D: Page 2 of 5

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL750V2)
Product No.	SL AAH 075 AA (Charge: 150213-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	18-Feb-15
Operator	IEN

Additional Information

TSL Density	1.284 g/cm ³
TSL Heat-capacity	2.701 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
600	44.6	22.42	0.75	42.7	0.88	4.5	-15.1
625	44.3	22.20	0.77	42.6	0.88	3.9	-12.7
650	43.9	21.98	0.79	42.5	0.89	3.3	-10.3
675	43.5	21.75	0.82	42.3	0.89	2.8	-8.0
700	43.1	21.53	0.84	42.2	0.89	2.2	-5.7
725	42.8	21.36	0.86	42.1	0.89	1.8	-3.3
750	42.5	21.22	0.89	41.9	0.89	1.3	-0.9
775	42.2	21.06	0.91	41.8	0.90	0.8	1.4
800	41.8	20.90	0.93	41.7	0.90	0.3	3.7
825	41.5	20.77	0.95	41.6	0.91	-0.2	5.1
838	41.4	20.71	0.96	41.5	0.91	-0.4	5.8
850	41.2	20.65	0.98	41.5	0.92	-0.7	6.6
875	40.9	20.53	1.00	41.5	0.94	-1.4	6.0
900	40.6	20.42	1.02	41.5	0.97	-2.1	5.4
925	40.4	20.32	1.05	41.5	0.98	-2.6	6.5
950	40.1	20.22	1.07	41.4	0.99	-3.2	7.5
975	39.8	20.14	1.09	41.4	1.00	-3.8	8.7
1000	39.5	20.05	1.12	41.3	1.01	-4.3	9.9

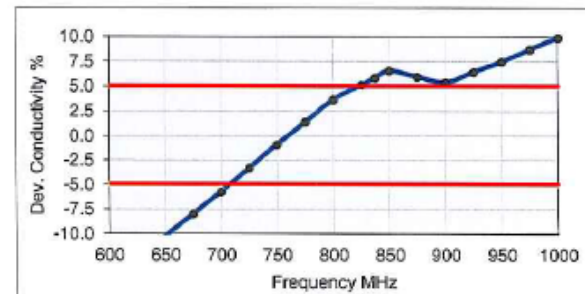
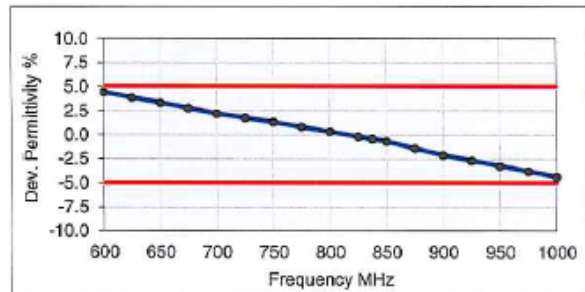


Figure D-3
750MHz Head Tissue Equivalent Matter

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset			APPENDIX D: Page 3 of 5

2 Composition / Information on ingredients

The Item is composed of the following ingredients:

H ₂ O	Water, 52 – 75%
C ₈ H ₁₈ O ₃	Diethylene glycol monobutyl ether (DGBE), 25 – 48% (CAS-No. 112-34-5, EC-No. 203-961-6, EC-index-No. 603-096-00-8) Relevant for safety; Refer to the respective Safety Data Sheet*.
NaCl	Sodium Chloride, <1.0%

Figure D-4

Composition of 2300-2600 GHz Head Tissue Equivalent Matter

Note: 2300-2600 GHz head liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL2450V2)
Product No.	SL AAH 245 BA (Charge: 150206-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	23°C
Test Date	11-Feb-15
Operator	IEN

Additional Information

TSL Density	0.988 g/cm ³
TSL Heat-capacity	3.680 kJ/(kg·K)

f (MHz)	Measured			Target		Diff. to Target (%)	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
1900	40.4	11.89	1.26	40.0	1.40	1.0	-10.2
1925	40.3	11.98	1.28	40.0	1.40	0.7	-8.3
1950	40.2	12.07	1.31	40.0	1.40	0.4	-6.4
1975	40.1	12.15	1.34	40.0	1.40	0.2	-4.6
2000	40.0	12.23	1.36	40.0	1.40	-0.1	-2.8
2025	39.9	12.32	1.39	40.0	1.42	-0.2	-2.4
2050	39.8	12.41	1.42	39.9	1.44	-0.3	-2.0
2075	39.7	12.50	1.44	39.9	1.47	-0.4	-1.6
2100	39.6	12.59	1.47	39.8	1.49	-0.5	-1.2
2125	39.5	12.66	1.50	39.8	1.51	-0.7	-0.9
2150	39.4	12.73	1.52	39.7	1.53	-0.8	-0.7
2175	39.3	12.83	1.55	39.7	1.56	-0.9	-0.2
2200	39.2	12.92	1.58	39.6	1.58	-1.1	0.2
2225	39.1	13.00	1.61	39.6	1.60	-1.2	0.6
2250	39.0	13.08	1.64	39.6	1.62	-1.3	0.9
2275	38.9	13.17	1.67	39.5	1.64	-1.5	1.4
2300	38.8	13.26	1.70	39.5	1.67	-1.7	1.8
2325	38.7	13.34	1.73	39.4	1.69	-1.8	2.2
2350	38.6	13.42	1.75	39.4	1.71	-2.0	2.5
2375	38.5	13.50	1.78	39.3	1.73	-2.1	2.9
2400	38.4	13.58	1.81	39.3	1.76	-2.3	3.3
2425	38.3	13.65	1.84	39.2	1.78	-2.4	3.6
2450	38.2	13.73	1.87	39.2	1.80	-2.6	3.9
2475	38.1	13.80	1.90	39.2	1.83	-2.8	4.0
2500	38.0	13.87	1.93	39.1	1.85	-3.0	4.0
2525	37.9	13.90	1.95	39.1	1.88	-3.1	3.8
2550	37.8	13.93	1.98	39.1	1.91	-3.2	3.5
2575	37.7	14.05	2.01	39.0	1.94	-3.5	4.0
2600	37.6	14.17	2.05	39.0	1.96	-3.7	4.4
2625	37.4	14.23	2.08	39.0	1.99	-3.9	4.4
2650	37.3	14.29	2.11	38.9	2.02	-4.1	4.4
2675	37.2	14.37	2.14	38.9	2.05	-4.3	4.6
2700	37.1	14.45	2.17	38.9	2.07	-4.5	4.7

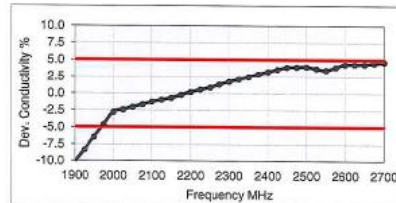
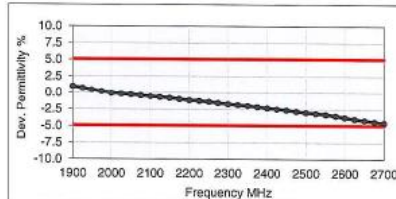


Figure D-5

2300-2600 GHz Head Tissue Equivalent Matter

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset			APPENDIX D: Page 4 of 5

2 Composition / Information on ingredients

The Item is composed of the following ingredients:

Water	50 – 65%
Mineral oil	10 – 30%
Emulsifiers	8 – 25%
Sodium salt	0 – 1.5%

Figure D-6

Composition of 5 GHz Head Tissue Equivalent Matter

Note: 5GHz head liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HBBL3500-5800V5)
Product No.	SL AAH 502 AE (Charge: 141104-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	25-Feb-15
Operator	IEN

Additional Information

TSL Density	0.985 g/cm ³
TSL Heat-capacity	3.383 kJ/(kg*K)

f [MHz]	Measured			Target			Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Delta-eps	Delta-sigma	
3400	38.5	15.11	2.86	38.0	2.81	1.2	1.8	
3500	38.4	15.08	2.94	37.9	2.91	1.2	0.9	
3600	38.2	15.07	3.02	37.8	3.02	1.0	0.2	
3700	38.1	15.05	3.10	37.7	3.12	1.1	-0.6	
3800	38.0	15.04	3.18	37.6	3.22	1.1	-1.2	
3900	37.9	15.05	3.27	37.5	3.32	1.1	-1.6	
4000	37.8	15.07	3.35	37.4	3.43	1.2	-2.2	
4100	37.6	15.09	3.44	37.2	3.53	1.0	-2.5	
4200	37.5	15.14	3.54	37.1	3.63	1.0	-2.5	
4300	37.4	15.18	3.63	37.0	3.73	1.0	-2.7	
4400	37.3	15.24	3.73	36.9	3.84	1.1	-2.7	
4500	37.1	15.29	3.83	36.8	3.94	0.9	-2.7	
4600	37.0	15.37	3.93	36.7	4.04	0.9	-2.7	
4700	36.8	15.42	4.03	36.6	4.14	0.7	-2.7	
4800	36.7	15.47	4.13	36.4	4.25	0.7	-2.7	
4850	36.6	15.50	4.18	36.4	4.30	0.6	-2.7	
4900	36.5	15.54	4.24	36.3	4.35	0.5	-2.5	
4950	36.5	15.55	4.28	36.3	4.40	0.6	-2.7	
5000	36.4	15.59	4.34	36.2	4.45	0.5	-2.5	
5050	36.3	15.62	4.39	36.2	4.50	0.4	-2.5	
5100	36.2	15.66	4.44	36.1	4.55	0.3	-2.5	
5150	36.2	15.67	4.49	36.0	4.60	0.4	-2.5	
5200	36.1	15.71	4.55	36.0	4.66	0.3	-2.3	
5250	36.0	15.73	4.59	35.9	4.71	0.2	-2.5	
5300	35.9	15.76	4.65	35.9	4.76	0.1	-2.3	
5350	35.9	15.78	4.70	35.8	4.81	0.2	-2.3	
5400	35.8	15.81	4.75	35.8	4.86	0.1	-2.3	
5450	35.7	15.82	4.80	35.7	4.91	0.0	-2.3	
5500	35.6	15.84	4.85	35.6	4.96	-0.1	-2.3	
5550	35.6	15.87	4.90	35.6	5.01	0.0	-2.3	
5600	35.5	15.90	4.95	35.5	5.07	-0.1	-2.3	
5650	35.4	15.94	5.01	35.5	5.12	-0.2	-2.1	
5700	35.4	15.96	5.06	35.4	5.17	0.0	-2.1	
5750	35.3	16.00	5.12	35.4	5.22	-0.2	-1.9	
5800	35.2	16.01	5.16	35.3	5.27	-0.3	-2.1	
5850	35.1	16.04	5.22	35.3	5.34	-0.6	-2.2	
5900	35.1	16.06	5.27	35.3	5.40	-0.6	-2.4	

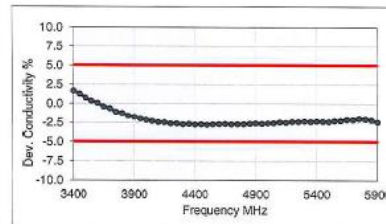
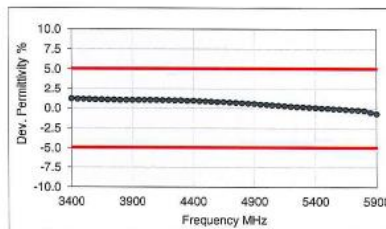


Figure D-7

5GHz Head Tissue Equivalent Matter

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset			APPENDIX D: Page 5 of 5

APPENDIX E: SAR SYSTEM VALIDATION

Per FCC KDB Publication 865664 D02v01r02, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in FCC KDB Publication 865664 D01v01r04 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

Table E-I
SAR System Validation Summary – 1 g

SAR SYSTEM #	FREQ. [MHz]	DATE	PROBE SN	PROBE TYPE	PROBE CAL. POINT		COND.	PERM.	CW VALIDATION			MOD. VALIDATION		
							(σ)	(ε)	SENSITIVITY	PROBE LINEARITY	PROBE ISOTROPY	MOD. TYPE	DUTY FACTOR	PAR
J	750	3/9/2016	3318	ES3DV3	750	Head	0.909	43.100	PASS	PASS	PASS	N/A	N/A	N/A
J	750	2/2/2017	3334	ES3DV3	750	Head	0.895	41.120	PASS	PASS	PASS	N/A	N/A	N/A
H	835	4/7/2016	3319	ES3DV3	835	Head	0.914	42.395	PASS	PASS	PASS	GMSK	PASS	N/A
D	1750	5/19/2016	3213	ES3DV3	1750	Head	1.412	39.009	PASS	PASS	PASS	N/A	N/A	N/A
I	1750	1/12/2017	3209	ES3DV3	1750	Head	1.342	39.160	PASS	PASS	PASS	N/A	N/A	N/A
J	1900	3/11/2016	3318	ES3DV3	1900	Head	1.405	39.979	PASS	PASS	PASS	GMSK	PASS	N/A
F	1900	10/9/2016	3332	ES3DV3	1900	Head	1.430	38.937	PASS	PASS	PASS	GMSK	PASS	N/A
G	2300	9/28/2016	3287	ES3DV3	2300	Head	1.702	38.385	PASS	PASS	PASS	N/A	N/A	N/A
G	2450	9/28/2016	3287	ES3DV3	2450	Head	1.875	37.737	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
J	5250	4/25/2016	7357	EX3DV4	5250	Head	4.508	34.565	PASS	PASS	PASS	OFDM	N/A	PASS
J	5600	4/25/2016	7357	EX3DV4	5600	Head	4.852	34.028	PASS	PASS	PASS	OFDM	N/A	PASS
J	5750	4/25/2016	7357	EX3DV4	5750	Head	5.021	33.850	PASS	PASS	PASS	OFDM	N/A	PASS
F	750	10/10/2016	3332	ES3DV3	750	Body	0.966	55.020	PASS	PASS	PASS	N/A	N/A	N/A
J	750	3/9/2016	3318	ES3DV3	750	Body	0.956	53.115	PASS	PASS	PASS	N/A	N/A	N/A
H	835	4/7/2016	3319	ES3DV3	835	Body	1.000	54.246	PASS	PASS	PASS	GMSK	PASS	N/A
I	1750	12/19/2016	3209	ES3DV3	1750	Body	1.503	51.815	PASS	PASS	PASS	N/A	N/A	N/A
K	1900	5/24/2016	7409	EX3DV4	1900	Body	1.583	51.303	PASS	PASS	PASS	GMSK	PASS	N/A
J	1900	2/3/2017	3334	ES3DV3	1900	Body	1.561	51.227	PASS	PASS	PASS	GMSK	PASS	N/A
E	2300	4/28/2016	7406	EX3DV4	2300	Body	1.811	52.213	PASS	PASS	PASS	N/A	N/A	N/A
E	2450	4/27/2016	7406	EX3DV4	2450	Body	2.016	51.629	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
H	2450	4/6/2016	3319	ES3DV3	2450	Body	2.023	51.922	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
E	2600	4/29/2016	7406	EX3DV4	2600	Body	2.225	50.688	PASS	PASS	PASS	TDD	PASS	N/A
D	5250	3/1/2016	3914	EX3DV4	5250	Body	5.438	47.912	PASS	PASS	PASS	OFDM	N/A	PASS
D	5600	3/1/2016	3914	EX3DV4	5600	Body	5.895	47.321	PASS	PASS	PASS	OFDM	N/A	PASS
D	5750	3/1/2016	3914	EX3DV4	5750	Body	6.111	47.085	PASS	PASS	PASS	OFDM	N/A	PASS

Table E-II
SAR System Validation Summary – 10 g

SAR SYSTEM #	FREQ. [MHz]	DATE	PROBE SN	PROBE TYPE	PROBE CAL.	POINT	COND.	PERM.	CW VALIDATION			MOD. VALIDATION		
							(σ)	(ε)	SENSITIVITY	PROBE LINEARITY	PROBE ISOTROPY	MOD. TYPE	DUTY FACTOR	PAR
I	1750	12/19/2016	3209	ES3DV3	1750	Body	1.503	51.815	PASS	PASS	PASS	N/A	N/A	N/A
K	1900	5/24/2016	7409	EX3DV4	1900	Body	1.583	51.303	PASS	PASS	PASS	GMSK	PASS	N/A
E	2300	4/28/2016	7406	EX3DV4	2300	Body	1.811	52.213	PASS	PASS	PASS	N/A	N/A	N/A
E	2450	4/27/2016	7406	EX3DV4	2450	Body	2.016	51.629	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
D	5250	3/1/2016	3914	EX3DV4	5250	Body	5.438	47.912	PASS	PASS	PASS	OFDM	N/A	PASS
D	5600	3/1/2016	3914	EX3DV4	5600	Body	5.895	47.321	PASS	PASS	PASS	OFDM	N/A	PASS

NOTE: While the probes have been calibrated for both CW and modulated signals, all measurements were performed using communication systems calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r04 for scenarios when CW probe calibrations are used with other signal types. SAR systems were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to FCC KDB Publication 865664 D01v01r04.

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset	APPENDIX E: Page 1 of 1		

APPENDIX G: CONDUCTED POWERS FOR 4X4 DL MIMO

This device supports downlink 4x4 MIMO operations for LTE Bands 2, 4, 25 and 66 only. Uplink transmission is limited to a single output stream. Power measurements were performed with downlink 4x4 MIMO active for the configuration with highest measured maximum conducted power with 4x4 downlink MIMO inactive measured among the channel bandwidth, modulation, and RB combinations in each frequency band.

Per FCC Guidance, SAR for downlink 4x4 MIMO was not needed since the maximum average output power in 4x4 downlink MIMO mode was not > 0.25 dB higher than the maximum output power with downlink 4x4 MIMO inactive. When carrier aggregation is applicable, power measurements were performed with the downlink carrier aggregation and 4x4 DL MIMO active for the configuration with highest measured maximum conducted power with downlink carrier aggregation inactive measured among the channel bandwidth, modulation, and RB combinations in each frequency band.

Note: Per FCC guidance LTE Band 66 SISO powers were used to select measurement configurations for LTE Band 4 and LTE B25 SISO powers were used to select measurement configurations for LTE Band 2.

G.1 Single Carrier 4x4 Downlink MIMO

Table G-1
Additional Maximum Output Powers

LTE Band	Bandwidth [MHz]	Channel	Frequency [MHz]	Modulation	RB Size	RB Offset	4x4 DL MIMO Tx. Power [dBm]	Single Antenna Tx. Power [dBm]	Target Power [dBm]
2	15	19125	1902.5	QPSK	1	0	23.20	23.54	24.0
25	15	26615	1907.5	QPSK	1	0	23.15	23.54	24.0
4	20	20300	1745.0	QPSK	1	0	24.45	24.85	24.5
66	20	132322	1745	QPSK	1	0	24.90	24.85	24.5

Table G-2
Additional Hotspot Reduced Output Powers

LTE Band	Bandwidth [MHz]	Channel	Frequency [MHz]	Modulation	RB Size	RB Offset	4x4 DL MIMO Tx. Power [dBm]	Single Antenna Tx. Power [dBm]	Target Power [dBm]
2	20	19100	1900	64QAM	1	0	20.43	20.50	20.0
25	20	26590	1905	64QAM	1	0	20.40	20.50	20.0
4	20	20050	1720	QPSK	50	0	20.75	20.79	20.5
66	20	132072	1720	QPSK	50	0	20.76	20.79	20.5

Table G-3
Additional Grip Sensor Reduced Output Powers

LTE Band	Bandwidth [MHz]	Channel	Frequency [MHz]	Modulation	RB Size	RB Offset	4x4 DL MIMO Tx. Power [dBm]	Single Antenna Tx. Power [dBm]	Target Power [dBm]
2	20	19100	1900	16QAM	1	0	22.31	22.32	22.0
25	20	26590	1905	16QAM	1	0	22.30	22.32	22.0
4	20	20300	1745.0	16QAM	1	0	22.40	22.50	22.0
66	20	132572	1770.0	16QAM	1	0	22.39	22.50	22.0

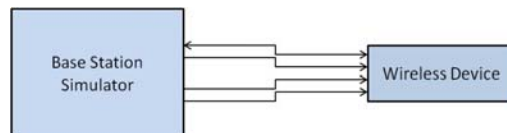


Figure G-1
Power Measurement Setup

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset			APPENDIX G: Page 1 of 4

G.2 Carrier Aggregation Scenarios with 2 Component Carriers with 4x4 Downlink MIMO

Table G-4
Additional Maximum Output Powers – 2 Component Carriers

PCC										SCC					Power	
PCC Band	PCC Bandwidth [MHz]	PCC (UL) Channel	PCC (UL) Frequency [MHz]	Modulation	PCC UL# RB	PCC UL RB Offset	PCC (DL) Channel	PCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	23.15	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	23.16	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	23.19	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	23.19	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	23.09	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	23.18	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	23.16	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B66	20	66786	2145	2x2 MIMO	23.13	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	2x2 MIMO	LTE B66	20	66786	2145	4x4 MIMO	23.16	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B66	20	66786	2145	4x4 MIMO	23.05	23.54
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	24.40	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.41	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.41	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B4	5	1975	2112.5	2x2 MIMO	24.43	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	2x2 MIMO	LTE B4	5	1975	2112.5	4x4 MIMO	24.44	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	24.49	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	24.39	24.85
LTE B5	10	20525	836.5	QPSK	1	0	2525	881.5	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.58	25.00
LTE B5	10	20525	836.5	QPSK	1	0	2525	881.5	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	24.60	25.00
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	24.88	24.85
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.93	24.85
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.86	24.85
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	24.88	24.85
LTE B66	15	132047	1717.5	QPSK	1	0	66511	2117.5	4x4 MIMO	LTE B66	5	66604	2126.8	4x4 MIMO	24.80	24.84
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	4x4 MIMO	LTE B66	20	66588	2125.2	4x4 MIMO	24.92	24.85
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	4x4 MIMO	LTE B66	5	66461	2112.5	2x2 MIMO	24.88	24.85
LTE B66	20	132322	1745	QPSK	1	0	66786	2145	2x2 MIMO	LTE B66	5	66461	2112.5	4x4 MIMO	24.94	24.85
LTE B12	5	23095	707.5	QPSK	1	0	5095	737.5	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	24.52	24.48

Table G-5
Additional Hotspot Reduced Output Powers – 2 Component Carriers

PCC										SCC					Power	
PCC Band	PCC Bandwidth [MHz]	PCC (UL) Channel	PCC (UL) Frequency [MHz]	Modulation	PCC UL# RB	PCC UL RB Offset	PCC (DL) Channel	PCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	20.48	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	20.49	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	20.32	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	20.41	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	20.38	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	20.39	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.37	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B66	20	66786	2145	2x2 MIMO	20.28	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	2x2 MIMO	LTE B66	20	66786	2145	4x4 MIMO	20.33	20.50
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B66	20	66786	2145	4x4 MIMO	20.36	20.50
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	20.65	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	20.61	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	20.70	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B4	5	2375	2152.5	2x2 MIMO	20.60	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	2x2 MIMO	LTE B4	5	2375	2152.5	4x4 MIMO	20.61	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	20.62	20.79
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.68	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	20.63	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	20.65	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	20.63	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.67	20.79
LTE B66	15	132597	1772.5	16QAM	1	0	67061	2172.5	4x4 MIMO	LTE B66	5	66968	2163.2	4x4 MIMO	20.75	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	4x4 MIMO	LTE B66	20	66734	2139.8	4x4 MIMO	20.67	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	4x4 MIMO	LTE B66	5	67111	2177.5	2x2 MIMO	20.64	20.79
LTE B66	20	132072	1720	QPSK	50	0	66536	2120	2x2 MIMO	LTE B66	5	67111	2177.5	4x4 MIMO	20.64	20.79

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset	APPENDIX G: Page 2 of 4		

Table G-6
Additional Grip Sensor Reduced Output Powers – 2 Component Carriers

PCC										SCC					Power	
PCC Band	PCC Bandwidth [MHz]	PCC (UL) Channel	PCC (UL) Frequency [MHz]	Modulation	PCC UL# RB	PCC UL RB Offset	PCC (DL) Channel	PCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	22.01	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	22.06	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	22.02	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	22.05	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	22.03	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	22.13	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.08	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B66	20	66786	2145	2x2 MIMO	22.11	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	2x2 MIMO	LTE B66	20	66786	2145	4x4 MIMO	22.15	22.32
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B66	20	66786	2145	4x4 MIMO	22.08	22.32
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	22.27	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	22.26	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	22.25	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B4	5	1975	2112.5	2x2 MIMO	22.32	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	2x2 MIMO	LTE B4	5	1975	2112.5	4x4 MIMO	22.32	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B5	10	2525	881.5	2x2 MIMO	22.27	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.23	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	22.26	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	22.21	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	4x4 MIMO	LTE B2	20	900	1960	4x4 MIMO	22.23	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.25	22.50
LTE B66	15	132047	1717.5	16QAM	1	0	66511	2117.5	4x4 MIMO	LTE B66	5	66604	2126.8	4x4 MIMO	22.21	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	4x4 MIMO	LTE B66	20	66838	2150.2	4x4 MIMO	22.07	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	4x4 MIMO	LTE B66	5	66461	2112.5	2x2 MIMO	22.28	22.50
LTE B66	20	132572	1770	16QAM	1	0	67036	2170	2x2 MIMO	LTE B66	5	66461	2112.5	4x4 MIMO	22.22	22.50

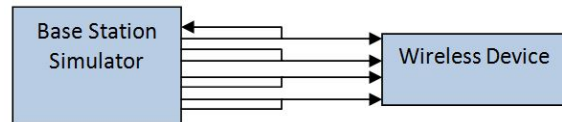


Figure G-2
Power Measurement Setup

G.3 Carrier Aggregation Scenarios with 3 Component Carriers with 4x4 Downlink MIMO

Table G-7
Additional Maximum Output Powers – 3 Component Carriers

PCC										SCC1					SCC2					Power	
PCC Band	PCC Bandwidth [MHz]	PCC (UL) Channel	PCC (UL) Frequency [MHz]	Modulation	PCC UL# RB	PCC UL RB Offset	PCC (DL) Channel	PCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	23.17	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	23.26	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	23.16	23.54
LTE B2	15	19125	1902.5	QPSK	1	0	1125	1982.5	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	23.13	23.54
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	24.73	24.85
LTE B4	20	20300	1745	QPSK	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	24.73	24.85
LTE B12	5	23095	707.5	QPSK	1	0	5095	737.5	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	LTE B2	5	1175	1987.5	2x2 MIMO	24.47	24.48

Table G-8
Additional Hotspot Reduced Output Powers – 3 Component Carriers

PCC																			SCC 1					SCC 2					Power	
PCC Band	PCC Bandwidth [MHz]	PCC (UL) Channel	PCC (UL) Frequency [MHz]	Modulation	PCC UL RB	PCC UL RB Offset	PCC (DL) Channel	PCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC (DL) Channel	SCC (DL) Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)									
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.42	20.50									
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.48	20.50									
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.49	20.50									
LTE B2	20	19100	1900	64QAM	1	0	1100	1980	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.43	20.50									
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.75	20.79									
LTE B4	20	20050	1720	QPSK	50	0	2050	2120	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	20.72	20.79									

FCC ID: A3LSMG955U		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset	APPENDIX G: Page 3 of 4		

Table G-9
Additional Grip Sensor Reduced Output Powers – 3 Component Carriers

PCC										SCC 1				SCC 2				Power			
PCC Band	PCC Bandwidth [MHz]	PCC [UL] Channel	PCC [UL] Frequency [MHz]	Modulation	PCC UL RB	PCC UL RB Offset	PCC [DL] Channel	PCC [DL] Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC [DL] Channel	SCC [DL] Frequency [MHz]	DL Antenna Configuration	SCC Band	SCC Bandwidth [MHz]	SCC [DL] Channel	SCC [DL] Frequency [MHz]	DL Antenna Configuration	LTE Tx Power with DL CA Enabled (dBm)	LTE Single Carrier Tx Power (dBm)
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B2	5	625	1932.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.01	22.12
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	2x2 MIMO	LTE B2	5	625	1932.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.06	22.12
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	4x4 MIMO	LTE B4	20	2175	2132.5	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.05	22.12
LTE B2	20	19100	1900	16QAM	1	0	1100	1980	2x2 MIMO	LTE B4	20	2175	2132.5	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.08	22.12
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	4x4 MIMO	LTE B2	20	900	1960	2x2 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.38	22.50
LTE B4	20	20300	1745	16QAM	1	0	2300	2145	2x2 MIMO	LTE B2	20	900	1960	4x4 MIMO	LTE B12	10	5095	737.5	2x2 MIMO	22.35	22.50

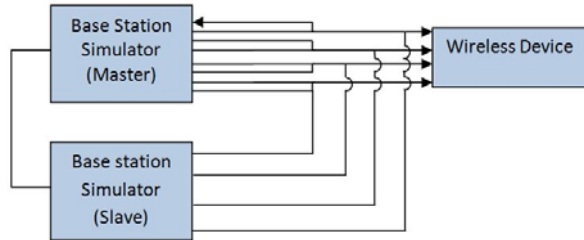


Figure G-3
Power Measurement Setup

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/16 – 02/08/17	DUT Type: Portable Handset	APPENDIX G: Page 4 of 4		

APPENDIX H: SENSOR TRIGGERING DATA SUMMARY

A3LSMG955U Sensor Triggering Data Summary

Per FCC KDB Publication 616217 D04v01r02, this device was tested by the manufacturer to determine the proximity sensor triggering distances for all applicable sides and edges of the device. The measured output power at distances within ± 5 mm of the triggering points (or until touching the phantom) is included for back and front sides and each applicable edge per Step i) in Section 6.2 of the KDB. The technical descriptions in the filing contain the complete set of triggering data required by Section 6 of FCC KDB Publication 616217 D04v01r02.

To ensure all production units are compliant, it is necessary to test SAR at a distance 1 mm less than the smallest distance between the device and SAR phantom (determined from the sensor triggering tests according to FCC KDB 616217 D04v01r02) with the device at the maximum output power (without power reduction). These SAR tests are included in addition to the SAR tests for the device touching the SAR phantom (at the reduced output power level).

The operational description contains information explaining how this device remains compliant in the event of a sensor malfunction.

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/2016 – 02/08/2017	DUT Type: Portable Handset			APPENDIX H: Page 1 of 4

Back Side

Moving device toward the phantom:

KDB 616217 6.2.f Measured Power [dBm]											
Distance[mm]	10	9	8	7	6	5	4	3	2	1	0
GSM 1900	30.71	30.74	30.86	30.84	30.88	27.86	27.62	27.88	27.65	27.80	27.81
GPRS 1900 1Tx	30.75	30.76	30.94	30.69	30.92	27.76	27.80	27.73	27.82	27.77	27.83
GPRS 1900 2Tx	28.31	28.14	28.42	28.29	28.10	25.31	25.44	25.16	25.38	25.29	25.38
GPRS 1900 3Tx	26.42	26.34	26.23	26.26	26.27	23.43	23.45	23.23	23.39	23.32	23.28
GPRS 1900 4Tx	24.40	24.45	24.35	24.18	24.41	21.41	21.28	21.26	21.10	21.43	21.26
EDGE1900 1Tx	25.95	25.82	25.68	25.64	25.61	24.94	24.60	24.62	24.67	24.76	24.93
EDGE1900 2Tx	24.79	24.84	24.62	24.81	24.62	23.76	23.62	23.71	23.95	23.78	23.91
EDGE1900 3Tx	22.89	22.80	22.83	22.82	22.80	21.66	21.60	21.92	21.85	21.79	21.63
EDGE1900 4Tx	21.35	21.10	21.13	21.31	21.14	20.28	20.12	20.27	20.45	20.32	20.16
UMTS B4	24.86	24.72	24.80	24.85	24.65	21.90	21.78	21.78	21.78	21.69	21.64
UMTS B2	24.27	24.26	24.29	24.30	24.19	21.13	21.23	21.21	21.43	21.31	21.17
CDMA BC1	24.28	24.36	24.34	24.41	24.37	22.11	22.24	22.43	22.21	22.41	22.17
LTE FDD B66	24.72	24.67	24.72	24.73	24.71	22.40	22.31	22.18	22.33	22.35	22.36
LTE FDD B4	24.72	24.65	24.89	24.91	24.60	22.20	22.44	22.36	22.28	22.34	22.26
LTE FDD B25	24.16	24.34	24.27	24.25	24.32	22.45	22.17	22.10	22.24	22.35	22.36
LTE FDD B2	24.29	24.29	24.28	24.41	24.42	22.22	22.27	22.42	22.16	22.43	22.30
LTE FDD B30	23.89	23.79	23.65	23.70	23.66	22.27	22.33	22.42	22.26	22.27	22.43
LTE TDD B41(PC2)	26.78	26.70	26.93	26.62	26.85	23.85	23.86	23.90	23.60	23.69	23.93

Moving device away from the phantom:

KDB 616217 6.2.h Measured Power [dBm]											
Distance[mm]	10	9	8	7	6	5	4	3	2	1	0
GSM 1900	30.89	30.65	30.63	30.66	30.69	27.93	27.88	27.76	27.92	27.94	27.91
GPRS 1900 1Tx	30.79	30.83	30.91	30.95	30.89	27.83	27.60	27.71	27.88	27.62	27.81
GPRS 1900 2Tx	28.42	28.39	28.12	28.36	28.21	25.11	25.26	25.25	25.36	25.14	25.31
GPRS 1900 3Tx	26.29	26.42	26.19	26.43	26.14	23.15	23.17	23.45	23.40	23.17	23.21
GPRS 1900 4Tx	24.43	24.42	24.25	24.21	24.25	21.34	21.41	21.40	21.30	21.15	21.35
EDGE1900 1Tx	25.94	25.74	25.86	25.74	25.76	24.72	24.80	24.61	24.72	24.79	24.82
EDGE1900 2Tx	24.61	24.67	24.86	24.64	24.79	23.75	23.90	23.87	23.62	23.65	23.68
EDGE1900 3Tx	22.64	22.82	22.94	22.70	22.77	21.85	21.65	21.79	21.81	21.65	21.63
EDGE1900 4Tx	21.28	21.34	21.13	21.45	21.11	20.27	20.11	20.15	20.16	20.26	20.27
UMTS B4	24.93	24.86	24.72	24.87	24.73	21.61	21.84	21.81	21.82	21.88	21.75
UMTS B2	24.21	24.42	24.16	24.36	24.31	21.36	21.30	21.19	21.25	21.29	21.12
CDMA BC1	24.23	24.24	24.43	24.21	24.22	22.29	22.20	22.19	22.36	22.12	22.13
LTE FDD B66	24.60	24.94	24.76	24.86	24.88	22.17	22.13	22.32	22.39	22.25	22.23
LTE FDD B4	24.87	24.61	24.72	24.71	24.74	22.23	22.23	22.24	22.13	22.39	22.28
LTE FDD B25	24.25	24.37	24.12	24.19	24.22	22.18	22.34	22.19	22.14	22.31	22.34
LTE FDD B2	24.31	24.10	24.22	24.31	24.36	22.13	22.44	22.33	22.11	22.15	22.32
LTE FDD B30	23.60	23.66	23.60	23.79	23.62	22.14	22.31	22.19	22.31	22.19	22.41
LTE TDD B41(PC2)	26.69	26.74	26.81	26.82	26.81	23.67	23.92	23.87	23.61	23.81	23.84

Based on the most conservative measured triggering distance of 5 mm, additional SAR measurements were required at 4 mm from the back side.

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/2016 – 02/08/2017	DUT Type: Portable Handset			APPENDIX H: Page 2 of 4

Front Side

Moving device toward the phantom:

KDB 616217 6.2.f Measured Power [dBm]											
Distance[mm]	10	9	8	7	6	5	4	3	2	1	0
GSM 1900	30.78	30.63	30.63	30.68	30.74	27.78	27.94	27.75	27.93	27.69	27.87
GPRS 1900 1Tx	30.82	30.64	30.79	30.68	30.66	27.65	27.60	27.87	27.87	27.94	27.74
GPRS 1900 2Tx	28.23	28.26	28.18	28.15	28.21	25.34	25.31	25.17	25.23	25.42	25.20
GPRS 1900 3Tx	26.33	26.19	26.26	26.27	26.17	23.26	23.35	23.36	23.24	23.43	23.24
GPRS 1900 4Tx	24.10	24.36	24.23	24.38	24.29	21.43	21.21	21.35	21.11	21.21	21.43
EDGE1900 1Tx	25.85	25.85	25.84	25.69	25.80	24.73	24.75	24.72	24.94	24.80	24.79
EDGE1900 2Tx	24.80	24.93	24.95	24.80	24.95	23.64	23.71	23.69	23.90	23.91	23.77
EDGE1900 3Tx	22.72	22.84	22.76	22.86	22.90	21.78	21.94	21.80	21.91	21.79	21.60
EDGE1900 4Tx	21.12	21.39	21.13	21.11	21.28	20.28	20.44	20.21	20.31	20.39	20.40
UMTS B4	24.66	24.78	24.95	24.84	24.61	21.74	21.82	21.70	21.83	21.91	21.95
UMTS B2	24.21	24.22	24.22	24.13	24.41	21.18	21.17	21.26	21.36	21.15	21.35
CDMA BC1	24.43	24.33	24.37	24.16	24.44	22.29	22.12	22.40	22.28	22.29	22.10
LTE FDD B66	24.81	24.67	24.94	24.78	24.84	22.34	22.14	22.14	22.17	22.41	22.32
LTE FDD B4	24.95	24.74	24.76	24.72	24.91	22.27	22.32	22.41	22.31	22.36	22.30
LTE FDD B25	24.43	24.19	24.28	24.18	24.26	22.44	22.22	22.43	22.36	22.12	22.18
LTE FDD B2	24.29	24.30	24.17	24.12	24.38	22.30	22.42	22.39	22.33	22.41	22.21
LTE FDD B30	23.85	23.60	23.77	23.74	23.82	22.37	22.42	22.15	22.33	22.27	22.17
LTE TDD B41(PC2)	26.91	26.94	26.61	26.77	26.70	23.73	23.65	23.80	23.89	23.74	23.69

Moving device away from the phantom:

KDB 616217 6.2.h Measured Power [dBm]											
Distance[mm]	10	9	8	7	6	5	4	3	2	1	0
GSM 1900	30.76	30.86	30.83	30.75	30.82	27.71	27.66	27.66	27.67	27.70	27.61
GPRS 1900 1Tx	30.91	30.76	30.90	30.69	30.84	27.94	27.66	27.66	27.85	27.68	27.61
GPRS 1900 2Tx	28.34	28.14	28.41	28.16	28.19	25.31	25.31	25.42	25.17	25.21	25.37
GPRS 1900 3Tx	26.36	26.26	26.12	26.44	26.10	23.21	23.20	23.39	23.41	23.43	23.27
GPRS 1900 4Tx	24.25	24.37	24.37	24.11	24.29	21.43	21.37	21.14	21.35	21.45	21.34
EDGE1900 1Tx	25.82	25.60	25.93	25.94	25.61	24.80	24.76	24.61	24.92	24.66	24.90
EDGE1900 2Tx	24.62	24.73	24.66	24.95	24.69	23.65	23.67	23.81	23.63	23.86	23.68
EDGE1900 3Tx	22.85	22.68	22.88	22.73	22.73	21.74	21.69	21.68	21.95	21.64	21.91
EDGE1900 4Tx	21.28	21.45	21.13	21.38	21.21	20.26	20.30	20.12	20.16	20.35	20.29
UMTS B4	24.85	24.60	24.89	24.64	24.74	21.94	21.94	21.85	21.84	21.82	21.95
UMTS B2	24.24	24.45	24.11	24.23	24.22	21.21	21.24	21.37	21.17	21.39	21.33
CDMA BC1	24.34	24.44	24.41	24.21	24.15	22.45	22.14	22.27	22.29	22.10	22.20
LTE FDD B66	24.61	24.86	24.67	24.78	24.79	22.34	22.28	22.12	22.37	22.26	22.14
LTE FDD B4	24.83	24.87	24.72	24.70	24.67	22.13	22.25	22.16	22.17	22.13	22.34
LTE FDD B25	24.36	24.14	24.42	24.15	24.19	22.27	22.29	22.18	22.13	22.29	22.42
LTE FDD B2	24.15	24.27	24.12	24.20	24.12	22.19	22.22	22.15	22.43	22.39	22.35
LTE FDD B30	23.78	23.71	23.81	23.69	23.64	22.37	22.23	22.45	22.12	22.20	22.14
LTE TDD B41(PC2)	26.81	26.72	26.69	26.95	26.81	23.85	23.87	23.69	23.83	23.90	23.90

Based on the most conservative measured triggering distance of 5 mm, additional SAR measurements were required at 4 mm from the front side.

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/2016 – 02/08/2017	DUT Type: Portable Handset			APPENDIX H: Page 3 of 4

Bottom Edge

Moving device toward the phantom:

KDB 616217 6.2.f Measured Power [dBm]											
Distance[mm]	12	11	10	9	8	7	6	5	4	3	2
GSM 1900	30.90	30.93	30.92	30.92	30.73	27.66	27.89	27.61	27.90	27.67	27.70
GPRS 1900 1Tx	30.71	30.60	30.73	30.80	30.90	27.67	27.74	27.89	27.66	27.74	27.70
GPRS 1900 2Tx	28.23	28.40	28.26	28.34	28.25	25.19	25.19	25.29	25.32	25.12	25.31
GPRS 1900 3Tx	26.28	26.29	26.18	26.29	26.37	23.27	23.16	23.40	23.11	23.23	23.19
GPRS 1900 4Tx	24.19	24.33	24.12	24.20	24.30	21.13	21.38	21.45	21.43	21.23	21.26
EDGE1900 1Tx	25.84	25.60	25.82	25.66	25.69	24.71	24.90	24.94	24.89	24.80	24.94
EDGE1900 2Tx	24.70	24.61	24.71	24.61	24.76	23.90	23.63	23.82	23.94	23.88	23.75
EDGE1900 3Tx	22.73	22.84	22.90	22.88	22.77	21.93	21.76	21.77	21.95	21.79	21.81
EDGE1900 4Tx	21.33	21.11	21.38	21.41	21.14	20.45	20.17	20.41	20.19	20.37	20.22
UMTS B4	24.78	24.74	24.79	24.93	24.70	21.79	21.79	21.61	21.66	21.66	21.73
UMTS B2	24.27	24.25	24.40	24.12	24.11	21.43	21.22	21.10	21.11	21.29	21.37
CDMA BC1	24.37	24.12	24.13	24.44	24.30	22.15	22.42	22.21	22.44	22.12	22.44
LTE FDD B66	24.85	24.81	24.72	24.82	24.67	22.34	22.41	22.20	22.34	22.14	22.44
LTE FDD B4	24.94	24.64	24.75	24.89	24.67	22.18	22.20	22.37	22.35	22.36	22.14
LTE FDD B25	24.43	24.45	24.36	24.11	24.25	22.37	22.22	22.25	22.11	22.40	22.39
LTE FDD B2	24.31	24.31	24.34	24.16	24.41	22.35	22.12	22.38	22.17	22.40	22.27
LTE FDD B30	23.81	23.79	23.69	23.67	23.61	22.18	22.25	22.40	22.21	22.35	22.40
LTE TDD B41 (PC2)	26.87	26.63	26.61	26.84	26.60	23.79	23.79	23.85	23.65	23.73	23.60

Moving device away from the phantom:

KDB 616217 6.2.h Measured Power [dBm]											
Distance[mm]	12	11	10	9	8	7	6	5	4	3	2
GSM 1900	30.71	30.91	30.86	30.77	30.76	27.64	27.87	27.93	27.79	27.73	27.84
GPRS 1900 1Tx	30.81	30.71	30.63	30.94	30.89	27.93	27.85	27.86	27.64	27.63	27.90
GPRS 1900 2Tx	28.20	28.21	28.37	28.35	28.21	25.25	25.32	25.31	25.35	25.21	25.14
GPRS 1900 3Tx	26.18	26.39	26.29	26.39	26.19	23.18	23.19	23.16	23.30	23.25	23.39
GPRS 1900 4Tx	24.22	24.10	24.23	24.29	24.43	21.37	21.21	21.26	21.24	21.33	21.18
EDGE1900 1Tx	25.83	25.90	25.73	25.87	25.84	24.80	24.69	24.77	24.70	24.94	24.86
EDGE1900 2Tx	24.77	24.66	24.95	24.81	24.64	23.77	23.60	23.83	23.86	23.86	23.69
EDGE1900 3Tx	22.75	22.69	22.79	22.88	22.79	21.67	21.81	21.76	21.85	21.84	21.84
EDGE1900 4Tx	21.21	21.40	21.34	21.16	21.20	20.10	20.38	20.41	20.37	20.32	20.32
UMTS B4	24.64	24.72	24.91	24.90	24.69	21.65	21.86	21.64	21.73	21.78	21.94
UMTS B2	24.39	24.15	24.19	24.44	24.19	21.27	21.14	21.30	21.28	21.28	21.13
CDMA BC1	24.42	24.27	24.14	24.29	24.29	22.31	22.41	22.27	22.35	22.44	22.21
LTE FDD B66	24.75	24.93	24.81	24.70	24.74	22.27	22.44	22.38	22.23	22.21	22.21
LTE FDD B4	24.76	24.69	24.69	24.82	24.72	22.18	22.13	22.40	22.12	22.15	22.35
LTE FDD B25	24.10	24.28	24.36	24.33	24.34	22.12	22.22	22.19	22.32	22.28	22.21
LTE FDD B2	24.30	24.32	24.42	24.21	24.16	22.22	22.20	22.11	22.15	22.34	22.41
LTE FDD B30	23.68	23.93	23.92	23.78	23.84	22.44	22.17	22.23	22.28	22.14	22.41
LTE TDD B41 (PC2)	26.61	26.82	26.73	26.84	26.81	23.91	23.67	23.64	23.83	23.71	23.82

Based on the most conservative measured triggering distance of 7 mm, additional SAR measurements were required at 6 mm from the bottom edge.

FCC ID: A3LSMG955U	 PCTEST ENGINEERING LABORATORY, INC.	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 12/26/2016 – 02/08/2017	DUT Type: Portable Handset			APPENDIX H: Page 4 of 4