

**HCT Co., Ltd.**

74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383 KOREA
Tel. +82 31 634 6300 Fax. +82 31 645 6401

Appendix A: Test Setup Photo

FCC ID
A3LSMM236B

File No.

HCT-RF-2201-FC090-P	HCT-RF-2201-FC095-P
HCT-RF-2201-FC091-P	HCT-RF-2201-FC096-P
HCT-RF-2201-FC092-P	HCT-RF-2201-FC097-P
HCT-RF-2201-FC093-P	HCT-RF-2201-FC098-P
HCT-RF-2201-FC094-P	


REVISION HISTORY

The revision history for this document is shown in table.

Revision No.	Date of Issue	Description
0	January 26, 2022	Initial Release

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	


1. Radiated Test Setup Photo

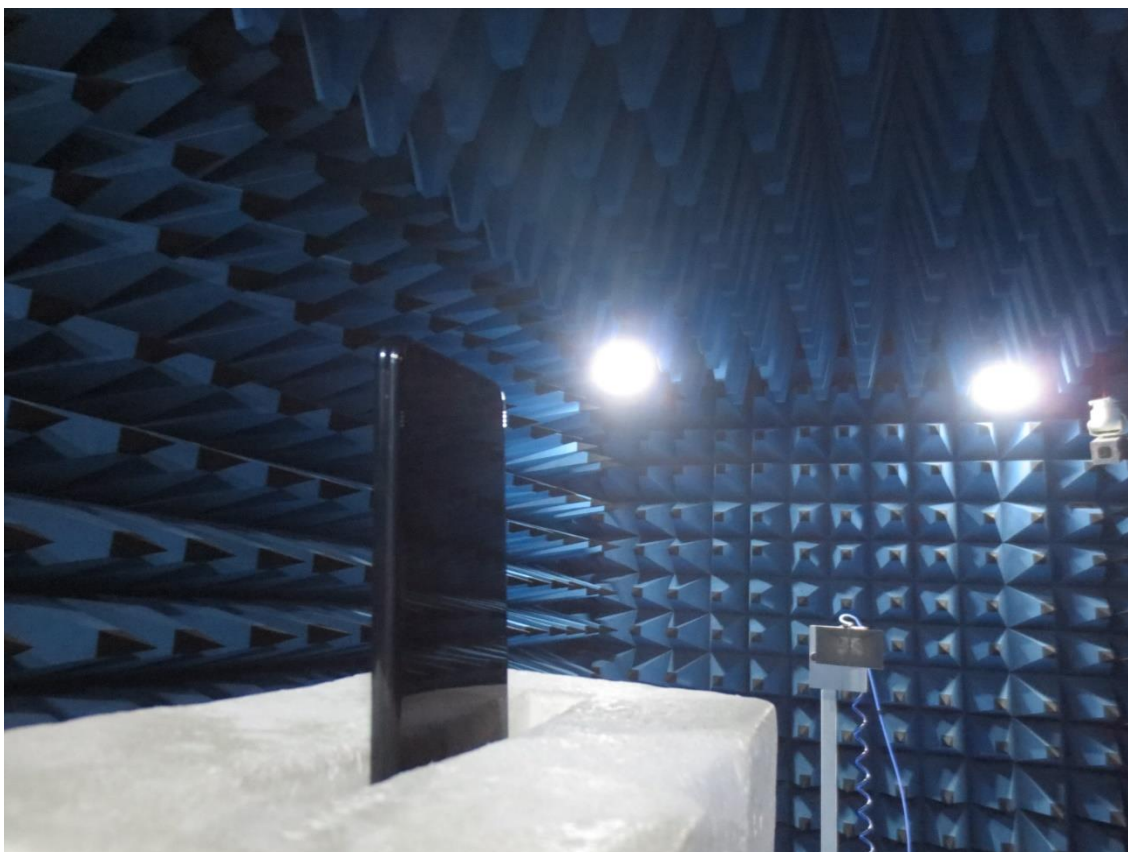


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	




File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

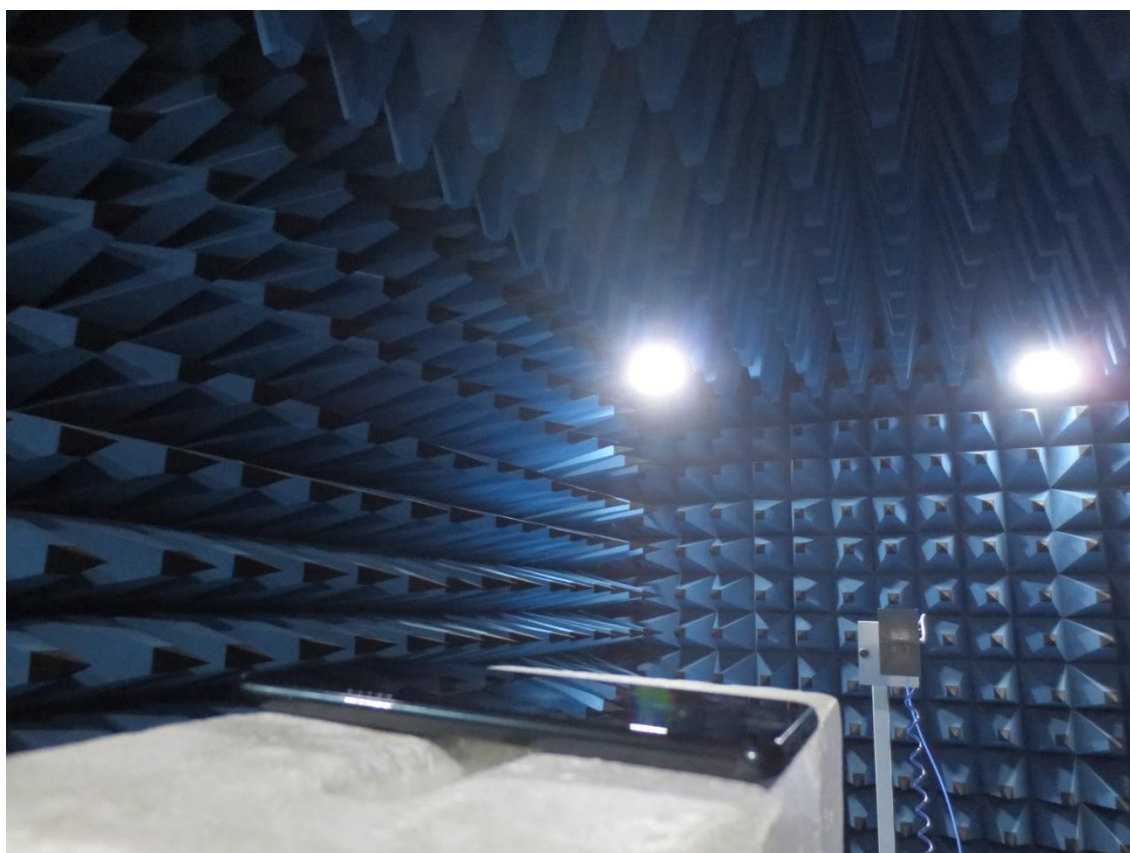


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

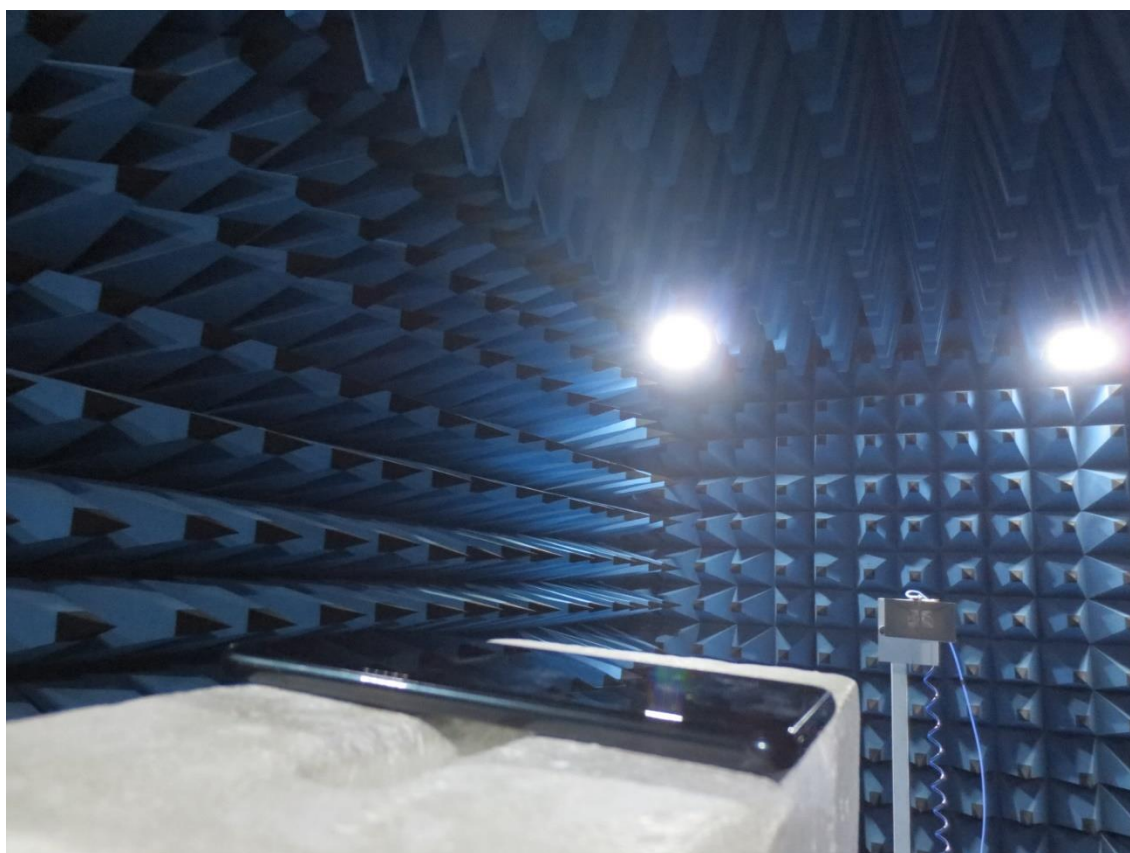


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

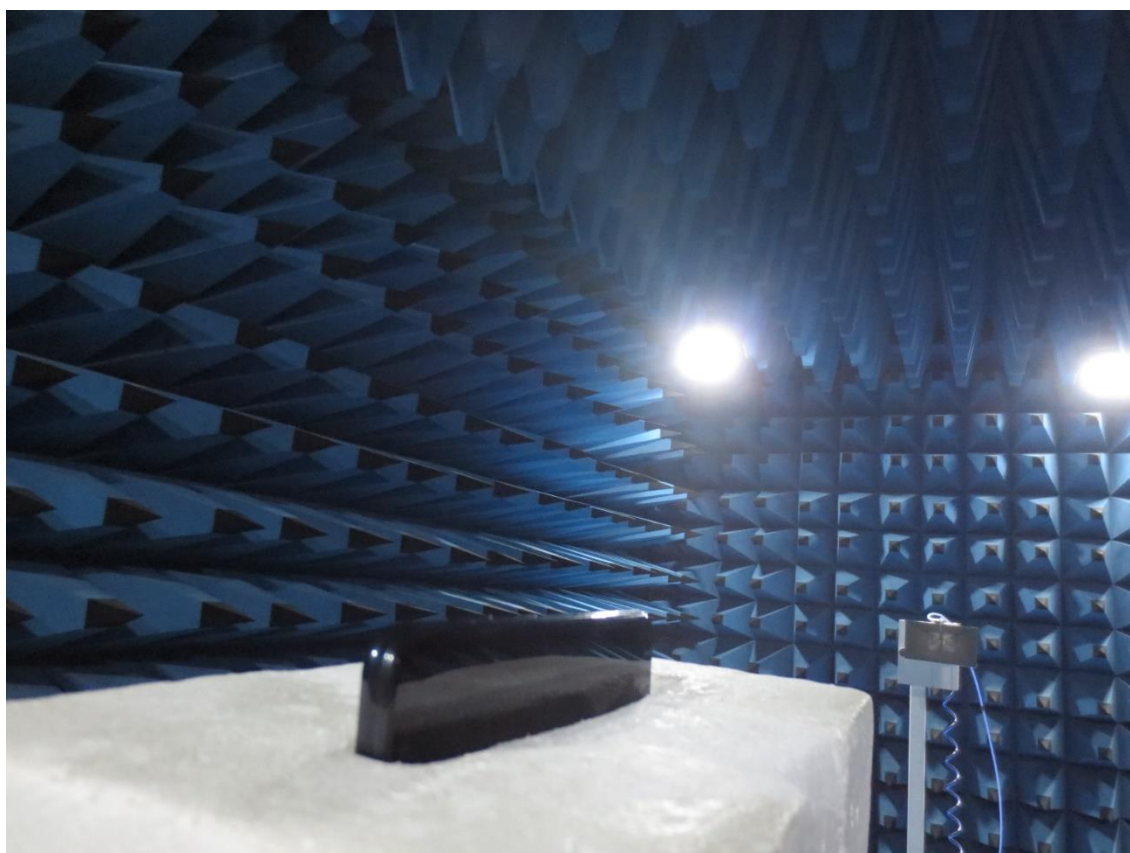

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

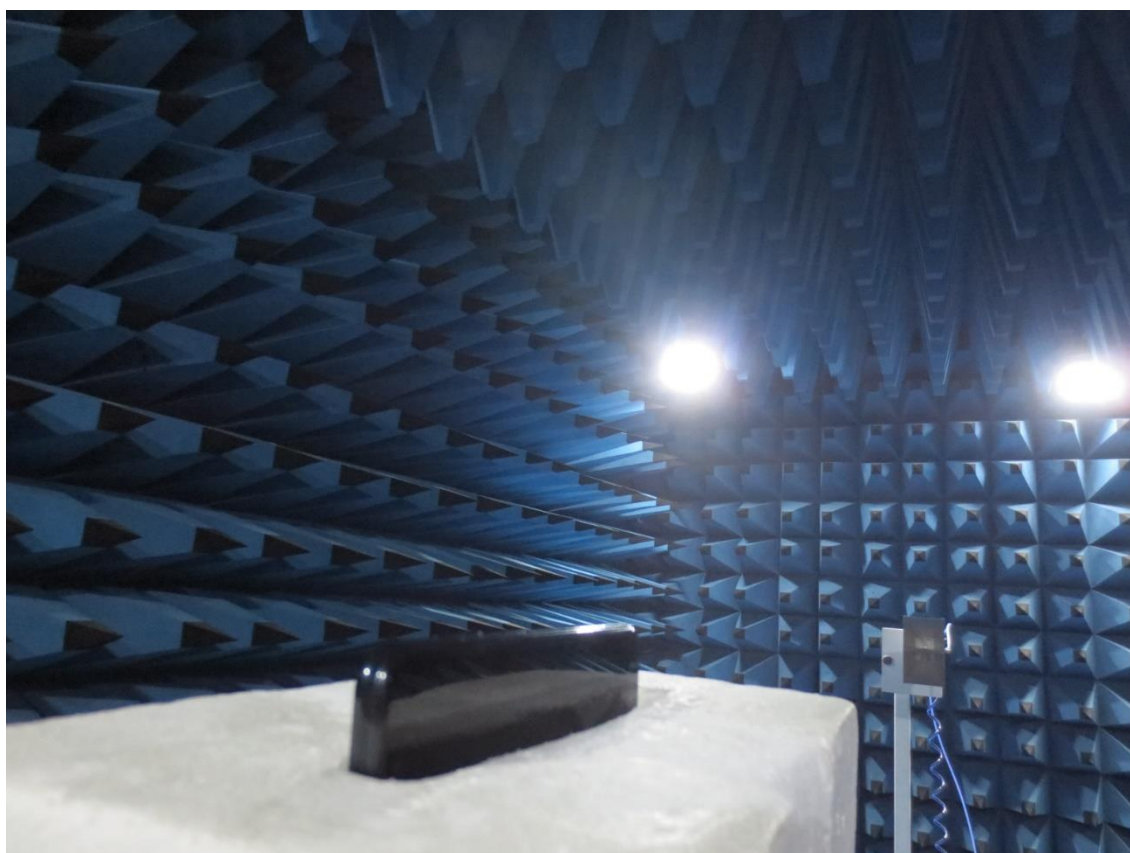


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

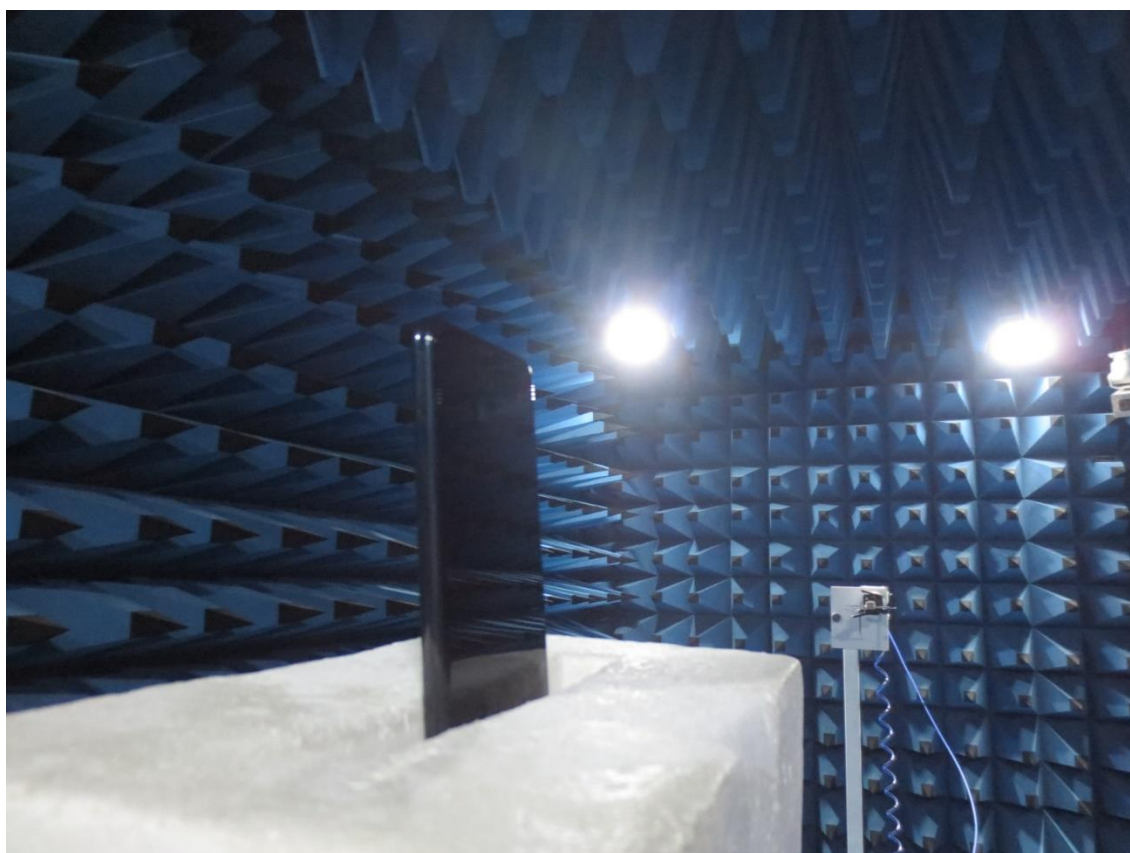


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	




File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

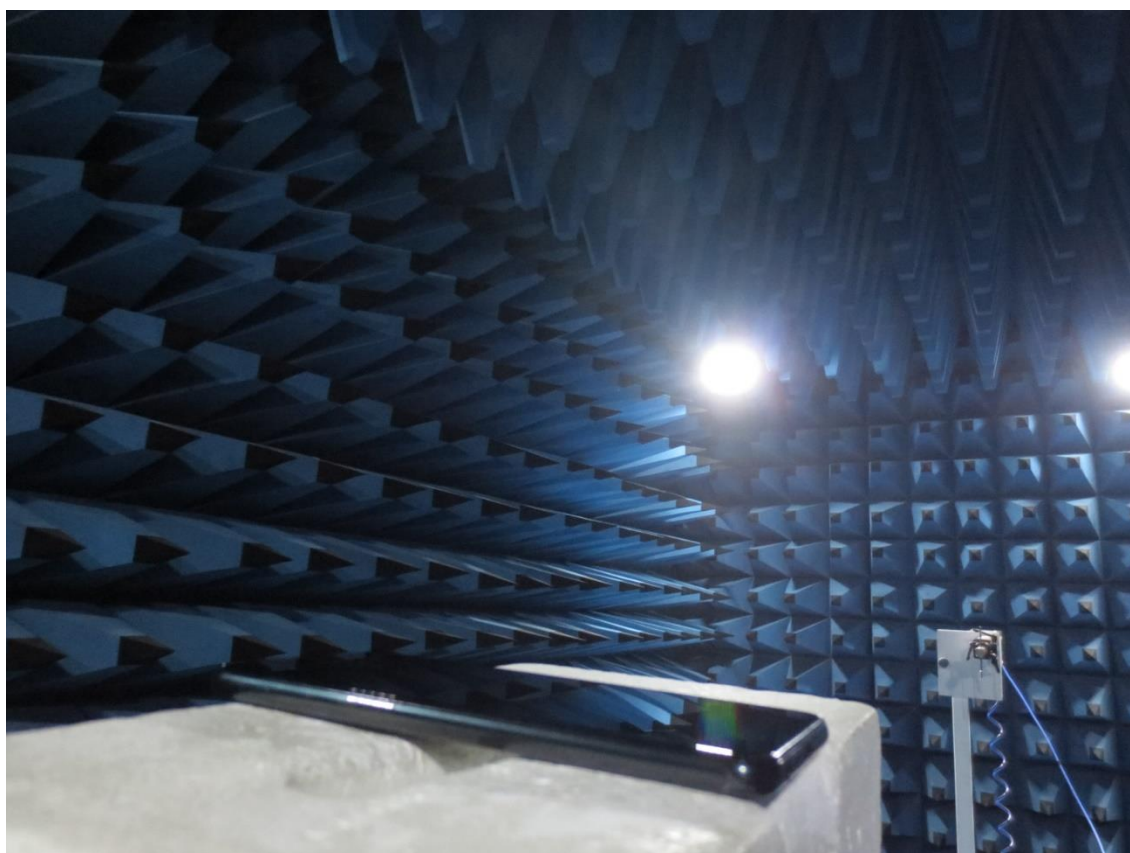


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

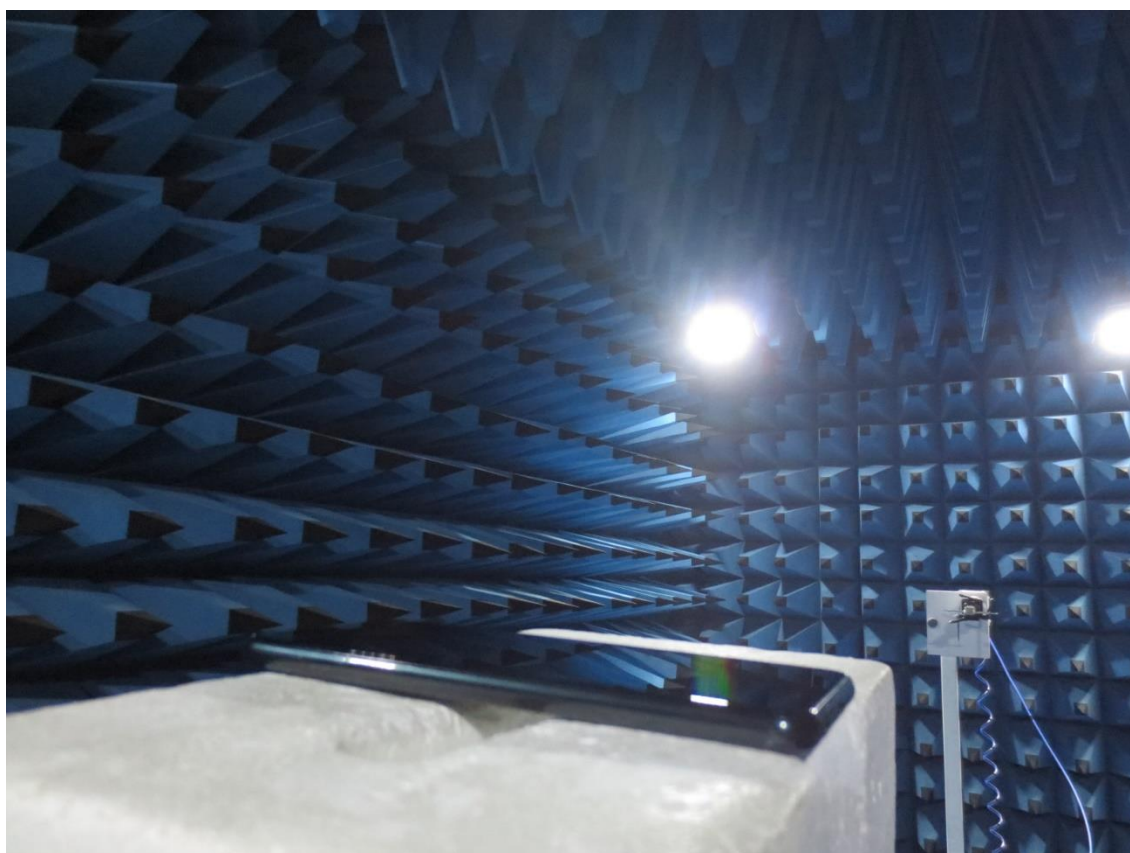

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

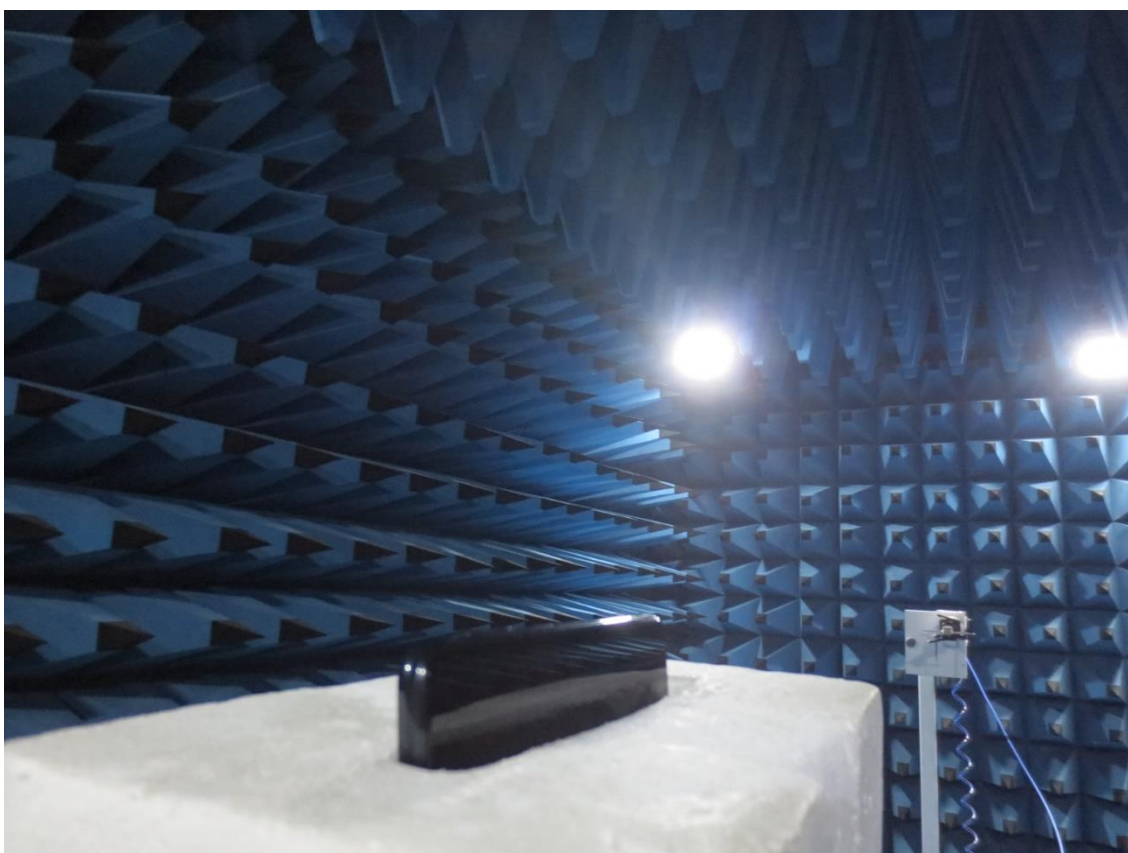


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

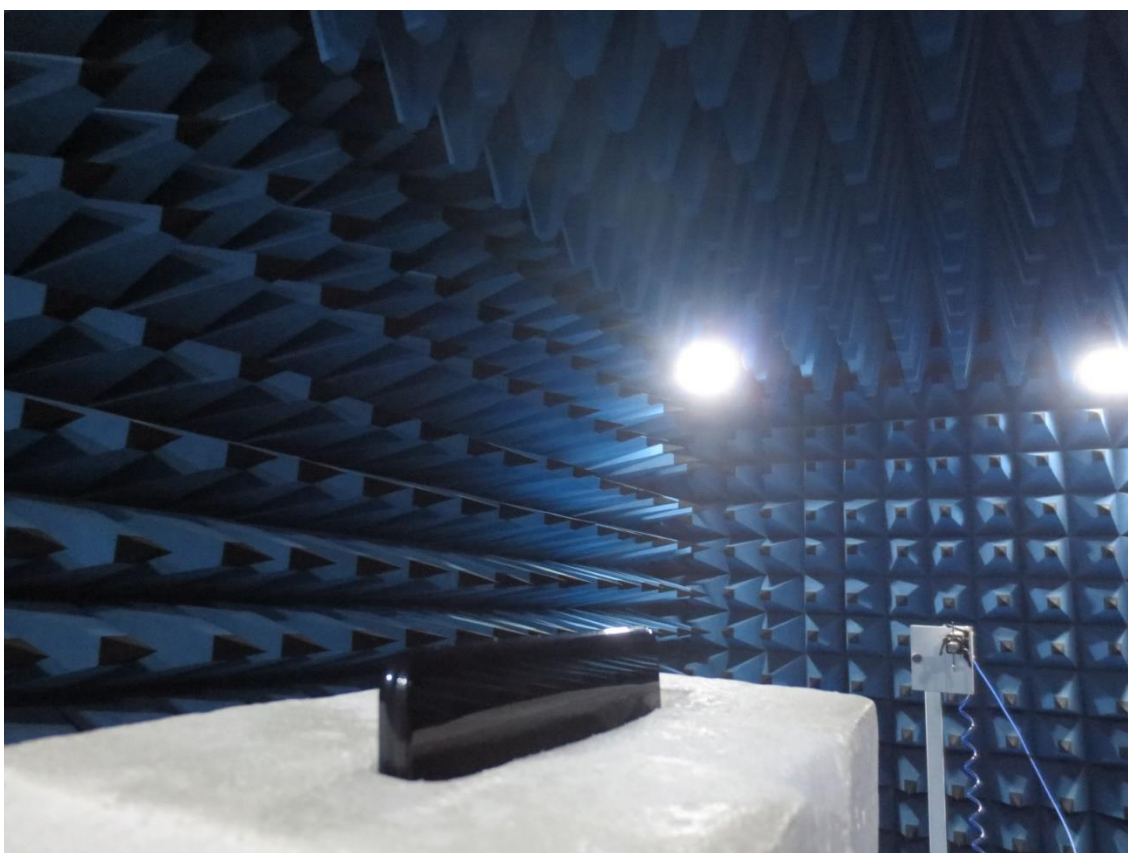


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	



File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

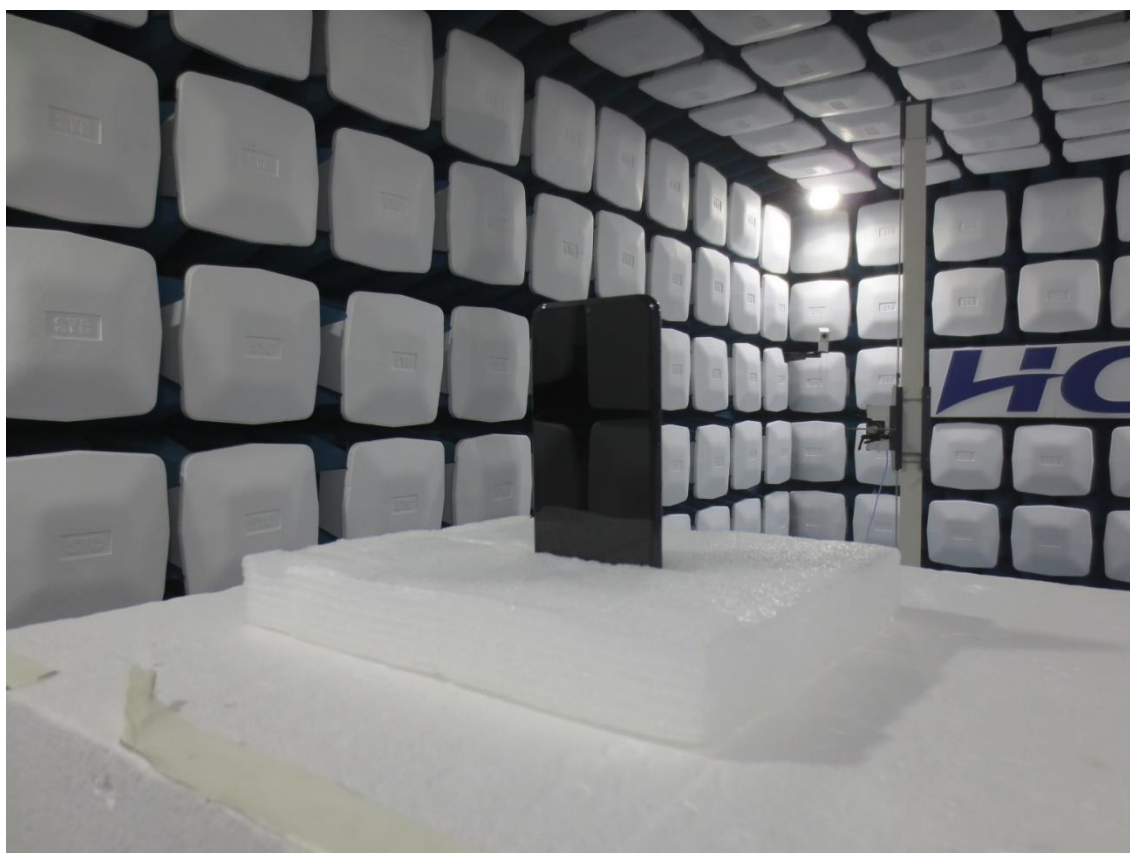


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

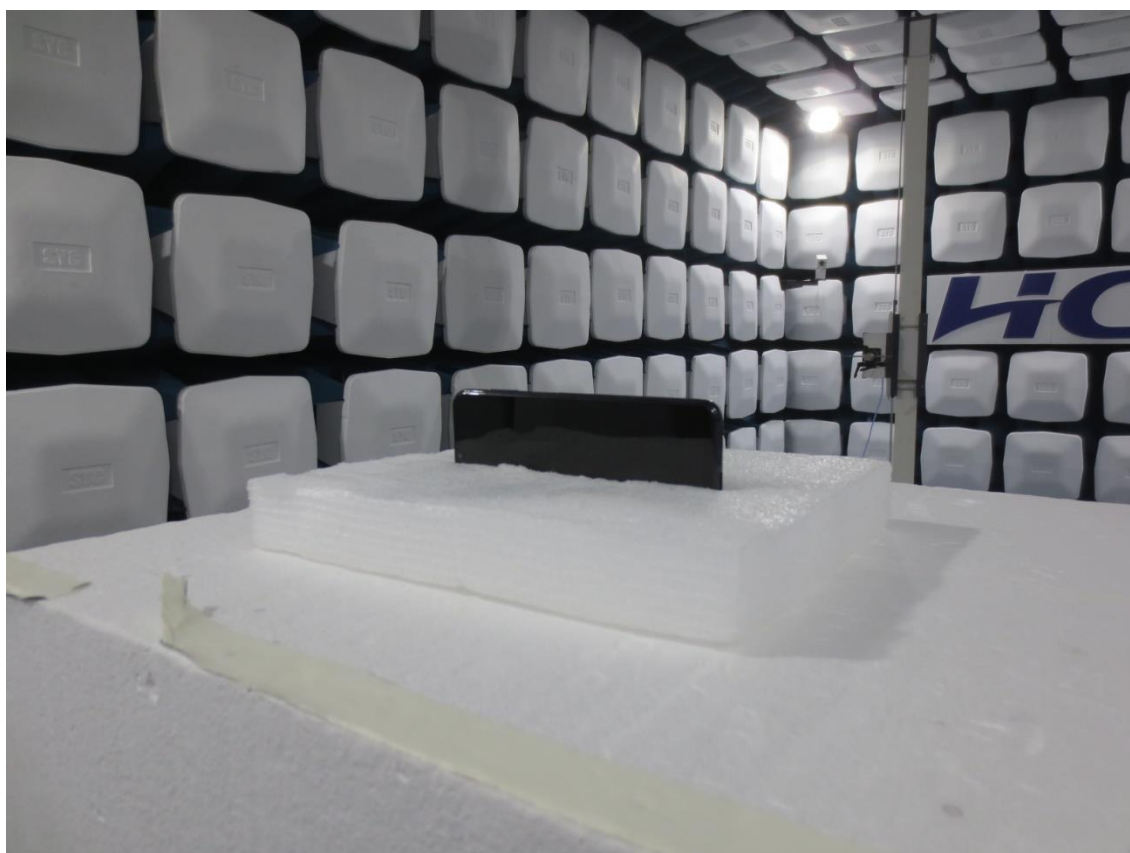


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	




File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

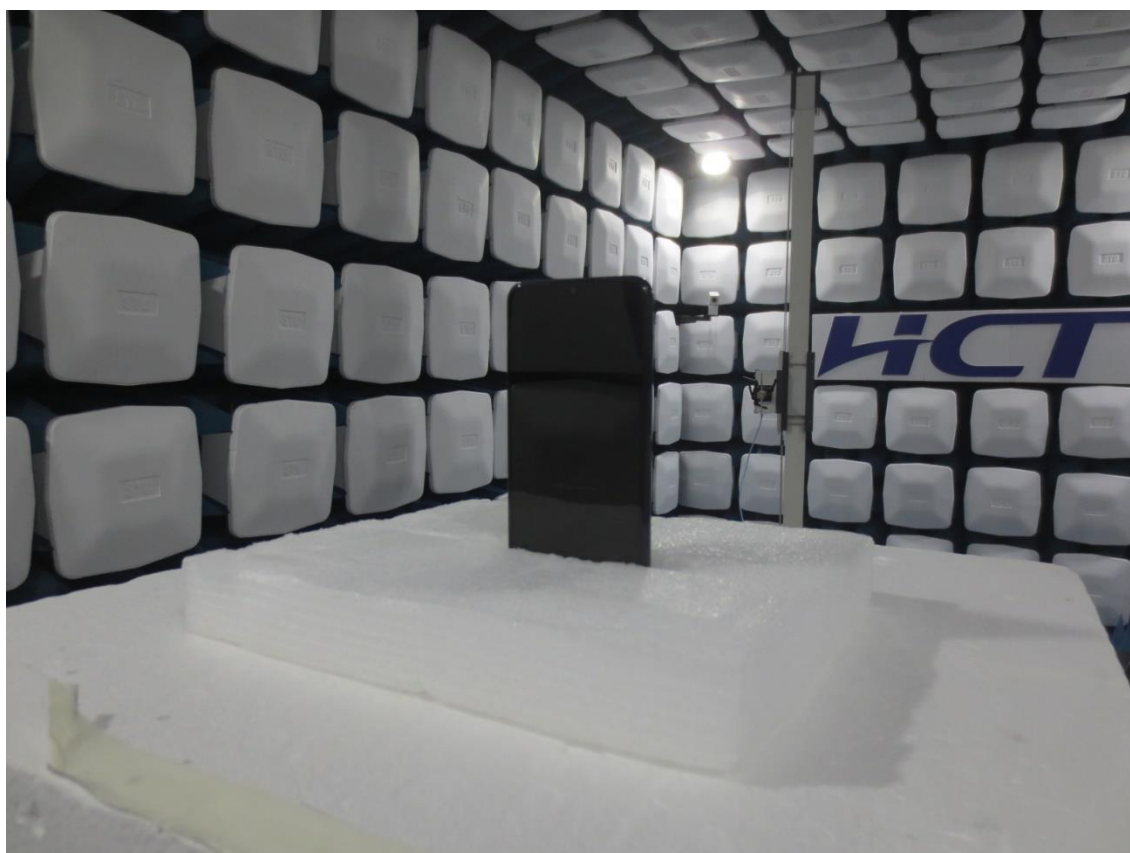


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

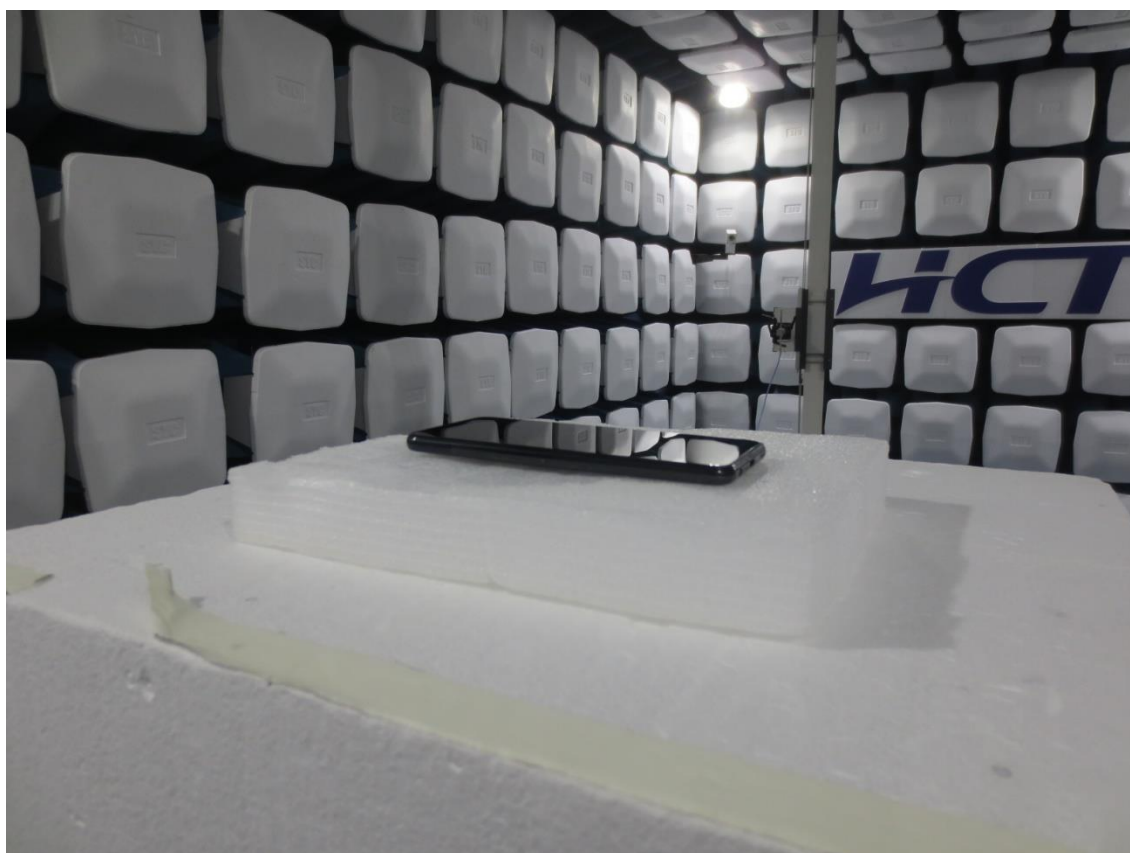

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

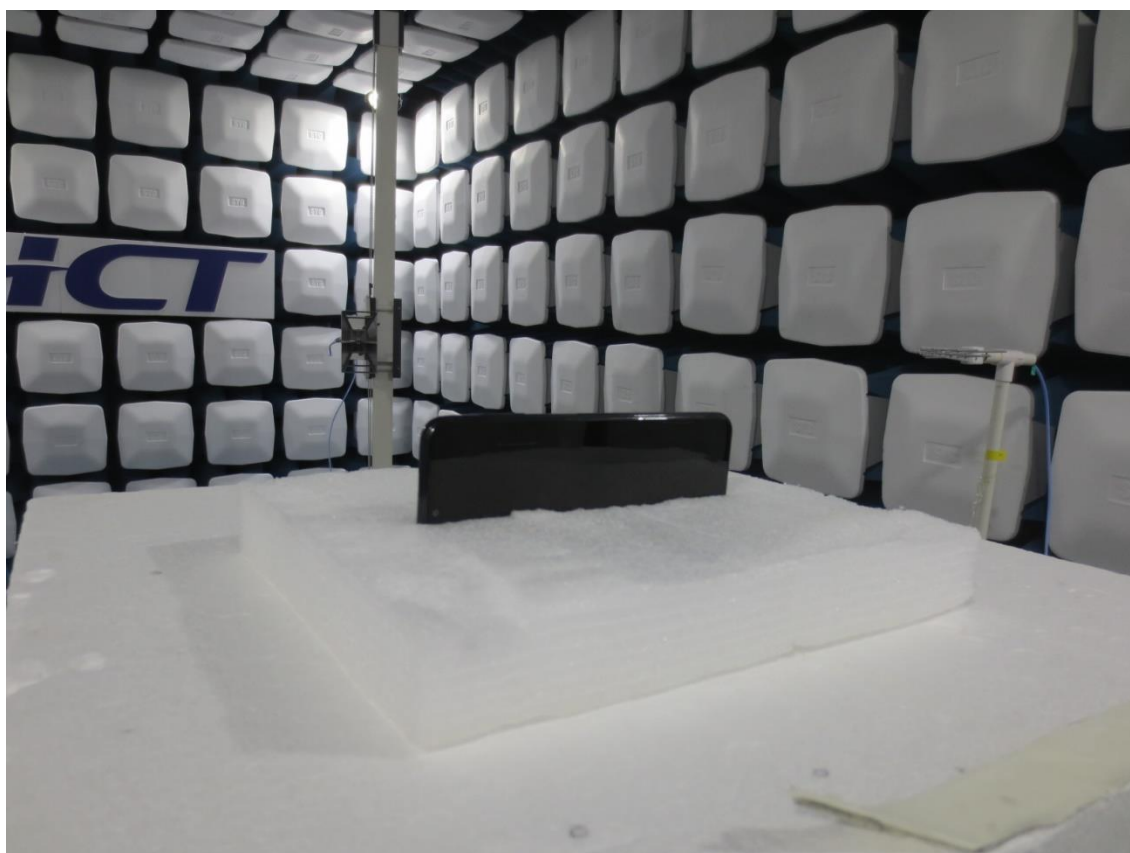


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

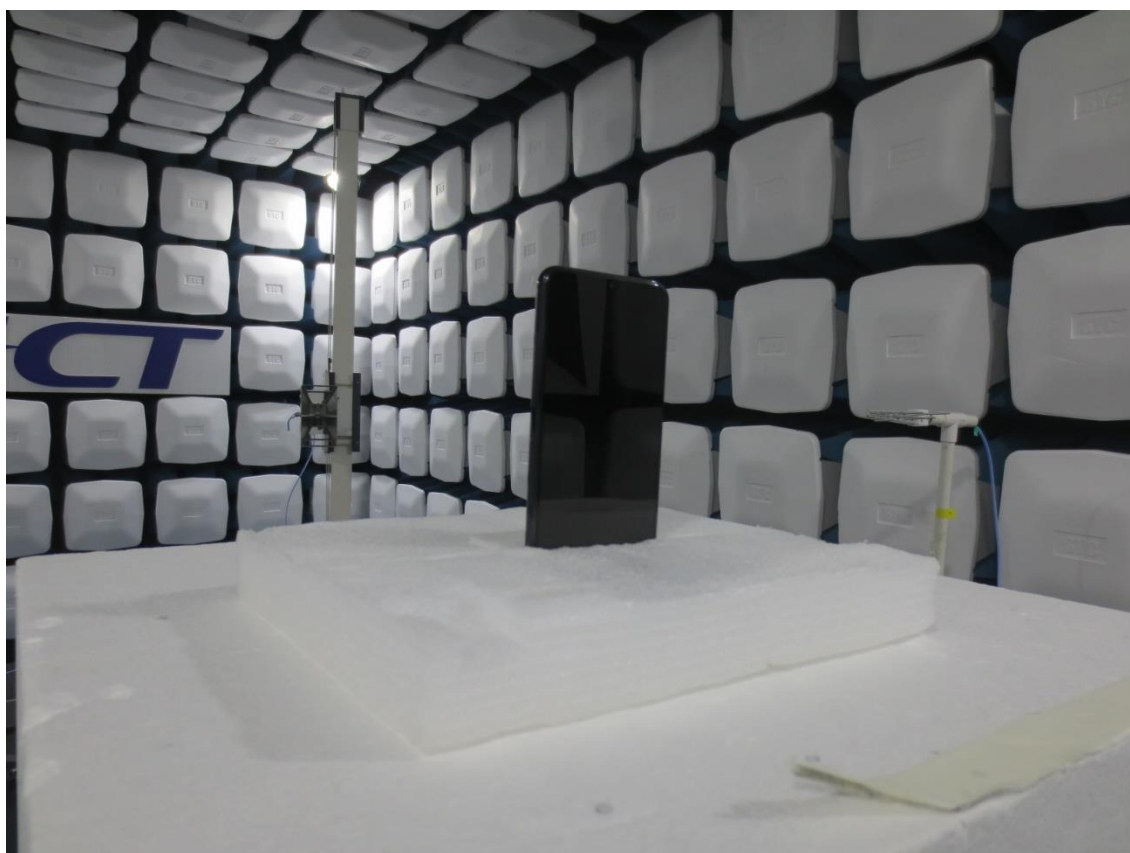


File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	




File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

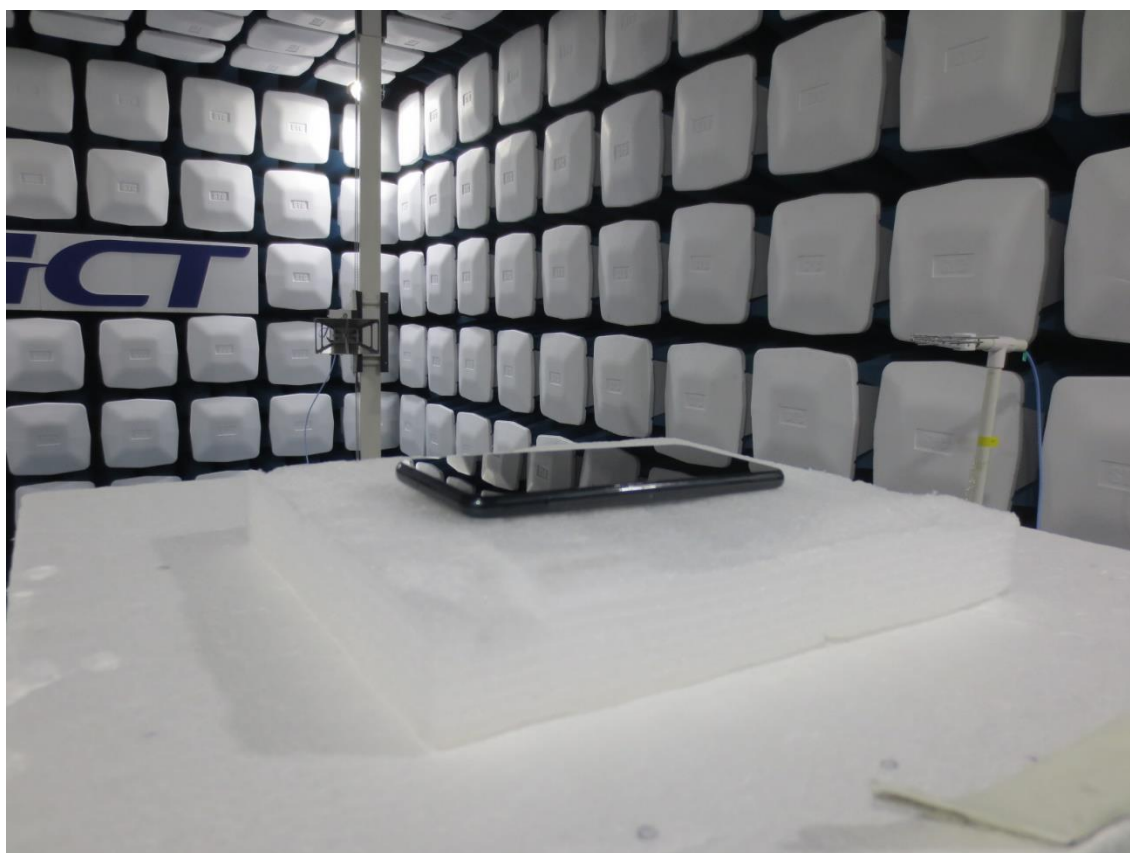

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

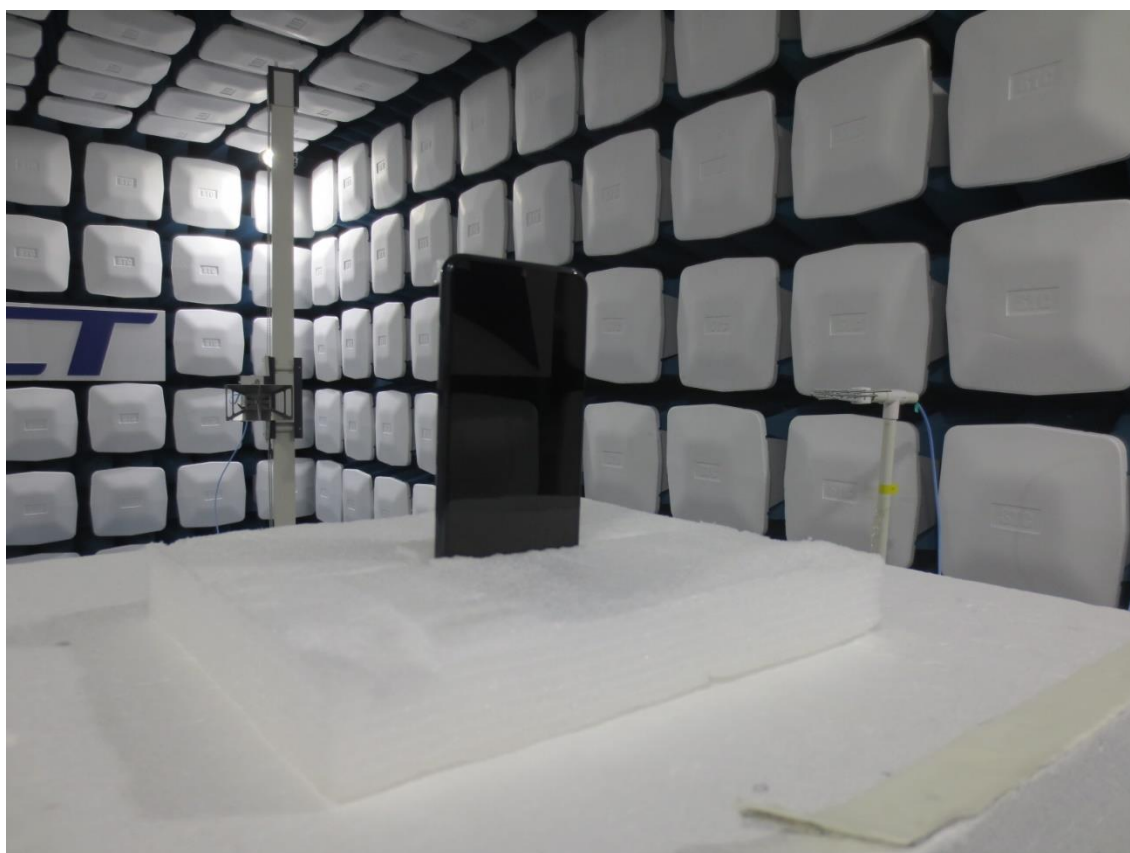

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

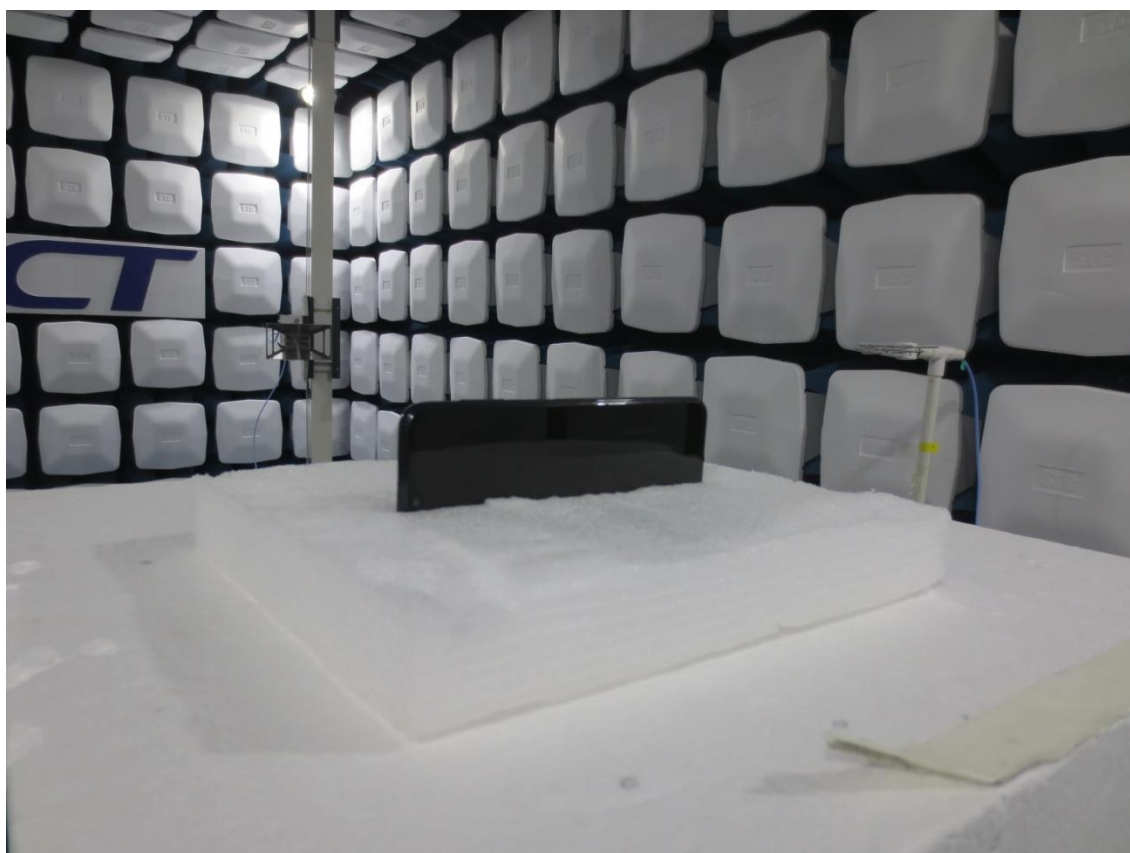

File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	

2. Conducted Test Setup Photo



File	HCT-RF-2201-FC090-P	HCT-RF-2201-FC091-P	HCT-RF-2201-FC092-P	HCT-RF-2201-FC093-P	HCT-RF-2201-FC094-P
No.	HCT-RF-2201-FC095-P	HCT-RF-2201-FC096-P	HCT-RF-2201-FC097-P	HCT-RF-2201-FC098-P	