



HCT Co., Ltd.

74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, 17383 KOREA
Tel. +82 31 634 6300 Fax. +82 31 645 6401

Appendix A:
Test Setup
Photo

FCC ID
A3LSMM356B

File No.

HCT-RF-2403-FC003-P	HCT-RF-2403-FC007-P	HCT-RF-2403-FC011-P
HCT-RF-2403-FC004-P	HCT-RF-2403-FC008-P	HCT-RF-2403-FC012-P
HCT-RF-2403-FC005-P	HCT-RF-2403-FC009-P	HCT-RF-2403-FC013-P
HCT-RF-2403-FC006-P	HCT-RF-2403-FC010-P	


REVISION HISTORY

The revision history for this document is shown in table.


Revision No.	Date of Issue	Description
0	March 21, 2024	Initial Release

File No.	HCT-RF-2403-FC003-P	HCT-RF-2403-FC004-P	HCT-RF-2403-FC005-P	HCT-RF-2403-FC006-P	HCT-RF-2403-FC007-P
	HCT-RF-2403-FC008-P	HCT-RF-2403-FC009-P	HCT-RF-2403-FC010-P	HCT-RF-2403-FC011-P	HCT-RF-2403-FC012-P
	HCT-RF-2403-FC013-P				

1. Radiated Test Setup Photo

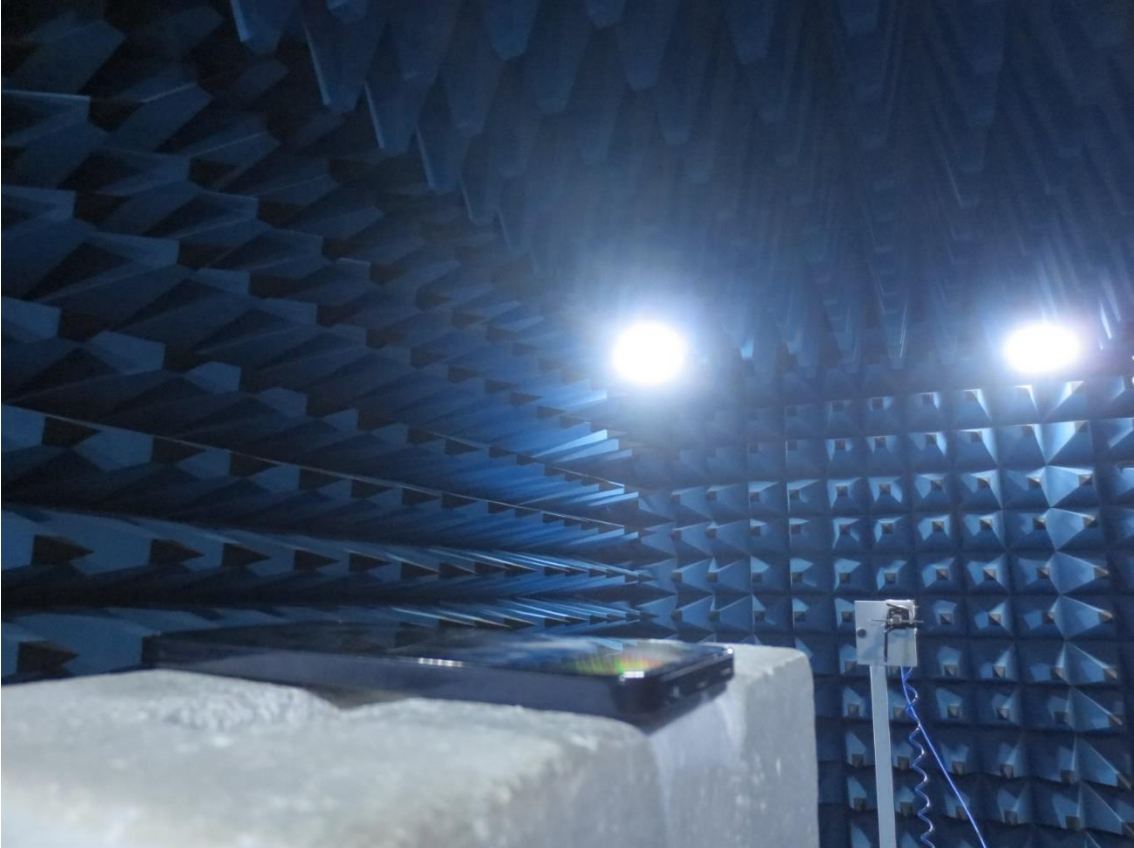

File No.	HCT-RF-2403-FC003-P	HCT-RF-2403-FC004-P	HCT-RF-2403-FC005-P	HCT-RF-2403-FC006-P	HCT-RF-2403-FC007-P
	HCT-RF-2403-FC008-P	HCT-RF-2403-FC009-P	HCT-RF-2403-FC010-P	HCT-RF-2403-FC011-P	HCT-RF-2403-FC012-P
	HCT-RF-2403-FC013-P				

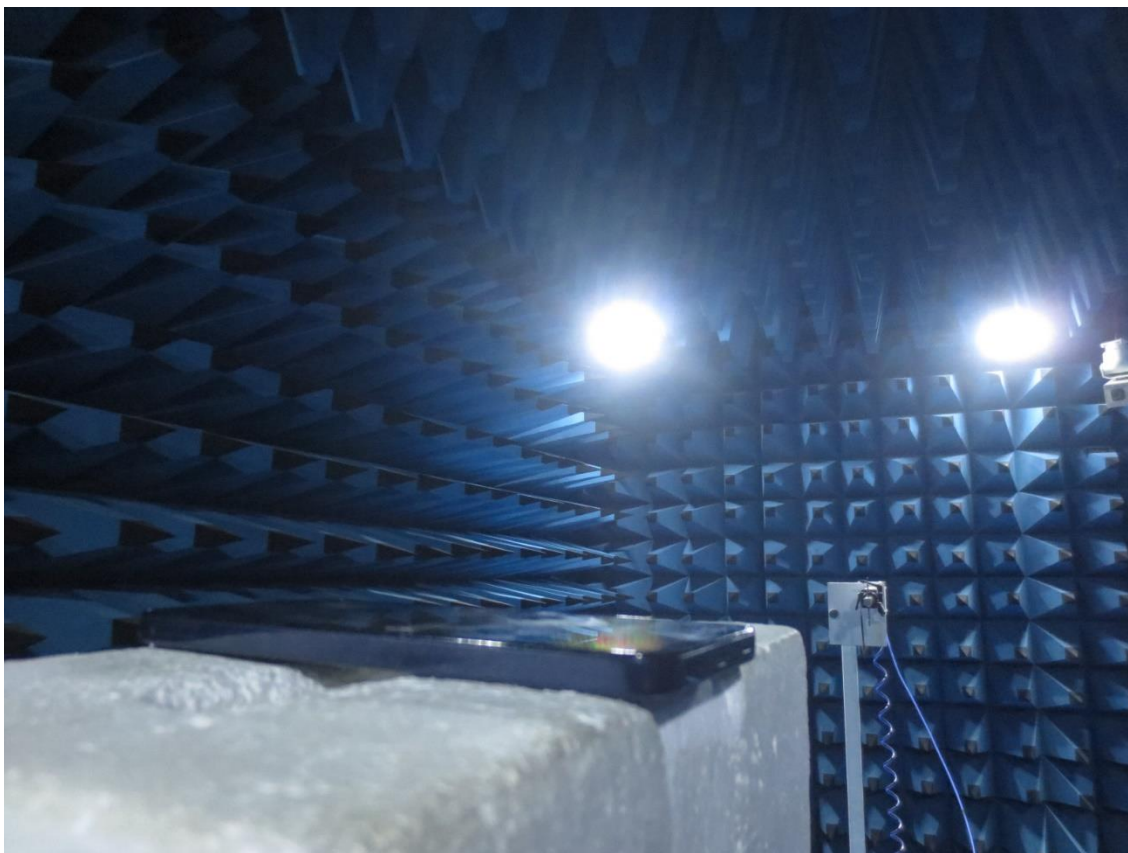

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

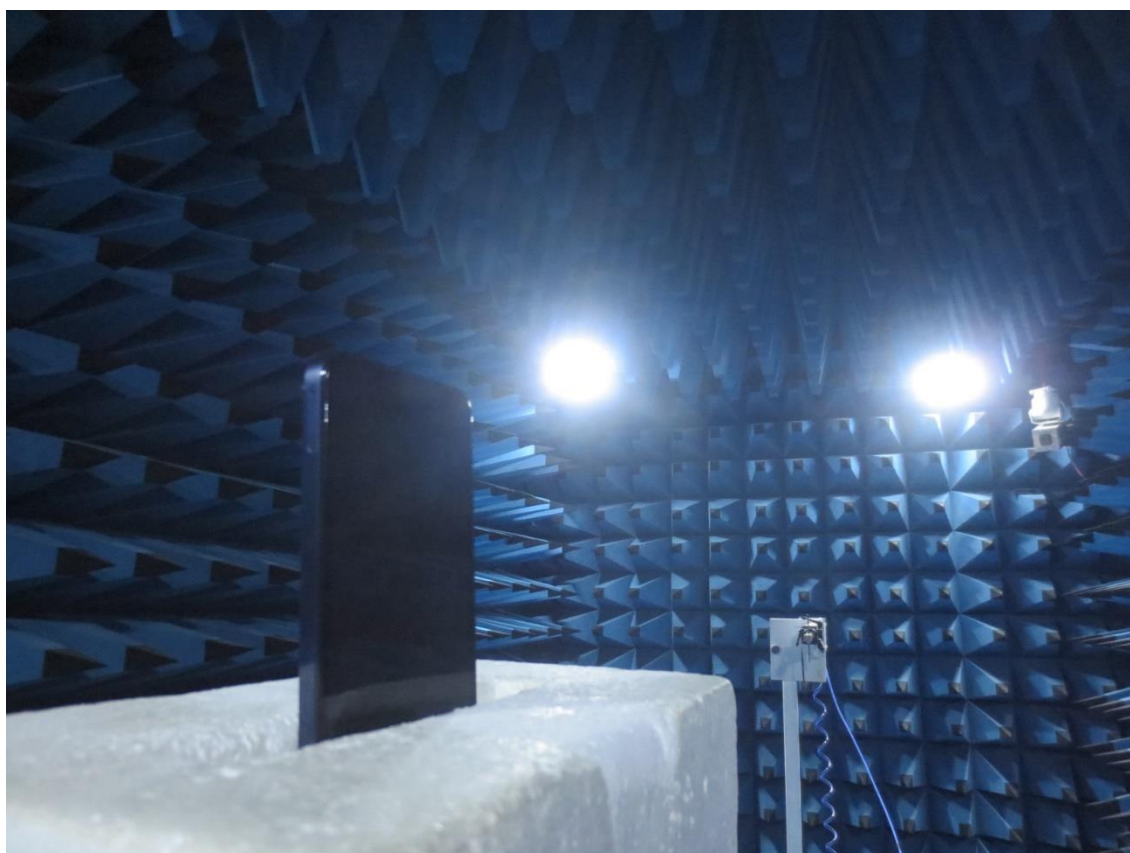

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

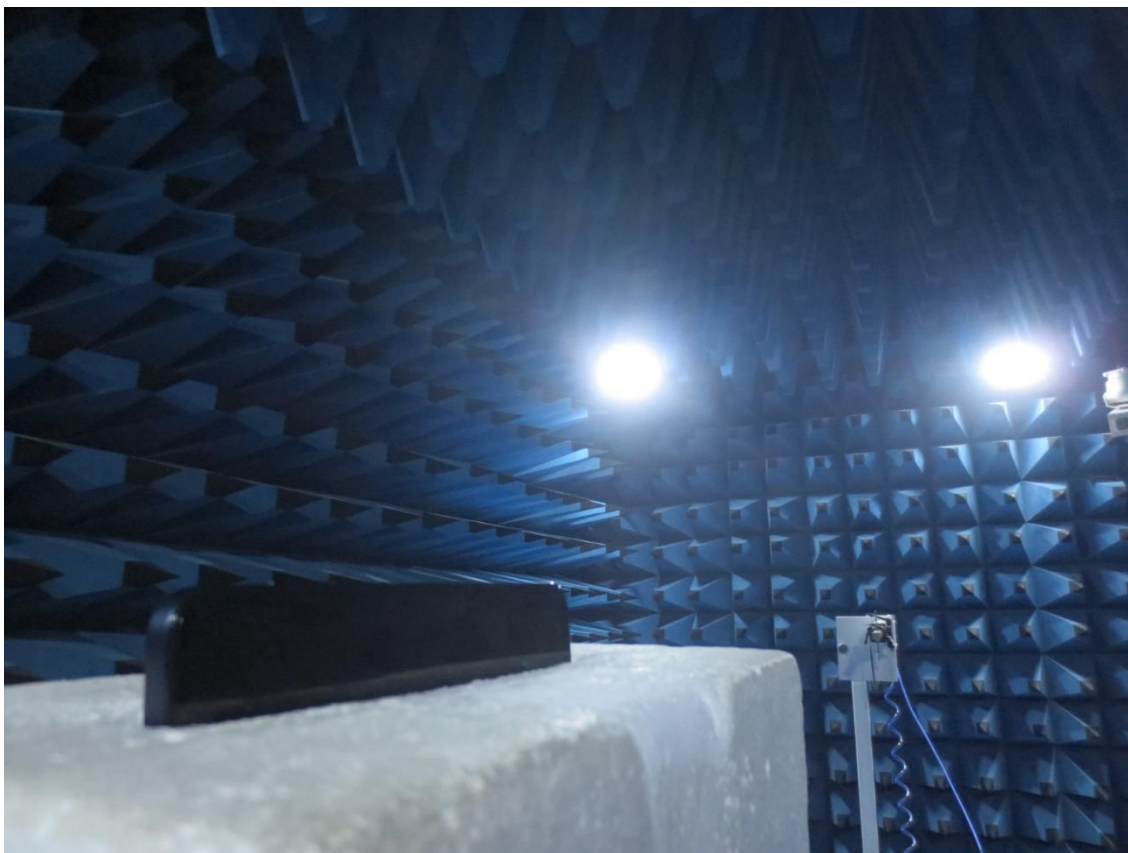

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

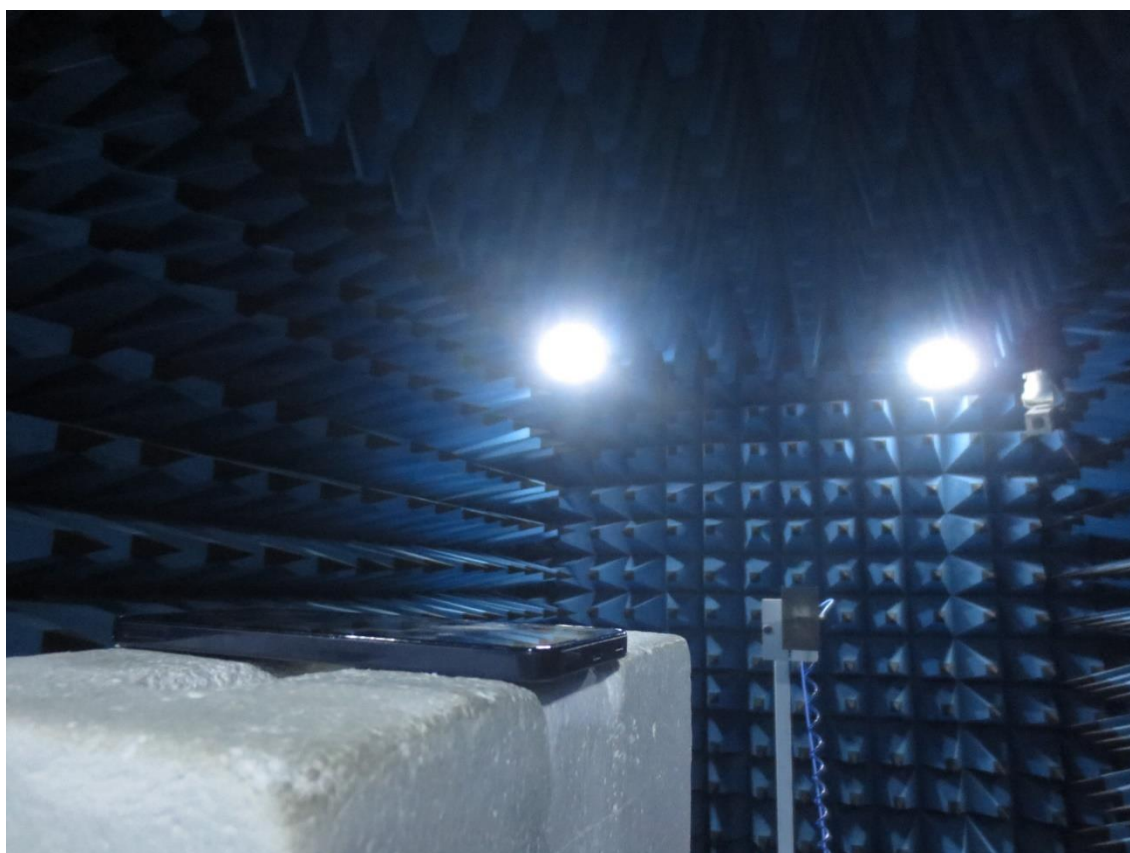

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

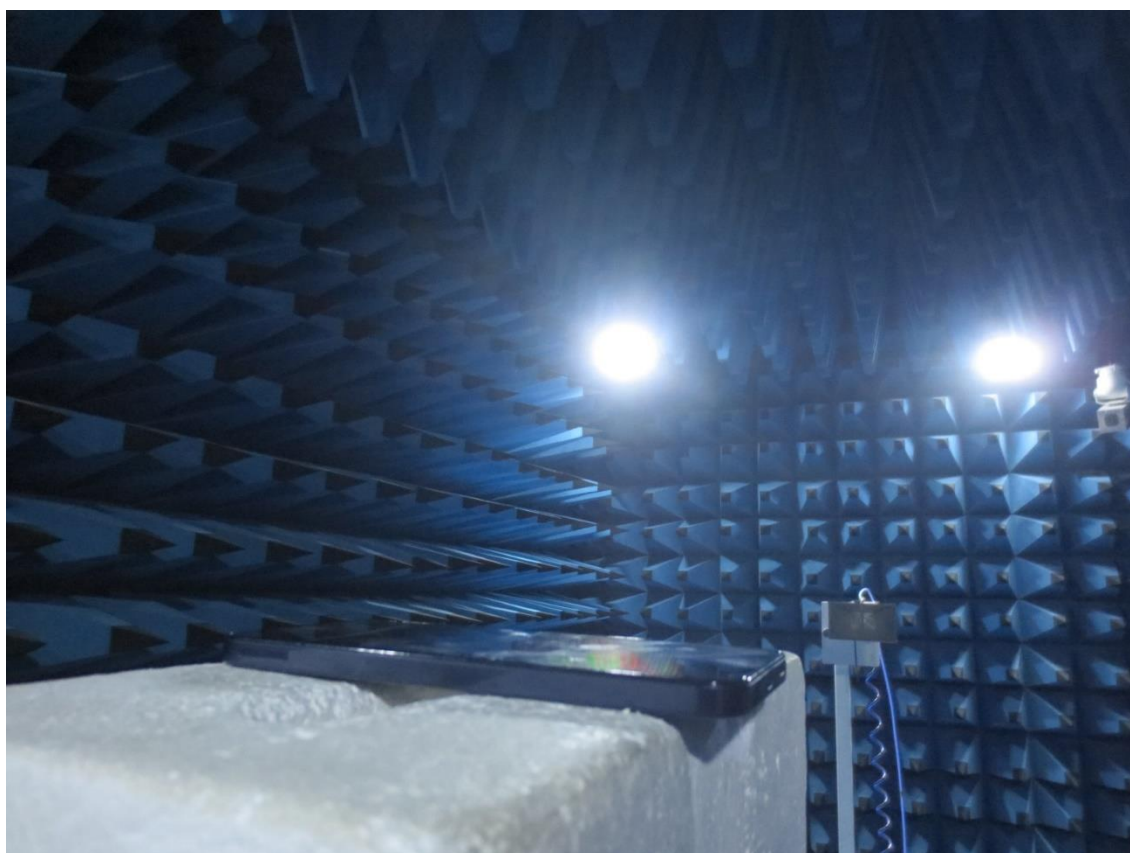

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

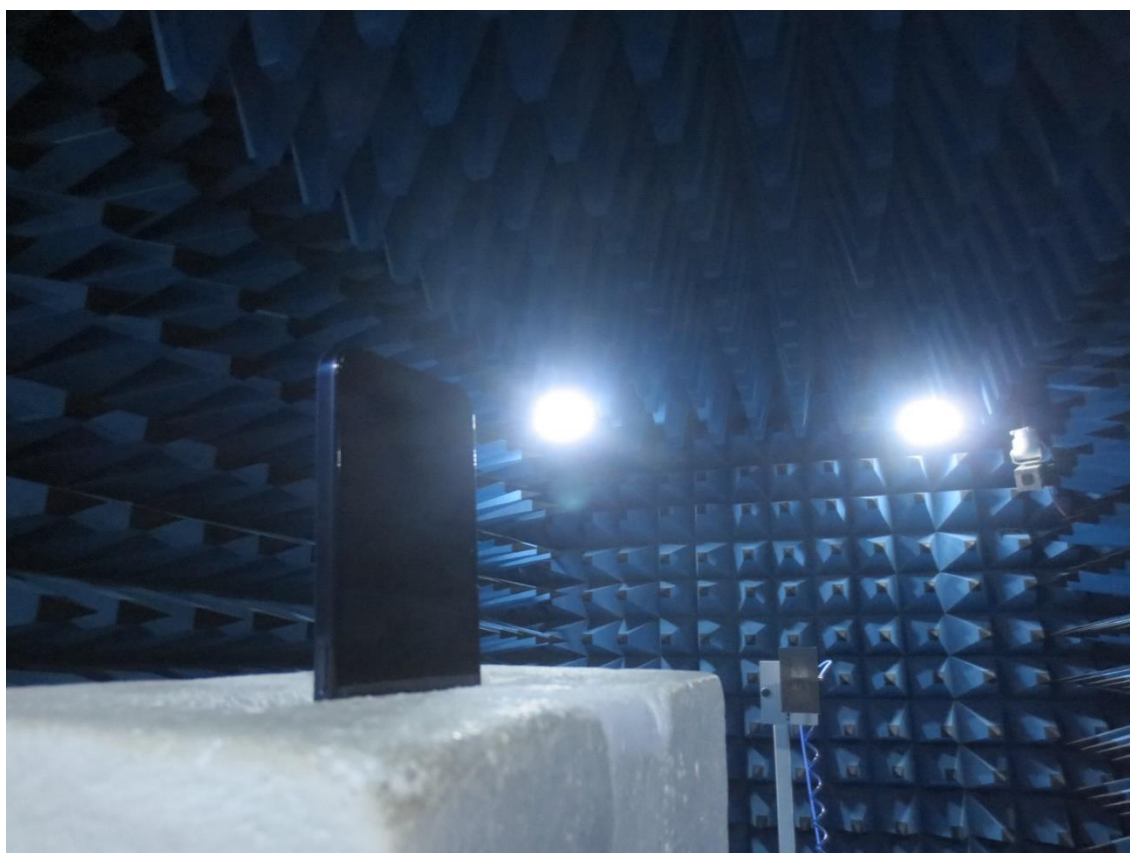

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

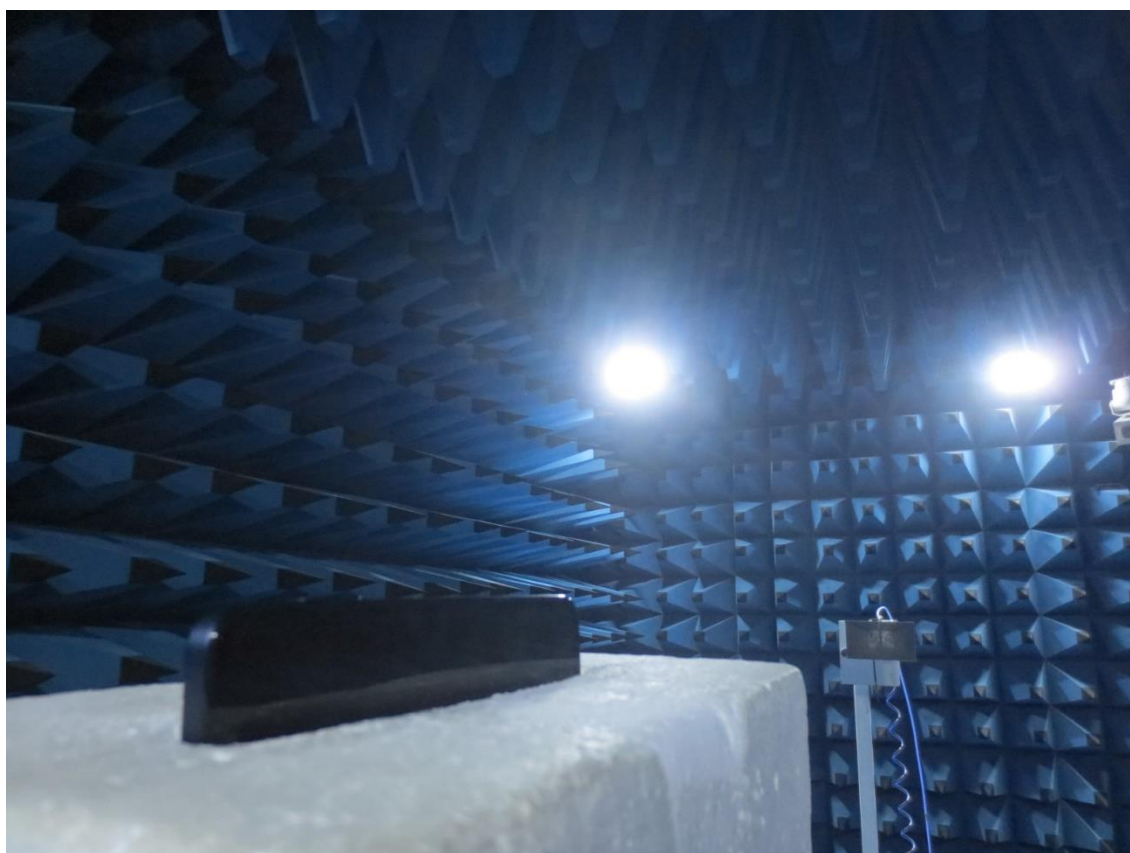

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

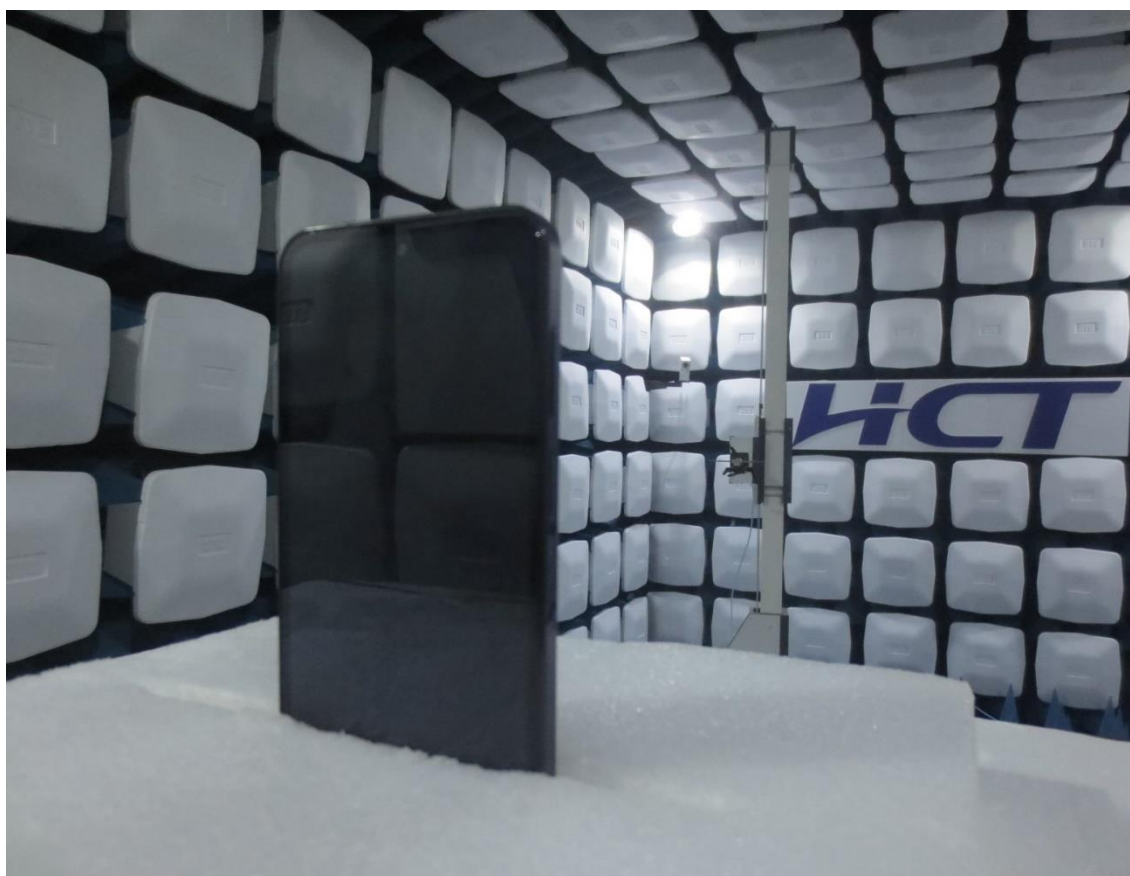

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

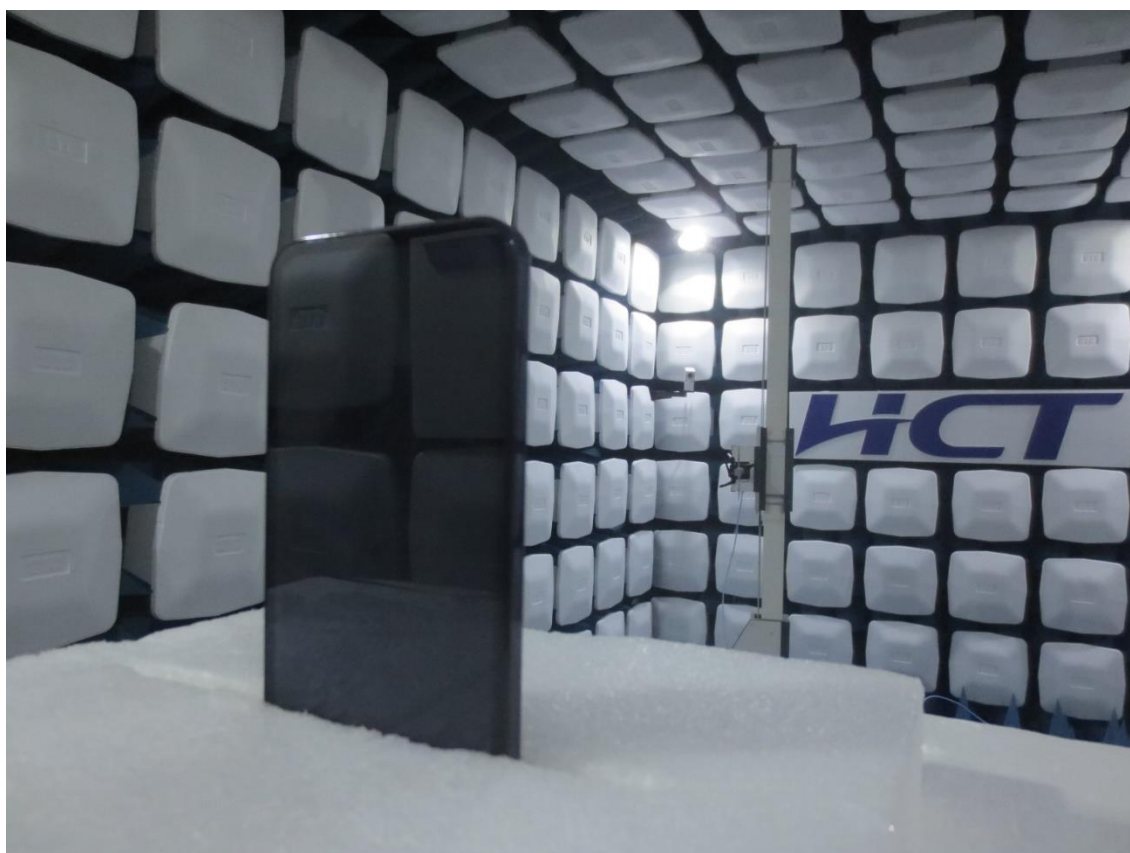

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

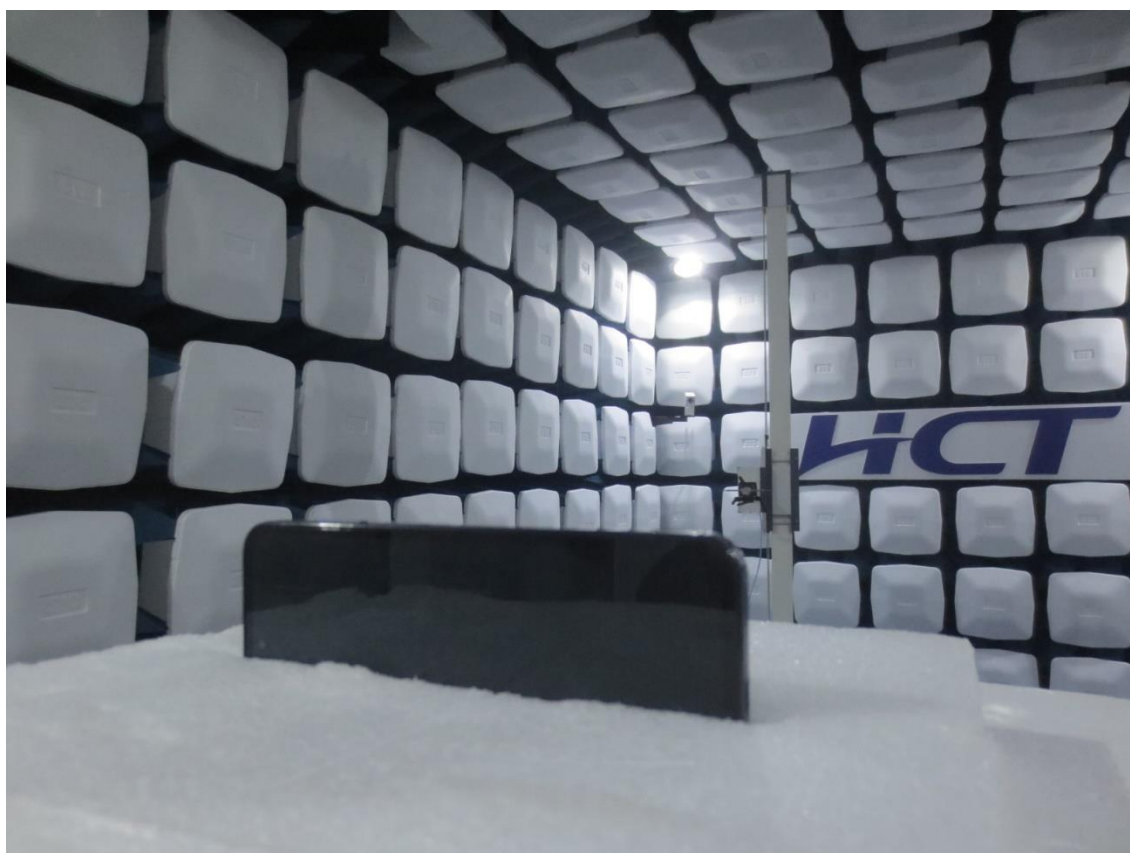

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

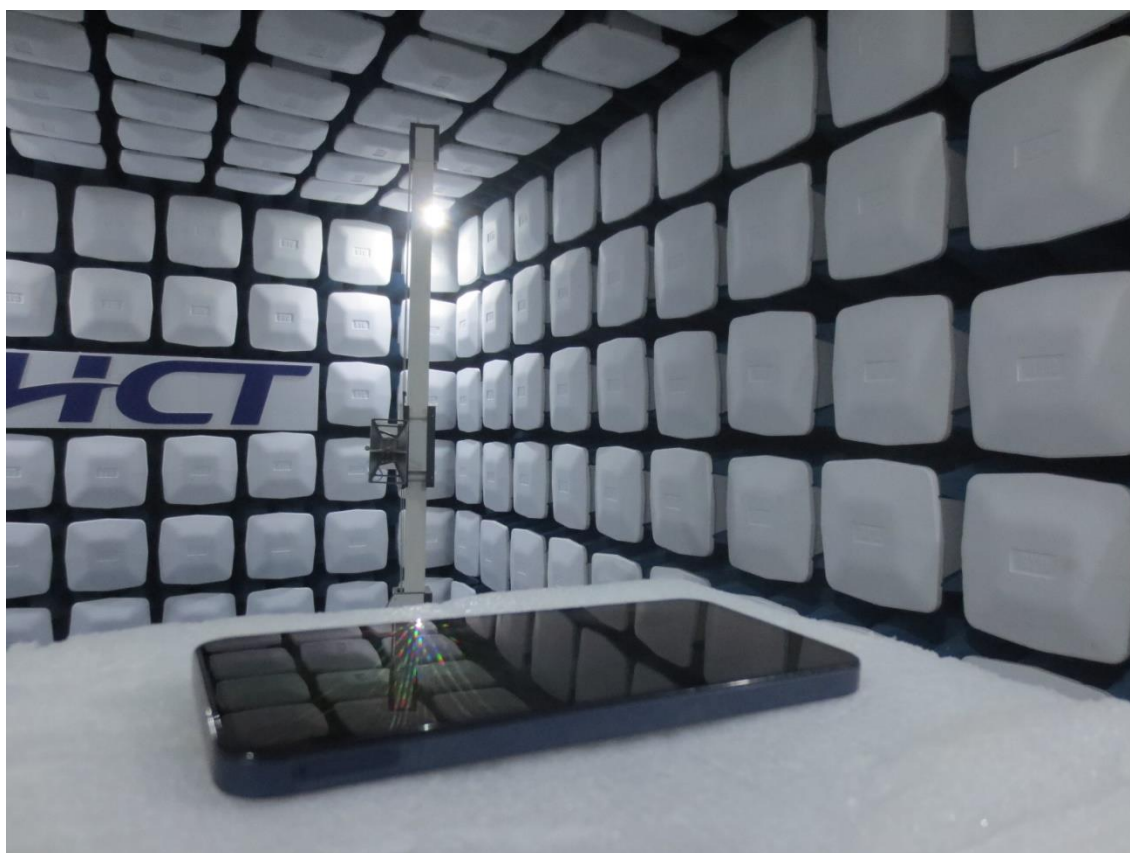

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

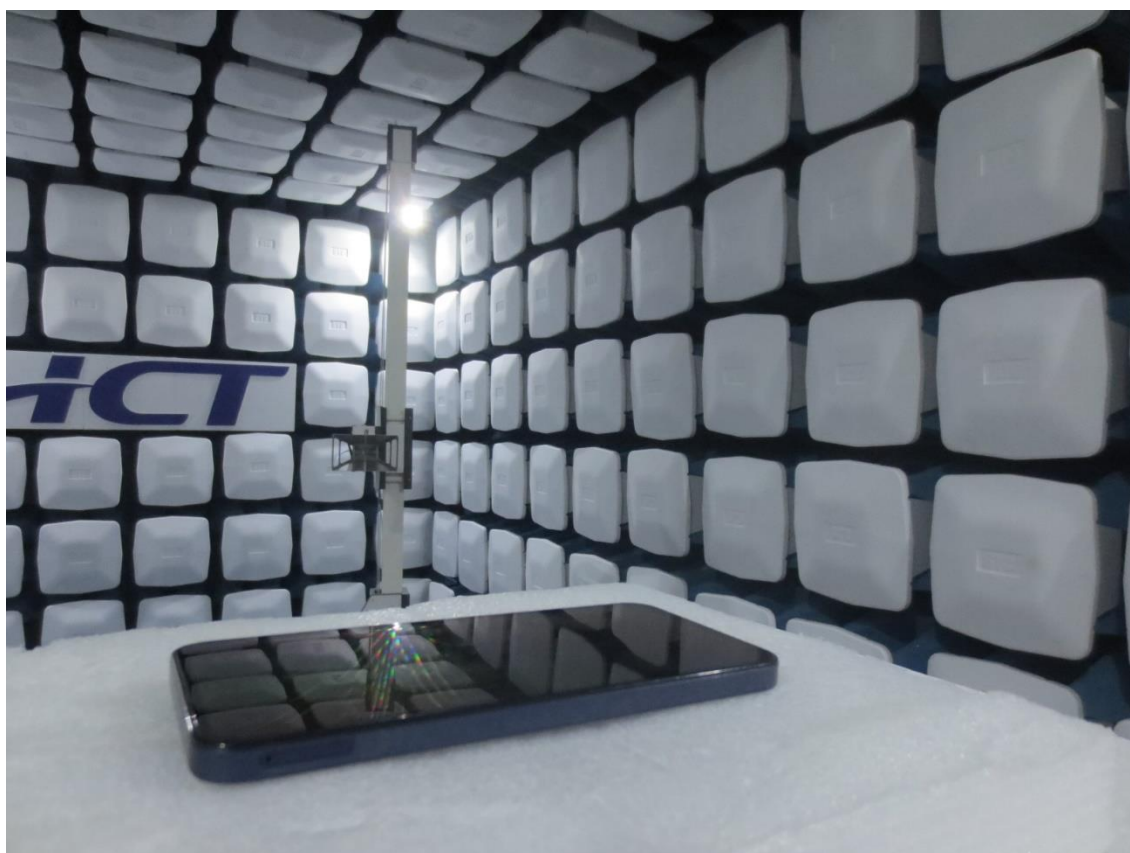

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

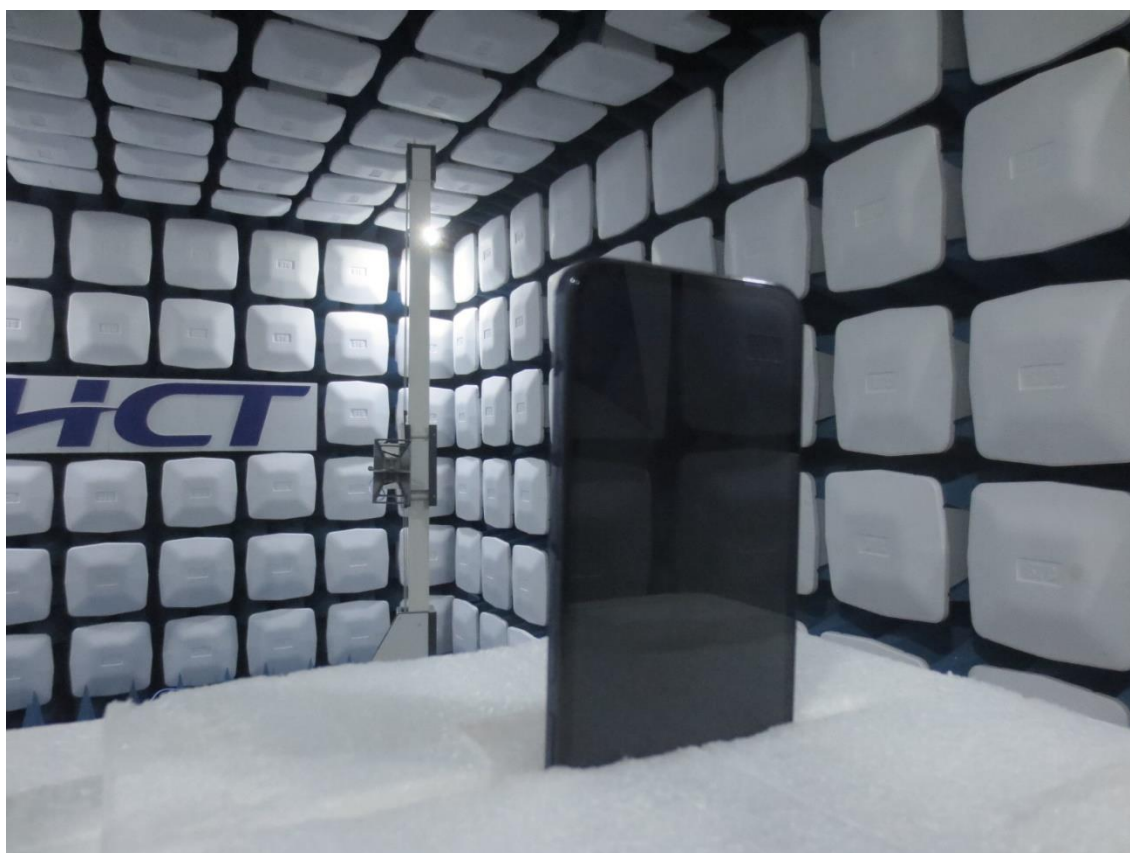

File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

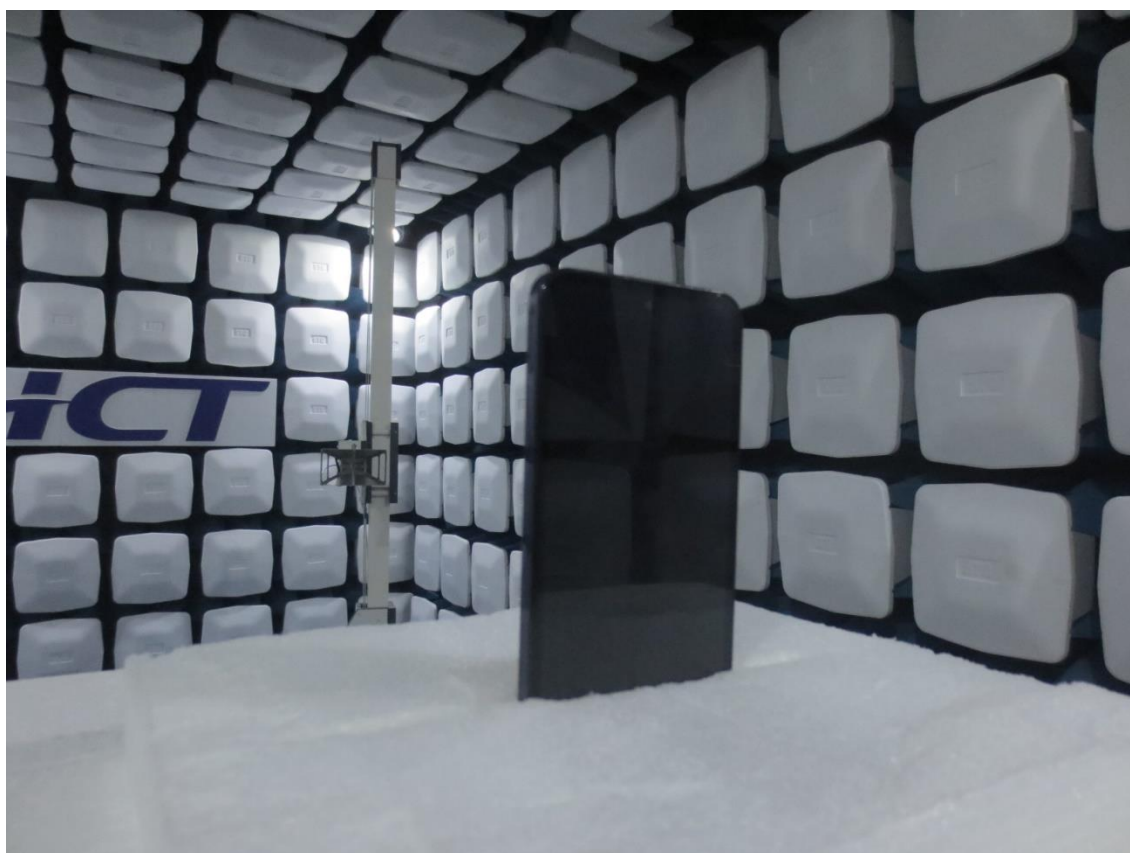

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P



File
No.


HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P

HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

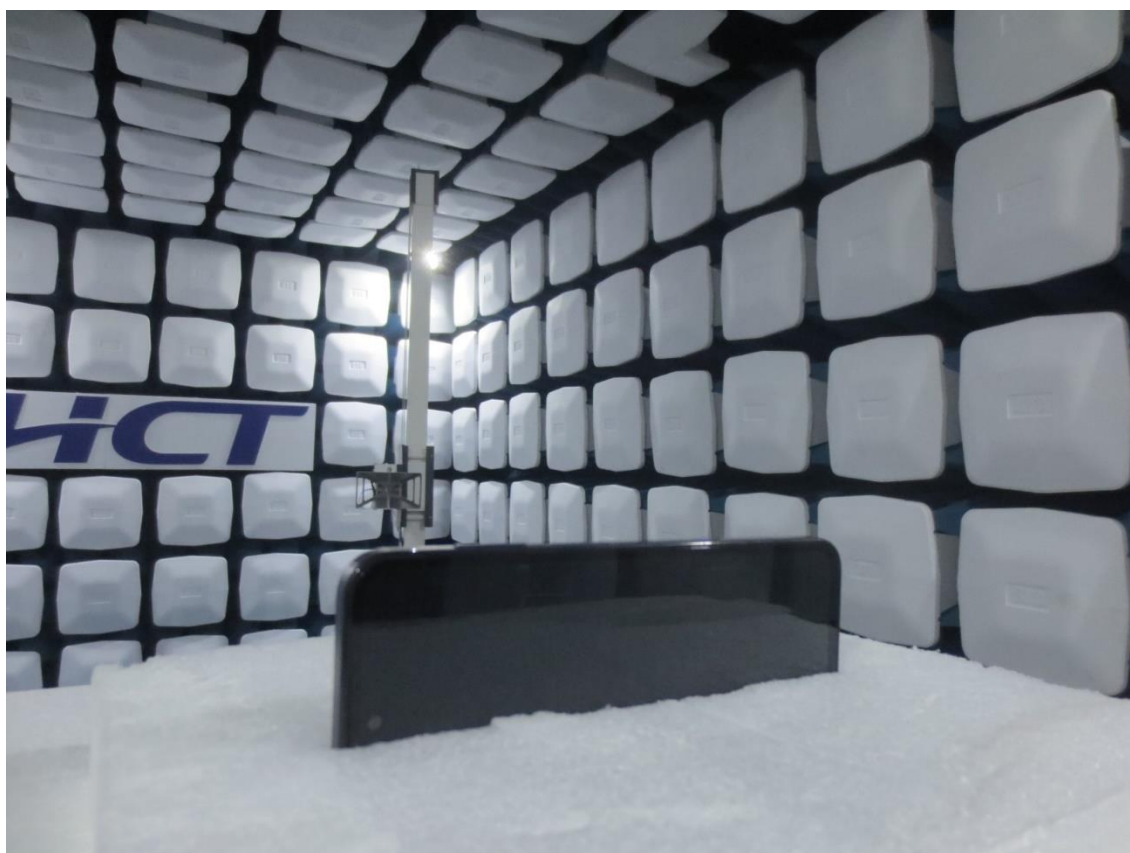

File
No.

HCT-RF-2403-FC003-P
HCT-RF-2403-FC008-P
HCT-RF-2403-FC013-P


HCT-RF-2403-FC004-P
HCT-RF-2403-FC009-P

HCT-RF-2403-FC005-P
HCT-RF-2403-FC010-P

HCT-RF-2403-FC006-P
HCT-RF-2403-FC011-P

HCT-RF-2403-FC007-P
HCT-RF-2403-FC012-P

2. Conducted Test Setup Photo

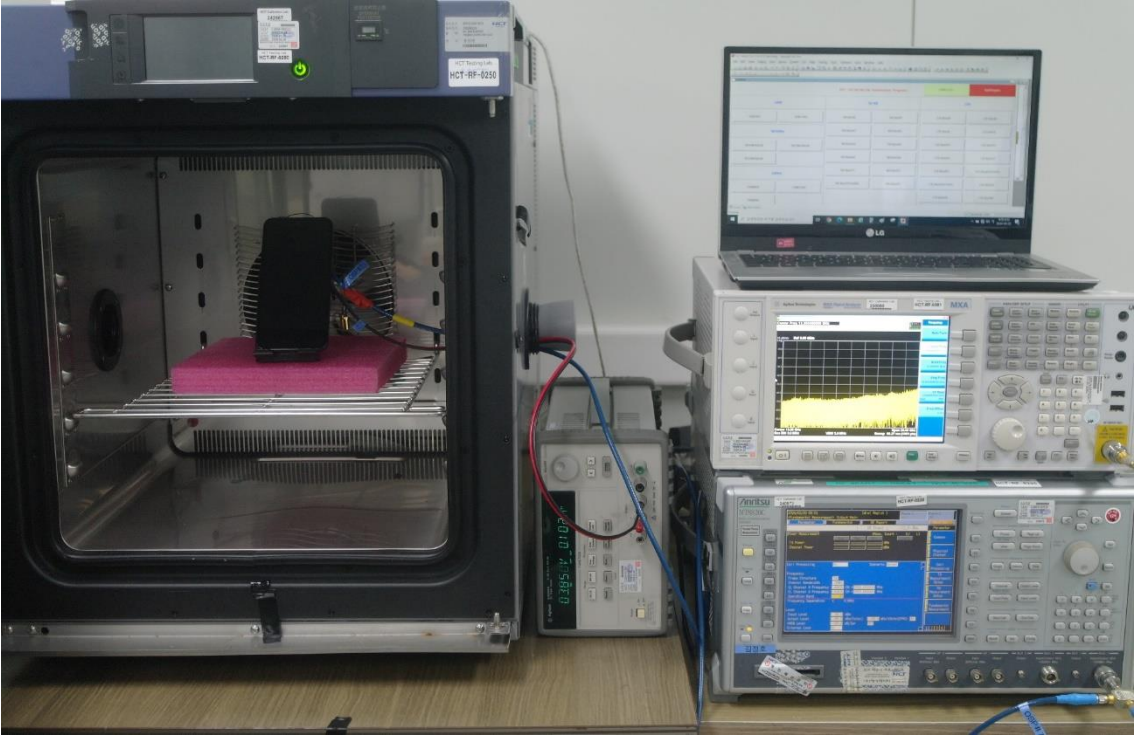

File	HCT-RF-2403-FC003-P	HCT-RF-2403-FC004-P	HCT-RF-2403-FC005-P	HCT-RF-2403-FC006-P	HCT-RF-2403-FC007-P
No.	HCT-RF-2403-FC008-P	HCT-RF-2403-FC009-P	HCT-RF-2403-FC010-P	HCT-RF-2403-FC011-P	HCT-RF-2403-FC012-P
	HCT-RF-2403-FC013-P				