



HCT Co., Ltd.

2-6, 73, 74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, Republic of Korea

Tel. +82 31 645 6300 Fax. +82 31 645 6401

Appendix A: Test Setup Photo

FCC ID
A3LSMS731B

File No.

HCT-RF-2507-FC057-P	HCT-RF-2507-FC070-P
HCT-RF-2507-FC058-P	HCT-RF-2507-FC072-P
HCT-RF-2507-FC059-P	HCT-RF-2507-FC073-P
HCT-RF-2507-FC060-P	HCT-RF-2507-FC074-P
HCT-RF-2507-FC061-P	HCT-RF-2507-FC075-P
HCT-RF-2507-FC062-P	HCT-RF-2507-FC076-P
HCT-RF-2507-FC066-P	
HCT-RF-2507-FC067-P	
HCT-RF-2507-FC068-P	
HCT-RF-2507-FC069-P	


REVISION HISTORY

The revision history for this document is shown in table.


Revision No.	Date of Issue	Description
0	July 15, 2025	Initial Release

	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

1. Radiated Test Setup Photo

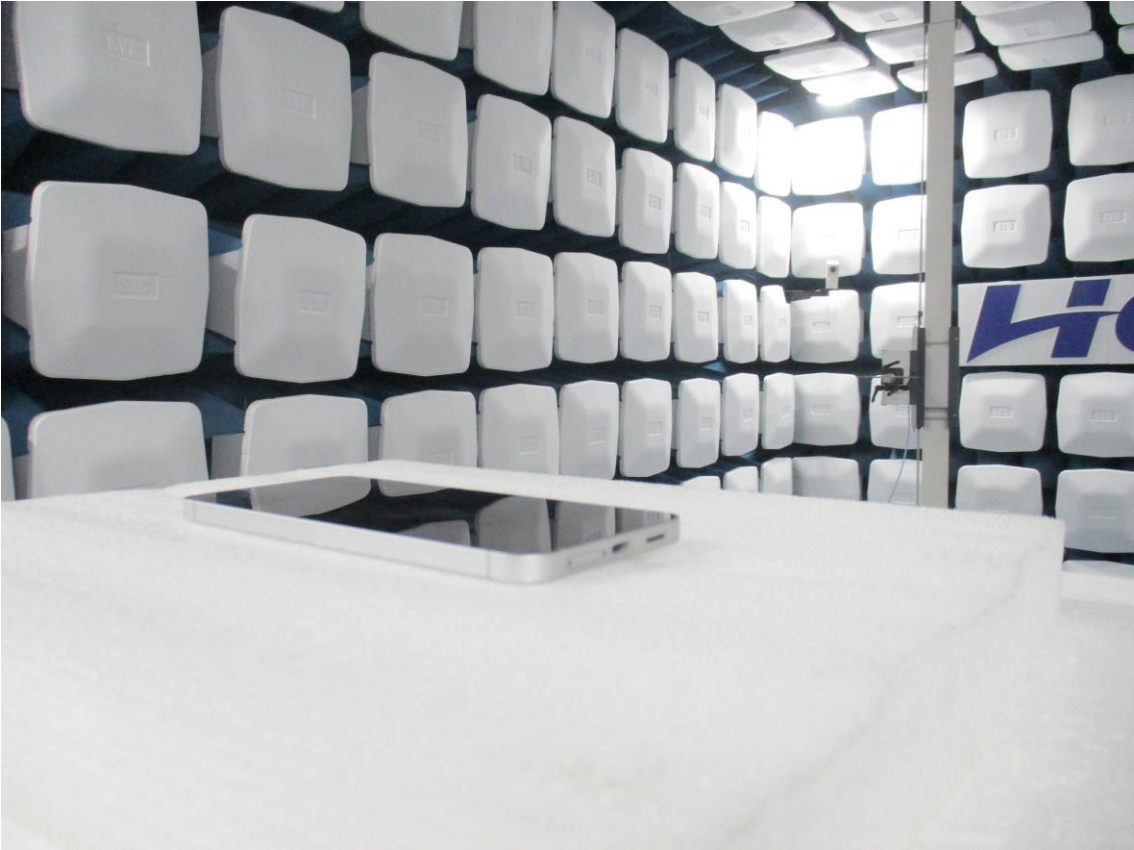


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

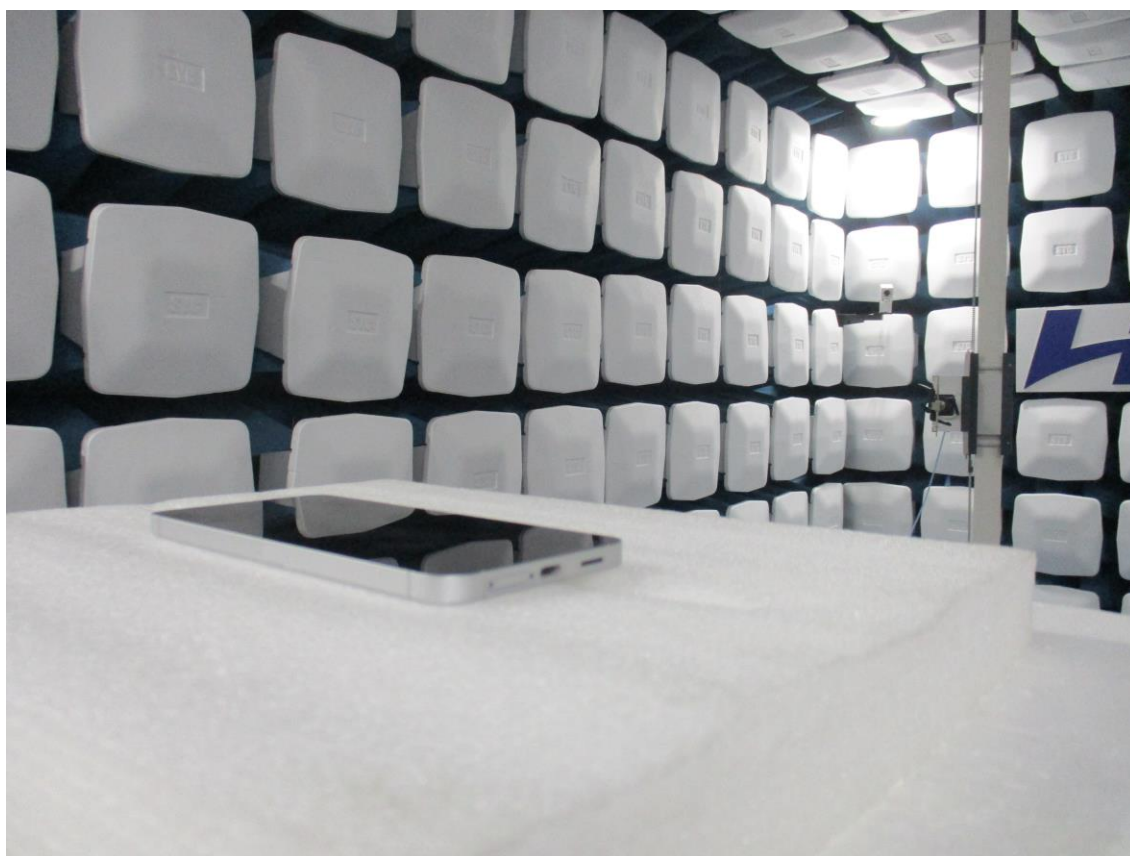


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				




	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

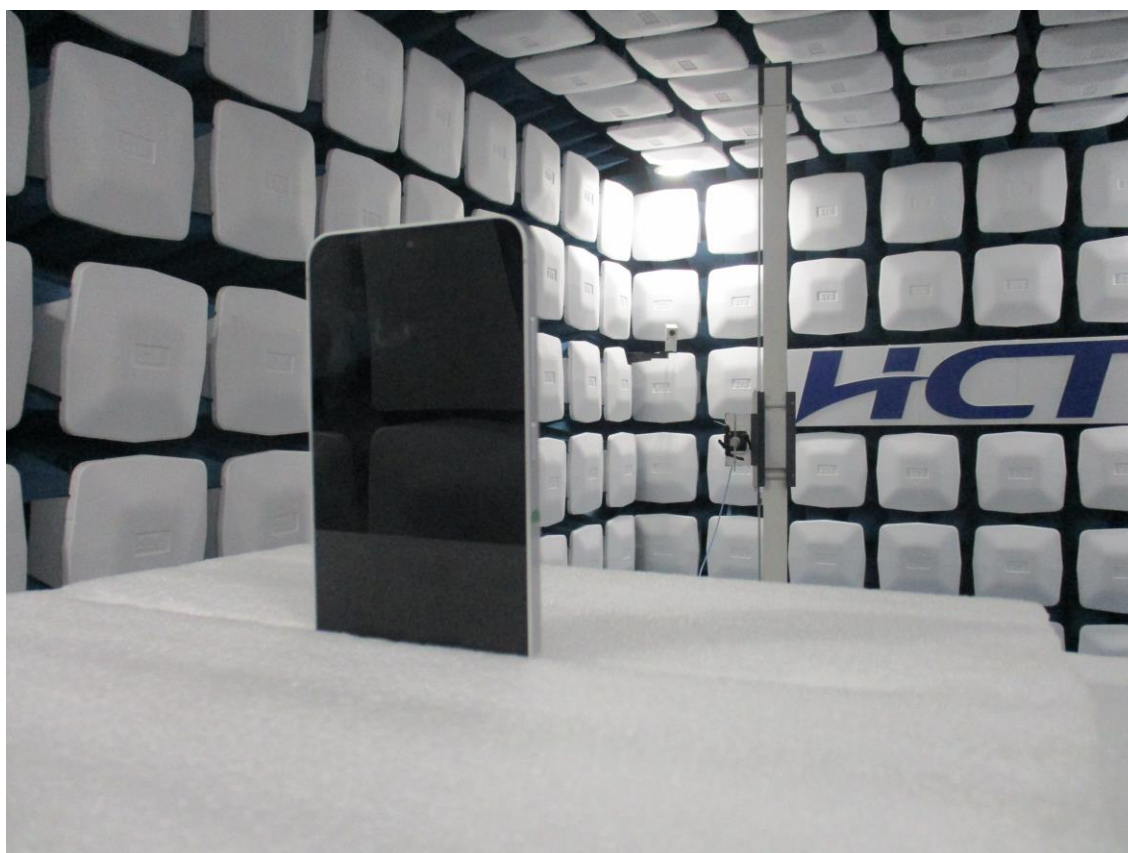


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

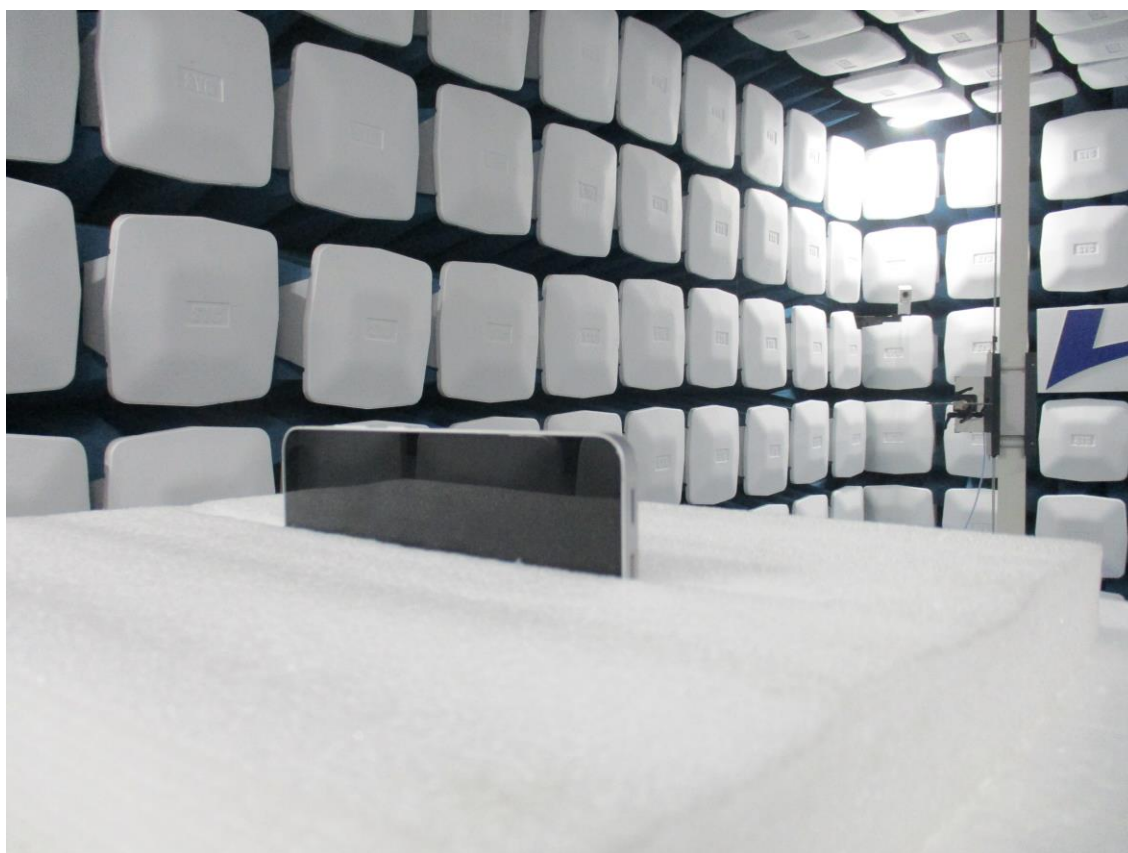


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

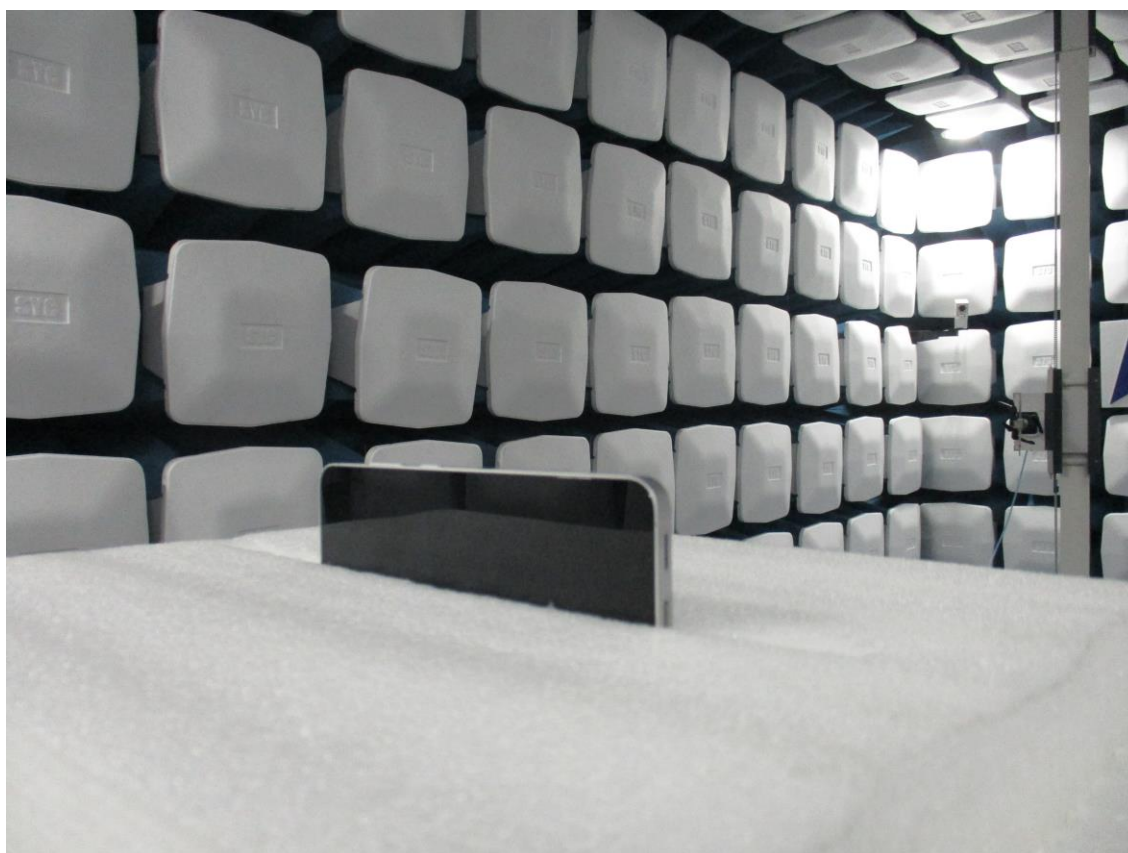


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

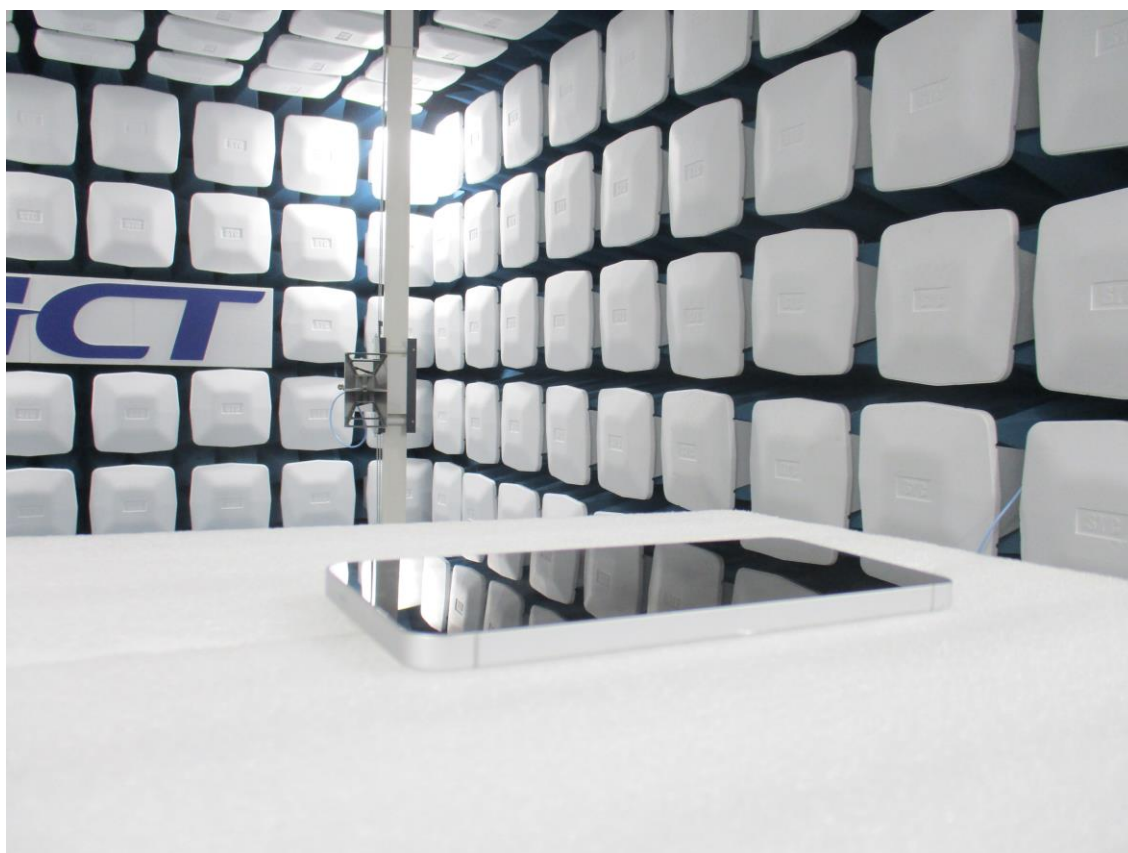


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

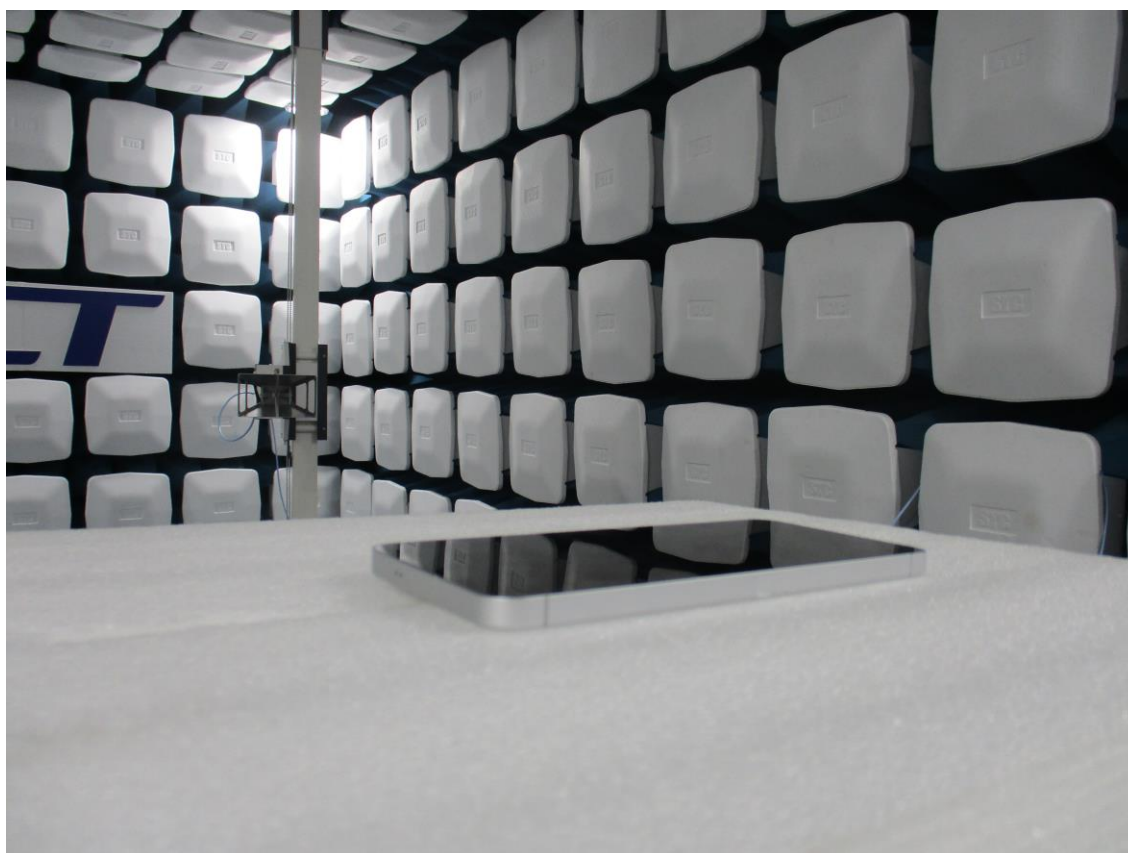


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

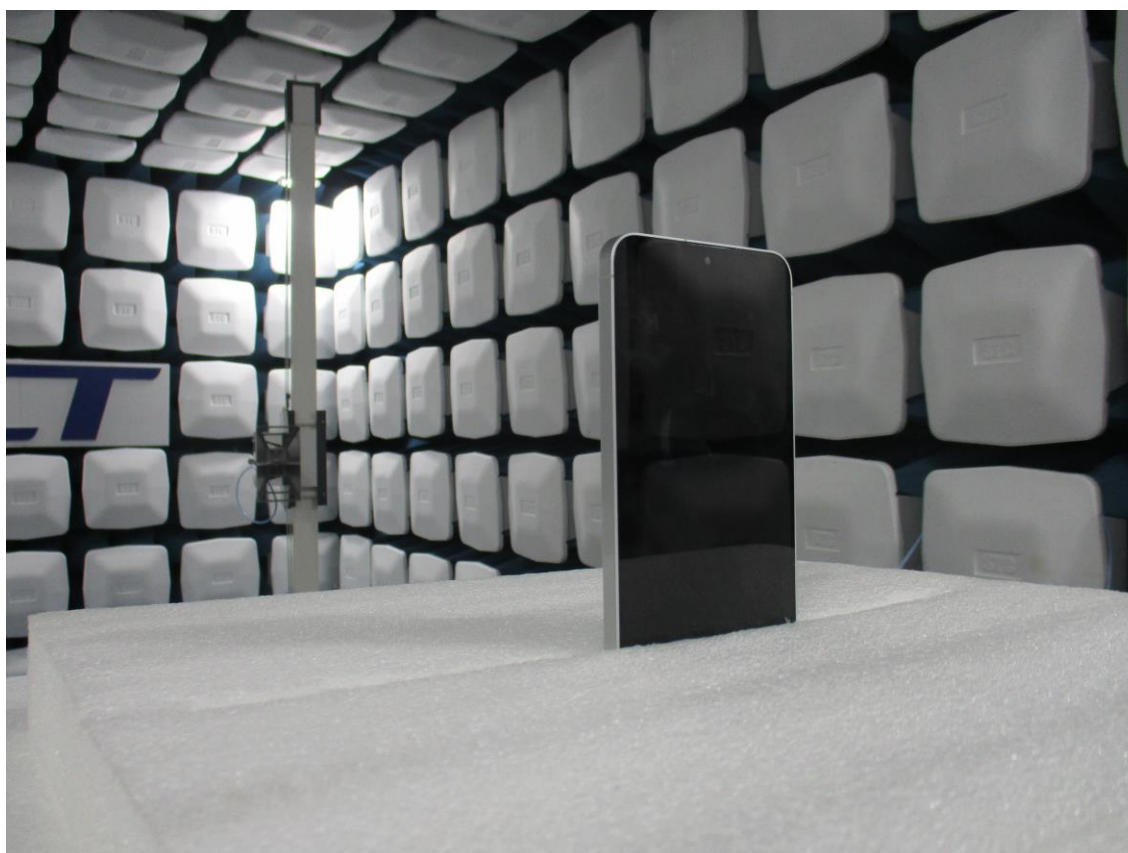


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

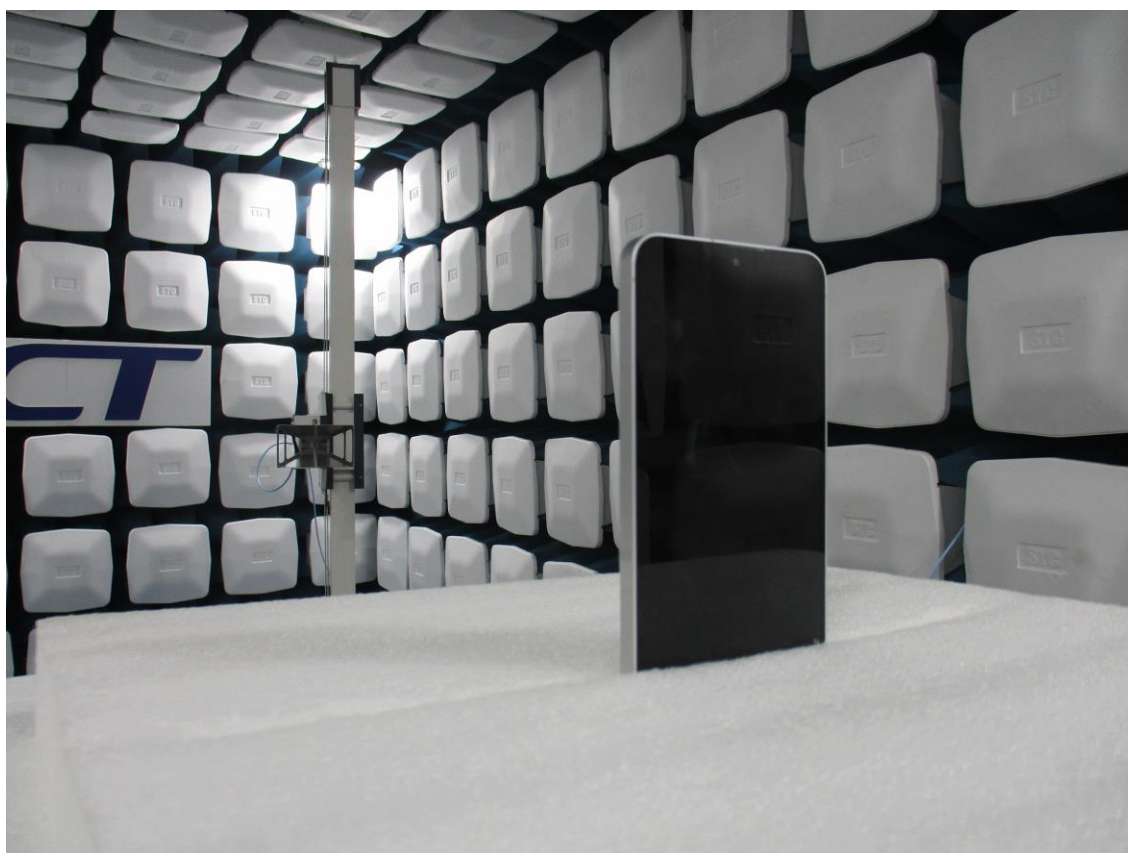

	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

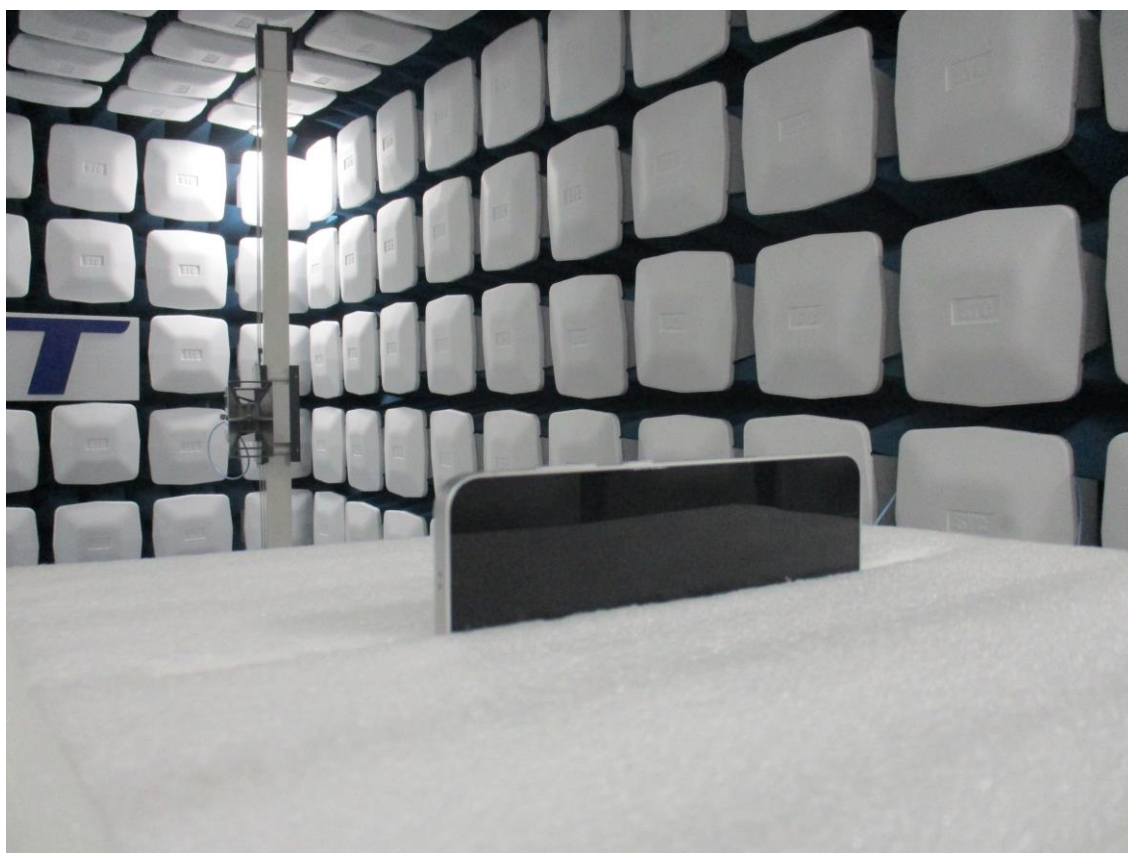


	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

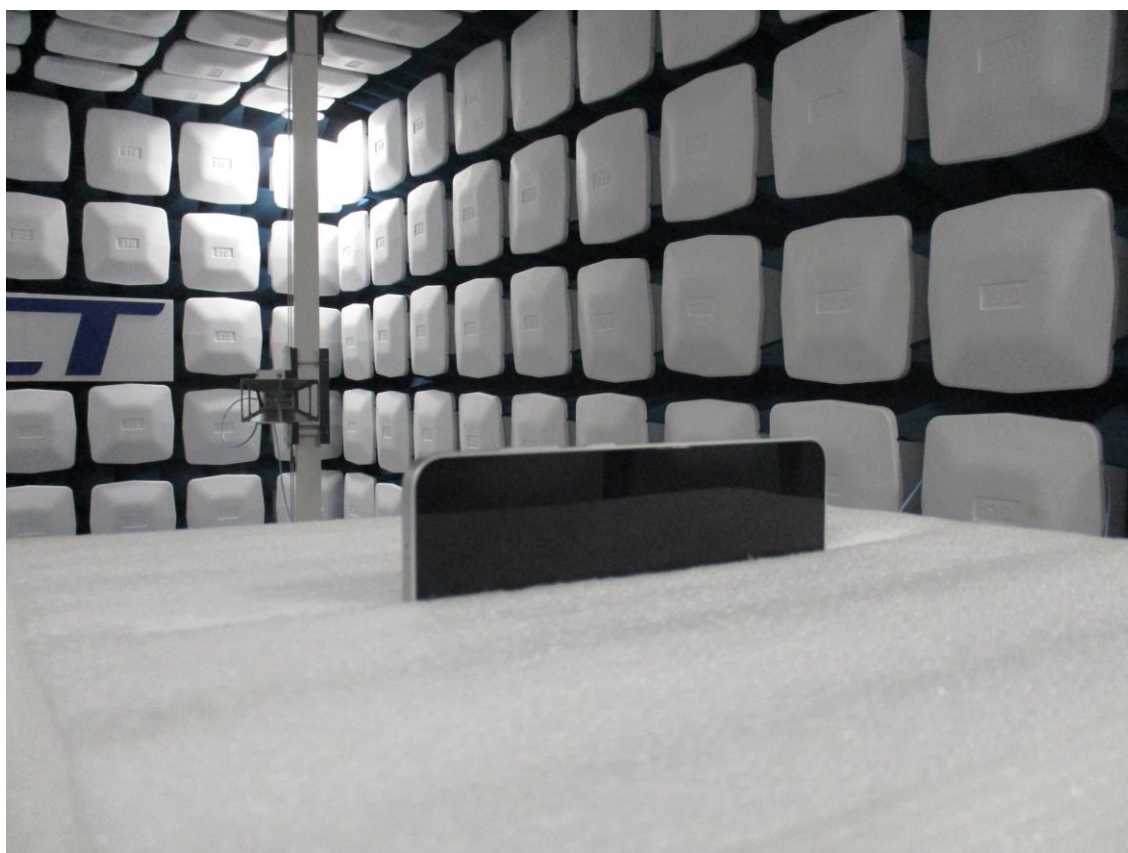

	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				

2. Conducted Test Setup Photo

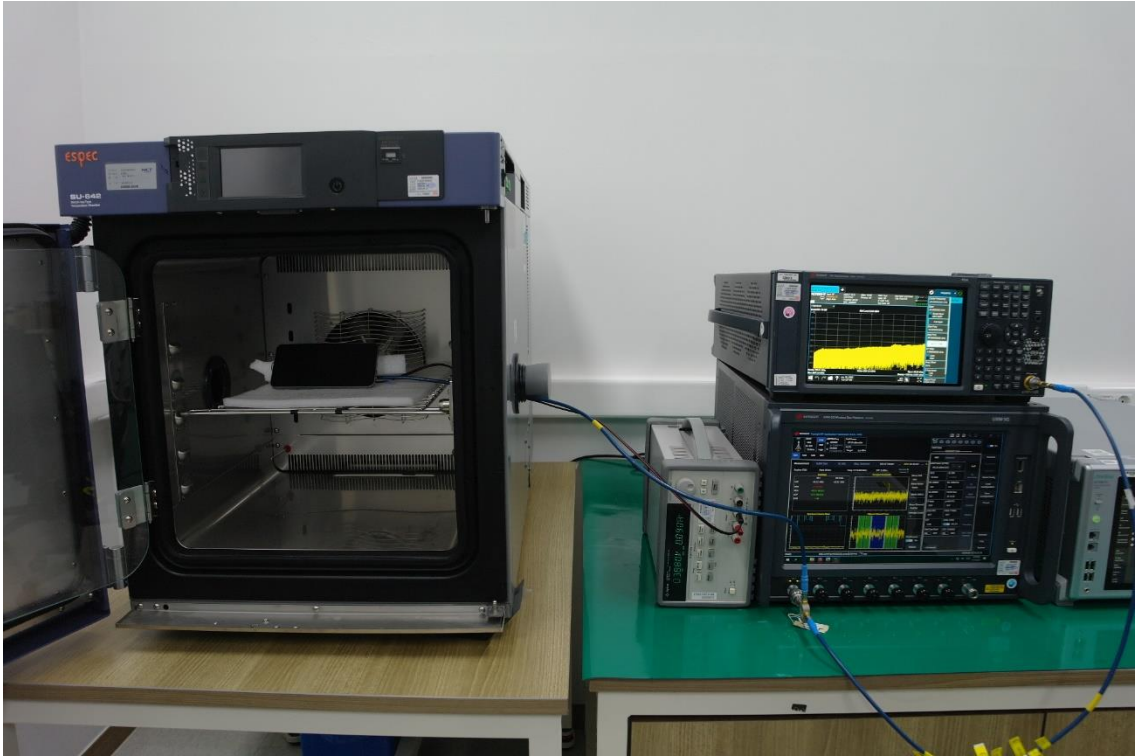

End of Report

	HCT-RF-2507-FC057-P	HCT-RF-2507-FC058-P	HCT-RF-2507-FC059-P	HCT-RF-2507-FC060-P	HCT-RF-2507-FC061-P
File	HCT-RF-2507-FC062-P	HCT-RF-2507-FC066-P	HCT-RF-2507-FC067-P	HCT-RF-2507-FC068-P	HCT-RF-2507-FC069-P
No.	HCT-RF-2507-FC070-P	HCT-RF-2507-FC072-P	HCT-RF-2507-FC073-P	HCT-RF-2507-FC074-P	HCT-RF-2507-FC075-P
	HCT-RF-2507-FC076-P				