

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	14.3, 16.56,15.27

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-24	22.5	22.6	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.768	54.0	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.135	4.81
psSAR10g	0.082	-1.71
Peak SAR (Extrapolated)	0.280	5.41
psAPD (4.0 cm², sq)	N/A	N/A

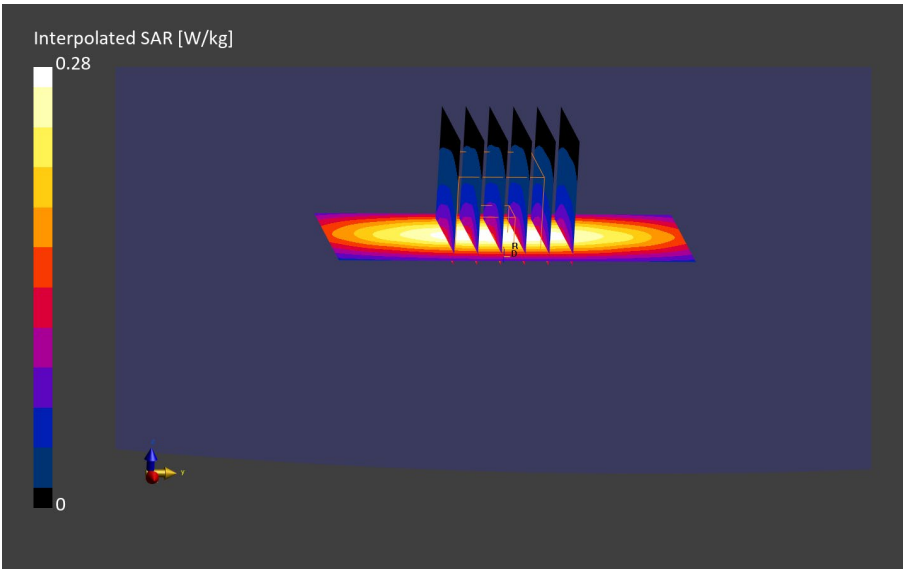

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.65, 9.71,9.7

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	20.8	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.860	43.8	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.417	-4.25
psSAR10g	0.275	-3.57
Peak SAR (Extrapolated)	0.615	-2.61
psAPD (4.0 cm², sq)	N/A	N/A

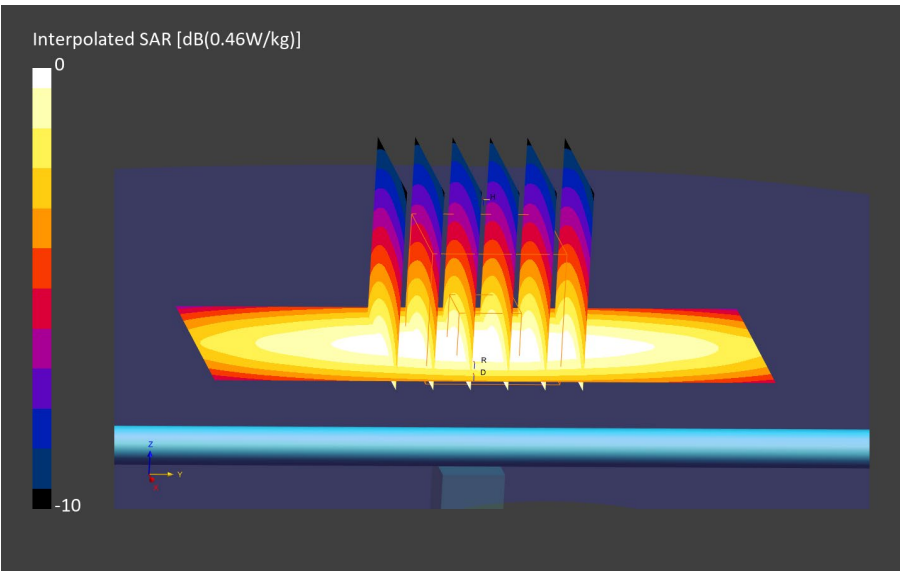

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	20.8	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.891	43.6	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.499	1.39
psSAR10g	0.328	2.74
Peak SAR (Extrapolated)	0.743	5.14
psAPD (4.0 cm², sq)	N/A	N/A

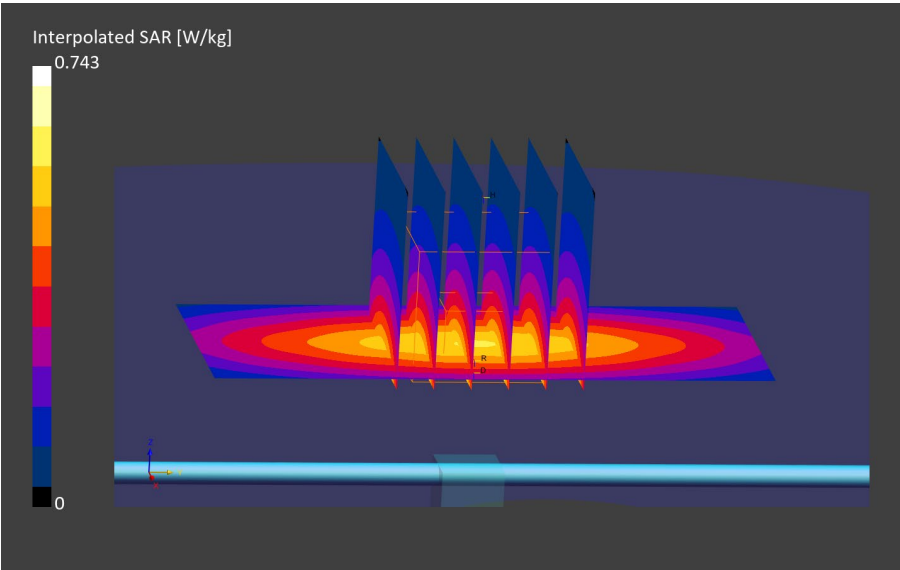

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 8.71, 8.68

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-08	21	20.2	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.894	44.5	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.490	-0.44
psSAR10g	0.324	1.49
Peak SAR (Extrapolated)	0.702	-0.66
psAPD (4.0 cm², sq)	N/A	N/A

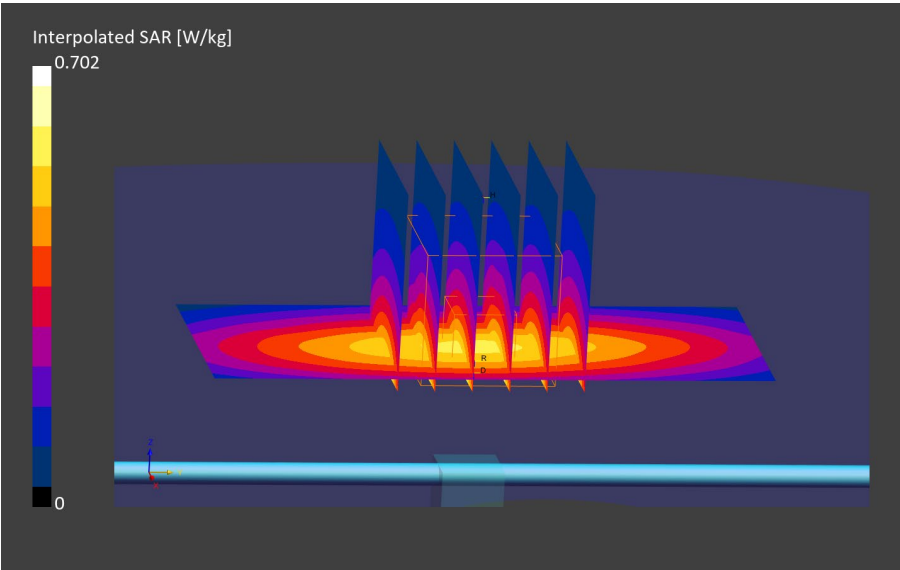

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-27	23.7	22	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.886	45.1	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.498	1.19
psSAR10g	0.327	2.43
Peak SAR (Extrapolated)	0.732	3.58
psAPD (4.0 cm², sq)	N/A	N/A

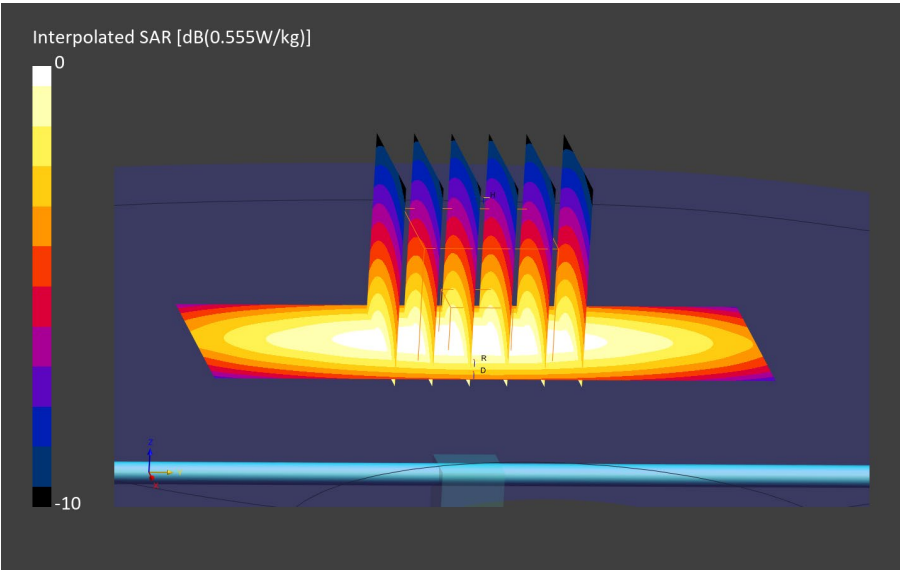

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	22.8	21.4	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.882	44.7	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.505	2.61
psSAR10g	0.331	3.68
Peak SAR (Extrapolated)	0.749	5.99
psAPD (4.0 cm², sq)	N/A	N/A

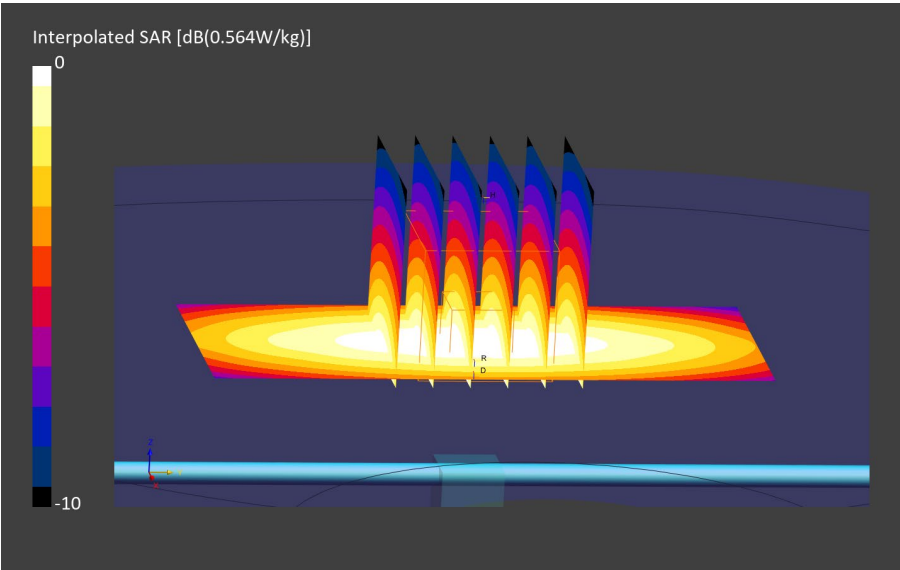

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65, 7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	20.8	21	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.28	40.0	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.78	-2.7
psSAR10g	0.948	-1.48
Peak SAR (Extrapolated)	2.98	-8.38
psAPD (4.0 cm², sq)	N/A	N/A

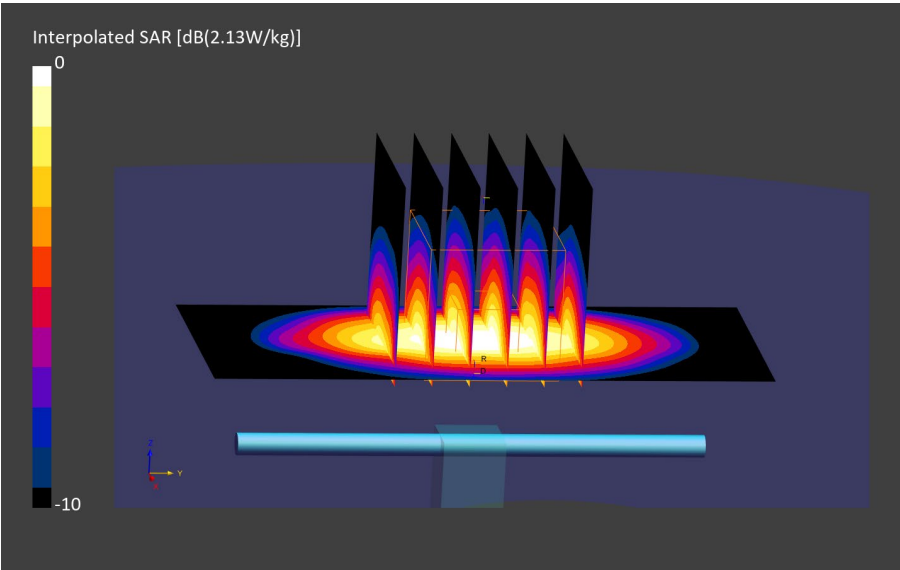

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65, 7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-07	21.1	20	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.31	41.7	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.75	-4.34
psSAR10g	0.940	-2.32
Peak SAR (Extrapolated)	2.95	-9.31
psAPD (4.0 cm², sq)	N/A	N/A

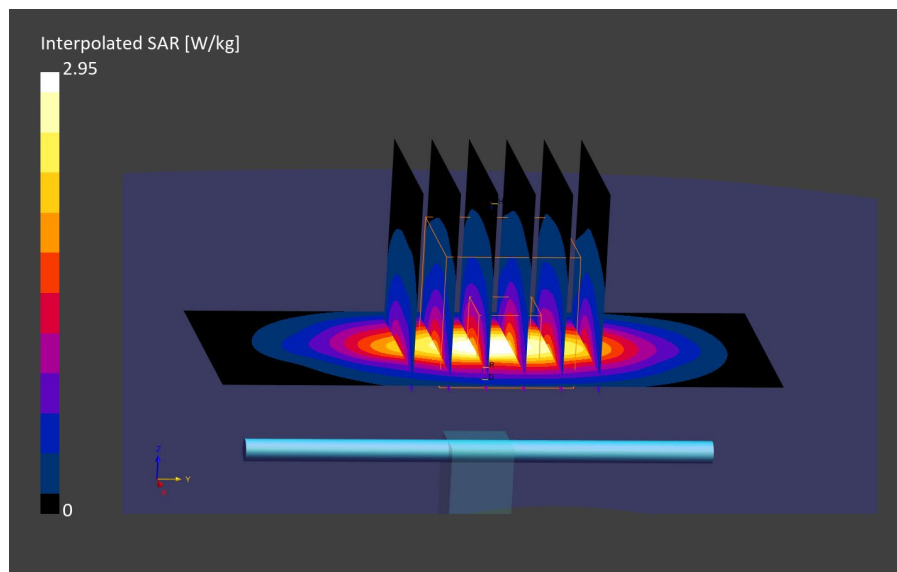

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.37, 7.61, 8.49

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.36	42.9	EX3DV4 – SN7836, 2026-04-23	DAE4ip Sn1839, 2026-06-09

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.78	-2.7
psSAR10g	0.952	-1.07
Peak SAR (Extrapolated)	3.06	-5.92
psAPD (4.0 cm², sq)	N/A	N/A

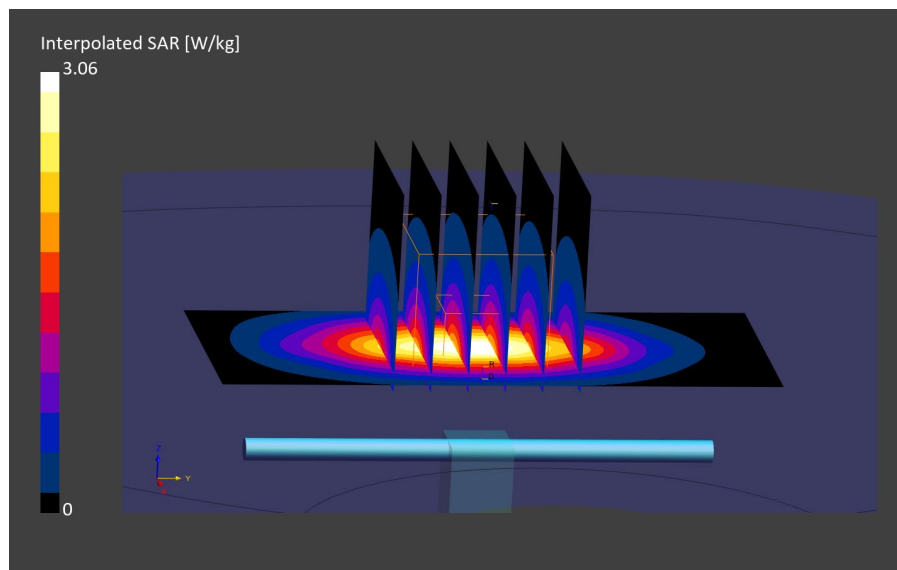

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	20.8	21	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.36	39.7	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.88	-5.75
psSAR10g	0.990	-5.94
Peak SAR (Extrapolated)	3.29	-8.95
psAPD (4.0 cm², sq)	N/A	N/A

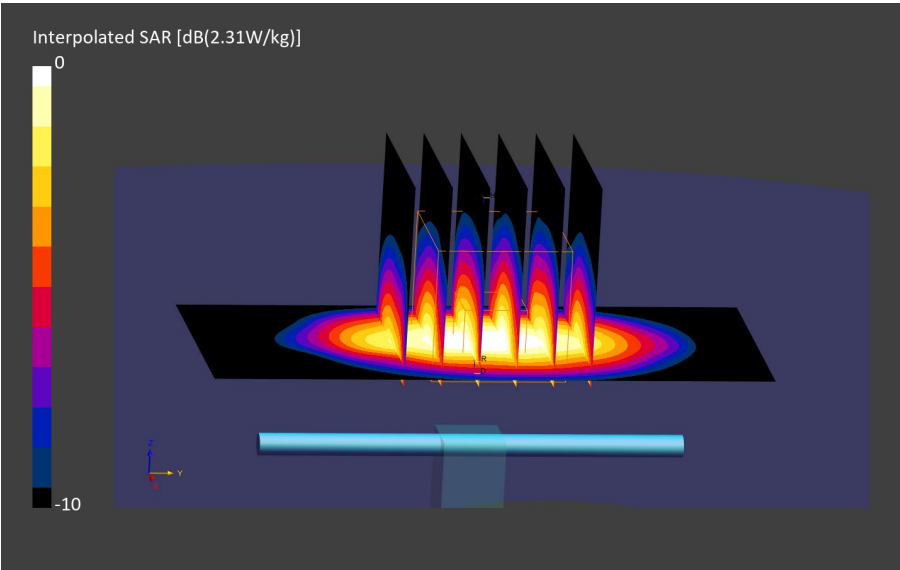

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-30	24.7	21.1	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.39	41.8	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.90	-4.75
psSAR10g	0.996	-5.37
Peak SAR (Extrapolated)	3.34	-7.57
psAPD (4.0 cm², sq)	N/A	N/A

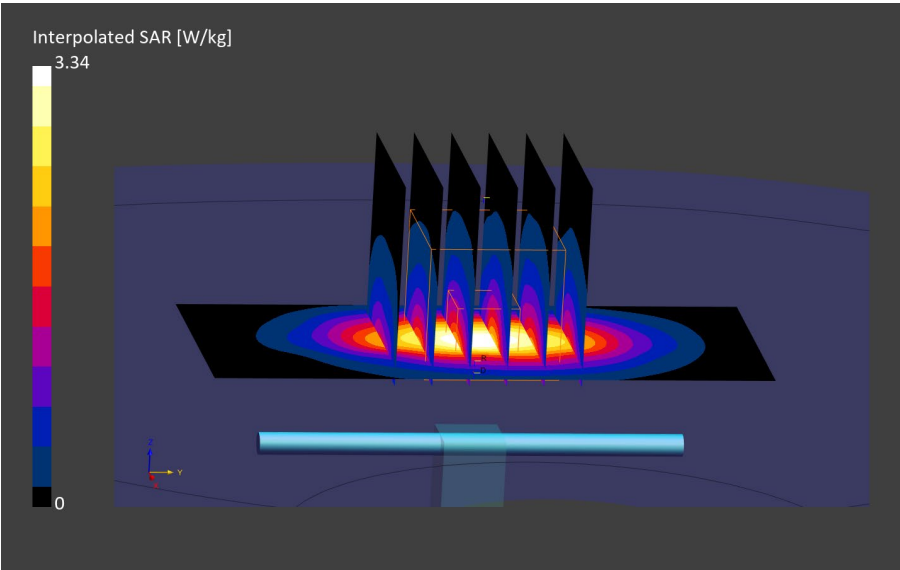

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.26, 7.5, 8.37

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.45	42.7	EX3DV4 – SN7836, 2026-04-23	DAE4ip Sn1839, 2026-06-09

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.91	-4.25
psSAR10g	1.00	-4.99
Peak SAR (Extrapolated)	3.40	-5.91
psAPD (4.0 cm², sq)	N/A	N/A

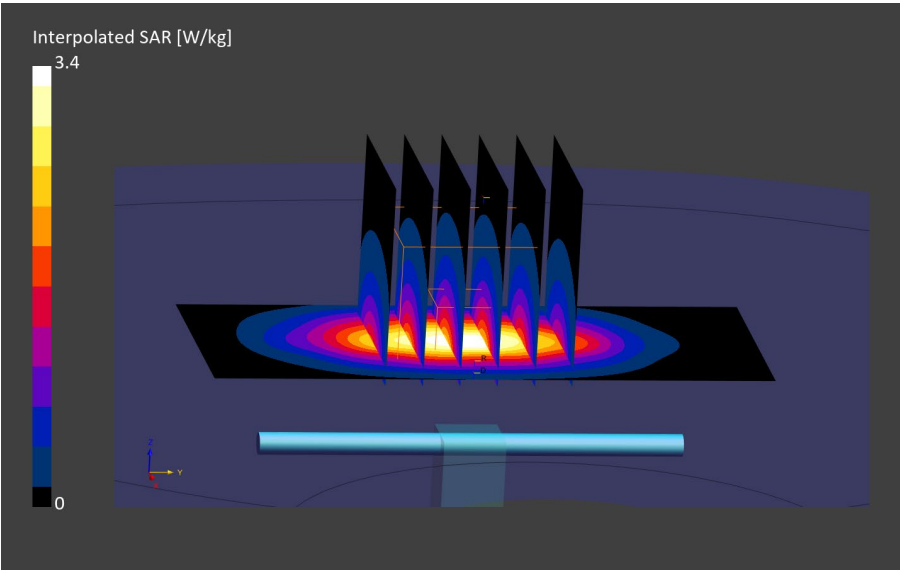

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.39, 7.44, 7.43

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	22.8	21.4	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	1.79	42.1	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.40	-5.36
psSAR10g	1.13	-4.87
Peak SAR (Extrapolated)	4.69	-10.19
psAPD (4.0 cm², sq)	N/A	N/A

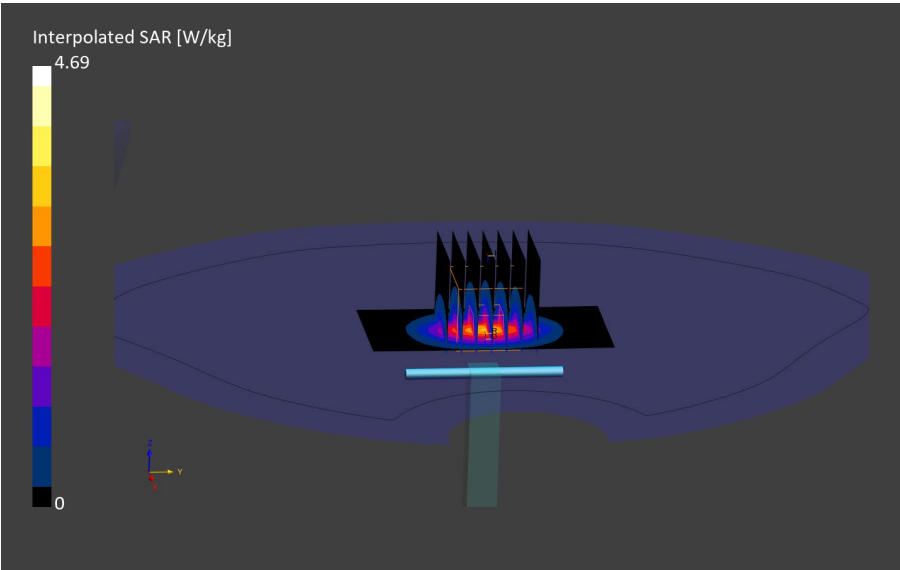

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.87, 6.85,6.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	21.9	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.87	38.7	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.70	-2.58
psSAR10g	1.22	-2.24
Peak SAR (Extrapolated)	5.56	-6.07
psAPD (4.0 cm², sq)	N/A	N/A

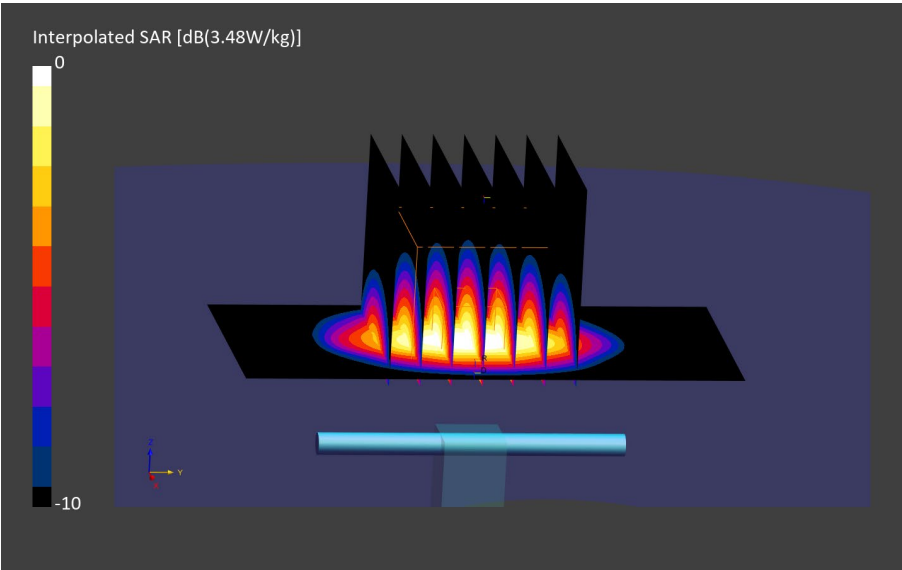

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.87, 6.85, 6.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-08	22.4	20.9	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.86	38.0	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.70	-2.58
psSAR10g	1.22	-2.24
Peak SAR (Extrapolated)	5.55	-6.23
psAPD (4.0 cm², sq)	N/A	N/A

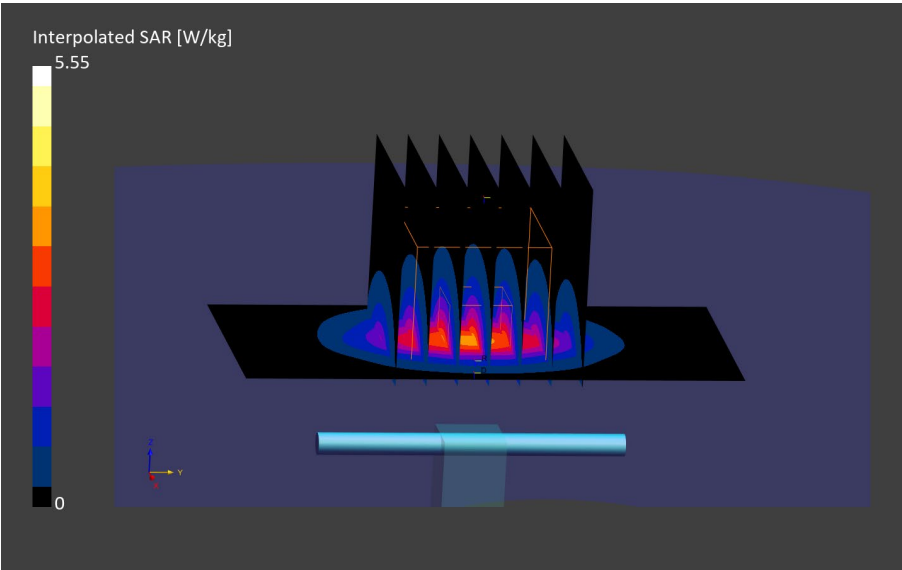

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.18, 6.38, 7.12

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	22.8	22.3	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	2.75	40.4	EX3DV4 – SN7836, 2026-04-23	DAE4ip Sn1839, 2026-06-09

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.97	-8.97
psSAR10g	1.13	-8.35
Peak SAR (Extrapolated)	7.24	-14.47
psAPD (4.0 cm², sq)	N/A	N/A

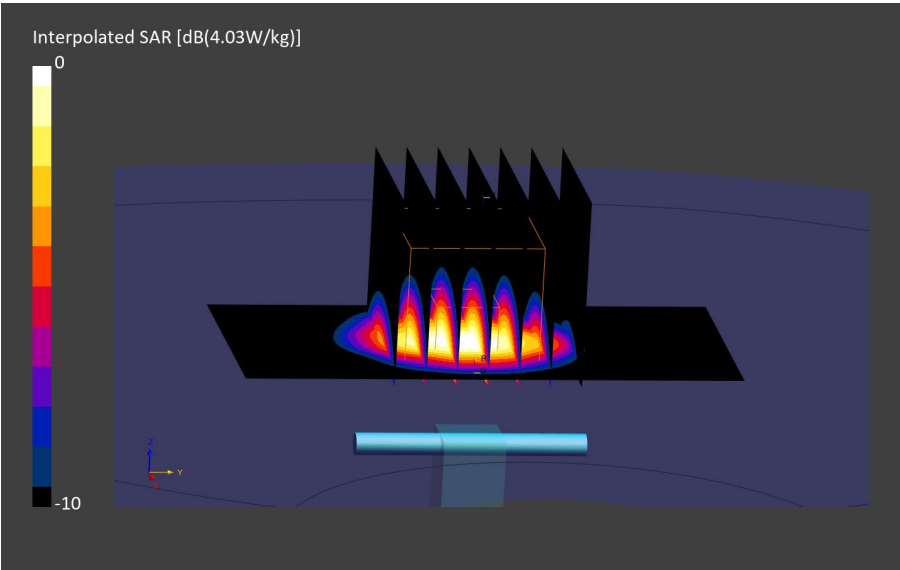

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	6.07, 6.26, 6.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	22.8	22.3	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	2.94	40.1	EX3DV4 – SN7836, 2026-04-23	DAE4ip Sn1839, 2026-06-09

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.13	-6.23
psSAR10g	1.17	-4.72
Peak SAR (Extrapolated)	7.95	-9.72
psAPD (4.0 cm², sq)	N/A	N/A

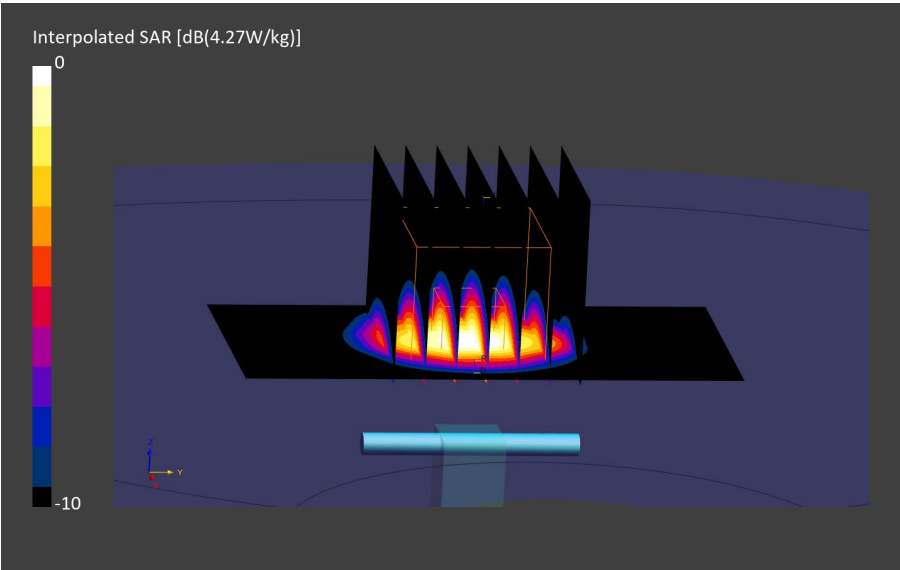

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3900V2 – SN1101	17.0	Flat	10	CW, 0	3900.000	5.96, 6.16, 6.87

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	22.8	22.3	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	3.14	39.8	EX3DV4 – SN7836, 2026-04-23	DAE4ip Sn1839, 2026-06-09

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.28	-6.77
psSAR10g	1.16	-5.91
Peak SAR (Extrapolated)	8.91	-8.13
psAPD (4.0 cm², sq)	N/A	N/A

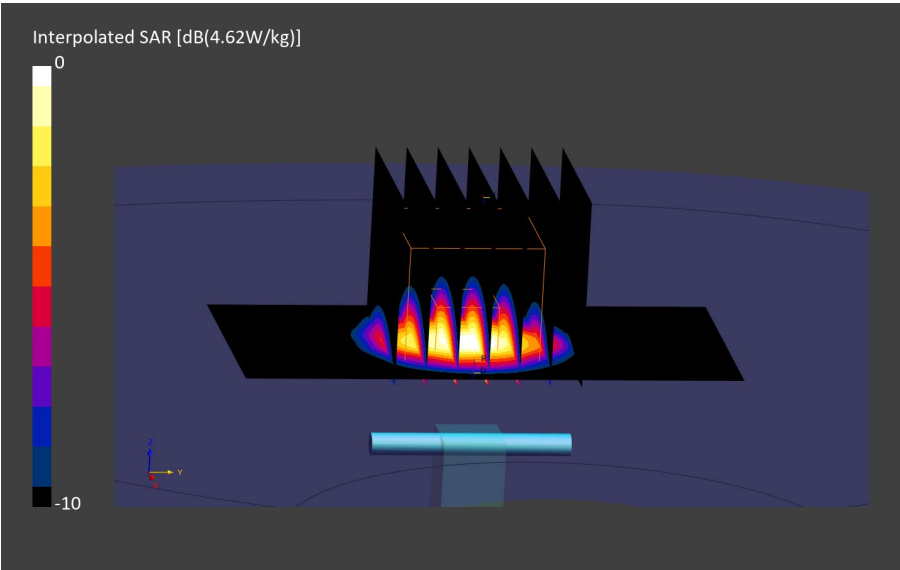

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.17, 5.15,4.86

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	4.56	37.5	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.93	0.66
psSAR10g	1.13	0.65
Peak SAR (Extrapolated)	16.0	2.91
psAPD (4.0 cm², sq)	N/A	N/A

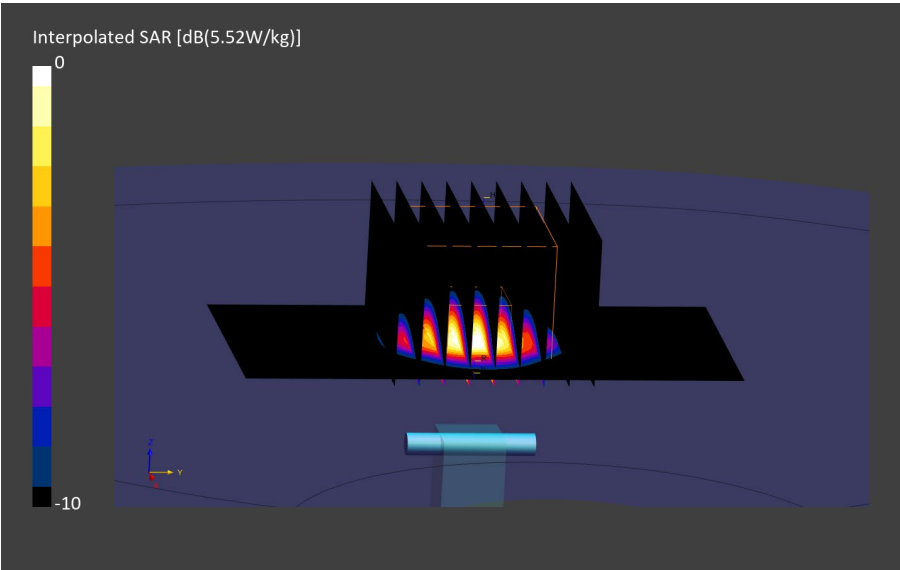

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	4.73, 4.72,4.45

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	4.95	36.9	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.25	4.56
psSAR10g	1.20	2.76
Peak SAR (Extrapolated)	19.0	11.57
psAPD (4.0 cm², sq)	N/A	N/A

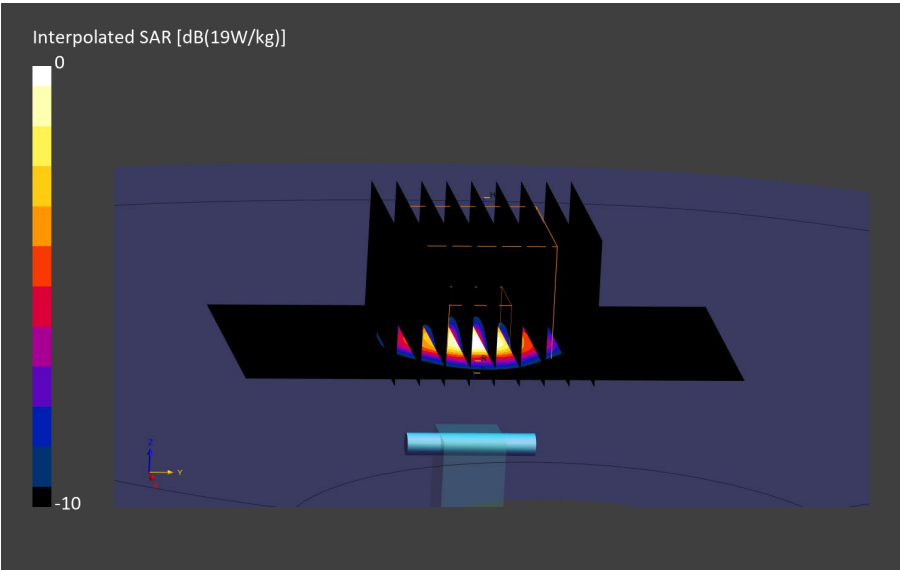

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	4.8, 4.78,4.52

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	5.12	36.6	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.07	1.38
psSAR10g	1.16	1.51
Peak SAR (Extrapolated)	18.6	11.41
psAPD (4.0 cm², sq)	N/A	N/A

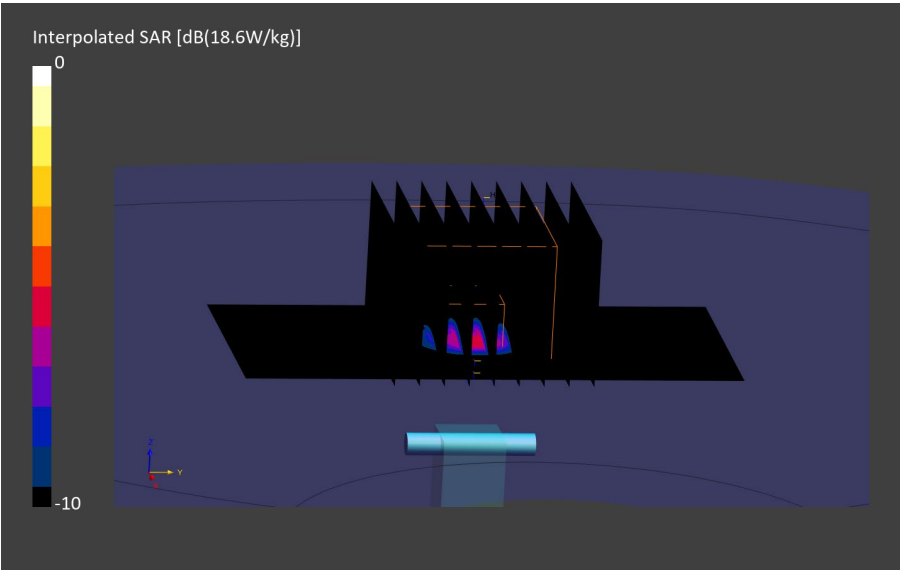

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5850.000	4.69, 4.67,4.41

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-07-06	22.4	22.5	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	5.24	36.4	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.20	8.97
psSAR10g	1.19	7.93
Peak SAR (Extrapolated)	19.9	13.87
psAPD (4.0 cm², sq)	N/A	N/A

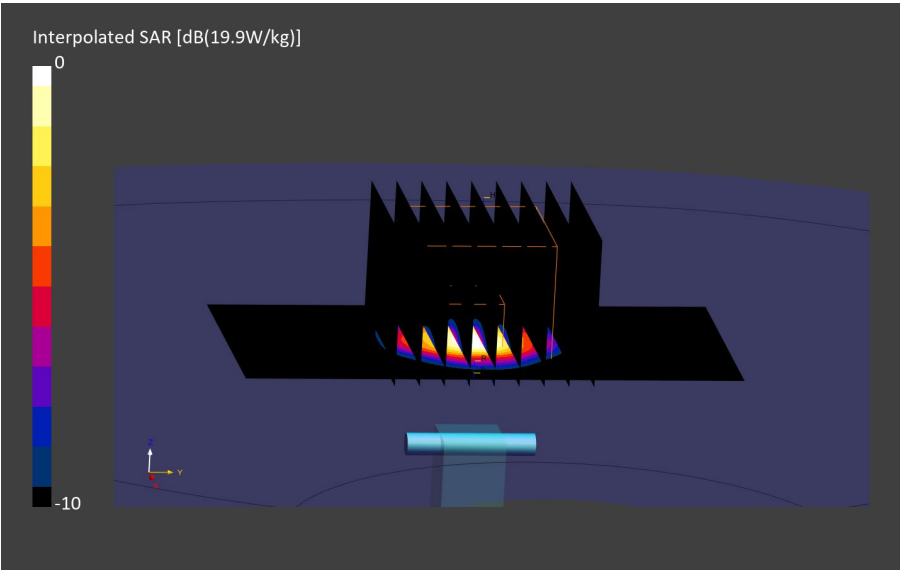

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	5.23, 5.66, 5.2

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-22	23	21.8	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	6.17	35.4	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	23.8 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.90	-2.68
psSAR10g	0.546	-0.73
Peak SAR (Extrapolated)	18.0	-8.86
psAPD (4.0 cm², sq)	13.1	-2.24

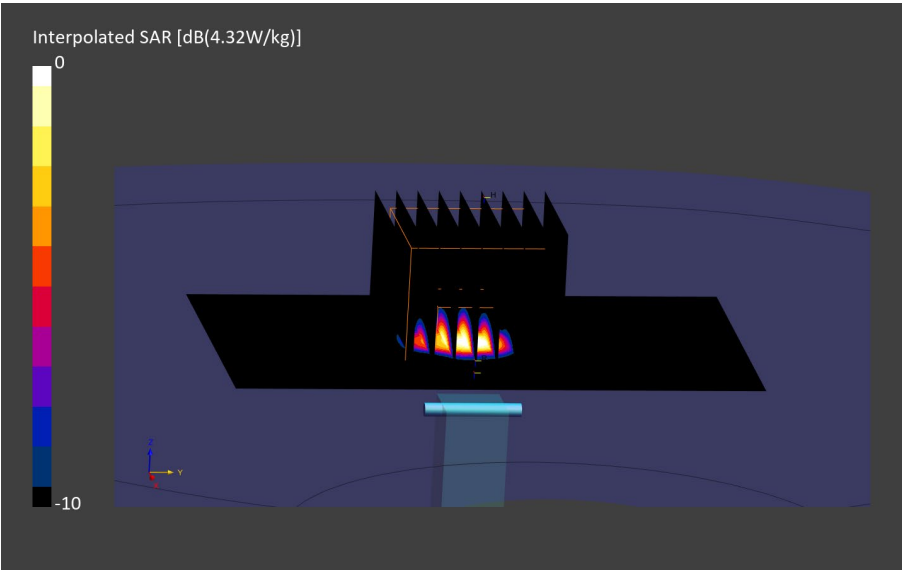

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Serial Number	Test Distance [mm]	Signal, UID	Frequency [MHz]
10 GHz System Verification	1074	10.00	CW	10000.0

Test Setup

Test Date	Measurement SW	Probe, Cal. Date	DAE, Cal. Date
2026-06-29	3.2.2.2358	EUmmWV4 – SN9690_F1–55GHz – 2025-09-17	DAE4ip Sn1905 – 2026-05-08

Scans Setup

Grid Extents [mm]	Grid Steps [lambda]	Sensor Surface Distance [mm]
60.0x60.0	0.125x0.125	10.0

Measurement Results

Averaging Area [cm²]	E _{max} [V/m]	psPD _{n+} [W/m²]	psPD _{tot+} [W/m²]
4.00	126	37.3	37.5

