

Appendix A: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.8, 6.79,6.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.5	21.6	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.85	41.3	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.74	8.04
psSAR10g	1.30	9.44
Peak SAR (Extrapolated)	5.49	5.12
psAPD (4.0 cm², sq)	N/A	N/A

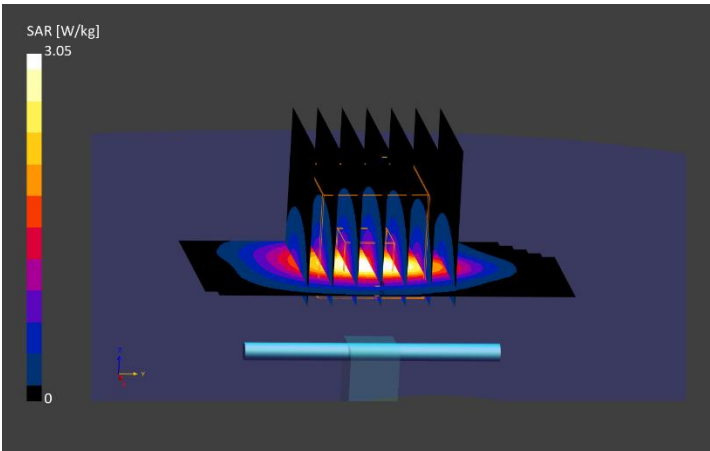

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.17, 5.15,4.86

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-22	22.6	22.1	18.0.0.7250	Twin-SAM V8.0 – 2159	Head Simulating Liquid	4.61	37.4	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.13	5.78
psSAR10g	1.18	5.11
Peak SAR (Extrapolated)	16.8	8.06
psAPD (4.0 cm², sq)	N/A	N/A

