

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	14.3, 16.56,15.27

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	22.8	23.4	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.752	52.9	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 36.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.137	6.37
psSAR10g	0.084	0.69
Peak SAR (Extrapolated)	0.287	8.07
psAPD (4.0 cm², sq)	N/A	N/A

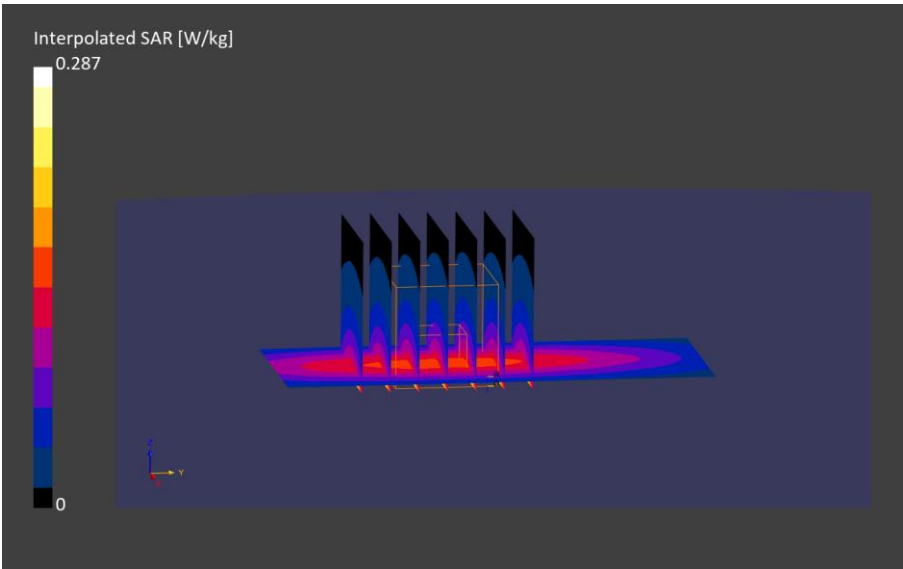

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.65, 9.71,9.7

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-06	22.8	23.4	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.891	41.0	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.414	-4.94
psSAR10g	0.273	-4.27
Peak SAR (Extrapolated)	0.636	0.71
psAPD (4.0 cm², sq)	N/A	N/A

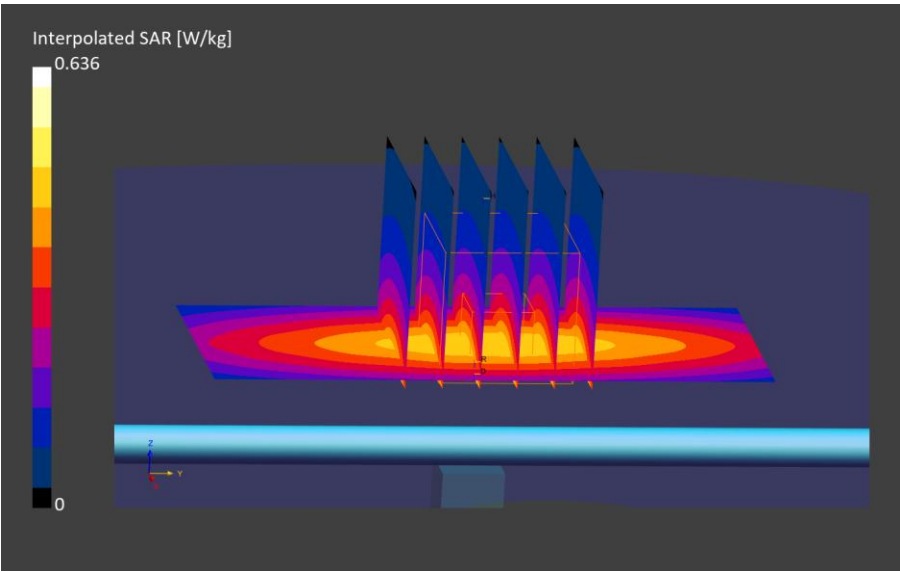

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.62, 9.46,9.15

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.8	20.5	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	0.849	43.8	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.400	-8.16
psSAR10g	0.266	-6.72
Peak SAR (Extrapolated)	0.558	-11.64
psAPD (4.0 cm², sq)	N/A	N/A

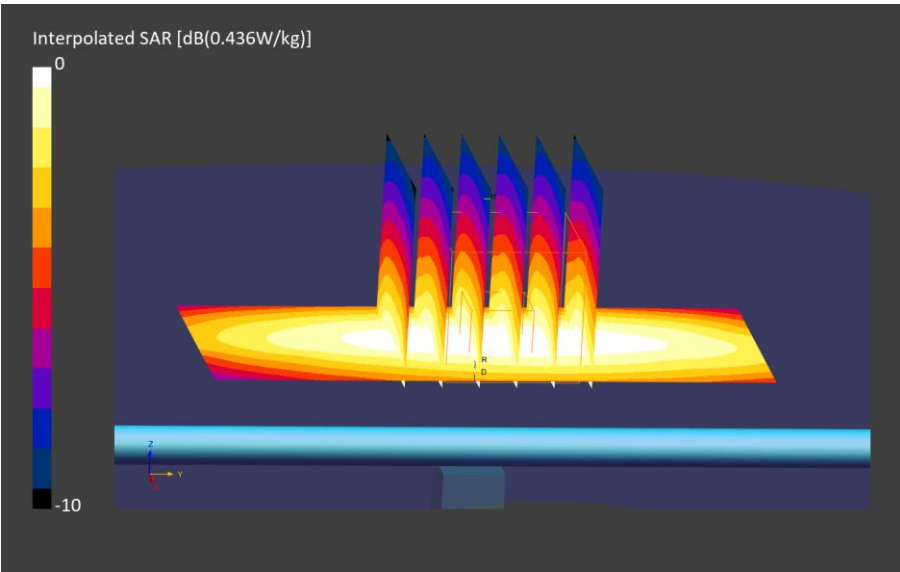

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.65, 9.71,9.7

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	21.7	21.8	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.867	43.8	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.410	-5.86
psSAR10g	0.271	-4.97
Peak SAR (Extrapolated)	0.598	-5.3
psAPD (4.0 cm², sq)	N/A	N/A

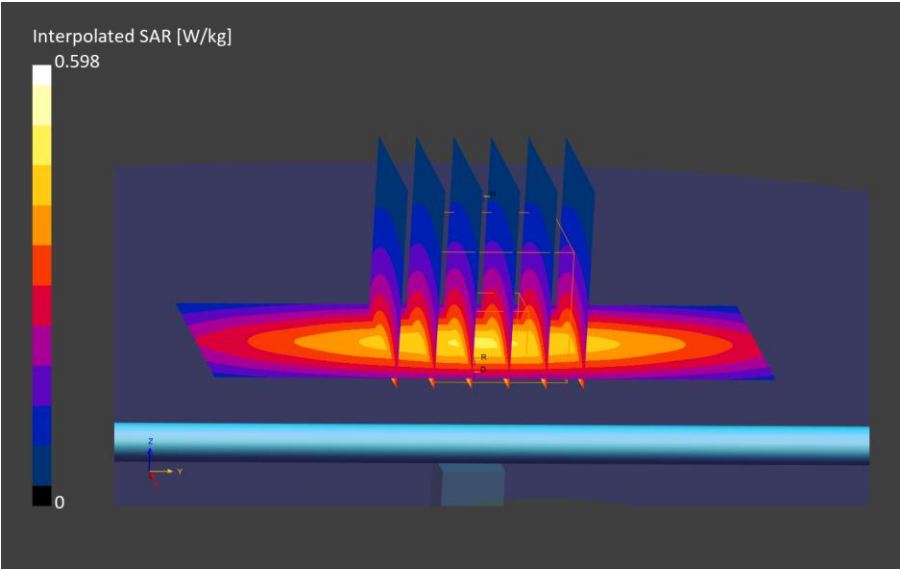

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.65, 9.71,9.7

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-08	23	21.5	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.870	43.2	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.407	-6.55
psSAR10g	0.269	-5.67
Peak SAR (Extrapolated)	0.605	-4.2
psAPD (4.0 cm², sq)	N/A	N/A

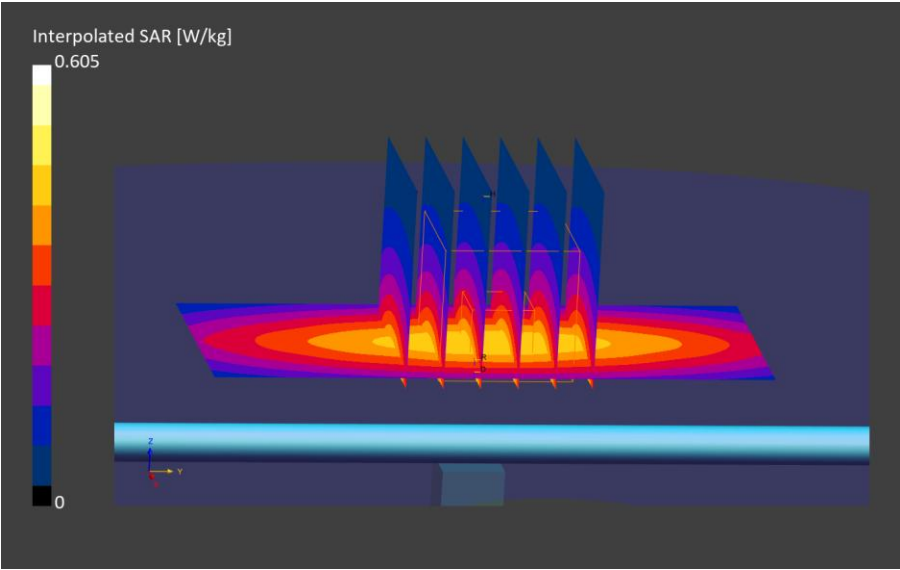

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.65, 9.71, 9.7

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-11	23.1	22.7	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.890	40.5	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.428	-1.73
psSAR10g	0.283	-0.76
Peak SAR (Extrapolated)	0.664	5.15
psAPD (4.0 cm², sq)	N/A	N/A

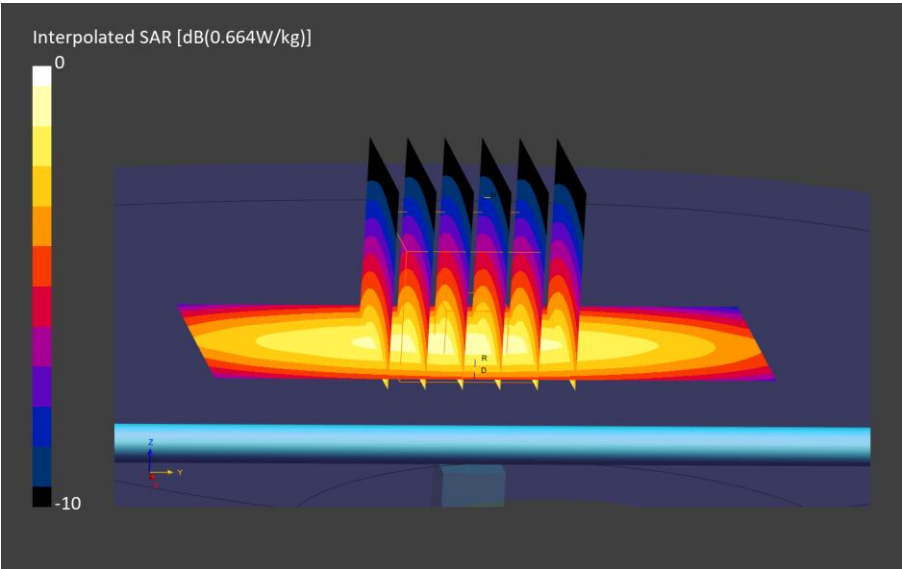

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-11	23.1	22.7	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.917	40.3	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.506	2.81
psSAR10g	0.332	3.99
Peak SAR (Extrapolated)	0.781	10.52
psAPD (4.0 cm², sq)	N/A	N/A

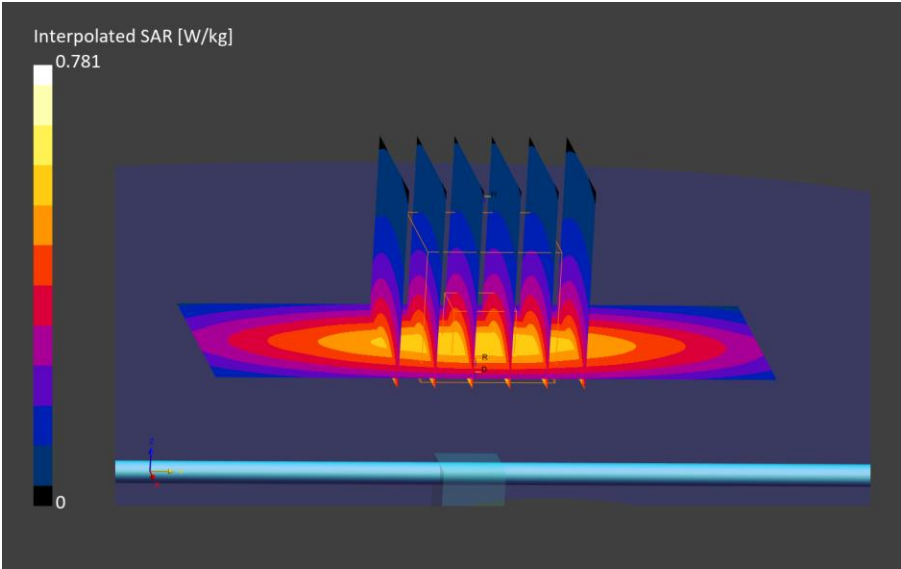

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.48, 9.32,9.02

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-13	21.5	20.3	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	0.877	43.0	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.476	-3.28
psSAR10g	0.314	-1.65
Peak SAR (Extrapolated)	0.671	-5.05
psAPD (4.0 cm², sq)	N/A	N/A

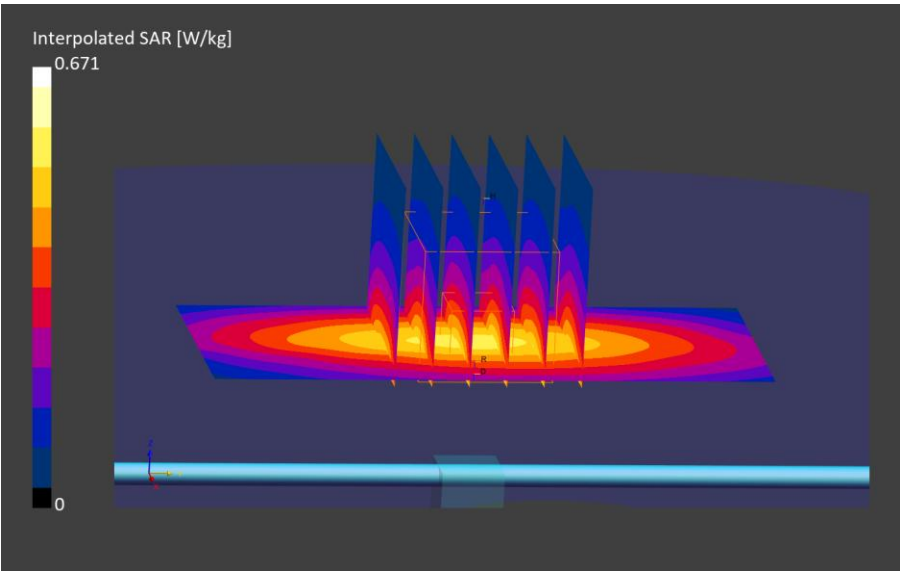

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-18	20.5	21.3	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.879	45.5	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.503	2.2
psSAR10g	0.331	3.68
Peak SAR (Extrapolated)	0.726	2.73
psAPD (4.0 cm², sq)	N/A	N/A

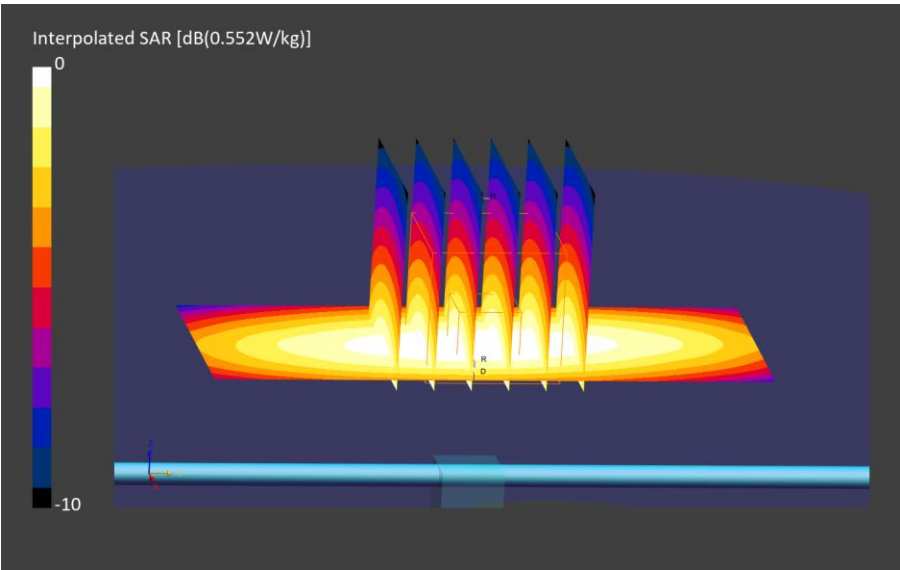

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.48, 9.32,9.02

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.8	20.5	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	0.880	43.6	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.477	-3.08
psSAR10g	0.316	-1.02
Peak SAR (Extrapolated)	0.680	-3.77
psAPD (4.0 cm², sq)	N/A	N/A

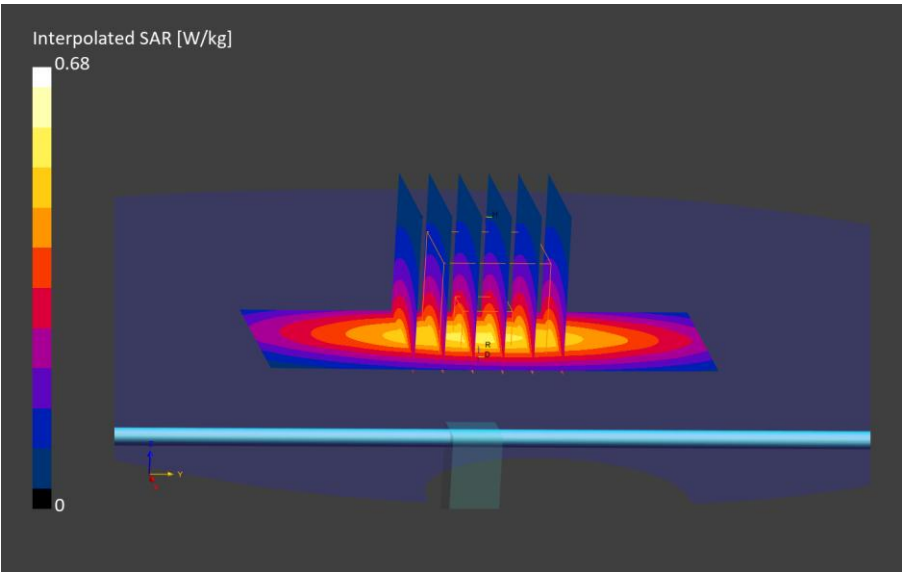

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	21.7	21.8	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.898	43.6	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.497	0.98
psSAR10g	0.327	2.43
Peak SAR (Extrapolated)	0.749	5.99
psAPD (4.0 cm², sq)	N/A	N/A

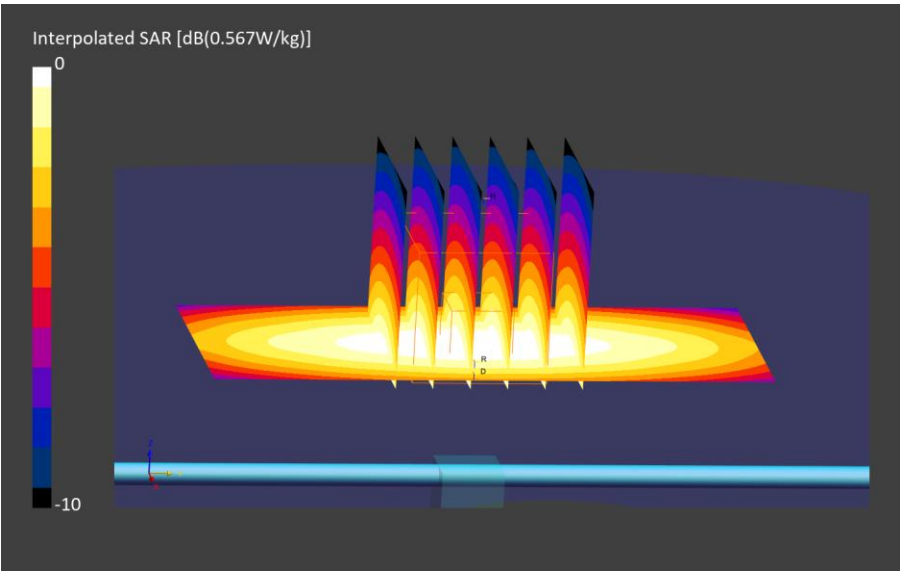

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.17, 9.24,9.23

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.1	23	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	0.905	42.5	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.484	-1.66
psSAR10g	0.318	-0.39
Peak SAR (Extrapolated)	0.744	5.28
psAPD (4.0 cm², sq)	N/A	N/A

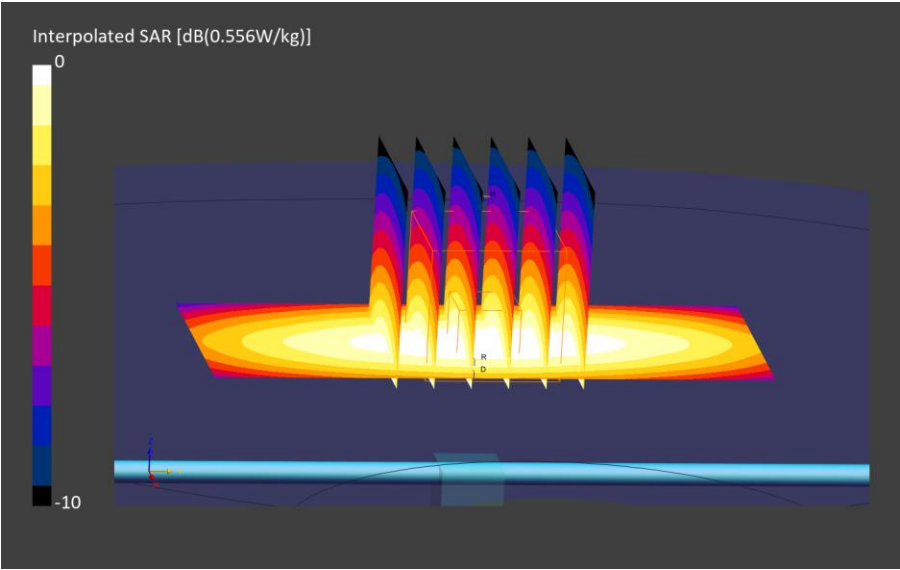

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.68, 7.4,7.37

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-06	22.7	22.4	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.32	41.1	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.80	-1.6
psSAR10g	0.963	0.07
Peak SAR (Extrapolated)	3.08	-5.31
psAPD (4.0 cm², sq)	N/A	N/A

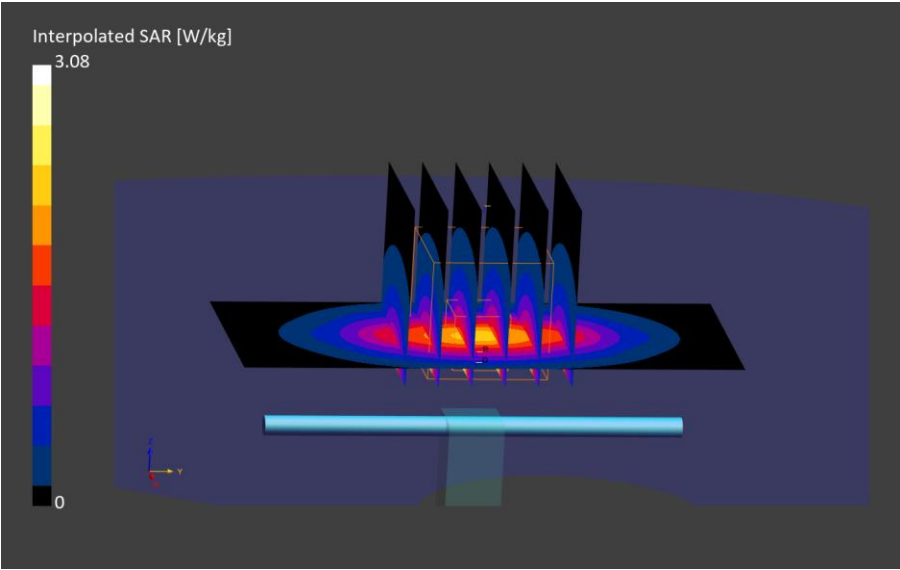

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.68, 7.4,7.37

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.3	21.1	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.36	43.8	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.80	-1.6
psSAR10g	0.966	0.39
Peak SAR (Extrapolated)	3.06	-5.92
psAPD (4.0 cm², sq)	N/A	N/A

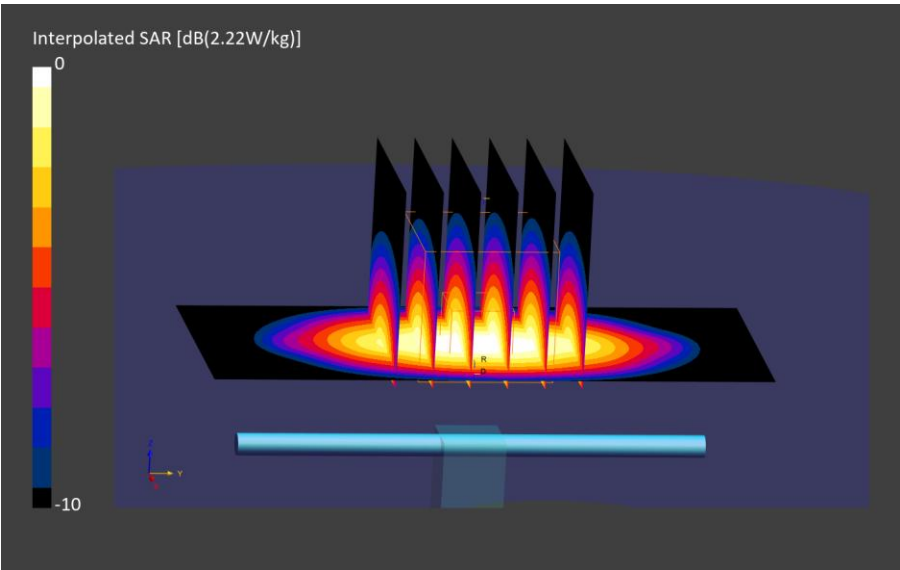

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65, 7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-26	21.5	20.5	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.31	40.9	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.82	-0.51
psSAR10g	0.970	0.8
Peak SAR (Extrapolated)	3.14	-3.46
psAPD (4.0 cm², sq)	N/A	N/A

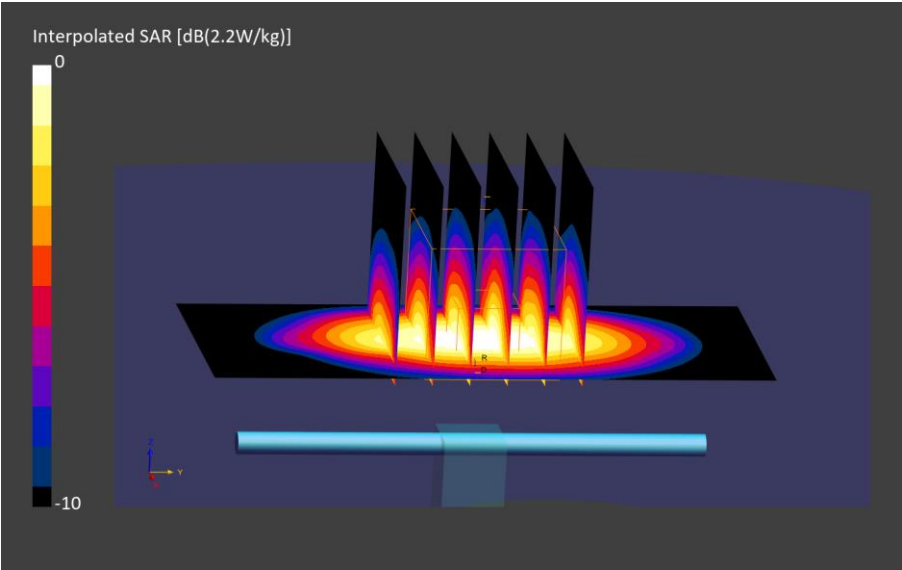

21.56917

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65,7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	20.8	21	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.28	40.0	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.78	-2.7
psSAR10g	0.948	-1.48
Peak SAR (Extrapolated)	2.98	-8.38
psAPD (4.0 cm², sq)	N/A	N/A

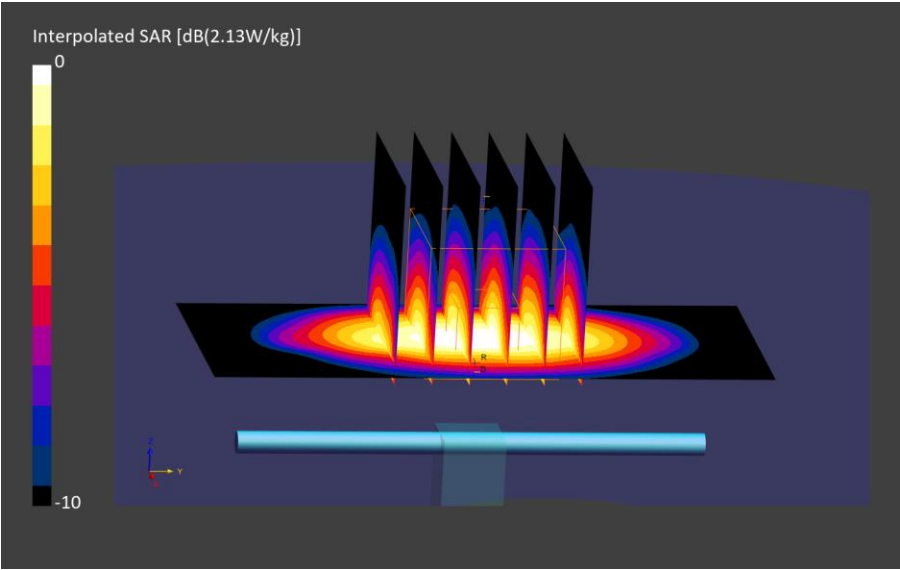

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65, 7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-07	21.1	20	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.31	41.7	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.75	-4.34
psSAR10g	0.940	-2.32
Peak SAR (Extrapolated)	2.95	-9.31
psAPD (4.0 cm², sq)	N/A	N/A

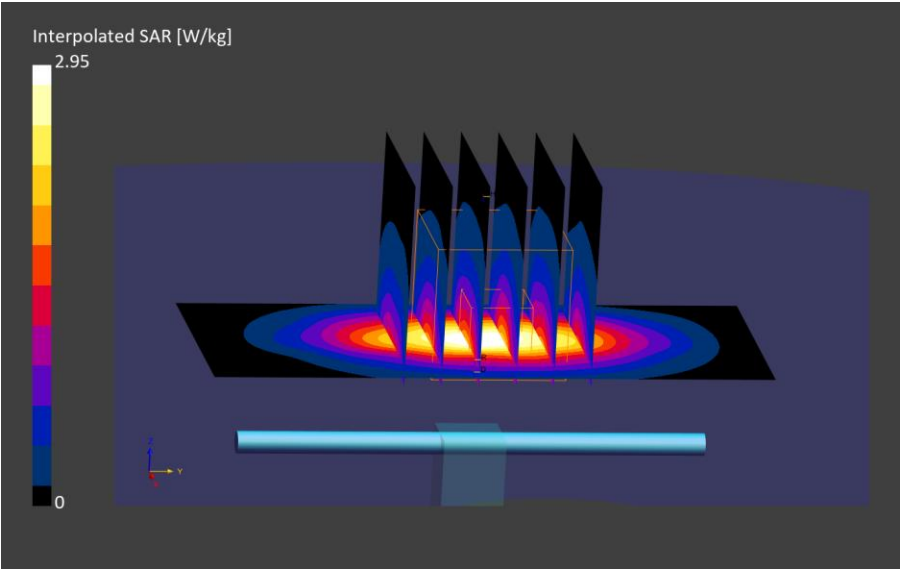

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.78, 7.65,7.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-30	24.7	21.1	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.32	42.1	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.75	-4.34
psSAR10g	0.938	-2.52
Peak SAR (Extrapolated)	2.97	-8.69
psAPD (4.0 cm², sq)	N/A	N/A

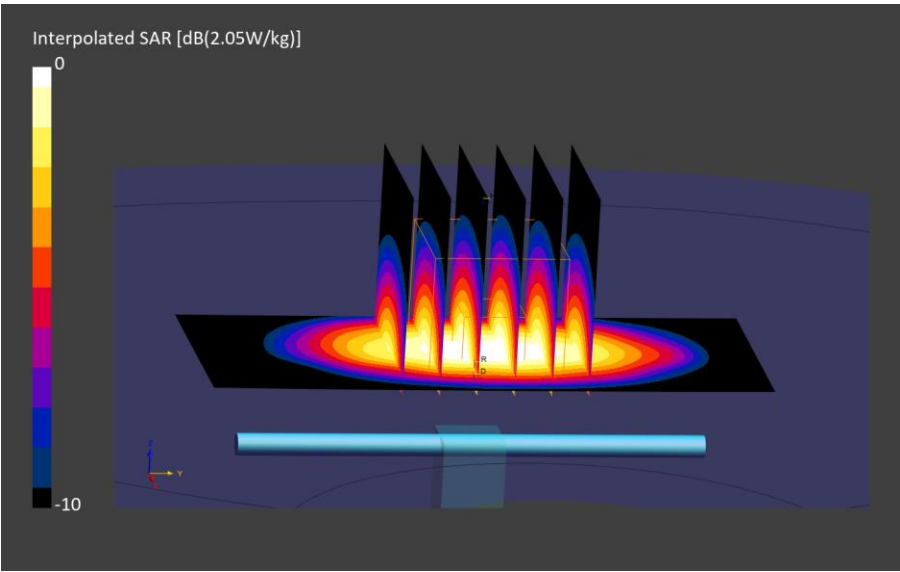

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-04	22.3	22.2	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.41	39.2	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.01	0.77
psSAR10g	1.06	0.71
Peak SAR (Extrapolated)	3.63	0.45
psAPD (4.0 cm², sq)	N/A	N/A

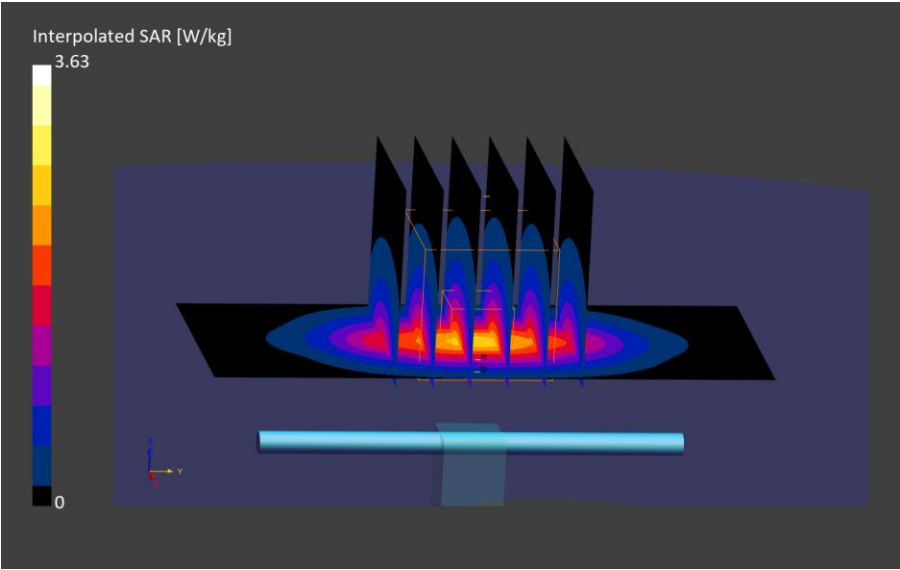

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-06	22.7	22.4	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.39	40.8	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.04	2.27
psSAR10g	1.07	1.66
Peak SAR (Extrapolated)	3.62	0.18
psAPD (4.0 cm², sq)	N/A	N/A

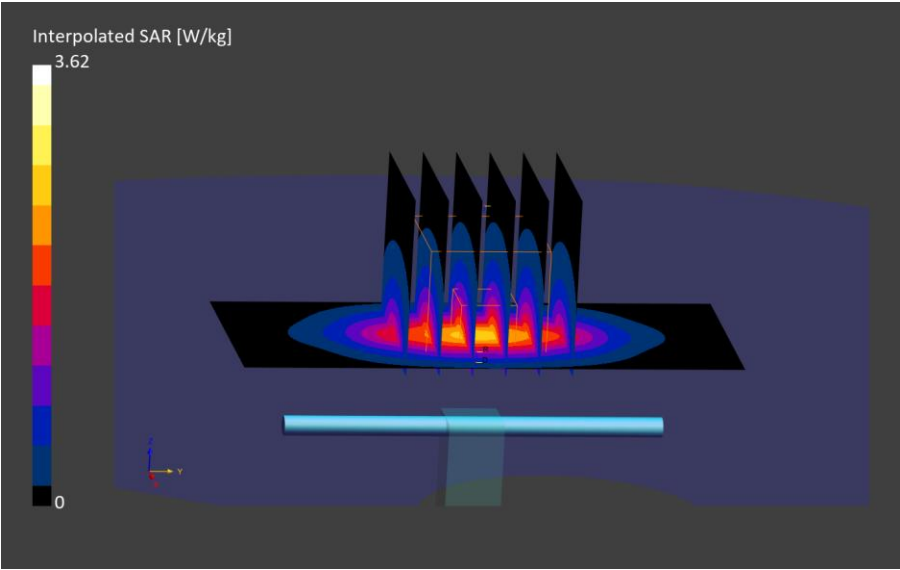

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46,7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-11	22.5	22.2	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.38	40.5	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.87	-6.25
psSAR10g	0.981	-6.79
Peak SAR (Extrapolated)	3.30	-8.68
psAPD (4.0 cm², sq)	N/A	N/A

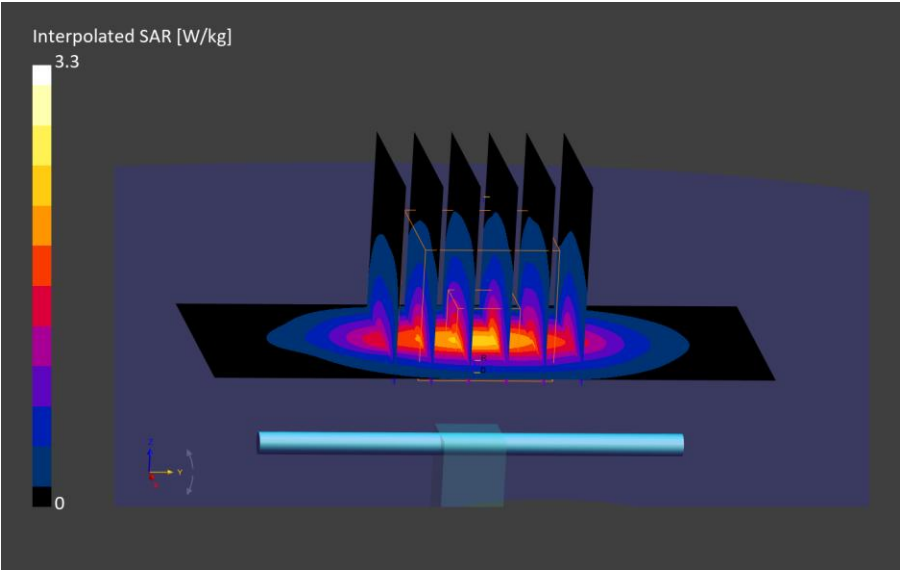

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.3	21.1	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.45	43.5	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.02	1.27
psSAR10g	1.06	0.71
Peak SAR (Extrapolated)	3.58	-0.93
psAPD (4.0 cm², sq)	N/A	N/A

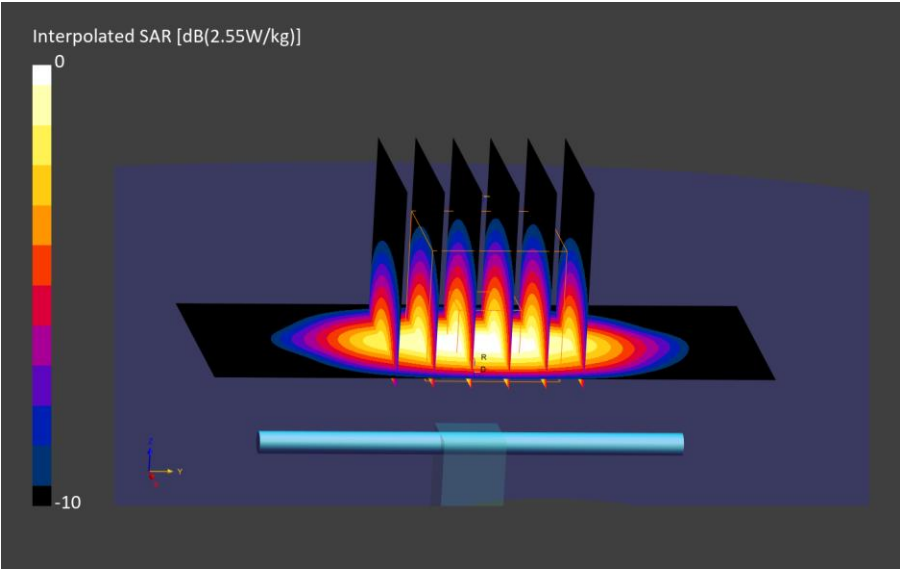

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46,7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	20.8	21	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.36	39.7	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.88	-5.75
psSAR10g	0.990	-5.94
Peak SAR (Extrapolated)	3.29	-8.95
psAPD (4.0 cm², sq)	N/A	N/A

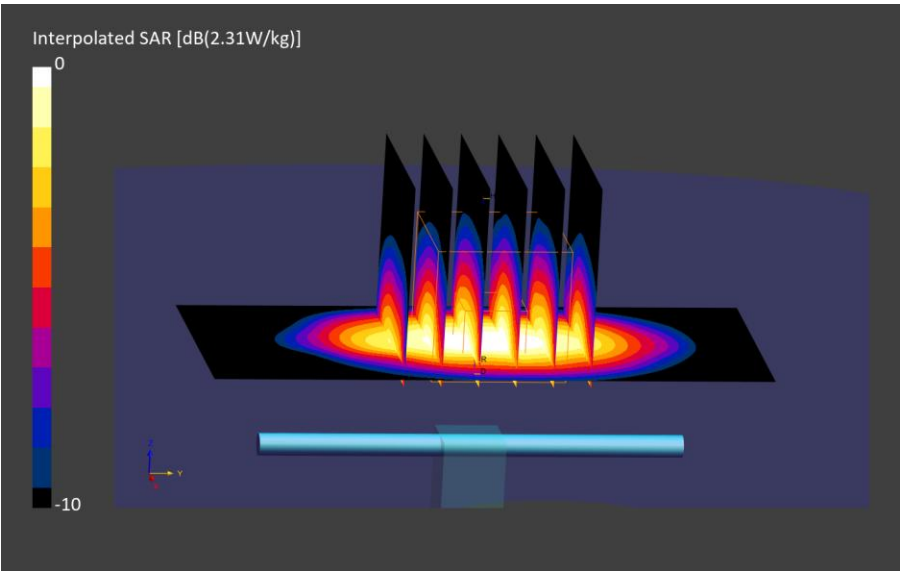

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46,7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-07	21.1	20	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.41	41.4	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.93	-3.24
psSAR10g	1.02	-3.09
Peak SAR (Extrapolated)	3.44	-4.8
psAPD (4.0 cm², sq)	N/A	N/A

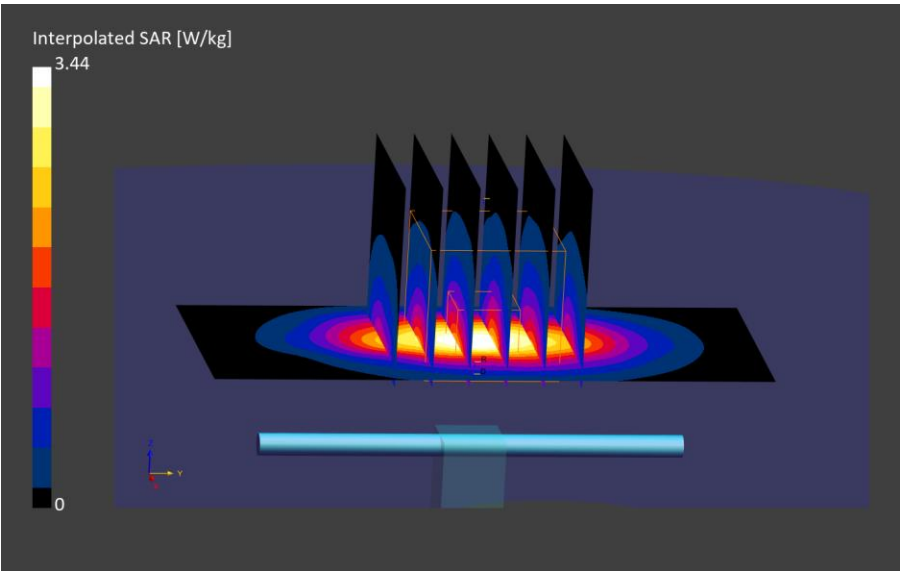

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-24	21.6	21.9	18.0.0.7250	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.41	41.9	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.00	0.26
psSAR10g	1.05	-0.24
Peak SAR (Extrapolated)	3.57	-1.21
psAPD (4.0 cm², sq)	N/A	N/A

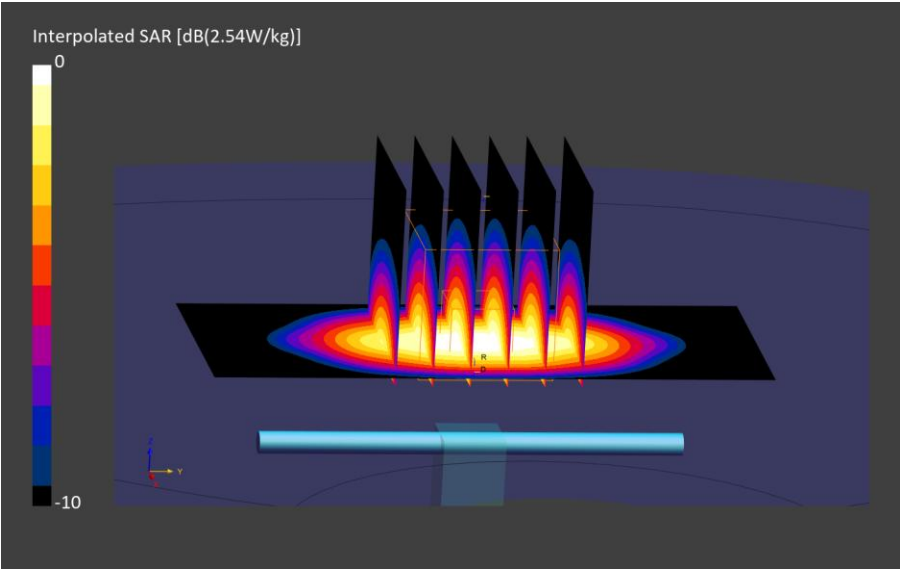

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2300V2 – SN1139	17.0	Flat	10	CW, 0	2300.000	7.11, 7.69,7.07

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-12	24.7	23.1	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.65	40.1	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.44	-0.64
psSAR10g	1.18	-0.66
Peak SAR (Extrapolated)	4.78	2.77
psAPD (4.0 cm², sq)	N/A	N/A

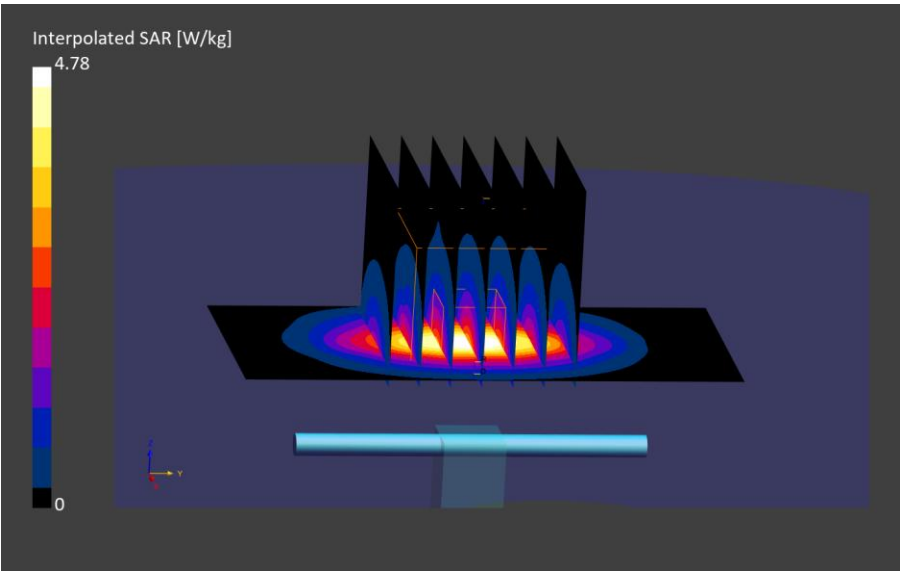

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2300V2 – SN1139	17.0	Flat	10	CW, 0	2300.000	6.99, 6.97, 6.58

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-26	22.6	22.2	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.71	40.7	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.50	1.8
psSAR10g	1.21	1.87
Peak SAR (Extrapolated)	4.95	6.43
psAPD (4.0 cm², sq)	N/A	N/A

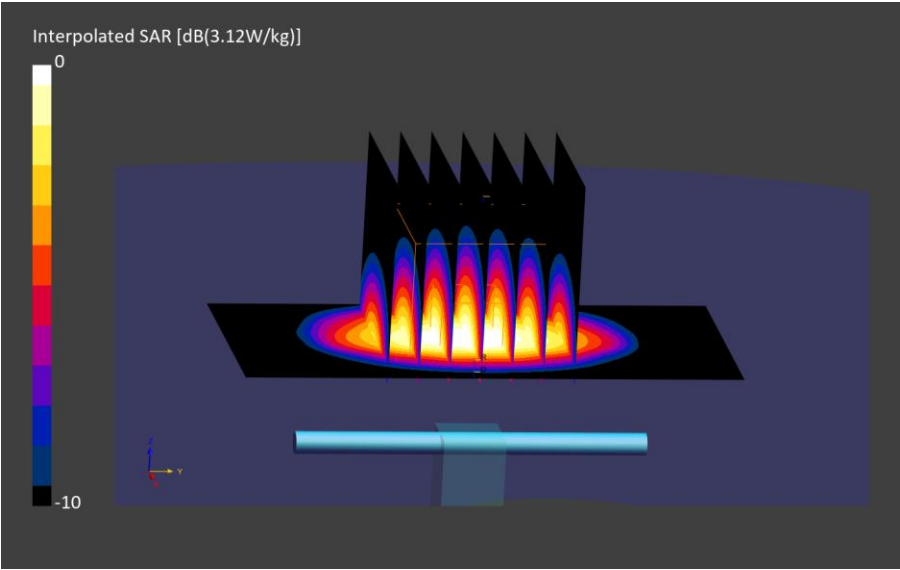

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.8, 6.79,6.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-28	21.9	22.2	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.79	39.6	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.56	0.95
psSAR10g	1.21	1.87
Peak SAR (Extrapolated)	5.16	-1.19
psAPD (4.0 cm², sq)	N/A	N/A

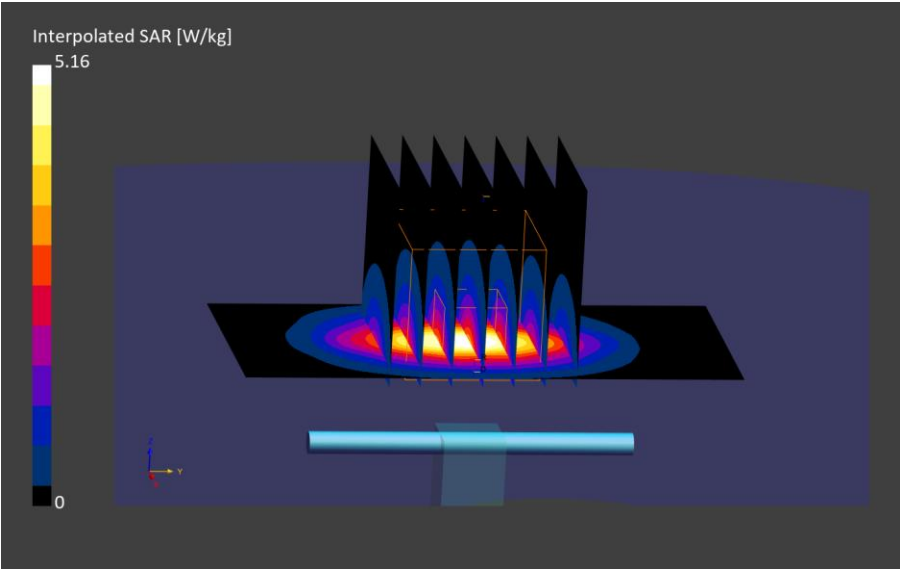

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.8, 6.79,6.4

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-08	22.4	20.9	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.74	38.2	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.60	2.52
psSAR10g	1.23	3.55
Peak SAR (Extrapolated)	5.17	-1
psAPD (4.0 cm², sq)	N/A	N/A

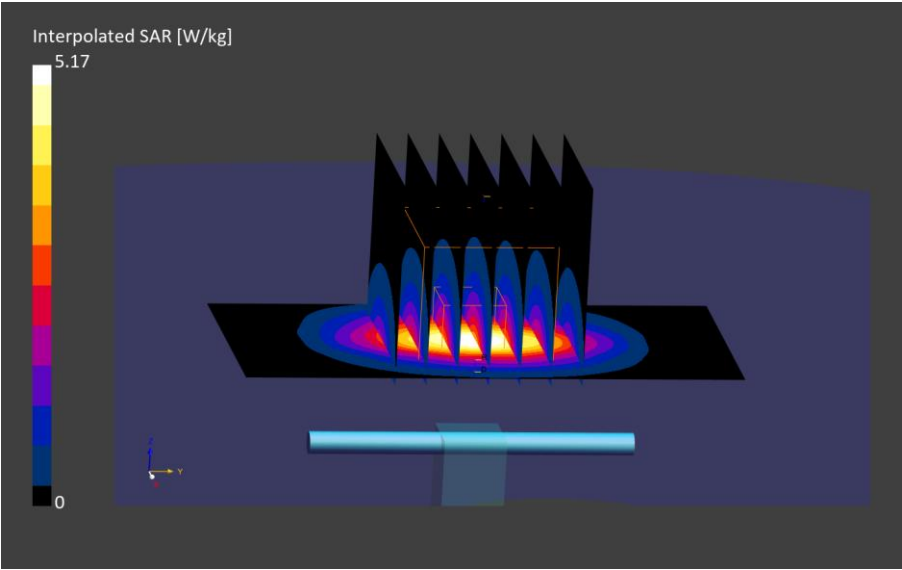

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.39, 7.44,7.43

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.7	20.9	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	1.77	39.0	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.40	-5.36
psSAR10g	1.14	-4.03
Peak SAR (Extrapolated)	4.79	-8.28
psAPD (4.0 cm², sq)	N/A	N/A

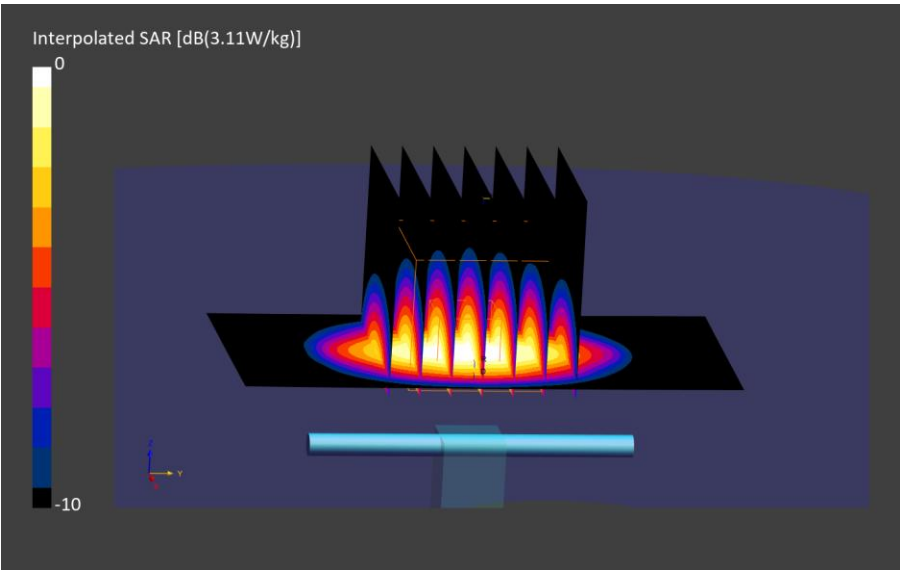

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.94, 6.68,6.66

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	20.4	20.8	18.0.0.7250	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.80	40.6	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.50	-1.42
psSAR10g	1.17	-1.5
Peak SAR (Extrapolated)	4.94	-5.41
psAPD (4.0 cm², sq)	N/A	N/A

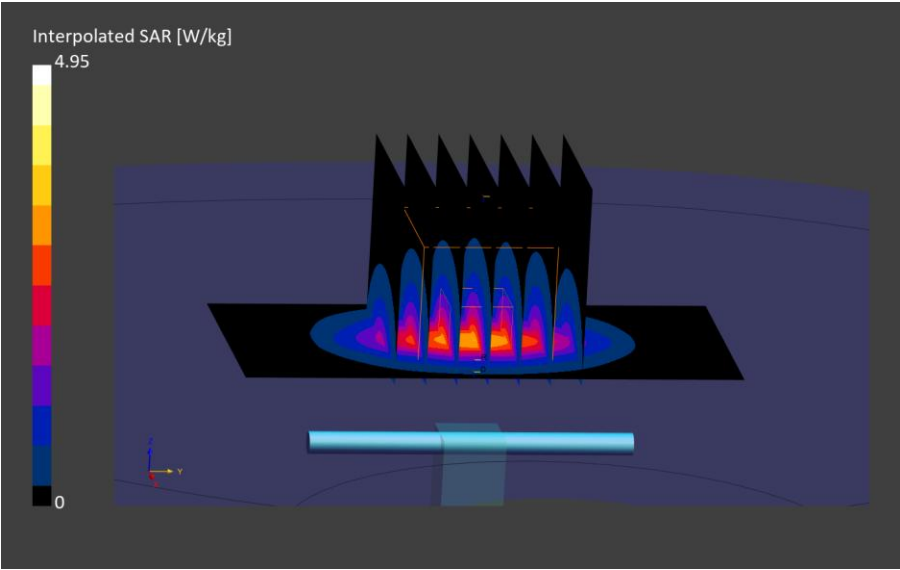

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.39, 7.44,7.43

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	21.2	21.2	18.0.0.7250	Twin-SAM V8.0 – 2233	Head Simulating Liquid	1.76	39.2	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.45	-3.39
psSAR10g	1.16	-2.34
Peak SAR (Extrapolated)	4.80	-8.09
psAPD (4.0 cm², sq)	N/A	N/A

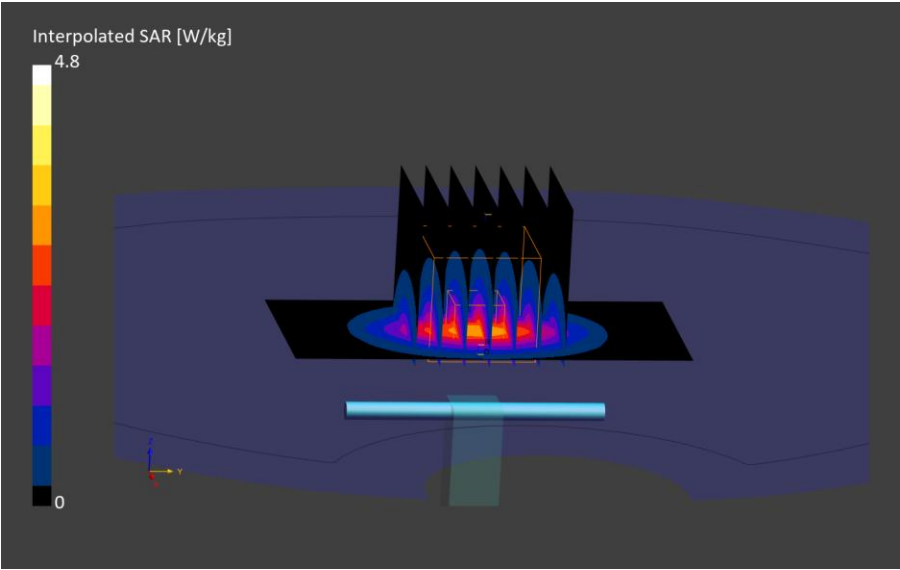

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.87, 6.85,6.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-18	21.7	20.4	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.99	42.1	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.75	-0.78
psSAR10g	1.25	0.16
Peak SAR (Extrapolated)	5.78	-2.35
psAPD (4.0 cm², sq)	N/A	N/A

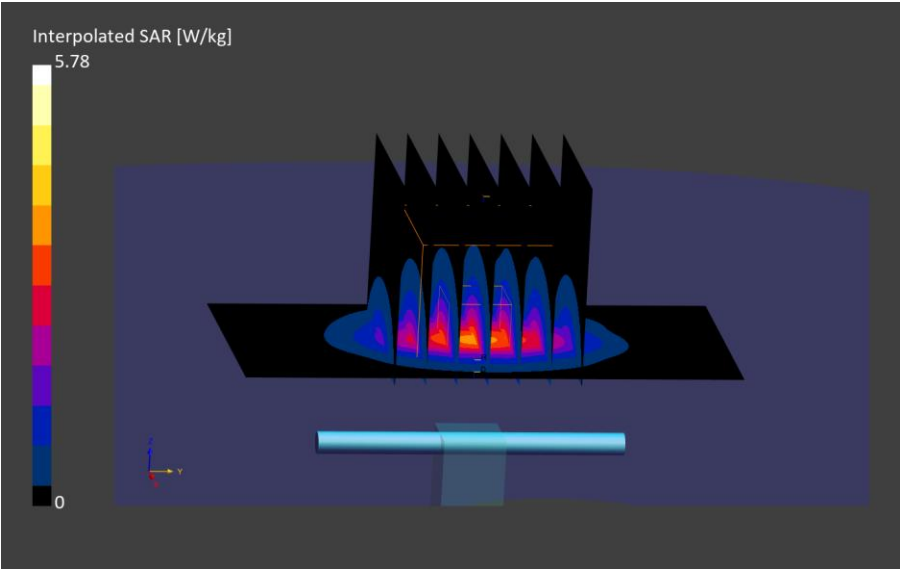

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	7.07, 6.81,6.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-27	22.8	22.1	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.94	40.1	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.60	-6.19
psSAR10g	1.18	-5.45
Peak SAR (Extrapolated)	5.25	-11.3
psAPD (4.0 cm², sq)	N/A	N/A

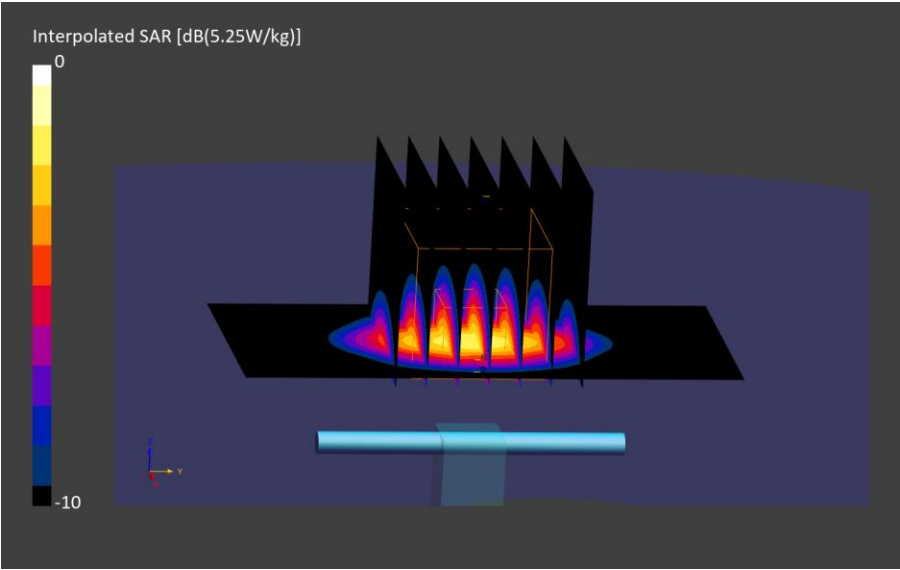

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	7.07, 6.81,6.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-01	21.9	21.8	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.90	40.2	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.53	-8.72
psSAR10g	1.14	-8.65
Peak SAR (Extrapolated)	5.06	-14.51
psAPD (4.0 cm², sq)	N/A	N/A

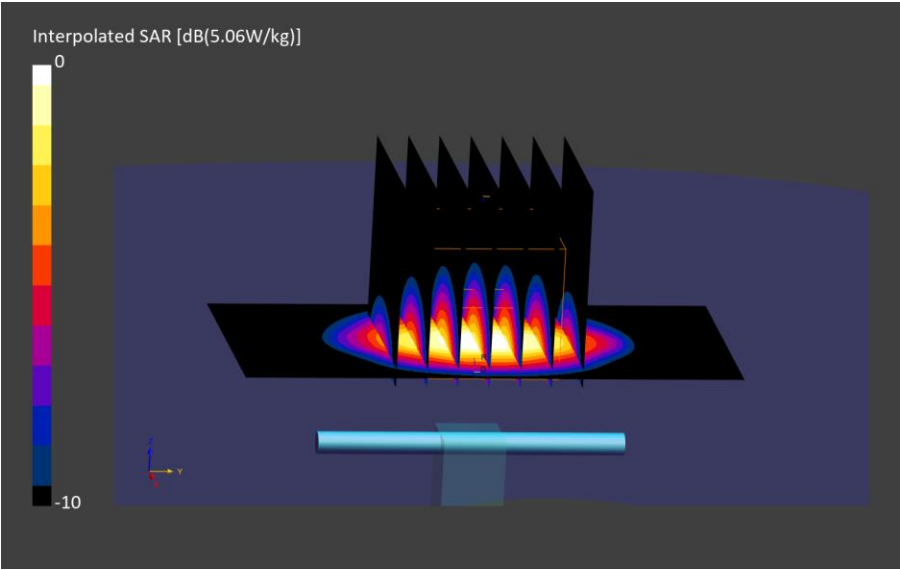

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.87, 6.85,6.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	21.9	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.87	38.7	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.70	-2.58
psSAR10g	1.22	-2.24
Peak SAR (Extrapolated)	5.56	-6.07
psAPD (4.0 cm², sq)	N/A	N/A

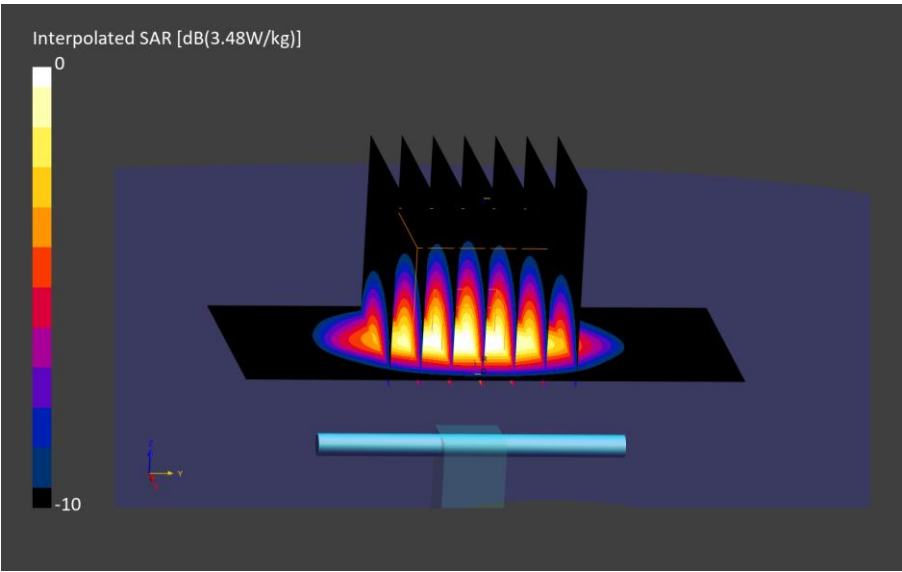

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.87, 6.85,6.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-05	22.1	21.7	17.0.4.7034	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.84	37.6	EX3DV4 – SN7857, 2025-12-09	DAE4ip Sn1838, 2025-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.68	-3.3
psSAR10g	1.21	-3.04
Peak SAR (Extrapolated)	5.46	-7.76
psAPD (4.0 cm², sq)	N/A	N/A

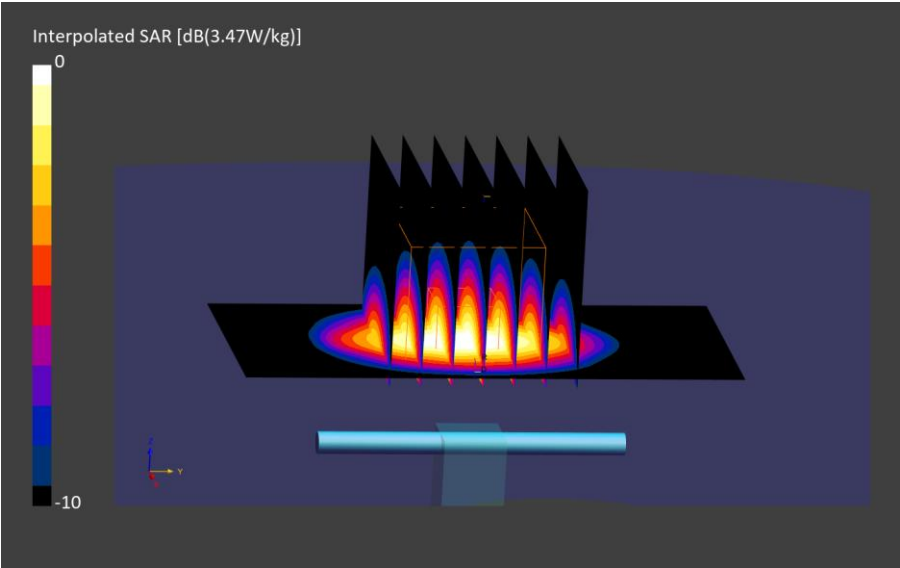

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	7.12, 7.0,6.77

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.1	22	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.90	40.2	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.59	-6.55
psSAR10g	1.18	-5.45
Peak SAR (Extrapolated)	5.22	-11.81
psAPD (4.0 cm², sq)	N/A	N/A

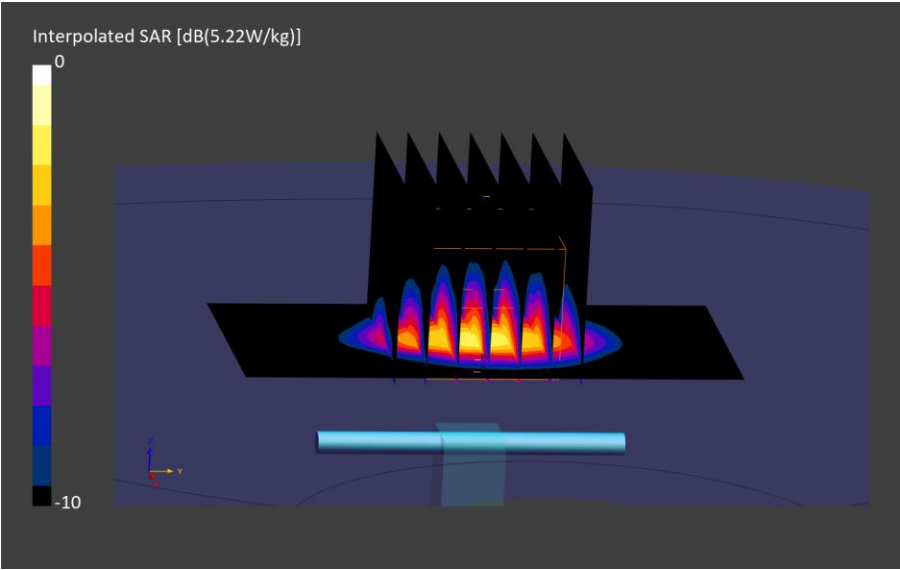

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.22, 5.99, 5.97

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-13	21.5	20.8	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.73	39.9	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.09	-5.29
psSAR10g	1.18	-4.29
Peak SAR (Extrapolated)	7.82	-7.62
psAPD (4.0 cm², sq)	N/A	N/A

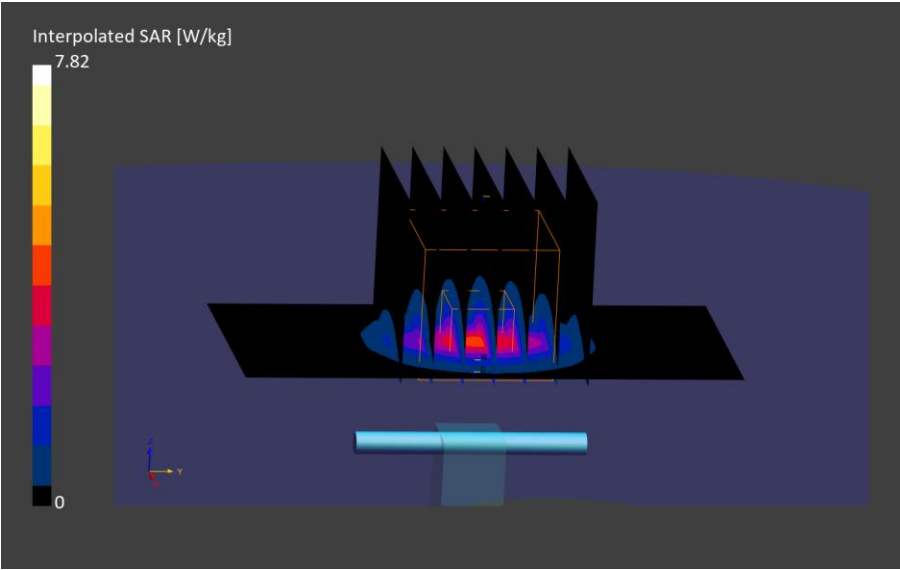

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.35, 6.87,6.31

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	20.8	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	2.77	39.6	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.25	-0.39
psSAR10g	1.24	0.57
Peak SAR (Extrapolated)	8.17	-3.49
psAPD (4.0 cm², sq)	N/A	N/A

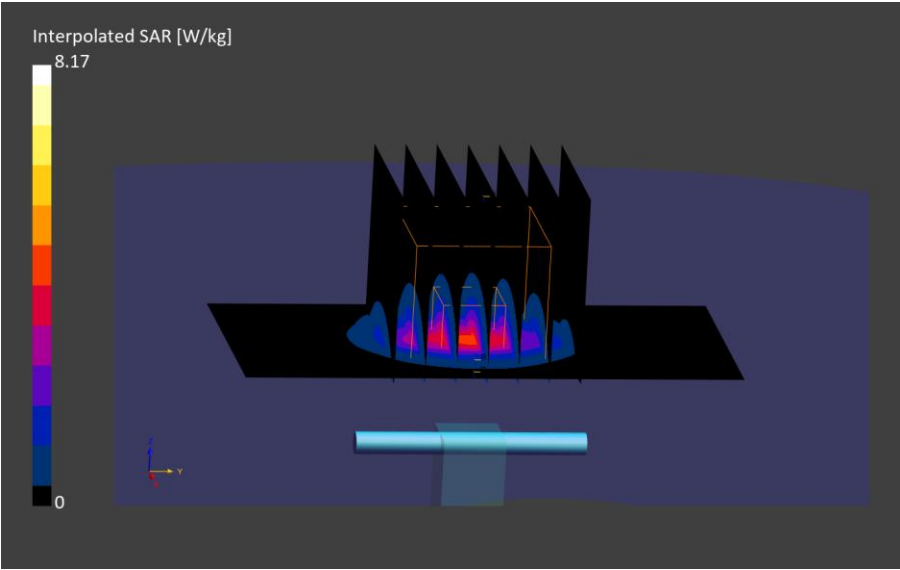

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.22, 5.99, 5.97

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-07	20.5	20.9	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.72	39.7	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.12	-4.37
psSAR10g	1.19	-3.48
Peak SAR (Extrapolated)	7.61	-10.1
psAPD (4.0 cm², sq)	N/A	N/A

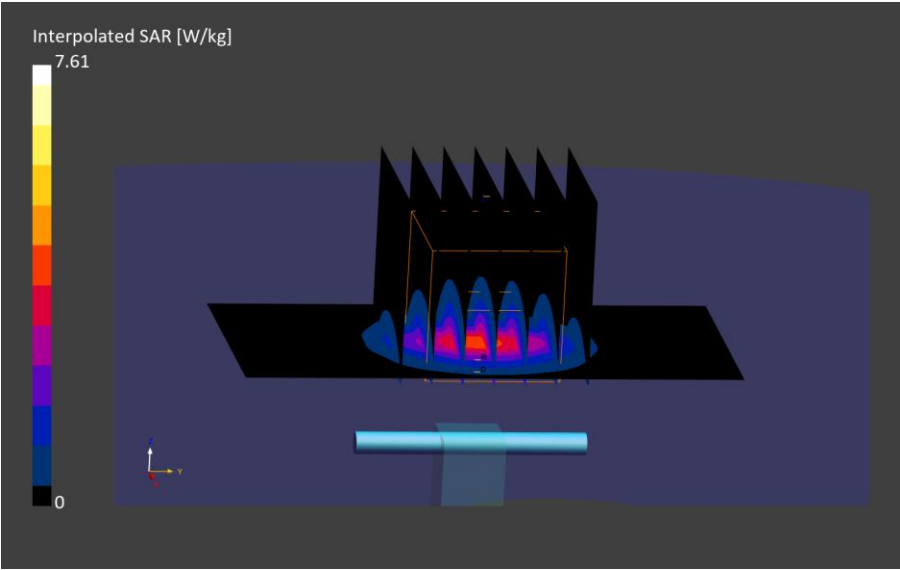

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.22, 5.99, 5.97

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-24	22.8	21.3	18.0.0.7250	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.71	40.5	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.12	-4.37
psSAR10g	1.18	-4.29
Peak SAR (Extrapolated)	7.55	-10.81
psAPD (4.0 cm², sq)	N/A	N/A

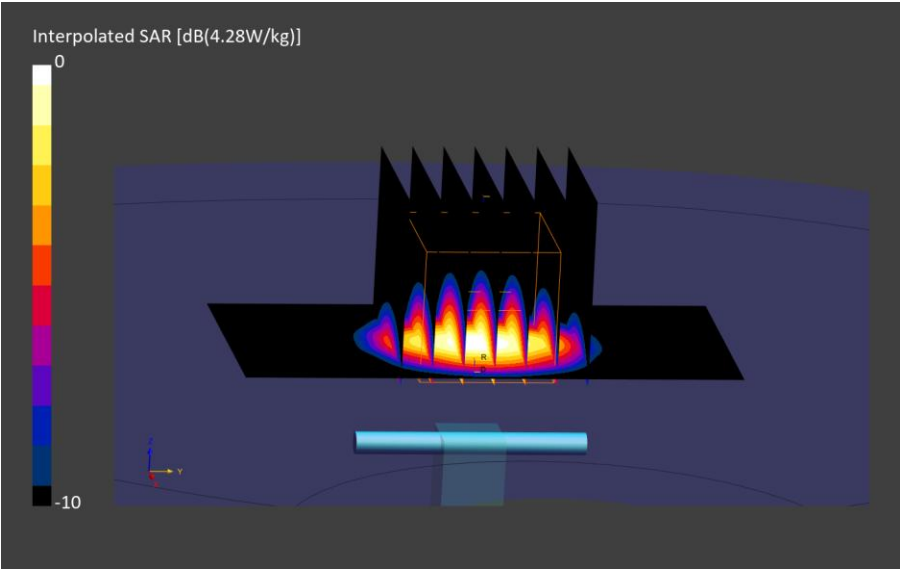

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	6.2, 5.97,5.95

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-13	21.5	20.8	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.93	39.6	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.24	-2.93
psSAR10g	1.21	-1.46
Peak SAR (Extrapolated)	8.38	-4.84
psAPD (4.0 cm², sq)	N/A	N/A

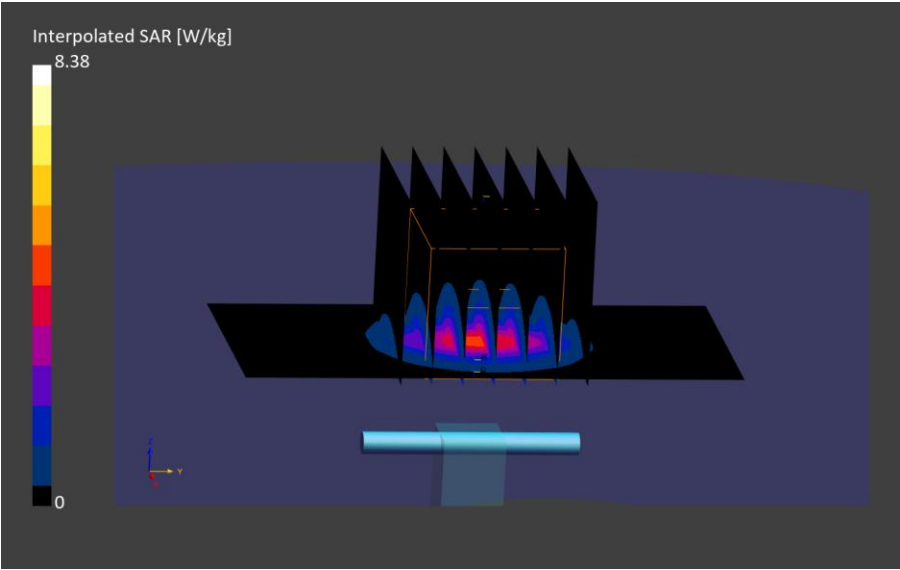

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	6.3, 6.81,6.26

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-03	21.9	20.8	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	2.96	39.3	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.38	1.26
psSAR10g	1.26	2.61
Peak SAR (Extrapolated)	8.84	0.39
psAPD (4.0 cm², sq)	N/A	N/A

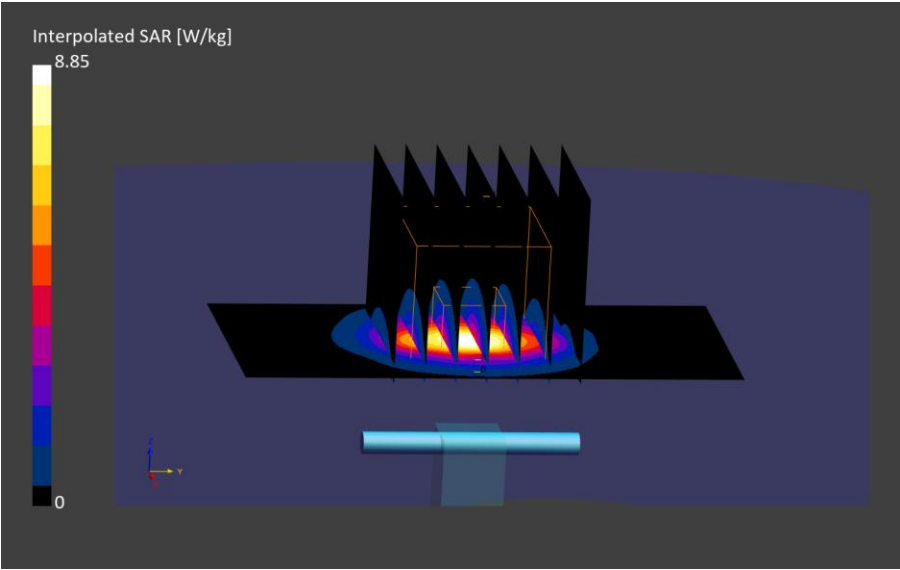

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	6.2, 5.97, 5.95

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-07	20.5	20.9	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.91	39.4	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.12	-6.53
psSAR10g	1.17	-4.72
Peak SAR (Extrapolated)	8.00	-9.15
psAPD (4.0 cm², sq)	N/A	N/A

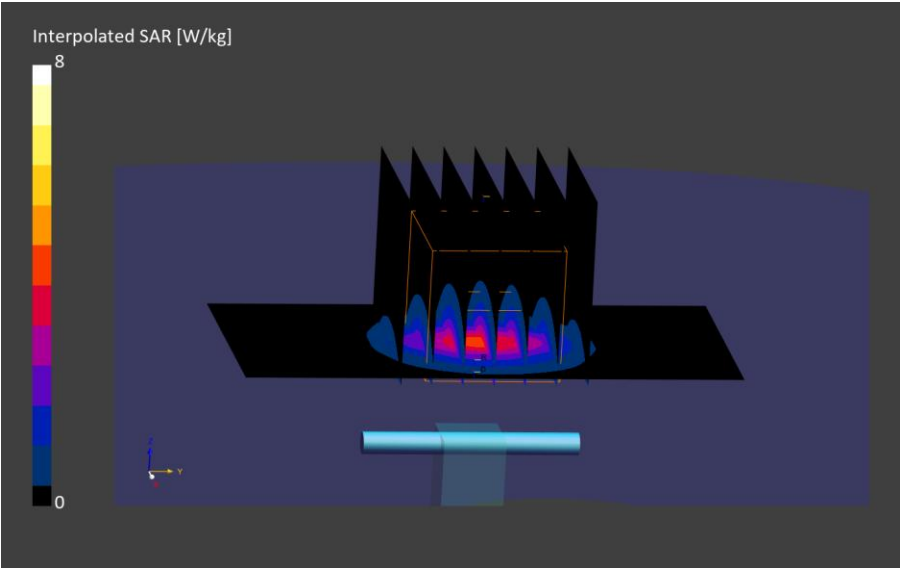

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	6.2, 5.97,5.95

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-24	22.8	21.3	18.0.0.7250	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.90	40.2	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.15	-5.63
psSAR10g	1.18	-3.9
Peak SAR (Extrapolated)	7.95	-9.72
psAPD (4.0 cm², sq)	N/A	N/A

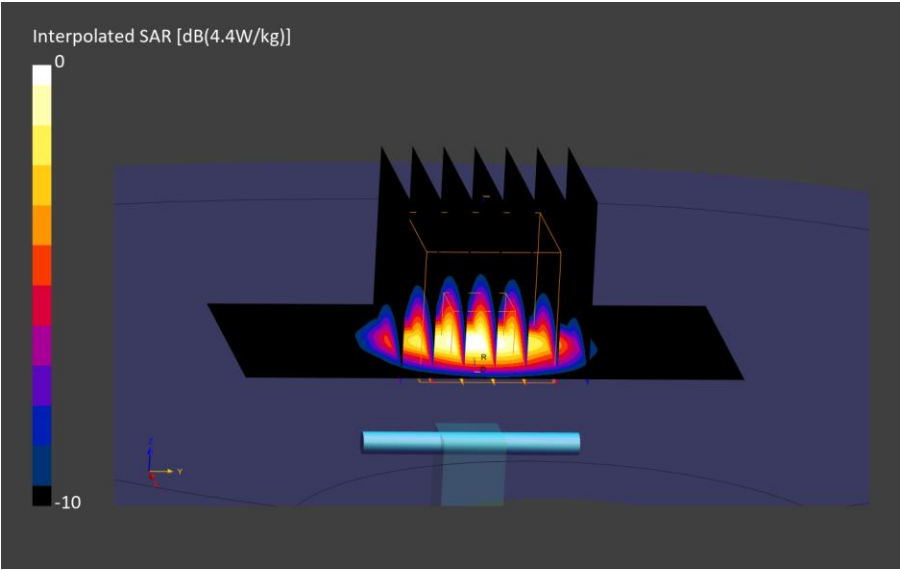

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3900V2 – SN1101	17.0	Flat	10	CW, 0	3900.000	6.18, 5.95, 5.93

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-13	21.5	20.8	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	3.13	39.3	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.25	-7.63
psSAR10g	1.15	-6.73
Peak SAR (Extrapolated)	9.00	-7.2
psAPD (4.0 cm², sq)	N/A	N/A

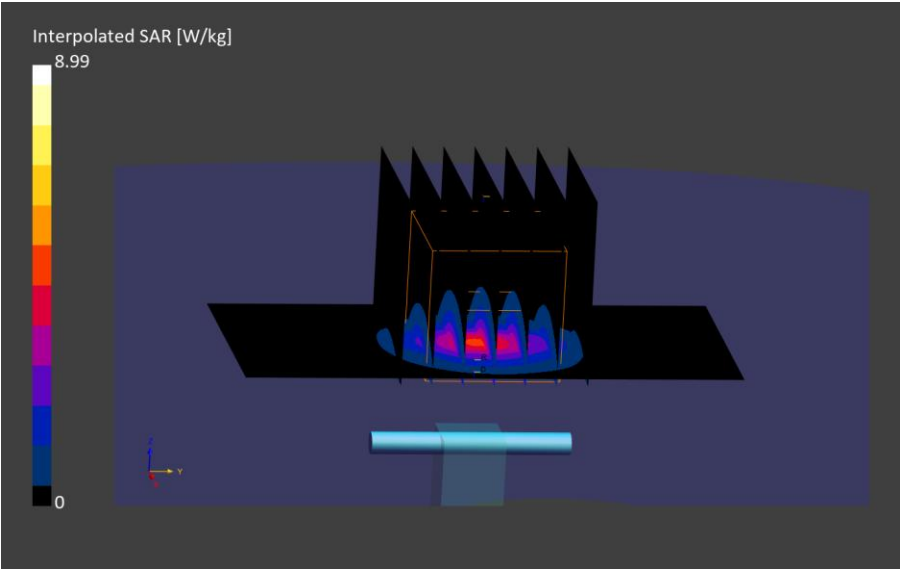

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.43, 5.87,5.39

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.1	21.9	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.56	36.4	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.88	-0.62
psSAR10g	1.11	-1.13
Peak SAR (Extrapolated)	15.9	2.27
psAPD (4.0 cm², sq)	N/A	N/A

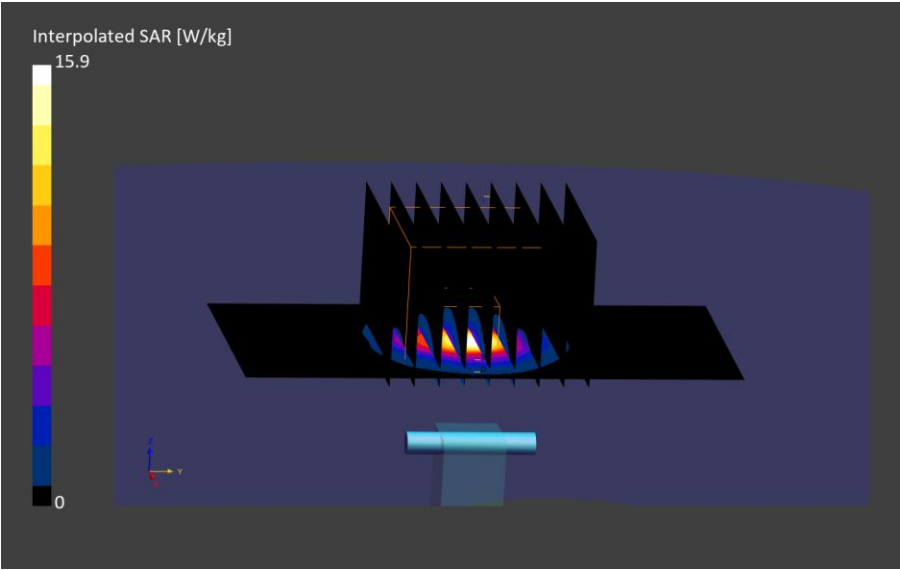

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.43, 5.87,5.39

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	21.4	21.1	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.58	36.1	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.93	0.66
psSAR10g	1.12	-0.24
Peak SAR (Extrapolated)	16.2	4.2
psAPD (4.0 cm², sq)	N/A	N/A

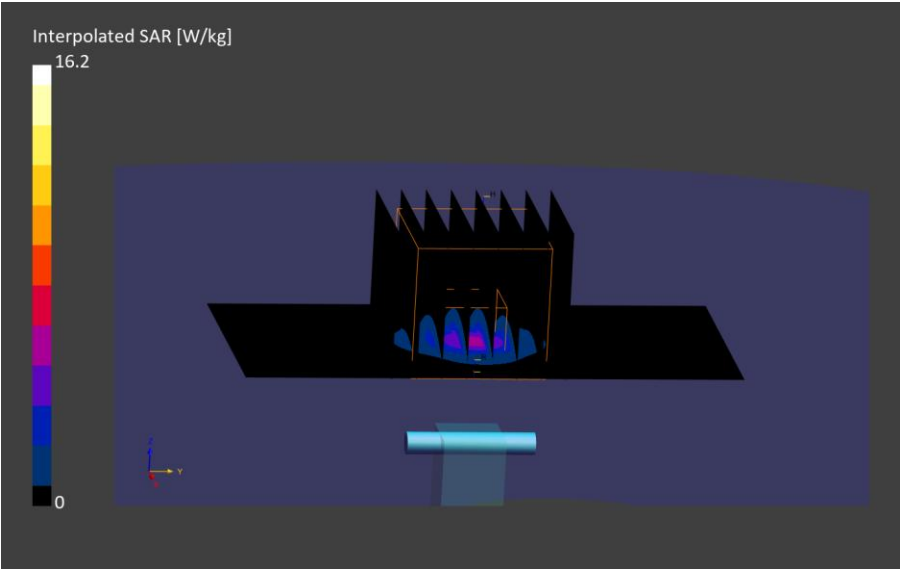

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.43, 5.87, 5.39

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.5	24	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.54	37.2	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.94	0.92
psSAR10g	1.13	0.65
Peak SAR (Extrapolated)	15.9	2.27
psAPD (4.0 cm², sq)	N/A	N/A

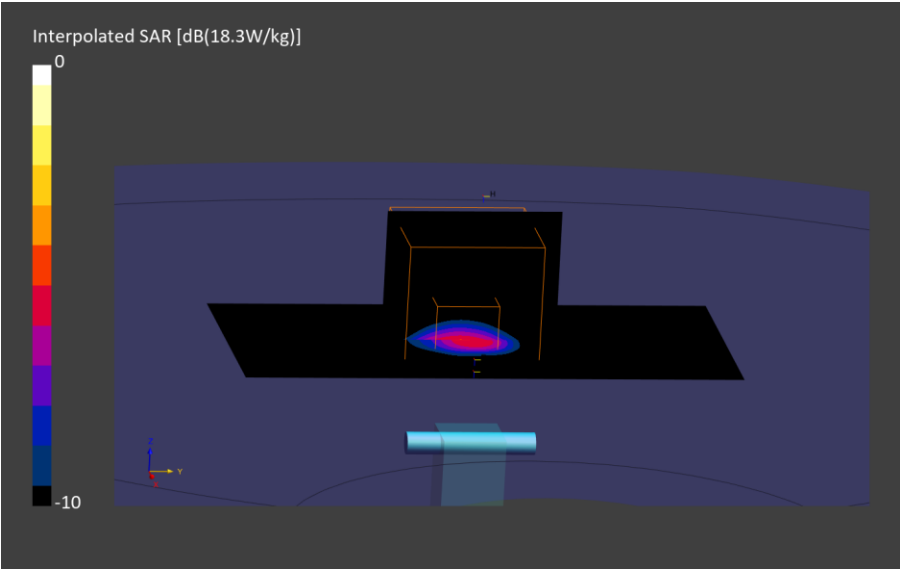

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	5.03, 5.45, 5.0

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.1	21.9	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.94	35.8	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.18	2.84
psSAR10g	1.18	1.05
Peak SAR (Extrapolated)	18.6	9.22
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	5.03, 5.45, 5.0

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	21.4	21.1	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.96	35.5	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.17	2.59
psSAR10g	1.17	0.19
Peak SAR (Extrapolated)	18.7	9.8
psAPD (4.0 cm², sq)	N/A	N/A

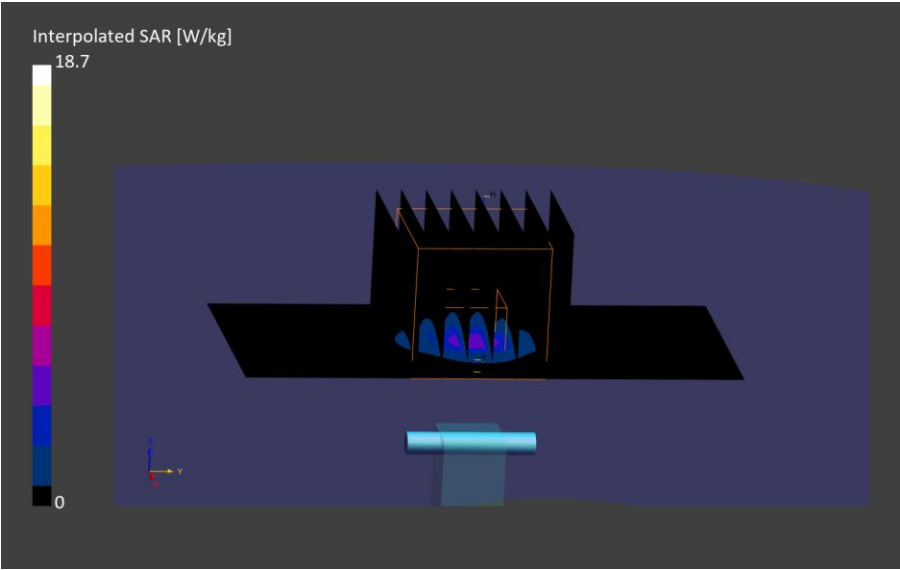

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5600.000	5.03, 5.45, 5.0

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.5	24	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.92	36.7	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 32.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.17	2.59
psSAR10g	1.18	1.05
Peak SAR (Extrapolated)	18.2	6.87
psAPD (4.0 cm², sq)	N/A	N/A

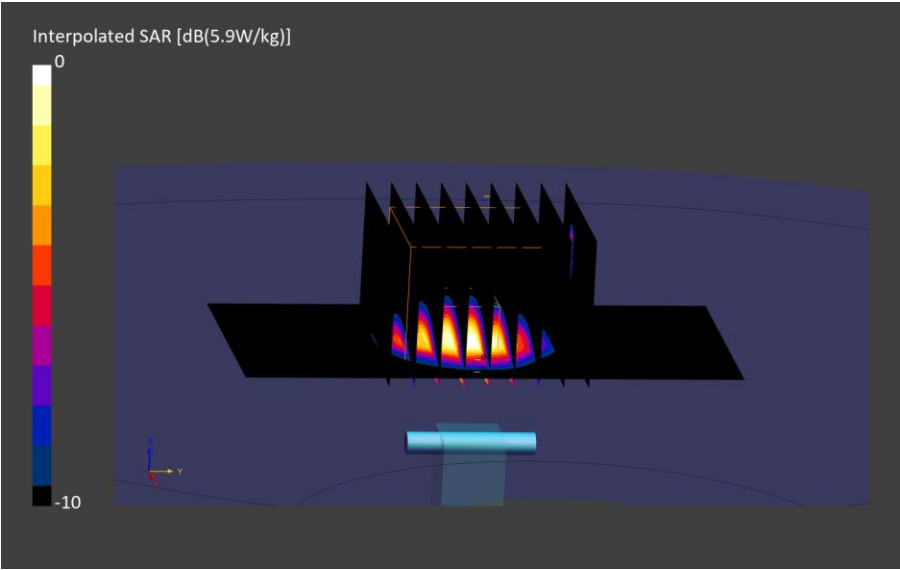

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	5.08, 5.49,5.05

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.1	21.9	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.10	35.5	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.03	0.39
psSAR10g	1.15	0.64
Peak SAR (Extrapolated)	18.5	10.81
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	5.08, 5.49,5.05

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	21.4	21.1	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.14	35.3	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.03	0.39
psSAR10g	1.13	-1.11
Peak SAR (Extrapolated)	18.8	12.61
psAPD (4.0 cm², sq)	N/A	N/A

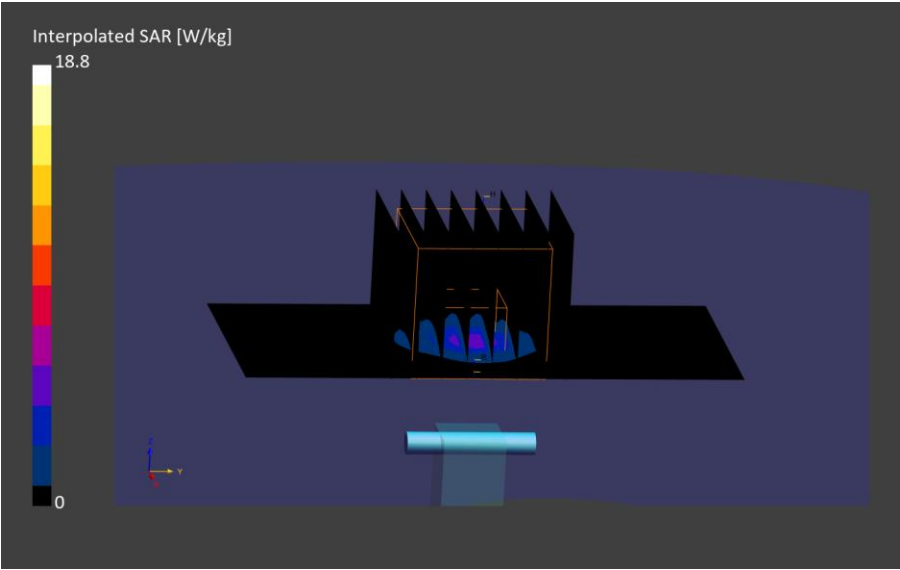

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5750.000	5.08, 5.49,5.05

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.5	24	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.10	36.4	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.93	-2.11
psSAR10g	1.11	-2.86
Peak SAR (Extrapolated)	17.8	6.62
psAPD (4.0 cm², sq)	N/A	N/A

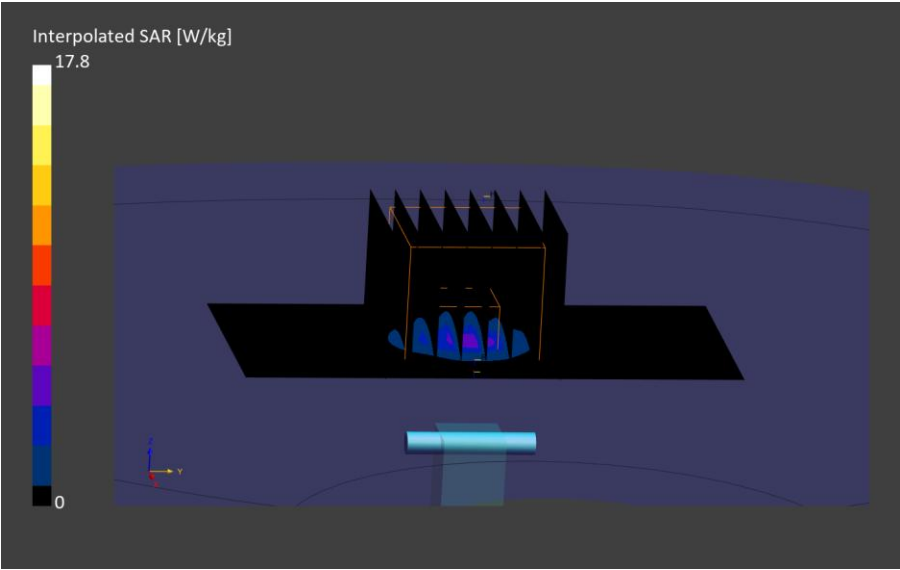

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5850.000	4.93, 5.34,4.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	21.1	21.9	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.22	35.3	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.05	5.08
psSAR10g	1.14	3.39
Peak SAR (Extrapolated)	19.1	9.29
psAPD (4.0 cm², sq)	N/A	N/A

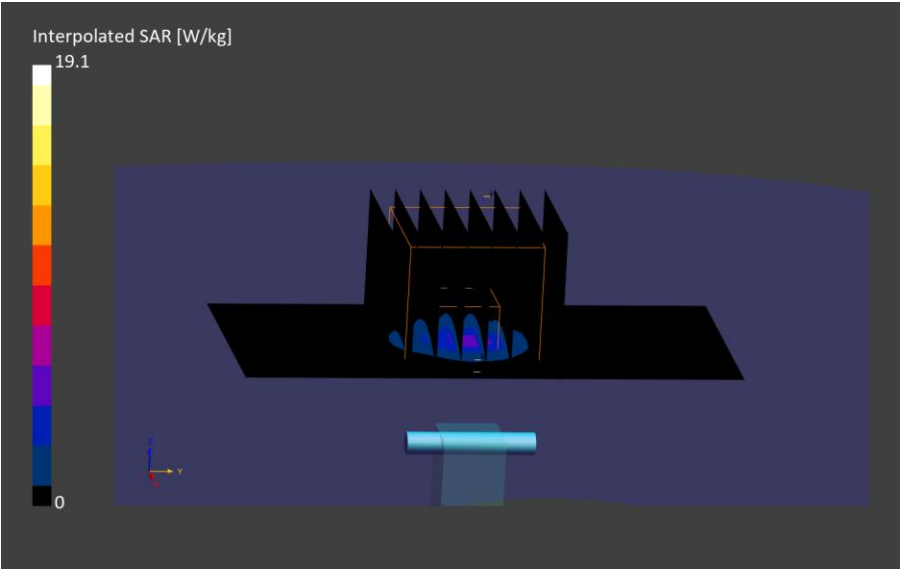

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5850.000	4.93, 5.34,4.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-14	21.4	21.1	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.25	35.1	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	4.11	6.64
psSAR10g	1.17	6.11
Peak SAR (Extrapolated)	19.6	12.15
psAPD (4.0 cm², sq)	N/A	N/A

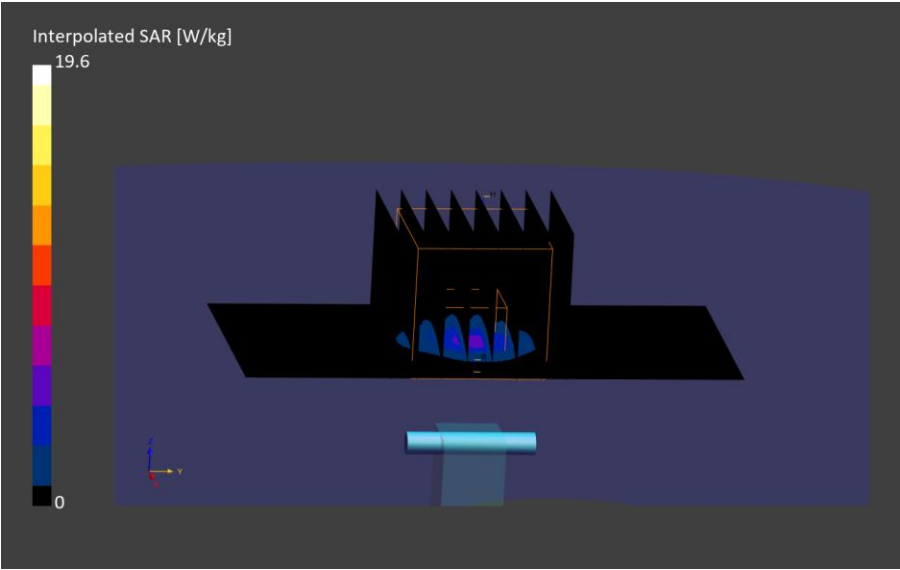

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5850.000	4.93, 5.34,4.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	24.5	24	18.0.0.7250	Twin-SAM V8.0 – 2165	Head Simulating Liquid	5.21	36.2	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 28.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.93	1.97
psSAR10g	1.13	2.48
Peak SAR (Extrapolated)	18.3	4.71
psAPD (4.0 cm², sq)	N/A	N/A

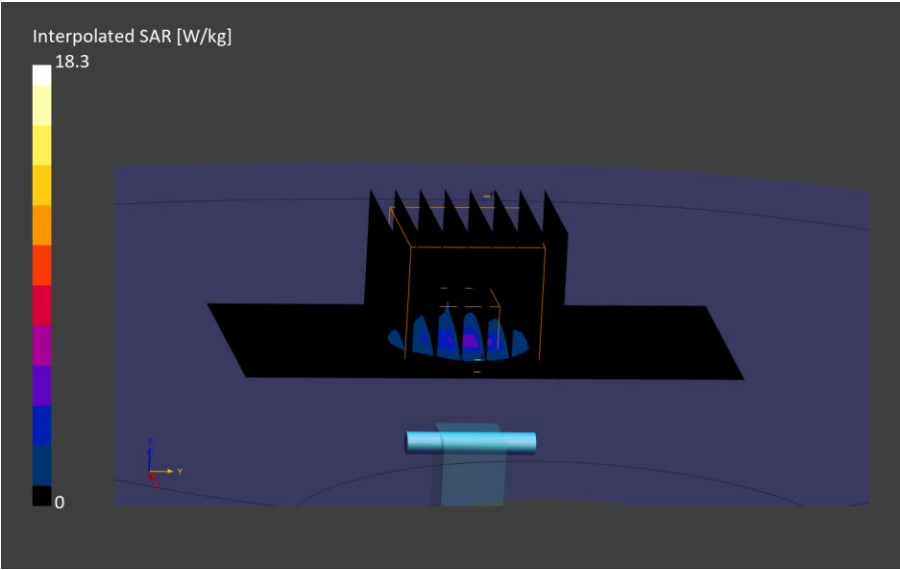

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	5.23, 5.66,5.2

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-05	22.1	21.5	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	6.06	34.0	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	27.2 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.89	-3.02
psSAR10g	0.534	-2.91
Peak SAR (Extrapolated)	18.3	-7.34
psAPD (4.0 cm², sq)	13.0	-3.0

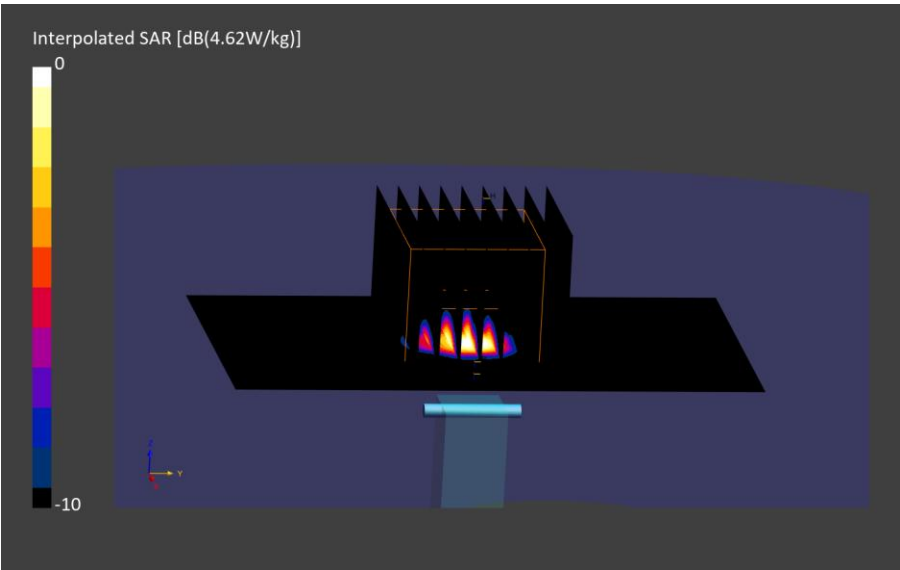

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	5.23, 5.66,5.2

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-08	23.1	22.3	17.0.4.7034	Twin-SAM V8.0 – 2165	Head Simulating Liquid	6.11	34.6	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	23.8 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.12	4.7
psSAR10g	0.575	4.55
Peak SAR (Extrapolated)	19.6	-0.76
psAPD (4.0 cm², sq)	13.9	3.7

