

APPENDIX B: SYSTEM VERIFICATION

PCTEST

DUT: Dipole 750.0 MHz; Type: D750V3; Serial: 1003

Communication System: UID: 0, CW; Frequency: 750.0 MHz

Medium: 750 Head; Medium parameters used:

$f = 750.0$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.5 cm

Test Date: 09/28/2021; Ambient Temp: 23.9°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN7406; ConvF:(10.08,10.08,10.08); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.0.0.65

750 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.63 W/kg

SAR(1 g) = 1.63 W/kg

Deviation (1 g) = -7.18%

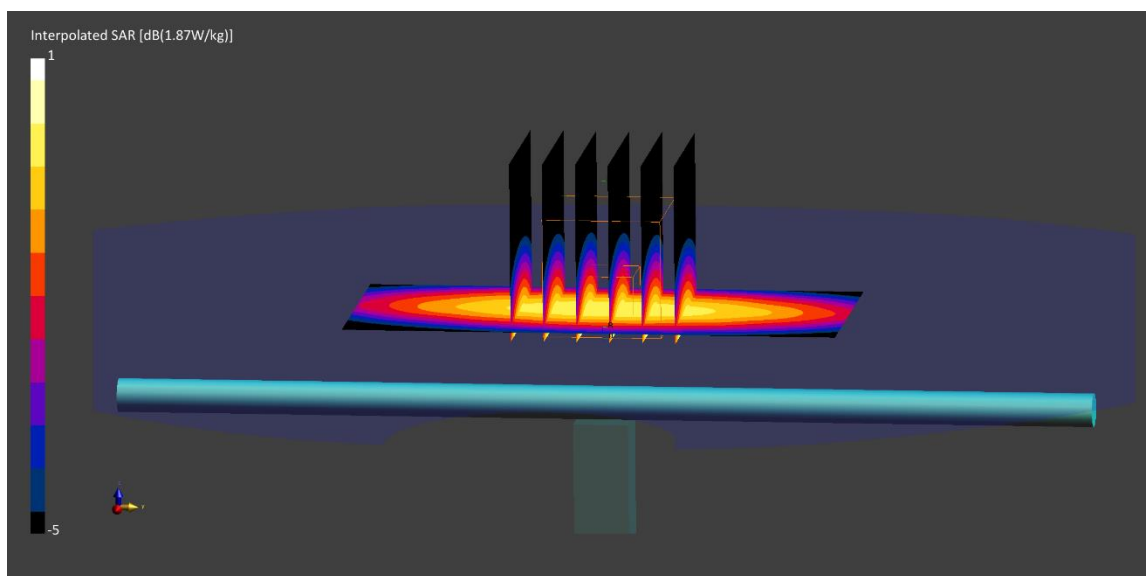

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Head Medium parameters used:

$f = 750 \text{ MHz}$; $\sigma = 0.913 \text{ S/m}$; $\epsilon_r = 42.687$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/07/2021; Ambient Temp: 22.2°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7402; ConvF(10.26, 10.26, 10.26) @ 750 MHz; Calibrated: 4/16/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/9/2021

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.49 W/kg

SAR(1 g) = 1.69 W/kg

Deviation(1 g) = -2.20%

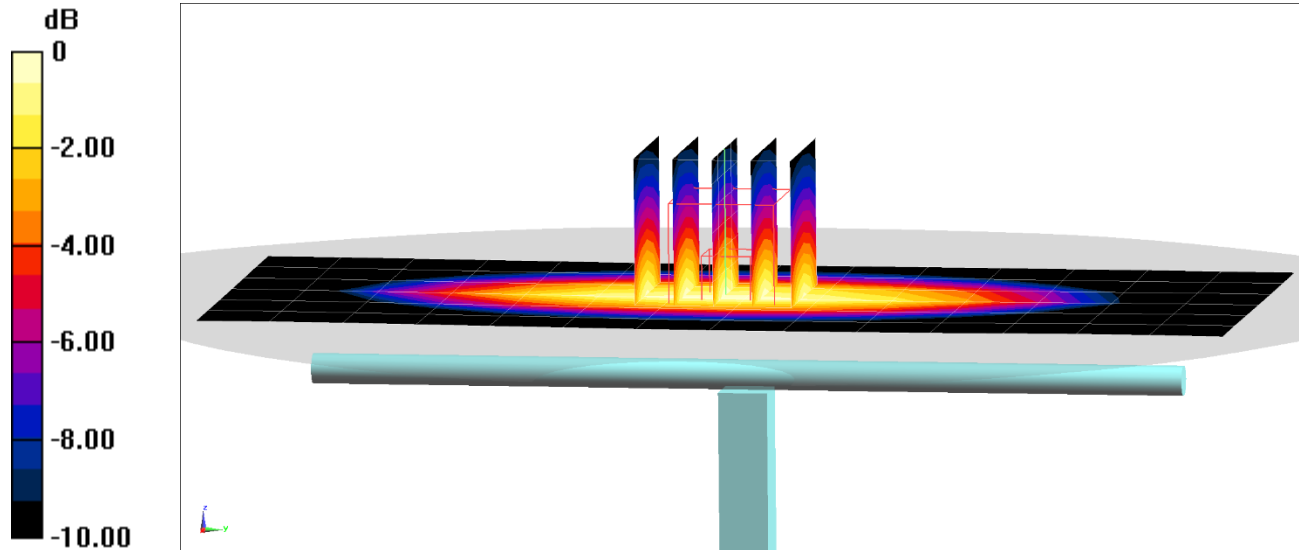

PCTEST

DUT: Dipole 750.0 MHz; Type: D750V3; Serial: 1161

Communication System: UID: 0, CW; Frequency: 750.0 MHz

Medium: 750 Head; Medium parameters used:

$f = 750.0$ MHz; $\sigma = 0.917$ S/m; $\epsilon_r = 41.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.5 cm

Test Date: 10/12/2021; Ambient Temp: 23.1°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7571; ConvF:(10.02,10.02,10.02); Calibrated: 2020-12-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1533; Calibrated: 2020-12-07

Phantom: Twin-SAM V5.0; Serial: 1648

Measurement SW: DASY Module SAR V16.0.0.116

750 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.64 W/kg

SAR(1 g) = 1.73 W/kg

Deviation (1 g) = 7.72%

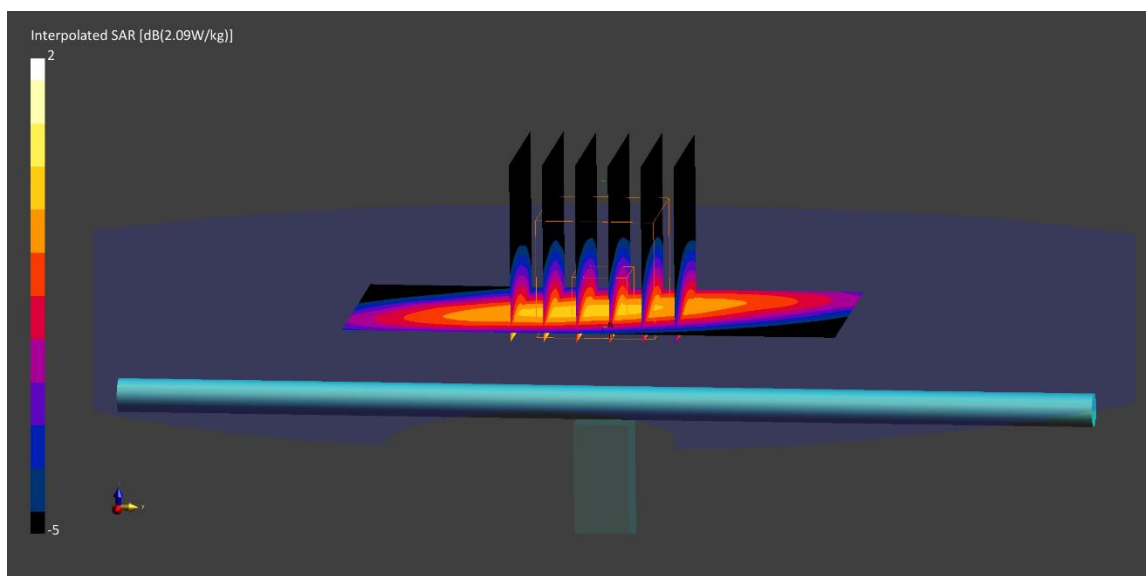

PCTEST

DUT: Dipole 750 MHz Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Head Medium parameters used:

$f = 750 \text{ MHz}$; $\sigma = 0.915 \text{ S/m}$; $\epsilon_r = 40.566$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/14/2021; Ambient Temp: 21.6°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7402; ConvF(10.26, 10.26, 10.26) @ 750 MHz; Calibrated: 4/16/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/9/2021

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.54 W/kg

SAR(1 g) = 1.71 W/kg

Deviation(1 g) = -1.04%

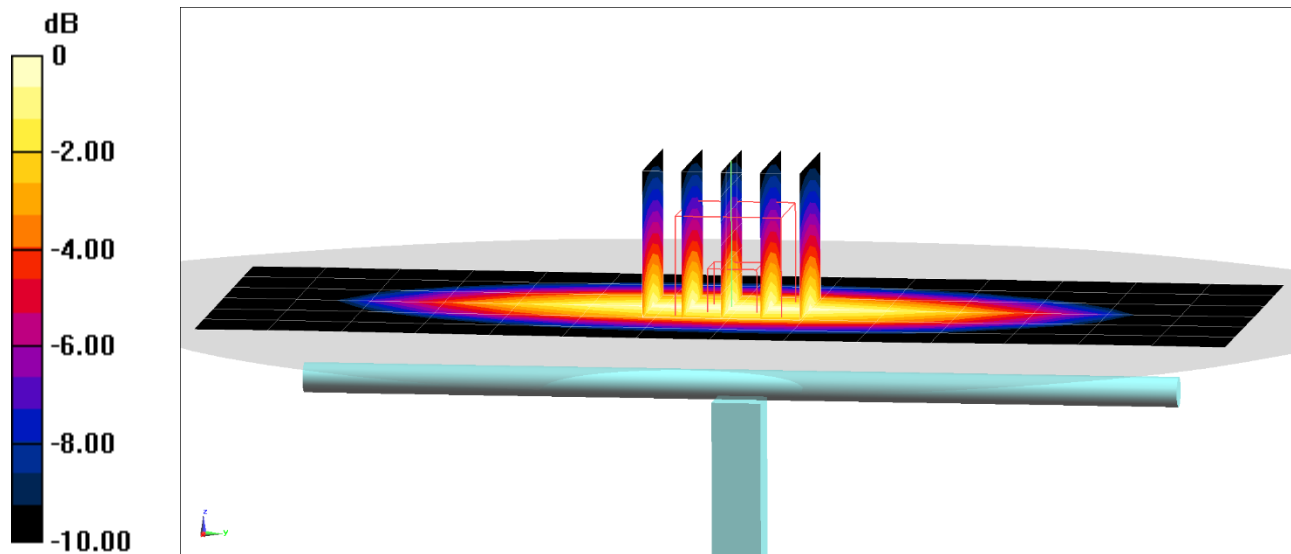

0 dB = 2.27 W/kg = 3.56 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d119

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.894 \text{ S/m}$; $\epsilon_r = 40.28$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/23/2021; Ambient Temp: 20.2°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7565; ConvF(9.11, 9.11, 9.11) @ 835 MHz; Calibrated: 11/12/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1466; Calibrated: 11/6/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1626

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.95 W/kg

SAR(1 g) = 2.02 W/kg

Deviation(1 g) = 4.77%

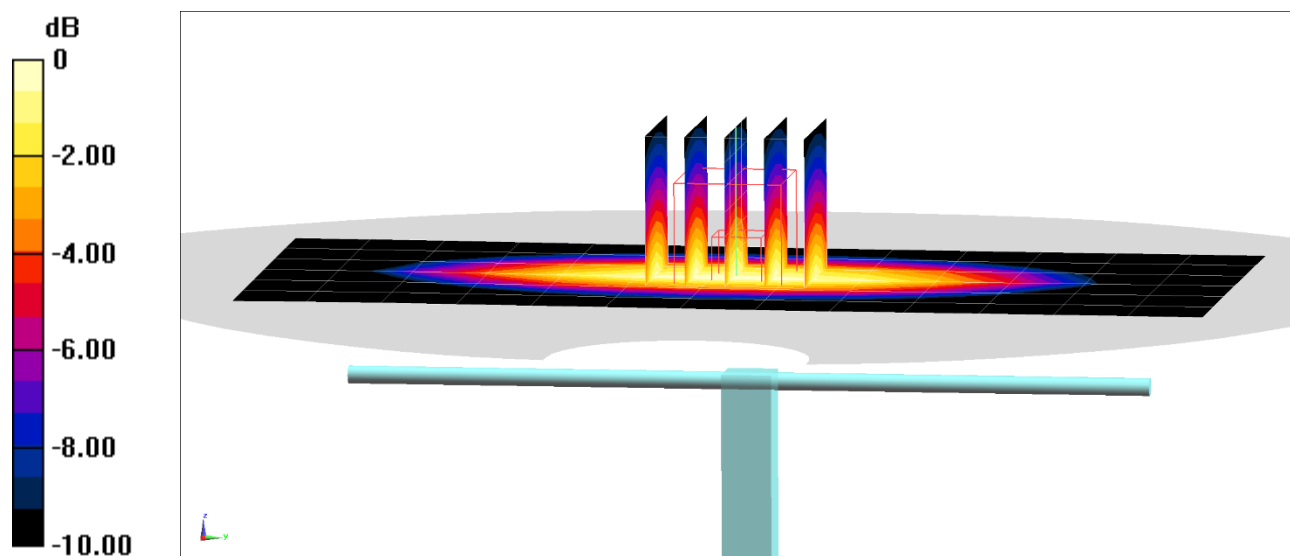

0 dB = 2.67 W/kg = 4.27 dBW/kg

PCTEST

DUT: Dipole 835 MHz Type: D835V2; Serial: 4d180

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.929 \text{ S/m}$; $\epsilon_r = 43.21$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/27/2021; Ambient Temp: 19.5°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN7402; ConvF(10.05, 10.05, 10.05) @ 835 MHz; Calibrated: 04/16/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 04/09/2021

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.95 W/kg

SAR(1 g) = 1.97 W/kg

Deviation(1 g) = 4.23%

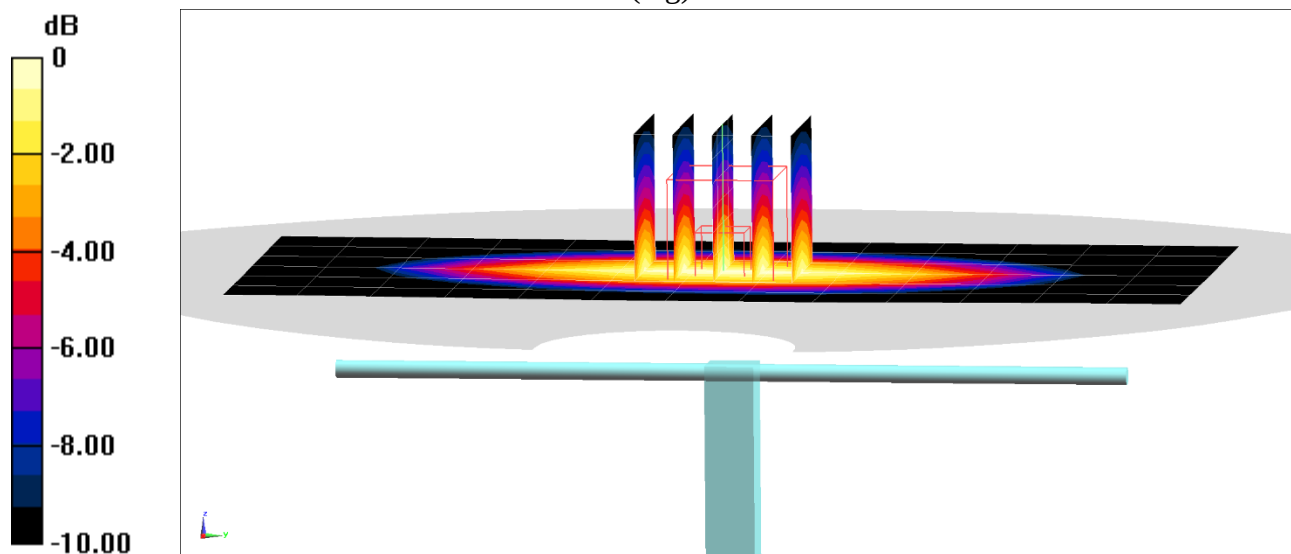

0 dB = 2.63 W/kg = 4.20 dBW/kg

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2; Serial: 4d132

Communication System: UID: 0, CW; Frequency: 835.0 MHz

Medium: 835 Head; Medium parameters used:

$f = 835.0$ MHz; $\sigma = 0.939$ S/m; $\epsilon_r = 41.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.5 cm

Test Date: 09/30/2021; Ambient Temp: 24.9°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7406; ConvF:(9.68,9.68,9.68); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.0.0.65

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.17 W/kg

SAR(1 g) = 1.98 W/kg

Deviation (1 g) = 2.48%

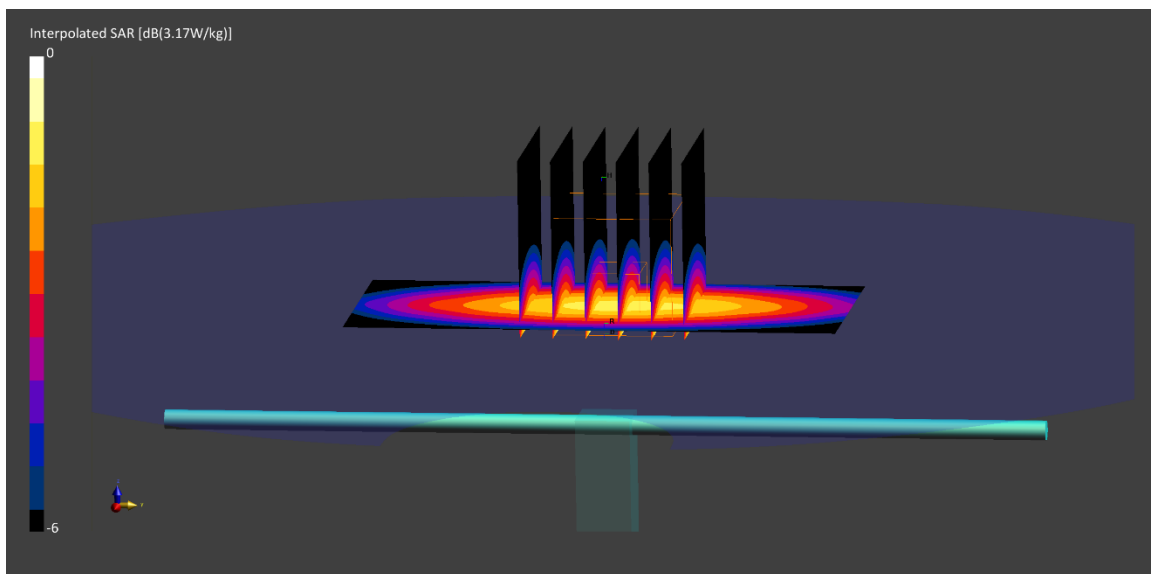

PCTEST

DUT: Dipole 835.0 MHz; Type: D835V2; Serial: 4d132

Communication System: UID: 0, CW; Frequency: 835.0 MHz

Medium: 750 Head; Medium parameters used:

$f = 835.0$ MHz; $\sigma = 0.920$ S/m; $\epsilon_r = 40.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.5 cm

Test Date: 10/18/2021; Ambient Temp: 22.7°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7571; ConvF:(9.76,9.76,9.76); Calibrated: 2020-12-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1533; Calibrated: 2020-12-07

Phantom: Twin-SAM V5.0; Serial: 1648

Measurement SW: DASY Module SAR V16.0.0.116

835 MHz System Verification at 23 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.99 W/kg

SAR(1 g) = 1.92 W/kg

Deviation (1 g) = -0.62%

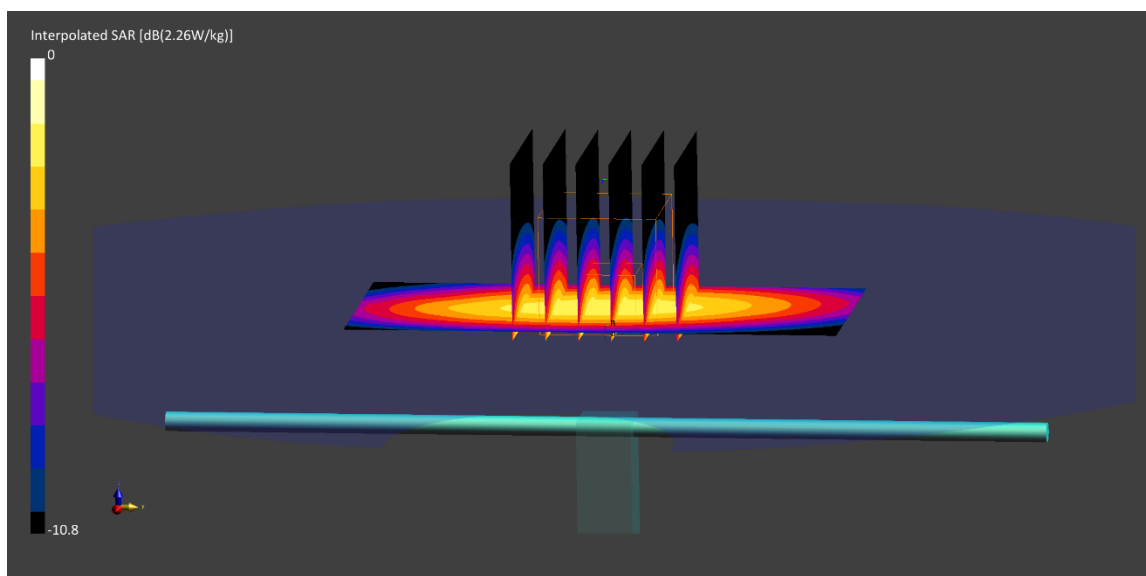

PCTEST

DUT: Dipole 1750.0 MHz; Type: D1750V2; Serial: 1150

Communication System: UID: 0, CW; Frequency: 1750.0 MHz

Medium: 1750 Head; Medium parameters used:

$f = 1750.0$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/06/2021; Ambient Temp: 23.9°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7406; ConvF:(8.26,8.26,8.26); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.0.0.65

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.50 W/kg

SAR(1 g) = 3.76 W/kg

Deviation (1 g) = 3.01%

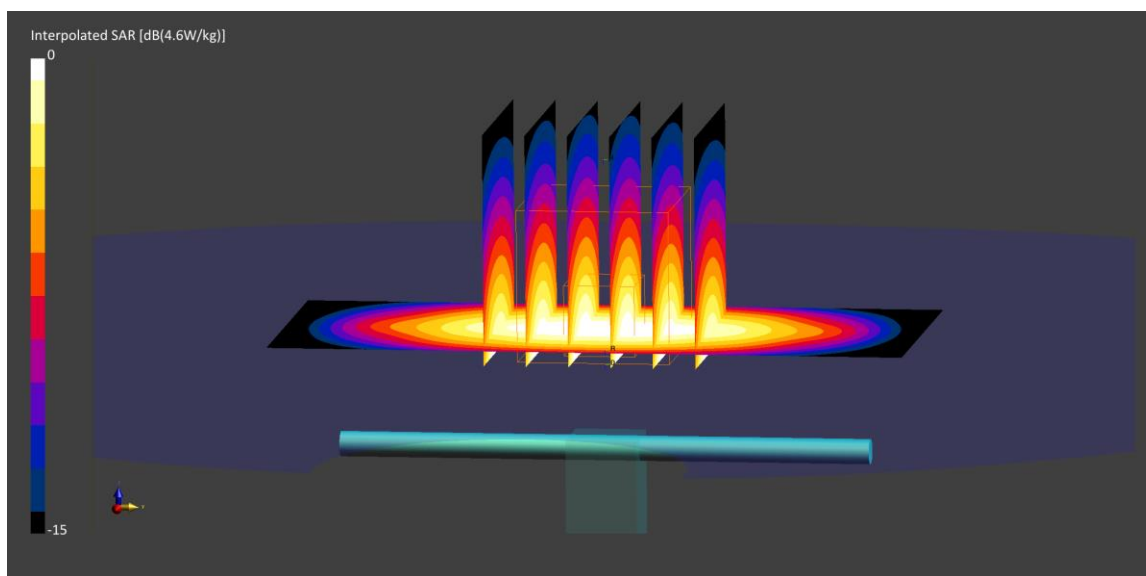

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1148

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Head Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.351 \text{ S/m}$; $\epsilon_r = 40.506$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/24/2021; Ambient Temp: 21.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7409; ConvF(8.3, 8.3, 8.3) @ 1750 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.03 W/kg

SAR(1 g) = 3.82 W/kg

Deviation(1 g) = 6.41%

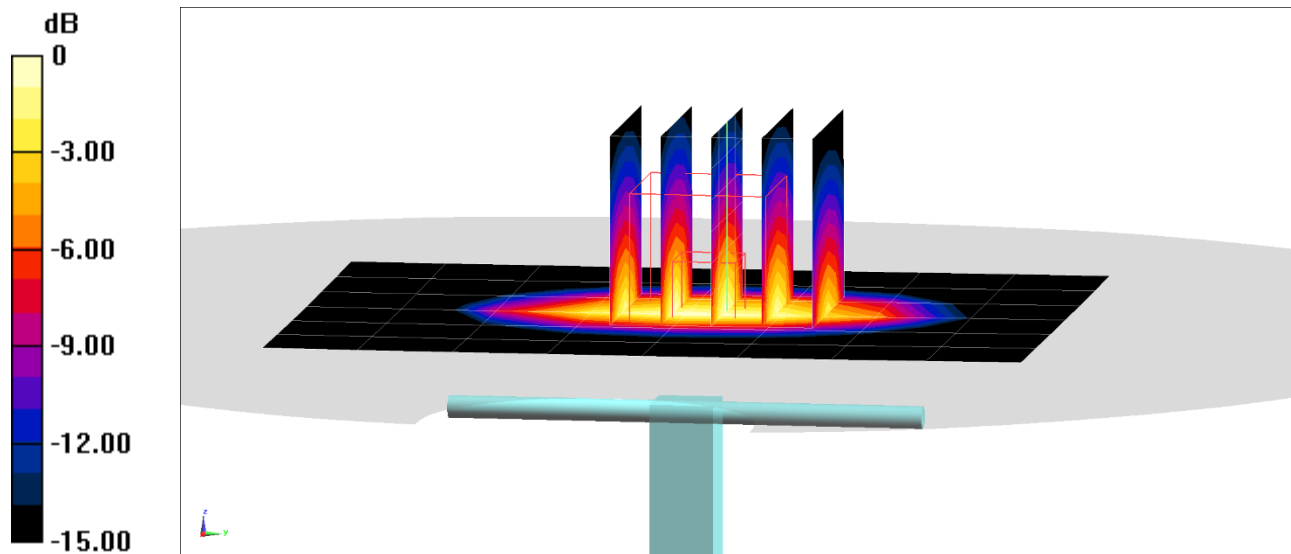

0 dB = 5.87 W/kg = 7.69 dBW/kg

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2; Serial: 5d080

Communication System: UID: 0, CW; Frequency: 1900.0 MHz

Medium: 1900 Head; Medium parameters used:

$f = 1900.0$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.0$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/10/2021; Ambient Temp: 23.7°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7406; ConvF:(7.98,7.98,7.98); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.0.0.65

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.40 W/kg

SAR(1 g) = 4.13 W/kg

Deviation (1 g) = 3.77%

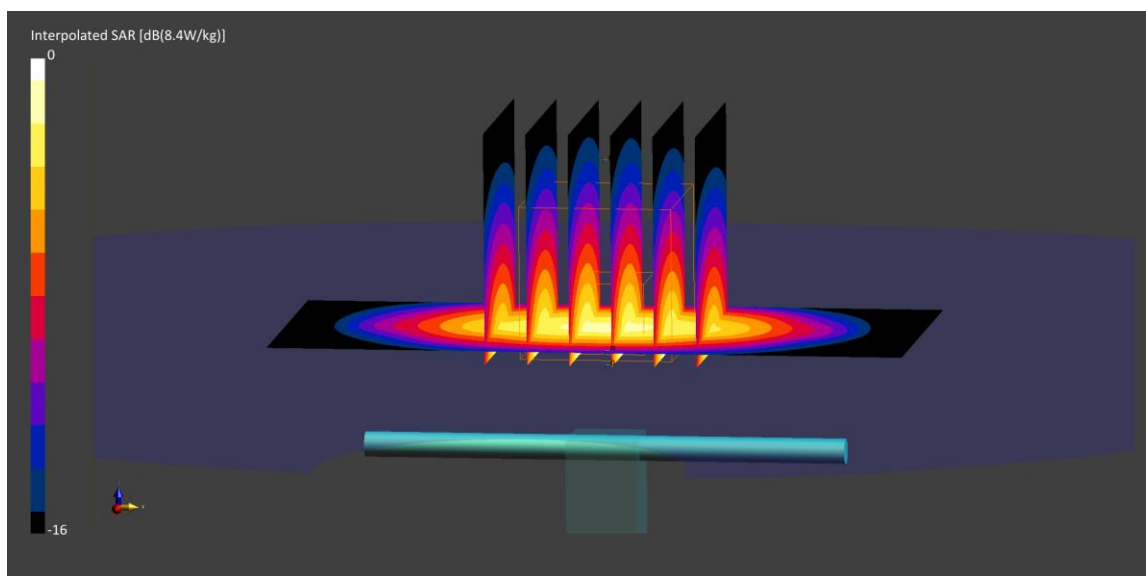

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2; Serial: 5d080

Communication System: UID: 0, CW; Frequency: 1900.0 MHz

Medium: 1900 Head; Medium parameters used:

$f = 1900.0$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 38.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/12/2021; Ambient Temp: 23.5°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7406; ConvF:(7.98,7.98,7.98); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY8 Module SAR V16.0.0.65

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.35 W/kg

SAR(1 g) = 4.27 W/kg

Deviation (1 g) = 7.29%

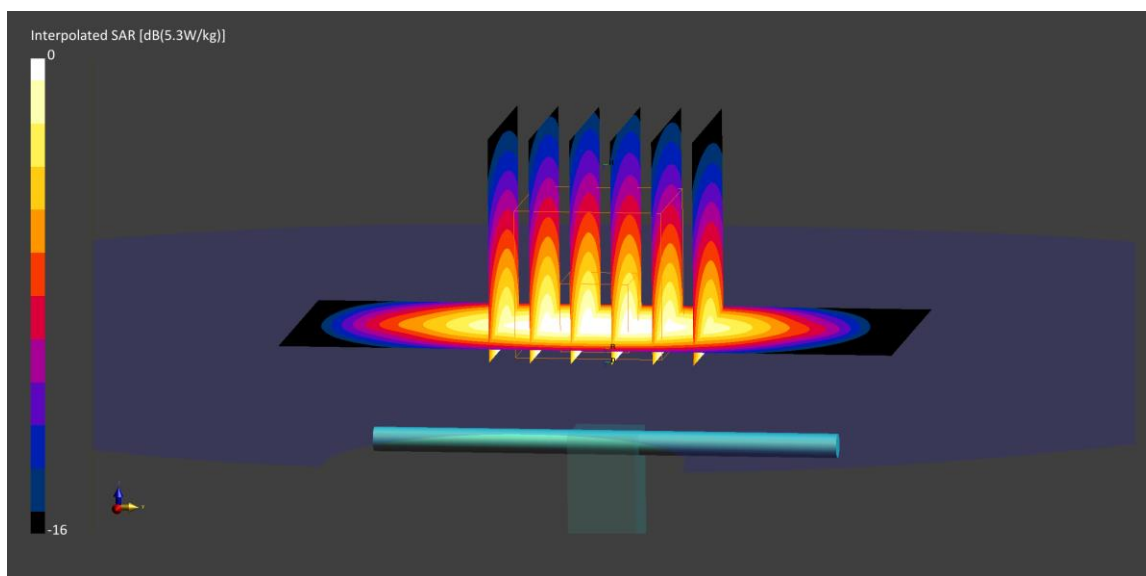

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2; Serial: 5d149

Communication System: UID: 0, CW; Frequency: 1900.0 MHz

Medium: 1900 Head; Medium parameters used:

$f = 1900.0$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 38.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/25/2021; Ambient Temp: 23.1°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7406; ConvF:(7.98,7.98,7.98); Calibrated: 2021-07-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1676; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.0.0.65

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.06 W/kg

SAR(1 g) = 4.11 W/kg

Deviation (1 g) = 1.48%

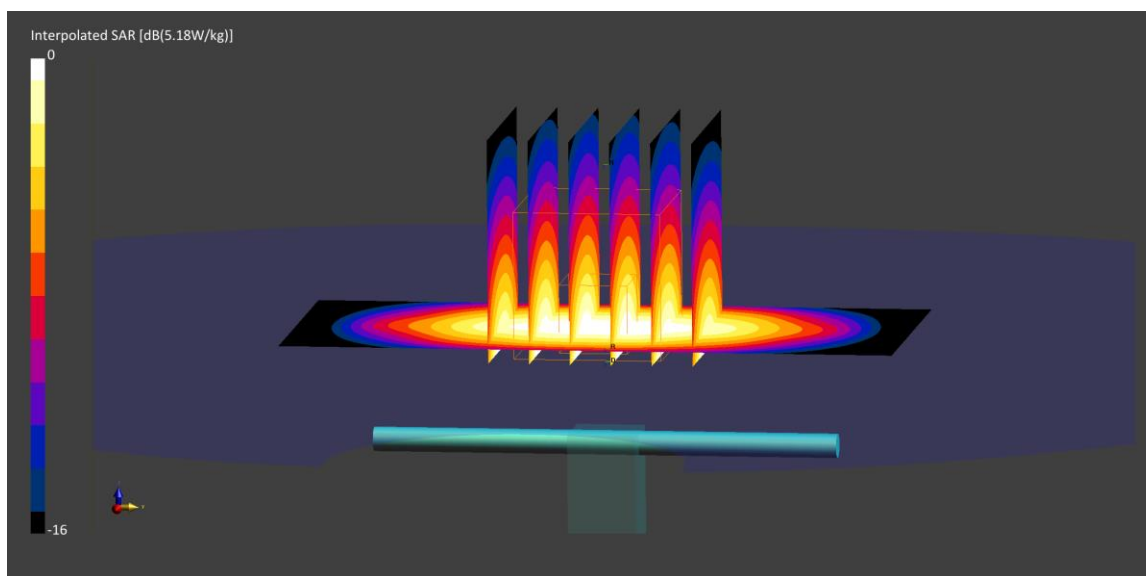

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V2; Serial: 1116

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.69$ S/m; $\epsilon_r = 39.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/20/2021; Ambient Temp: 23.5°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7660; ConvF:(8.66,8.66,8.66); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.7 W/kg

SAR(1 g) = 5.07 W/kg

Deviation (1 g) = 2.22%

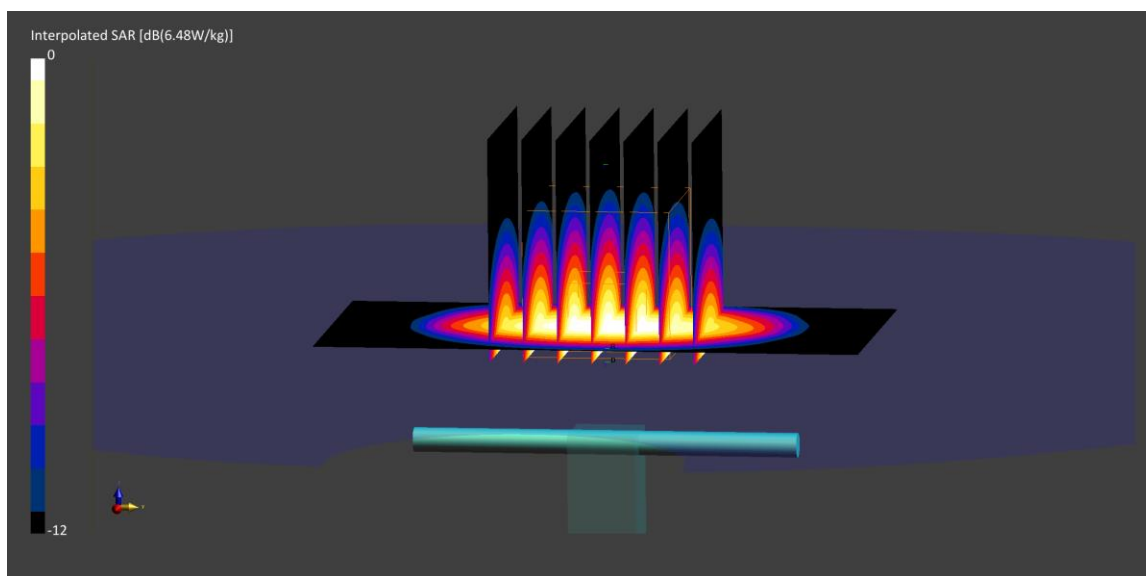

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V2; Serial: 1116

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 39.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/14/2021; Ambient Temp: 22.9°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7660; ConvF:(8.66,8.66,8.66); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.94 W/kg

SAR(1 g) = 4.74 W/kg

Deviation (1 g) = -4.44%

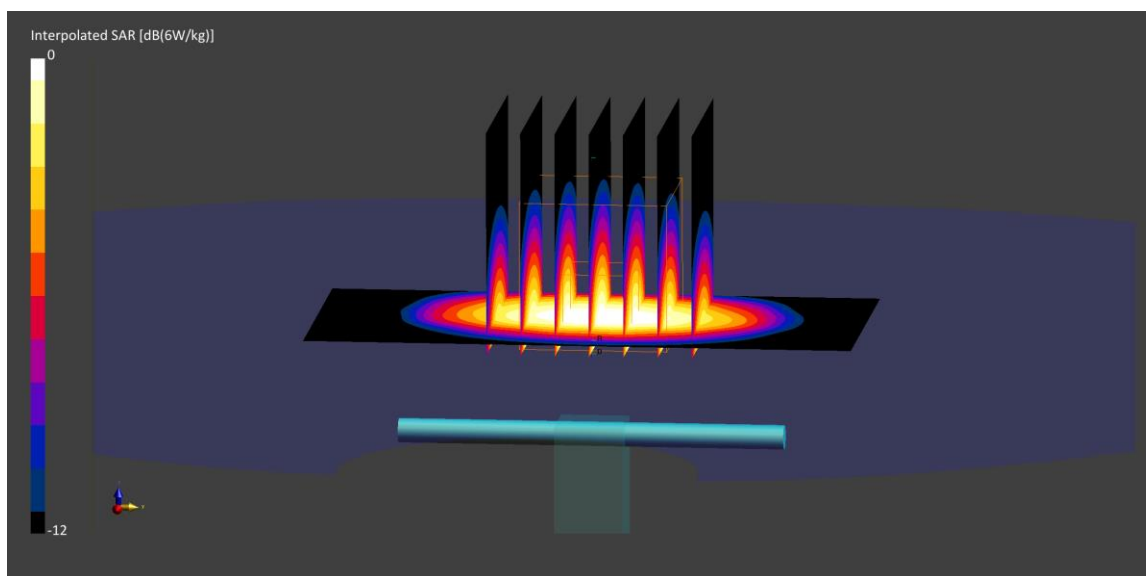

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 1.88$ S/m; $\epsilon_r = 38.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/10/2021; Ambient Temp: 23.4°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7660; ConvF:(8.49,8.49,8.49); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.7 W/kg

SAR(1 g) = 5.08 W/kg

Deviation (1 g) = -3.05%

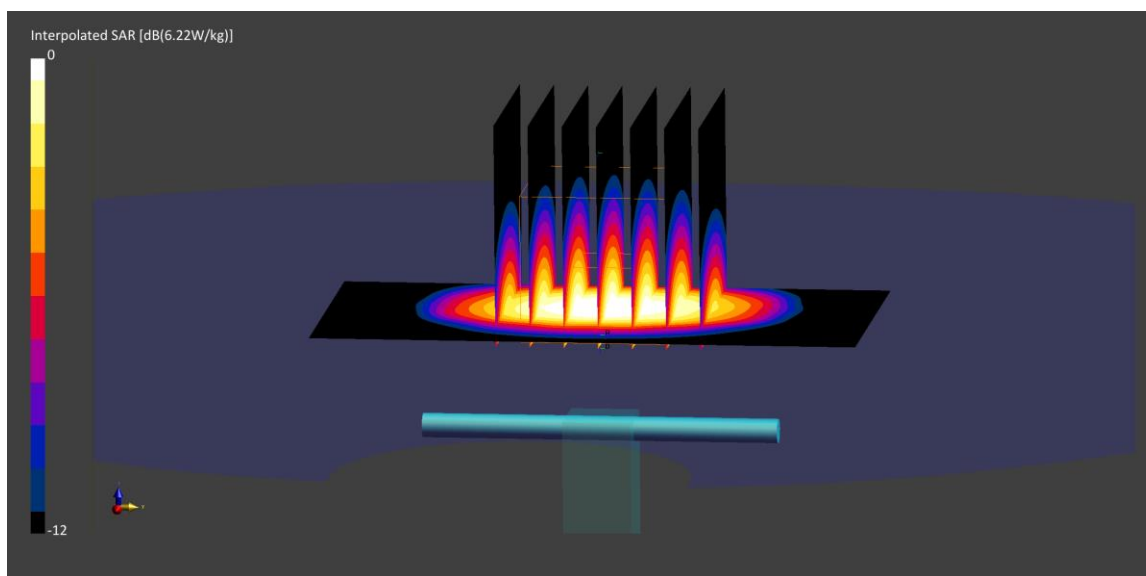

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 39.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/13/2021; Ambient Temp: 24.0°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7660; ConvF:(8.49,8.49,8.49); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.6 W/kg

SAR(1 g) = 4.86 W/kg

Deviation (1 g) = -7.25%

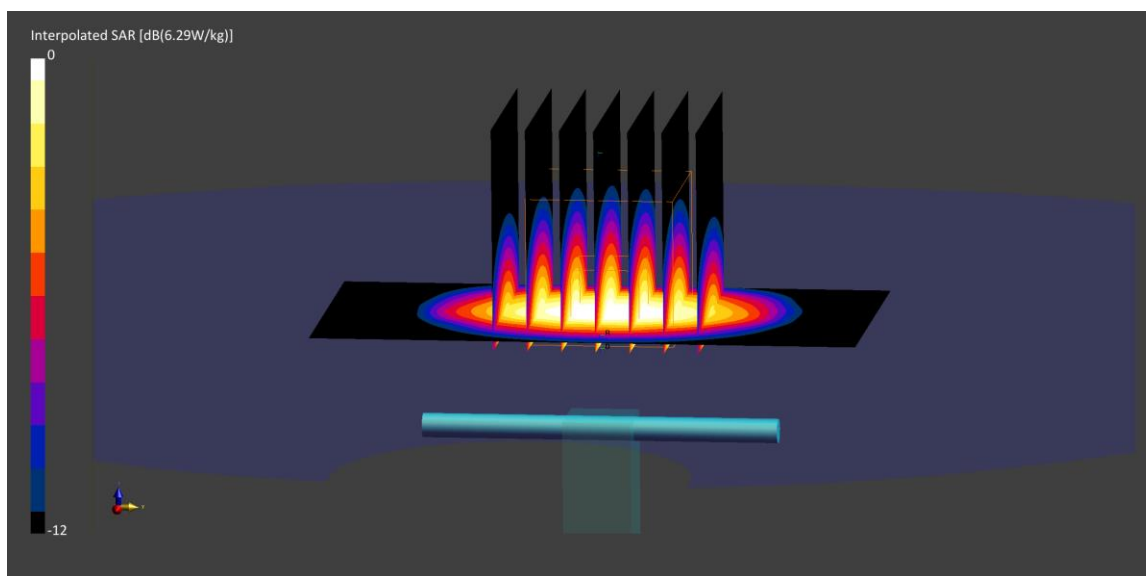

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 882

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 39.2$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/22/2021; Ambient Temp: 22.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7637; ConvF:(8.69,8.69,8.69); Calibrated: 2021-03-03

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1652; Calibrated: 2021-03-01

Phantom: Twin-SAM V8.0 (30); Serial: 1934

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.24 W/kg

Deviation (1 g) = -0.19%

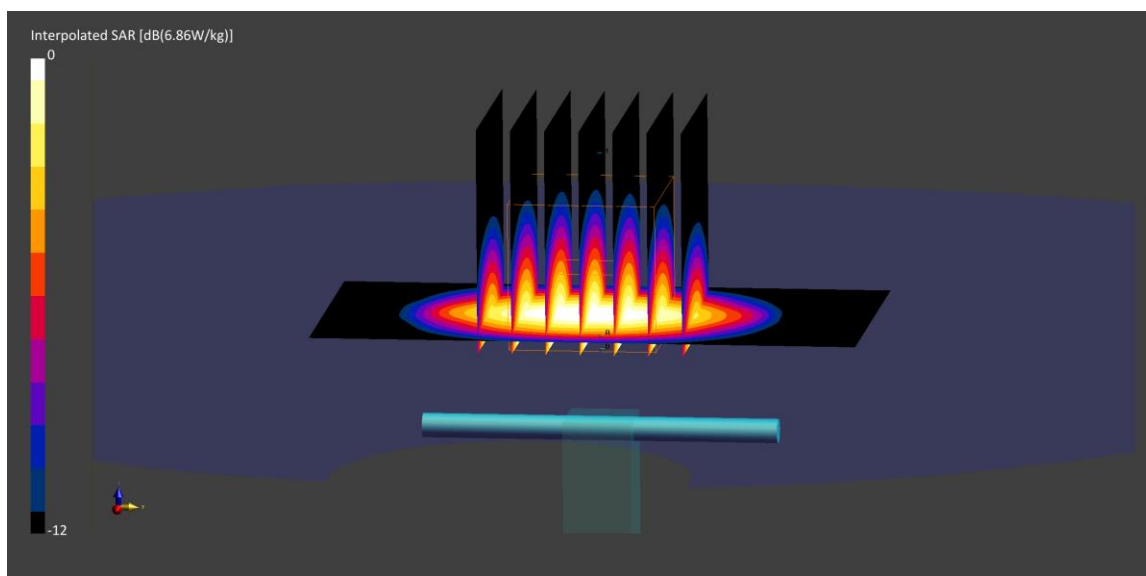

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 945

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 37.9$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/02/2021; Ambient Temp: 21.4°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7402; ConvF:(7.9,7.9,7.9); Calibrated: 2021-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1502; Calibrated: 2021-04-09

Phantom: Twin-SAM V5.0 (30); Serial: 1868

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.4 W/kg

SAR(1 g) = 5.31 W/kg

Deviation (1 g) = 0.76%

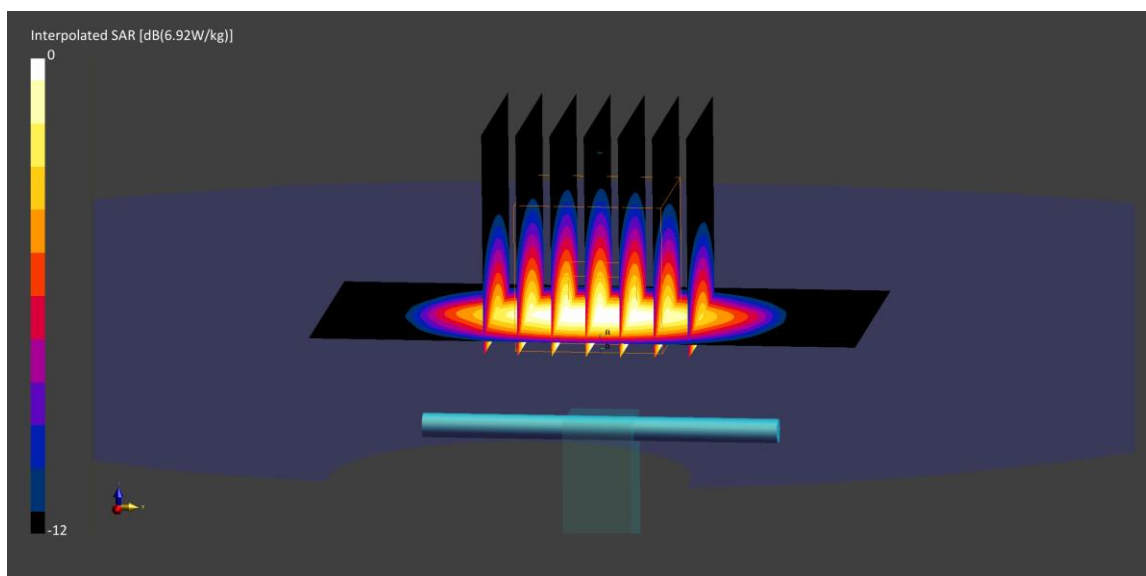

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 38.0$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/10/2021; Ambient Temp: 23.4°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7660; ConvF:(8.26,8.26,8.26); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.4 W/kg

SAR(1 g) = 5.72 W/kg

Deviation (1 g) = -1.55%

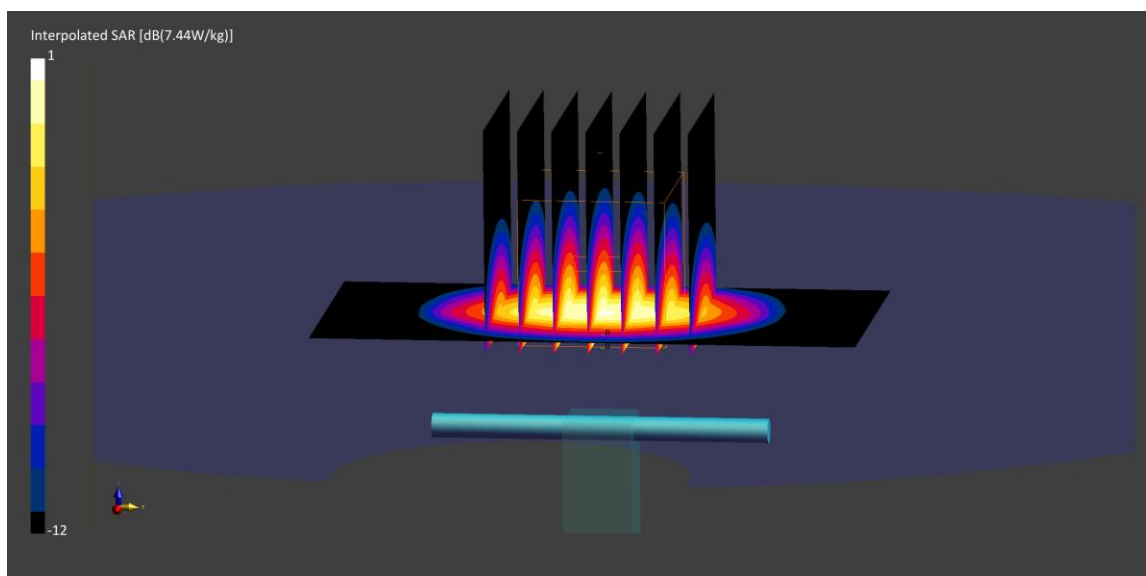

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.02$ S/m; $\epsilon_r = 38.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/13/2021; Ambient Temp: 24.0°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7660; ConvF:(8.26,8.26,8.26); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.3 W/kg

SAR(1 g) = 5.39 W/kg

Deviation (1 g) = -7.23%

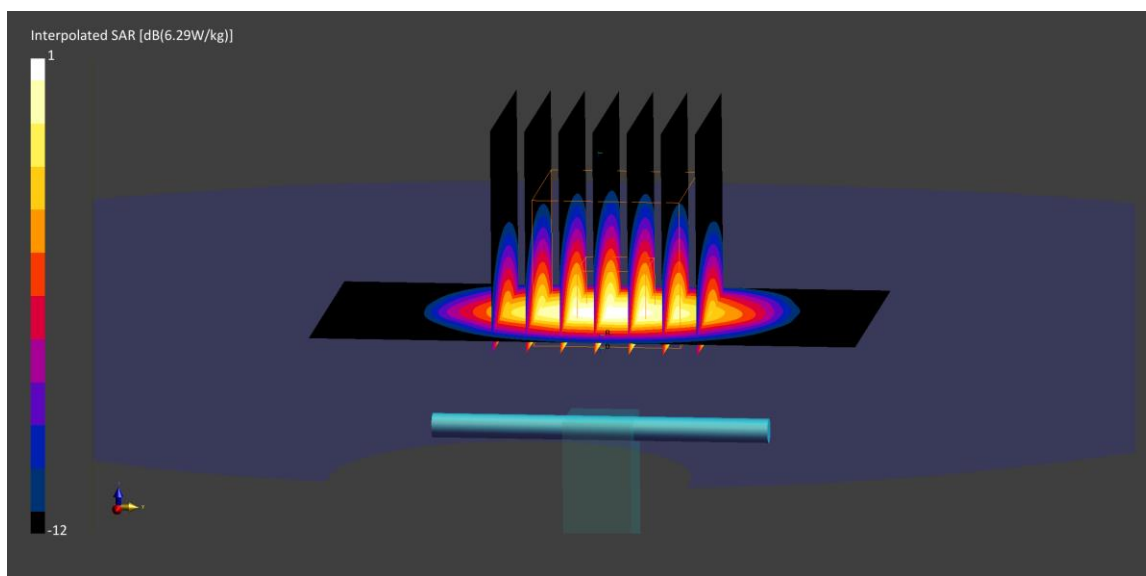

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1071

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 38.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/20/2021; Ambient Temp: 23.5°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7660; ConvF:(8.26,8.26,8.26); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.7 W/kg

SAR(1 g) = 5.55 W/kg

Deviation (1 g) = -1.07%

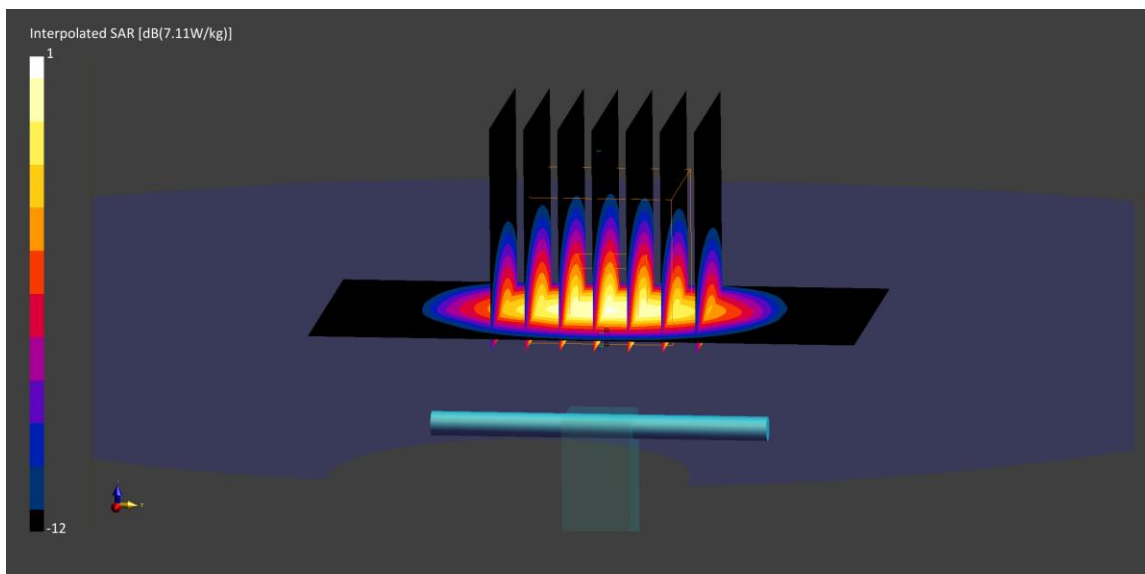

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 38.0$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/31/2021; Ambient Temp: 23.2°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN7571; ConvF:(7.05,7.05,7.05); Calibrated: 2020-12-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1533; Calibrated: 2020-12-07

Phantom: Twin-SAM V5.0; Serial: 1648

Measurement SW: DASY Module SAR V16.0.0.116

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.8 W/kg

SAR(1 g) = 5.91 W/kg

Deviation (1 g) = 2.25%

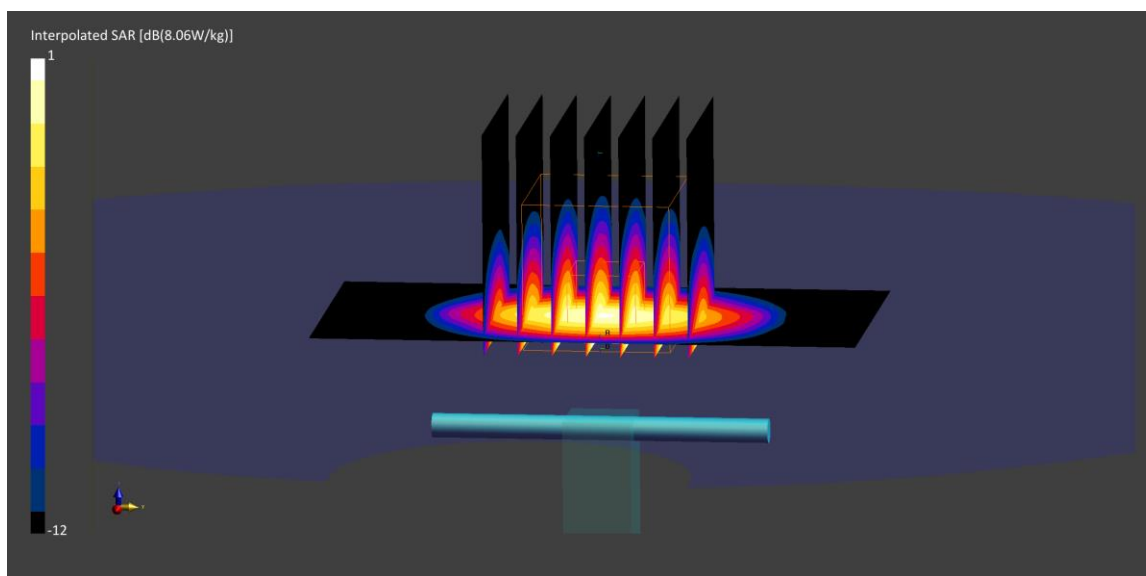

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 39.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 11/14/2021; Ambient Temp: 22.9°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7660; ConvF:(8.26,8.26,8.26); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.2 W/kg

SAR(1 g) = 5.62 W/kg

Deviation (1 g) = -2.77%

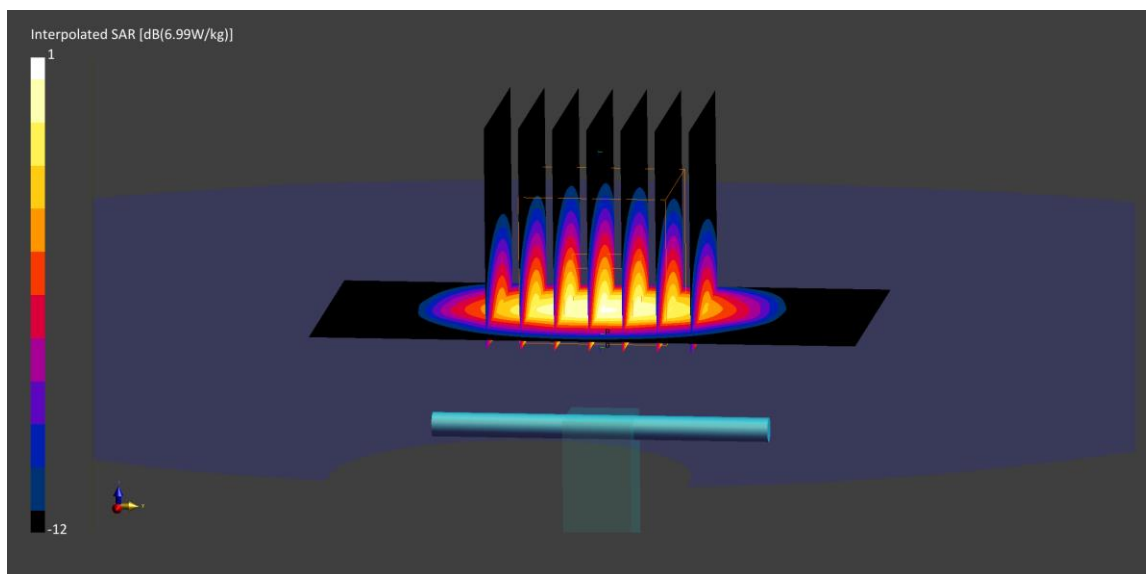

PCTEST

DUT: Dipole 3500.0 MHz; Type: D3500V2; Serial: 1097

Communication System: UID: 0, CW; Frequency: 3500.0 MHz

Medium: 3600 Head; Medium parameters used:

$f = 3500.0$ MHz; $\sigma = 2.79$ S/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/11/2021; Ambient Temp: 20.5°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7539; ConvF:(6.69,6.69,6.69); Calibrated: 2020-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1415; Calibrated: 2021-03-10

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

3500 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 6.73 W/kg

Deviation (1 g) = 1.36%

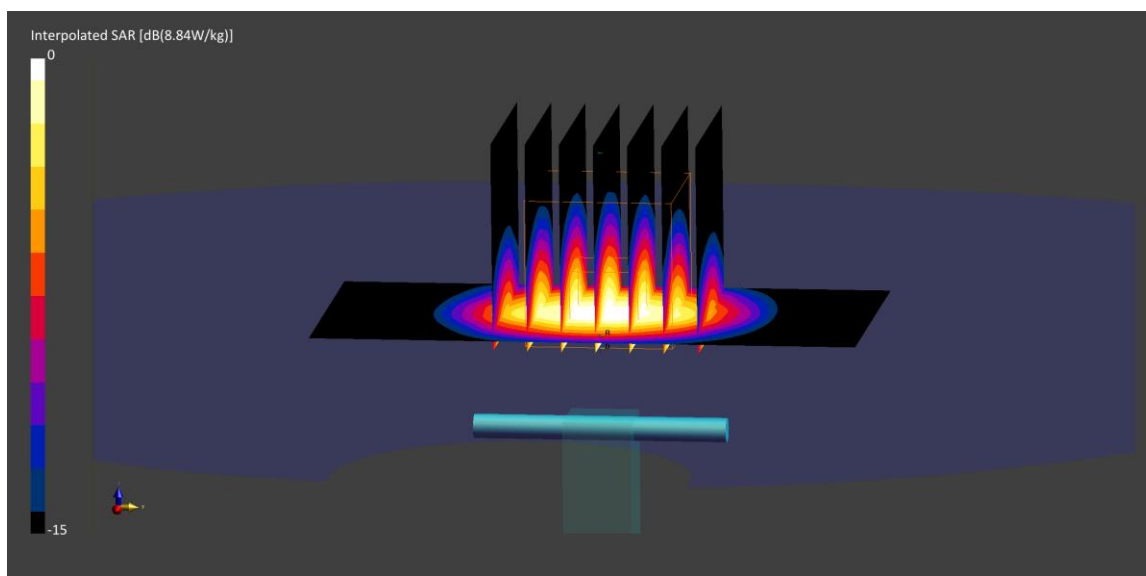

PCTEST

DUT: Dipole 3500.0 MHz; Type: D3500V2; Serial: 1097

Communication System: UID: 0, CW; Frequency: 3500.0 MHz

Medium: 3600 Head; Medium parameters used:

$f = 3500.0$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 39.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/20/2021; Ambient Temp: 22.7°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7670; ConvF:(7.14,7.14,7.14); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

3500 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm

Peak SAR (extrapolated) = 15.9 W/kg

SAR(1 g) = 6.11 W/kg

Deviation (1 g) = -7.98%

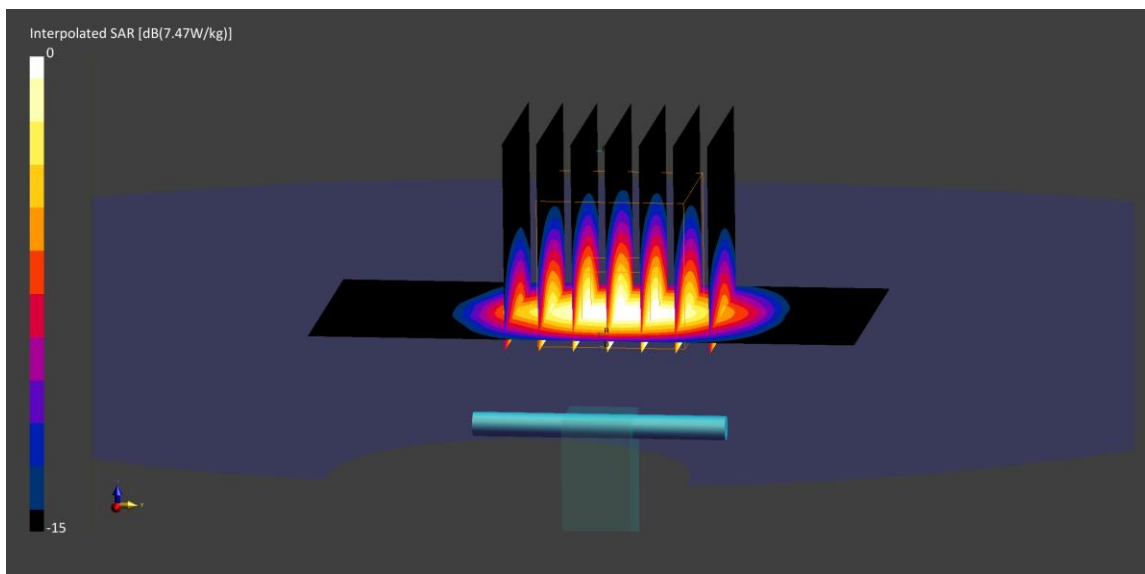

PCTEST

DUT: Dipole 3700.0 MHz; Type: D3700V2; Serial: 1067

Communication System: UID: 0, CW; Frequency: 3700.0 MHz

Medium: 3600 Head; Medium parameters used:

$f = 3700.0$ MHz; $\sigma = 3.00$ S/m; $\epsilon_r = 39.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/20/2021; Ambient Temp: 22.7°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7670; ConvF:(6.93,6.93,6.93); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

3700 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm

Peak SAR (extrapolated) = 17.3 W/kg

SAR(1 g) = 6.51 W/kg

Deviation (1 g) = -3.13%

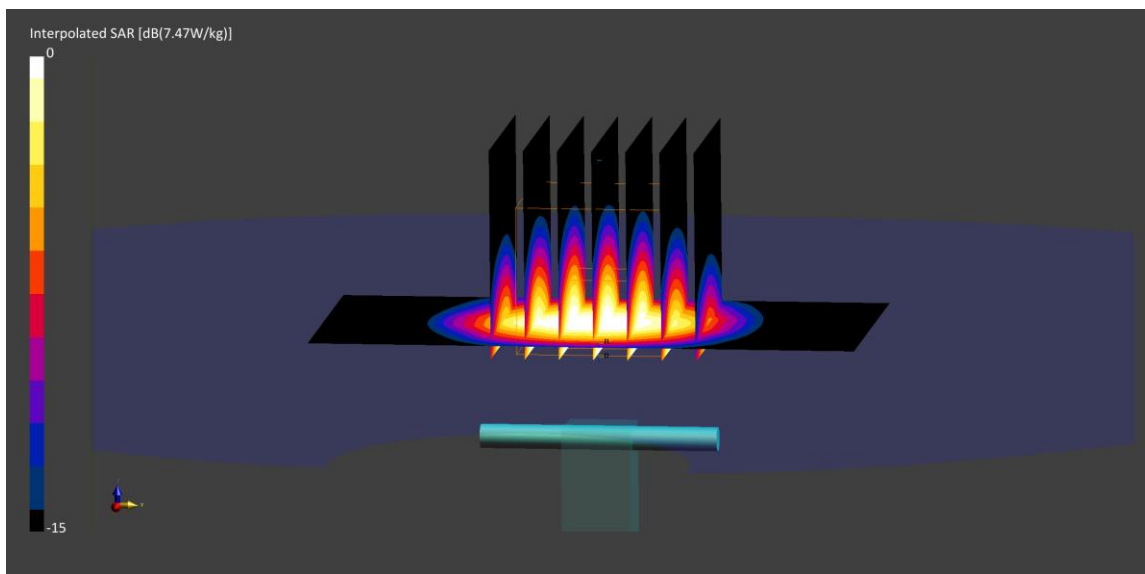

PCTEST

DUT: Dipole 3700.0 MHz; Type: D3700V2; Serial: 1067

Communication System: UID: 0, CW; Frequency: 3700.0 MHz

Medium: 3600 Head; Medium parameters used:

$f = 3700.0$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.9$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/01/2021; Ambient Temp: 21.3°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7670; ConvF:(6.93,6.93,6.93); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

3700 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.7 W/kg

SAR(1 g) = 6.67 W/kg

Deviation (1 g) = -0.74%

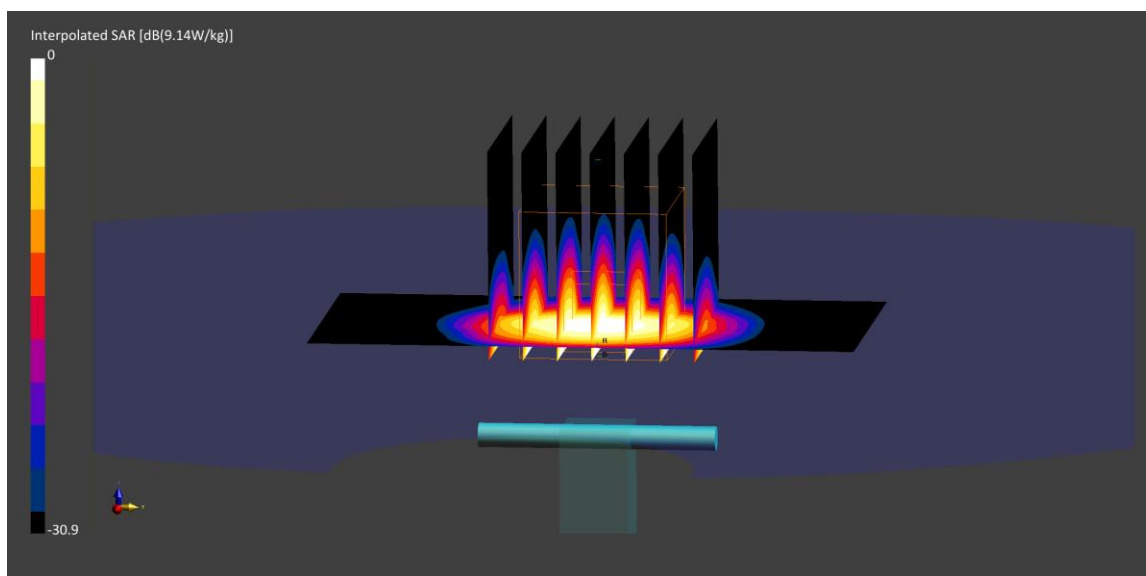

PCTEST

DUT: Dipole 3900.0 MHz; Type: D3900V2; Serial: 1056

Communication System: UID: 0, CW; Frequency: 3900.0 MHz

Medium: 3600 Head; Medium parameters used:

$f = 3900.0$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 38.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/01/2021; Ambient Temp: 21.3°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7670; ConvF:(6.5,6.5,6.5); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

3900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 6.66 W/kg

Deviation (1 g) = -3.34%

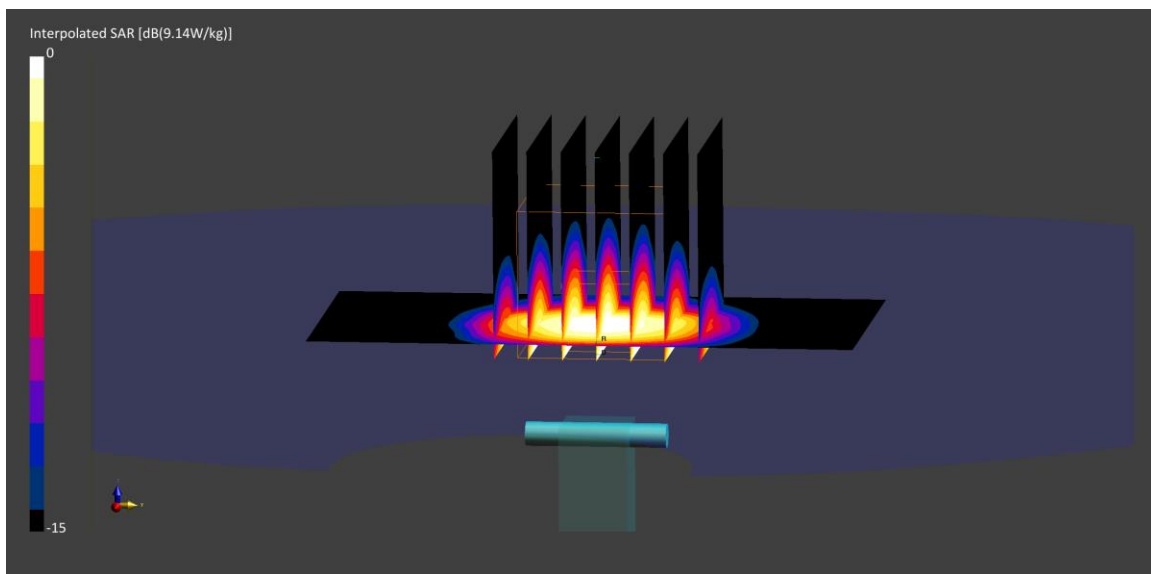

PCTEST

DUT: Dipole 5250.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5250.0$ MHz; $\sigma = 4.71$ S/m; $\epsilon_r = 34.8$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/07/2021; Ambient Temp: 19.5°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7526; ConvF:(5.45,5.45,5.45); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V8.0; Serial: 2063

Measurement SW: DASY Module SAR V16.0.0.116

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.4 W/kg

SAR(1 g) = 3.71 W/kg

Deviation (1 g) = -6.90%

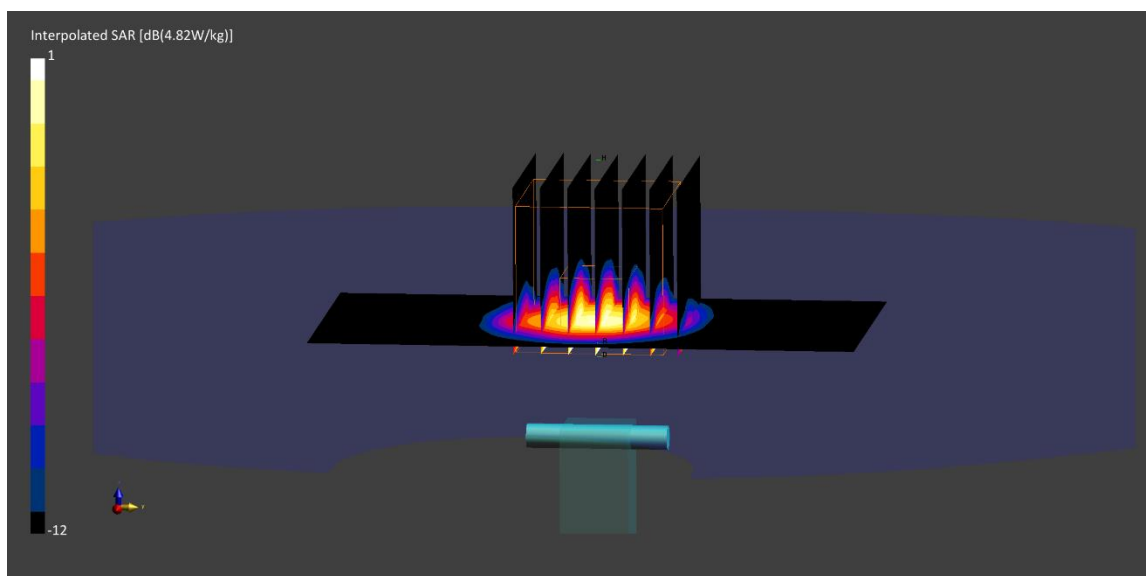

PCTEST

DUT: Dipole 5600.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5600.0$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 34.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/07/2021; Ambient Temp: 19.5°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.92,4.92,4.92); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V8.0; Serial: 2063

Measurement SW: DASY Module SAR V16.0.0.116

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.99 W/kg

Deviation (1 g) = -4.77%

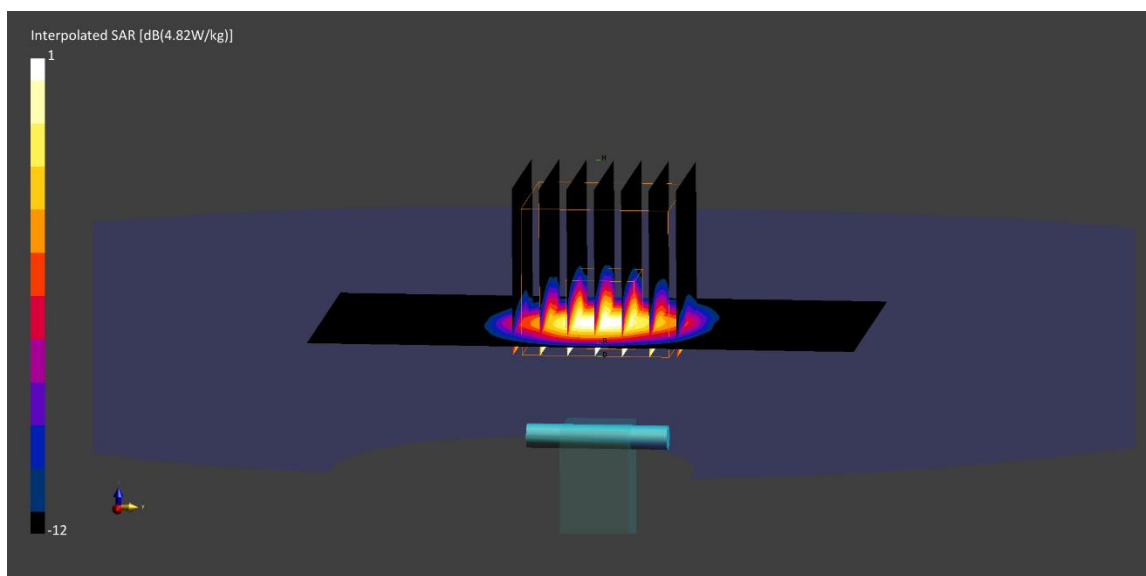

PCTEST

DUT: Dipole 5750.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5750.0$ MHz; $\sigma = 5.30$ S/m; $\epsilon_r = 33.9$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/07/2021; Ambient Temp: 19.5°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7526; ConvF:(5.01,5.01,5.01); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V8.0; Serial: 2063

Measurement SW: DASY Module SAR V16.0.0.116

5750 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 3.76 W/kg

Deviation (1 g) = -6.12%

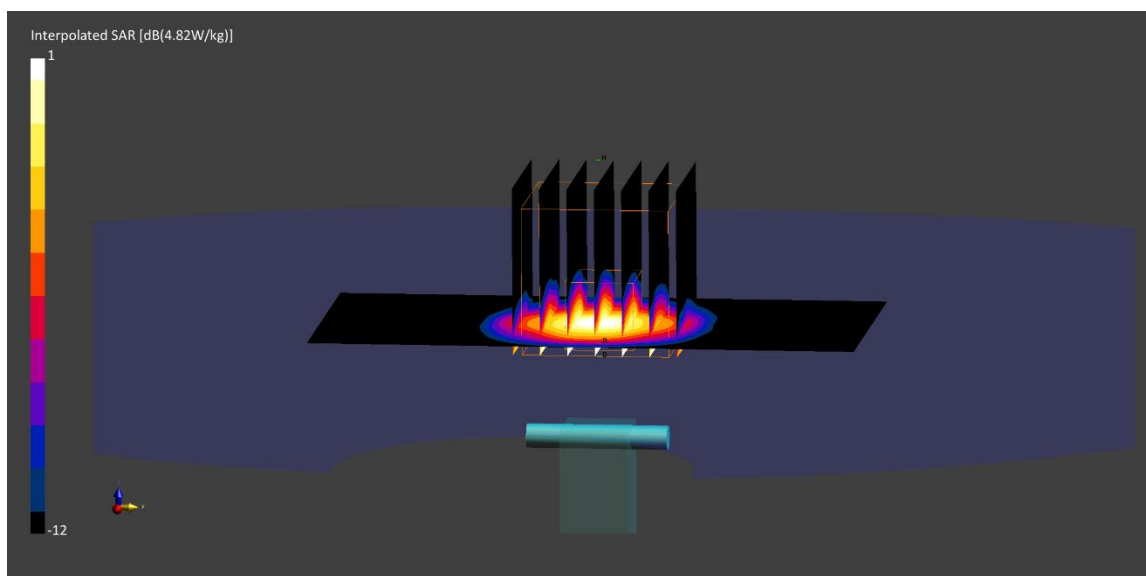

PCTEST

DUT: Dipole 5800.0 MHz; Type: D5GHzV2; Serial: 1191

Communication System: UID: 0, CW; Frequency: 5800.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5800.0$ MHz; $\sigma = 5.39$ S/m; $\epsilon_r = 35.0$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 11/01/2021; Ambient Temp: 22.5°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7552; ConvF:(4.58,4.58,4.58); Calibrated: 2021-09-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

5800 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.7 W/kg

SAR(1 g) = 3.71 W/kg

Deviation (1 g) = -6.31%

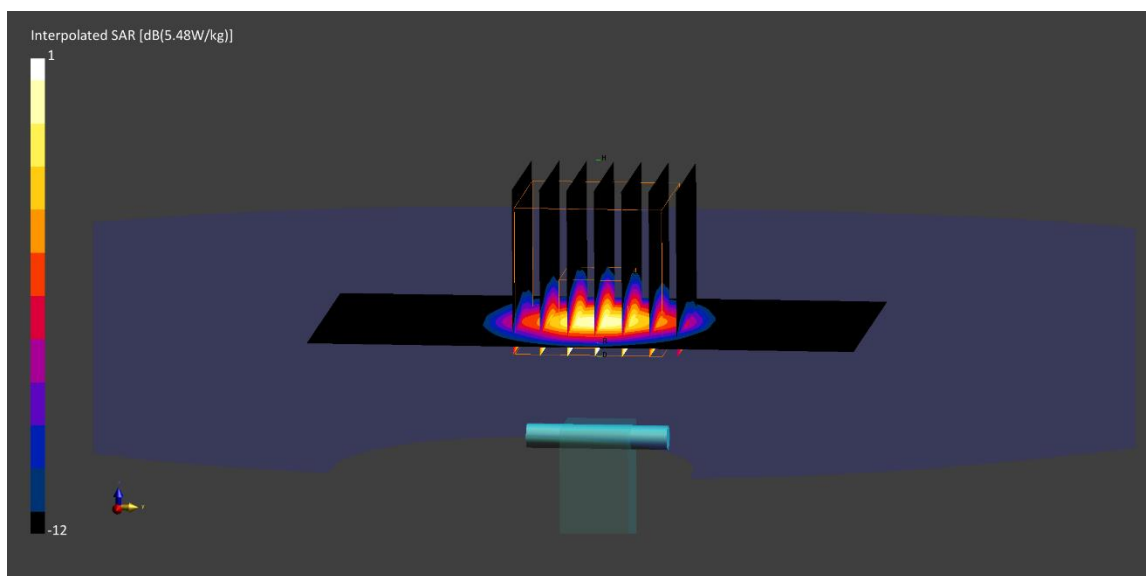

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1046

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used:

$f = 750 \text{ MHz}$; $\sigma = 0.977 \text{ S/m}$; $\epsilon_r = 54.347$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/11/2021; Ambient Temp: 20.5°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7565; ConvF(9.77, 9.77, 9.77) @ 750 MHz; Calibrated: 11/12/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1466; Calibrated: 11/6/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1626

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.55 W/kg

SAR(1 g) = 1.71 W/kg

Deviation(1 g) = -2.73%

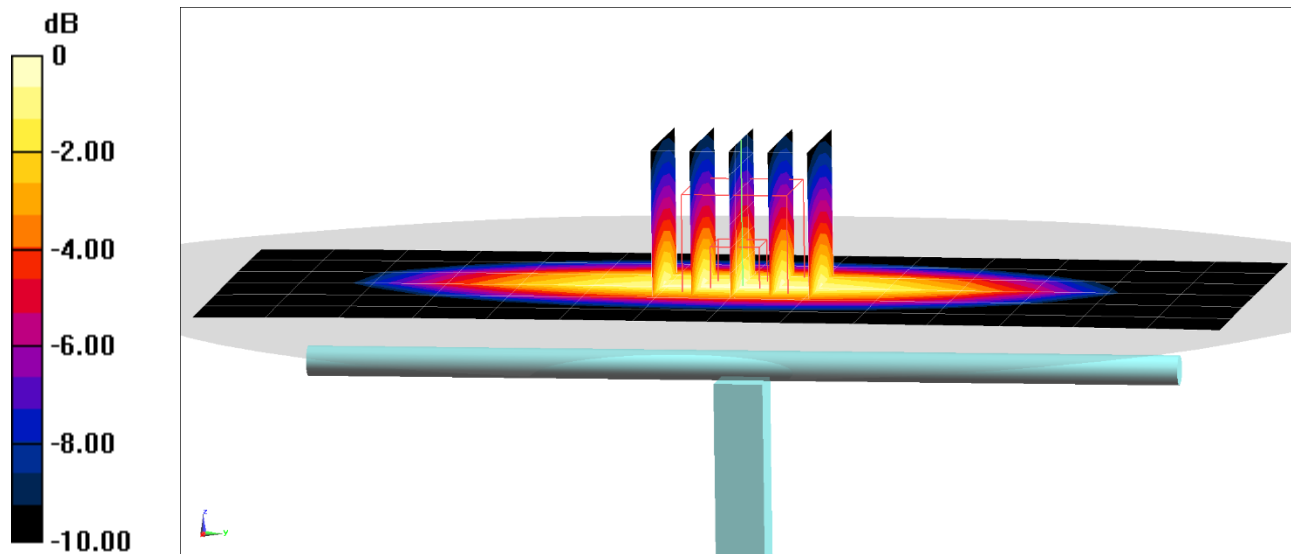

0 dB = 2.27 W/kg = 3.56 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1046

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used:

$f = 750 \text{ MHz}$; $\sigma = 0.977 \text{ S/m}$; $\epsilon_r = 53.794$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/13/2021; Ambient Temp: 20.9°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7565; ConvF(9.77, 9.77, 9.77) @ 750 MHz; Calibrated: 11/12/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1466; Calibrated: 11/6/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1626

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.61 W/kg

SAR(1 g) = 1.74 W/kg

Deviation(1 g) = -1.02%

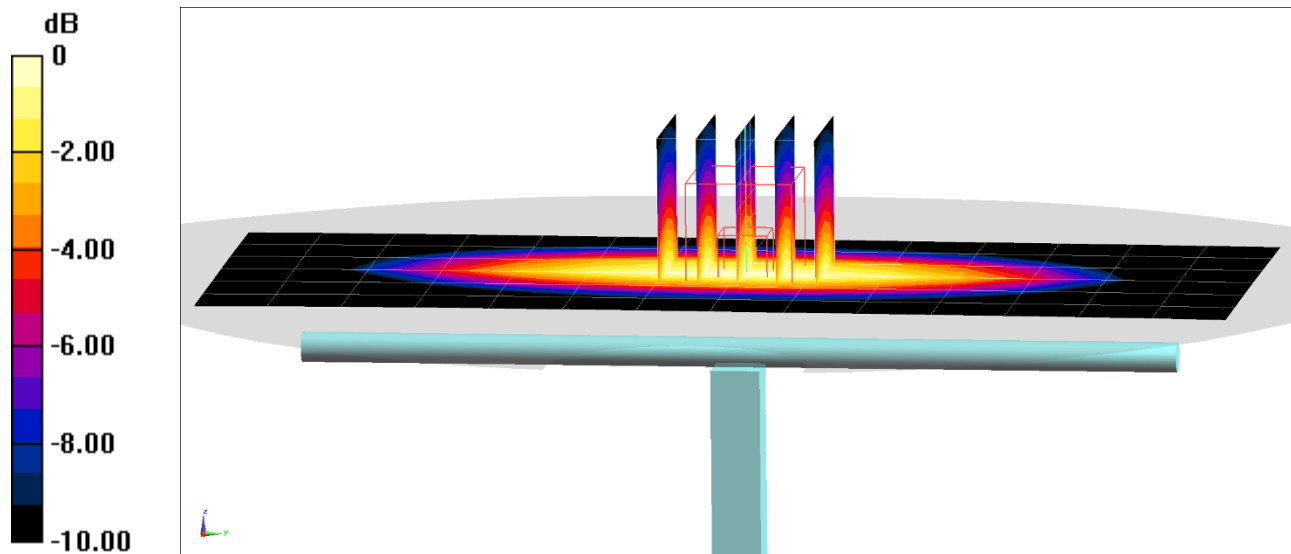

0 dB = 2.32 W/kg = 3.65 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1161

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used:

$f = 750 \text{ MHz}$; $\sigma = 0.973 \text{ S/m}$; $\epsilon_r = 53.309$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/14/2021; Ambient Temp: 21.2°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7409; ConvF(9.96, 9.96, 9.96) @ 750 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.72 W/kg

SAR(1 g) = 1.77 W/kg

Deviation(1 g) = 4.98%

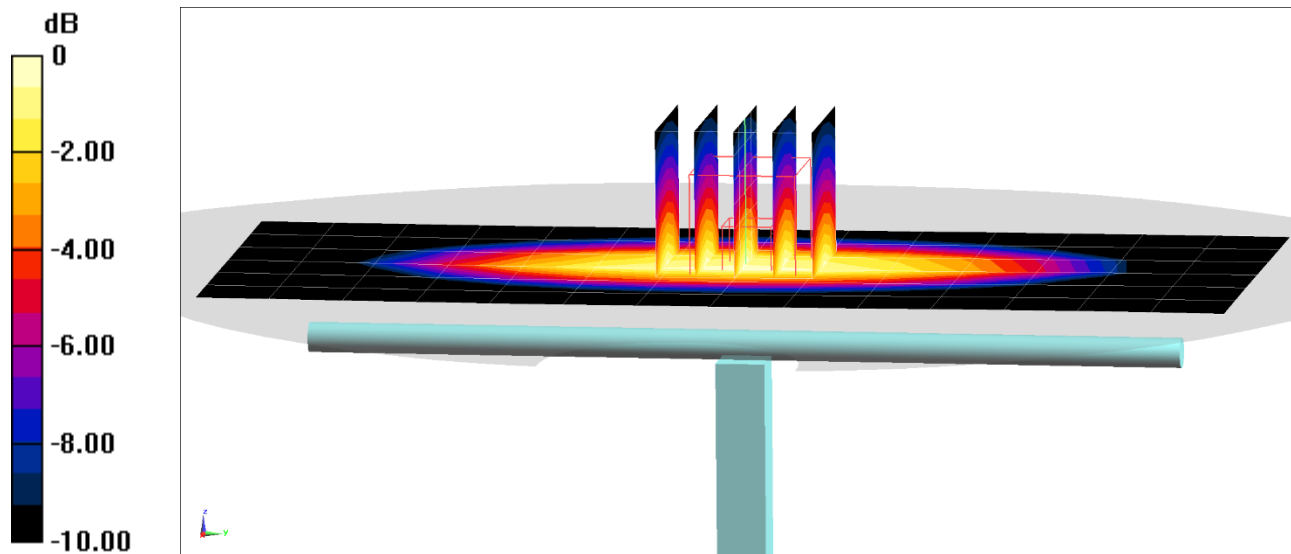

0 dB = 2.39 W/kg = 3.78 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d119

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 1.015 \text{ S/m}$; $\epsilon_r = 54.779$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/27/2021; Ambient Temp: 20.5°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7565; ConvF(9.53, 9.53, 9.53) @ 835 MHz; Calibrated: 11/12/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1466; Calibrated: 11/6/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1626

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 3.12 W/kg

SAR(1 g) = 2.08 W/kg

Deviation(1 g) = 5.05%

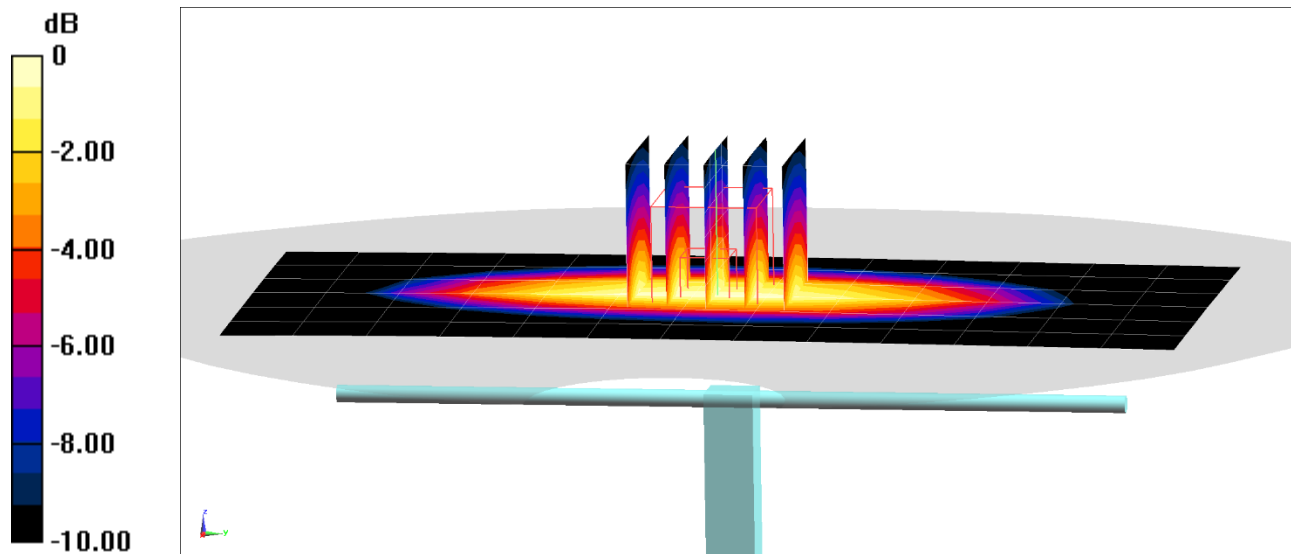

0 dB = 2.78 W/kg = 4.44 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d180

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 1.011 \text{ S/m}$; $\epsilon_r = 52.832$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/29/2021; Ambient Temp: 21.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7402; ConvF(10.04, 10.04, 10.04) @ 835 MHz; Calibrated: 04/16/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 04/09/2021

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 2.99 W/kg

SAR(1 g) = 2.01 W/kg

Deviation(1 g) = 3.93%

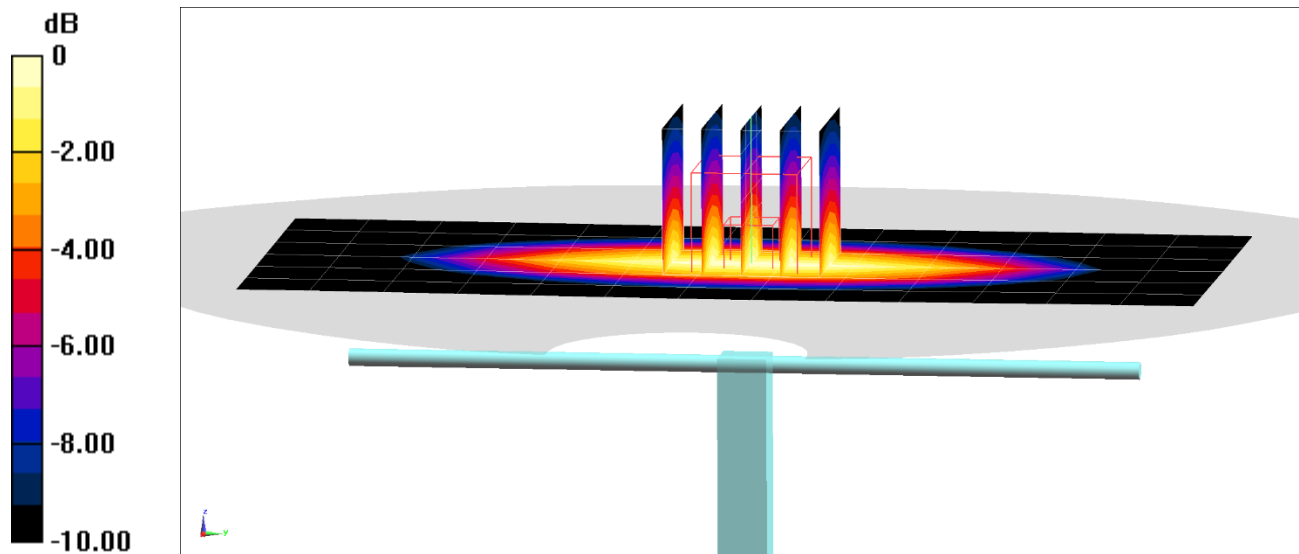

0 dB = 2.67 W/kg = 4.27 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d132

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.953 \text{ S/m}$; $\epsilon_r = 54.827$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/05/2021; Ambient Temp: 21.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7409; ConvF(9.66, 9.66, 9.66) @ 835 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 3.11 W/kg

SAR(1 g) = 2.02 W/kg

Deviation(1 g) = 2.96%

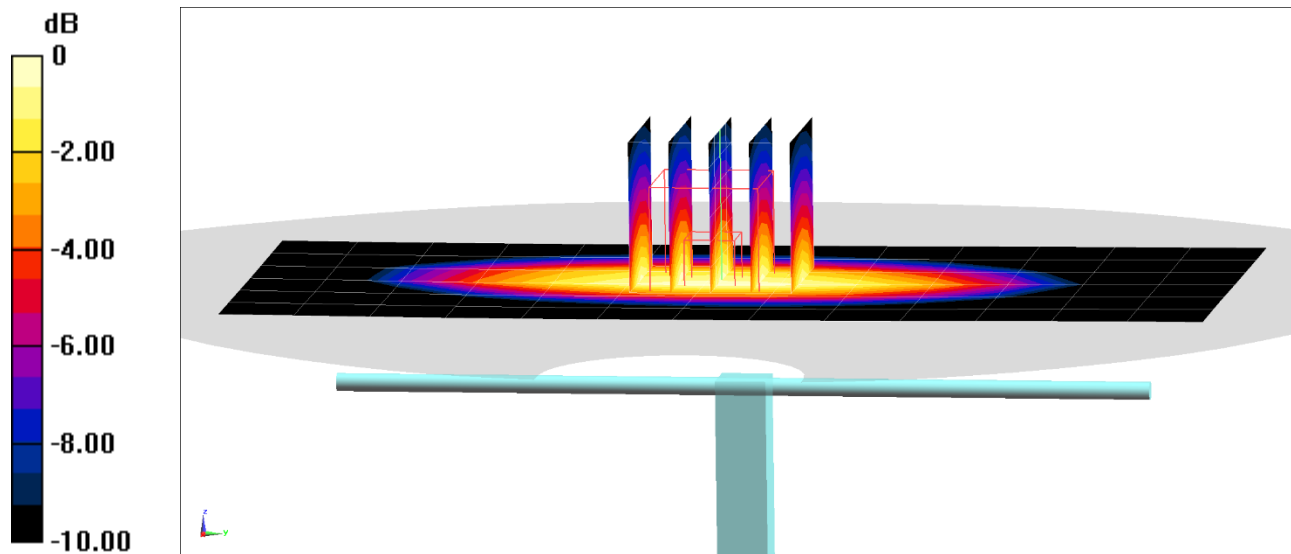

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d132

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.953 \text{ S/m}$; $\epsilon_r = 54.235$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/07/2021; Ambient Temp: 21.1°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7409; ConvF(9.66, 9.66, 9.66) @ 835 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 3.05 W/kg

SAR(1 g) = 2 W/kg

Deviation(1 g) = 1.94%

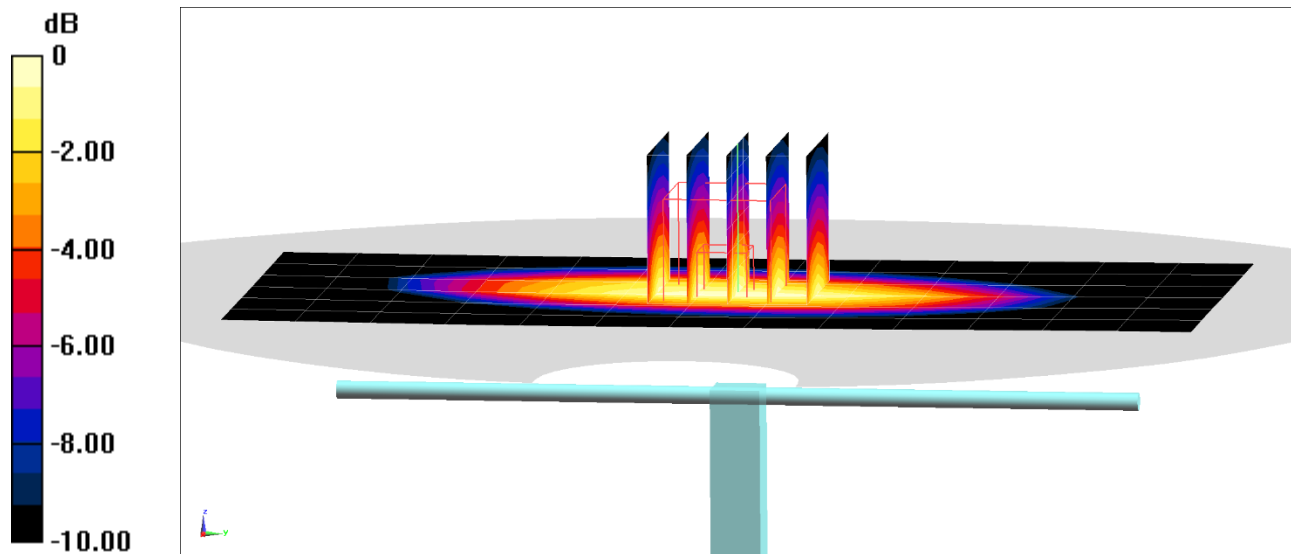

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1150

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.465 \text{ S/m}$; $\epsilon_r = 52.496$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/19/2021; Ambient Temp: 24.2°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.17 W/kg

SAR(1 g) = 3.93 W/kg; SAR(10 g) = 2.09 W/kg

Deviation(1 g) = 7.38%; Deviation(10 g) = 7.73%

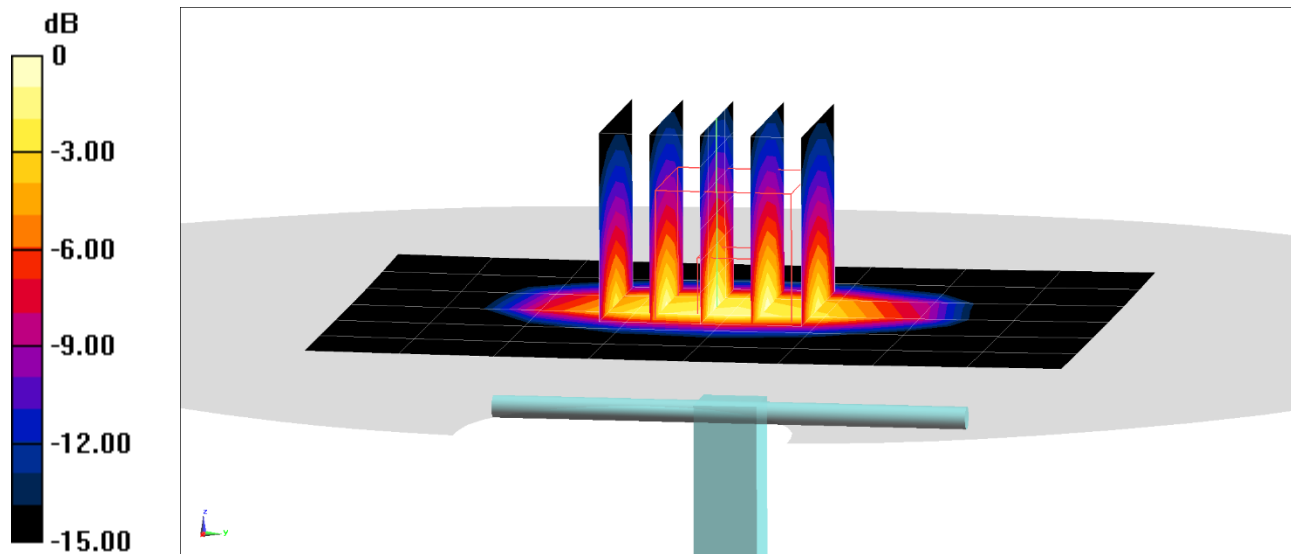

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1148

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.501 \text{ S/m}$; $\epsilon_r = 51.79$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2021; Ambient Temp: 23.0°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.09 W/kg

SAR(1 g) = 3.89 W/kg

Deviation(1 g) = 7.16%

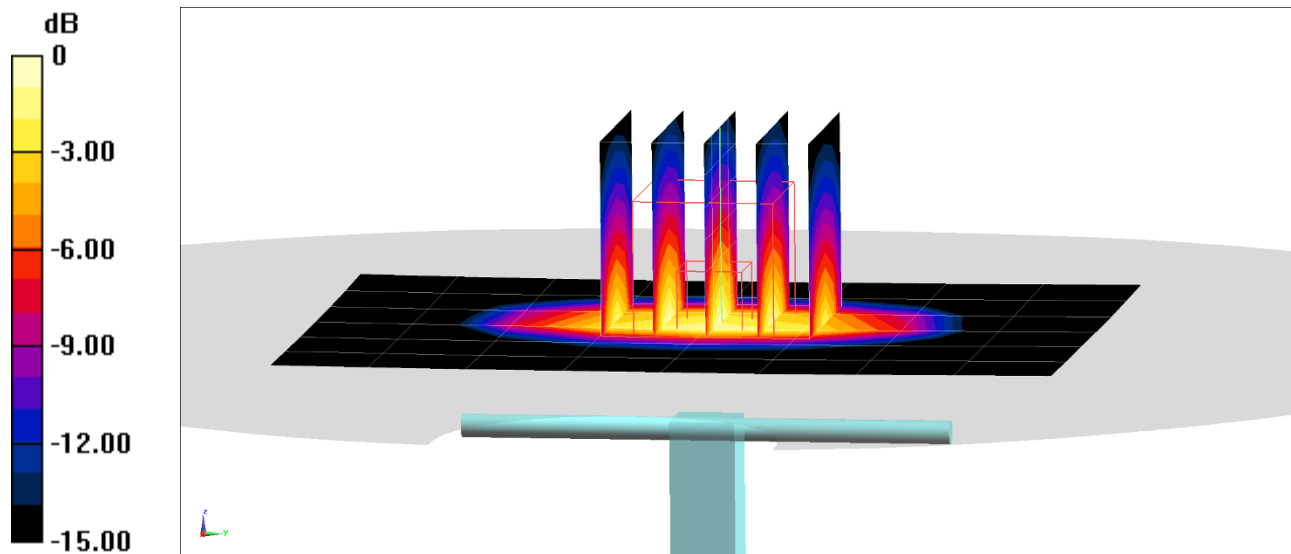

0 dB = 5.98 W/kg = 7.77 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1150

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.499 \text{ S/m}$; $\epsilon_r = 52.735$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2021; Ambient Temp: 24.6°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 6.93 W/kg

SAR(10 g) = 2.05 W/kg

Deviation(10 g) = 5.67%

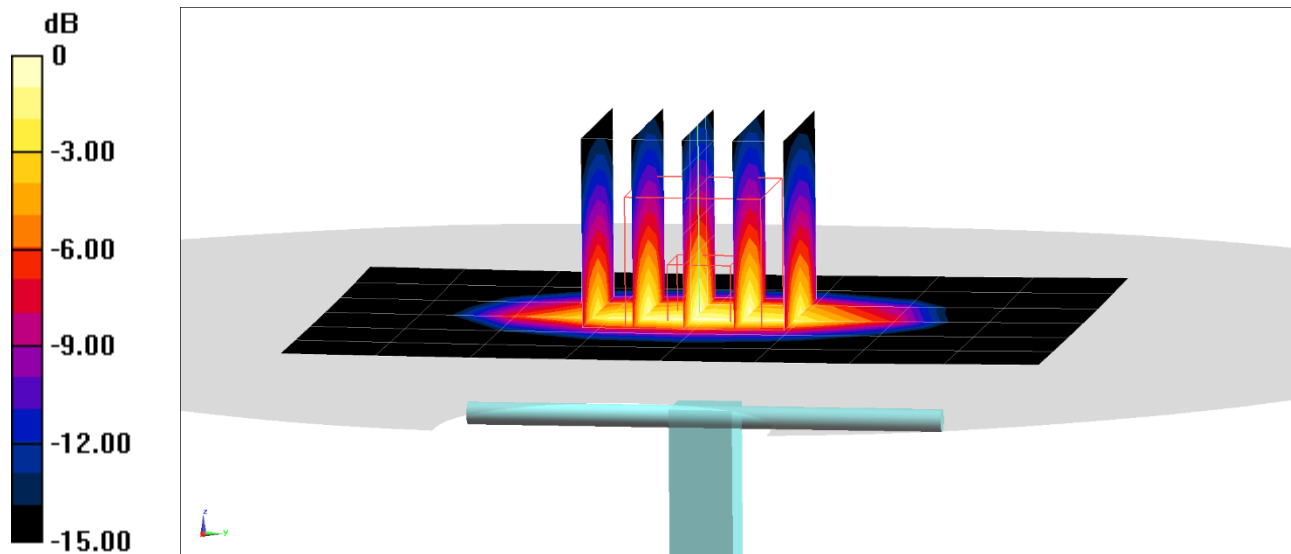

0 dB = 5.84 W/kg = 7.66 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1150

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.499 \text{ S/m}$; $\epsilon_r = 52.026$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2021; Ambient Temp: 24.2°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.08 W/kg

SAR(1 g) = 3.94 W/kg

Deviation(1 g) = 7.65%

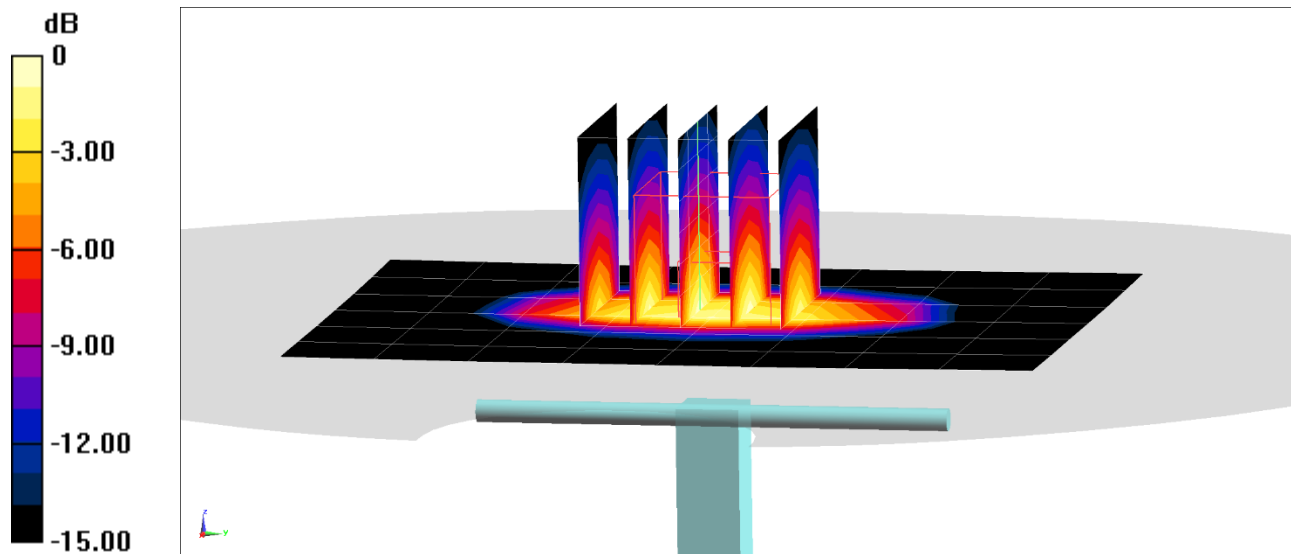

0 dB = 5.98 W/kg = 7.77 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1150

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.507 \text{ S/m}$; $\epsilon_r = 52.289$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/03/2021; Ambient Temp: 22.2°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.24 W/kg

SAR(10 g) = 2.09 W/kg

Deviation(10 g) = 7.73%

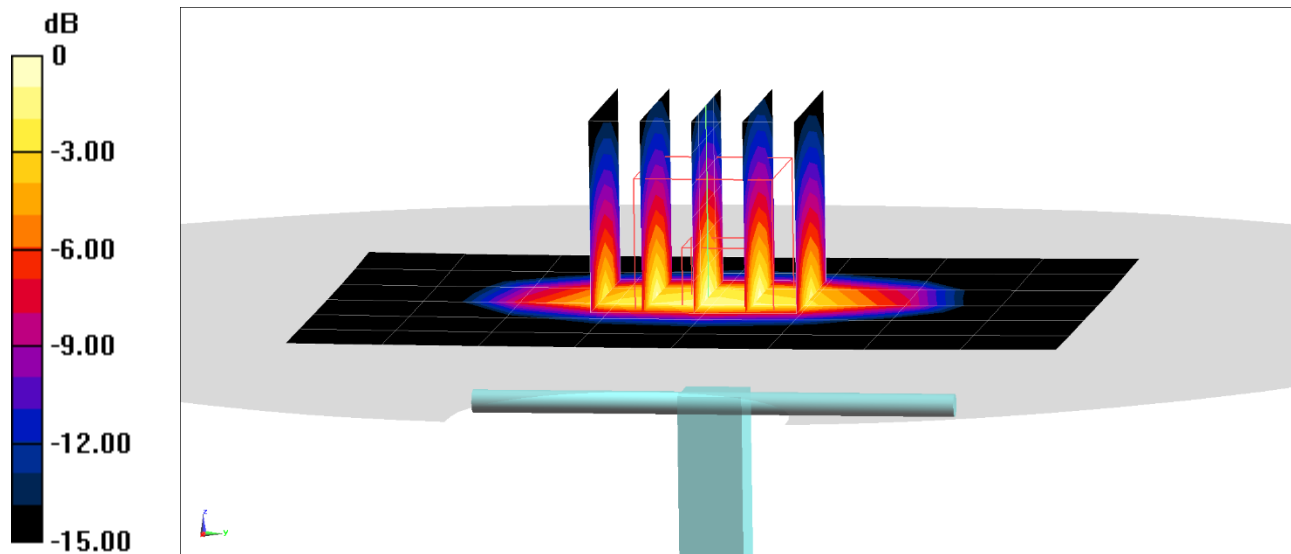

0 dB = 6.10 W/kg = 7.85 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1148

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.496 \text{ S/m}$; $\epsilon_r = 54.264$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/28/2021; Ambient Temp: 22.8°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7357; ConvF(8.12, 8.12, 8.12) @ 1750 MHz; Calibrated: 4/19/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1407; Calibrated: 4/7/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 6.88 W/kg

SAR(1 g) = 3.85 W/kg

Deviation(1 g) = 6.06%

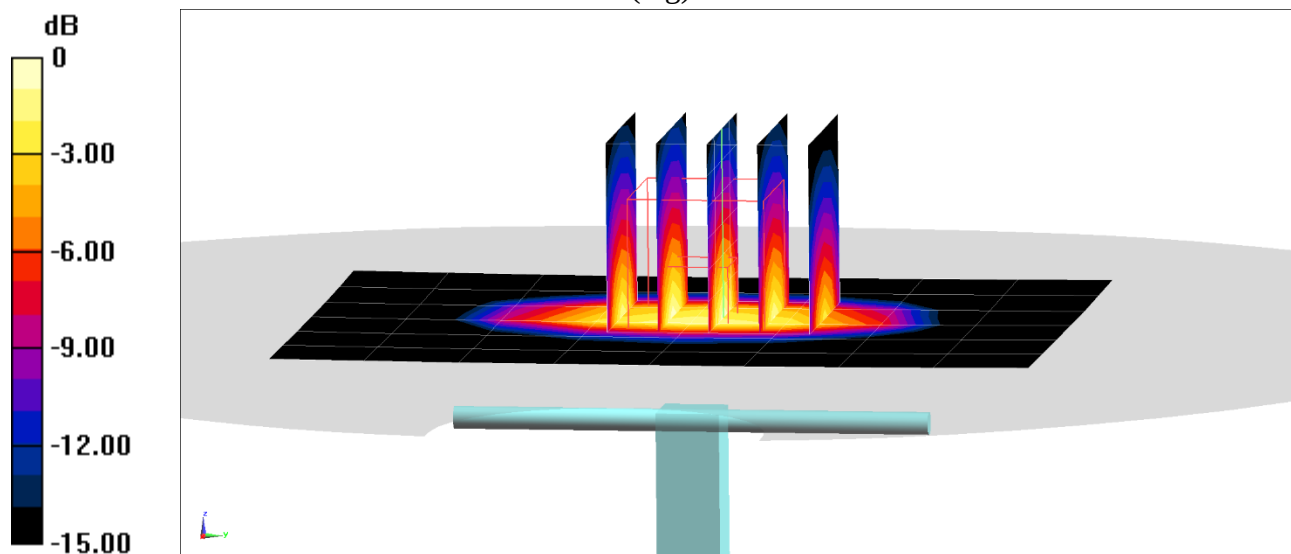

0 dB = 5.80 W/kg = 7.63 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d080

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1900 \text{ MHz}$; $\sigma = 1.505 \text{ S/m}$; $\epsilon_r = 51.276$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/26/2021; Ambient Temp: 23.0°C; Tissue Temp: 25.0°C

Probe: EX3DV4 - SN7409; ConvF(7.68, 7.68, 7.68) @ 1900 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.95 W/kg

SAR(1 g) = 4.13 W/kg; SAR(10 g) = 2.13 W/kg

Deviation(1 g) = 5.36%; Deviation(10 g) = 3.40%

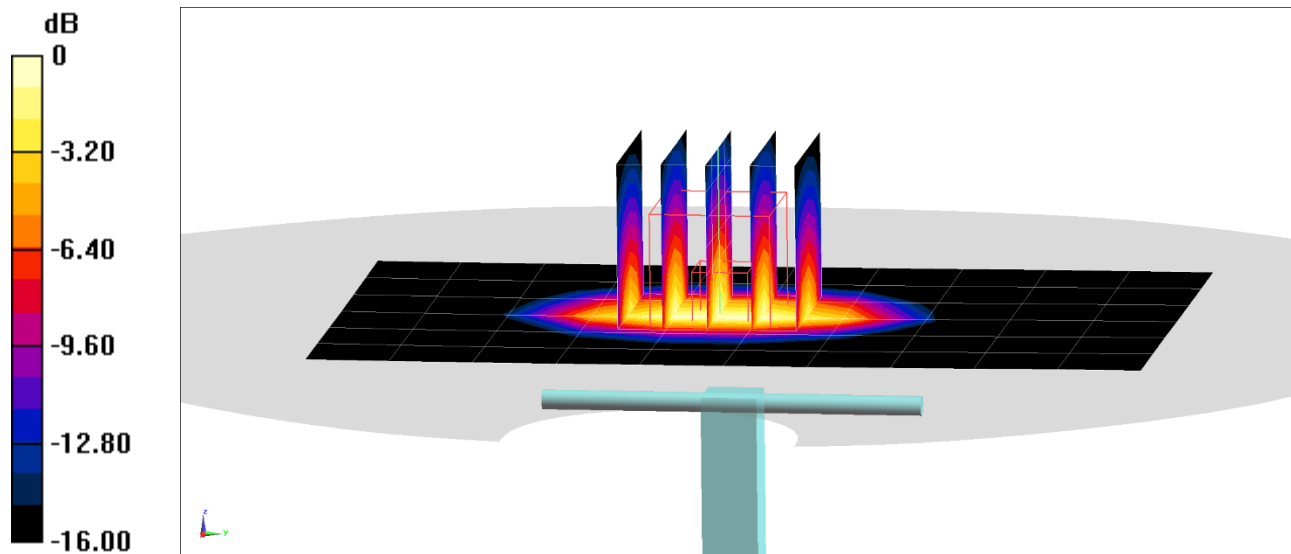

0 dB = 6.57 W/kg = 8.18 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d080

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body; Medium parameters used:

$f = 1900 \text{ MHz}$; $\sigma = 1.561 \text{ S/m}$; $\epsilon_r = 50.748$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2021; Ambient Temp: 23.5°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7409; ConvF(7.68, 7.68, 7.68) @ 1900 MHz; Calibrated: 6/21/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/15/2021

Phantom: Twin-SAM V5.0 Front (20); Type: QD 000 P40 CD; Serial: 1759

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.93 W/kg

SAR(1 g) = 4.1 W/kg

Deviation(1 g) = 4.59%

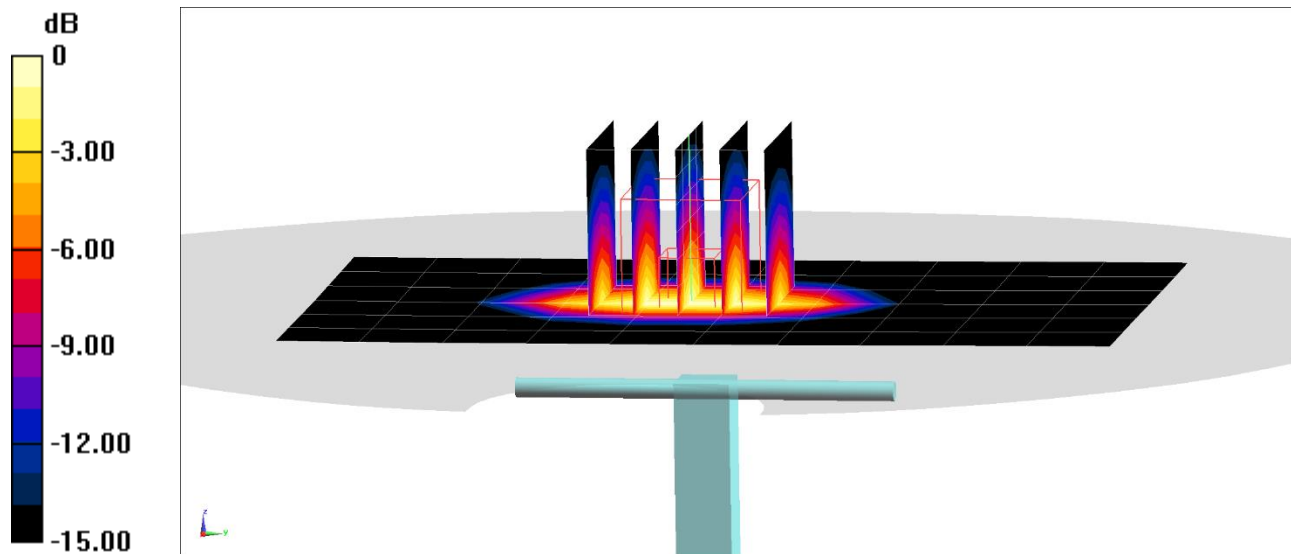

0 dB = 6.56 W/kg = 8.17 dBW/kg

PCTEST

DUT: Dipole 1900.0 MHz; Type: D1900V2; Serial: 5d148

Communication System: UID: 0, CW; Frequency: 1900.0 MHz

Medium: 1900 Body; Medium parameters used:

$f = 1900.0$ MHz; $\sigma = 1.53$ S/m; $\epsilon_r = 51.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/12/2021; Ambient Temp: 21.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7659; ConvF:(9.07,9.07,9.07); Calibrated: 2021-06-29

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1678; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.0.65

1900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.71 W/kg

SAR(10 g) = 2.09 W/kg

Deviation (10 g) = 1.95%

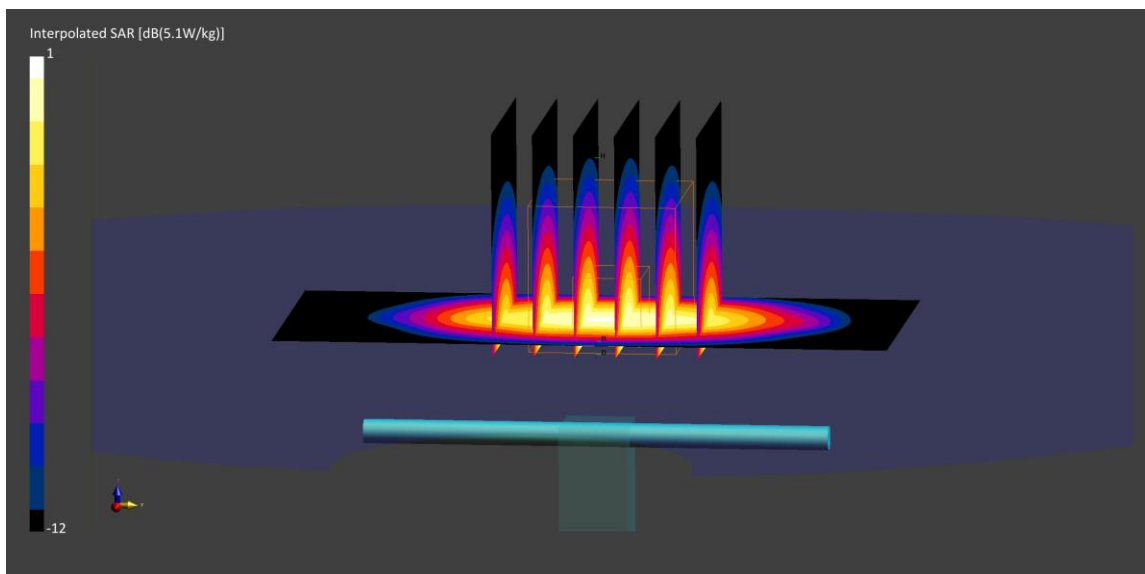

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d148

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used

$f = 1900 \text{ MHz}$; $\sigma = 1.569 \text{ S/m}$; $\epsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/17/2021; Ambient Temp: 20.9°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7410; ConvF(7.7, 7.7, 7.7) @ 1900 MHz; Calibrated: 7/20/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 7/13/2021

Phantom: Twin-SAM V5.0 (Front); Type: QD 000 P40 CD; Serial: 1792

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.76 W/kg

SAR(10 g) = 2.09 W/kg

Deviation(10 g) = 1.95%

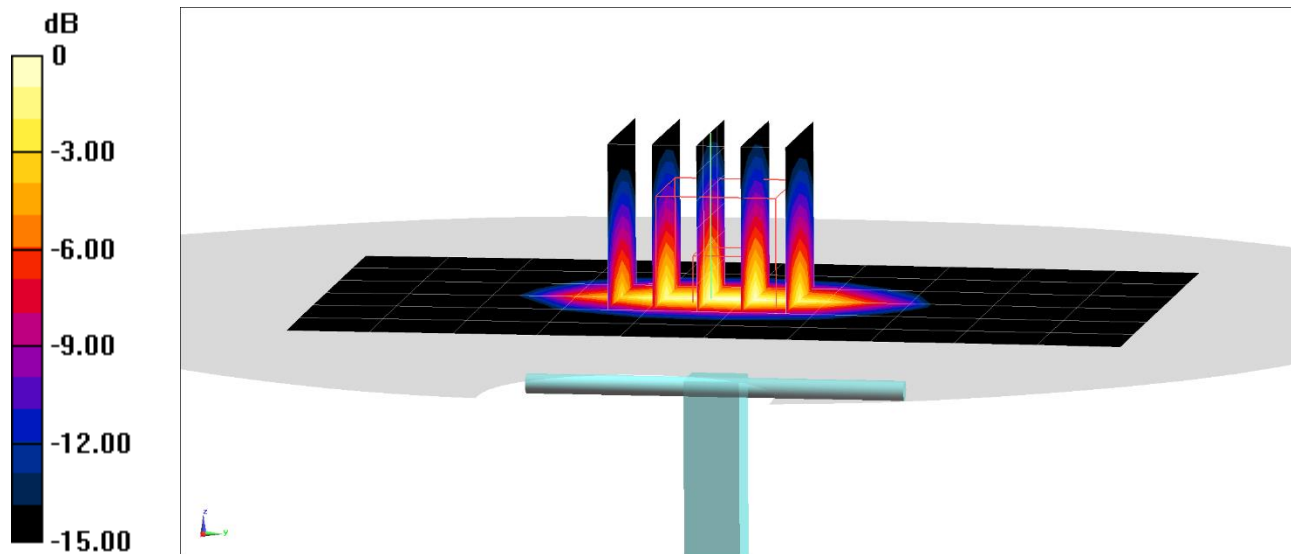

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d148

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1900 \text{ MHz}$; $\sigma = 1.576 \text{ S/m}$; $\epsilon_r = 51.048$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/24/2021; Ambient Temp: 23.7°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7410; ConvF(7.7, 7.7, 7.7) @ 1900 MHz; Calibrated: 7/20/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 7/13/2021

Phantom: Twin-SAM V5.0 (Front); Type: QD 000 P40 CD; Serial: 1792

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.67 W/kg

SAR(1 g) = 4.17 W/kg

Deviation(1 g) = 6.65%

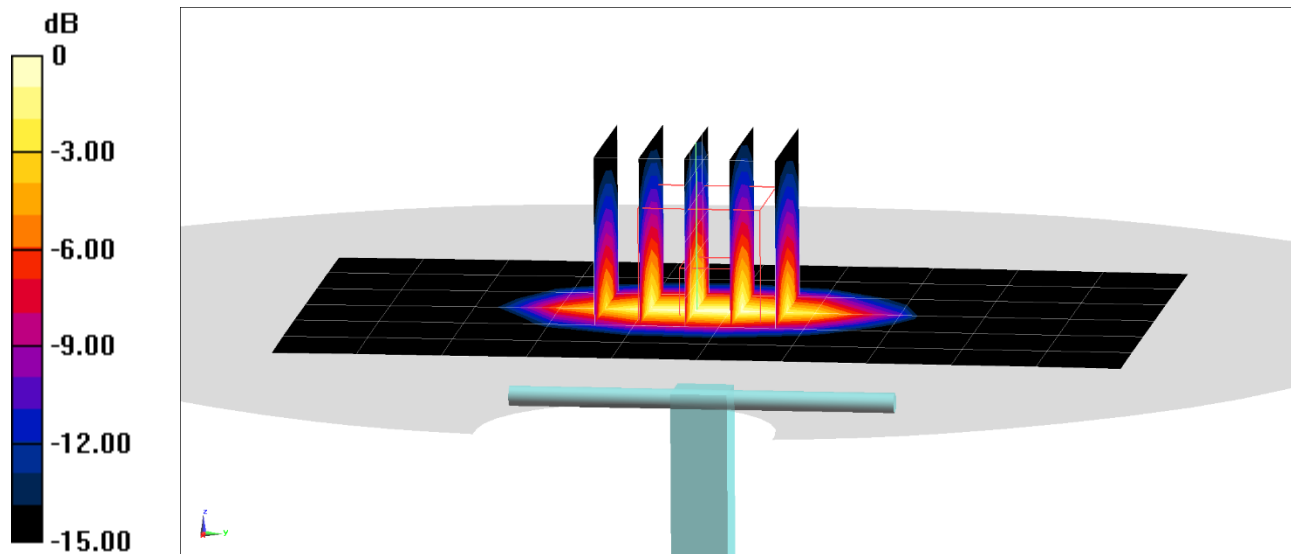

0 dB = 6.53 W/kg = 8.15 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d148

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body; Medium parameters used:

$f = 1900 \text{ MHz}$; $\sigma = 1.56 \text{ S/m}$; $\epsilon_r = 51.117$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/28/2021; Ambient Temp: 22.3°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN7410; ConvF(7.7, 7.7, 7.7) @ 1900 MHz; Calibrated: 7/20/2021

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 7/13/2021

Phantom: Twin-SAM V5.0 (Front); Type: QD 000 P40 CD; Serial: 1792

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Peak SAR (extrapolated) = 7.60 W/kg

SAR(1 g) = 4.12 W/kg

Deviation(1 g) = 5.37%

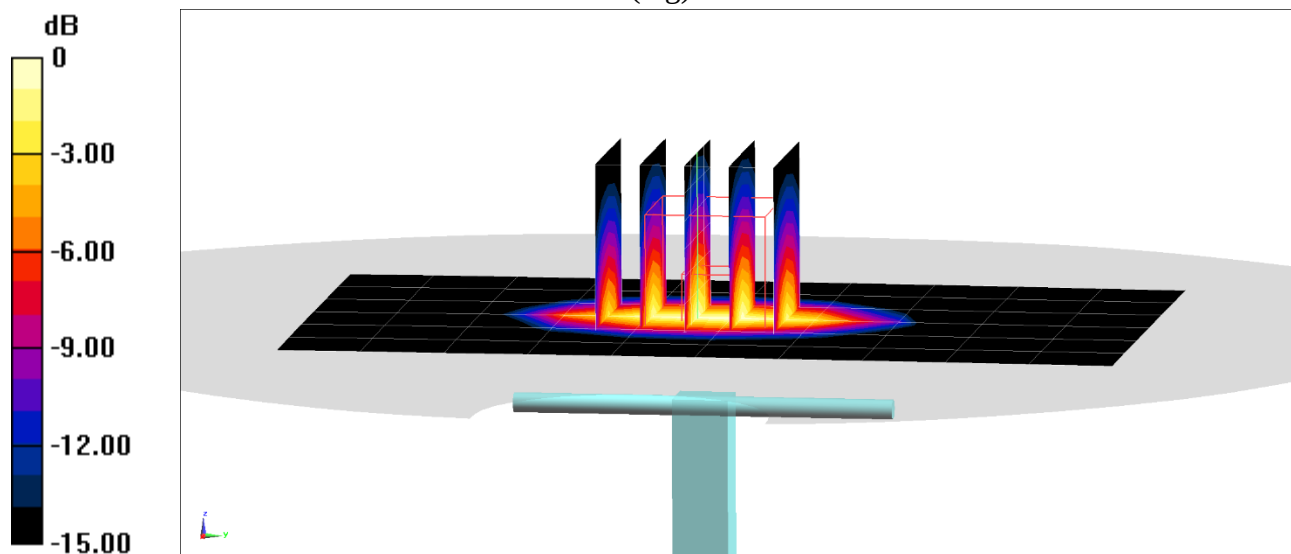

0 dB = 6.36 W/kg = 8.03 dBW/kg

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V2; Serial: 1116

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2021; Ambient Temp: 23.6°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF:(7.41,7.41,7.41); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0 (Left); Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.92 W/kg

SAR(1 g) = 4.90 W/kg

Deviation (1 g) = -0.41%

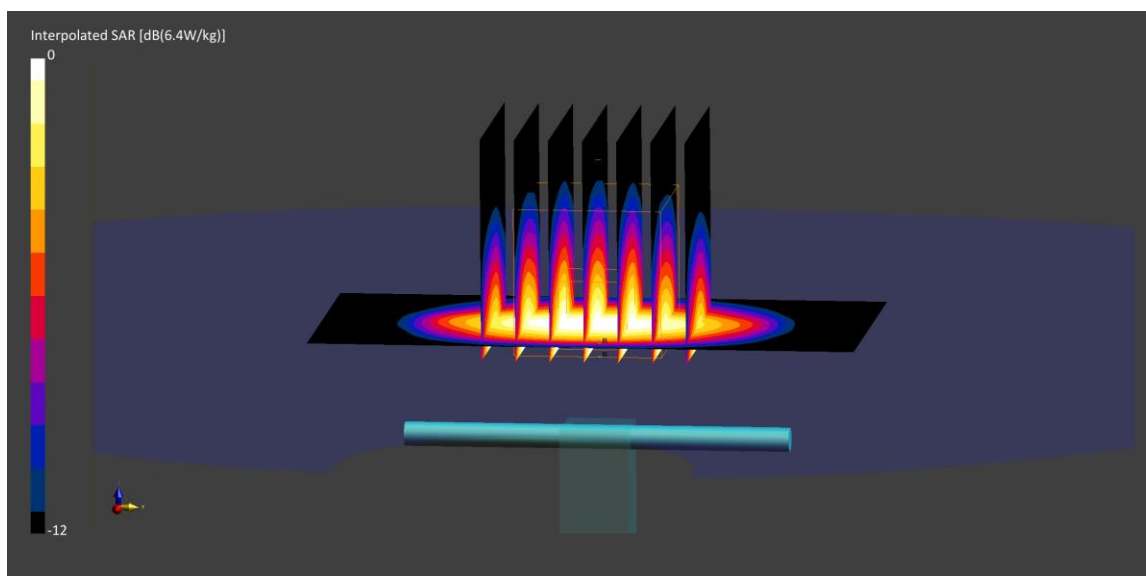

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V2; Serial: 1116

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: Unnamed Medium; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.87$ S/m; $\epsilon_r = 51.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 09/26/2021; Ambient Temp: 20.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN3914; ConvF:(7.41,7.41,7.41); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0 (Left); Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.62 W/kg

SAR(1 g) = 4.78 W/kg; SAR(10 g) = 2.29 W/kg

Deviation (1 g) = -2.85%; Deviation (10 g) = -3.38%

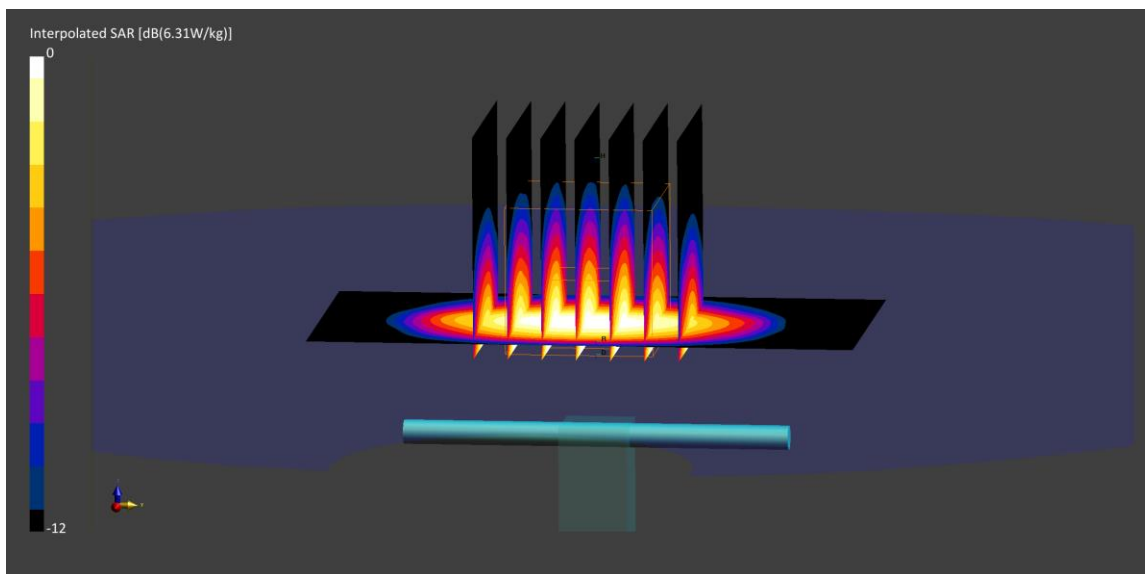

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V3; Serial: 1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/31/2021; Ambient Temp: 22.1°C; Tissue Temp: 24.5°C

Probe: EX3DV4 - SN3914; ConvF:(7.41,7.41,7.41); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0; Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.4 W/kg

SAR(1 g) = 4.88 W/kg

Deviation (1 g) = 0.83%

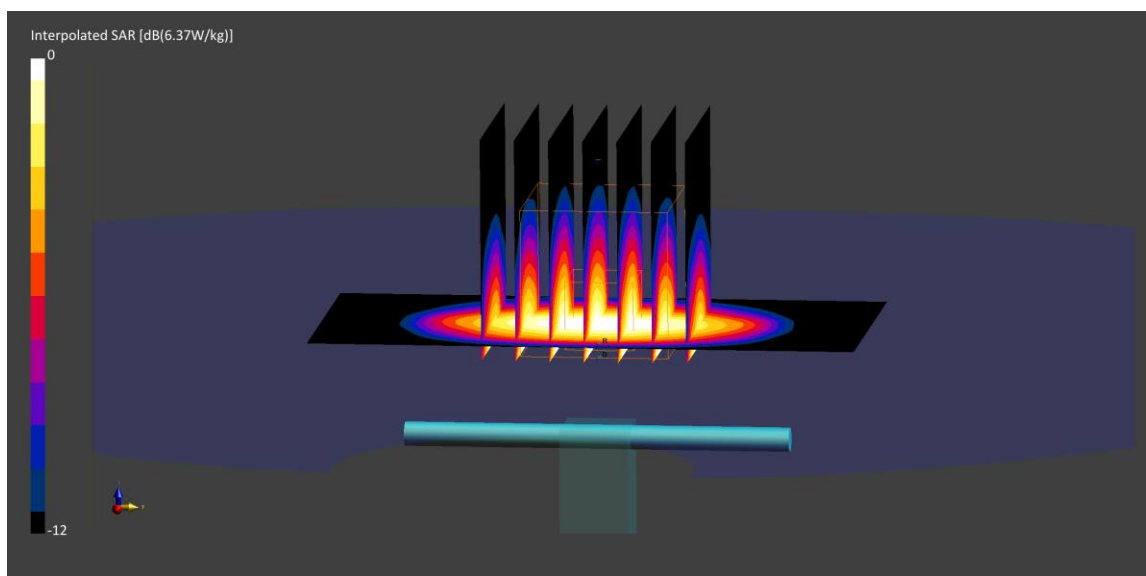

PCTEST

DUT: Dipole 2300.0 MHz; Type: D2300V3; Serial: 1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2300.0$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 53.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/03/2021; Ambient Temp: 22.2°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN3914; ConvF:(7.41,7.41,7.41); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0; Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.2 W/kg

SAR(1 g) = 4.99 W/kg; SAR(10 g) = 2.37 W/kg

Deviation (1 g) = 3.10%; Deviation (10 g) = 1.28%

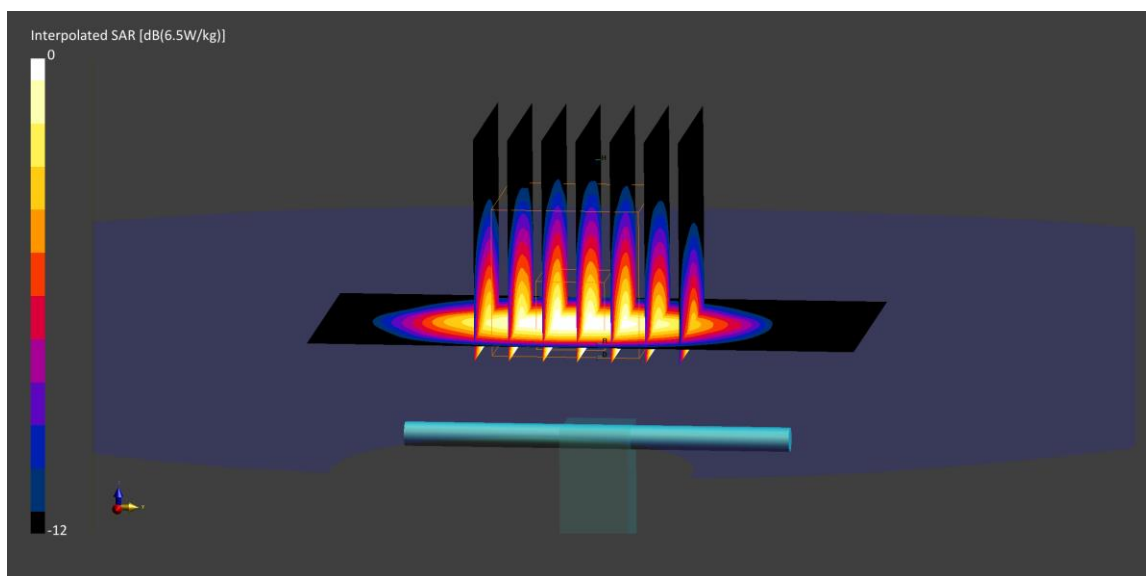

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 2.02$ S/m; $\epsilon_r = 53.9$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2021; Ambient Temp: 20.7°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7539; ConvF:(7.62,7.62,7.62); Calibrated: 2020-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1415; Calibrated: 2021-03-10

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.6 W/kg

SAR(1 g) = 4.94 W/kg

Deviation (1 g) = 0.00%

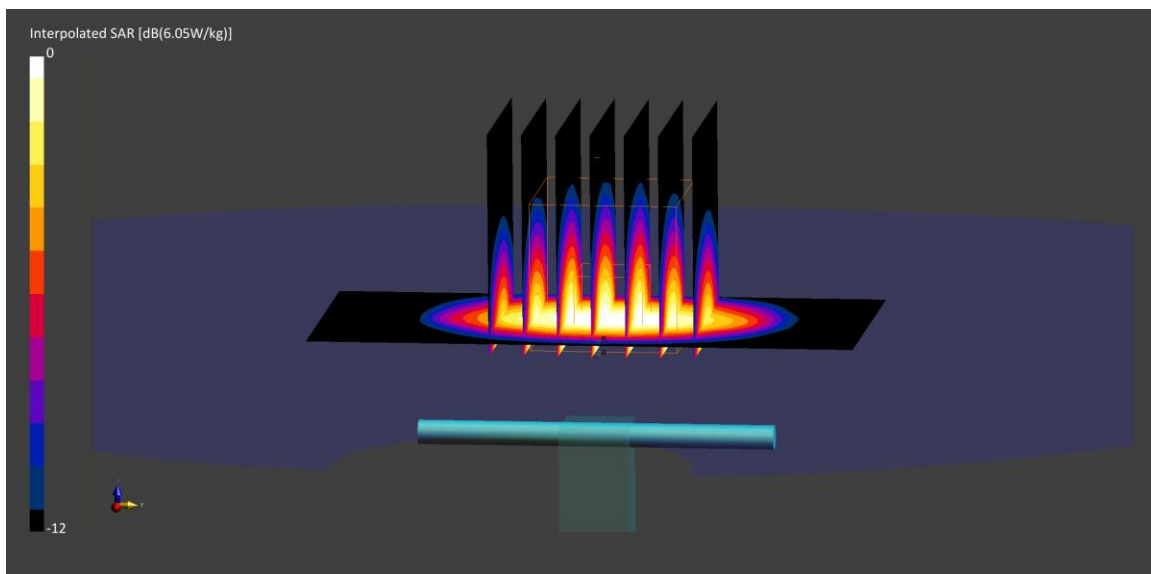

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 2.04$ S/m; $\epsilon_r = 53.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/21/2021; Ambient Temp: 22.4°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN3914; ConvF:(7.33,7.33,7.33); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0; Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.0 W/kg

SAR(10 g) = 2.40 W/kg

Deviation (10 g) = -2.83%

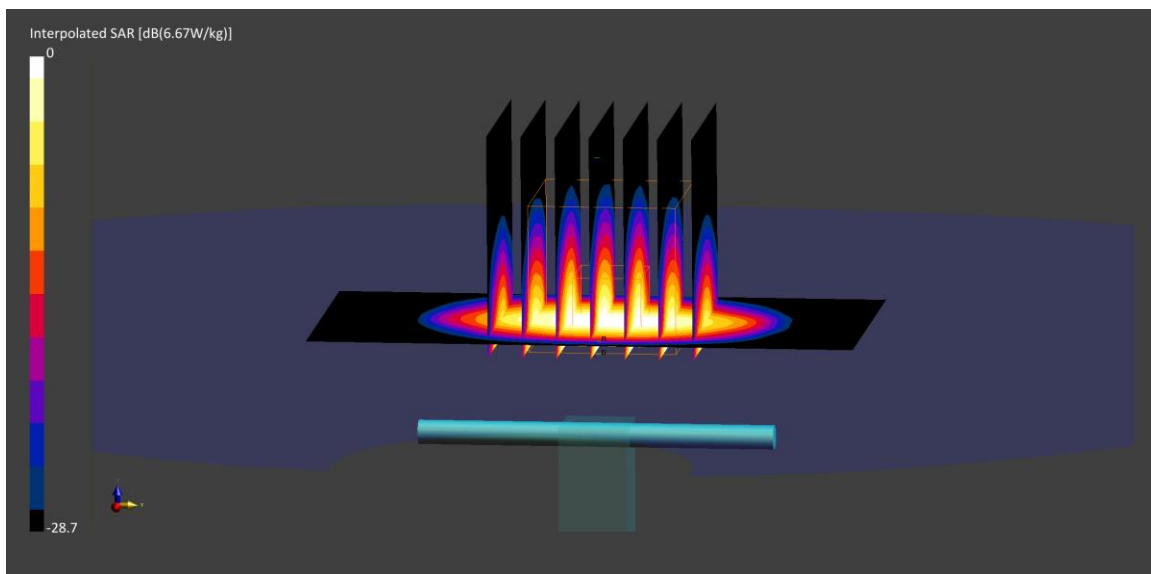

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 882

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 51.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/21/2021; Ambient Temp: 21.0°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7637; ConvF:(8.77,8.77,8.77); Calibrated: 2021-03-03

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1652; Calibrated: 2021-03-01

Phantom: Twin-SAM V8.0 (30); Serial: 1934

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.86 W/kg

SAR(1 g) = 4.86 W/kg

Deviation (1 g) = -3.95%

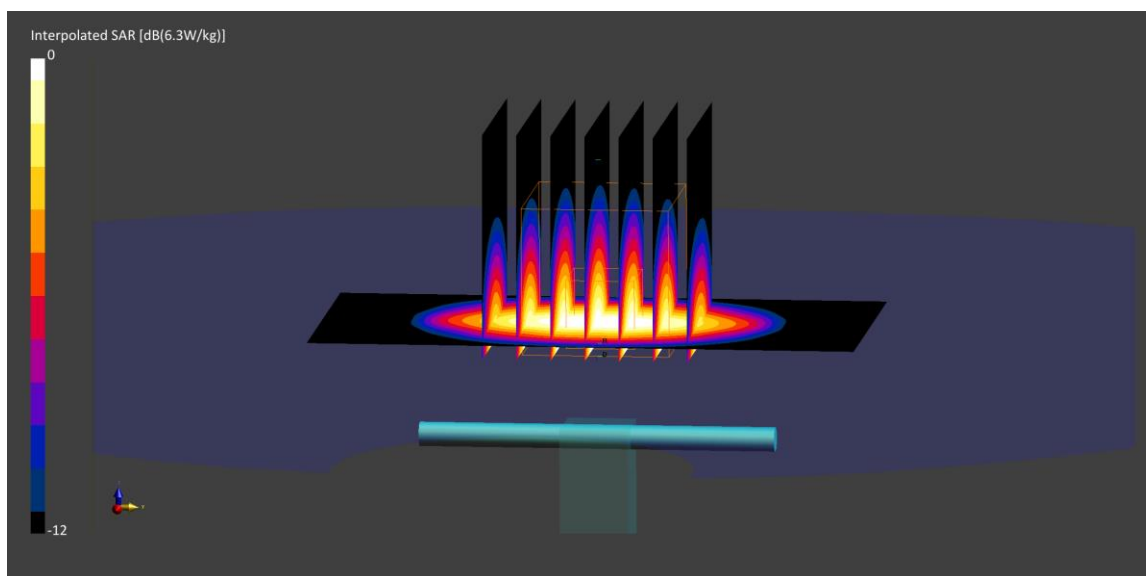

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 882

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 51.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/27/2021; Ambient Temp: 21.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7637; ConvF:(8.77,8.77,8.77); Calibrated: 2021-03-03

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1652; Calibrated: 2021-03-01

Phantom: Twin-SAM V8.0 (30); Serial: 1934

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.59 W/kg

SAR(1 g) = 4.88 W/kg

Deviation (1 g) = -3.56%

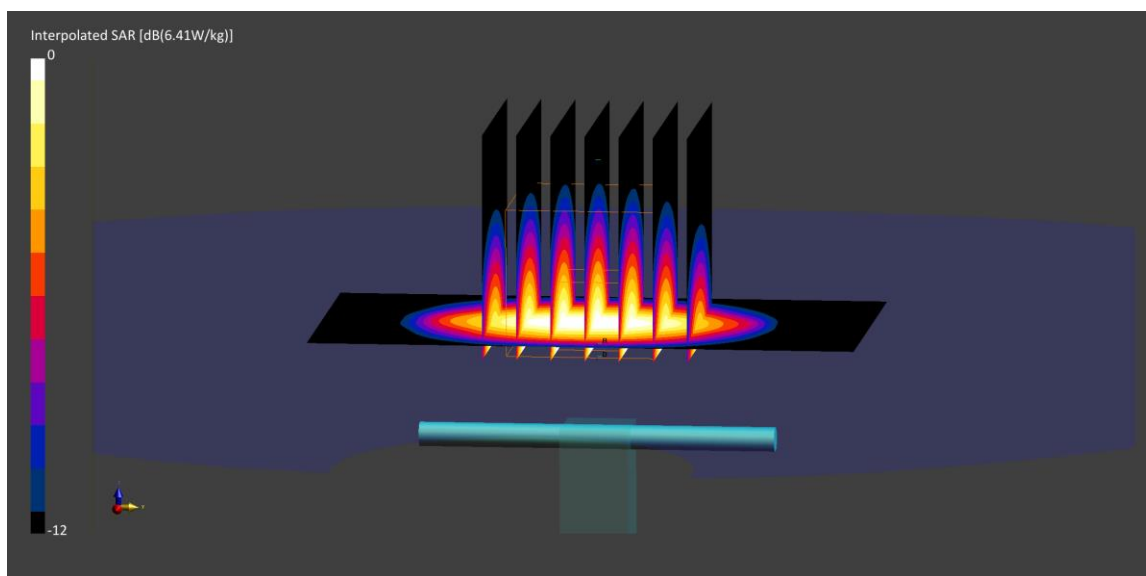

PCTEST

DUT: Dipole 2450.0 MHz; Type: D2450V2; Serial: 719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2450.0$ MHz; $\sigma = 2.02$ S/m; $\epsilon_r = 51.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/01/2021; Ambient Temp: 21.3°C; Tissue Temp: 23.3°C

Probe: EX3DV4 - SN7670; ConvF:(7.81,7.81,7.81); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1966

Measurement SW: DASY Module SAR V16.0.0.116

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.5 W/kg

SAR(1 g) = 4.94 W/kg; SAR(10 g) = 2.25 W/kg

Deviation (1 g) = -5.00%; Deviation (10 g) = -8.91%

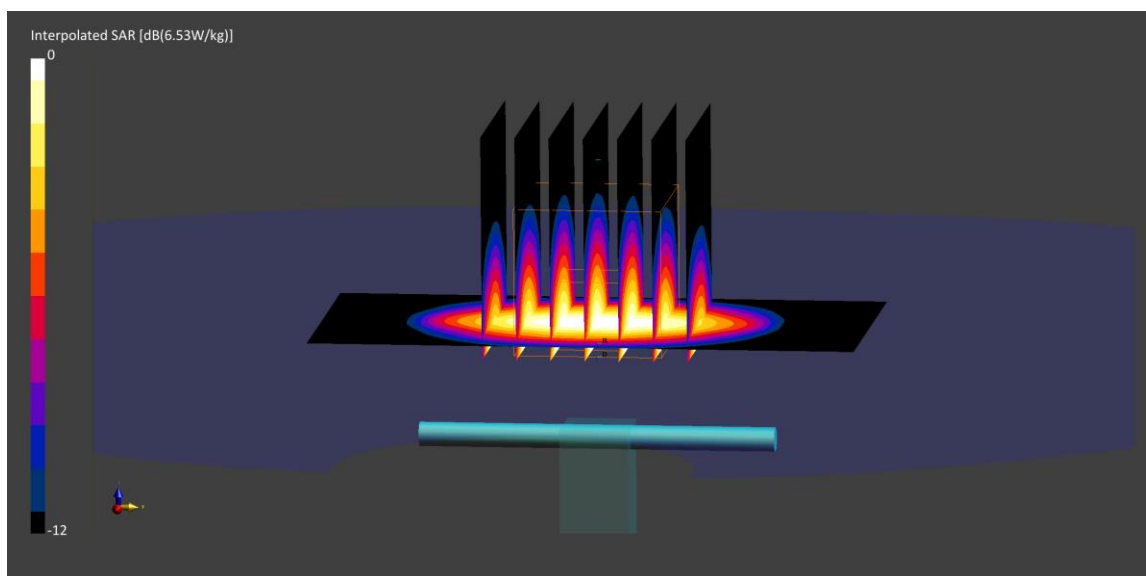

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.24$ S/m; $\epsilon_r = 53.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2021; Ambient Temp: 20.7°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7539; ConvF:(7.55,7.55,7.55); Calibrated: 2020-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1415; Calibrated: 2021-03-10

Phantom: Twin-SAM V8.0; Serial: 1630

Measurement SW: DASY Module SAR V16.0.0.116

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.4 W/kg

SAR(1 g) = 5.45 W/kg

Deviation (1 g) = -1.62%

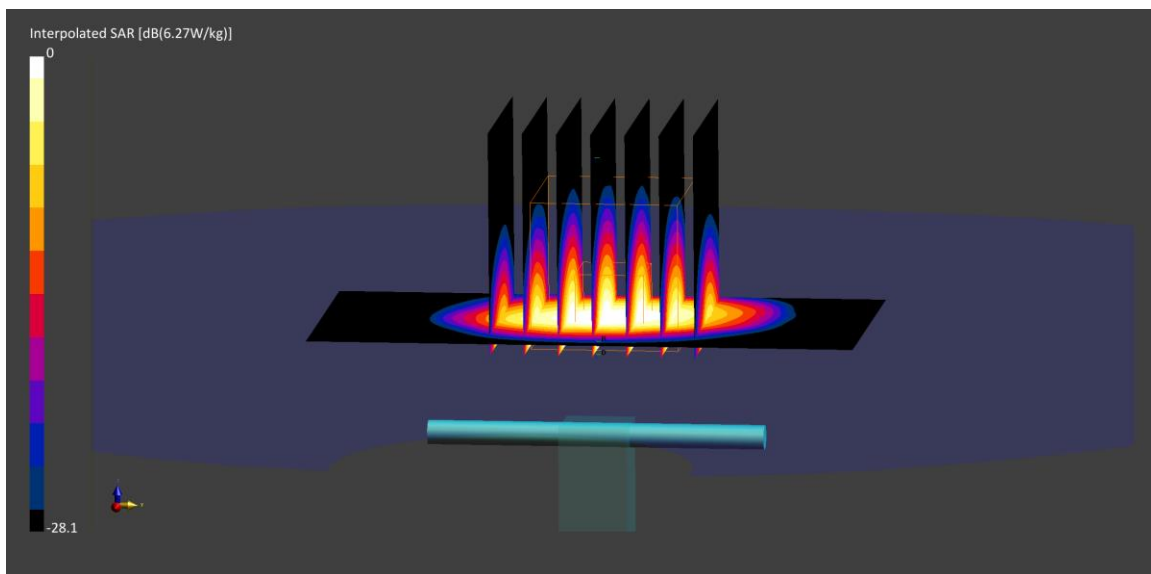

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.22$ S/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/21/2021; Ambient Temp: 22.4°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN3914; ConvF:(7.14,7.14,7.14); Calibrated: 2021-05-18

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn728; Calibrated: 2021-05-11

Phantom: Twin-SAM V5.0; Serial: 1873

Measurement SW: DASY Module SAR V16.0.0.116

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.5 W/kg

SAR(10 g) = 2.46 W/kg

Deviation (10 g) = -0.81%

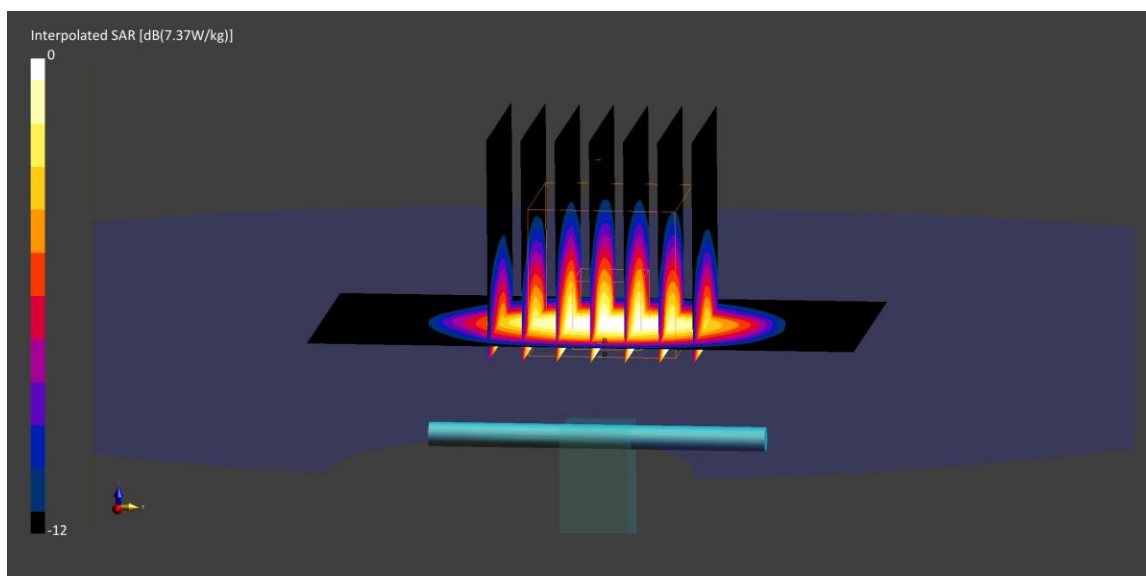

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.20$ S/m; $\epsilon_r = 52.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/25/2021; Ambient Temp: 22.1°C; Tissue Temp: 23.6°C

Probe: EX3DV4 - SN7659; ConvF:(8.37,8.37,8.37); Calibrated: 2021-06-29

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1678; Calibrated: 2021-06-21

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.0.65

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

SAR(1 g) = 5.41 W/kg; SAR(10 g) = 2.42 W/kg

Deviation (1 g) = -2.70%; Deviation (10 g) = -3.20%

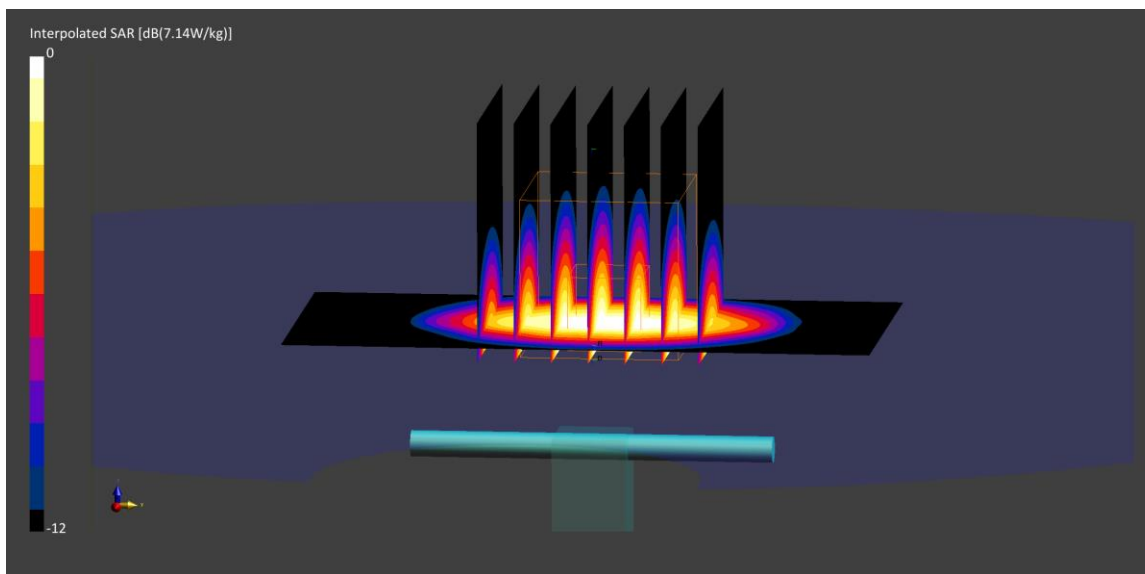

PCTEST

DUT: Dipole 2600.0 MHz; Type: D2600V2; Serial: 1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Body; Medium parameters used:

$f = 2600.0$ MHz; $\sigma = 2.23$ S/m; $\epsilon_r = 51.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/01/2021; Ambient Temp: 21.3°C; Tissue Temp: 23.3°C

Probe: EX3DV4 - SN7670; ConvF:(7.7,7.7,7.7); Calibrated: 2021-08-05

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2021-08-03

Phantom: Twin-SAM V8.0; Serial: 1966

Measurement SW: DASY Module SAR V16.0.0.116

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.1 W/kg

SAR(1 g) = 5.25 W/kg; SAR(10 g) = 2.28 W/kg

Deviation (1 g) = -5.23%; Deviation (10 g) = -8.06%

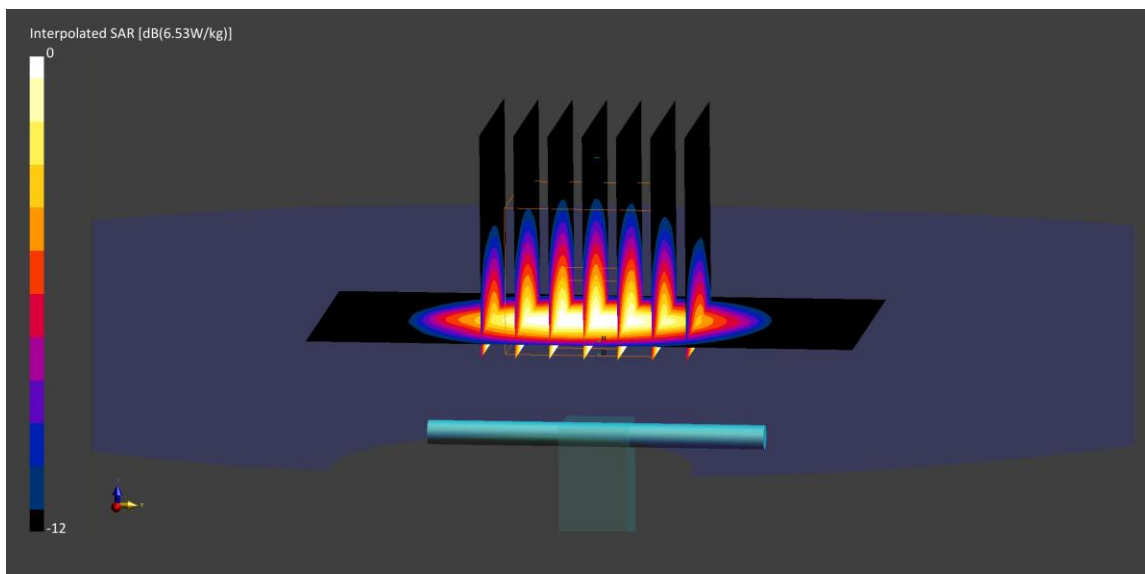

PCTEST

DUT: Dipole 3500.0 MHz; Type: D3500V2; Serial: 1059

Communication System: UID: 0, CW; Frequency: 3500.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3500.0$ MHz; $\sigma = 3.23$ S/m; $\epsilon_r = 49.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/18/2021; Ambient Temp: 20.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7661; ConvF:(6.7,6.7,6.7); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1450; Calibrated: 2021-08-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3500 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 6.74 W/kg

Deviation (1 g) = 6.98%

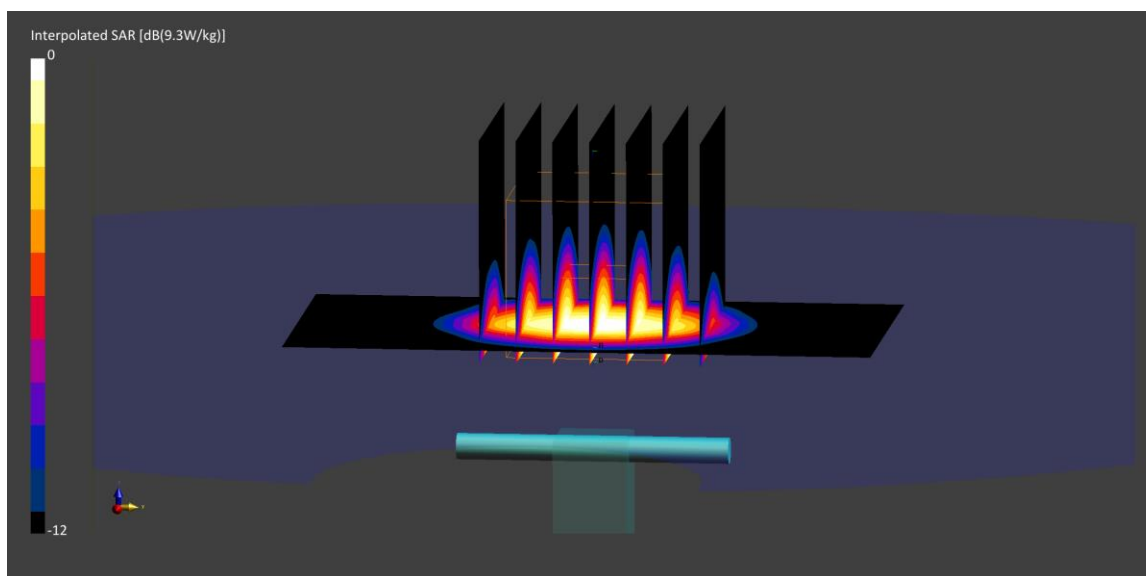

PCTEST

DUT: Dipole 3500.0 MHz; Type: D3500V2; Serial: 1059

Communication System: UID: 0, CW; Frequency: 3500.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3500.0$ MHz; $\sigma = 3.17$ S/m; $\epsilon_r = 49.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/21/2021; Ambient Temp: 21.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7661; ConvF:(6.7,6.7,6.7); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1450; Calibrated: 2021-08-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3500 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.2 W/kg

SAR(1 g) = 6.76 W/kg

Deviation (1 g) = 7.30%

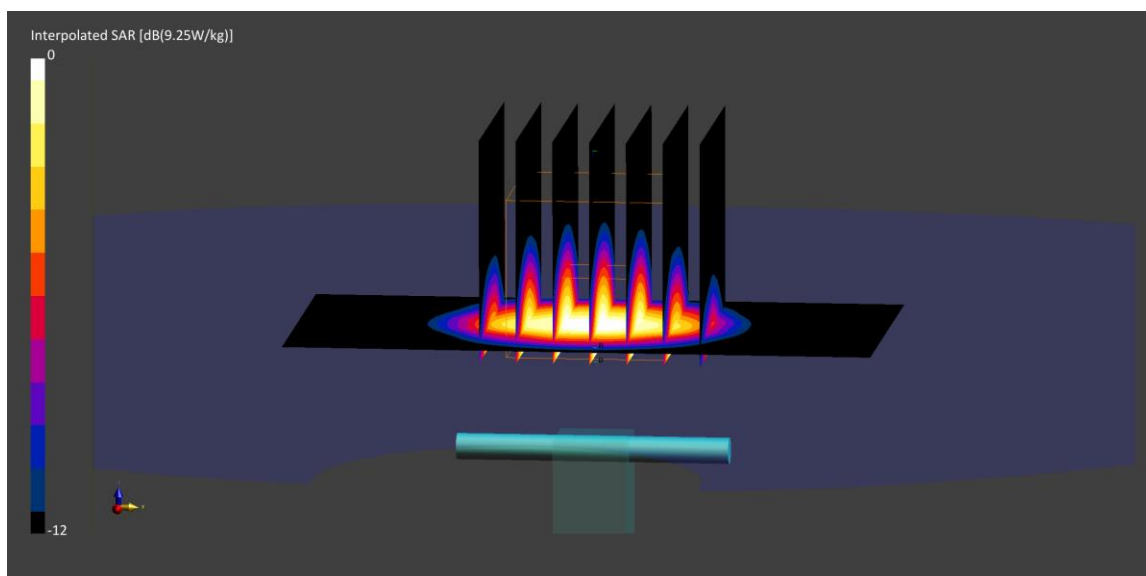

PCTEST

DUT: Dipole 3500.0 MHz; Type: D3500V2; Serial: 1059

Communication System: UID: 0, CW; Frequency: 3500.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3500.0$ MHz; $\sigma = 3.22$ S/m; $\epsilon_r = 51.1$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 0.0 cm

Test Date: 11/15/2021; Ambient Temp: 20.0°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7661; ConvF:(6.7,6.7,6.7); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1450; Calibrated: 2021-08-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3500 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.2 W/kg

SAR(10 g) = 2.39 W/kg

Deviation (10 g) = 2.58%

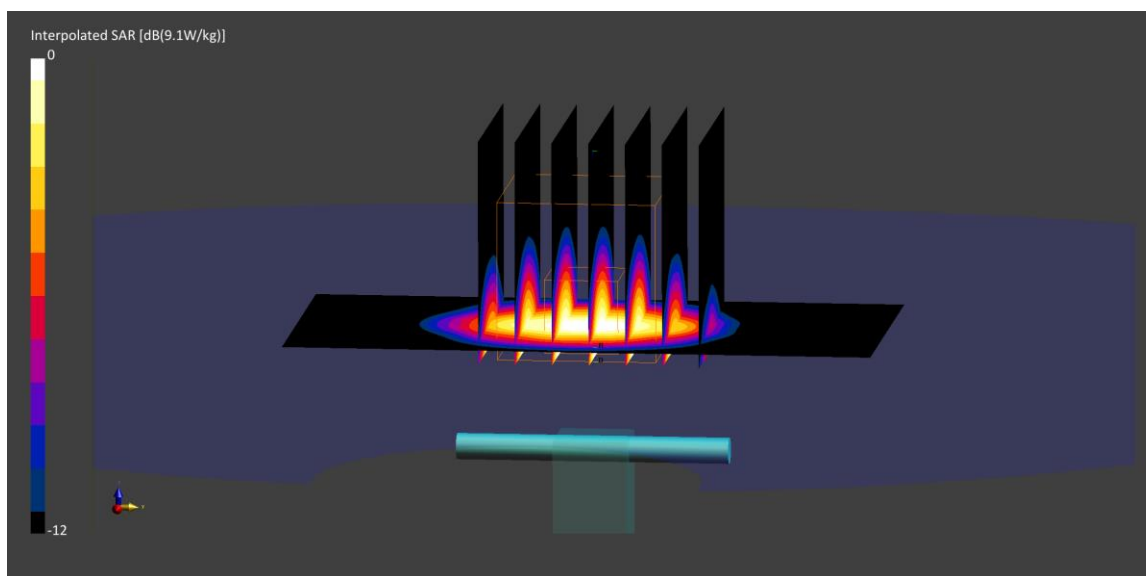

PCTEST

DUT: Dipole 3700.0 MHz; Type: D3700V2; Serial: 1018

Communication System: UID: 0, CW; Frequency: 3700.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3700.0$ MHz; $\sigma = 3.40$ S/m; $\epsilon_r = 50.2$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/07/2021; Ambient Temp: 21.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7551; ConvF:(6.33,6.33,6.33); Calibrated: 2020-10-20

Sensor-Surface: 1.4mm (All points)

Electronics: DAE4 Sn1333; Calibrated: 2020-10-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3700 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 15.7 W/kg

SAR(1 g) = 6.15 W/kg; SAR(10 g) = 2.28 W/kg

Deviation (1 g) = -3.15%; Deviation (10 g) = 1.33%

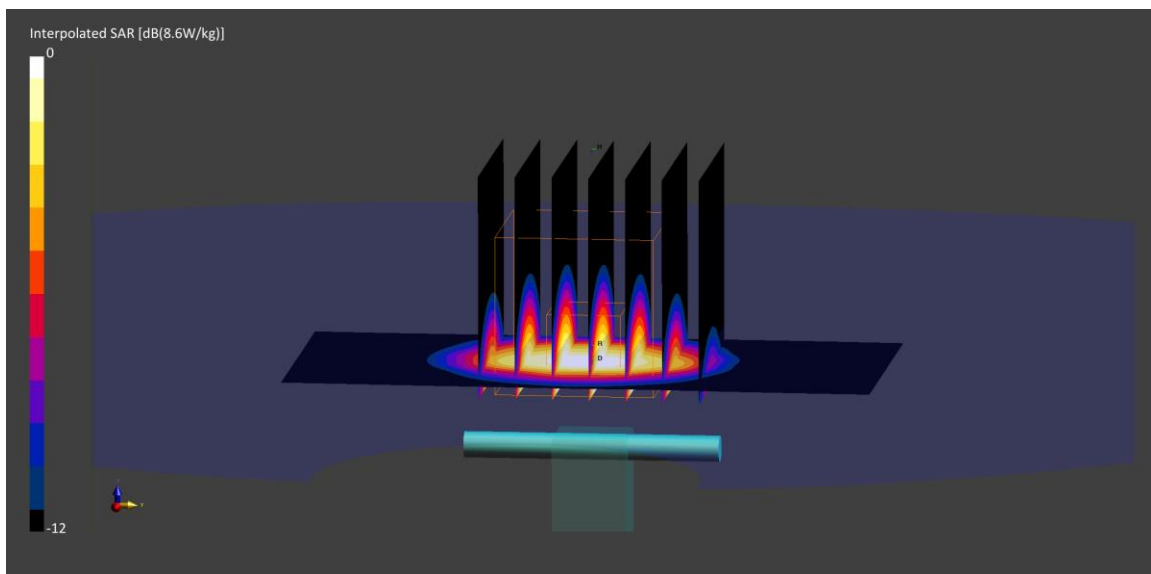

PCTEST

DUT: Dipole 3700.0 MHz; Type: D3700V2; Serial: 1018

Communication System: UID: 0, CW; Frequency: 3700.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3700.0$ MHz; $\sigma = 3.46$ S/m; $\epsilon_r = 49.2$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/18/2021; Ambient Temp: 20.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7661; ConvF:(6.66,6.66,6.66); Calibrated: 2021-06-28

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1450; Calibrated: 2021-08-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3700 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.7 W/kg

SAR(1 g) = 6.55 W/kg

Deviation (1 g) = 3.15%

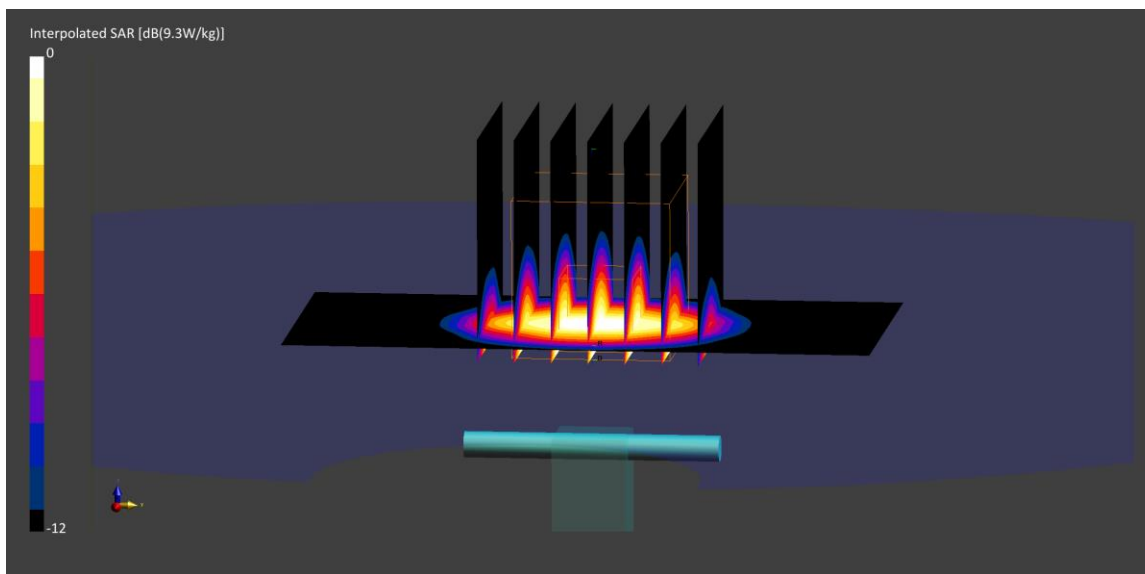

PCTEST

DUT: Dipole 3900.0 MHz; Type: D3900V2; Serial: 1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz

Medium: 3600 Body; Medium parameters used:

$f = 3900.0$ MHz; $\sigma = 3.63$ S/m; $\epsilon_r = 49.8$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 10/07/2021; Ambient Temp: 21.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7551; ConvF:(5.91,5.91,5.91); Calibrated: 2020-10-20

Sensor-Surface: 1.4mm (All points)

Electronics: DAE4 Sn1333; Calibrated: 2020-10-16

Phantom: Twin-SAM V5.0; Serial: 1692 Right Back

Measurement SW: DASY Module SAR V16.0.0.116

3900 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.9 W/kg

SAR(1 g) = 6.73 W/kg; SAR(10 g) = 2.36 W/kg

Deviation (1 g) = 4.67%; Deviation (10 g) = 7.27%

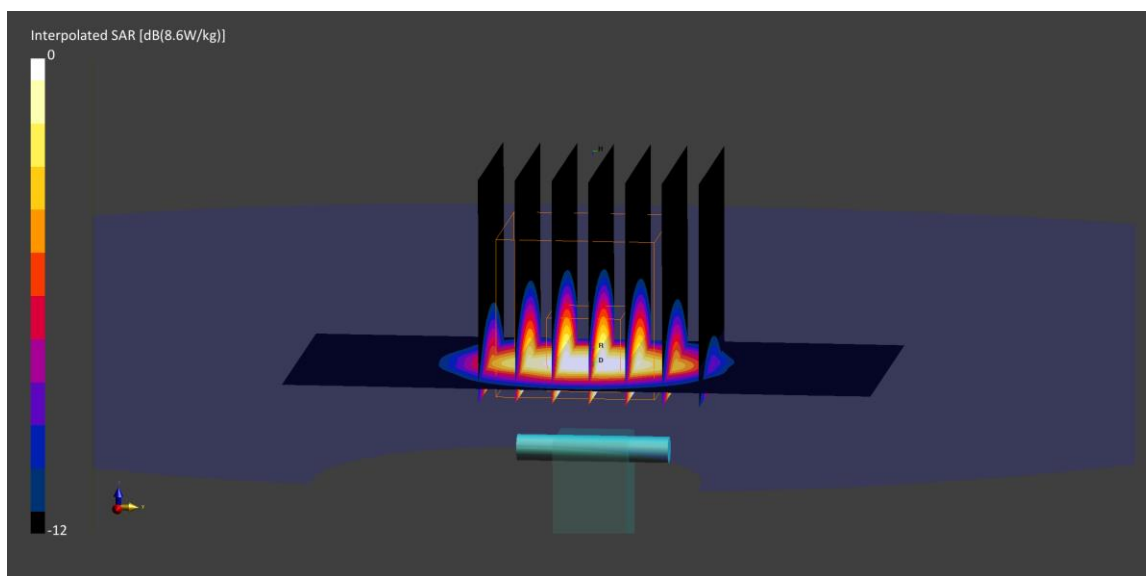

PCTEST

DUT: Dipole 5250.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5250.0$ MHz; $\sigma = 5.42$ S/m; $\epsilon_r = 47.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/03/2021; Ambient Temp: 19.7°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.55,4.55,4.55); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.9 W/kg

SAR(1 g) = 3.68 W/kg

Deviation (1 g) = -0.94%

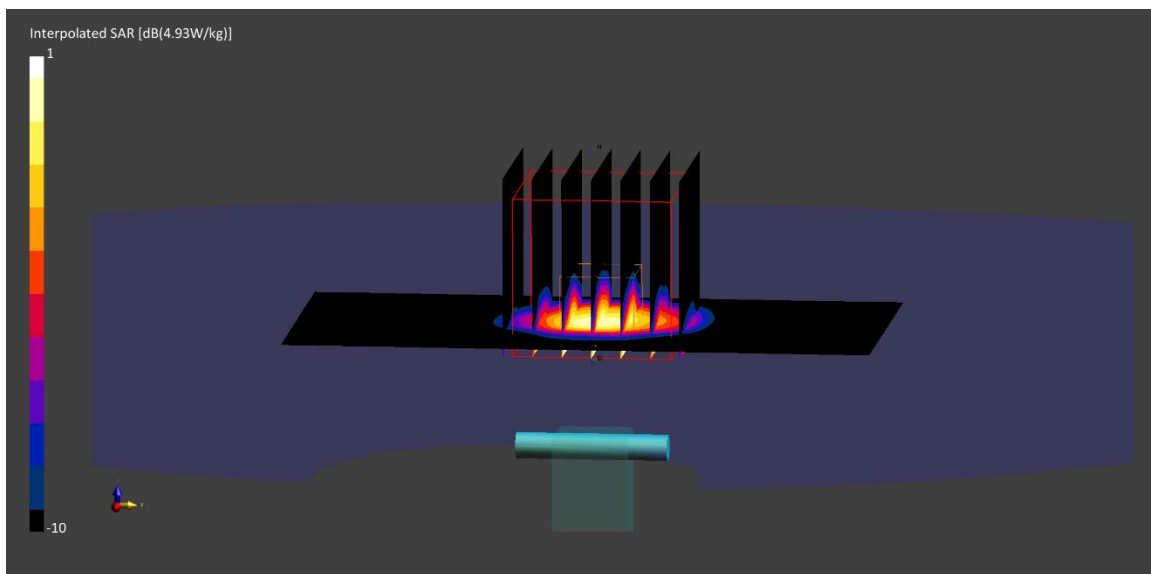

PCTEST

DUT: Dipole 5600.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5600.0$ MHz; $\sigma = 5.92$ S/m; $\epsilon_r = 46.7$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/03/2021; Ambient Temp: 19.7°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.16,4.16,4.16); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.1 W/kg

SAR(1 g) = 3.64 W/kg

Deviation (1 g) = -5.94%

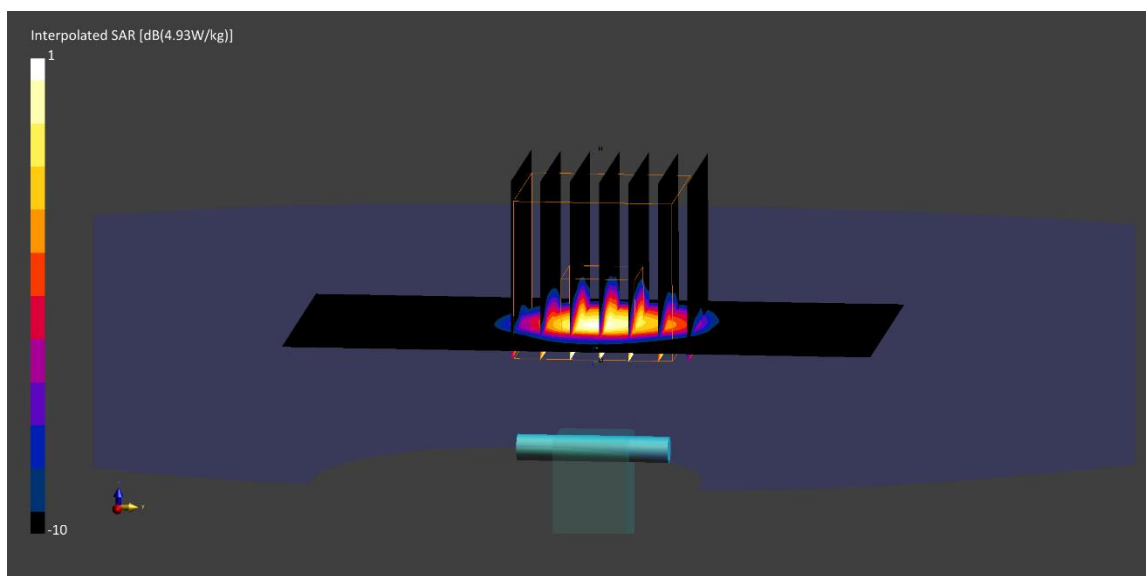

PCTEST

DUT: Dipole 5750.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5750.0$ MHz; $\sigma = 6.15$ S/m; $\epsilon_r = 46.4$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/03/2021; Ambient Temp: 19.7°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.18,4.18,4.18); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5750 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.4 W/kg

SAR(1 g) = 3.62 W/kg

Deviation (1 g) = -0.55%

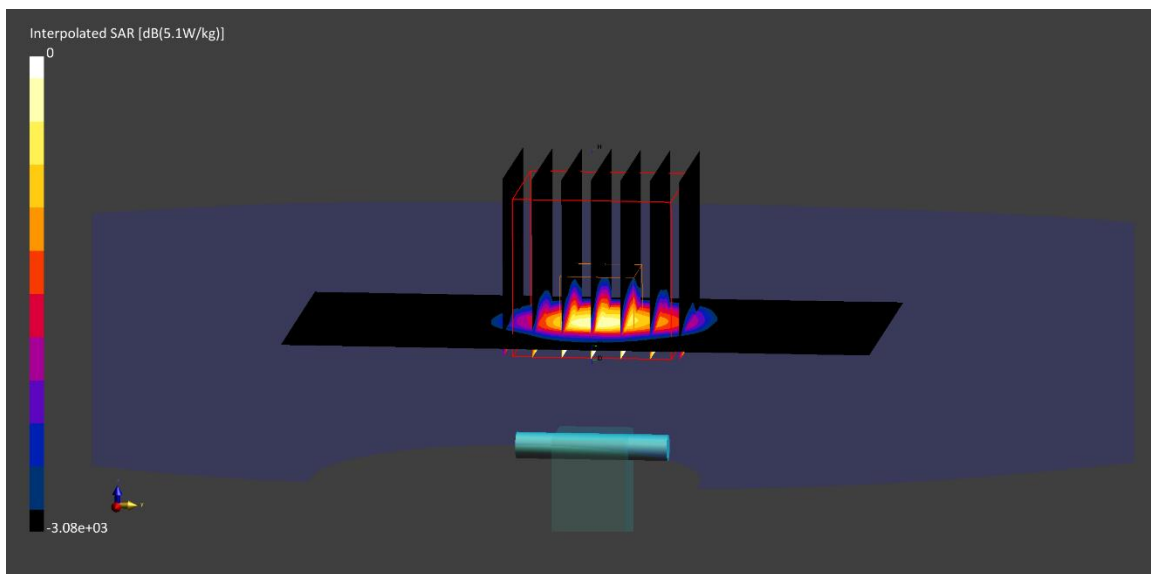

PCTEST

DUT: Dipole 5250.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5250.0$ MHz; $\sigma = 5.30$ S/m; $\epsilon_r = 48.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/15/2021; Ambient Temp: 20.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.55,4.55,4.55); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.0 W/kg

SAR(10 g) = 1.04 W/kg

Deviation (10 g) = 0.48%

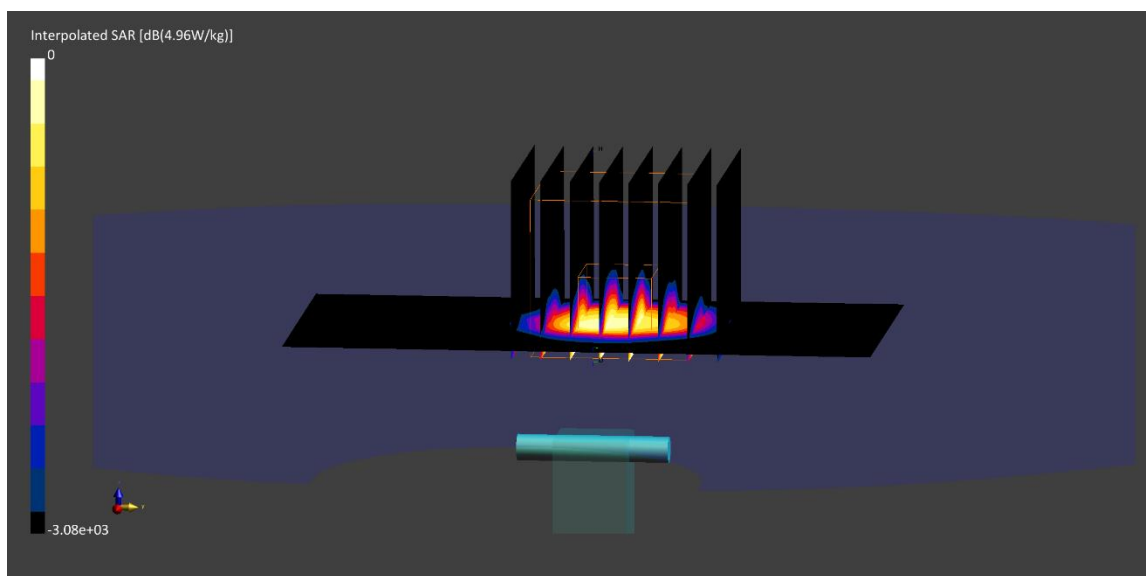

PCTEST

DUT: Dipole 5600.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5600.0$ MHz; $\sigma = 5.80$ S/m; $\epsilon_r = 47.6$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/15/2021; Ambient Temp: 20.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.16,4.16,4.16); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.9 W/kg

SAR(10 g) = 1.07 W/kg

Deviation (10 g) = 0.00%

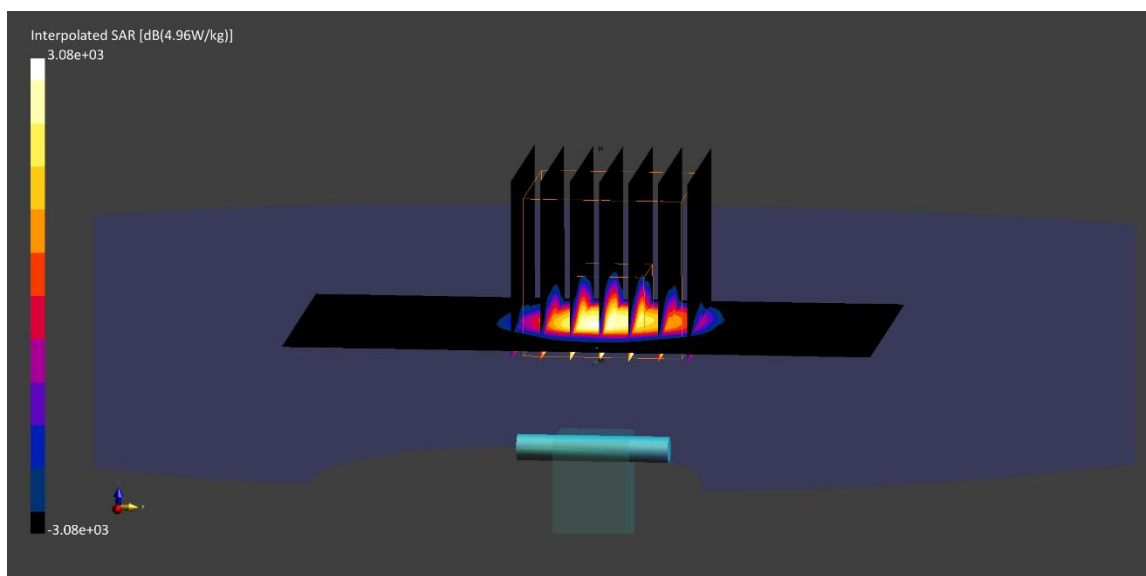

PCTEST

DUT: Dipole 5750.0 MHz; Type: D5GHzV2; Serial: 1057

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5750.0$ MHz; $\sigma = 6.02$ S/m; $\epsilon_r = 47.3$; $\rho = 1000$ kg/m³

Phantom Section: Flat Section; Space: 1.0 cm

Test Date: 11/15/2021; Ambient Temp: 20.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7526; ConvF:(4.18,4.18,4.18); Calibrated: 2021-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1272; Calibrated: 2021-03-18

Phantom: Twin-SAM V5.0; Serial: 1800

Measurement SW: DASY Module SAR V16.0.0.116

5750 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.3 W/kg

SAR(10 g) = 1.02 W/kg

Deviation (10 g) = 2.00%

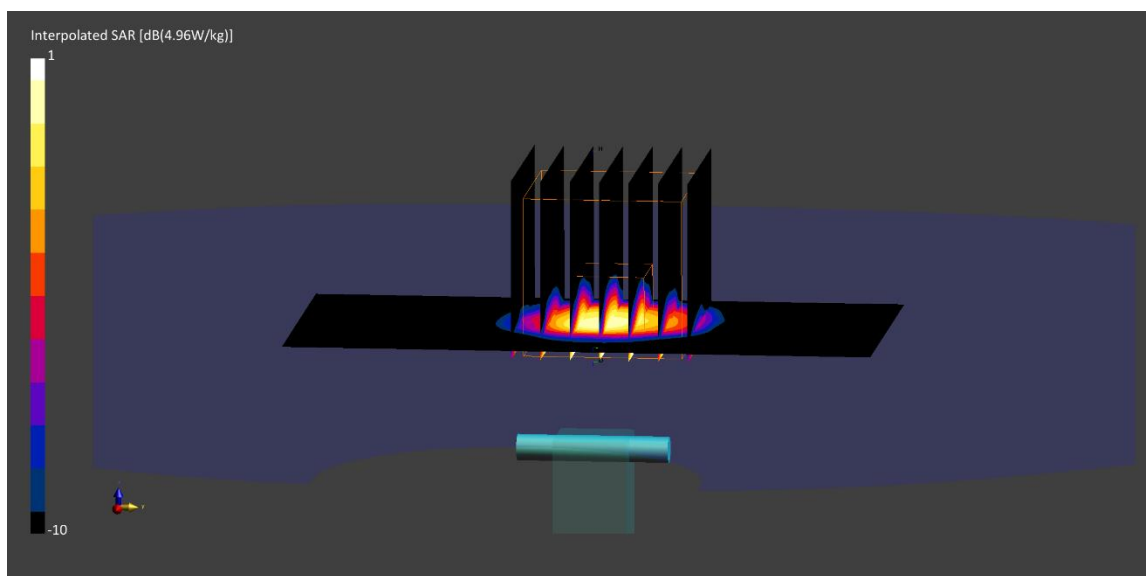

PCTEST

DUT: Dipole 5800.0 MHz; Type: D5GHzV2; Serial: 1191

Communication System: UID: 0, CW; Frequency: 5800.0 MHz

Medium: 5200-5800 Body; Medium parameters used:

$f = 5800.0$ MHz; $\sigma = 6.26$ S/m; $\epsilon_r = 46.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 11/04/2021; Ambient Temp: 24.5°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7552; ConvF:(4.05,4.05,4.05); Calibrated: 2021-09-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1677; Calibrated: 2021-06-22

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.0.65

5800 MHz System Verification at 17 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.5 W/kg

SAR(1 g) = 3.44 W/kg; SAR(10 g) = 0.970 W/kg

Deviation (1 g) = -6.39%; Deviation (10 g) = -3.96%;

