

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	14.3, 16.56,15.27

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-24	22.8	22.2	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.708	51.4	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.124	-3.73
psSAR10g	0.076	-8.90
Peak SAR (Extrapolated)	0.257	-3.18
psAPD (4.0 cm², sq)	N/A	N/A

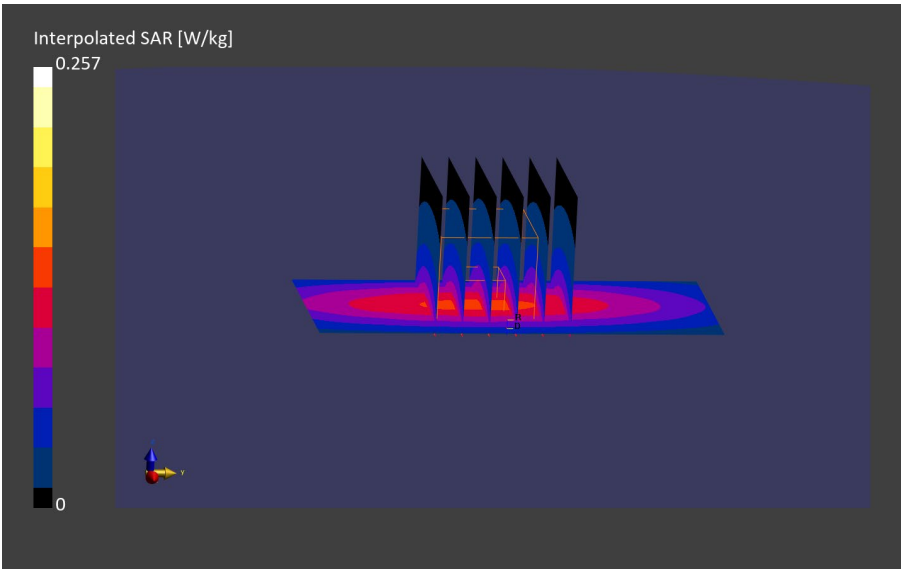

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-09	21.5	21.3	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.881	42.0	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.417	-4.25
psSAR10g	0.274	-3.92
Peak SAR (Extrapolated)	0.634	0.4
psAPD (4.0 cm², sq)	N/A	N/A

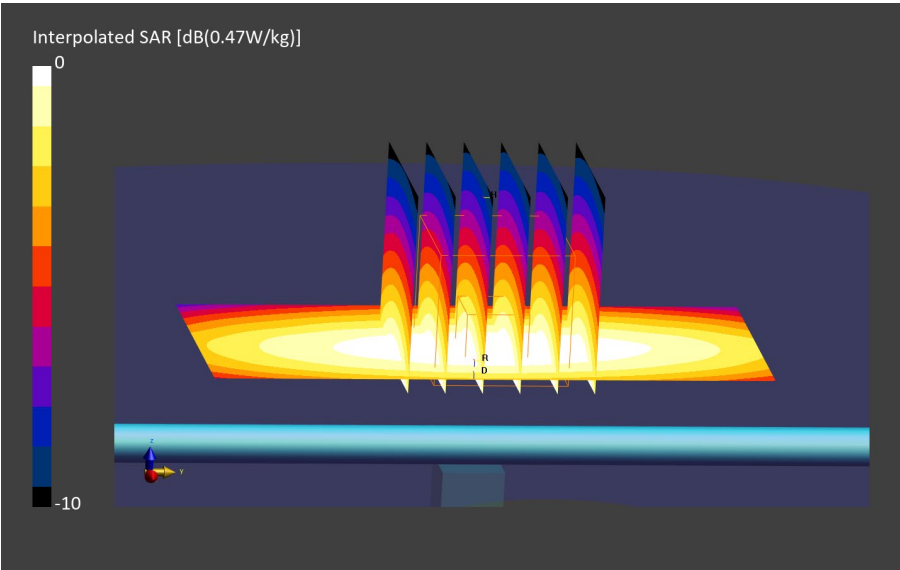

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-11	23.2	21.5	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.870	41.3	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.412	-5.4
psSAR10g	0.271	-4.97
Peak SAR (Extrapolated)	0.617	-2.3
psAPD (4.0 cm², sq)	N/A	N/A

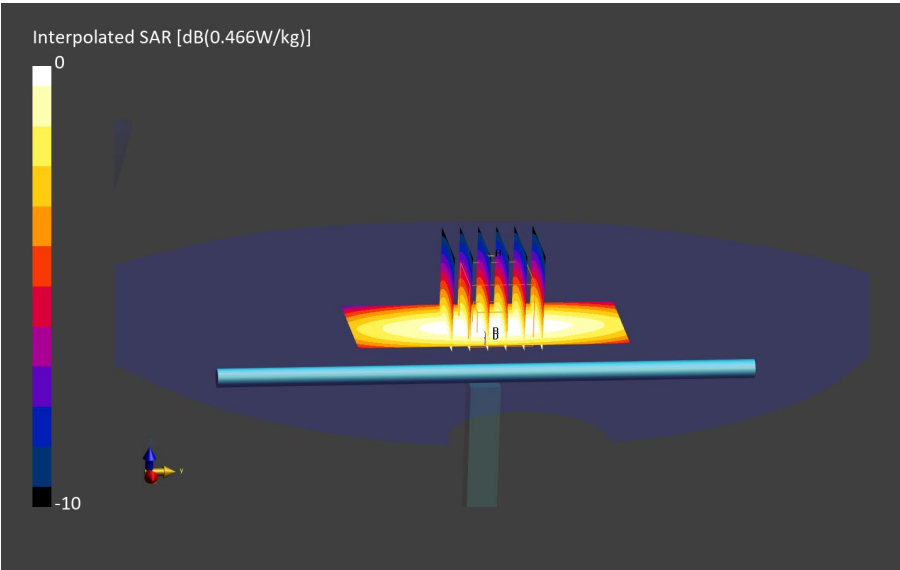

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-14	23.9	22.5	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.899	40.3	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.418	-4.03
psSAR10g	0.275	-3.57
Peak SAR (Extrapolated)	0.645	2.14
psAPD (4.0 cm², sq)	N/A	N/A

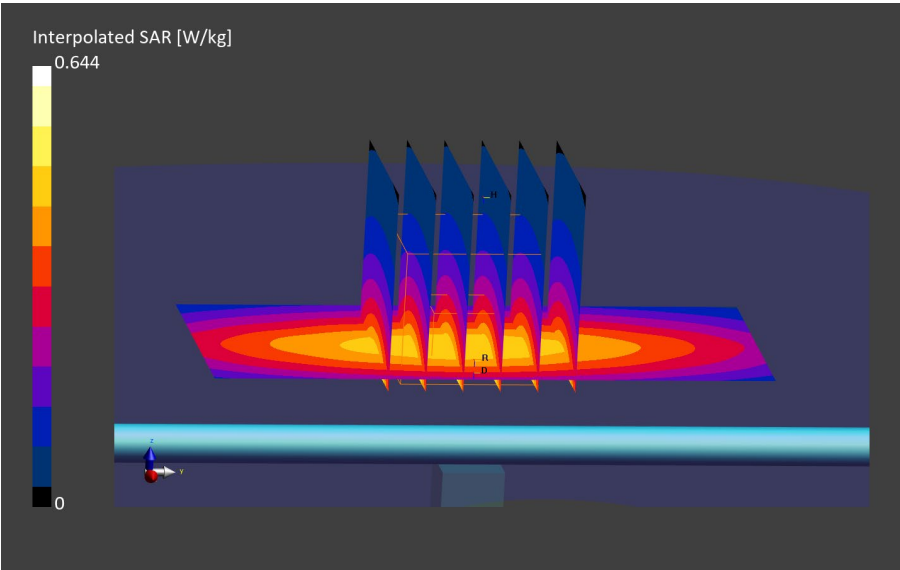

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-15	23.1	21.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.884	43.6	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.419	-3.8
psSAR10g	0.277	-2.87
Peak SAR (Extrapolated)	0.621	-1.66
psAPD (4.0 cm², sq)	N/A	N/A

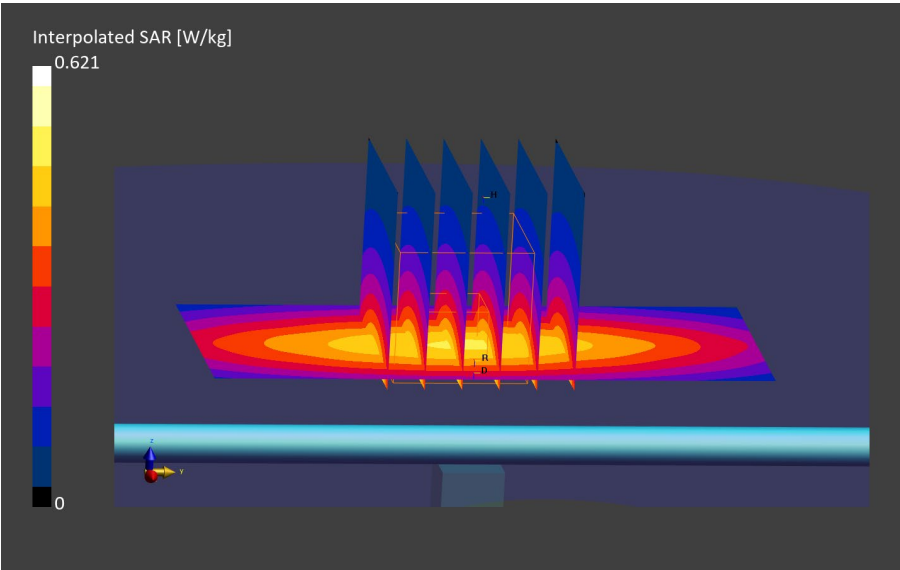

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.46, 9.07,8.79

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-27	24.3	22.2	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.884	43.1	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.417	-4.25
psSAR10g	0.275	-3.57
Peak SAR (Extrapolated)	0.618	-2.14
psAPD (4.0 cm², sq)	N/A	N/A

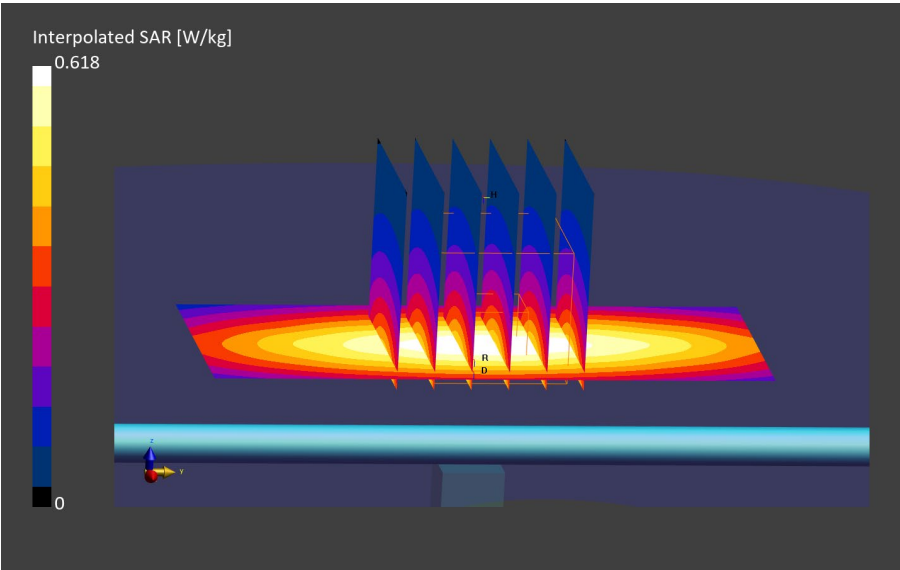

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.51, 9.27,10.14

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-06	23.1	21.9	17.0.0.6455	Twin-SAM V8.0 – 2158	Head Simulating Liquid	0.885	43.1	EX3DV4 – SN7836, 2025-09-15	DAE4ip Sn1839, 2025-09-15

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.404	-7.24
psSAR10g	0.267	-6.37
Peak SAR (Extrapolated)	0.606	-4.04
psAPD (4.0 cm², sq)	N/A	N/A

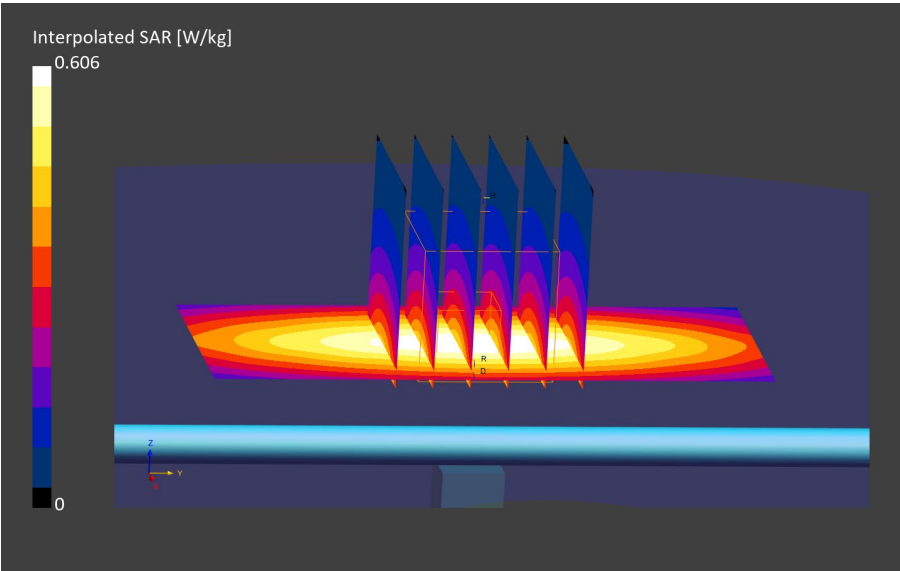

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.51, 9.27,10.14

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-22	22.4	22.3	17.0.0.6455	Twin-SAM V8.0 – 2158	Head Simulating Liquid	0.884	41.8	EX3DV4 – SN7836, 2025-09-15	DAE4ip Sn1839, 2025-09-15

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.399	-8.39
psSAR10g	0.264	-7.43
Peak SAR (Extrapolated)	0.593	-6.1
psAPD (4.0 cm², sq)	N/A	N/A

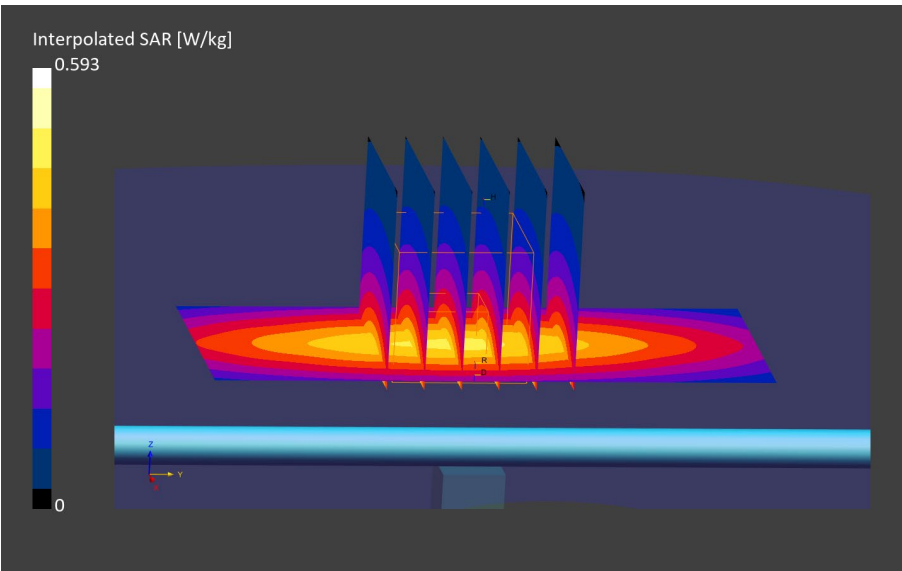

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.29, 8.95, 8.92

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-12-07	21.1	20.9	17.0.0.6455	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.859	42.5	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.422	-3.11
psSAR10g	0.278	-2.52
Peak SAR (Extrapolated)	0.619	-1.98
psAPD (4.0 cm², sq)	N/A	N/A

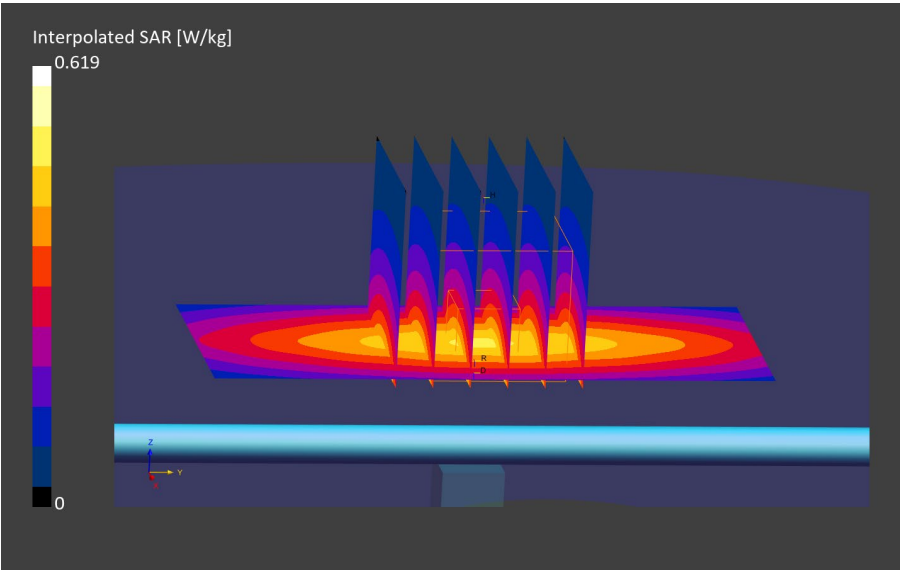

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.21, 8.83, 8.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-09	21.5	21.3	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.912	41.8	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.498	1.19
psSAR10g	0.326	2.11
Peak SAR (Extrapolated)	0.758	7.26
psAPD (4.0 cm², sq)	N/A	N/A

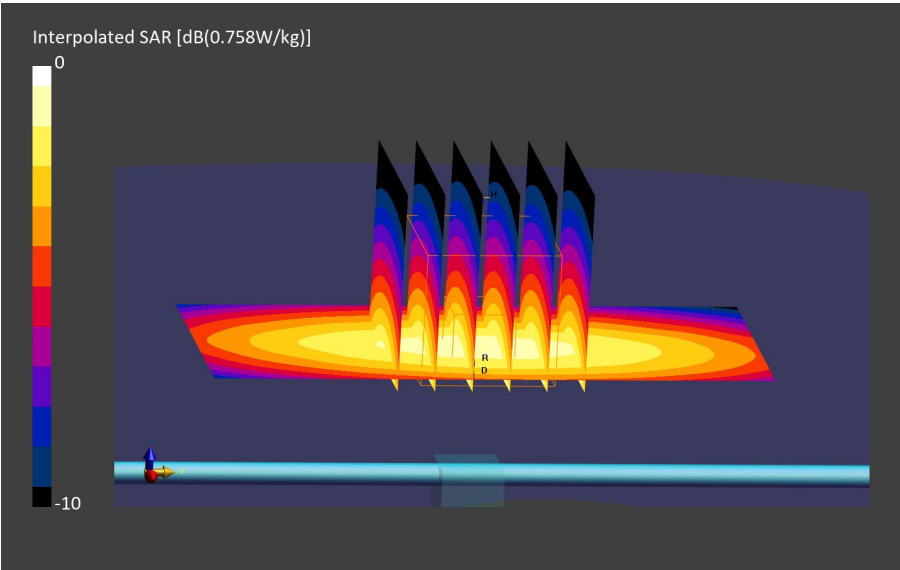

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 9.79,8.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-19	23.2	21.7	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.919	42.4	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.502	2
psSAR10g	0.330	3.37
Peak SAR (Extrapolated)	0.770	8.96
psAPD (4.0 cm², sq)	N/A	N/A

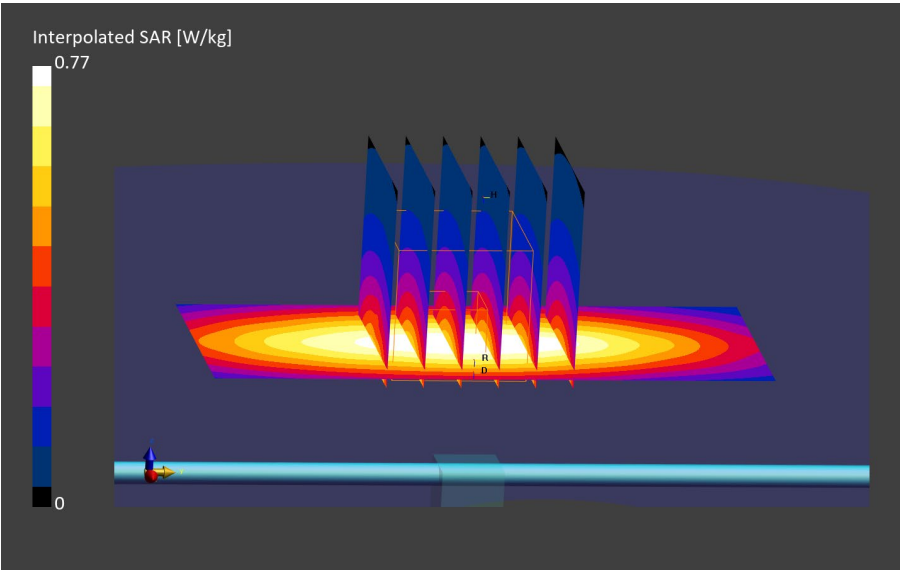

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.21, 8.83, 8.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-22	22.3	20.6	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	0.906	43.8	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.505	2.61
psSAR10g	0.331	3.68
Peak SAR (Extrapolated)	0.764	8.11
psAPD (4.0 cm², sq)	N/A	N/A

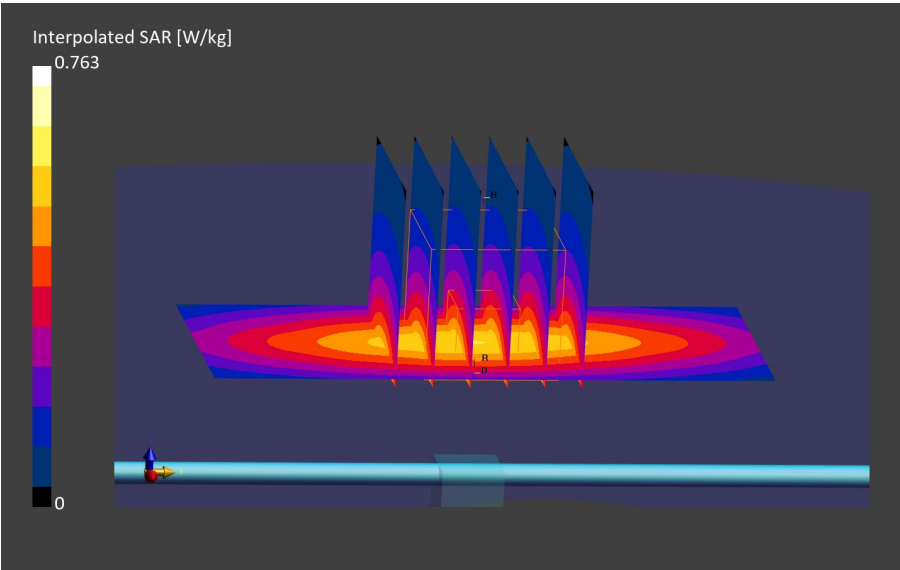

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 9.79,8.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-13	21.9	21	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.900	45.5	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 42.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.509	3.42
psSAR10g	0.336	5.24
Peak SAR (Extrapolated)	0.758	7.26
psAPD (4.0 cm², sq)	N/A	N/A

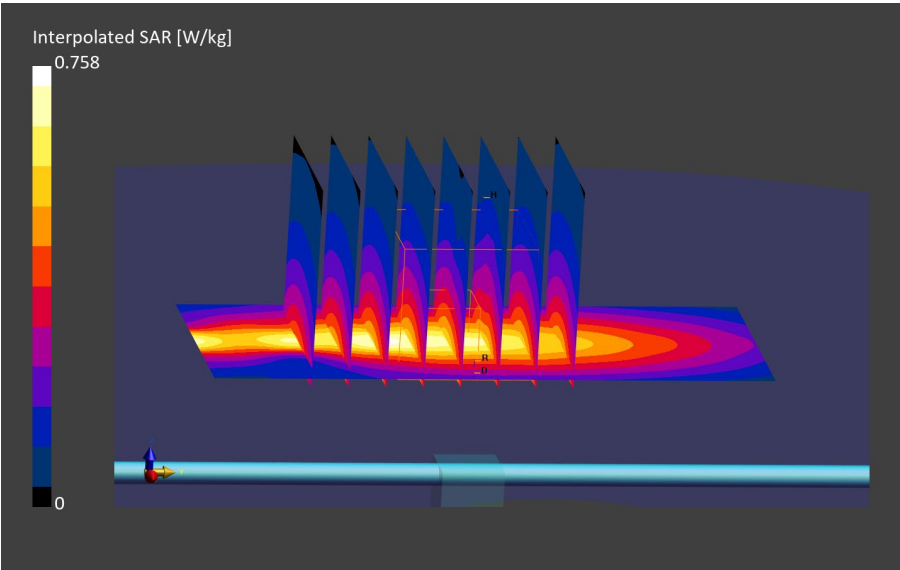

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 9.79,8.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-16	21.7	22	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.904	45.3	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.511	3.83
psSAR10g	0.333	4.3
Peak SAR (Extrapolated)	0.771	9.1
psAPD (4.0 cm², sq)	N/A	N/A

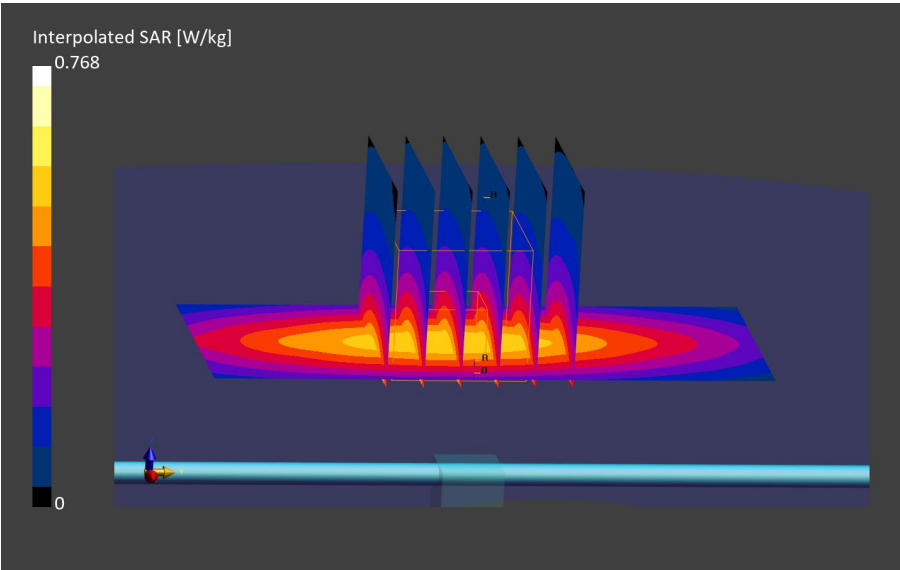

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 9.79, 8.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-19	22.6	20.7	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.919	43.9	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.506	2.81
psSAR10g	0.329	3.05
Peak SAR (Extrapolated)	0.778	10.09
psAPD (4.0 cm², sq)	N/A	N/A

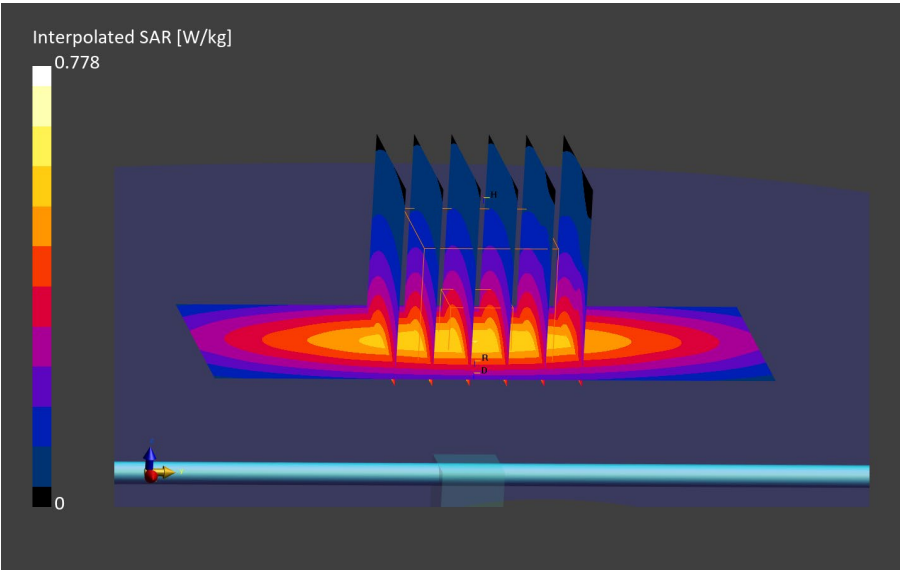

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D835V2 – SN4d311	17.0	Flat	15	CW, 0	835.000	9.05, 9.79, 8.99

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-24	22.8	21.8	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	0.915	41.0	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.497	0.98
psSAR10g	0.326	2.11
Peak SAR (Extrapolated)	0.787	11.37
psAPD (4.0 cm², sq)	N/A	N/A

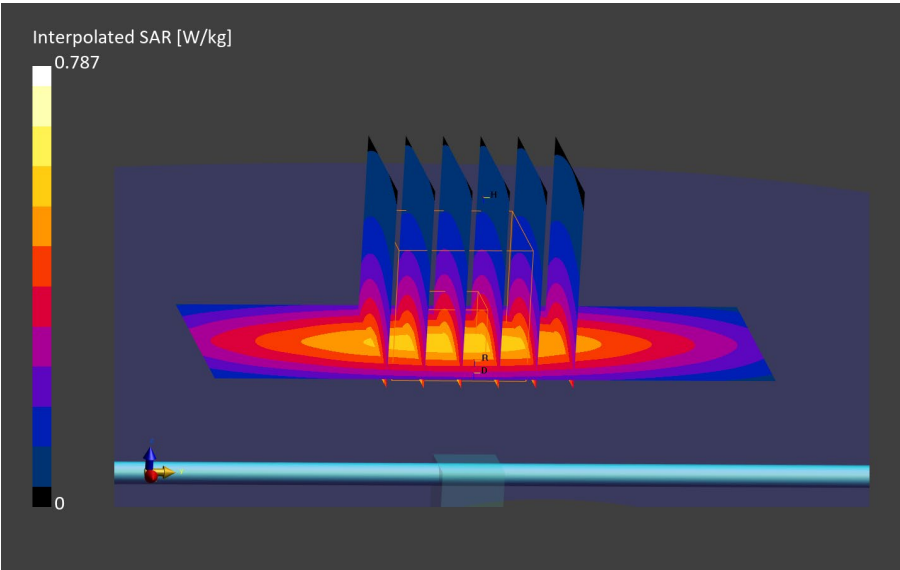

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1640V2 – SN356	17.0	Flat	10	CW, 0	1640.000	7.8, 8.44,7.75

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-05	23	21.2	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.31	43.7	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.72	0.35
psSAR10g	0.941	0.94
Peak SAR (Extrapolated)	3.04	0.42
psAPD (4.0 cm², sq)	N/A	N/A

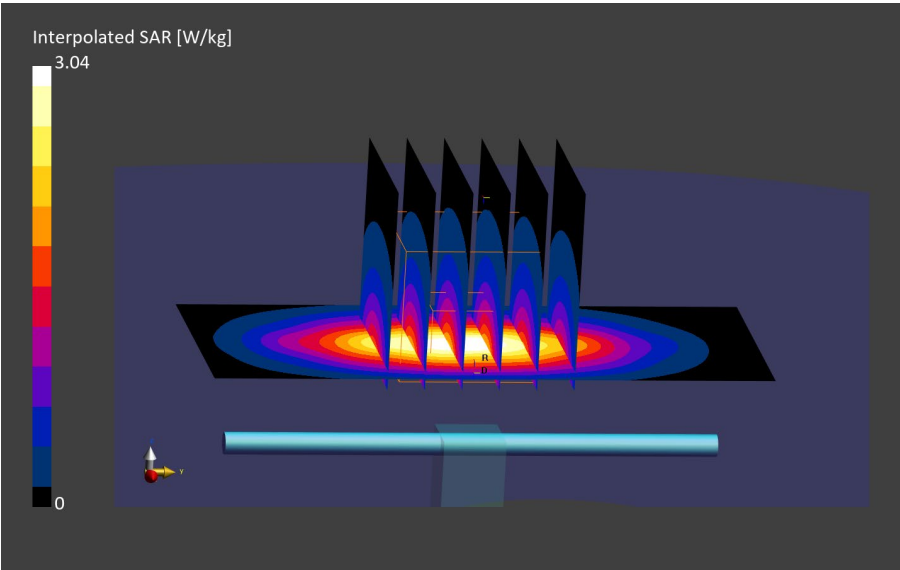

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.52, 7.93,7.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-10	22.6	22.5	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.38	39.9	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.74	-4.88
psSAR10g	0.935	-2.83
Peak SAR (Extrapolated)	2.99	-8.08
psAPD (4.0 cm², sq)	N/A	N/A

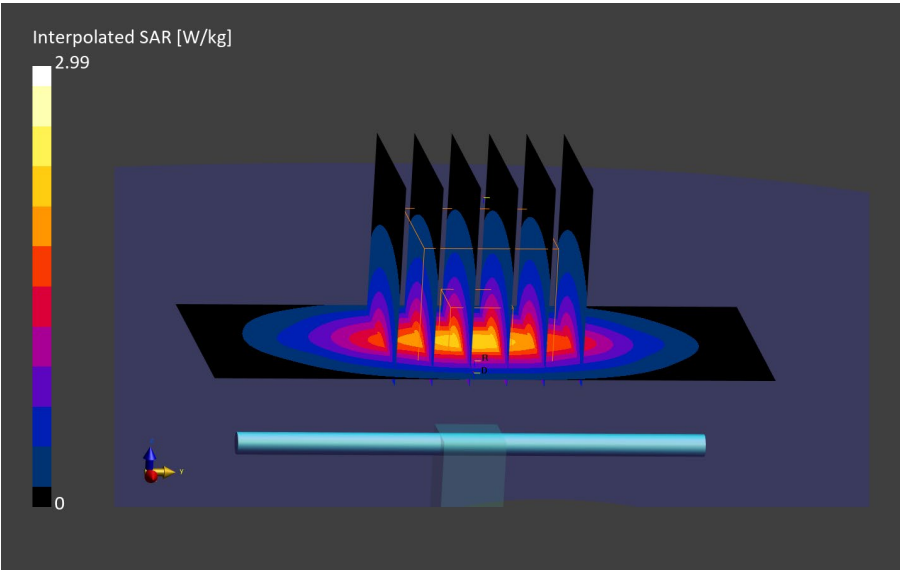

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.52, 7.93,7.47

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-14	23.9	22.9	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.38	39.4	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.73	-5.43
psSAR10g	0.931	-3.25
Peak SAR (Extrapolated)	2.98	-8.38
psAPD (4.0 cm², sq)	N/A	N/A

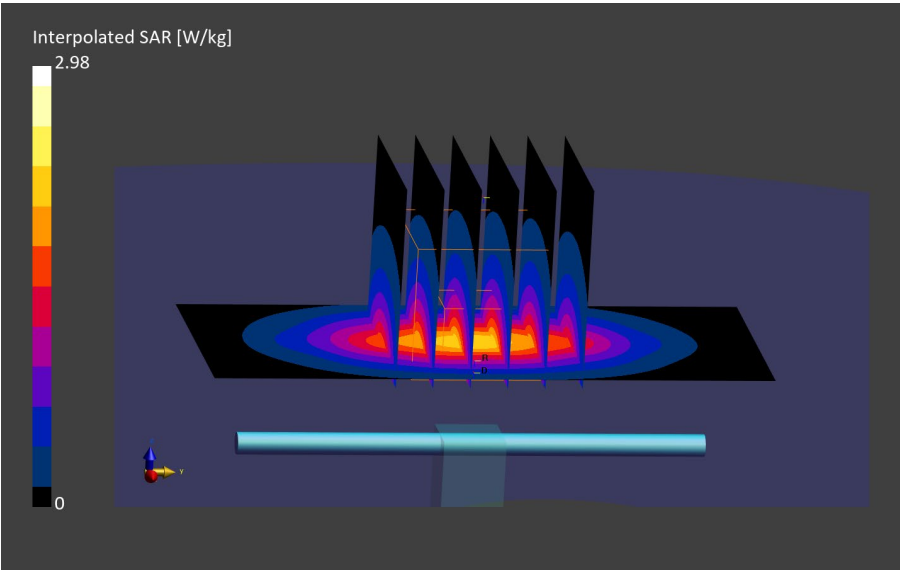

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.8, 7.6, 8.31

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-23	22.8	22	17.0.0.6455	Twin-SAM V8.0 – 2158	Head Simulating Liquid	1.33	39.4	EX3DV4 – SN7836, 2025-09-15	DAE4ip Sn1838, 2024-12-04

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.78	-2.7
psSAR10g	0.951	-1.17
Peak SAR (Extrapolated)	3.21	-1.31
psAPD (4.0 cm², sq)	N/A	N/A

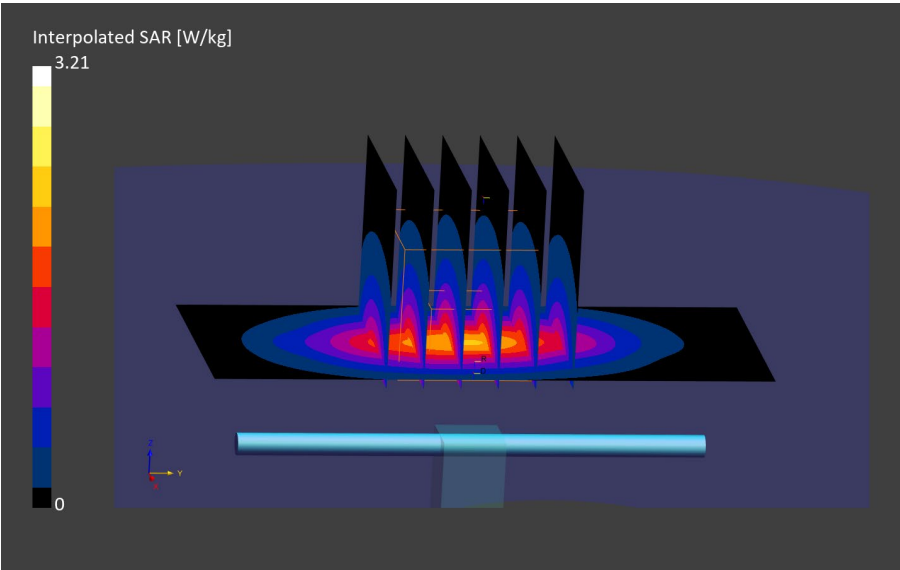

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.09, 7.69, 7.42

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-24	23	21.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.36	40.6	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.76	-3.79
psSAR10g	0.937	-2.63
Peak SAR (Extrapolated)	3.24	-0.39
psAPD (4.0 cm², sq)	N/A	N/A

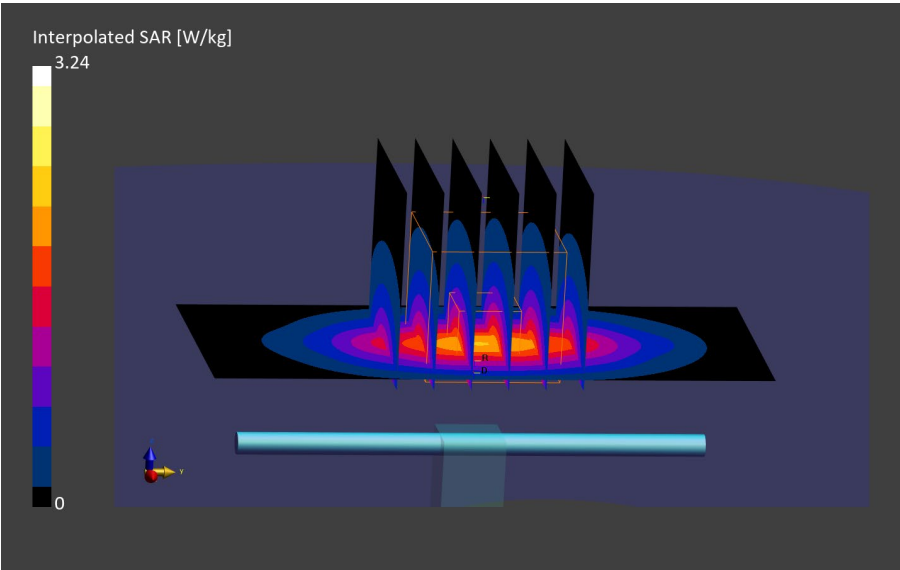

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.09, 7.69, 7.42

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-28	20.6	21.4	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.35	39.6	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.85	1.13
psSAR10g	0.989	2.78
Peak SAR (Extrapolated)	3.32	2.07
psAPD (4.0 cm², sq)	N/A	N/A

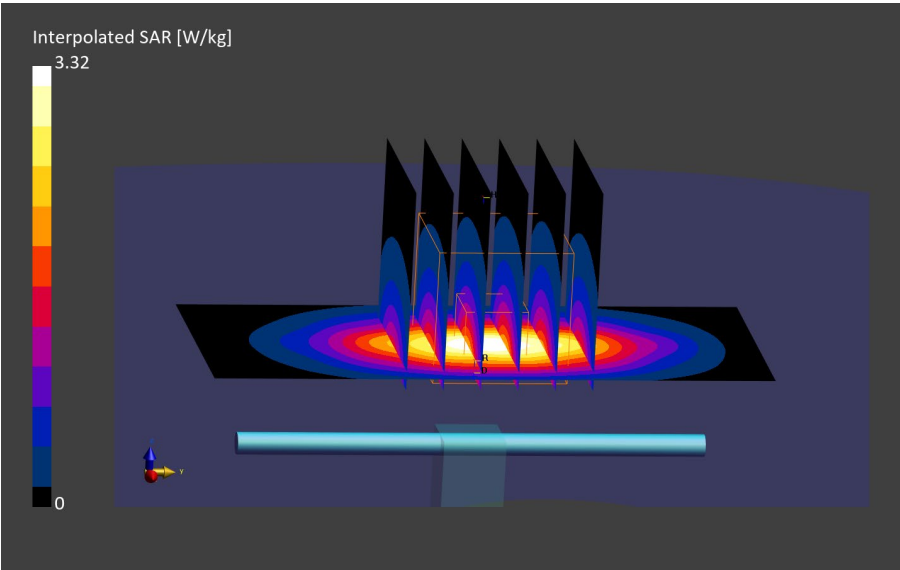

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.67, 8.3,7.63

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-27	24.3	22.2	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.38	40.0	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.86	1.68
psSAR10g	0.996	3.5
Peak SAR (Extrapolated)	3.35	2.99
psAPD (4.0 cm², sq)	N/A	N/A

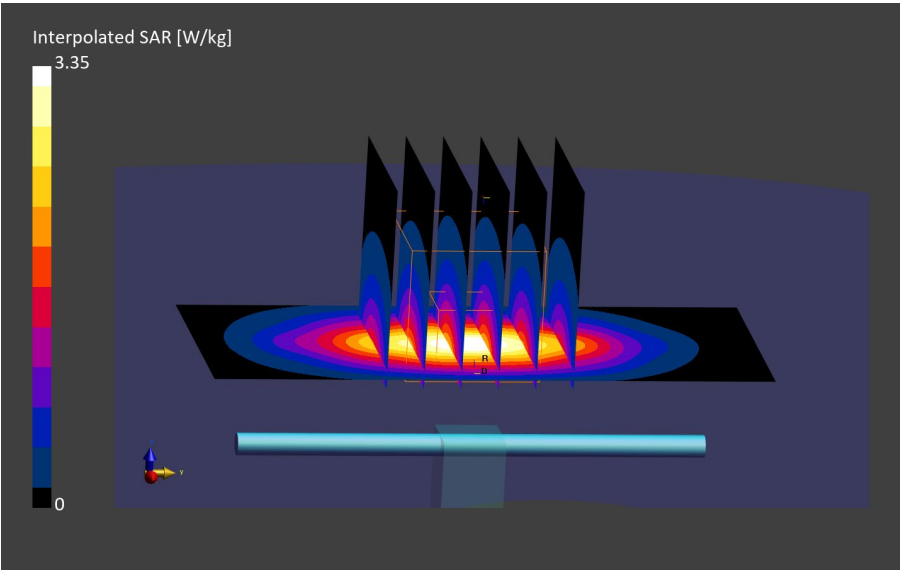

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.09, 7.69,7.42

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-05	22.5	21.6	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.34	38.9	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.84	0.58
psSAR10g	0.988	2.67
Peak SAR (Extrapolated)	3.42	5.14
psAPD (4.0 cm², sq)	N/A	N/A

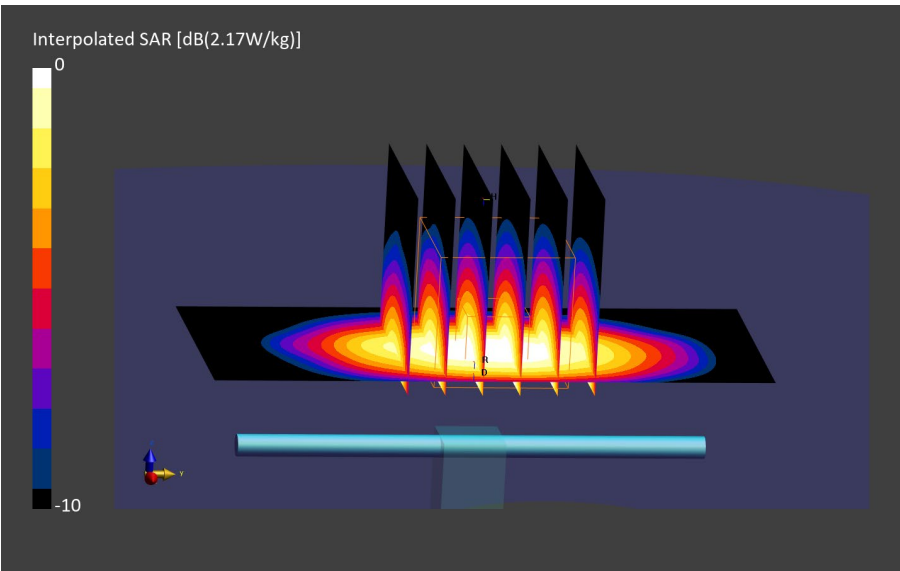

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.26, 7.65, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-10	22.6	22.2	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.47	39.7	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.89	-5.25
psSAR10g	1.00	-4.99
Peak SAR (Extrapolated)	3.31	-8.4
psAPD (4.0 cm², sq)	N/A	N/A

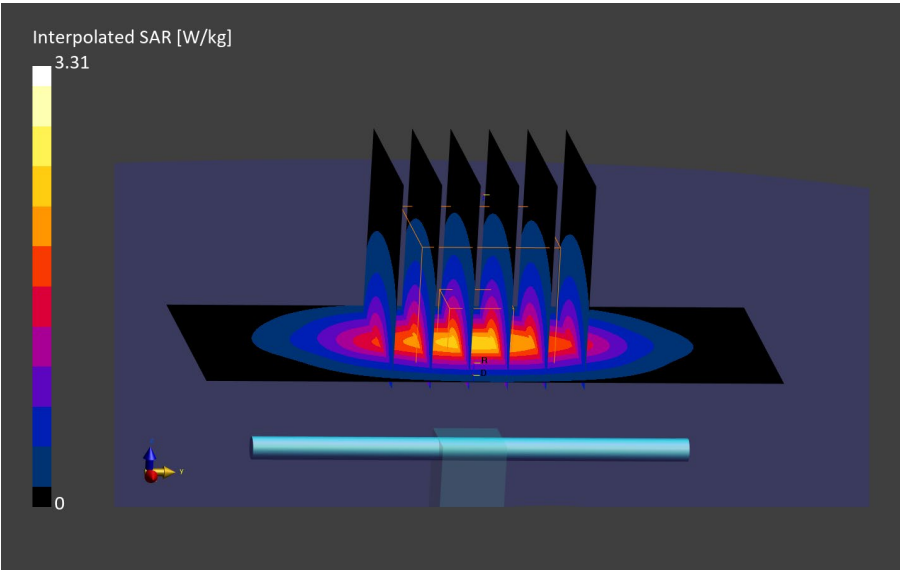

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.26, 7.65, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-12	23.7	21.9	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.44	38.4	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.92	-3.75
psSAR10g	1.01	-4.04
Peak SAR (Extrapolated)	3.36	-7.02
psAPD (4.0 cm², sq)	N/A	N/A

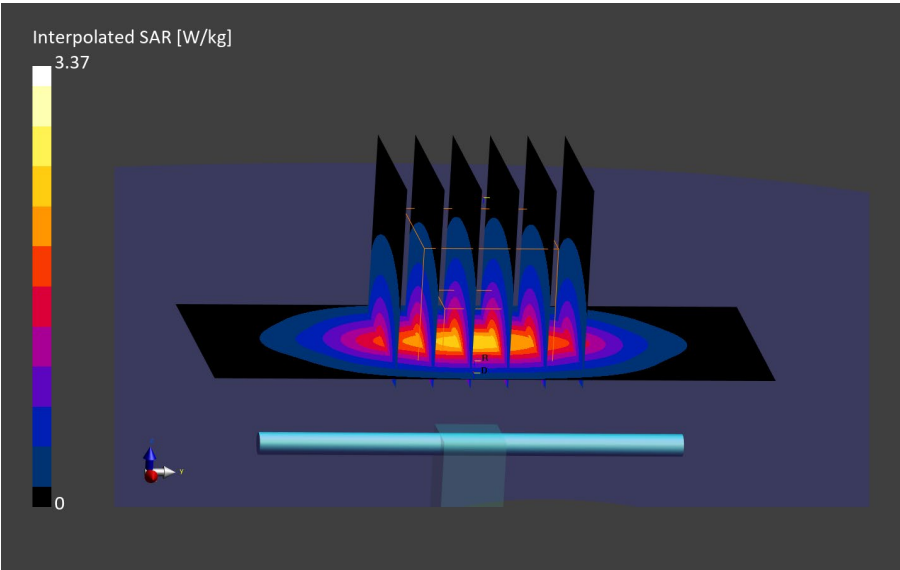

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.54, 8.16, 7.5

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-21	22.5	21.3	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.42	38.6	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.01	0.77
psSAR10g	1.04	-1.19
Peak SAR (Extrapolated)	3.72	2.95
psAPD (4.0 cm², sq)	N/A	N/A



RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	6.86, 7.44, 7.18

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-28	20.6	21.4	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.43	39.4	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.04	2.27
psSAR10g	1.07	1.66
Peak SAR (Extrapolated)	3.75	3.78
psAPD (4.0 cm², sq)	N/A	N/A

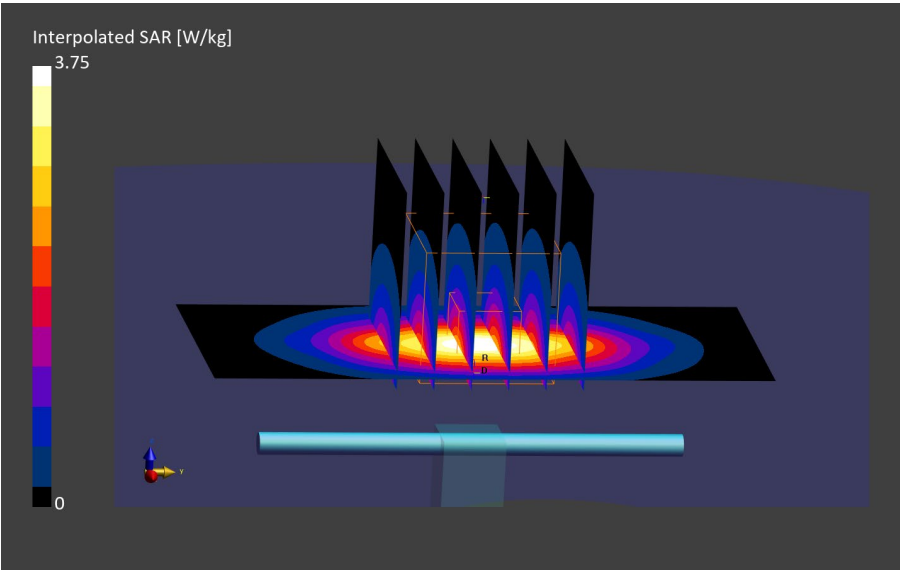

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.26, 7.65, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-16	21.7	22.3	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.43	40.8	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.90	-4.75
psSAR10g	1.00	-4.99
Peak SAR (Extrapolated)	3.30	-8.68
psAPD (4.0 cm², sq)	N/A	N/A

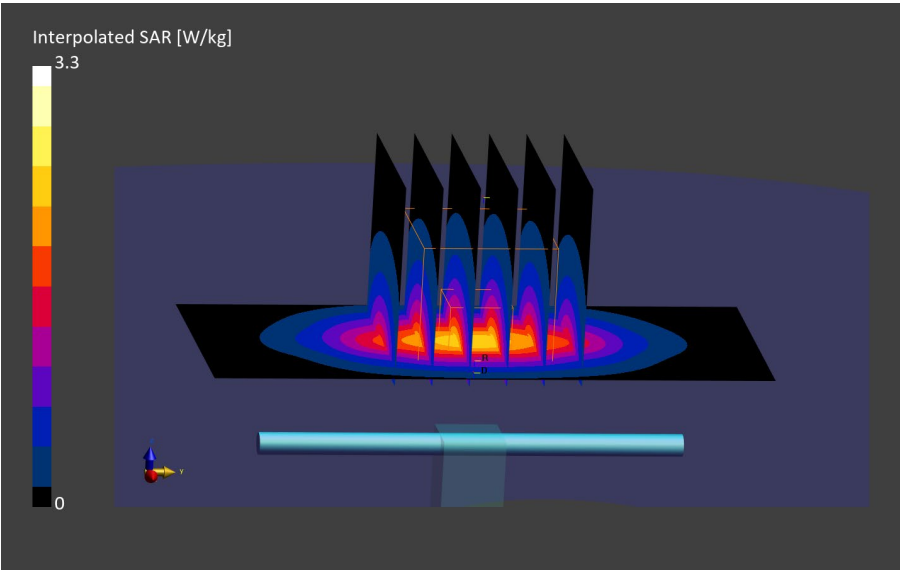

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2300V2 – SN1139	17.0	Flat	10	CW, 0	2300.000	7.02, 7.4,6.97

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-11	23.5	21.9	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.71	38.5	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.34	-4.72
psSAR10g	1.13	-4.87
Peak SAR (Extrapolated)	4.43	-4.75
psAPD (4.0 cm², sq)	N/A	N/A

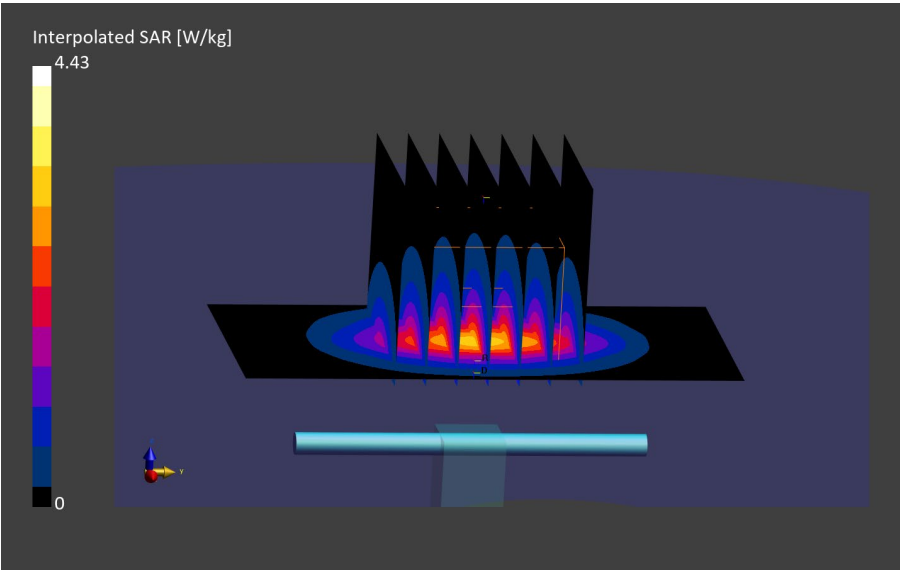

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2300V2 – SN1139	17.0	Flat	10	CW, 0	2300.000	7.02, 7.4,6.97

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-23	23.7	23	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.69	40.3	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.23	-9.2
psSAR10g	1.08	-9.08
Peak SAR (Extrapolated)	4.25	-8.62
psAPD (4.0 cm², sq)	N/A	N/A

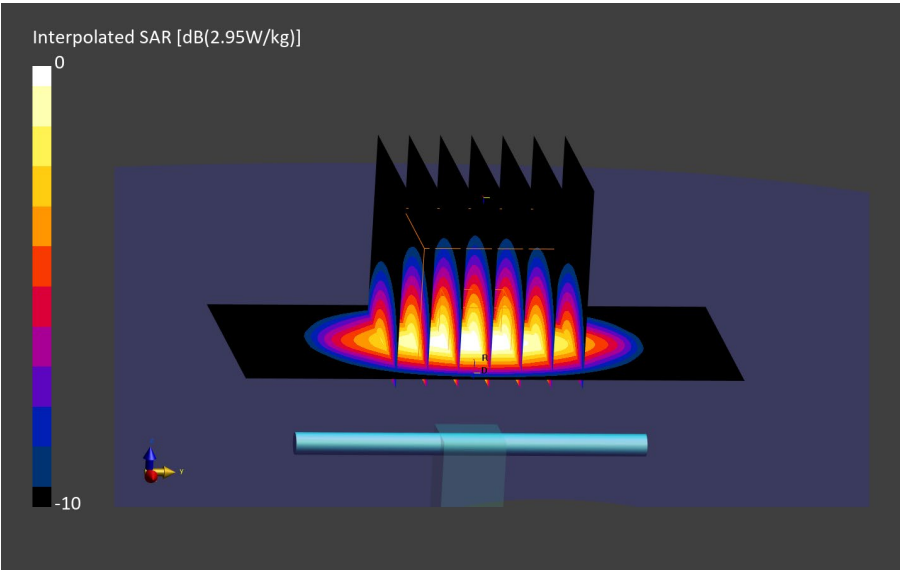

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.72, 7.08, 6.68

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-26	22.2	21.2	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.93	38.6	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.58	1.73
psSAR10g	1.19	0.18
Peak SAR (Extrapolated)	5.18	-0.81
psAPD (4.0 cm², sq)	N/A	N/A

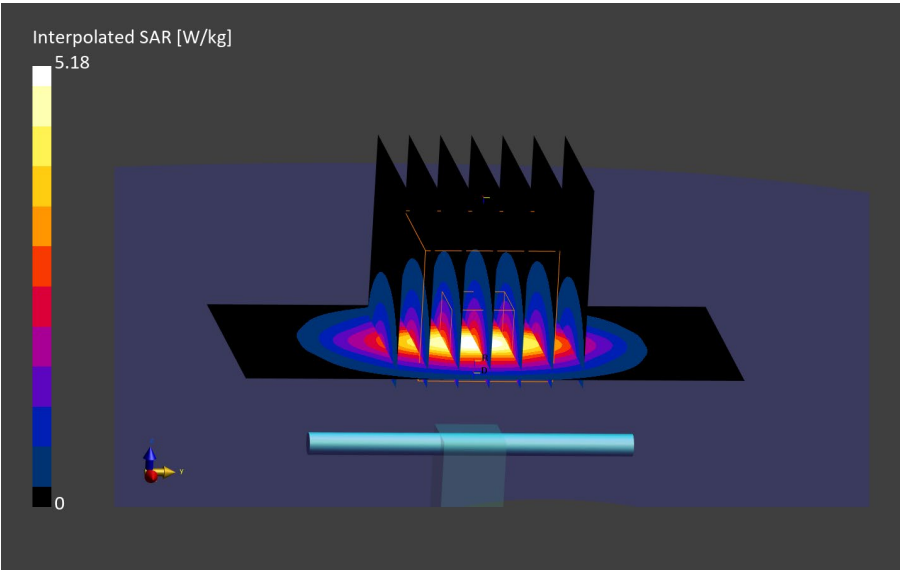

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.72, 7.08,6.68

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-06	22.4	21.9	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.84	40.5	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.46	-3
psSAR10g	1.16	-2.34
Peak SAR (Extrapolated)	4.80	-8.09
psAPD (4.0 cm², sq)	N/A	N/A

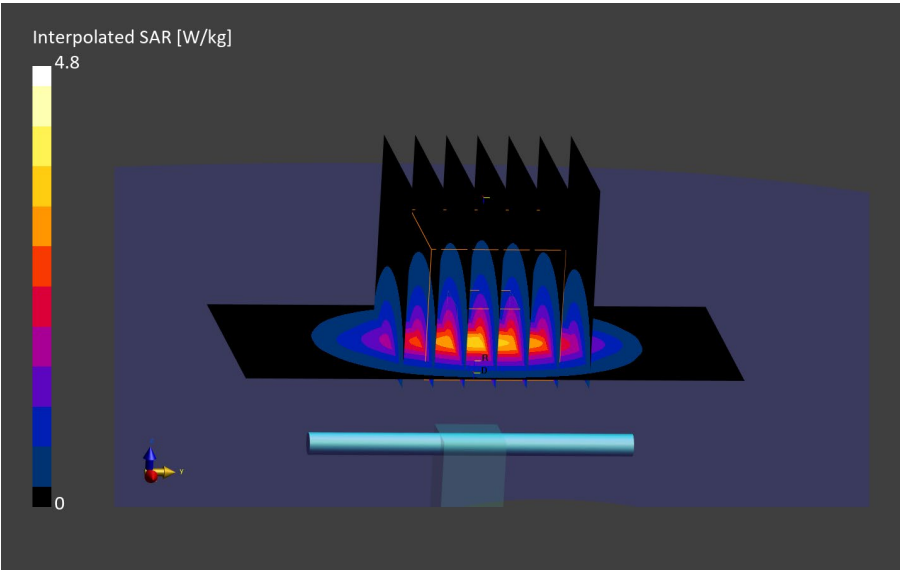

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.72, 7.08, 6.68

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-18	22.5	22.2	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.83	38.7	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.49	-1.81
psSAR10g	1.18	-0.66
Peak SAR (Extrapolated)	4.88	-6.56
psAPD (4.0 cm², sq)	N/A	N/A

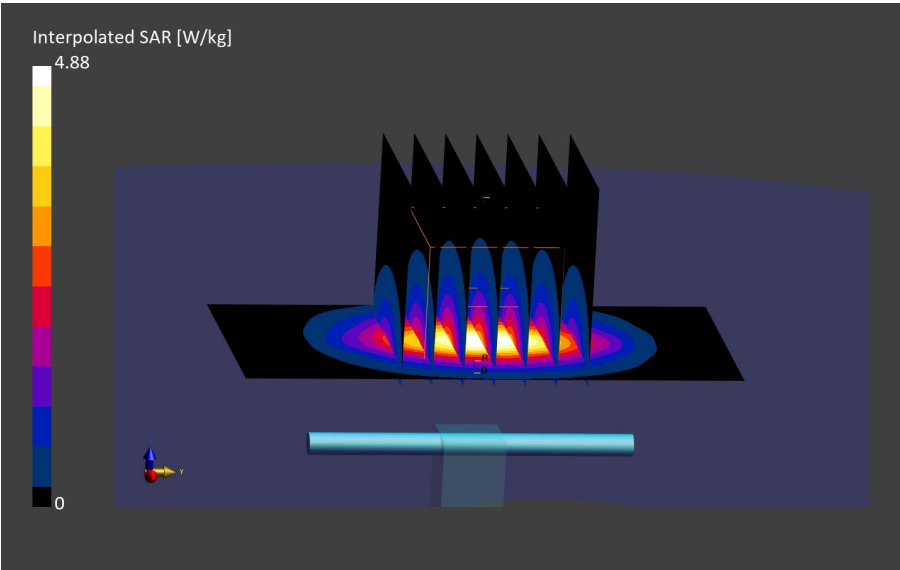

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.82, 7.38,6.78

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-14	23.7	23	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	1.96	38.8	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.76	-0.42
psSAR10g	1.24	-0.64
Peak SAR (Extrapolated)	5.89	-0.49
psAPD (4.0 cm², sq)	N/A	N/A

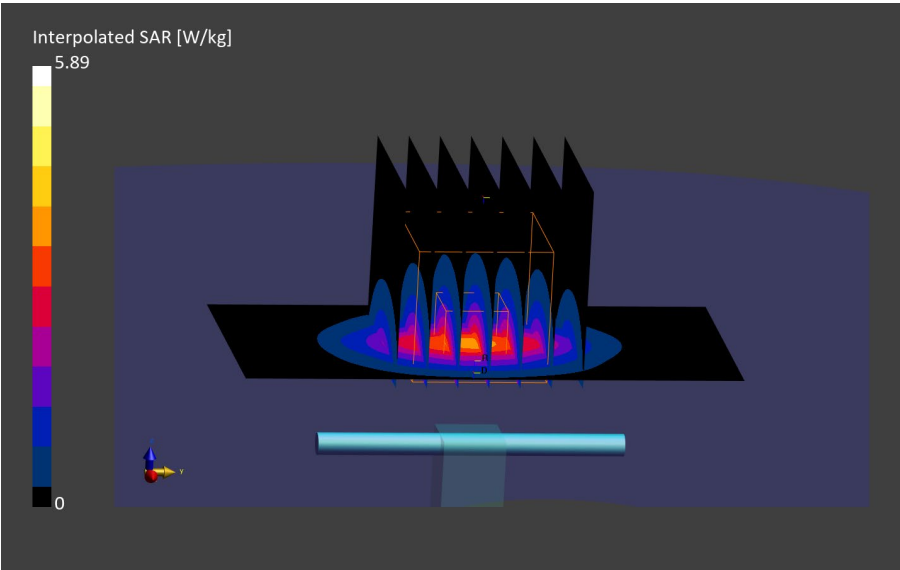

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.78, 7.14, 6.73

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-23	23.7	23	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	2.02	39.3	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.82	1.75
psSAR10g	1.28	2.57
Peak SAR (Extrapolated)	5.67	-4.21
psAPD (4.0 cm², sq)	N/A	N/A

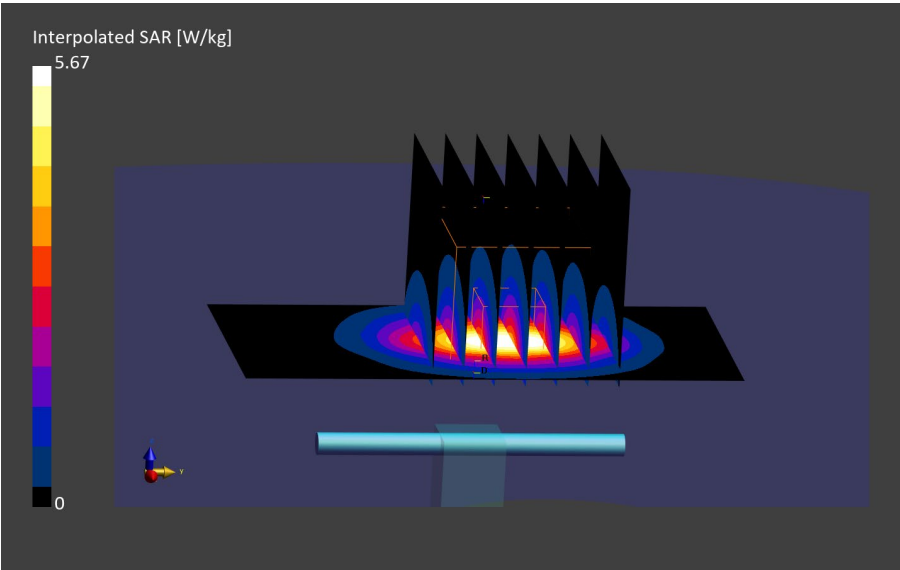

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.78, 7.14, 6.73

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-02	22.2	21.5	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	2.12	38.4	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.78	0.3
psSAR10g	1.24	-0.64
Peak SAR (Extrapolated)	5.84	-1.34
psAPD (4.0 cm², sq)	N/A	N/A

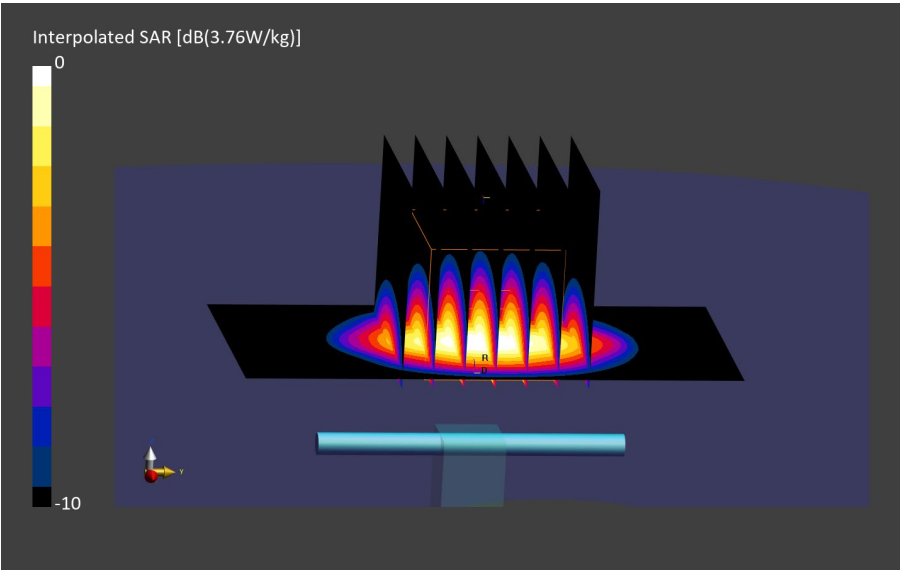

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.72, 7.29, 7.04

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-09	22.3	22.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.93	39.5	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.57	-7.27
psSAR10g	1.15	-7.85
Peak SAR (Extrapolated)	5.39	-8.94
psAPD (4.0 cm², sq)	N/A	N/A

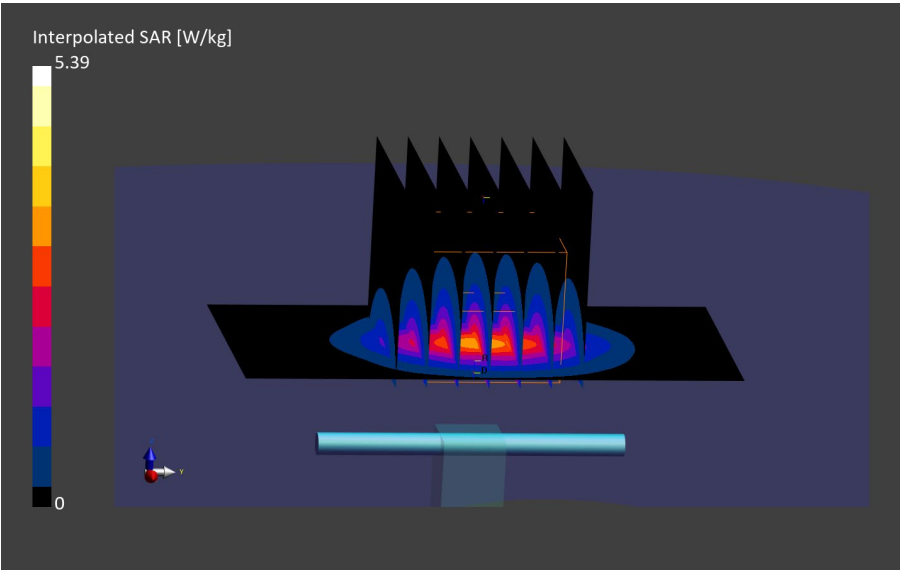

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.72, 7.29, 7.04

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-17	22.7	21.5	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.91	37.8	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.67	-3.66
psSAR10g	1.20	-3.84
Peak SAR (Extrapolated)	5.66	-4.38
psAPD (4.0 cm², sq)	N/A	N/A

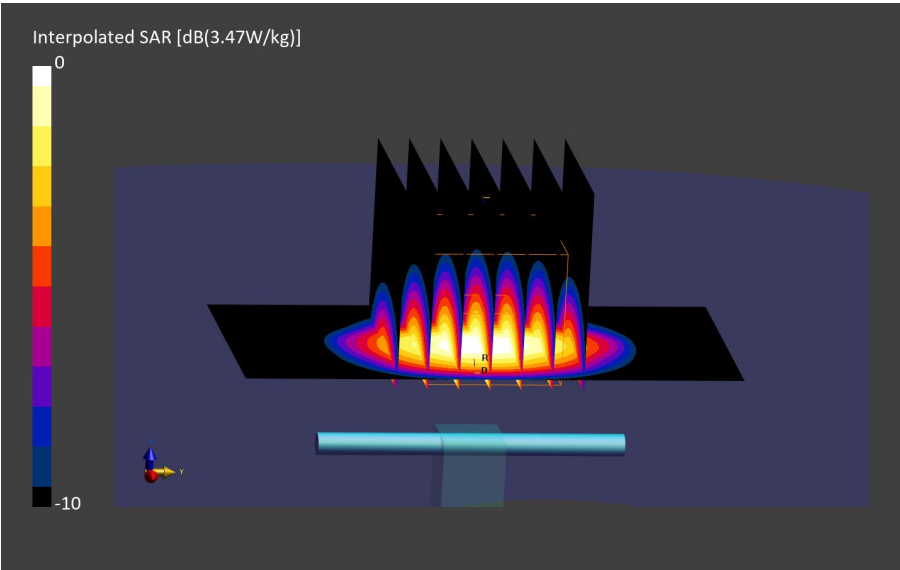

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2600V2 – SN1215	17.0	Flat	10	CW, 0	2600.000	6.78, 7.14, 6.73

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-12-05	24.9	22.7	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	1.95	42.0	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.72	-1.86
psSAR10g	1.24	-0.64
Peak SAR (Extrapolated)	5.28	-10.8
psAPD (4.0 cm², sq)	N/A	N/A

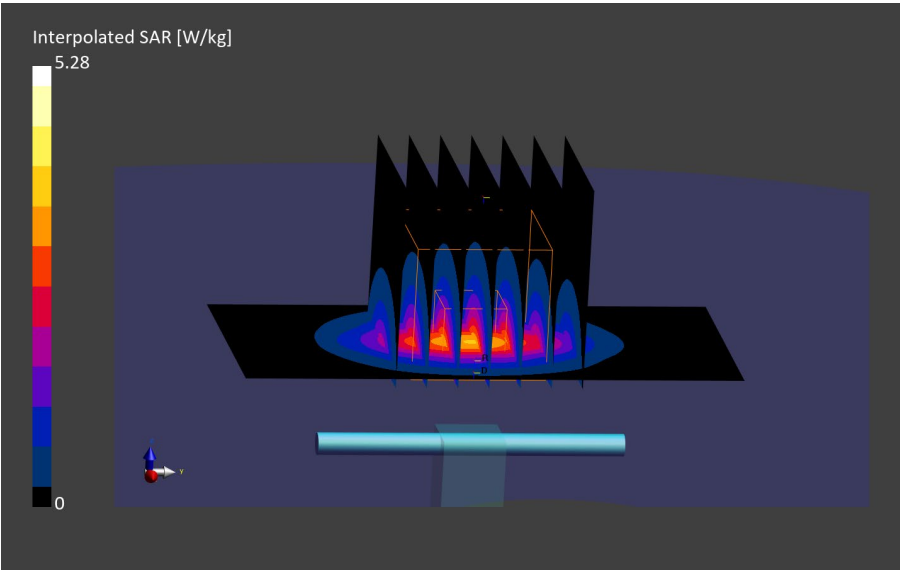

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.36, 6.09, 5.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-17	23.7	21.9	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.67	36.7	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.20	-1.92
psSAR10g	1.21	-1.86
Peak SAR (Extrapolated)	8.06	-4.78
psAPD (4.0 cm², sq)	N/A	N/A

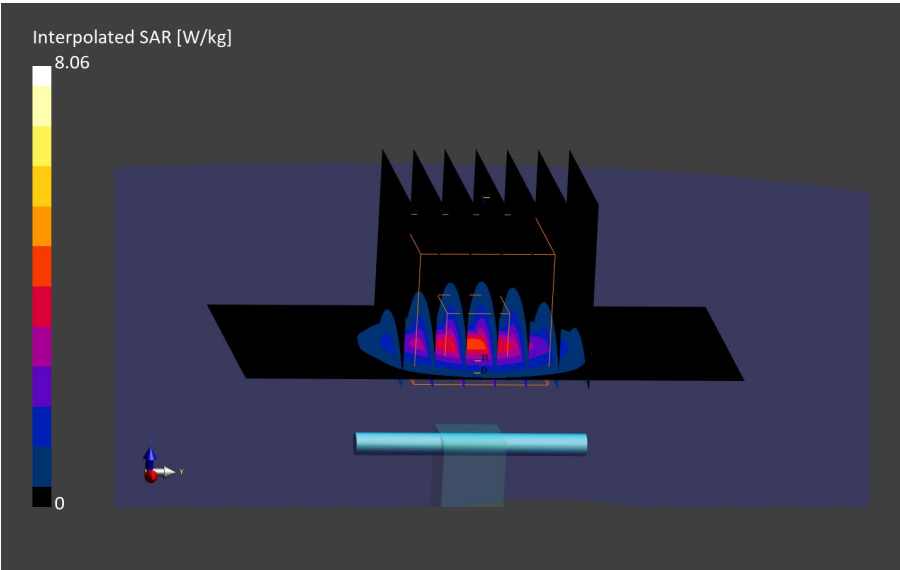

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.36, 6.09, 5.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-19	22.8	21.3	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.77	39.5	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.14	-3.76
psSAR10g	1.20	-2.67
Peak SAR (Extrapolated)	7.77	-8.21
psAPD (4.0 cm², sq)	N/A	N/A

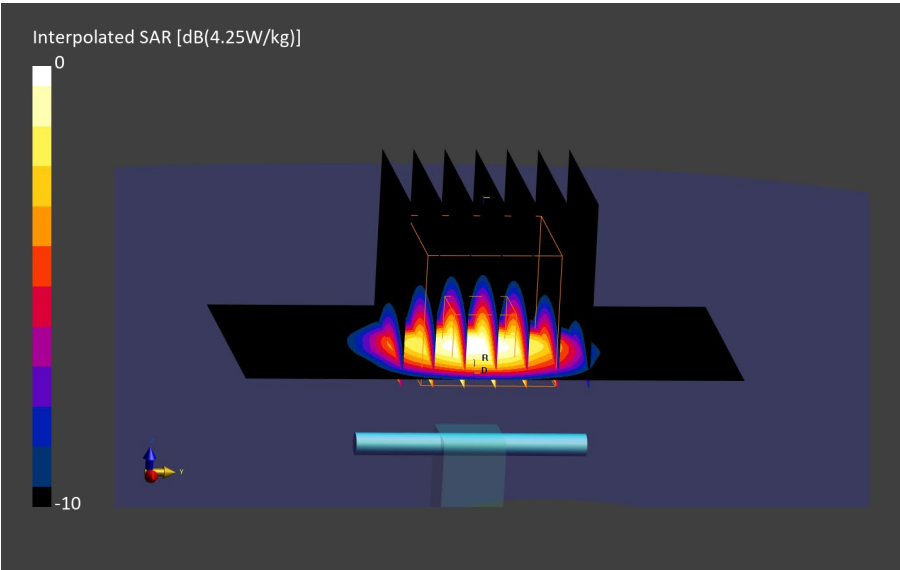

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.36, 6.09, 5.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-21	22	22.1	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.78	40.1	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.09	-5.29
psSAR10g	1.18	-4.29
Peak SAR (Extrapolated)	7.88	-6.91
psAPD (4.0 cm², sq)	N/A	N/A

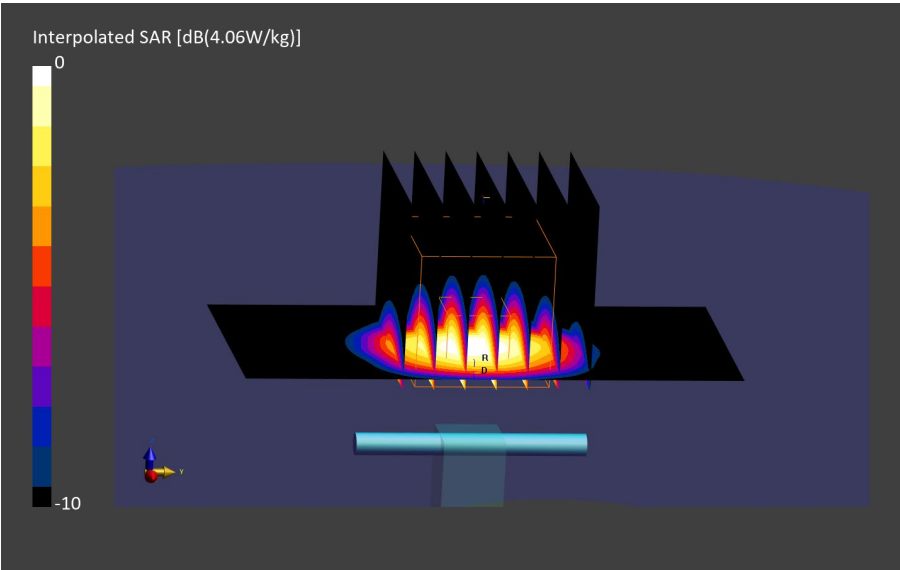

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.36, 6.09, 5.9

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-09	22.3	20.6	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.78	39.3	EX3DV4 – SN7853, 2024-11-07	DAE4ip Sn1844, 2024-11-06

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.20	-1.92
psSAR10g	1.21	-1.86
Peak SAR (Extrapolated)	8.06	-4.78
psAPD (4.0 cm², sq)	N/A	N/A

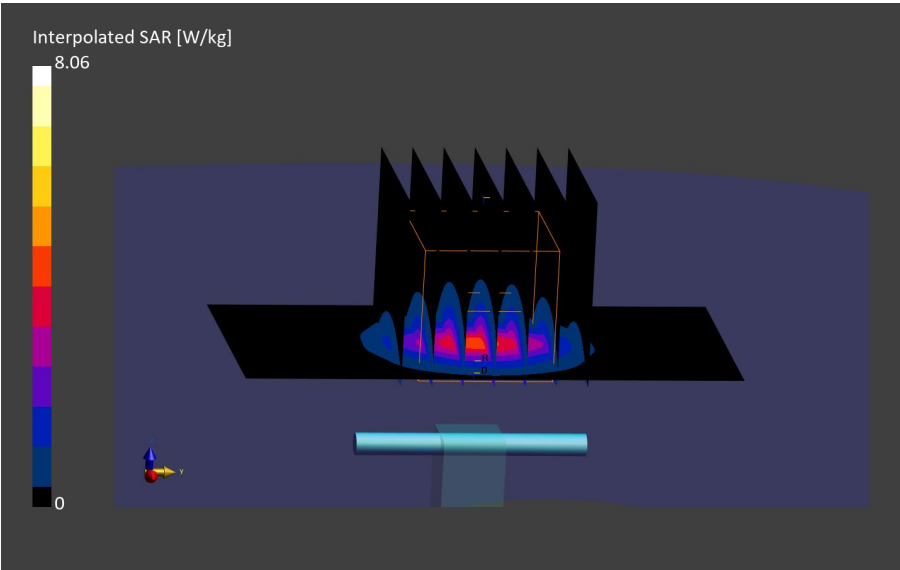

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3500V2 – SN1154	17.0	Flat	10	CW, 0	3500.000	6.13, 6.65,6.41

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-21	22.4	20.8	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.79	38.2	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.13	-4.07
psSAR10g	1.19	-3.48
Peak SAR (Extrapolated)	7.97	-5.85
psAPD (4.0 cm², sq)	N/A	N/A

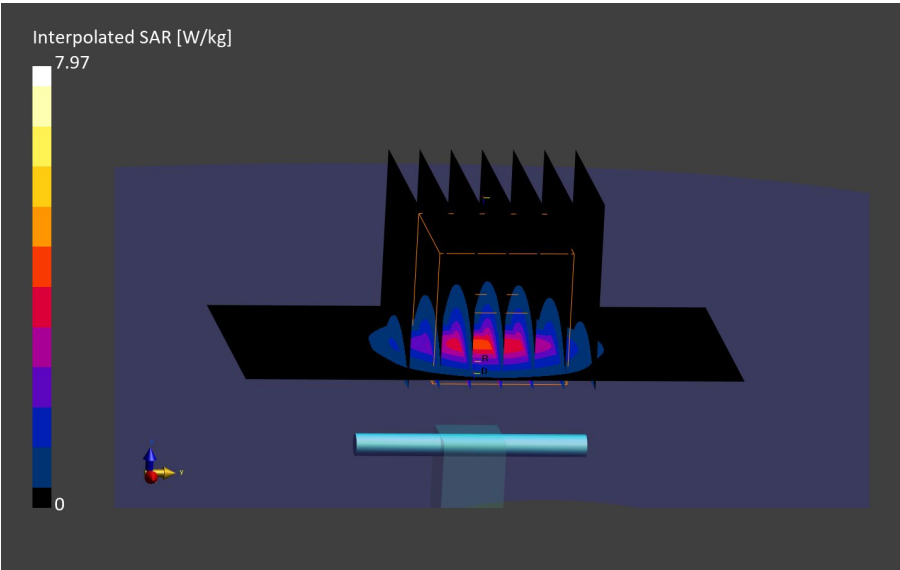

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3700V2 – SN1130	17.0	Flat	10	CW, 0	3700.000	5.89, 6.38,6.16

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-21	22.4	20.8	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	2.97	37.8	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.25	-2.63
psSAR10g	1.21	-1.46
Peak SAR (Extrapolated)	8.58	-2.56
psAPD (4.0 cm², sq)	N/A	N/A

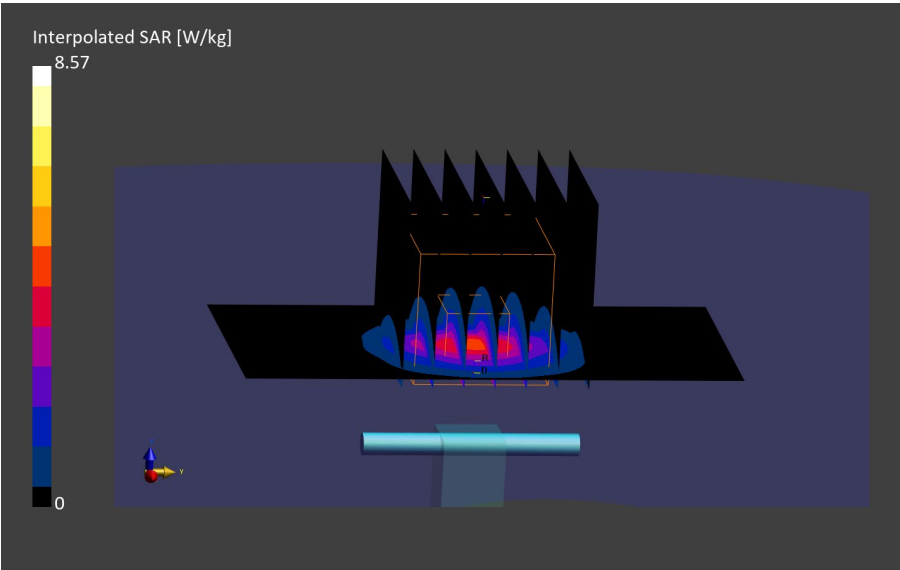

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D3900V2 – SN1101	17.0	Flat	10	CW, 0	3900.000	5.79, 6.28,6.06

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-21	22.4	20.8	16.4.0.5005	Twin-SAM V8.0 – 2164	Head Simulating Liquid	3.17	37.5	EX3DV4 – SN7857, 2024-12-10	DAE4ip Sn1862, 2025-01-16

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 29.1
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.28	-6.77
psSAR10g	1.15	-6.73
Peak SAR (Extrapolated)	9.21	-5.03
psAPD (4.0 cm², sq)	N/A	N/A

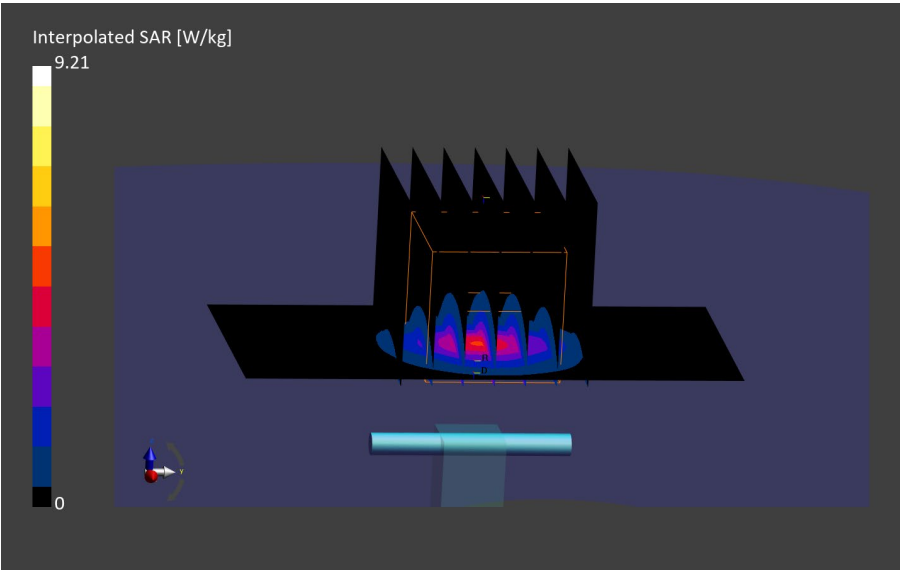

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D5GHzV2 – SN1396	17.0	Flat	10	CW, 0	5250.000	5.43, 5.87,5.39

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-09-29	22.8	22.4	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	4.47	34.1	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	32.0 x 36.0 x 22.9
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.90	-0.11
psSAR10g	1.11	-1.13
Peak SAR (Extrapolated)	15.8	1.63
psAPD (4.0 cm², sq)	N/A	N/A

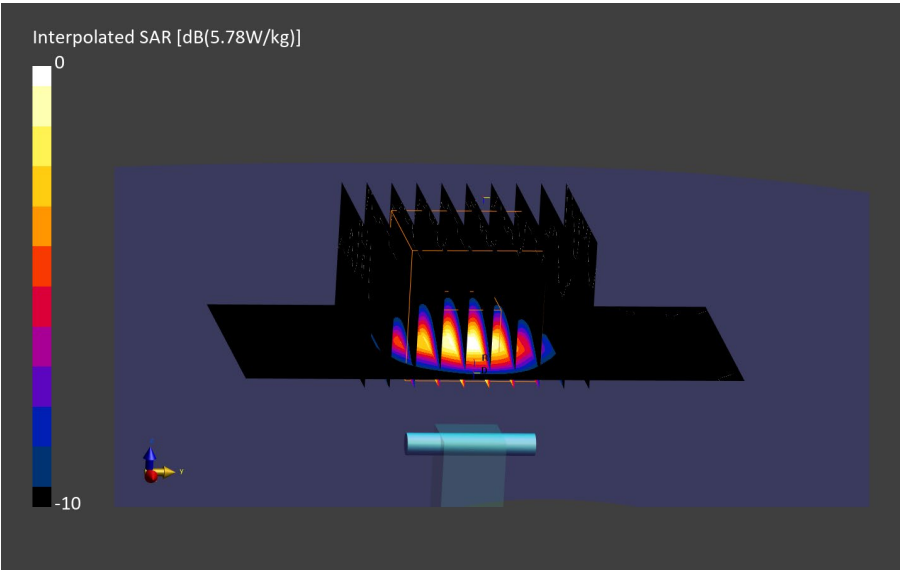

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	5.23, 5.66,5.2

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-02	21.8	21.5	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	6.42	36.0	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	27.2 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.76	-7.38
psSAR10g	0.542	-1.45
Peak SAR (Extrapolated)	17.6	-10.89
psAPD (4.0 cm², sq)	13.1	-2.2

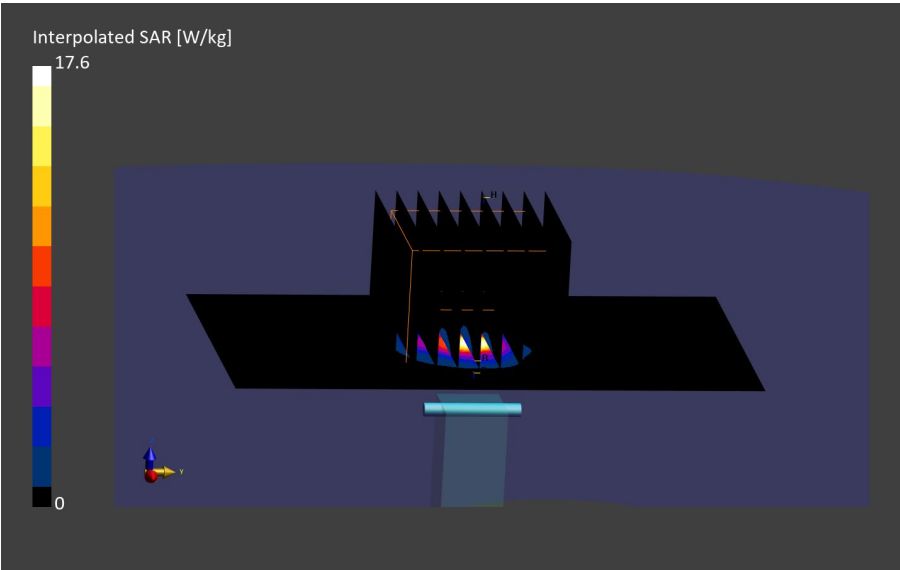

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	5.23, 5.66,5.2

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-10-07	23	20.6	16.4.0.5005	Twin-SAM V8.0 – 2165	Head Simulating Liquid	6.39	35.2	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	27.2 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.83	-5.03
psSAR10g	0.541	-1.64
Peak SAR (Extrapolated)	18.0	-8.86
psAPD (4.0 cm², sq)	13.0	-3.00

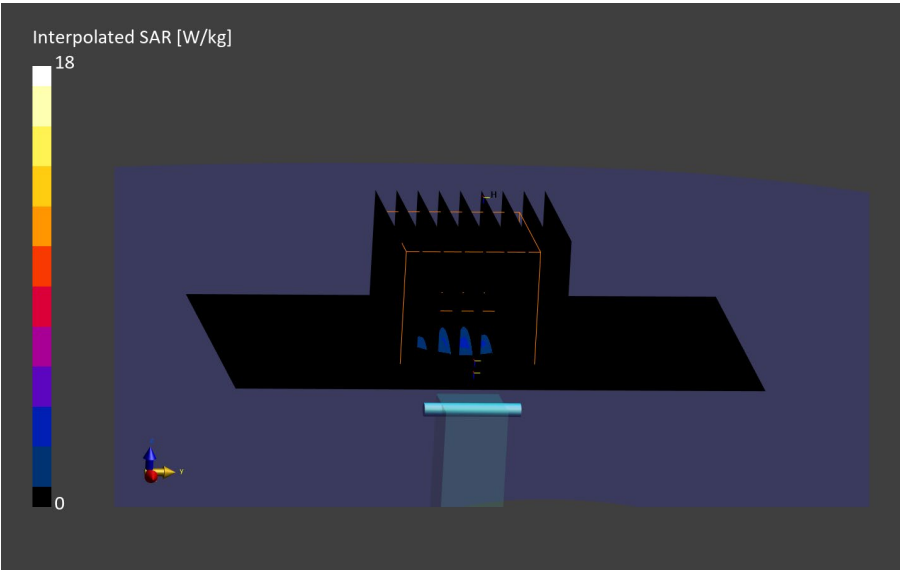

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D6.5GHzV2 – SN1104	10.0	Flat	5	CW, 0	6500.000	4.79, 5.05,4.76

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2025-11-21	22.5	21.8	16.4.0.5005	Twin-SAM V8.0 – 2159	Head Simulating Liquid	6.36	35.8	EX3DV4 – SN7859, 2025-05-05	DAE4ip Sn1905, 2025-04-25

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	51.0 x 85.0	23.8 x 27.2 x 22.9
Grid Steps [mm]	8.5 x 8.5	3.4 x 3.4 x 1.4
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.4

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	3.06	2.68
psSAR10g	0.576	4.73
Peak SAR (Extrapolated)	19.2	-2.78
psAPD (4.0 cm², sq)	13.8	3.00

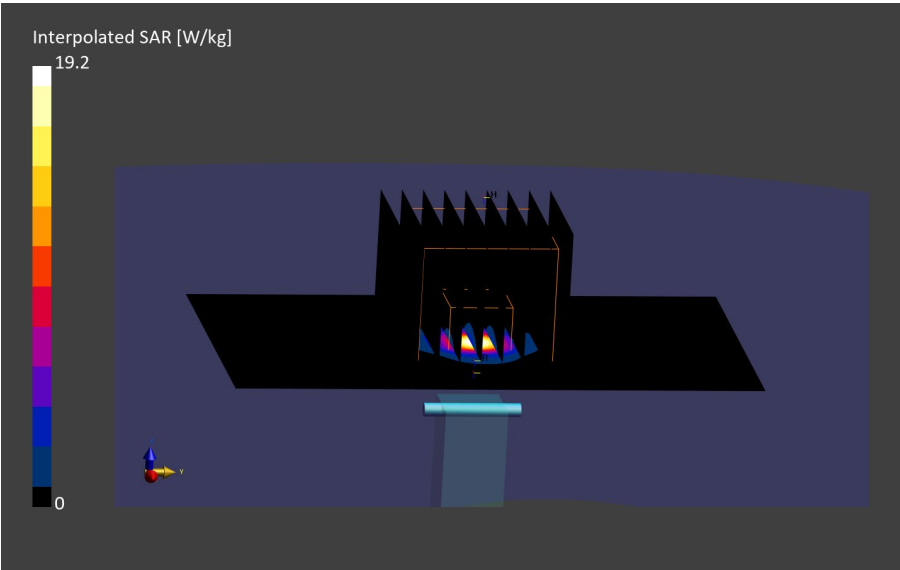

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Serial Number	Test Distance [mm]	Signal, UID	Frequency [MHz]
10 GHz System Verification	1074	10.00	CW	10000.0

Test Setup


Test Date	Measurement SW	Probe, Cal. Date	DAE, Cal. Date
2025-11-16	3.2.2.2358	EUmmWV4 – SN9690_F1–55GHz – 2025-09-17	DAE4ip Sn1839 – 2025-09-15

Scans Setup

Grid Extents [mm]	Grid Steps [lambda]	Sensor Surface Distance [mm]
60.0x60.0	0.125x0.125	10.0

Measurement Results

Averaging Area [cm²]	E _{max} [V/m]	psPDn+ [W/m²]	psPDtot+ [W/m²]
4.00	152	54.0	54.5

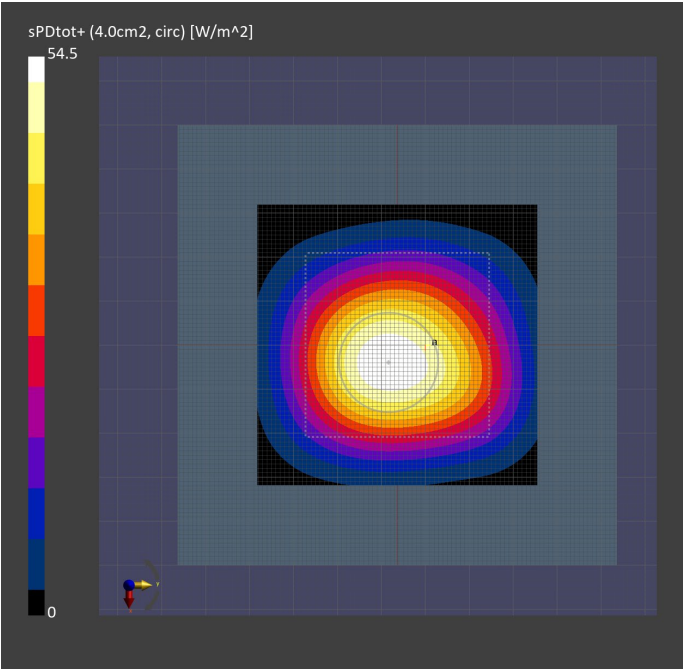

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Serial Number	Test Distance [mm]	Signal, UID	Frequency [MHz]
10 GHz System Verification	1074	10.00	CW	10000.0

Test Setup


Test Date	Measurement SW	Probe, Cal. Date	DAE, Cal. Date
2025-11-23	3.2.2.2358	EUmmWV4 – SN9690_F1–55GHz – 2025-09-17	DAE4ip Sn1839 – 2025-09-15

Scans Setup

Grid Extents [mm]	Grid Steps [lambda]	Sensor Surface Distance [mm]
60.0x60.0	0.125x0.125	10.0

Measurement Results

Averaging Area [cm²]	E _{max} [V/m]	psPDn+ [W/m²]	psPDtot+ [W/m²]
4.00	151	53.4	53.7

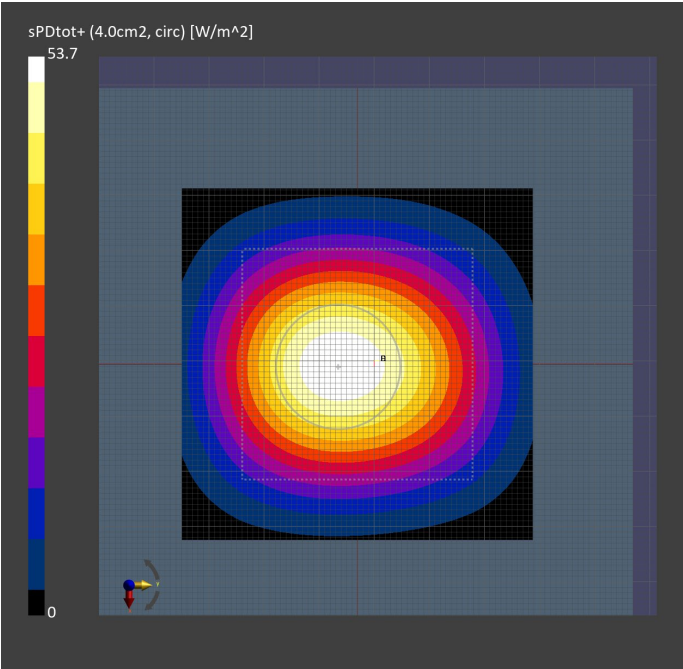

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Serial Number	Test Distance [mm]	Signal, UID	Frequency [MHz]
10 GHz System Verification	1074	10.00	CW	10000.0

Test Setup

Test Date	Measurement SW	Probe, Cal. Date	DAE, Cal. Date
2025-11-28	3.2.2.2358	EUmmWV4 – SN9690_F1–55GHz – 2025-09-17	DAE4ip Sn1839 – 2025-09-15

Scans Setup

Grid Extents [mm]	Grid Steps [lambda]	Sensor Surface Distance [mm]
60.0x60.0	0.125x0.125	10.0

Measurement Results

Averaging Area [cm²]	E _{max} [V/m]	psPD _{n+} [W/m²]	psPD _{tot+} [W/m²]
4.00	148	53.4	53.6

