



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **CLA13-1041_Oct24**

CALIBRATION CERTIFICATE

Object **CLA13 - SN: 1041**

Calibration procedure(s) **QA CAL-15.v11**
Calibration Procedure for SAR Validation Sources below 700 MHz

Mars 10/21/24

Calibration date: **October 11, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	26-Mar-24 (No. 217-04036/04037)	Mar-25
Power sensor NRP-Z91	SN: 103244	26-Mar-24 (No. 217-04036)	Mar-25
Power sensor NRP-Z91	SN: 103245	26-Mar-24 (No. 217-04037)	Mar-25
Reference 20 dB Attenuator	SN: CC2552 (20x)	26-Mar-24 (No. 217-04046)	Mar-25
Type-N mismatch combination	SN: 310982 / 06327	26-Mar-24 (No. 217-04047)	Mar-25
Reference Probe EX3DV4	SN: 3877	10-Jan-24 (No. EX3-3877_Jan24)	Jan-25
DAE4	SN: 654	15-Jan-24 (No. DAE4-654_Jan24)	Jan-25

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter NRP2	SN: 107193	08-Nov-21 (in house check Dec-22)	In house check: Dec-24
Power sensor NRP-Z91	SN: 100922	15-Dec-09 (in house check Dec-22)	In house check: Dec-24
Power sensor NRP-Z91	SN: 100418	01-Jan-04 (in house check Dec-22)	In house check: Dec-24
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-24)	In house check: Jun-26
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Sep-24)	In house check: Sep-26

Calibrated by: **Paulo Pina** **Laboratory Technician** *[Signature]*

Approved by: **Sven Kühn** **Technical Manager** *[Signature]*

Issued: October 14, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	13 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	55.0	0.75 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	53.1 ± 6 %	0.72 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	1 W input power	0.446 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	0.457 W/kg ± 18.4 % (k=2)

SAR averaged over 10 cm^3 (10 g) of Head TSL	condition	
SAR measured	1 W input power	0.289 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	0.296 W/kg ± 18.0 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.5 \Omega - 0.9 j\Omega$
Return Loss	- 27.1 dB

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 11.10.2024

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA13; Type: CLA13; Serial: CLA13 - SN: 1041

Communication System: UID 0 - CW; Frequency: 13 MHz

Medium parameters used: $f = 13$ MHz; $\sigma = 0.72$ S/m; $\epsilon_r = 53.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(15.33, 15.33, 15.33) @ 13 MHz; Calibrated: 10.01.2024
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 15.01.2024
- Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2034
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

CLA Calibration for HSL-LF Tissue/CLA-13, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 28.80 V/m; Power Drift = 0.05 dB


Peak SAR (extrapolated) = 0.947 W/kg

SAR(1 g) = 0.446 W/kg; SAR(10 g) = 0.289 W/kg

Smallest distance from peaks to all points 3 dB below = 19.9 mm


Ratio of SAR at M2 to SAR at M1 = 78.3%

Maximum value of SAR (measured) = 0.687 W/kg

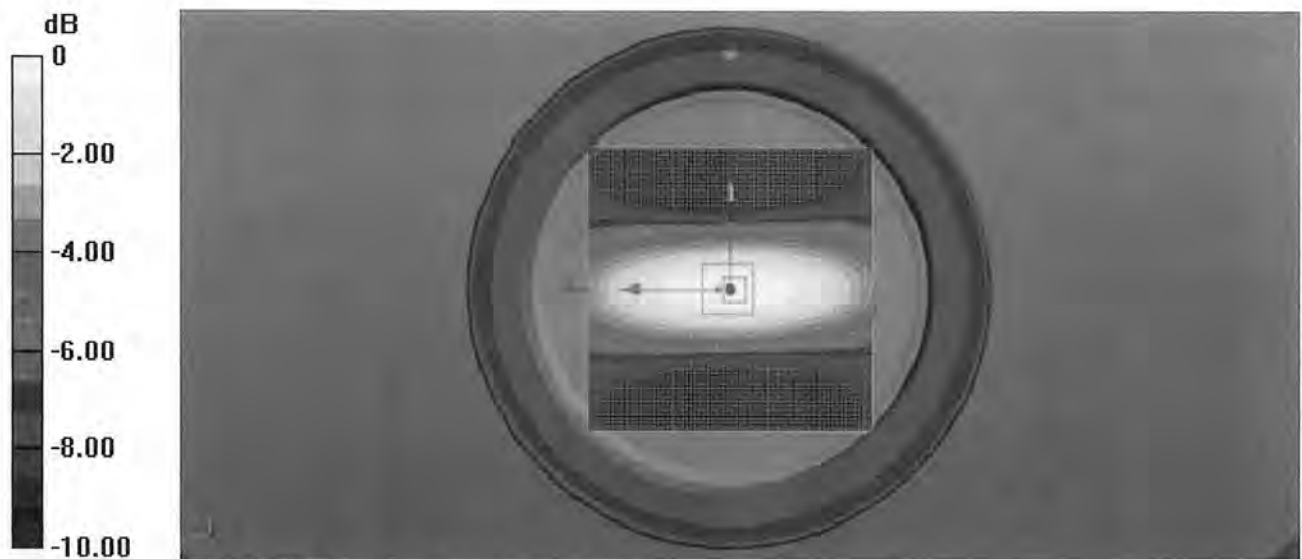

0 dB = 0.687 W/kg = -1.63 dBW/kg

Impedance Measurement Plot for Head TSL

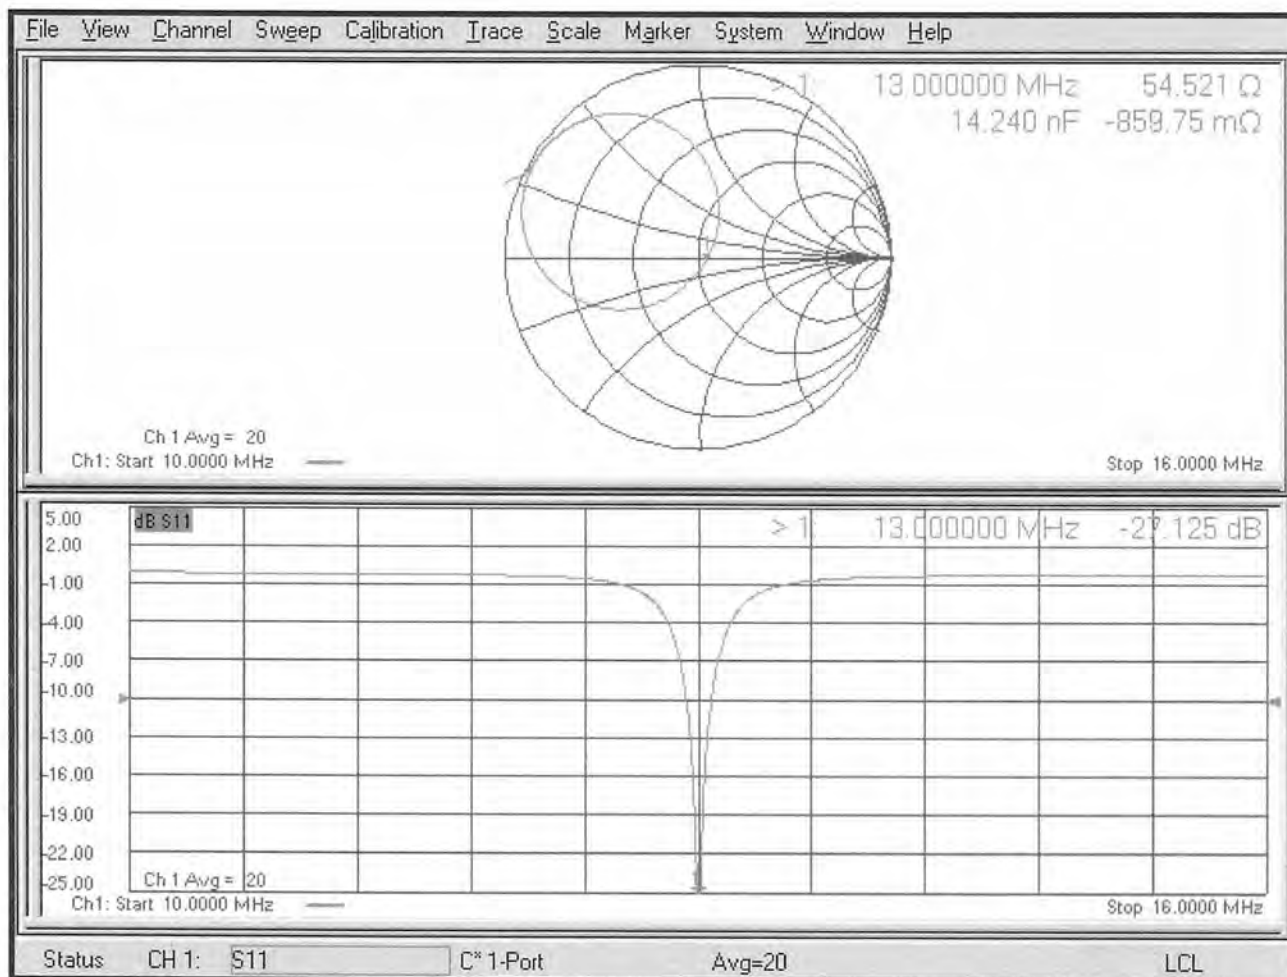

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: CLA13 – SN: 1041
Description: SAR Validation Source at 13 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/24	9/12/25	
Rohde & Schwarz	ZN-Z135	VNA Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/23	8/28/25	
Control Company	4040	Ambient Thermometer	230581662	8/28/23	8/28/25	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/23	9/28/25	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/23	9/28/25	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/24	12/28/25	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
Mini-Circuits	VLK-8400+	Coaxial Low Pass Filter (DC - 8.4 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/24	9/4/25	
SPEAG	DAK-12	DAK-12 Dielectric Probe	1194	10/14/24	10/14/25	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/24	9/12/25	
Anritsu	MA24118A	Microwave USB Power Sensor (10MHz - 18 GHz)	2123431	1/13/25	1/13/26	
Rohde & Schwarz	SMCV100B	R&S SMCV100B Vector Signal Generator (VSG)	103882	12/21/23	12/19/25	
Mini-Circuits	CBL-6FT-SMNM+	Precision Test Cable SMA/N (DC - 18 GHz)	3318			✓

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
1041	13	11/13/2024	10/11/2024							54.5	54.5	53.0	-1.5	-0.9	-0.9	-3.5	-2.6	-27.1	-27.1	-27.0	2.10%	PASS	In-house check after Calibration
1041	13	7/30/2025	10/11/2024	0.457	0.13	-0.62%	0.296	0.08	-5.30%	54.5	53.0	54.6	1.6	-0.9	-3.5	-1.0	2.5	-27.1	-27.0	-27.0	1.10%	PASS	-

Impedance and Return-Loss Measurement Plot for Head TSL

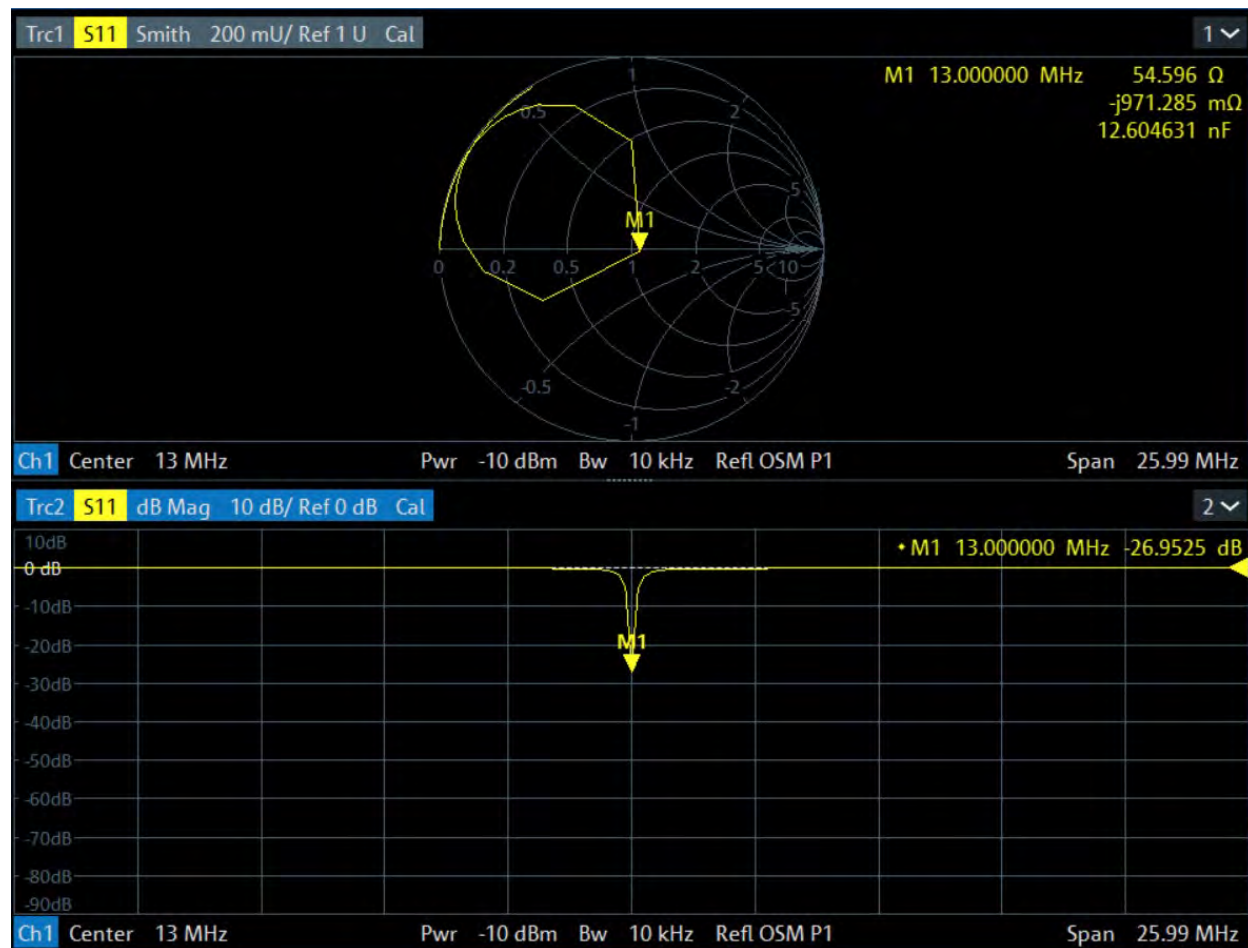



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D750V3-1235_Oct23**

CALIBRATION CERTIFICATE

Object **D750V3 - SN:1235**

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 11, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	10-Jan-23 (No. EX3-7349_Jan23)	Jan-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** **Function**
Laboratory Technician

Approved by: **Sven Kühn** **Technical Manager**

Signature

Issued: October 12, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	42.2 $\pm$ 6 %	0.89 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.17 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.69 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.42 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.69 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	55.5 $\pm$ 6 %	0.95 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.16 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.72 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.42 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.73 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.3 Ω - 1.0 j Ω
Return Loss	- 27.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.1 Ω - 3.3 j Ω
Return Loss	- 29.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.043 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 11.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1235

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.89 \text{ S/m}$; $\epsilon_r = 42.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.11, 10.11, 10.11) @ 750 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 60.95 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 3.31 W/kg

SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 17 mm


Ratio of SAR at M2 to SAR at M1 = 65.5%

Maximum value of SAR (measured) = 2.90 W/kg

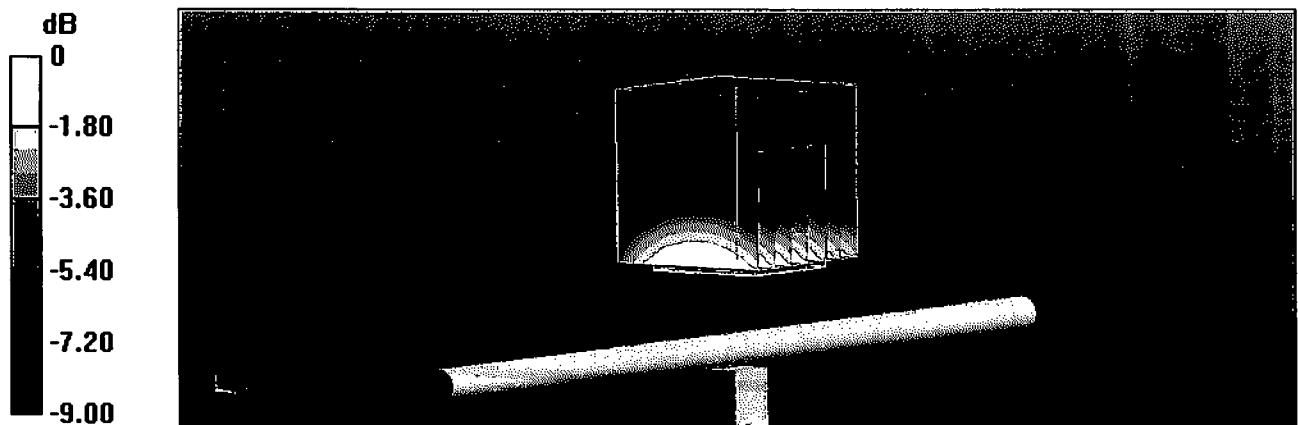

0 dB = 2.90 W/kg = 4.62 dBW/kg

Impedance Measurement Plot for Head TSL

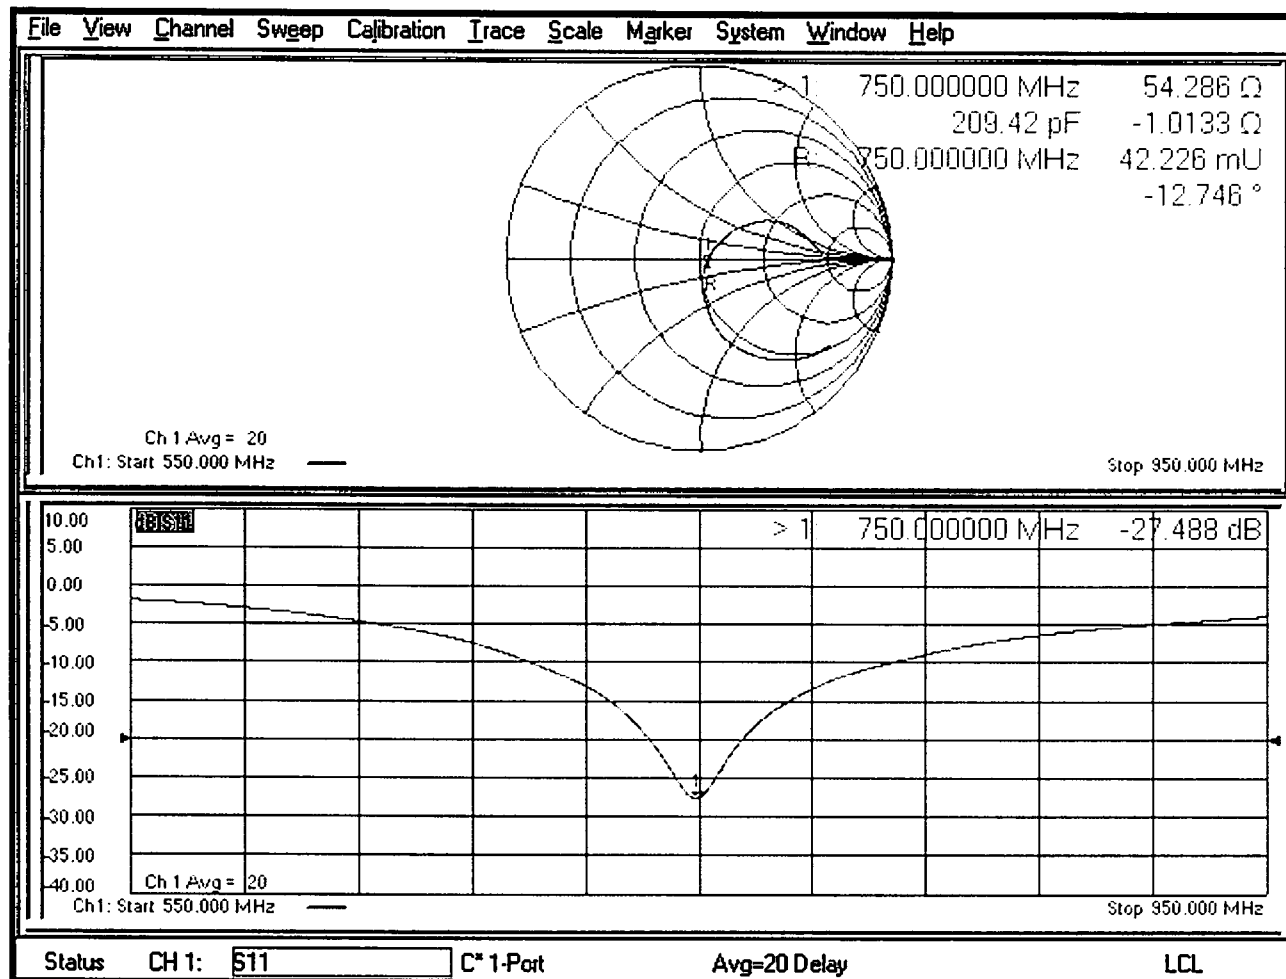

DASY5 Validation Report for Body TSL

Date: 09.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1235

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.95 \text{ S/m}$; $\epsilon_r = 55.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.23, 10.23, 10.23) @ 750 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 55.70 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 3.30 W/kg

SAR(1 g) = 2.16 W/kg; SAR(10 g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm


Ratio of SAR at M2 to SAR at M1 = 66%

Maximum value of SAR (measured) = 2.89 W/kg

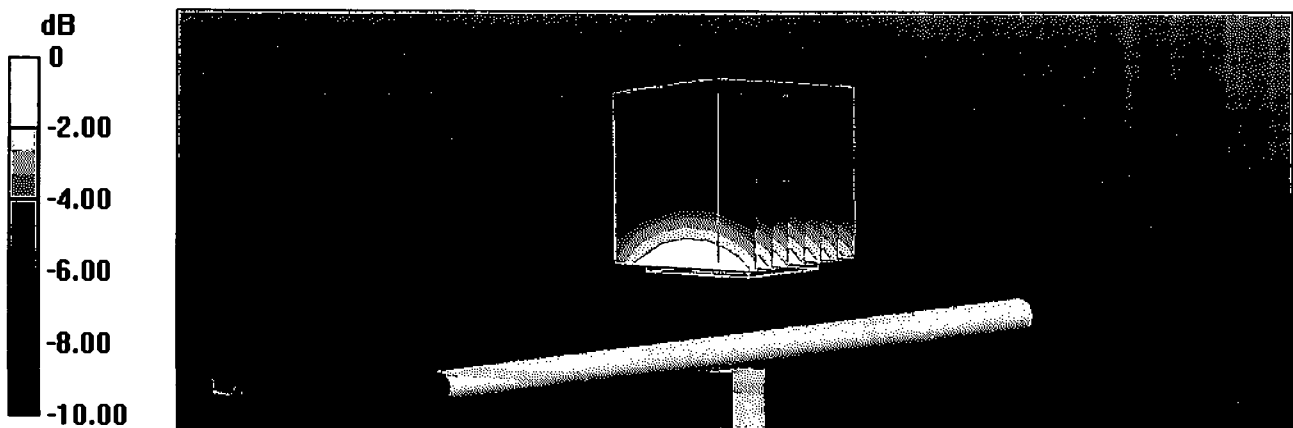

0 dB = 2.89 W/kg = 4.62 dBW/kg

Impedance Measurement Plot for Body TSL

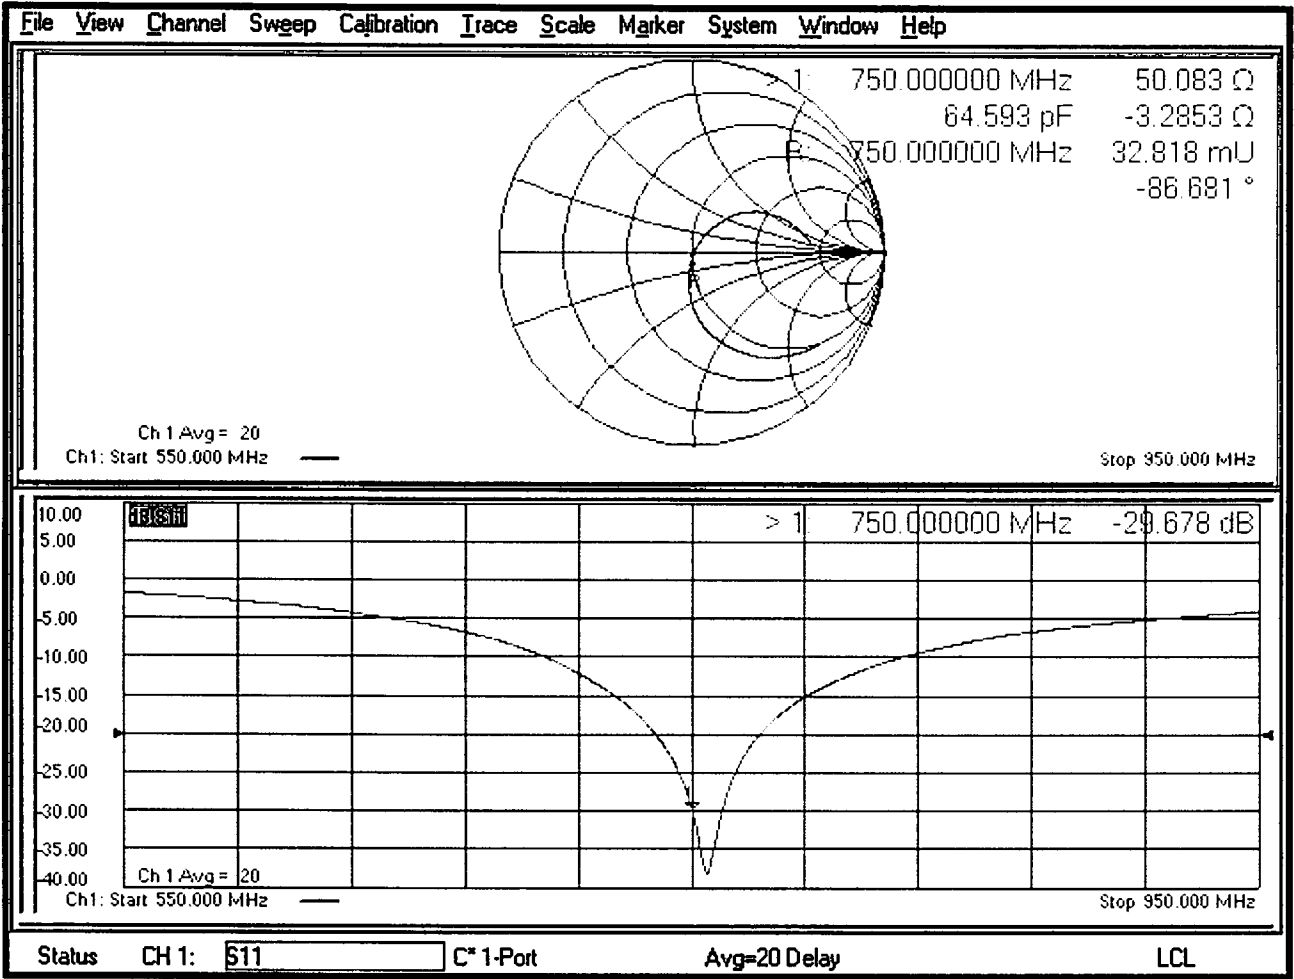

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object D750V3 – SN: 1235
Description SAR Validation Dipole at 750 MHz
Procedure (s) Procedure for SAR Verification Source Calibration Extension
In-house Check Date 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1235	750	11/7/2024	10/11/2023	8.69	0.44	0.80%	5.69	0.29	1.34%	54.3	54.8	0.5	-1.0	0.4	1.4	-27.5	-26.8	17.22%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

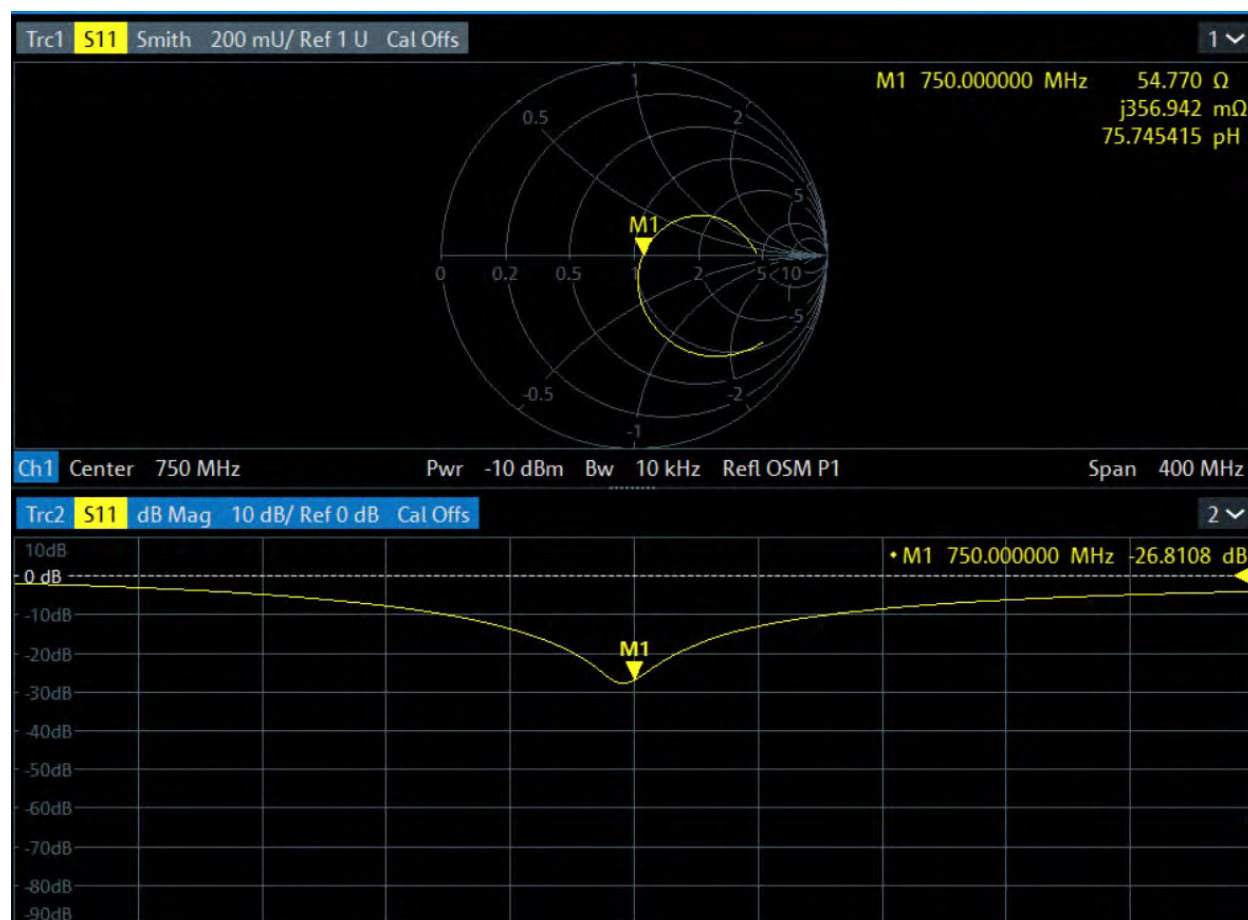

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D750V3 – SN: 1235
Description: SAR Validation Dipole at 750 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1844	11/6/2024	11/6/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7853	11/7/2024	11/7/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	YL	Engineer	
Approved By:	PN	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev(%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1235	750	11/7/2024	10/11/2023	8.69	0.44	0.80%	5.69	0.29	1.34%	54.3	54.3	54.8	0.5	-1.0	-1.0	0.4	1.4	-27.5	-27.5	-26.8	17.22%	PASS
1235	750	7/30/2025	10/11/2023	8.69	0.42	-4.25%	5.69	0.27	-3.92%	54.3	54.8	54.6	-0.2	-1.0	0.4	-1.3	-1.7	-27.5	-26.8	-26.8	1.04%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

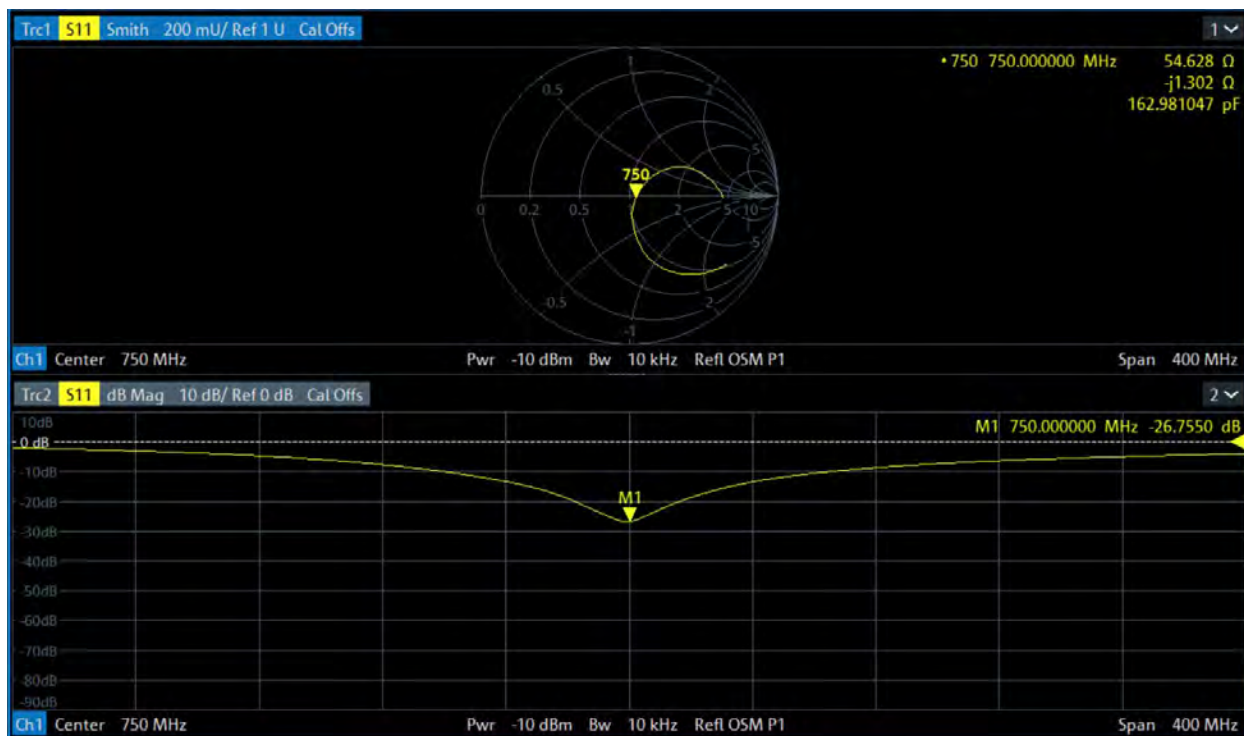



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D835V2-4d311_Oct23**

CALIBRATION CERTIFICATE

Object **D835V2 - SN:4d311**

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 09, 2023**

*MAR
11/20/23*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	10-Jan-23 (No. EX3-7349_Jan23)	Jan-24
DAE4	SN: 900	09-Aug-23 (No. DAE4-900_Aug23)	Aug-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** **Laboratory Technician**

Approved by: **Sven Kühn** **Technical Manager**

Signature

Issued: October 11, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	42.0 $\pm$ 6 %	0.92 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.49 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.82 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.61 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.37 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	55.3 $\pm$ 6 %	0.98 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.93 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.64 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.52 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.9 Ω - 2.4 j Ω
Return Loss	- 32.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.2 Ω - 6.0 j Ω
Return Loss	- 22.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.392 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 03.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d311

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.92 \text{ S/m}$; $\epsilon_r = 42$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.69, 9.69, 9.69) @ 835 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn900; Calibrated: 09.08.2023
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 64.08 V/m; Power Drift = -0.06 dB


Peak SAR (extrapolated) = 3.72 W/kg

SAR(1 g) = 2.49 W/kg; SAR(10 g) = 1.61 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm


Ratio of SAR at M2 to SAR at M1 = 66.5%

Maximum value of SAR (measured) = 3.30 W/kg

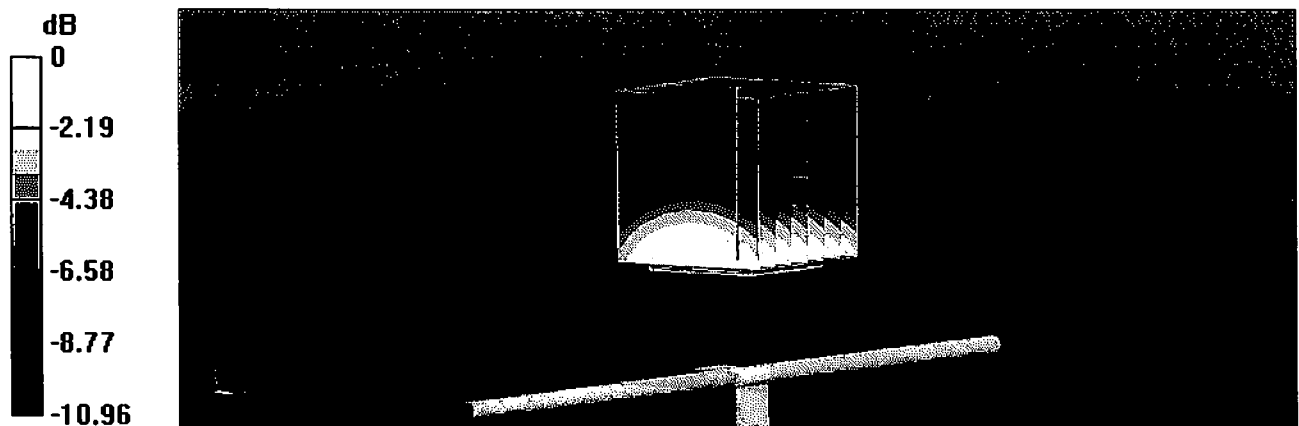

0 dB = 3.30 W/kg = 5.19 dBW/kg

Impedance Measurement Plot for Head TSL

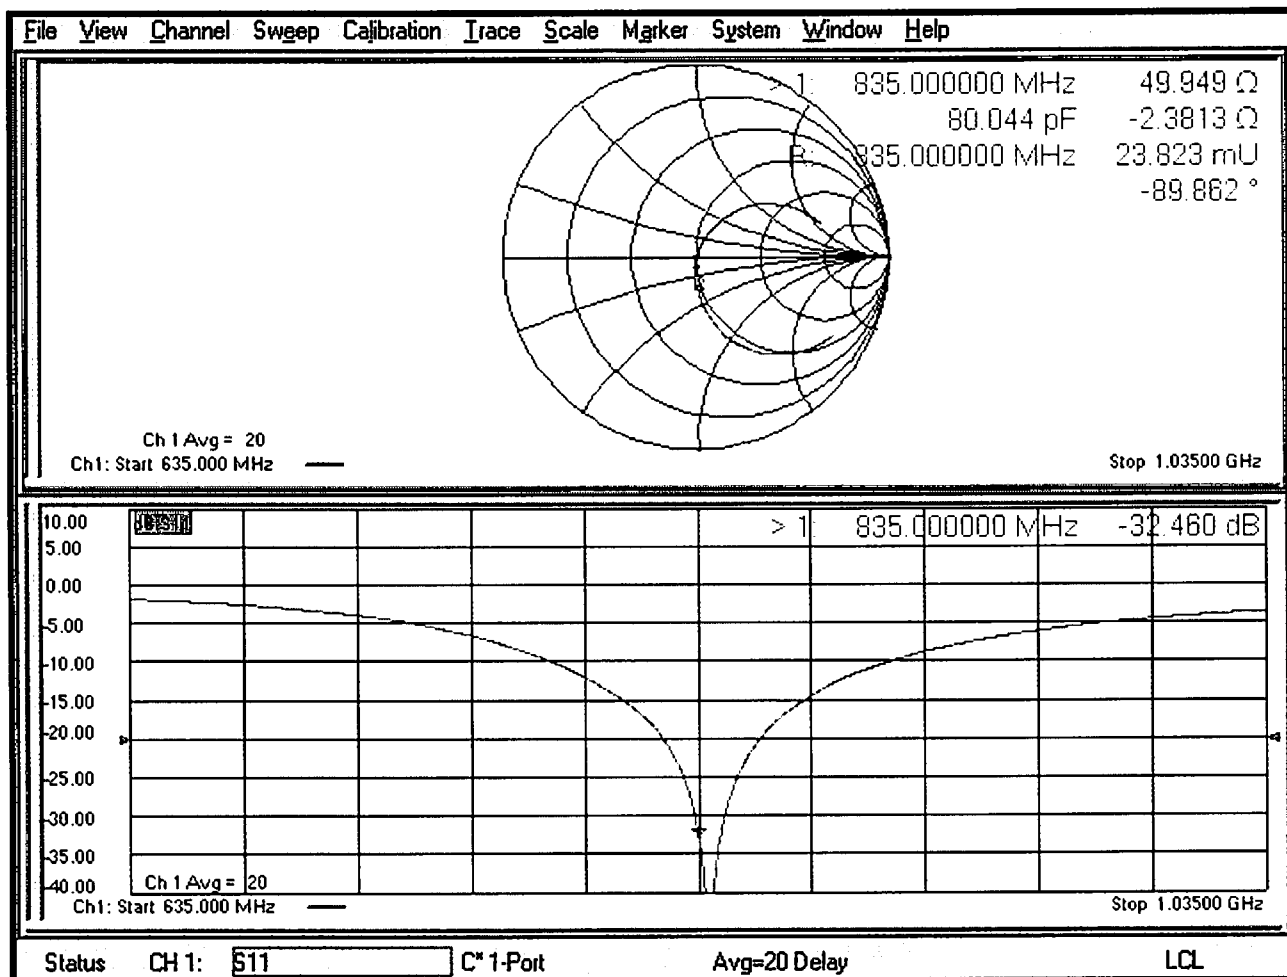

DASY5 Validation Report for Body TSL

Date: 09.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d311

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.98$ S/m; $\epsilon_r = 55.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.85, 9.85, 9.85) @ 835 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.74 V/m; Power Drift = -0.06 dB



Peak SAR (extrapolated) = 3.68 W/kg

SAR(1 g) = 2.50 W/kg; SAR(10 g) = 1.64 W/kg

Smallest distance from peaks to all points 3 dB below = 15.1 mm


Ratio of SAR at M2 to SAR at M1 = 68.2%

Maximum value of SAR (measured) = 3.30 W/kg

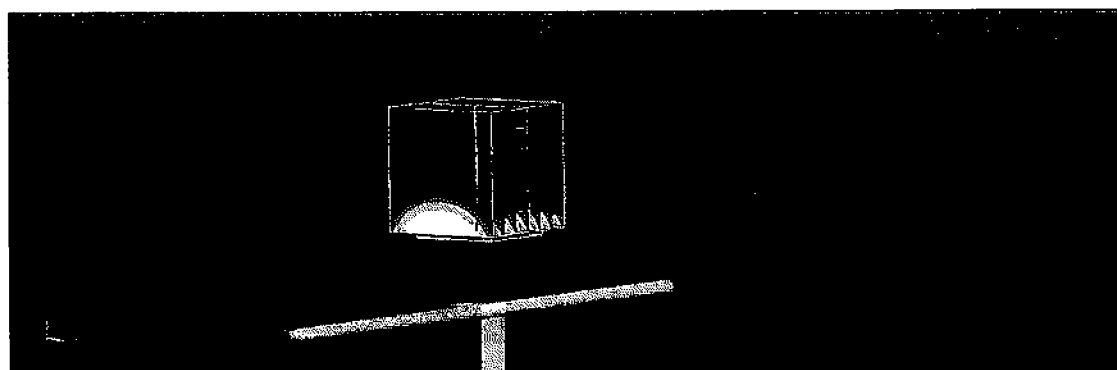

0 dB = 3.30 W/kg = 5.19 dBW/kg

Impedance Measurement Plot for Body TSL

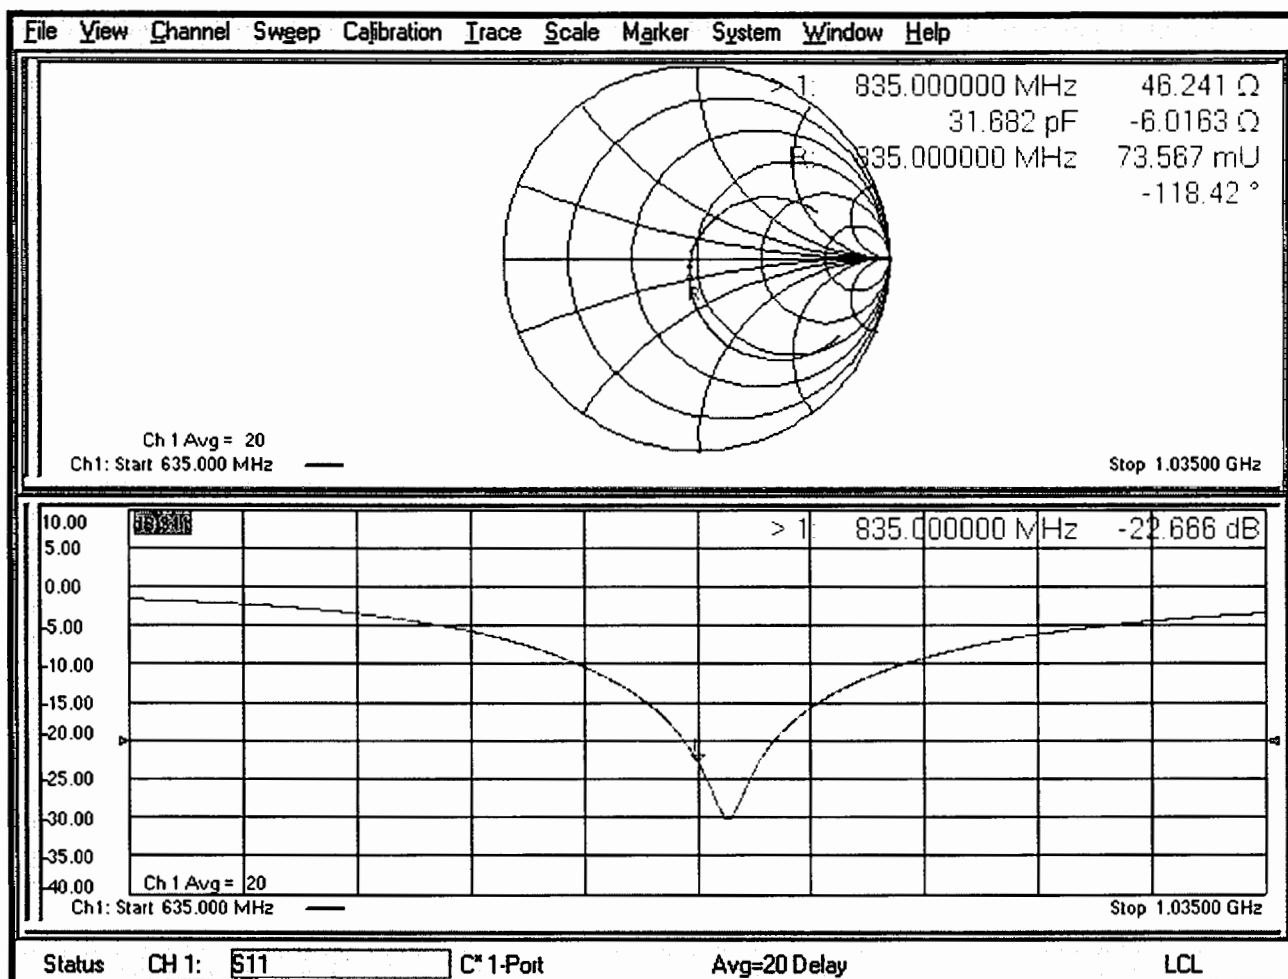

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D835V2 – SN: 4d311
Description: SAR Validation Dipole at 835 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
4d311	835	11/7/2024	10/9/2023	9.82	0.53	7.48%	6.37	0.35	8.06%	49.9	49.4	-0.5	-2.4	-2.0	0.4	-32.5	-33.4	-18.68%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

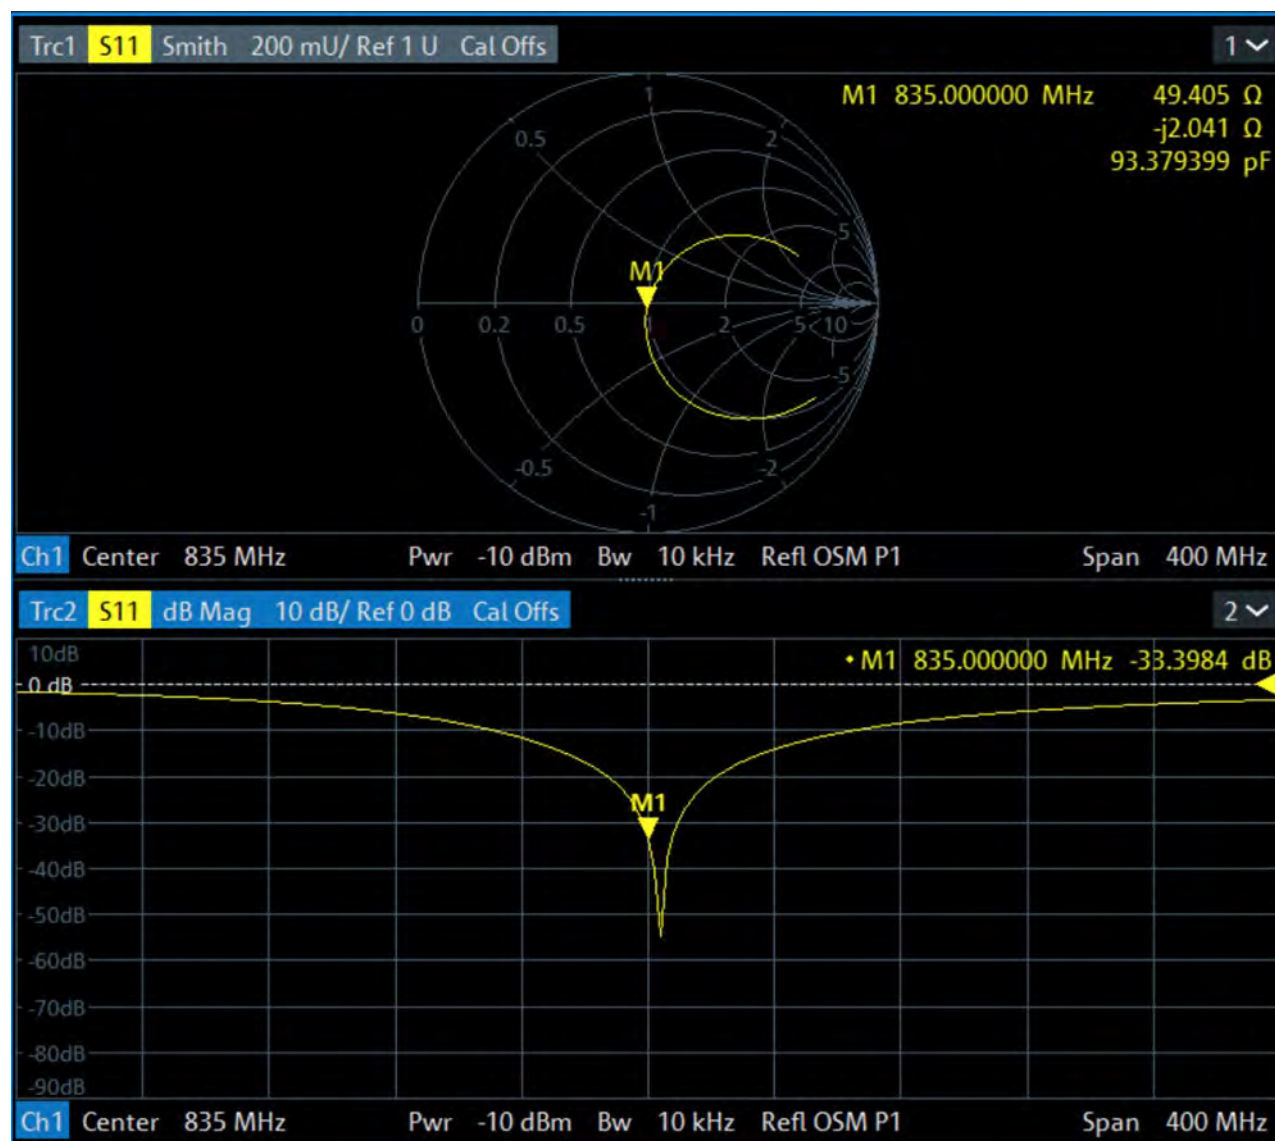

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D835V2 – SN: 4d311
Description: SAR Validation Dipole at 835 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/29/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	YL	Engineer	
Approved By:	PN	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
4d311	835	11/7/2024	10/9/2023	9.82	0.53	7.48%	6.37	0.35	8.06%	49.9	49.9	49.4	-0.5	-2.4	-2.4	-2.0	0.4	-32.5	-32.5	-33.4	-18.68%	PASS
4d311	835	7/29/2025	10/9/2023	9.82	0.51	3.01%	6.37	0.33	3.05%	49.9	49.4	49.7	0.3	-2.4	-2.0	-2.2	-0.2	-32.5	-33.4	-33.0	10.26%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

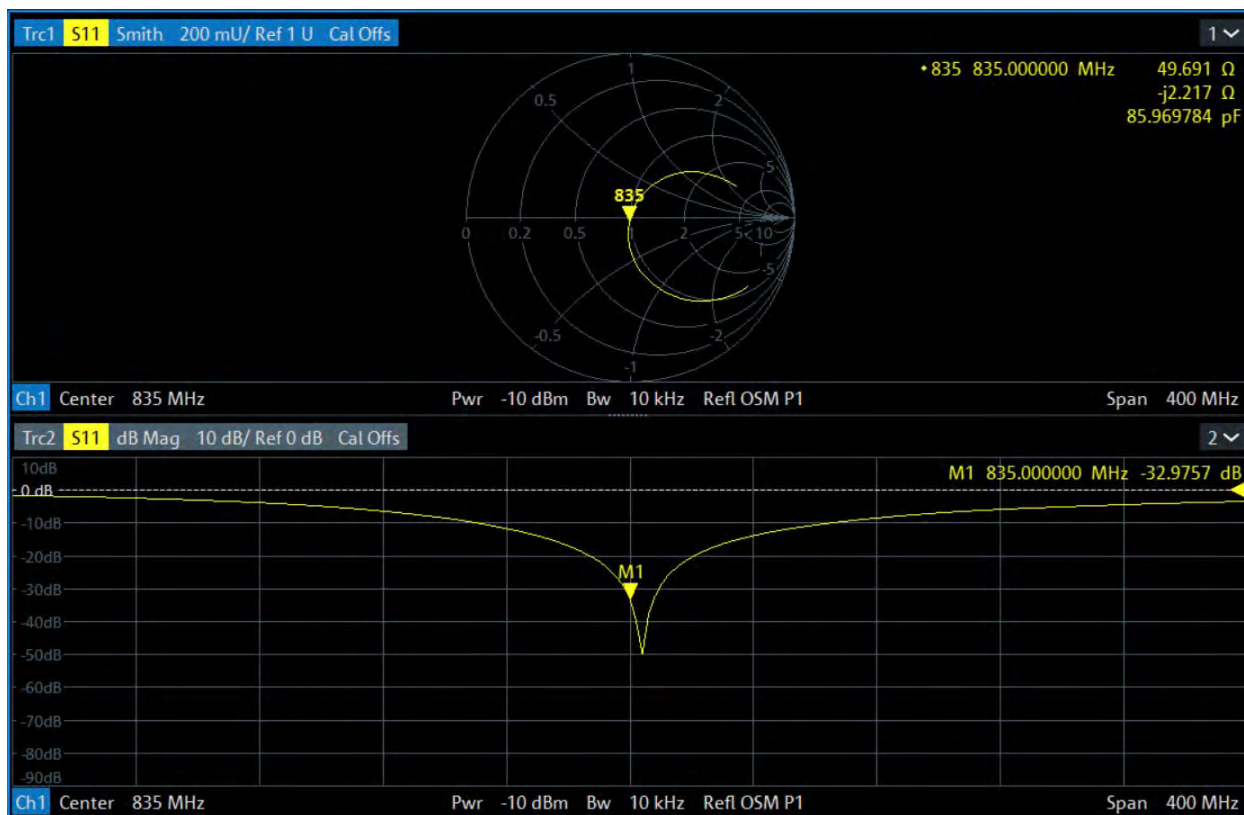



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

RF Safety Lab
Catonsville, USA

Certificate No.

D1640V2-356_Sep24

CALIBRATION CERTIFICATE

Object

D1640V2 - SN: 356

MAS 9/17/24

Calibration procedure(s)

QA CAL-05.v12

Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz

Calibration date

September 13, 2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Cal
Power Sensor R&S NRP-33T	SN: 100967	28-Mar-24 (No. 217-04038)	Mar-25
Power Sensor R&S NRP18A	SN: 101859	22-Jul-24 (No. 4030A315008547)	Jul-25
Spectrum Analyzer R&S FSV40	SN: 101832	25-Jan-24 (No. 4030-315007551)	Jan-25
Mismatch; Short [S4188] Attenuator [S4423]	SN: 1152	28-Mar-24 (No. 217-04050)	Mar-25
OCP DAK-12	SN: 1016	05-Oct-23 (No. OCP-DAK12-1016_Oct23)	Oct-24
OCP DAK-3.5	SN: 1249	05-Oct-23 (No. OCP-DAK3.5-1249_Oct23)	Oct-24
Reference Probe EX3DV4	SN: 7349	03-Jun-24 (No. EX3-7349_Jun24)	Jun-25
DAE4ip	SN: 1836	10-Jan-24 (No. DAE4ip-1836_Jan24)	Jan-25

Secondary Standards	ID	Check Date (in house)	Scheduled Check
ACAD Source Box	SN: 1000	28-May-24 (No. 675-ACAD_Source_Box-240528)	May-25
Signal Generator R&S SMB100A	SN: 182081	28-May-24 (No. 675-CAL16-S4588-240528)	May-25
Mismatch; SMA	SN: 1102	22-May-24 (No. 675-Mismatch_SMA-240522)	May-25

	Name	Function	Signature
Calibrated by	Paulo Pina	Laboratory Technician	
Approved by	Sven Kühn	Technical Manager	
Issued: September 13, 2024			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 0108**

Glossary

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation

- DASY System Handbook

Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY8 Module SAR	16.4.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with spacer
Zoom Scan Resolution	dx, dy = 6mm, dz = 1.5mm	Graded Ratio = 1.5 mm (Z direction)
Frequency	1640MHz $\pm$ 1MHz	

Head TSL parameters at 1640 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.2	1.31 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	41.5 $\pm$ 6%	1.28 mho/m $\pm$ 6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 1640 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	8.58 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	34.2 W/kg $\pm$ 17.0% (k = 2)

SAR averaged over 10 cm³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	4.68 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	18.6 W/kg $\pm$ 16.5% (k = 2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL at 1640 MHz**

Impedance	49.7 Ω + 2.2 j Ω
Return Loss	-32.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.227 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D1640V2 - SN356	1640	HSL	24

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10		CW, 0---	1640, 0	7.92	1.28	41.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Right	HSL, 2024-09-13	EX3DV4 - SN7349, 2024-06-03	DAE4ip Sn1836, 2024-01-10

Scans Setup


	Zoom Scan
Grid Extents [mm]	30 x 30 x 30
Grid Steps [mm]	6.0 x 6.0 x 1.5
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.5
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-09-13
psSAR1g [W/Kg]	8.58
psSAR10g [W/Kg]	4.68
Power Drift [dB]	0.00
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

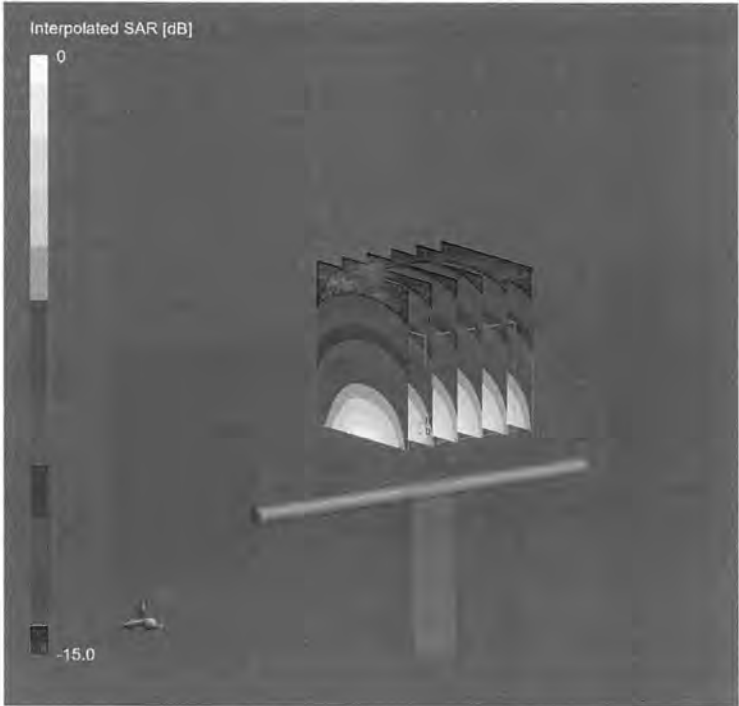

0 dB = 14.6 W/Kg

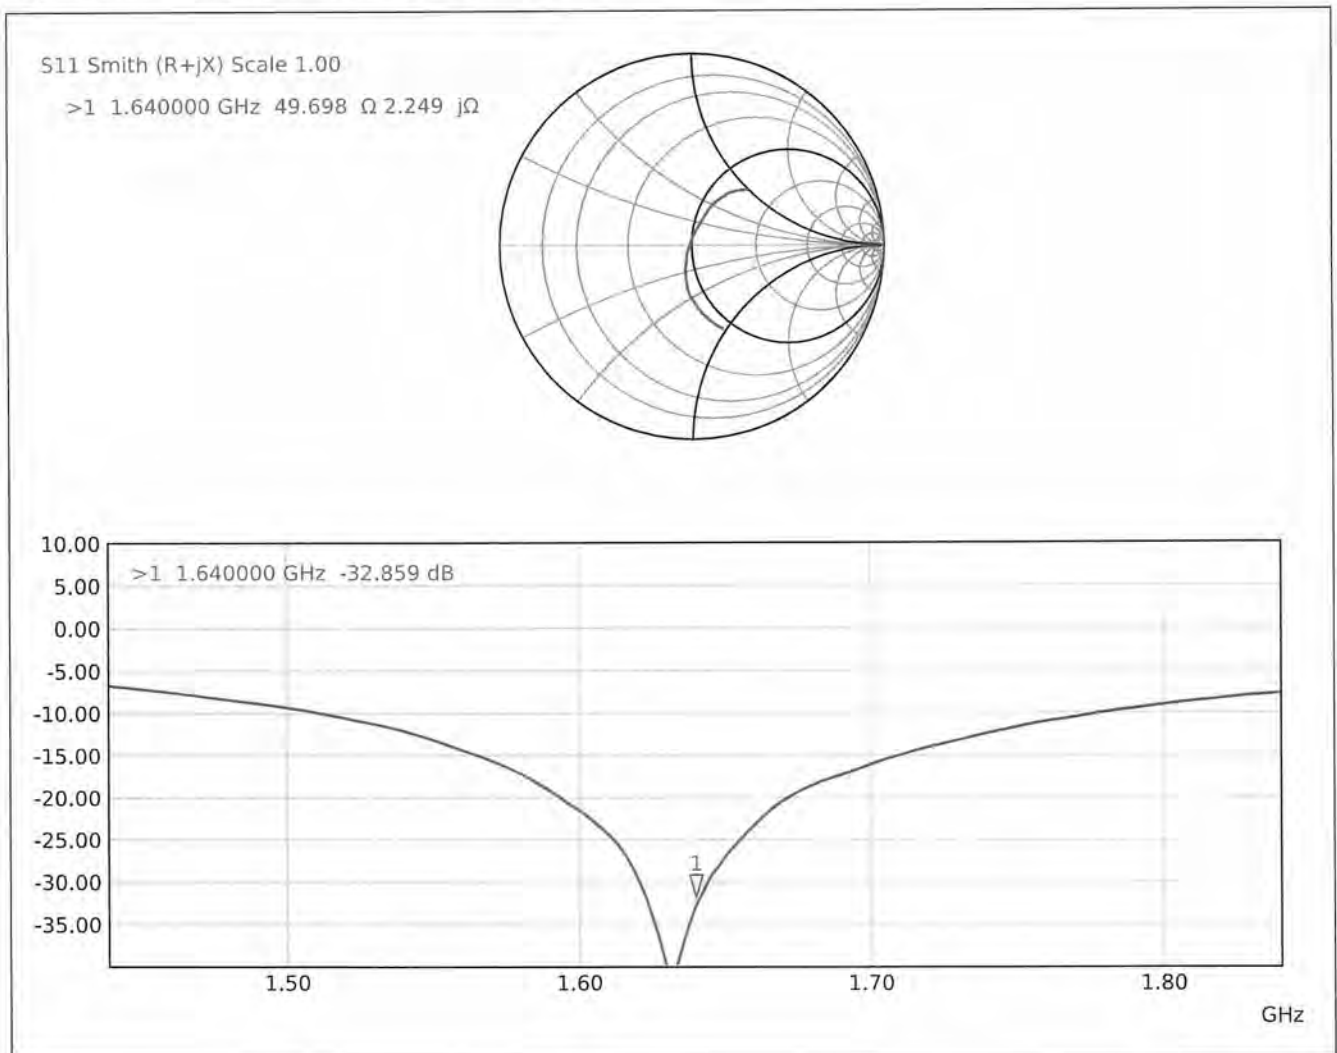Impedance Measurement Plot for Head TSL

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D1640V2 – SN: 356
Description: SAR Validation Dipole at 1640 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	YL	Engineer	
Approved By:	PN	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
356	1640	11/7/2024	9/13/2024							49.7	49.7	48.5	-1.2	2.2	2.2	1.8	-0.4	-32.9	-32.9	-32.3	14.66%	PASS	In-house check after Calibration
356	1640	7/30/2025	9/13/2024	34.2	1.81	5.60%	18.6	0.99	6.09%	49.7	48.5	47.9	-0.6	2.2	1.8	0.7	-1.1	-32.9	-32.3	-32.9	-13.30%	PASS	-

Impedance and Return-Loss Measurement Plot for Head TSL

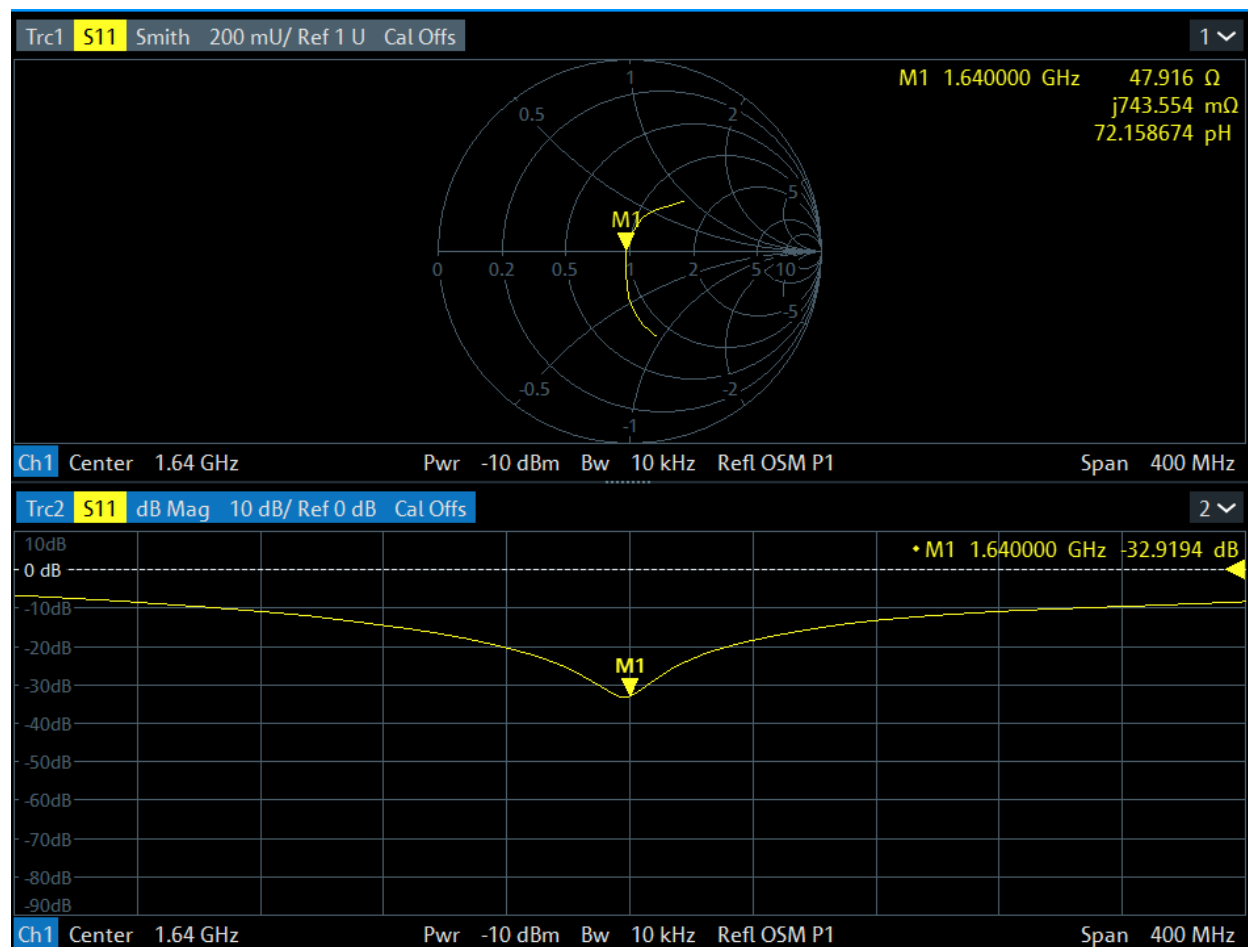

✓ KOK
11/15/2023

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S
C
S** Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: **SCS 0108**

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D1750V2-1205_Oct23**

CALIBRATION CERTIFICATE

Object **D1750V2 - SN:1205**

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 11, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	10-Jan-23 (No. EX3-7349_Jan23)	Jan-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
DAE4	SN: 900	09-Aug-23 (No. DAE4-900_Aug23)	Aug-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** **Paulo Pina** **Paulo Pina**
Name Function Laboratory Technician

Approved by: **Sven Kühn** **Sven Kühn** **Sven Kühn**
Name Function Technical Manager

Signature

Issued: October 12, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.3 $\pm$ 6 %	1.35 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.04 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.5 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.77 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.2 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.4	1.49 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.9 $\pm$ 6 %	1.46 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.19 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	37.3 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.90 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	19.8 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	46.6 Ω + 3.9 j Ω
Return Loss	- 25.4 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	41.9 Ω + 3.3 j Ω
Return Loss	- 20.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.214 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 04.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1205

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.76, 8.76, 8.76) @ 1750 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn900; Calibrated: 09.08.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 106.8 V/m; Power Drift = -0.06 dB



Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 9.04 W/kg; SAR(10 g) = 4.77 W/kg

Smallest distance from peaks to all points 3 dB below = 10 mm


Ratio of SAR at M2 to SAR at M1 = 54.1%

Maximum value of SAR (measured) = 14.0 W/kg

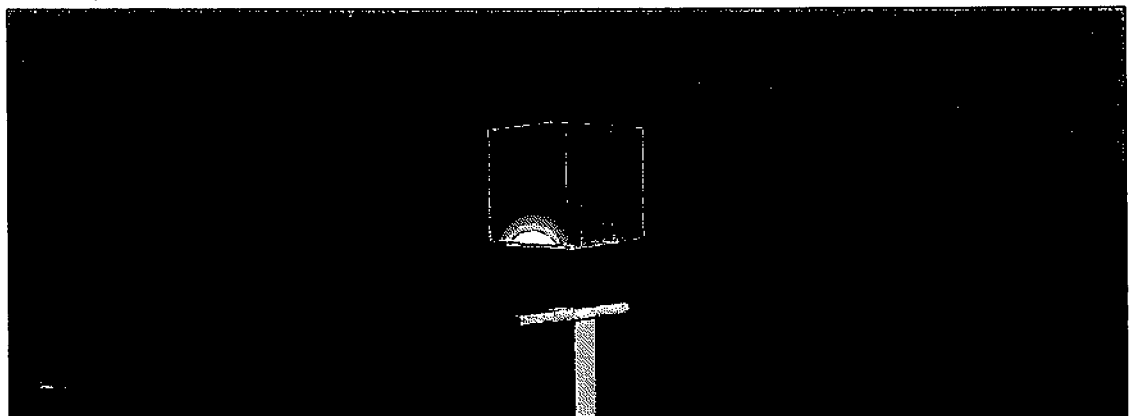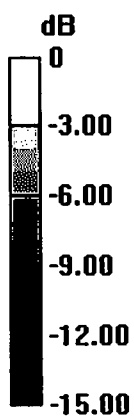

0 dB = 14.0 W/kg = 11.46 dBW/kg

Impedance Measurement Plot for Head TSL

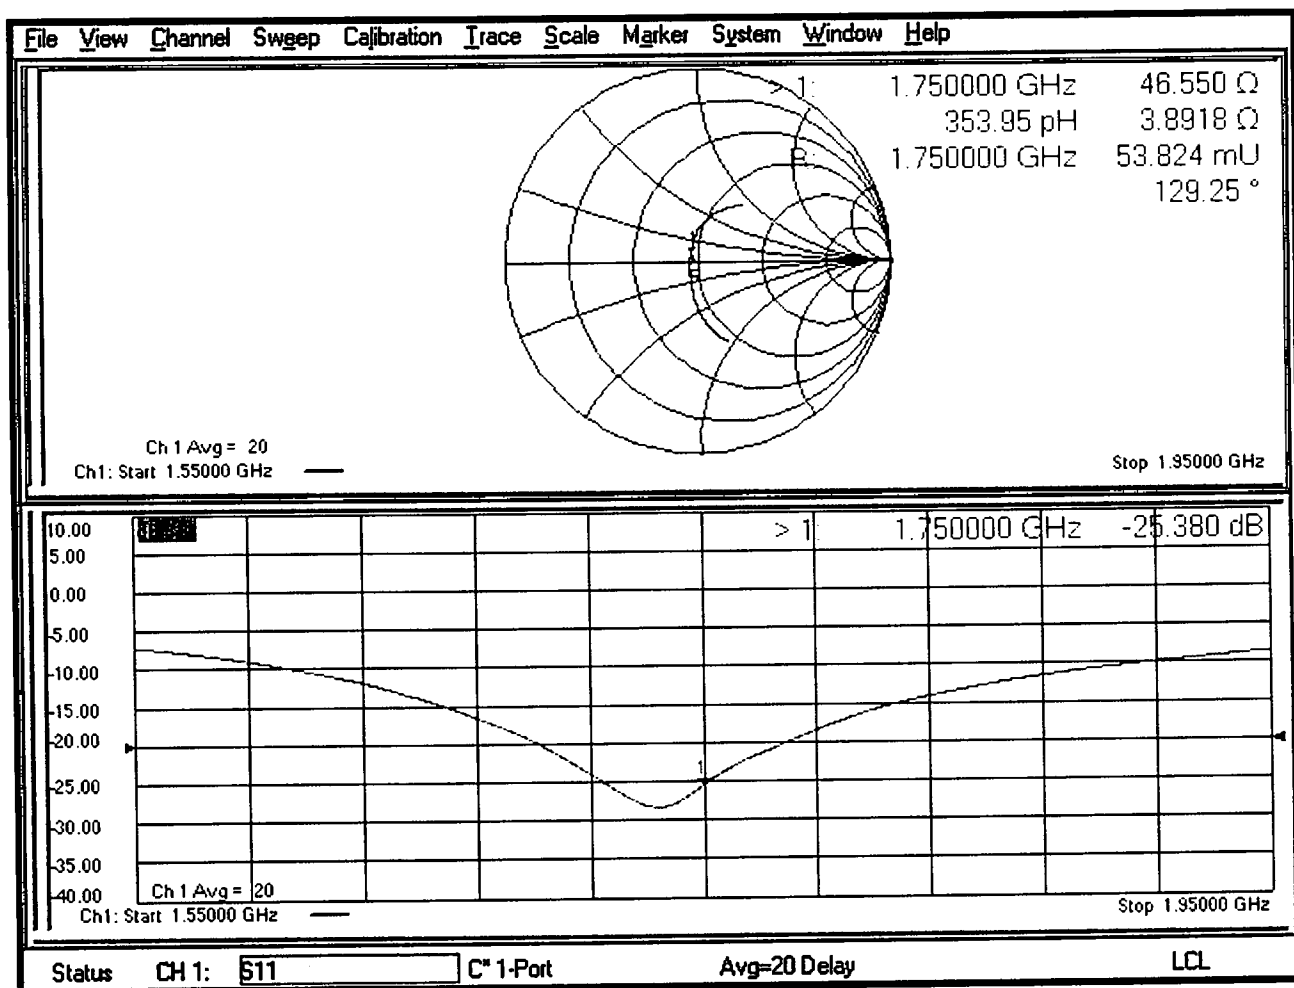

DASY5 Validation Report for Body TSL

Date: 11.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1205

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 53.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.48, 8.48, 8.48) @ 1750 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.4 V/m; Power Drift = 0.00 dB


Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 9.19 W/kg; SAR(10 g) = 4.90 W/kg

Smallest distance from peaks to all points 3 dB below = 9.2 mm


Ratio of SAR at M2 to SAR at M1 = 56.1%

Maximum value of SAR (measured) = 14.1 W/kg

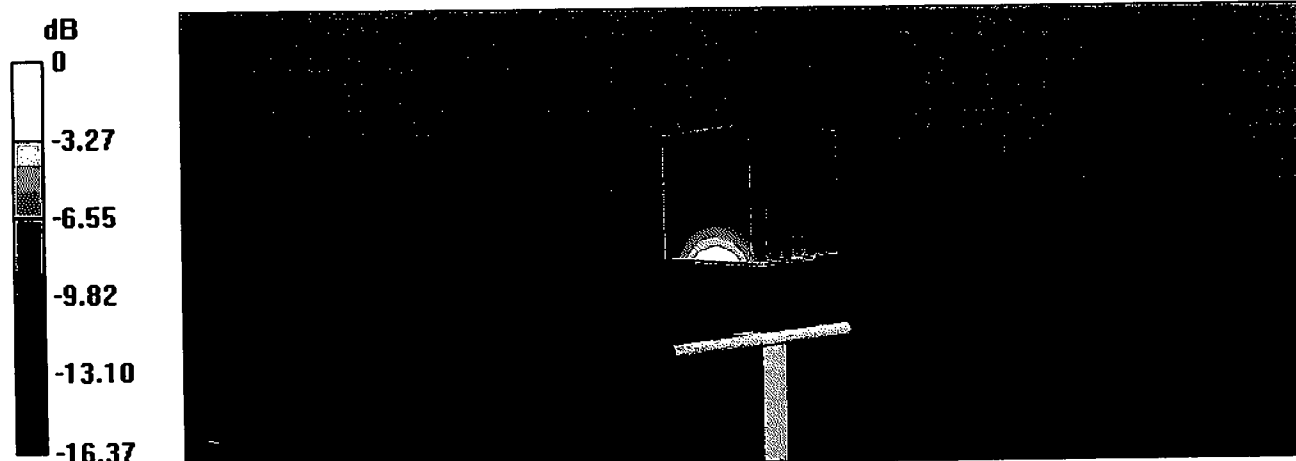

0 dB = 14.1 W/kg = 11.50 dBW/kg

Impedance Measurement Plot for Body TSL

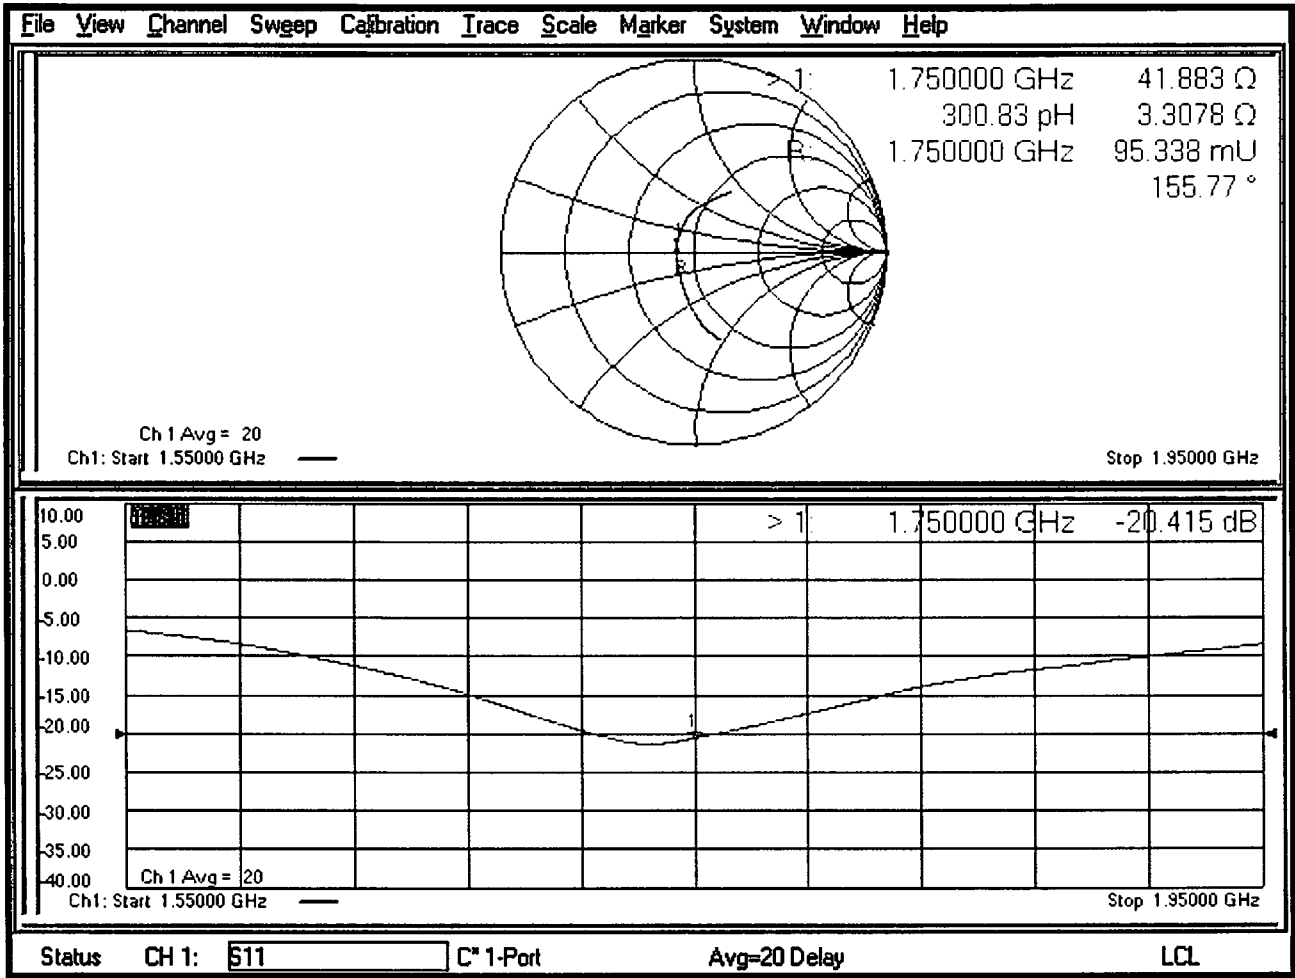

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D1750V2 – SN: 1205
Description: SAR Validation Dipole at 1750 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	

Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:


1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1205	1750	11/7/2024	10/11/2023	36.5	1.80	-1.60%	19.2	0.96	0.07%	46.6	46.9	0.3	3.9	4.3	0.4	-25.4	-25.2	5.68%	PASS



Impedance and Return-Loss Measurement Plot for Head TSL

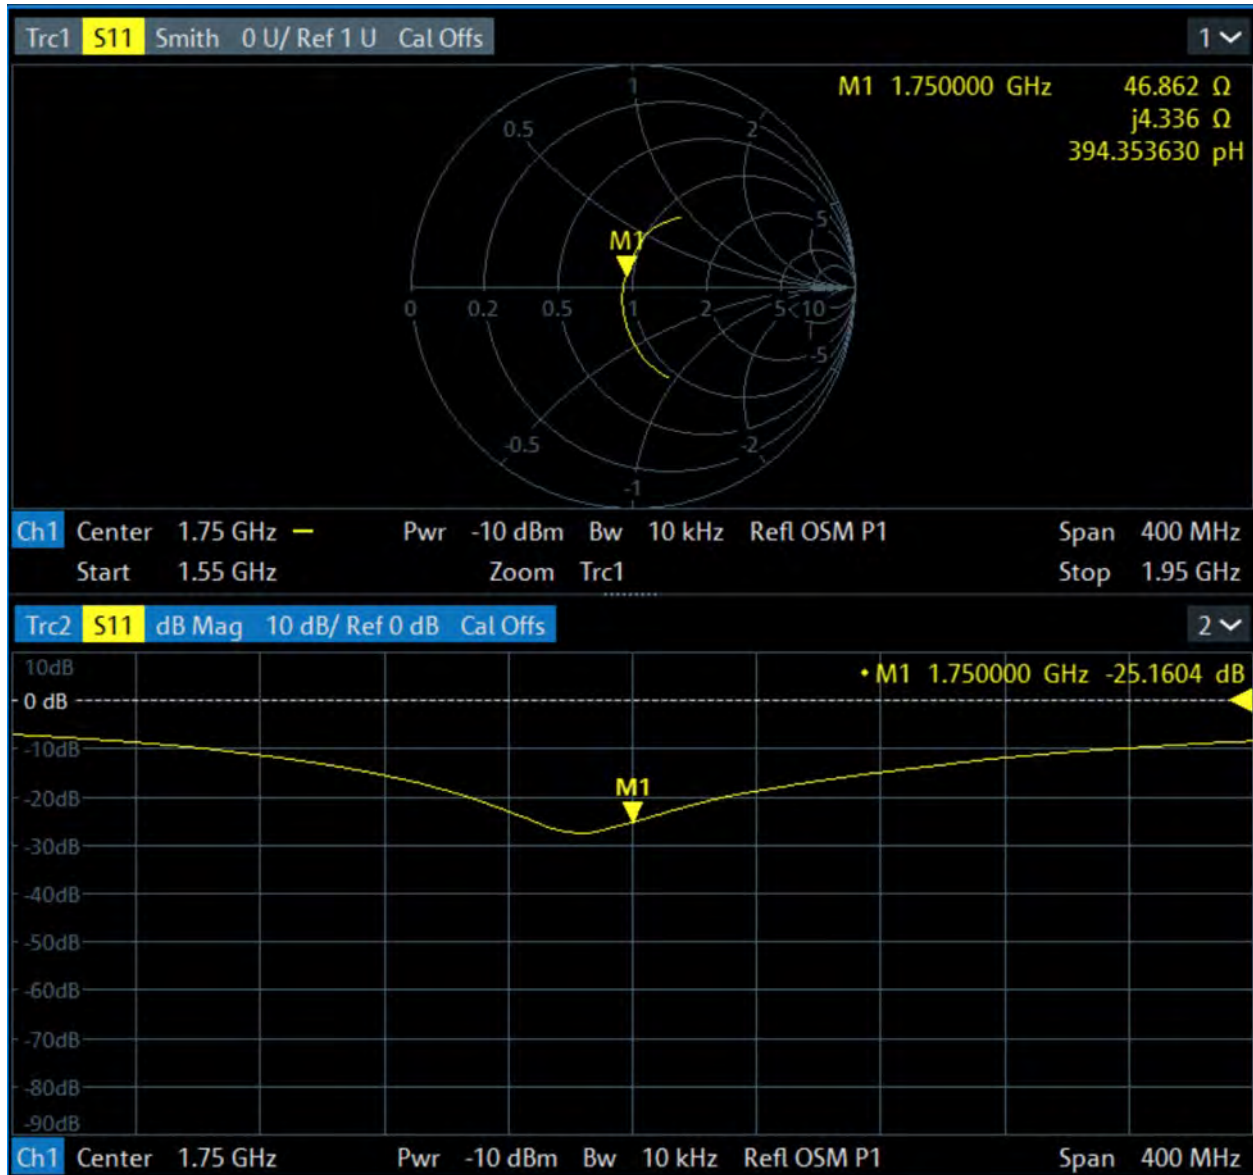

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D1750V2 – SN: 1205
Description: SAR Validation Dipole at 1750 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 7/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev(%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1205	1750	11/7/2024	10/11/2023	36.5	1.80	-1.60%	19.2	0.96	0.07%	46.6	46.6	46.9	0.3	3.9	3.9	4.3	0.4	-25.4	-25.4	-25.2	5.68%	PASS
1205	1750	7/30/2025	10/11/2023	36.5	1.83	0.04%	19.2	0.98	2.05%	46.6	46.9	47.0	0.1	3.9	4.3	3.9	-0.4	-25.4	-25.2	-25.9	-15.04%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

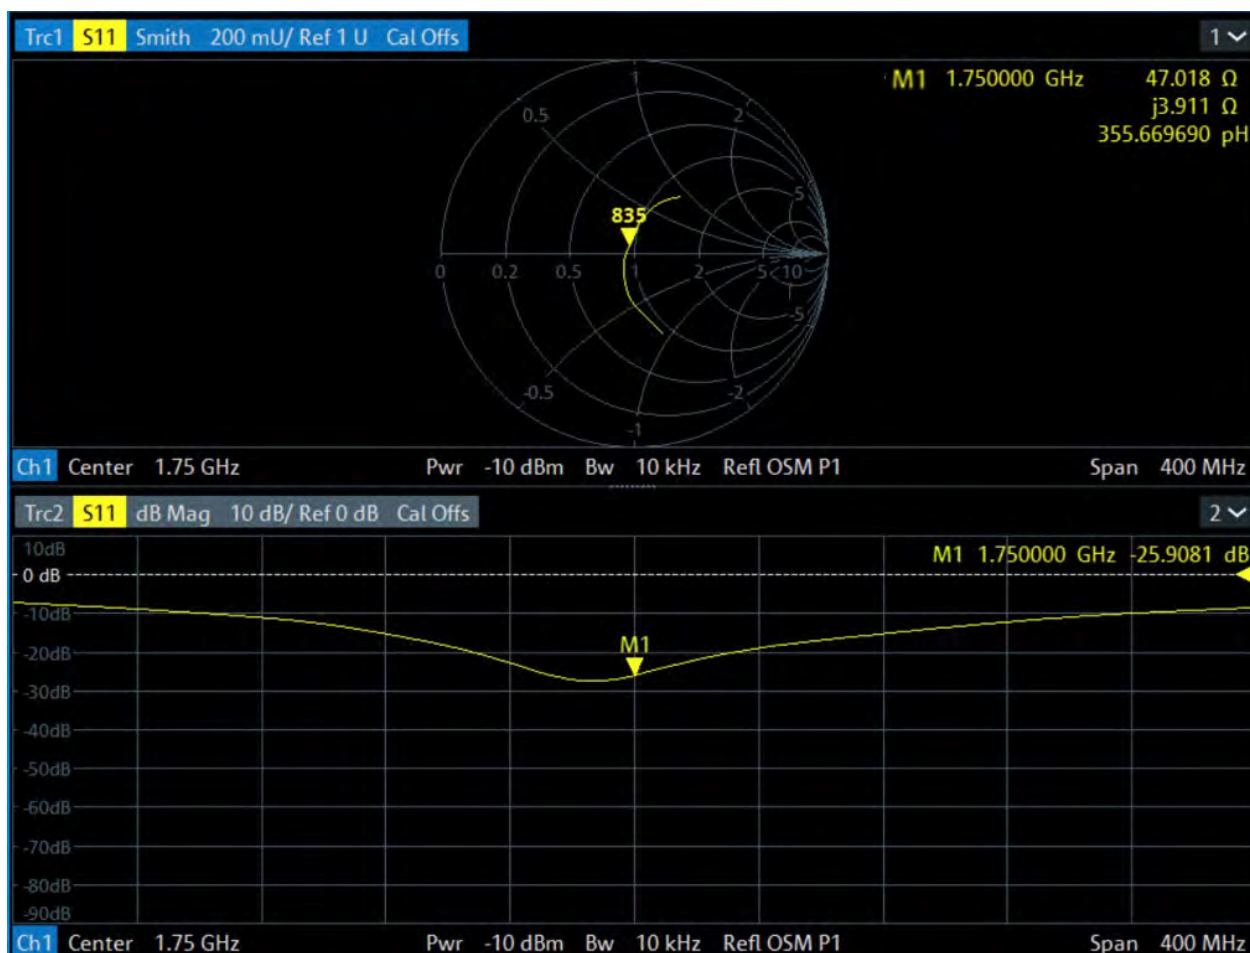



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D1900V2-5d252_Oct23**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN:5d252**

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 06, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	10-Jan-23 (No. EX3-7349_Jan23)	Jan-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** **Paulo Pina** **Laboratory Technician**

Approved by: **Sven Kühn** **Sven Kühn** **Technical Manager**

Signature

[Signature of Paulo Pina]

[Signature of Sven Kühn]

Issued: October 12, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.7 $\pm$ 6 %	1.40 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.92 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	39.8 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.25 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.0 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.1 $\pm$ 6 %	1.51 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.9 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.22 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.9 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$48.8 \Omega + 5.9 j\Omega$
Return Loss	- 24.4 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$45.0 \Omega + 5.8 j\Omega$
Return Loss	- 21.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.194 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 06.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d252

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.4$ S/m; $\epsilon_r = 40.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.43, 8.43, 8.43) @ 1900 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.7 V/m; Power Drift = 0.08 dB


Peak SAR (extrapolated) = 18.2 W/kg

SAR(1 g) = 9.92 W/kg; SAR(10 g) = 5.25 W/kg

Smallest distance from peaks to all points 3 dB below = 10 mm


Ratio of SAR at M2 to SAR at M1 = 55.9%

Maximum value of SAR (measured) = 15.0 W/kg

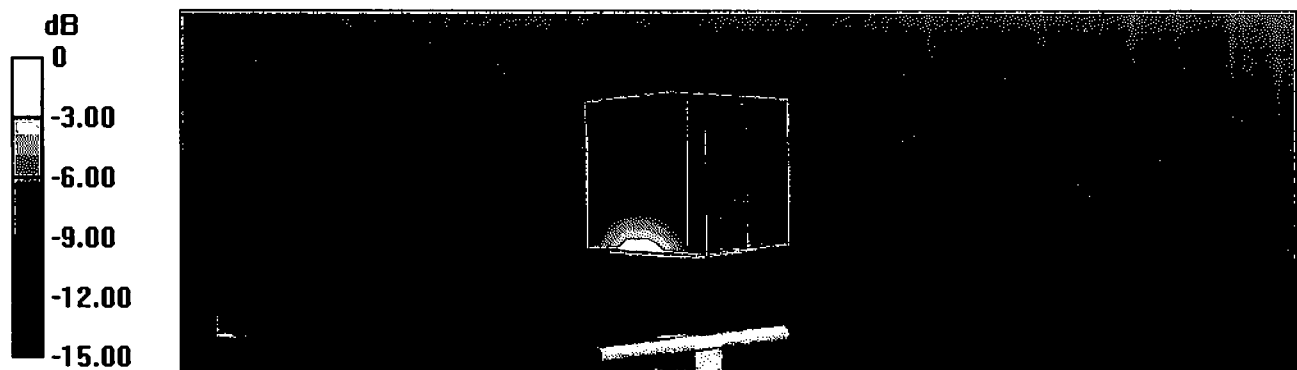

0 dB = 15.0 W/kg = 11.75 dBW/kg

Impedance Measurement Plot for Head TSL

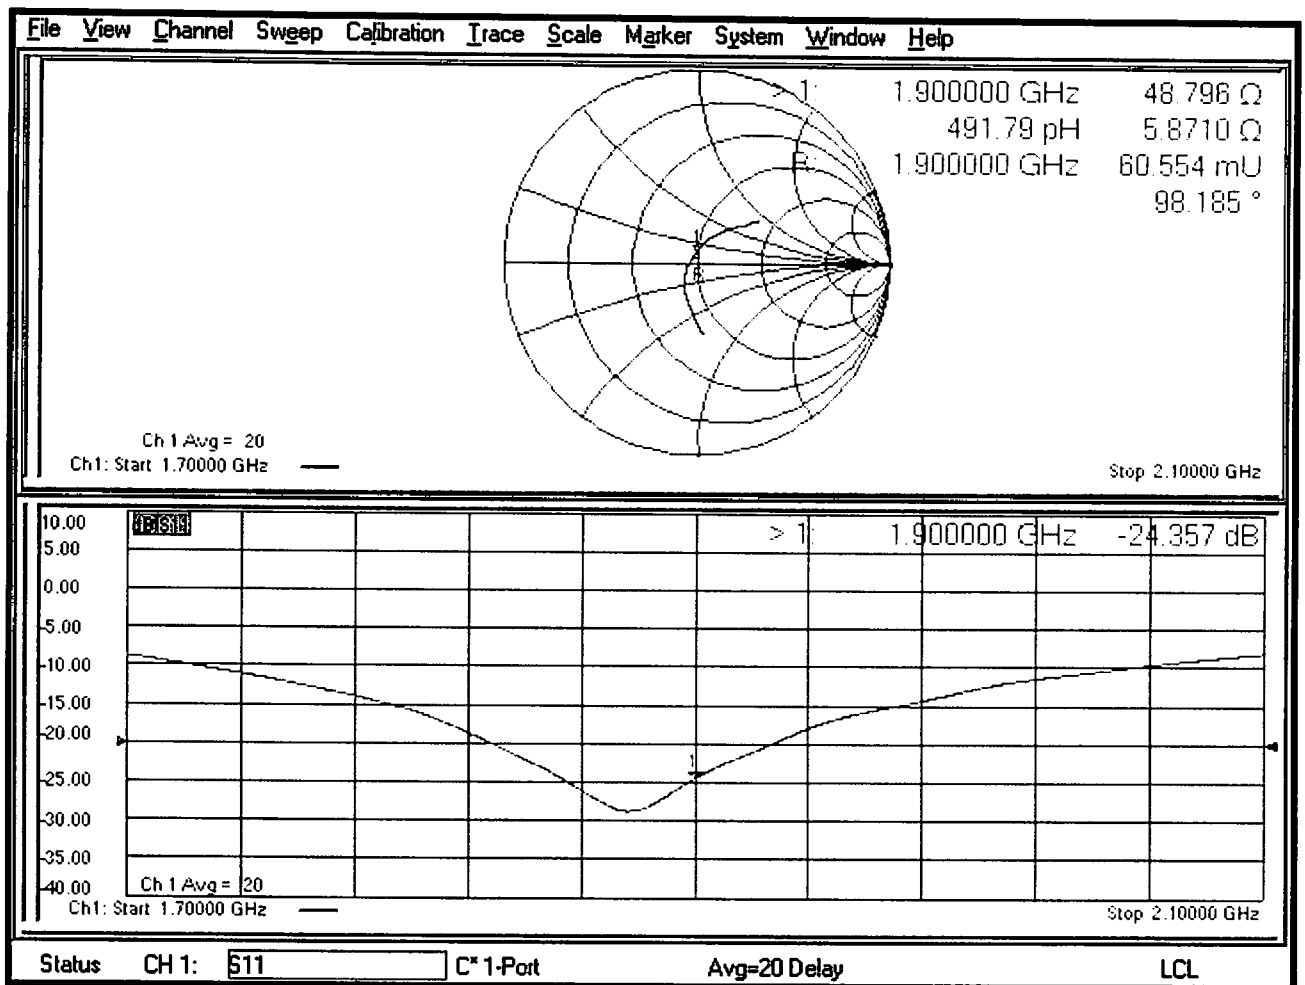

DASY5 Validation Report for Body TSL

Date: 06.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d252

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.51$ S/m; $\epsilon_r = 53.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.42, 8.42, 8.42) @ 1900 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.3 V/m; Power Drift = -0.04 dB



Peak SAR (extrapolated) = 18.4 W/kg

SAR(1 g) = 9.94 W/kg; SAR(10 g) = 5.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 55.5%

Maximum value of SAR (measured) = 15.2 W/kg

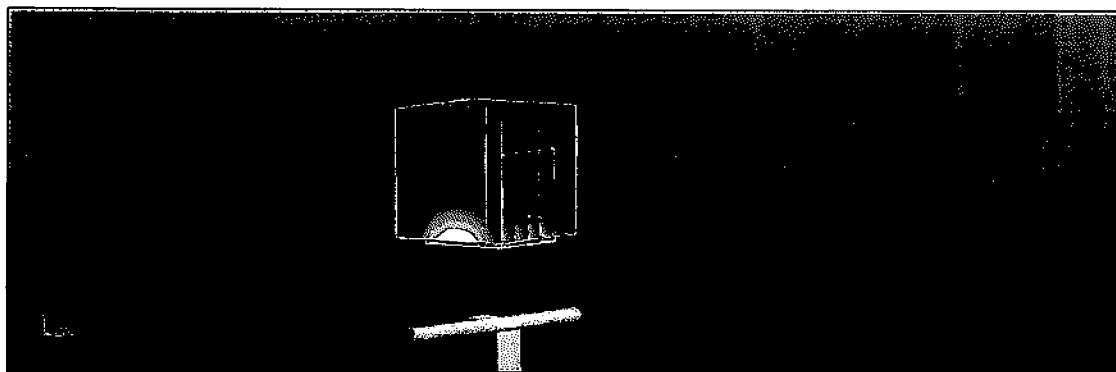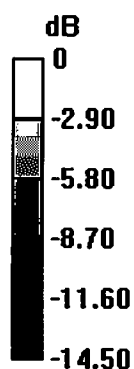

0 dB = 15.2 W/kg = 11.81 dBW/kg

Impedance Measurement Plot for Body TSL

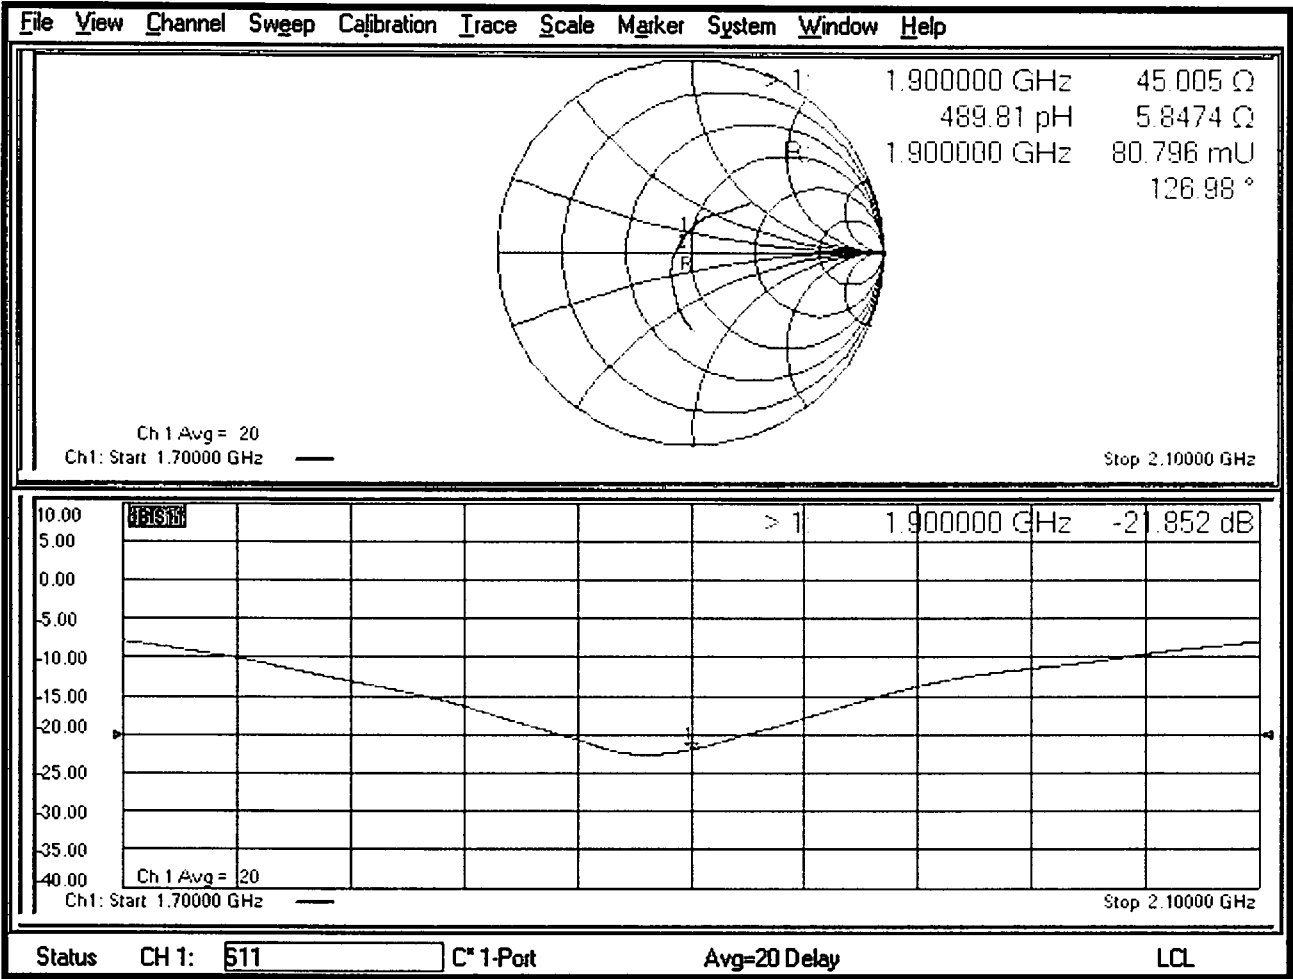

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D1900V2 – SN: 5d252
Description: SAR Validation Dipole at 1900 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
5d252	1900	11/7/2024	10/6/2023	39.8	2.07	3.77%	21	1.08	2.61%	48.8	47.6	-1.2	5.9	5.7	-0.2	-24.4	-23.9	11.17%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

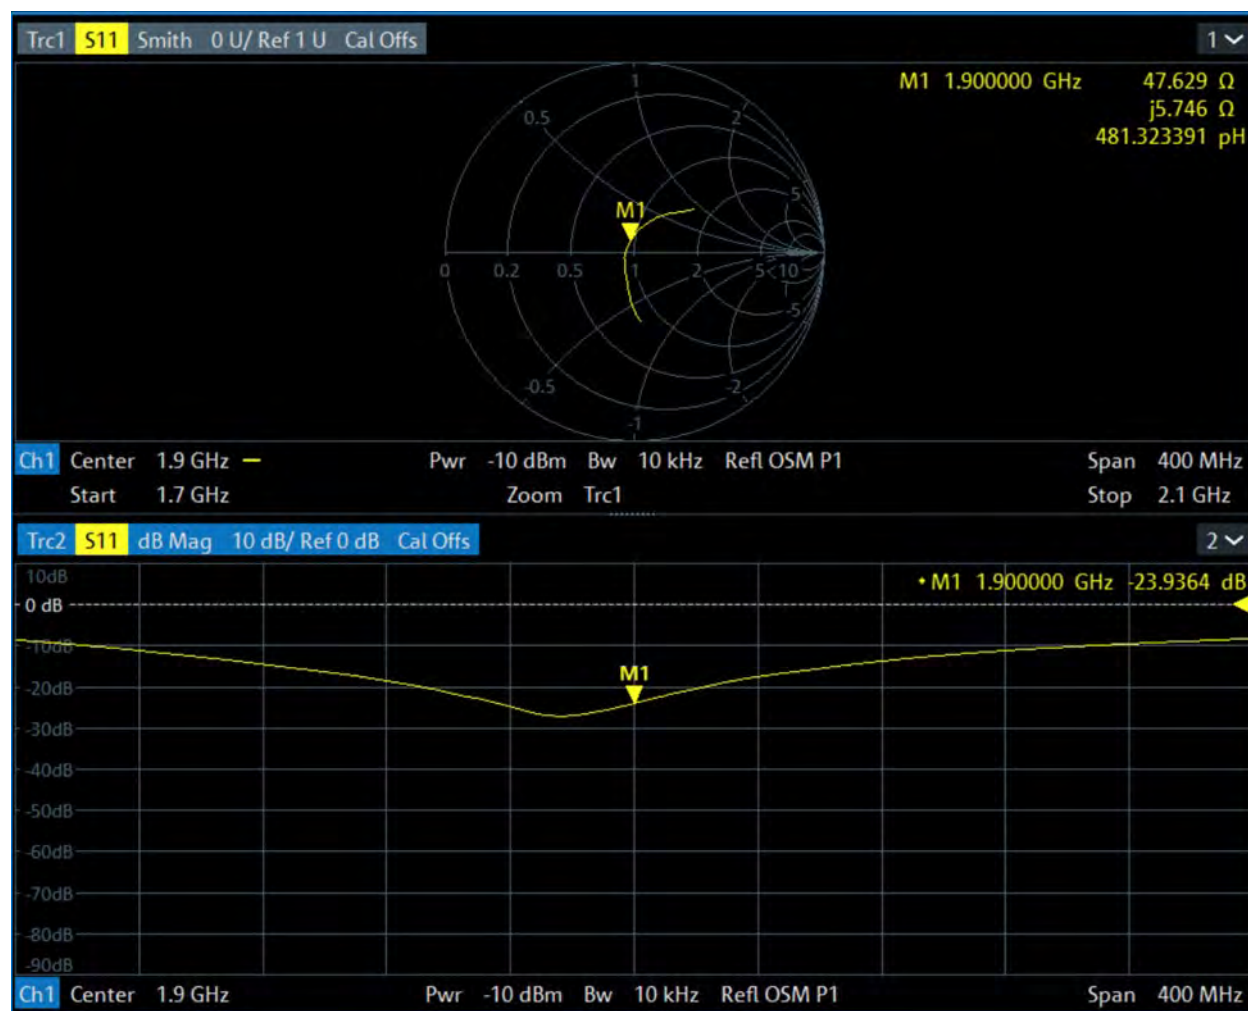

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D1900V2 – SN: 5d252
Description: SAR Validation Dipole at 1900 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/29/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
5d252	1900	11/7/2024	10/6/2023	39.8	2.07	3.77%	21	1.08	2.61%	48.8	48.8	47.6	-1.2	5.9	5.9	5.7	-0.2	-24.4	-24.4	-23.9	11.17%	PASS
5d252	1900	7/29/2025	10/6/2023	39.8	2.02	1.27%	21	1.06	0.71%	48.8	47.6	47.8	0.2	5.9	5.7	5.3	-0.4	-24.4	-23.9	-24.6	-15.64%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

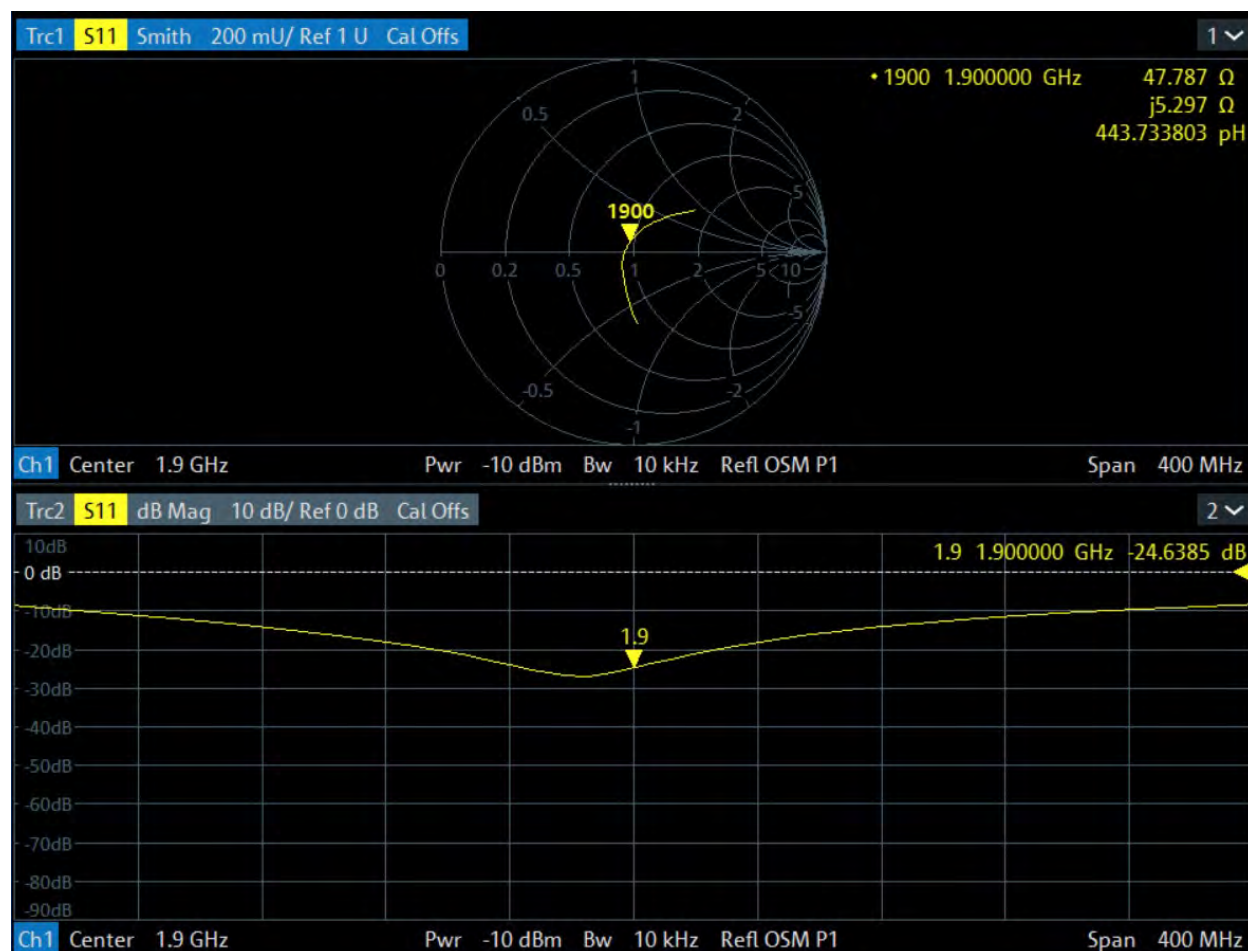



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D2300V2-1139_Oct23**

CALIBRATION CERTIFICATE

Object **D2300V2 - SN:1139**

MAB 11/20/23

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz

Calibration date: **October 09, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	10-Jan-23 (No. EX3-7349_Jan23)	Jan-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
DAE4	SN: 900	09-Aug-23 (No. DAE4-900_Aug23)	Aug-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** Name: **Paulo Pina** Function: **Laboratory Technician**

Approved by: **Sven Kühn** Technical Manager

Signature

[Signature]

[Signature]

Issued: October 12, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2300 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.0 $\pm$ 6 %	1.71 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	49.0 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.01 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.9	1.81 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.2 $\pm$ 6 %	1.84 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	11.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	47.4 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.81 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.2 W/kg $\pm$ 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	45.0 Ω - 0.8 j Ω
Return Loss	- 25.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	43.0 Ω + 0.6 j Ω
Return Loss	- 22.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.164 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 05.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1139

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: $f = 2300$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 38$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.98, 7.98, 7.98) @ 2300 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn900; Calibrated: 09.08.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 116.7 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 23.0 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 6.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 54.5%

Maximum value of SAR (measured) = 19.8 W/kg



0 dB = 19.8 W/kg = 12.97 dBW/kg

Impedance Measurement Plot for Head TSL

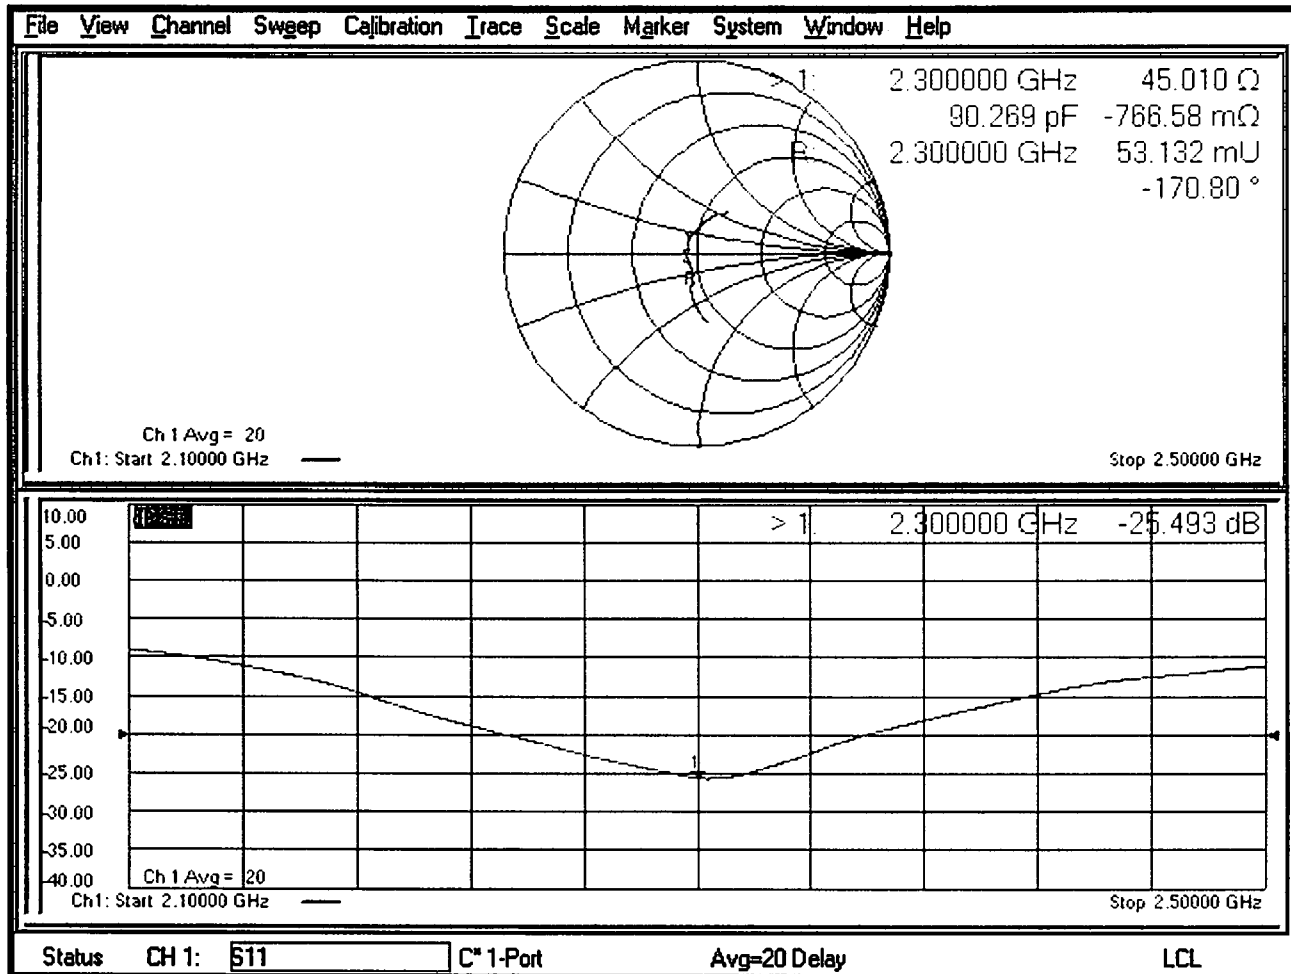

DASY5 Validation Report for Body TSL

Date: 09.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1139

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: $f = 2300$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.97, 7.97, 7.97) @ 2300 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 105.1 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 21.9 W/kg

SAR(1 g) = 11.9 W/kg; SAR(10 g) = 5.81 W/kg


Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 55.5%

Maximum value of SAR (measured) = 18.6 W/kg

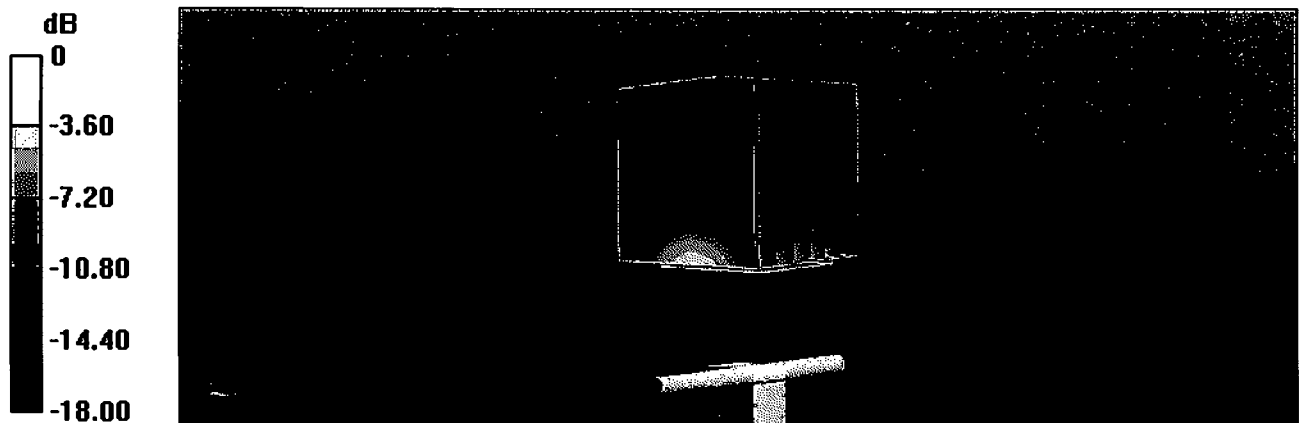

Impedance Measurement Plot for Body TSL

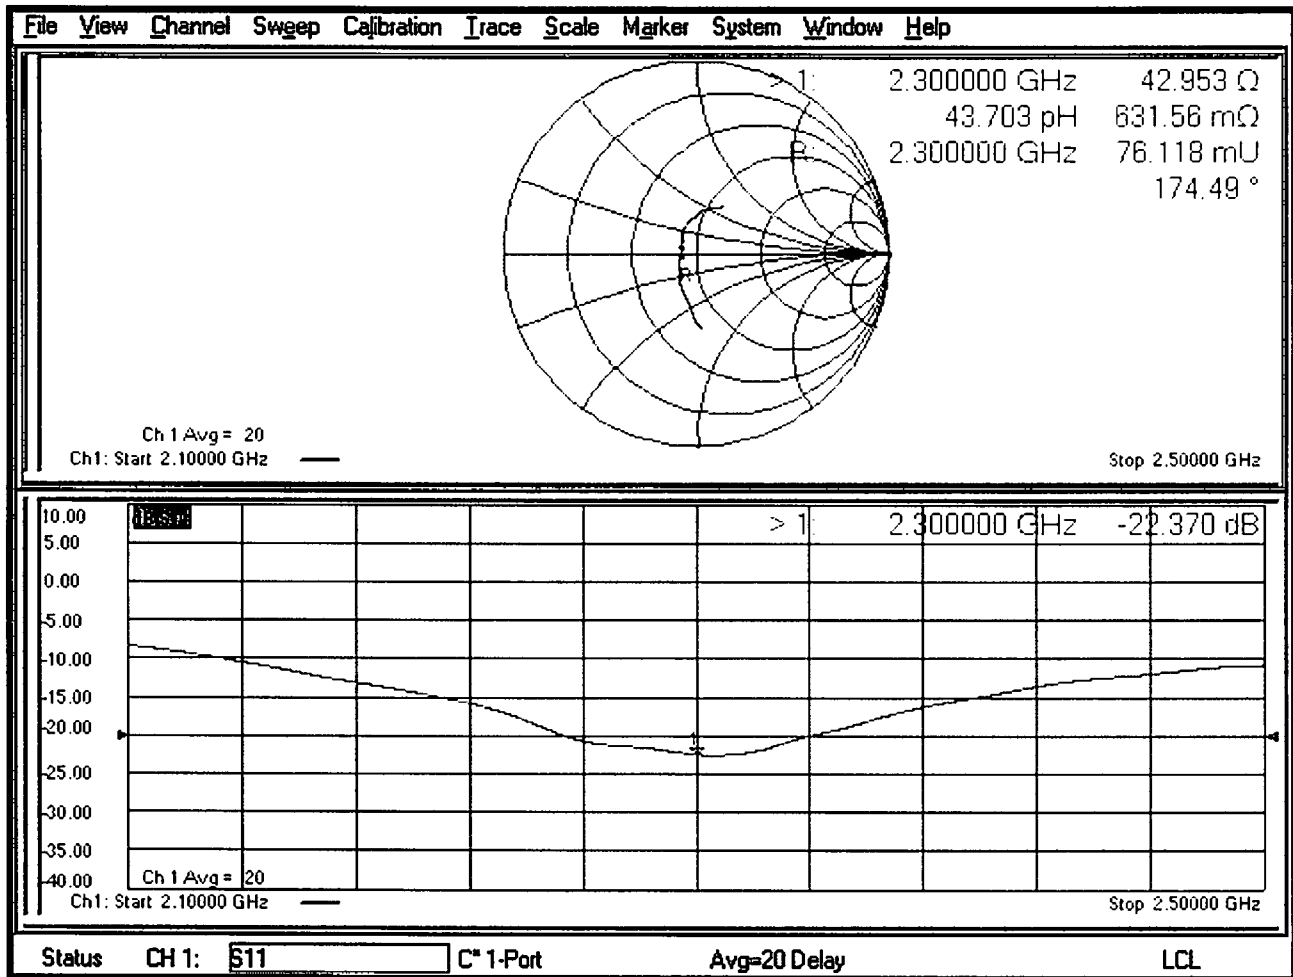

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D2300V2 – SN: 1139
Description: SAR Validation Dipole at 2300 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1139	2300	11/7/2024	10/9/2023	49	2.40	-2.27%	23.7	1.15	-3.18%	45.0	45.4	0.4	-0.8	0.9	1.7	-25.5	-26.1	-13.78%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

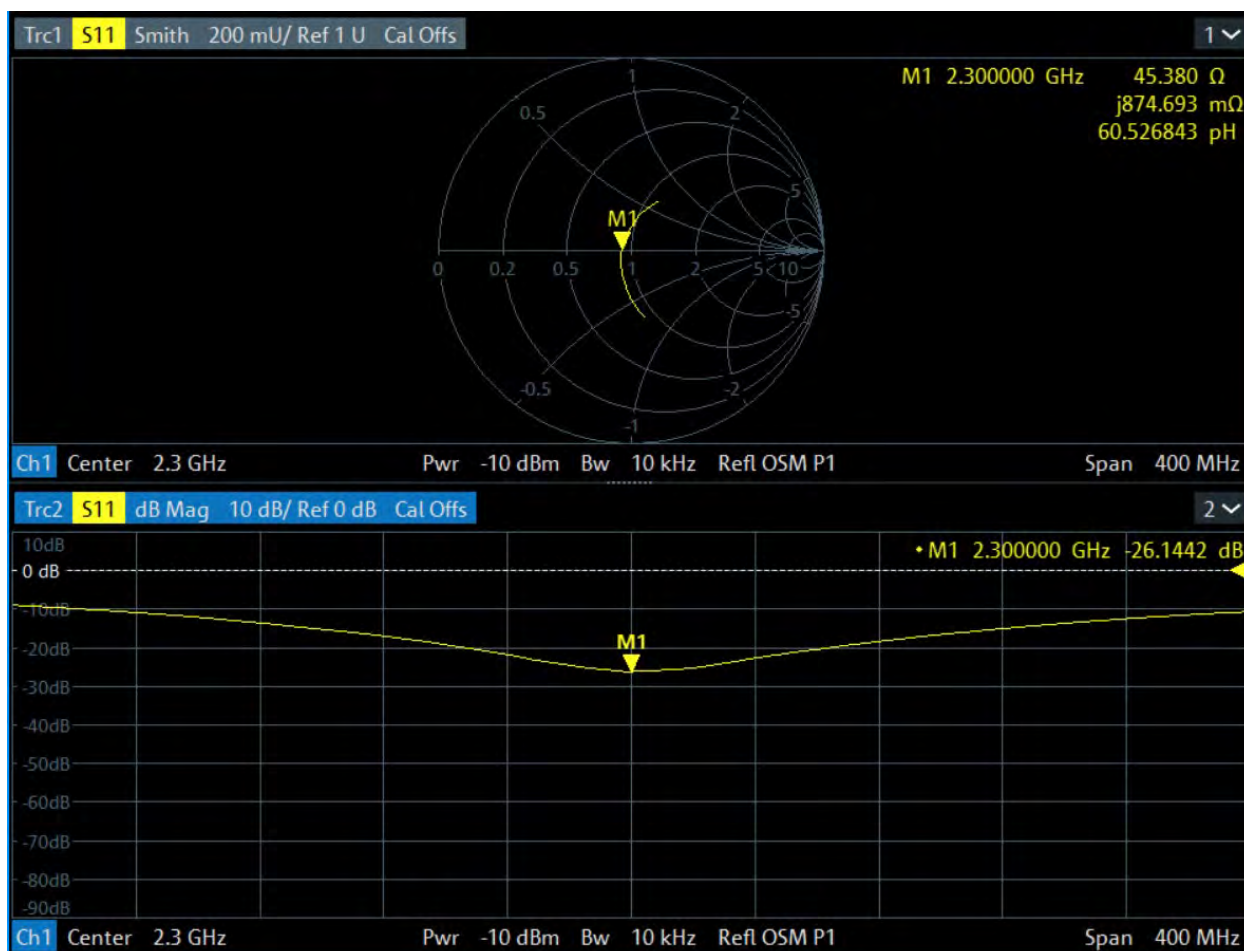

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D2300V2 – SN: 1139
Description: SAR Validation Dipole at 2300 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1139	2300	11/7/2024	10/9/2023	49	2.40	-2.27%	23.7	1.15	-3.18%	45.0	45.0	45.4	0.4	-0.8	-0.8	0.9	1.7	-25.5	-25.5	-26.1	-13.78%	PASS
1139	2300	7/30/2025	10/9/2023	49	2.32	-5.53%	23.7	1.12	-5.71%	45.0	45.4	45.1	-0.3	-0.8	0.9	1.1	0.2	-25.5	-26.1	-25.6	13.45%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

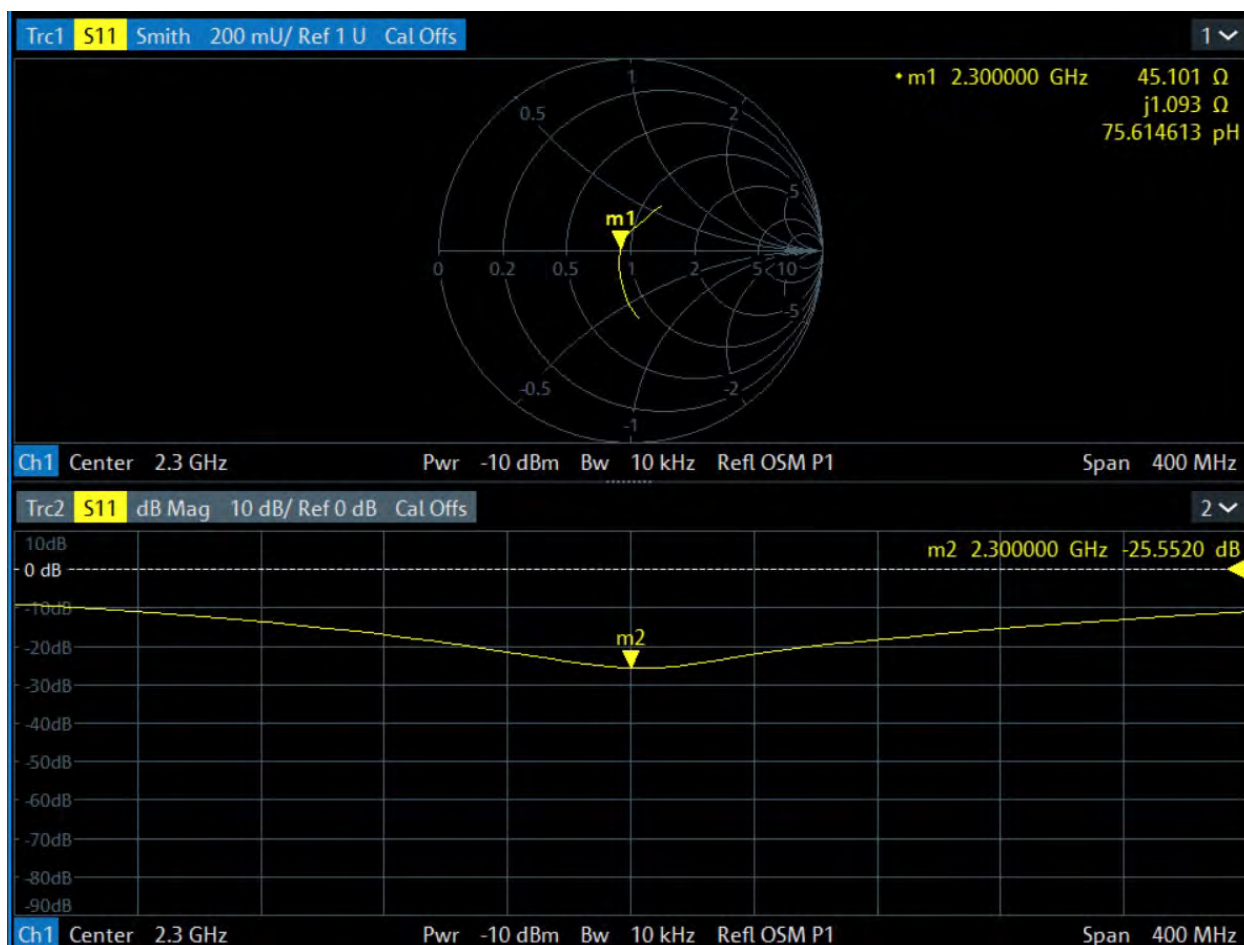



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

RF Safety Lab
Catonsville, USA

Certificate No.

D2450V2-1112_Nov24

CALIBRATION CERTIFICATE

MAB 11/21/24

Object D2450V2 - SN: 1112

Calibration procedure(s) QA CAL-05.v12
Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz

Calibration date November 15, 2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Cal
Power Sensor R&S NRP-33T	SN: 100967	28-Mar-24 (No. 217-04038)	Mar-25
Power Sensor R&S NRP18A	SN: 101859	22-Jul-24 (No. 4030A315008547)	Jul-25
Spectrum Analyzer R&S FSV40	SN: 101832	25-Jan-24 (No. 4030-315007551)	Jan-25
Mismatch; Short [S4188] Attenuator [S4423]	SN: 1152	28-Mar-24 (No. 217-04050)	Mar-25
OCP DAK-12	SN: 1016	24-Sep-24 (No. OCP-DAK12-1016_Sep24)	Sep-25
OCP DAK-3.5	SN: 1249	23-Sep-24 (No. OCP-DAK3.5-1249_Sep24)	Sep-25
Reference Probe EX3DV4	SN: 7349	03-Jun-24 (No. EX3-7349_Jun24)	Jun-25
DAE4ip	SN: 1836	28-Oct-24 (No. DAE4ip-1836_Oct24)	Oct-25

Secondary Standards	ID	Check Date (in house)	Scheduled Check
ACAD Source Box	SN: 1000	28-May-24 (No. 675-ACAD_Source_Box-240528)	May-25
Signal Generator R&S SMB100A	SN: 182081	28-May-24 (No. 675-CAL16-S4588-240528)	May-25
Mismatch; SMA	SN: 1102	22-May-24 (No. 675-Mismatch_SMA-240522)	May-25

	Name	Function	Signature
Calibrated by	Paulo Pina	Laboratory Technician	
Approved by	Sven Kühn	Technical Manager	

Issued: November 15, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 0108**

Glossary

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation

- DASY System Handbook

Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY8 Module SAR	16.4.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with spacer
Zoom Scan Resolution	dx, dy = 5mm, dz = 1.5mm	Graded Ratio = 1.5 mm (Z direction)
Frequency	2450MHz $\pm$ 1MHz	

Head TSL parameters at 2450 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2)°C	37.8 $\pm$ 6%	1.83 mho/m $\pm$ 6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 2450 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	12.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	50.6 W/kg $\pm$ 17.0% (k = 2)

SAR averaged over 10 cm³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	5.95 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg $\pm$ 16.5% (k = 2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL at 2450 MHz**

Impedance	$51.6 \Omega + 4.2 j\Omega$
Return Loss	-27.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.152 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D2450V2 - SN1112	2450	HSL	24

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10		CW, 0--	2450, 0	7.24	1.83	37.8

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 - SN7349, 2024-06-03	DAE4ip Sn1836, 2024-10-28

Scans Setup


	Zoom Scan
Grid Extents [mm]	30 x 30 x 30
Grid Steps [mm]	5.0 x 5.0 x 1.5
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.5
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	12.7
psSAR10g [W/Kg]	5.95
Power Drift [dB]	0.00
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

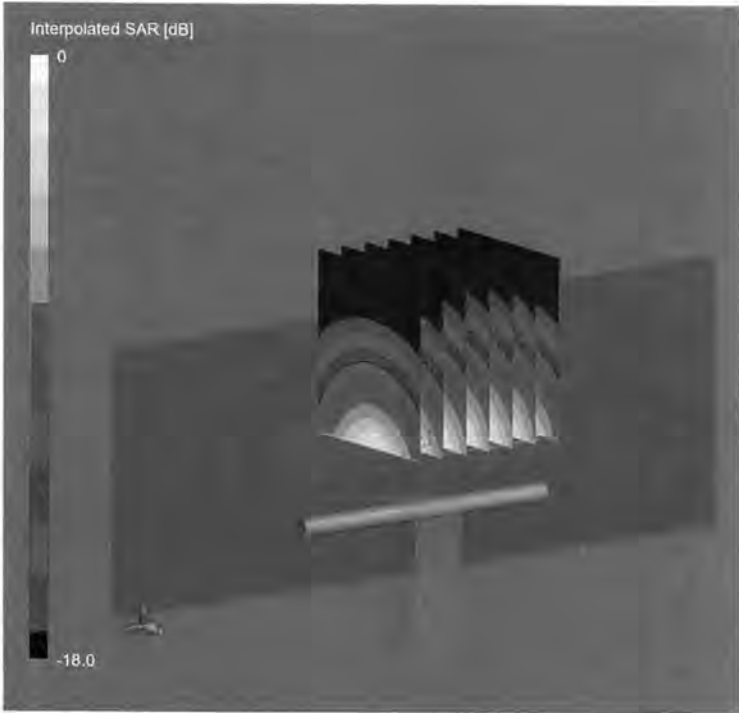

0 dB = 26.1 W/Kg

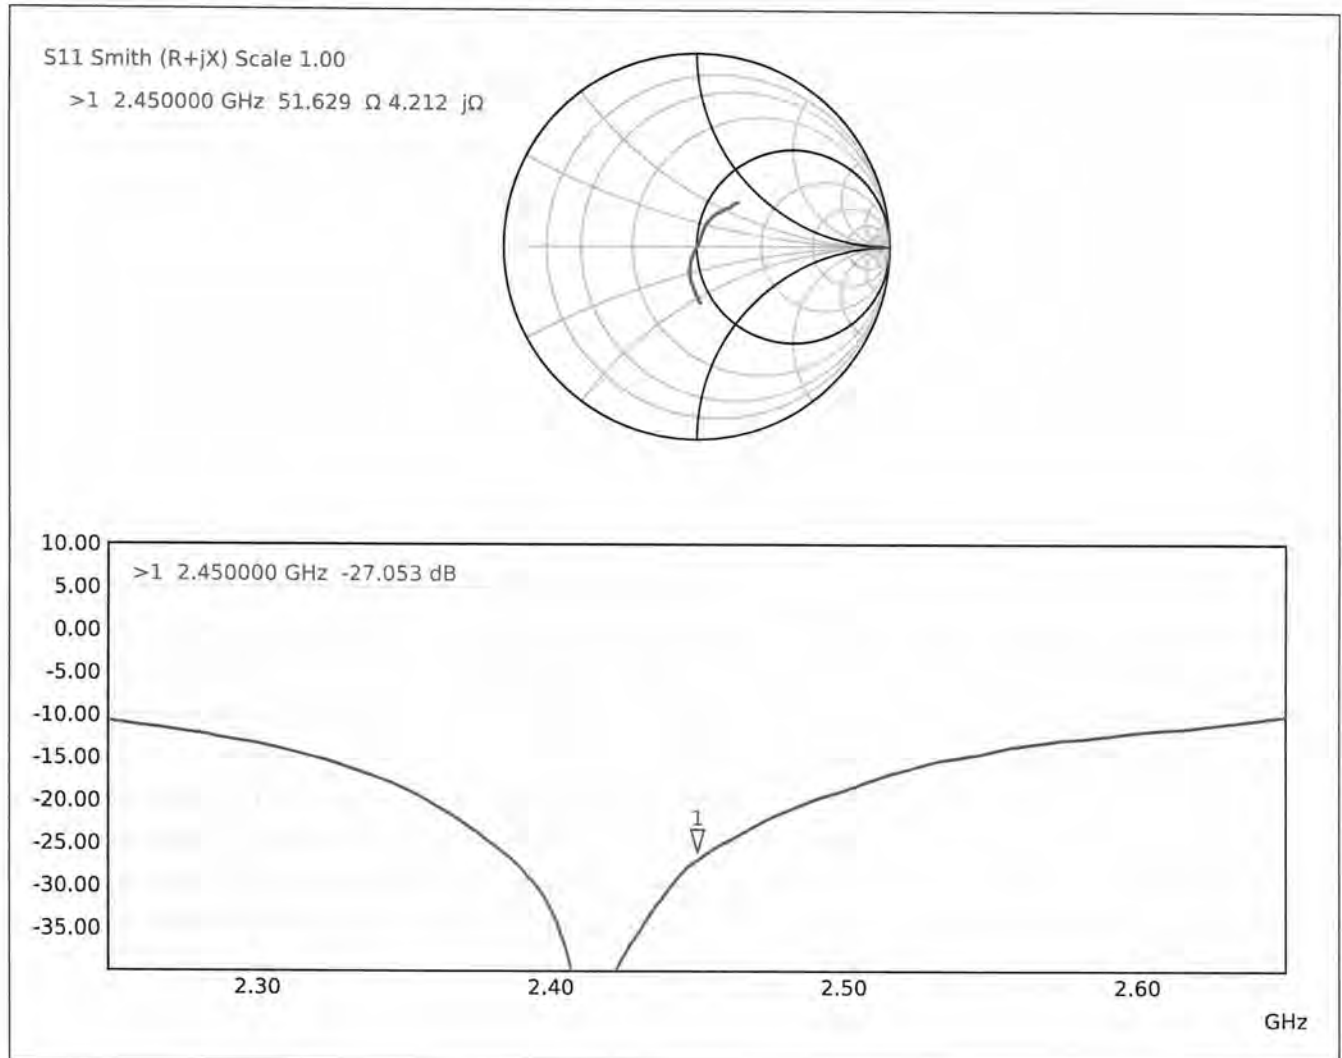Impedance Measurement Plot for Head TSL

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D2450V2 – SN: 1112
Description: SAR Validation Dipole at 2450 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/29/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
1112	2450	11/21/2024	11/15/2024							51.6	51.6	49.4	-2.2	4.2	4.3	4.3	0.1	-27.1	-27.1	-27.3	-4.22%	PASS	In-house check after Calibration
1112	2450	7/29/2025	11/15/2024	50.6	2.53	-0.54%	23.7	1.19	0.18%	51.6	49.4	51.6	-2.2	4.2	4.3	3.7	-0.6	-27.1	-27.3	-28.0	-13.97%	PASS	-

Impedance and Return-Loss Measurement Plot for Head TSL

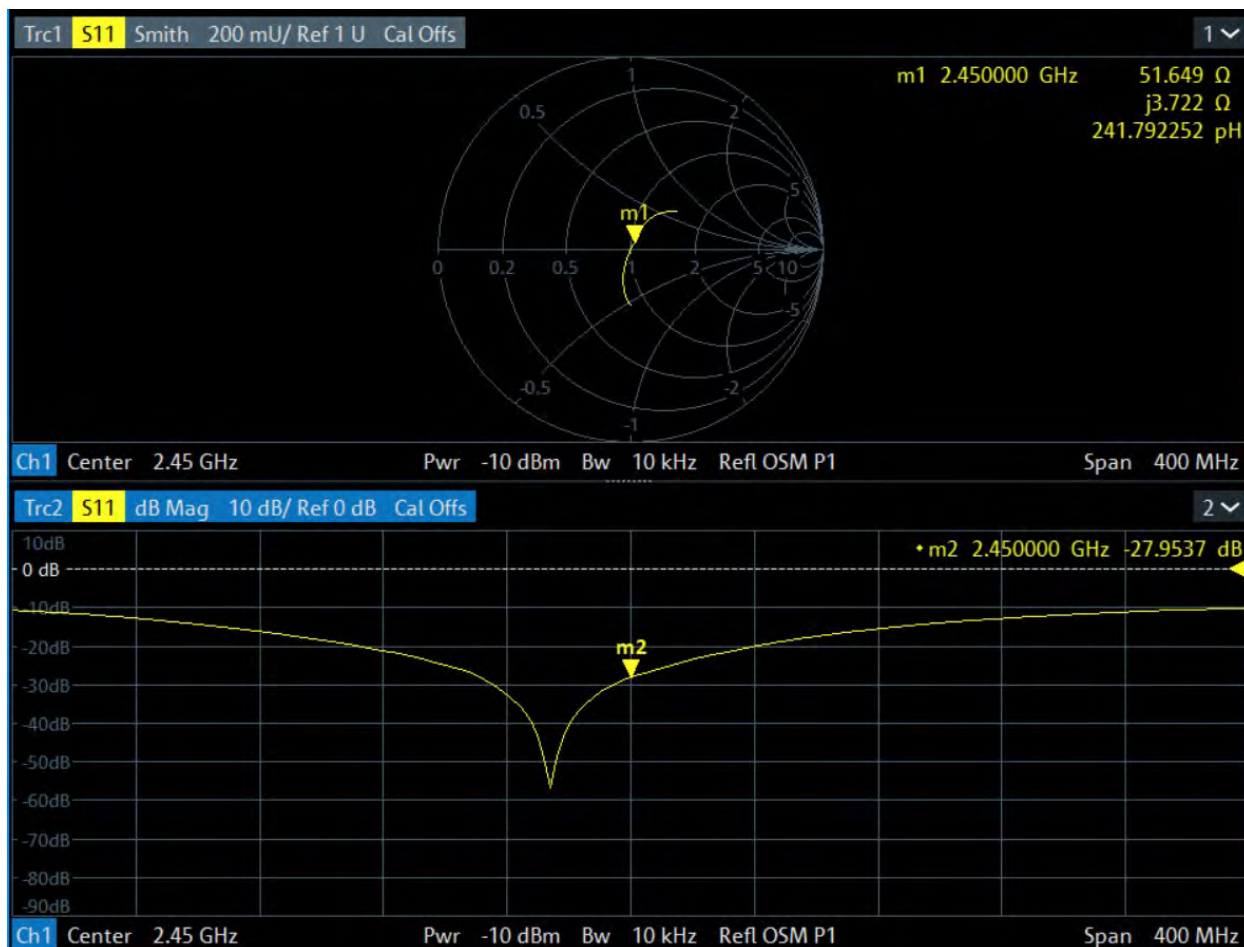



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

RF Safety Lab
 Catonsville, USA

Certificate No.

D2600V2-1215_Nov24

CALIBRATION CERTIFICATE

APB 11/21/24

Object **D2600V2 - SN: 1215**

Calibration procedure(s) **QA CAL-05.v12**
Calibration Procedure for SAR Validation Sources between 0.7 - 3 GHz

Calibration date **November 15, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Cal
Power Sensor R&S NRP-33T	SN: 100967	28-Mar-24 (No. 217-04038)	Mar-25
Power Sensor R&S NRP18A	SN: 101859	22-Jul-24 (No. 4030A315008547)	Jul-25
Spectrum Analyzer R&S FSV40	SN: 101832	25-Jan-24 (No. 4030-315007551)	Jan-25
Mismatch; Short [S4188] Attenuator [S4423]	SN: 1152	28-Mar-24 (No. 217-04050)	Mar-25
OCP DAK-12	SN: 1016	24-Sep-24 (No. OCP-DAK12-1016_Sep24)	Sep-25
OCP DAK-3.5	SN: 1249	23-Sep-24 (No. OCP-DAK3.5-1249_Sep24)	Sep-25
Reference Probe EX3DV4	SN: 7349	03-Jun-24 (No. EX3-7349_Jun24)	Jun-25
DAE4ip	SN: 1836	28-Oct-24 (No. DAE4ip-1836_Oct24)	Oct-25

Secondary Standards	ID	Check Date (in house)	Scheduled Check
ACAD Source Box	SN: 1000	28-May-24 (No. 675-ACAD_Source_Box-240528)	May-25
Signal Generator R&S SMB100A	SN: 182081	28-May-24 (No. 675-CAL16-S4588-240528)	May-25
Mismatch; SMA	SN: 1102	22-May-24 (No. 675-Mismatch_SMA-240522)	May-25

	Name	Function	Signature
Calibrated by	Paulo Pina	Laboratory Technician	
Approved by	Sven Kühn	Technical Manager	
Issued: November 15, 2024 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: SCS 0108

Glossary

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation

- DASY System Handbook

Methods Applied and Interpretation of Parameters

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY8 Module SAR	16.4.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with spacer
Zoom Scan Resolution	dx, dy = 5mm, dz = 1.5mm	Graded Ratio = 1.5 mm (Z direction)
Frequency	2600MHz $\pm$ 1MHz	

Head TSL parameters at 2600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2)°C	37.2 $\pm$ 6%	1.99 mho/m $\pm$ 6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 2600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	13.9 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	55.3 W/kg $\pm$ 17.0% (k = 2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	24 dBm input power	6.25 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.9 W/kg $\pm$ 16.5% (k = 2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL at 2600 MHz**

Impedance	46.9 Ω + 0.1 j Ω
Return Loss	-29.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.142 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D2600V2 - SN1215	2600	HSL	24

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		2600, 0	7.3	1.99	37.2

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 - SN7349, 2024-06-03	DAE4ip Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	30 x 30 x 30
Grid Steps [mm]	5.0 x 5.0 x 1.5
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.5
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured


Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	13.9
psSAR10g [W/Kg]	6.25
Power Drift [dB]	0.01
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

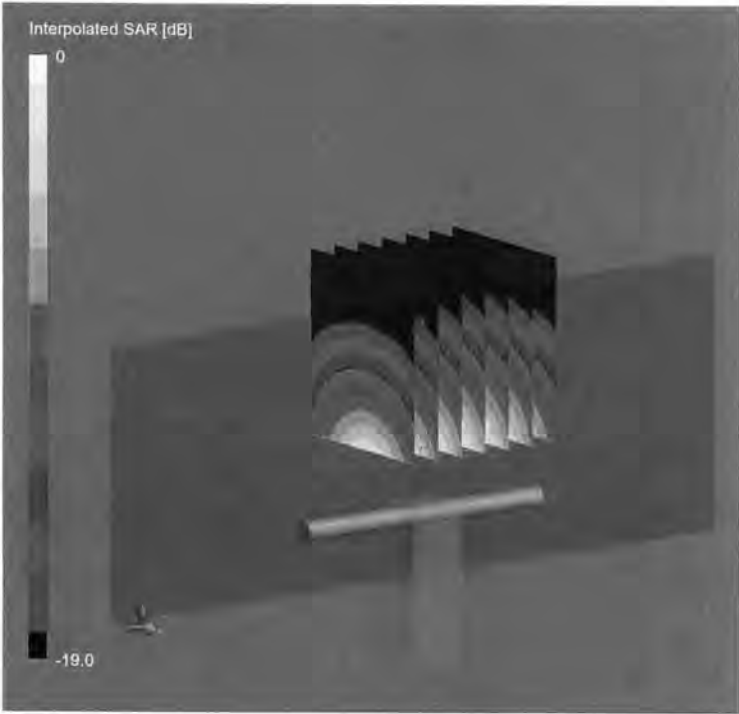

0 dB = 29.9 W/Kg

Impedance Measurement Plot for Head TSL

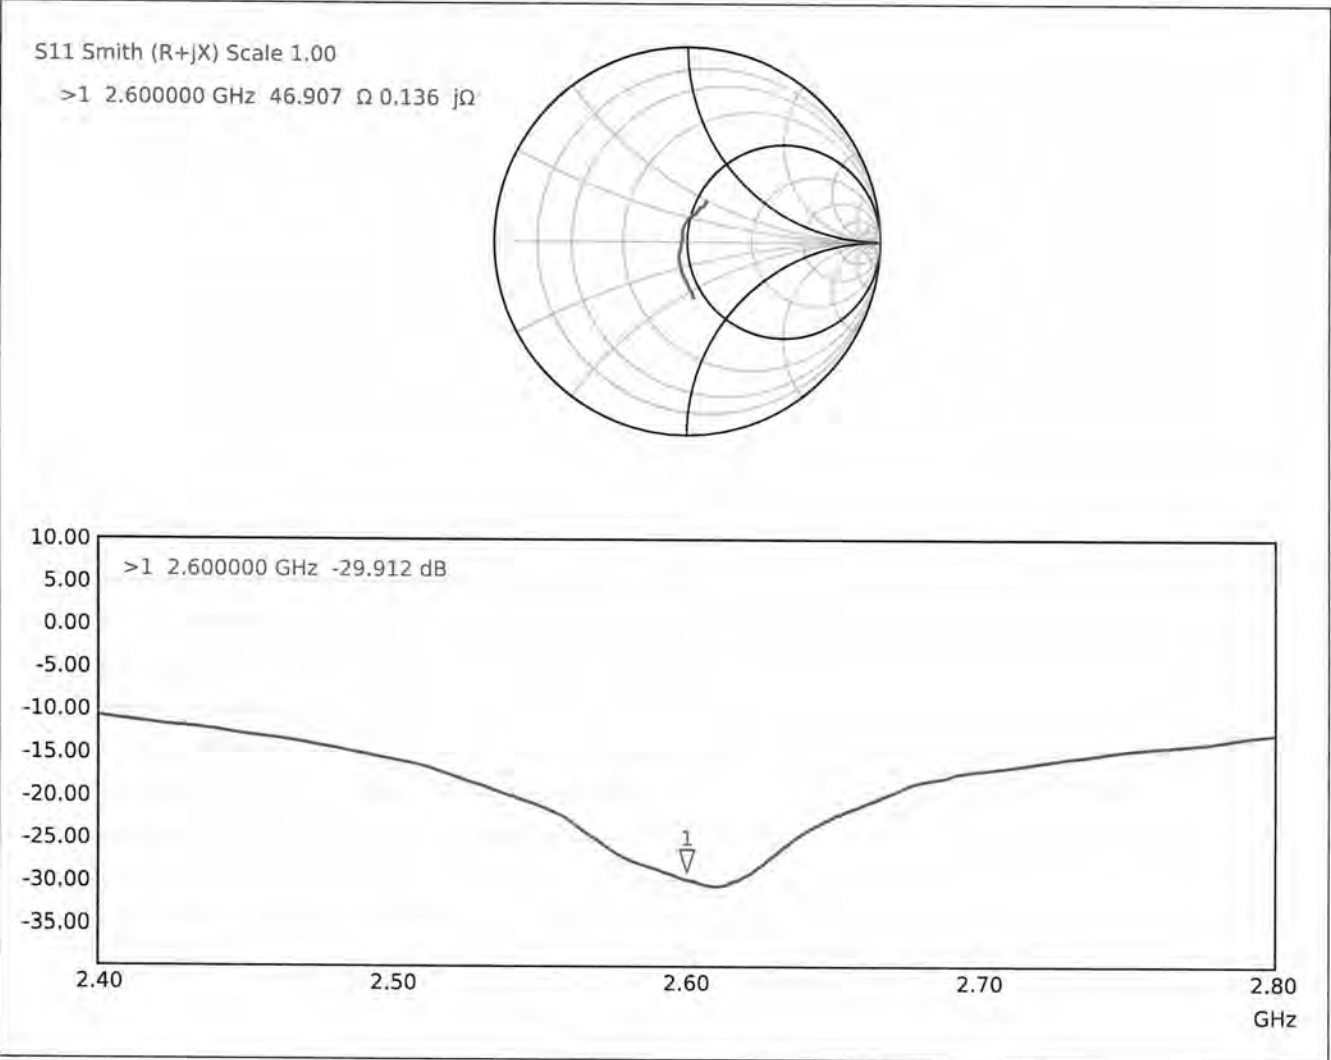

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D2600V2 – SN: 1215
Description: SAR Validation Dipole at 2600 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/29/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	

Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
1215	2600	11/21/2024	11/15/2024							46.9	46.9	47.2	0.3	0.1	0.1	1.3	1.2	-29.9	-29.9	-29.9	-0.03%	PASS	In-house check after Calibration
1215	2600	7/29/2025	11/15/2024	55.3	2.59	-8.55%	24.9	1.17	-6.25%	46.9	47.2	47.3	0.1	0.1	1.3	1.0	-0.3	-29.9	-29.9	-29.4	12.20%	PASS	-



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D3500V2-1154_Oct23**

CALIBRATION CERTIFICATE

Object **D3500V2 - SN:1154**

MAR 11/20/23

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **October 02, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 3503	07-Mar-23 (No. EX3-3503_Mar23)	Mar-24
DAE4	SN: 601	19-Dec-22 (No. DAE4-601_Dec22)	Dec-23

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** Function: **Laboratory Technician**

Approved by: **Sven Kühn** Technical Manager

Signature

Issued: October 6, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	3500 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	37.9	2.91 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	37.2 $\pm$ 6 %	2.97 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.57 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	65.1 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.47 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg $\pm$ 19.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	51.3	3.31 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.5 $\pm$ 6 %	3.29 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	6.25 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	62.7 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.37 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.7 W/kg $\pm$ 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.3 Ω - 3.2 j Ω
Return Loss	- 28.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	54.8 Ω - 0.6 j Ω
Return Loss	- 26.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.132 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 02.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3500 MHz; Type: D3500V2; Serial: D3500V2 - SN:1154

Communication System: UID 0 - CW; Frequency: 3500 MHz

Medium parameters used: $f = 3500$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 37.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.91, 7.91, 7.91) @ 3500 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100 mW, d=10mm, f=3500MHz/Zoom Scan, dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.83 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 6.57 W/kg; SAR(10 g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8.2 mm


Ratio of SAR at M2 to SAR at M1 = 74.6%

Maximum value of SAR (measured) = 12.4 W/kg

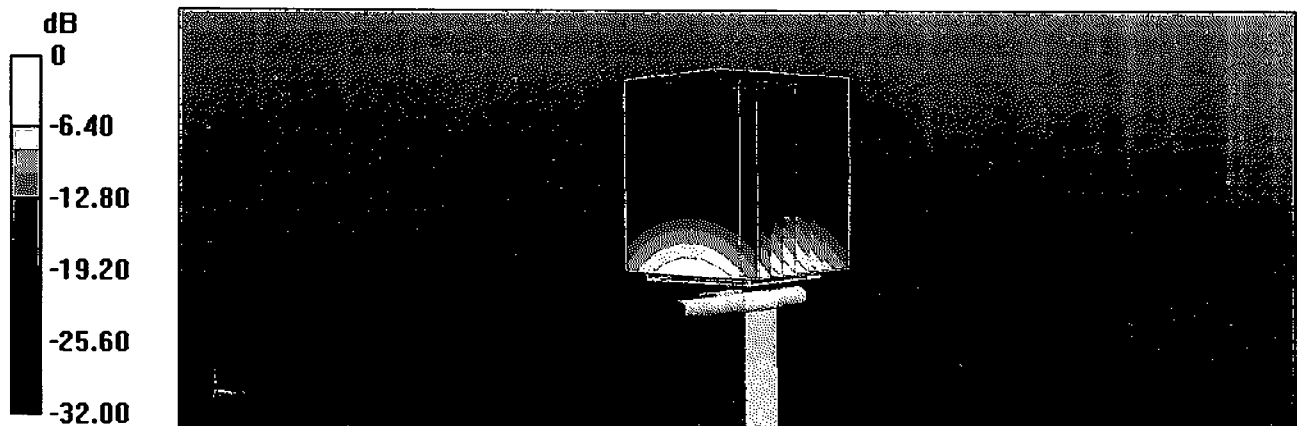

0 dB = 12.4 W/kg = 10.93 dBW/kg

Impedance Measurement Plot for Head TSL

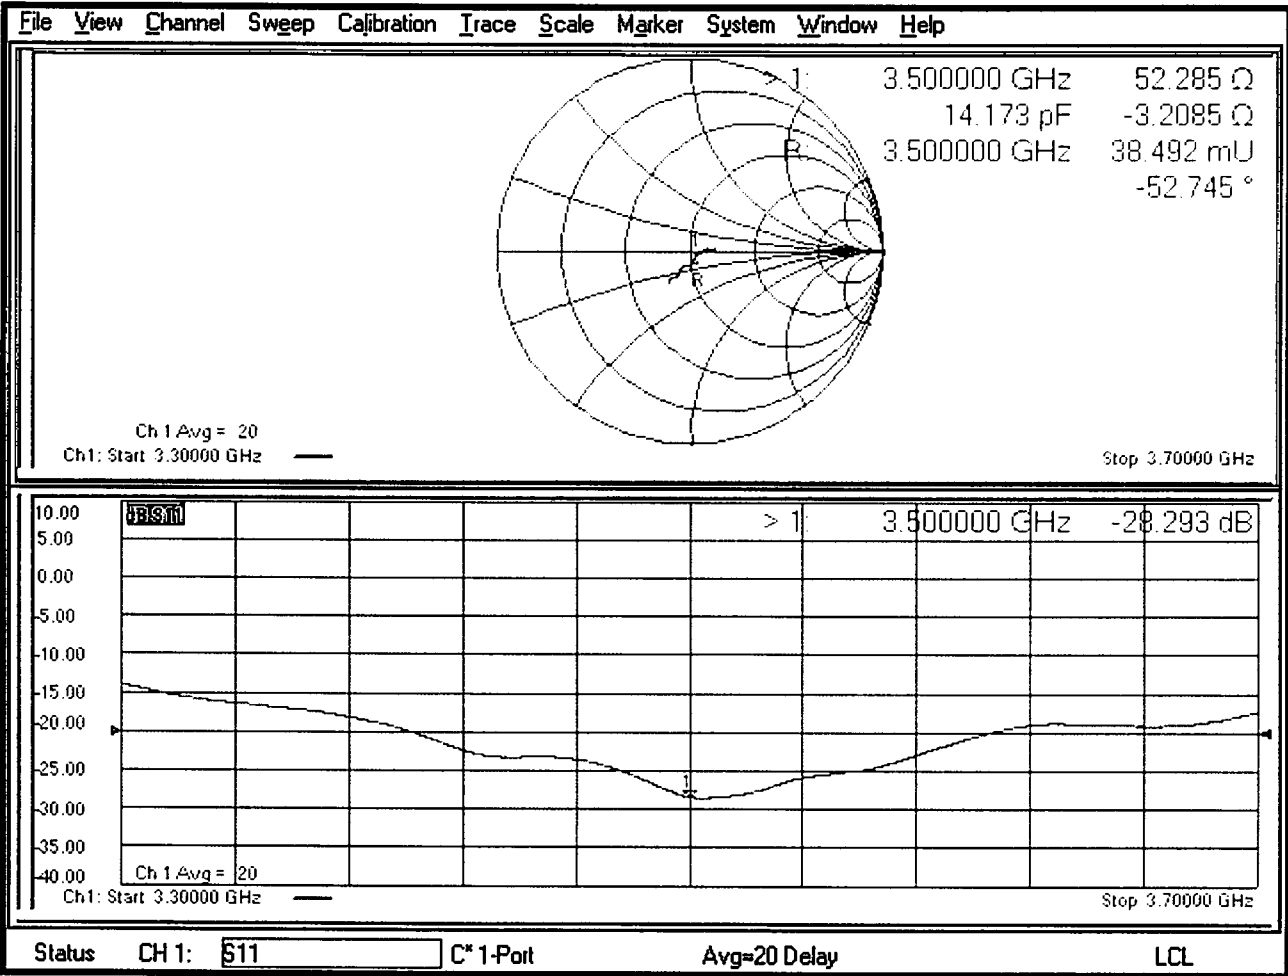

DASY5 Validation Report for Body TSL

Date: 02.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3500 MHz; Type: D3500V2; Serial: D3500V2 - SN:1154

Communication System: UID 0 - CW; Frequency: 3500 MHz

Medium parameters used: $f = 3500$ MHz; $\sigma = 3.29$ S/m; $\epsilon_r = 51.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.46, 7.46, 7.46) @ 3500 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=100 mW, d=10mm, f=3500MHz/Zoom Scan , dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 63.36 V/m; Power Drift = 0.00 dB


Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 6.25 W/kg; SAR(10 g) = 2.37 W/kg


Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 77.2%

Maximum value of SAR (measured) = 11.4 W/kg

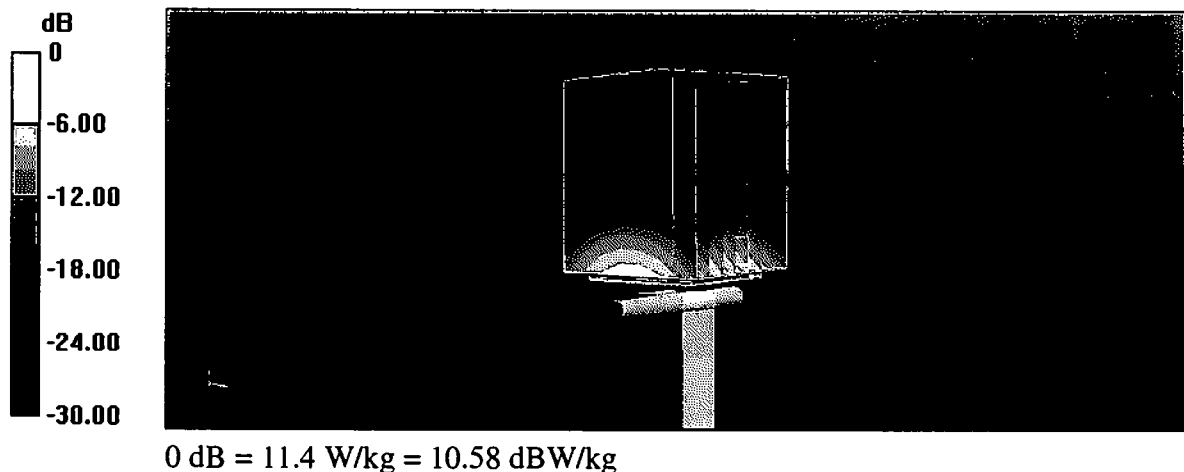

Impedance Measurement Plot for Body TSL

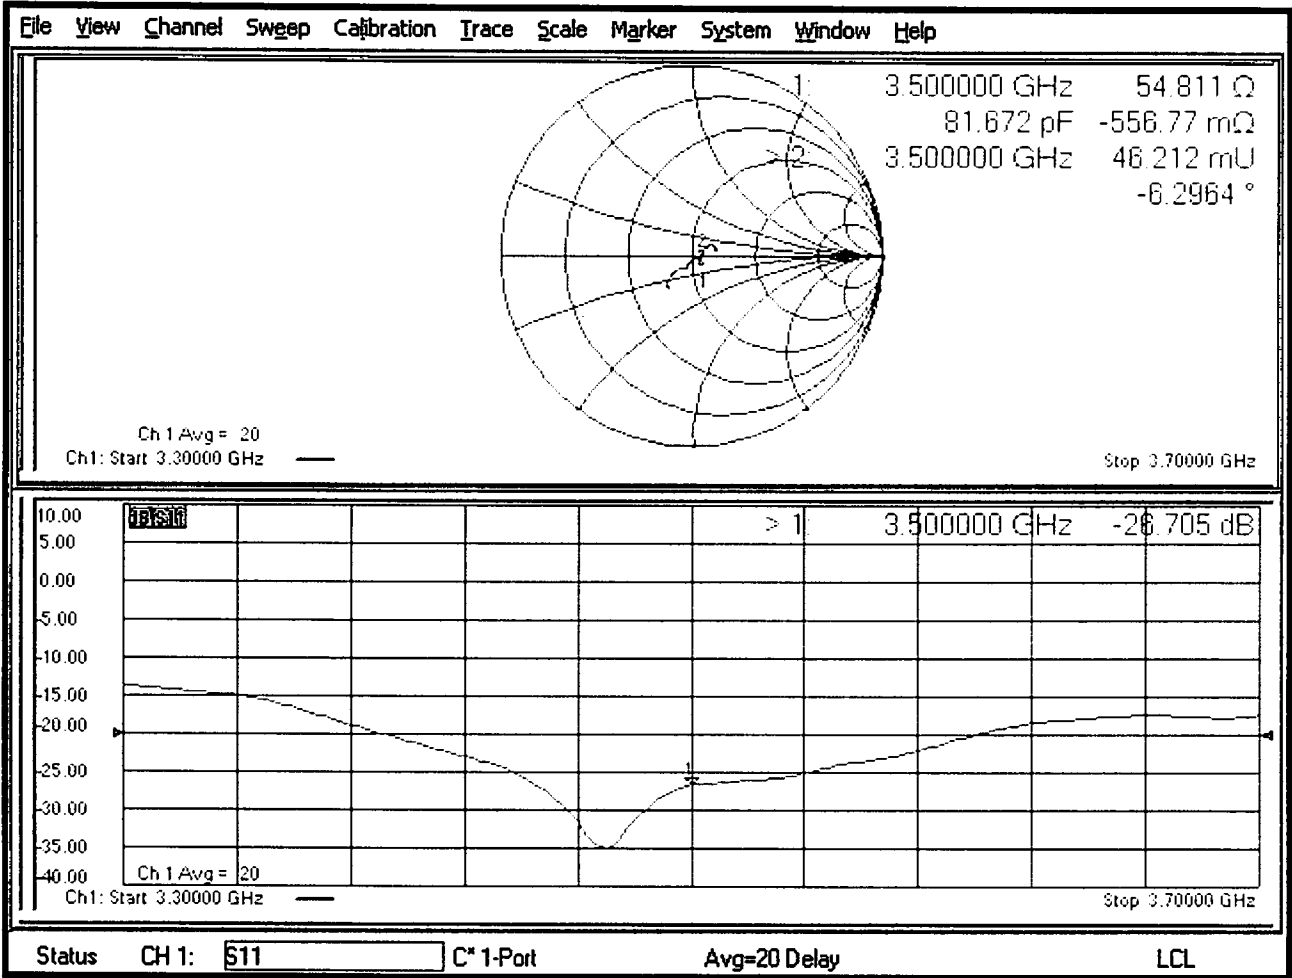

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D3500V2 – SN: 1154
Description: SAR Validation Dipole at 3500 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	

Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:


1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1154	3500	11/7/2024	10/2/2023	65.1	3.00	-8.05%	24.6	1.14	-7.54%	52.3	50.6	-1.7	-3.2	-3.8	-0.6	-28.3	-28.4	-2.66%	PASS



Impedance and Return-Loss Measurement Plot for Head TSL

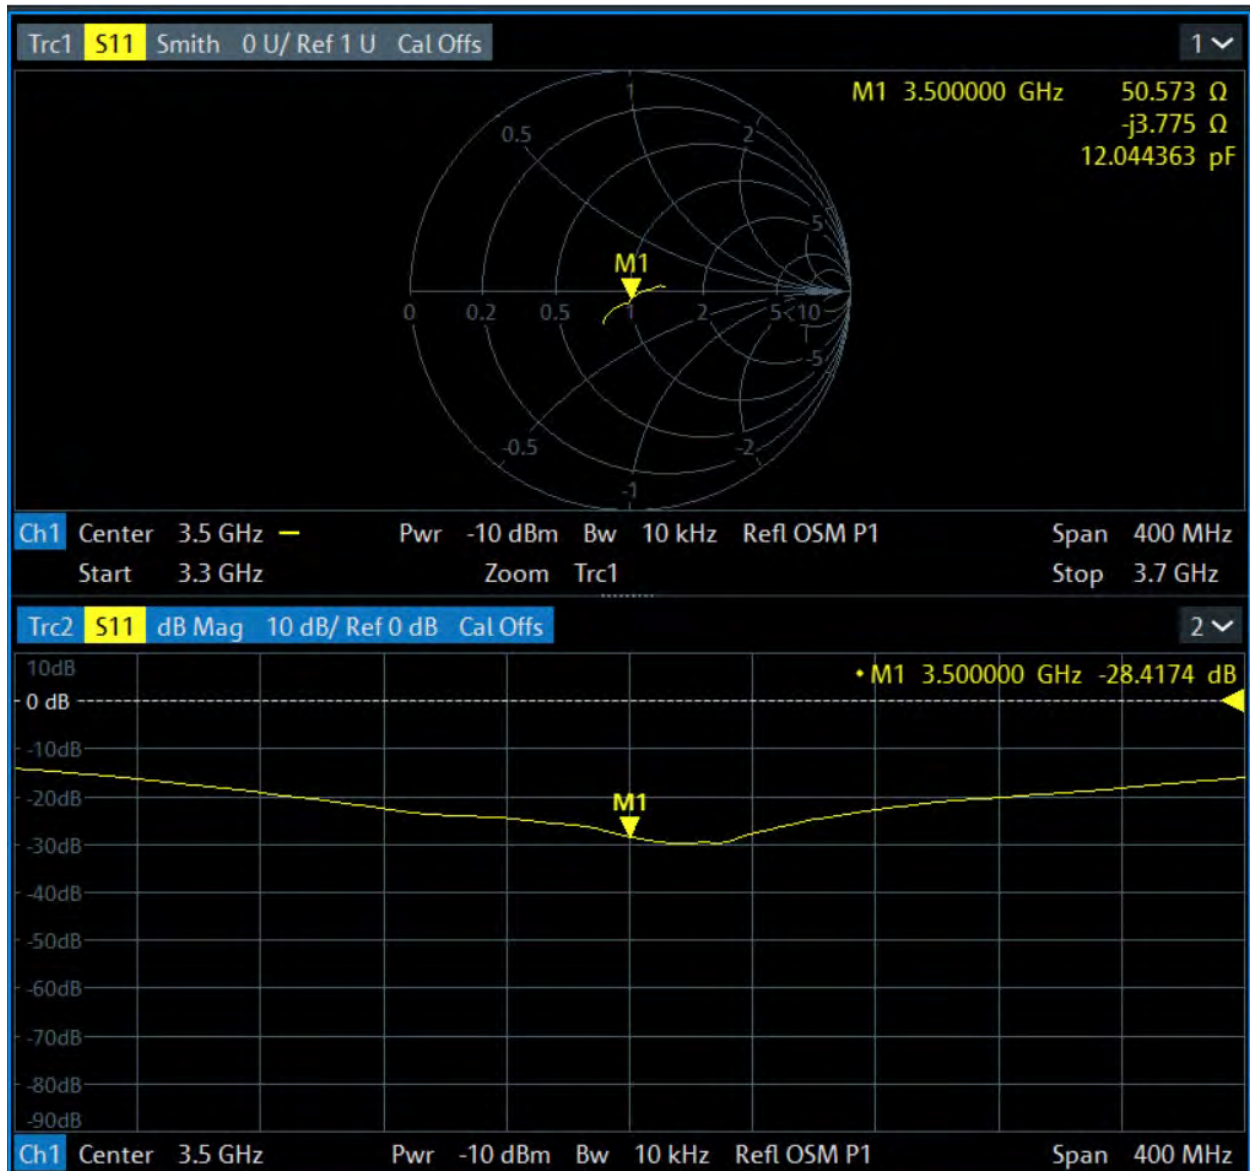

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D3500V2 – SN: 1154
Description: SAR Validation Dipole at 3500 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1844	11/6/2024	11/6/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7853	11/7/2024	11/7/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	YL	Engineer	
Approved By:	PN	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.


The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev(%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1154	3500	11/7/2024	10/2/2023	65.1	3.00	-8.05%	24.6	1.14	-7.54%	52.3	52.3	50.6	-1.7	-3.2	-3.2	-3.8	-0.6	-28.3	-28.3	-28.4	-2.66%	PASS
1154	3500	7/30/2025	10/2/2023	65.1	2.94	-9.89%	24.6	1.13	-8.35%	52.3	50.6	51.5	0.9	-3.2	-3.8	-3.4	0.4	-28.3	-28.4	-28.6	-4.39%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

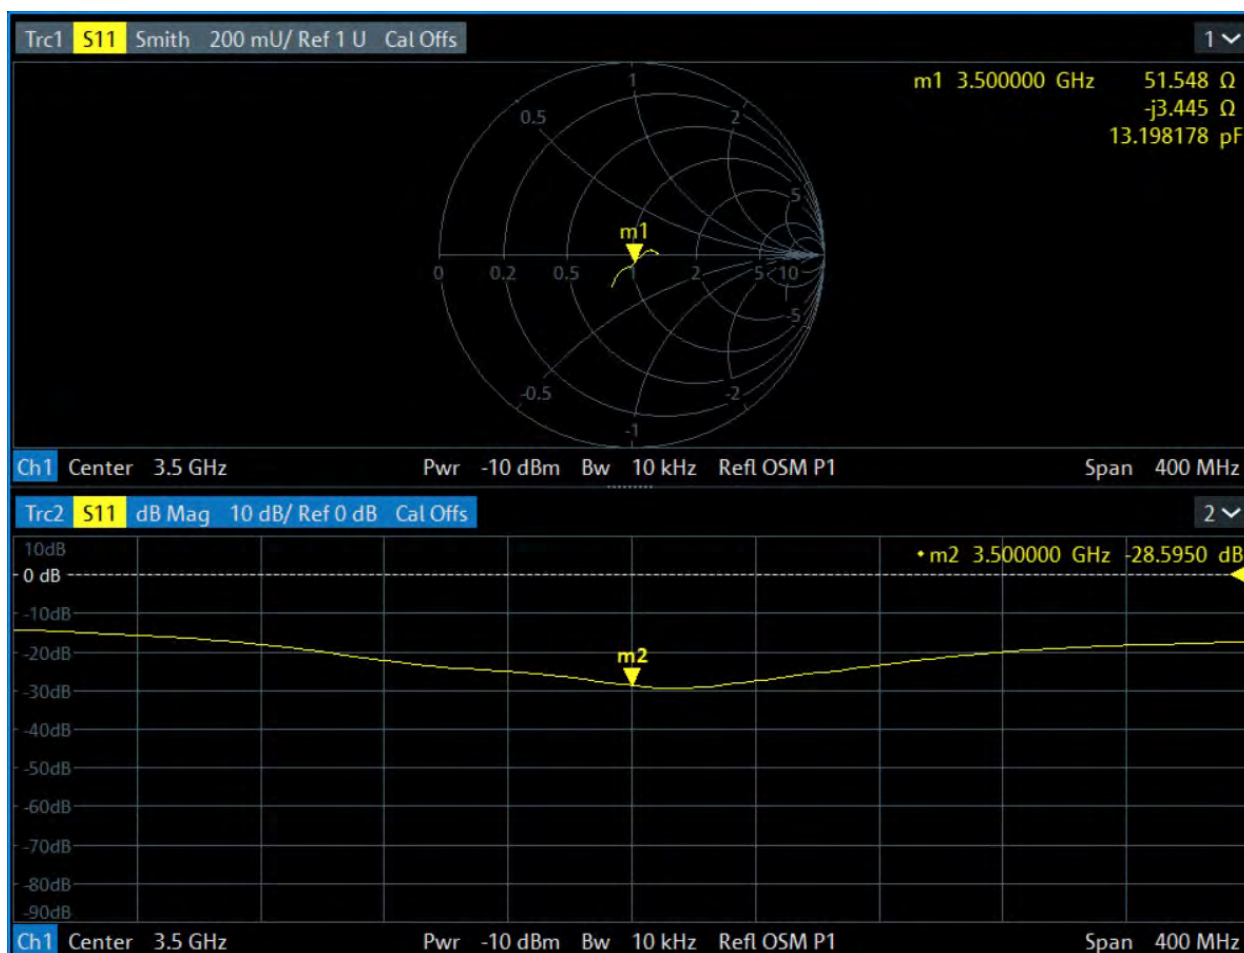

Impedance and Return-Loss Measurement Plot for Head TSL

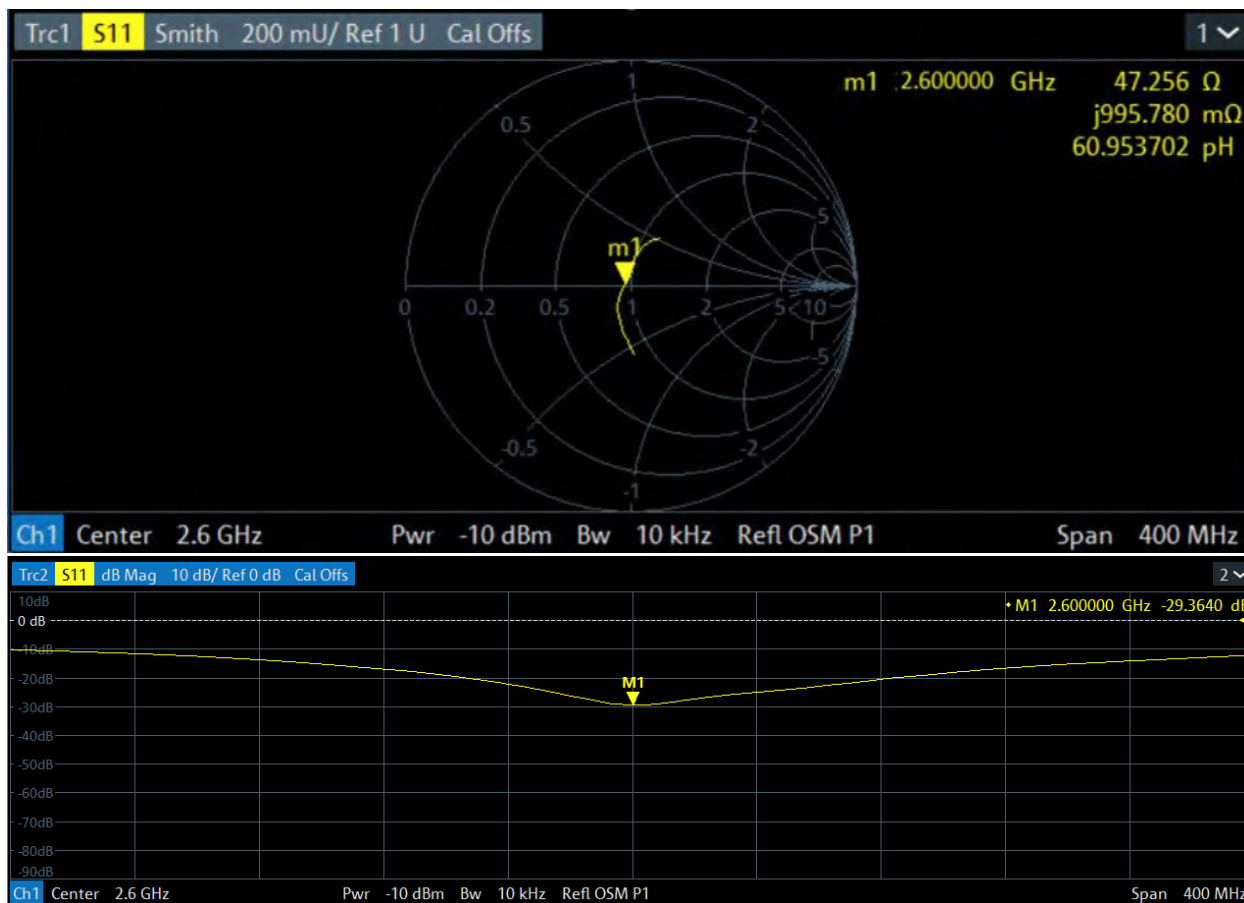



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D3700V2-1130_Oct23**

CALIBRATION CERTIFICATE

Object **D3700V2 - SN:1130**

MAS 11/20/23

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **October 12, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 3503	07-Mar-23 (No. EX3-3503_Mar23)	Mar-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

	Name	Function	Signature
Calibrated by:	Paulo Pina	Laboratory Technician	
Approved by:	Sven Kühn	Technical Manager	

Issued: October 12, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	3700 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	37.7	3.12 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	37.7 $\pm$ 6 %	3.09 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.65 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	66.6 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg $\pm$ 19.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	51.0	3.55 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.8 $\pm$ 6 %	3.49 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	6.25 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	62.9 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.29 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.0 W/kg $\pm$ 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	46.0 Ω + 4.4 j Ω
Return Loss	- 24.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.1 Ω + 6.1 j Ω
Return Loss	- 21.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.129 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 12.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3700 MHz; Type: D3700V2; Serial: D3700V2 - SN:1130

Communication System: UID 0 - CW; Frequency: 3700 MHz

Medium parameters used: $f = 3700$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.73, 7.73, 7.73) @ 3700 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100 mW, d=10mm, f=3700MHz/Zoom Scan, dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.63 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 6.65 W/kg; SAR(10 g) = 2.45 W/kg


Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 74.1%

Maximum value of SAR (measured) = 12.8 W/kg

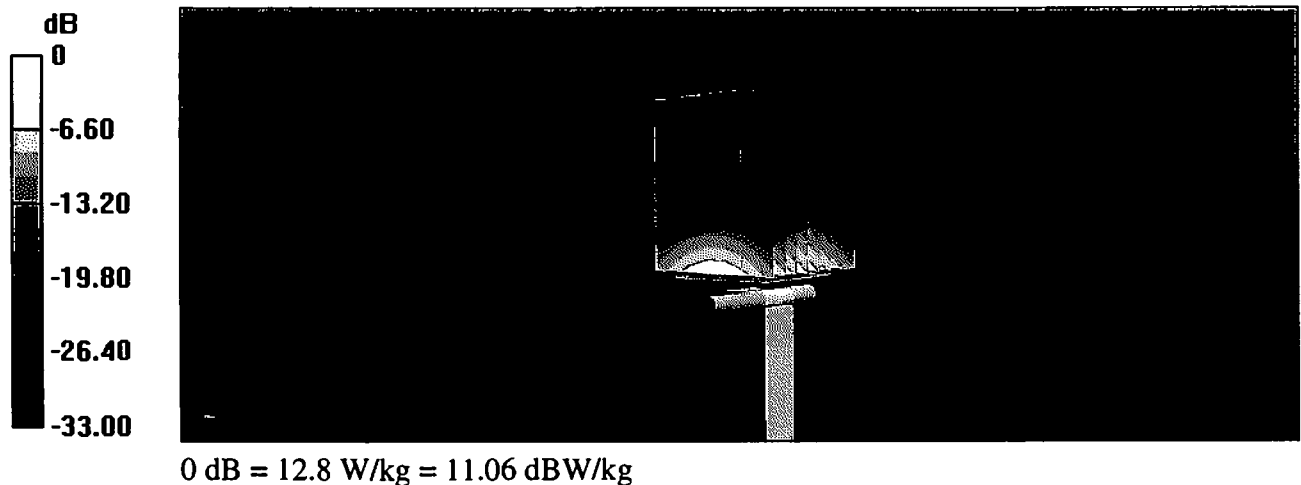

Impedance Measurement Plot for Head TSL

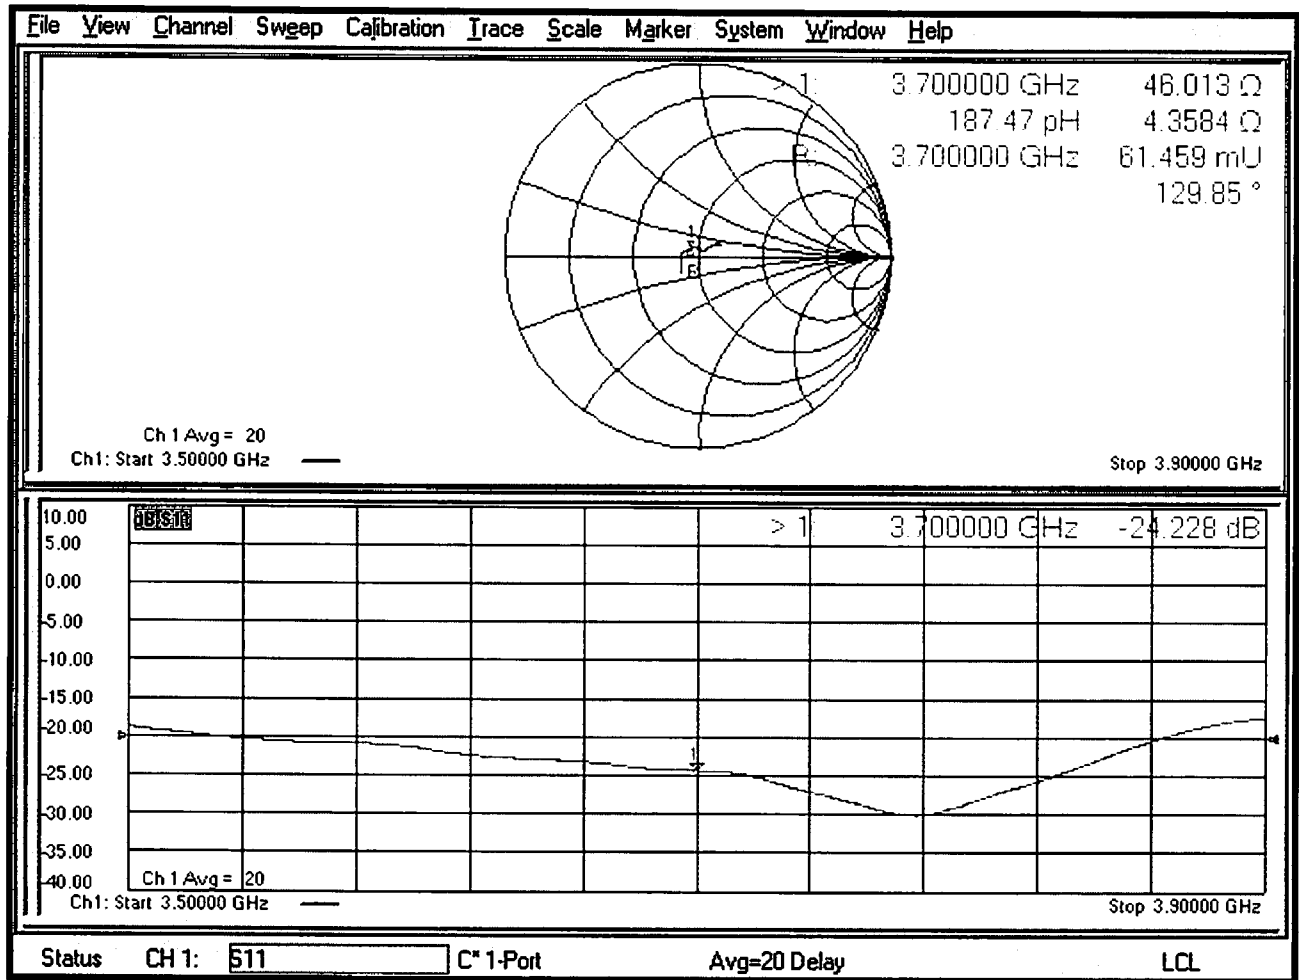

DASY5 Validation Report for Body TSL

Date: 10.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3700 MHz; Type: D3700V2; Serial: D3700V2 - SN:1130

Communication System: UID 0 - CW; Frequency: 3700 MHz

Medium parameters used: $f = 3700$ MHz; $\sigma = 3.49$ S/m; $\epsilon_r = 51.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.31, 7.31, 7.31) @ 3700 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=100 mW, d=10mm, f=3700MHz/Zoom Scan , dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.60 V/m; Power Drift = -0.03 dB



Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 6.25 W/kg; SAR(10 g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8 mm


Ratio of SAR at M2 to SAR at M1 = 75.6%

Maximum value of SAR (measured) = 11.8 W/kg

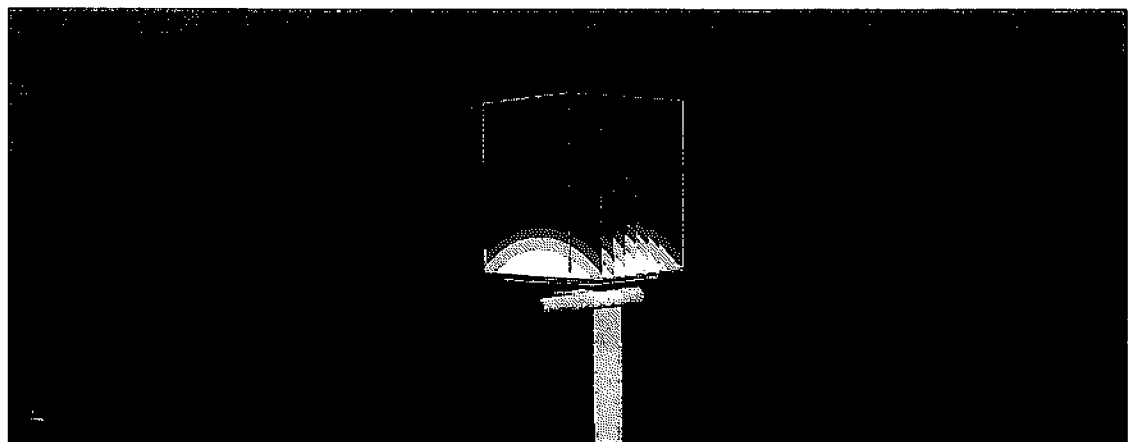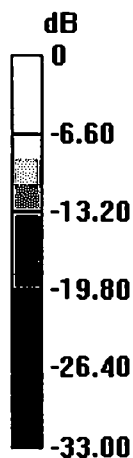

0 dB = 11.8 W/kg = 10.74 dBW/kg

Impedance Measurement Plot for Body TSL

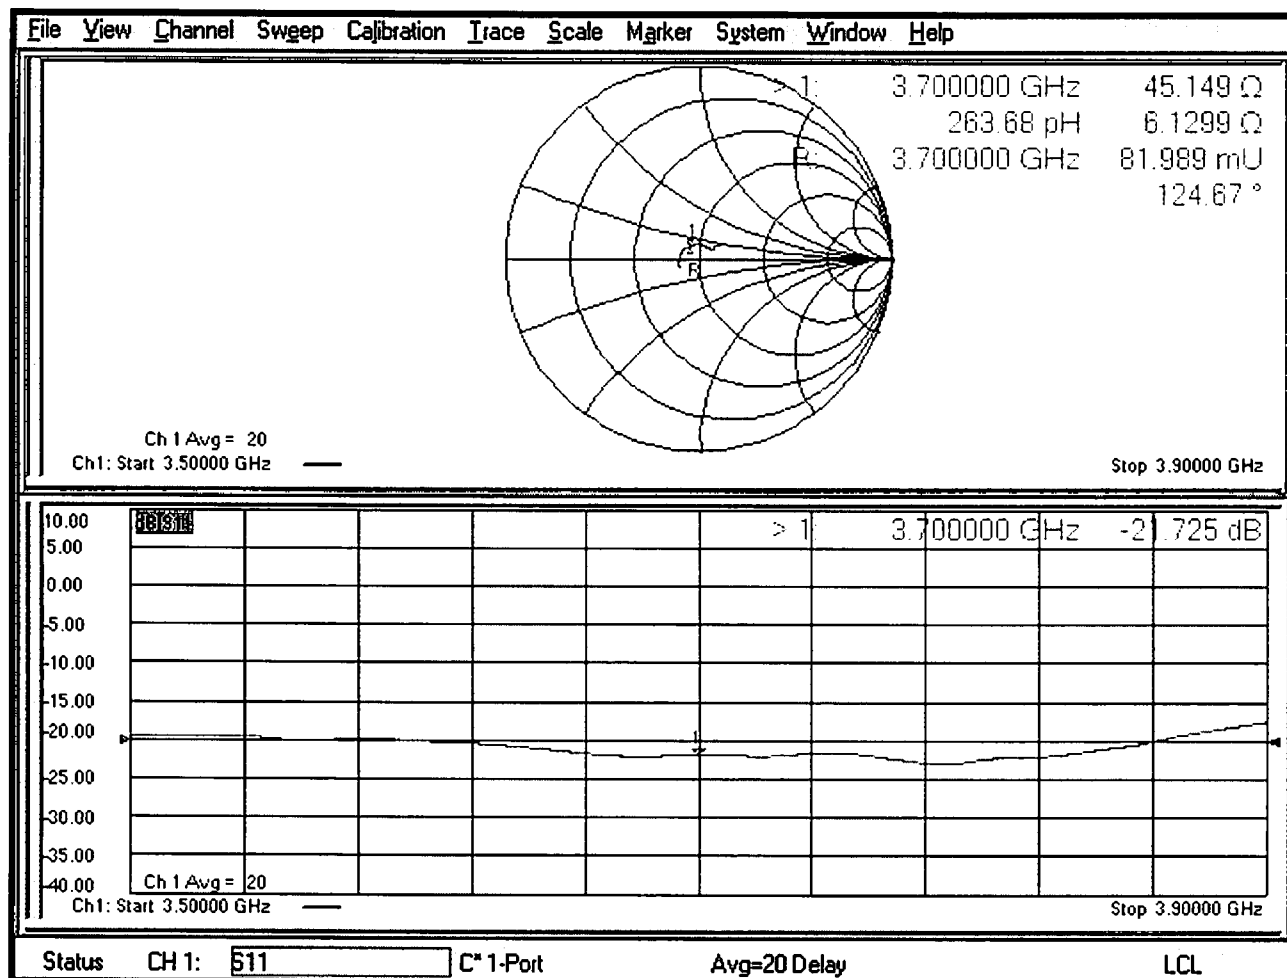

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D3700V2 – SN: 1130
Description: SAR Validation Dipole at 3700 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 11/7/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1130	3700	11/7/2024	10/12/2023	66.6	3.11	-6.83%	24.5	1.16	-5.53%	46.0	47.1	1.1	4.4	5.2	0.8	-24.2	-24.3	-1.60%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

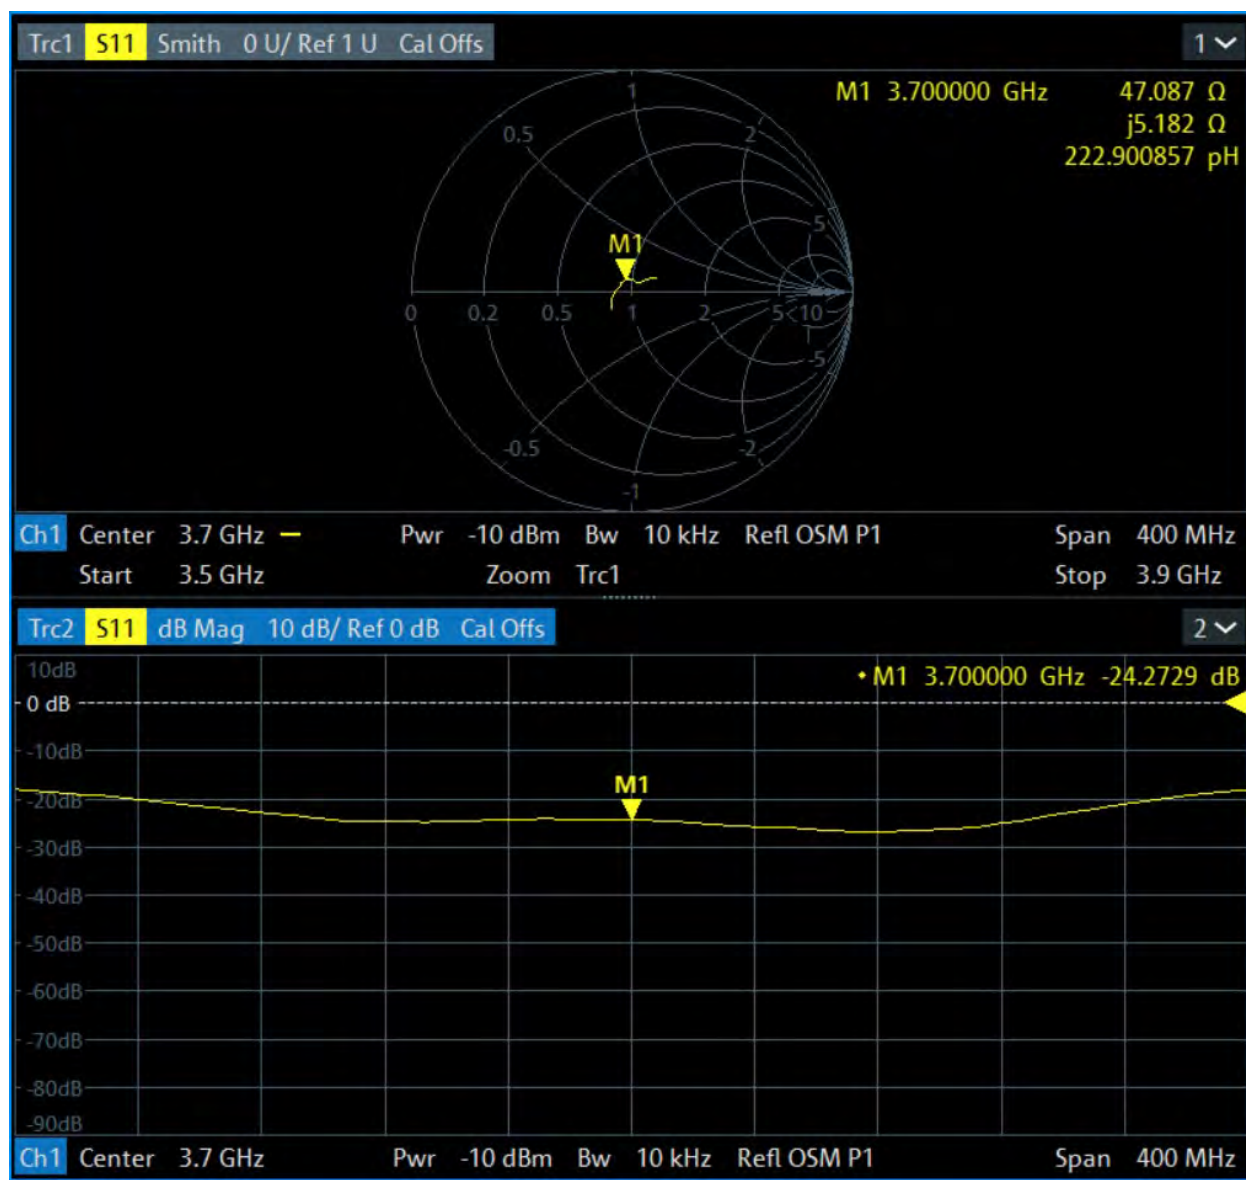

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D3700V2 – SN: 1130
Description: SAR Validation Dipole at 3700 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1844	11/6/2024	11/6/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7853	11/7/2024	11/7/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	

Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:


1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev(%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1130	3700	11/7/2024	10/12/2023	66.6	3.11	-6.83%	24.5	1.16	-5.53%	46.0	46.0	47.1	1.1	4.4	4.4	5.2	0.8	-24.2	-24.2	-24.3	-1.60%	PASS
1130	3700	7/30/2025	10/12/2023	66.6	3.22	-3.53%	24.5	1.20	-2.27%	46.0	47.1	47.0	-0.1	4.4	5.2	4.4	-0.8	-24.2	-24.3	-25.2	-19.19%	PASS



Impedance and Return-Loss Measurement Plot for Head TSL

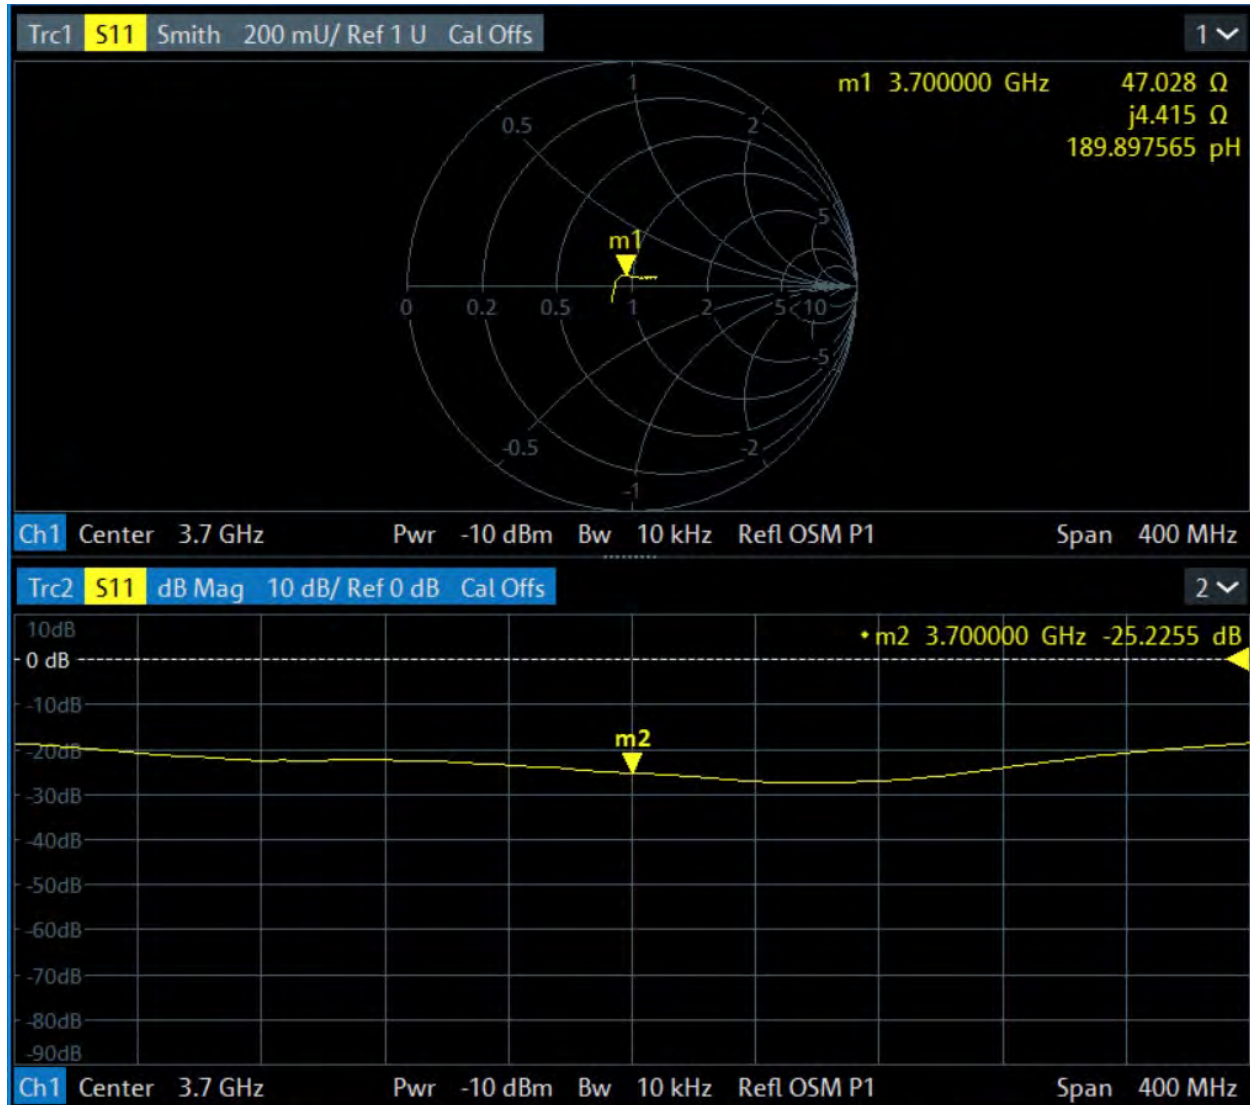



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D3900V2-1101_Oct23**

CALIBRATION CERTIFICATE

Object **D3900V2 - SN:1101**

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

MAB 11/20/23

Calibration date: **October 02, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 3503	07-Mar-23 (No. EX3-3503_Mar23)	Mar-24
DAE4	SN: 601	19-Dec-22 (No. DAE4-601_Dec22)	Dec-23

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by: **Paulo Pina** **Function**
Laboratory Technician

Approved by: **Sven Kühn** **Technical Manager**

Signature

Issued: October 6, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	3900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	37.5	3.32 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	36.7 $\pm$ 6 %	3.28 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.03 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	70.2 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.47 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg $\pm$ 19.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	50.8	3.78 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	51.0 $\pm$ 6 %	3.72 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	6.41 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	64.3 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.22 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.3 W/kg $\pm$ 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.9 Ω - 5.1 j Ω
Return Loss	- 25.8 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.2 Ω - 3.8 j Ω
Return Loss	- 28.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.103 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 02.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3900 MHz; Type: D3900V2; Serial: D3900V2 - SN:1101

Communication System: UID 0 - CW; Frequency: 3900 MHz

Medium parameters used: $f = 3900$ MHz; $\sigma = 3.28$ S/m; $\epsilon_r = 36.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.39, 7.39, 7.39) @ 3900 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100 mW, d=10mm, f=3900MHz/Zoom Scan, dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 70.38 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 19.8 W/kg

SAR(1 g) = 7.03 W/kg; SAR(10 g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8 mm


Ratio of SAR at M2 to SAR at M1 = 74.5%

Maximum value of SAR (measured) = 13.8 W/kg

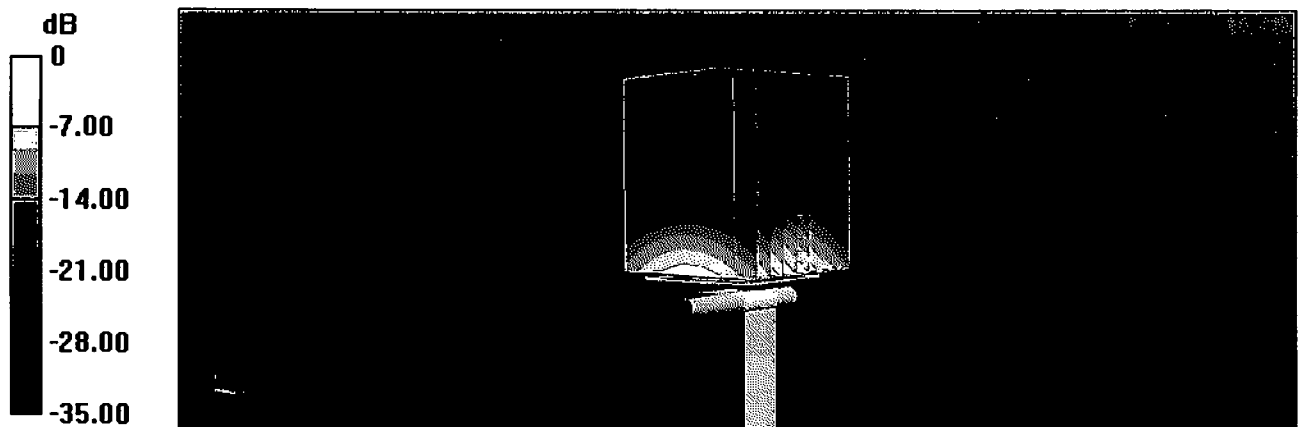

0 dB = 13.8 W/kg = 11.40 dBW/kg

Impedance Measurement Plot for Head TSL

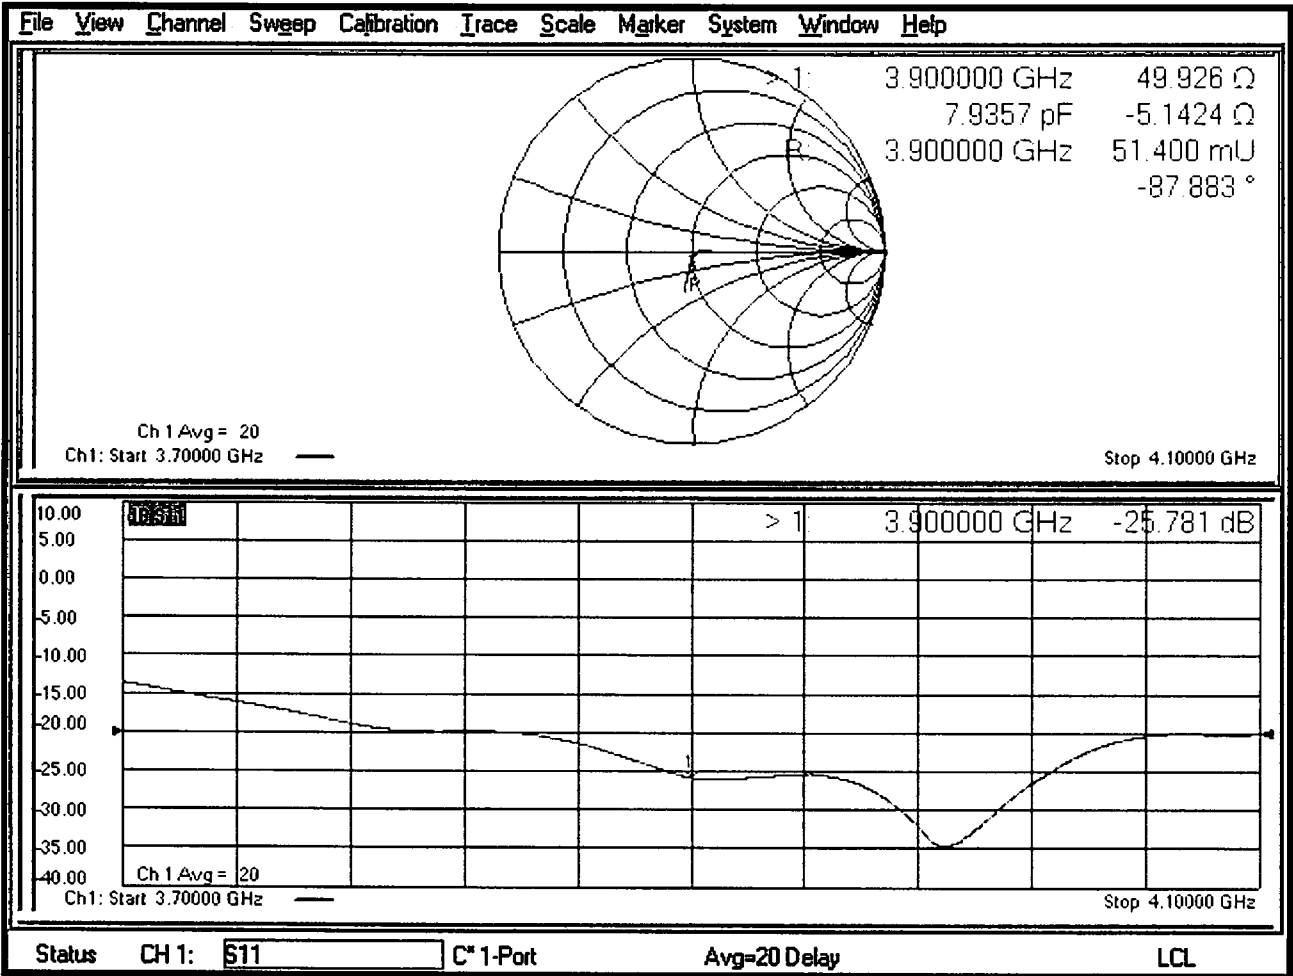

DASY5 Validation Report for Body TSL

Date: 02.10.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3900 MHz; Type: D3900V2; Serial: D3900V2 - SN:1101

Communication System: UID 0 - CW; Frequency: 3900 MHz

Medium parameters used: $f = 3900$ MHz; $\sigma = 3.72$ S/m; $\epsilon_r = 51$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.18, 7.18, 7.18) @ 3900 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=100 mW, d=10mm, f=3900MHz/Zoom Scan , dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.76 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 6.41 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.9 mm


Ratio of SAR at M2 to SAR at M1 = 73.2%

Maximum value of SAR (measured) = 12.4 W/kg

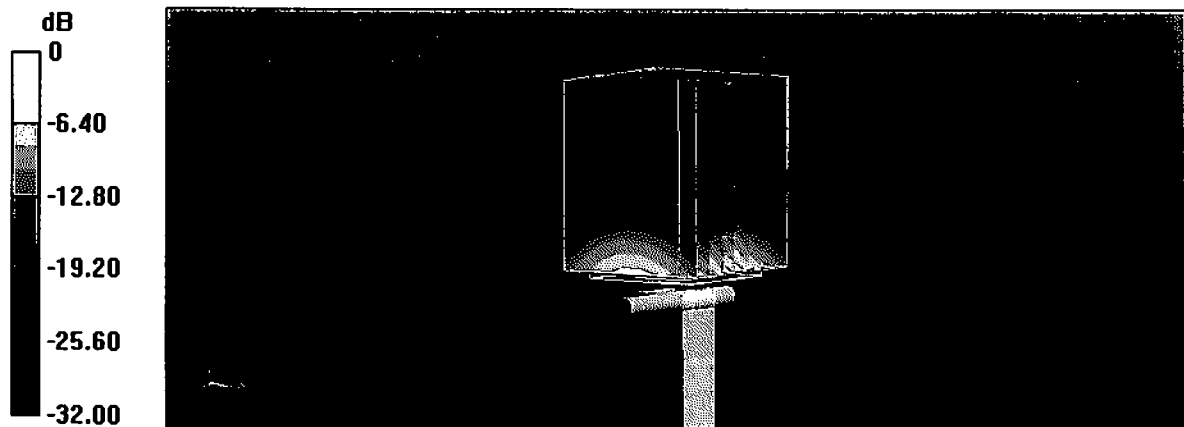

0 dB = 12.4 W/kg = 10.92 dBW/kg

Impedance Measurement Plot for Body TSL

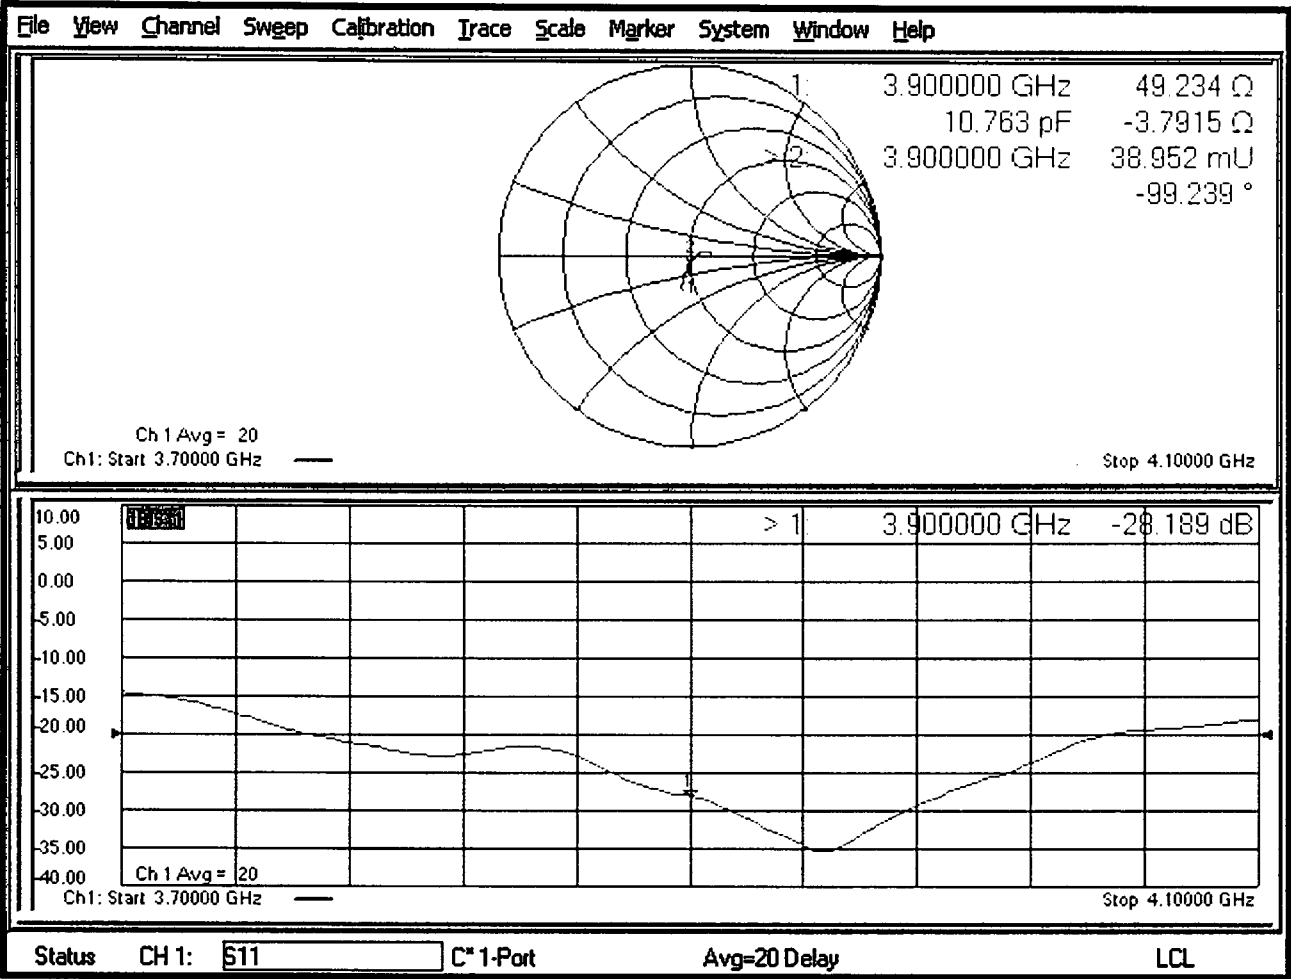



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **RF Safety Lab**
Caronsville, USA

Certificate No. **D3900V2-1101_Jan24**

CALIBRATION CERTIFICATE

Object **D3900V2 - SN-1101**

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **January 09, 2024**

BN ✓
1-17-2024

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 3503	07-Mar-23 (No. EX3-3503_Mar23)	Mar-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

	Name	Function	Signature
Calibrated by:	Paulo Pina	Laboratory Technician	
Approved by:	Sven Kühn	Technical Manager	

Issued: January 11, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	4100 MHz $\pm$ 1 MHz	

Head TSL parameters at 4100 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	37.2	3.53 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.1 $\pm$ 6 %	3.45 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 4100 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	68.4 W/kg $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg $\pm$ 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 4100 MHz

Impedance, transformed to feed point	$59.4 \Omega + 0.7 j\Omega$
Return Loss	- 21.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.103 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 09.01.2024

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3900 MHz; Type: D3900V2; Serial: D3900V2 - SN:1101

Communication System: UID 0 - CW; Frequency: 4100 MHz

Medium parameters used: $f = 4100$ MHz; $\sigma = 3.45$ S/m; $\epsilon_r = 38.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(7.26, 7.26, 7.26) @ 4100 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100 mW, d=10mm, f=4100MHz/Zoom Scan, dist=1.4mm (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.85 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 19.0 W/kg

SAR(1 g) = 6.79 W/kg; SAR(10 g) = 2.36 W/kg

Smallest distance from peaks to all points 3 dB below = 8 mm


Ratio of SAR at M2 to SAR at M1 = 74.2%

Maximum value of SAR (measured) = 13.3 W/kg

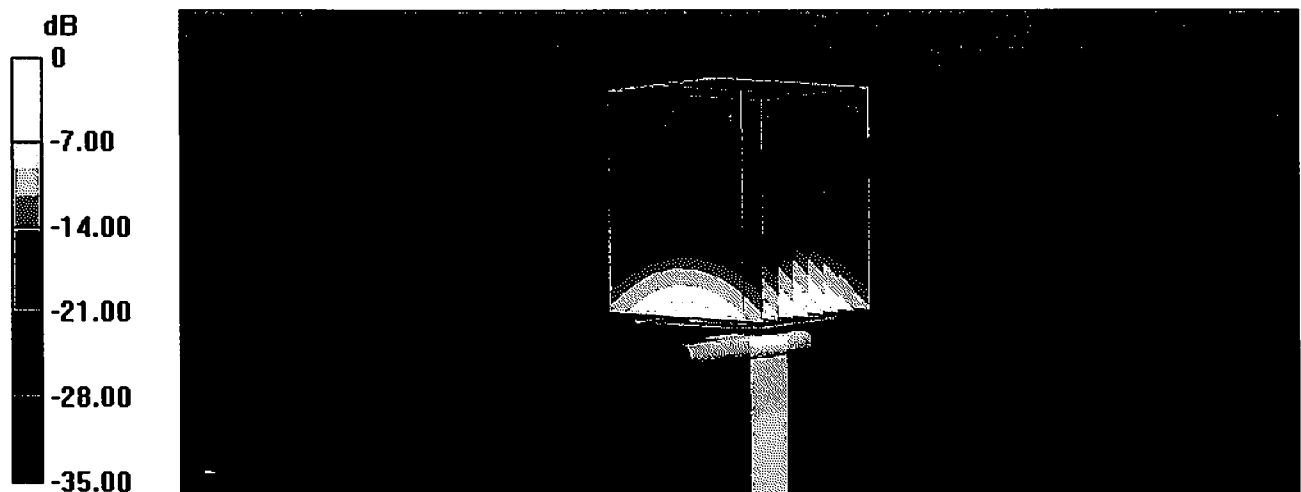

0 dB = 13.3 W/kg = 11.23 dBW/kg

Impedance Measurement Plot for Head TSL

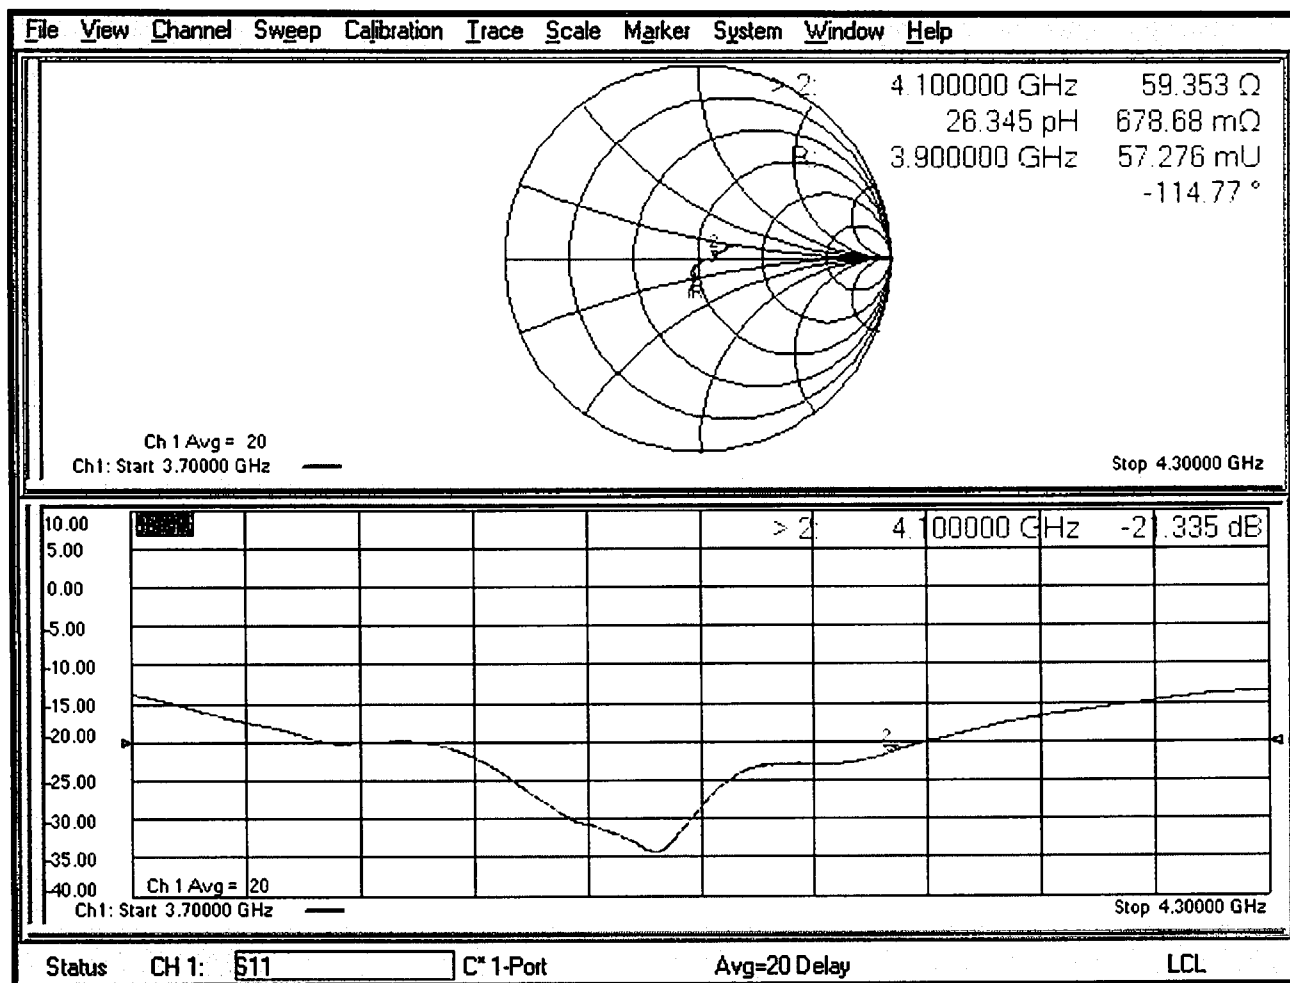

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object D3900V2 – SN: 1101
Description SAR Validation Dipole at 3900 MHz and 4100 MHz
Procedure (s) Procedure for SAR Verification Source Calibration Extension
In-house Check Date 11/8/2024

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Mini-Circuits	BW-N20W20+	20dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	NF-SF50+	RF Adapter N Male to SMA Female (DC - 18 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	8/14/2024	8/14/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	3/15/2024	3/15/2025	
SPEAG	Powersource1	Signal Generator	4341	1/5/2024	1/5/2025	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	


Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:


1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Deviation (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Deviation (%)	Cert Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Deviation (%)	PASS/FAIL
1101	3900	11/8/2024	10/2/2023	70.2	3.35	-4.78%	24.6	1.18	-4.29%	49.9	47.9	-2.0	-5.1	-4.0	1.1	-25.8	-26.7	-18.34%	PASS
1101	4100	11/8/2024	1/9/2024	68.4	3.28	-4.32%	23.7	1.15	-3.18%	59.4	59.7	0.3	0.7	-0.5	-1.2	-21.3	-21.1	5.93%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

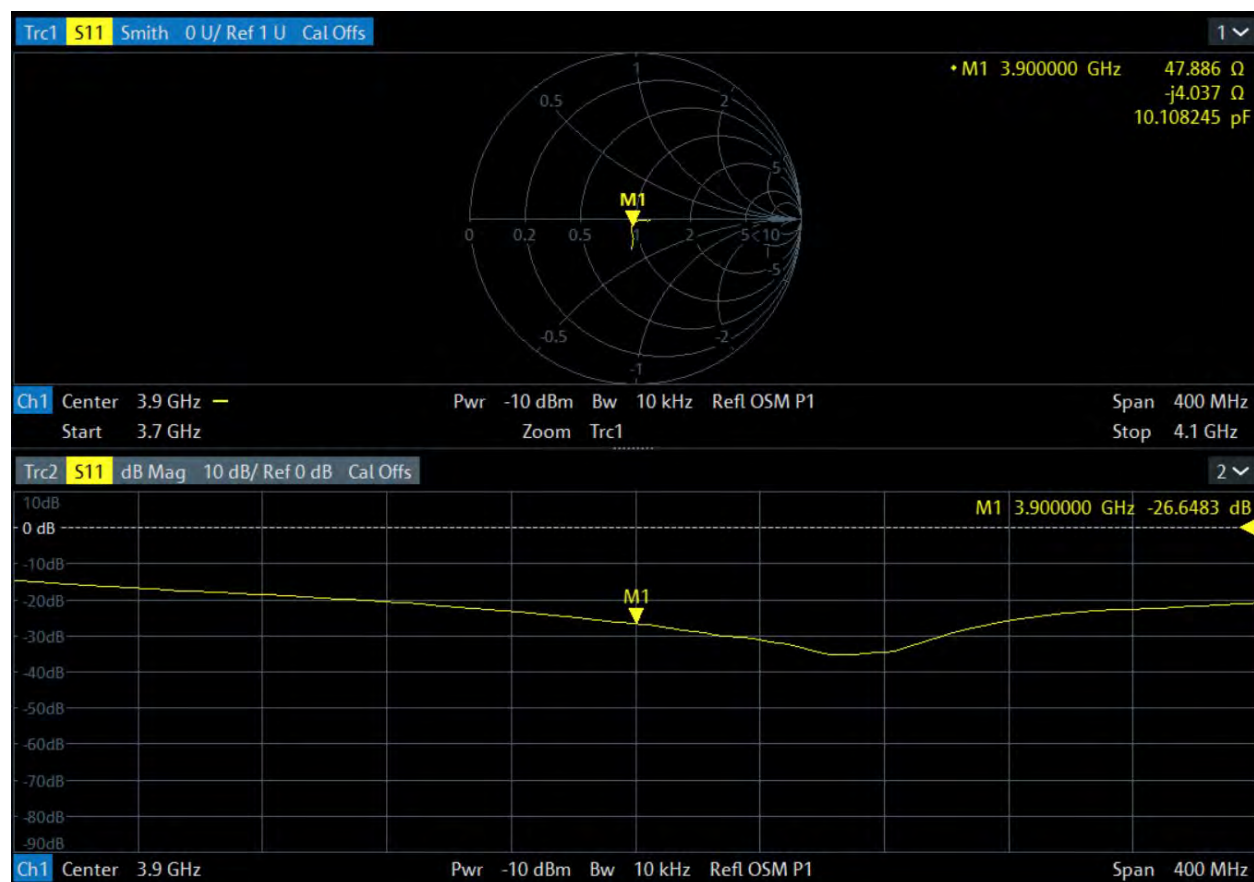

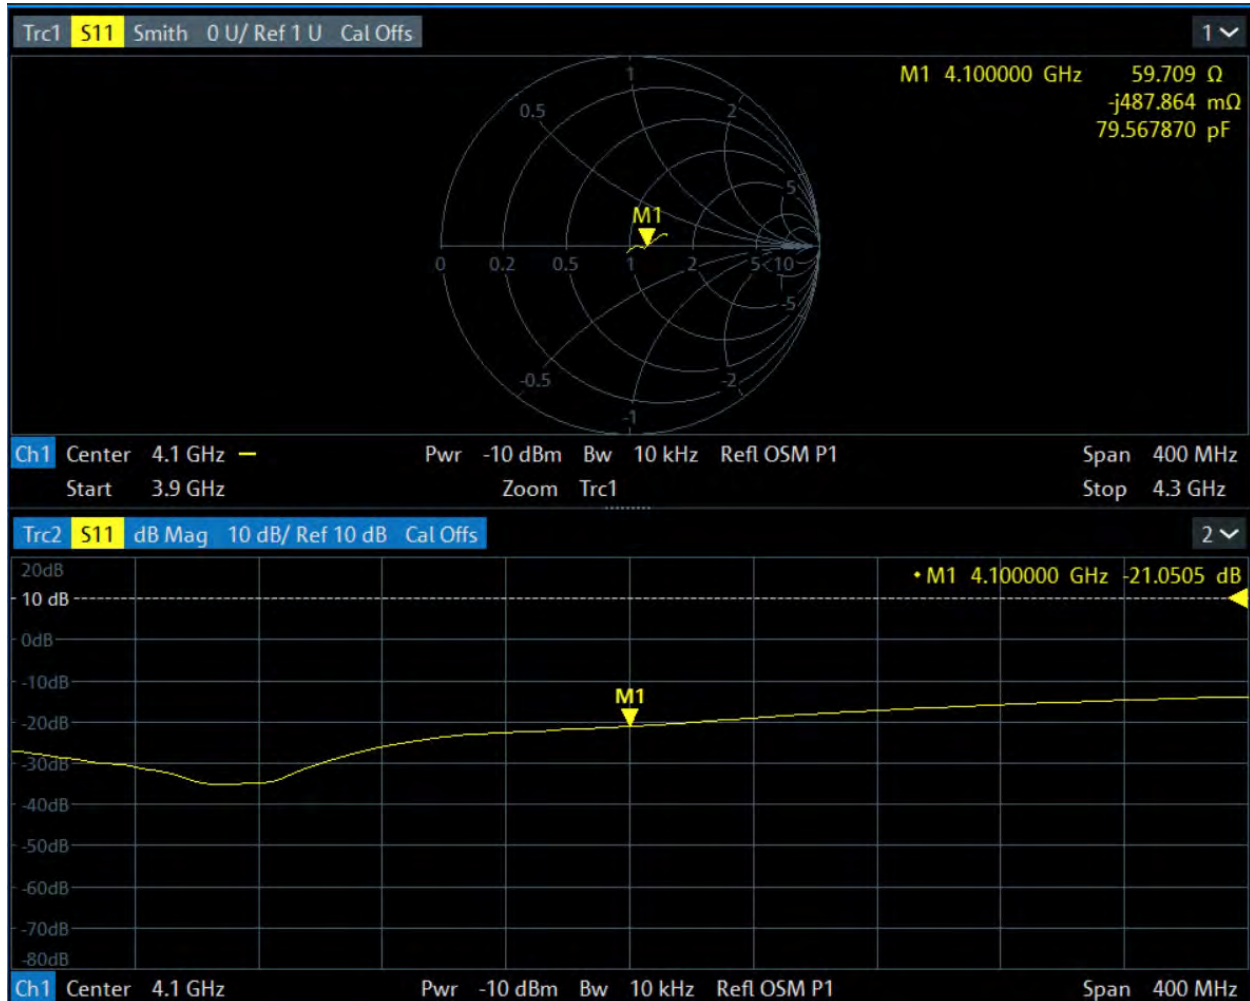

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D3900V2 – SN: 1101
Description: SAR Validation Dipole at 3900 MHz and 4100 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF Test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1844	11/6/2024	11/6/2025	
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/24	9/4/25	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7853	11/7/2024	11/7/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/24	9/12/25	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	



Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL
1101	3900	11/8/2024	10/2/2023	70.2	3.35	-4.78%	24.6	1.18	-4.29%	49.9	49.9	47.9	-2.0	-5.1	-5.1	-4.0	1.1	-25.8	-25.8	-26.7	-18.34%	PASS
1101	4100	11/8/2024	1/9/2024	68.4	3.28	-4.32%	23.7	1.15	-3.18%	59.4	59.4	59.7	0.3	0.7	0.7	-0.5	-1.2	-21.3	-21.3	-21.1	5.93%	PASS
1101	3900	7/30/2025	10/2/2023	70.2	3.32	-5.64%	24.6	1.17	-5.10%	49.9	47.9	48.5	0.6	-5.1	-4.0	-4.4	-0.4	-25.8	-26.7	-26.5	3.75%	PASS
1101	4100	7/30/2025	1/9/2024	68.4	3.29	-4.03%	23.7	1.16	-2.34%	59.4	59.7	59.8	0.1	0.7	-0.5	-0.4	0.1	-21.3	-21.1	-21.0	2.68%	PASS

Impedance and Return-Loss Measurement Plot for Head TSL

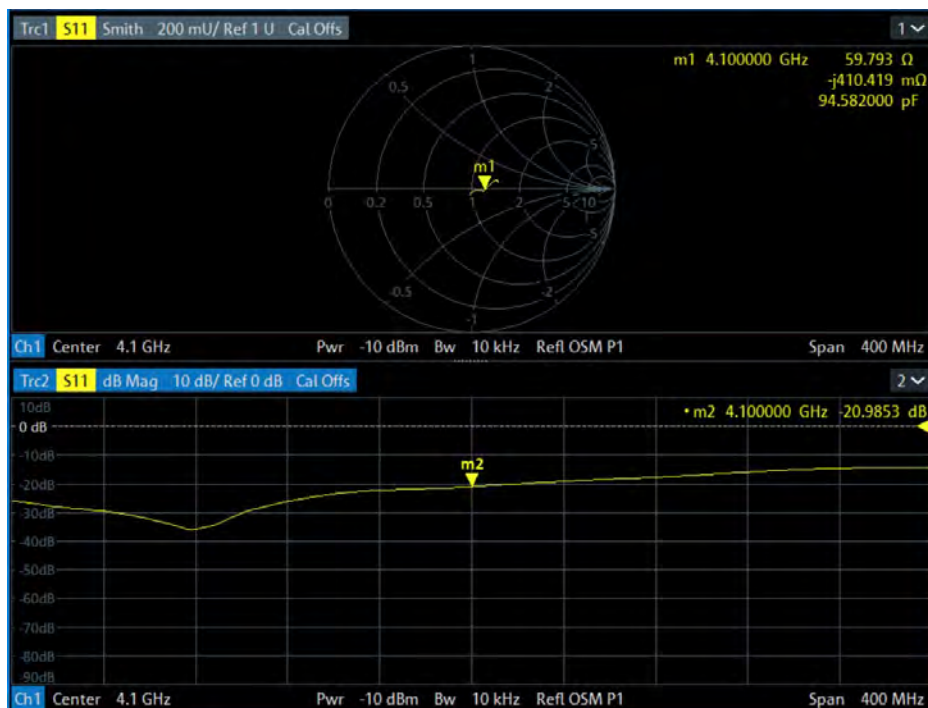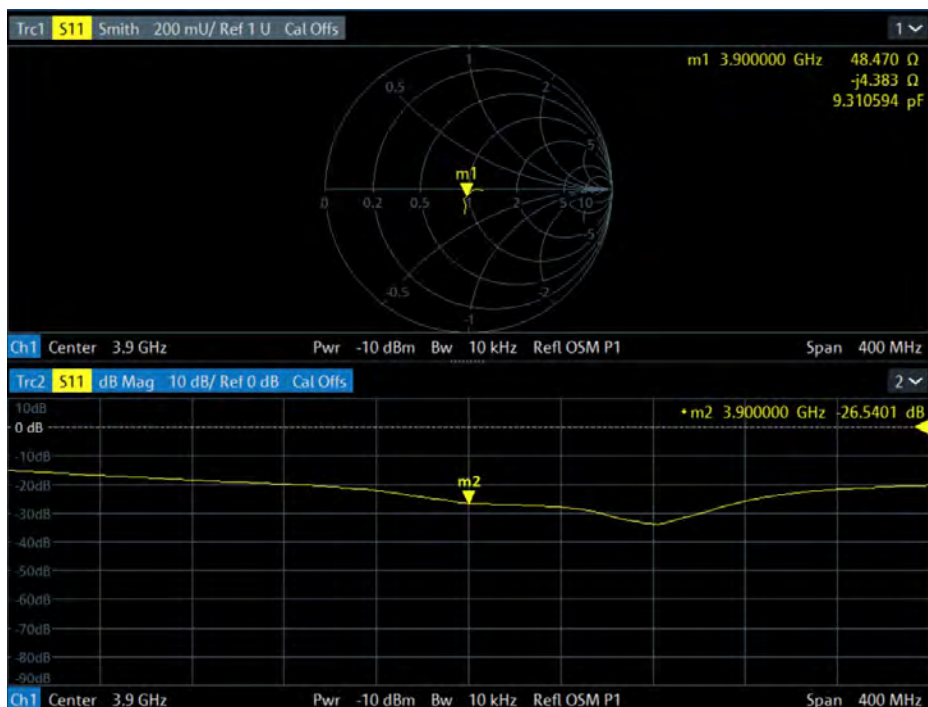



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client

RF Safety Lab
Catonsville, USA

Certificate No.

D5GHzV2-1396_Nov24

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1396**

WAB 11/21/24

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3 - 10 GHz

Calibration date **November 15, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Cal
Power Sensor R&S NRP-33T	SN: 100967	28-Mar-24 (No. 217-04038)	Mar-25
Power Sensor R&S NRP18A	SN: 101859	22-Jul-24 (No. 4030A315008547)	Jul-25
Spectrum Analyzer R&S FSV40	SN: 101832	25-Jan-24 (No. 4030-315007551)	Jan-25
Mismatch; Short [S4188] Attenuator [S4423]	SN: 1152	28-Mar-24 (No. 217-04050)	Mar-25
OCP DAK-12	SN: 1016	24-Sep-24 (No. OCP-DAK12-1016_Sep24)	Sep-25
OCP DAK-3.5	SN: 1249	23-Sep-24 (No. OCP-DAK3.5-1249_Sep24)	Sep-25
Reference Probe EX3DV4	SN: 7349	03-Jun-24 (No. EX3-7349_Jun24)	Jun-25
DAE4ip	SN: 1836	28-Oct-24 (No. DAE4ip-1836_Oct24)	Oct-25

Secondary Standards	ID	Check Date (in house)	Scheduled Check
ACAD Source Box	SN: 1000	28-May-24 (No. 675-ACAD_Source_Box-240528)	May-25
Signal Generator R&S SMB100A	SN: 182081	28-May-24 (No. 675-CAL16-S4588-240528)	May-25
Mismatch; SMA	SN: 1102	22-May-24 (No. 675-Mismatch_SMA-240522)	May-25

	Name	Function	Signature
Calibrated by	Paulo Pina	Laboratory Technician	<i>[Signature]</i>
Approved by	Sven Kühn	Technical Manager	<i>[Signature]</i>

Issued: November 15, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation

- DASY System Handbook

Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY8 Module SAR	16.4.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with spacer
Zoom Scan Resolution	dx, dy = 4mm, dz = 1.4mm	Graded Ratio = 1.4 mm (Z direction)
Frequency	5250MHz $\pm$ 1MHz 5600MHz $\pm$ 1MHz 5750MHz $\pm$ 1MHz 5850MHz $\pm$ 1MHz	

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2)°C	36.1 $\pm$ 6%	4.55 mho/m $\pm$ 6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.9 W/kg $\pm$ 19.9% (k = 2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	2.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.4 W/kg $\pm$ 19.5% (k = 2)

Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ±0.2)°C	35.5 ±6%	4.91 mho/m ±6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	8.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.1 W/kg ±19.9% (k = 2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	2.33 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ±19.5% (k = 2)

Head TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ±0.2)°C	35.3 ±6%	5.08 mho/m ±6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5750 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	8.01 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.1 W/kg ±19.9% (k = 2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	2.28 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.8 W/kg ±19.5% (k = 2)

Head TSL parameters at 5850 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.2	5.32 mho/m
Measured Head TSL parameters	(22.0 ±0.2)°C	35.2 ±6%	5.18 mho/m ±6%
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5850 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	7.69 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.9 W/kg ±19.9% (k = 2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR for nominal Head TSL parameters	20 dBm input power	2.20 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.0 W/kg ±19.5% (k = 2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance	46.9 Ω – 1.3 j Ω
Return Loss	-29.1 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance	53.9 Ω + 3.2 j Ω
Return Loss	-26.2 dB

Antenna Parameters with Head TSL at 5750 MHz

Impedance	51.8 Ω + 2.6 j Ω
Return Loss	-30.1 dB

Antenna Parameters with Head TSL at 5850 MHz

Impedance	54.7 Ω – 1.0 j Ω
Return Loss	-26.8 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.189 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN1396	5250	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0---		5250, 0	5.39	4.55	36.1

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 – SN7349, 2024-06-03	DAE4ip Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	7.79
psSAR10g [W/Kg]	2.24
Power Drift [dB]	0.03
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

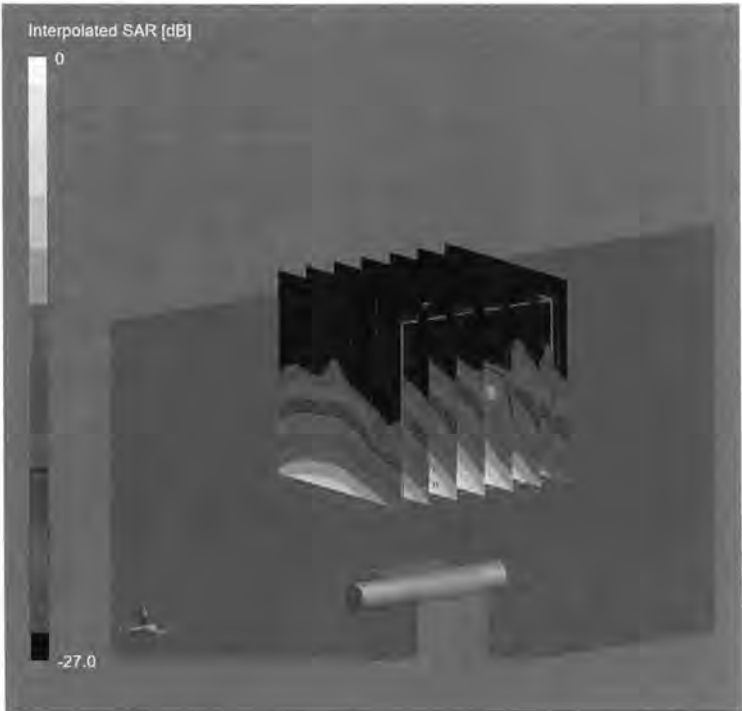

0 dB = 31.1 W/Kg

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN1396	5600	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		5600, 0	4.93	4.91	35.5

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 – SN7349, 2024-06-03	DAE4ip Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	8.11
psSAR10g [W/Kg]	2.33
Power Drift [dB]	0.00
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

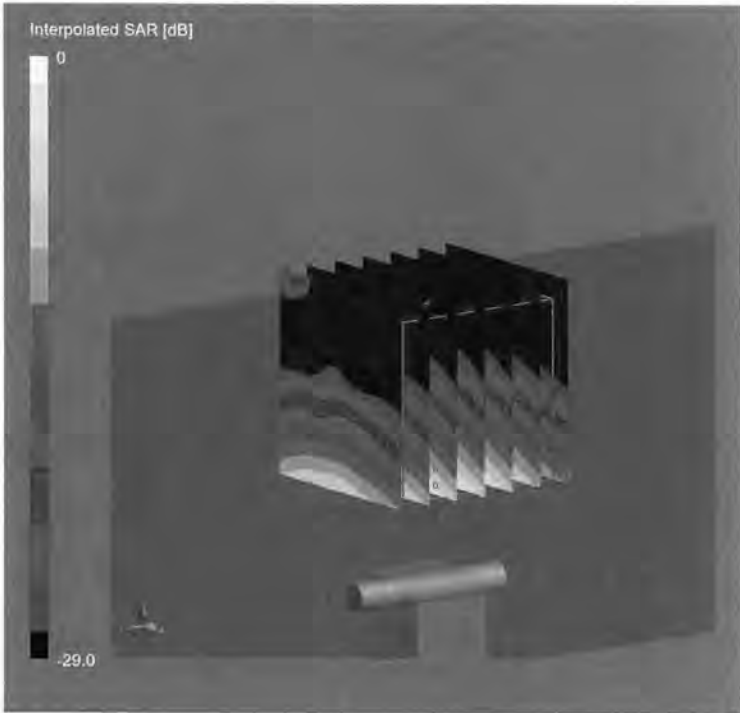

0 dB = 35.0 W/Kg

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN1396	5750	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10		CW, 0--	5750, 0	4.93	5.08	35.3

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 – SN7349, 2024-06-03	DAE4lp Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	8.01
psSAR10g [W/Kg]	2.28
Power Drift [dB]	0.00
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

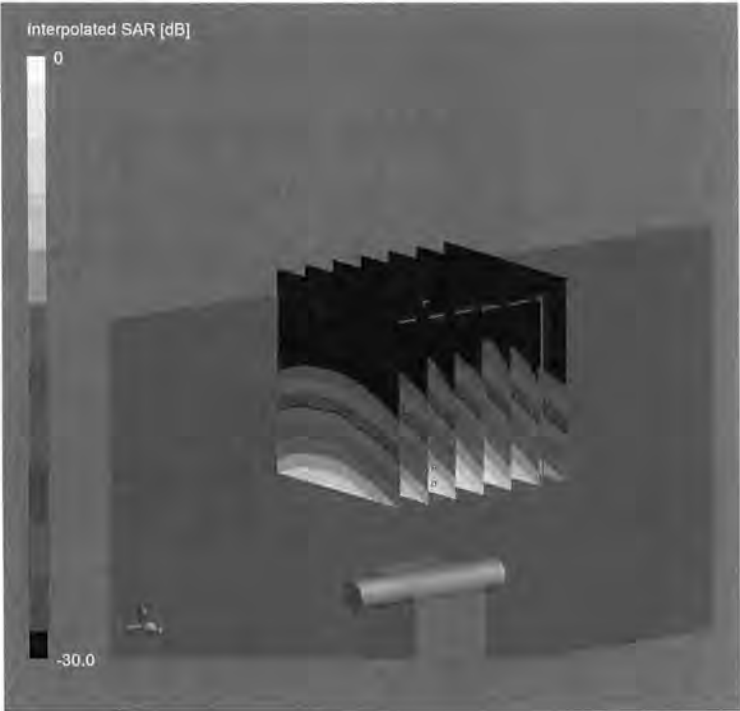

0 dB = 35.6 W/Kg

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 - SN1396	5850	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		5850, 0	4.96	5.18	35.2

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2024-11-15	EX3DV4 - SN7349, 2024-06-03	DAE4lp Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured


Measurement Results

	Zoom Scan
Date	2024-11-15
psSAR1g [W/Kg]	7.69
psSAR10g [W/Kg]	2.20
Power Drift [dB]	0.00
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative



0 dB = 34.8 W/Kg

Impedance Measurement Plot for Head TSL

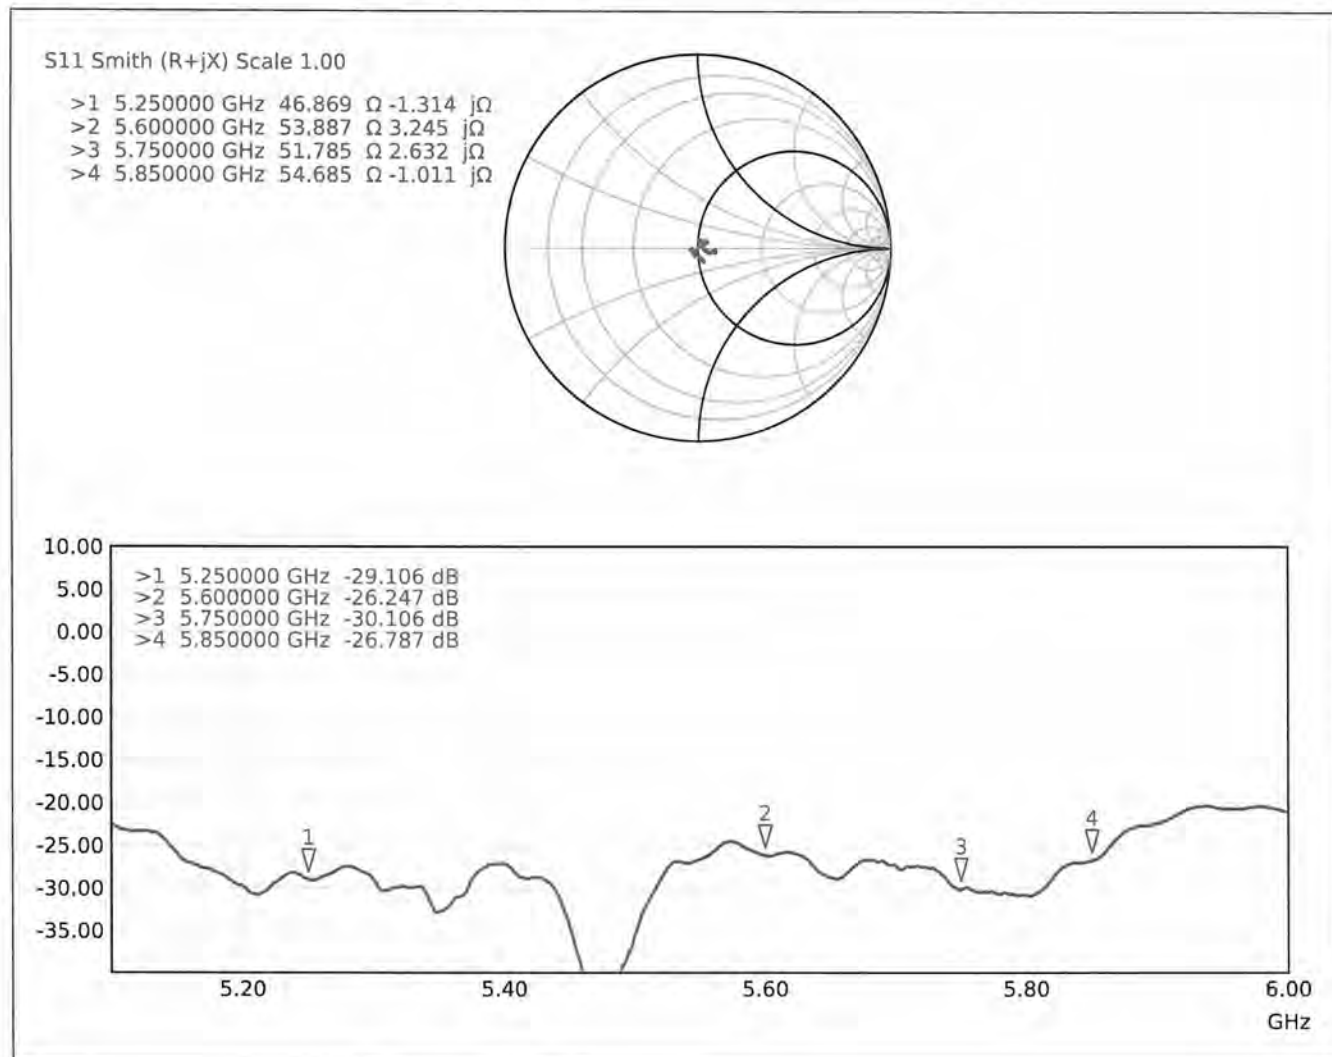

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION

Object: D5GHzV2 – SN: 1396
Description: SAR Validation Dipole at 5250, 5600, 5750, and 5850 MHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/2024	9/12/2025	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/2023	8/28/2025	
Control Company	4040	Ambient Thermometer	230581662	8/28/2023	8/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/2023	9/28/2025	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/2023	9/28/2025	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/2024	12/28/2025	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/2024	9/4/2025	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/2024	9/2/2025	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/2024	9/12/2025	
SPEAG	Powersource1	Signal Generator	4341	1/9/2025	1/9/2026	

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ (k=2)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	



Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:



1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
1396	5250	11/21/2024	11/15/2024							46.9	46.9	46.8	-0.1	-1.3	-1.3	-0.2	1.1	-29.1	-29.1	-29.5	-8.91%	PASS	In-house check after Calibration
1396	5600	11/21/2024	11/15/2024							53.9	53.9	53.3	-0.6	3.2	3.2	4.1	0.9	-26.2	-26.2	-25.9	7.60%	PASS	In-house check after Calibration
1396	5750	11/21/2024	11/15/2024							51.8	51.8	51.9	0.1	2.6	2.6	2.5	-0.1	-30.1	-30.1	-30.2	-2.27%	PASS	In-house check after Calibration
1396	5850	11/21/2024	11/15/2024							54.7	54.7	54.2	-0.5	-1.0	-1.0	-2.1	-1.1	-26.8	-26.8	-26.9	-1.76%	PASS	In-house check after Calibration
1396	5250	7/30/2025	11/15/2024	77.9	3.77	-3.44%	22.4	1.07	-4.69%	46.9	46.8	47.7	0.9	-1.3	-0.2	-2.5	-2.3	-29.1	-29.5	-29.1	10.90%	PASS	-
1396	5600	7/30/2025	11/15/2024	81.1	4.07	0.13%	23.3	1.15	-1.52%	53.9	53.3	52.8	-0.5	3.2	4.1	4.4	0.3	-26.2	-25.9	-25.9	-0.97%	PASS	-
1396	5750	7/30/2025	11/15/2024	80.1	3.79	-5.59%	22.8	1.08	-5.49%	51.8	51.9	52.7	0.8	2.6	2.5	1.9	-0.6	-30.1	-30.2	-29.9	7.42%	PASS	-
1396	5850	7/30/2025	11/15/2024	76.9	3.96	2.75%	22	1.12	1.58%	54.7	54.2	54.2	0.0	-1.0	-2.1	-3.8	0.3	-26.8	-26.9	-27.1	-4.66%	PASS	-

Impedance and Return-Loss Measurement Plot for Head TSL

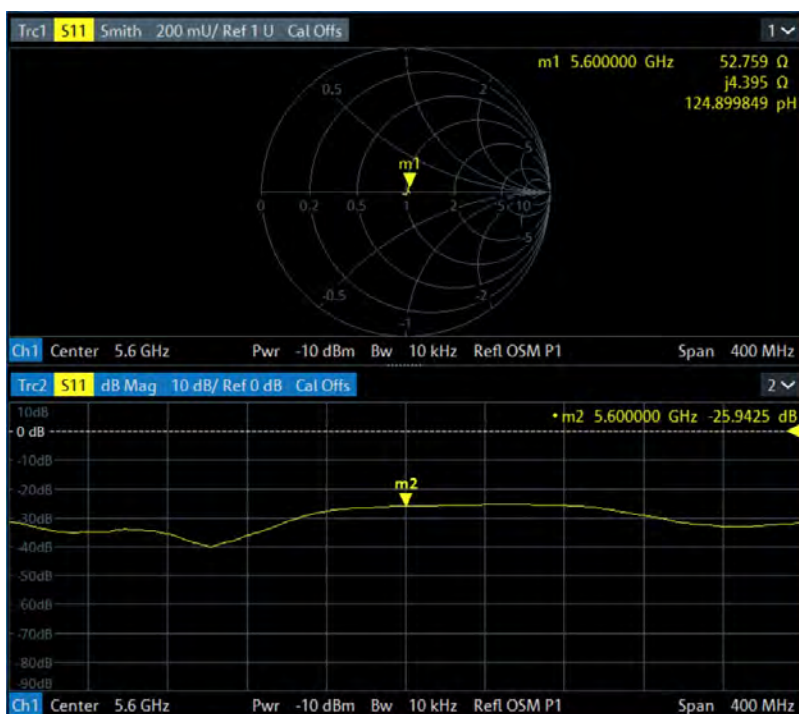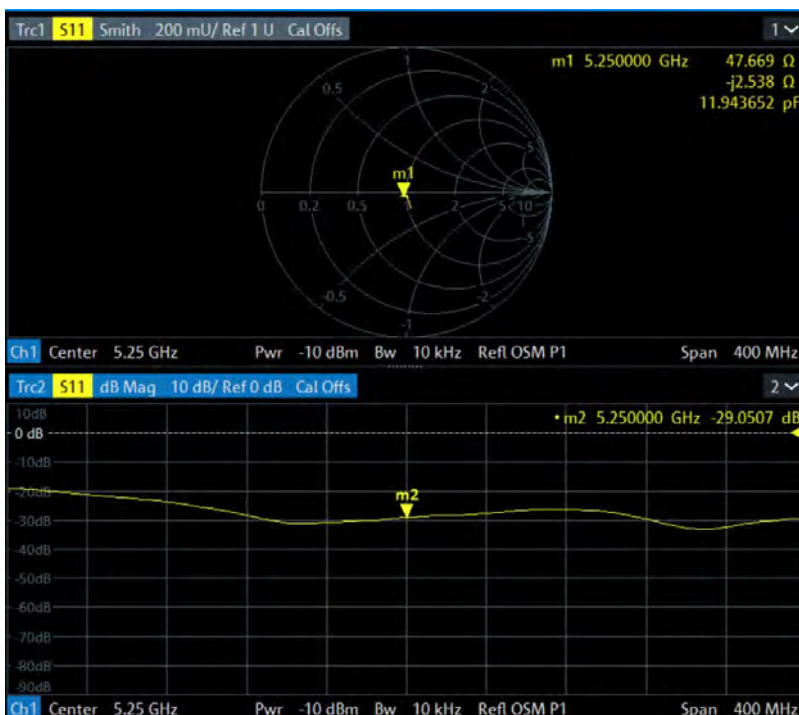

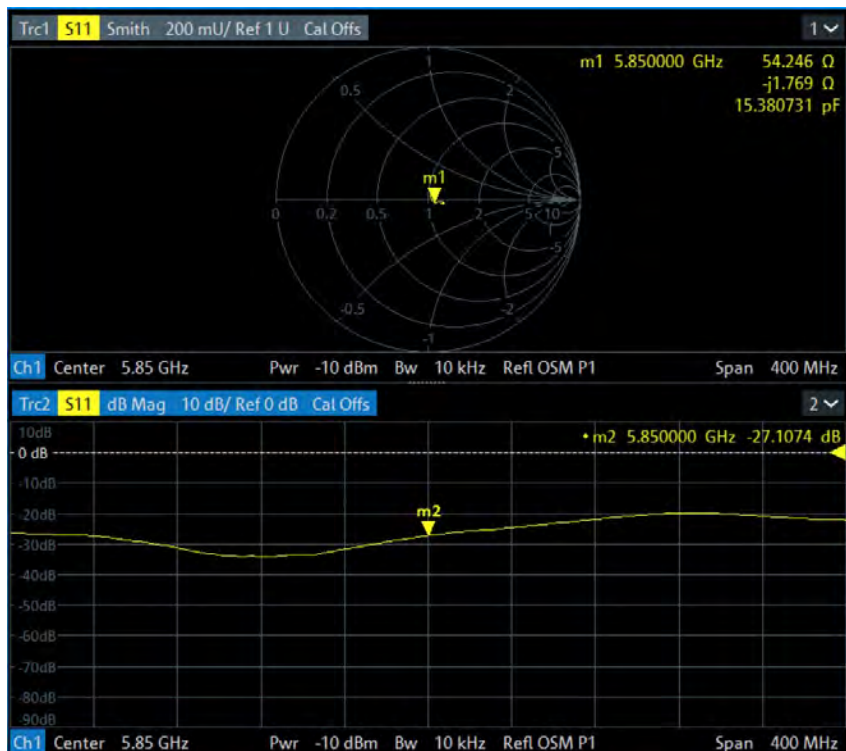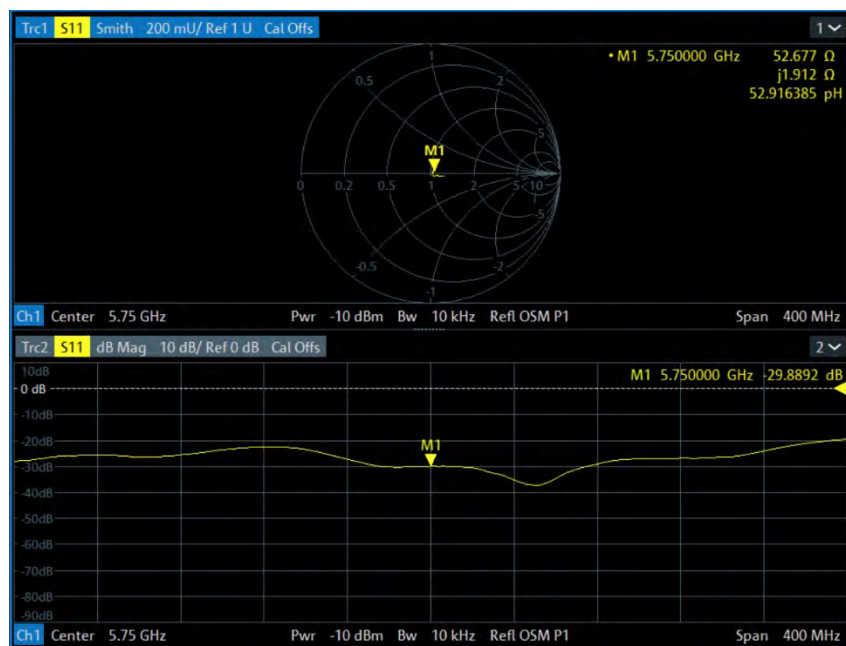



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **RF Safety Lab**
Catonsville, USA

Certificate No. **D6.5GHzV2-1104_Nov24**

CALIBRATION CERTIFICATE

Object **D6.5GHzV2 - SN:1104**

MAG 11/21/24

Calibration procedure(s) **QA CAL-22.v7**
Calibration Procedure for SAR Validation Sources between 3-10 GHz

Calibration date: **November 14, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power sensor R&S NRP33T	SN: 100967	28-Mar-24 (No. 217-04038)	Mar-25
Reference 20 dB Attenuator	SN: BH9394 (20k)	26-Mar-24 (No. 217-04046)	Mar-25
Mismatch combination	SN: 84224 / 360D	28-Mar-24 (No. 217-04050)	Mar-25
Reference Probe EX3DV4	SN: 7405	01-Jul-24 (No. EX3-7405_Jul24)	Jul-25
DAE4	SN: 908	27-Mar-24 (No. DAE4-908_Mar24)	Mar-25

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator Anapico APSIN20G	SN: 827	18-Dec-18 (in house check Jan-24)	In house check: Jan-25
Power sensor NRP-Z23	SN: 100169	10-Jan-19 (in house check Jan-24)	In house check: Jan-25
Power sensor NRP-18T	SN: 100950	28-Sep-22 (in house check Jan-24)	In house check: Jan-25
Network Analyzer Keysight E5063A	SN:MY54504221	31-Oct-19 (in house check Sep-24)	In house check: Sep-26

Calibrated by:	Name Aidonia Georgiadou	Function Laboratory Technician	Signature
Approved by:	Sven Kühn	Technical Manager	

Issued: November 14, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range Of 4 MHz To 10 GHz)", October 2020.

Additional Documentation:

- b) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.
- *The absorbed power density (APD):* The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	5 mm	with Spacer
Zoom Scan Resolution	dx, dy = 3.4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	6500 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.6 $\pm$ 6 %	6.21 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	29.8 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	298 W/kg $\pm$ 24.7 % (k=2)

SAR averaged over 8 cm ³ (8 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	67.2 W/kg $\pm$ 24.4 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.50 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	55.0 W/kg $\pm$ 24.4 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.1 Ω + 1.1 j Ω
Return Loss	- 33.1 dB

APD (Absorbed Power Density)

APD averaged over 1 cm ²	Condition	
APD measured	100 mW input power	297 W/m ²
APD measured	normalized to 1W	2970 W/m ² $\pm$ 29.2 % (k=2)

APD averaged over 4 cm ²	condition	
APD measured	100 mW input power	134 W/m ²
APD measured	normalized to 1W	1340 W/m ² $\pm$ 28.9 % (k=2)

*The reported APD values have been derived using the psSAR1g and psSAR8g.

General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY6 Validation Report for Head TSL

Measurement Report for D6.5GHz-1104, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties

Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
D6.5GHz	16.0 x 6.0 x 300.0	SN: 1104	-

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat, HSL	5.00	Band	CW,	6500	5.14	6.21	34.6

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center - 1182	HBBL600-10000V6	EX3DV4 - SN7405, 2024-07-01	DAE4 Sn908, 2024-03-27

Scan Setup


	Zoom Scan
Grid Extents [mm]	22.0 x 22.0 x 22.0
Grid Steps [mm]	3.4 x 3.4 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2024-11-14, 11:13
psSAR1g [W/Kg]	29.8
psSAR8g [W/Kg]	6.71
psSAR10g [W/Kg]	5.50
Power Drift [dB]	-0.01
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	No correction
M2/M1 [%]	49.9
Dist 3dB Peak [mm]	4.6

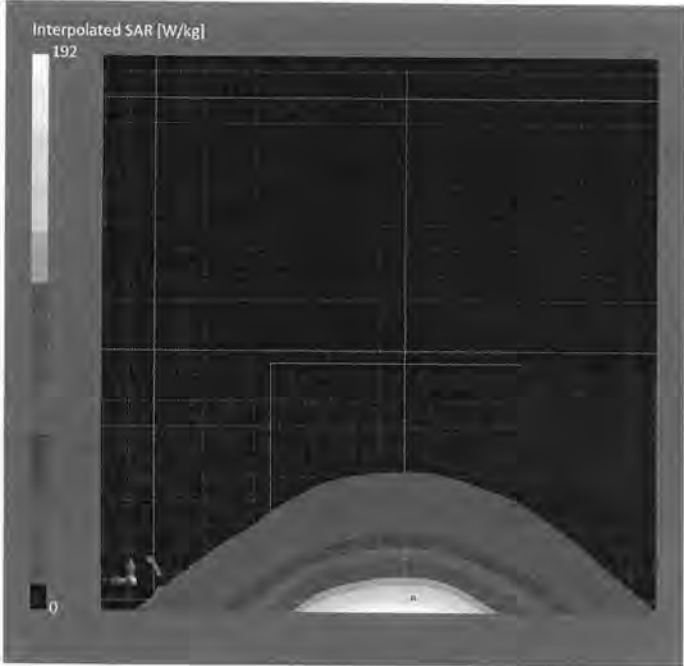

Impedance Measurement Plot for Head TSL

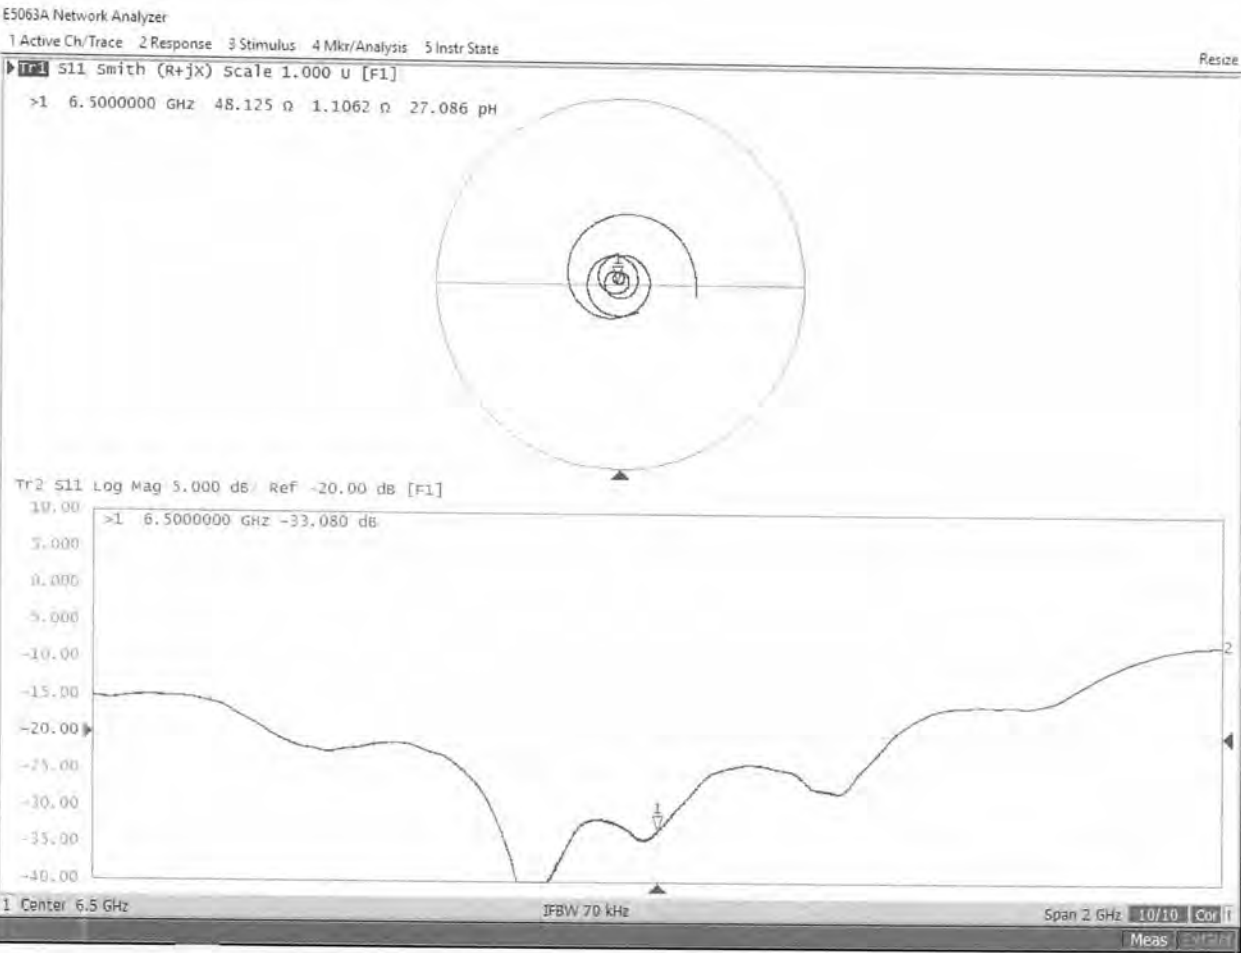

IN-HOUSE SAR VERIFICATION SOURCE CALIBRATION EXTENSION


Object: D6.5GHzV2 – SN: 1104
Description: SAR Validation Dipole at 6.5 GHz
Procedure (s): Procedure for SAR Verification Source Calibration Extension
In-house Check Date: 07/30/2025

Equipment List

Manufacturer	Model	Description	Serial Number	Calibration Date	Calibration Due	CBT
Rohde & Schwarz	ZNL20	Vector Network Analyzer	101202	9/12/24	9/12/25	
Rohde & Schwarz	ZN-Z135	Calibration Kit	5000-309192839	10/31/24	10/31/26	
Control Company	4040	Ambient Thermometer	230581657	8/28/23	8/28/25	
Control Company	4040	Ambient Thermometer	230581662	8/28/23	8/28/25	
Control Company	4352	Long Stem Liquid Thermometer	230662223	9/28/23	9/28/25	
Control Company	4352	Long Stem Liquid Thermometer	230662212	9/28/23	9/28/25	
Micro-Coax	UFB205A-0-0240-30x30	SMA M-F RF test Cable (DC - 18 GHz)	-			✓
Maury-Micro	360D	10dB RF Fixed Attenuator (DC - 18 GHz) + Short Circuit Termination	7799	12/28/24	12/28/25	
Huber+Suhner	SF126	High Performance RF Cable	570292/126			✓
Mini-Circuits	VLK-8400+	Coaxial Low Pass Filter (DC - 8.4 GHz)	-			✓
SPEAG	DAE4ip	Data Acquisition Electronics with Integ. Power	1839	9/4/24	9/4/25	
SPEAG	DAK-3.5	DAK-3.5 Dielectric Probe	1349	9/2/24	9/2/25	
SPEAG	EX3DV4	SAR Measurement Probe	7836	9/12/24	9/12/25	
Anritsu	MA24118A	Microwave USB Power Sensor (10MHz - 18 GHz)	2123431	1/13/25	1/13/26	
Anritsu	MA24118A	Microwave USB Power Sensor (10MHz - 18 GHz)	2123500	1/13/25	1/13/26	
Rohde & Schwarz	SMCV100B	R&S SMCV100B Vector Signal Generator (VSG)	103882	12/21/23	12/19/25	
Amplifier Research	1554G8AM1	RF Broadband Amplifier (4 - 8 GHz)	0554497			✓
Mini-Circuits	VLK-8400+	Coaxial Low Pass Filter (DC - 8.4 GHz)	-			✓
Narda	4226-20 (26733)	20 dB SMA Directional Coupler (0.5 - 18 GHz)	0201			✓
Mini-Circuits	BW-S3W2+	3dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	BW-S3W2+	3dB RF Fixed Attenuator (DC - 18 GHz)	-			✓
Mini-Circuits	CBL-6FT-SMNM+	Precision Test Cable SMA/N (DC - 18 GHz)	3318			✓
Mini-Circuits	CBL-6FT-SMNM+	Precision Test Cable SMA/N (DC - 18 GHz)	3335			✓

CBT: Components calibrated before testing. Prior to testing, the measurement paths containing a cable, attenuator, coupler or filter were connected to a calibrated source (i.e. a signal generator, power sensor, or VNA) to determine the losses of the measurement path. The power meter offset was then adjusted to compensate for the measurement system losses. This level offset is stored within the power meter before measurements are made. This calibration verification procedure applies to the system verification and output power measurements. The calibrated reading is then taken directly from the power meter after compensation of the losses for all final power measurements.

Measurement Uncertainty = $\pm 27\%$ ($k=2$)

	Name	Function	Signature
Tested By:	Yue Li	Engineer	
Approved By:	Phuong Nguyen	Technical Manager	

Per FCC KDB Publication 865664 D01, dipole can have longer calibration intervals of up to three years when it is demonstrated that the SAR target, impedance and return loss of the dipole have remained stable according to the following requirements:

1. Measured SAR does not deviate from the calibrated SAR value by more than 10%.
2. Return loss does not deviate by more than 20% from the previous measurement (i.e. value in dB x 0.2) and meet the required minimum return-loss.
3. Real and imaginary part of the impedance do not deviate by more than 5 Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have an extended calibration interval:

Dipole SN	Freq (MHz)	In-house Check Date	Cal Date	Head SAR target (1g) @ 30dBm (W/kg)	Measured Head SAR (1g) @ 17dBm (W/kg)	1g SAR Dev (%)	Head SAR target (10g) @ 30dBm (W/kg)	Measured Head SAR (10g) @ 17dBm (W/kg)	10g SAR Dev (%)	Cert Head Impedance (Ohm) - Real	Previous Head Impedance (Ohm) - Real	Measured Head Impedance (Ohm) - Real	Head Impedance Deviation (Ohm) - Real	Cert Head Impedance (Ohm) - Imaginary	Previous Head Impedance (Ohm) - Imaginary	Measured Head Impedance (Ohm) - Imaginary	Head Impedance Deviation (Ohm) - Imaginary	Cert Head Return Loss (dB)	Previous Head Return Loss (dB)	Measured Head Return Loss (dB)	Return Loss Dev (%)	PASS/FAIL	Note
1104	6500	1/3/2025	11/14/2024							48.1	48.1	48.1	0.0	1.1	1.1	1.1	0.0	-33.1	-33.1	-33.1	0.00%	PASS	In-house check after Calibration
1104	6500	7/30/2025	11/14/2024	298	35.30	2.44%	55	2.83	2.67%	48.1	48.1	48.2	0.1	1.1	1.1	1.0	-0.1	-33.1	-33.1	-33.5	-8.00%	PASS	-

Impedance and Return-Loss Measurement Plot for Head TSL

