



Appendix D

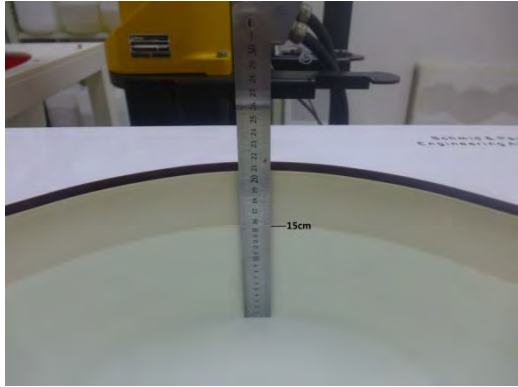
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position

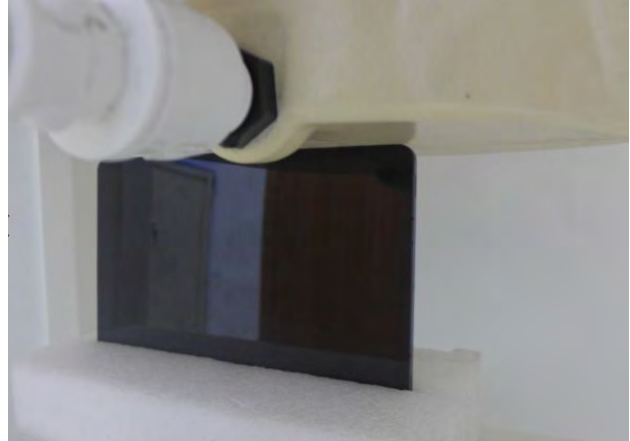
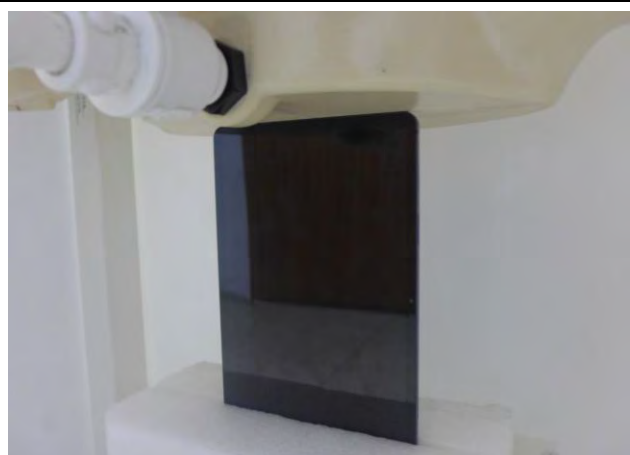
Photo 3: Back side 0mm	Photo 4: Left side 0mm
	
Photo 5: Right side 0mm	Photo 6: Top side 0mm
	



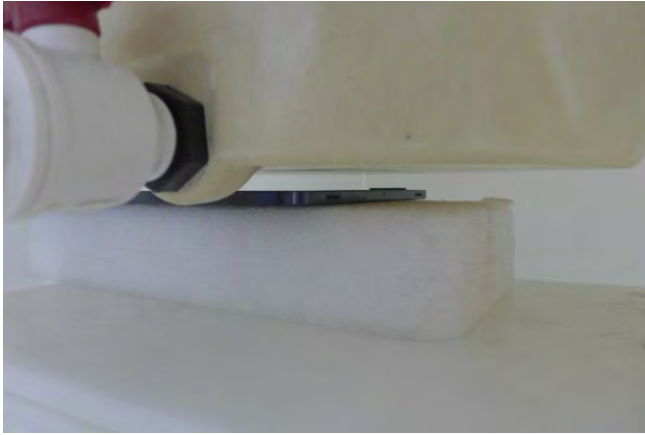
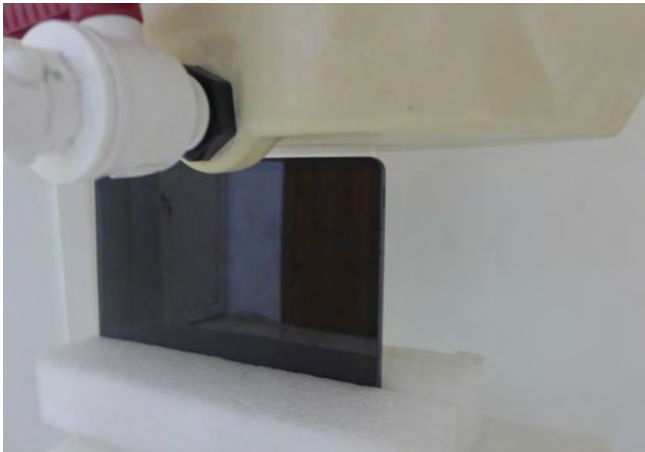
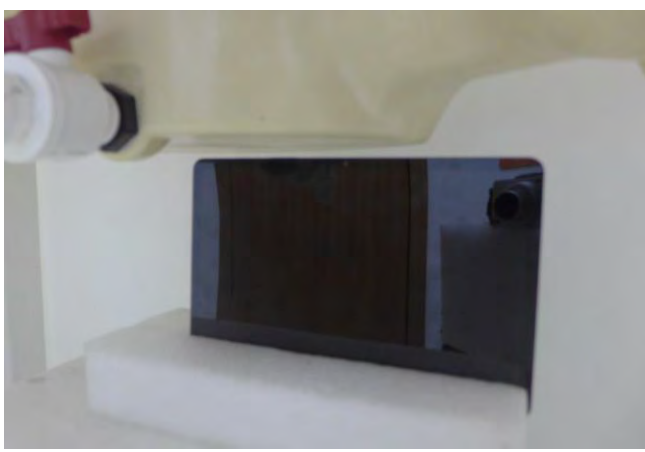
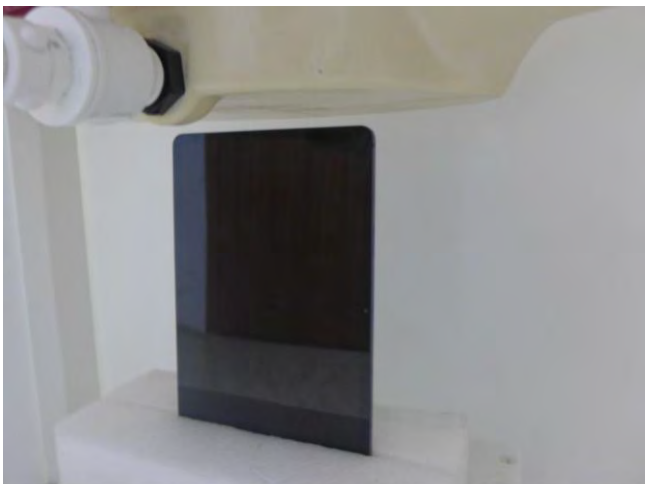
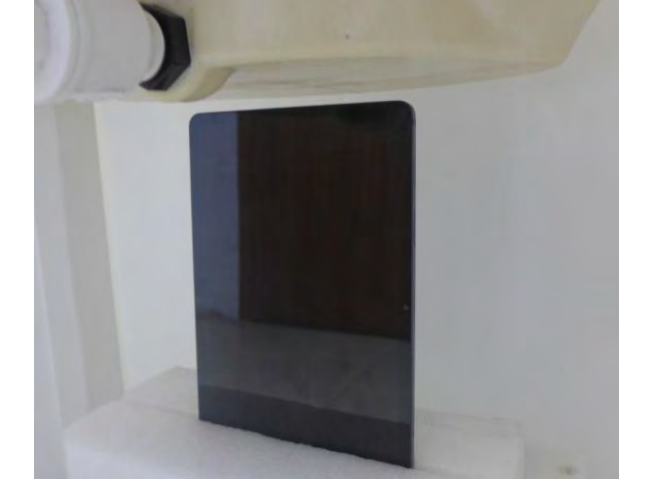
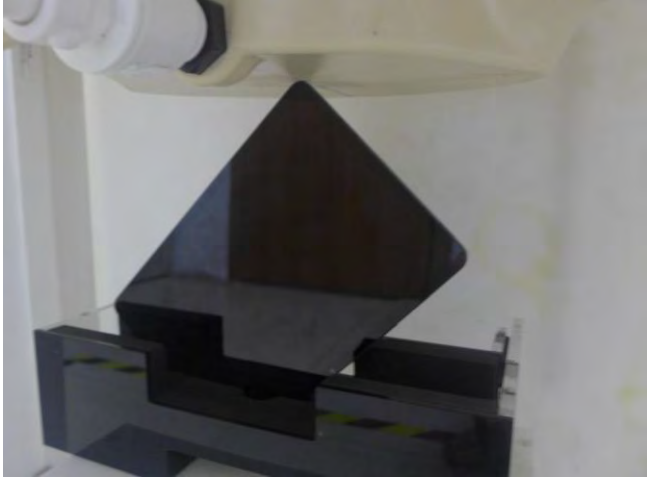
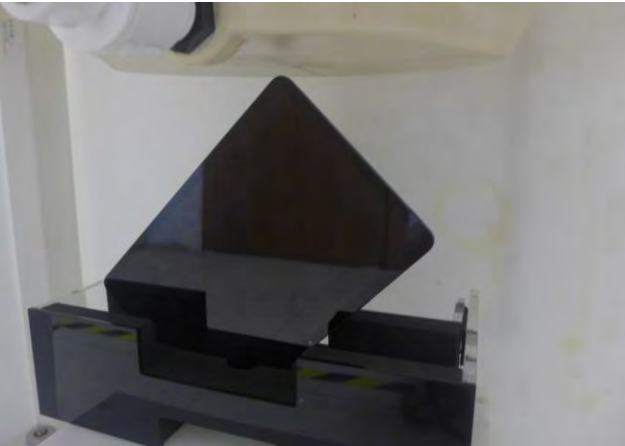
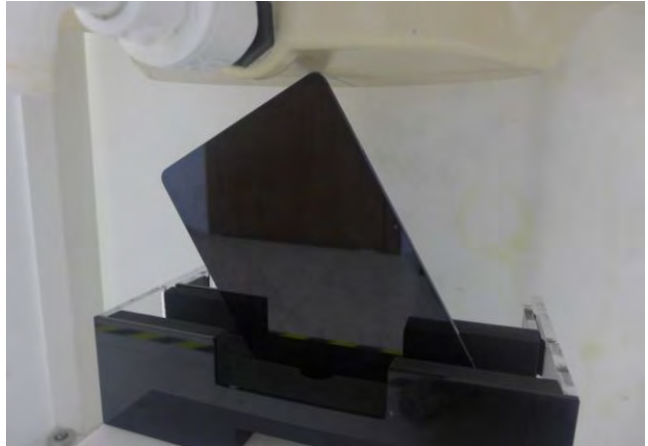
Photo 7: Back side 10mm	Photo 8: Back side 11mm
	
Photo 9: Left side 7mm	Photo 10: Right side 8mm
	
Photo 11: Top side 14mm	Photo 12: Top side 15mm
	



Photo 13: Keyboard Face 0mm	Photo 14: Left Corner 0mm
	
Photo 15: Left Corner 10mm	Photo 16: Right Corner 0mm
	
Photo 17: Right Corner-12mm	NA
	NA

4. EUT Constructional Details

Photo 18: Front View	Photo 19: Back View
	
Photo 20: Front View with Keyboard	Photo 21: Back View with Keyboard
	
Photo 22: Accessory	NA
	NA