

Date: 2025-09-02

System Check_Head_13MHz**DUT: CLA-13 - SN1011**

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_13_250902 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.757$ S/m; $\epsilon_r = 55.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(14.89, 13.85, 19.11); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041(Laptop); Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.146 W/kg; SAR (10g) = 0.117 W/kg;

TSL Correction: No correction

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 0.136 W/kg; SAR (8g) = 0.089 W/kg; SAR (10g) = 0.084 W/kg

Smallest distance from peaks to all points 3 dB below = 15.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: No correction

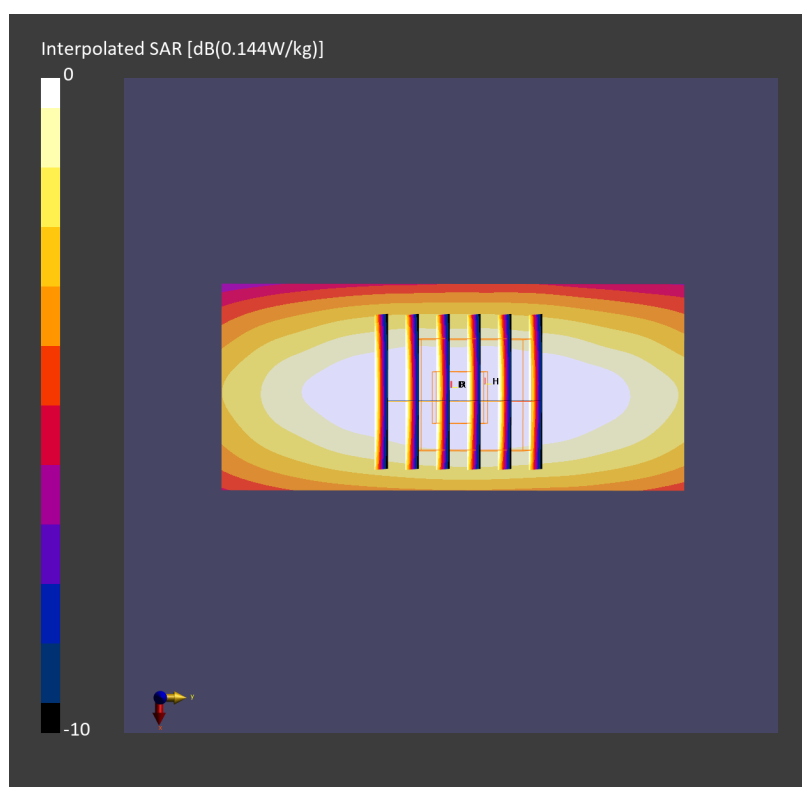

Date: 2025-08-01

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250801 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.446 W/kg; SAR (10g) = 0.297 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.12 dB

SAR (1g) = 0.435 W/kg; SAR (8g) = 0.310 W/kg; SAR (10g) = 0.295 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

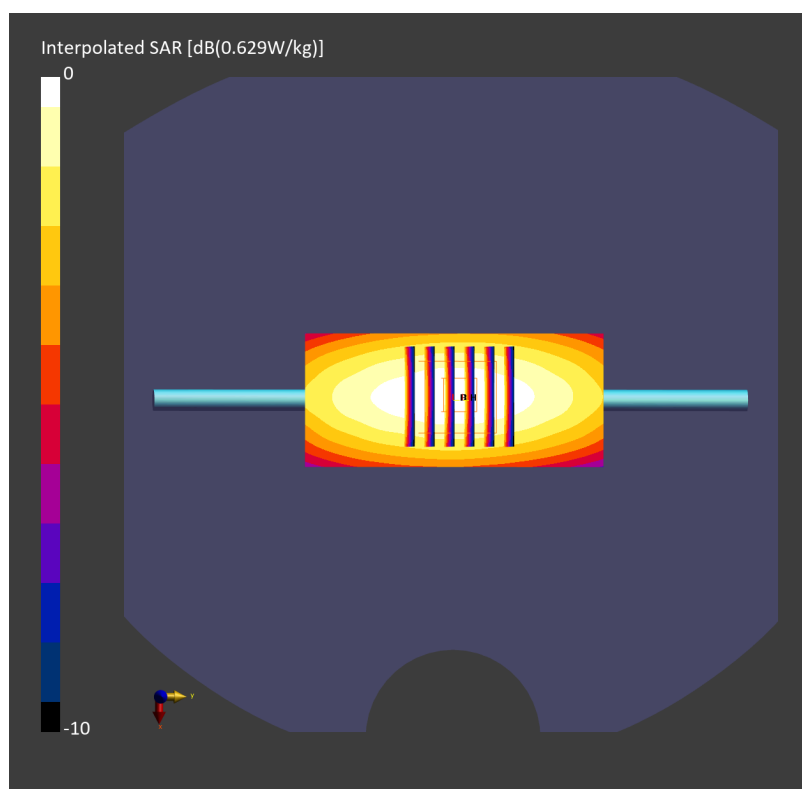

Date: 2025-08-03

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250803 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.877$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.423 W/kg; SAR (10g) = 0.281 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.423 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.286 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

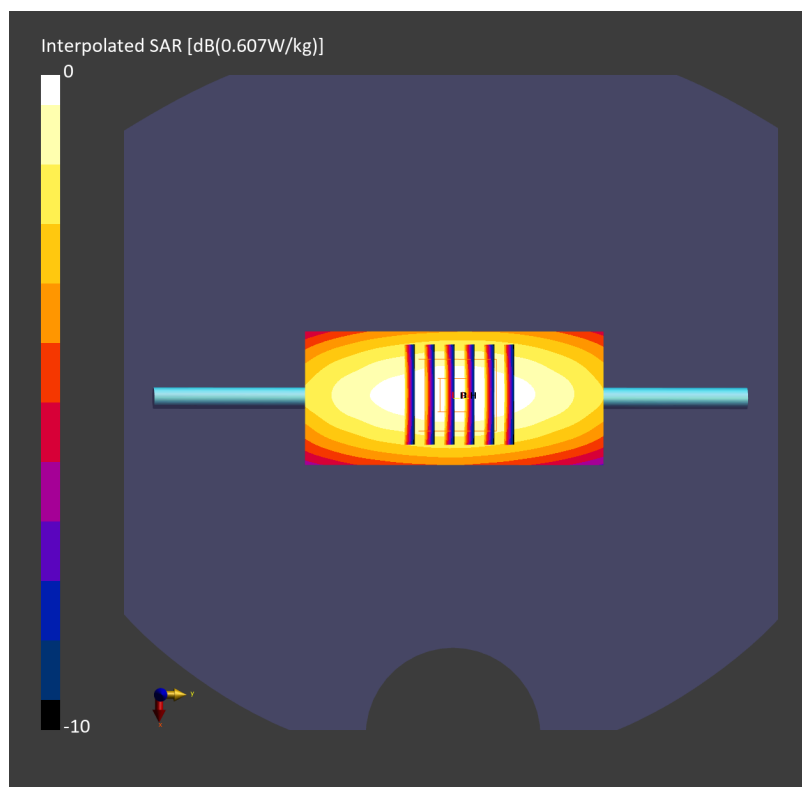

Date: 2025-08-05

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250805 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.868$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.278 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 0.419 W/kg; SAR (8g) = 0.299 W/kg; SAR (10g) = 0.285 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.9 %

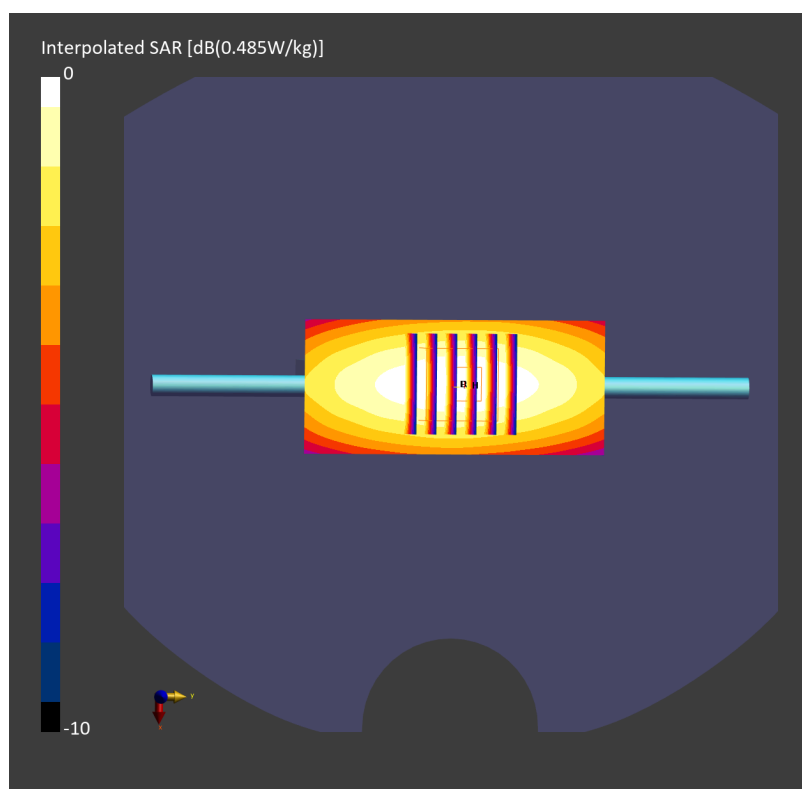

Date: 2025-08-06

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250806 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.428 W/kg; SAR (10g) = 0.285 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.428 W/kg; SAR (8g) = 0.306 W/kg; SAR (10g) = 0.291 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

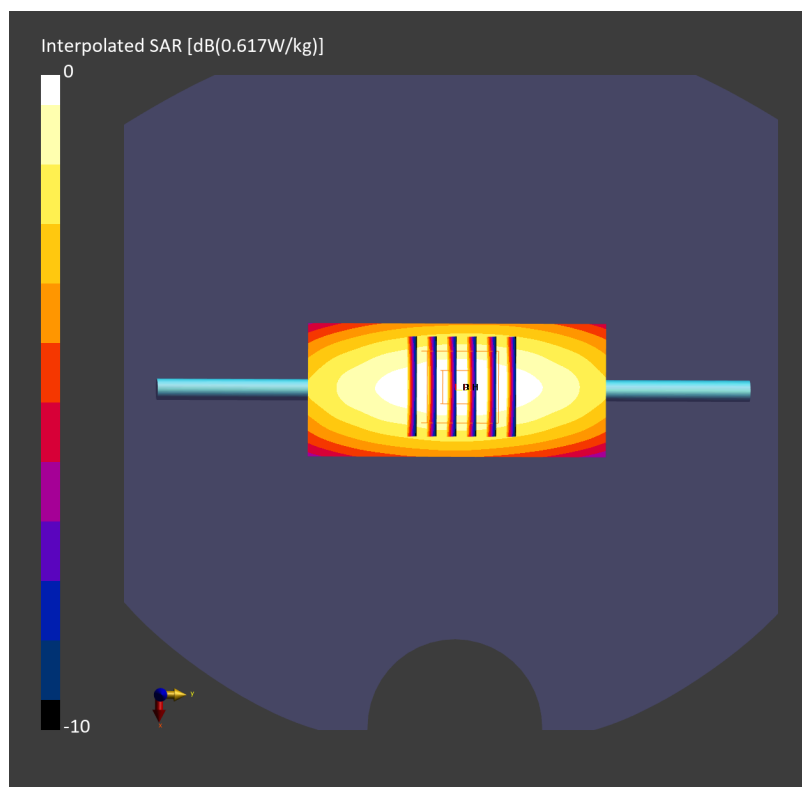

Date: 2025-08-10

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250810 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.877$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(9.63, 9.34, 9.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.41 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.09 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

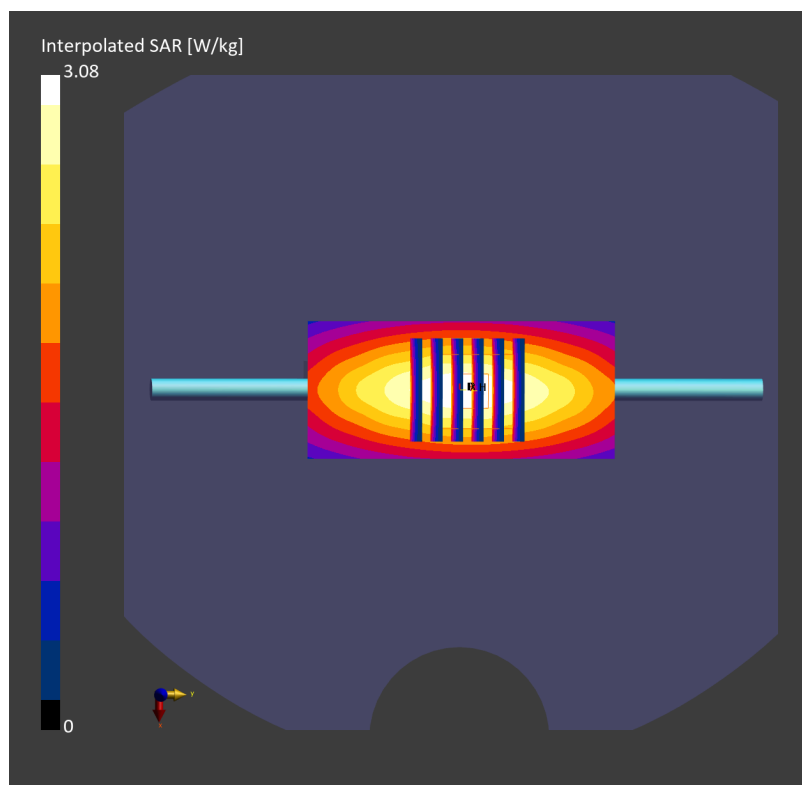

Date: 2025-08-11

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250811 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.883$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(9.63, 9.34, 9.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.42 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.11 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

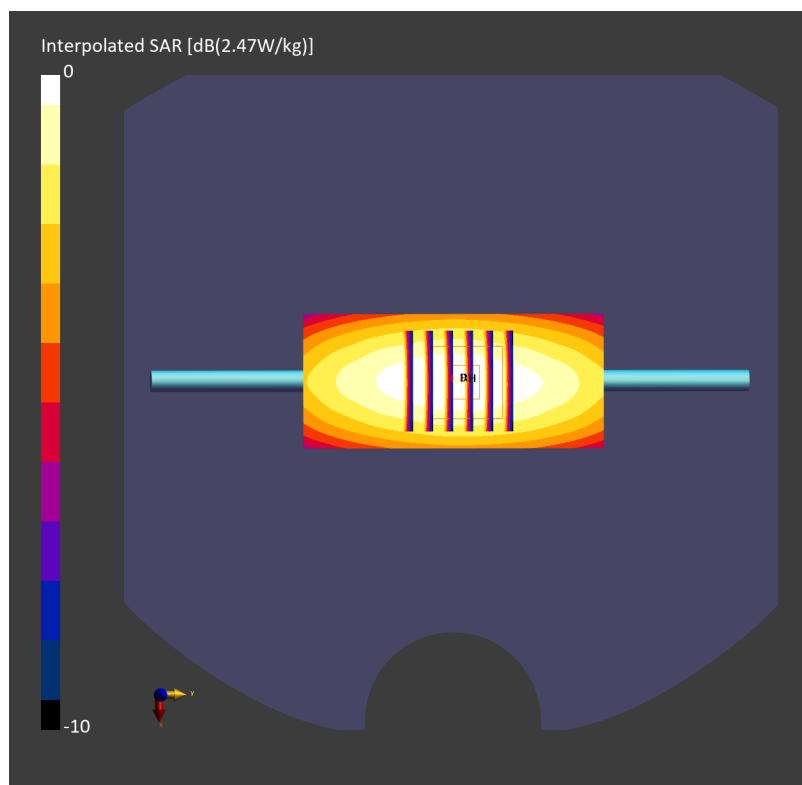

Date: 2025-08-12

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250812 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.881$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(9.63, 9.34, 9.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.43 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.12 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

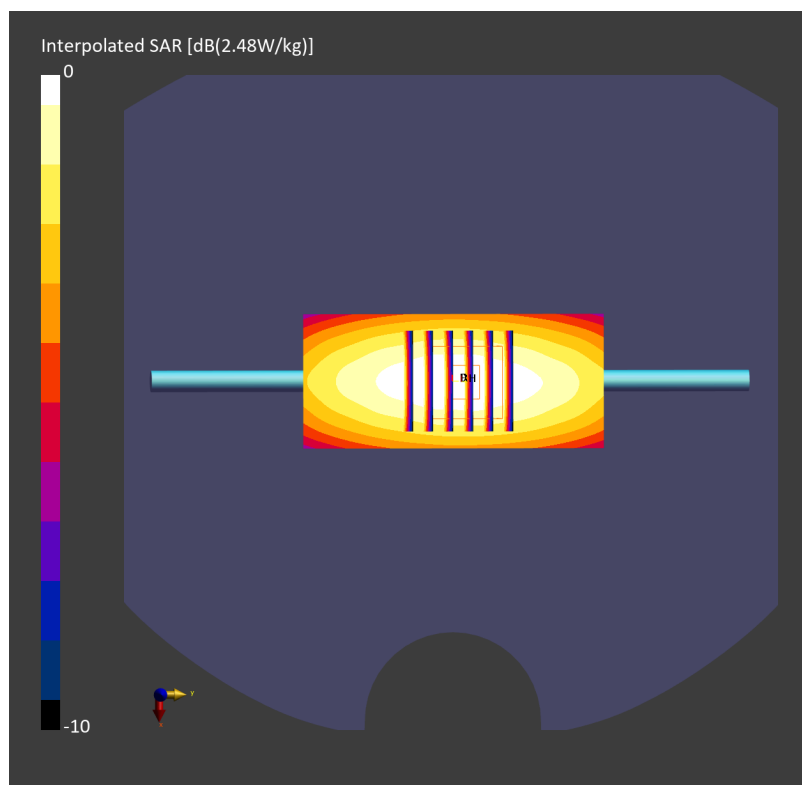

Date: 2025-08-19

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250819 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.279 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.420 W/kg; SAR (8g) = 0.295 W/kg; SAR (10g) = 0.281 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

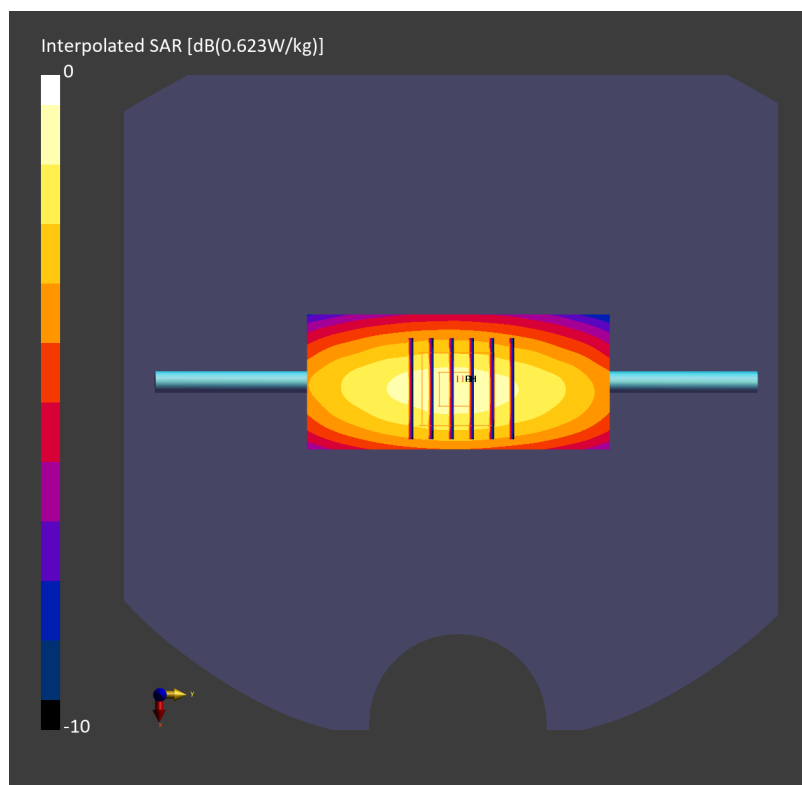

Date: 2025-08-23

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250823 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.876$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.413 W/kg; SAR (10g) = 0.274 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.411 W/kg; SAR (8g) = 0.289 W/kg; SAR (10g) = 0.274 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

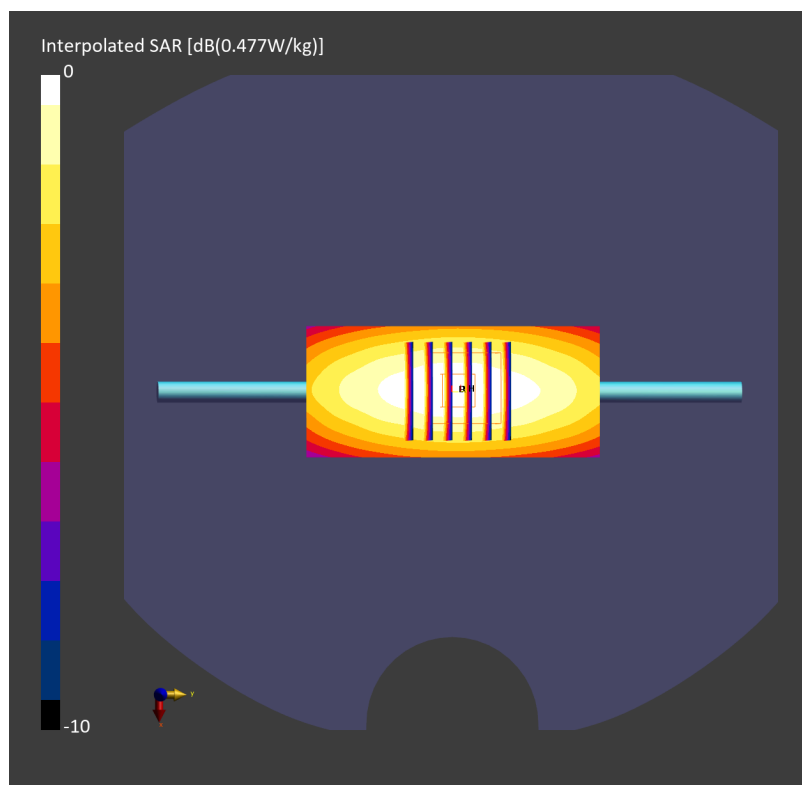

Date: 2025-08-27

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250827 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.905$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.431 W/kg; SAR (10g) = 0.286 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 0.430 W/kg; SAR (8g) = 0.303 W/kg; SAR (10g) = 0.288 W/kg

Smallest distance from peaks to all points 3 dB below = 22.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: No correction

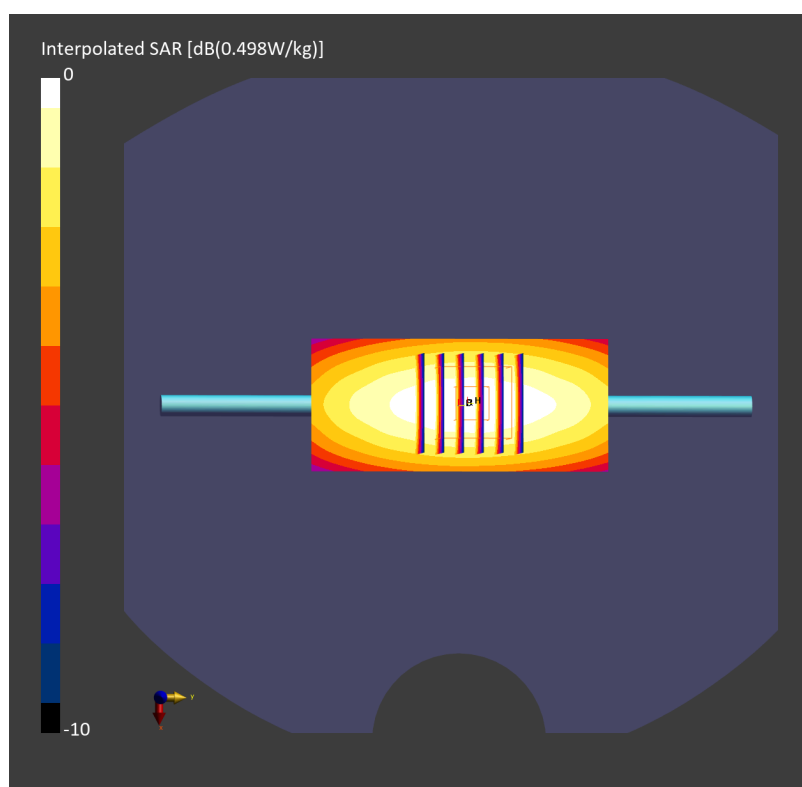

Date: 2025-08-28

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250828 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.879$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.416 W/kg; SAR (10g) = 0.280 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.417 W/kg; SAR (8g) = 0.295 W/kg; SAR (10g) = 0.280 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

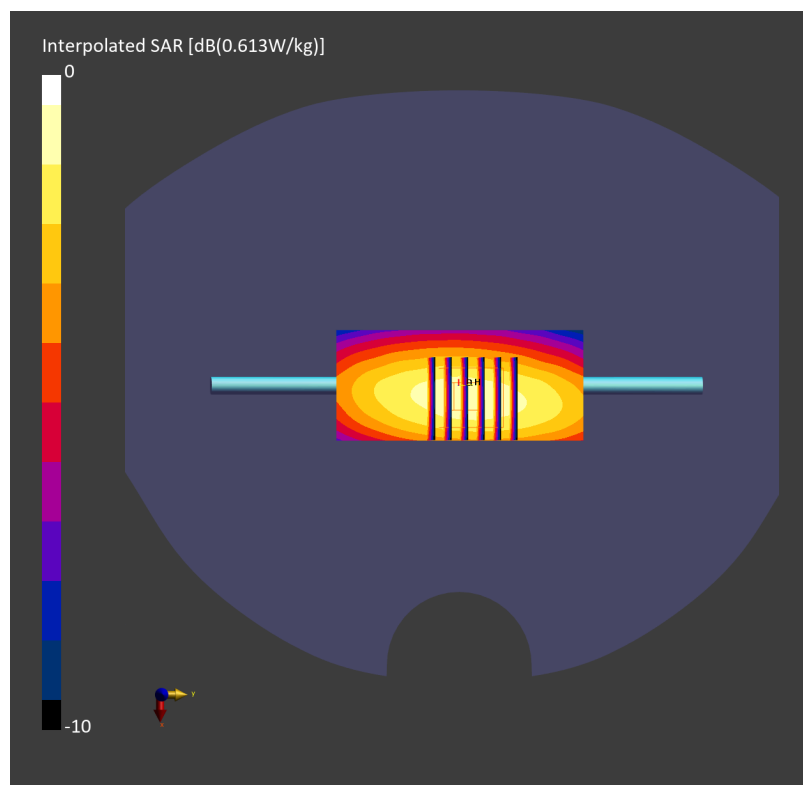

Date: 2025-08-30

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_250830 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.884$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.289 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 0.421 W/kg; SAR (8g) = 0.296 W/kg; SAR (10g) = 0.281 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

TSL Correction: No correction

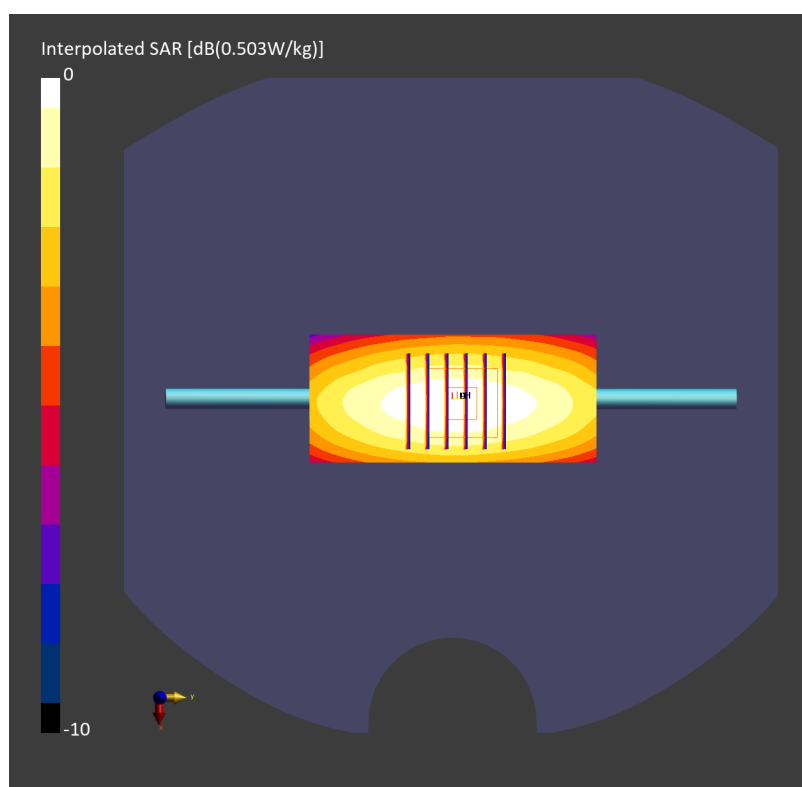

Date: 2025-08-02

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250802 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.917$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.36, 7.56, 9.63); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.496 W/kg; SAR (10g) = 0.328 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 0.502 W/kg; SAR (8g) = 0.360 W/kg; SAR (10g) = 0.323 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

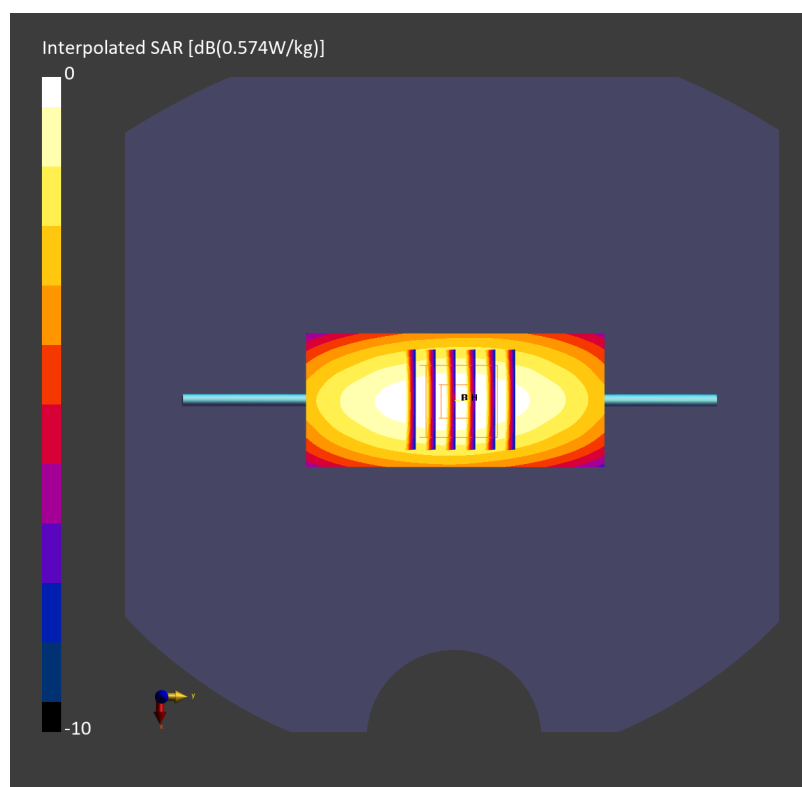

Date: 2025-08-04

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250804 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.913$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.36, 7.56, 9.63); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.494 W/kg; SAR (10g) = 0.326 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.501 W/kg; SAR (8g) = 0.359 W/kg; SAR (10g) = 0.321 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

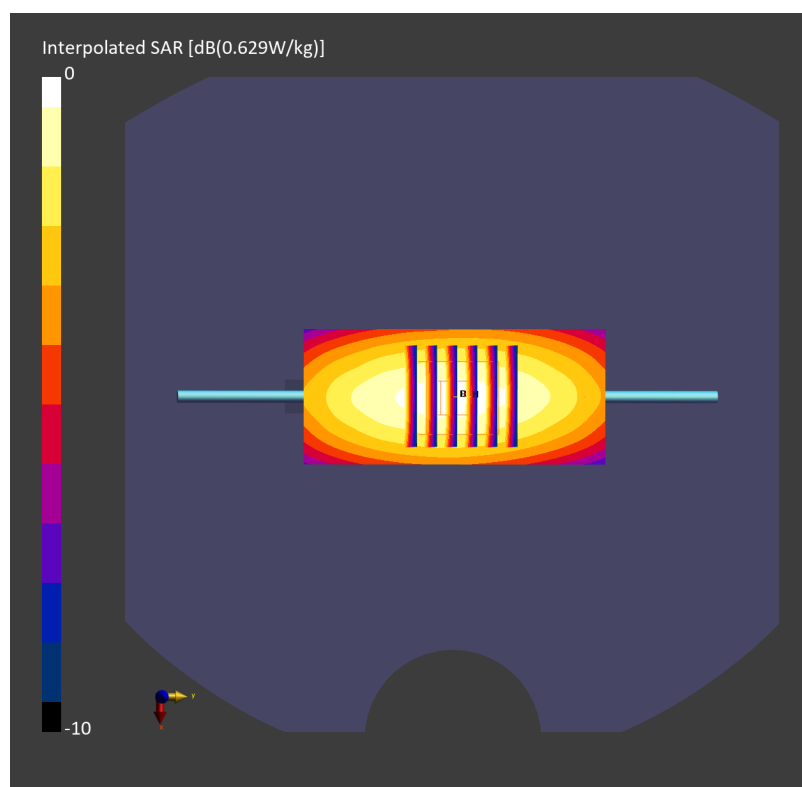

Date: 2025-08-09

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250809 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.910$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(9.45, 9.17, 9.66); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.61 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.68 W/kg; SAR (10g) = 1.60 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

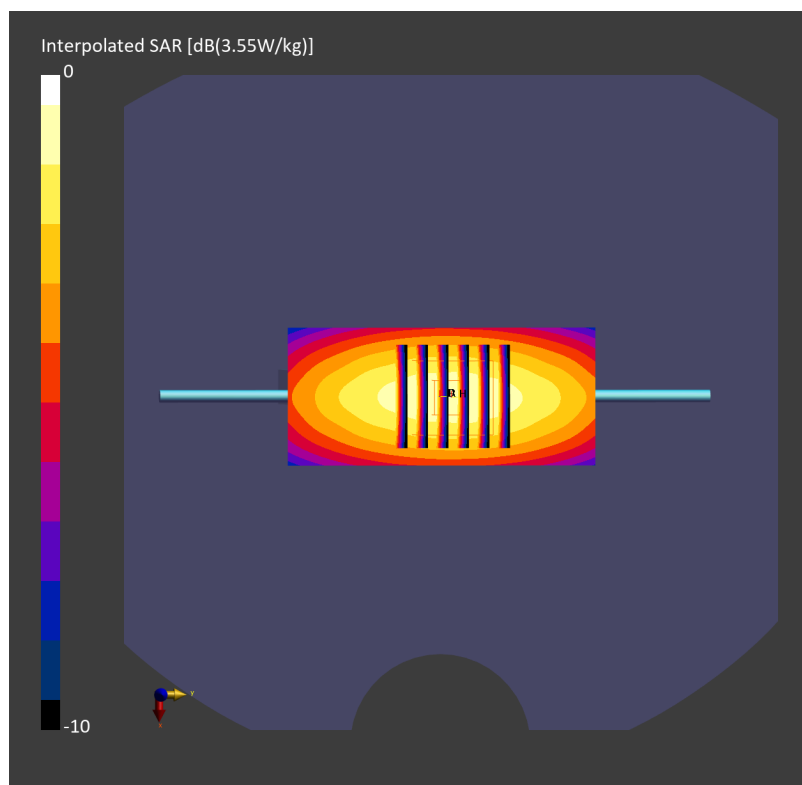

Date: 2025-08-10

System Check_Head_835MHz**DUT: D835V2 - SN499**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250810 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.906$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(9.45, 9.17, 9.66); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.60 W/kg;


Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.67 W/kg; SAR (10g) = 1.58 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

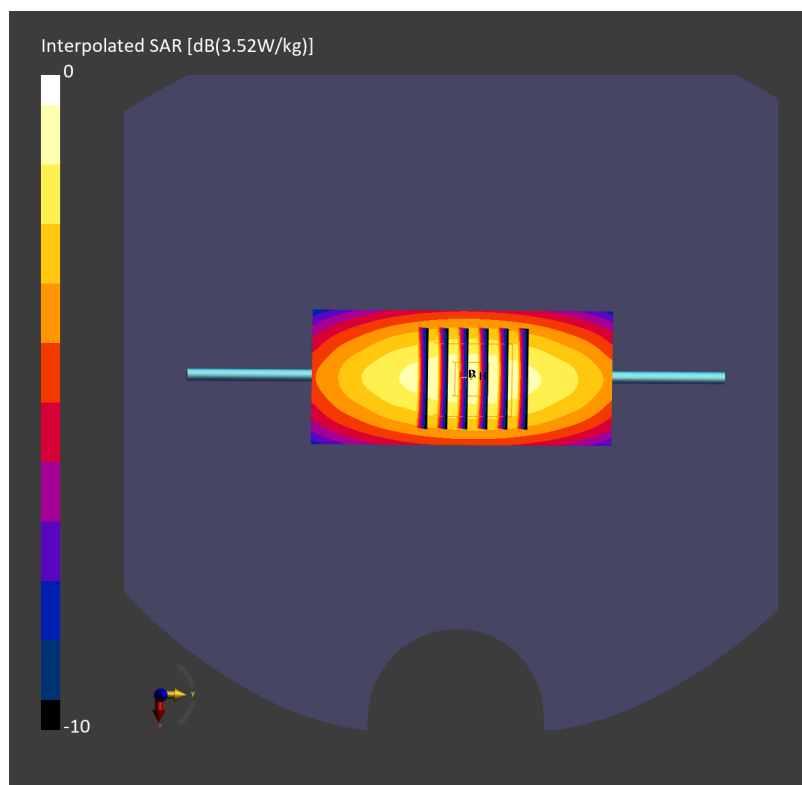

Date: 2025-08-18

System Check_Head_835MHz**DUT: D835V2 - SN499**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250818 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.922$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.500 W/kg; SAR (10g) = 0.329 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.500 W/kg; SAR (8g) = 0.349 W/kg; SAR (10g) = 0.331 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

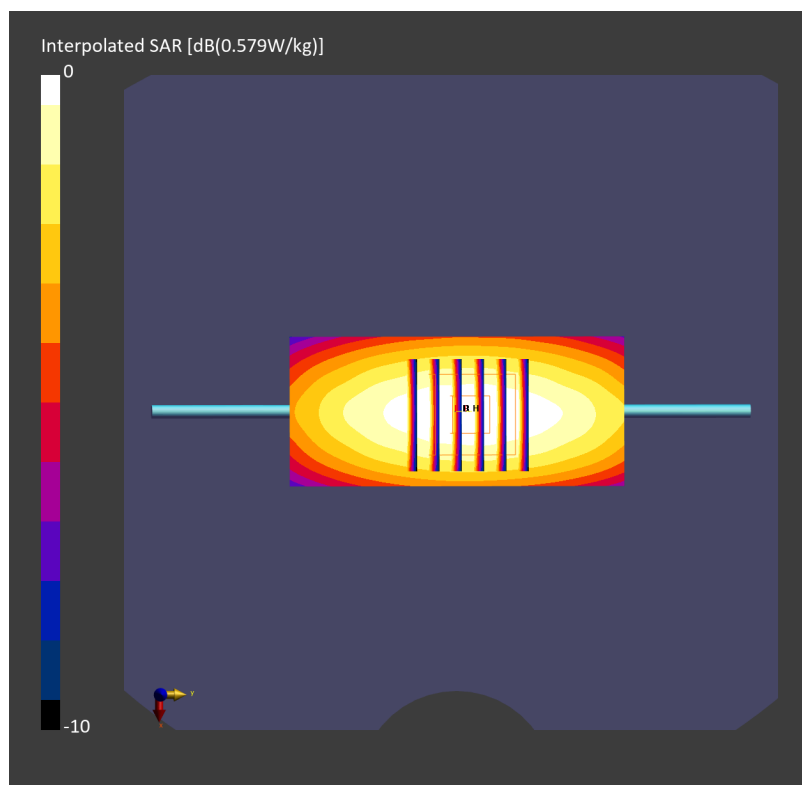

Date: 2025-08-19

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250819 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.496 W/kg; SAR (10g) = 0.329 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.501 W/kg; SAR (8g) = 0.350 W/kg; SAR (10g) = 0.322 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

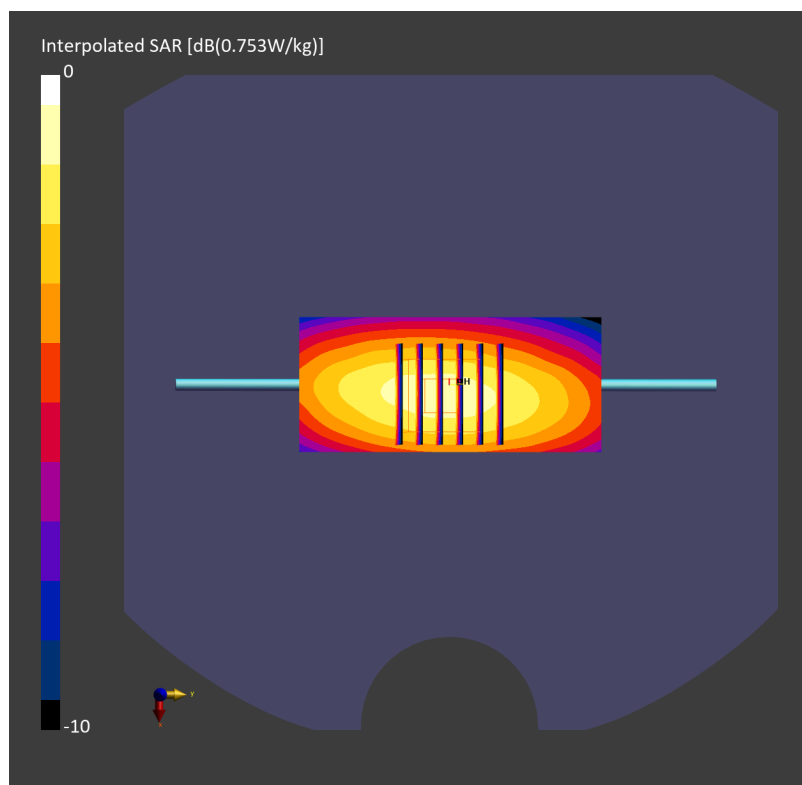

Date: 2025-08-23

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250823 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.909$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.488 W/kg; SAR (10g) = 0.320 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.488 W/kg; SAR (8g) = 0.341 W/kg; SAR (10g) = 0.324 W/kg

Smallest distance from peaks to all points 3 dB below = 18.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

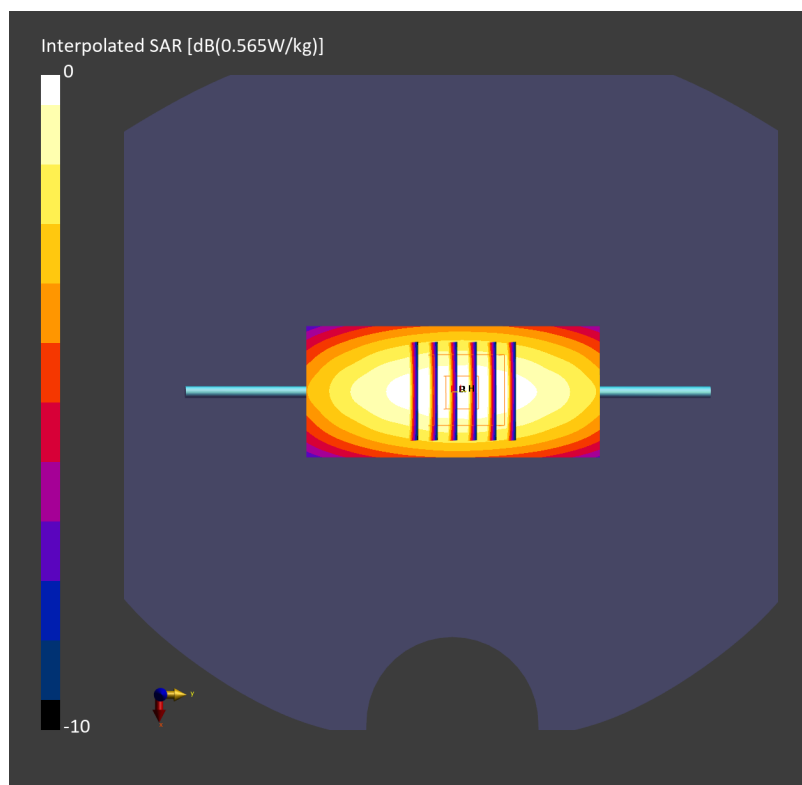

Date: 2025-08-27

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_250827 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.941$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.507 W/kg; SAR (10g) = 0.334 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 0.509 W/kg; SAR (8g) = 0.357 W/kg; SAR (10g) = 0.329 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

TSL Correction: No correction

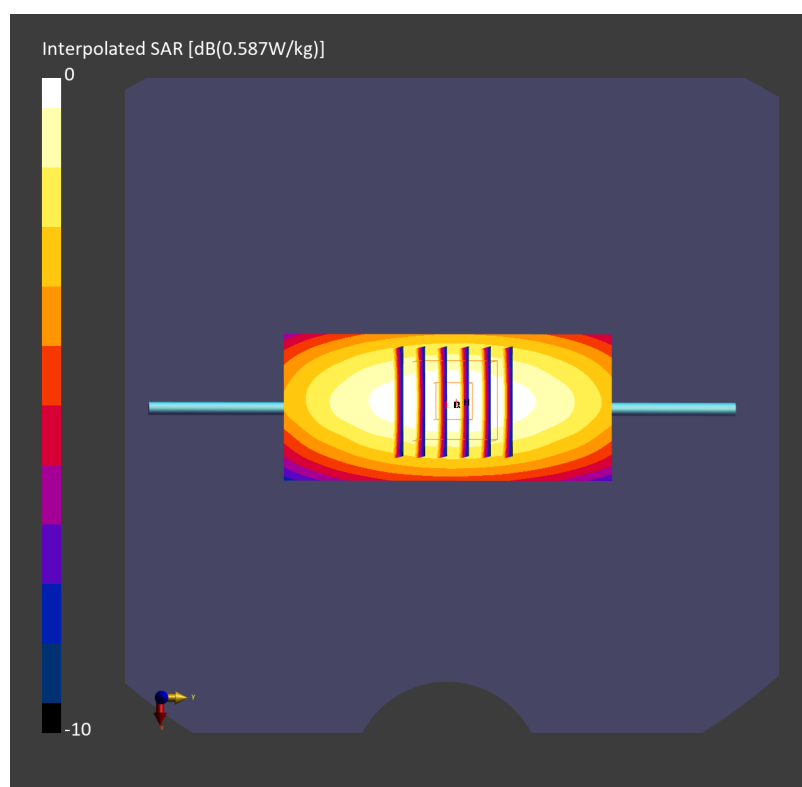

Date: 2025-08-28

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250828 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.911$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.499 W/kg; SAR (10g) = 0.329 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.501 W/kg; SAR (8g) = 0.352 W/kg; SAR (10g) = 0.323 W/kg

Smallest distance from peaks to all points 3 dB below = 20.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

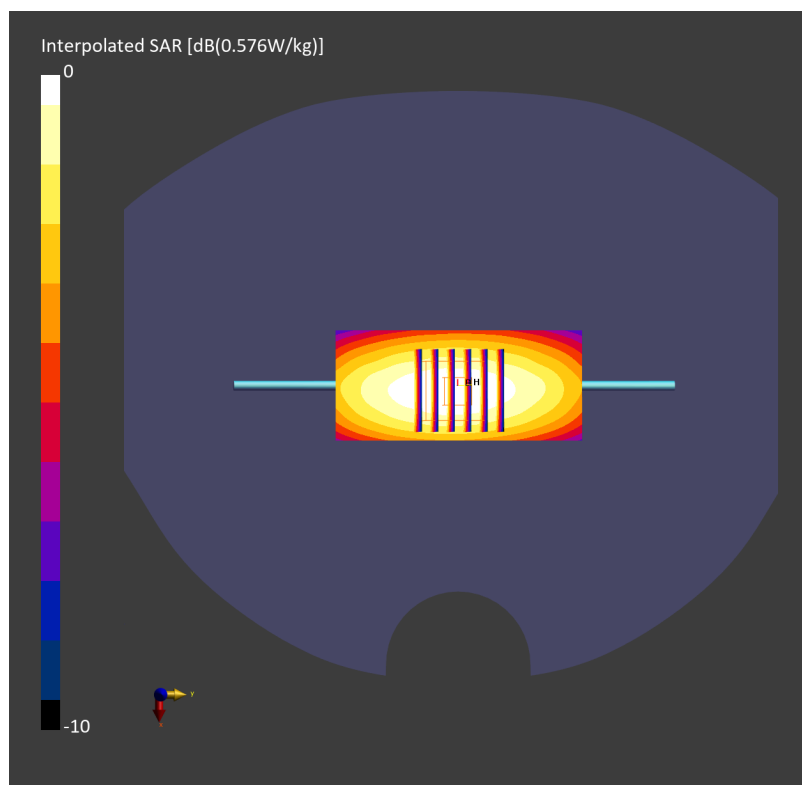

Date: 2025-08-30

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_835_250830 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.917$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.499 W/kg; SAR (10g) = 0.327 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 0.494 W/kg; SAR (8g) = 0.345 W/kg; SAR (10g) = 0.327 W/kg

Smallest distance from peaks to all points 3 dB below = 16.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

TSL Correction: No correction

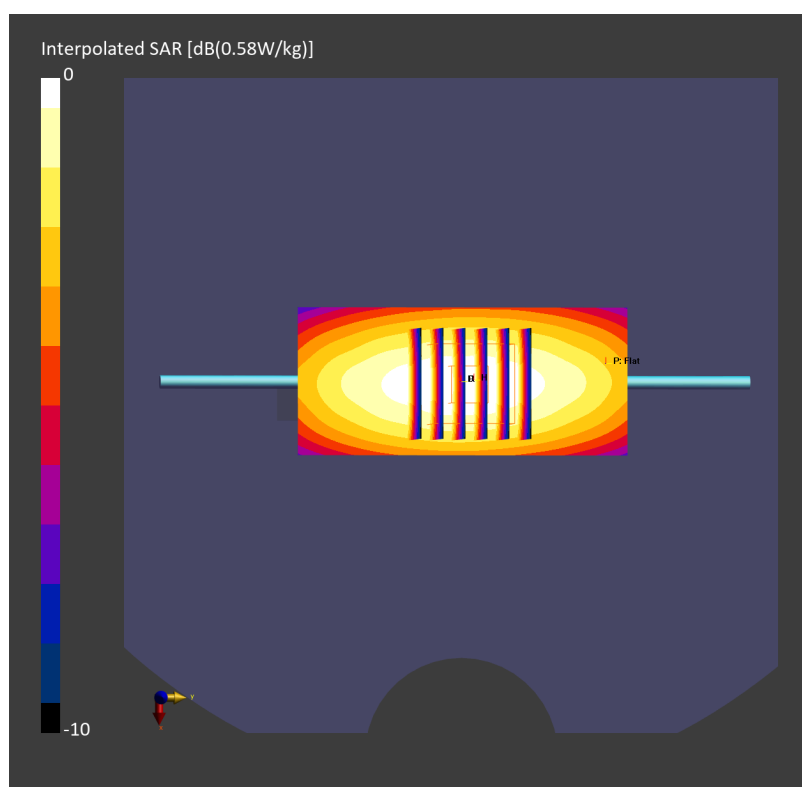

Date: 2025-07-19

System Check_Head_1640MHz**DUT: D1640V2 - SN346**

Communication System: CW; Frequency: 1640.000 MHz

Medium: HSL_1640_250719 Medium parameters used: $f = 1640.000$ MHz; $\sigma = 1.31$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.18, 6.5, 8.27); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.69 W/kg; SAR (10g) = 0.927 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 1.68 W/kg; SAR (8g) = 1.00 W/kg; SAR (10g) = 0.926 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.0 %

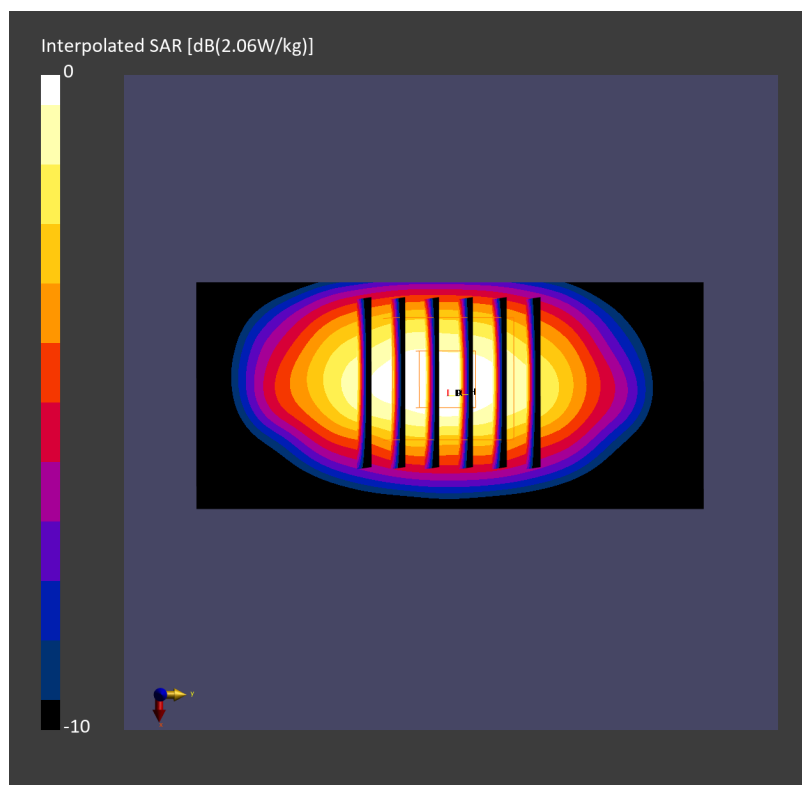

Date: 2025-08-07

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250807 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.948 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.984 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.5 %

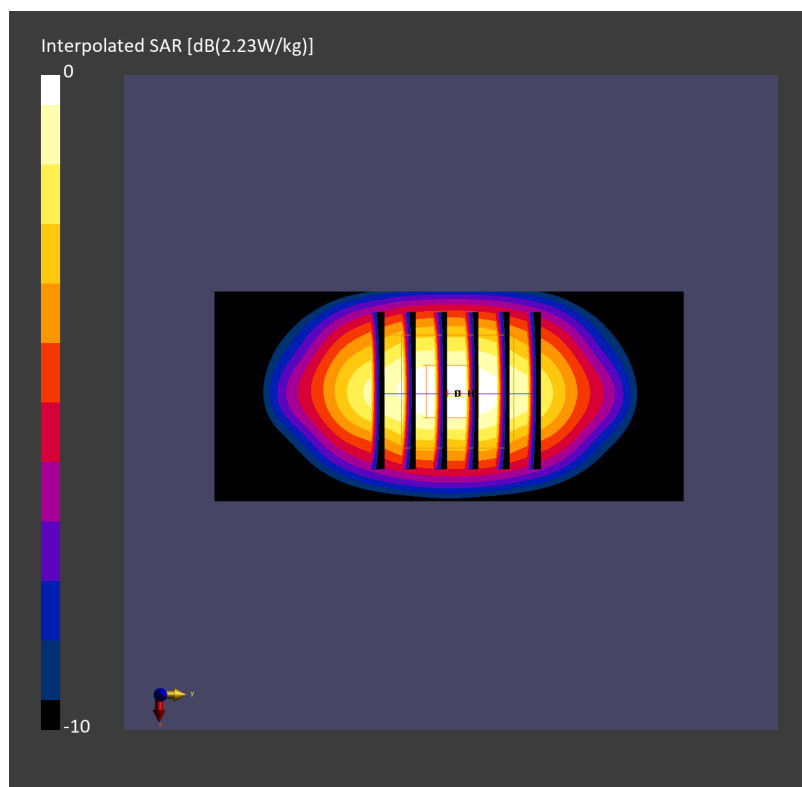

Date: 2025-08-07

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250807 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(7.75, 7.52, 7.93); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.960 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.77 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.952 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.0 %

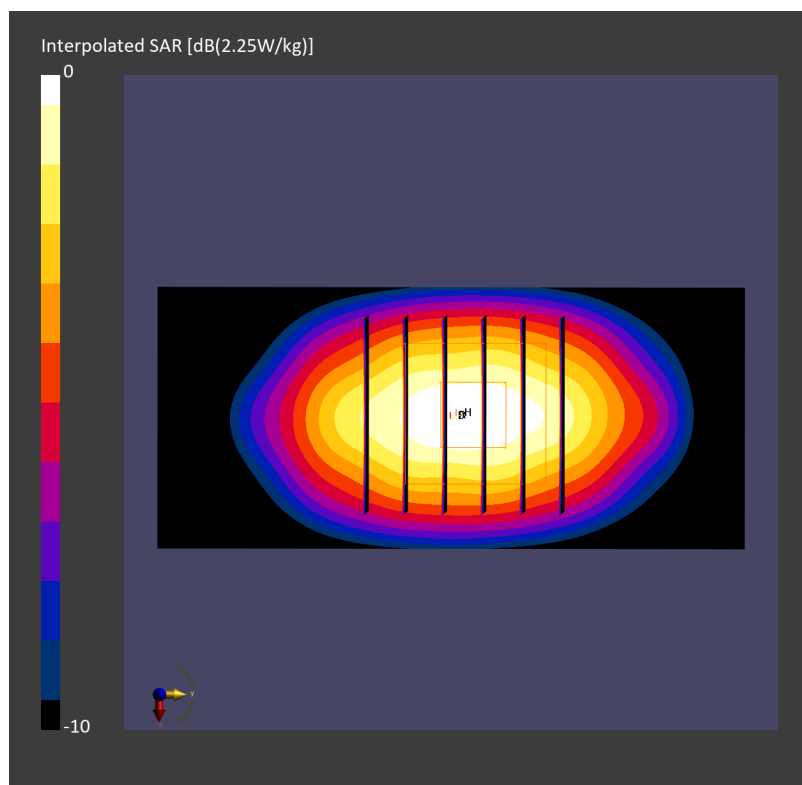

Date: 2025-08-08

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250808 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(7.75, 7.52, 7.93); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.946 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.73 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.934 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.8 %

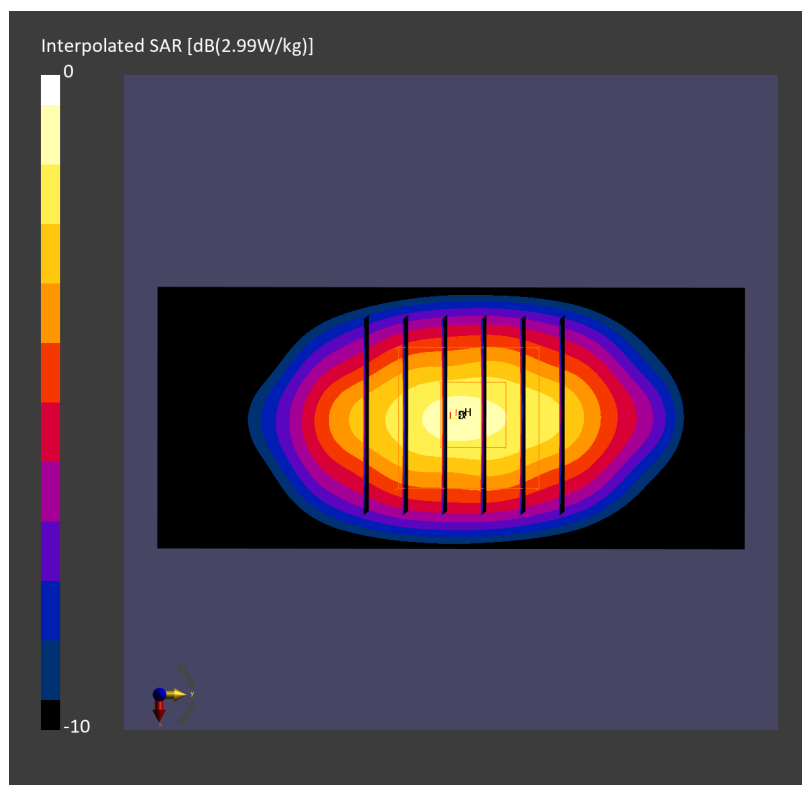

Date: 2025-08-09

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250809 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.964 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.6 %

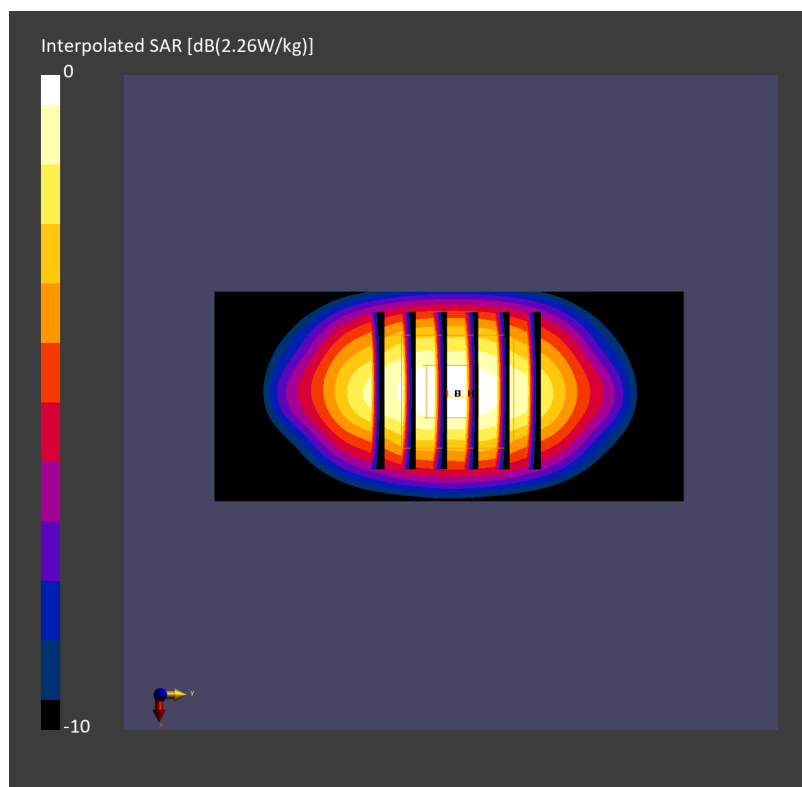

Date: 2025-08-11

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250811 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.33$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.950 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.986 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 86.5 %

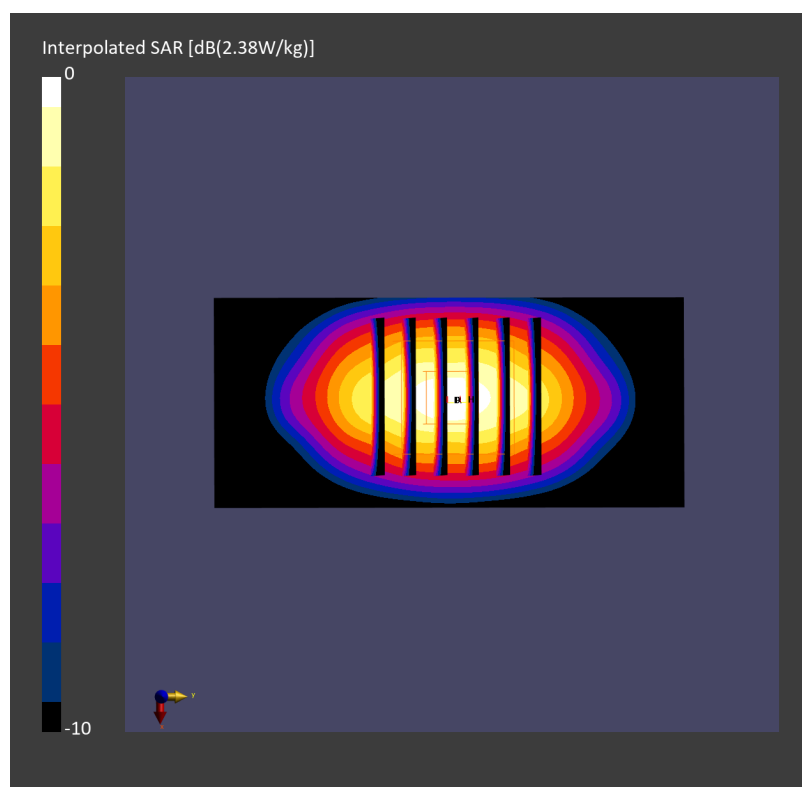

Date: 2025-08-13

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250813 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.962 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.80 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.999 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

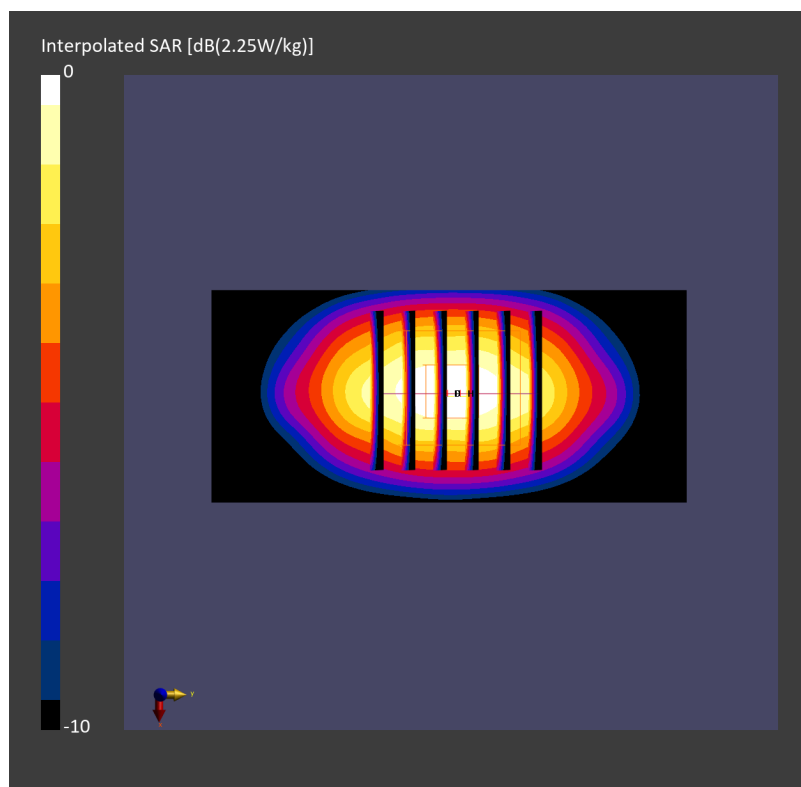

Date: 2025-08-18

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250818 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.88 W/kg; SAR (10g) = 0.997 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

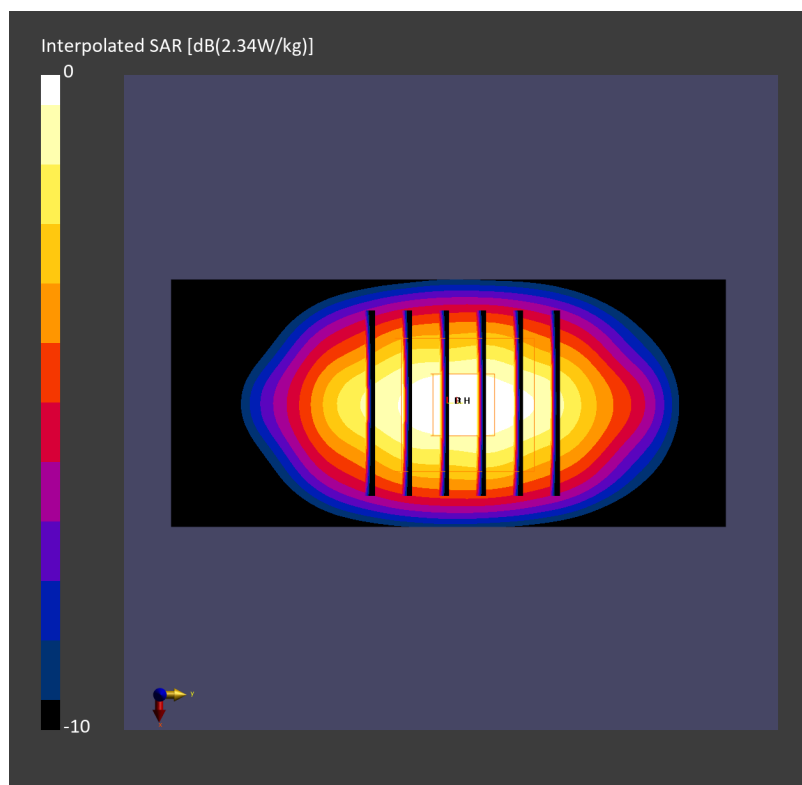

Date: 2025-08-20

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250820 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.01 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.1 %

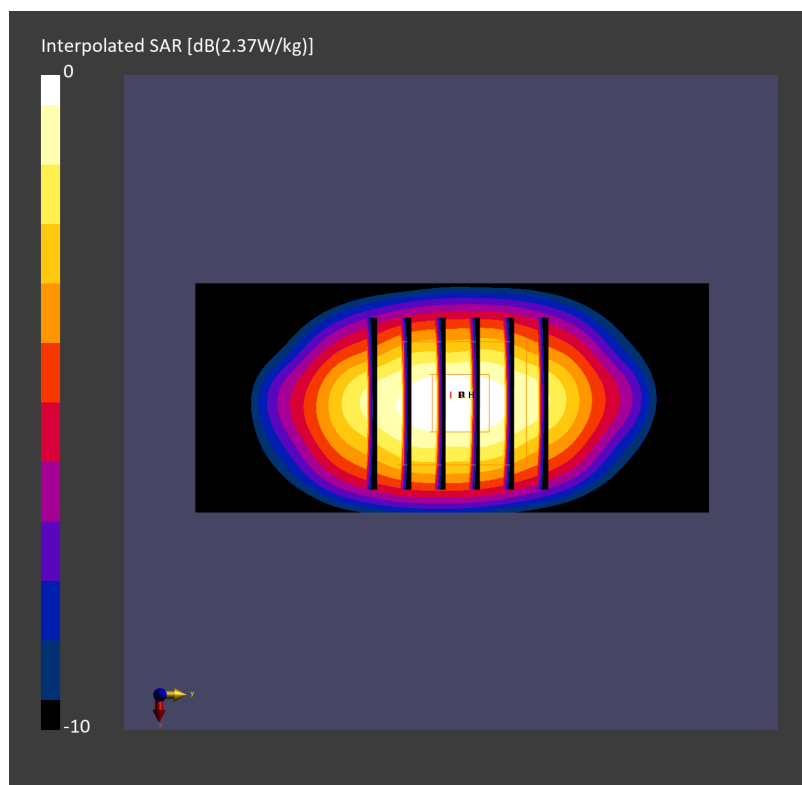

Date: 2025-08-26

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-10000_250826 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: No correction

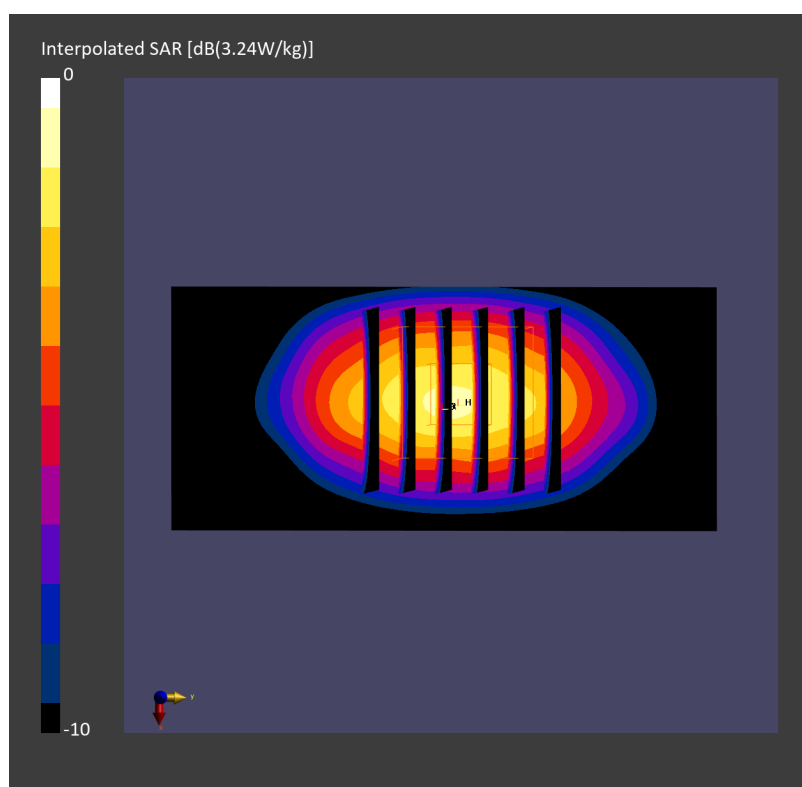

Date: 2025-08-29

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_250829 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 10.9 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: No correction

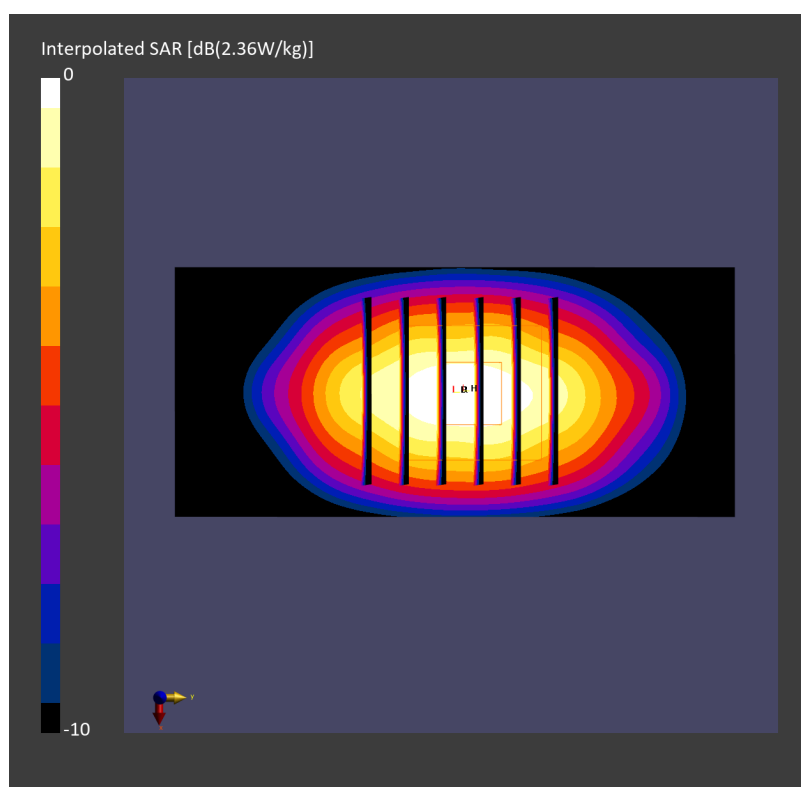

Date: 2025-08-05

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250805 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(7.58, 7.36, 7.76); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.94 W/kg; SAR (10g) = 0.999 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.997 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

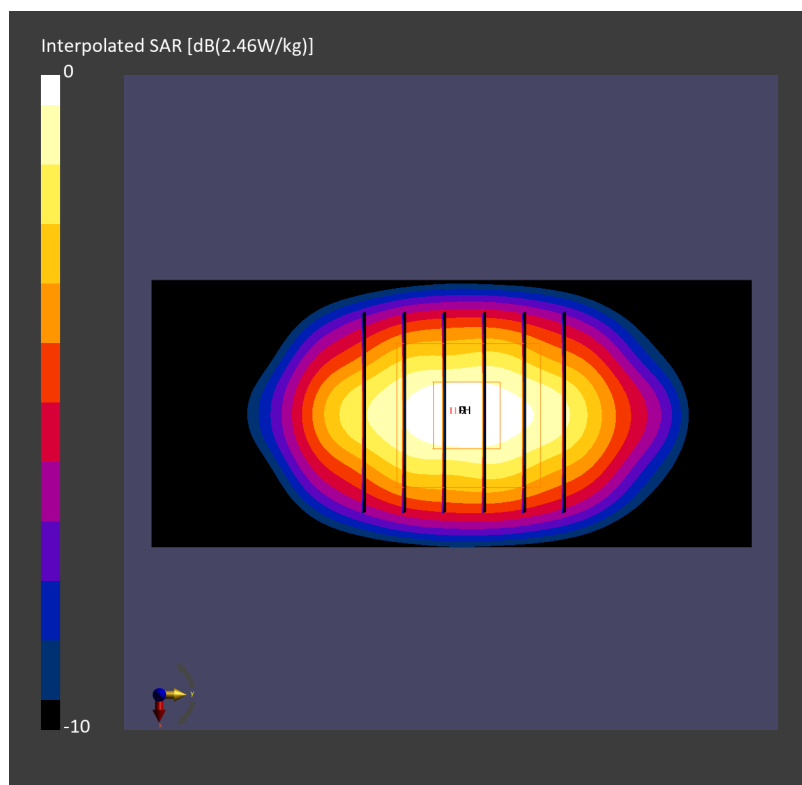

Date: 2025-08-06

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250806 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(7.58, 7.36, 7.76); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 1.01 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.92 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

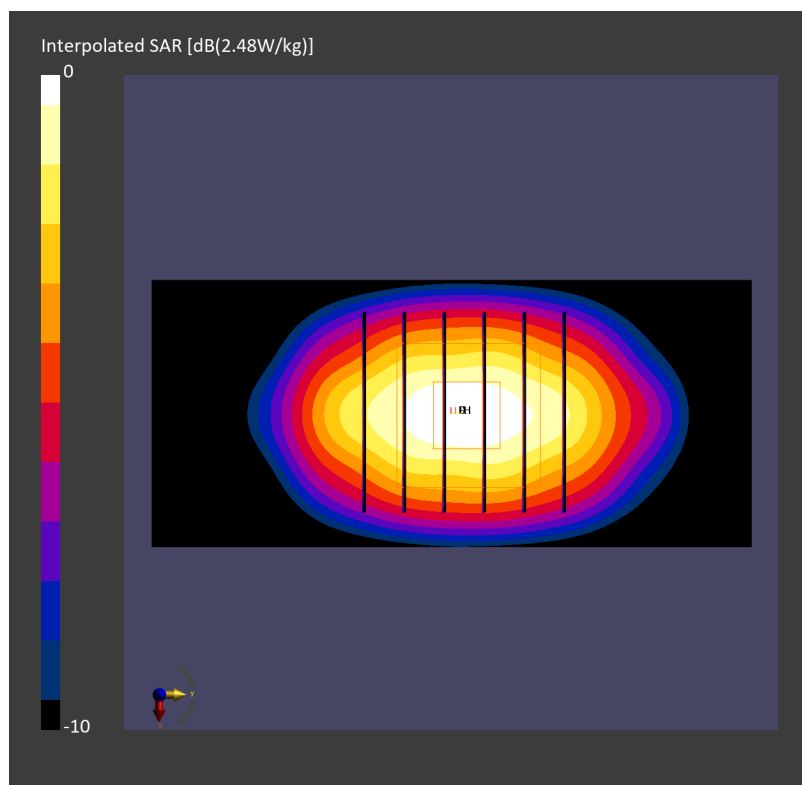

Date: 2025-08-08

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250808 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 0.978 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

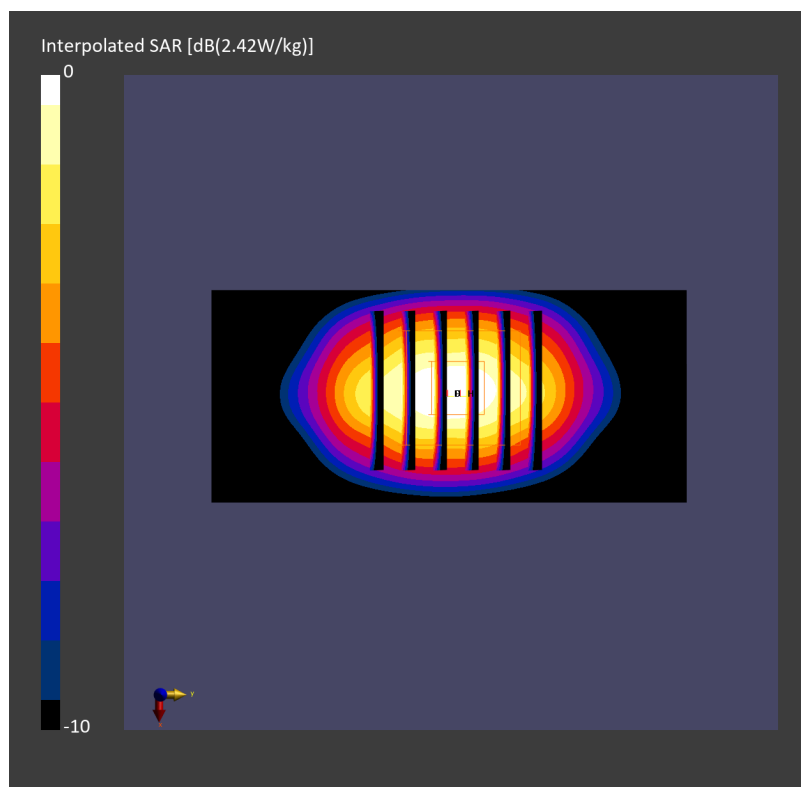

Date: 2025-08-10

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250810 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.94 W/kg; SAR (10g) = 0.996 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.94 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

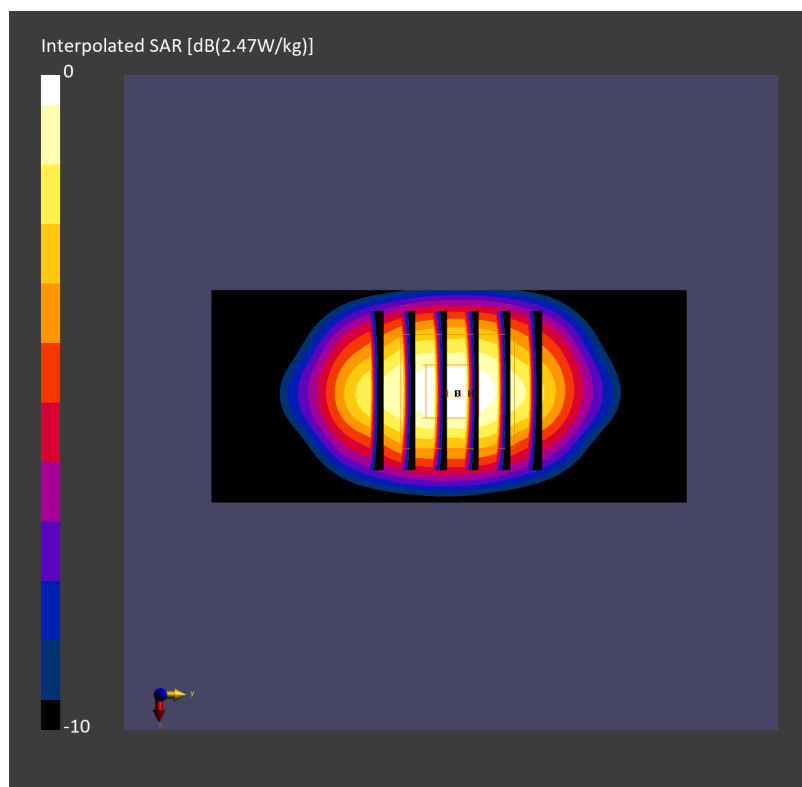

Date: 2025-08-12

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250812 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.969 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.89 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

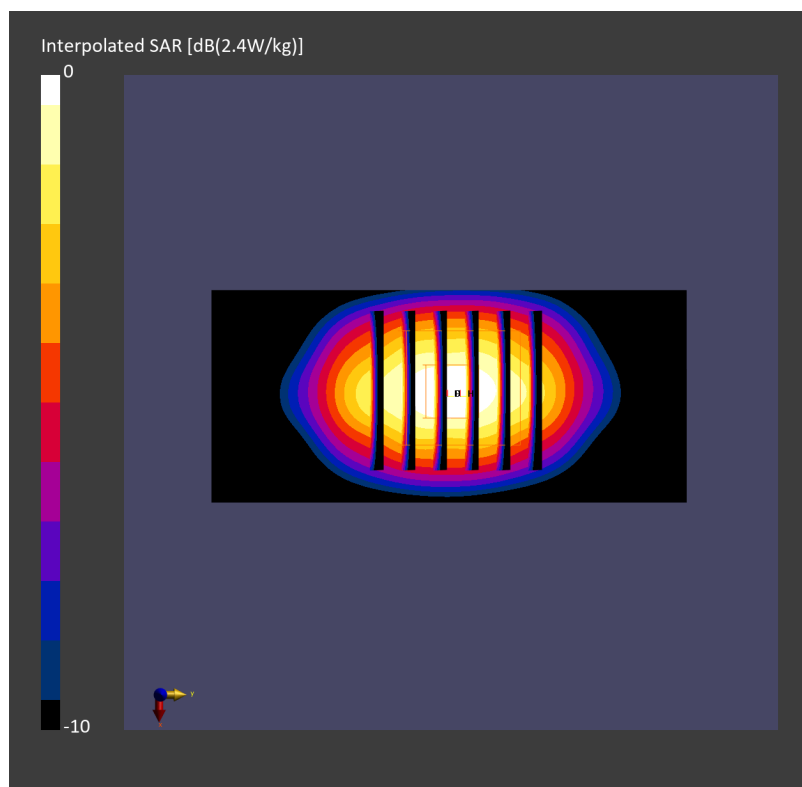

Date: 2025-08-14

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250814 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.985 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.92 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 86.4 %

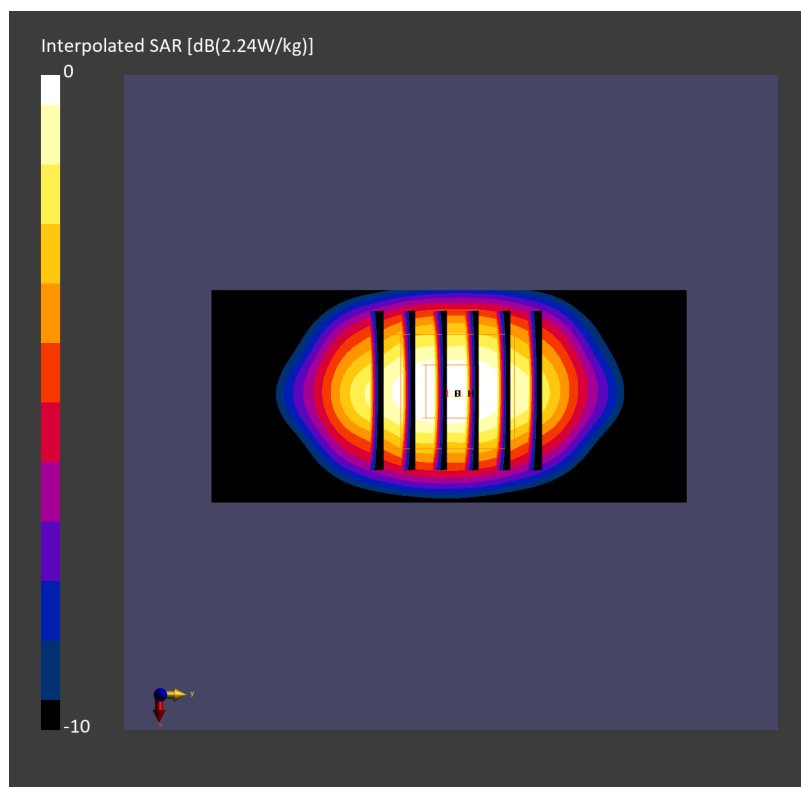

Date: 2025-08-18

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250818 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.00 W/kg; SAR (10g) = 1.03 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.98 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

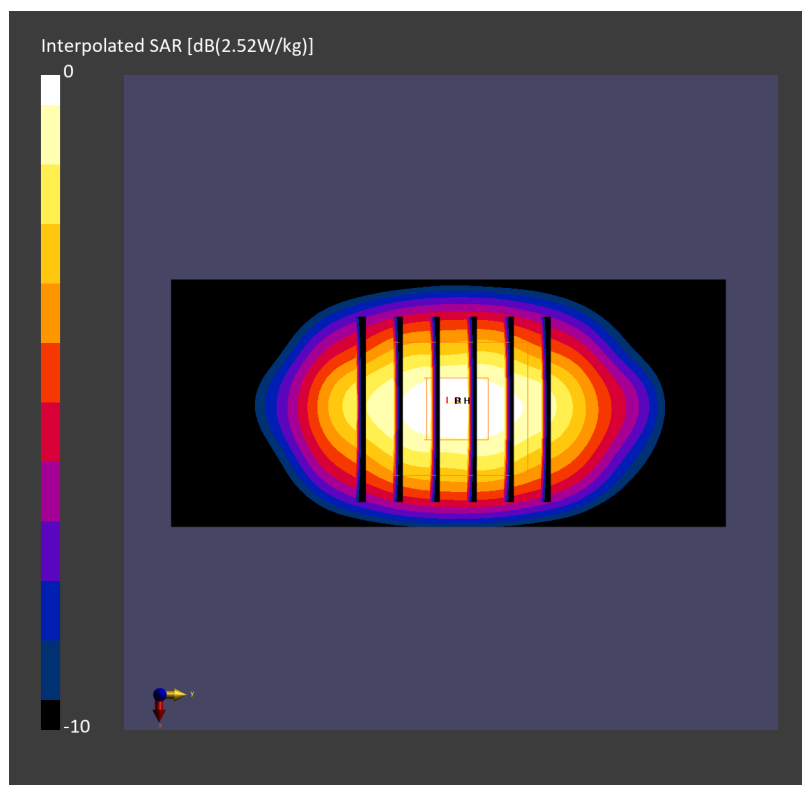

Date: 2025-08-20

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250820 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.04 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.00 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

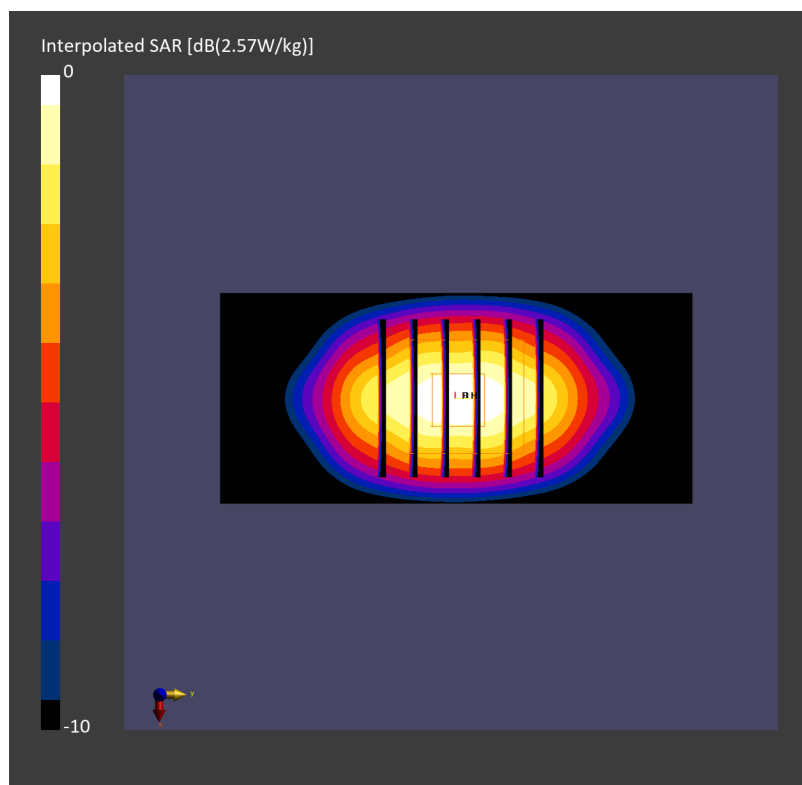

Date: 2025-08-26

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-10000_250826 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.03 W/kg; SAR (8g) = 1.17 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: No correction

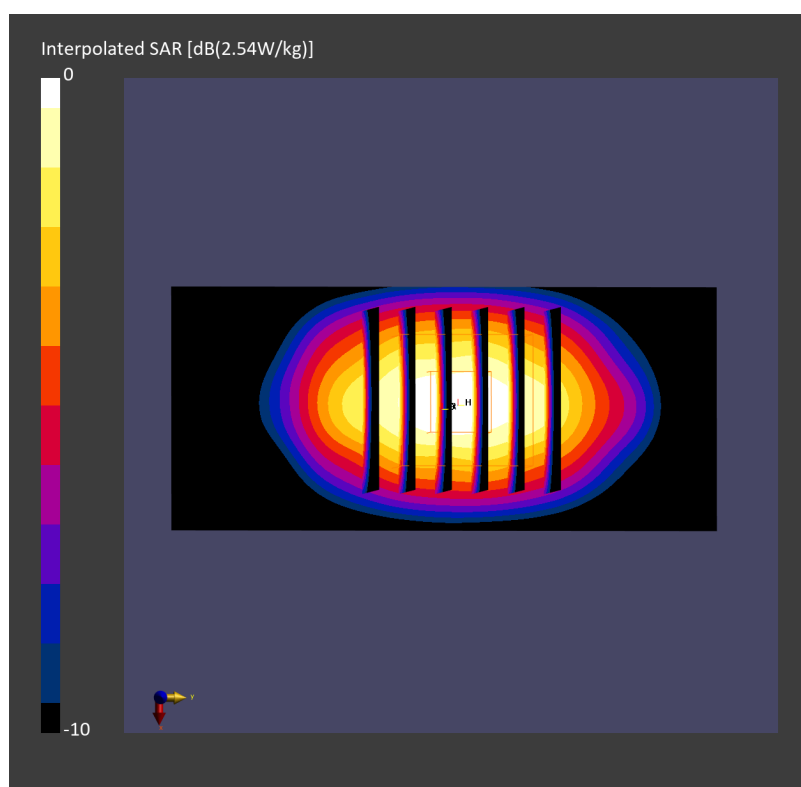

Date: 2025-08-29

System Check_Head_1900MHz**DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_250829 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.06 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.03 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 86.0 %

TSL Correction: No correction

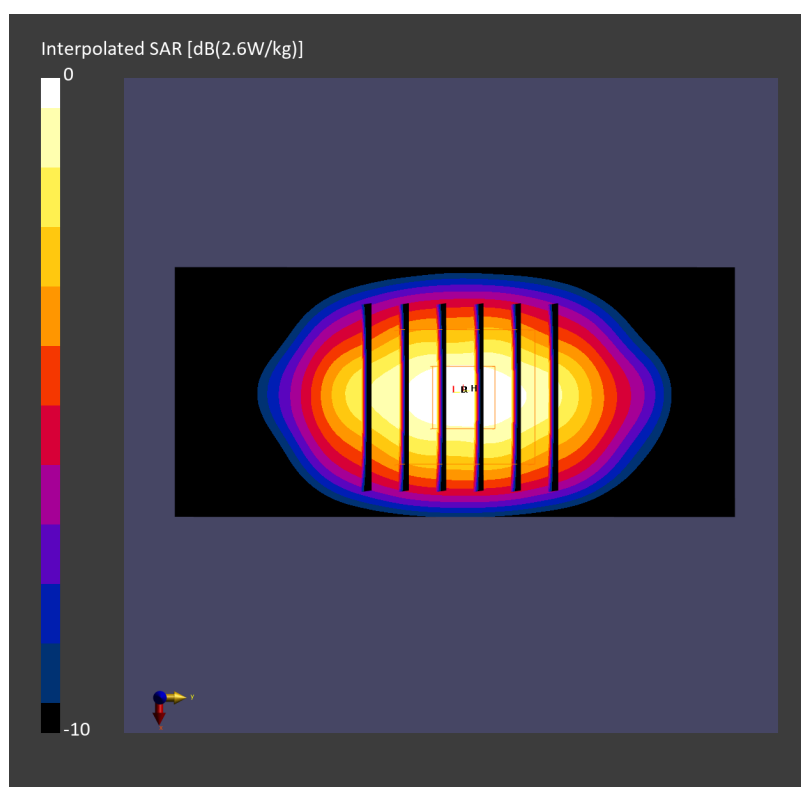

Date: 2025-07-19

System Check_Head_2000MHz**DUT: D2000V2 - SN1070**

Communication System: CW; Frequency: 2000.000 MHz

Medium: HSL_2000_250719 Medium parameters used: $f = 2000.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.21, 6.52, 8.3); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 0.968 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 1.93 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.989 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

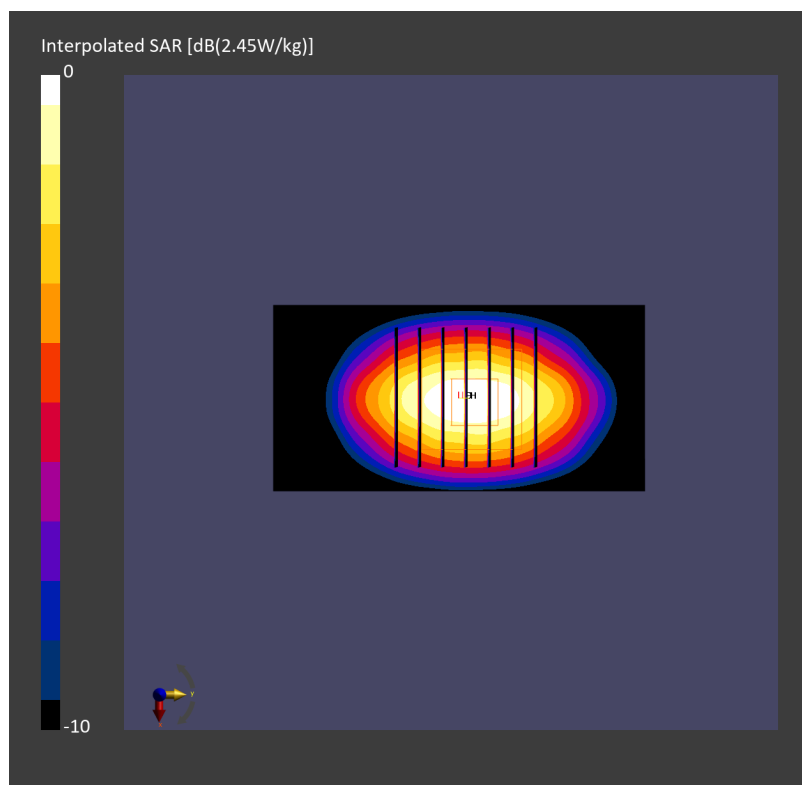

Date: 2025-08-04

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250804 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(7.15, 6.94, 7.32); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.09 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.26 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

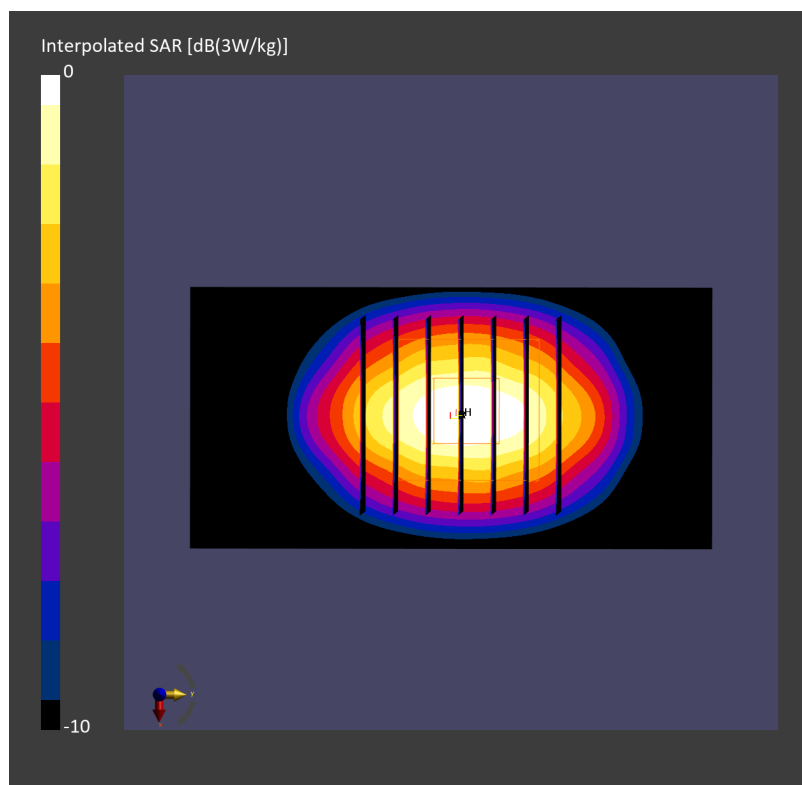

Date: 2025-08-15

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250815 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.95, 6.29, 8.0); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.89 W/kg; SAR (10g) = 1.38 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.12 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.4 %

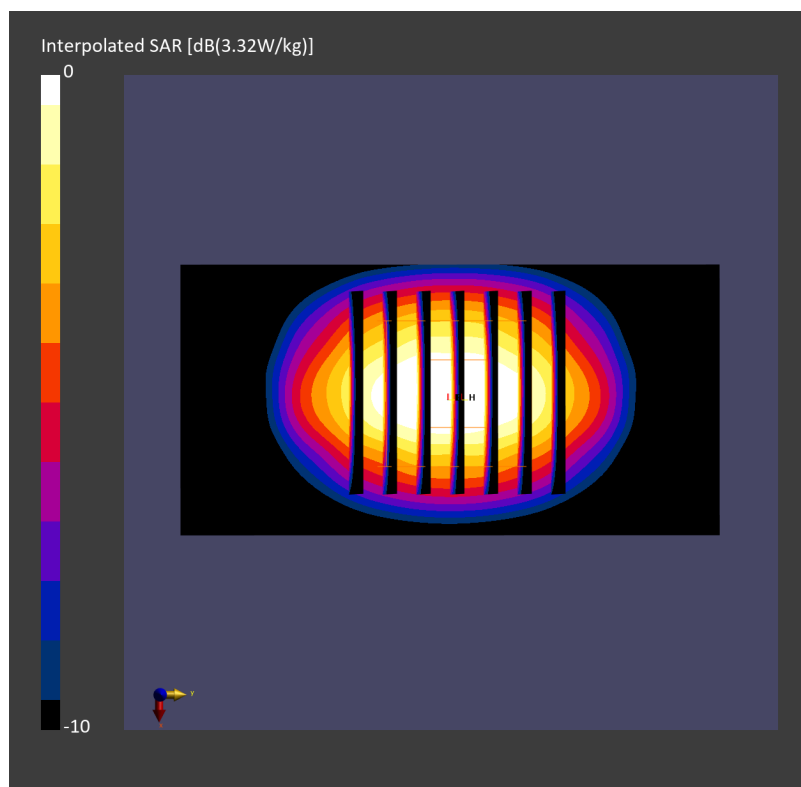

Date: 2025-08-21

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250821 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.78, 7.02, 6.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.35 W/kg; SAR (10g) = 1.11 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.34 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.3 %

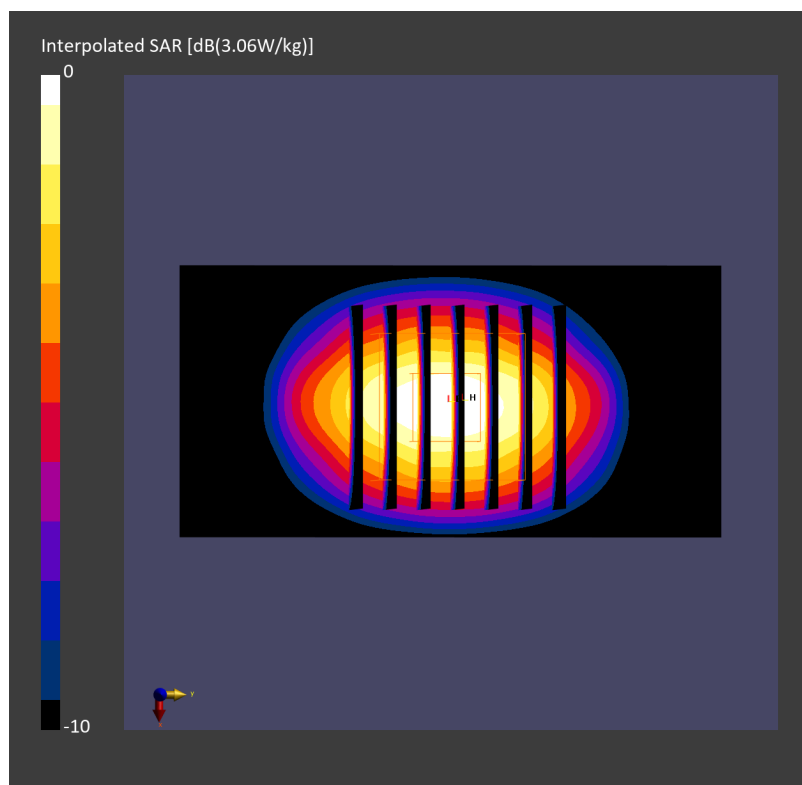

Date: 2025-08-26

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_250826 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.78, 7.02, 6.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 2.41 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

TSL Correction: No correction

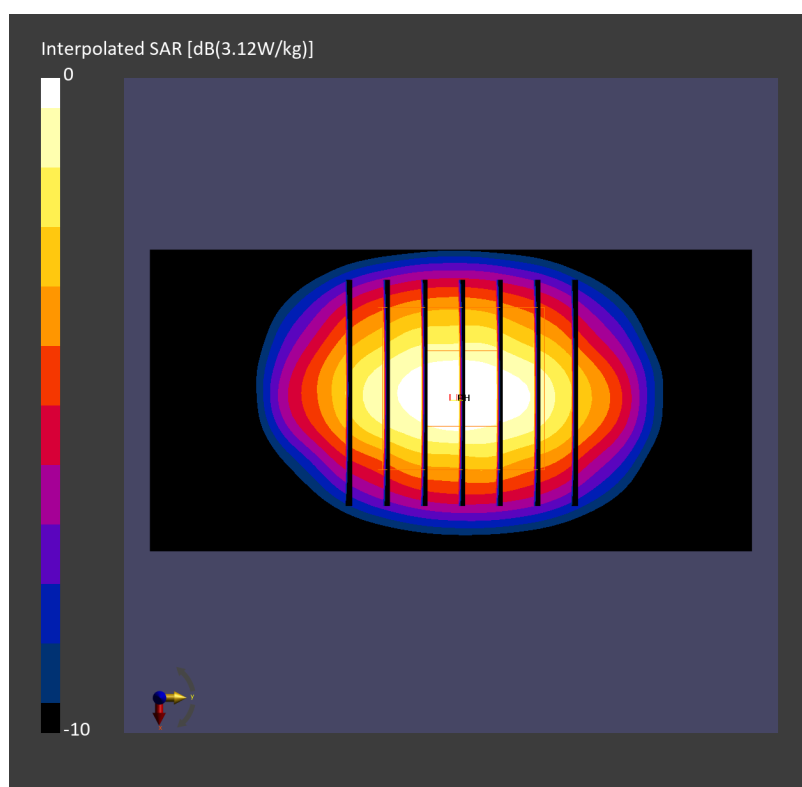

Date: 2025-08-18

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250818 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.02, 7.24, 7.0); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.66 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

TSL Correction: No correction

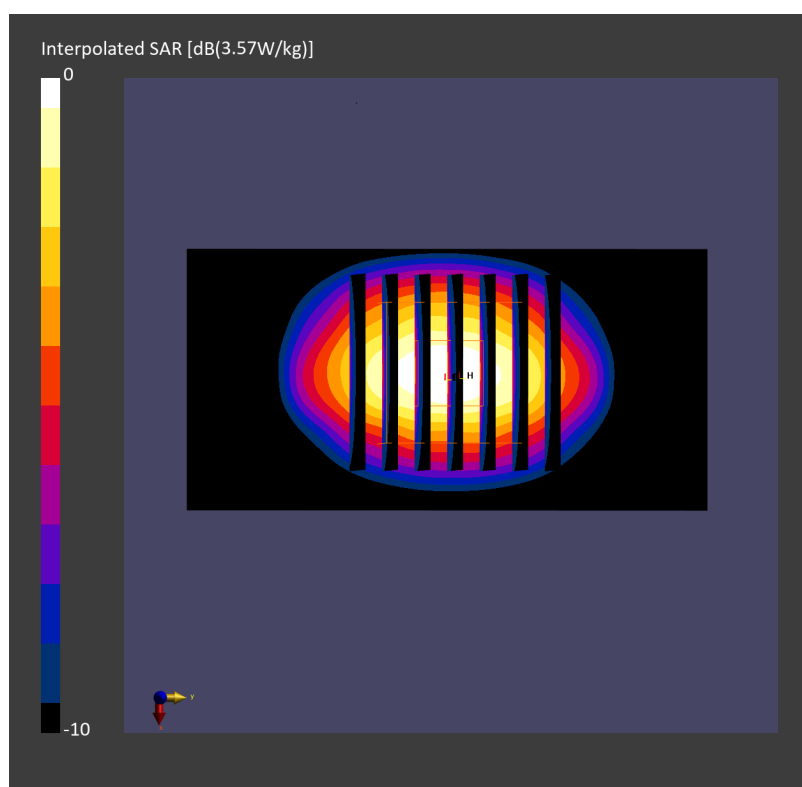

Date: 2025-08-24

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250824 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.02, 7.24, 7.0); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.69 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.2 %

TSL Correction: No correction

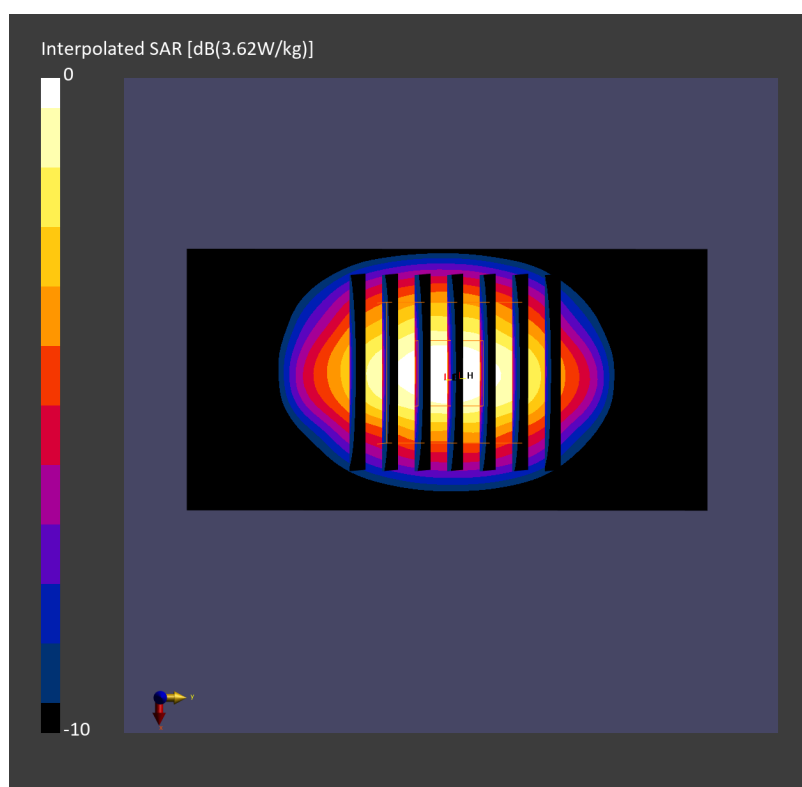

Date: 2025-08-25

System Check_Head_2450MHz**DUT: D2450V2 - SN806**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_250825 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.02, 7.24, 7.0); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.74 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.70 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

TSL Correction: No correction

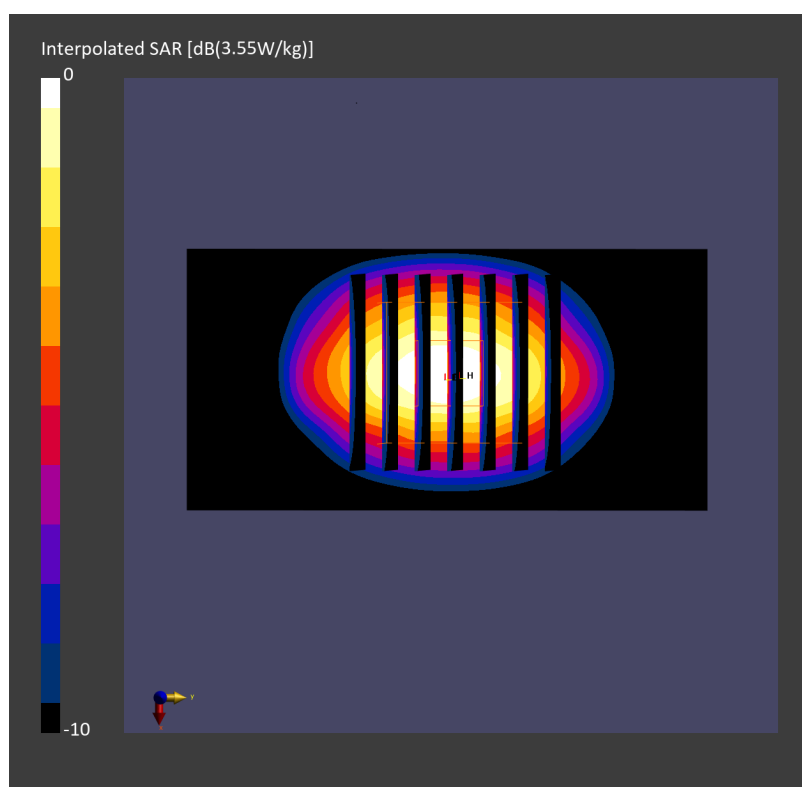

Date: 2025-08-01

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250801 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.86, 6.65, 7.02); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.75 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.68 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

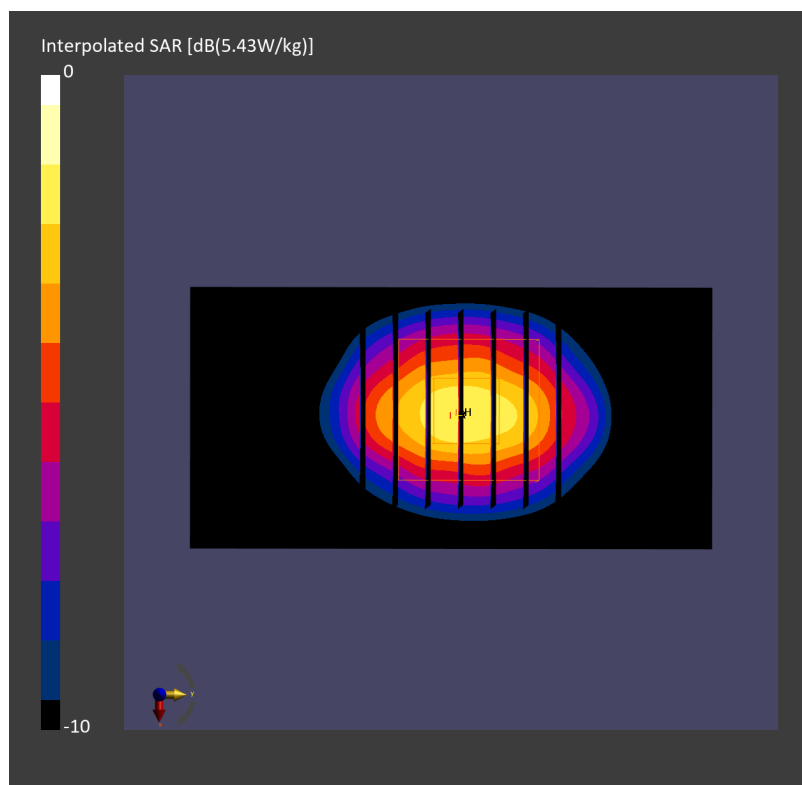

Date: 2025-08-02

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250802 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.86, 6.65, 7.02); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.70 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

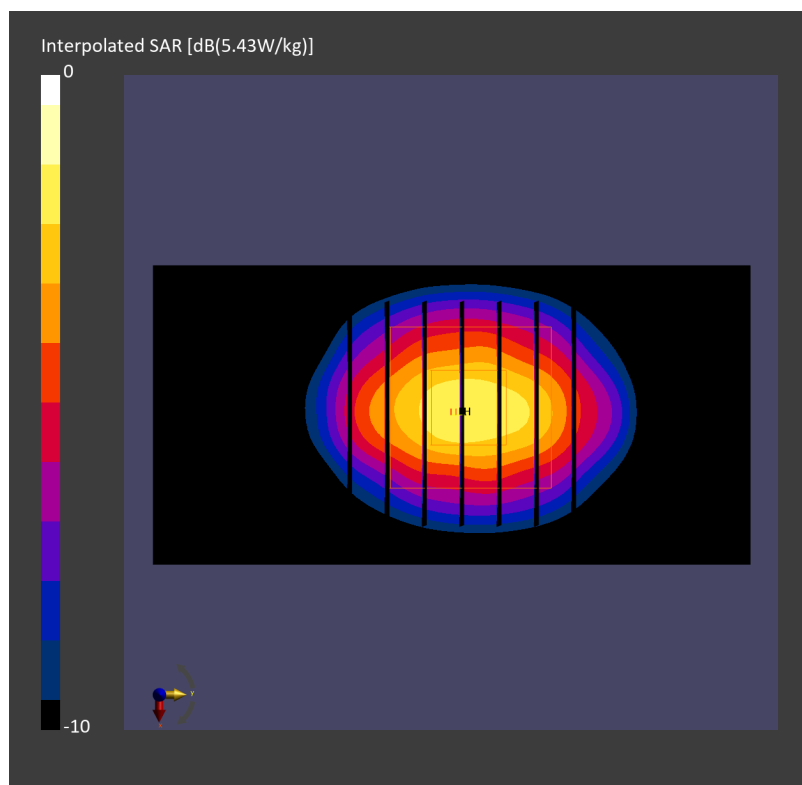

Date: 2025-08-03

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250803 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.86, 6.65, 7.02); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.78 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.73 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

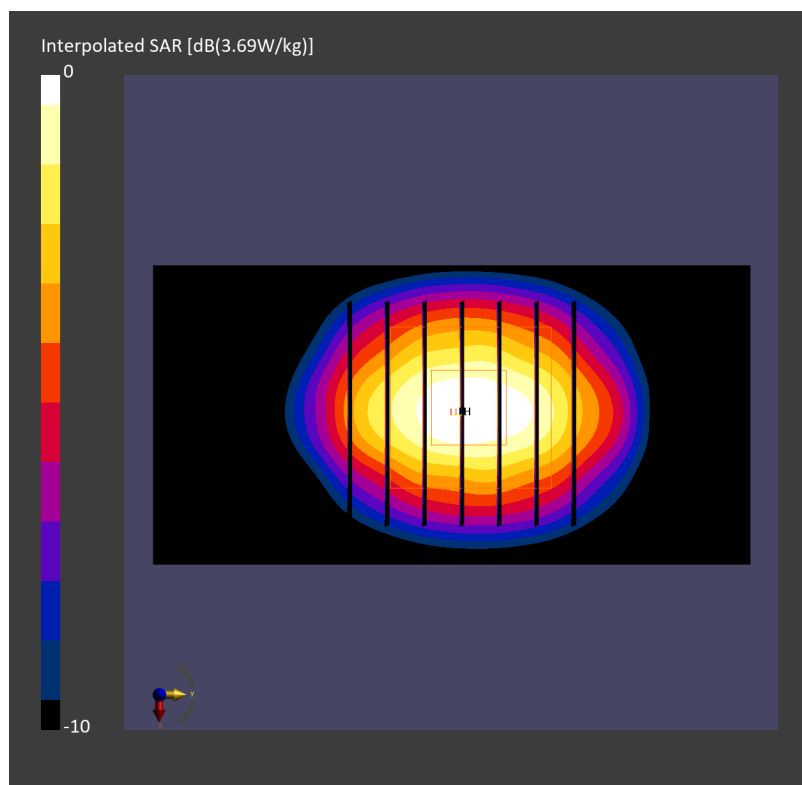

Date: 2025-08-16

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250816 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.21 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 2.64 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

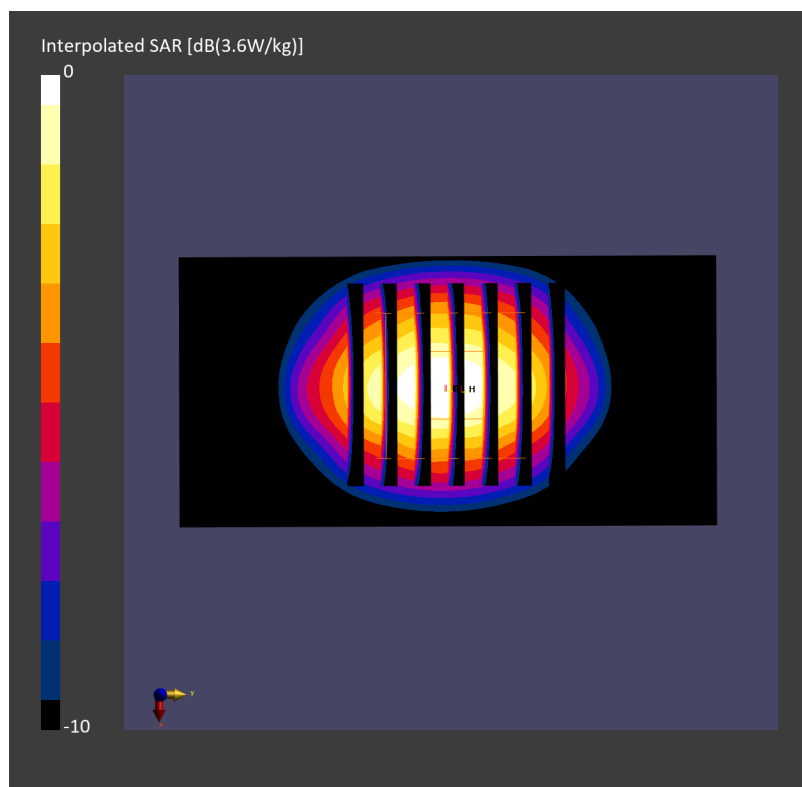

Date: 2025-08-17

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250817 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.21 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.3 %

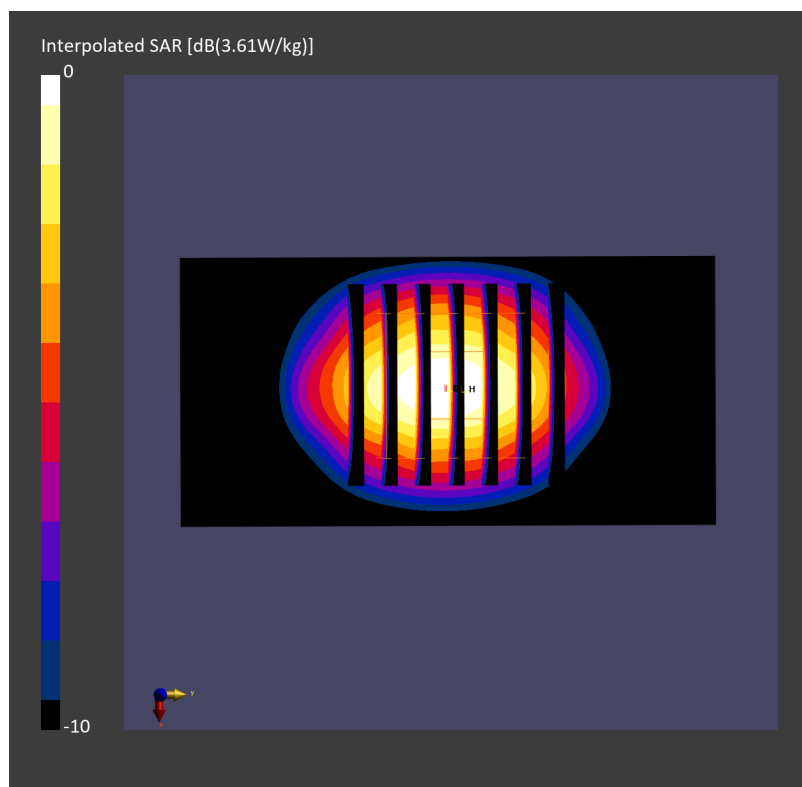

Date: 2025-08-18

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250818 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.66 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

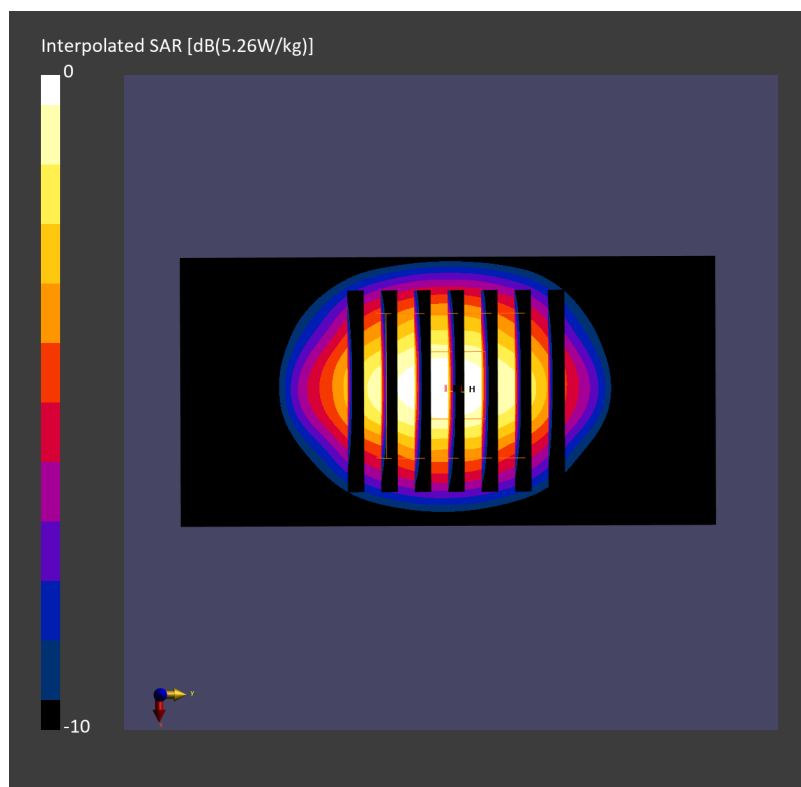

Date: 2025-08-19

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250819 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.76 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

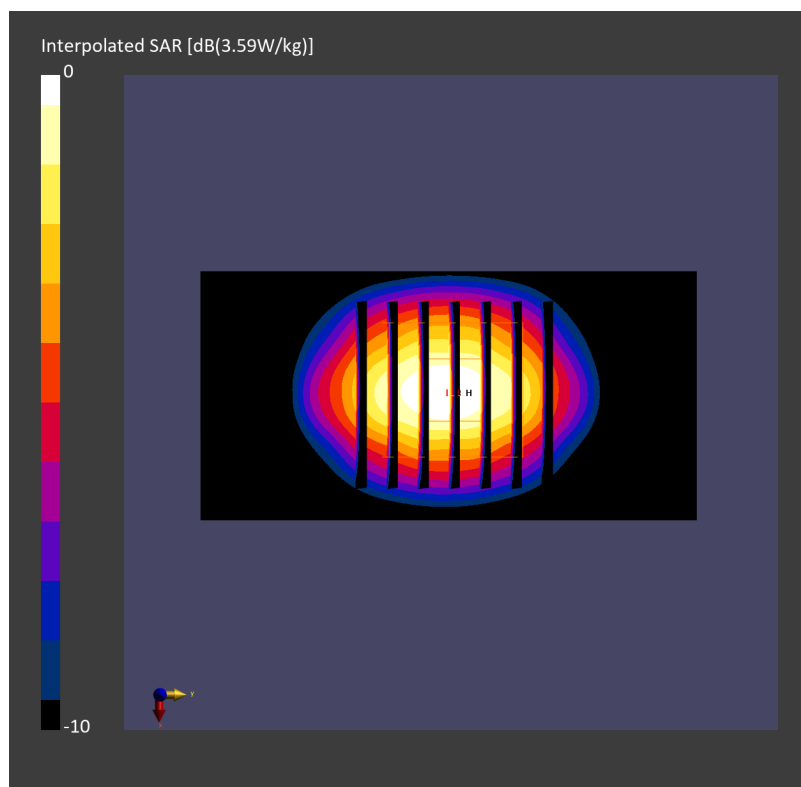

Date: 2025-08-20

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250820 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.04$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

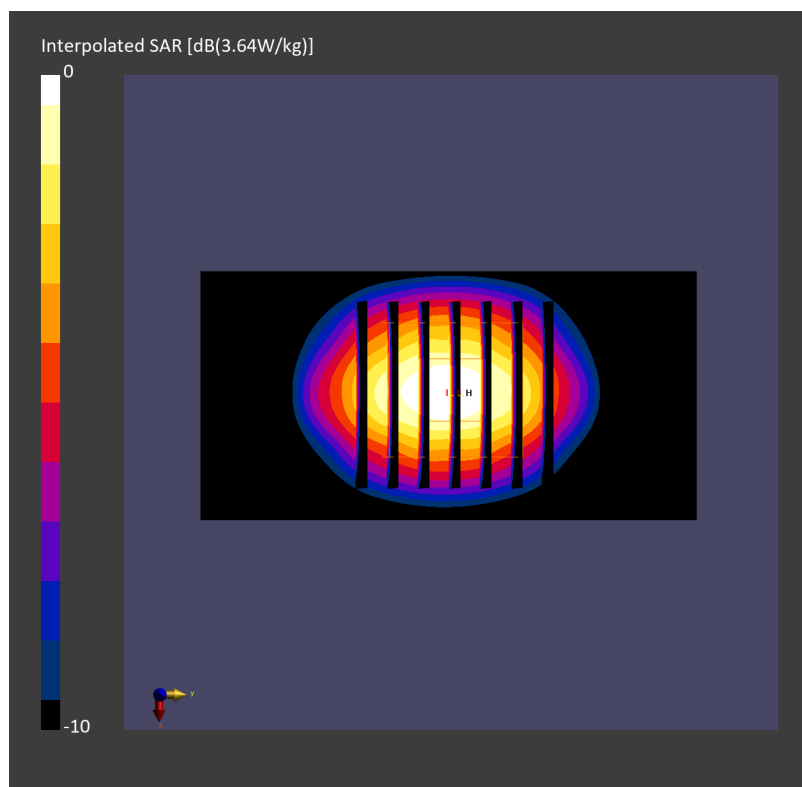

Date: 2025-08-21

System Check_Head_2600MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250821 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 2.69 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

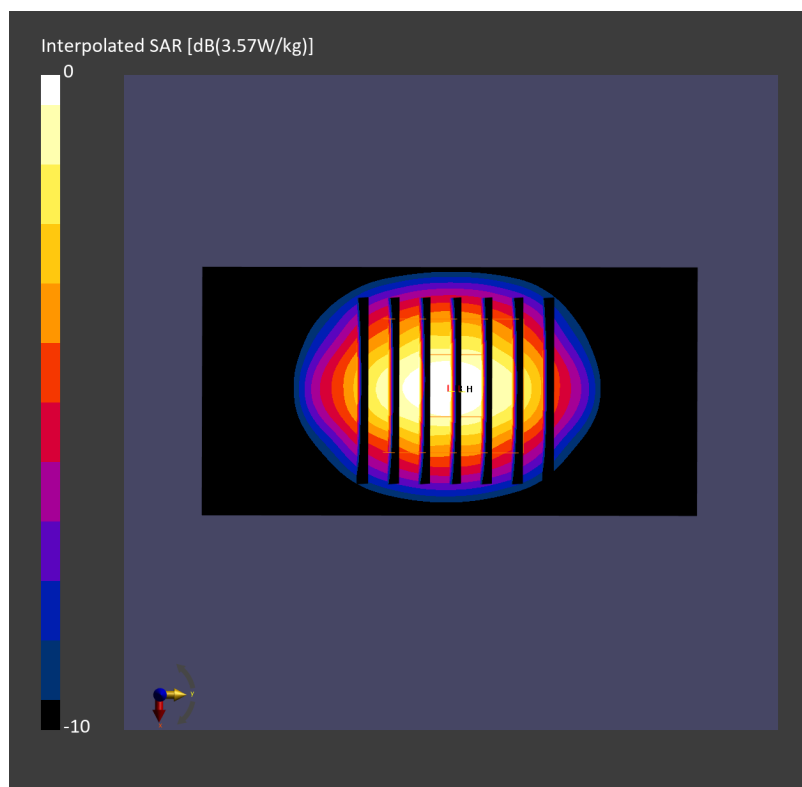

Date: 2025-08-21

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250821 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.78 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.83 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

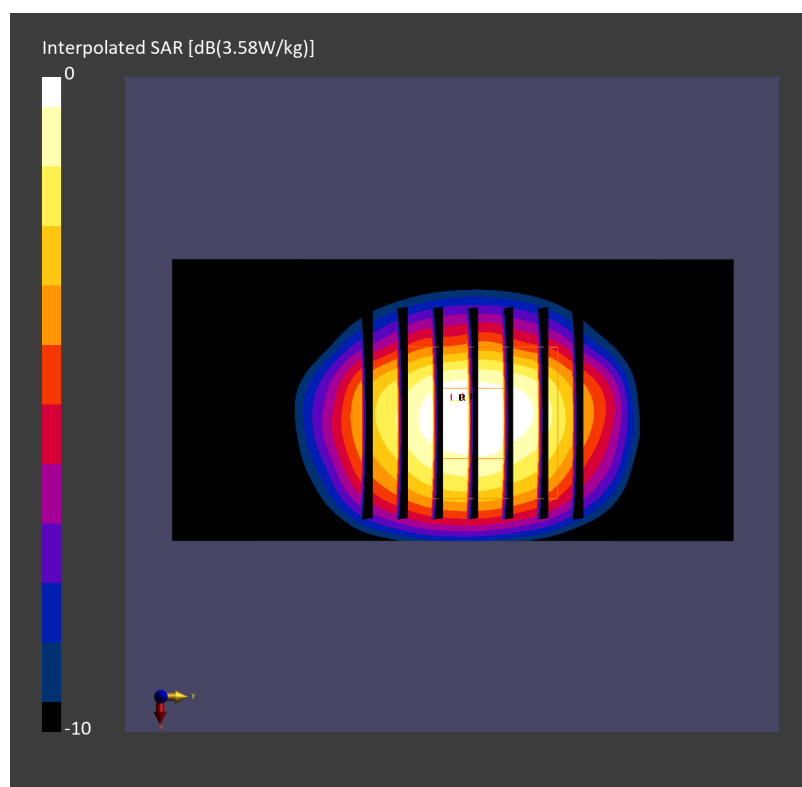

Date: 2025-08-25

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250825 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.92 W/kg; SAR (10g) = 1.31 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.91 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

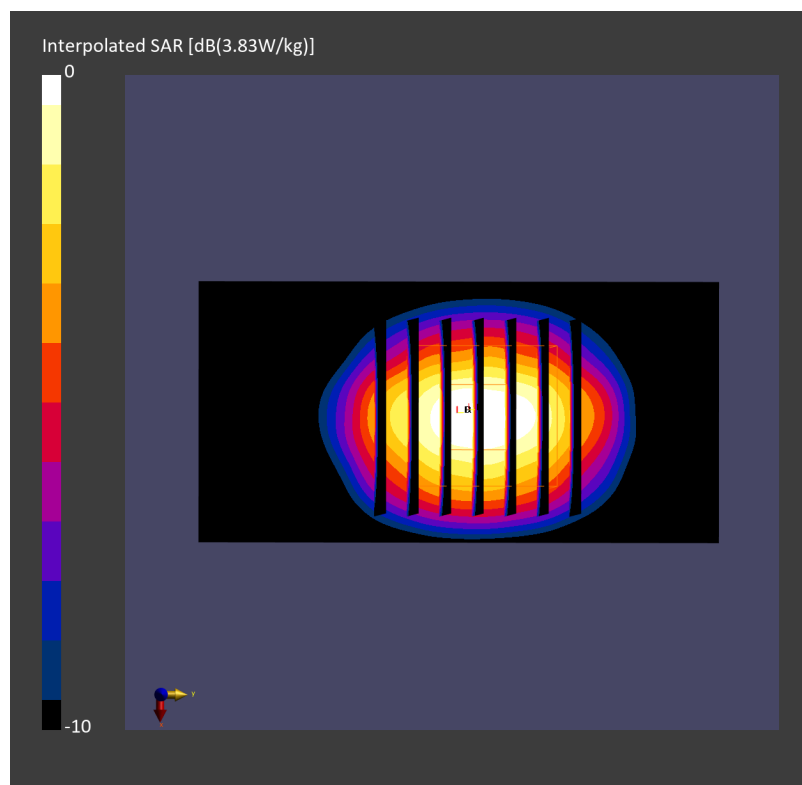

Date: 2025-08-26

System Check_Head_2300MHz**DUT: D2600V2 - SN1089**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_250826 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.82 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.84 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

TSL Correction: No correction

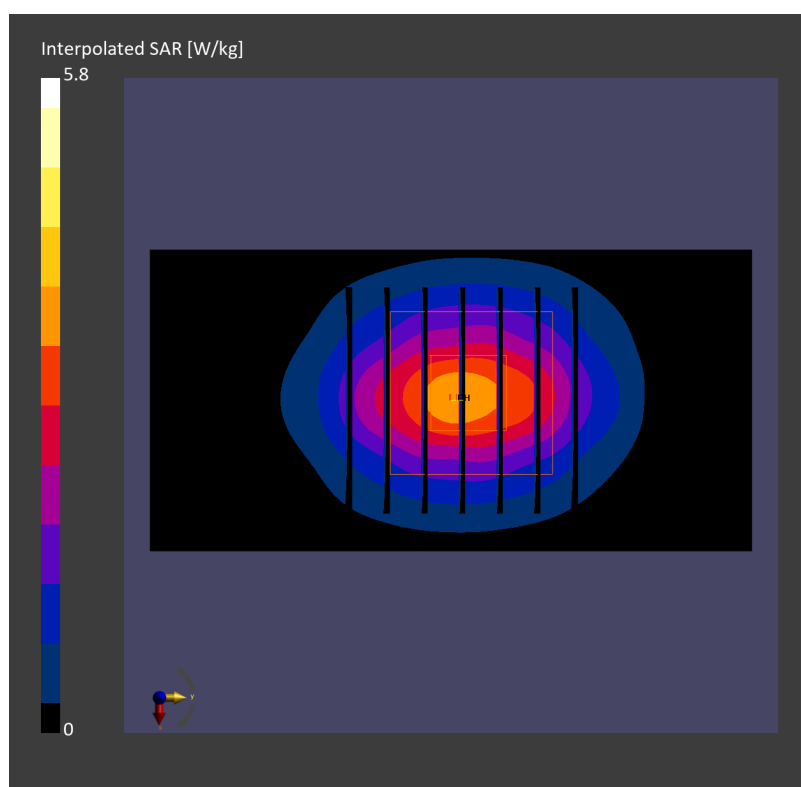

Date: 2025-08-14

System Check_Head_3300MHz**DUT: D3300V2 - SN1005**

Communication System: CW; Frequency: 3300.000 MHz

Medium: HSL_3300_250814 Medium parameters used: $f = 3300.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.48, 6.29, 6.63); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.32 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.38 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.9 %

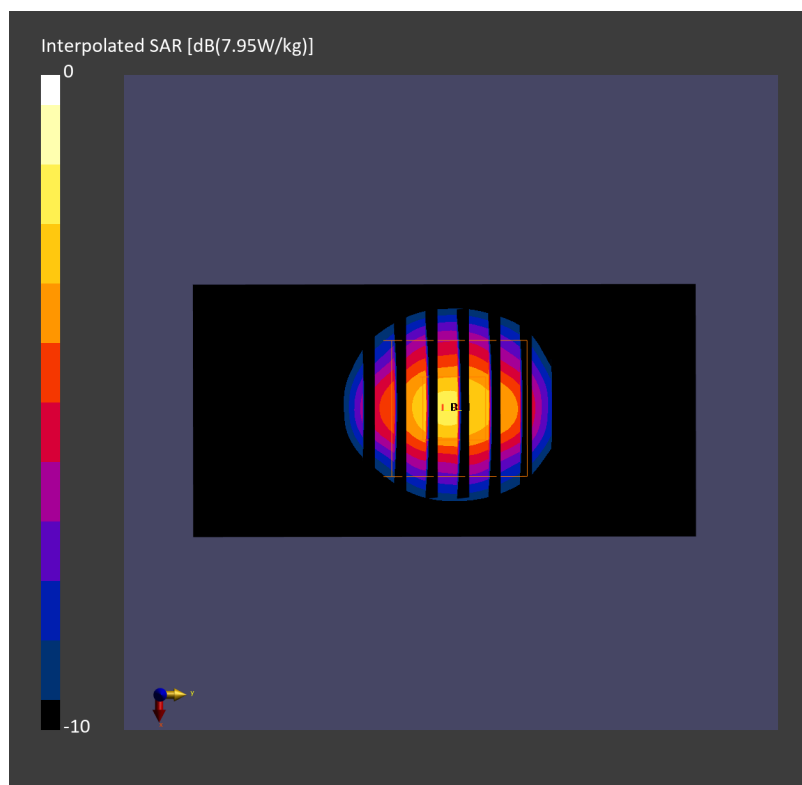

Date: 2025-08-15

System Check_Head_3300MHz**DUT: D3300V2 - SN1005**

Communication System: CW; Frequency: 3300.000 MHz

Medium: HSL_3300_250815 Medium parameters used: $f = 3300.000$ MHz; $\sigma = 2.70$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.48, 6.29, 6.63); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.32 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.7 %

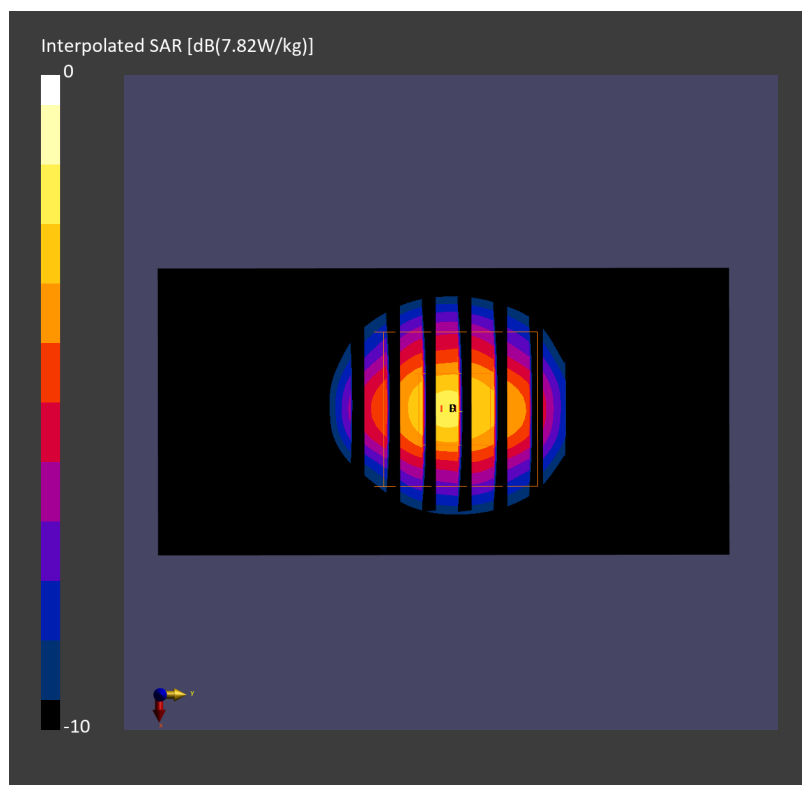

Date: 2025-08-16

System Check_Head_3300MHz**DUT: D3300V2 - SN1005**

Communication System: CW; Frequency: 3300.000 MHz

Medium: HSL_3300_250816 Medium parameters used: $f = 3300.000$ MHz; $\sigma = 2.68$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.48, 6.29, 6.63); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.2 %

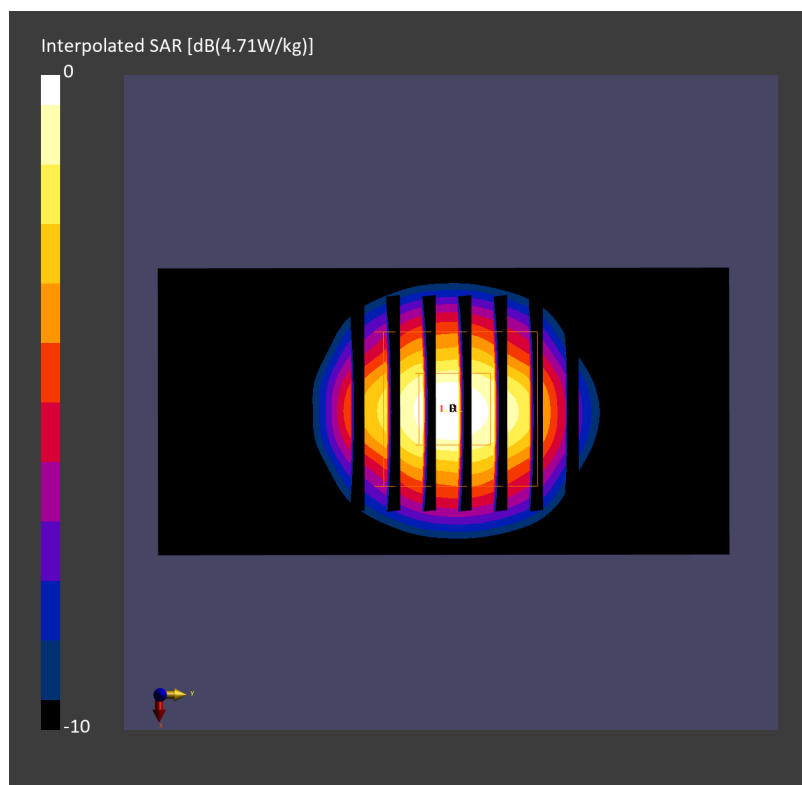

Date: 2025-08-17

System Check_Head_3300MHz**DUT: D3300V2 - SN1005**

Communication System: CW; Frequency: 3300.000 MHz

Medium: HSL_3300_250817 Medium parameters used: $f = 3300.000$ MHz; $\sigma = 2.66$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.48, 6.29, 6.63); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.2 %

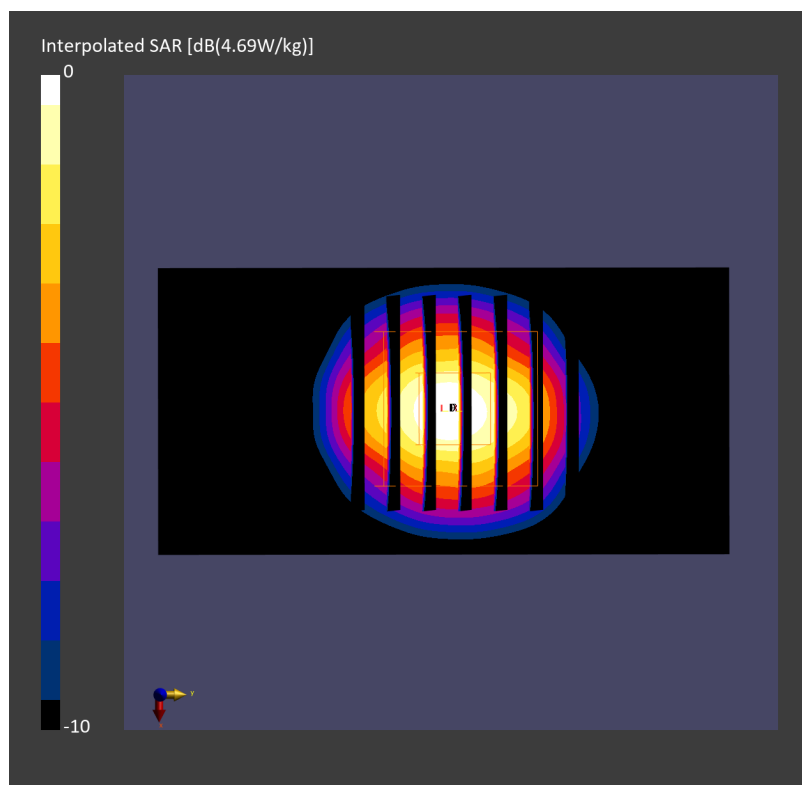

Date: 2025-07-22

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250722 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.25 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

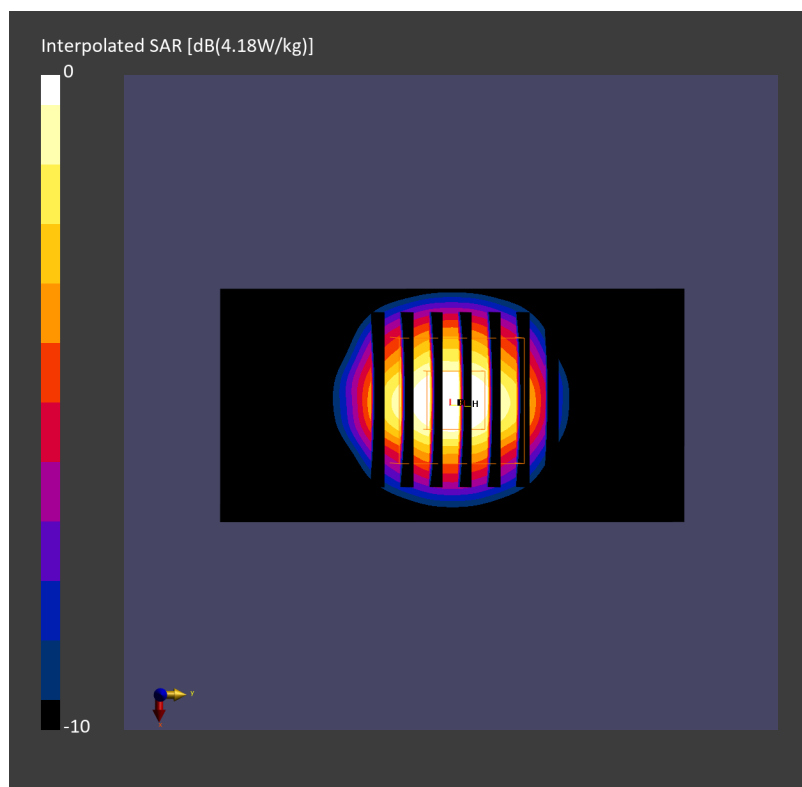

Date: 2025-07-23

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250723 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.26 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.0 %

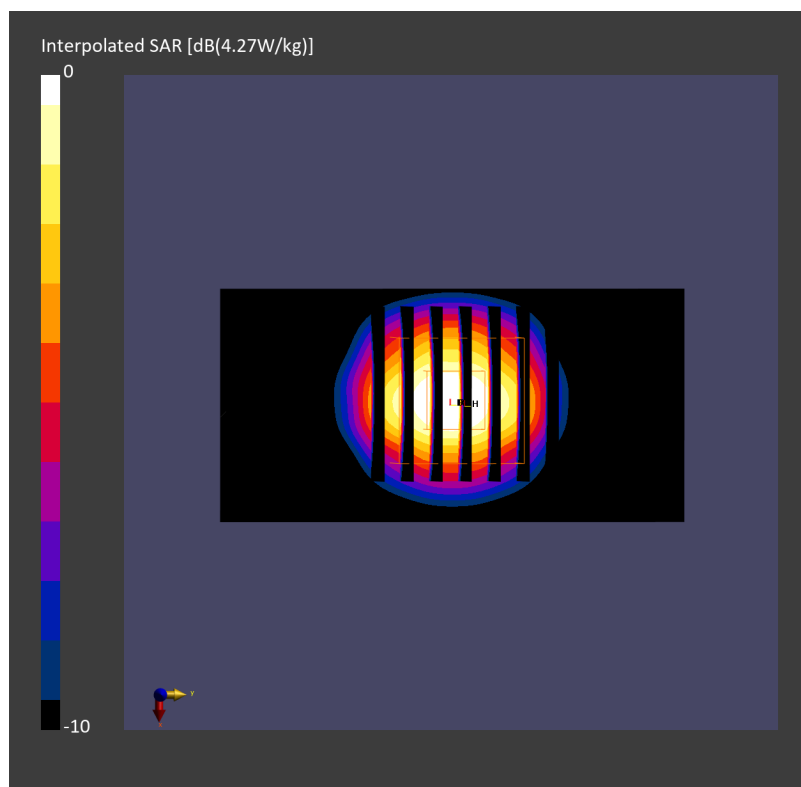

Date: 2025-07-24

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250724 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.25 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.31 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

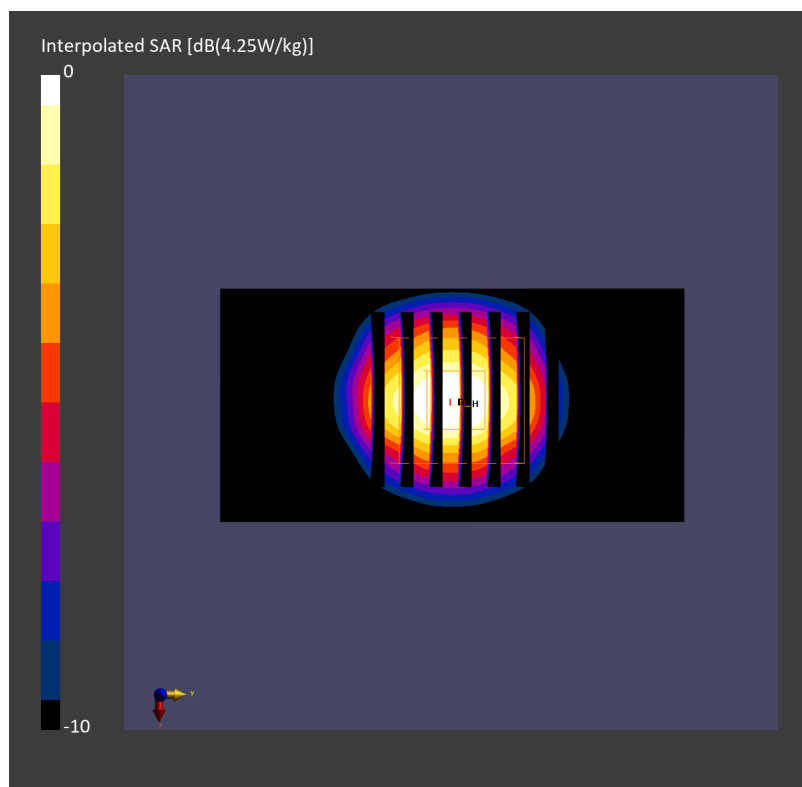

Date: 2025-07-25

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250725 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.93$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.8 %

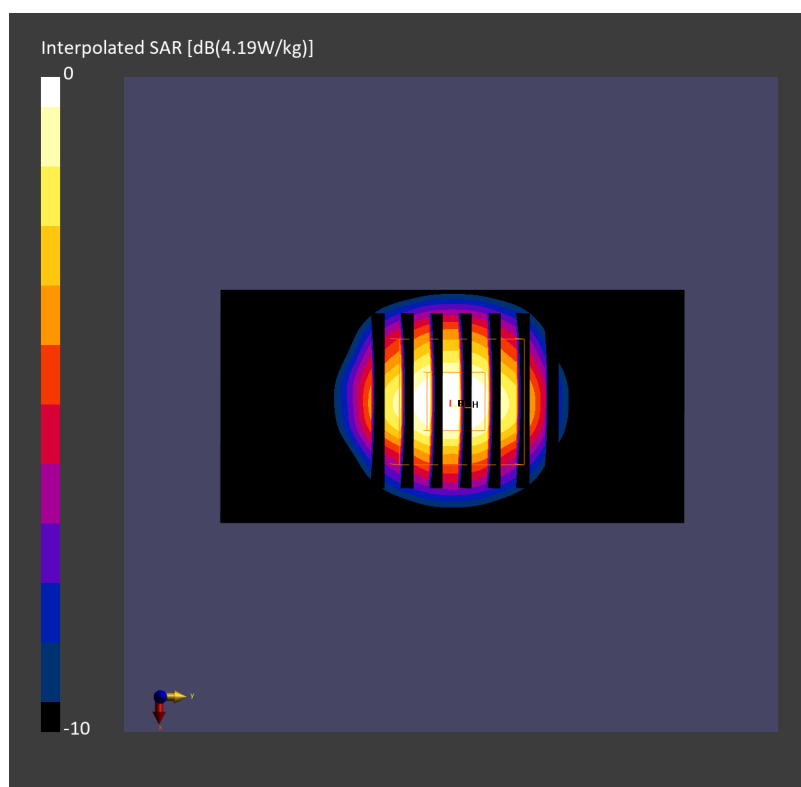

Date: 2025-07-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250727 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.25 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

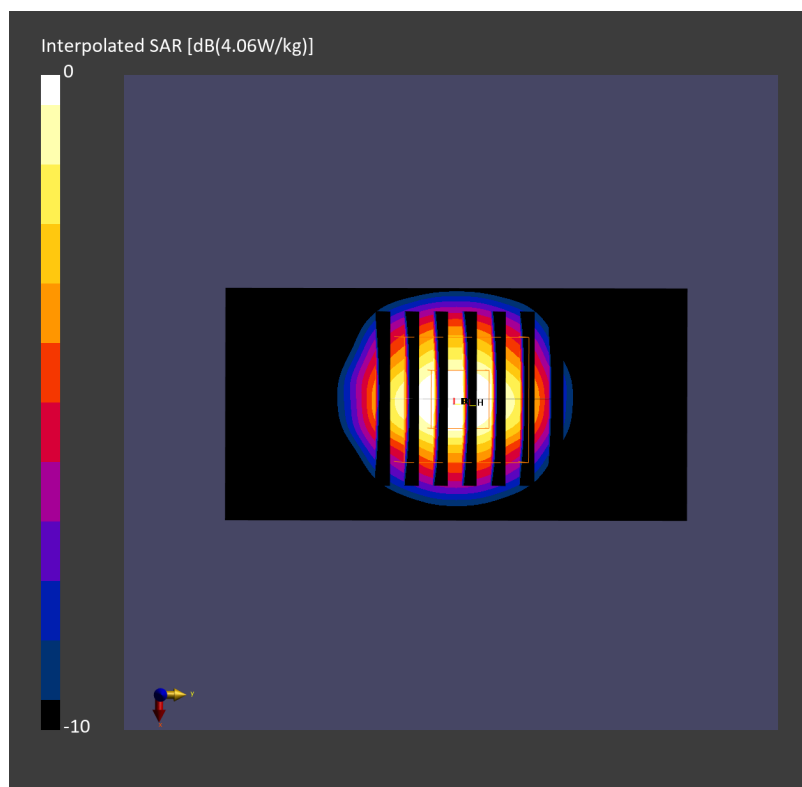

Date: 2025-07-28

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250728 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

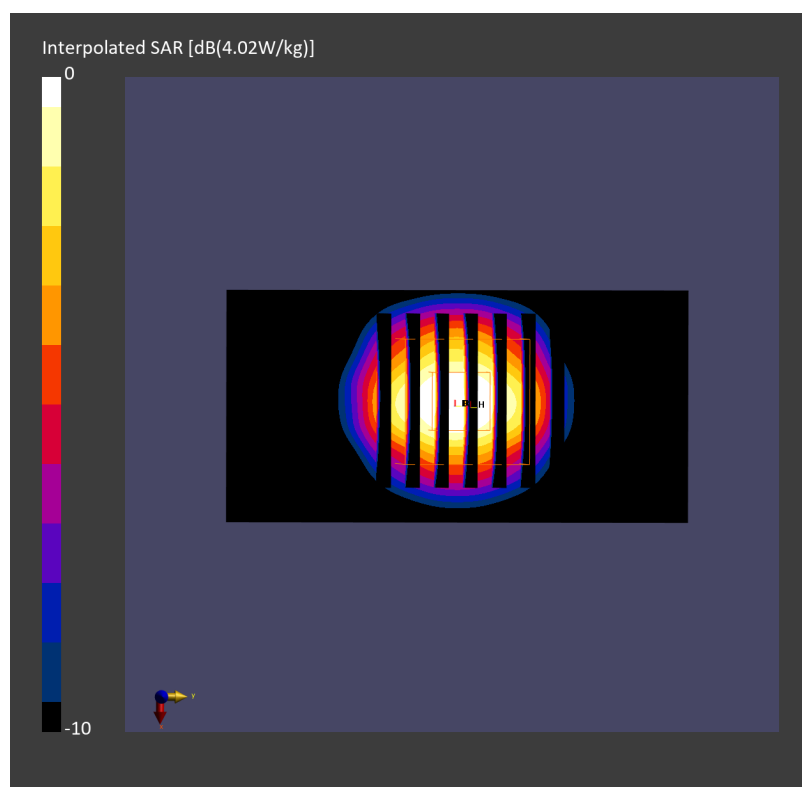

Date: 2025-07-30

System Check_Head_3500MHz_250730.d6sar**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250730 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.36 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

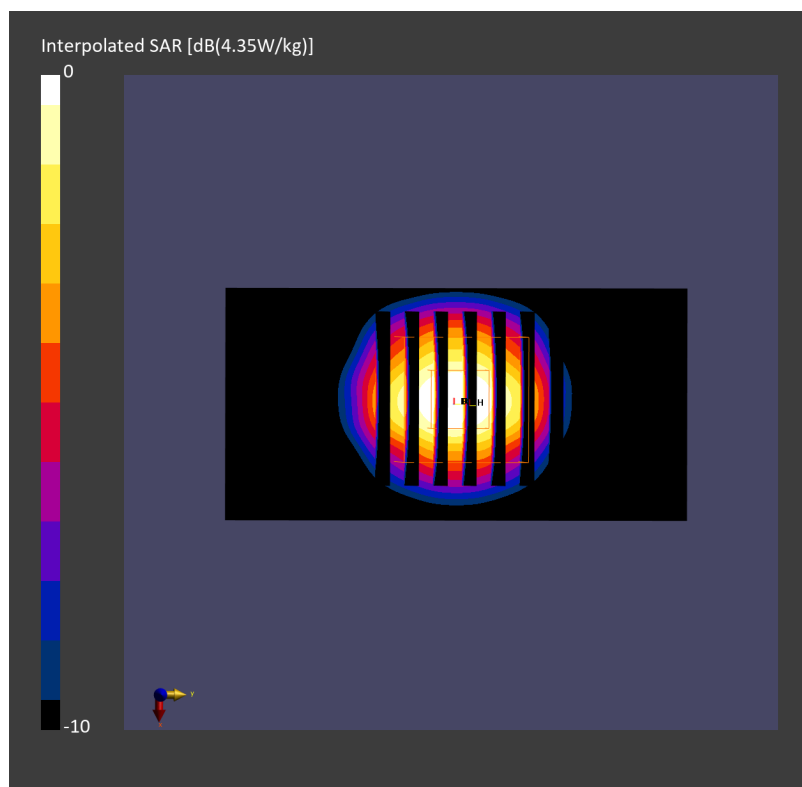

Date: 2025-07-31

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250731 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.9 %

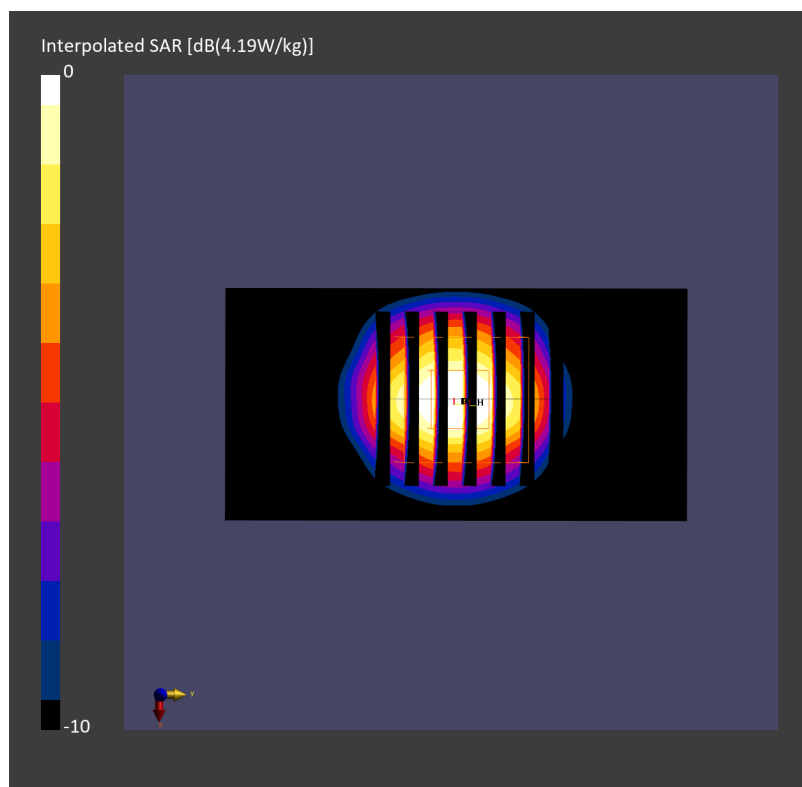

Date: 2025-08-13

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250813 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.39 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.0 %

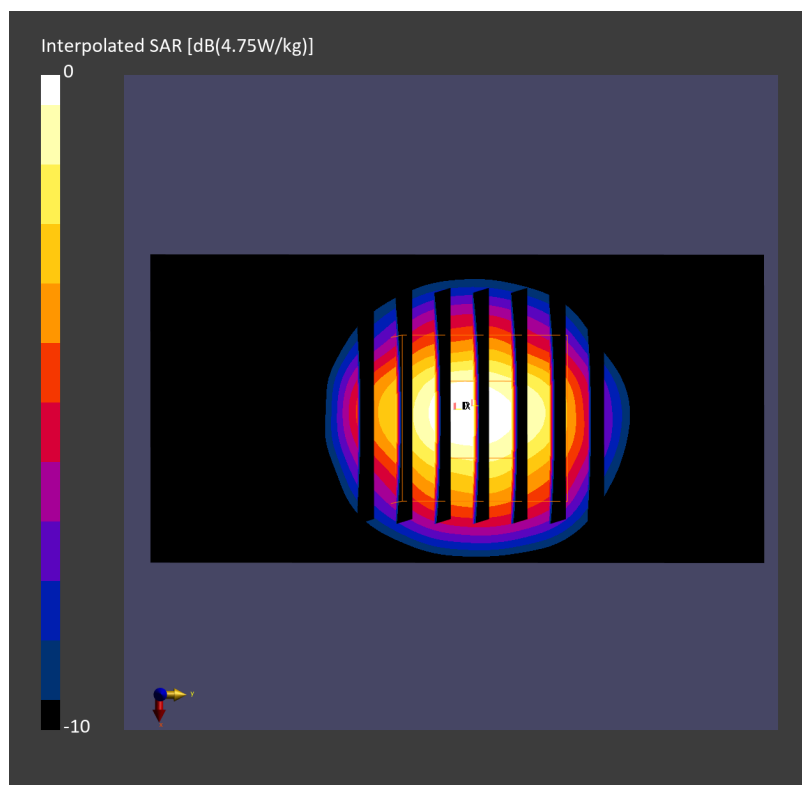

Date: 2025-08-14

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250814 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.93$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.51 W/kg; SAR (10g) = 1.34 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.52 W/kg; SAR (8g) = 1.52 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 78.0 %

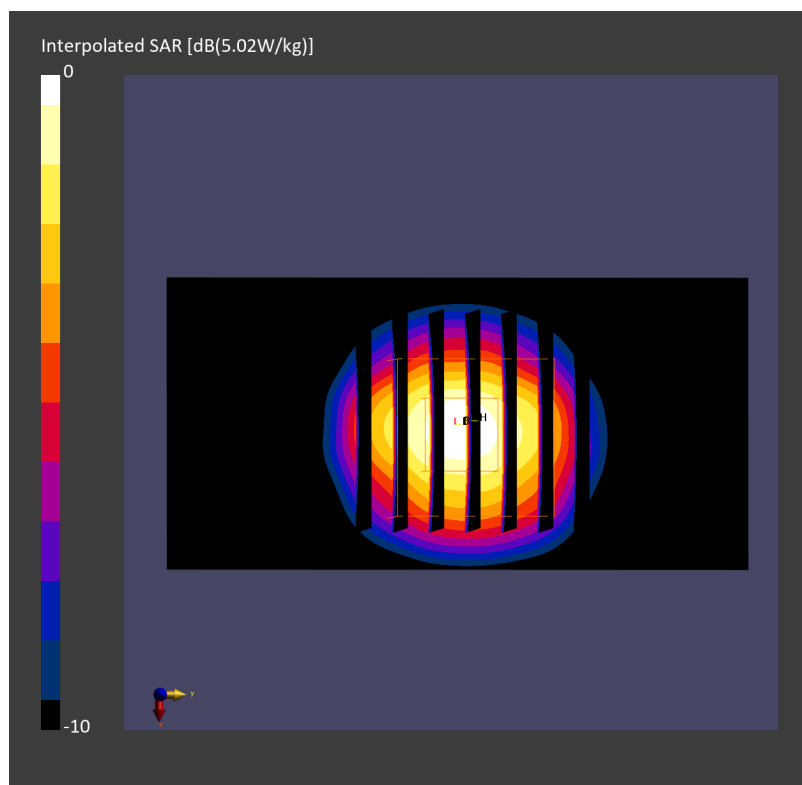

Date: 2025-08-15

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250815 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.38 W/kg; SAR (10g) = 1.29 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.43 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.32 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 78.1 %

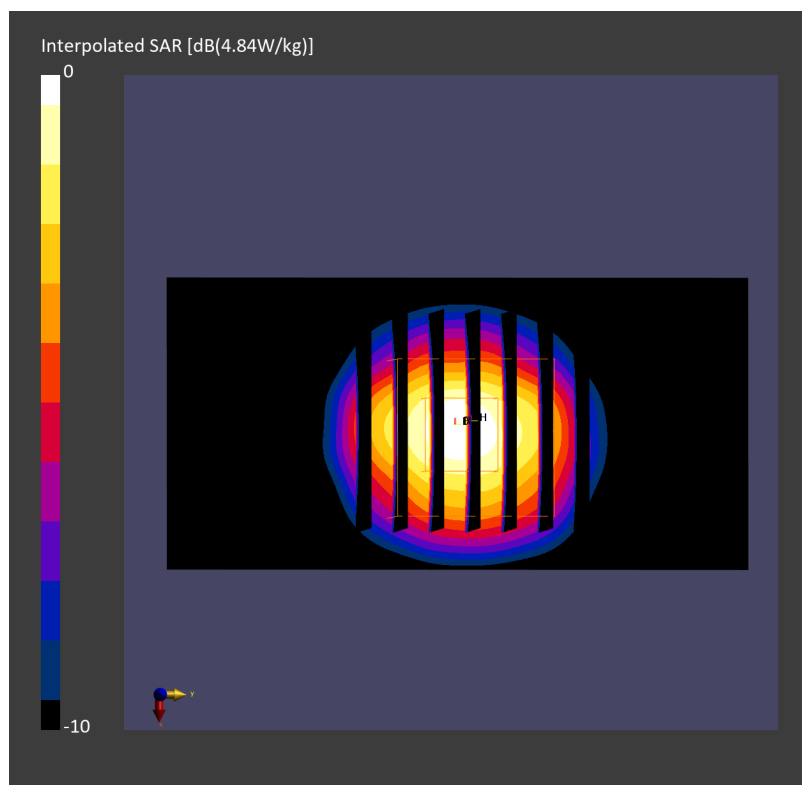

Date: 2025-08-16

System Check_Head_3500MH**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250816 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 78.2 %

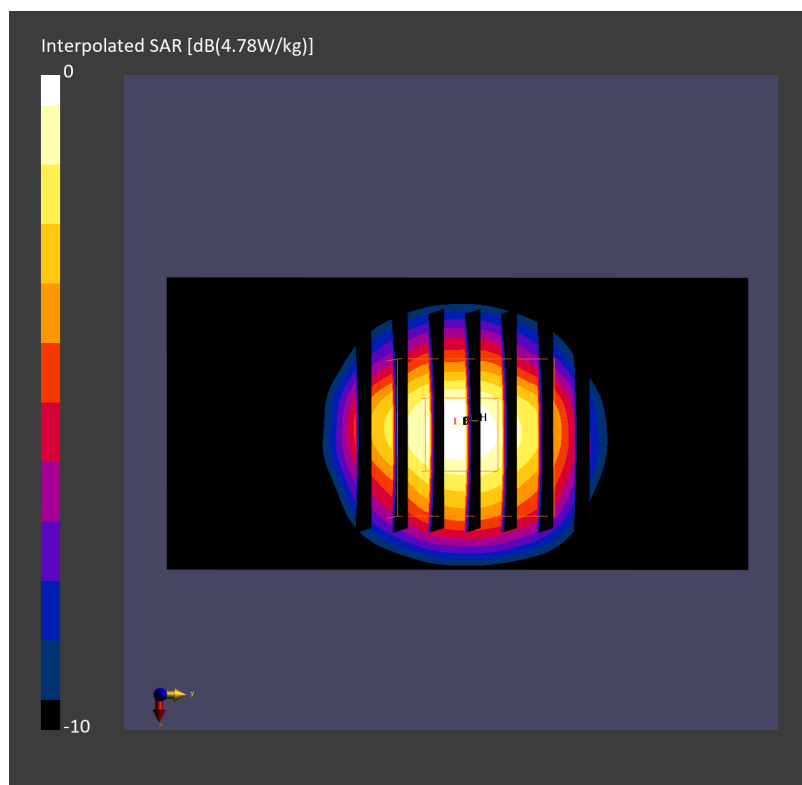

Date: 2025-08-17

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250817 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.37 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 78.2 %

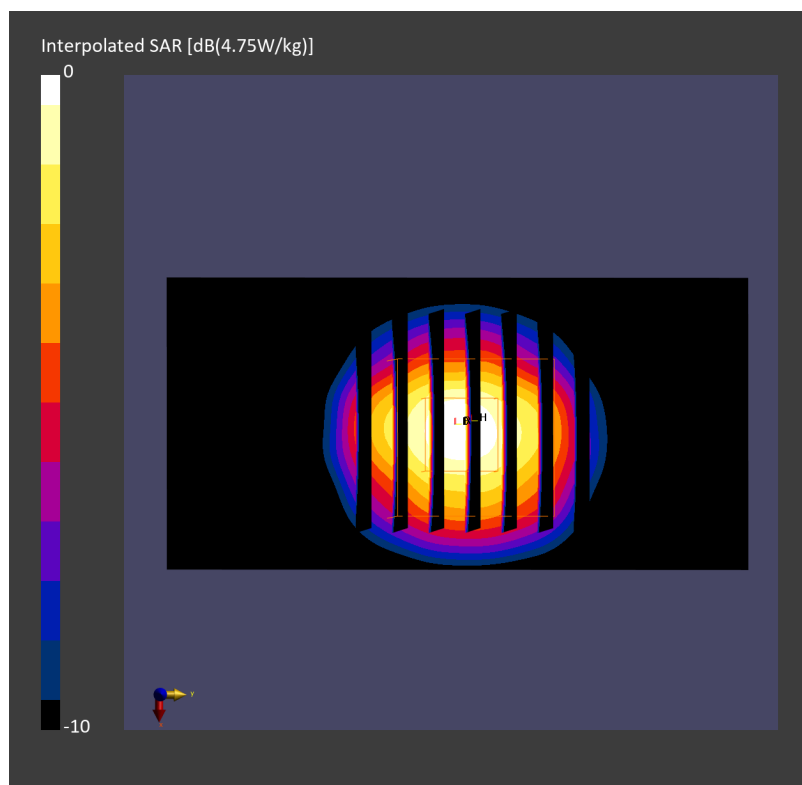

Date: 2025-08-22

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250822 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.85$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.44 W/kg; SAR (10g) = 1.30 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.51 W/kg; SAR (10g) = 1.34 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.8 %

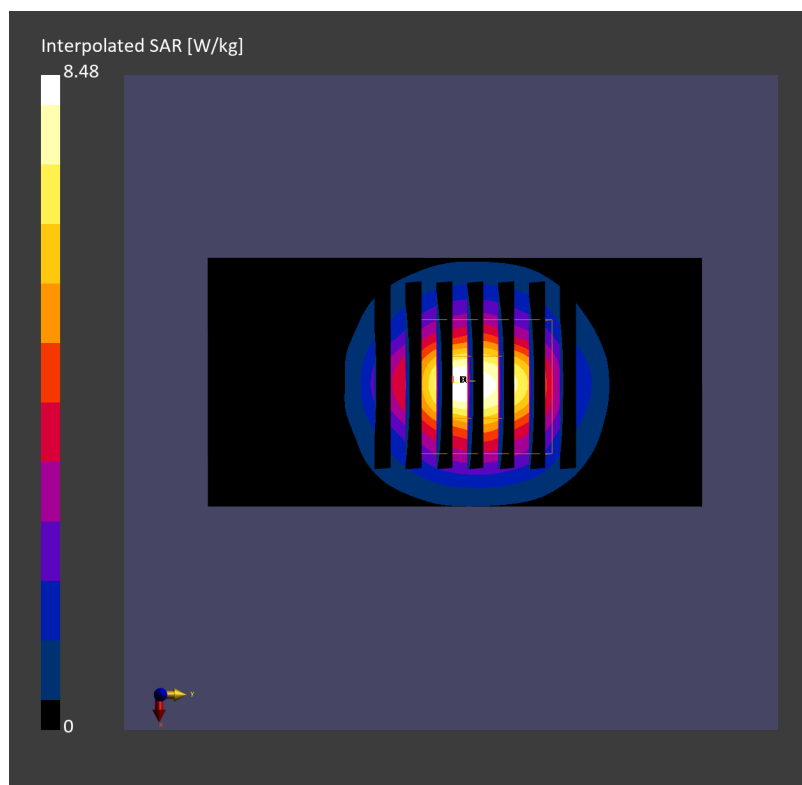

Date: 2025-08-24

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_250824 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.44 W/kg; SAR (10g) = 1.31 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.50 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.36 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.7 %

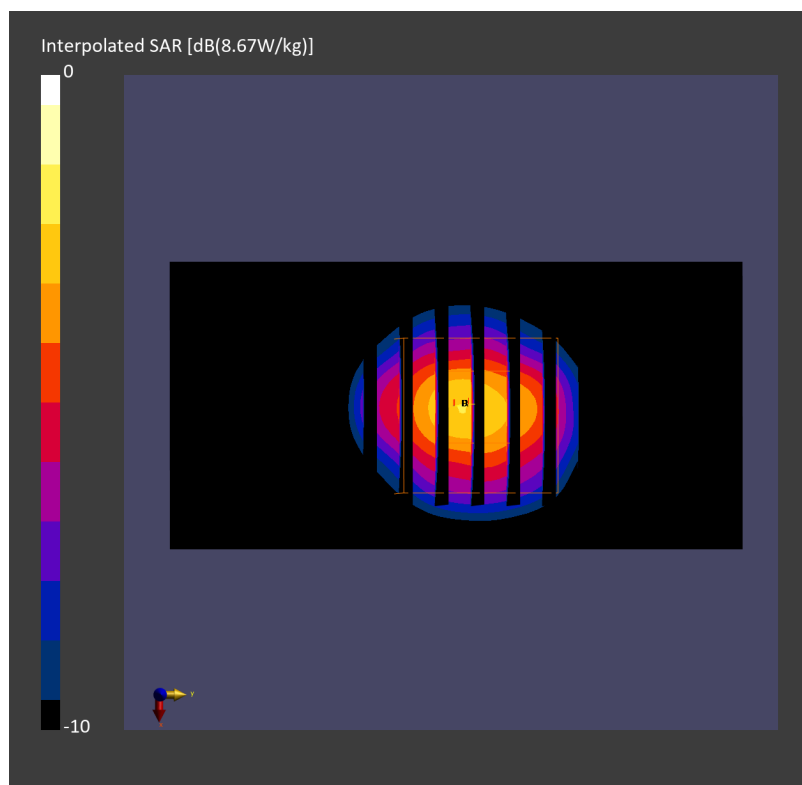

Date: 2025-07-22

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250722 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.17 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

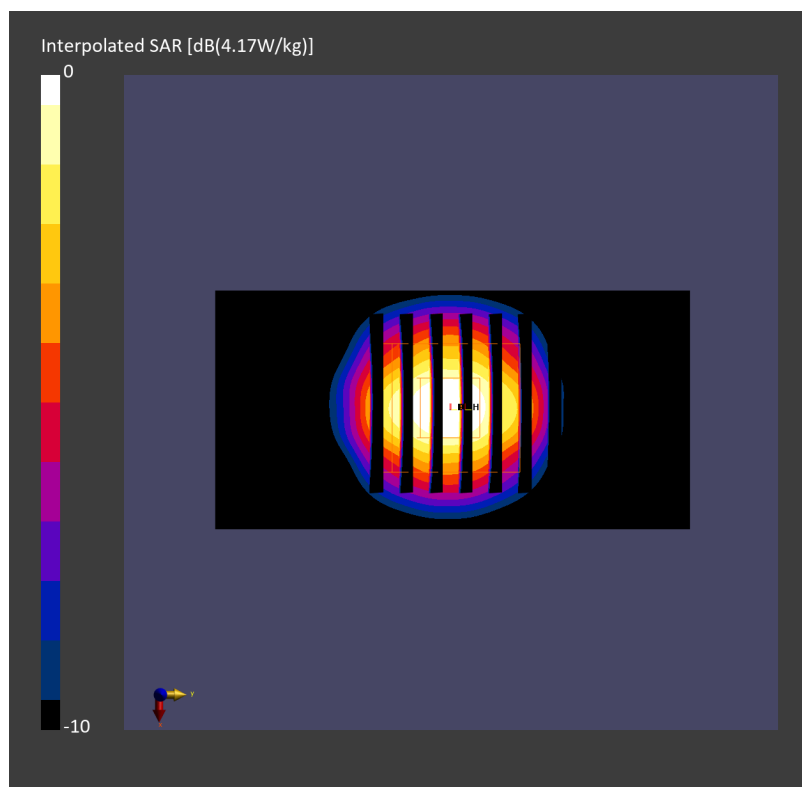

Date: 2025-07-23

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250723 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.21$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.26 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

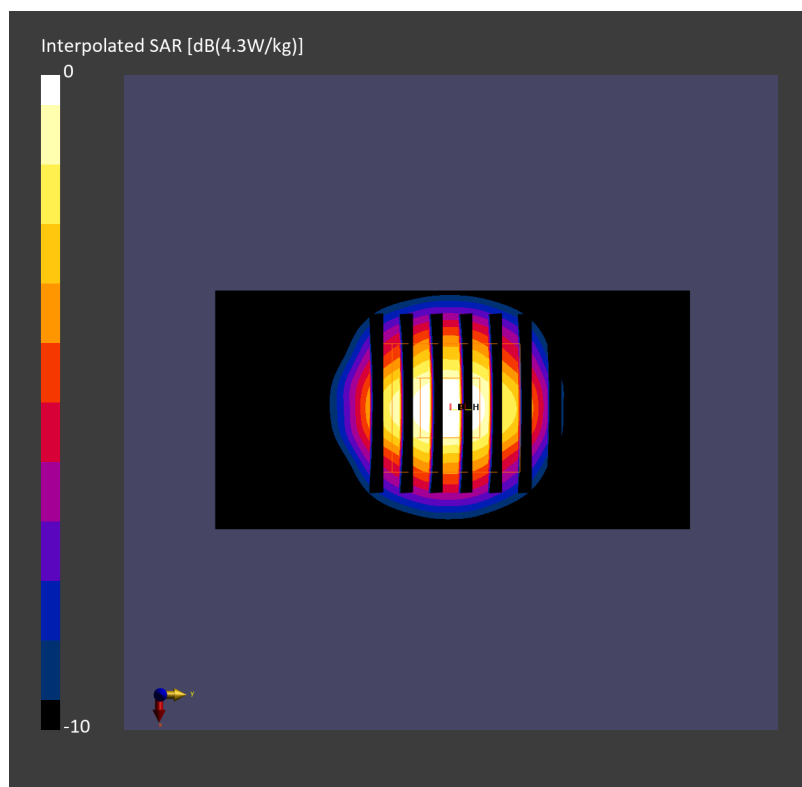

Date: 2025-07-24

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250724 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

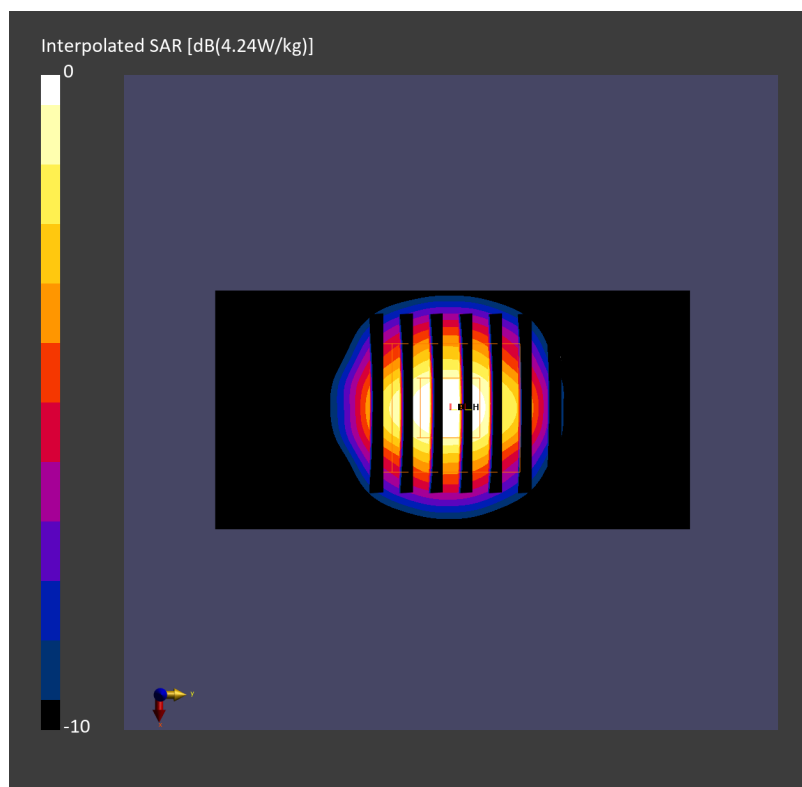

Date: 2025-07-26

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250726 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.14$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.16 W/kg; SAR (10g) = 1.16 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.16 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

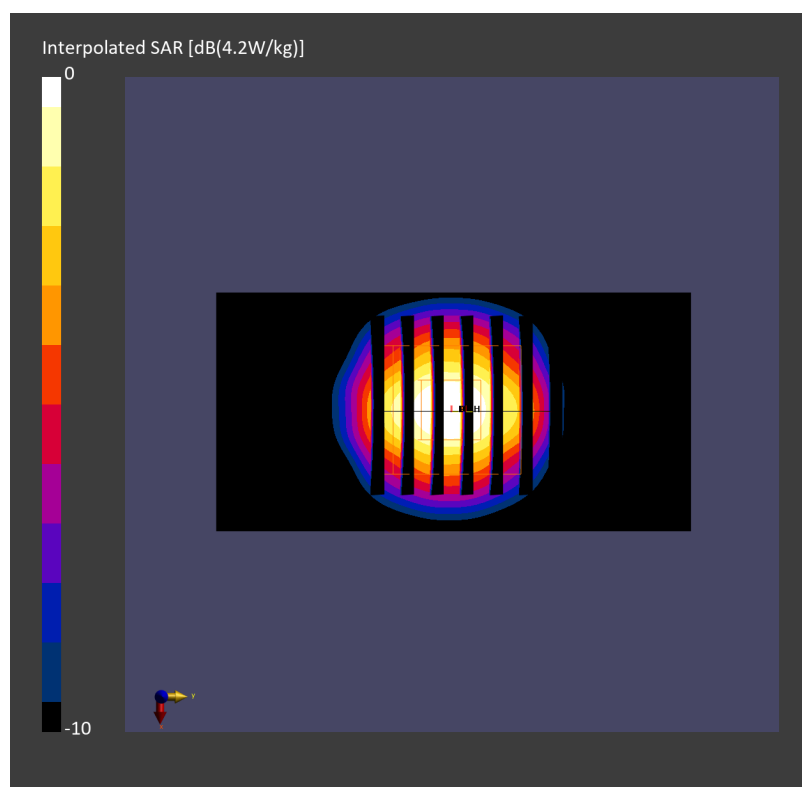

Date: 2025-07-27

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250727 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.07$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.13 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.07 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.7 %

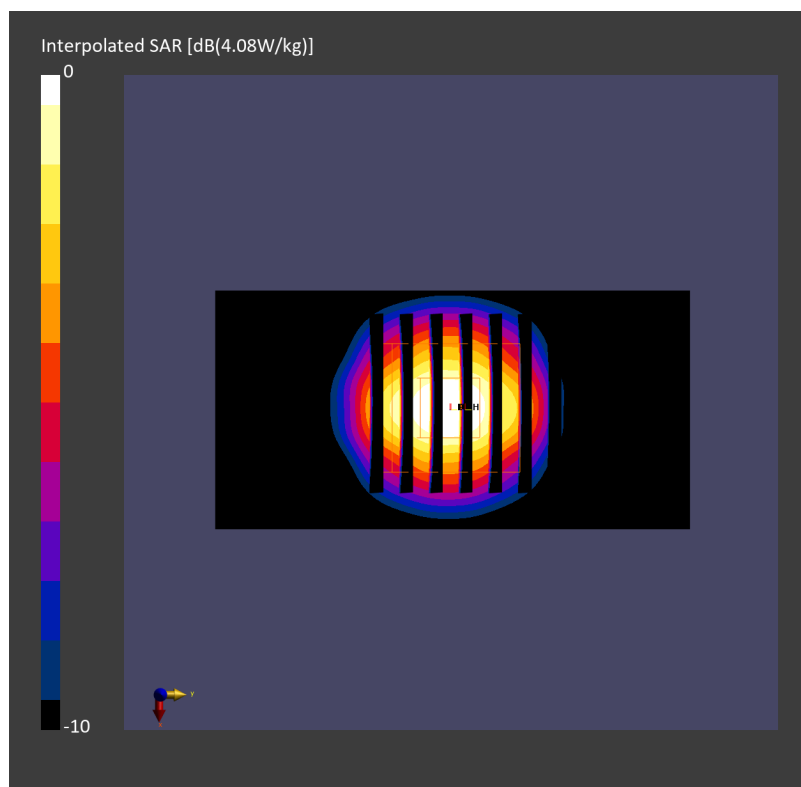

Date: 2025-07-28

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250728 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.04$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.10 dB

SAR (1g) = 3.09 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

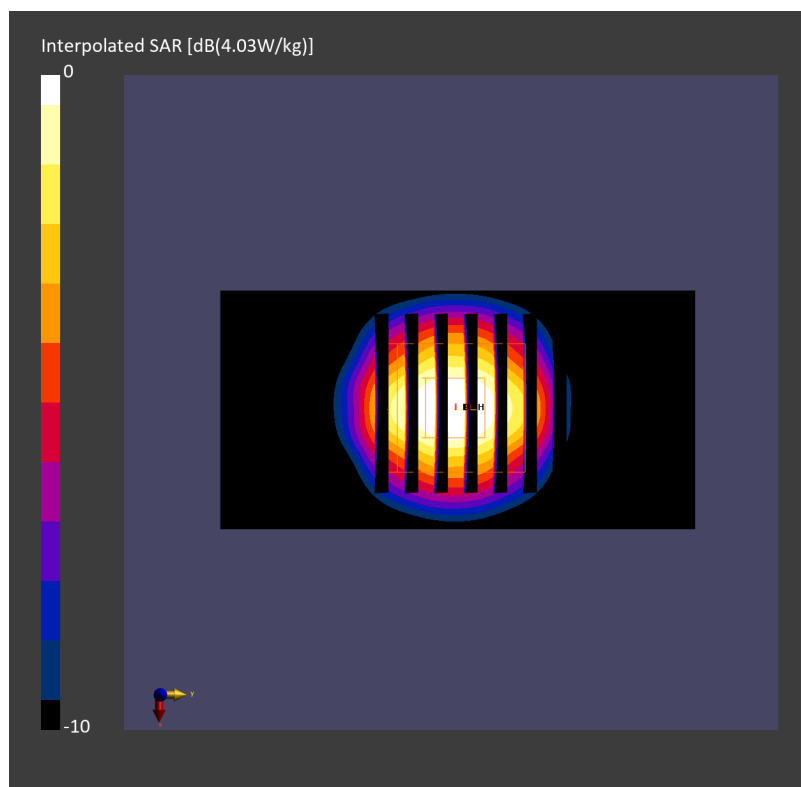

Date: 2025-07-30

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250730 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.20$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.19 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

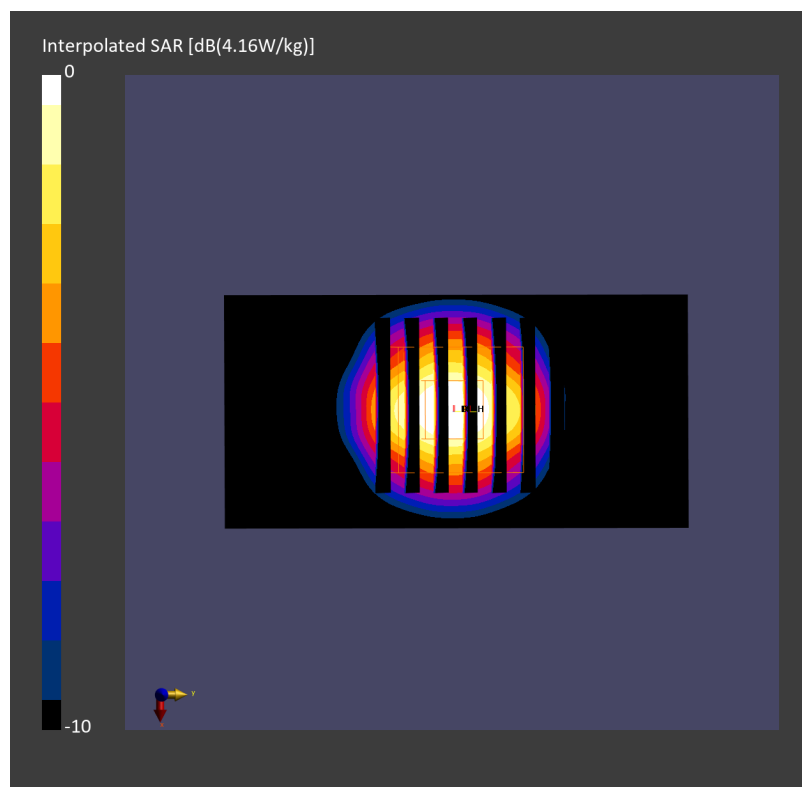

Date: 2025-07-31

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250731 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.14$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.14 W/kg; SAR (10g) = 1.15 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

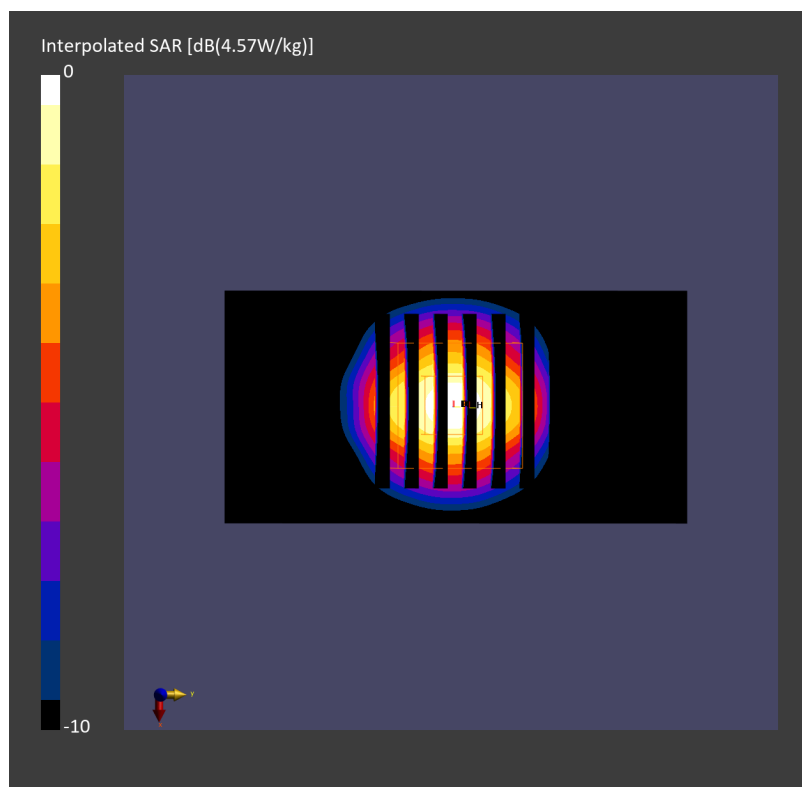

Date: 2025-08-06

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250806 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.44 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.47 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.9 %

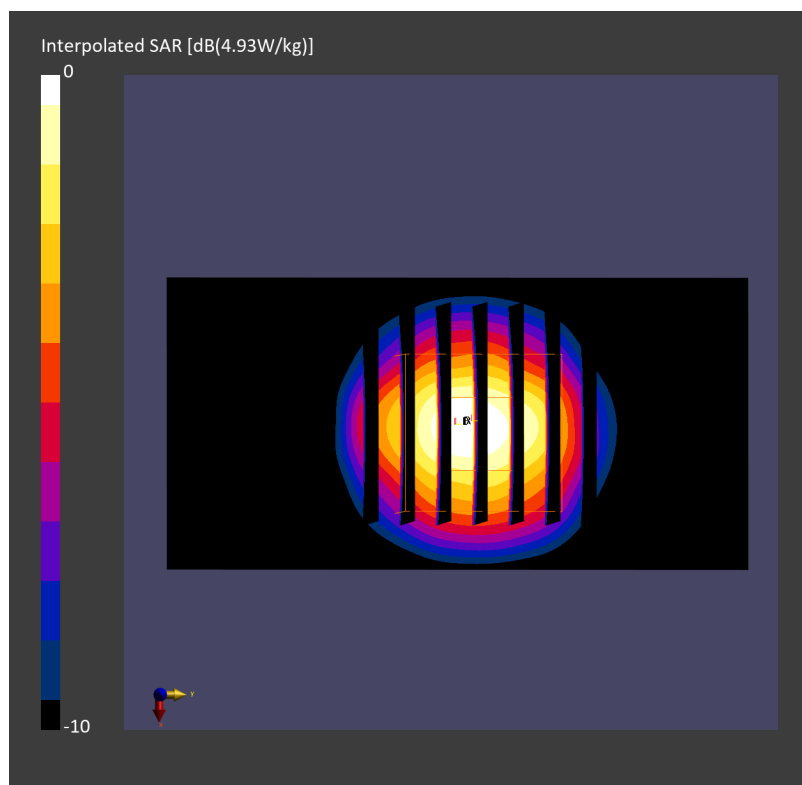

Date: 2025-08-13

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250813 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.16$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.41 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.45 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

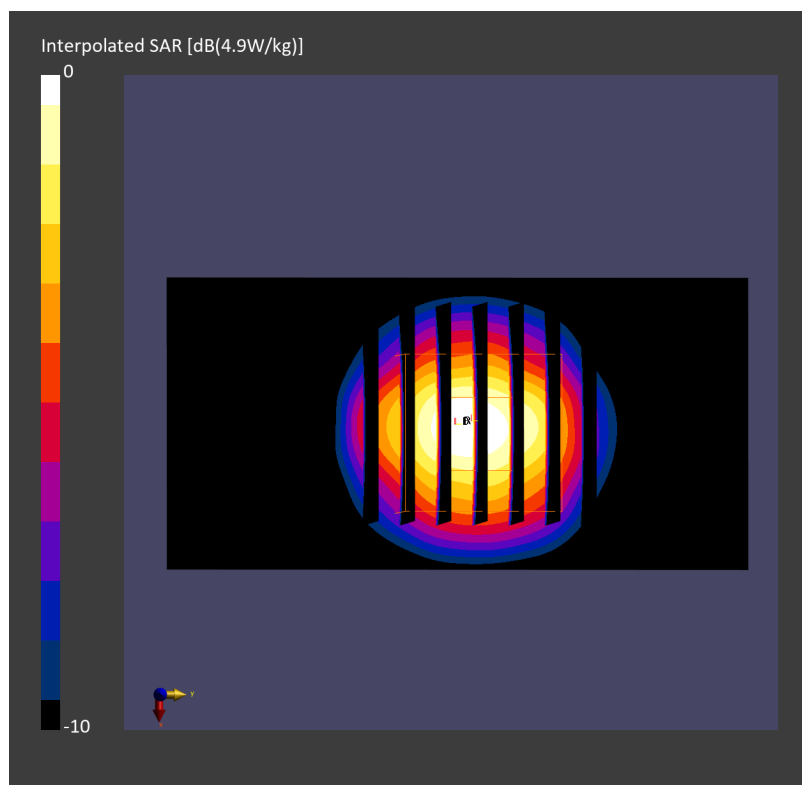

Date: 2025-08-14

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250814 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.13$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.38 W/kg; SAR (10g) = 1.26 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

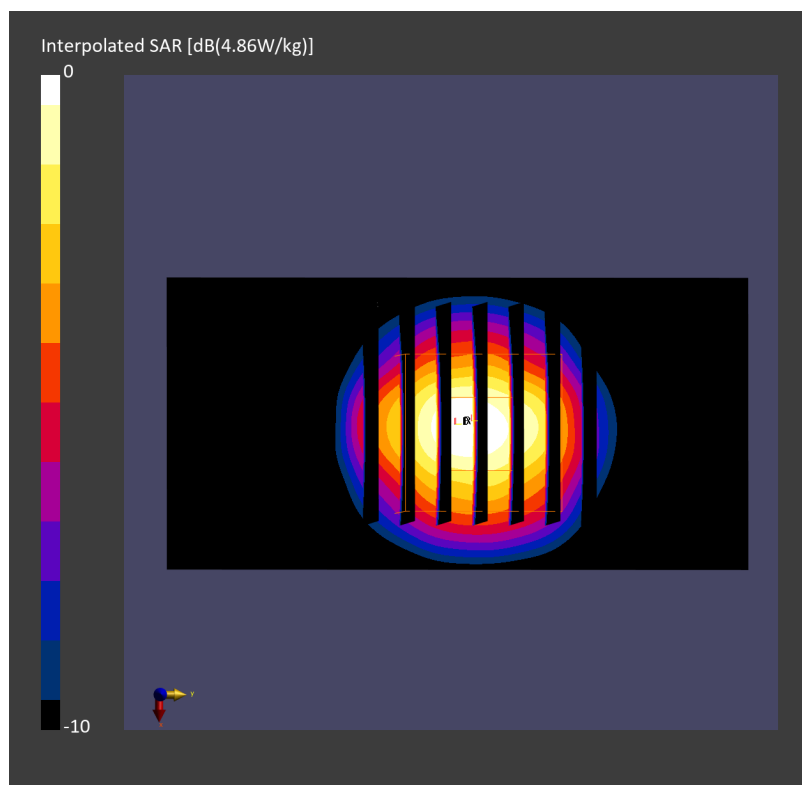

Date: 2025-08-15

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250815 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.11$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.25 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

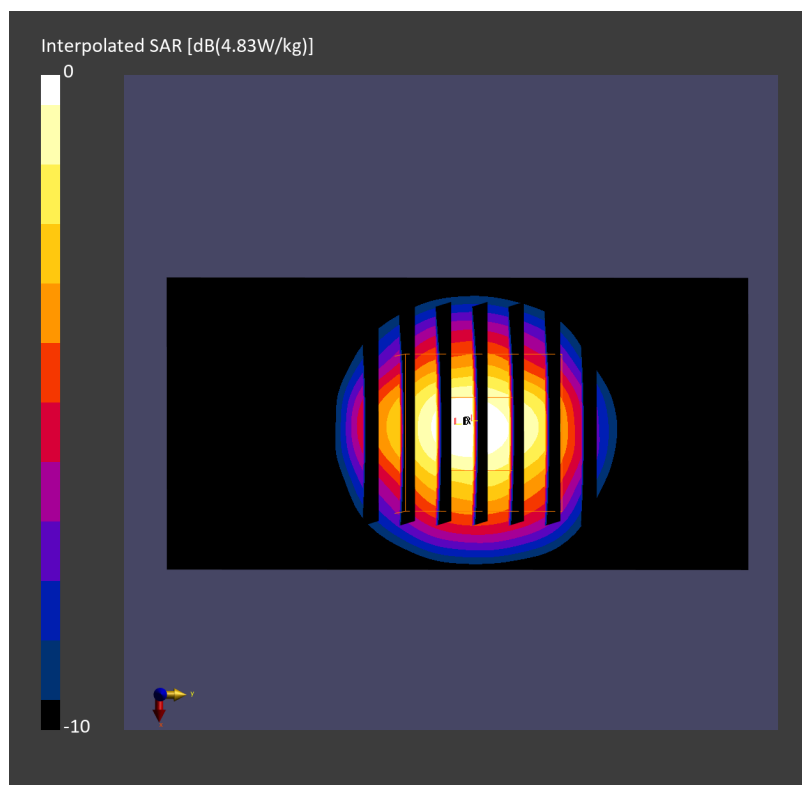

Date: 2025-08-16

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250816 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.37 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

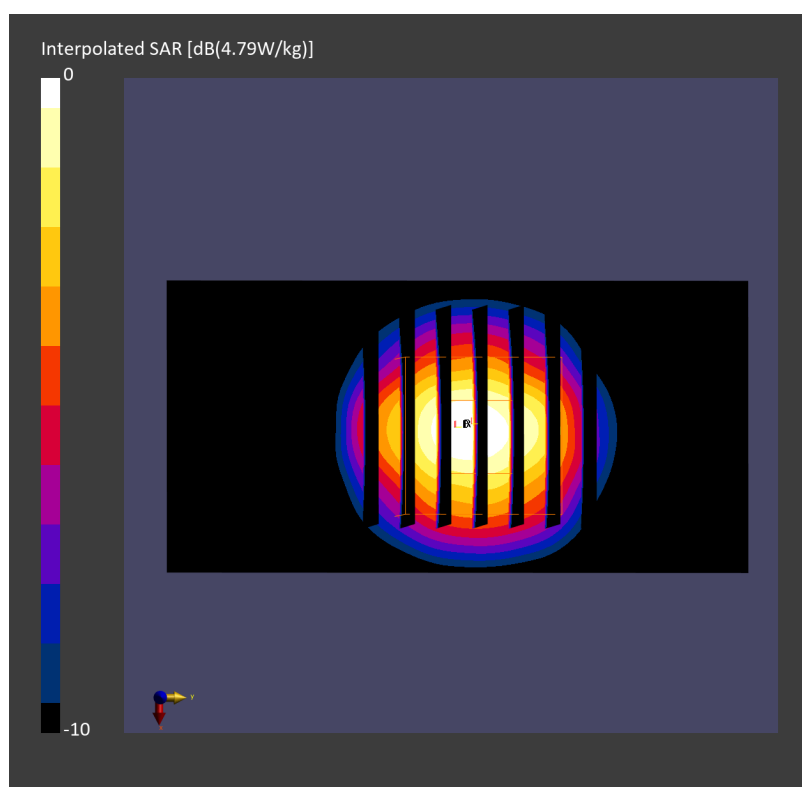

Date: 2025-08-17

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250817 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

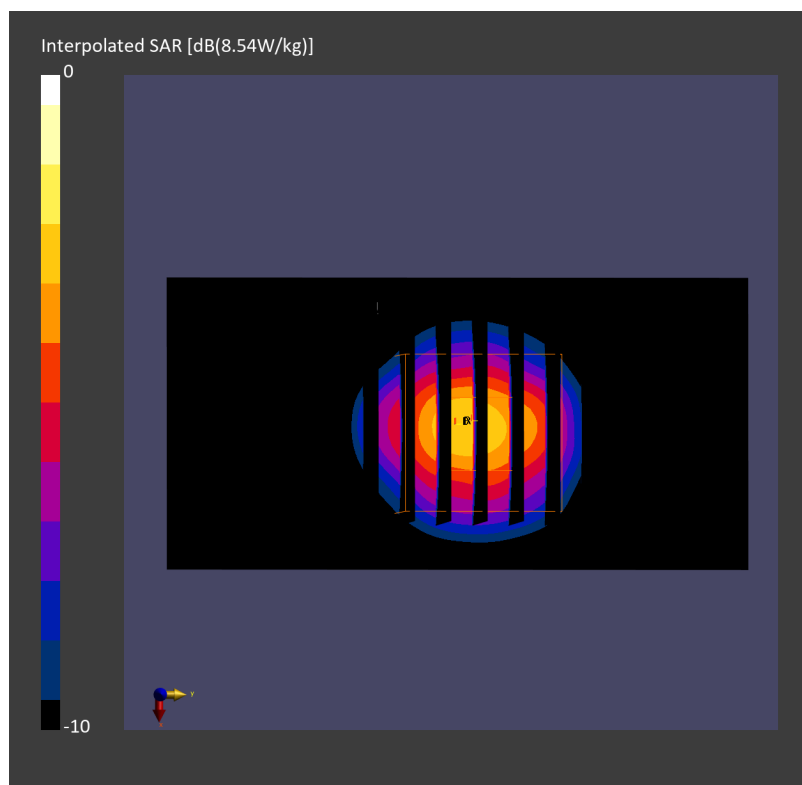

Date: 2025-08-22

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250822 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.03$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.49 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.32 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

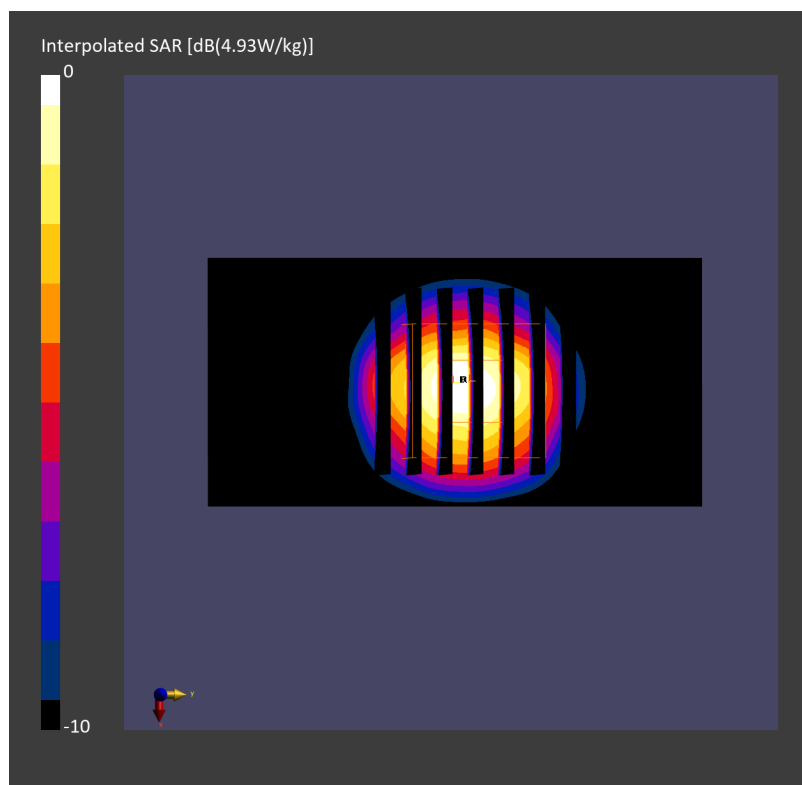

Date: 2025-08-24

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_250824 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2025-04-17
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.52 W/kg; SAR (8g) = 1.51 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.4 %

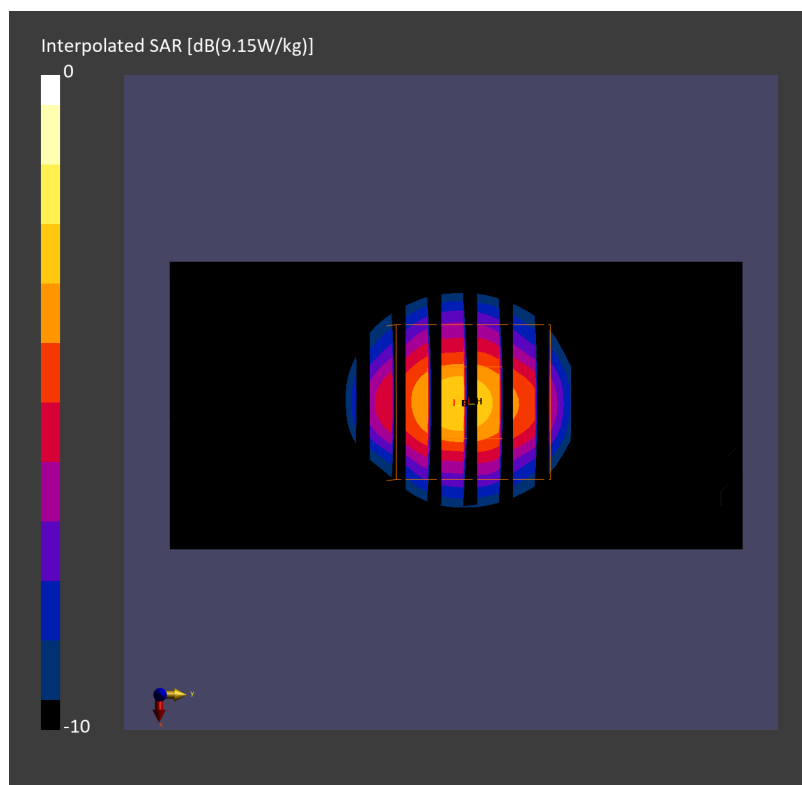

Date: 2025-07-26

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250726 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.35$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.48 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.6 %

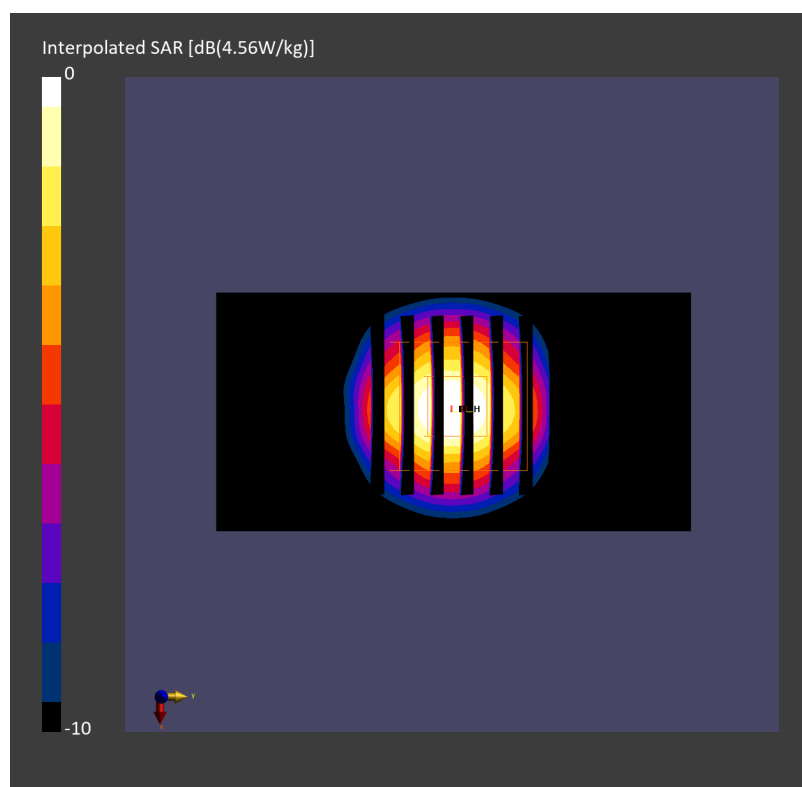

Date: 2025-07-27

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250727 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.23$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.36 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.3 %

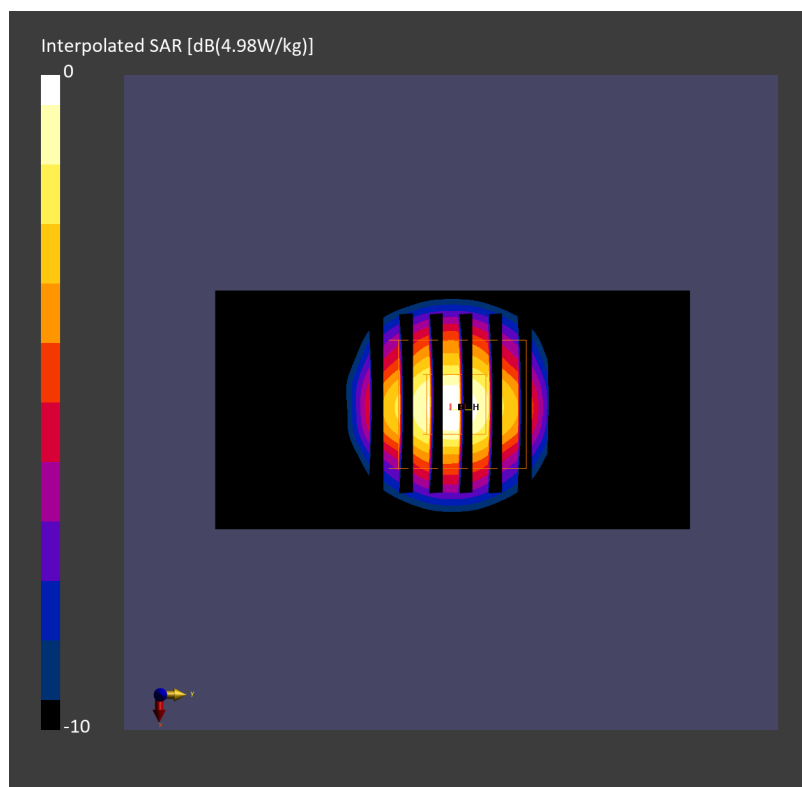

Date: 2025-07-28

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250728 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.20$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.16 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.33 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.4 %

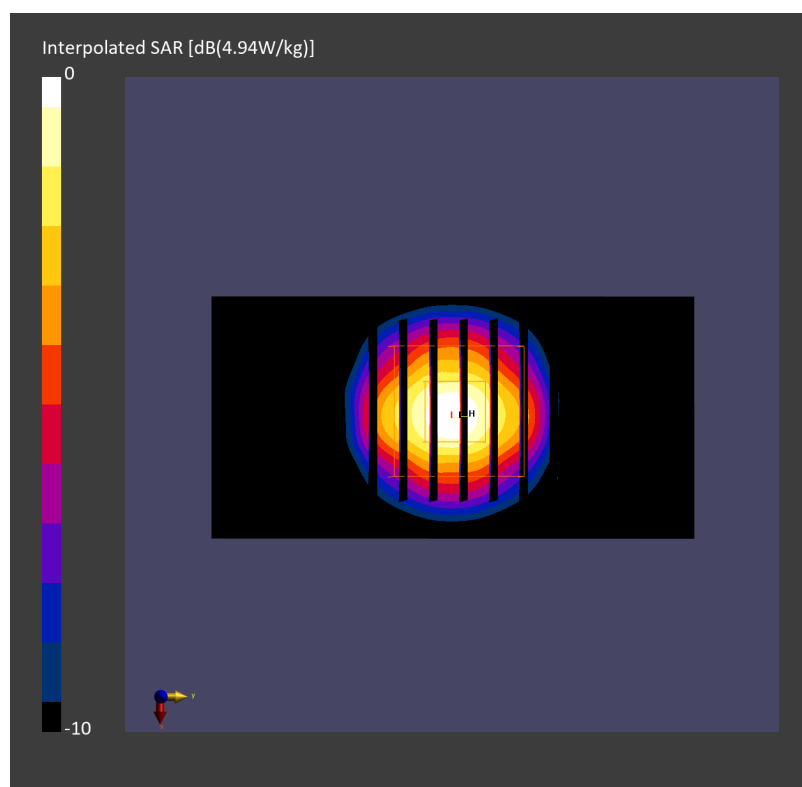

Date: 2025-07-29

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250729 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.28$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.18 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.4 %

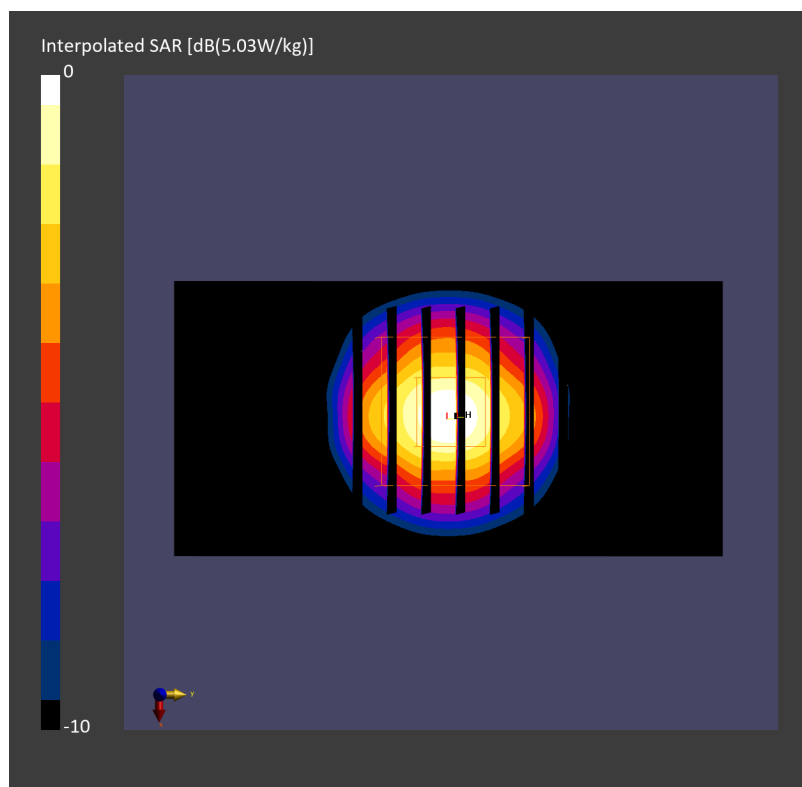

Date: 2025-07-30

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250730 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.39$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.52 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.5 %

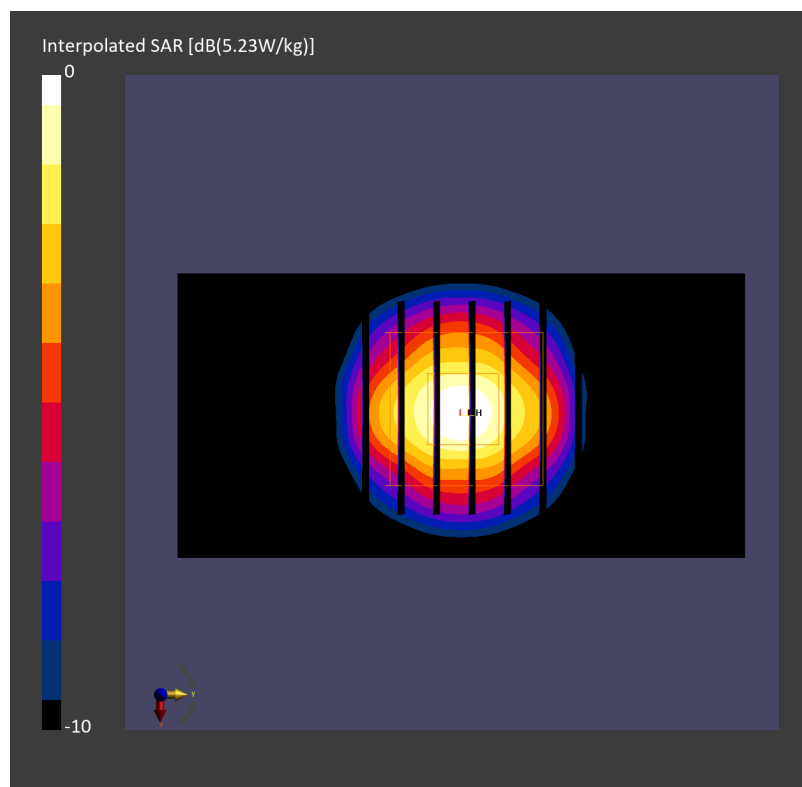

Date: 2025-07-31

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250731 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.34$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(5.96, 5.39, 6.86); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2025-06-11
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.4 %

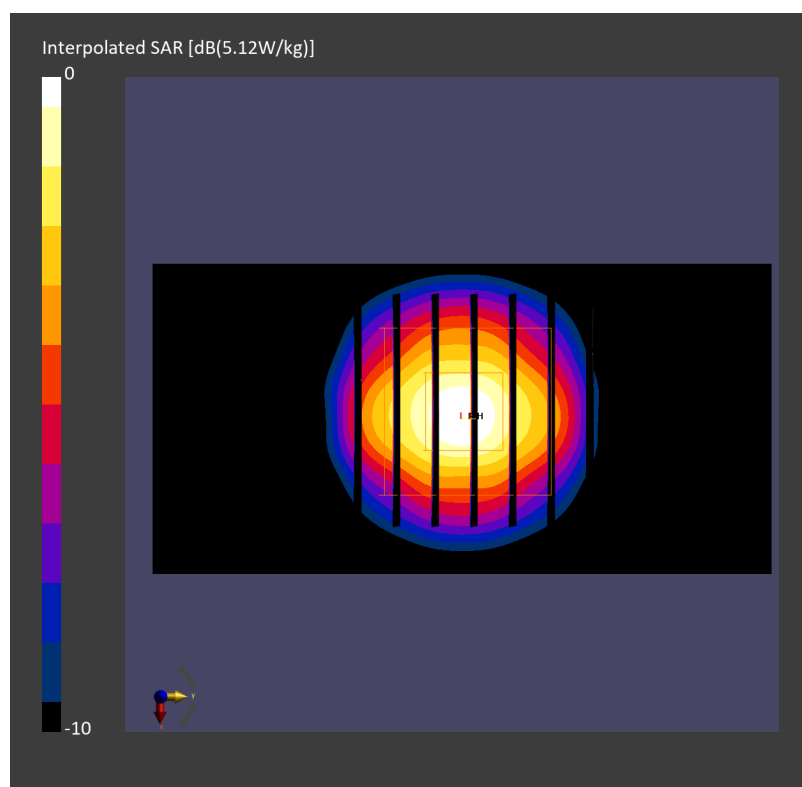

Date: 2025-08-14

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250814 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.34$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.68 W/kg; SAR (10g) = 1.29 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.58 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

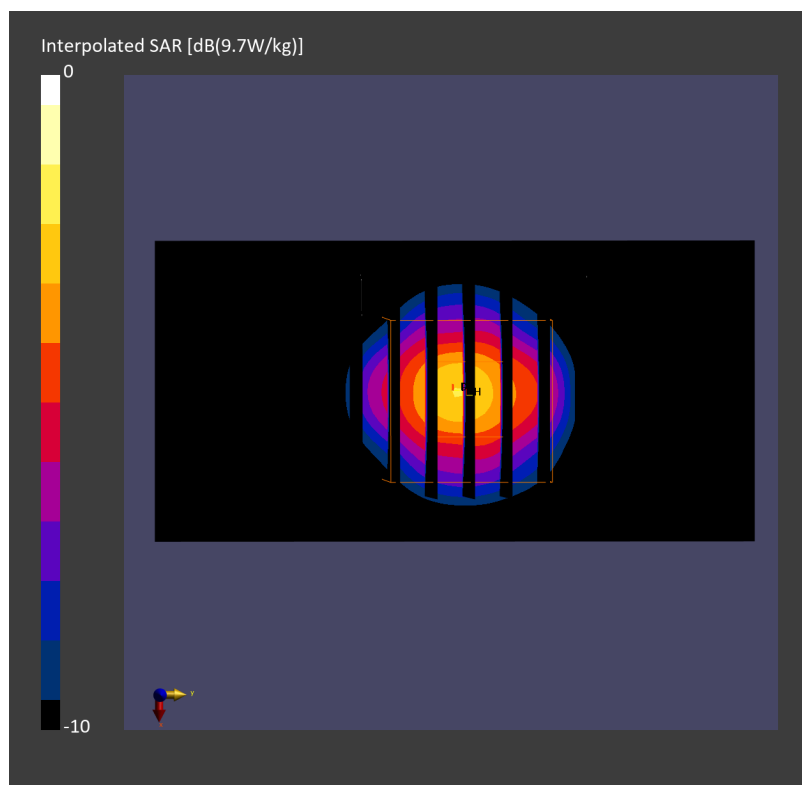

Date: 2025-08-15

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250815 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.31$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.54 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.53 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

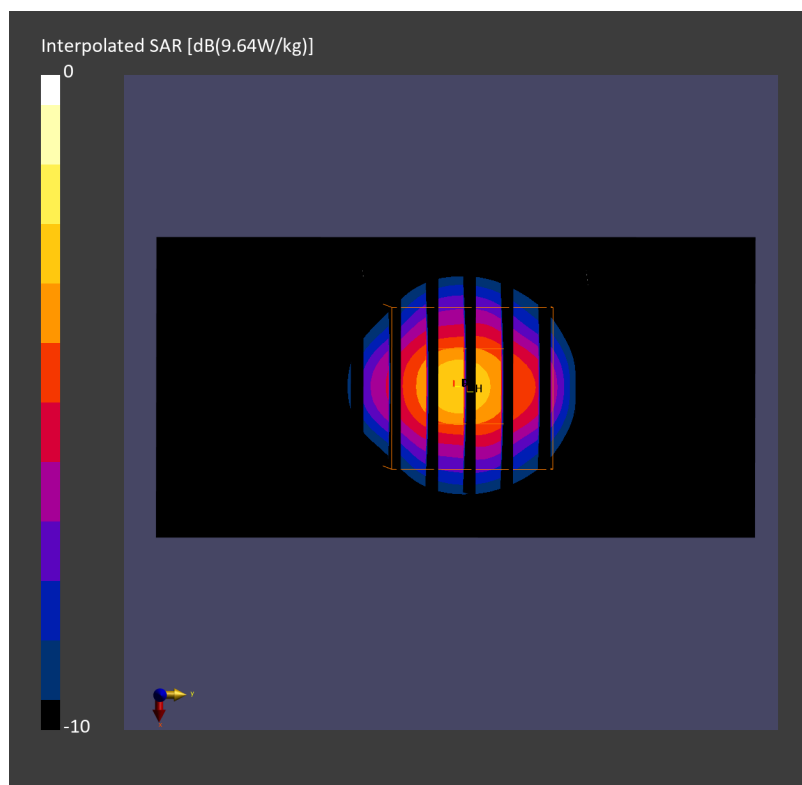

Date: 2025-08-16

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250816 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.29$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.52 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.51 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

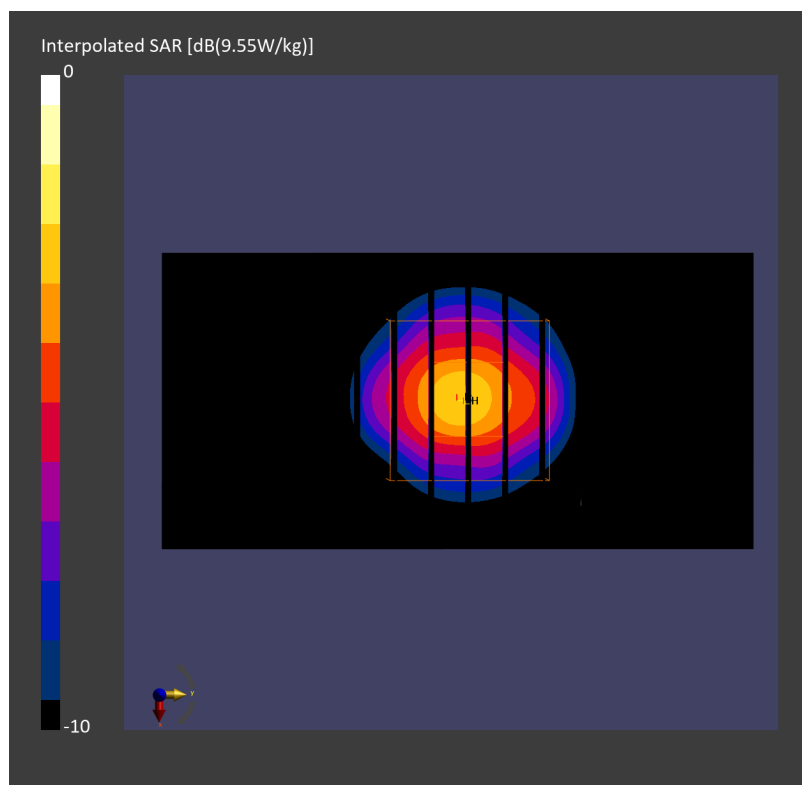

Date: 2025-08-17

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_250817 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.27$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.22 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.48 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

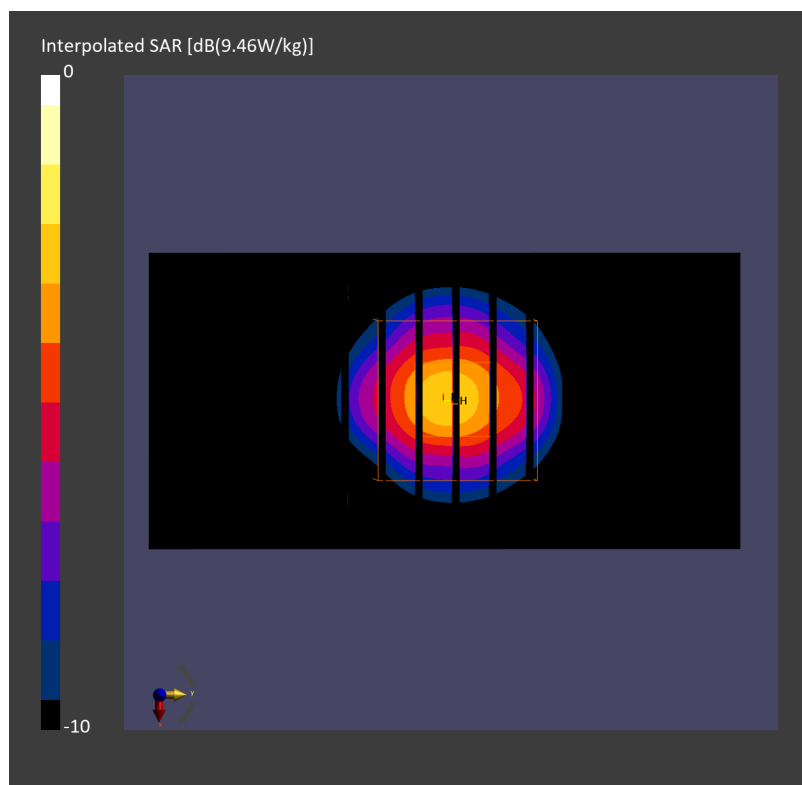

Date: 2025-08-19

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250819 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.63, 5.81, 5.62); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.62 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.79 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 63.1 %

TSL Correction: No correction

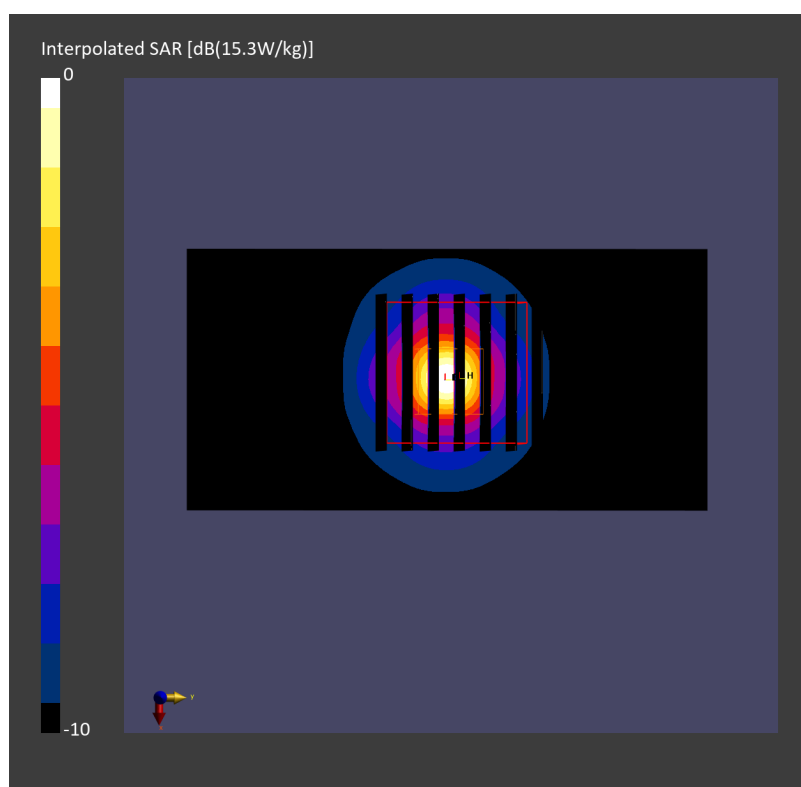

Date: 2025-08-20

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250820 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.71$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.63, 5.81, 5.62); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.60 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.77 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.0 %

TSL Correction: No correction

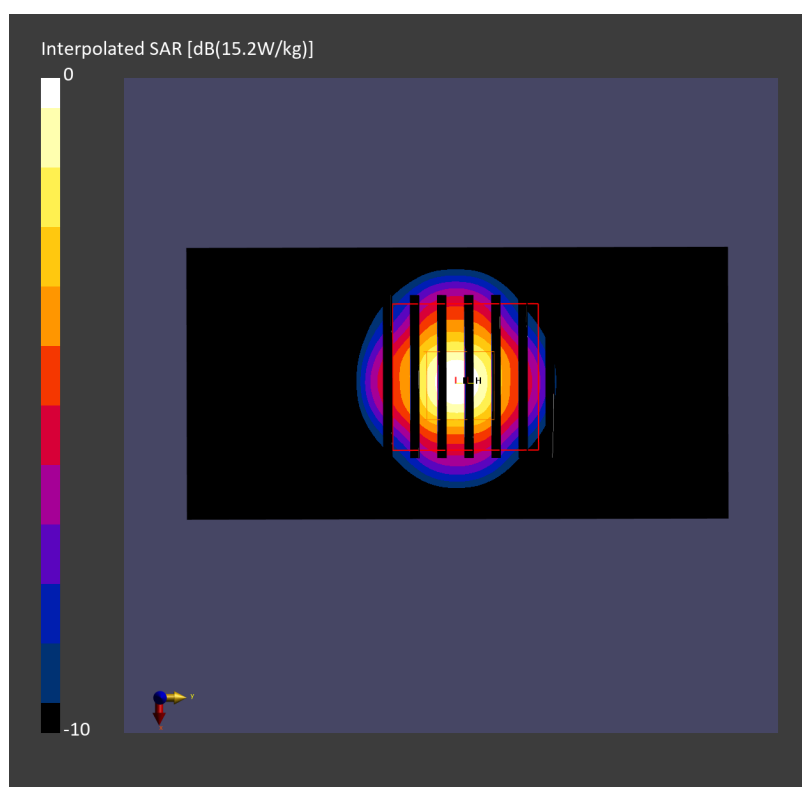

Date: 2025-08-26

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250826 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.63, 5.81, 5.62); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.51 W/kg; SAR (10g) = 0.977 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.06 dB

SAR (1g) = 3.68 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.0 %

TSL Correction: No correction

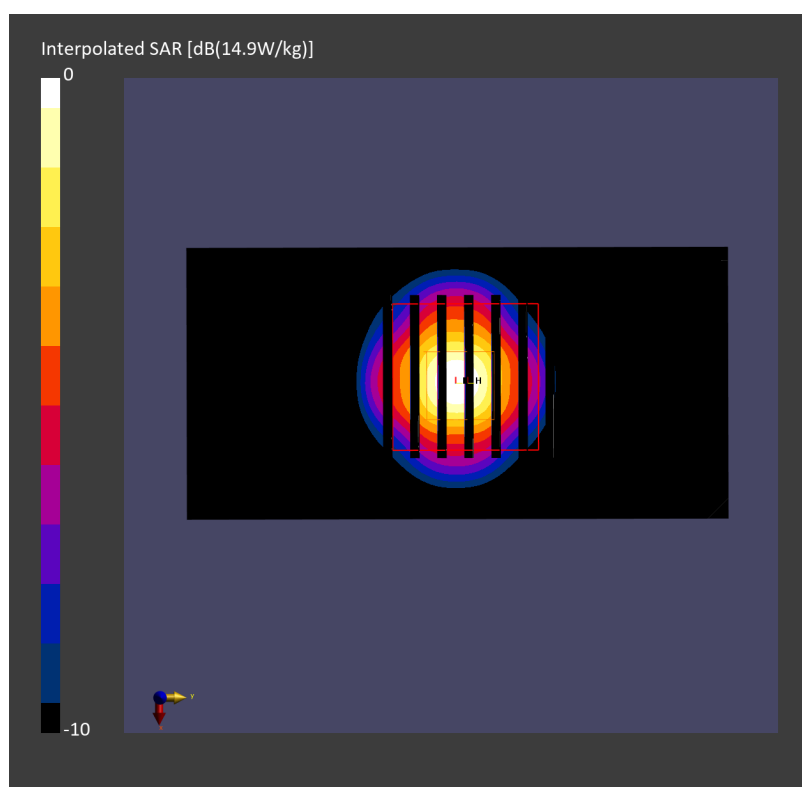

Date: 2025-08-29

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_250829 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.63, 5.81, 5.62); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.52 W/kg; SAR (10g) = 0.981 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.68 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 62.9 %

TSL Correction: No correction

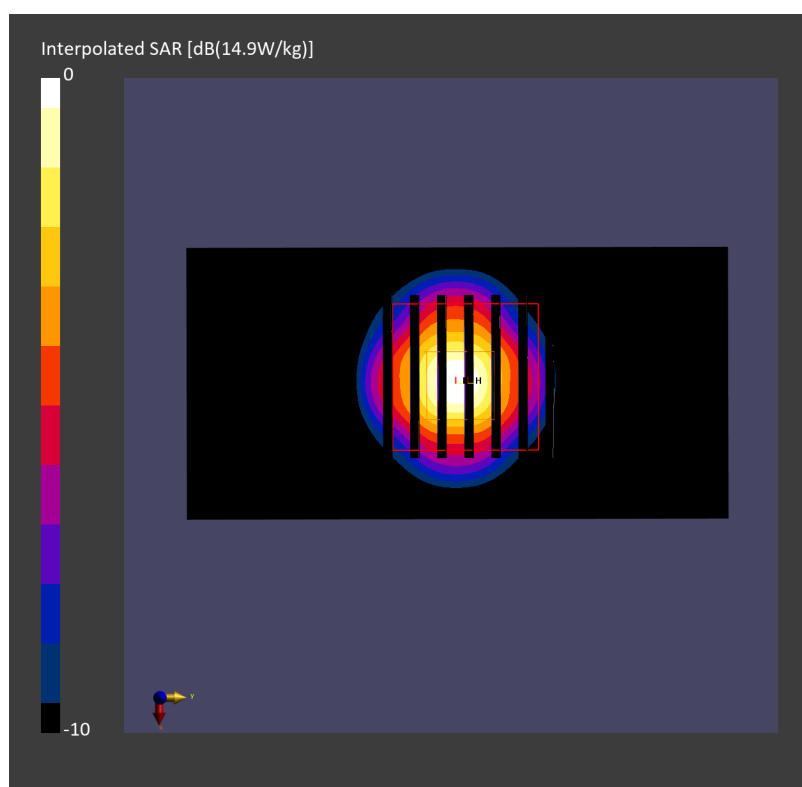

Date: 2025-08-21

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_250821 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.21, 5.37, 5.19); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.07 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 4.30 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 59.4 %

TSL Correction: No correction

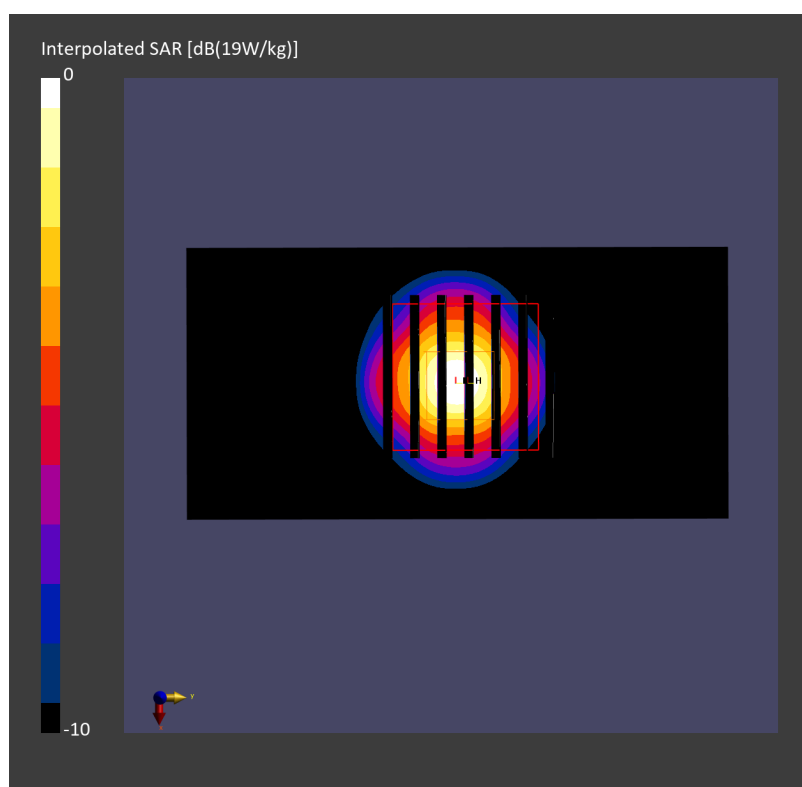

Date: 2025-08-27

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_250827 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.98$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(5.21, 5.37, 5.19); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.96 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: No correction

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 4.20 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 59.1 %

TSL Correction: No correction

