Date: 2026-01-12

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260112 Medium parameters used: f= 750.000 MHz; σ= 0.895 S/m; $\varepsilon_r$ = 42.8
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.6, 9.44, 9.5); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.22 W/kg; SAR (10g) = 1.48 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.23 W/kg; SAR (8g) = 1.56 W/kg; SAR (10g) = 1.48 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 88.2 %
TSL Correction: Positive only

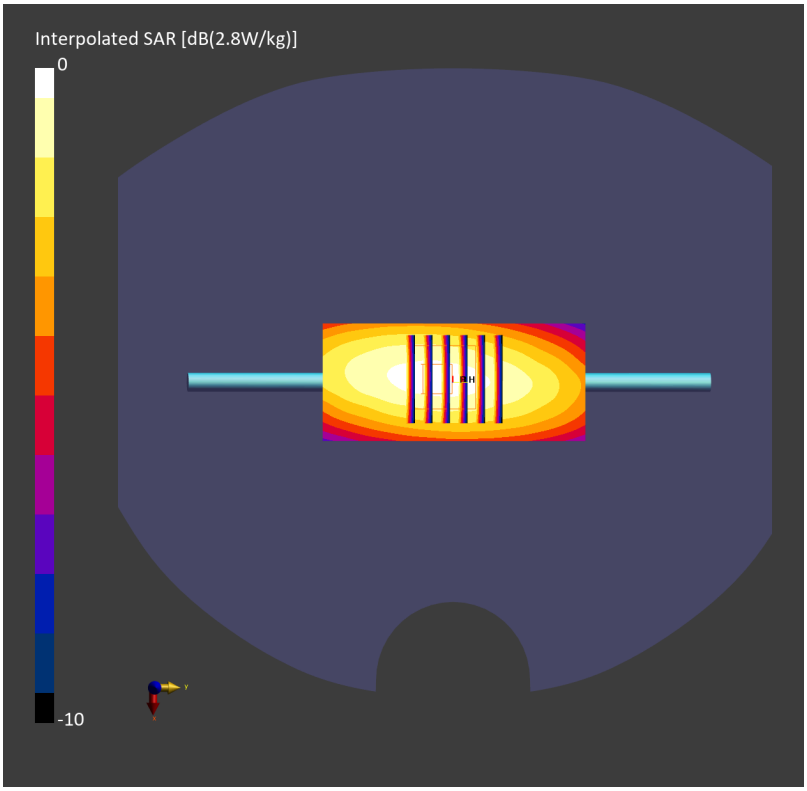

Date: 2026-01-18

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260118 Medium parameters used: f= 750.000 MHz; σ= 0.898 S/m; $\varepsilon_r$ = 42.7
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.6, 9.44, 9.5); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.14 W/kg; SAR (10g) = 1.43 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.13 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg
Smallest distance from peaks to all points 3 dB below = > 15.0 mm
Ratio of SAR at M2 to SAR at M1 = 87.4 %
TSL Correction: Positive only

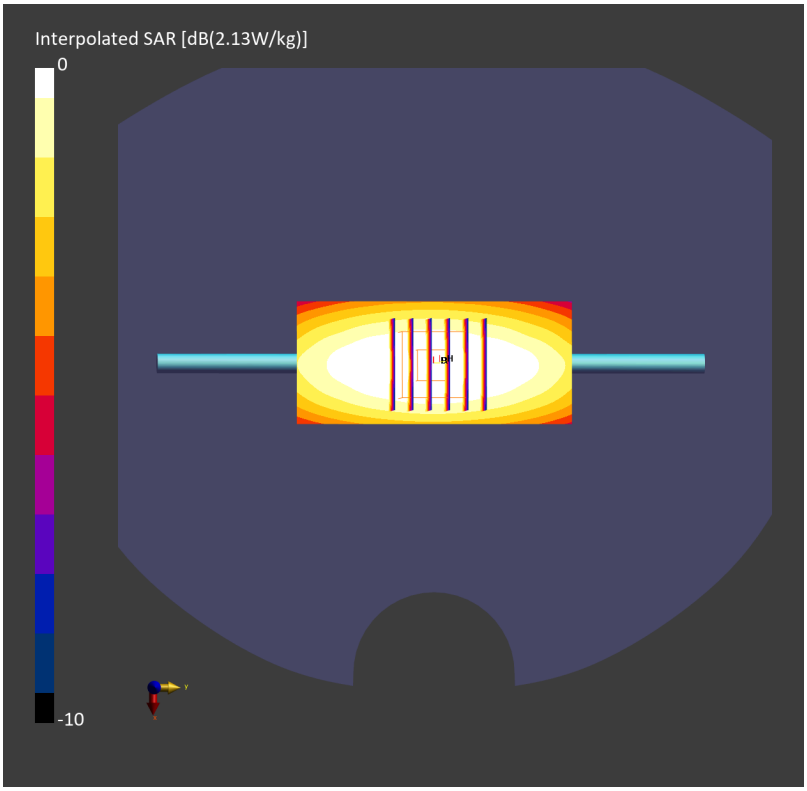

Date: 2026-01-19

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260119 Medium parameters used: f= 750.000 MHz; σ= 0.915 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.6, 9.44, 9.5); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.27 W/kg; SAR (10g) = 1.51 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 2.27 W/kg; SAR (8g) = 1.59 W/kg; SAR (10g) = 1.51 W/kg
Smallest distance from peaks to all points 3 dB below = 23.0 mm
Ratio of SAR at M2 to SAR at M1 = 87.9 %
TSL Correction: Positive only

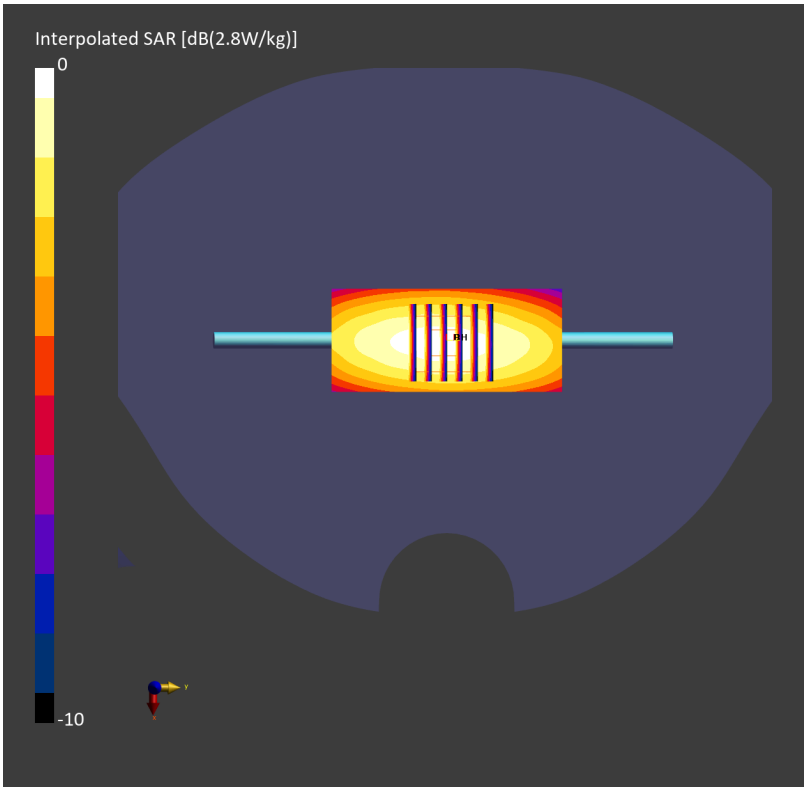

Date: 2026-02-06

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260206 Medium parameters used: f= 750.000 MHz; σ= 0.886 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.99 W/kg; SAR (10g) = 1.33 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 2.00 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.33 W/kg
Smallest distance from peaks to all points 3 dB below = 18.4 mm
Ratio of SAR at M2 to SAR at M1 = 88.4 %
TSL Correction: Positive only

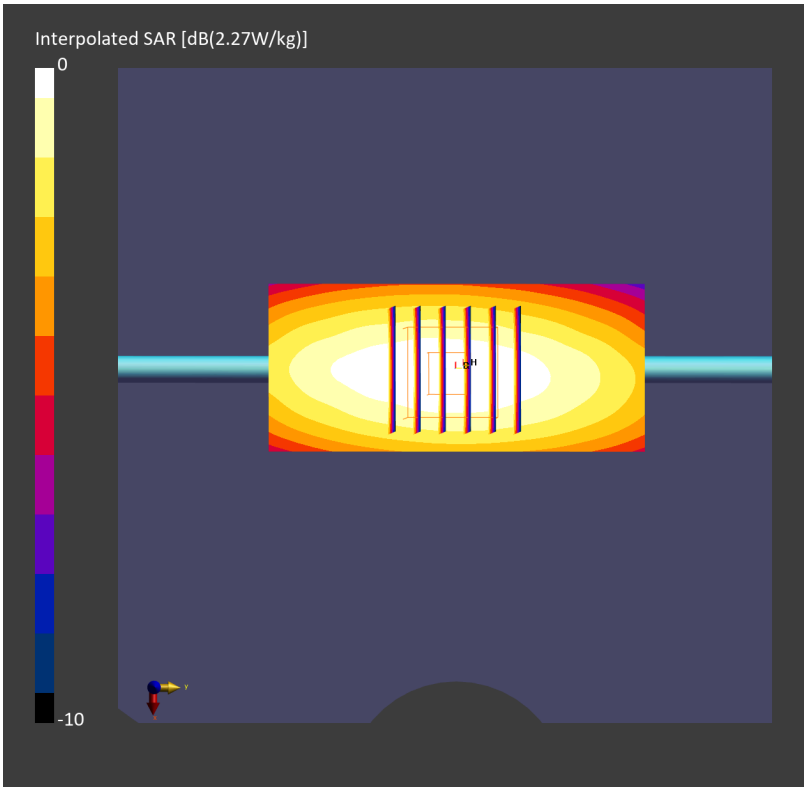

Date: 2026-02-08

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260208 Medium parameters used: f= 750.000 MHz; σ= 0.901 S/m; $\varepsilon_r$ = 42.6
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.26 W/kg; SAR (10g) = 1.51 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.26 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg
Smallest distance from peaks to all points 3 dB below = > 15.0 mm
Ratio of SAR at M2 to SAR at M1 = 88.7 %
TSL Correction: Positive only

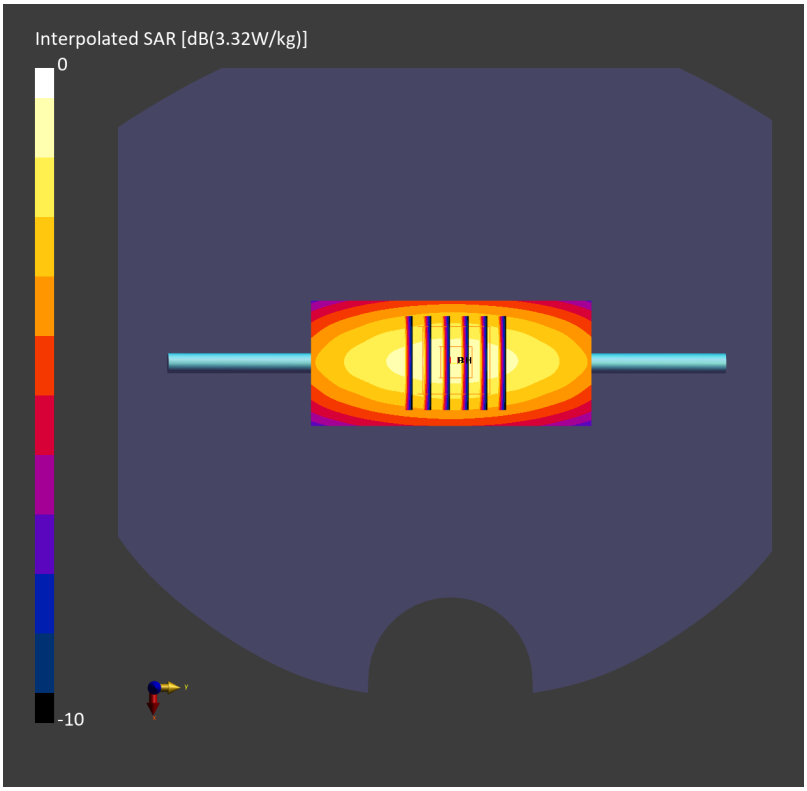

Date: 2026-02-20

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260220 Medium parameters used: f= 750.000 MHz; σ= 0.886 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.21 W/kg; SAR (10g) = 1.47 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.03 dB
SAR (1g) = 2.18 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.45 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 88.6 %
TSL Correction: Positive only

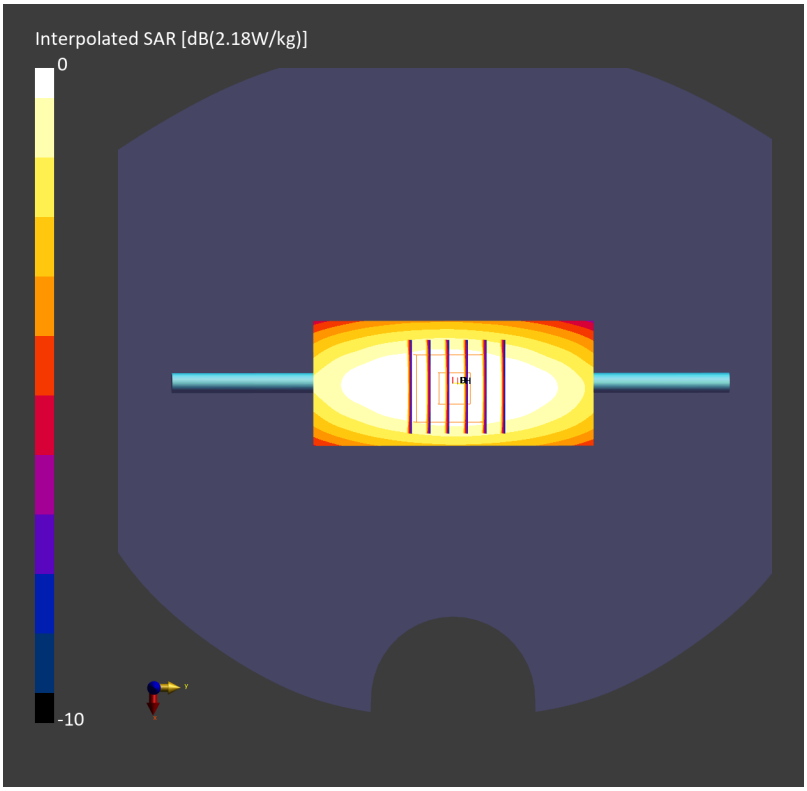

Date: 2026-03-02

**System Check_Head 750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260302 Medium parameters used: f= 750.000 MHz; σ= 0.891 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(9.69, 9.27, 10.31); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.02 W/kg; SAR (10g) = 1.35 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.02 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.34 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 86.9 %
TSL Correction: Positive only

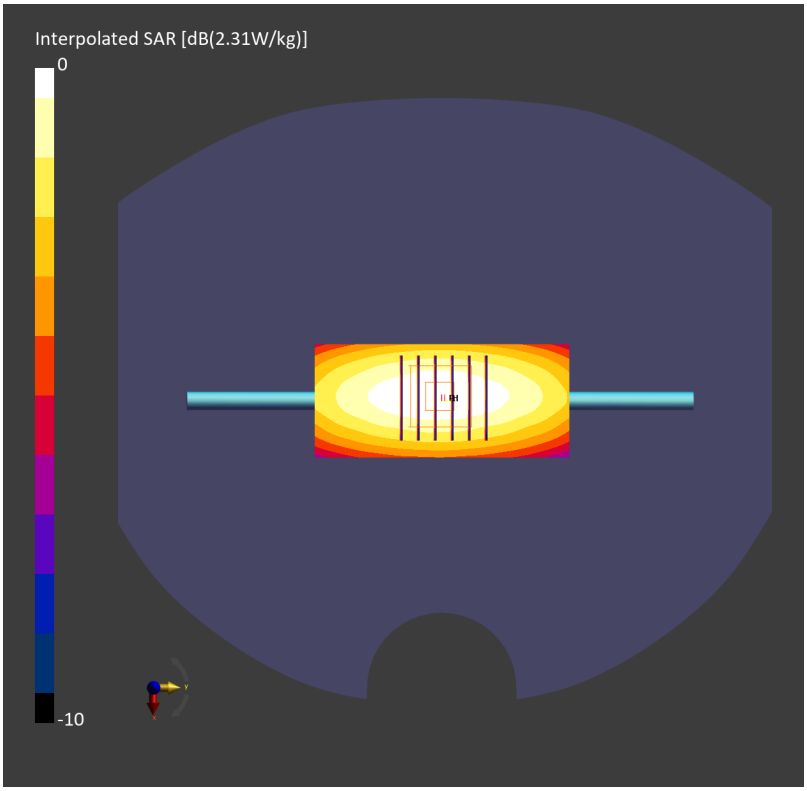

Date: 2026-03-11

**System Check_Head_750MHz**

**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260311 Medium parameters used: f= 750.000 MHz; σ= 0.893 S/m; $\varepsilon_r$ = 42.4
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.23 W/kg; SAR (10g) = 1.49 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.22 W/kg; SAR (8g) = 1.56 W/kg; SAR (10g) = 1.48 W/kg
Smallest distance from peaks to all points 3 dB below = 20.5 mm
Ratio of SAR at M2 to SAR at M1 = 88.3 %
TSL Correction: Positive only

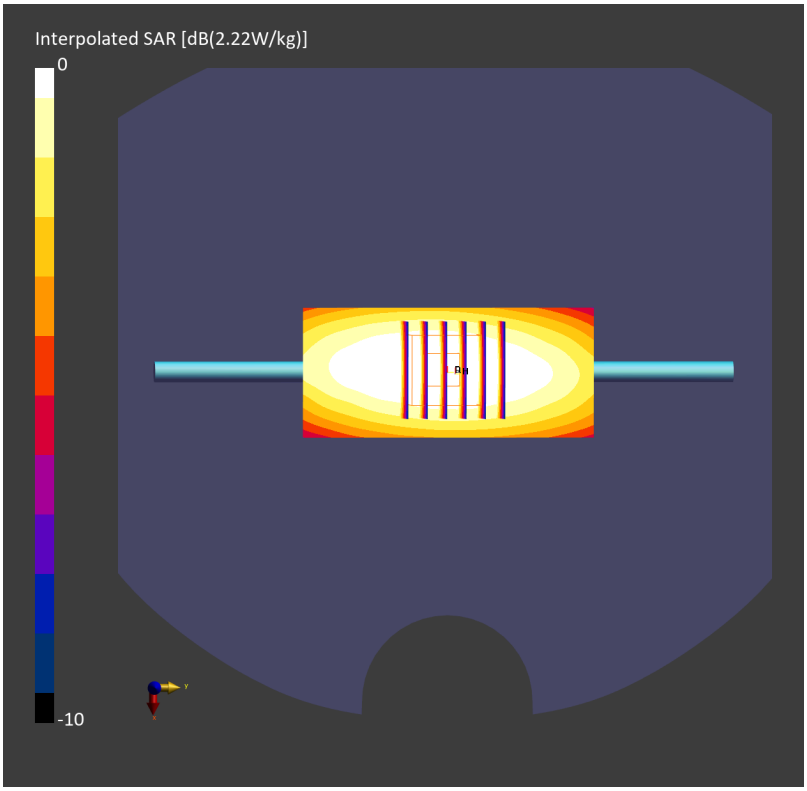

Date: 2026-03-16

**System Check_Head_750MHz**

**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260316 Medium parameters used: f= 750.000 MHz; σ= 0.883 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.26 W/kg; SAR (10g) = 1.51 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.03 dB
SAR (1g) = 2.27 W/kg; SAR (8g) = 1.59 W/kg; SAR (10g) = 1.51 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 88.9 %
TSL Correction: Positive only

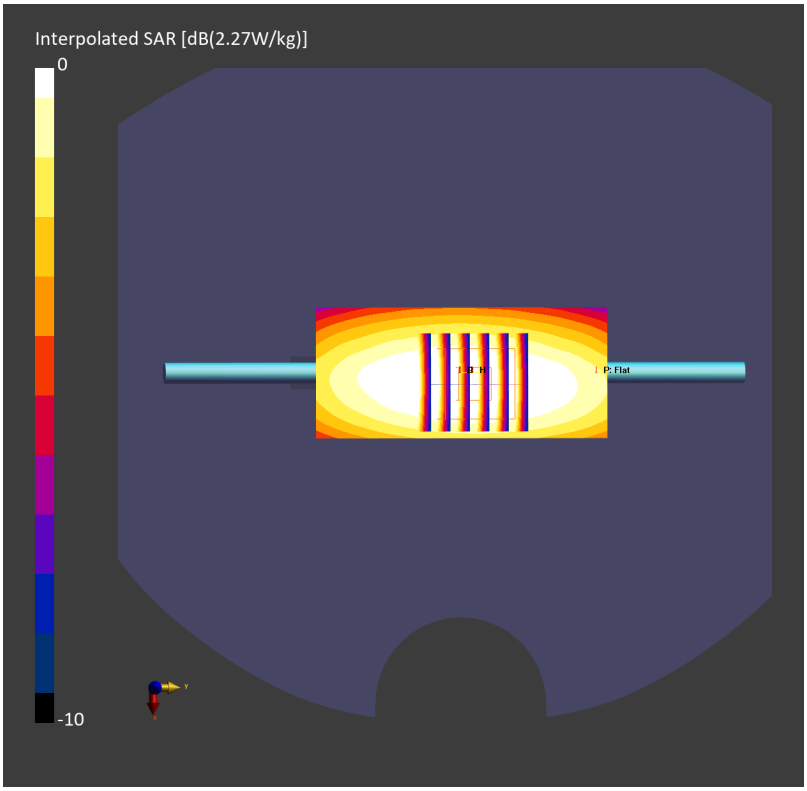

Date: 2026-04-05

**System Check_Head_750MHz**

**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_600-7200_260405 Medium parameters used: f= 750.000 MHz; σ= 0.871 S/m; $\varepsilon_r$ = 45.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN3728; ConvF(9.08, 8.91, 9.18); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.05 W/kg; SAR (10g) = 1.35 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.03 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.33 W/kg
Smallest distance from peaks to all points 3 dB below = > 15.0 mm
Ratio of SAR at M2 to SAR at M1 = 87.1 %
TSL Correction: Positive only

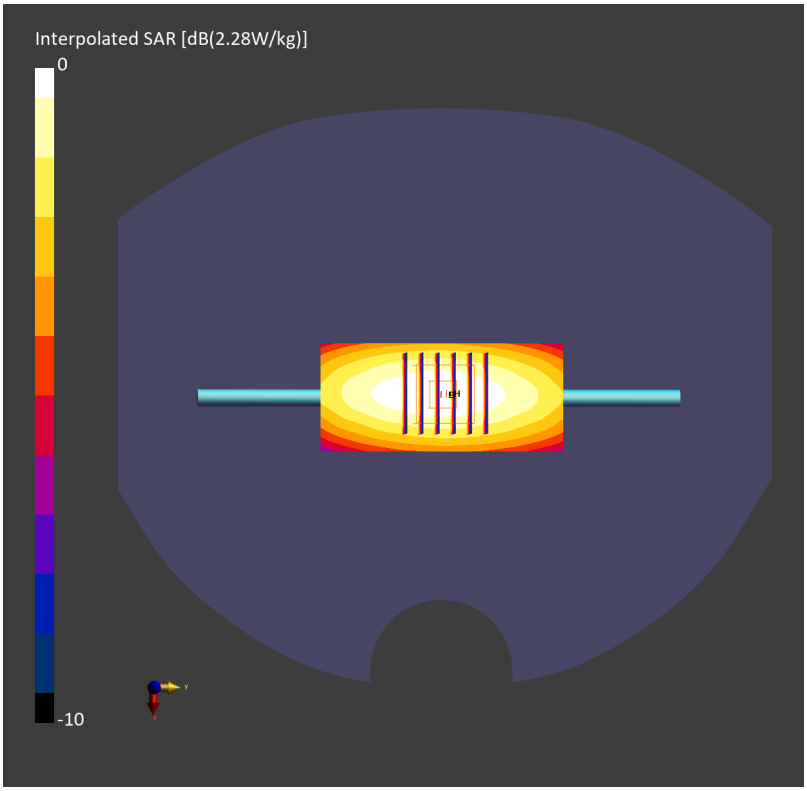

Date: 2026-01-05

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260105 Medium parameters used: f= 835.000 MHz; σ= 0.908 S/m; $\varepsilon_r$ = 42.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.27, 9.12, 9.17); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.46 W/kg; SAR (10g) = 1.62 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.06 dB
SAR (1g) = 2.43 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.60 W/kg
Smallest distance from peaks to all points 3 dB below = 16.8 mm
Ratio of SAR at M2 to SAR at M1 = 87.4 %
TSL Correction: Positive only

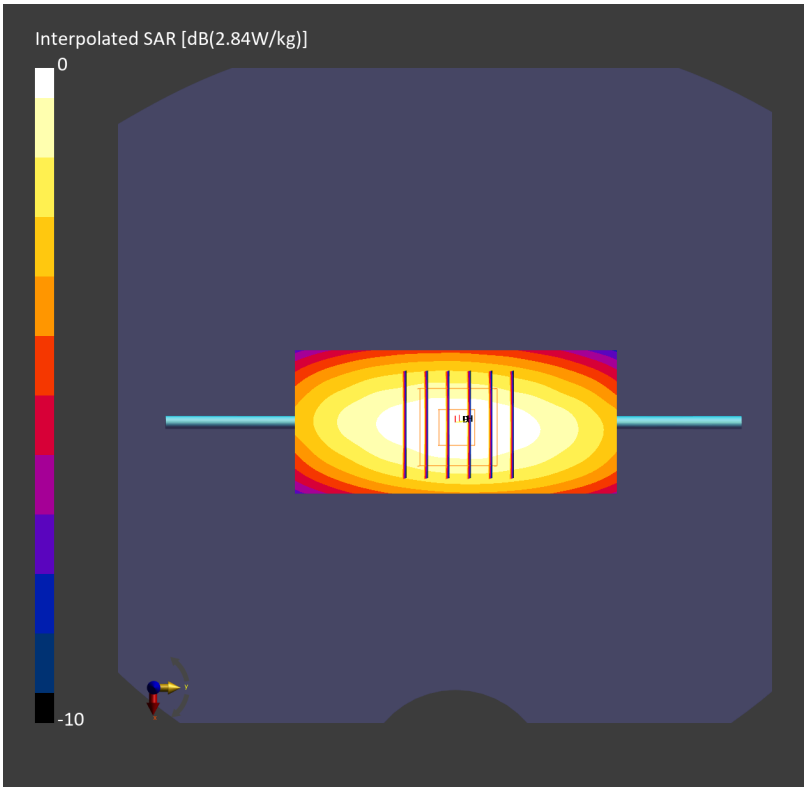

Date: 2026-01-12

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260112 Medium parameters used: f= 835.000 MHz; σ= 0.925 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.27, 9.12, 9.17); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.45 W/kg; SAR (10g) = 1.61 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.45 W/kg; SAR (8g) = 1.70 W/kg; SAR (10g) = 1.62 W/kg
Smallest distance from peaks to all points 3 dB below = 17.2 mm
Ratio of SAR at M2 to SAR at M1 = 88.1 %
TSL Correction: Positive only

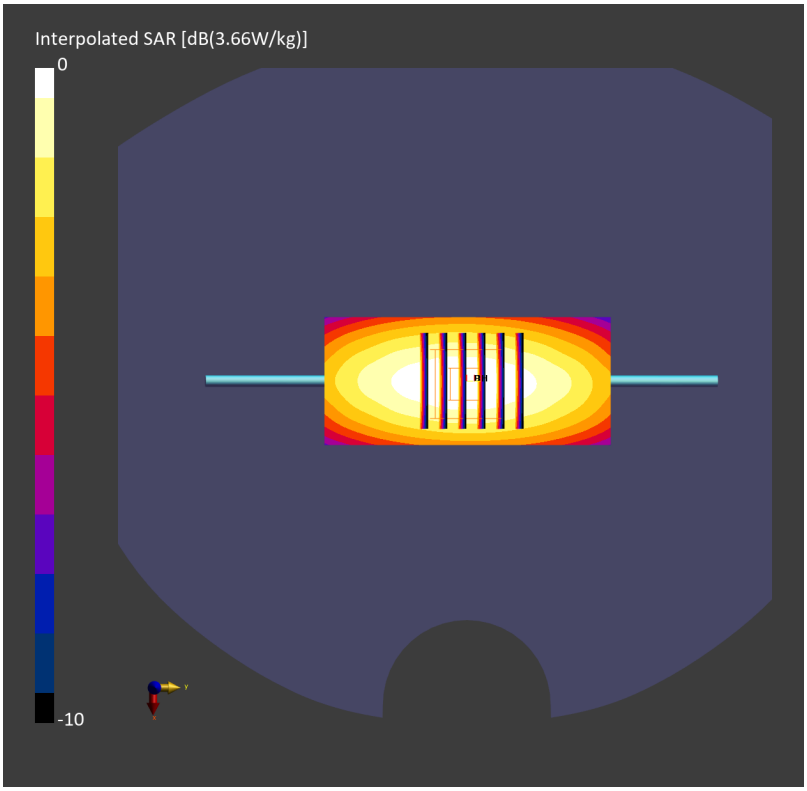

Date: 2026-01-18

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260118 Medium parameters used: f= 835.000 MHz; σ= 0.928 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.27, 9.12, 9.17); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.48 W/kg; SAR (10g) = 1.63 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.04 dB
SAR (1g) = 2.46 W/kg; SAR (8g) = 1.70 W/kg; SAR (10g) = 1.62 W/kg
Smallest distance from peaks to all points 3 dB below = 19.7 mm
Ratio of SAR at M2 to SAR at M1 = 87.9 %
TSL Correction: Positive only

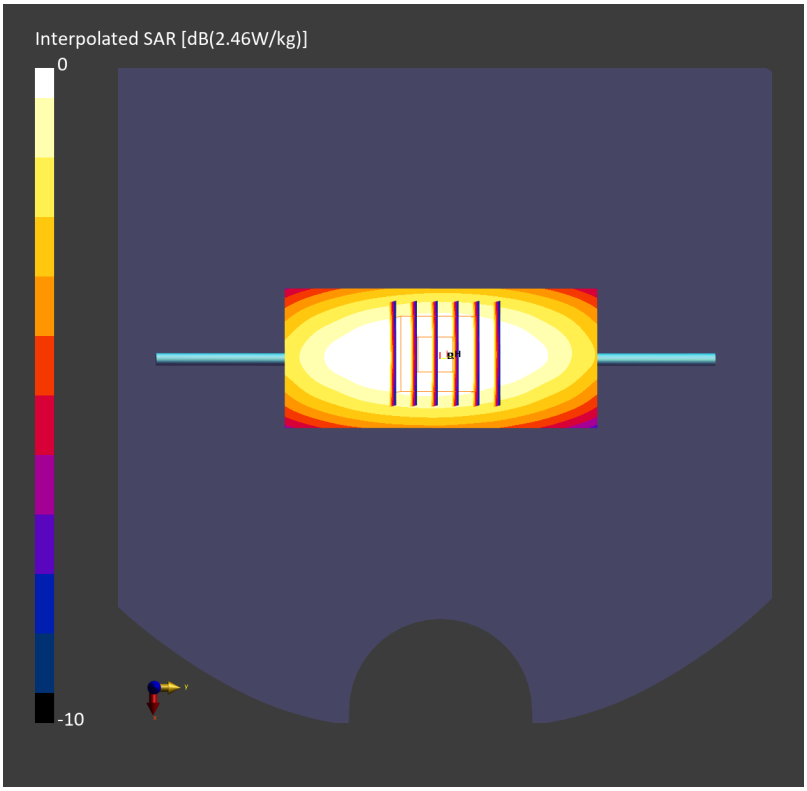

Date: 2026-01-19

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260119 Medium parameters used: f= 835.000 MHz; σ= 0.942 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(9.27, 9.12, 9.17); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.52 W/kg; SAR (10g) = 1.67 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.53 W/kg; SAR (8g) = 1.75 W/kg; SAR (10g) = 1.66 W/kg
Smallest distance from peaks to all points 3 dB below = 17.8 mm
Ratio of SAR at M2 to SAR at M1 = 87.7 %
TSL Correction: Positive only

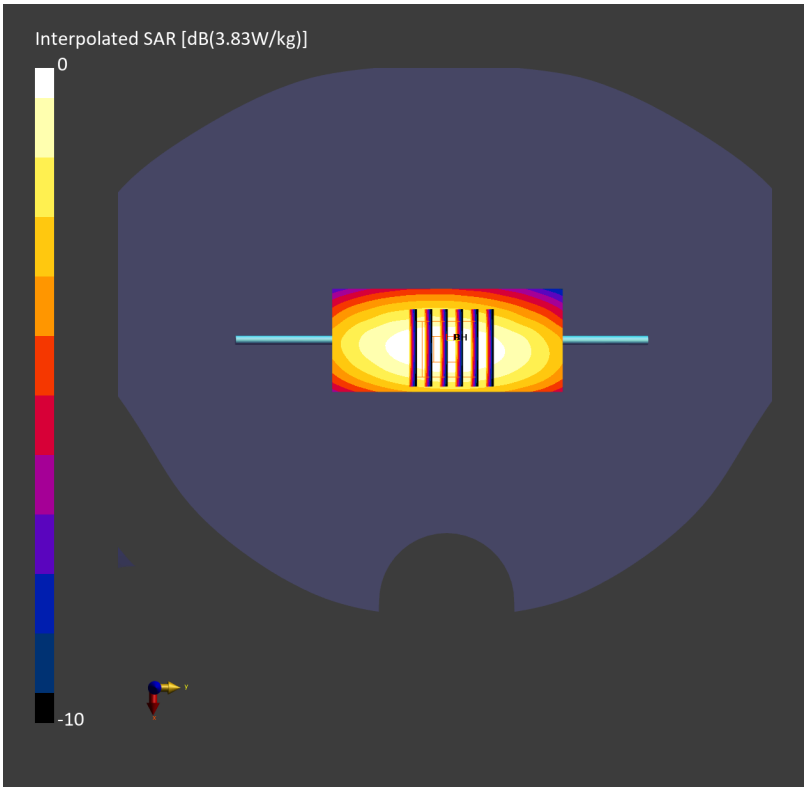

Date: 2026-02-06

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260206 Medium parameters used: f= 835.000 MHz; σ= 0.914 S/m; $\varepsilon_r$ = 42.4
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.42 W/kg; SAR (10g) = 1.59 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 2.43 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.60 W/kg
Smallest distance from peaks to all points 3 dB below = 18.4 mm
Ratio of SAR at M2 to SAR at M1 = 88.2 %
TSL Correction: Positive only

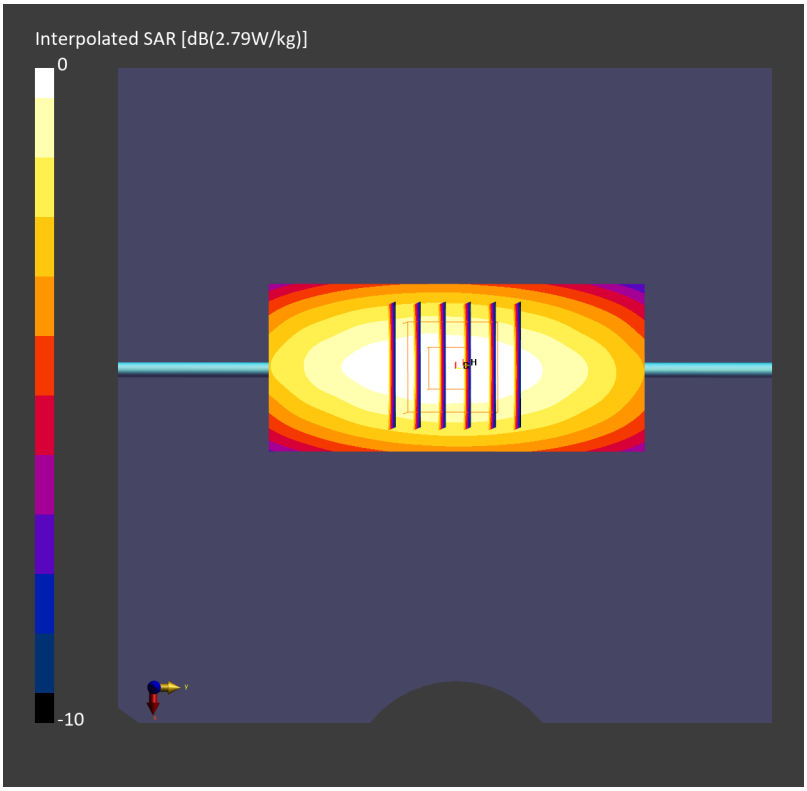

Date: 2026-02-11

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260211 Medium parameters used: f= 835.000 MHz; σ= 0.939 S/m; $\varepsilon_r$ = 42.6
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.48 W/kg; SAR (10g) = 1.63 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.48 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.64 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 88.9 %
TSL Correction: Positive only

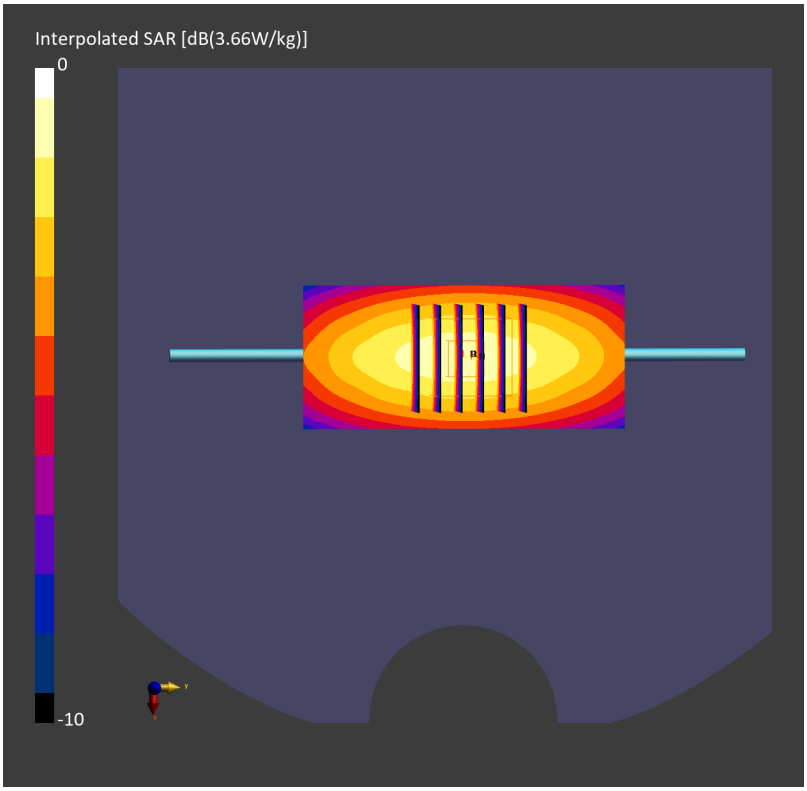

Date: 2026-02-20

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260220 Medium parameters used: f= 835.000 MHz; σ= 0.915 S/m; $\varepsilon_r$ = 42.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.63 W/kg; SAR (10g) = 1.67 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 2.57 W/kg; SAR (8g) = 1.70 W/kg; SAR (10g) = 1.60 W/kg
Smallest distance from peaks to all points 3 dB below = 13.2 mm
Ratio of SAR at M2 to SAR at M1 = 85.4 %
TSL Correction: Positive only

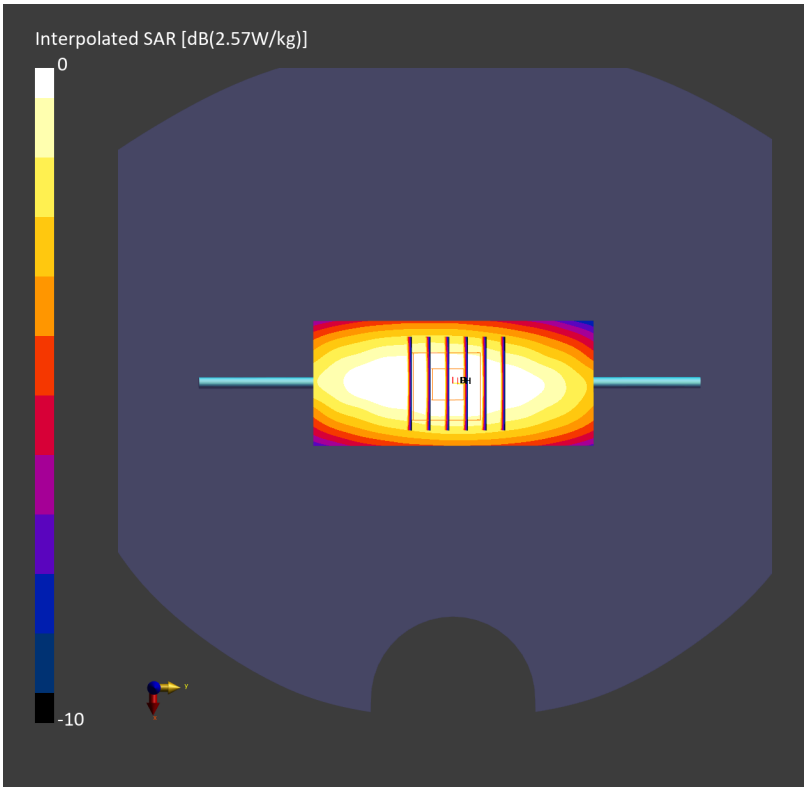

Date: 2026-03-02

**System Check_Head 835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260302 Medium parameters used: f= 835.000 MHz; σ= 0.921 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(9.56, 9.14, 10.17); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.39 W/kg; SAR (10g) = 1.57 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.38 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.57 W/kg
Smallest distance from peaks to all points 3 dB below = 21.3 mm
Ratio of SAR at M2 to SAR at M1 = 86.9 %
TSL Correction: Positive only

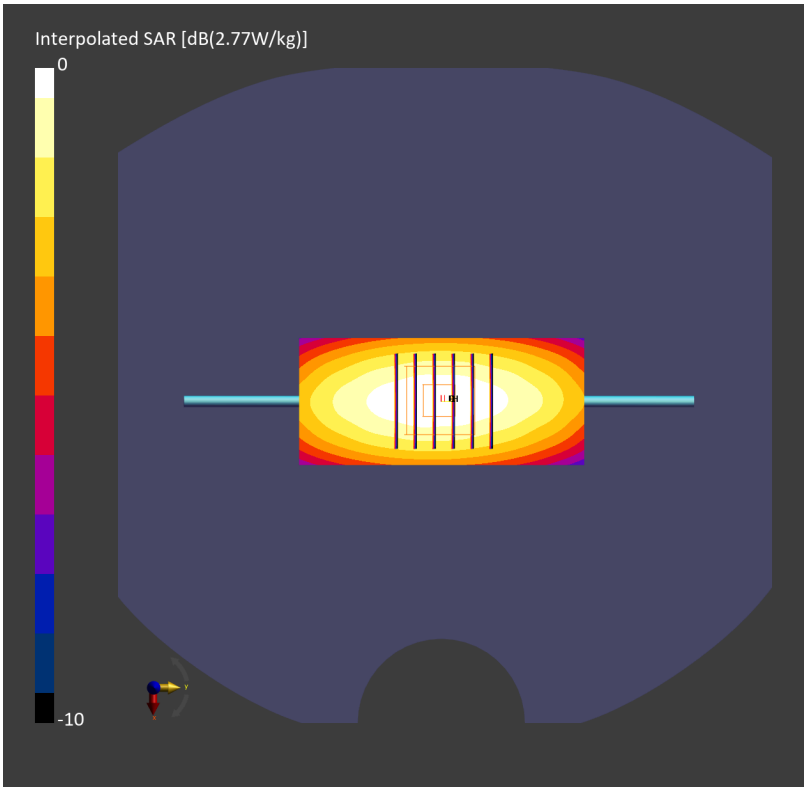

Date: 2026-03-11

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260311 Medium parameters used: f= 835.000 MHz; σ= 0.923 S/m; $\varepsilon_r$ = 42.1
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.46 W/kg; SAR (10g) = 1.62 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.44 W/kg; SAR (8g) = 1.70 W/kg; SAR (10g) = 1.62 W/kg
Smallest distance from peaks to all points 3 dB below = 16.8 mm
Ratio of SAR at M2 to SAR at M1 = 88.9 %
TSL Correction: Positive only

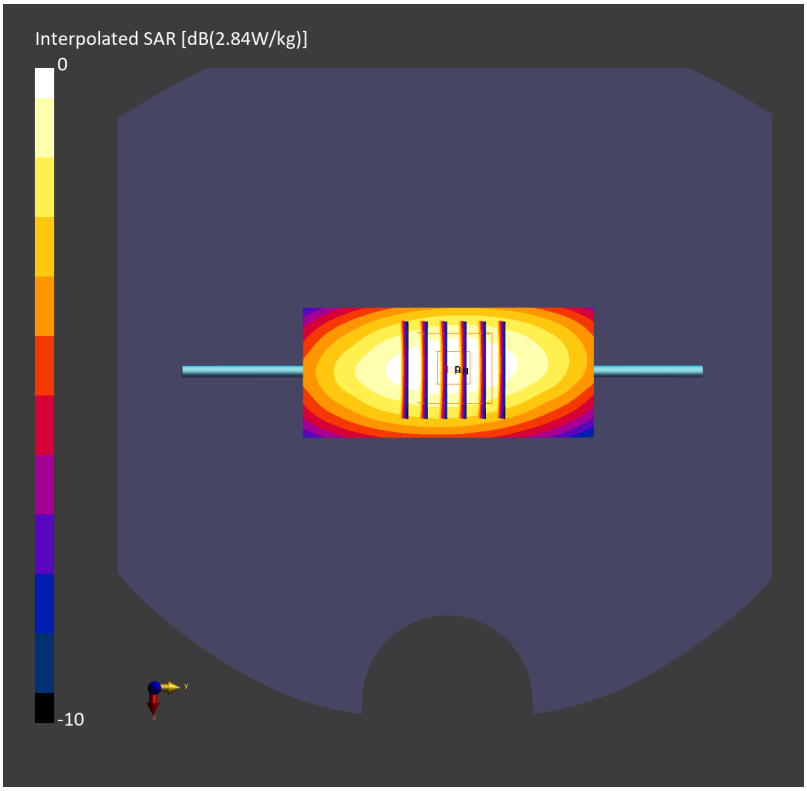

Date: 2026-03-12

**System Check_Head 835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 835.000 MHz; σ= 0.914 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(9.56, 9.14, 10.17); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.40 W/kg; SAR (10g) = 1.59 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 2.41 W/kg; SAR (8g) = 1.68 W/kg; SAR (10g) = 1.59 W/kg
Smallest distance from peaks to all points 3 dB below = 17.2 mm
Ratio of SAR at M2 to SAR at M1 = 87.2 %
TSL Correction: Positive only

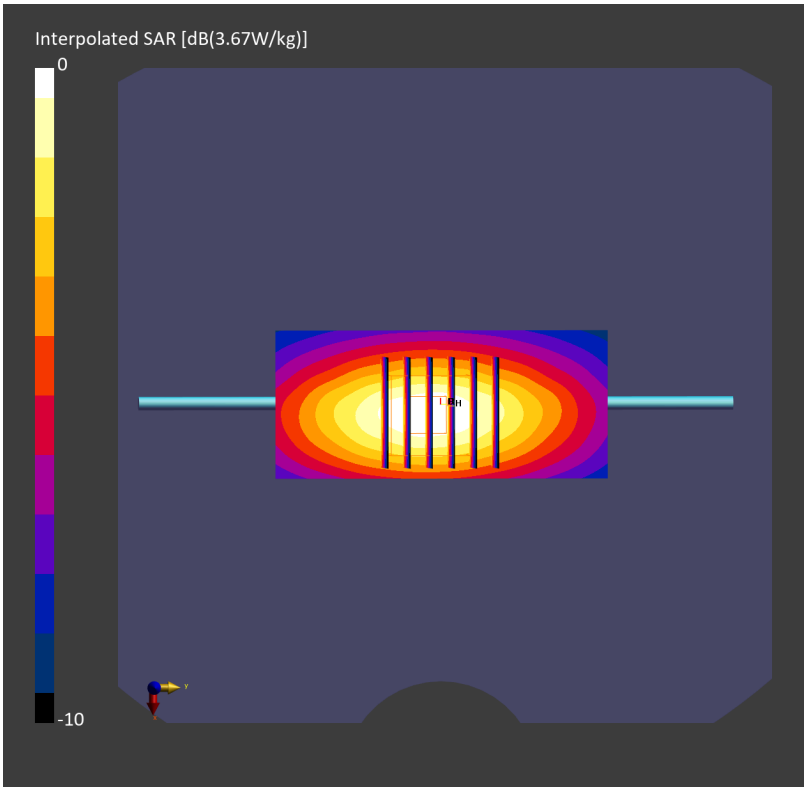

Date: 2026-03-14

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260314 Medium parameters used: f= 835.000 MHz; σ= 0.912 S/m; $\varepsilon_r$ = 42.0
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.38 W/kg; SAR (10g) = 1.56 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.37 W/kg; SAR (8g) = 1.66 W/kg; SAR (10g) = 1.57 W/kg
Smallest distance from peaks to all points 3 dB below = 19.0 mm
Ratio of SAR at M2 to SAR at M1 = 89.3 %
TSL Correction: Positive only

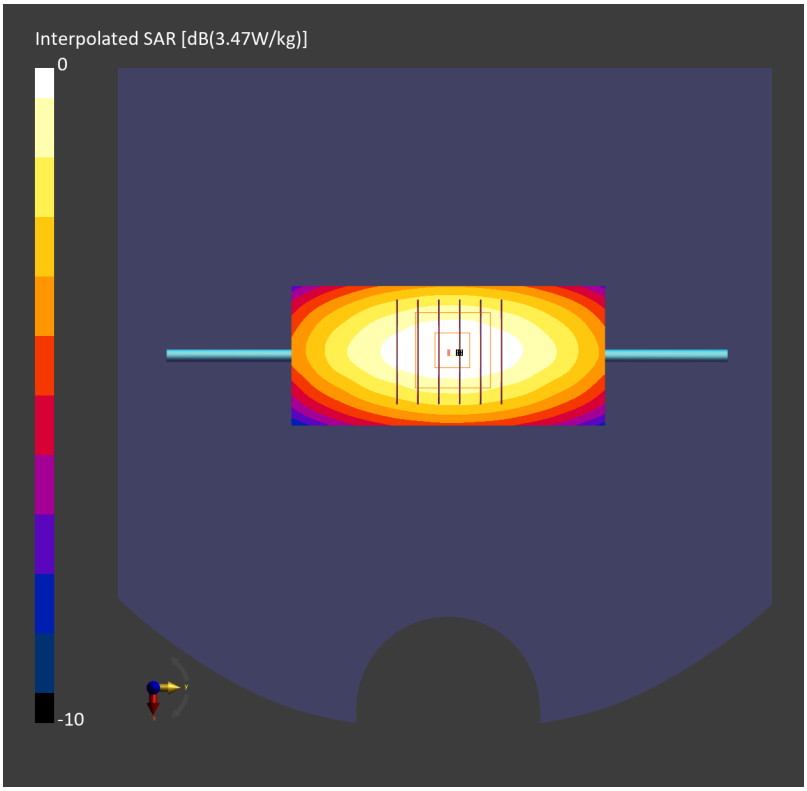

Date: 2026-03-24

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260324 Medium parameters used: f= 835.000 MHz; σ= 0.924 S/m; $\varepsilon_r$ = 44.8
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.55 W/kg; SAR (10g) = 1.67 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.55 W/kg; SAR (8g) = 1.76 W/kg; SAR (10g) = 1.67 W/kg
Smallest distance from peaks to all points 3 dB below = 17.8 mm
Ratio of SAR at M2 to SAR at M1 = 87.8 %
TSL Correction: Positive only

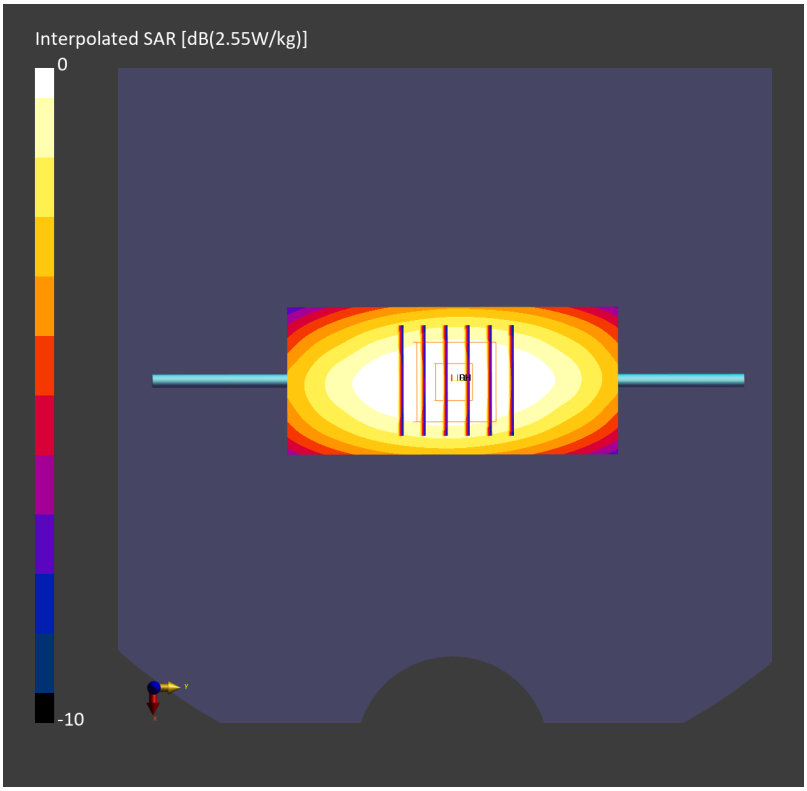

Date: 2026-03-28

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260328 Medium parameters used: f= 835.000 MHz; σ= 0.940 S/m; $\varepsilon_r$ = 42.0
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.59 W/kg; SAR (10g) = 1.70 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.38 W/kg; SAR (8g) = 1.72 W/kg; SAR (10g) = 1.59 W/kg
Smallest distance from peaks to all points 3 dB below = 16.7 mm
Ratio of SAR at M2 to SAR at M1 = 87.4 %
TSL Correction: Positive only

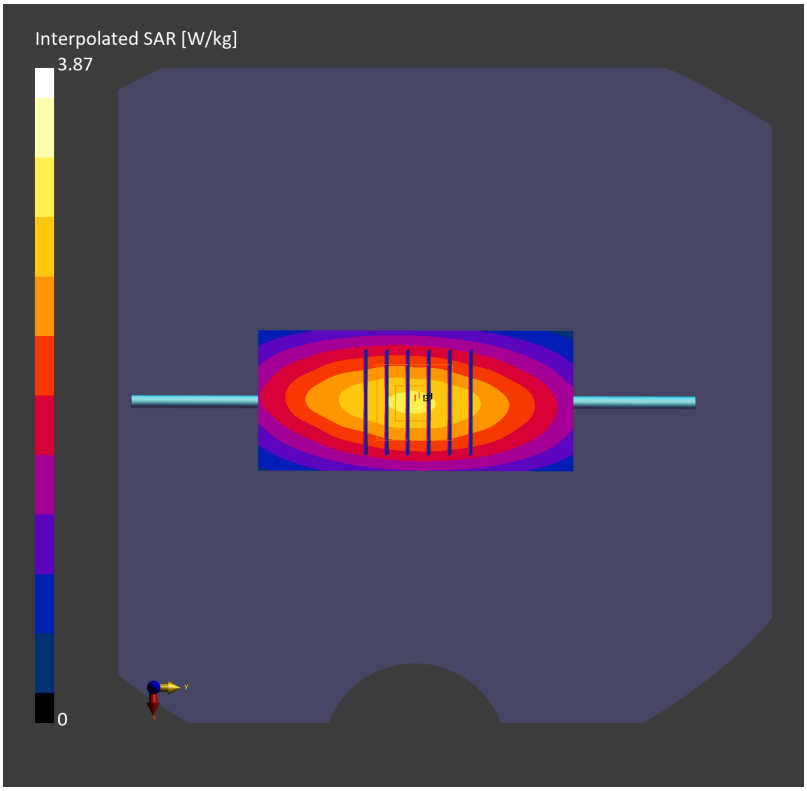

Date: 2026-04-05

**System Check_Head_835MHz**

**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_600-7200_260405 Medium parameters used: f= 835.000 MHz; σ= 0.901 S/m; $\varepsilon_r$ = 44.9
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN3728; ConvF(8.84, 8.67, 8.94); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.41 W/kg; SAR (10g) = 1.57 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.39 W/kg; SAR (8g) = 1.63 W/kg; SAR (10g) = 1.54 W/kg
Smallest distance from peaks to all points 3 dB below = 15.8 mm
Ratio of SAR at M2 to SAR at M1 = 88.1 %
TSL Correction: Positive only

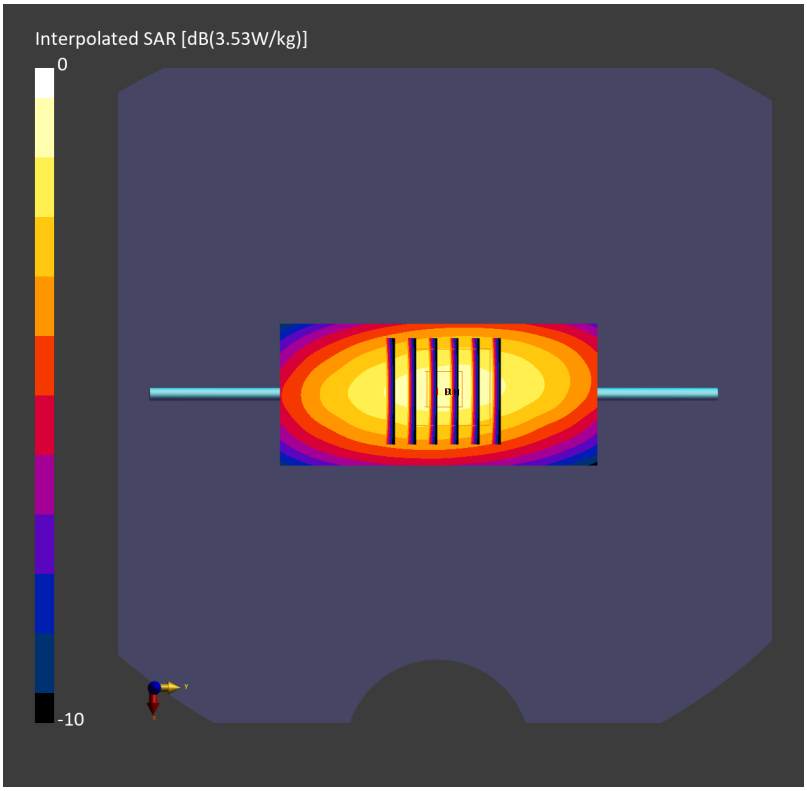

Date: 2026-03-21

**System Check_Head_1640MHz**

**DUT: D1640V2 - SN346**

Communication System: CW; Frequency: 1640.000 MHz
Medium: HSL_600-7200_260321 Medium parameters used: f= 1640.000 MHz; σ= 1.30 S/m; $\varepsilon_r$ = 43.0
Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.34, 7.33, 7.0); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.70 W/kg; SAR (10g) = 0.923 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 1.68 W/kg; SAR (8g) = 0.979 W/kg; SAR (10g) = 0.905 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 85.1 %
TSL Correction: Positive only

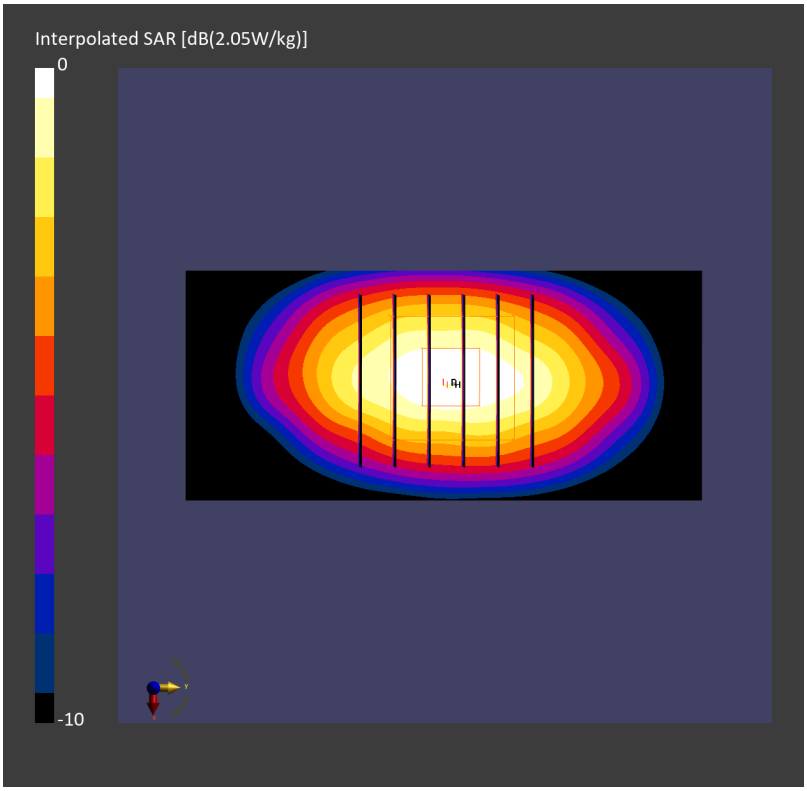

Date: 2026-04-08

**System Check_Head_1640MHz**

**DUT: D1640V2 - SN346**

Communication System: CW; Frequency: 1640.000 MHz
Medium: HSL_600-7200_260408 Medium parameters used: f= 1640.000 MHz; σ= 1.26 S/m; $\varepsilon_r$ = 43.6
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.34, 7.33, 7.0); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.72 W/kg; SAR (10g) = 0.920 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.70 W/kg; SAR (8g) = 0.985 W/kg; SAR (10g) = 0.911 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.8 %
TSL Correction: Positive only

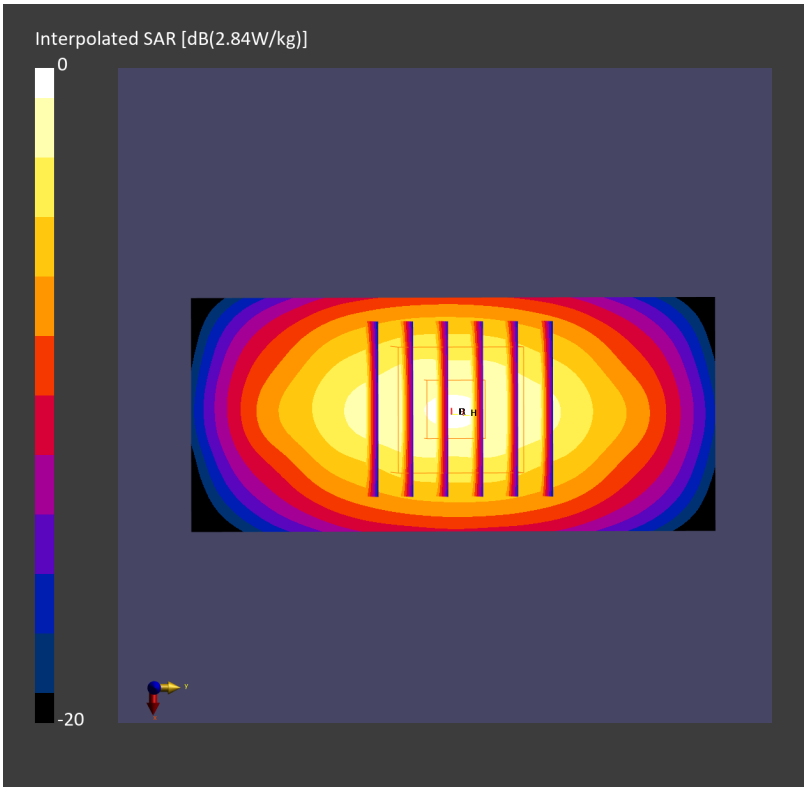

Date: 2026-01-03

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260103 Medium parameters used: f= 1750.000 MHz; σ= 1.35 S/m; $\varepsilon_r$ = 43.4
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.82 W/kg; SAR (10g) = 0.968 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.82 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.960 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.7 %
TSL Correction: Positive only

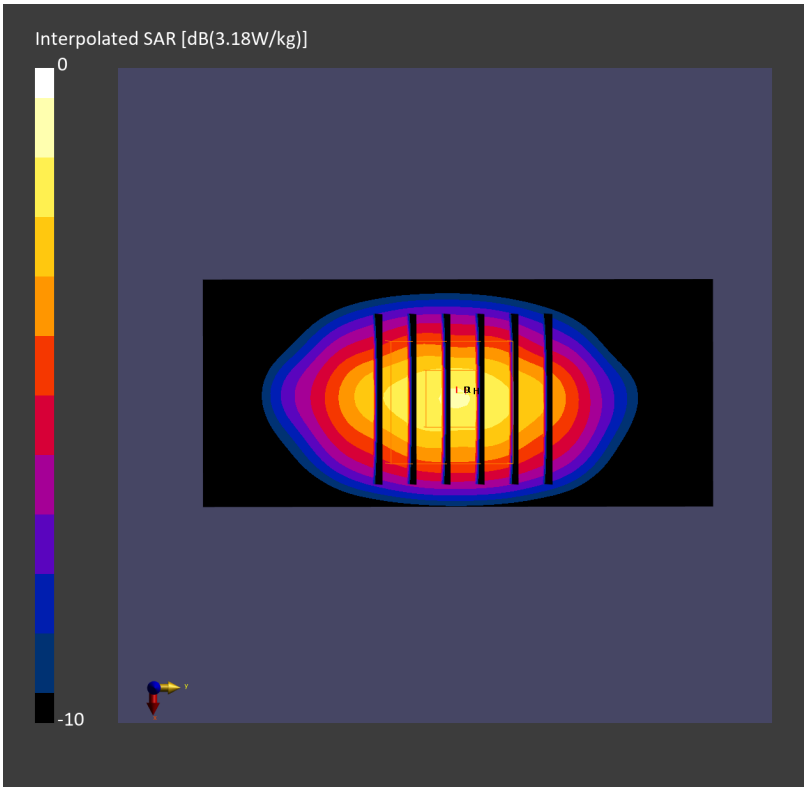

Date: 2026-01-05

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260105 Medium parameters used: f= 1750.000 MHz; σ= 1.33 S/m; $\varepsilon_r$ = 40.4
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.76 W/kg; SAR (10g) = 0.936 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 1.76 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.929 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 84.0 %
TSL Correction: Positive only

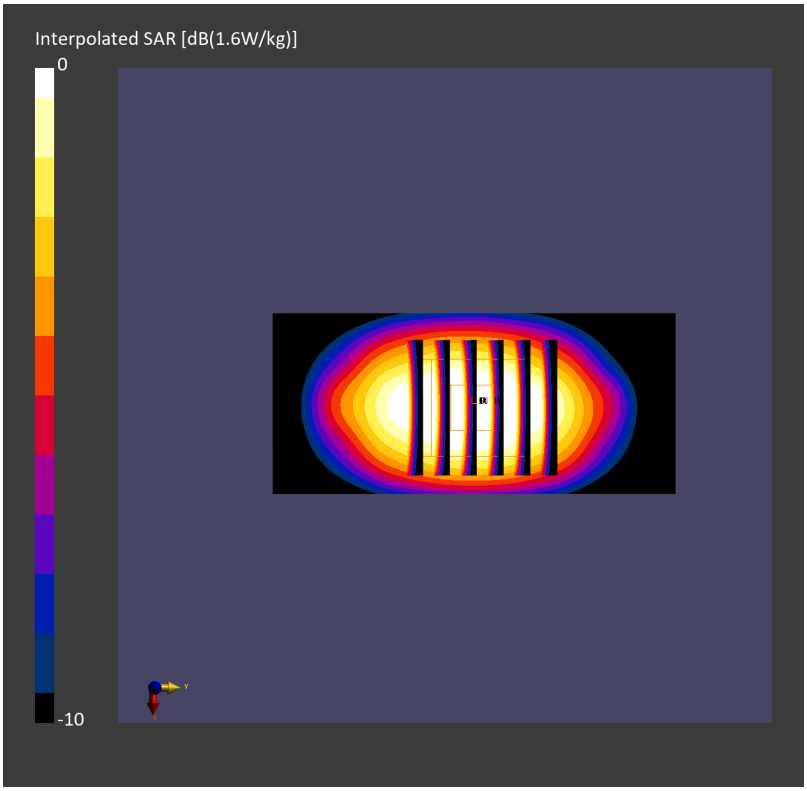

Date: 2026-01-06

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260106 Medium parameters used: f= 1750.000 MHz; σ= 1.36 S/m; $\varepsilon_r$ = 41.4
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.85 W/kg; SAR (10g) = 0.983 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 1.82 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.963 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 82.9 %
TSL Correction: Positive only

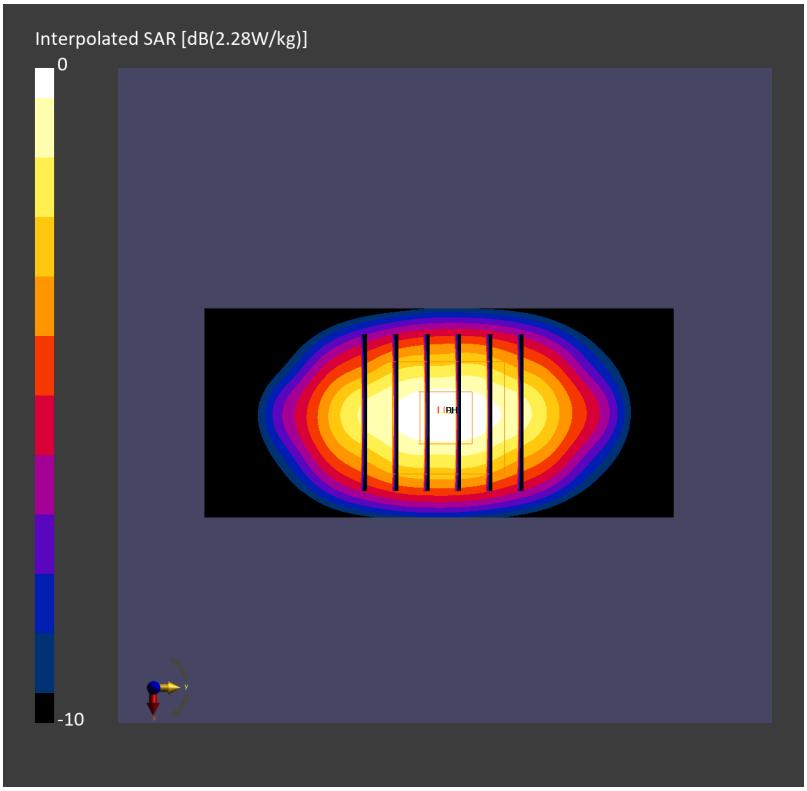

Date: 2026-01-07

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260107 Medium parameters used: f= 1750.000 MHz; σ= 1.38 S/m; $\varepsilon_r$ = 41.0
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.86 W/kg; SAR (10g) = 0.988 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.82 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.968 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.0 %
TSL Correction: Positive only

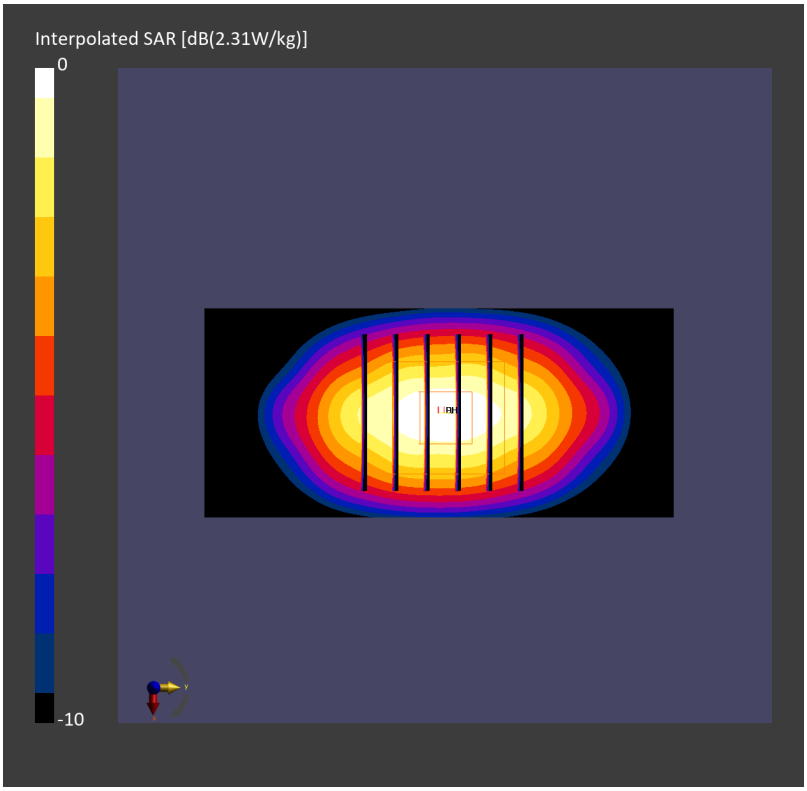

Date: 2026-01-13

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260113 Medium parameters used: f= 1750.000 MHz; σ= 1.38 S/m; $\varepsilon_r$ = 41.0
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.85 W/kg; SAR (10g) = 0.989 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.82 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.965 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 84.0 %
TSL Correction: Positive only

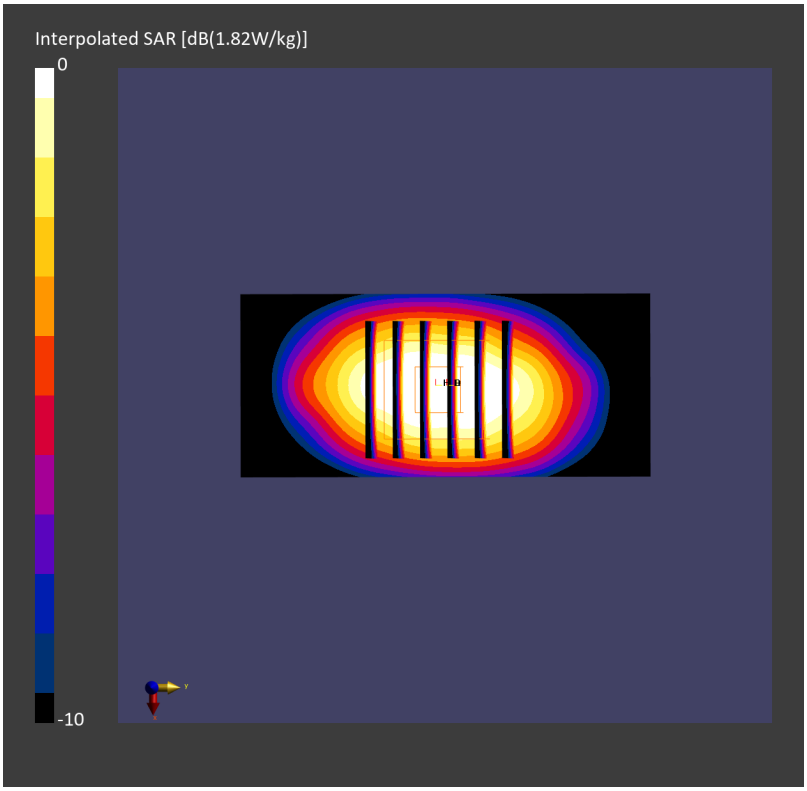

Date: 2026-01-20

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260120 Medium parameters used: f= 1750.000 MHz; $\sigma$= 1.35 S/m; $\varepsilon_r$ = 40.7
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.82 W/kg; SAR (10g) = 0.970 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.80 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.952 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.5 %
TSL Correction: Positive only

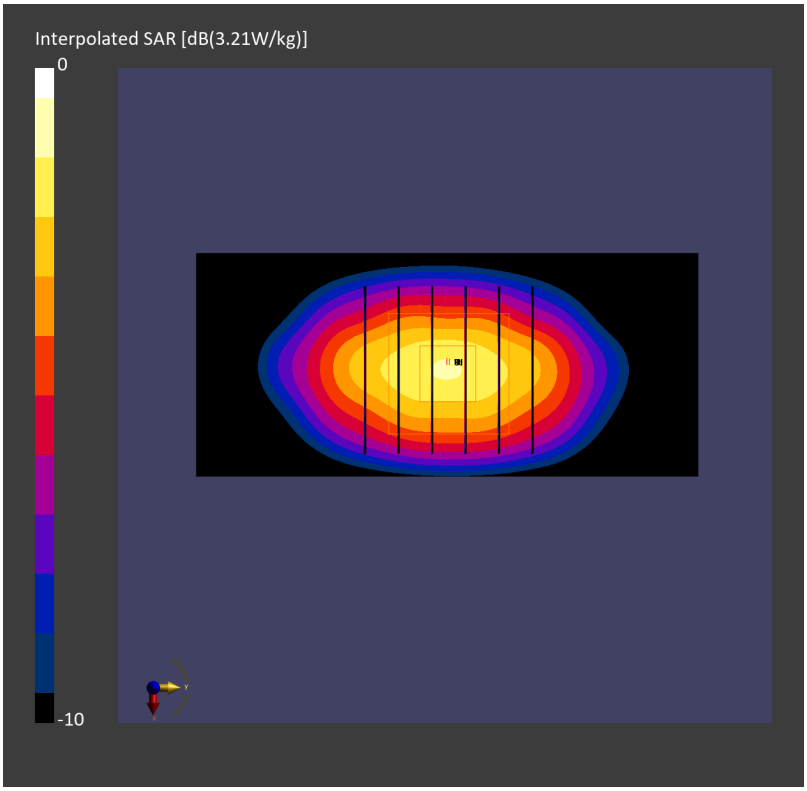

Date: 2026-02-10

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260210 Medium parameters used: f= 1750.000 MHz; σ= 1.38 S/m; $\varepsilon_r$ = 40.8
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 9.11 W/kg; SAR (10g) = 4.87 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 9.00 W/kg; SAR (8g) = 5.23 W/kg; SAR (10g) = 4.83 W/kg
Smallest distance from peaks to all points 3 dB below = 9.7 mm
Ratio of SAR at M2 to SAR at M1 = 85.4 %
TSL Correction: Positive only

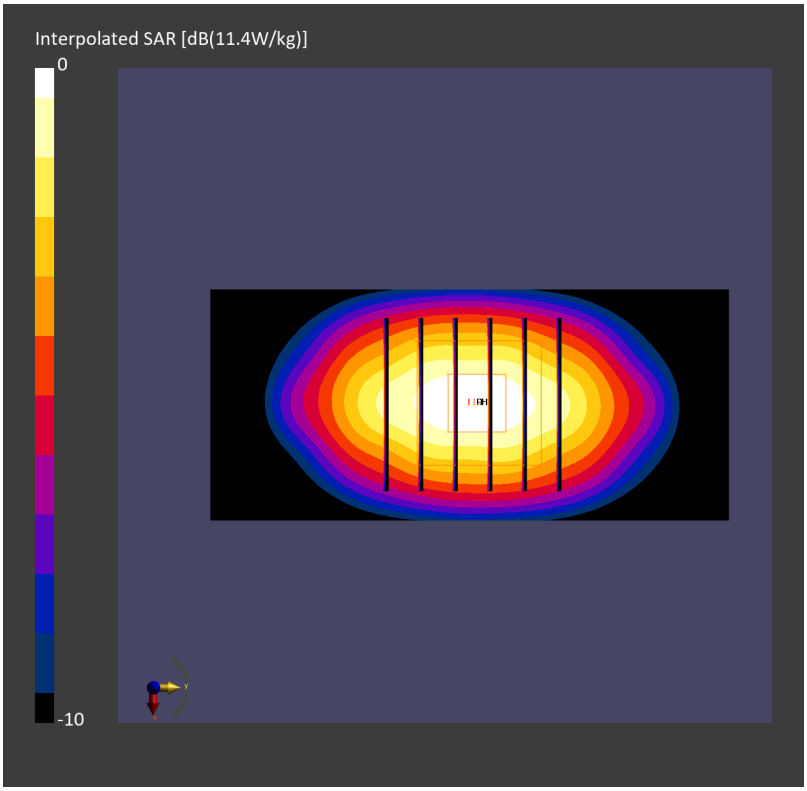

Date: 2026-02-18

**System Check_Head_1750MHz_260218**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 1750.000 MHz; $\sigma$= 1.35 S/m; $\varepsilon_r$ = 40.4
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.79 W/kg; SAR (10g) = 0.953 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 1.76 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.937 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.5 %
TSL Correction: Positive only

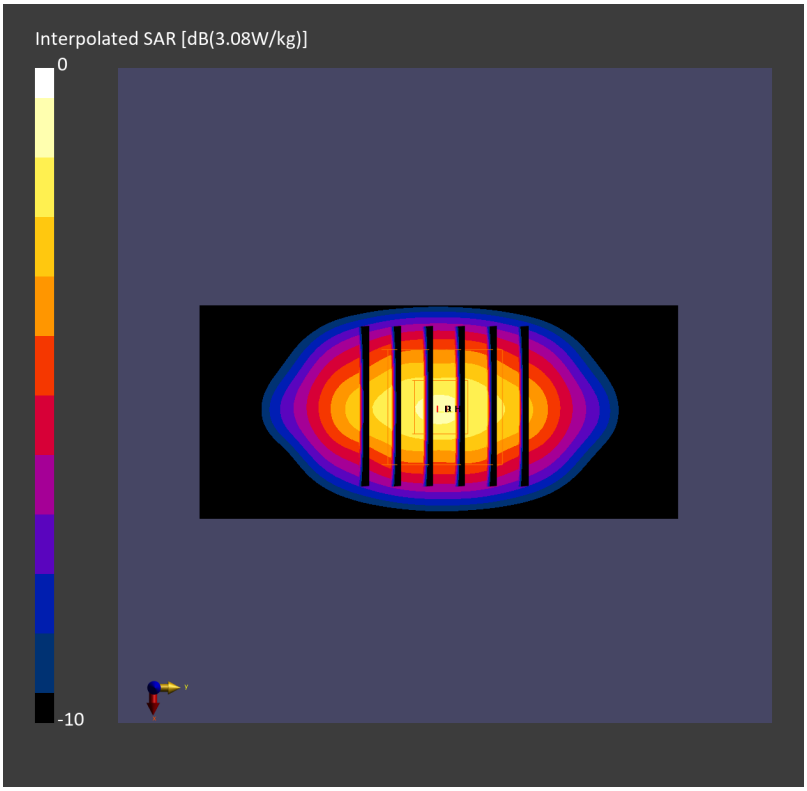

Date: 2026-02-23

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 1750.000 MHz; σ= 1.36 S/m; $\varepsilon_r$ = 40.7
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.78 W/kg; SAR (10g) = 0.971 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.79 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.950 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 84.0 %
TSL Correction: Positive only

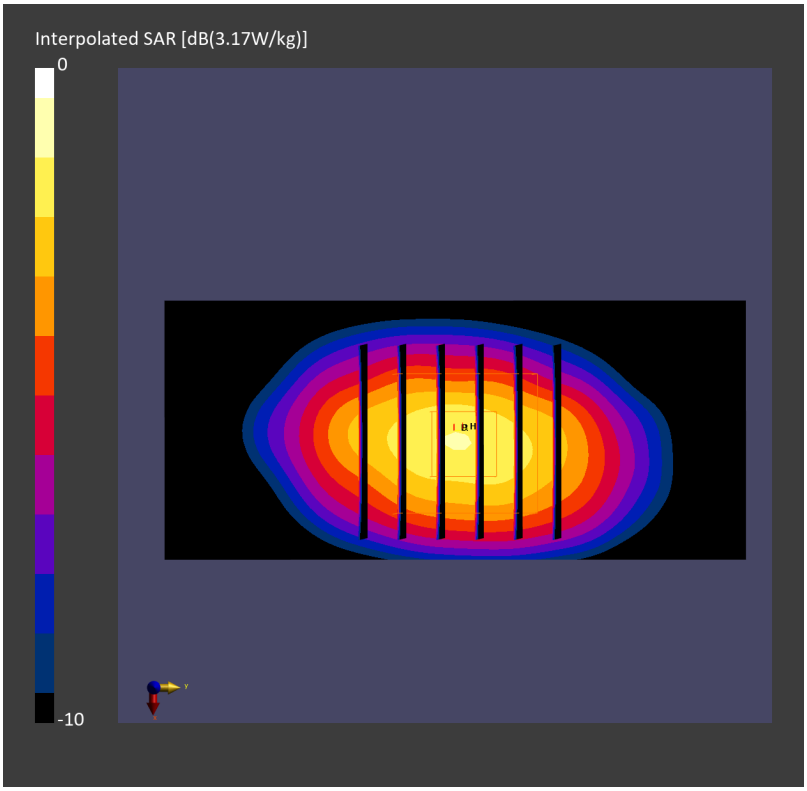

Date: 2026-02-26

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260226 Medium parameters used: f= 1750.000 MHz; $\sigma$= 1.31 S/m; $\varepsilon_r$ = 43.1
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.96, 7.83, 7.88); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.81 W/kg; SAR (10g) = 0.952 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.78 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.935 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.6 %
TSL Correction: Positive only

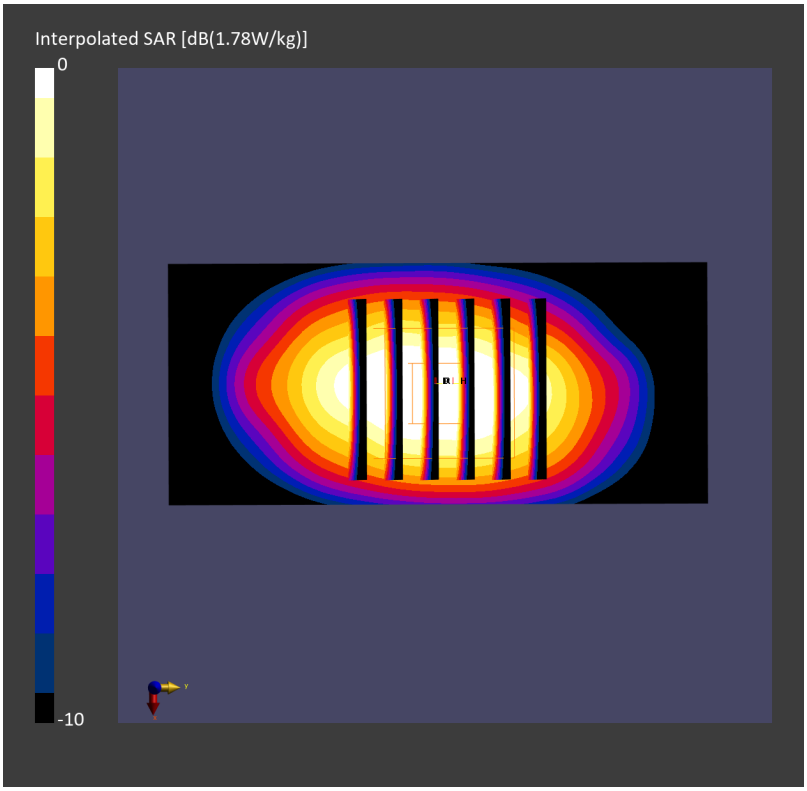

Date: 2026-03-10

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260310 Medium parameters used: f= 1750.000 MHz; σ= 1.34 S/m; $\varepsilon_r$ = 40.2
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.79 W/kg; SAR (10g) = 0.954 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.78 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.949 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 85.1 %
TSL Correction: Positive only

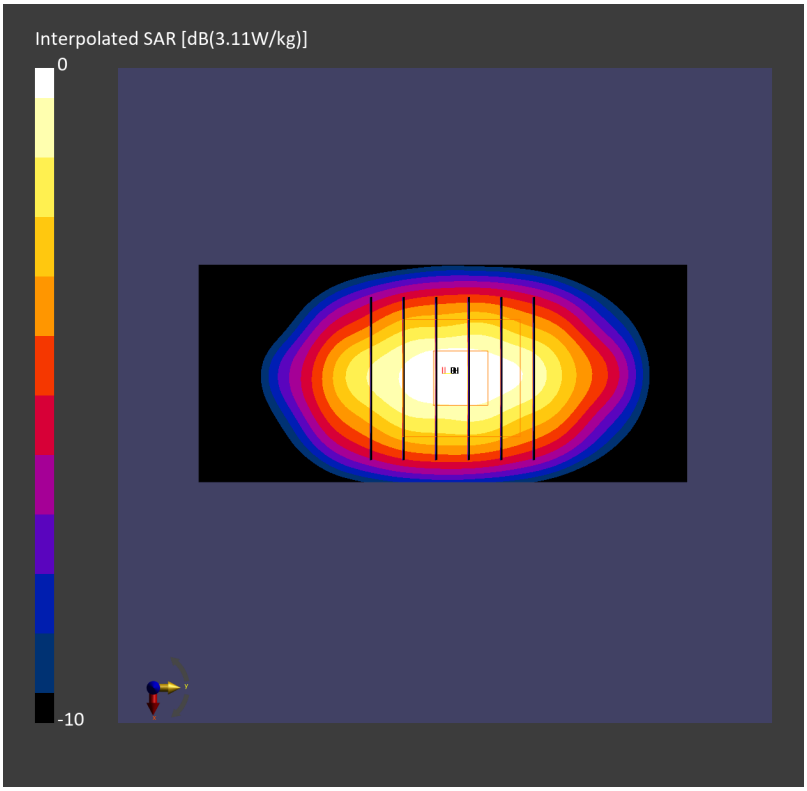

Date: 2026-03-12

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 1750.000 MHz; σ= 1.37 S/m; $\varepsilon_r$ = 40.8
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.77 W/kg; SAR (10g) = 0.944 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 1.75 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.935 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 85.3 %
TSL Correction: Positive only

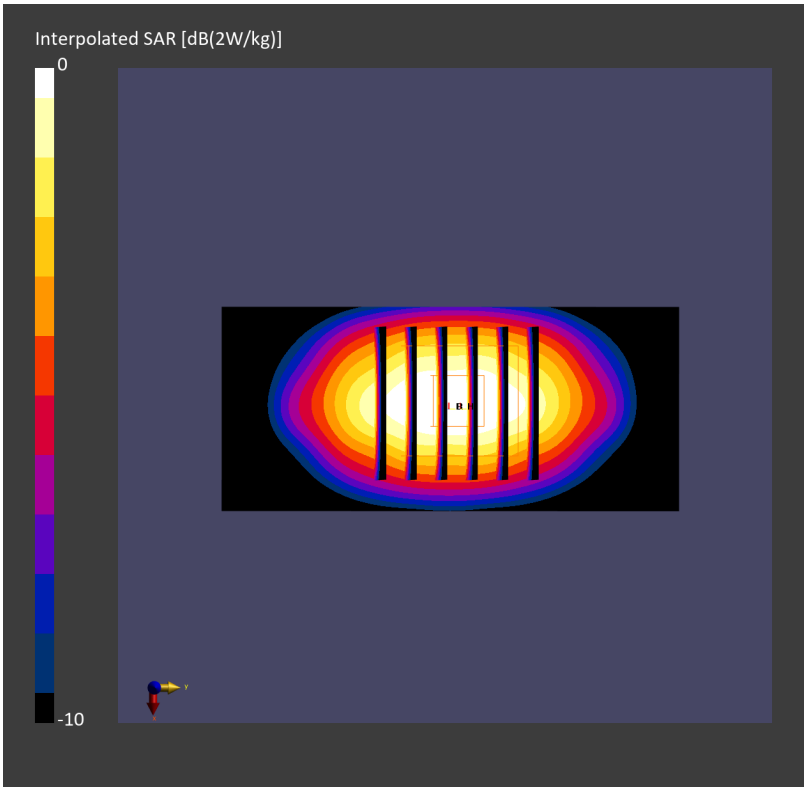

Date: 2026-03-12

**System Check_Head 1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 1750.000 MHz; σ= 1.35 S/m; $\varepsilon_r$ = 40.8
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(7.9, 7.56, 8.41); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.77 W/kg; SAR (10g) = 0.938 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.04 dB
SAR (1g) = 1.77 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.940 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 83.3 %
TSL Correction: Positive only

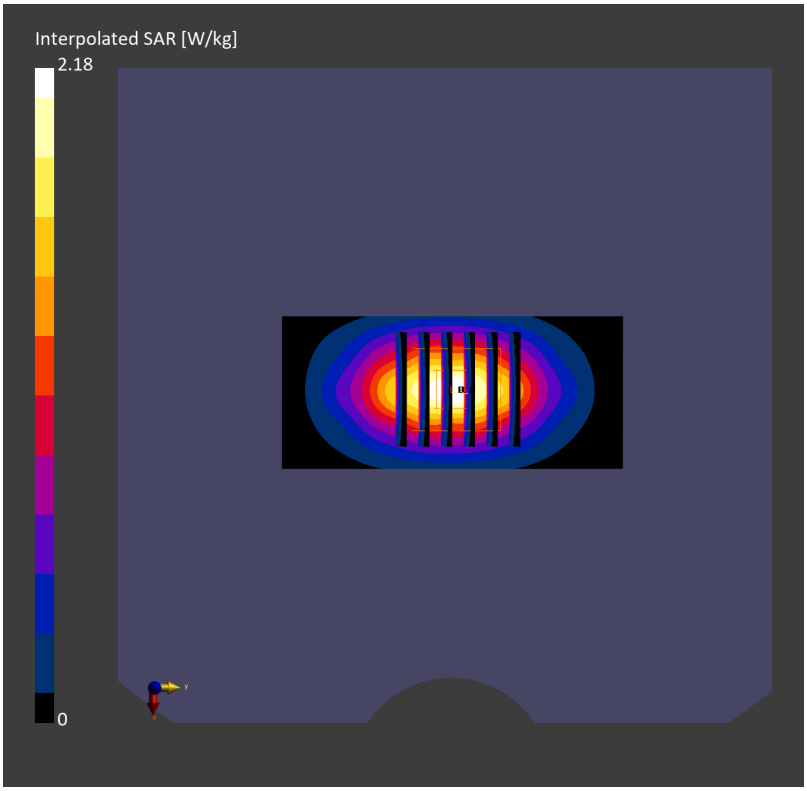

Date: 2026-03-17

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260317 Medium parameters used: f= 1750.000 MHz; σ= 1.38 S/m; $\varepsilon_r$ = 40.1
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.77 W/kg; SAR (10g) = 0.965 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.79 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.959 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 84.5 %
TSL Correction: Positive only

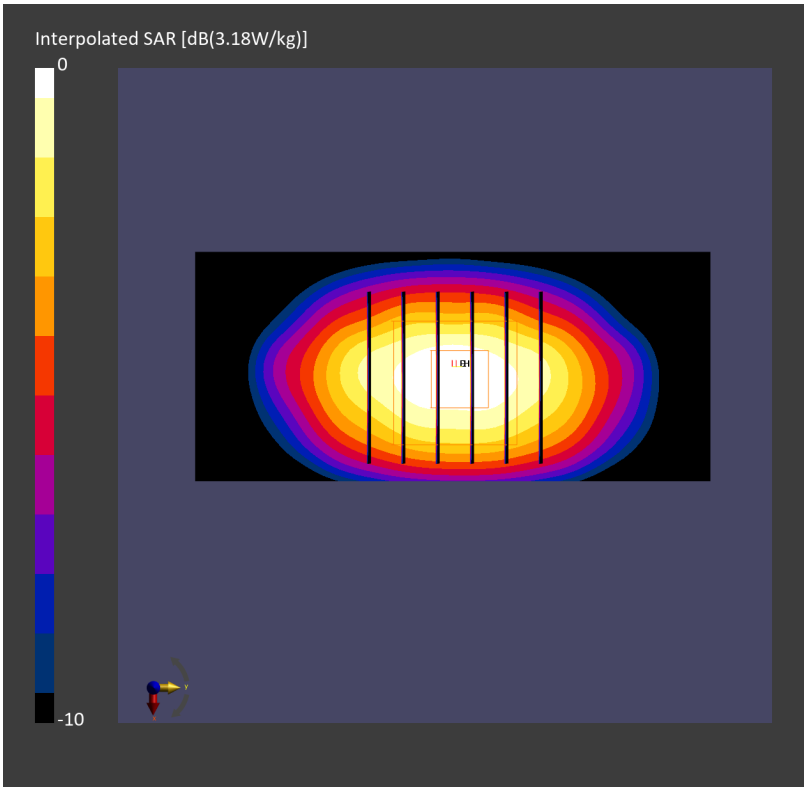

Date: 2026-03-28

**System Check_Head_1750MHz**

**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_600-7200_260328 Medium parameters used: f= 1750.000 MHz; σ= 1.39 S/m; $\varepsilon_r$ = 40.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.84 W/kg; SAR (10g) = 0.979 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 1.80 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.962 W/kg
Smallest distance from peaks to all points 3 dB below = 9.9 mm
Ratio of SAR at M2 to SAR at M1 = 83.4 %
TSL Correction: Positive only

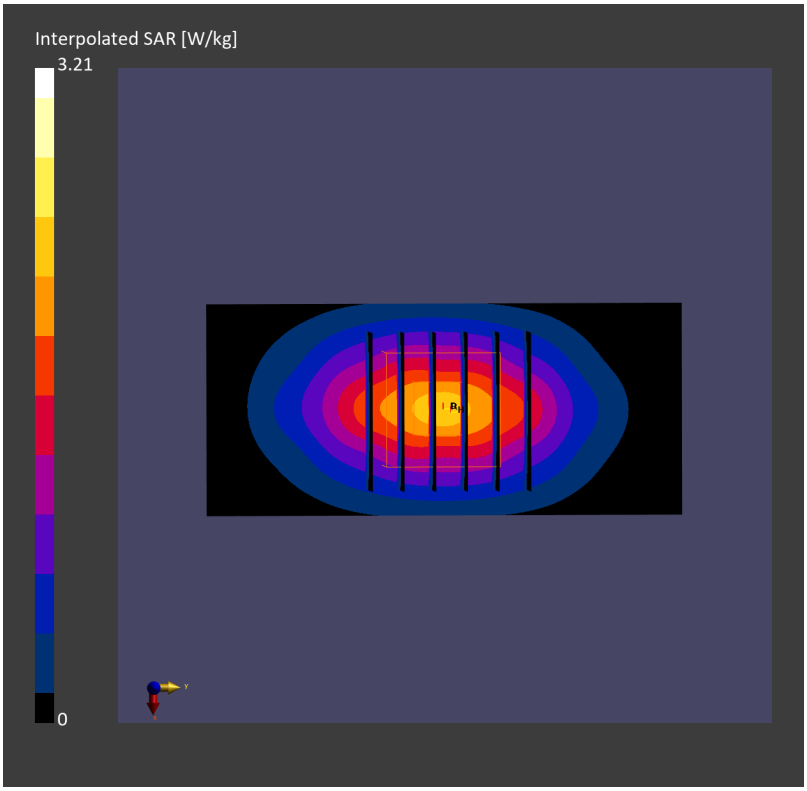

Date: 2026-01-03

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260103 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.44 S/m; $\varepsilon_r$ = 43.2
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.86 W/kg; SAR (10g) = 0.979 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.88 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.985 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 82.2 %
TSL Correction: Positive only

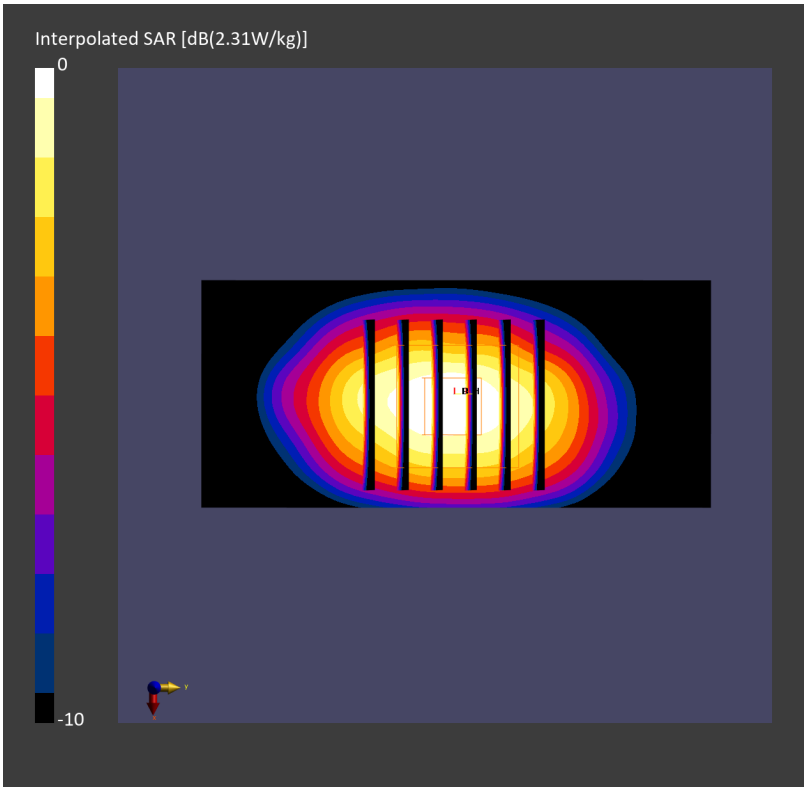

Date: 2026-01-05

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260105 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.41 S/m; $\varepsilon_r$ = 40.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.95 W/kg; SAR (10g) = 1.01 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.93 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.997 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 83.3 %
TSL Correction: Positive only

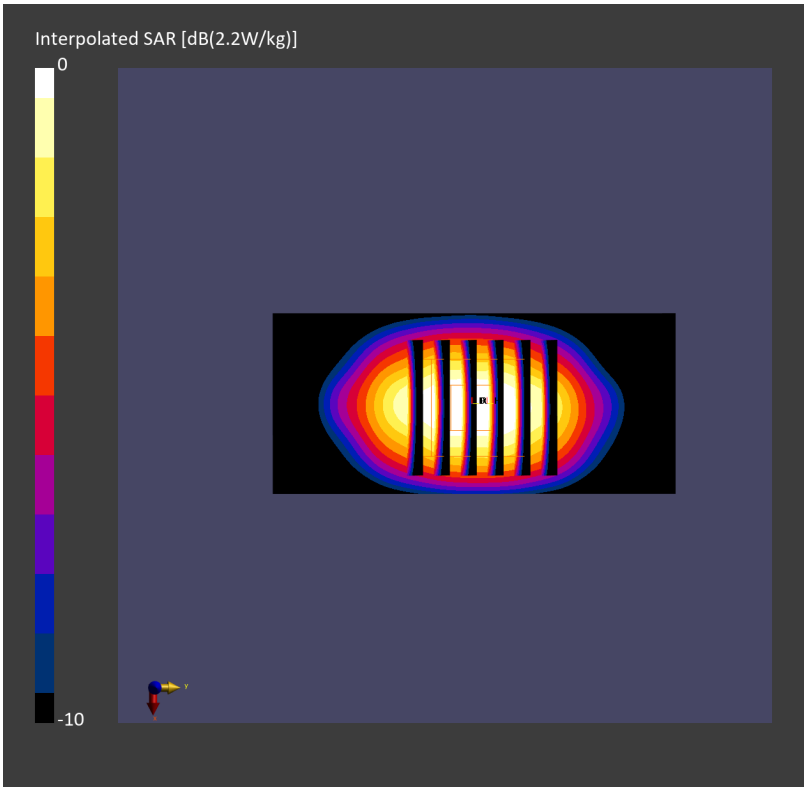

Date: 2026-01-07

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260107 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.45 S/m; $\varepsilon_r$ = 40.7
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.06 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.03 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 83.4 %
TSL Correction: Positive only

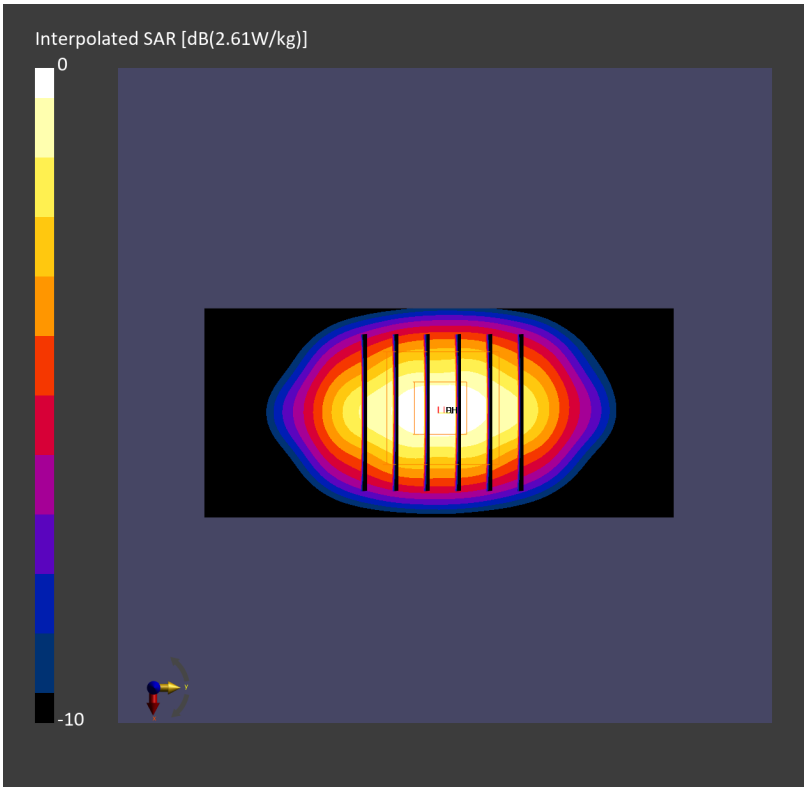

Date: 2026-01-13

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260113 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.45 S/m; $\varepsilon_r$ = 40.8
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.06 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.04 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg
Smallest distance from peaks to all points 3 dB below = 9.7 mm
Ratio of SAR at M2 to SAR at M1 = 82.9 %
TSL Correction: Positive only

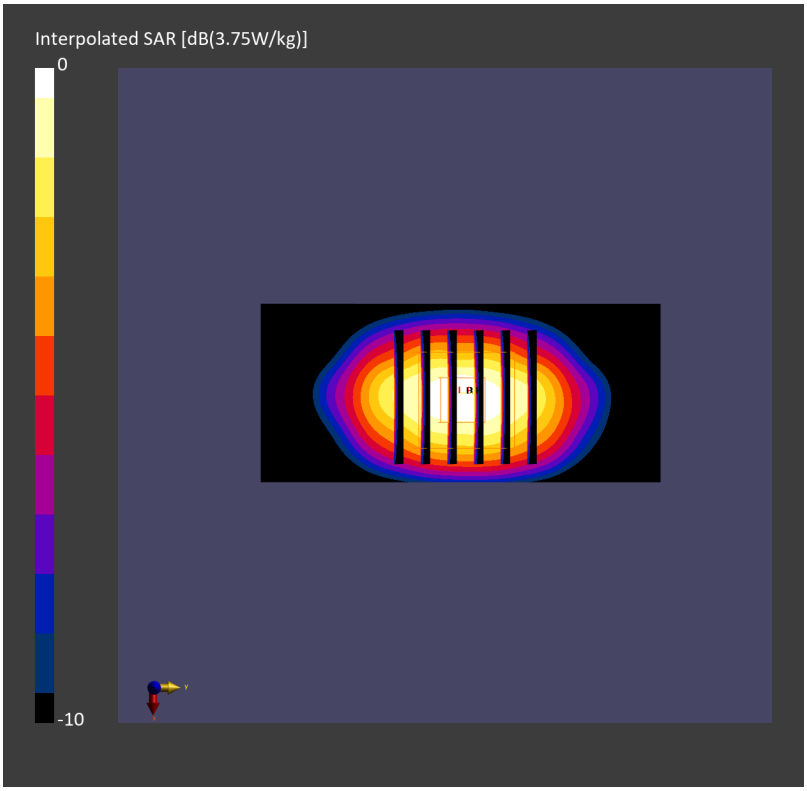

Date: 2026-01-18

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260118 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.45 S/m; $\varepsilon_r$ = 40.5
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.07 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.02 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg
Smallest distance from peaks to all points 3 dB below = 9.9 mm
Ratio of SAR at M2 to SAR at M1 = 83.6 %
TSL Correction: Positive only

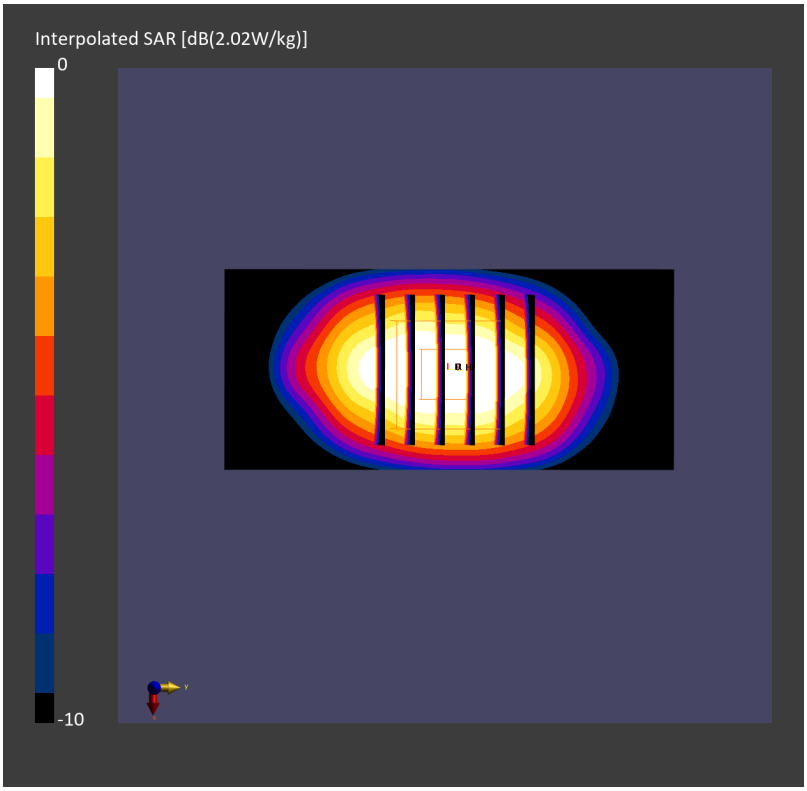

Date: 2026-01-20

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260120 Medium parameters used: f= 1900.000 MHz; σ= 1.43 S/m; $\varepsilon_r$ = 40.4
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.02 W/kg; SAR (10g) = 1.05 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.00 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 82.9 %
TSL Correction: Positive only

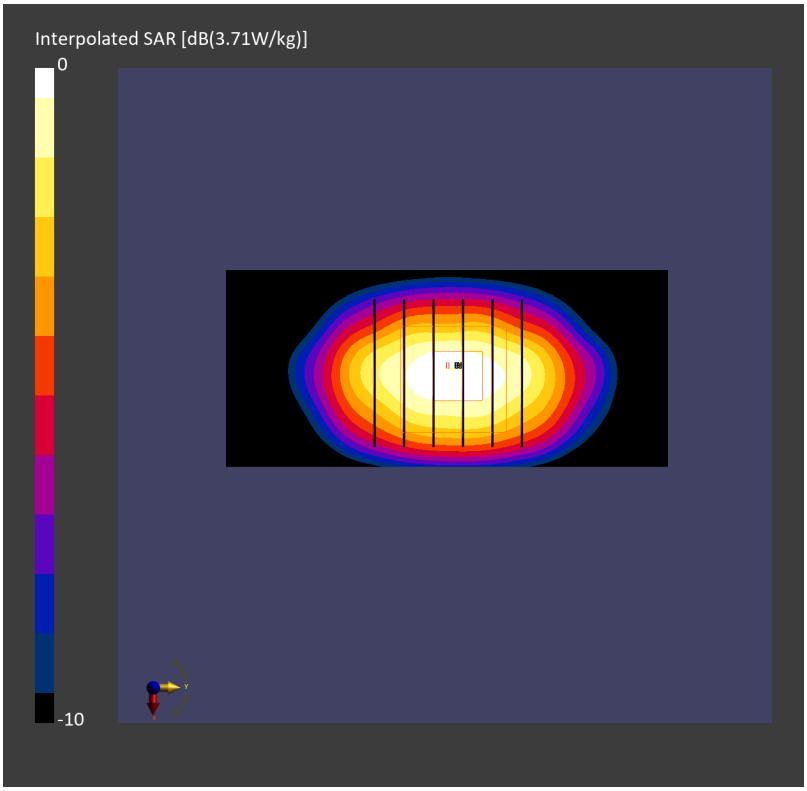

Date: 2026-02-10

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260210 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.46 S/m; $\varepsilon_r$ = 40.6
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 10.5 W/kg; SAR (10g) = 5.44 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 10.4 W/kg; SAR (8g) = 5.90 W/kg; SAR (10g) = 5.43 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 85.1 %
TSL Correction: Positive only

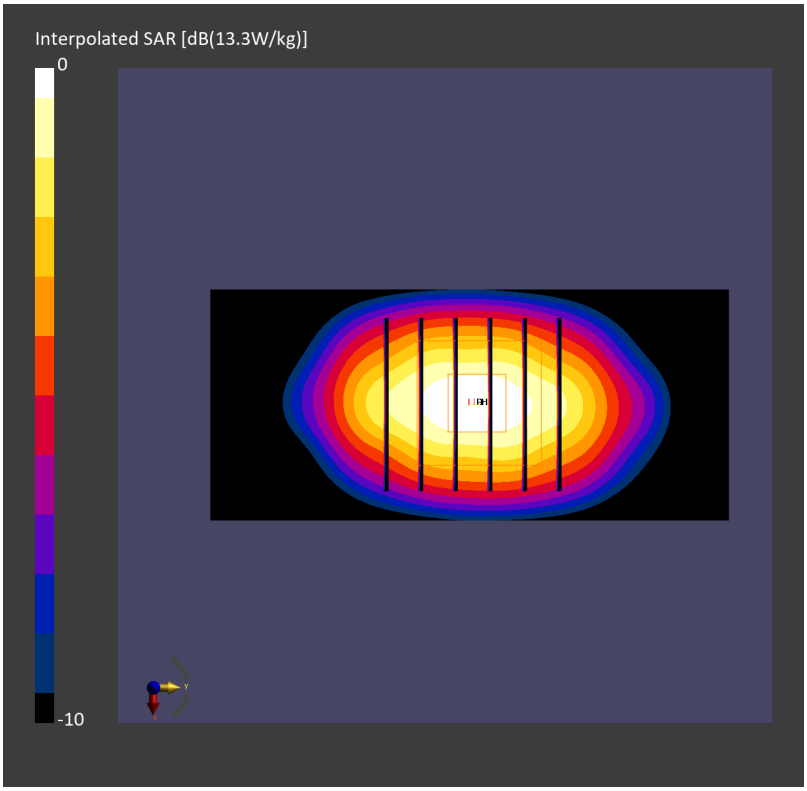

Date: 2026-02-18

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 1900.000 MHz; σ= 1.42 S/m; $\varepsilon_r$ = 40.1
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 10.7 W/kg; SAR (10g) = 5.61 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 10.5 W/kg; SAR (8g) = 5.95 W/kg; SAR (10g) = 5.47 W/kg
Smallest distance from peaks to all points 3 dB below = 9.7 mm
Ratio of SAR at M2 to SAR at M1 = 84.8 %
TSL Correction: Positive only

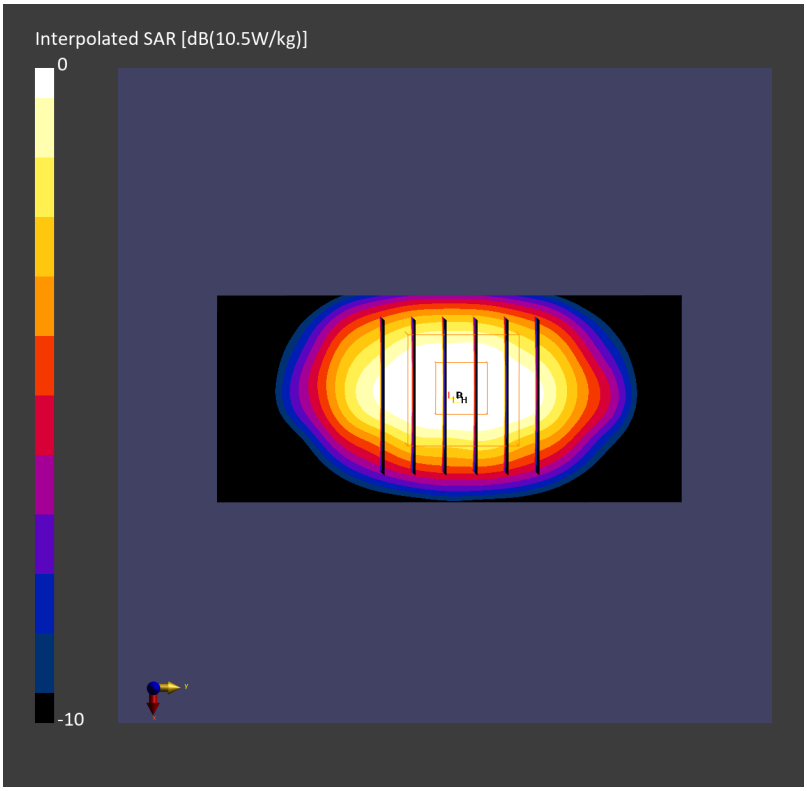

Date: 2026-02-23

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.44 S/m; $\varepsilon_r$ = 40.4
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.03 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.04 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 82.9 %
TSL Correction: Positive only

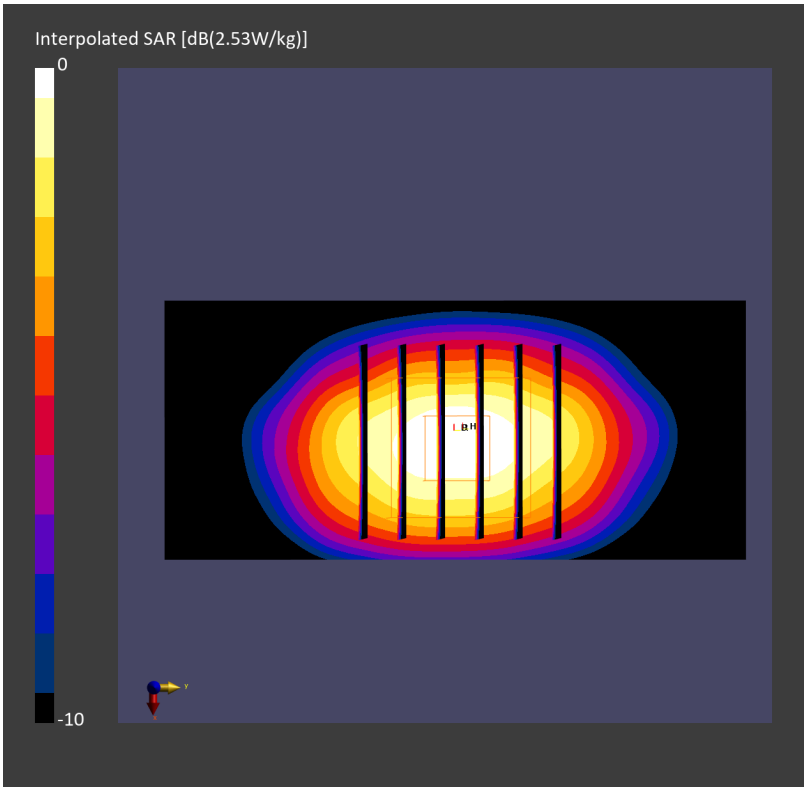

Date: 2026-02-26

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260226 Medium parameters used: f= 1900.000 MHz; σ= 1.40 S/m; $\varepsilon_r$ = 42.8
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.64, 7.52, 7.56); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.96 W/kg; SAR (10g) = 1.01 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.95 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 83.9 %
TSL Correction: Positive only

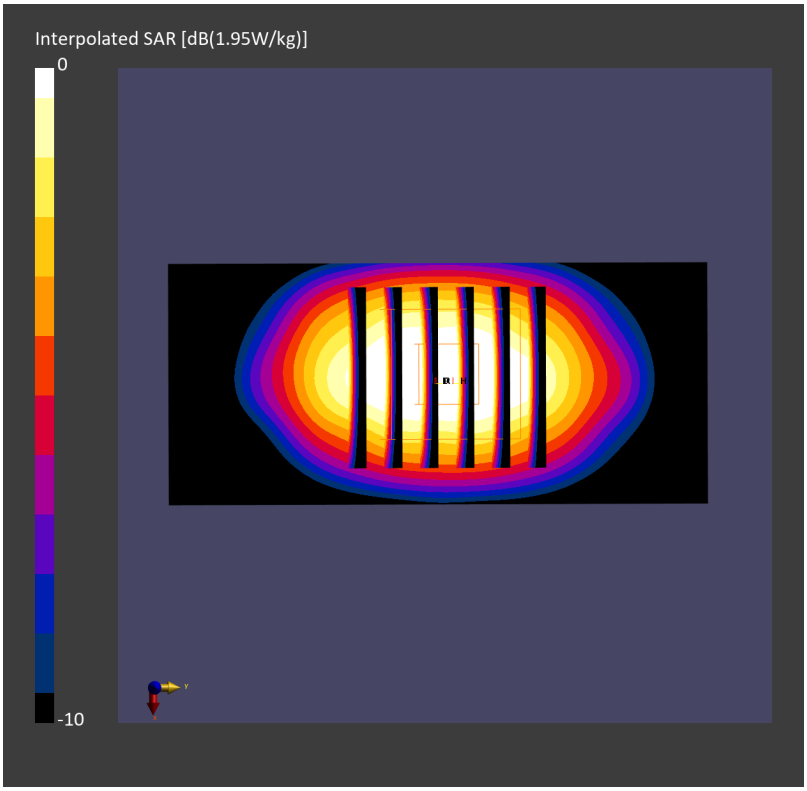

Date: 2026-03-03

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260303 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.43 S/m; $\varepsilon_r$ = 40.3
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.07 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.04 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 84.1 %
TSL Correction: Positive only

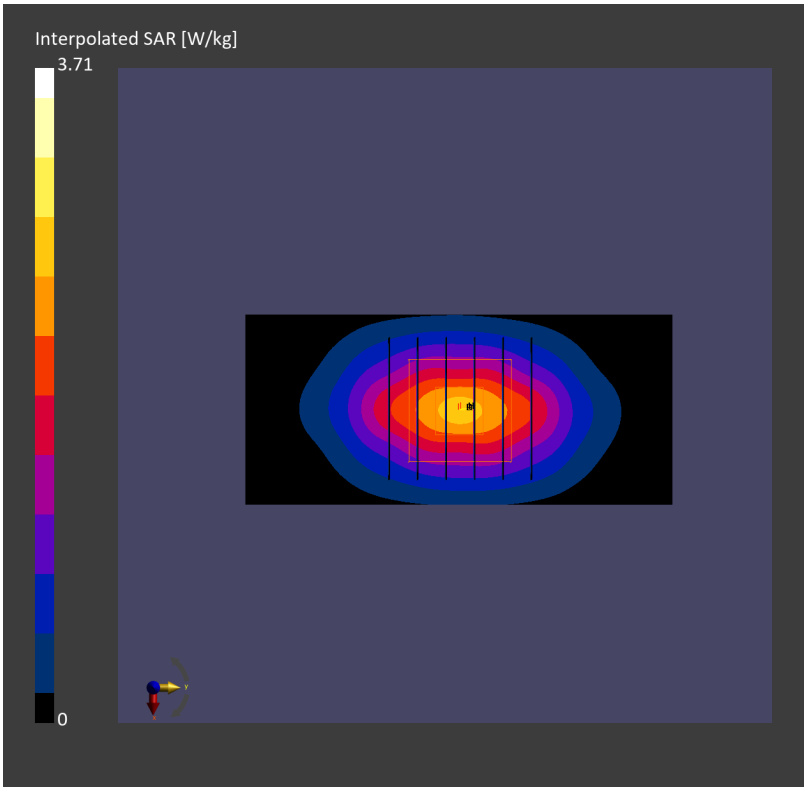

Date: 2026-03-06

**System Check_Head 1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260306 Medium parameters used: f= 1900.000 MHz; σ= 1.45 S/m; $\varepsilon_r$ = 40.6
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(7.54, 7.21, 8.01); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.00 W/kg; SAR (10g) = 1.04 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.99 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 82.5 %
TSL Correction: Positive only

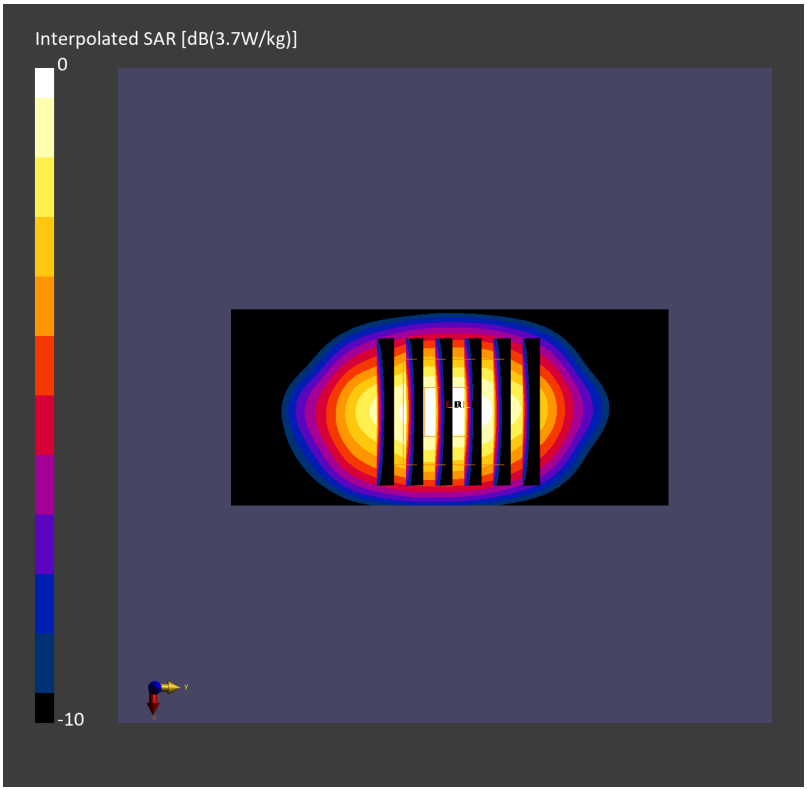

Date: 2026-03-10

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260310 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.42 S/m; $\varepsilon_r$ = 40.0
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.02 W/kg; SAR (10g) = 1.05 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 2.02 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg
Smallest distance from peaks to all points 3 dB below = 9.7 mm
Ratio of SAR at M2 to SAR at M1 = 83.9 %
TSL Correction: Positive only

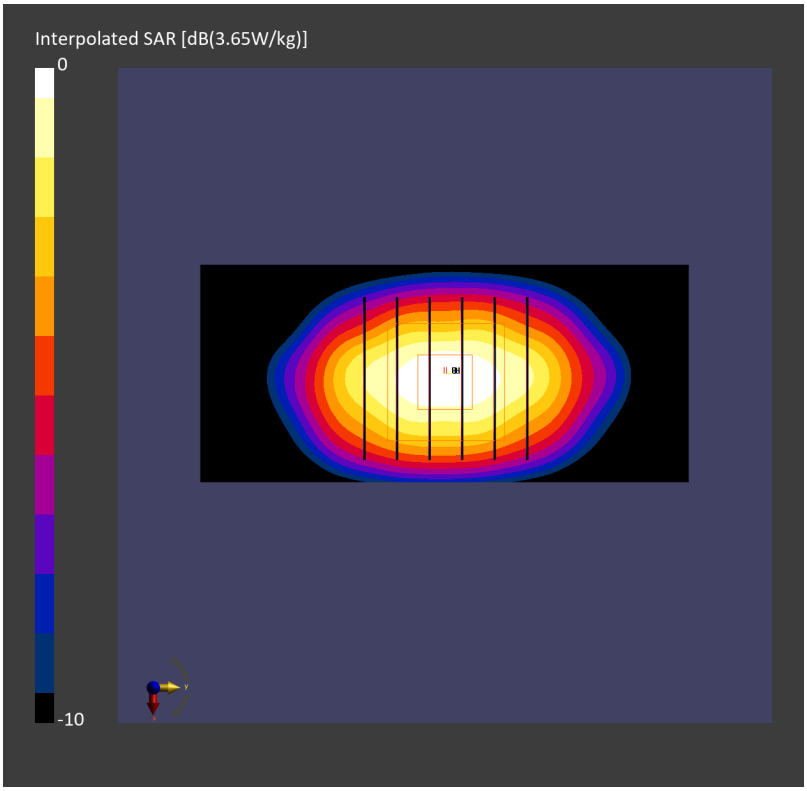

Date: 2026-03-12

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 1900.000 MHz; σ= 1.42 S/m; $\varepsilon_r$ = 40.2
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(7.72, 7.85, 7.52); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144_Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.78 W/kg; SAR (10g) = 0.960 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.03 dB
SAR (1g) = 1.87 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.982 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 83.7 %
TSL Correction: Positive only

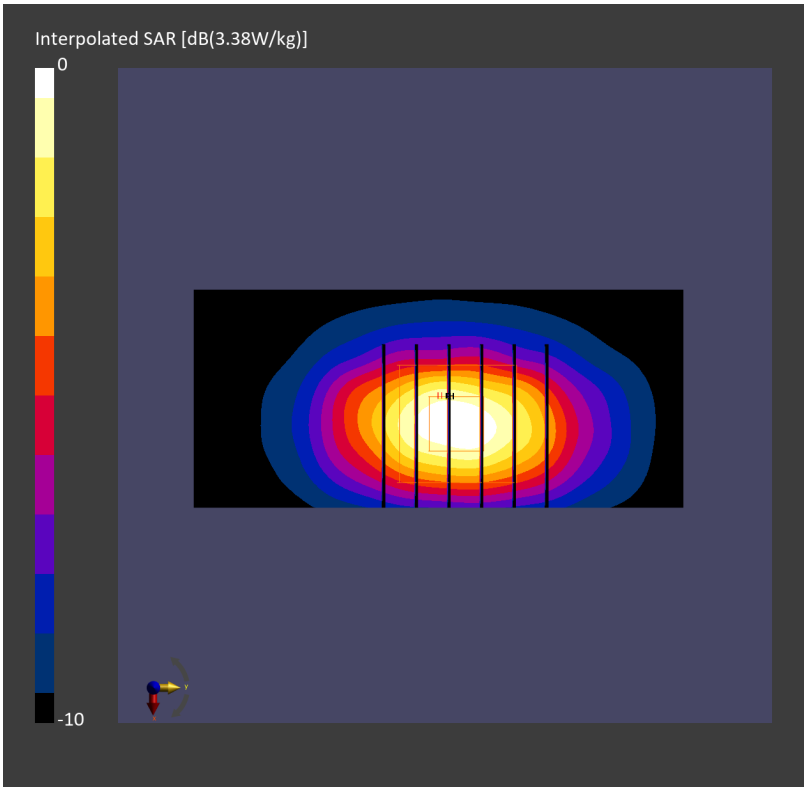

Date: 2026-03-14

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260314 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.42 S/m; $\varepsilon_r$ = 40.0
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.03 W/kg; SAR (10g) = 1.05 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.03 dB
SAR (1g) = 2.01 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 84.8 %
TSL Correction: Positive only

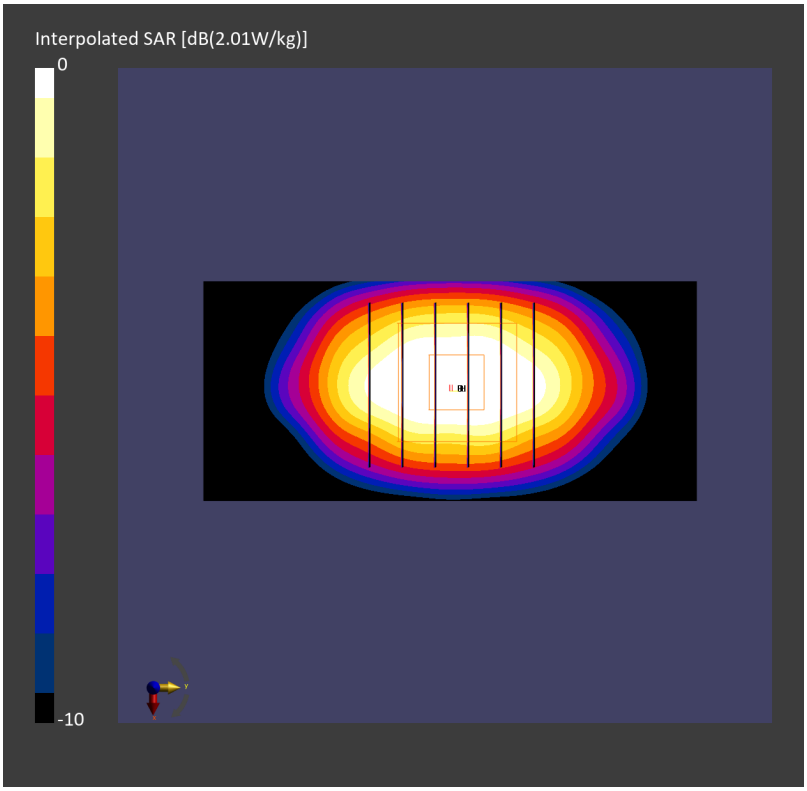

Date: 2026-03-17

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260317 Medium parameters used: f= 1900.000 MHz; $\sigma$= 1.46 S/m; $\varepsilon_r$ = 39.9
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.06 W/kg; SAR (10g) = 1.08 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.07 W/kg; SAR (8g) = 1.17 W/kg; SAR (10g) = 1.07 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 84.1 %
TSL Correction: Positive only

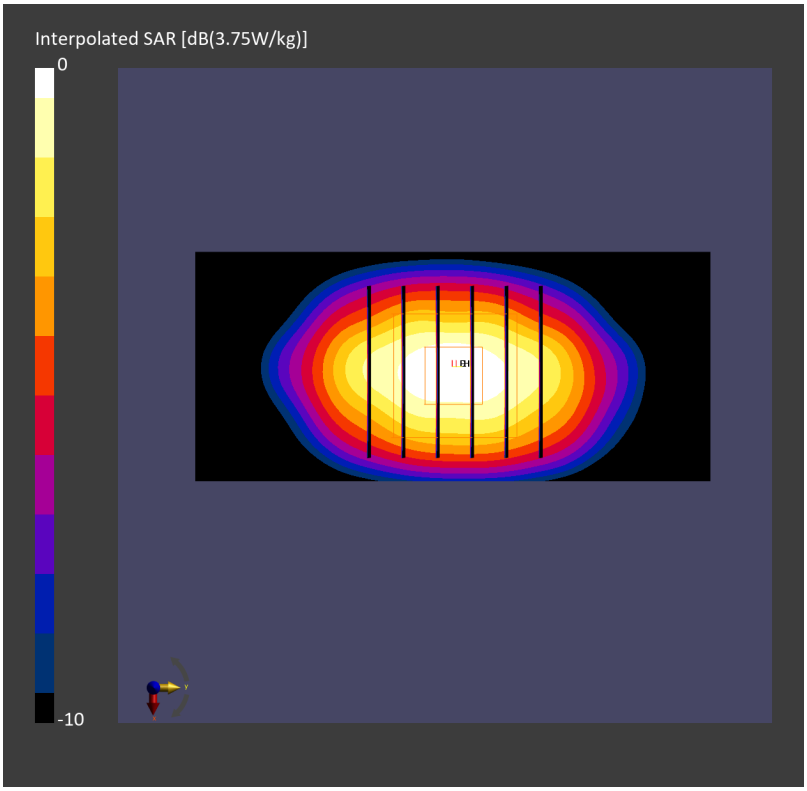

Date: 2026-03-28

**System Check_Head_1900MHz**

**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_600-7200_260328 Medium parameters used: f= 1900.000 MHz; σ= 1.47 S/m; $\varepsilon_r$ = 39.9
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm)**: Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.09 W/kg; SAR (10g) = 1.08 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.07 W/kg; SAR (8g) = 1.17 W/kg; SAR (10g) = 1.08 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 84.4 %
TSL Correction: Positive only

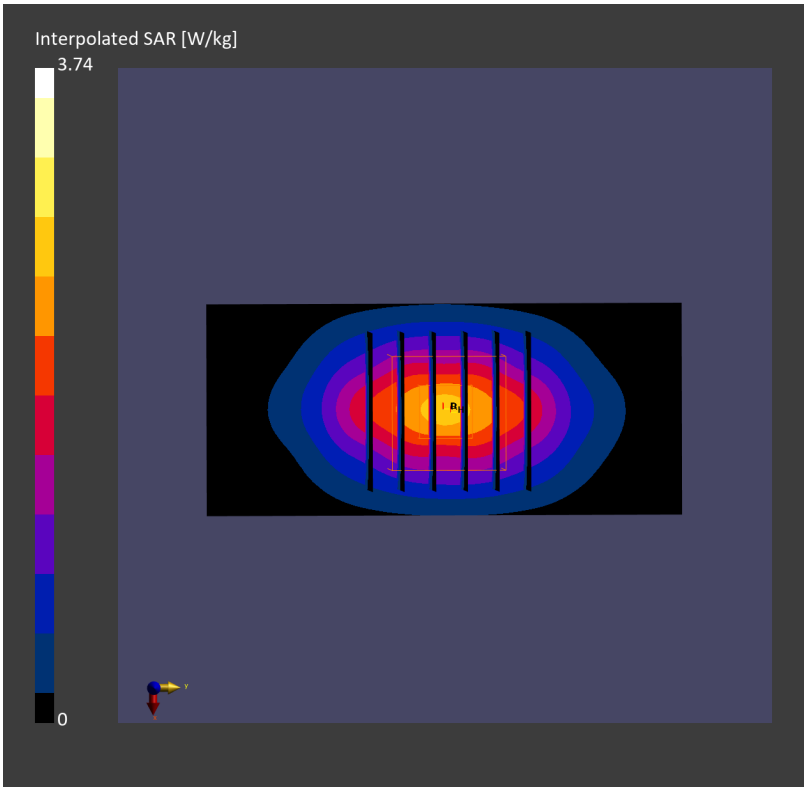

Date: 2026-03-21

**System Check_Head_2000MHz**

**DUT: D2000V2 - SN1070**

Communication System: CW; Frequency: 2000.000 MHz
Medium: HSL_600-7200_260321 Medium parameters used: f= 2000.000 MHz; σ= 1.52 S/m; $\varepsilon_r$ = 42.5
Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.85, 6.84, 6.53); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.13 W/kg; SAR (10g) = 1.10 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.10 W/kg; SAR (8g) = 1.17 W/kg; SAR (10g) = 1.07 W/kg
Smallest distance from peaks to all points 3 dB below = 10.0 mm
Ratio of SAR at M2 to SAR at M1 = 83.8 %
TSL Correction: Positive only

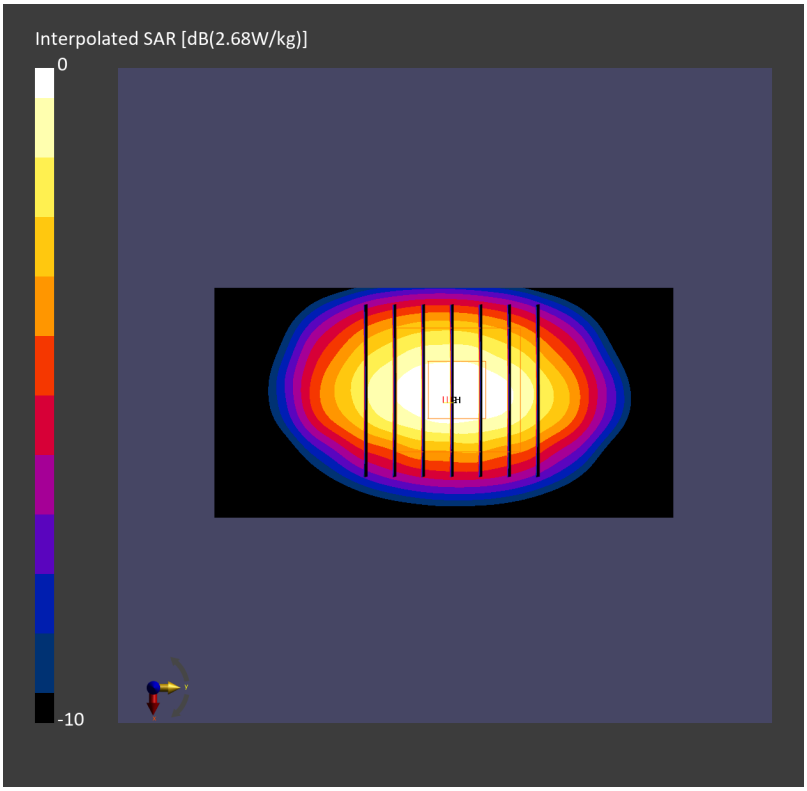

Date: 2026-04-08

**System Check_Head_2000MHz**

**DUT: D2000V2 - SN1010**

Communication System: CW; Frequency: 2000.000 MHz
Medium: HSL_600-7200_260408 Medium parameters used: f= 2000.000 MHz; σ= 1.47 S/m; $\varepsilon_r$ = 43.1
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.85, 6.84, 6.53); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.10 W/kg; SAR (10g) = 1.07 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.09 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.07 W/kg
Smallest distance from peaks to all points 3 dB below = 9.9 mm
Ratio of SAR at M2 to SAR at M1 = 83.2 %
TSL Correction: Positive only

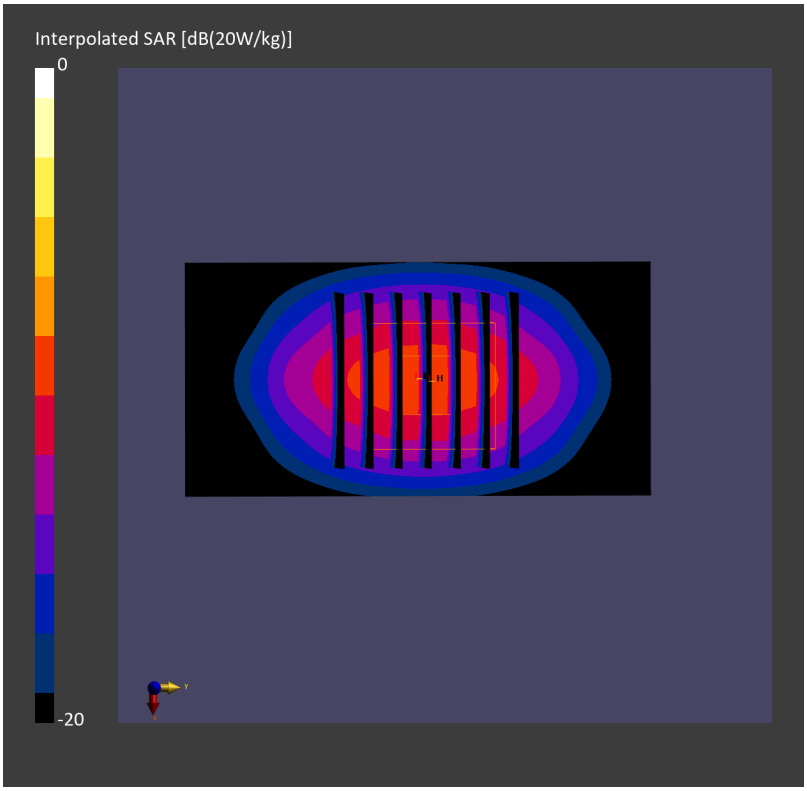

Date: 2026-01-04

**System Check_Head_2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260104 Medium parameters used: f= 2300.000 MHz; $\sigma$= 1.71 S/m; $\varepsilon_r$ = 42.7
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.37, 7.25, 7.29); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.0 W/kg; SAR (10g) = 6.22 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.03 dB
SAR (1g) = 12.8 W/kg; SAR (8g) = 6.75 W/kg; SAR (10g) = 6.13 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.8 %
TSL Correction: Positive only

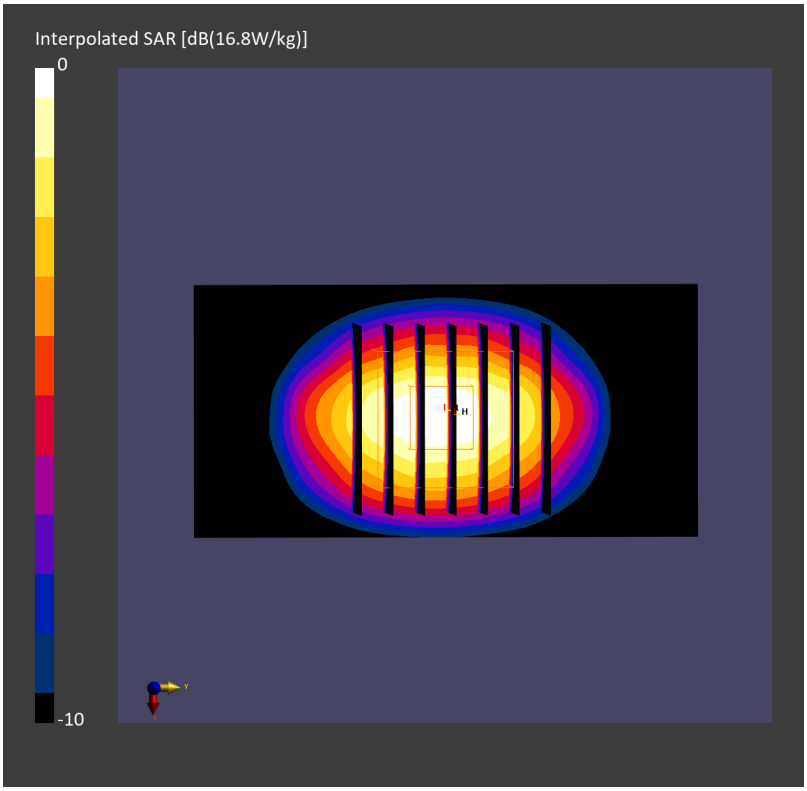

Date: 2026-01-16

**System Check_Head_2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260116 Medium parameters used: f= 2300.000 MHz; σ= 1.78 S/m; $\varepsilon_r$ = 40.3
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.37, 7.25, 7.29); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.54 W/kg; SAR (10g) = 1.21 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.51 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.20 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.3 %
TSL Correction: Positive only

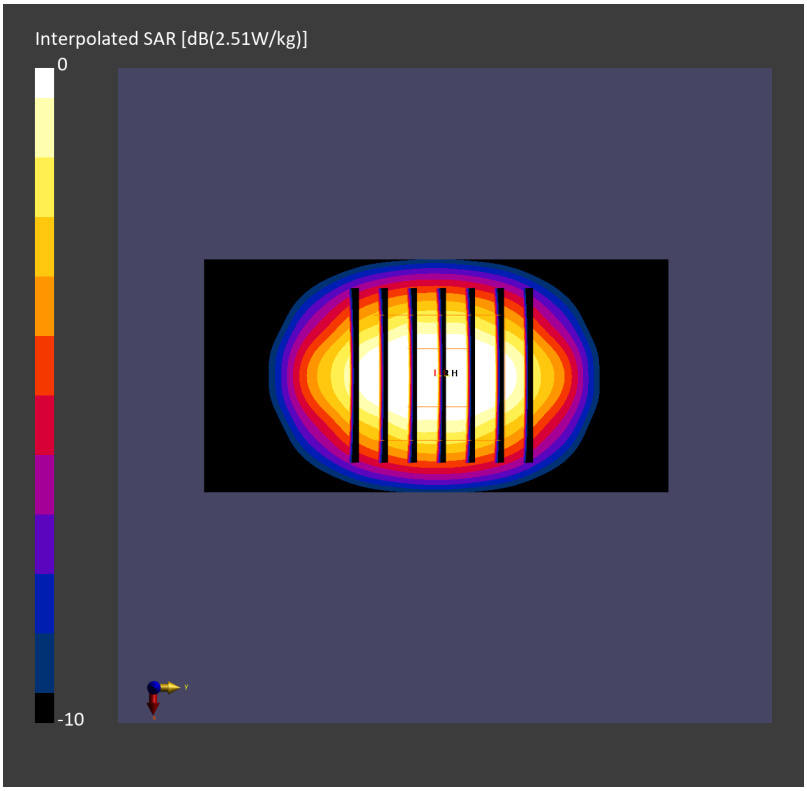

Date: 2026-02-07

**System Check_Head_2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260207 Medium parameters used: f= 2300.000 MHz; $\sigma$= 1.75 S/m; $\varepsilon_r$ = 39.8
Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.72, 6.71, 6.41); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.51 W/kg; SAR (10g) = 1.20 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.48 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 9.5 mm
Ratio of SAR at M2 to SAR at M1 = 82.0 %
TSL Correction: Positive only

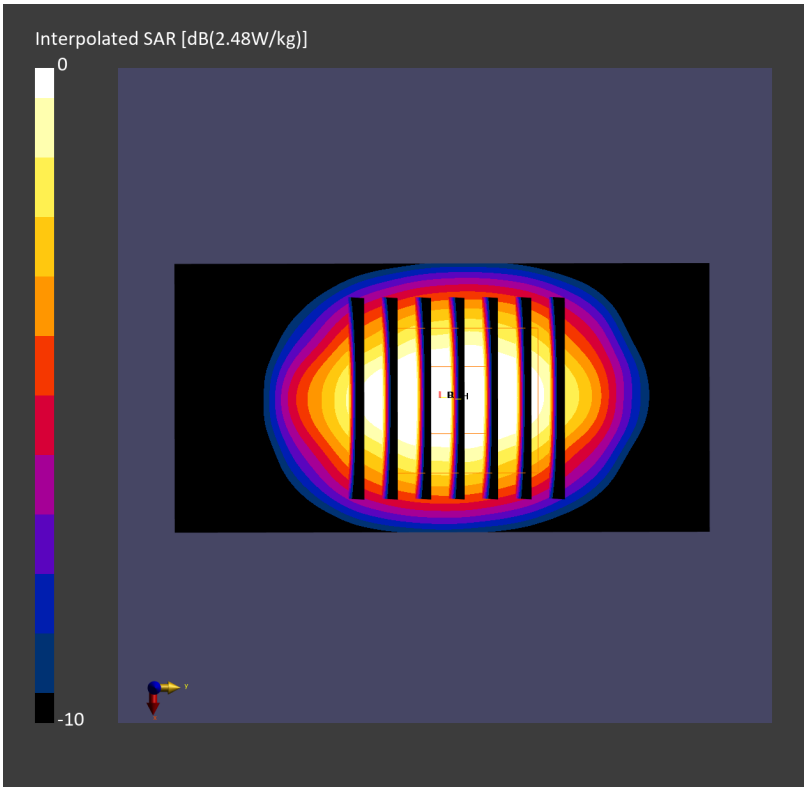

Date: 2026-02-18

**System Check_Head_2300MHz_260218**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 2300.000 MHz; $\sigma$= 1.71 S/m; $\varepsilon_r$ = 39.6
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.72, 6.71, 6.41); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.47 W/kg; SAR (10g) = 1.18 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.42 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg
Smallest distance from peaks to all points 3 dB below = 9.1 mm
Ratio of SAR at M2 to SAR at M1 = 82.6 %
TSL Correction: Positive only

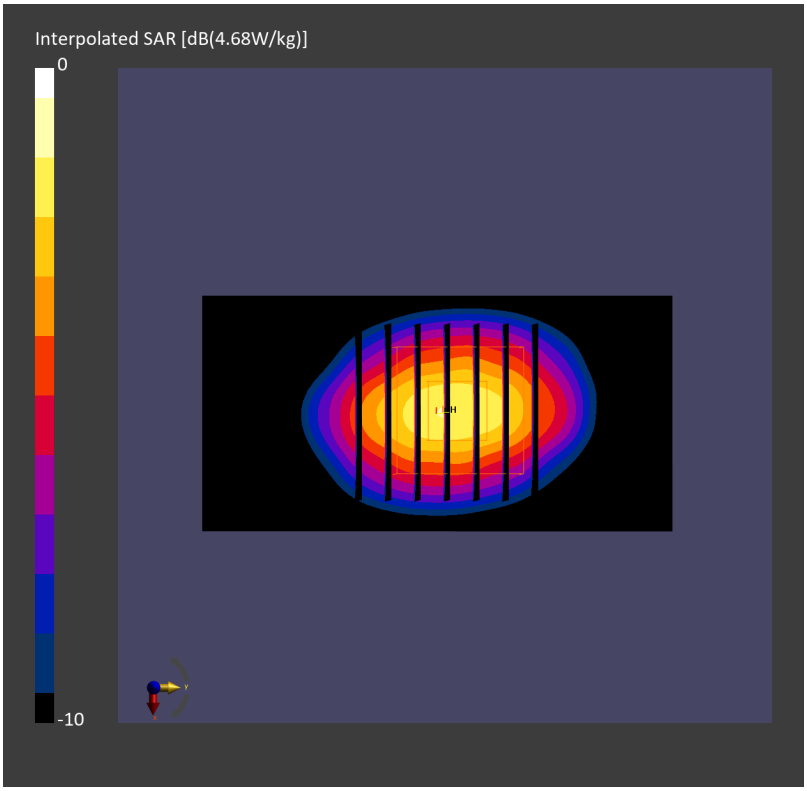

Date: 2026-02-23

**System Check_Head_2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 2300.000 MHz; $\sigma$= 1.73 S/m; $\varepsilon_r$ = 39.9
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.72, 6.71, 6.41); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.51 W/kg; SAR (10g) = 1.20 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.48 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 9.3 mm
Ratio of SAR at M2 to SAR at M1 = 82.4 %
TSL Correction: Positive only

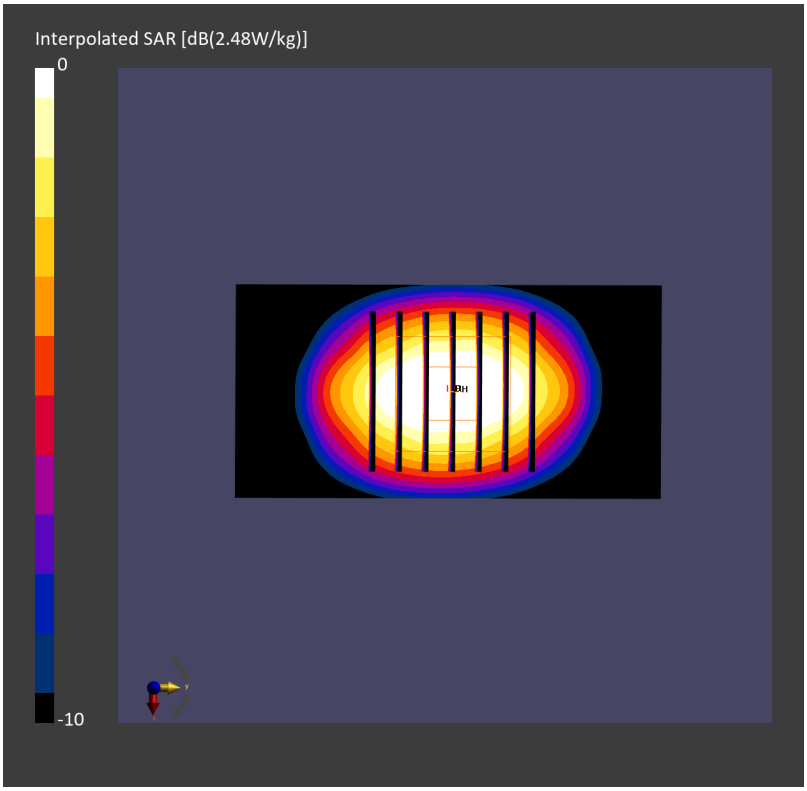

Date: 2026-03-12

**System Check_Head_2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 2300.000 MHz; $\sigma$= 1.73 S/m; $\varepsilon_r$ = 40.0
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.72, 6.71, 6.41); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.43 W/kg; SAR (10g) = 1.16 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 2.42 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.16 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.4 %
TSL Correction: Positive only

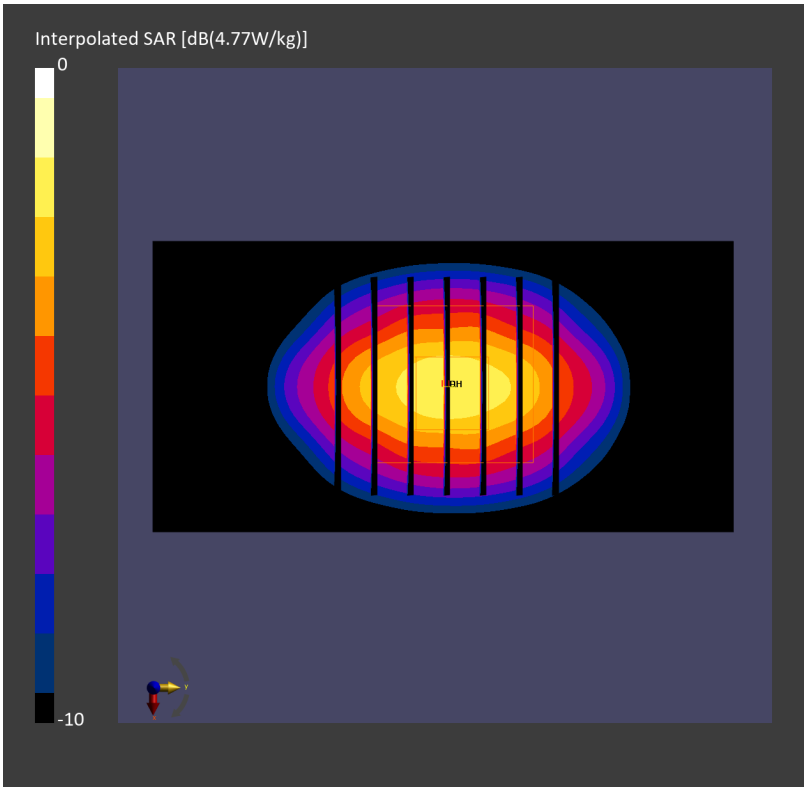

Date: 2026-03-14

**System Check_Head 2300MHz**

**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_600-7200_260314 Medium parameters used: f= 2300.000 MHz; σ= 1.74 S/m; $\varepsilon_r$ = 40.2
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(7.21, 6.9, 7.67); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.50 W/kg; SAR (10g) = 1.18 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.47 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.8 %
TSL Correction: Positive only

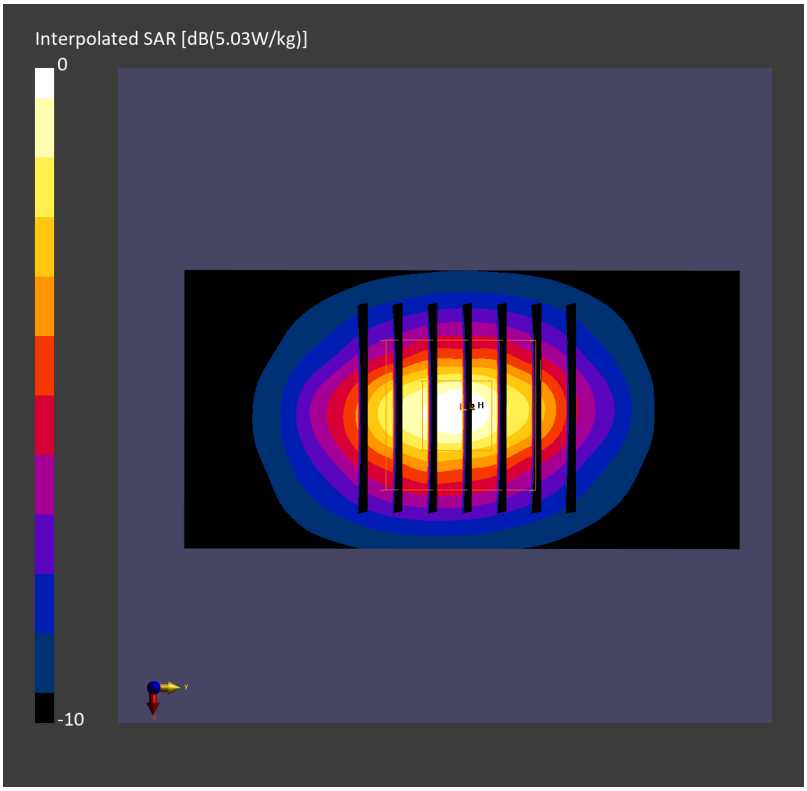

Date: 2026-01-04

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260104 Medium parameters used: f= 2600.000 MHz; σ= 1.94 S/m; $\varepsilon_r$ = 42.3
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 14.1 W/kg; SAR (10g) = 6.27 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 13.9 W/kg; SAR (8g) = 6.89 W/kg; SAR (10g) = 6.21 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.8 %
TSL Correction: Positive only

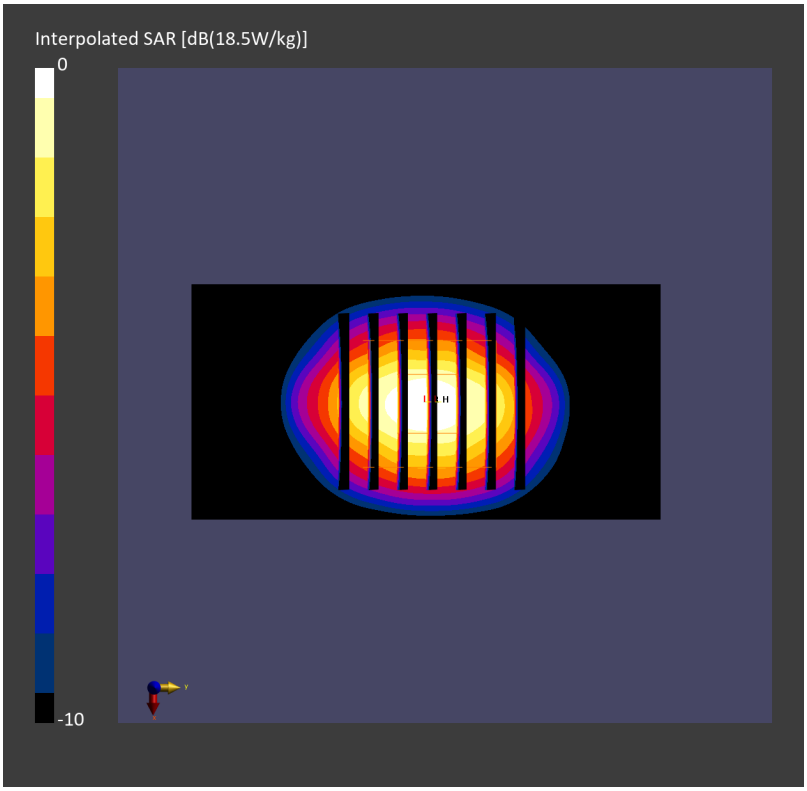

Date: 2026-01-12

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260112 Medium parameters used: f= 2600.000 MHz; σ= 1.97 S/m; $\varepsilon_r$ = 39.6
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.66 W/kg; SAR (10g) = 1.19 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.63 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.9 %
TSL Correction: Positive only

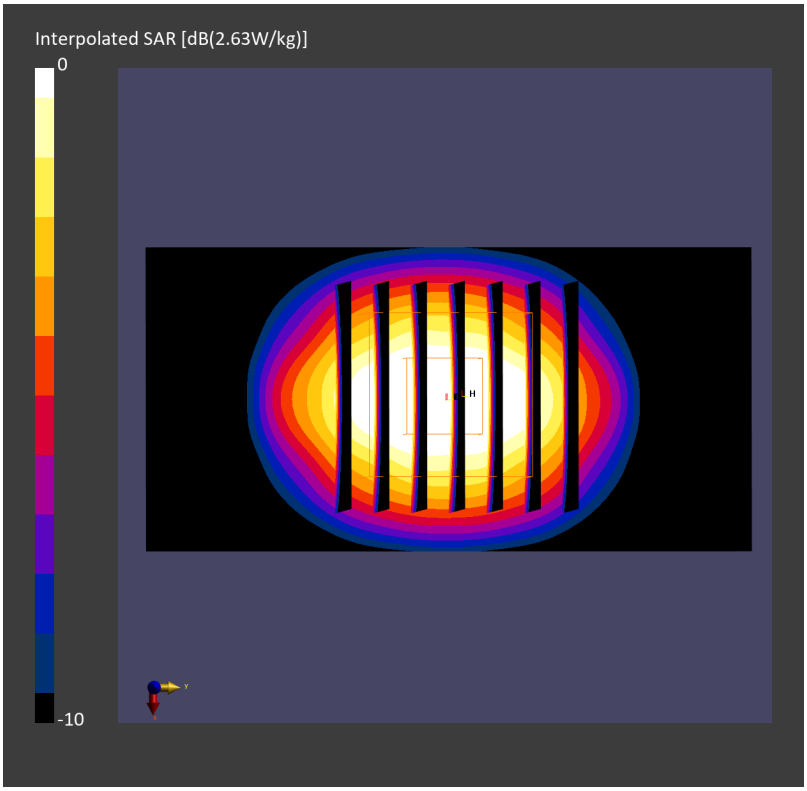

Date: 2026-01-16

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260116 Medium parameters used: f= 2600.000 MHz; σ= 2.02 S/m; $\varepsilon_r$ = 39.8
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.78 W/kg; SAR (10g) = 1.24 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.70 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg
Smallest distance from peaks to all points 3 dB below = 9.1 mm
Ratio of SAR at M2 to SAR at M1 = 79.8 %
TSL Correction: Positive only

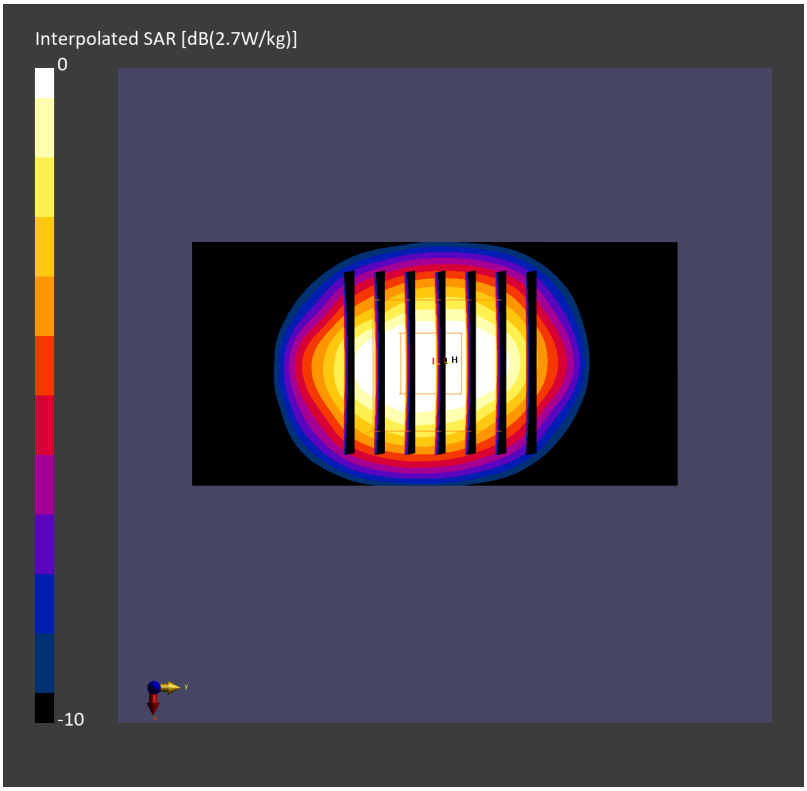

Date: 2026-02-08

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260208 Medium parameters used: f= 2600.000 MHz; $\sigma$= 1.93 S/m; $\varepsilon_r$ = 39.1
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 12.9 W/kg; SAR (10g) = 5.76 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 12.8 W/kg; SAR (8g) = 6.42 W/kg; SAR (10g) = 5.79 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.3 %
TSL Correction: Positive only

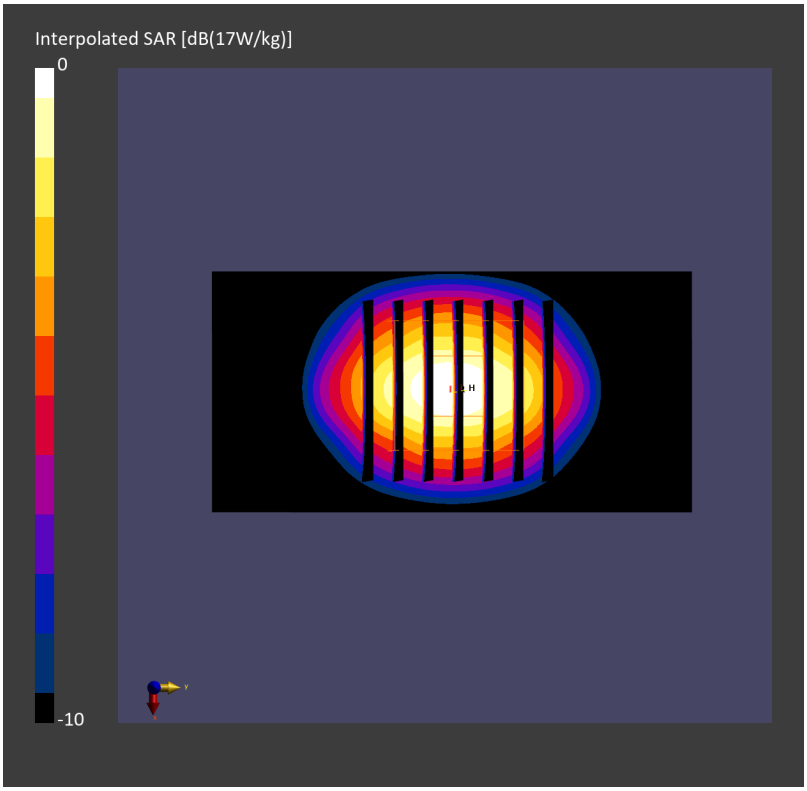

Date: 2026-02-10

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260210 Medium parameters used: f= 2600.000 MHz; $\sigma$= 1.97 S/m; $\varepsilon_r$ = 39.5
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.2 W/kg; SAR (10g) = 5.92 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 13.1 W/kg; SAR (8g) = 6.55 W/kg; SAR (10g) = 5.92 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.2 %
TSL Correction: Positive only

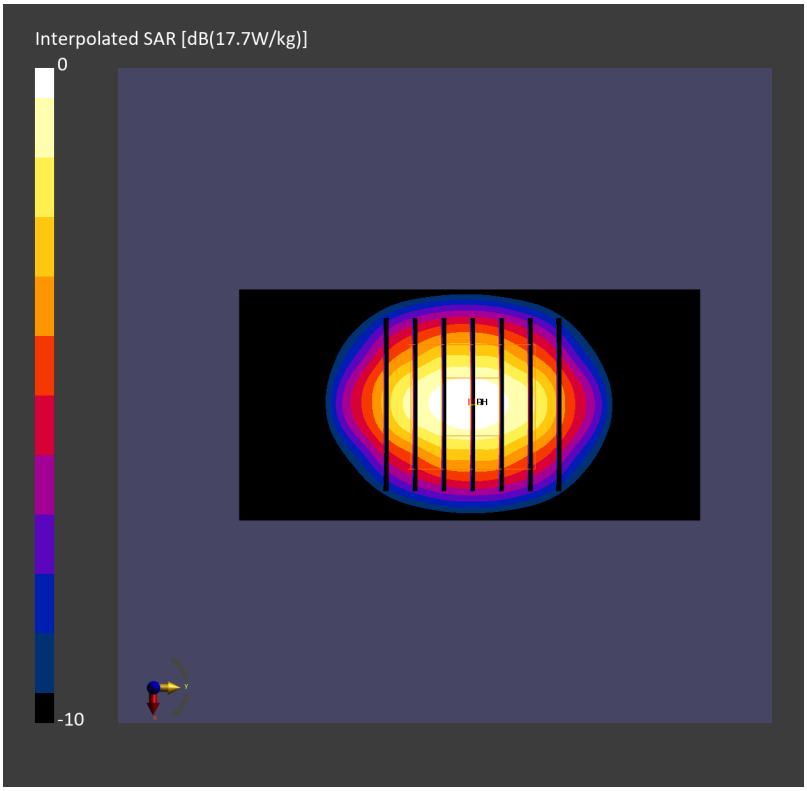

Date: 2026-02-12

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260212 Medium parameters used: f= 2600.000 MHz; σ= 1.97 S/m; $\varepsilon_r$ = 41.8
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.8 W/kg; SAR (10g) = 6.21 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.02 dB
SAR (1g) = 13.8 W/kg; SAR (8g) = 6.87 W/kg; SAR (10g) = 6.20 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.2 %
TSL Correction: Positive only

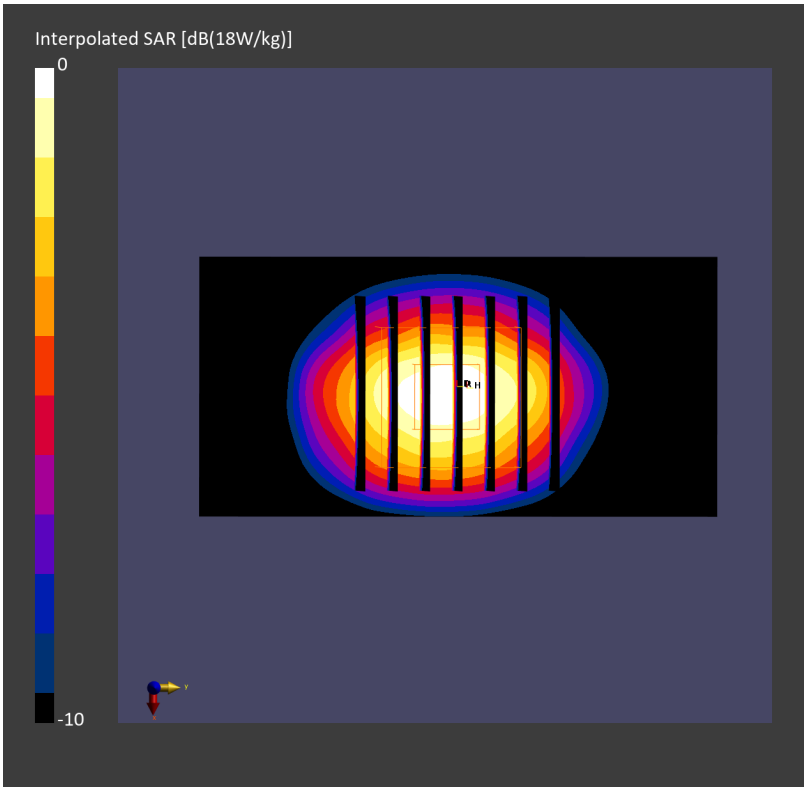

Date: 2026-02-14

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260214 Medium parameters used: f= 2600.000 MHz; σ= 1.95 S/m; $\varepsilon_r$ = 39.5
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=16.7dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.50 W/kg; SAR (10g) = 1.12 W/kg;
TSL Correction: Positive only

**Pin=16.7dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.48 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.11 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.8 %
TSL Correction: Positive only

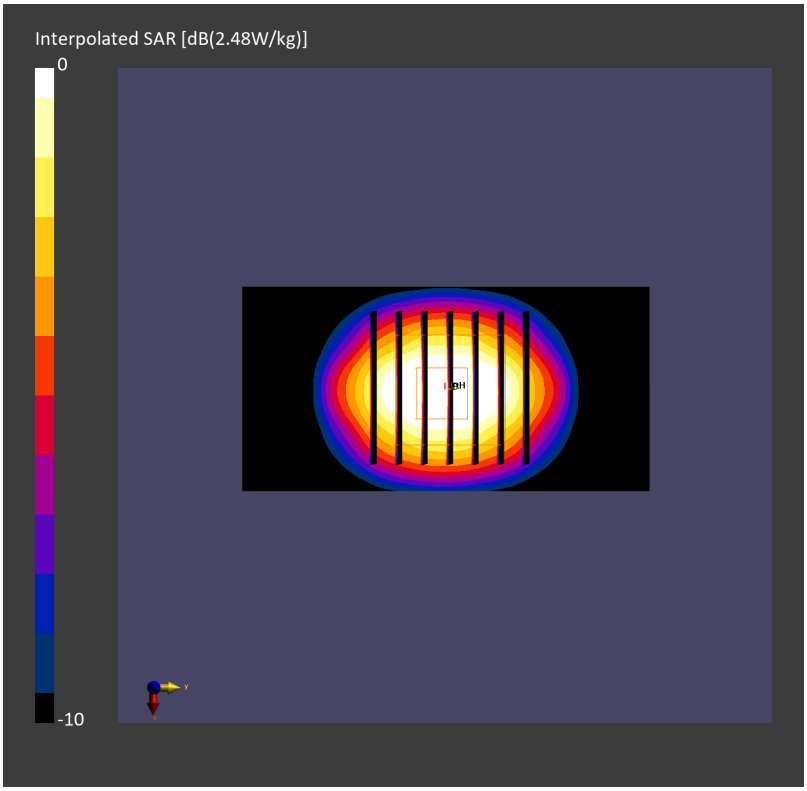

Date: 2026-02-15

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260215 Medium parameters used: f= 2600.000 MHz; σ= 1.97 S/m; $\varepsilon_r$ = 39.6
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(7.11, 6.99, 7.04); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.65 W/kg; SAR (10g) = 1.19 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 2.65 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.3 %
TSL Correction: Positive only

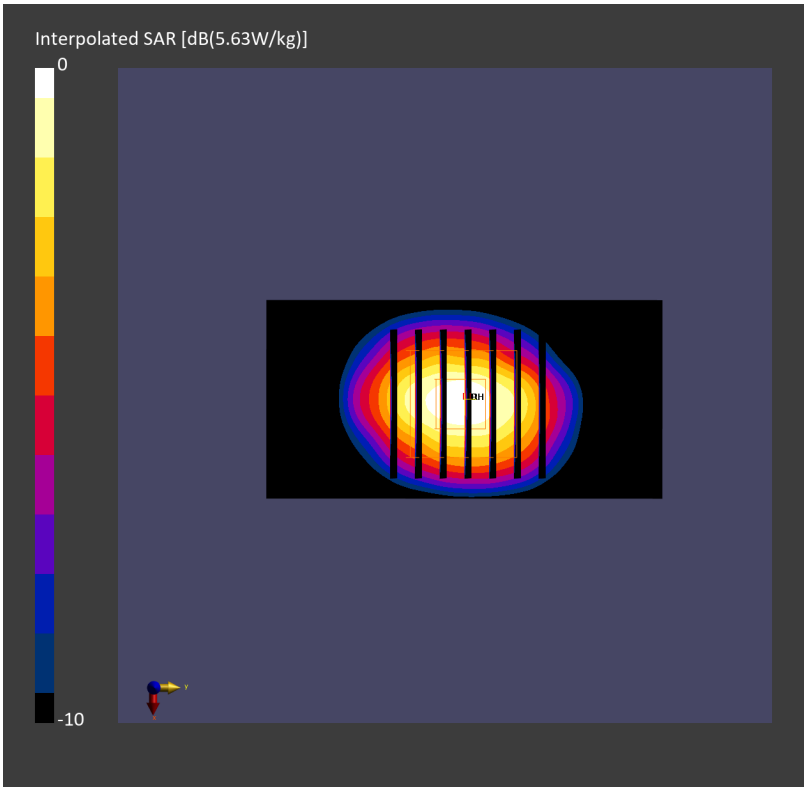

Date: 2026-02-18

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 2600.000 MHz; σ= 1.94 S/m; $\varepsilon_r$ = 39.0
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 13.1 W/kg; SAR (10g) = 5.97 W/kg;
TSL Correction: Positive only

**Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.07 dB
SAR (1g) = 12.8 W/kg; SAR (8g) = 6.39 W/kg; SAR (10g) = 5.77 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.5 %
TSL Correction: Positive only

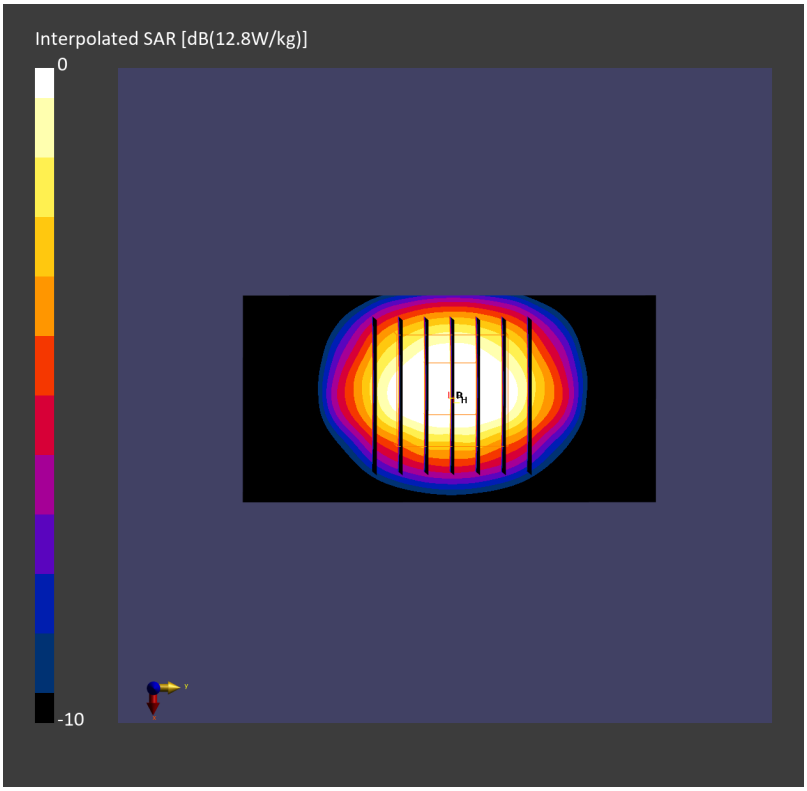

Date: 2026-03-03

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260303 Medium parameters used: f= 2600.000 MHz; σ= 1.95 S/m; $\varepsilon_r$ = 39.4
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.58 W/kg; SAR (10g) = 1.16 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 2.54 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.0 %
TSL Correction: Positive only

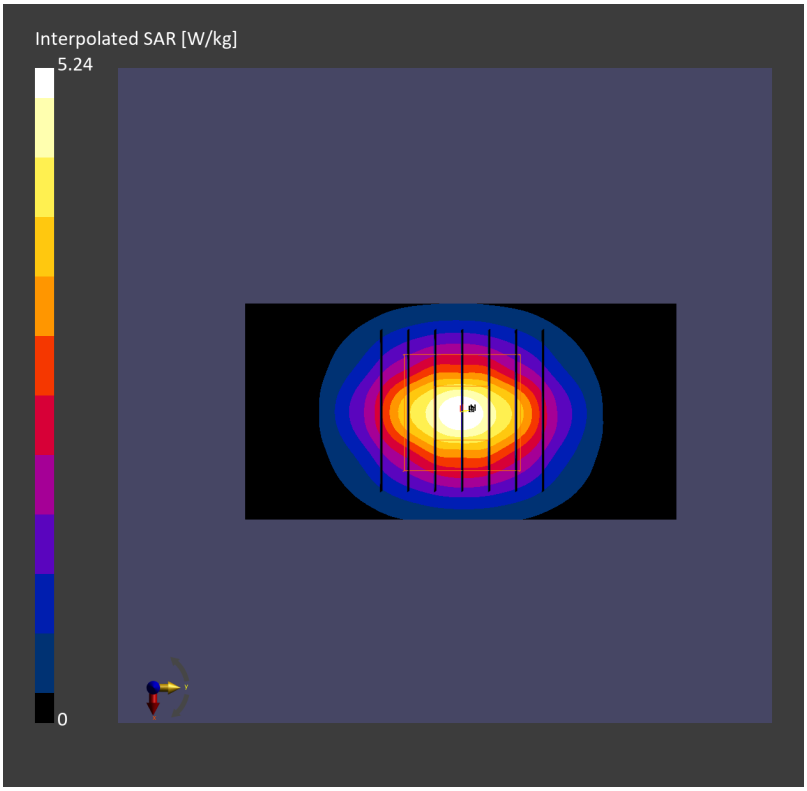

Date: 2026-03-12

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260312 Medium parameters used: f= 2600.000 MHz; σ= 1.97 S/m; $\varepsilon_r$ = 39.5
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.64 W/kg; SAR (10g) = 1.17 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.56 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.9 %
TSL Correction: Positive only

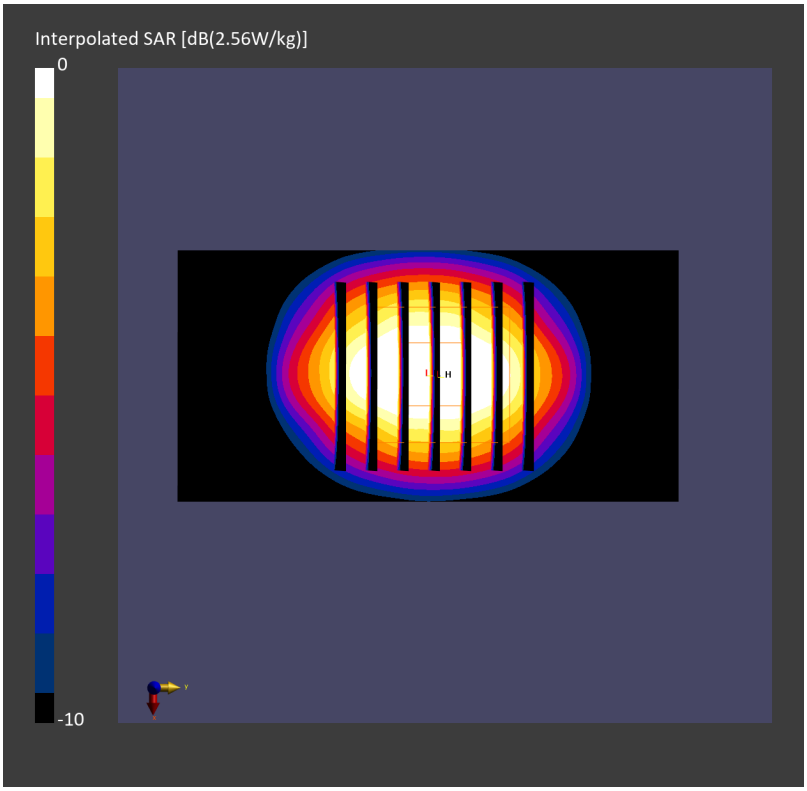

Date: 2026-04-08

**System Check_Head_2600MHz**

**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_600-7200_260408 Medium parameters used: f= 2600.000 MHz; σ= 1.96 S/m; $\varepsilon_r$ = 41.0
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(6.95, 6.65, 7.39); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.65 W/kg; SAR (10g) = 1.18 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.62 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.7 %
TSL Correction: Positive only

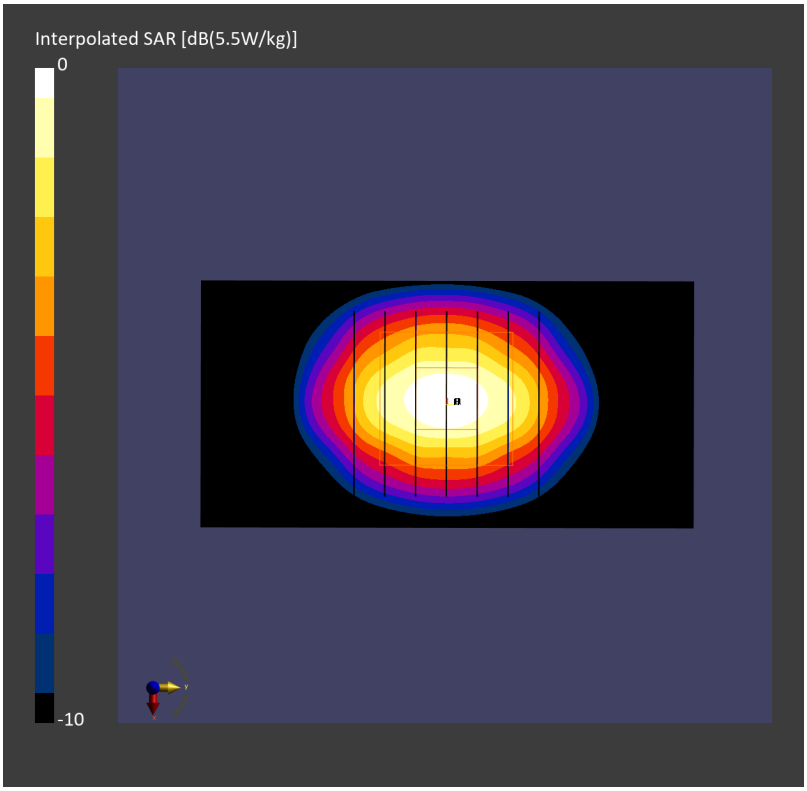

Date: 2026-01-06

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260106 Medium parameters used: f= 3500.000 MHz; σ= 2.74 S/m; $\varepsilon_r$ = 38.5
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.71 W/kg; SAR (10g) = 2.54 W/kg;
TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 6.75 W/kg; SAR (8g) = 2.90 W/kg; SAR (10g) = 2.57 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.8 %
TSL Correction: Positive only

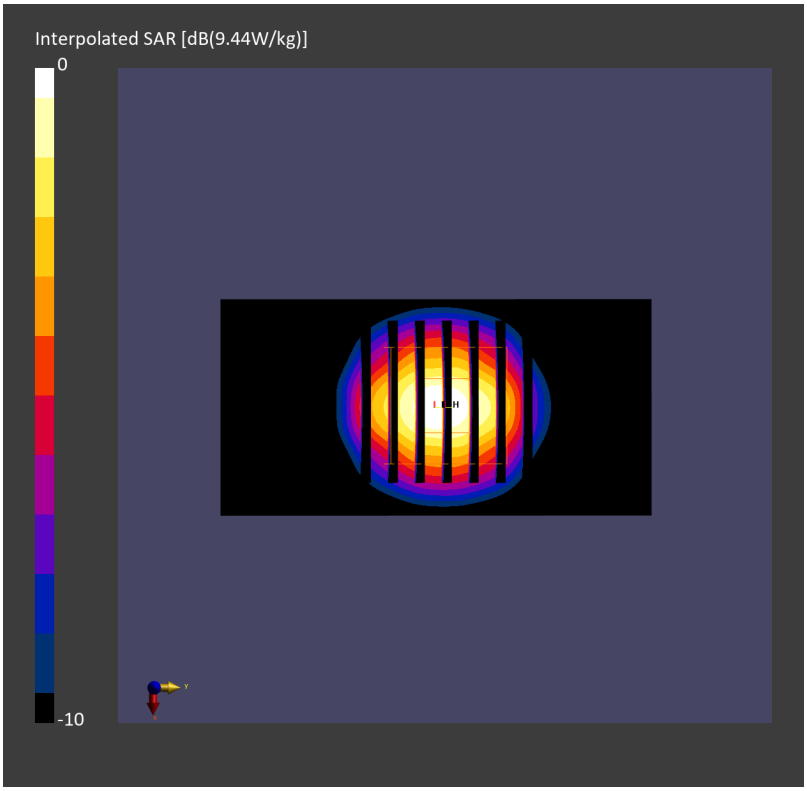

Date: 2026-02-12

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260212 Medium parameters used: f= 3500.000 MHz; σ= 2.72 S/m; $\varepsilon_r$ = 37.7
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.33 W/kg; SAR (10g) = 1.26 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.31 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.8 %
TSL Correction: Positive only

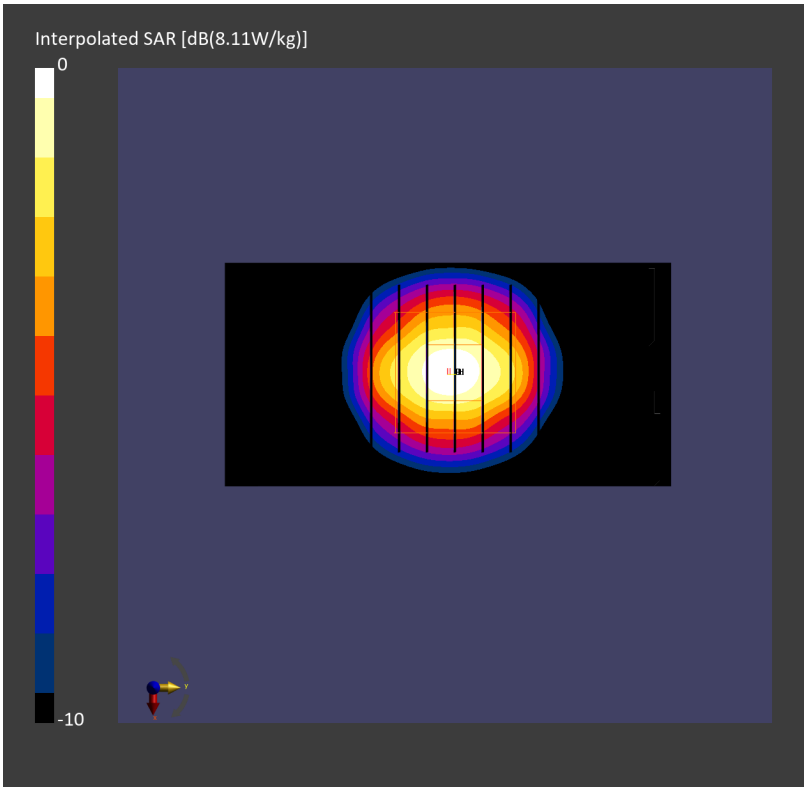

Date: 2026-02-18

**System Check_Head 3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 3500.000 MHz; σ= 2.74 S/m; $\varepsilon_r$ = 38.0
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(6.61, 6.32, 7.03); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.13 W/kg; SAR (10g) = 1.20 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.23 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.8 %
TSL Correction: Positive only

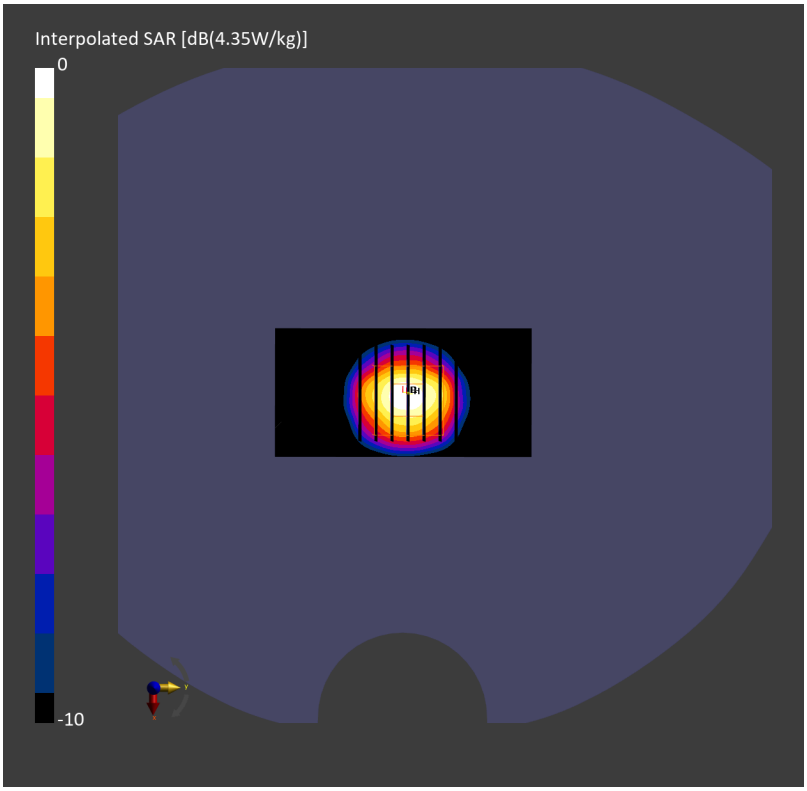

Date: 2026-02-21

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260221 Medium parameters used: f= 3500.000 MHz; σ= 2.72 S/m; $\varepsilon_r$ = 38.2
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.18 W/kg; SAR (10g) = 1.22 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.21 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.2 %
TSL Correction: Positive only

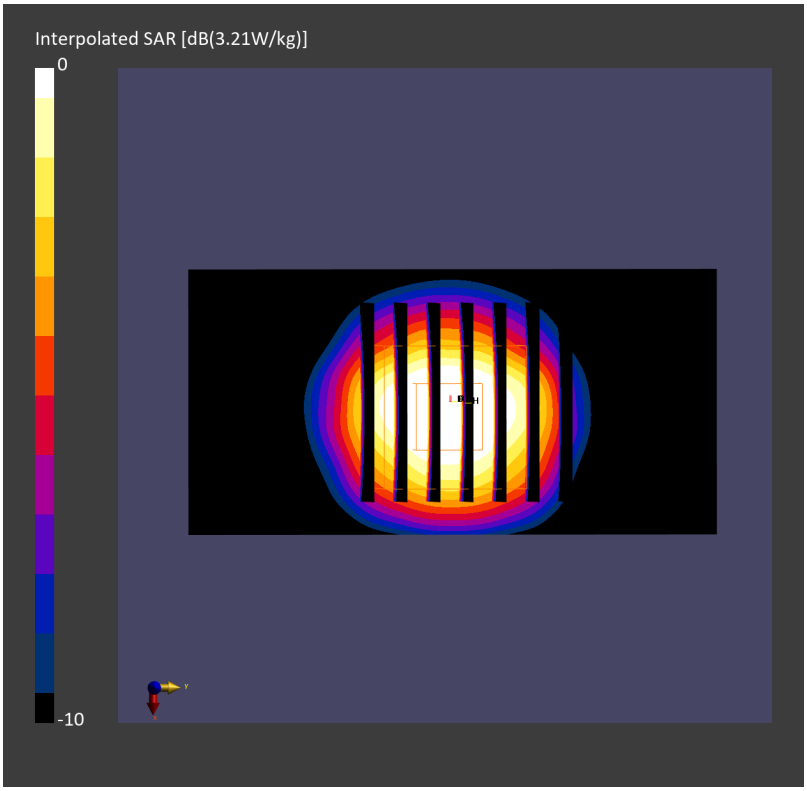

Date: 2026-02-22

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260222 Medium parameters used: f= 3500.000 MHz; σ= 2.75 S/m; $\varepsilon_r$ = 38.3
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.32 W/kg; SAR (10g) = 1.27 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.05 dB
SAR (1g) = 3.33 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.27 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 75.7 %
TSL Correction: Positive only

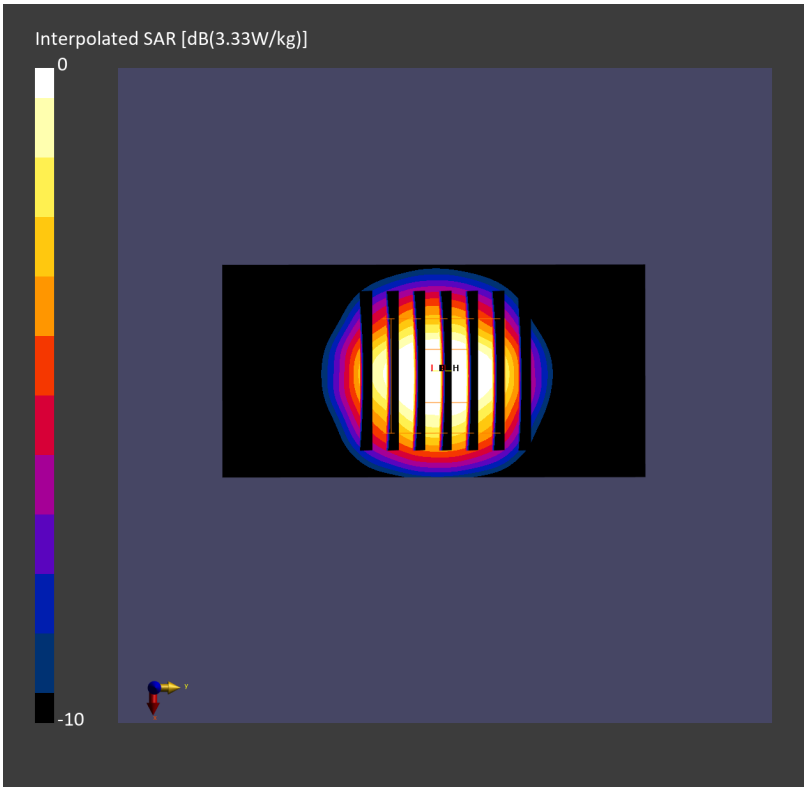

Date: 2026-02-23

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 3500.000 MHz; σ= 2.69 S/m; $\varepsilon_r$ = 40.7
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.25 W/kg; SAR (10g) = 1.23 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.27 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 76.1 %
TSL Correction: Positive only

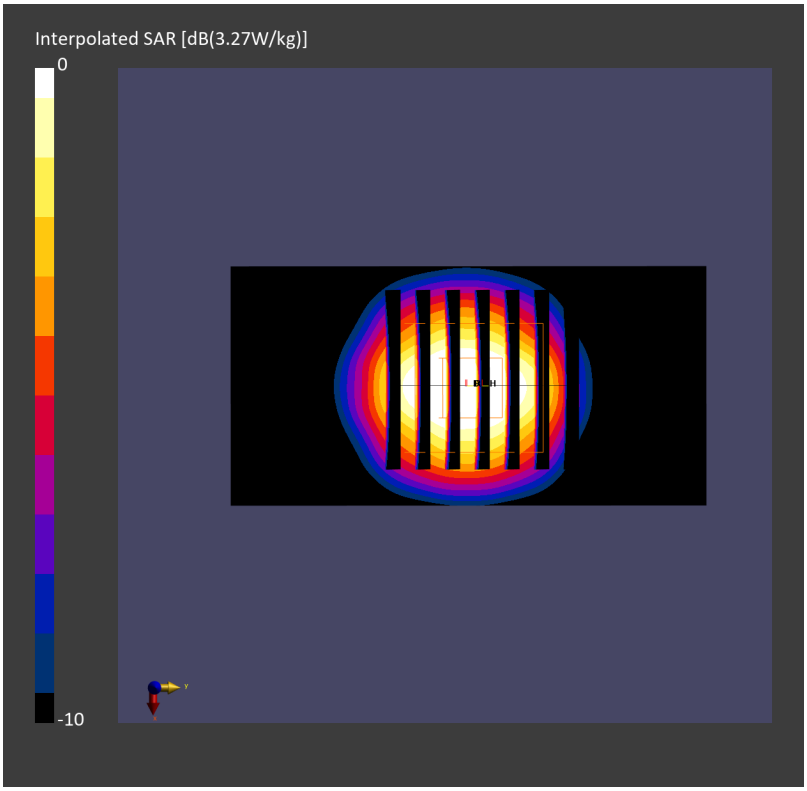

Date: 2026-02-24

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260224 Medium parameters used: f= 3500.000 MHz; σ= 2.71 S/m; $\varepsilon_r$ = 39.6
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.12 W/kg; SAR (10g) = 1.22 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.24 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 75.9 %
TSL Correction: Positive only

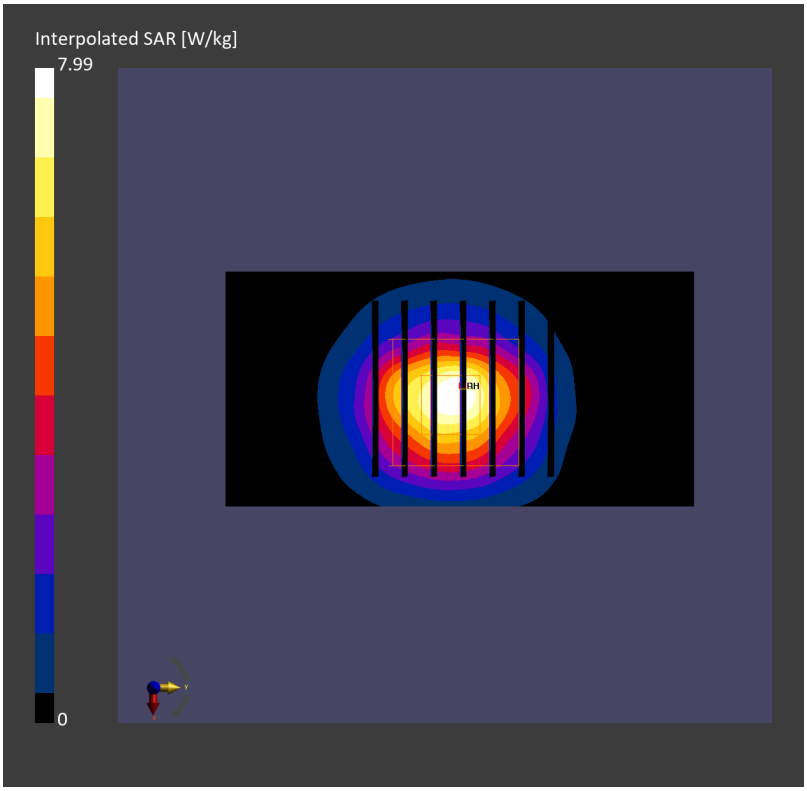

Date: 2026-02-25

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260225 Medium parameters used: f= 3500.000 MHz; σ= 2.74 S/m; $\varepsilon_r$ = 39.7
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.19 W/kg; SAR (10g) = 1.22 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 3.23 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.7 %
TSL Correction: Positive only

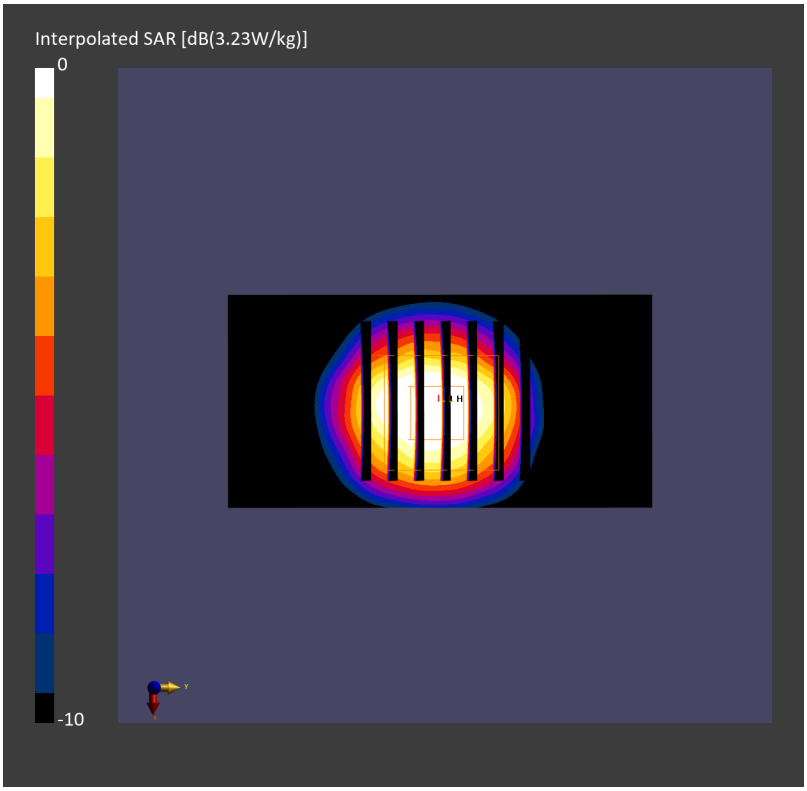

Date: 2026-03-02

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260302 Medium parameters used: f= 3500.000 MHz; σ= 2.75 S/m; $\varepsilon_r$ = 37.9
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.29 W/kg; SAR (10g) = 1.28 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.34 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 77.4 %
TSL Correction: Positive only

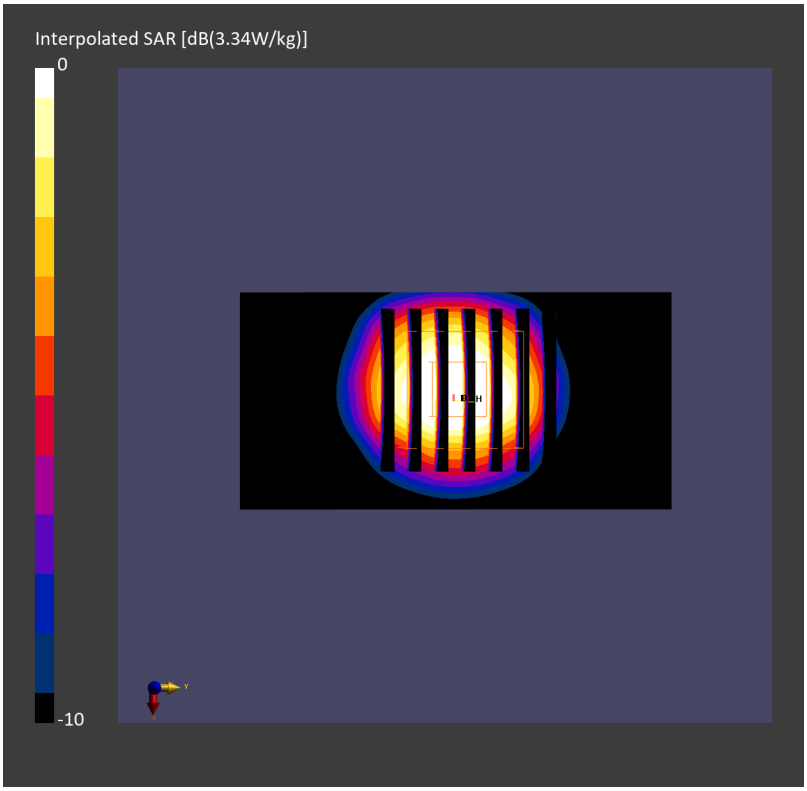

Date: 2026-03-18

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260318 Medium parameters used: f= 3500.000 MHz; σ= 2.73 S/m; $\varepsilon_r$ = 37.1
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.85 W/kg; SAR (10g) = 2.62 W/kg;
TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.04 dB
SAR (1g) = 7.10 W/kg; SAR (8g) = 3.05 W/kg; SAR (10g) = 2.71 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 77.1 %
TSL Correction: Positive only

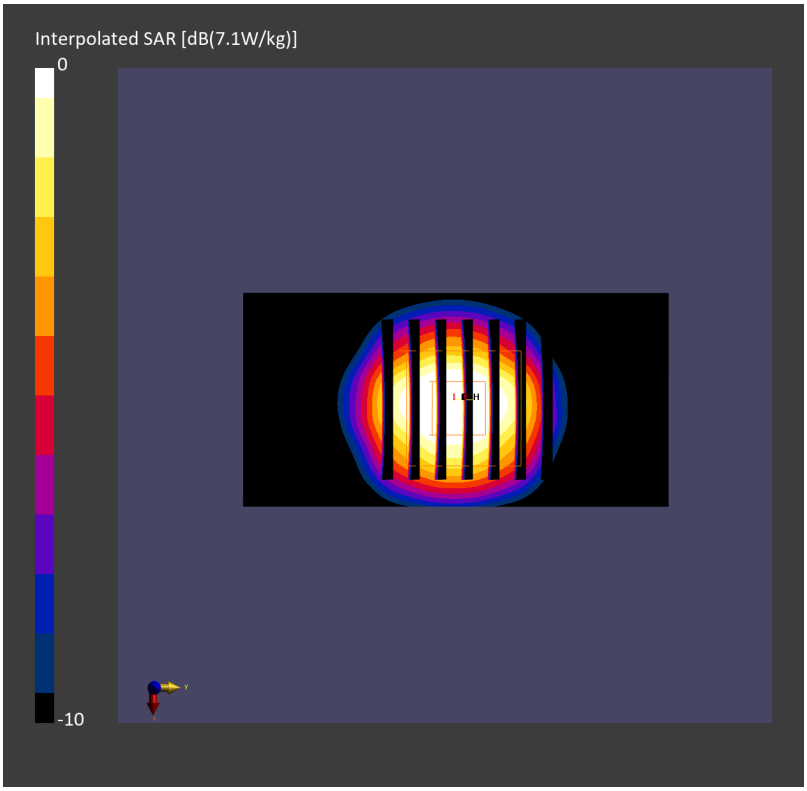

Date: 2026-03-19

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260319 Medium parameters used: f= 3500.000 MHz; σ= 2.77 S/m; $\varepsilon_r$ = 40.1
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.33 W/kg; SAR (10g) = 1.26 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.35 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.28 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.4 %
TSL Correction: Positive only

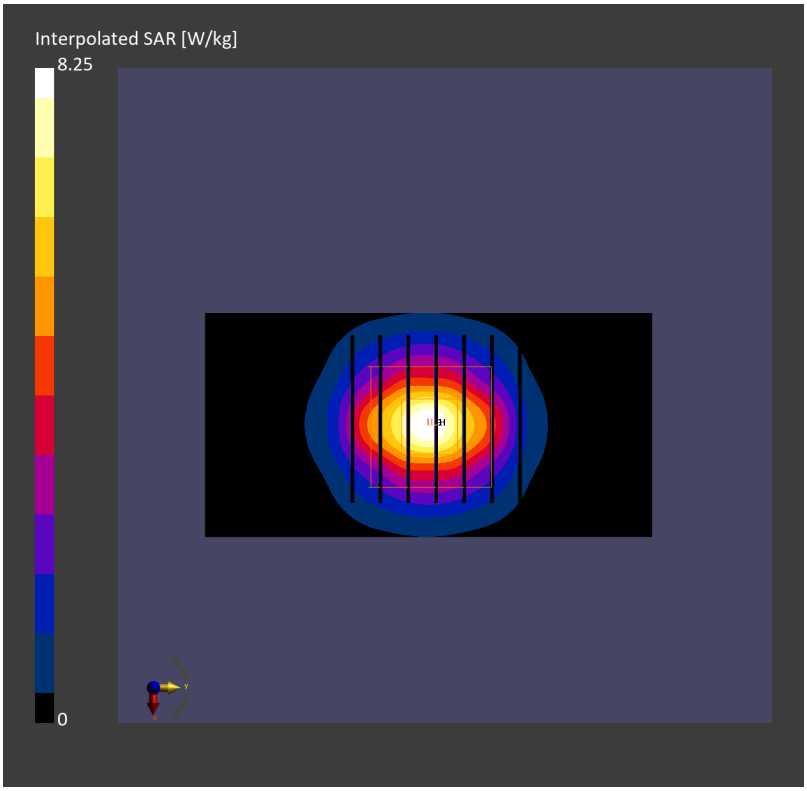

Date: 2026-04-16

**System Check_Head 3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260416 Medium parameters used: f= 3500.000 MHz; $\sigma$= 2.71 S/m; $\varepsilon_r$ = 37.7
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(6.67, 6.78, 6.49); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144_Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.00 W/kg; SAR (10g) = 1.12 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.02 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.8 %
TSL Correction: Positive only

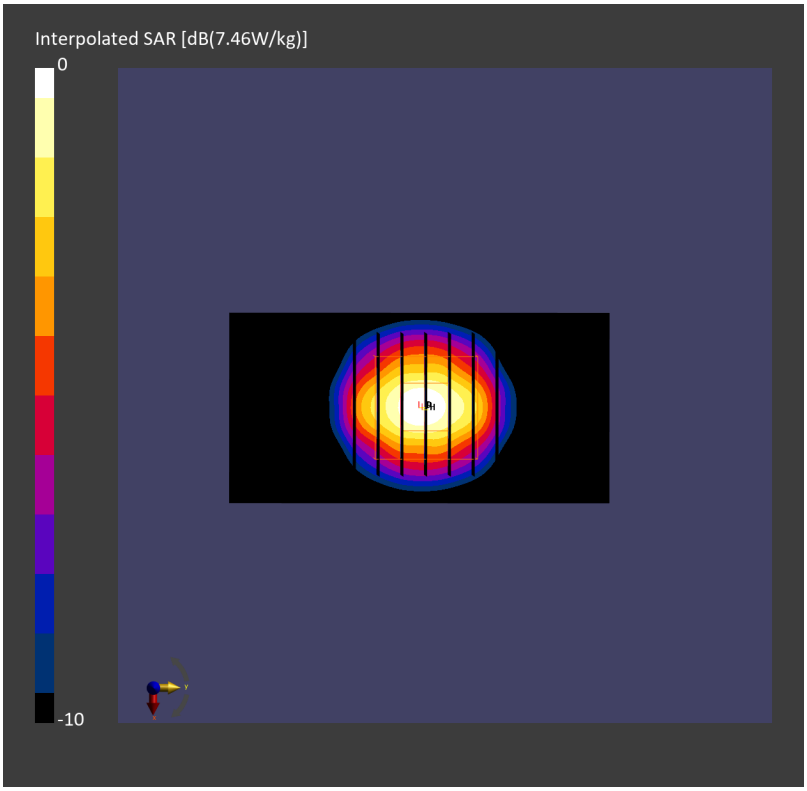

Date: 2026-04-17

**System Check_Head_3500MHz**

**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_600-7200_260417 Medium parameters used: f= 3500.000 MHz; σ= 2.72 S/m; $\varepsilon_r$ = 37.9
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.47, 6.37, 6.41); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.33 W/kg; SAR (10g) = 1.27 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.38 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.4 %
TSL Correction: Positive only

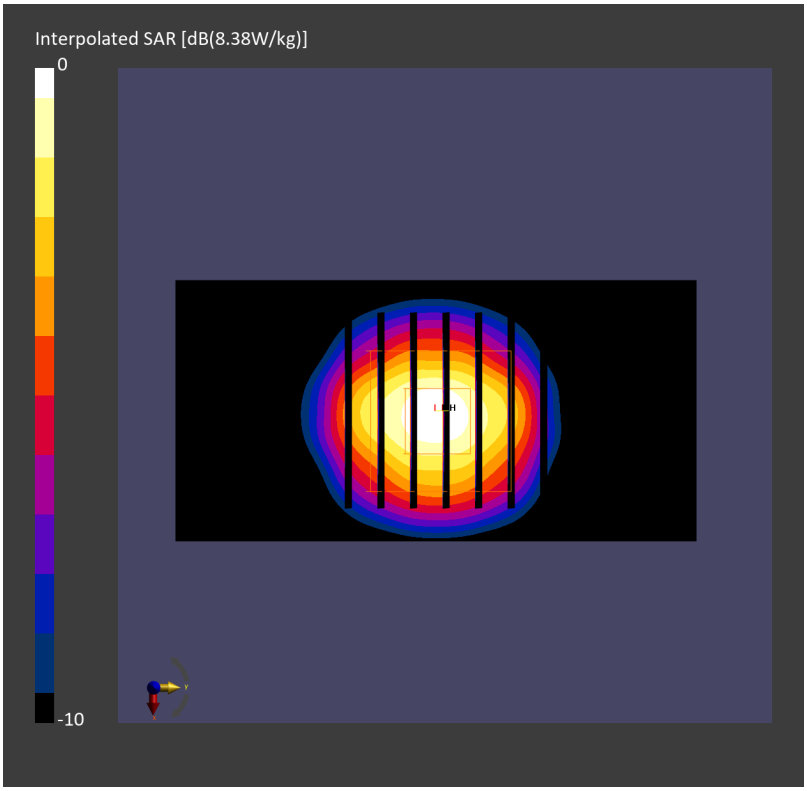

Date: 2026-01-06

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260106 Medium parameters used: f= 3700.000 MHz; σ= 2.92 S/m; $\varepsilon_r$ = 38.2
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.76 W/kg; SAR (10g) = 2.50 W/kg;
TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.04 dB
SAR (1g) = 6.87 W/kg; SAR (8g) = 2.87 W/kg; SAR (10g) = 2.54 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 75.0 %
TSL Correction: Positive only

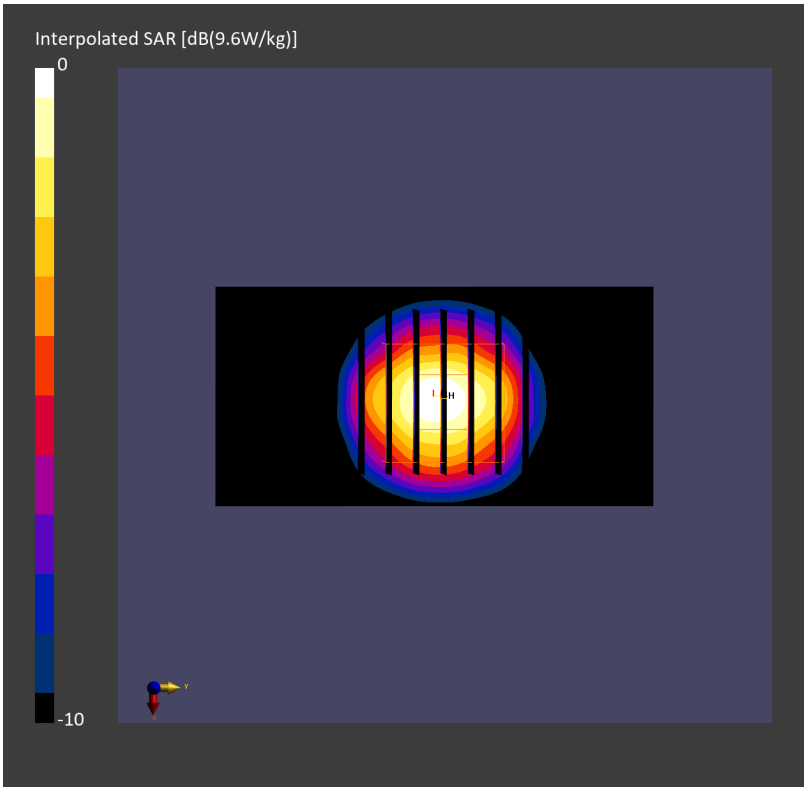

Date: 2026-02-12

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260212 Medium parameters used: f= 3700.000 MHz; σ= 2.90 S/m; $\varepsilon_r$ = 37.4
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.43 W/kg; SAR (10g) = 1.26 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.47 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 75.7 %
TSL Correction: Positive only

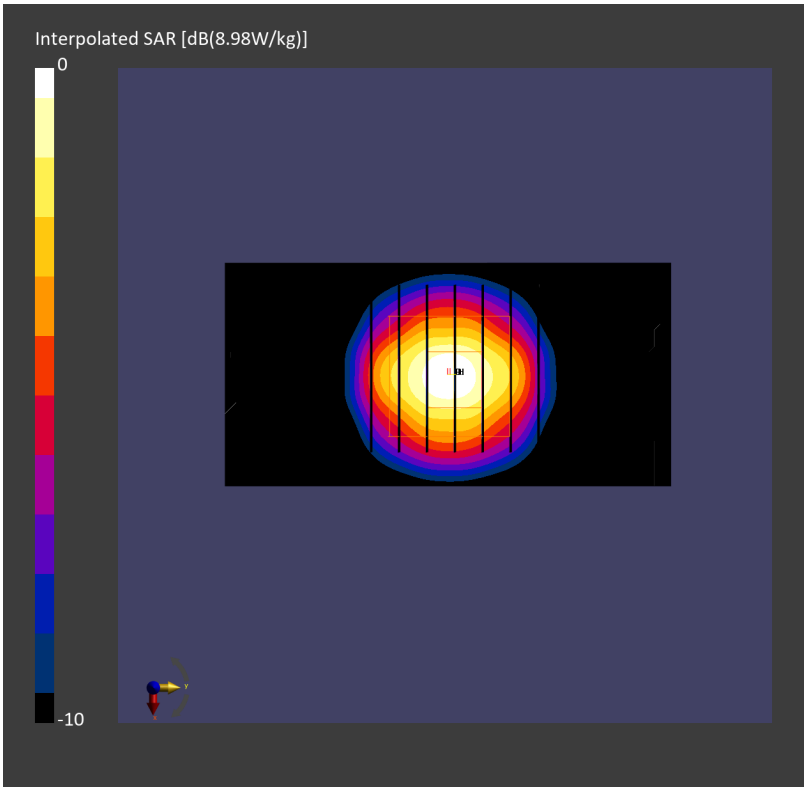

Date: 2026-02-18

**System Check_Head 3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 3700.000 MHz; σ= 2.93 S/m; $\varepsilon_r$ = 37.7
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(6.53, 6.24, 6.94); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.37 W/kg; SAR (10g) = 1.23 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.40 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 74.2 %
TSL Correction: Positive only

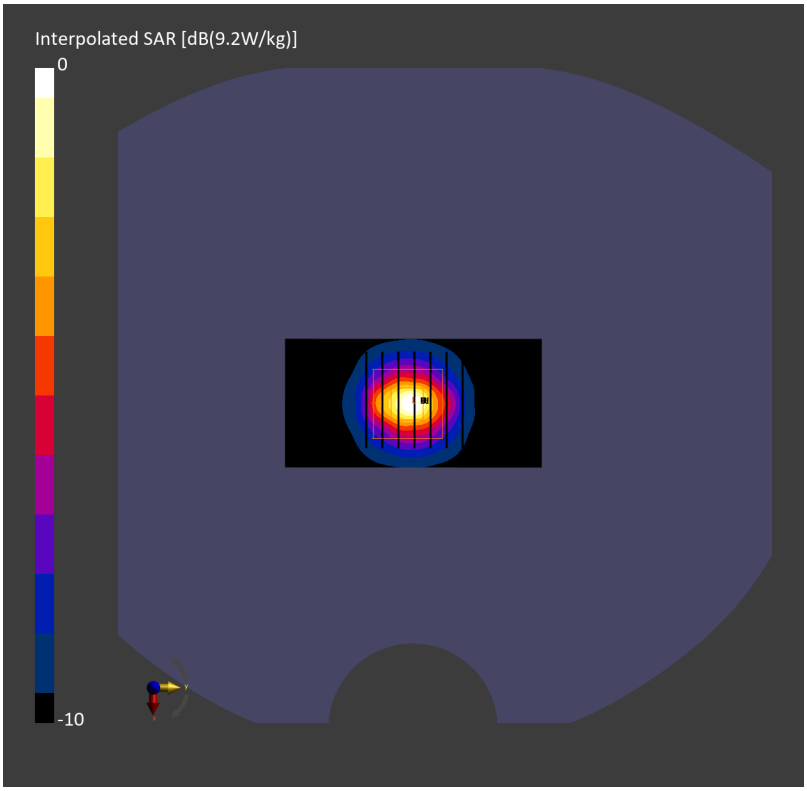

Date: 2026-02-21

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260221 Medium parameters used: f= 3700.000 MHz; σ= 2.89 S/m; $\varepsilon_r$ = 37.9
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.15 W/kg; SAR (10g) = 1.21 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 3.28 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 74.9 %
TSL Correction: Positive only

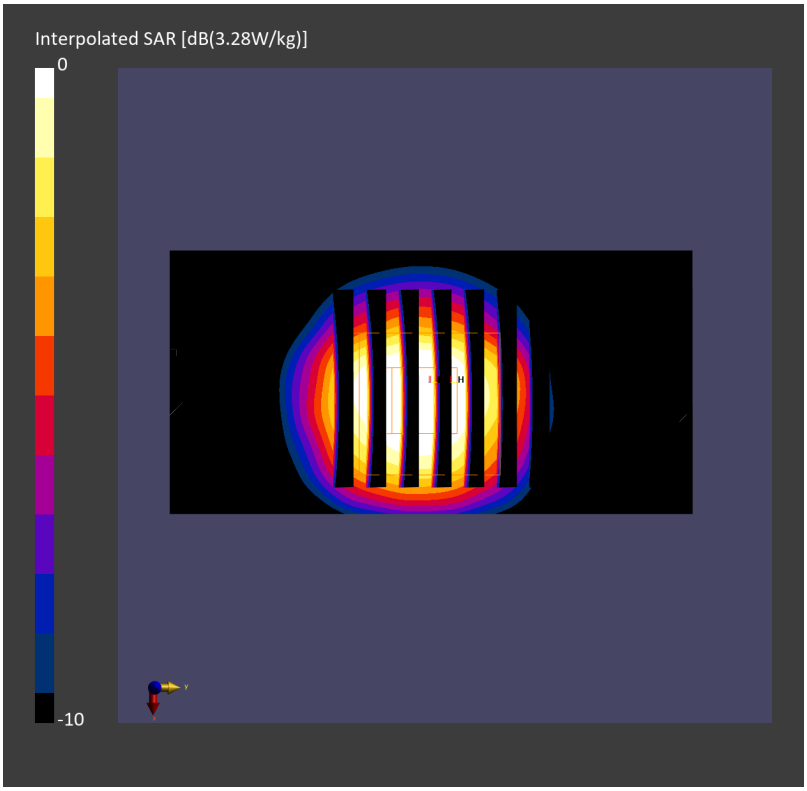

Date: 2026-02-22

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260222 Medium parameters used: f= 3700.000 MHz; σ= 2.92 S/m; $\varepsilon_r$ = 38.0
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.49 W/kg; SAR (10g) = 1.28 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.03 dB
SAR (1g) = 3.54 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.32 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 75.3 %
TSL Correction: Positive only

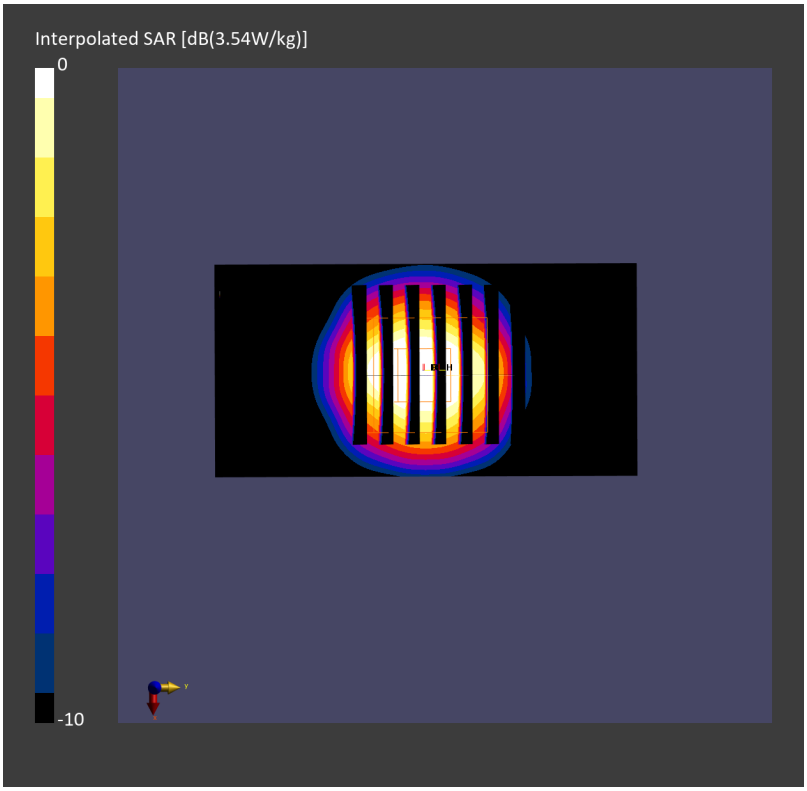

Date: 2026-02-23

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 3700.000 MHz; σ= 2.87 S/m; $\varepsilon_r$ = 40.4
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.46 W/kg; SAR (10g) = 1.28 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.53 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 74.4 %
TSL Correction: Positive only

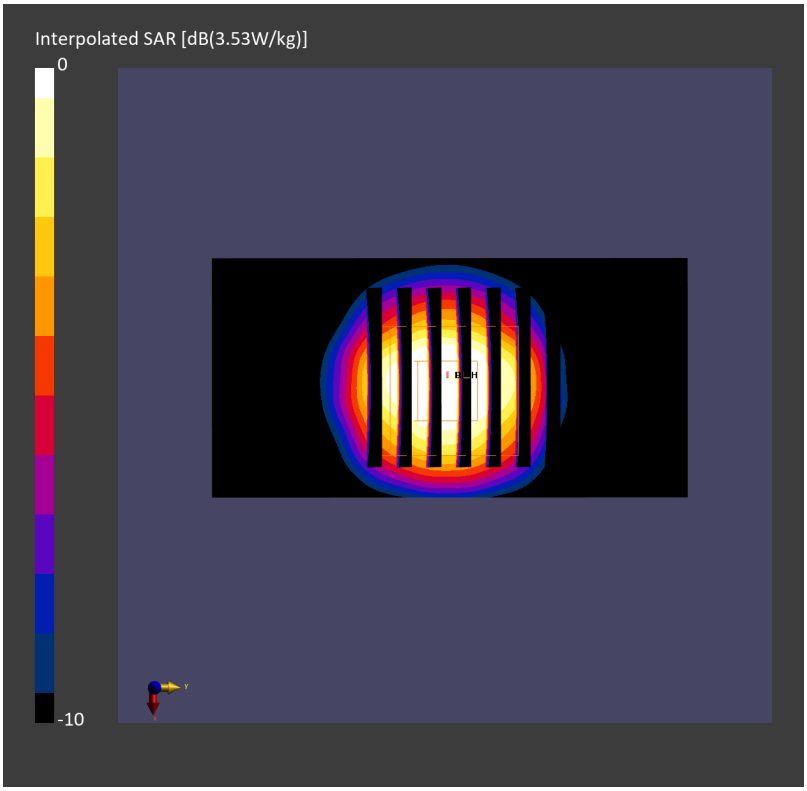

Date: 2026-02-24

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260224 Medium parameters used: f= 3700.000 MHz; σ= 2.89 S/m; $\varepsilon_r$ = 39.3
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.40 W/kg; SAR (10g) = 1.29 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.03 dB
SAR (1g) = 3.48 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 74.9 %
TSL Correction: Positive only

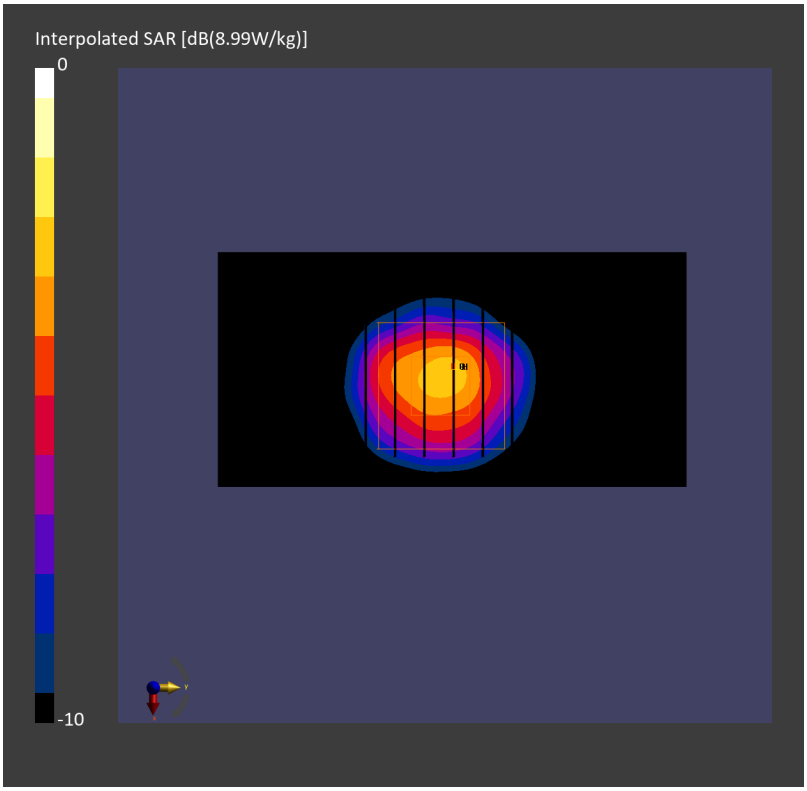

Date: 2026-02-25

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260225 Medium parameters used: f= 3700.000 MHz; σ= 2.92 S/m; $\varepsilon_r$ = 39.3
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.46 W/kg; SAR (10g) = 1.27 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.05 dB
SAR (1g) = 3.48 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 74.8 %
TSL Correction: Positive only

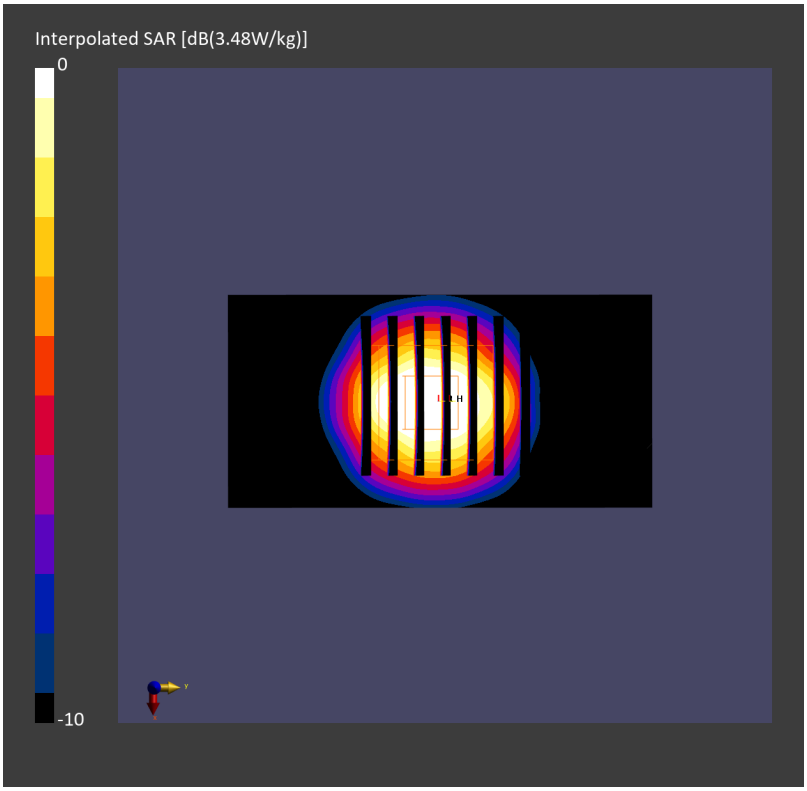

Date: 2026-03-02

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260302 Medium parameters used: f= 3700.000 MHz; σ= 2.93 S/m; $\varepsilon_r$ = 37.5
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.47 W/kg; SAR (10g) = 1.29 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.51 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.32 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.3 %
TSL Correction: Positive only

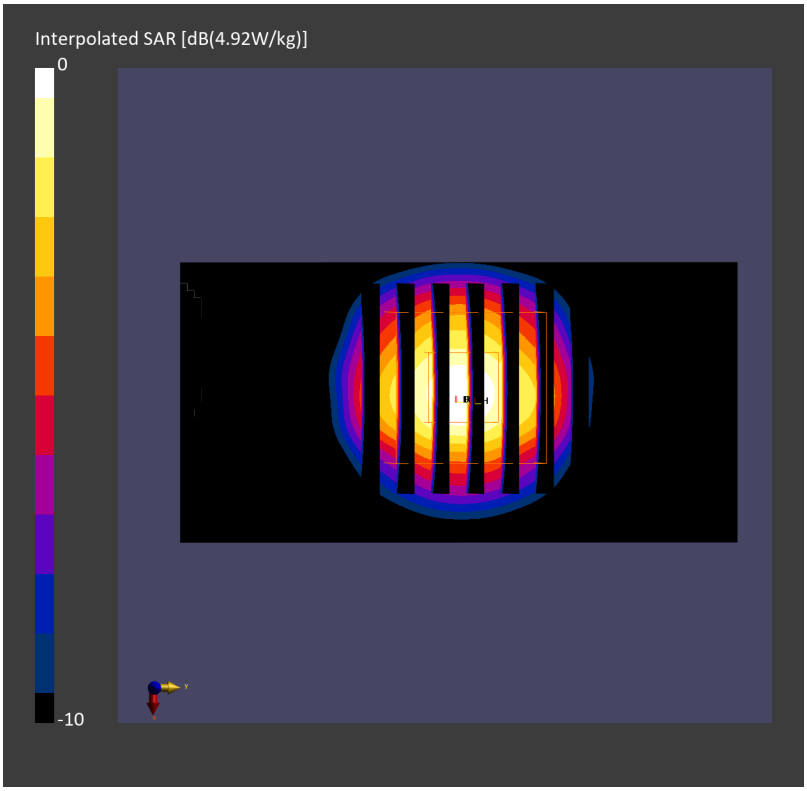

Date: 2026-03-18

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260318 Medium parameters used: f= 3700.000 MHz; σ= 2.91 S/m; $\varepsilon_r$ = 36.8
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 7.18 W/kg; SAR (10g) = 2.66 W/kg;
TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.04 dB
SAR (1g) = 7.46 W/kg; SAR (8g) = 3.13 W/kg; SAR (10g) = 2.77 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.7 %
TSL Correction: Positive only

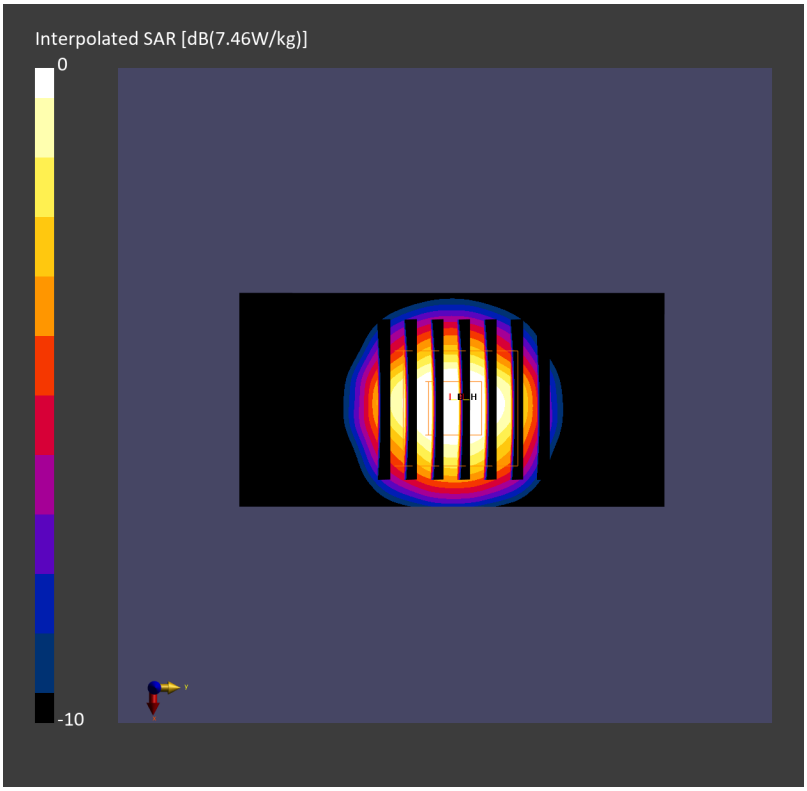

Date: 2026-03-19

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260319 Medium parameters used: f= 3700.000 MHz; σ= 2.95 S/m; $\varepsilon_r$ = 39.8
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.46 W/kg; SAR (10g) = 1.27 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.02 dB
SAR (1g) = 3.48 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 75.4 %
TSL Correction: Positive only

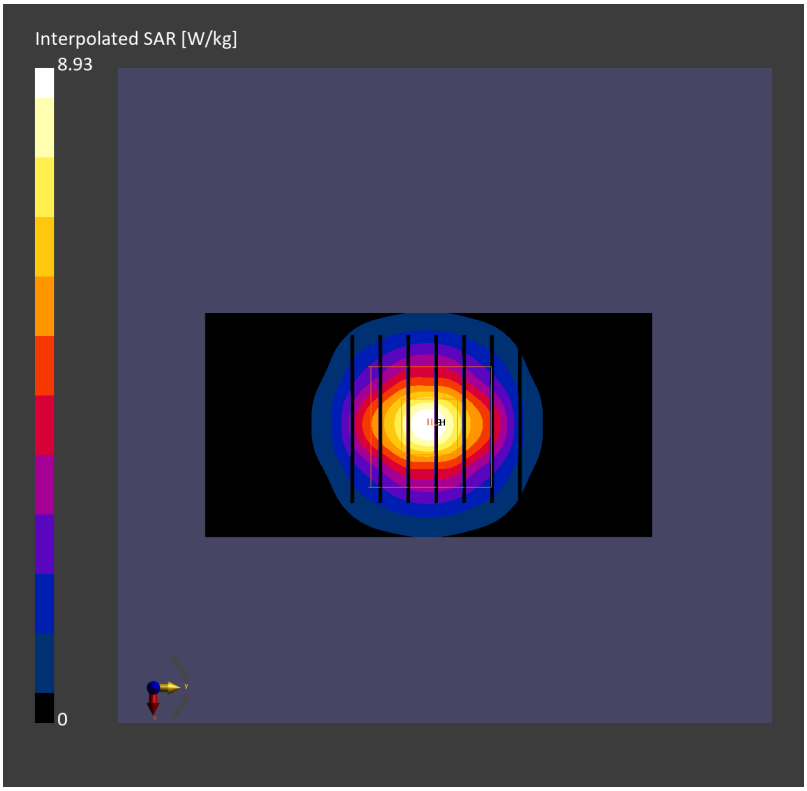

Date: 2026-04-16

**System Check_Head 3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260416 Medium parameters used: f= 3700.000 MHz; σ= 2.86 S/m; $\varepsilon_r$ = 37.4
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(6.61, 6.72, 6.43); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144_Gap; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=16.5dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.89 W/kg; SAR (10g) = 1.11 W/kg;
TSL Correction: Positive only

**Pin=16.5dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.04 dB
SAR (1g) = 3.09 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.6 %
TSL Correction: Positive only

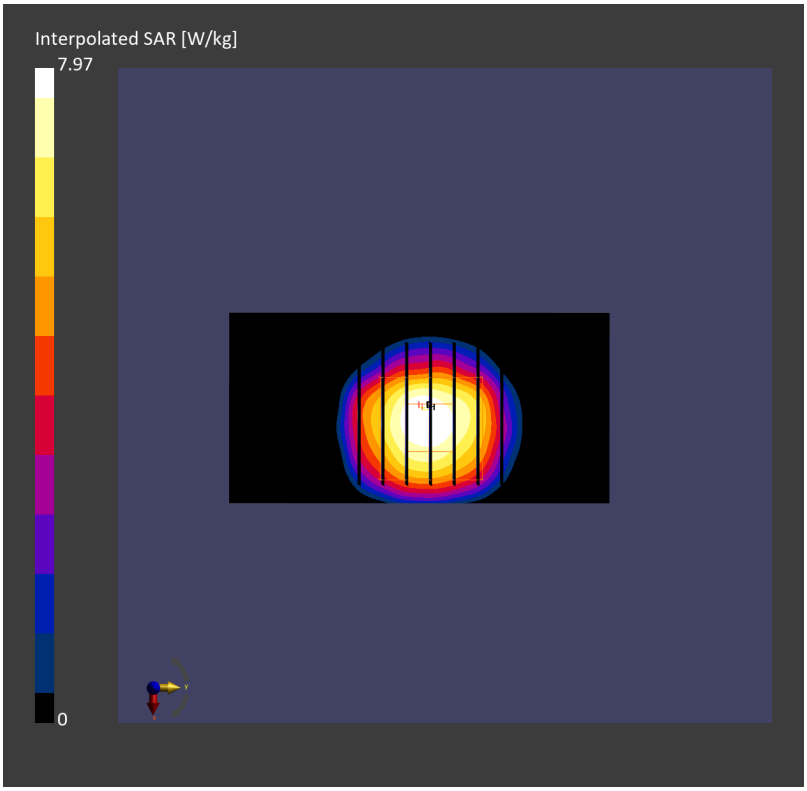

Date: 2026-04-17

**System Check_Head_3700MHz**

**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_600-7200_260417 Medium parameters used: f= 3700.000 MHz; σ= 2.90 S/m; $\varepsilon_r$ = 37.6
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.34, 6.24, 6.28); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.48 W/kg; SAR (10g) = 1.28 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.53 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.31 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.1 %
TSL Correction: Positive only

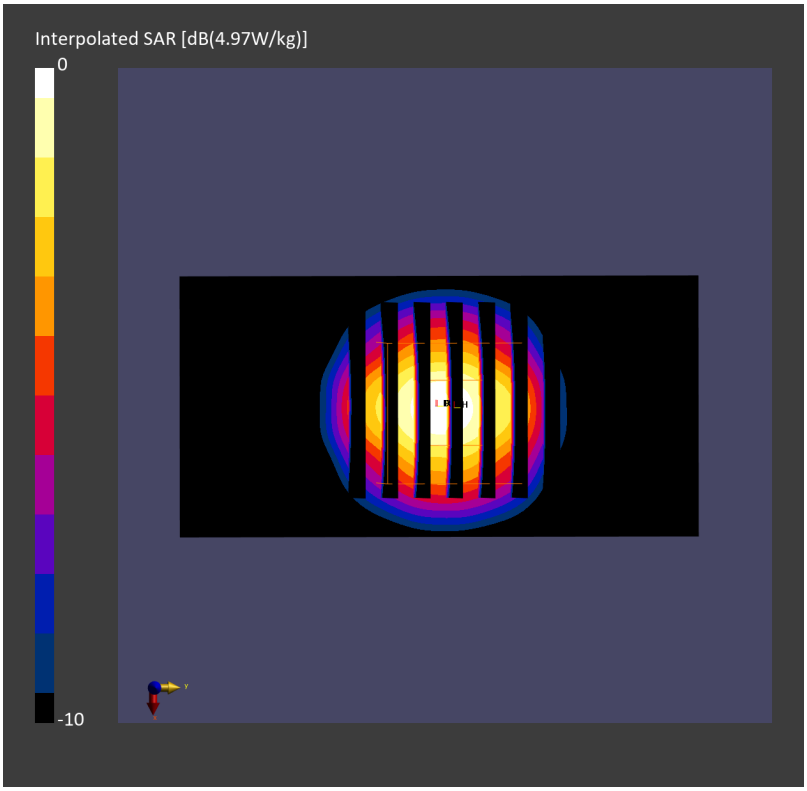

Date: 2026-01-06

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260106 Medium parameters used: f= 3900.000 MHz; σ= 3.14 S/m; $\varepsilon_r$ = 37.9
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2025-02-12
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.46 W/kg; SAR (10g) = 2.30 W/kg;
TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.02 dB
SAR (1g) = 6.71 W/kg; SAR (8g) = 2.70 W/kg; SAR (10g) = 2.37 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 72.9 %
TSL Correction: Positive only

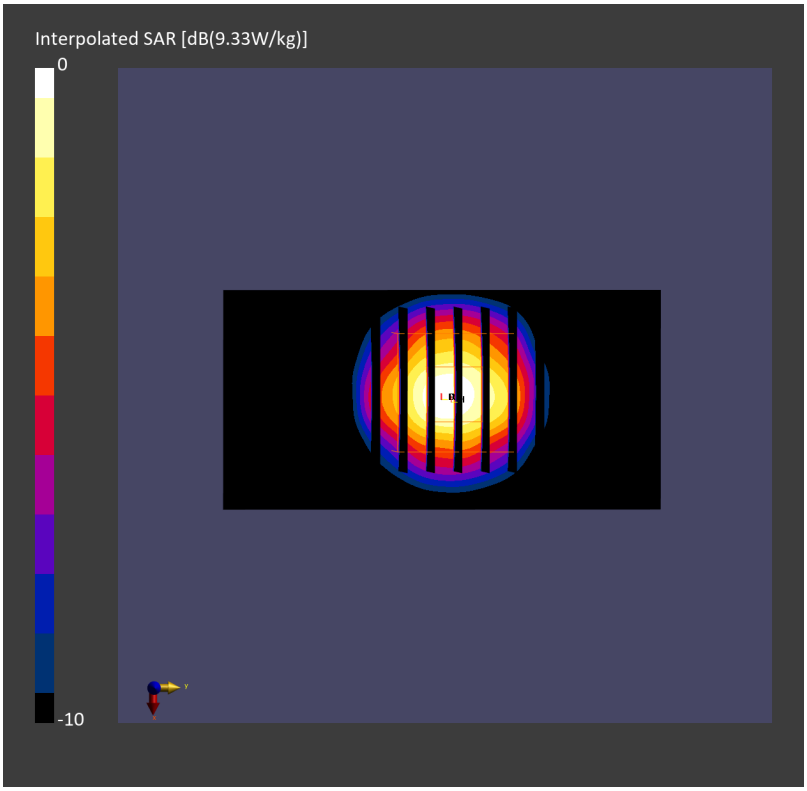

Date: 2026-02-18

**System Check_Head 3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260218 Medium parameters used: f= 3900.000 MHz; σ= 3.11 S/m; $\varepsilon_r$ = 37.4
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7625; ConvF(6.45, 6.17, 6.86); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2025-06-16
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.00 W/kg; SAR (10g) = 1.08 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.02 dB
SAR (1g) = 3.13 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 72.6 %
TSL Correction: Positive only

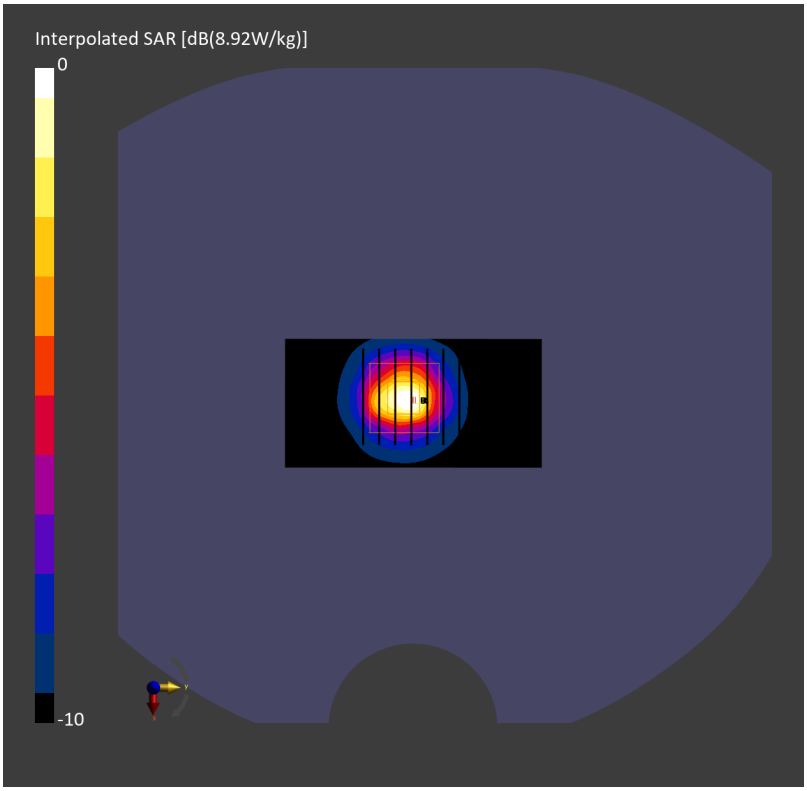

Date: 2026-02-21

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260221 Medium parameters used: f= 3900.000 MHz; σ= 3.09 S/m; $\varepsilon_r$ = 37.6
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.17 W/kg; SAR (10g) = 1.14 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.06 dB
SAR (1g) = 3.26 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 73.8 %
TSL Correction: Positive only

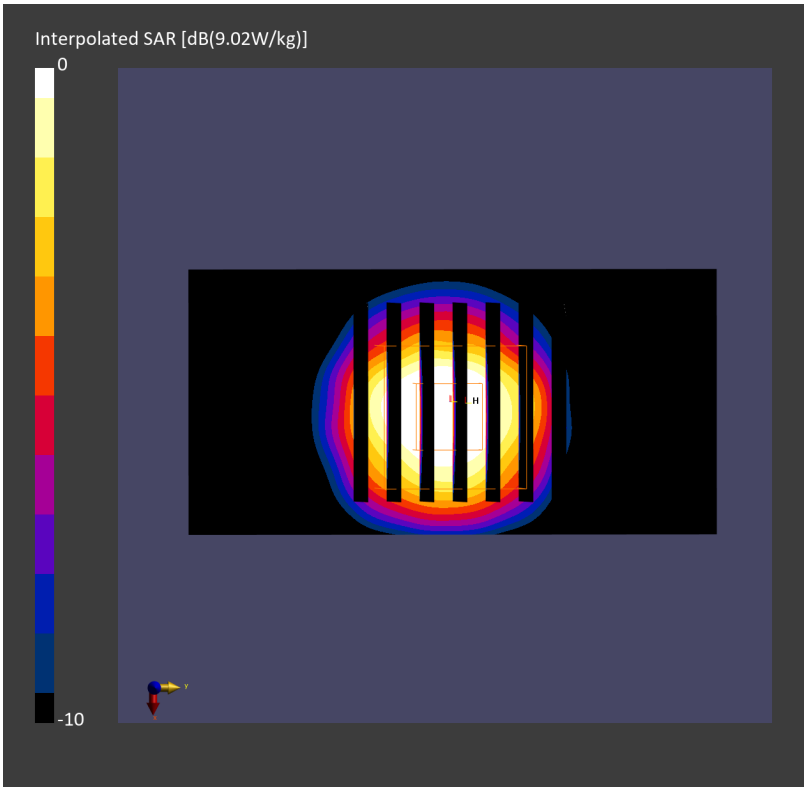

Date: 2026-02-22

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260222 Medium parameters used: f= 3900.000 MHz; σ= 3.11 S/m; $\varepsilon_r$ = 37.7
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.18 W/kg; SAR (10g) = 1.12 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.24 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 74.1 %
TSL Correction: Positive only

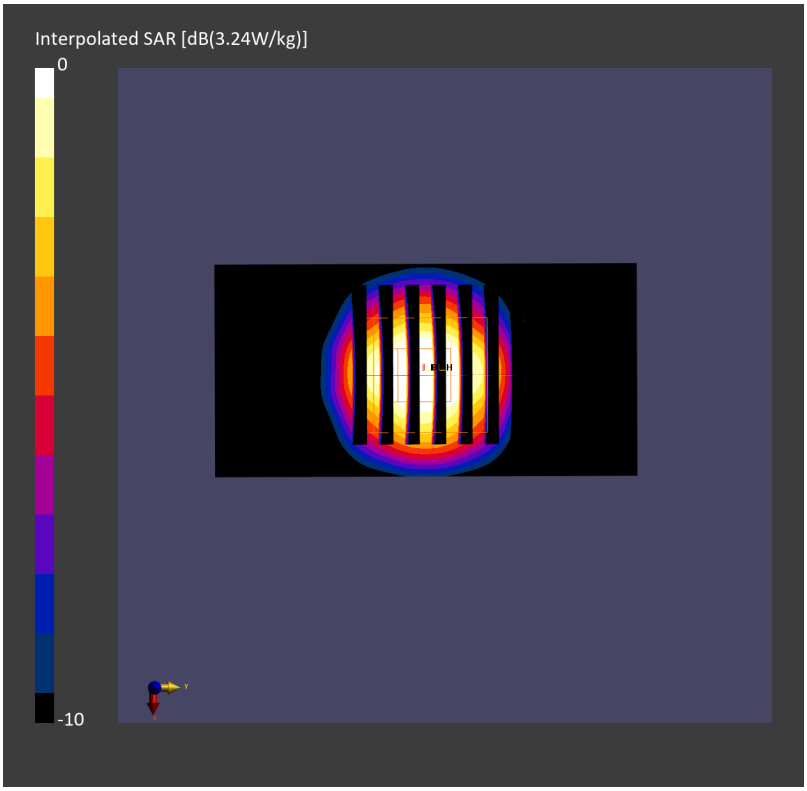

Date: 2026-02-23

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260223 Medium parameters used: f= 3900.000 MHz; σ= 3.06 S/m; $\varepsilon_r$ = 40.2
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.22 W/kg; SAR (10g) = 1.14 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.02 dB
SAR (1g) = 3.30 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.16 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 73.5 %
TSL Correction: Positive only

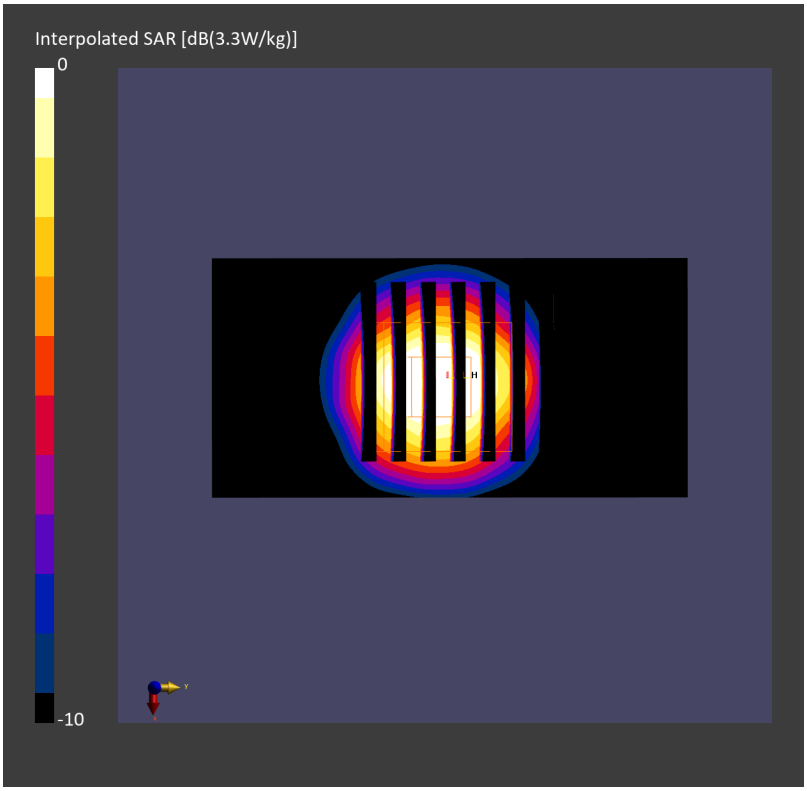

Date: 2026-02-24

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260224 Medium parameters used: f= 3900.000 MHz; σ= 3.08 S/m; $\varepsilon_r$ = 39.0
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.13 W/kg; SAR (10g) = 1.13 W/kg;
TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.03 dB
SAR (1g) = 3.22 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 73.8 %
TSL Correction: Positive only

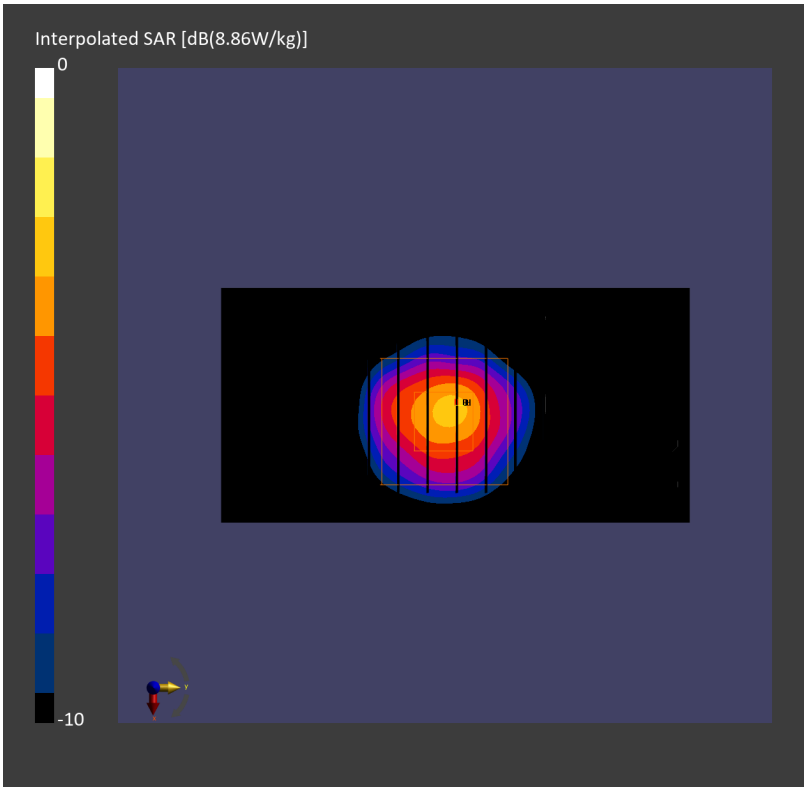

Date: 2026-02-25

**System Check_Head_3900MHz**

**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_600-7200_260225 Medium parameters used: f= 3900.000 MHz; σ= 3.10 S/m; $\varepsilon_r$ = 39.1
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:
- Probe: EX3DV4 - SN7814; ConvF(6.37, 6.27, 6.31); Calibrated: 2025-06-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2026-01-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm)**: Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.28 W/kg; SAR (10g) = 1.18 W/kg;
TSL Correction: Positive only
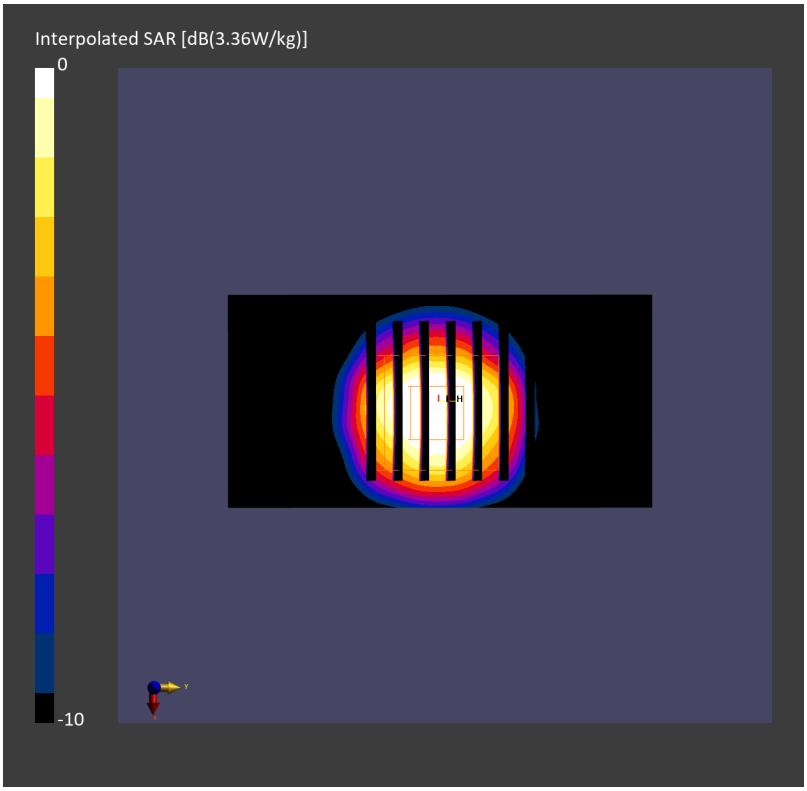
**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm)**: Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.04 dB
SAR (1g) = 3.36 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 73.8 %
TSL Correction: Positive only